



US00D865998S

(12) **United States Design Patent** (10) **Patent No.:** **US D865,998 S**  
**Mellett et al.** (45) **Date of Patent:** **\*\* Nov. 5, 2019**

(54) **USER INTERFACE FOR MEDICAL WORKSTATION**

(71) Applicant: **Hologic, Inc.**, Bedford, MA (US)

(72) Inventors: **Alyssa Mellett**, Kennesaw, GA (US);  
**Russell Kroll**, Atlanta, GA (US)

(73) Assignee: **Hologic, Inc.**, Marlborough, MA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/585,527**

(22) Filed: **Nov. 25, 2016**

(51) **LOC (12) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/234**; D24/186

(58) **Field of Classification Search**  
USPC ..... D24/231, 185, 186, 169, 142, 158, 177,  
D24/184, 216, 209, 108; D14/447, 344,  
D14/486, 341, 346, 336; D10/15  
CPC ..... A61B 5/1071  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D352,463 S *	11/1994	Kubo	.....	D10/15
D361,129 S *	8/1995	Collins	.....	D24/169
D365,996 S *	1/1996	Peterson	.....	D10/78
D372,981 S *	8/1996	McMahan, Jr.	.....	D24/186
D415,834 S *	10/1999	Bar	.....	D24/165
D426,833 S	6/2000	Vanelli		
D461,895 S *	8/2002	Barnes	.....	D24/158
6,792,801 B2	9/2004	Hoggan		
D504,516 S	4/2005	Yamazaki		
D507,832 S *	7/2005	Yanniello	.....	D24/108
D510,625 S *	10/2005	Widener	.....	D24/186
D526,063 S	8/2006	Widener		
D536,788 S *	2/2007	Trifilio	.....	D24/133
D538,243 S *	3/2007	Seo	.....	D14/129

D541,941 S *	5/2007	Nakanishi	.....	D24/165
D547,454 S *	7/2007	Hsieh	.....	D24/186
D547,873 S *	7/2007	Hood	.....	D24/188
D549,343 S *	8/2007	Schlagheck	.....	D24/169
D550,364 S *	9/2007	Glover	.....	D24/186
D551,350 S *	9/2007	Lorimer	.....	D24/186
D560,811 S	1/2008	Powell		
D587,376 S *	2/2009	Takano	.....	D24/169
D595,415 S	6/2009	Fukuzawa		
D598,113 S *	8/2009	Flaction	.....	D24/187
D601,256 S	9/2009	Takano		
D603,518 S	11/2009	Zafar		
D605,297 S	12/2009	Unsworth		
D605,771 S	12/2009	Unsworth		

(Continued)

*Primary Examiner* — Rhea Shields

(57) **CLAIM**


The ornamental design for a user interface for medical workstation, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a first embodiment of a user interface for medical workstation showing our new design. FIG. 2 is a front view of the user interface for medical workstation of FIG. 1. FIG. 3 is a back view of the user interface for medical workstation of FIG. 1. FIG. 4 is a right-side view of the user interface for medical workstation of FIG. 1. FIG. 5 is a left-side view of the user interface for medical workstation of FIG. 1. FIG. 6 is a top view of the user interface for medical workstation of FIG. 1; and, FIG. 7 is a bottom view of the user interface for medical workstation of FIG. 1.

In the drawings, the broken lines are for the purpose of illustrating environment only and form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

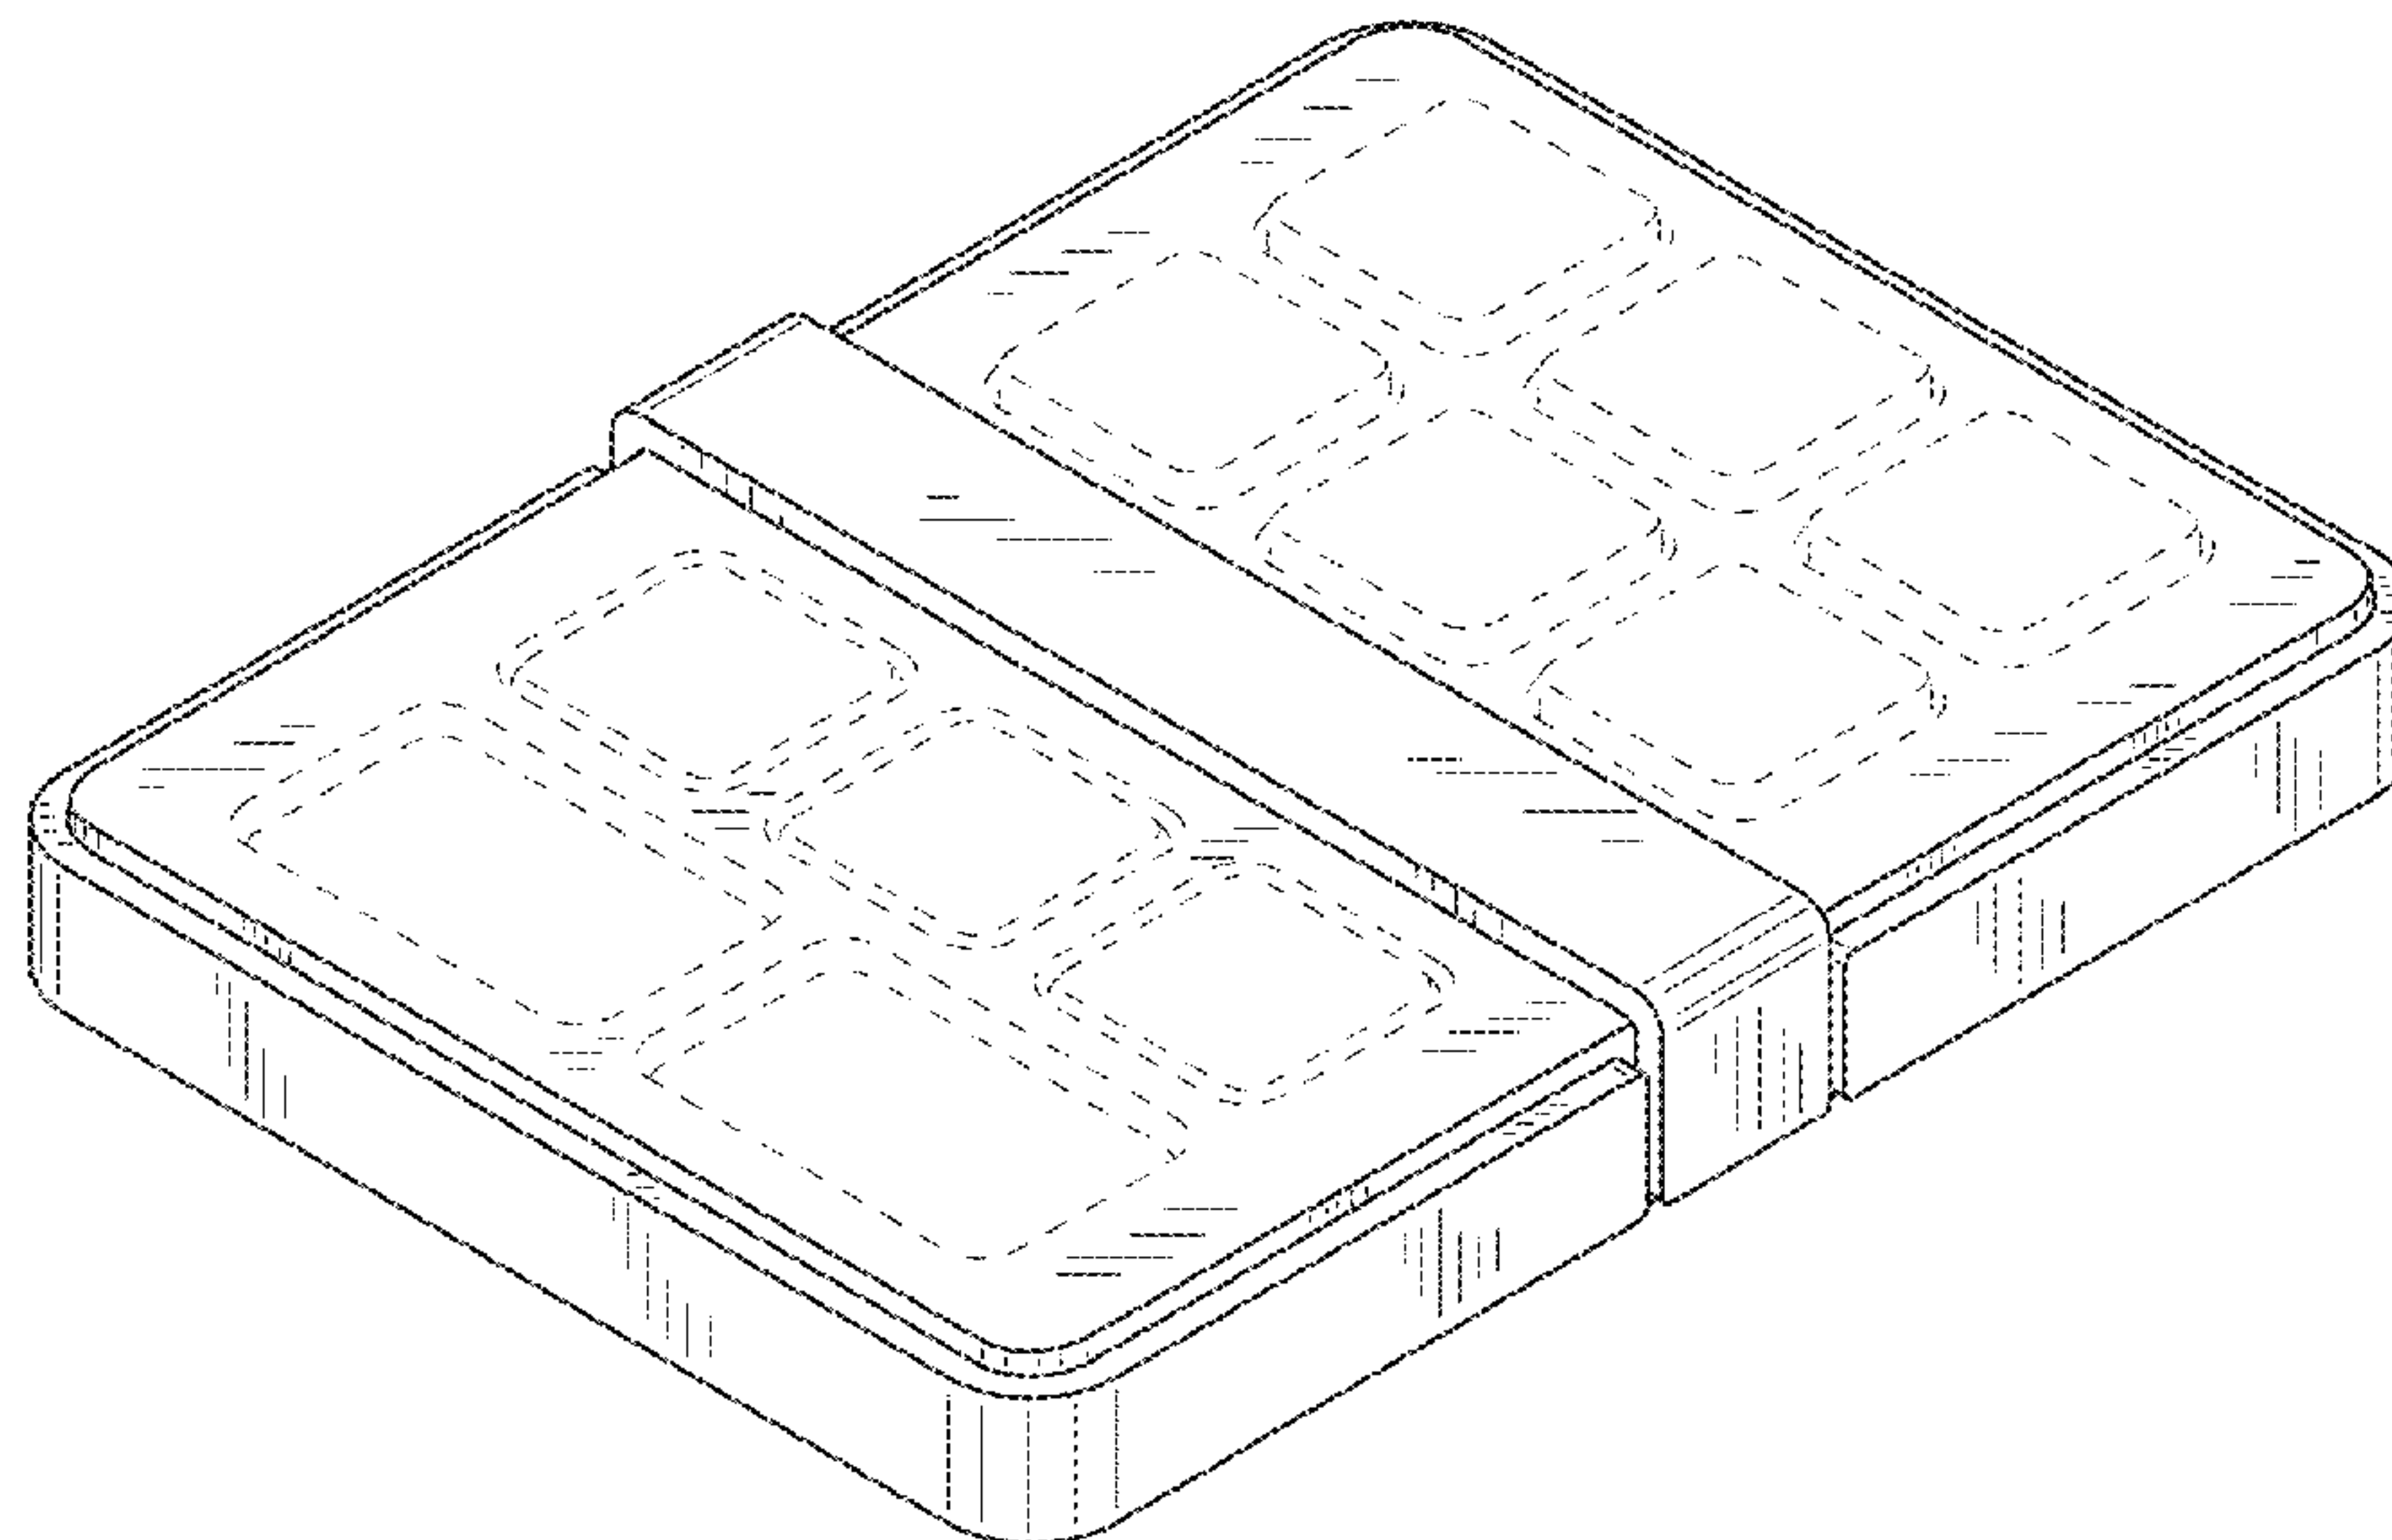

(56)

References Cited

U.S. PATENT DOCUMENTS

D606,199 S 12/2009 Vu  
 D606,203 S 12/2009 Husheer  
 D609,197 S \* 2/2010 Koskela ..... D13/168  
 D609,349 S 2/2010 Pelissier  
 D612,503 S \* 3/2010 Johnston ..... D24/186  
 D613,411 S \* 4/2010 Collins ..... D24/186  
 D616,993 S \* 6/2010 Muis ..... D24/186  
 D629,113 S \* 12/2010 Wodecki ..... D24/186  
 D634,435 S \* 3/2011 Chua ..... D24/186  
 D641,881 S \* 7/2011 Inami ..... D24/165  
 D670,810 S \* 11/2012 Fukuzawa ..... D24/169  
 D673,151 S \* 12/2012 Bousfield ..... D14/385  
 D673,153 S \* 12/2012 Bousfield ..... D14/385  
 D675,321 S \* 1/2013 Sanga ..... D24/177  
 D684,574 S \* 6/2013 Taunay da Graca Couto .....  
 D14/385  
 D687,540 S \* 8/2013 Nair ..... D24/111  
 D688,060 S 8/2013 Sizelove  
 D696,403 S \* 12/2013 Noguchi ..... D24/165  
 D696,404 S \* 12/2013 Golnik ..... D24/169  
 D698,443 S 1/2014 Prais  
 D700,702 S \* 3/2014 Kolb ..... D24/169  
 D705,190 S \* 5/2014 Shigeno ..... D14/186  
 D712,041 S \* 8/2014 Glaesker ..... D24/184  
 8,894,585 B2 11/2014 Hasbun  
 D719,999 S \* 12/2014 Sohrabi ..... D18/4.4  
 D721,814 S \* 1/2015 Creed ..... D13/168  
 D732,729 S \* 6/2015 McKechnie ..... D26/118  
 D736,111 S \* 8/2015 Klein ..... D10/78  
 D738,507 S 9/2015 Prais  
 D738,755 S \* 9/2015 Druce ..... D10/50  
 D739,938 S \* 9/2015 Schempp ..... D24/165  
 D742,371 S \* 11/2015 Bopp ..... D14/336

D743,035 S \* 11/2015 Uozumi ..... D24/165  
 D745,167 S \* 12/2015 Canas ..... D10/78  
 D748,271 S \* 1/2016 Clowry ..... D24/186  
 D749,073 S \* 2/2016 Navon ..... D14/346  
 D751,205 S \* 3/2016 Tan ..... D24/158  
 D755,977 S 5/2016 Winkelmann  
 D766,442 S 9/2016 Prais  
 D769,241 S \* 10/2016 Mazz ..... D14/341  
 D770,034 S \* 10/2016 McNall, III ..... D24/108  
 D770,052 S 10/2016 Abu-Tarif  
 D774,057 S \* 12/2016 Anderson ..... D14/486  
 D779,677 S \* 2/2017 Chen ..... D24/215  
 D784,541 S \* 4/2017 Hilbig ..... D24/186  
 D791,336 S 7/2017 Lei  
 D795,252 S 8/2017 Chung  
 D799,484 S \* 10/2017 Tamillow ..... D14/391  
 D800,909 S \* 10/2017 Jones ..... D24/169  
 D800,912 S \* 10/2017 Uzri ..... D24/216  
 D801,538 S \* 10/2017 Rondoni ..... D24/186  
 D804,033 S 11/2017 Wightman  
 D810,042 S \* 2/2018 Pazhoor ..... D14/158  
 D810,306 S \* 2/2018 Rondoni ..... D24/186  
 D810,947 S \* 2/2018 Larson ..... D24/186  
 D821,592 S \* 6/2018 Pham ..... D24/200  
 D822,216 S \* 7/2018 Barker ..... D24/186  
 D822,217 S \* 7/2018 Sebban ..... D24/186  
 D824,034 S \* 7/2018 Pushpala ..... D24/186  
 D829,337 S 9/2018 Klein  
 D833,624 S \* 11/2018 DeJong ..... D24/186  
 D834,583 S 11/2018 Janzen  
 D834,721 S 11/2018 Klein  
 D835,798 S \* 12/2018 Ito ..... D24/225  
 D836,639 S 12/2018 Volta  
 D836,769 S \* 12/2018 Kabel-Eckes ..... D24/111  
 D836,789 S 12/2018 Jiang  
 D839,424 S 1/2019 Golosarsky

\* cited by examiner

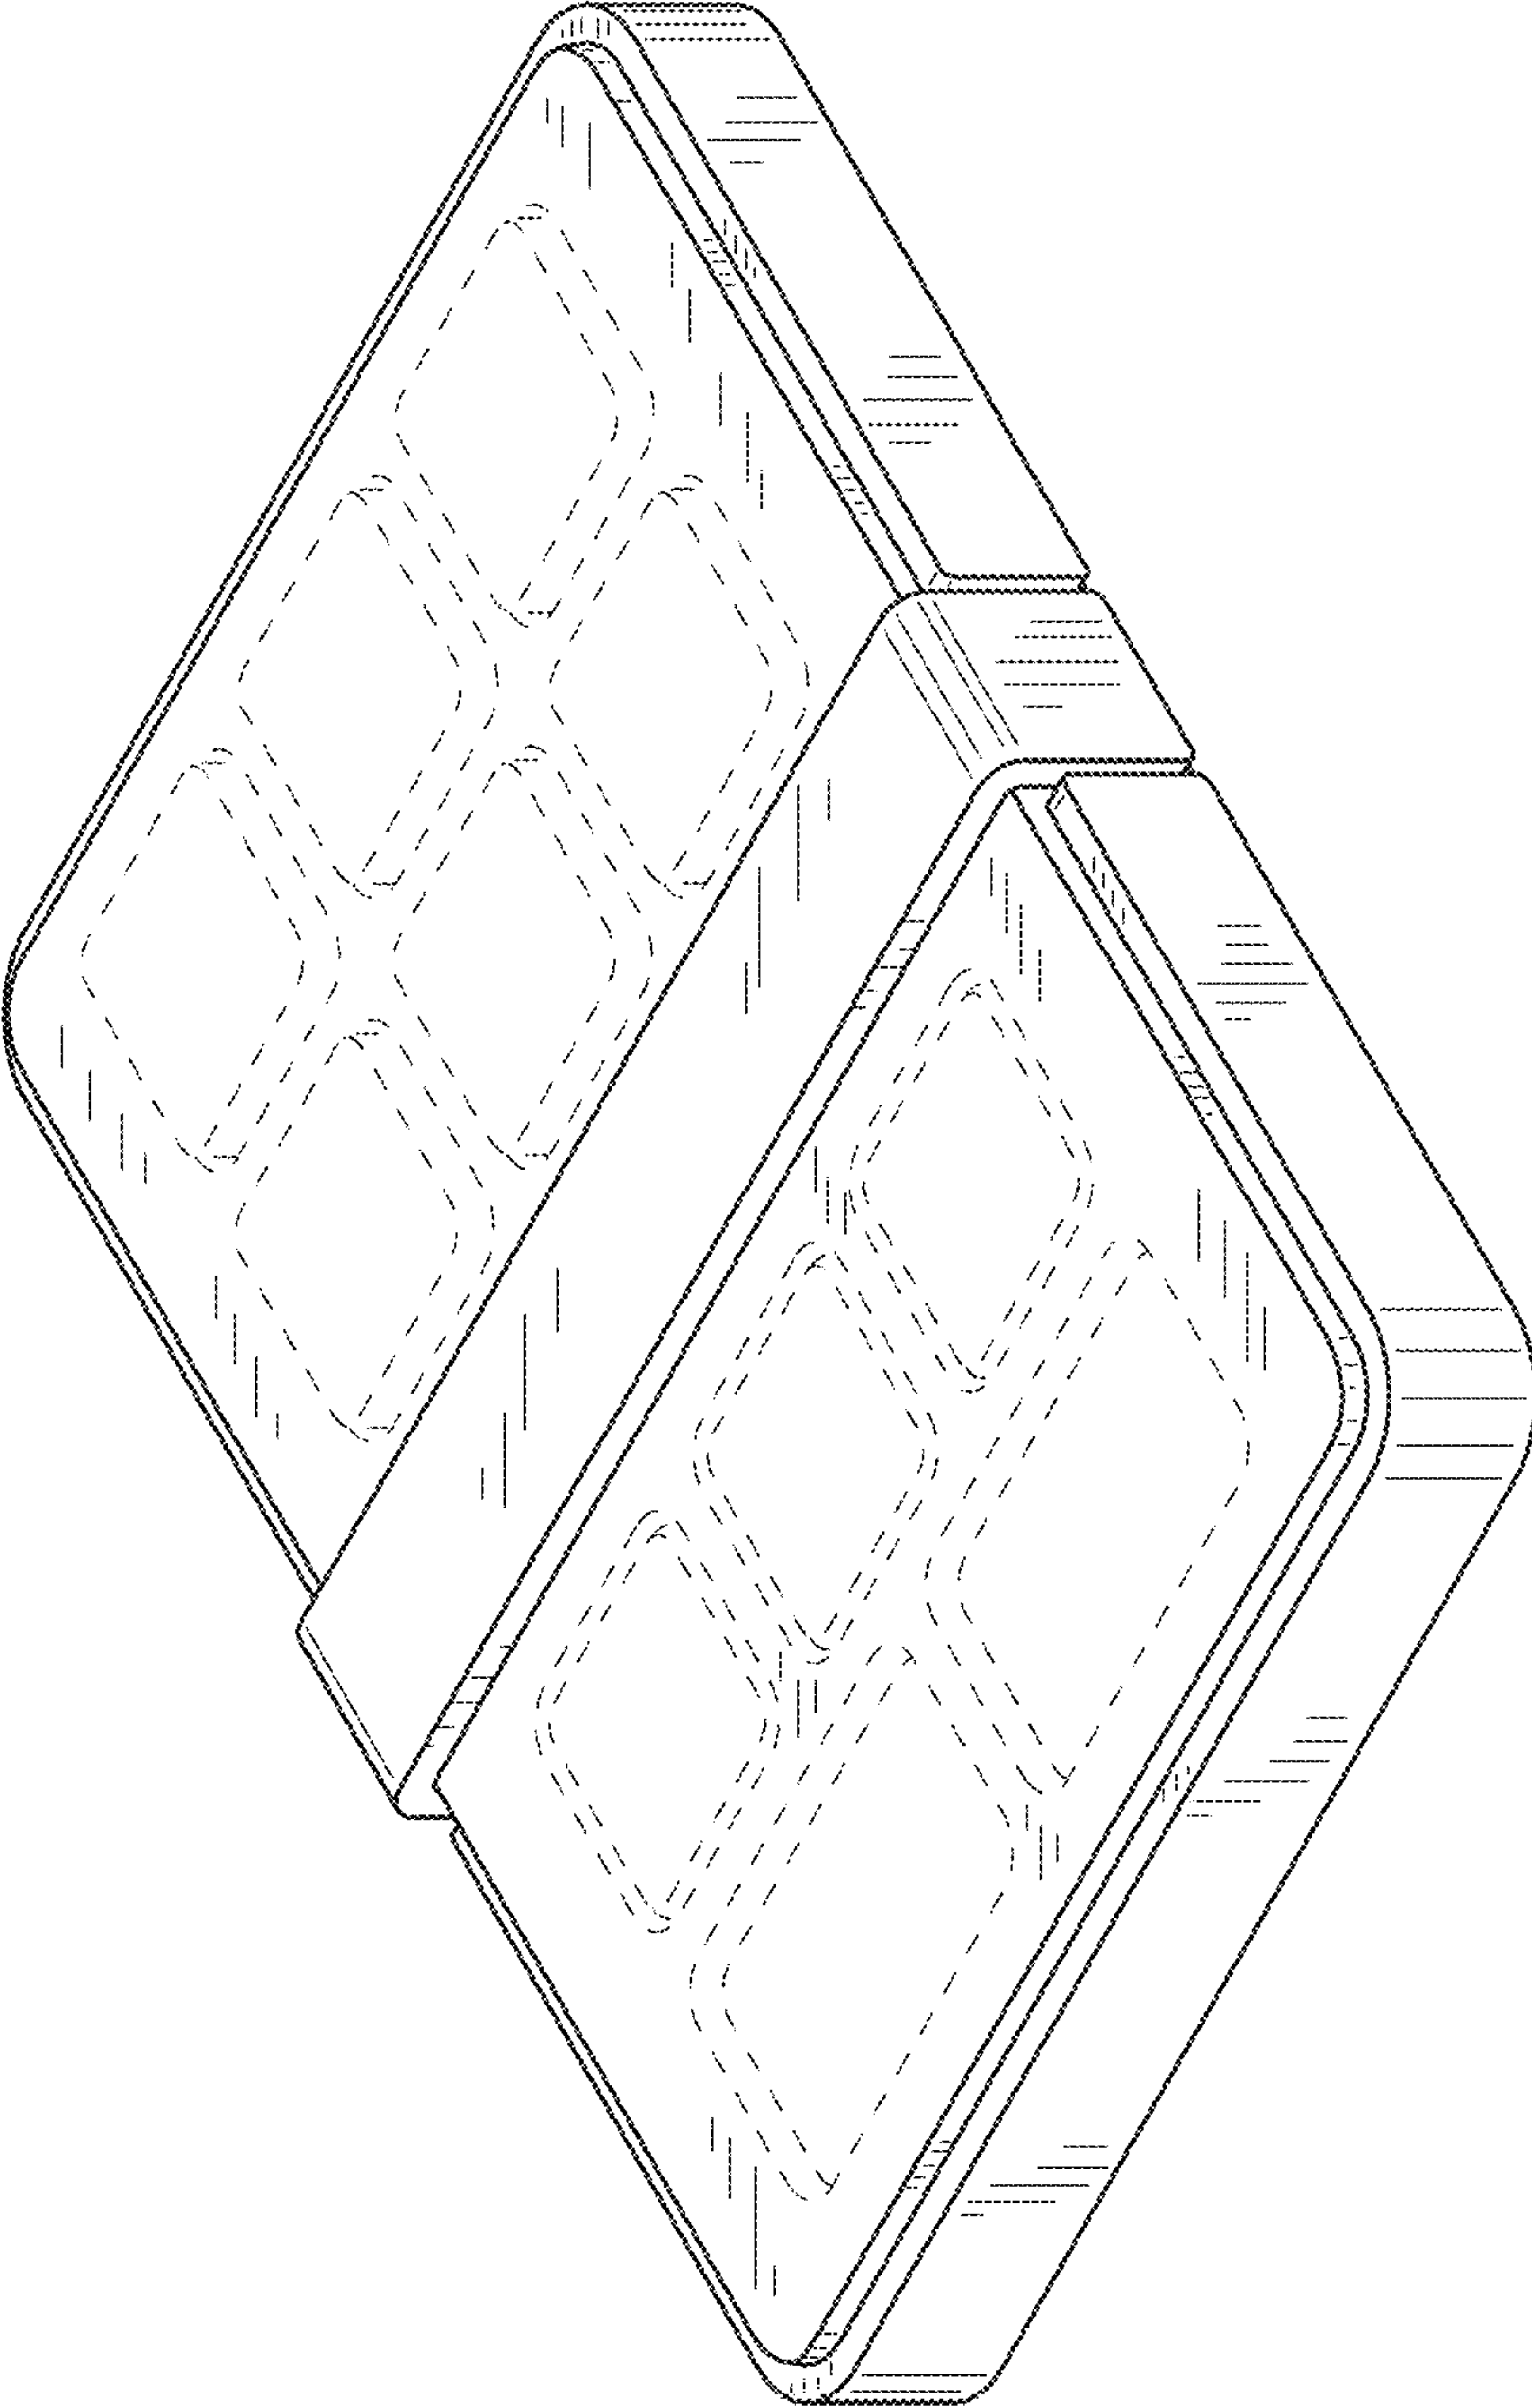


FIG.1



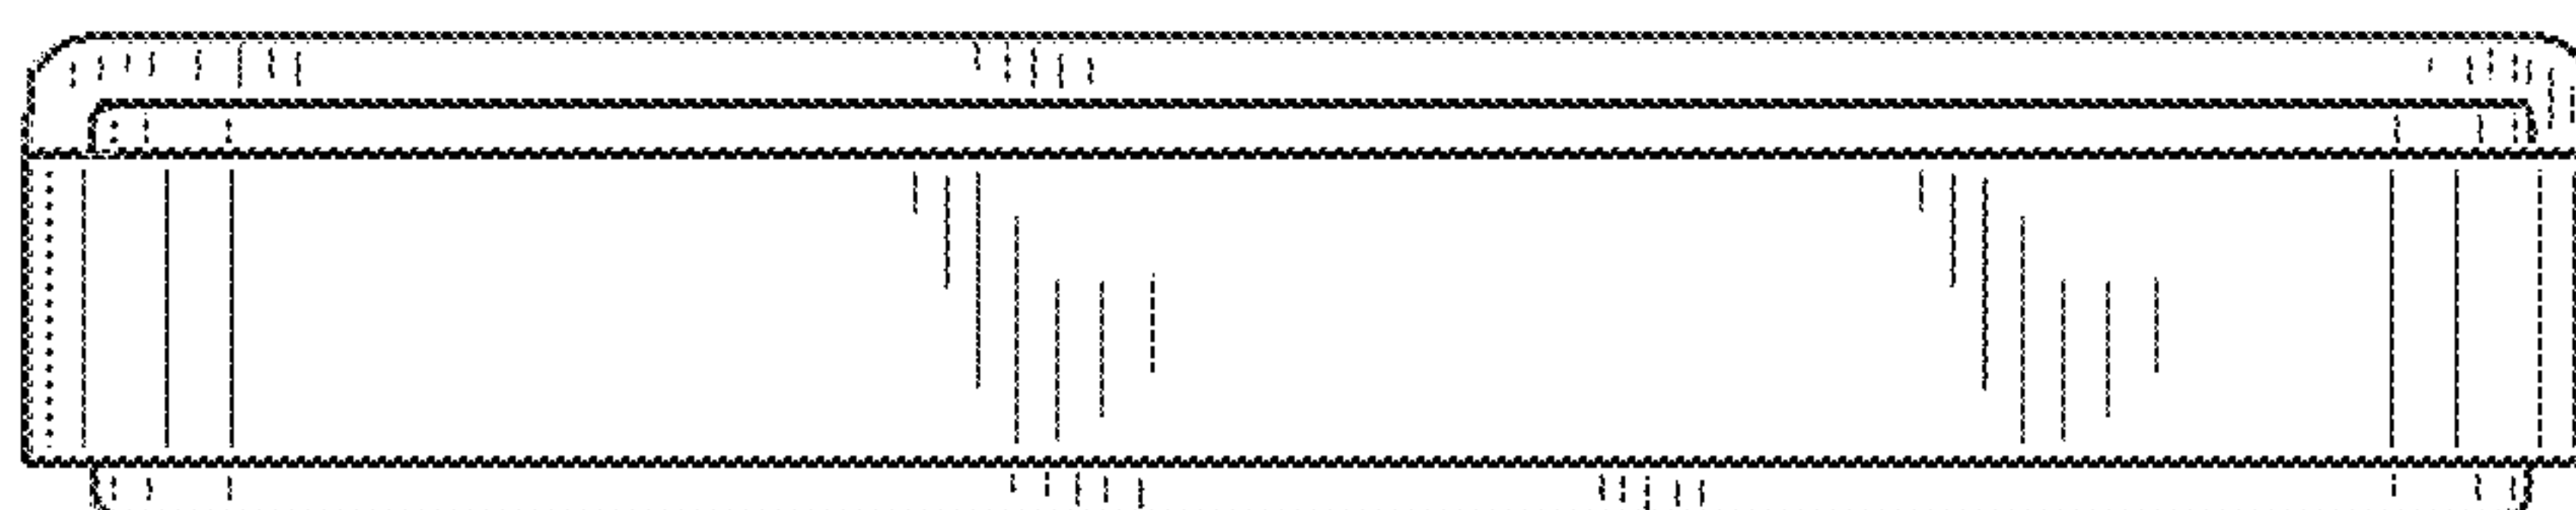


FIG.2

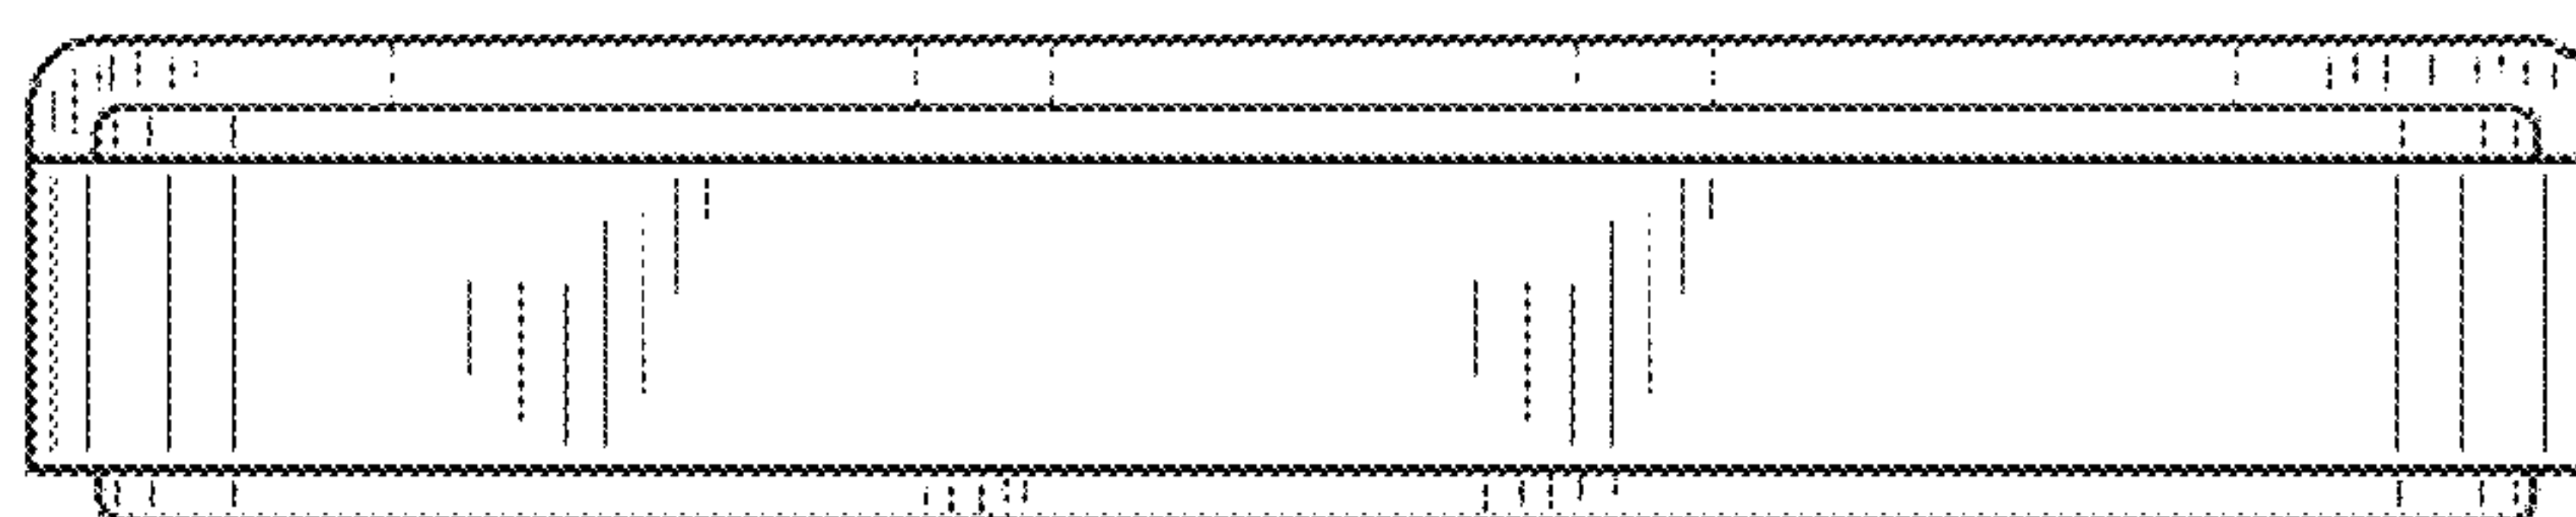


FIG.3

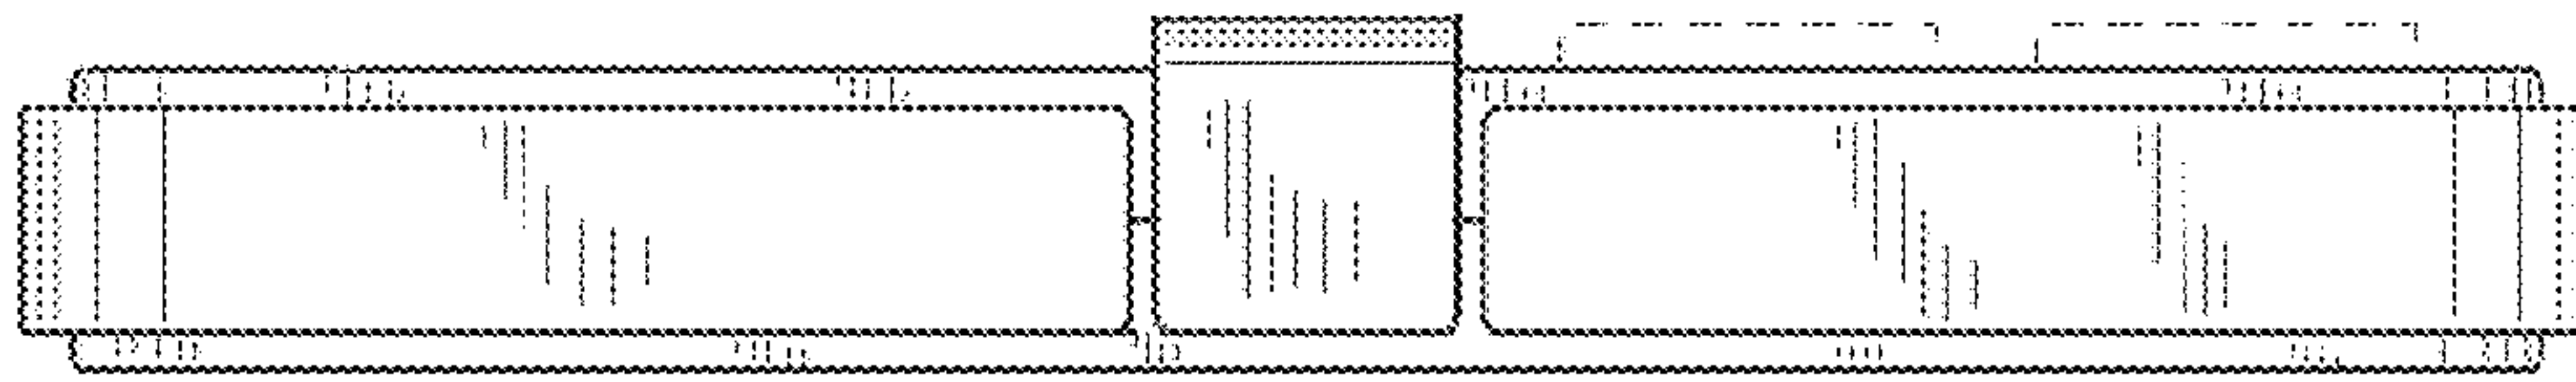


FIG. 4

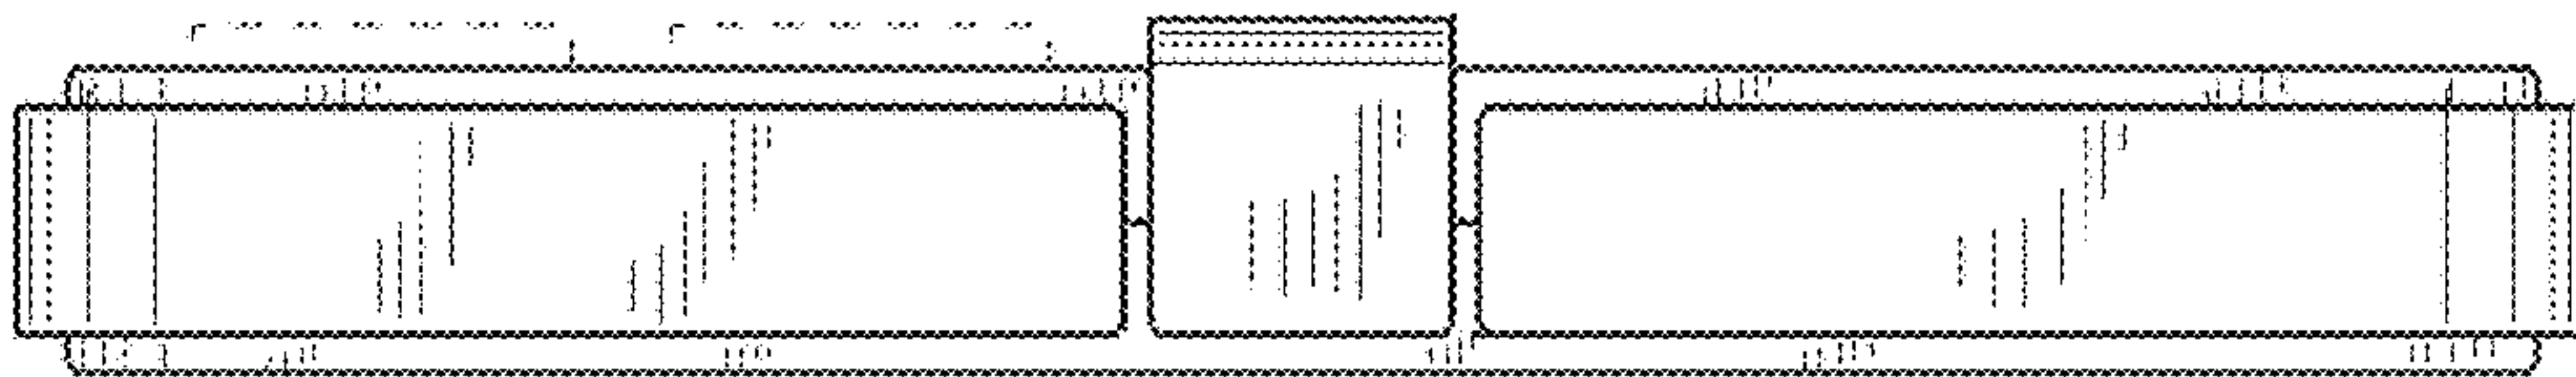


FIG. 5

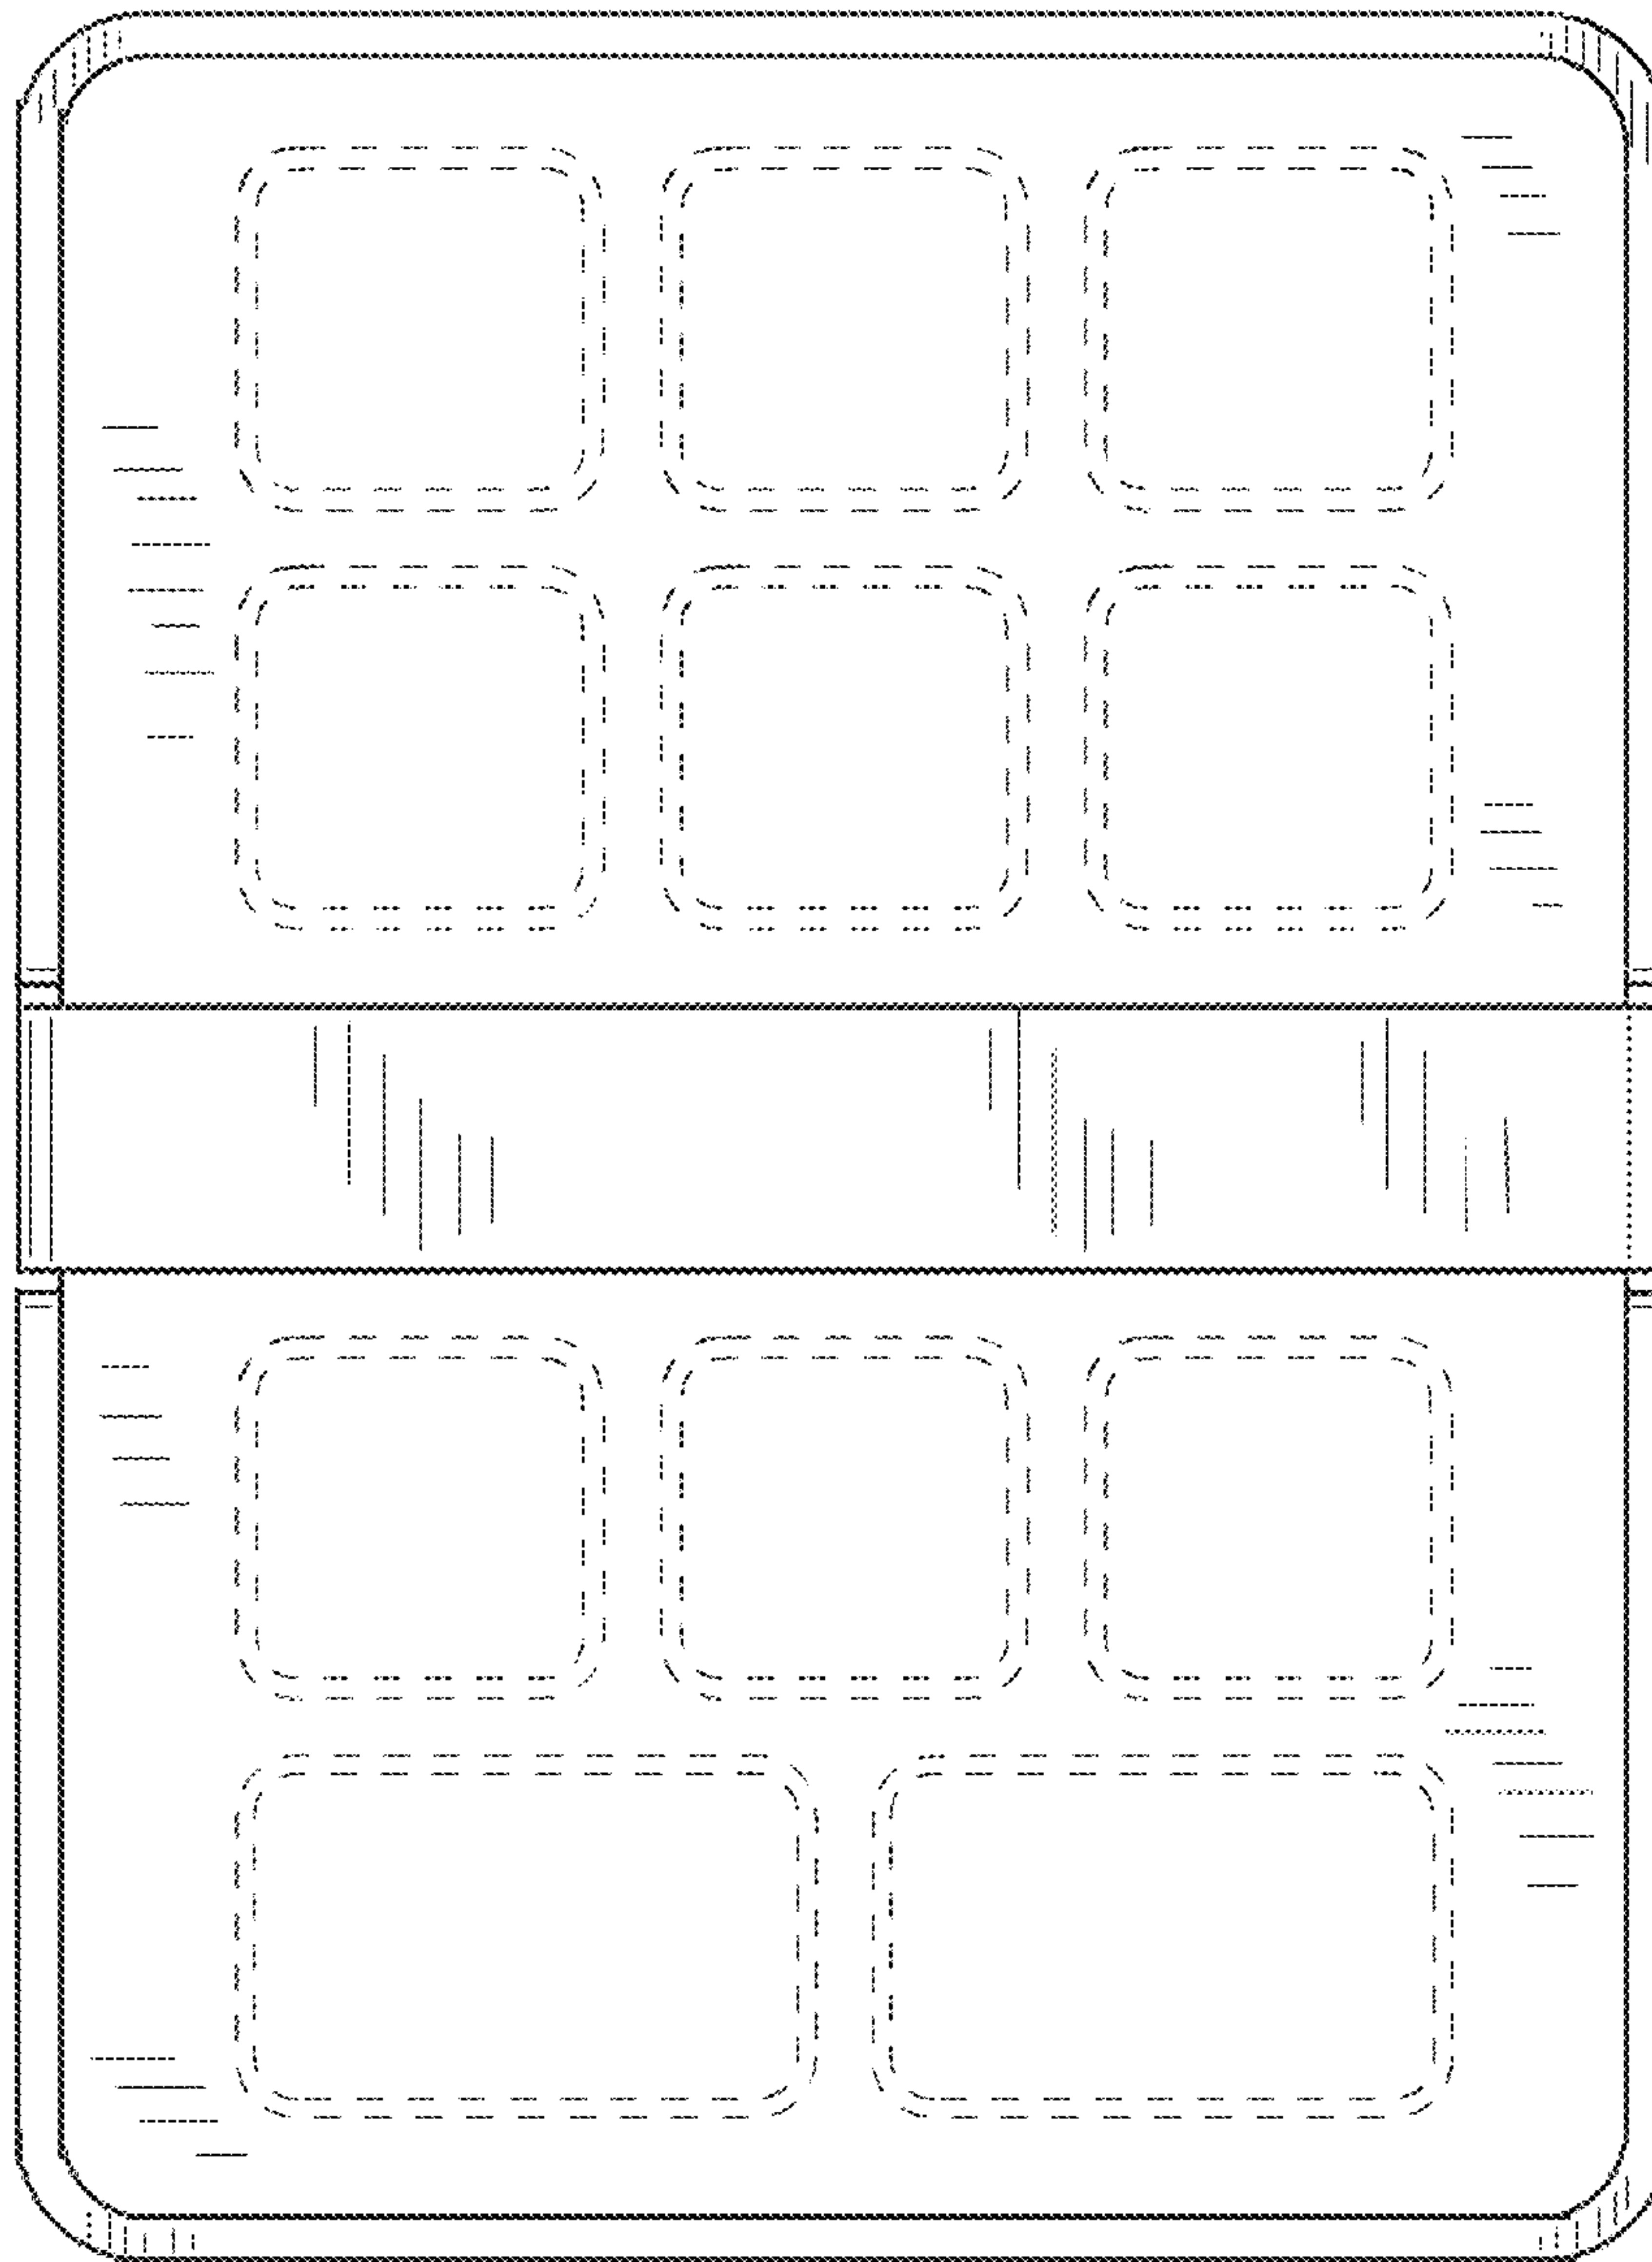


FIG.6

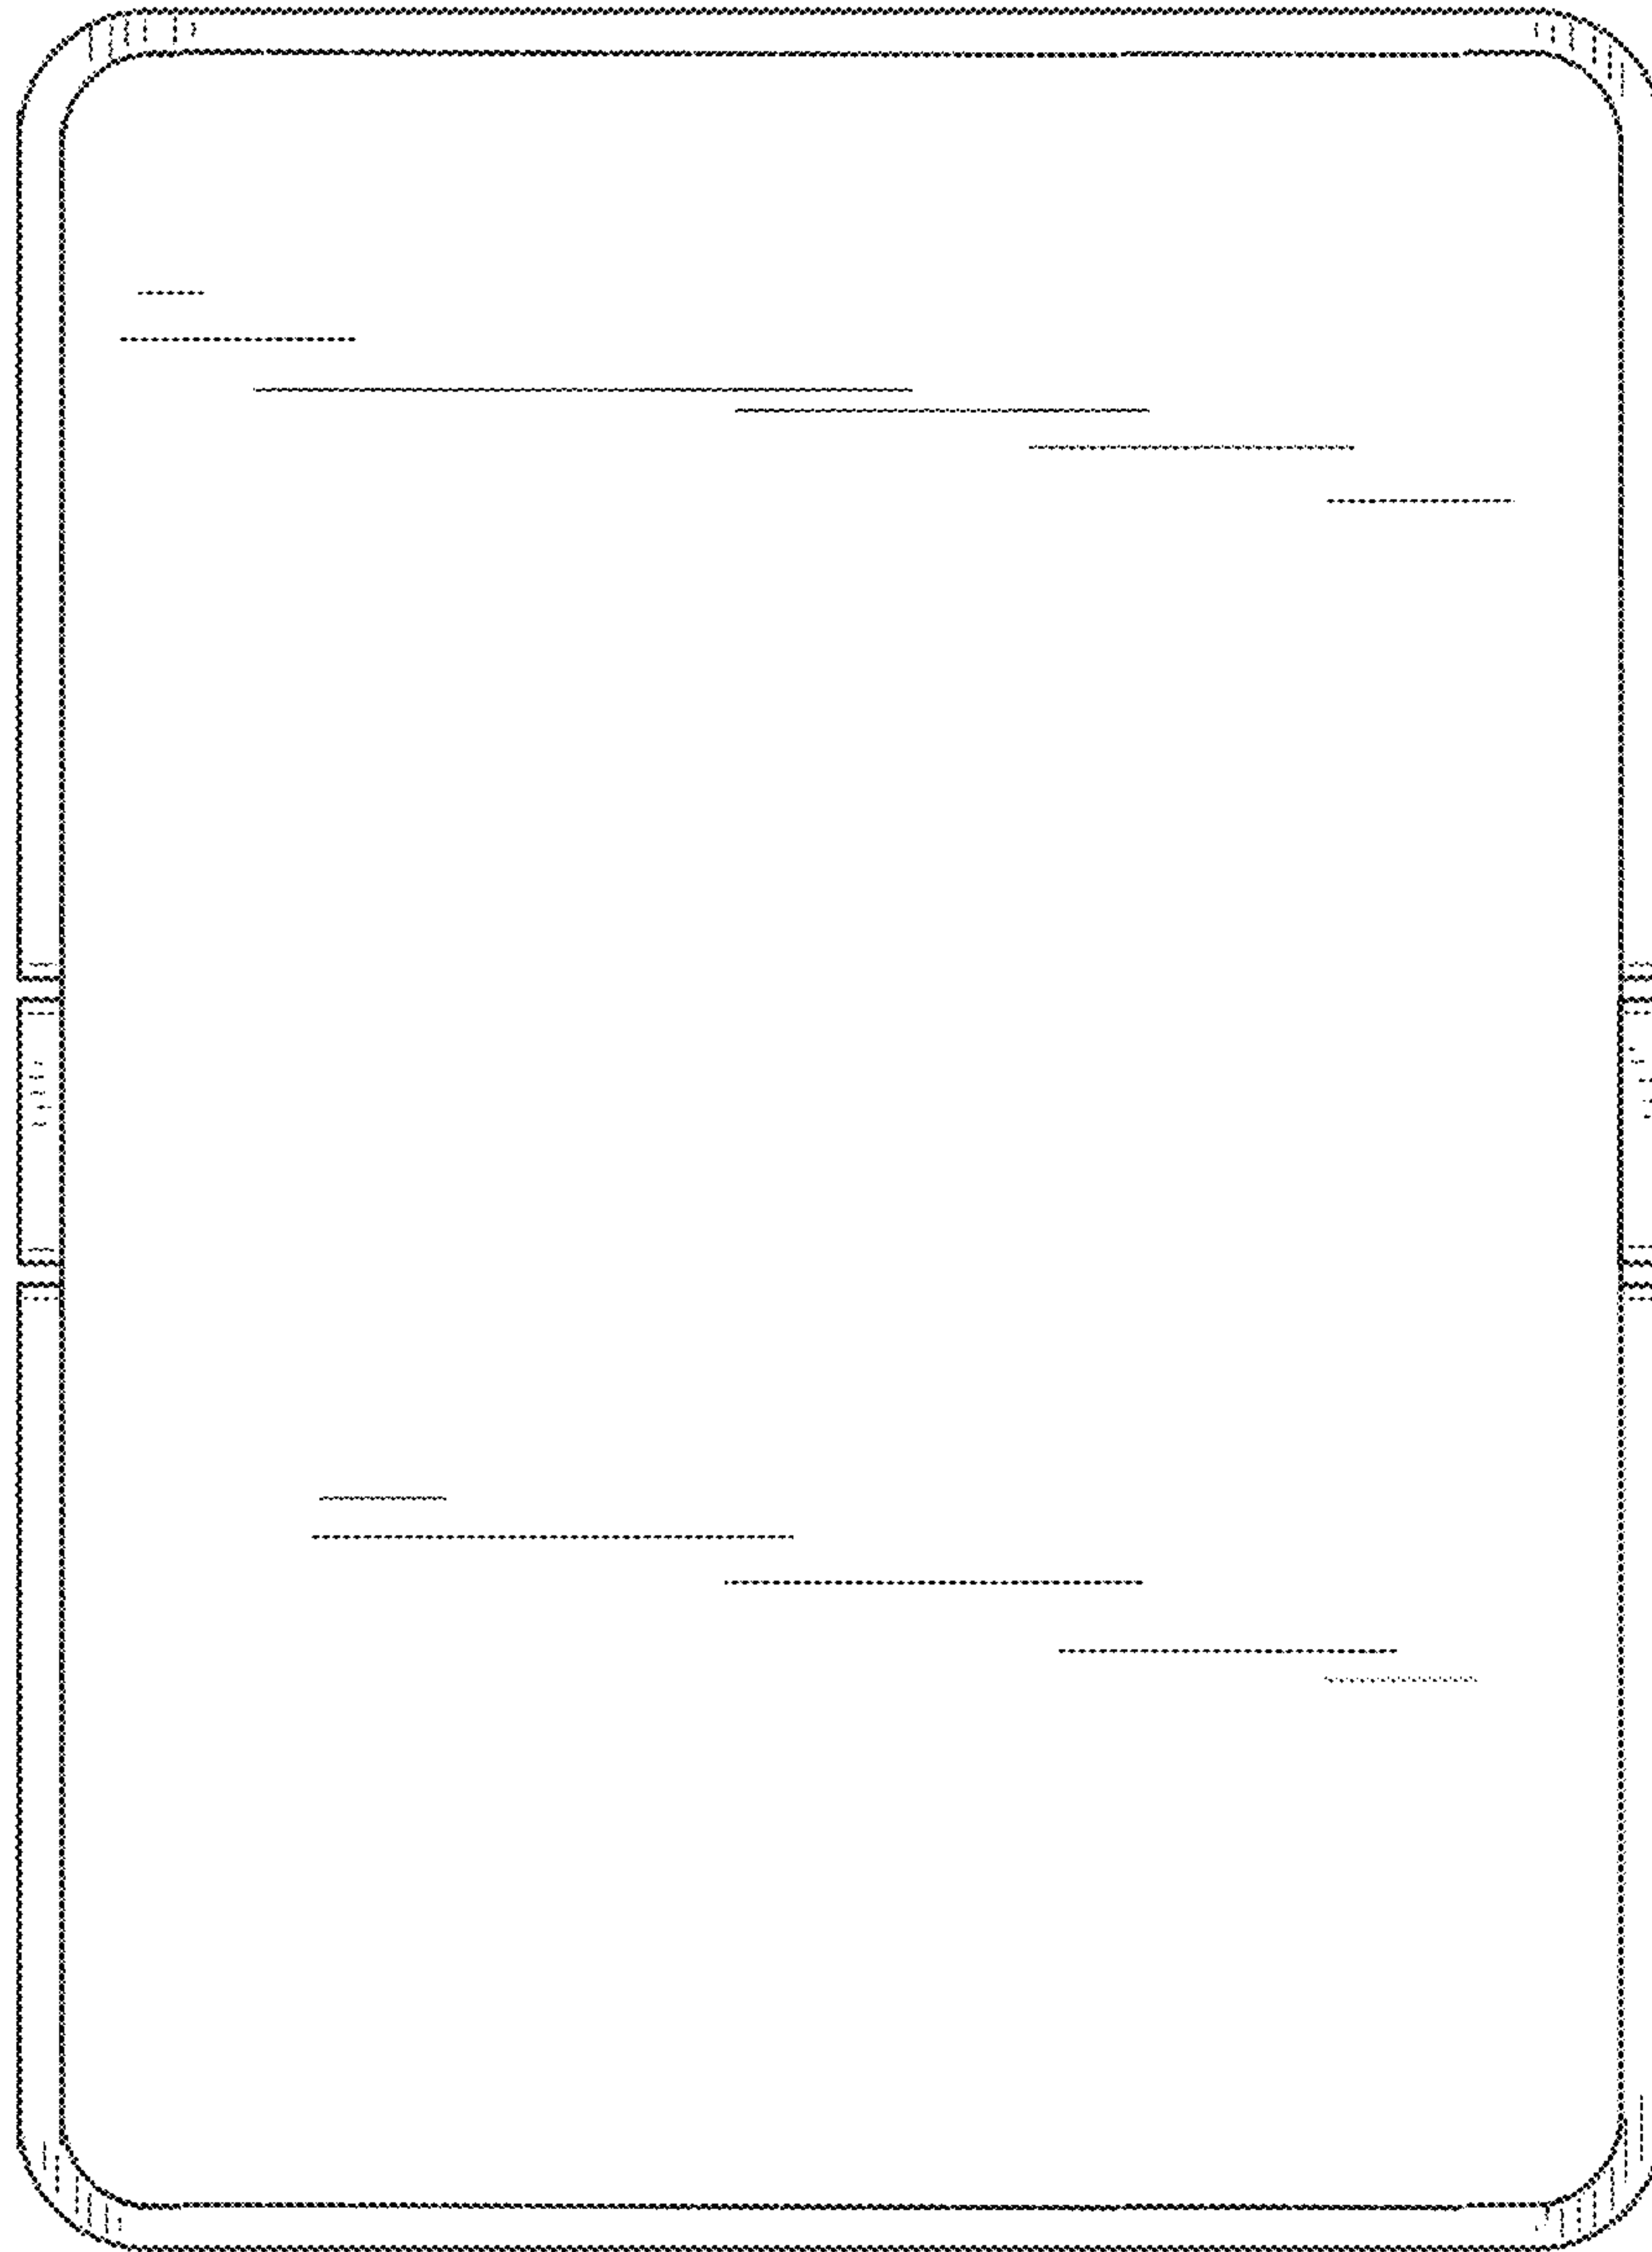


FIG. 7