



US00D867588S

(12) **United States Design Patent** (10) **Patent No.:** **US D867,588 S**
Rogge et al. (45) **Date of Patent:** **** Nov. 19, 2019**

(54) **CAP OF AN INJECTION DEVICE**
(71) Applicant: **Sanofi**, Paris (FR)
(72) Inventors: **Christian Rogge**, München (DE); **Philipp Oster**, München (DE); **Carolin Frontzek**, München (DE); **James Collins**, Bridgewater, NJ (US); **Alex Zuyev**, Frankfurt am Main (DE); **Kai Scheinert**, Frankfurt am Main (DE); **Uwe Dasbach**, Frankfurt am Main (DE)
(73) Assignee: **Sanofi**, Paris (FR)
(**) Term: **15 Years**
(21) Appl. No.: **29/648,584**
(22) Filed: **May 22, 2018**
(51) **LOC (12) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/130**
(58) **Field of Classification Search**
USPC D24/127–131, 112–114, 133, 186;
606/181, 185; 604/264, 272, 115, 232,
604/187, 158, 164.08, 192, 263, 163, 181,
604/184, 198, 227; 600/101, 139, 143;
128/200.24, 207.14, 207.15;
D19/115–123, 177, 193
CPC A61M 5/3156; A61M 5/31591; A61M
5/3155; A61M 5/3157; A61M 5/24;
A61M 5/31501; A61M 5/31551; A61M
5/31585; A61M 2005/2407; A61M
2005/2492; A61M 2205/581; A61M
2205/582
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS
D302,206 S * 7/1989 McAlister D24/130
D347,894 S * 6/1994 Hansen D24/114

D430,293 S * 8/2000 Jansen D24/129
D496,101 S * 9/2004 Davison D24/112
D568,469 S * 5/2008 Sudo D24/130
D616,984 S * 6/2010 Gilboa D24/129
D777,912 S * 1/2017 Wohlfahrt D24/130
D779,057 S * 2/2017 Wohlfahrt D24/130
D783,816 S * 4/2017 Wohlfahrt D24/130
D787,052 S * 5/2017 Heinz D24/130
D787,669 S * 5/2017 Huang D24/130
D789,528 S * 6/2017 Wohlfahrt D24/130
D794,781 S * 8/2017 Gilbert D24/129
9,844,629 B2 * 12/2017 Cronenberg A61M 5/50
D822,198 S * 7/2018 Stonecipher D24/113
D831,198 S * 10/2018 Ross D24/127
D834,187 S * 11/2018 Ryan A61M 39/20
D24/130
2004/0054336 A1 * 3/2004 Klint A61M 5/347
604/272
2004/0097882 A1 * 5/2004 DiBiasi A61J 1/2096
604/199


(Continued)

Primary Examiner — David G Muller
Assistant Examiner — Nathan M Johnston
(74) *Attorney, Agent, or Firm* — Fish & Richardson P.C.

(57) **CLAIM**
The ornamental design for a cap of an injection device, substantially as shown and described.

DESCRIPTION
FIG. 1 is a perspective view of an cap of an injection device showing our new design;
FIG. 2 is a front elevation view thereof;
FIG. 3 is a rear elevation view thereof;
FIG. 4 is a first side elevation view thereof;
FIG. 5 is a second side elevation view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The broken lines illustrate boundaries that form no part of the claimed design.

1 Claim, 4 Drawing Sheets

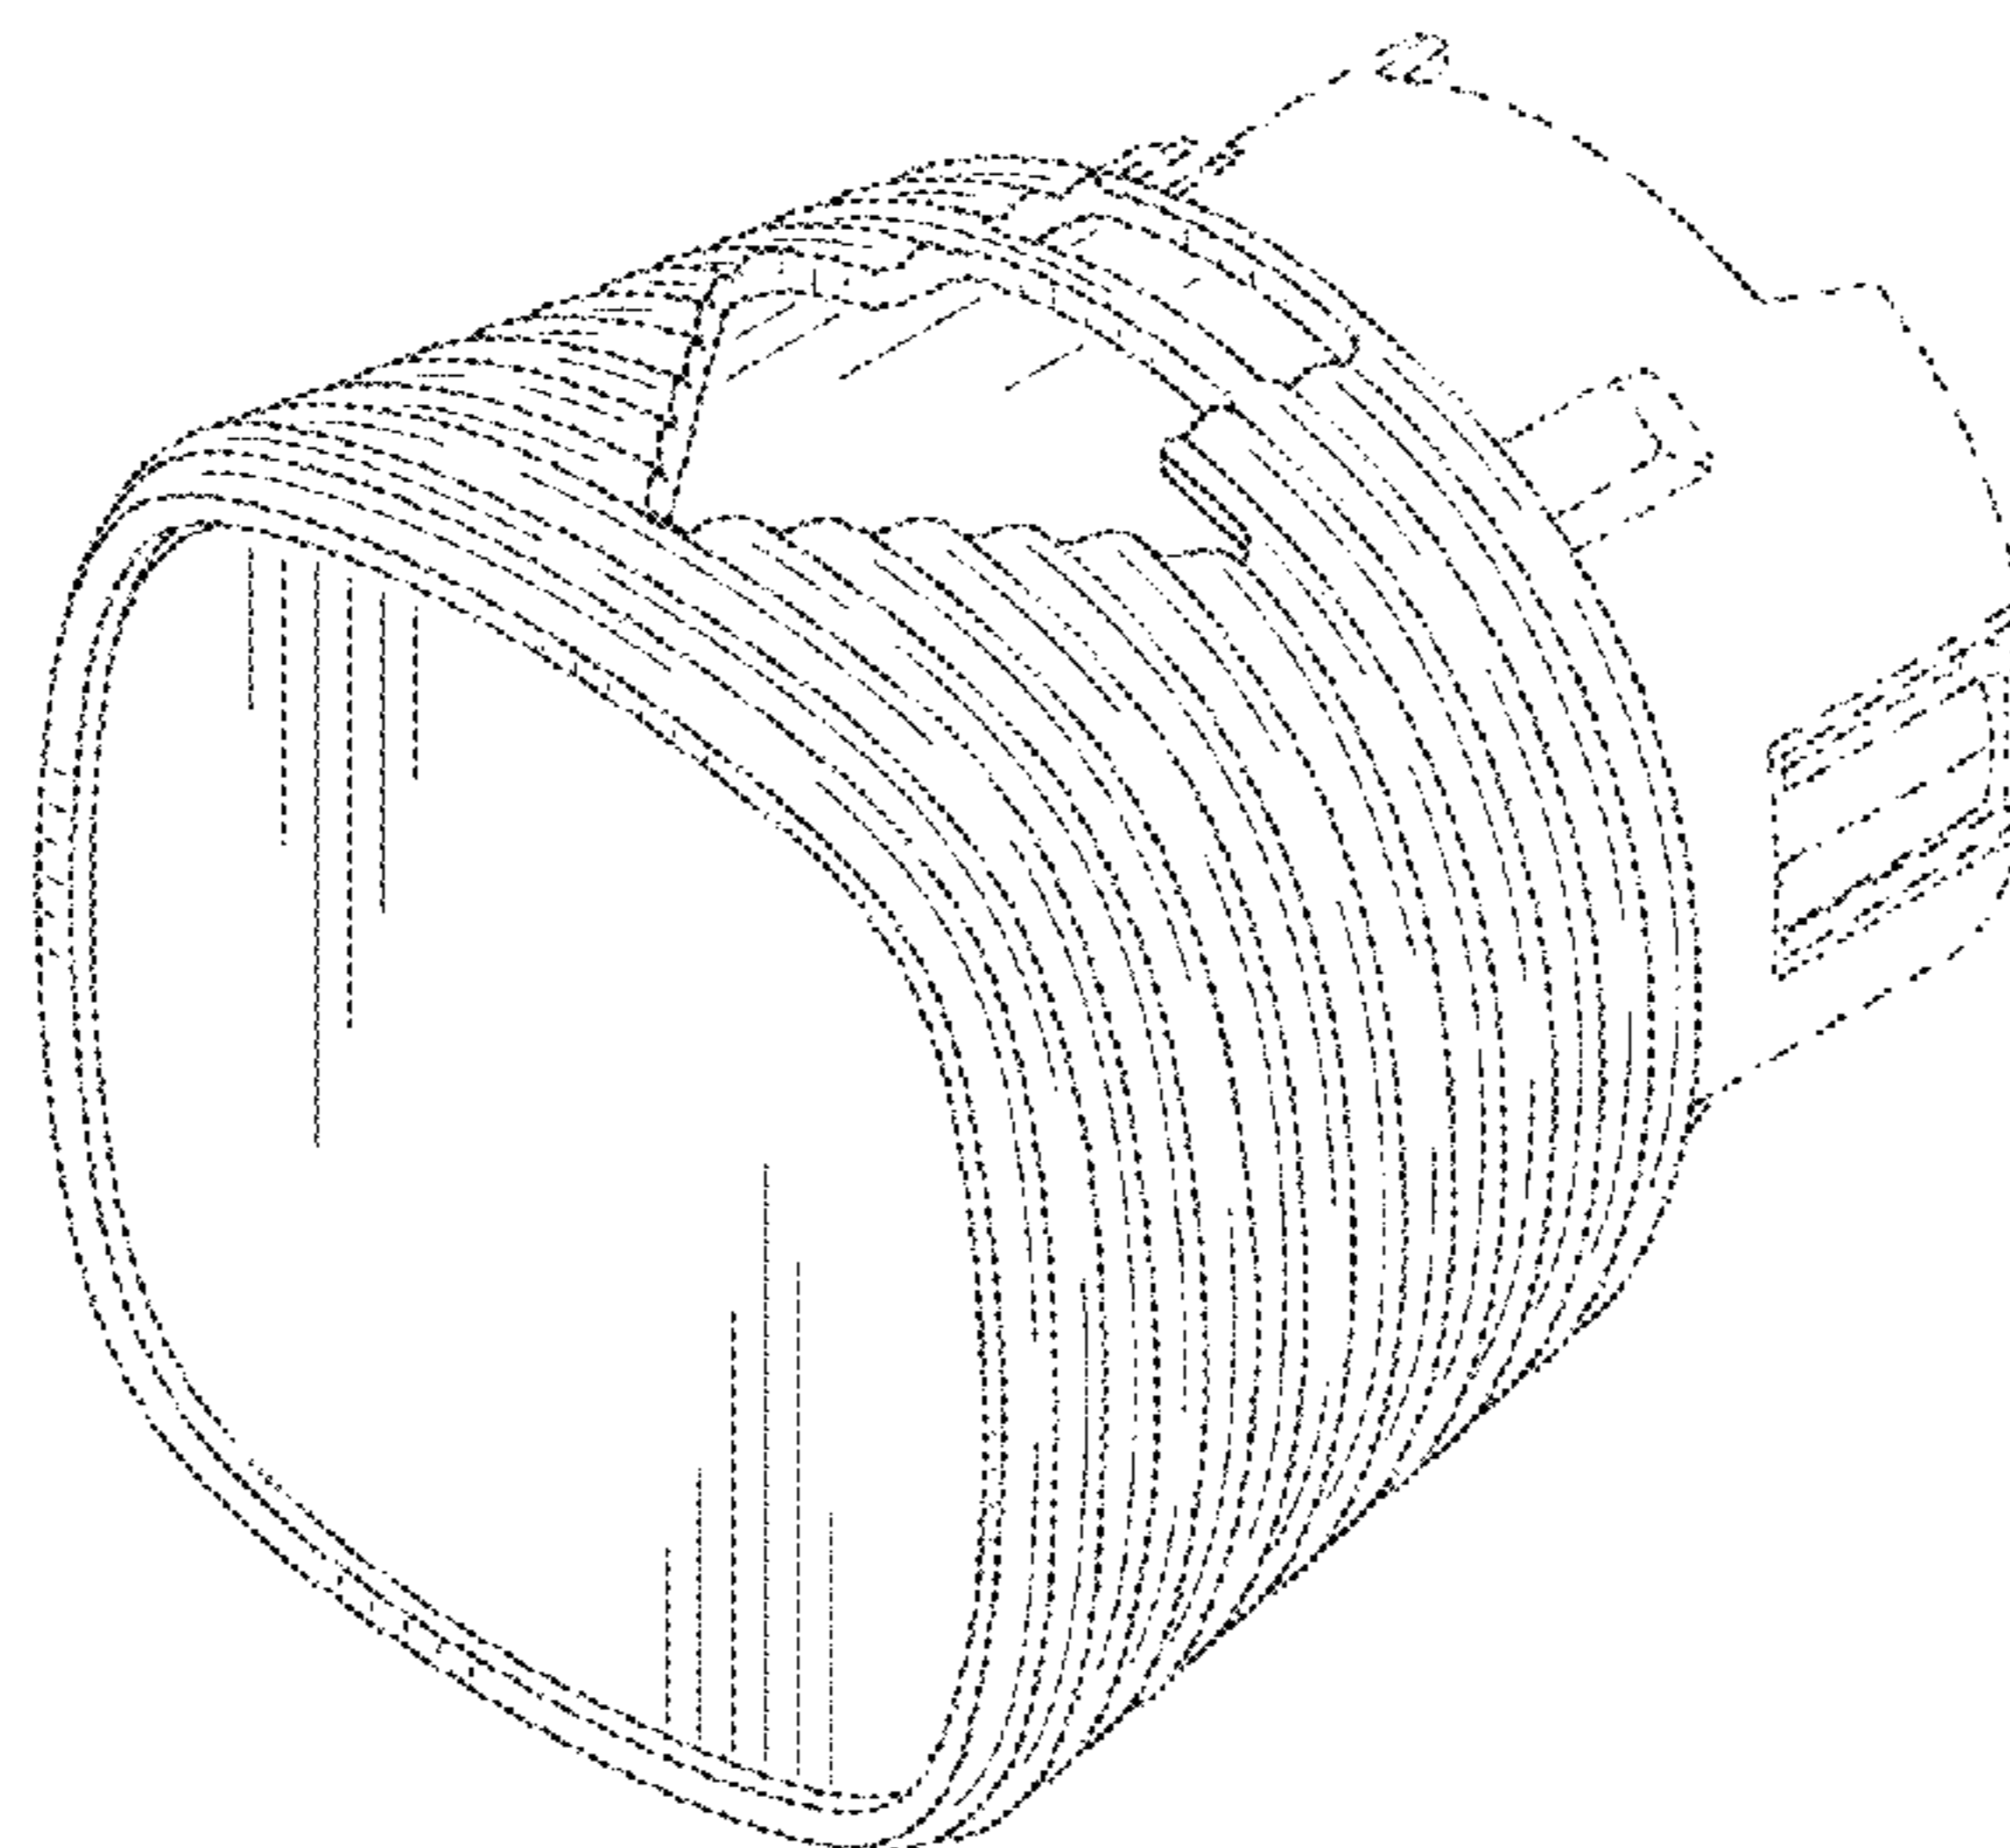

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0015578 A1* 1/2011 Lowke A61M 5/5086
604/192
2013/0030381 A1* 1/2013 Langley A61M 5/24
604/224
2017/0361027 A1* 12/2017 Srinivasan A61M 5/347
2018/0250473 A1* 9/2018 Ganzitti A61M 5/31551
2018/0272075 A1* 9/2018 Stefanov A61M 5/20
2018/0311442 A1* 11/2018 Saussaye A61M 5/2033
2018/0318526 A1* 11/2018 Yang C07K 16/40

* cited by examiner

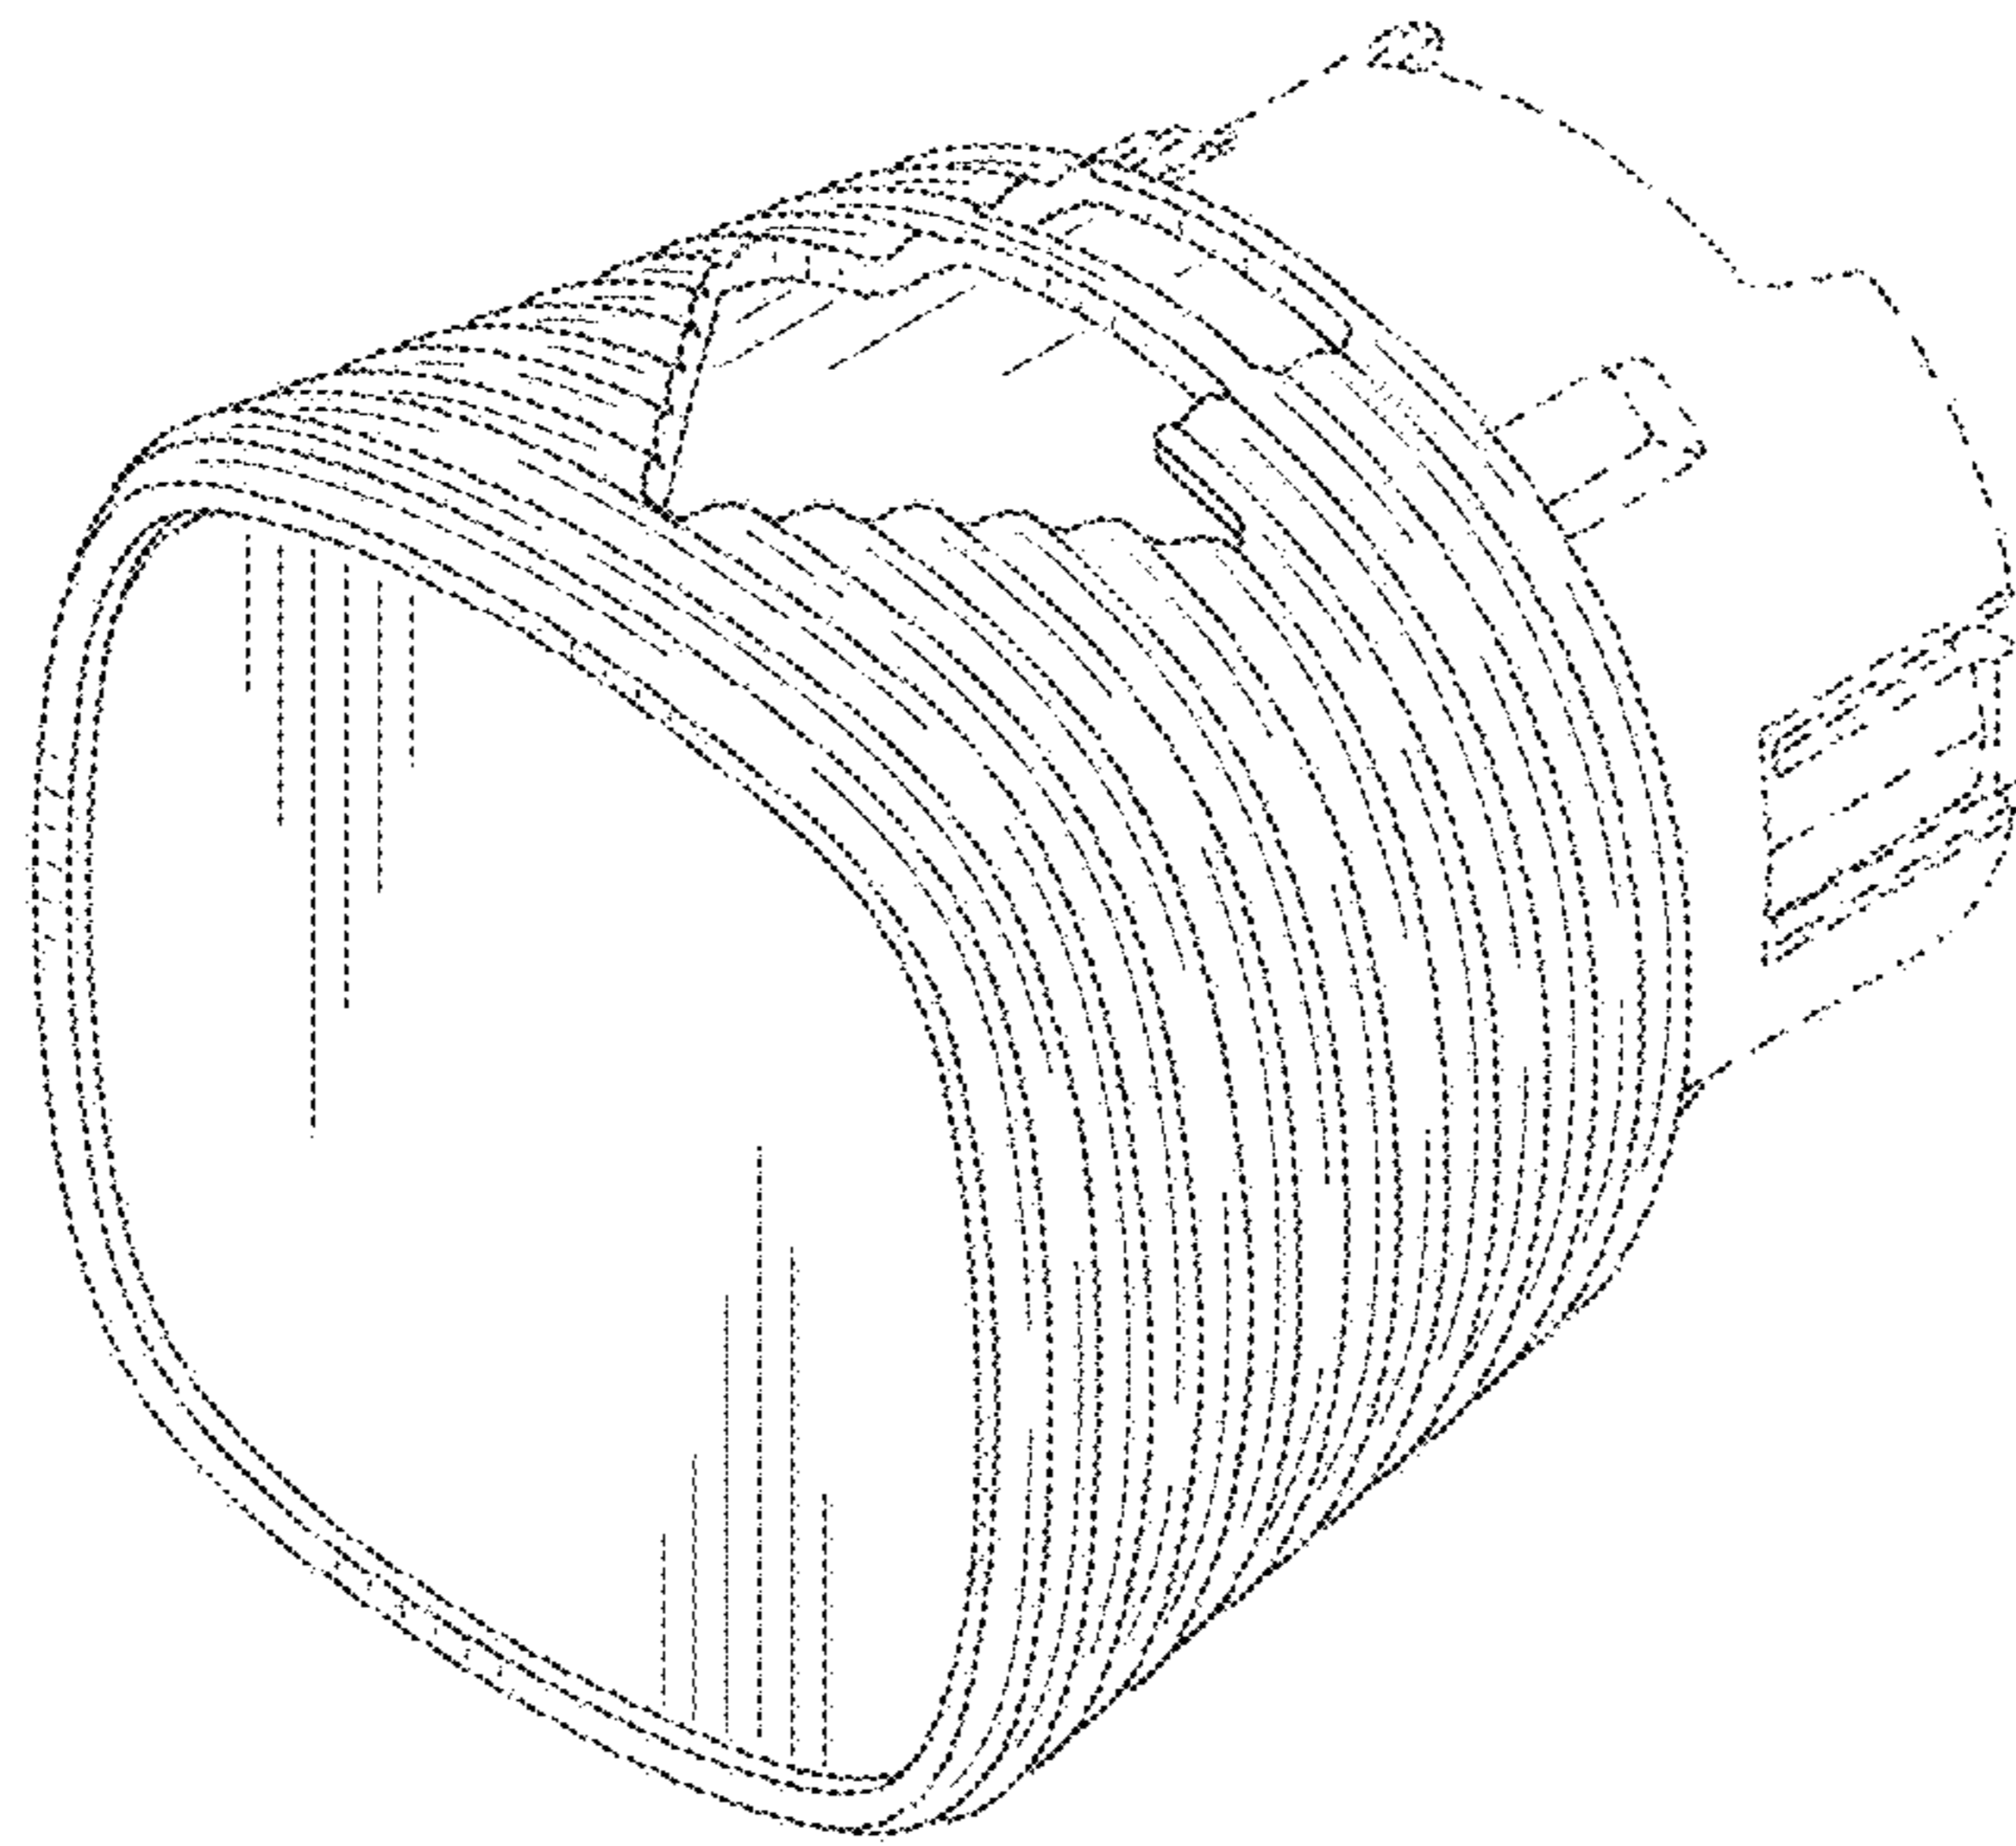


FIG. 1

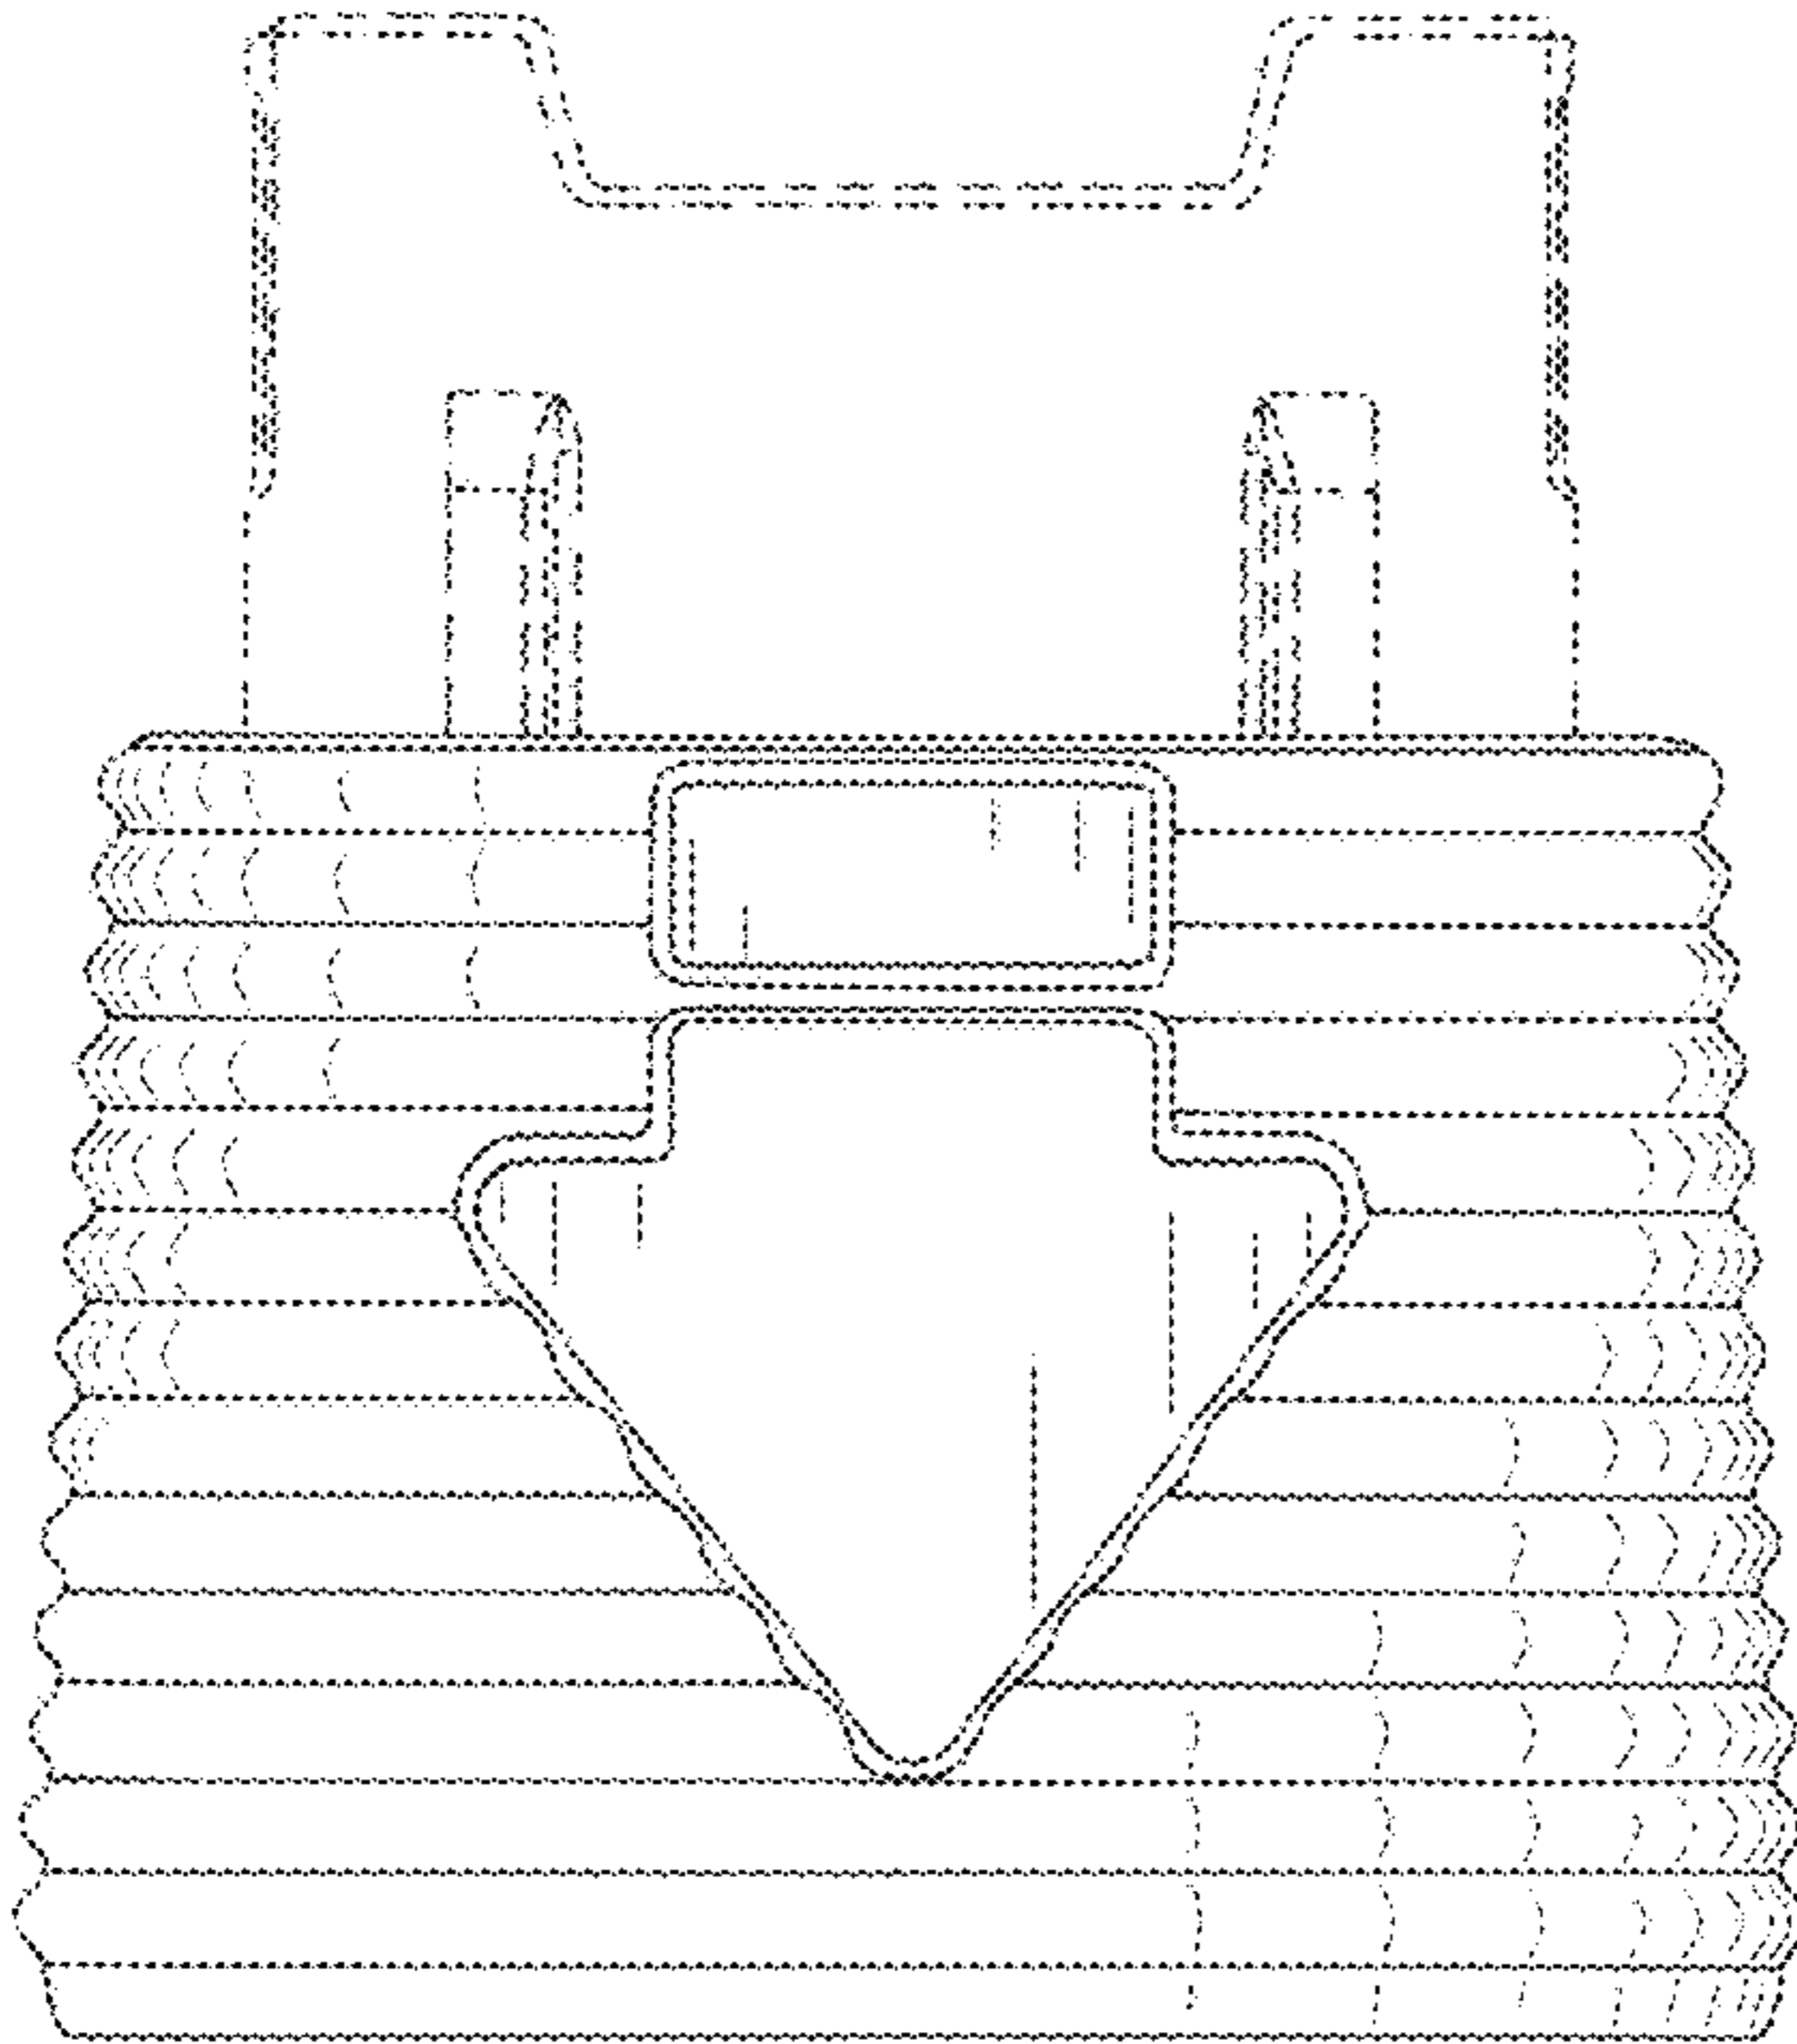


FIG. 2

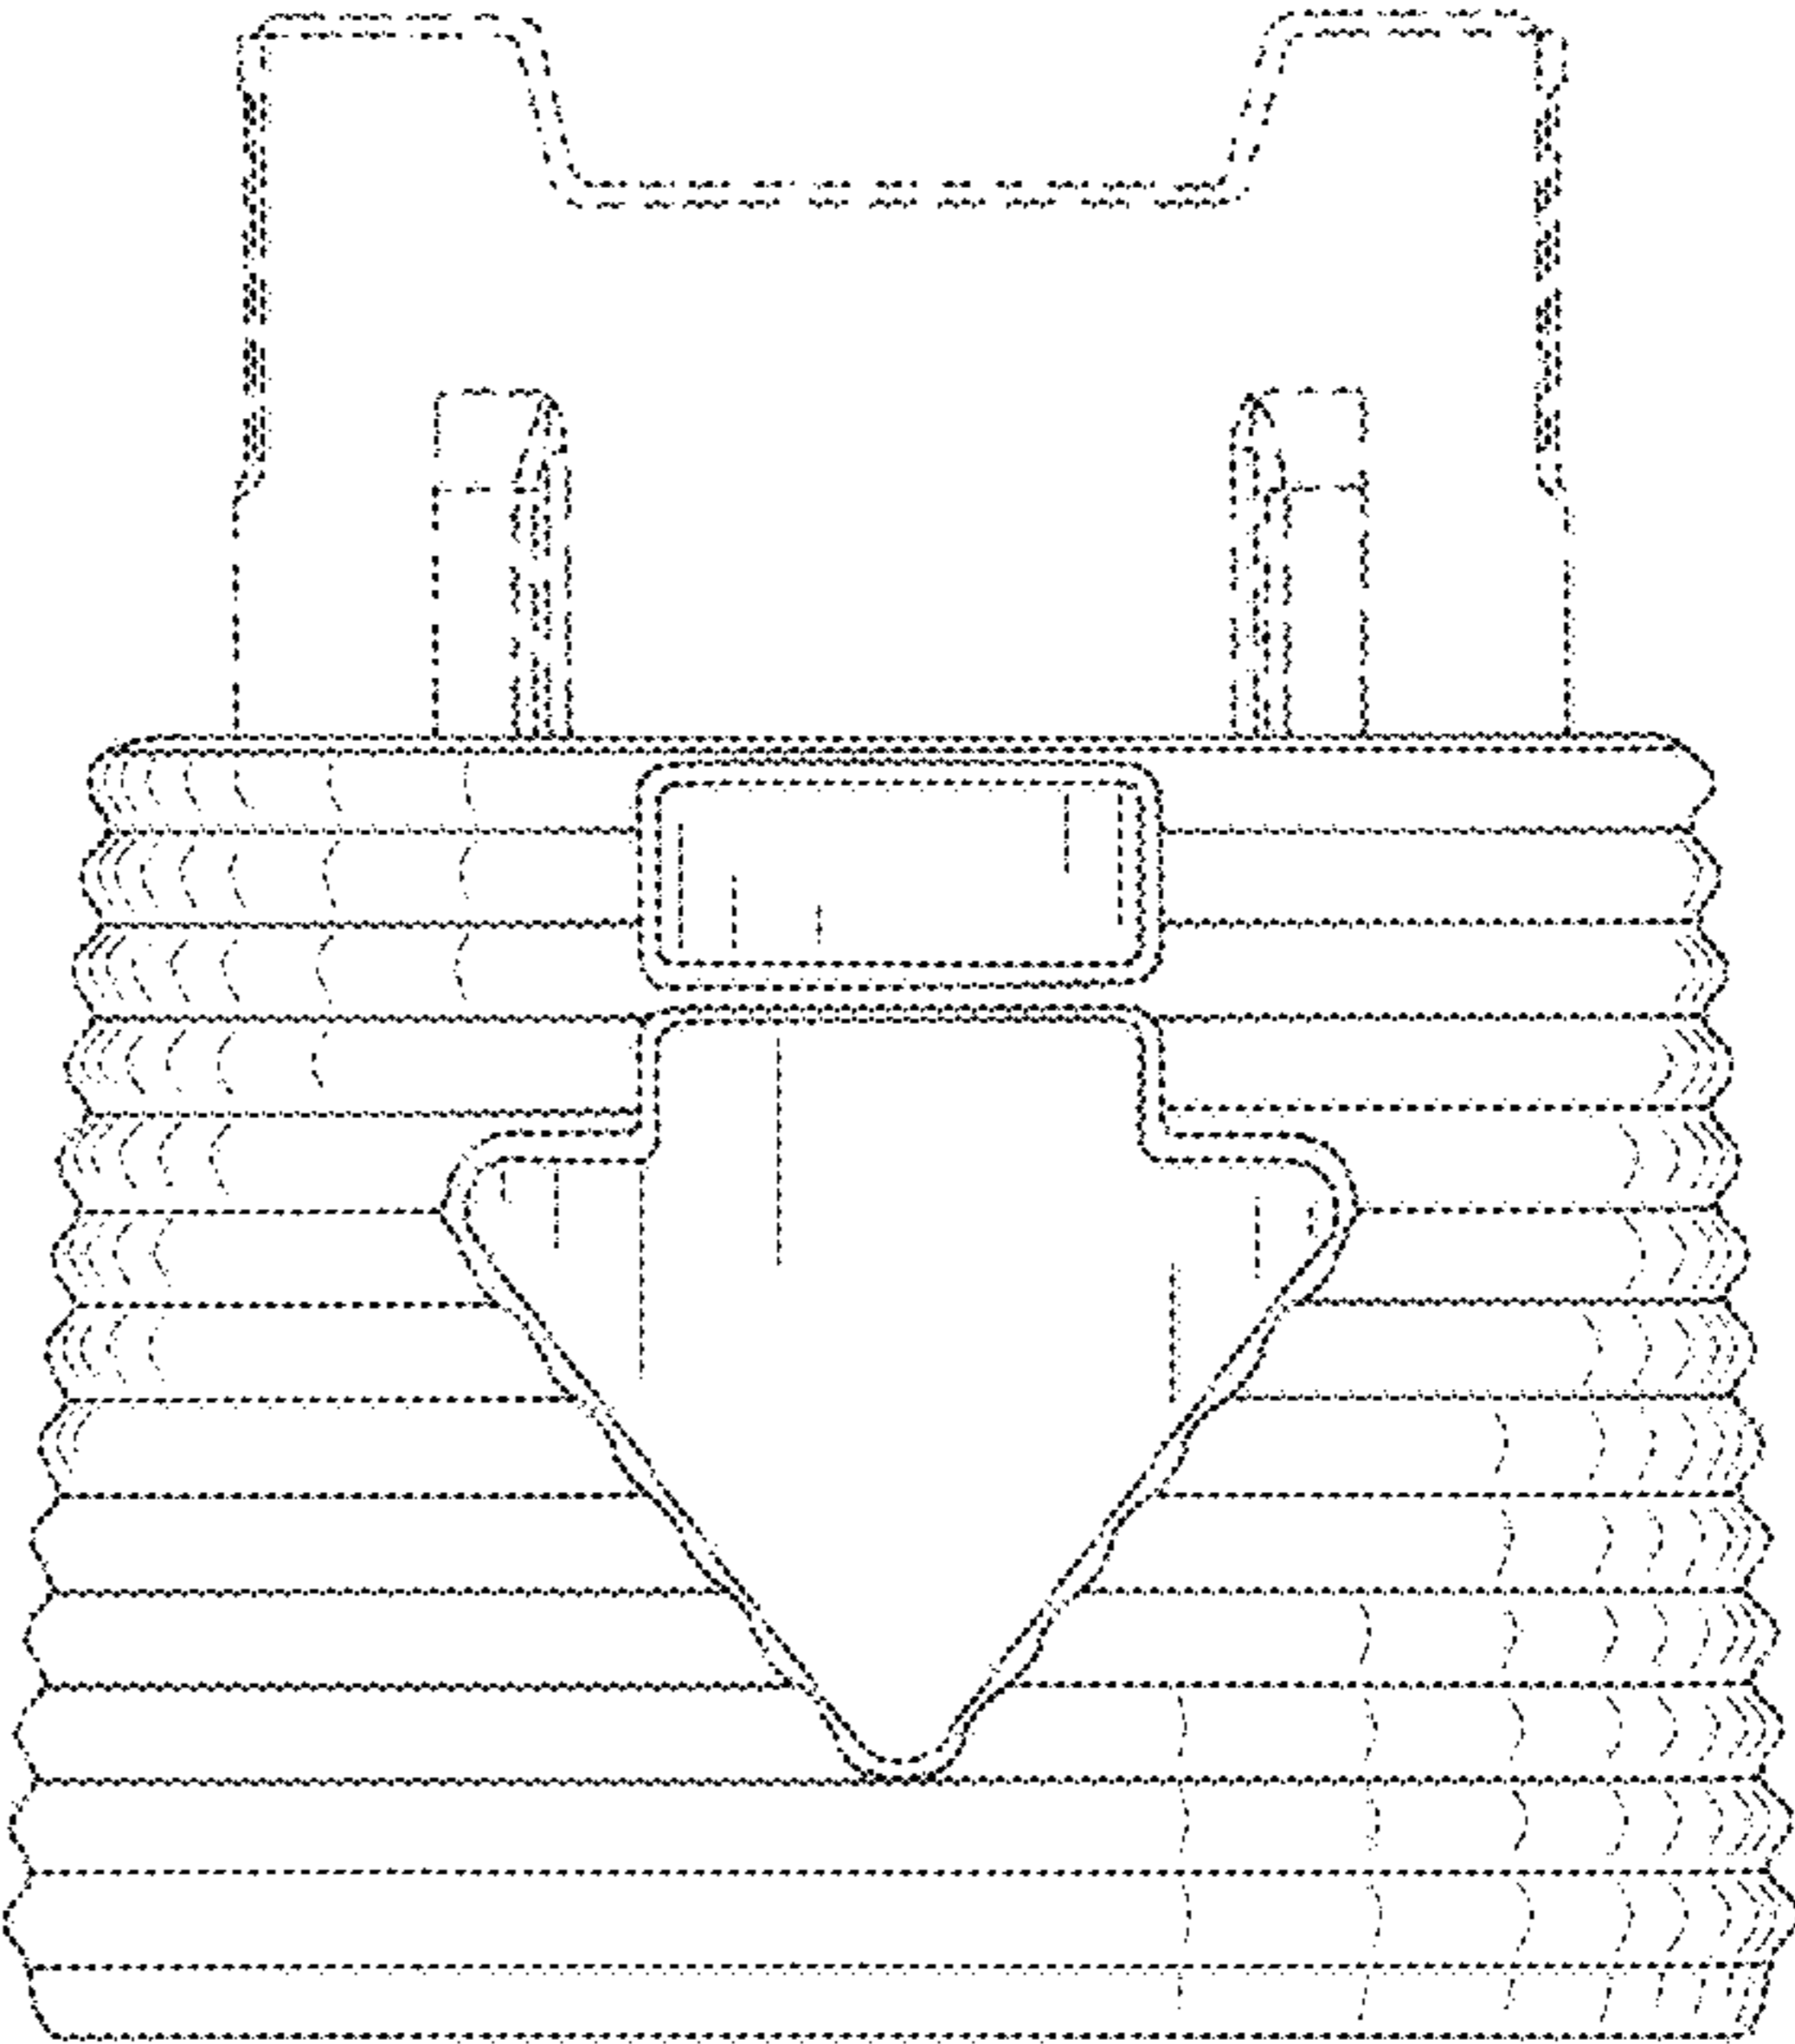


FIG. 3

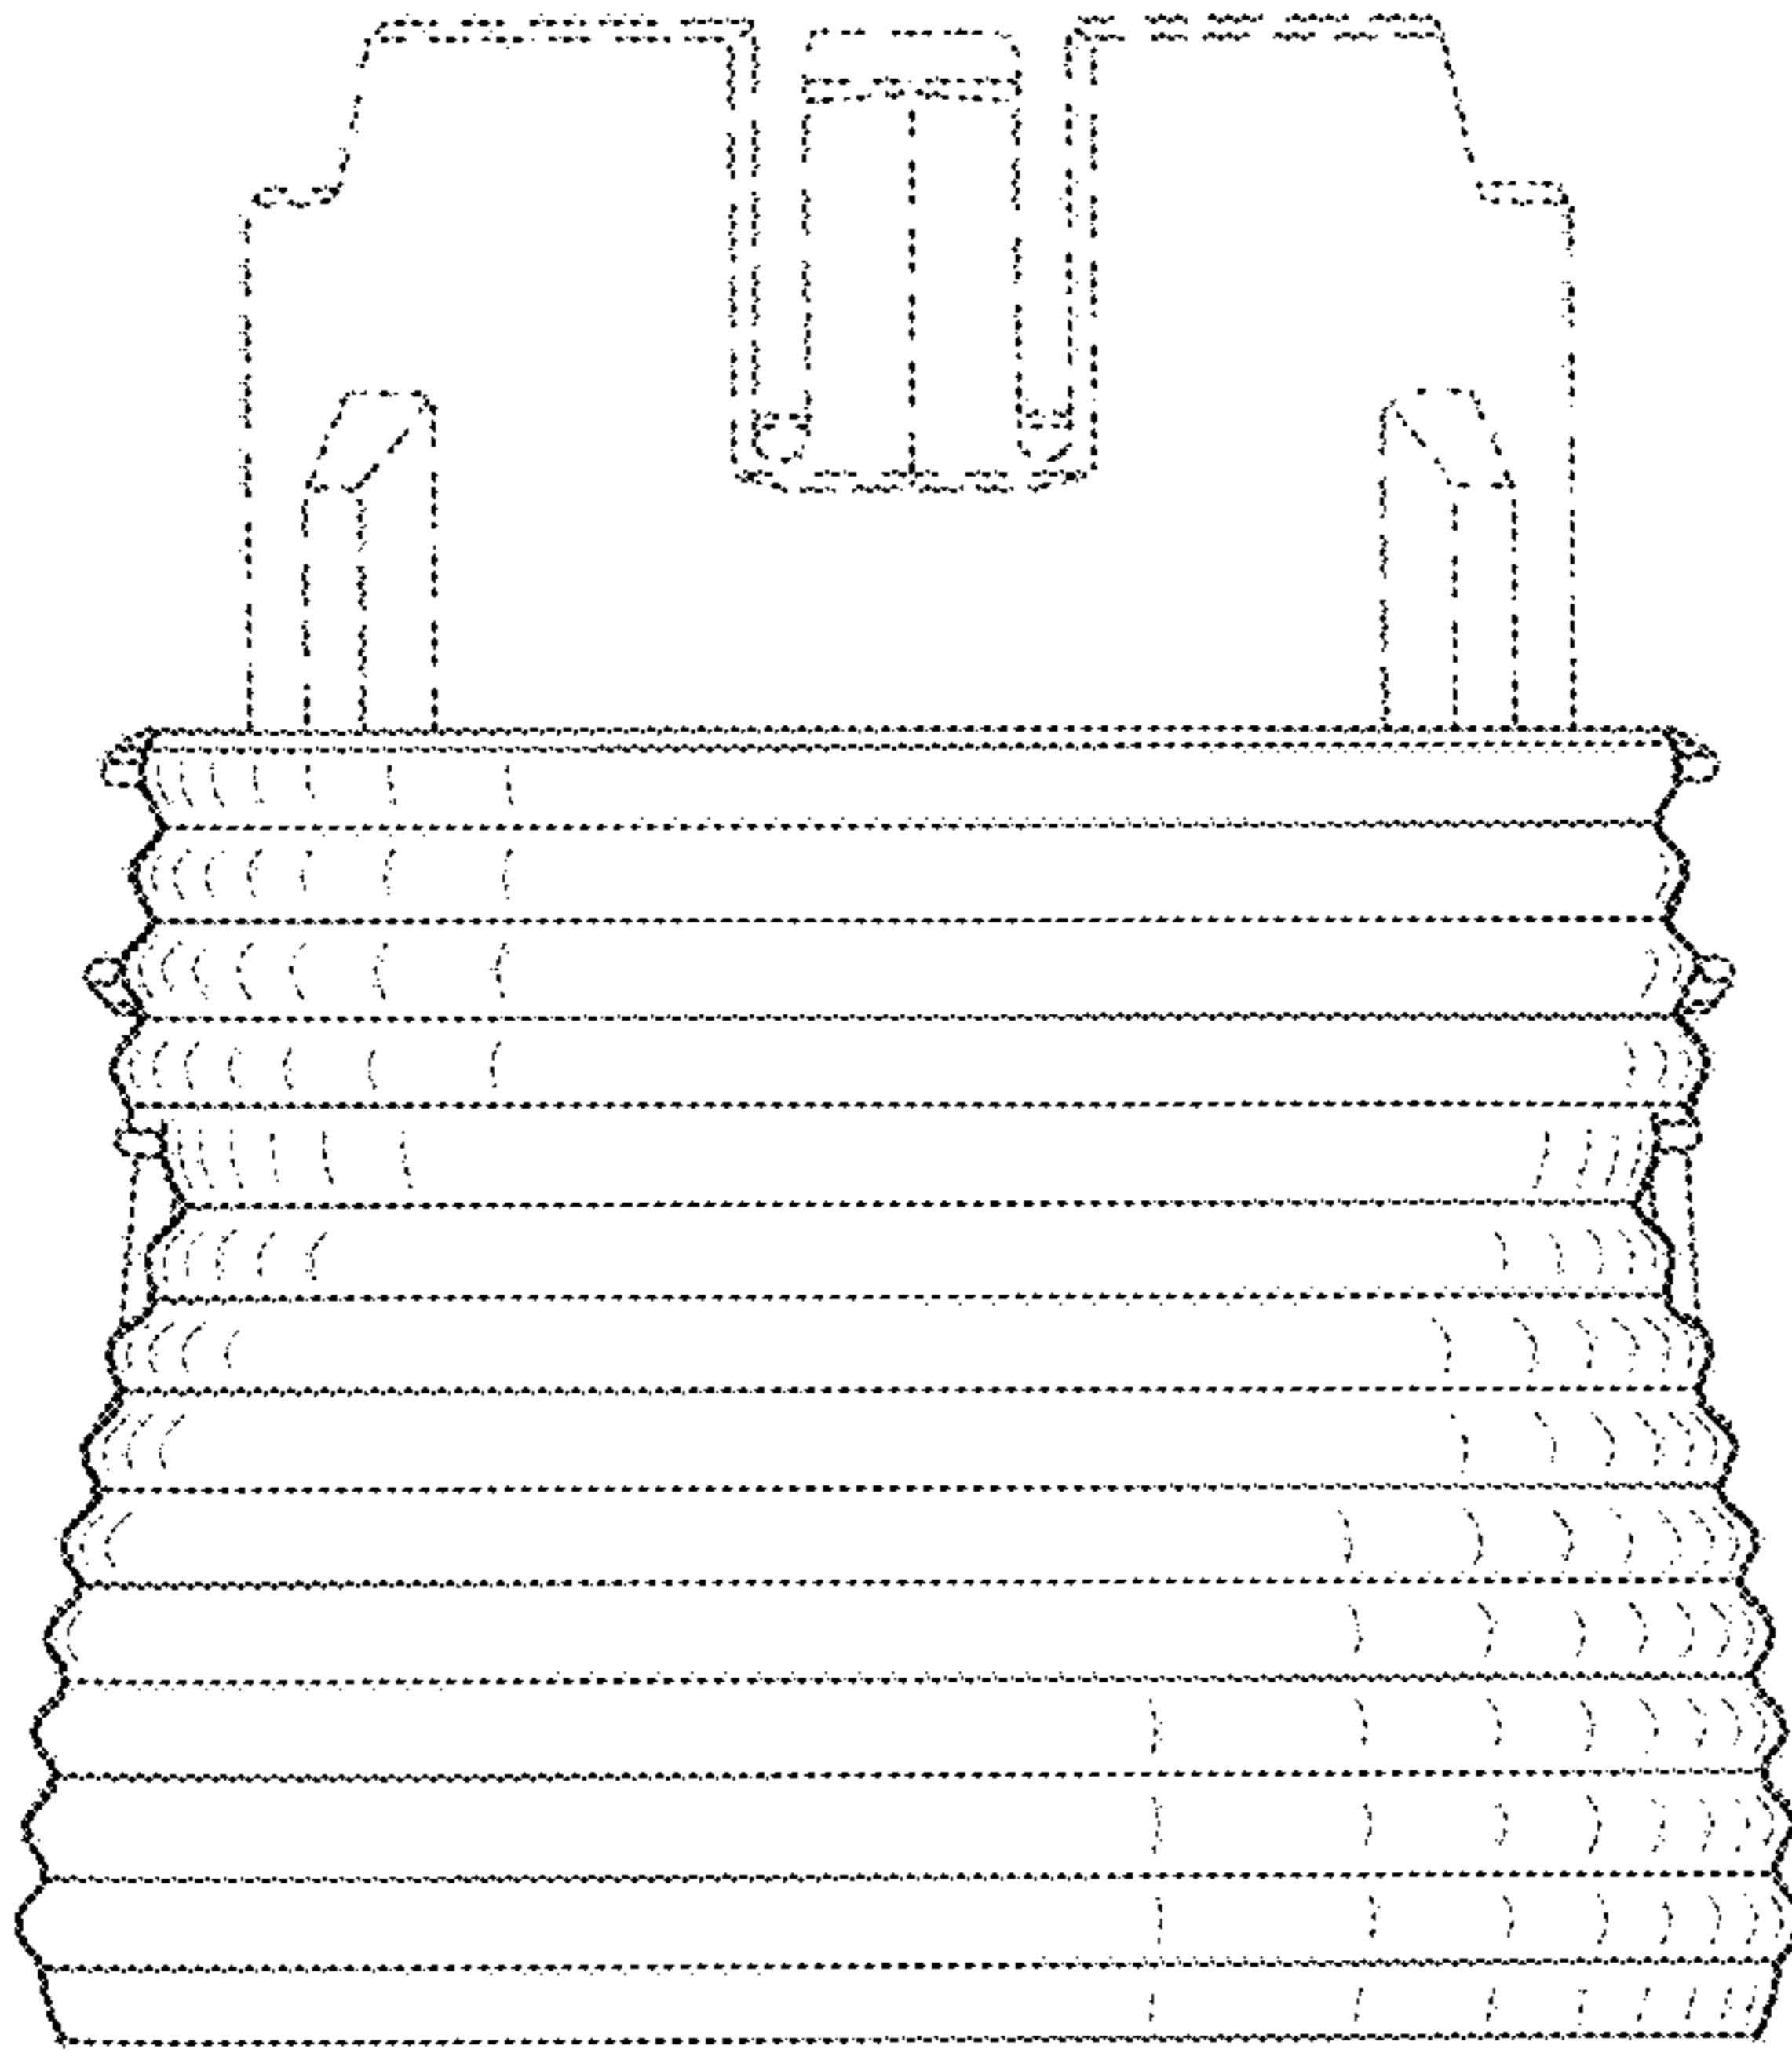


FIG. 4

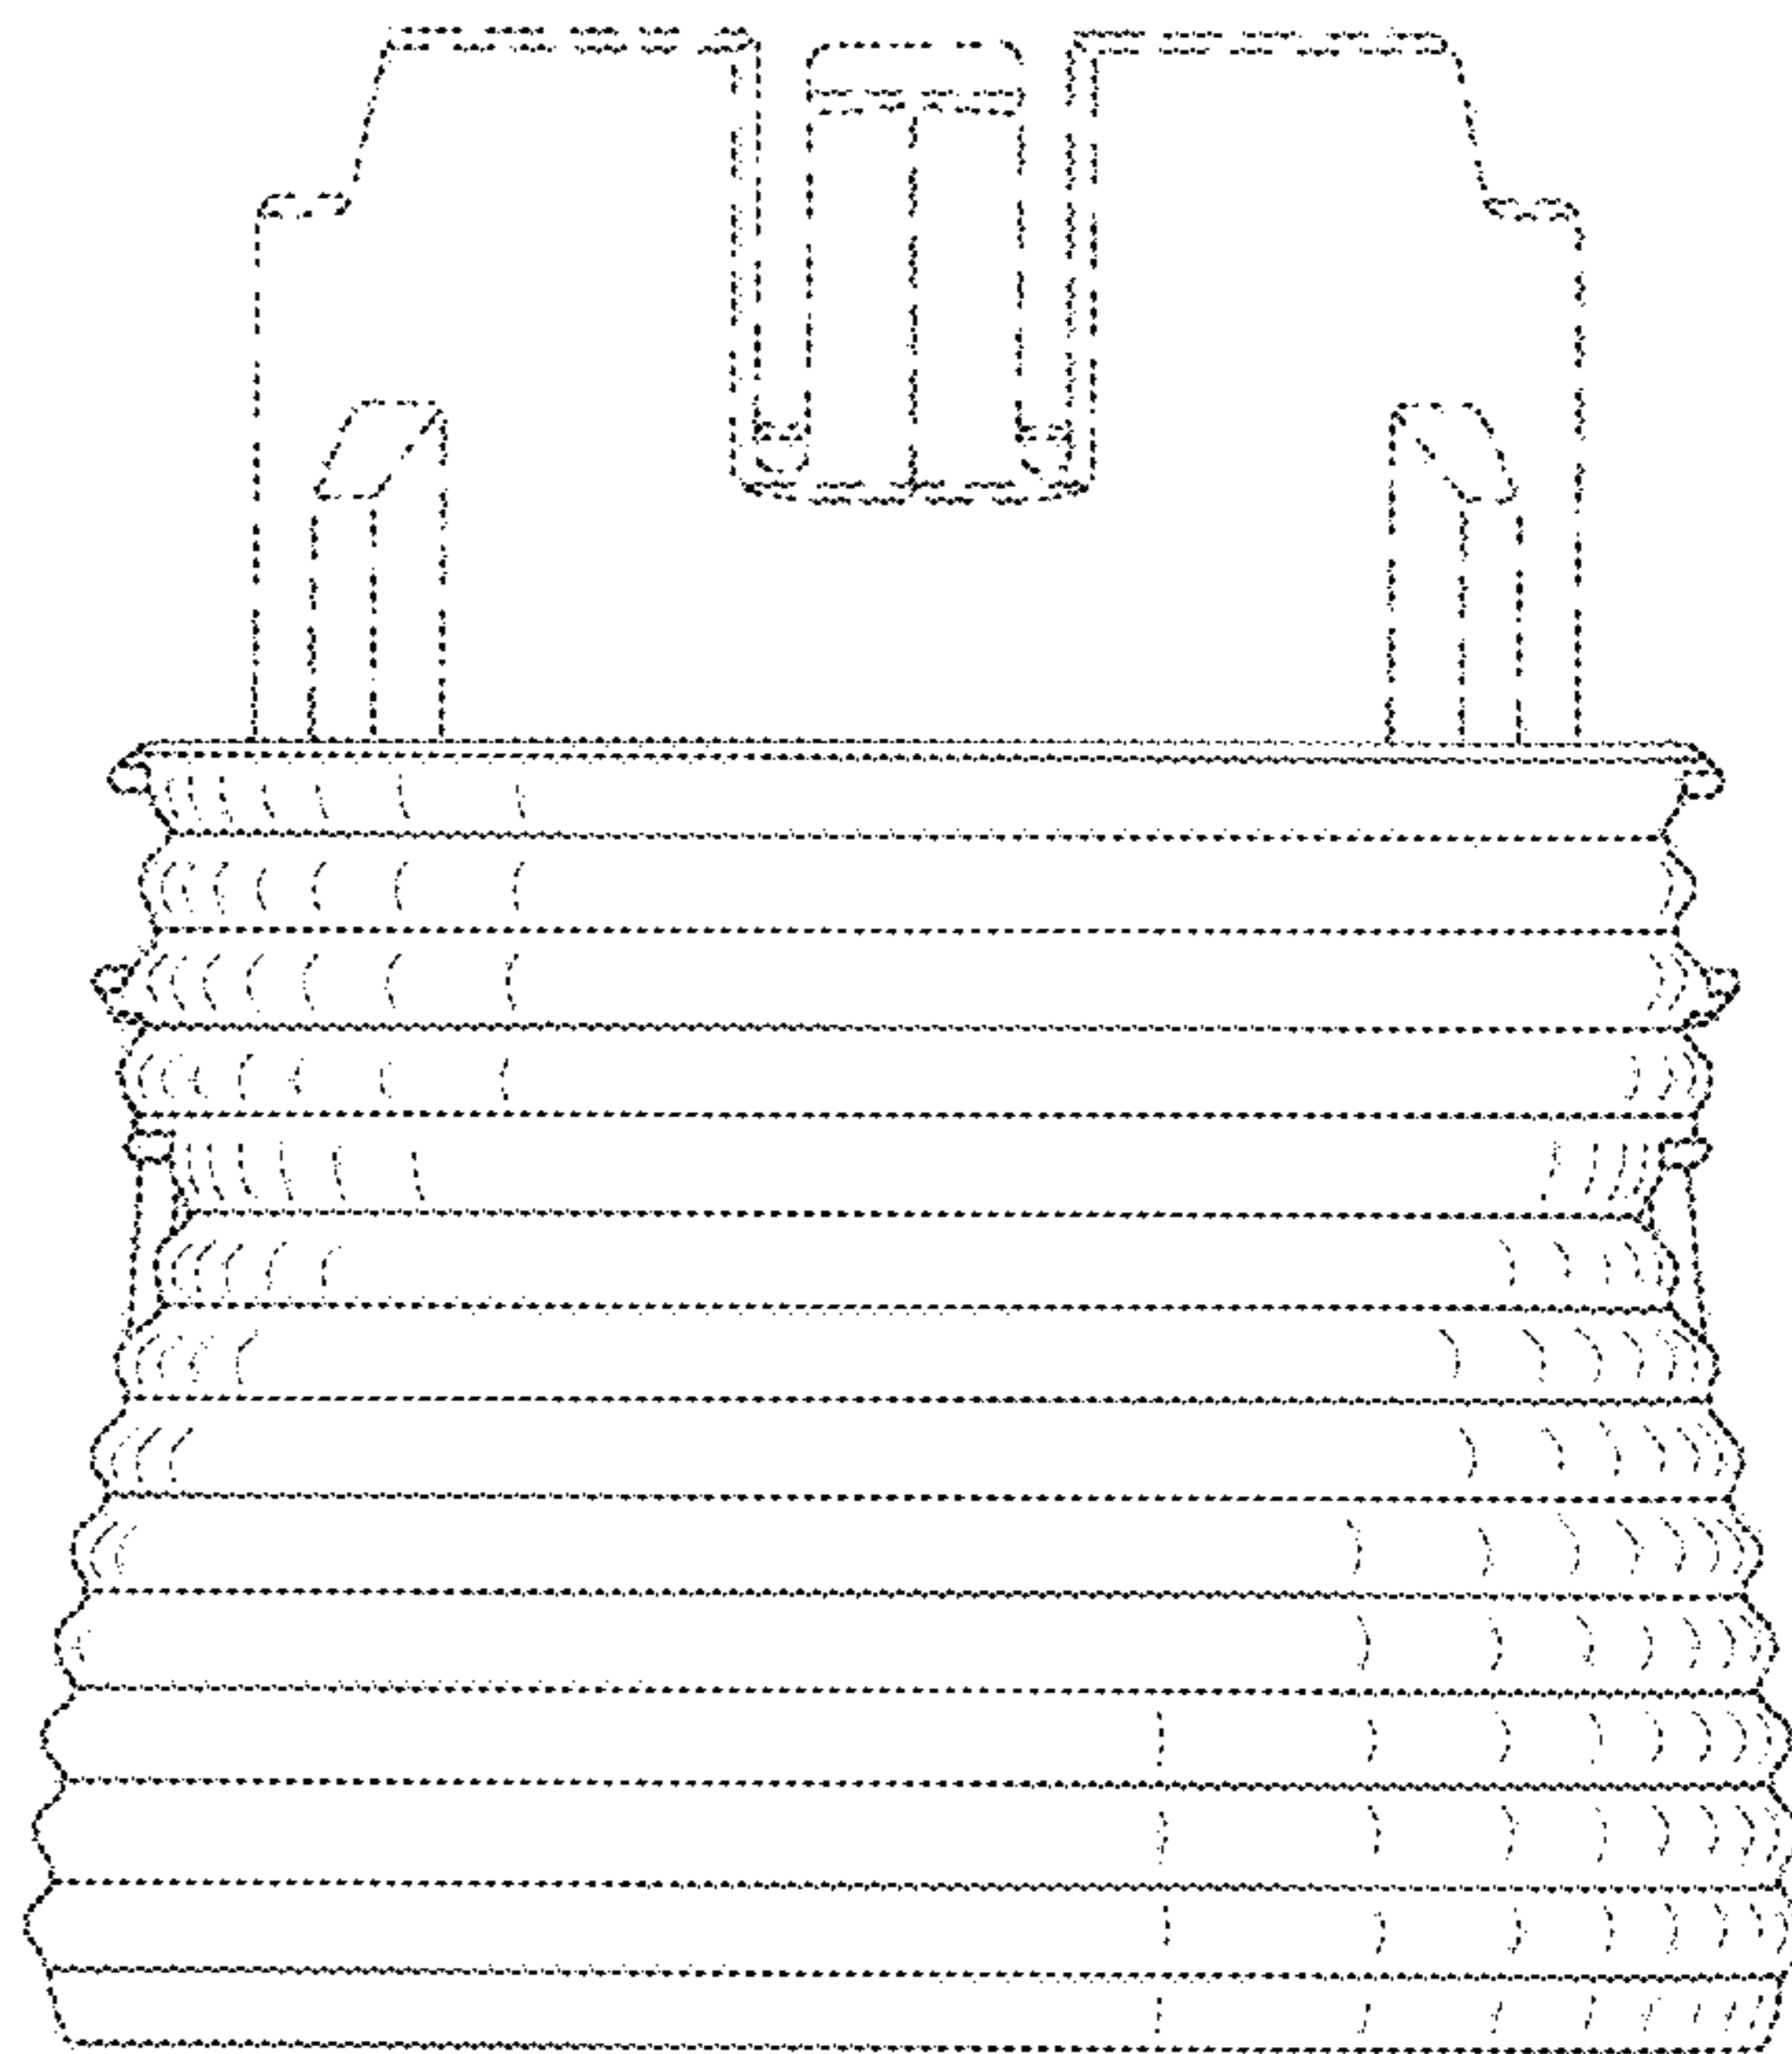


FIG. 5

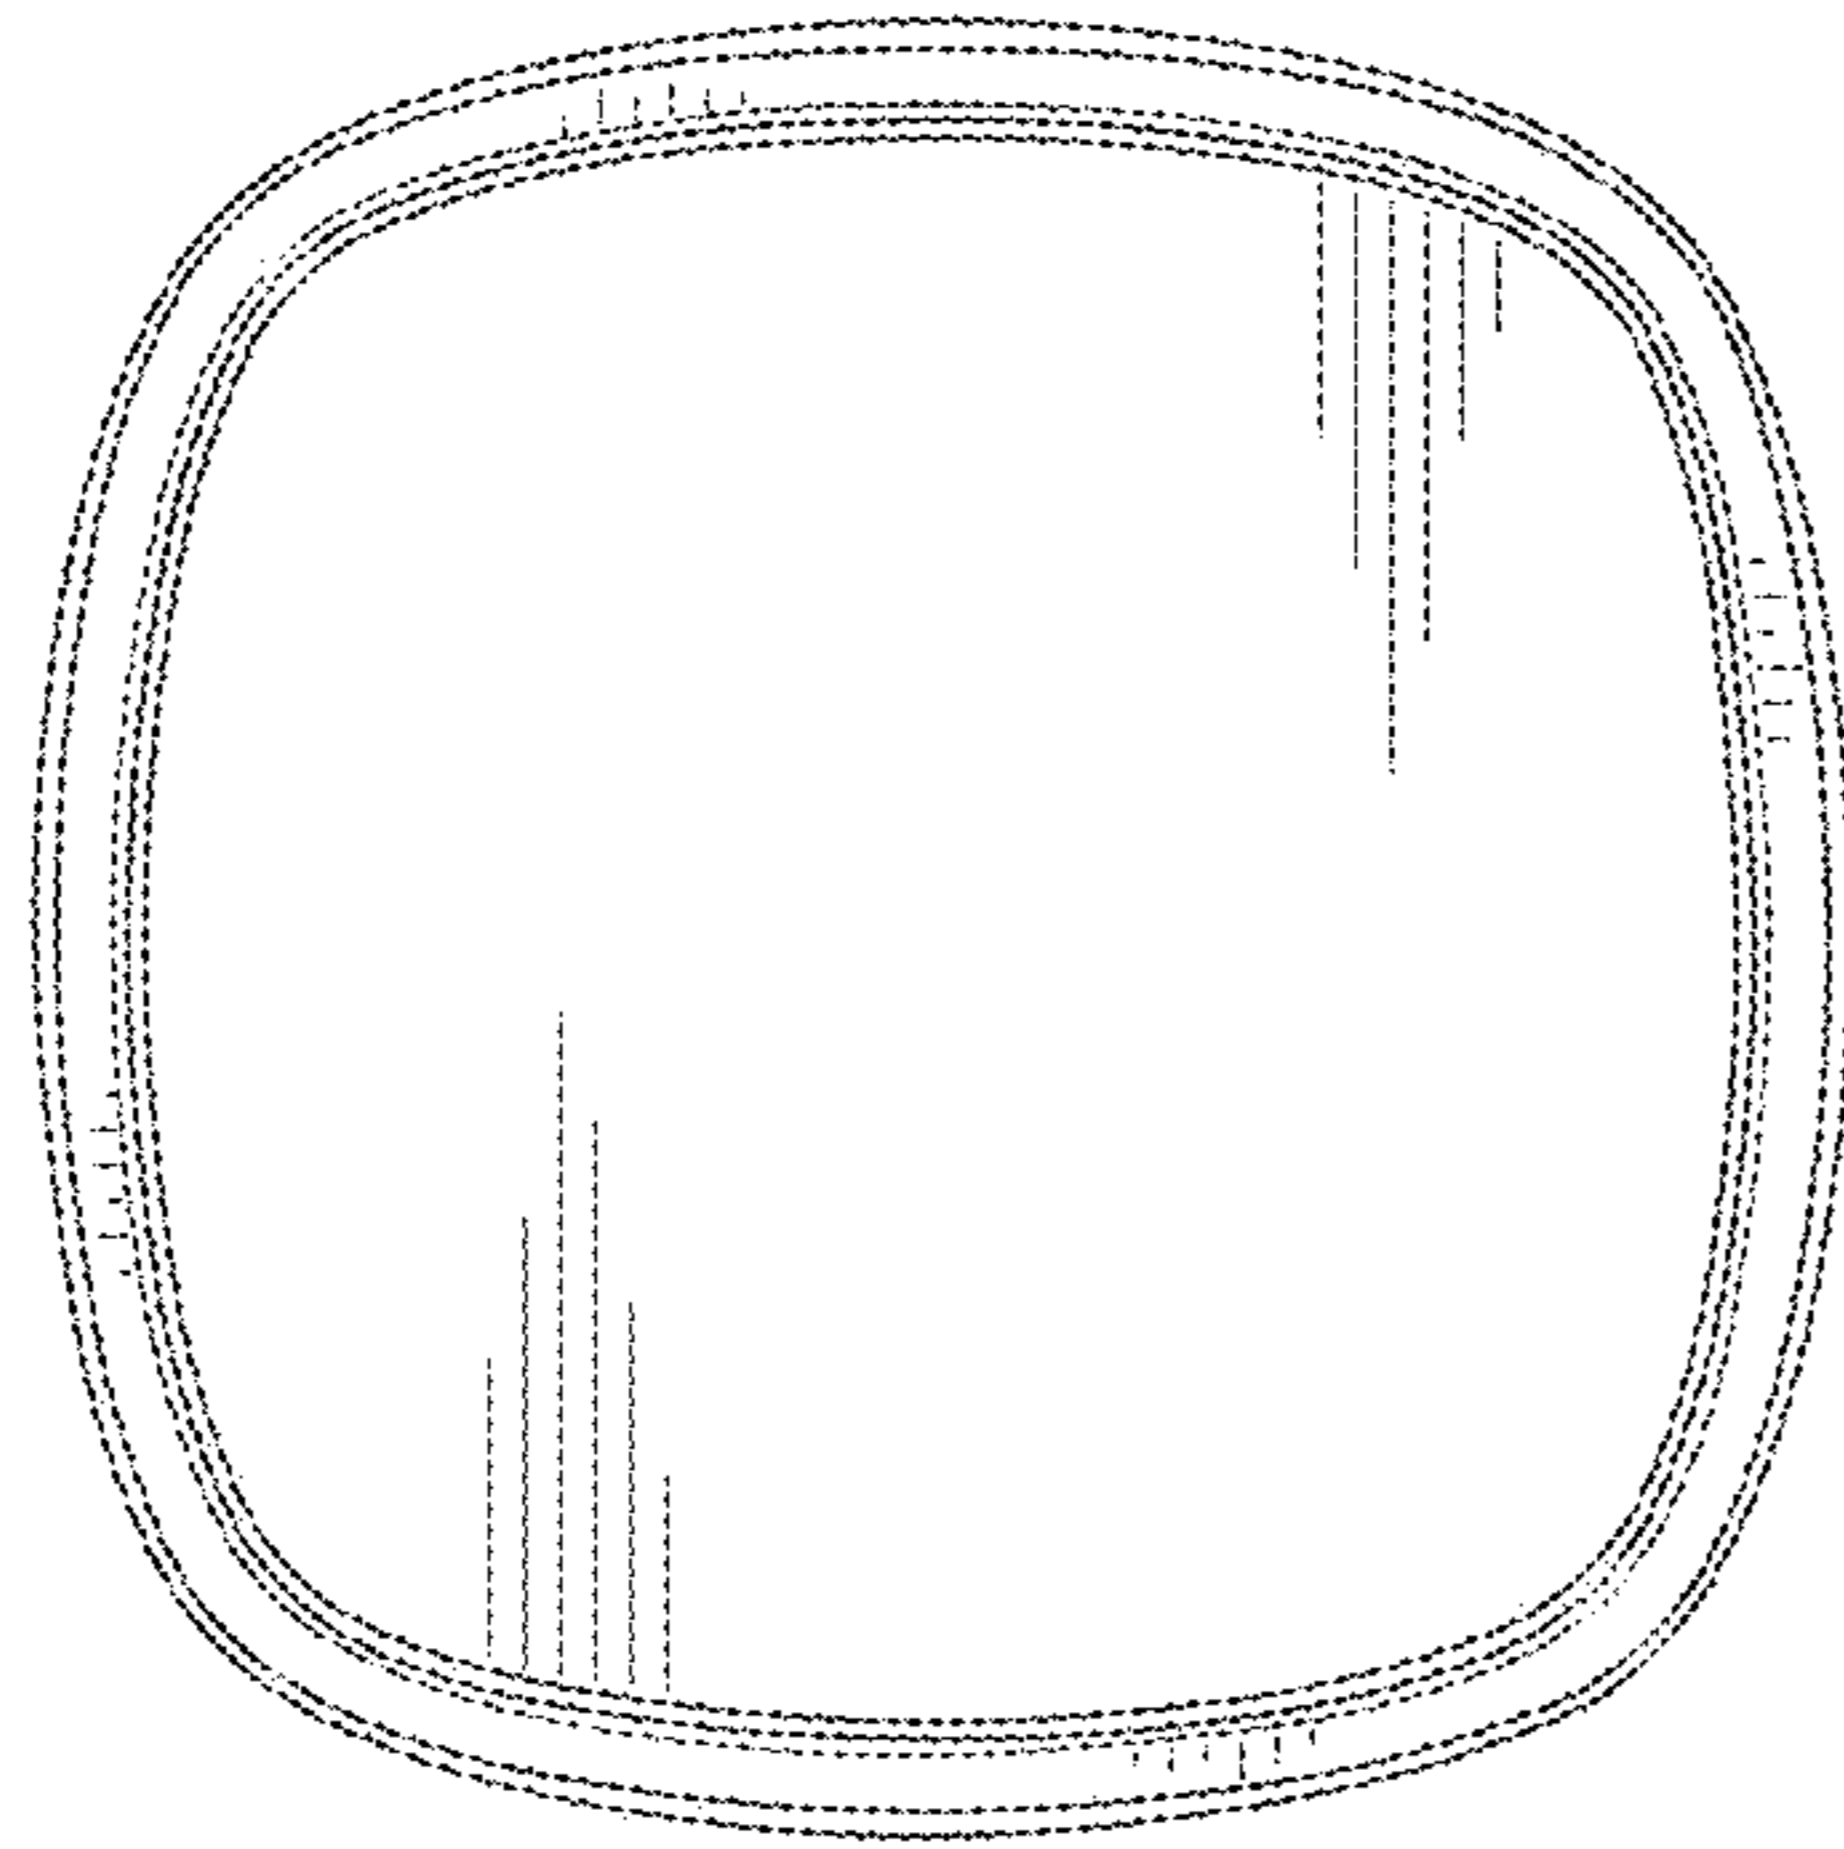


FIG. 6

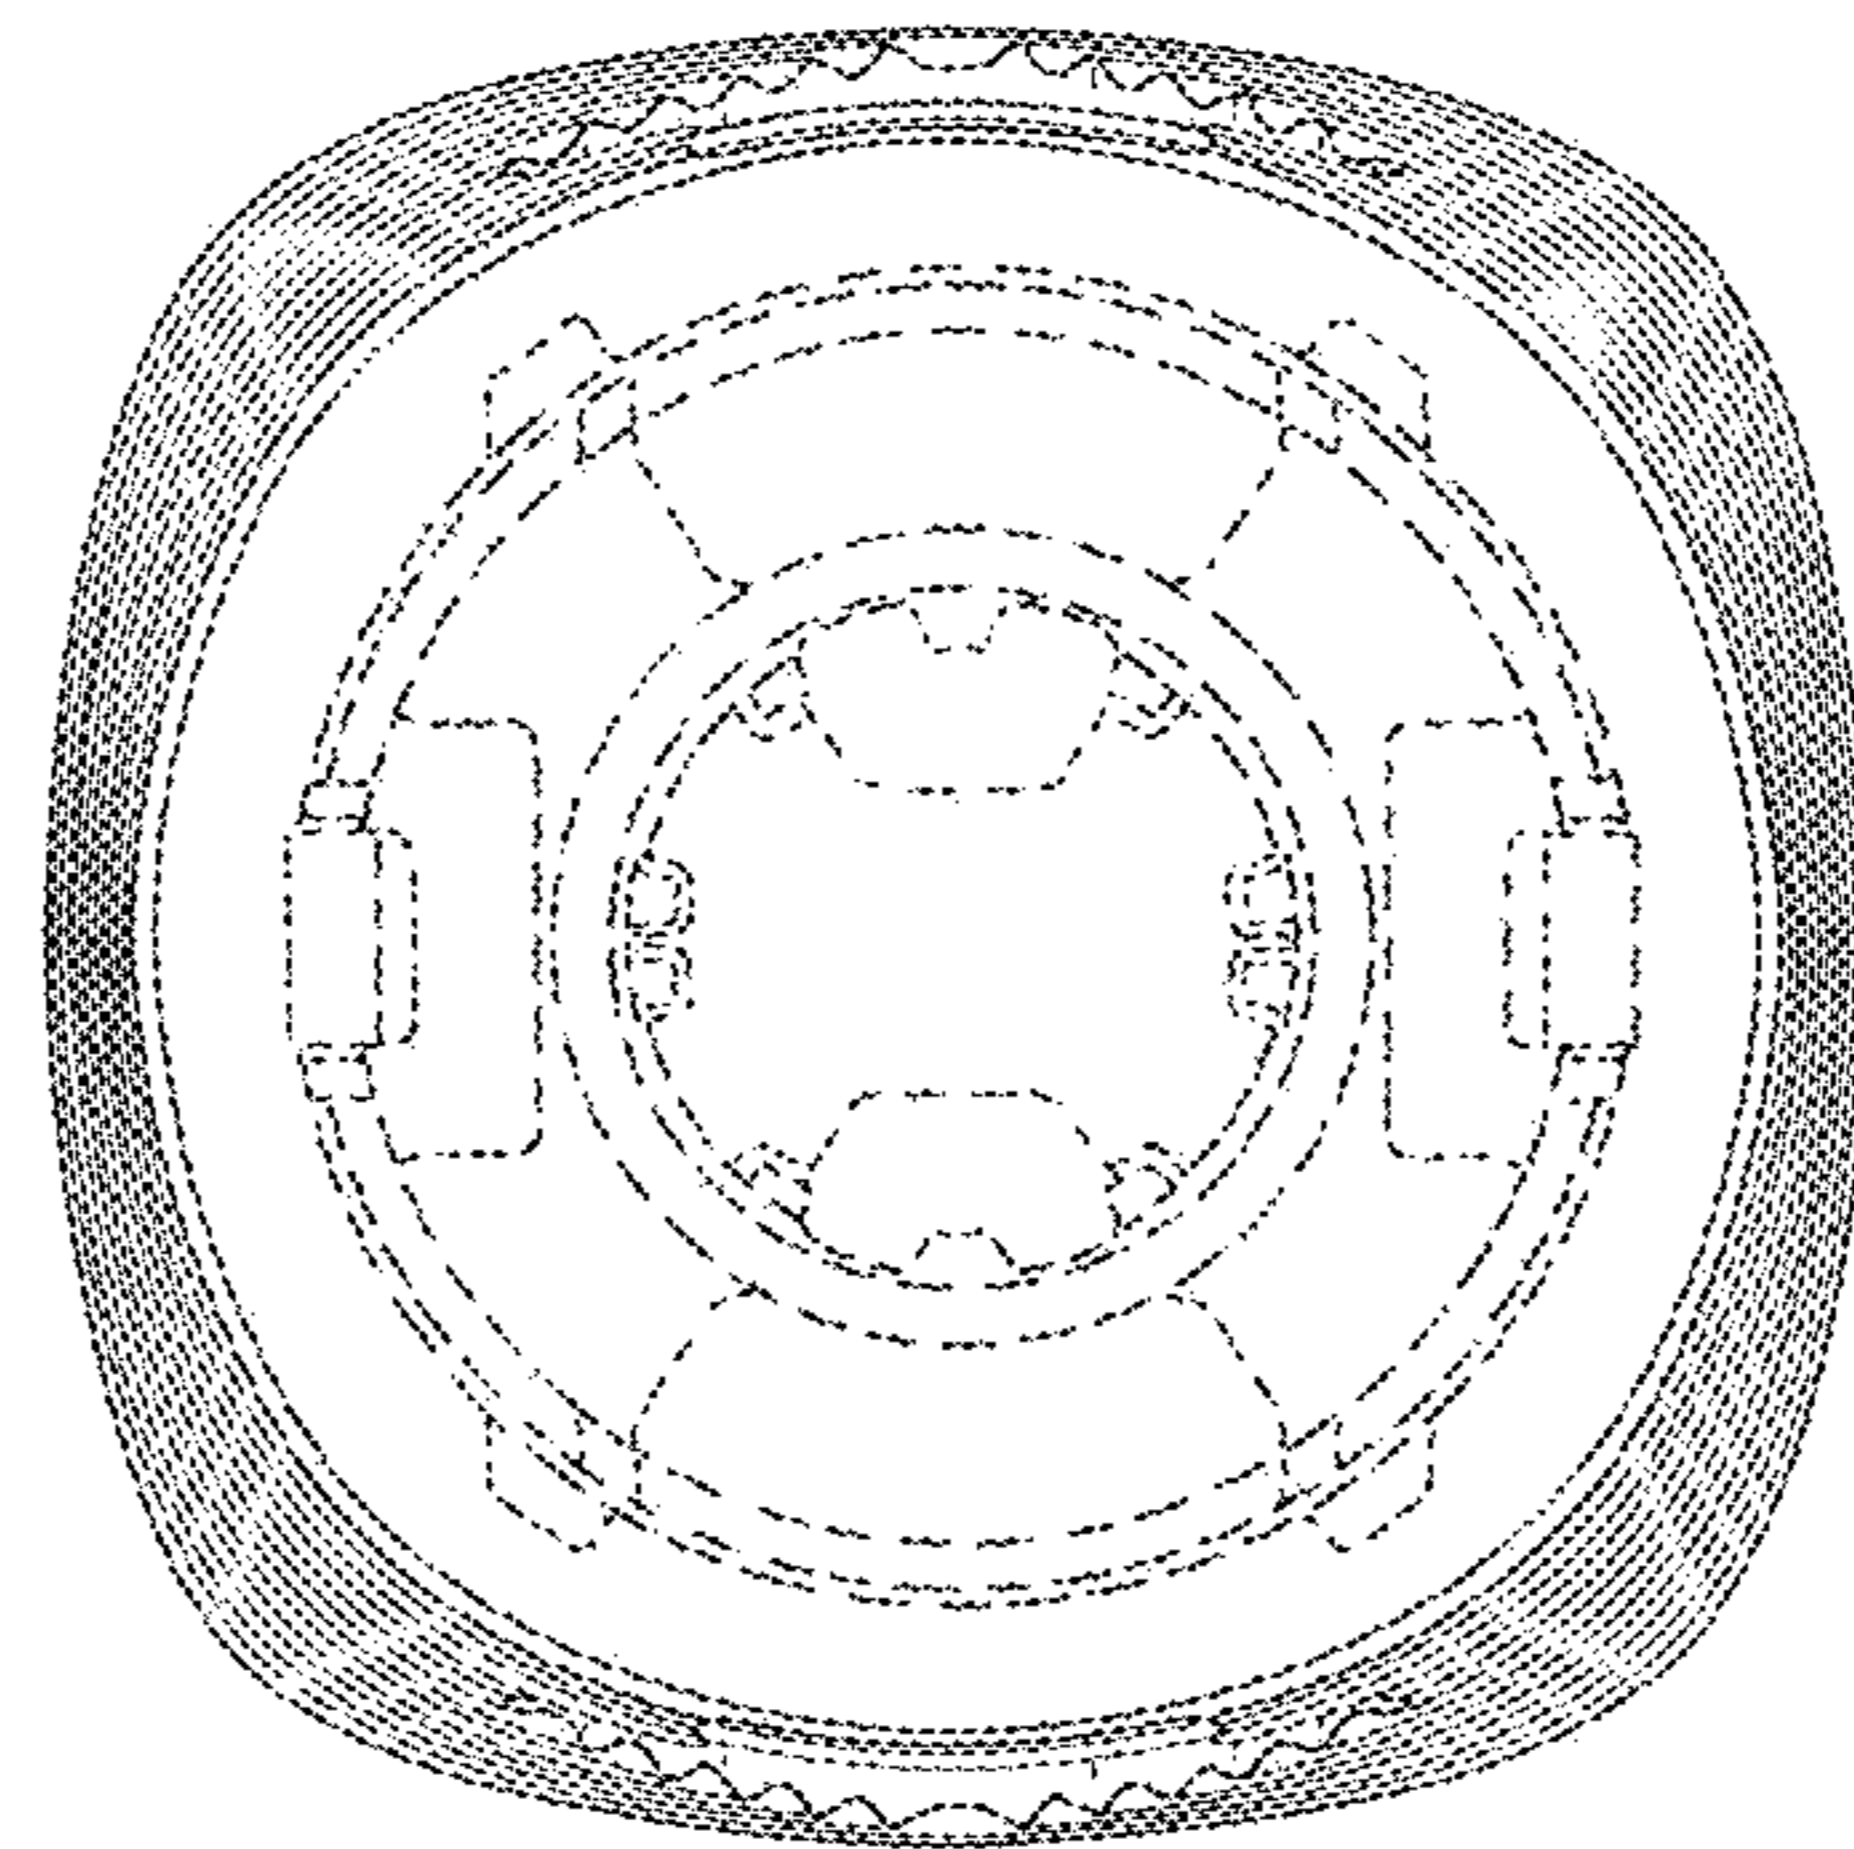


FIG. 7

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D867,588 S
APPLICATION NO. : 29/648584
DATED : November 19, 2019
INVENTOR(S) : Christian Rogge et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:


On the Title Page

After item (22), insert:

-- (30) **Foreign Application Priority Data**

Nov. 23, 2017 (EM) 004520054 --

Signed and Sealed this
Twenty-second Day of December, 2020

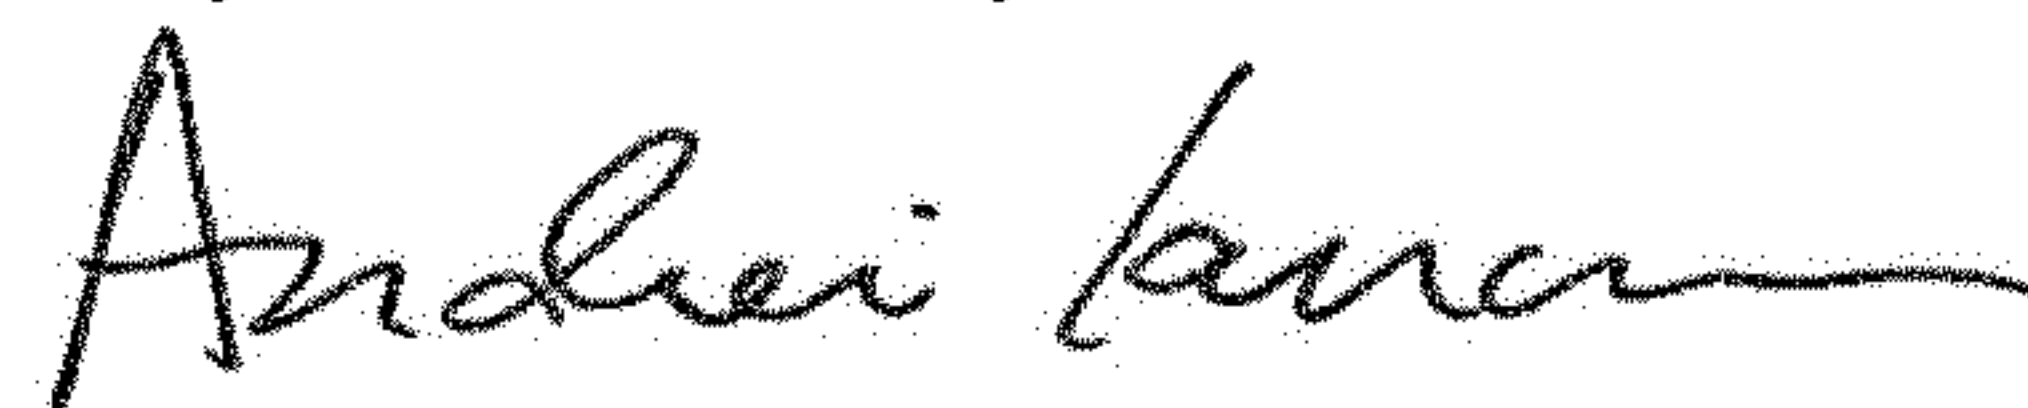

Andrei Iancu
Director of the United States Patent and Trademark Office