

US00D867738S

(12) **United States Design Patent** (10) **Patent No.:** **US D867,738 S**
Farkas (45) **Date of Patent:** **** *Nov. 26, 2019**

(54) **MEDICAL SHOE SOLE FOR CHILDREN**

(71) Applicant: **Daniela Farkas**, Davie, FL (US)

(72) Inventor: **Daniela Farkas**, Davie, FL (US)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **15 Years**

(21) Appl. No.: **29/554,173**

(22) Filed: **Feb. 9, 2016**

(51) **LOC (12) Cl.** **02-04**

(52) **U.S. Cl.**

USPC **D2/957**; D2/947; D2/951; D2/960

(58) **Field of Classification Search**

USPC D2/902, 906, 908, 916, 918, 925,
D2/946-962, 977; 36/1, 1.5, 3 B, 22 R,
36/24.5, 25 R, 28, 32 R, 34 R, 59 C,
36/67 A, 101-107, 114-116, 117.3, 117.4,
36/124-136

CPC A43B 13/00; A43B 13/02; A43B 13/023;
A43B 13/026; A43B 13/04; A43B 13/08;
A43B 13/10; A43B 13/12; A43B 13/14;
A43B 13/16; A43B 13/18; A43B 13/28;
A43B 13/30; A43B 13/32; A43B 13/34;
A43B 13/36; A43B 13/141; A43B
13/143; A43B 13/181; A43B 13/189;
A43B 13/223; A43B 13/224

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D278,851 S *	5/1985	Austin	D2/955
D297,185 S *	8/1988	Berzak	D2/957
D307,816 S *	5/1990	Schneider	D2/959
D322,153 S *	12/1991	Schneider	D2/959
D342,376 S *	12/1993	James	D2/951
D352,154 S *	11/1994	Merceron	D2/952
D352,157 S *	11/1994	Merceron	D2/957
D353,480 S *	12/1994	Merceron	D2/956

D368,358 S *	4/1996	Valle	D2/953
5,564,202 A *	10/1996	Hoppenstein	A43B 13/18 36/25 R
D379,114 S *	5/1997	Merceron	D2/952
D388,241 S *	12/1997	Merceron	D2/959
D389,995 S *	2/1998	Cockrell	D2/947

(Continued)

OTHER PUBLICATIONS

Ovation Medical Pneumatic Tall Walker, DME-Direct.com, [online], [site visited Jan. 24, 2017]. <URL: <http://www.dme-direct.com/ovation-medical-tall-pneumatic-walker>>.*

(Continued)

Primary Examiner — T Chase Nelson

Assistant Examiner — Jonathan J. Han

(74) *Attorney, Agent, or Firm* — Robert M. Schwartz

(57) **CLAIM**

I claim the ornamental design for a medical shoe sole for children, as shown and described.

DESCRIPTION

FIG. 1 is a right medial side view of a medical shoe sole for children showing my new design.

FIG. 2 is a bottom view thereof.

FIG. 3 is a left lateral side view thereof.

FIG. 4 is a cross sectional view taken along the section line marked 4-4 in FIG. 2 of the sole as seen from the left lateral side.

FIG. 5 is a top view thereof.


FIG. 6 is a cross sectional view taken along the section marked 6-6 in FIG. 2 at the level of the toes.

FIG. 7 is a cross sectional view taken along the section marked 7-7 in FIG. 2 at the level of metatarsal base.

FIG. 8 is a cross sectional view taken along the section marked 8-8 in FIG. 2 at the level of sub-talar joint; and,

FIG. 9 is a cross sectional view taken along the section marked 9-9 in FIG. 2 at the mid-heel.

1 Claim, 2 Drawing Sheets

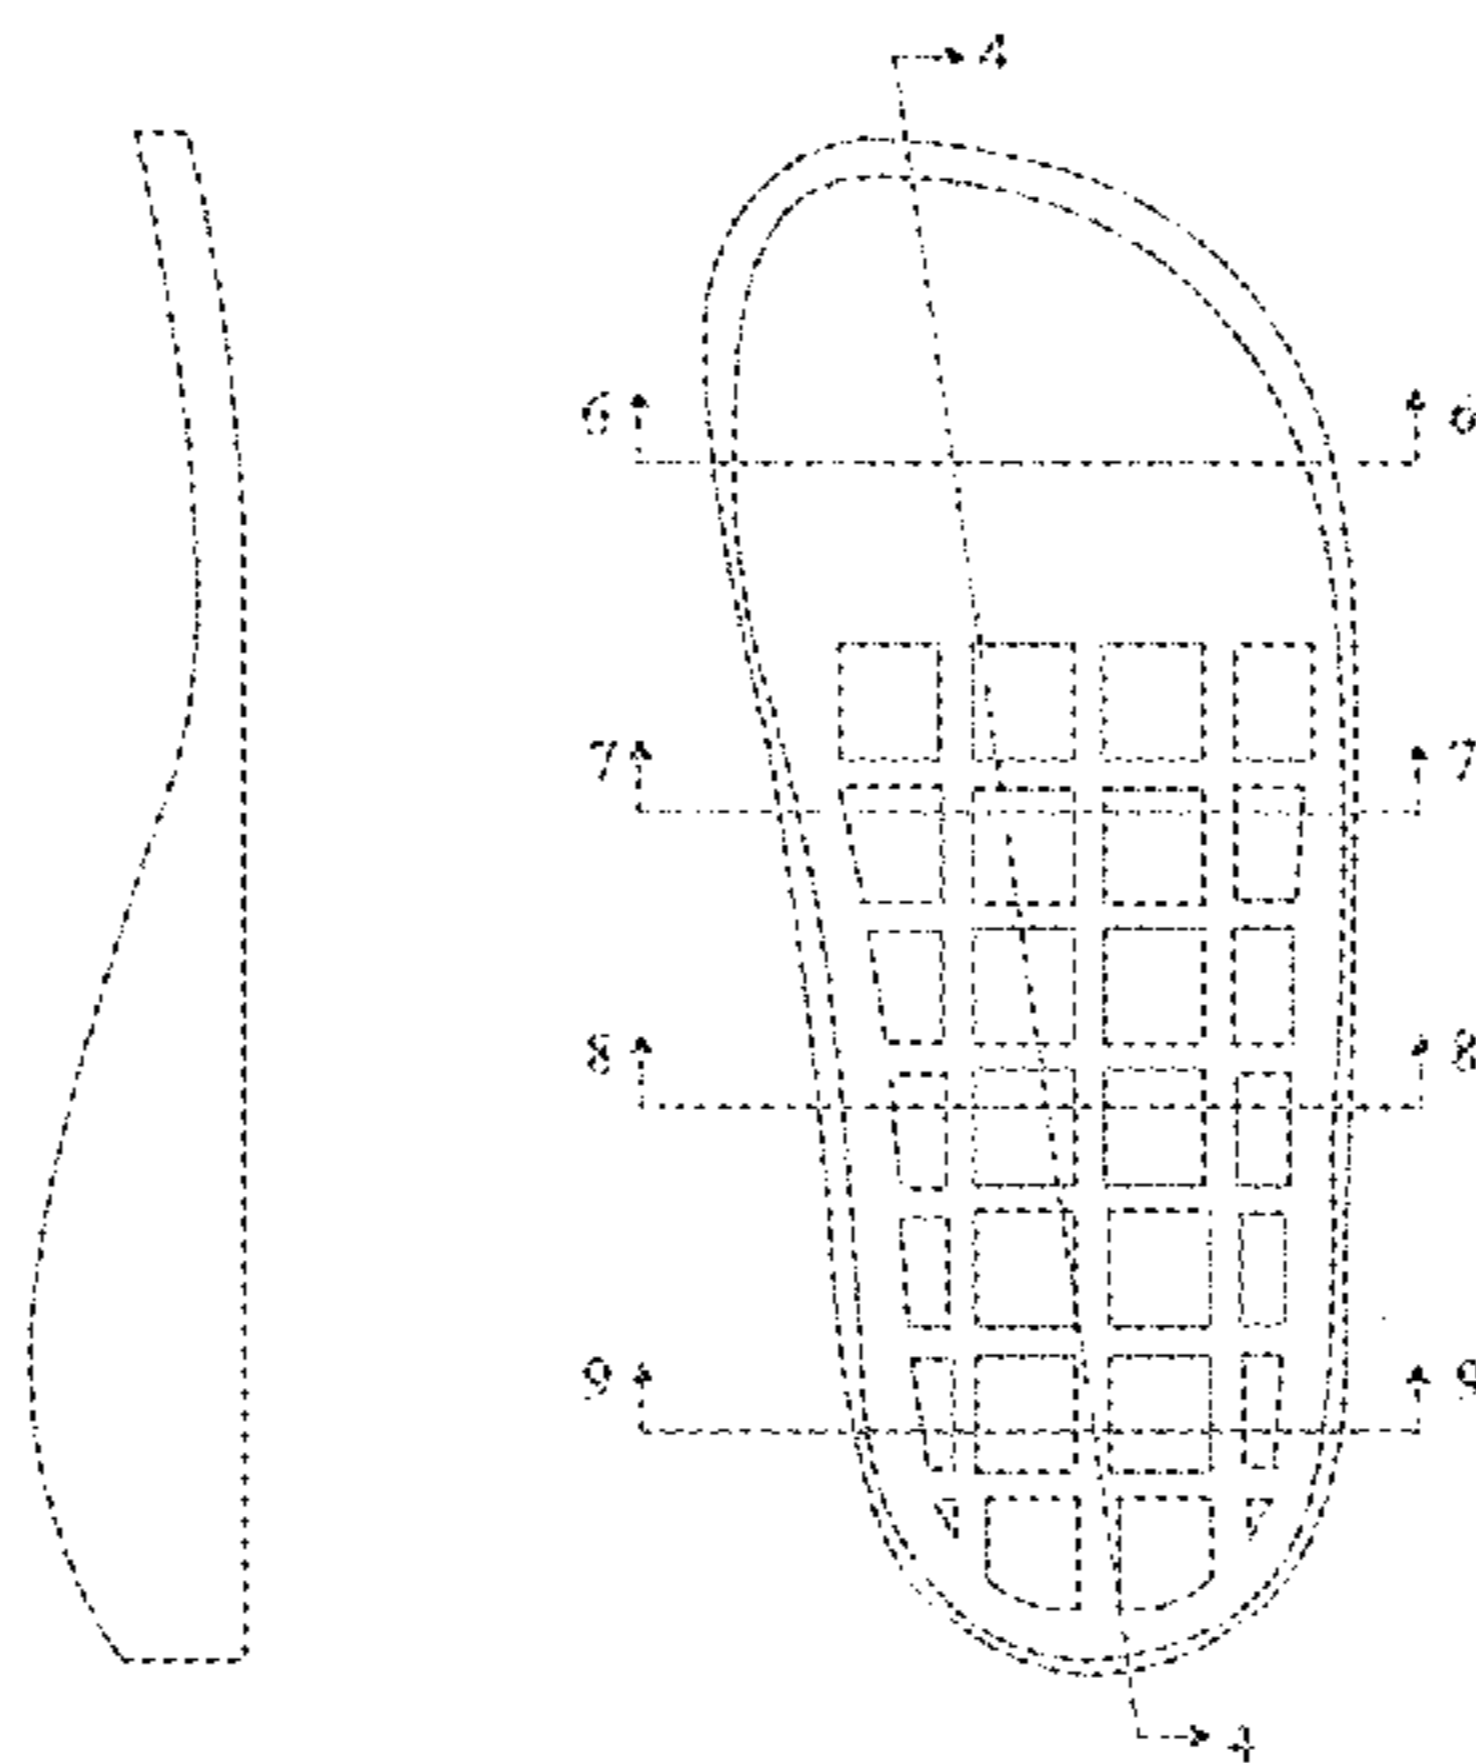

(56)

References Cited

U.S. PATENT DOCUMENTS

D394,142 S * 5/1998 Merceron D2/959
 5,768,806 A * 6/1998 Parisotto A43B 21/32
 36/102
 D397,546 S * 9/1998 Merceron D2/951
 D426,947 S * 6/2000 Pollastrelli D2/947
 6,105,279 A * 8/2000 Bouchoms A43B 9/10
 36/25 R
 6,126,179 A * 10/2000 Dodge A43B 5/0401
 280/14.22
 D445,243 S * 7/2001 Cockrell D2/947
 D446,635 S * 8/2001 Pollastrelli D2/947
 D446,914 S * 8/2001 Cockrell D2/959
 6,305,099 B1 * 10/2001 Chu A43B 7/08
 36/29
 D576,392 S * 9/2008 Cintra D2/947
 D582,641 S * 12/2008 Kielt D2/946
 D737,030 S * 8/2015 Bizzo D2/951
 D770,742 S * 11/2016 Reiser D2/947
 2001/0007181 A1 * 7/2001 Cagner A43B 9/12
 36/102
 2007/0214682 A1 * 9/2007 Smotrycz A43B 7/125
 36/3 B
 2008/0178496 A1 * 7/2008 Lin A43B 7/125
 36/30 R
 2009/0193690 A1 * 8/2009 Moretti A43B 7/125
 36/3 B
 2011/0232128 A1 * 9/2011 Propet A43B 13/181
 36/28
 2015/0040424 A1 * 2/2015 Lo A43B 7/081
 36/29
 2016/0331078 A1 * 11/2016 Conchieri A43B 13/026

OTHER PUBLICATIONS

Diabetic Shoe Insole for Orthopaedic Care, TopDealsGalore.com, [online], [site visited Jan. 24, 2017]. <URL: <https://topdealsgalore.com/product/orthopedic-insole-for-diabetic-foot-care>>.*
 Best work safety footwear waterproof anti-slip overshoes for sea food shop sushi shop men's medical nursing hospital shoes, AliExpress.com, [online], [site visited Jan. 24, 2017]. <URL: <https://www.aliexpress.com/item/Waterproof-anti-slip-overshoes-for-sea-food-shop-and-Sushi-shop-for-wet-floor/1347095753.html?spm=2114.40010708.4.34.Vivp1H>>.*
 Men's Waffle Sole Flip Flop Assortment Case of 36, MyShopify.com, [online], [site visited Jan. 24, 2017]. <URL: <http://test-store-1336.myshopify.com/products/mens-waffle-sole-flip-flop-assortment>>.*
 From Waffle Sole to Flyknit and Back Again: New Footwear Express Nike's 'Nature Amplified' Design Ethos, Core77.com, by Ray Hu—Jul. 17, 2013, [online], [site visited Jan. 24, 2017]. <URL: <http://www.core77.com/posts/25222/from-waffle-sole-to-flyknit-and-back-again-new-footwear-expresses-nikes-nature-amplified-design-ethos-25222>>.*
 Ultra Light ¾ Length orthotic Insoles, Bubble gel heel pad, arch supports, Amazon.CO.UK, Date first available at Amazon.co.uk: Mar. 30, 2016, [online], [site visited Jan. 24, 2017]. <URL: https://www.amazon.co.uk/Length-orthotic-Insoles-supports-MEDICAL/dp/B01DM4ST1M/ref=pd_lpo_309_tr_t_3/255-0677373-8718366?_encoding=UTF8&refRID=NER75RBHH47DMW2EYV9X>.*

* cited by examiner

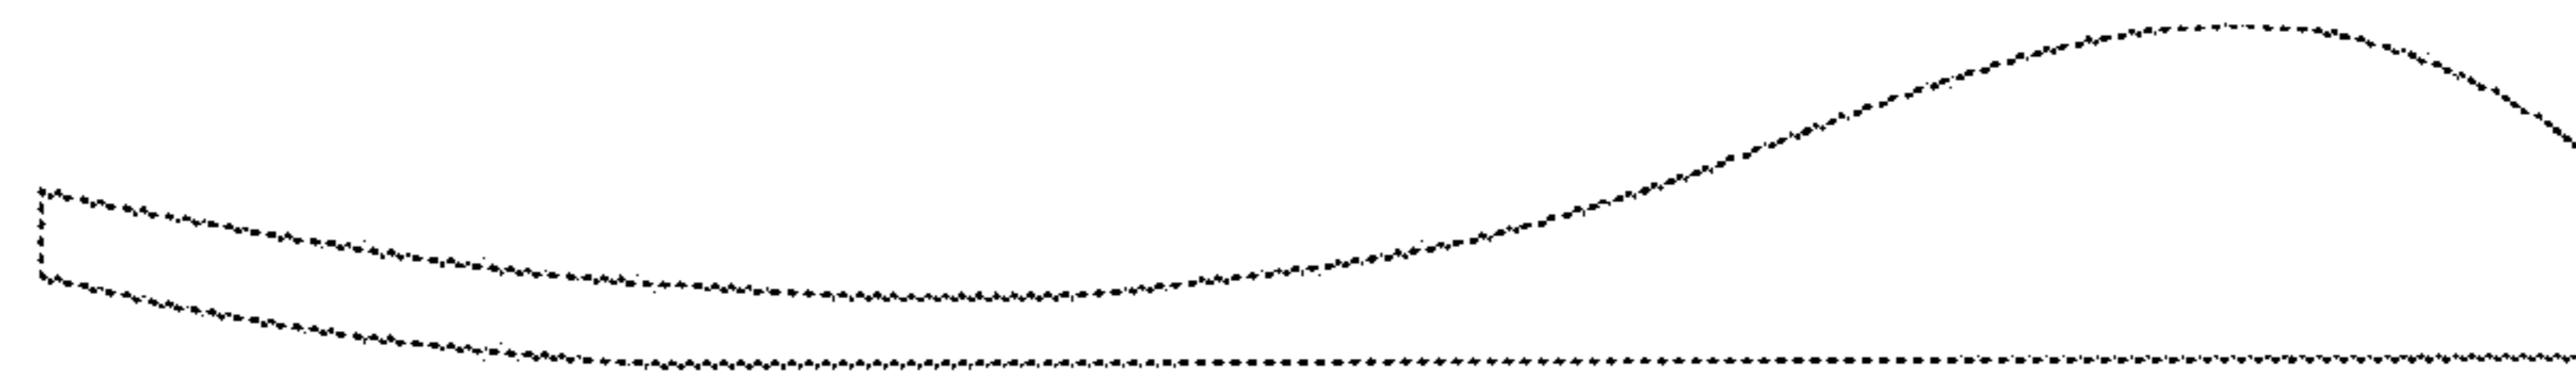


FIG. 3

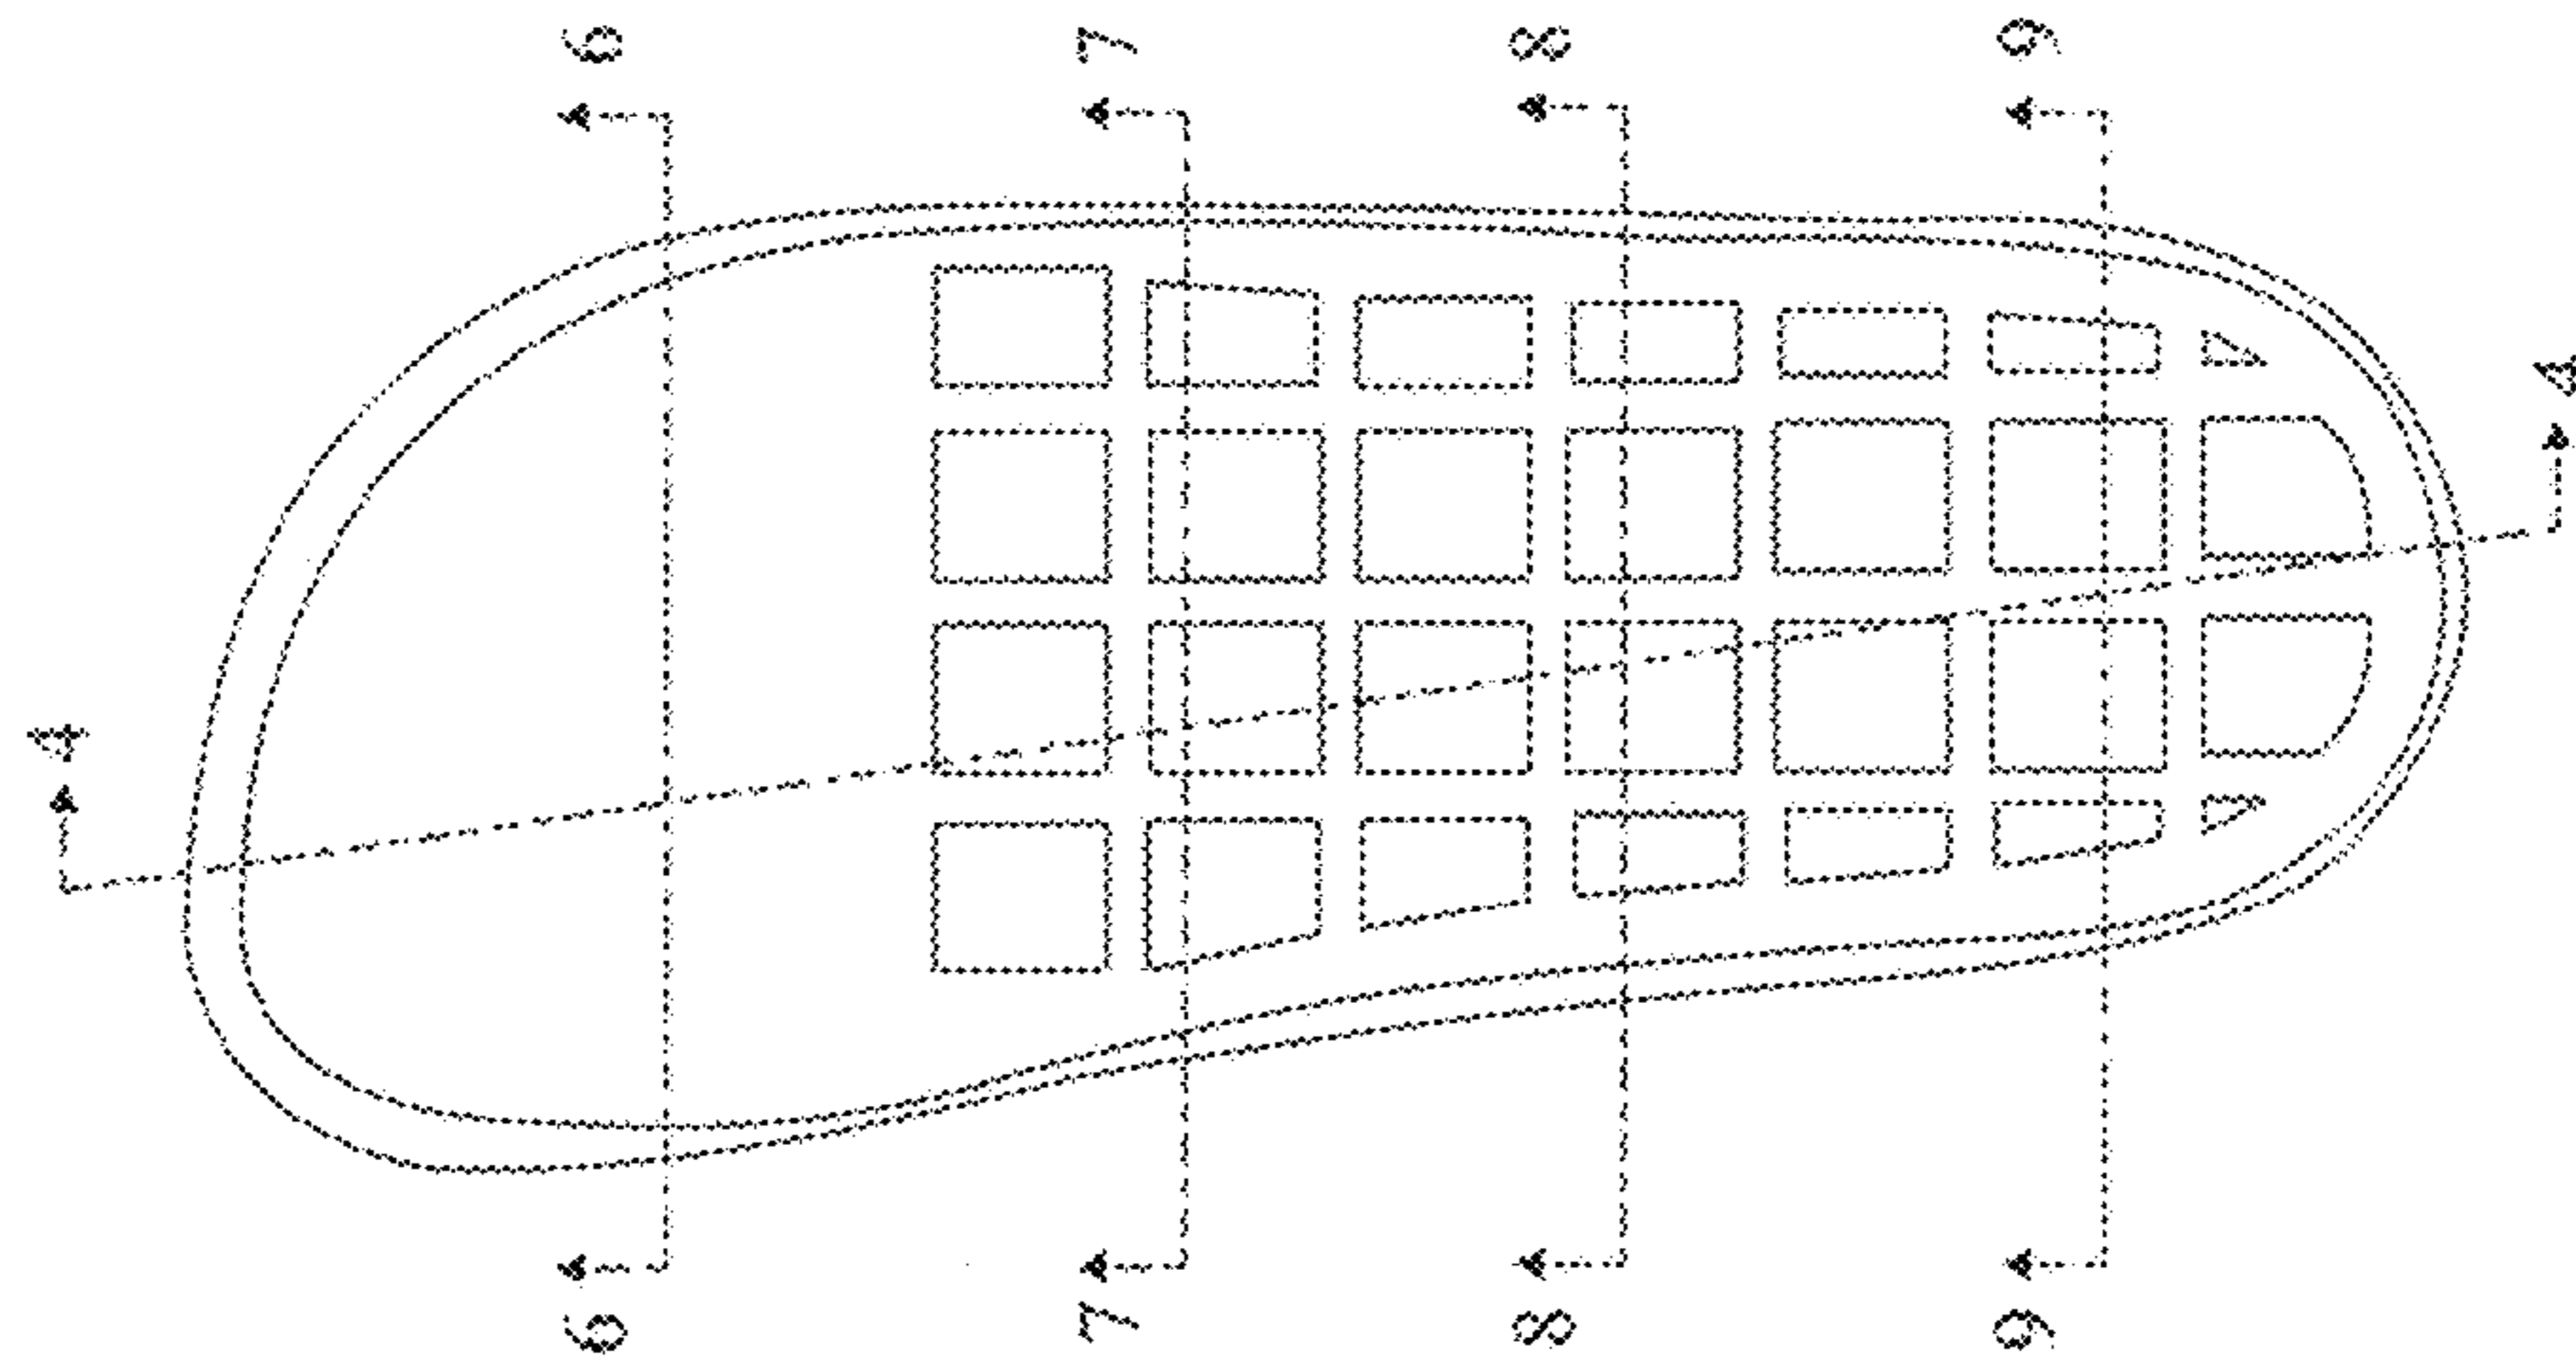


FIG. 2

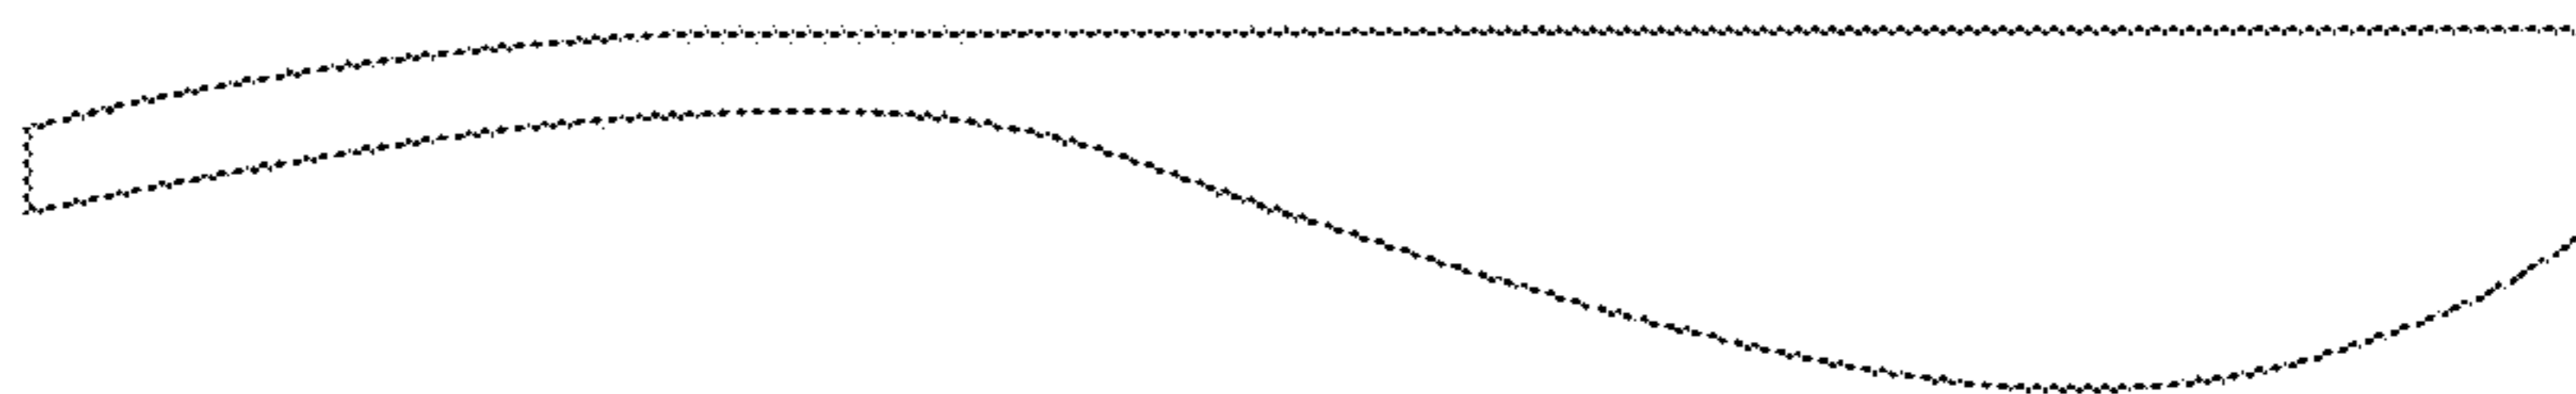


FIG. 1

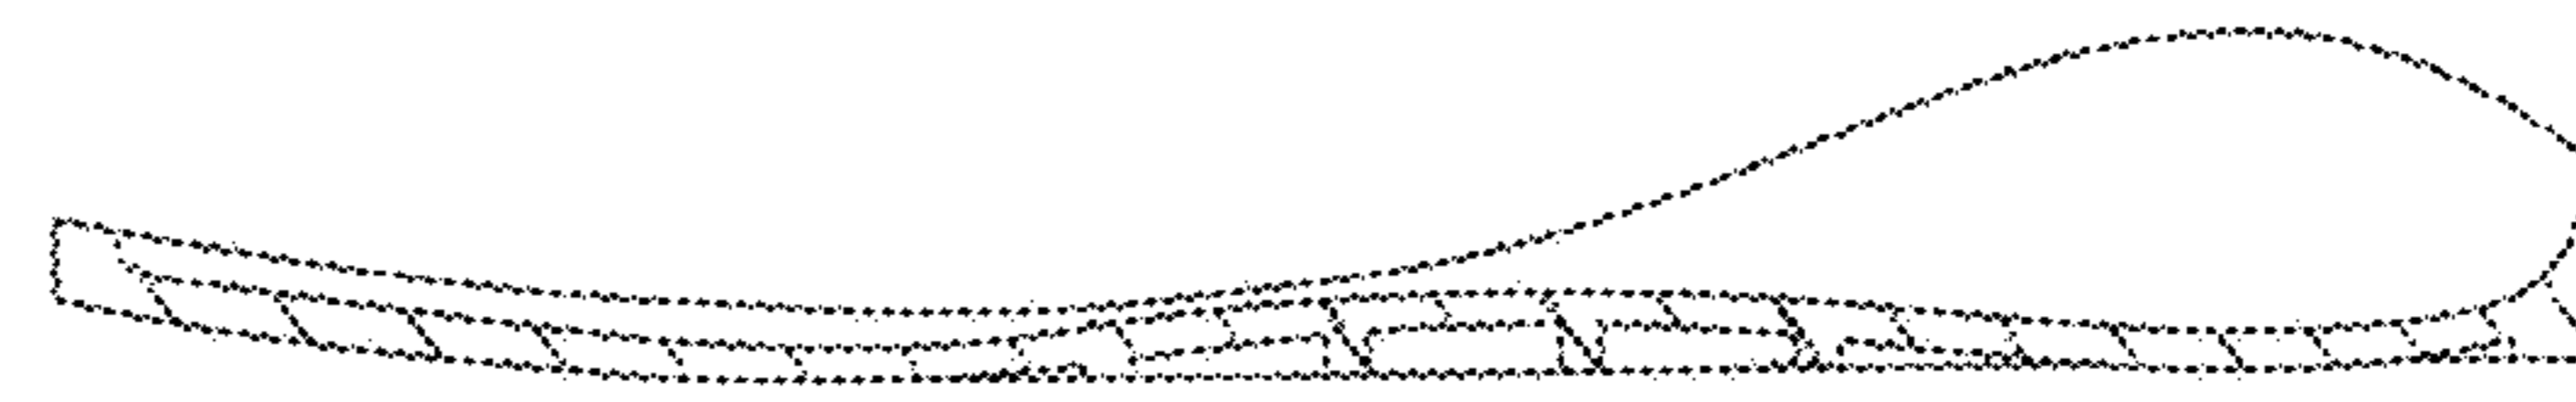


FIG. 4

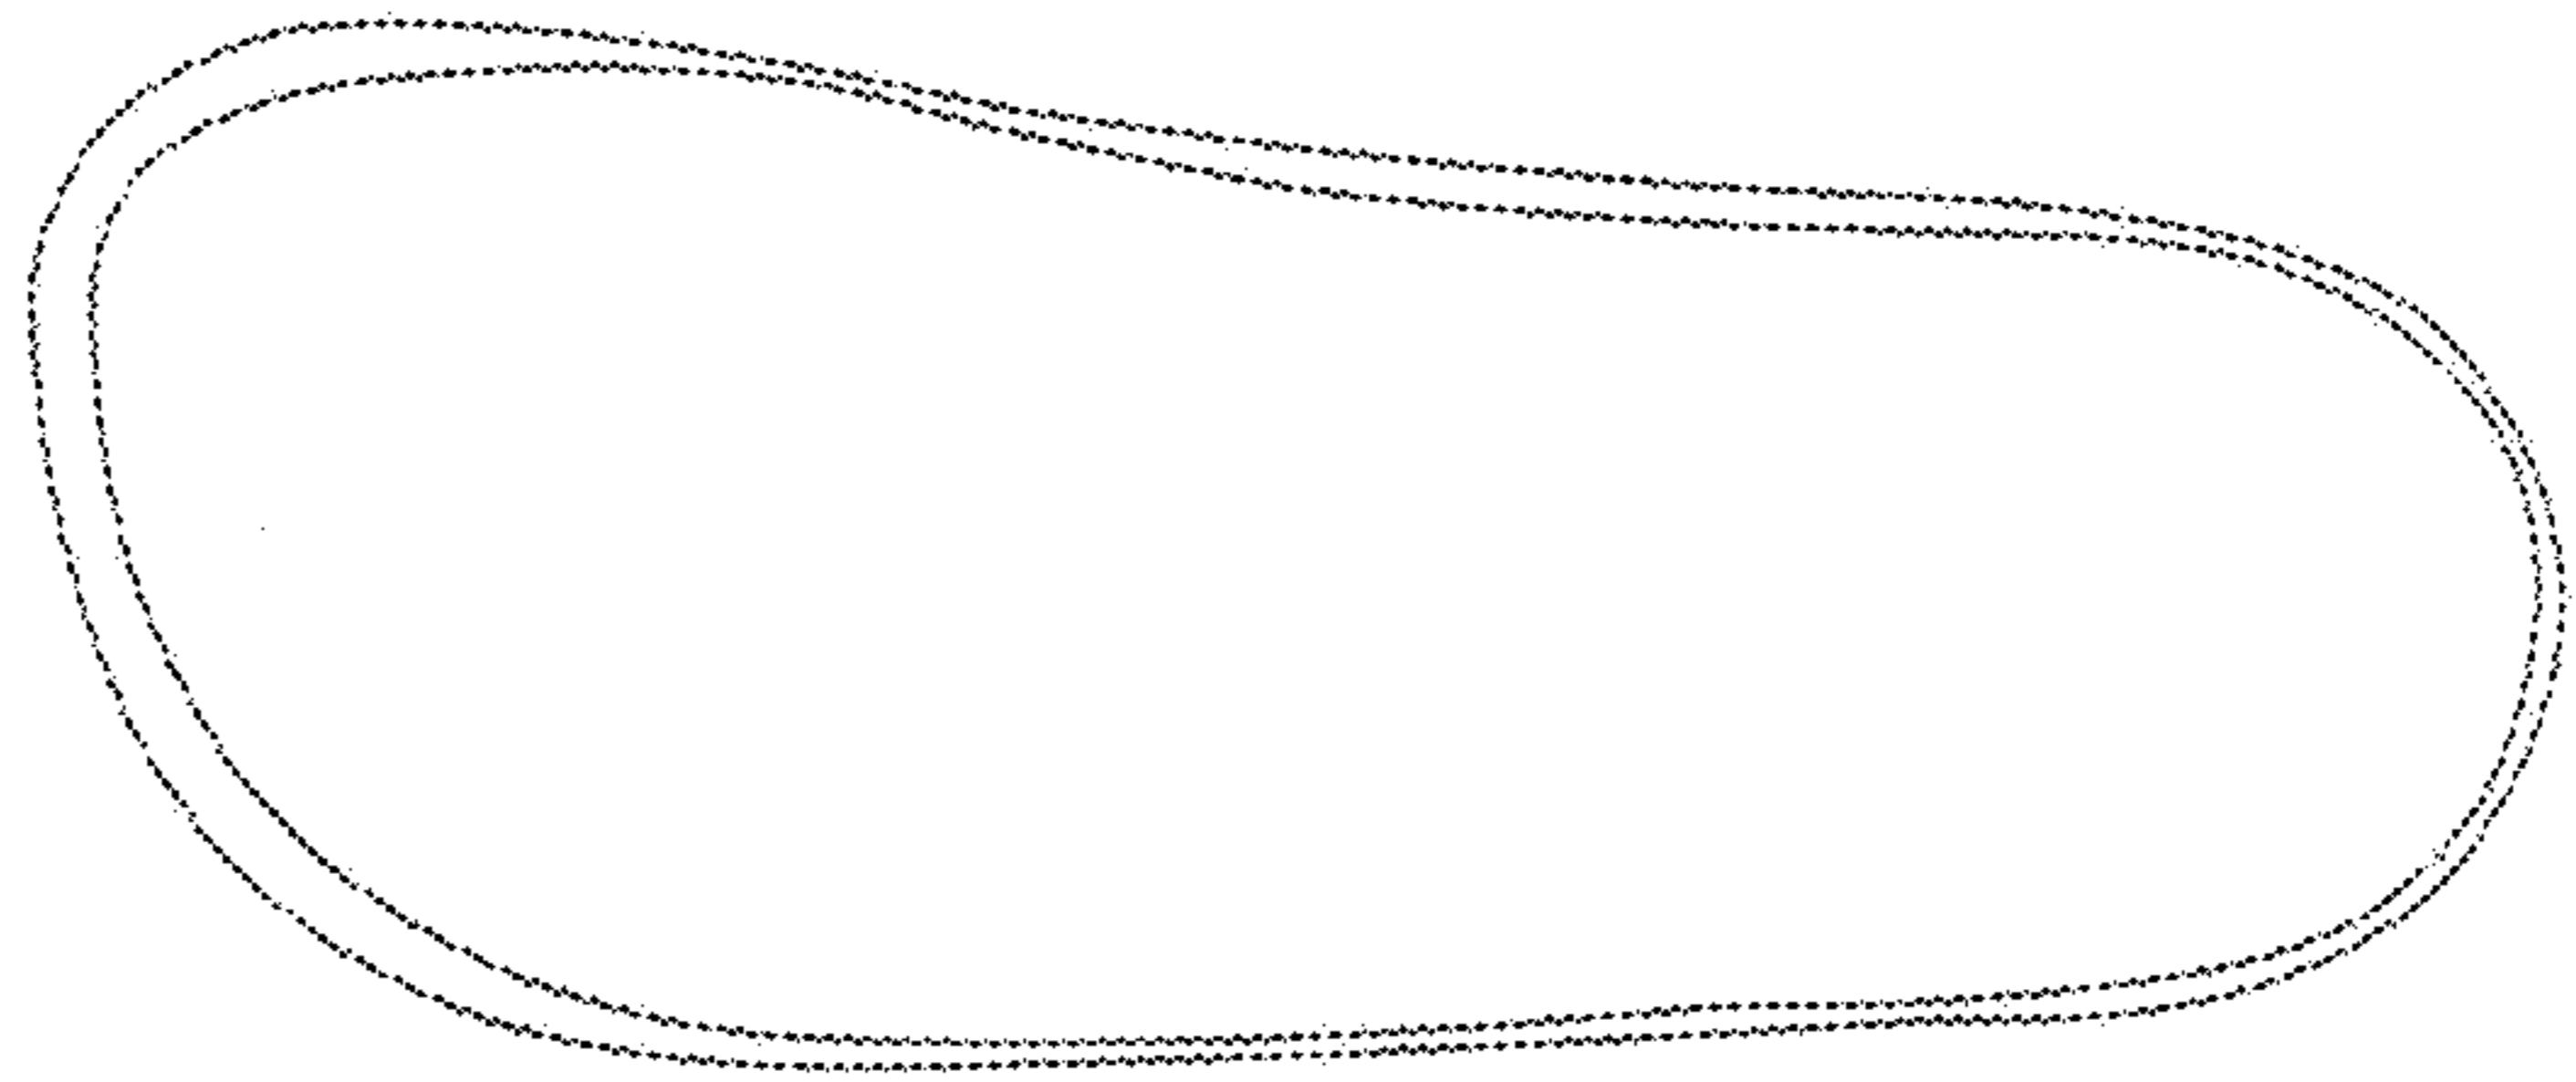


FIG. 5



FIG. 6



FIG. 7

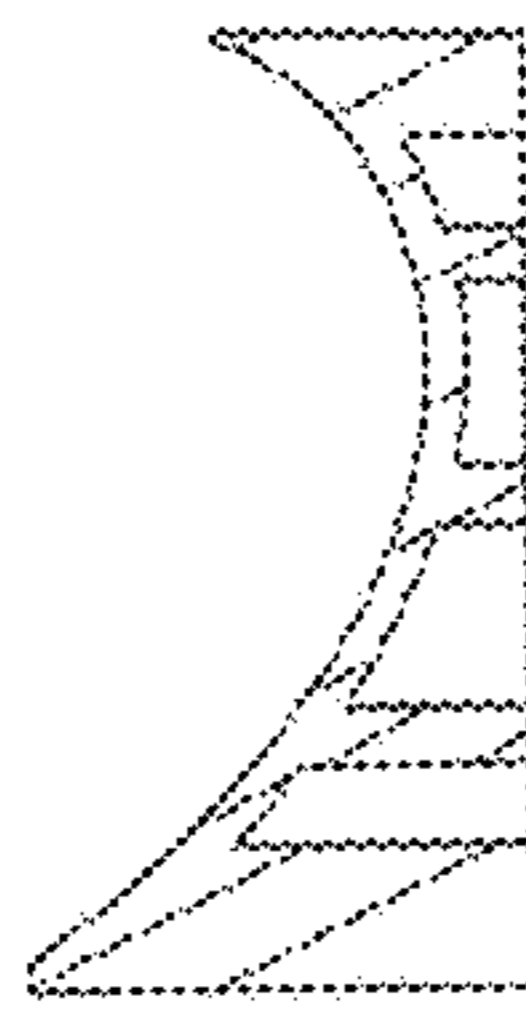


FIG. 8



FIG. 9