



US00D868082S

(12) **United States Design Patent**
Nishi et al.

(10) **Patent No.:** **US D868,082 S**

(45) **Date of Patent:** **** Nov. 26, 2019**

(54) **DISPLAY SCREEN OF A CONTROLLER FOR SURGICAL INSTRUMENT WITH GRAPHICAL USER INTERFACE**

(71) Applicant: **OLYMPUS CORPORATION**,
Hachioji-shi, Tokyo (JP)

(72) Inventors: **Hidefumi Nishi**, Tokyo (JP); **Kota Sugaya**, Tokyo (JP)

(73) Assignee: **OLYMPUS CORPORATION**, Tokyo (JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/602,486**

(22) Filed: **May 1, 2017**

(30) **Foreign Application Priority Data**

Nov. 2, 2016 (JP) 2016-023866

(51) **LOC (12) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495
CPC G06F 3/048; G06F 3/0481; G06F 3/04812;
G06F 3/04815; G06F 3/04817; G06F
3/0482; G06F 3/0483; G06F 3/0484;
G06F 3/04842; G06F 3/04845; G06F
3/04847; G06F 3/0485; G06F 3/04855;
G06F 3/0486; G06F 3/0487; G06F
3/0488; G06F 3/04883; G06F 3/04886
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D742,891 S * 11/2015 Sakamoto D14/485
D757,059 S * 5/2016 Gray D14/486
D770,462 S * 11/2016 Gray D14/485

D774,077 S * 12/2016 Donnelly D14/488
D781,897 S * 3/2017 Umezawa D14/486
D783,651 S * 4/2017 Voutta D14/486
D786,910 S * 5/2017 Higuchi D14/486
D787,529 S * 5/2017 Huang D14/485
D789,959 S * 6/2017 Hoang D14/486
D791,153 S * 7/2017 Rice D14/486
D791,164 S * 7/2017 Rice D14/487
D792,426 S * 7/2017 Theodore D14/485
D795,904 S * 8/2017 Pei D14/486
D796,523 S * 9/2017 Bhandari D14/485
D797,128 S * 9/2017 Shewman D14/485
D801,355 S * 10/2017 Hoang D14/486

(Continued)

Primary Examiner — Melanie H Tung

Assistant Examiner — Bao-Yen T Nguyen

(74) *Attorney, Agent, or Firm* — Oliff PLC

(57) **CLAIM**

The ornamental design for a display screen of a controller for surgical instrument with graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a display screen of a controller for surgical instrument with graphical user interface, showing our new design;

FIG. 2 is a rear view thereof;

FIG. 3 is a top view thereof;

FIG. 4 is a bottom view thereof;

FIG. 5 is a left side view thereof;


FIG. 6 is a right side view thereof; and,

FIG. 7 is an enlarged front view of the display screen with graphical user interface.

The evenly spaced broken lines in the figures show a controller for surgical instrument, and form no part of the claimed design.

The dot-dash broken lines in the figures show portions of a graphical user interface and form no part of the claimed design.

1 Claim, 5 Drawing Sheets

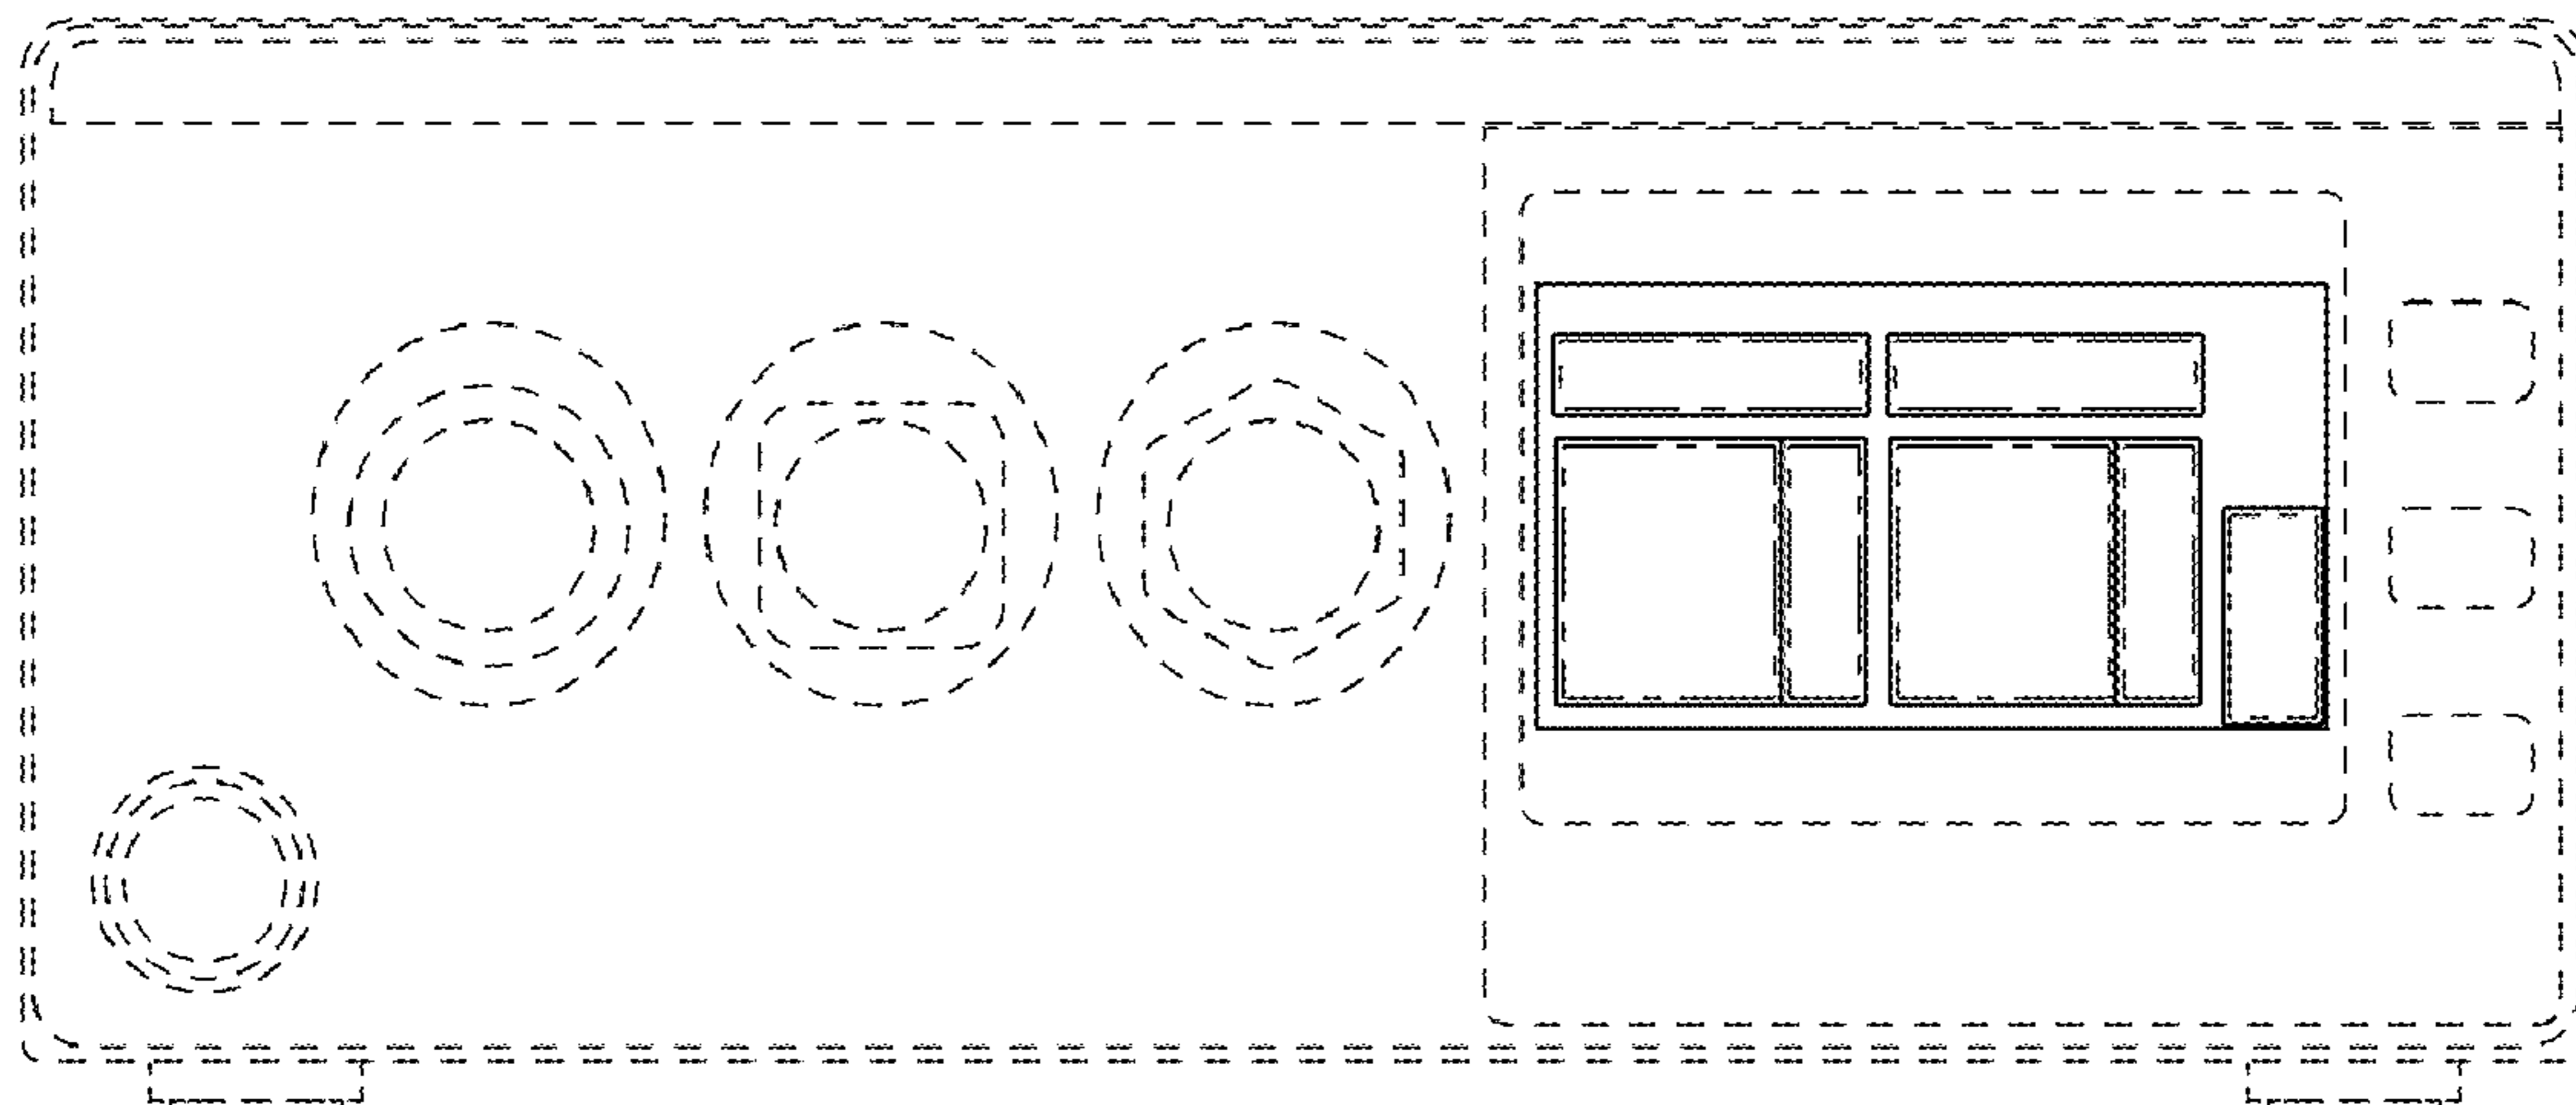

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|------------|------|---------|----------|-------|--------------|
| D801,371 | S * | 10/2017 | Dahlen | | D14/486 |
| D803,852 | S * | 11/2017 | Hoffman | | D14/485 |
| D804,498 | S * | 12/2017 | Akatsu | | D14/485 |
| D807,902 | S * | 1/2018 | Cong | | D14/486 |
| D808,989 | S * | 1/2018 | Ayvazian | | D14/485 |
| D808,996 | S * | 1/2018 | Ambielli | | D14/486 |
| D810,769 | S * | 2/2018 | Zhou | | D14/486 |
| D811,425 | S * | 2/2018 | Olsen | | D14/486 |
| 10,073,515 | B2 * | 9/2018 | Awdeh | | G06T 11/00 |
| 10,105,485 | B2 * | 10/2018 | Piferi | | A61B 5/055 |
| 10,130,378 | B2 * | 11/2018 | Bryan | | A61B 17/1684 |

* cited by examiner

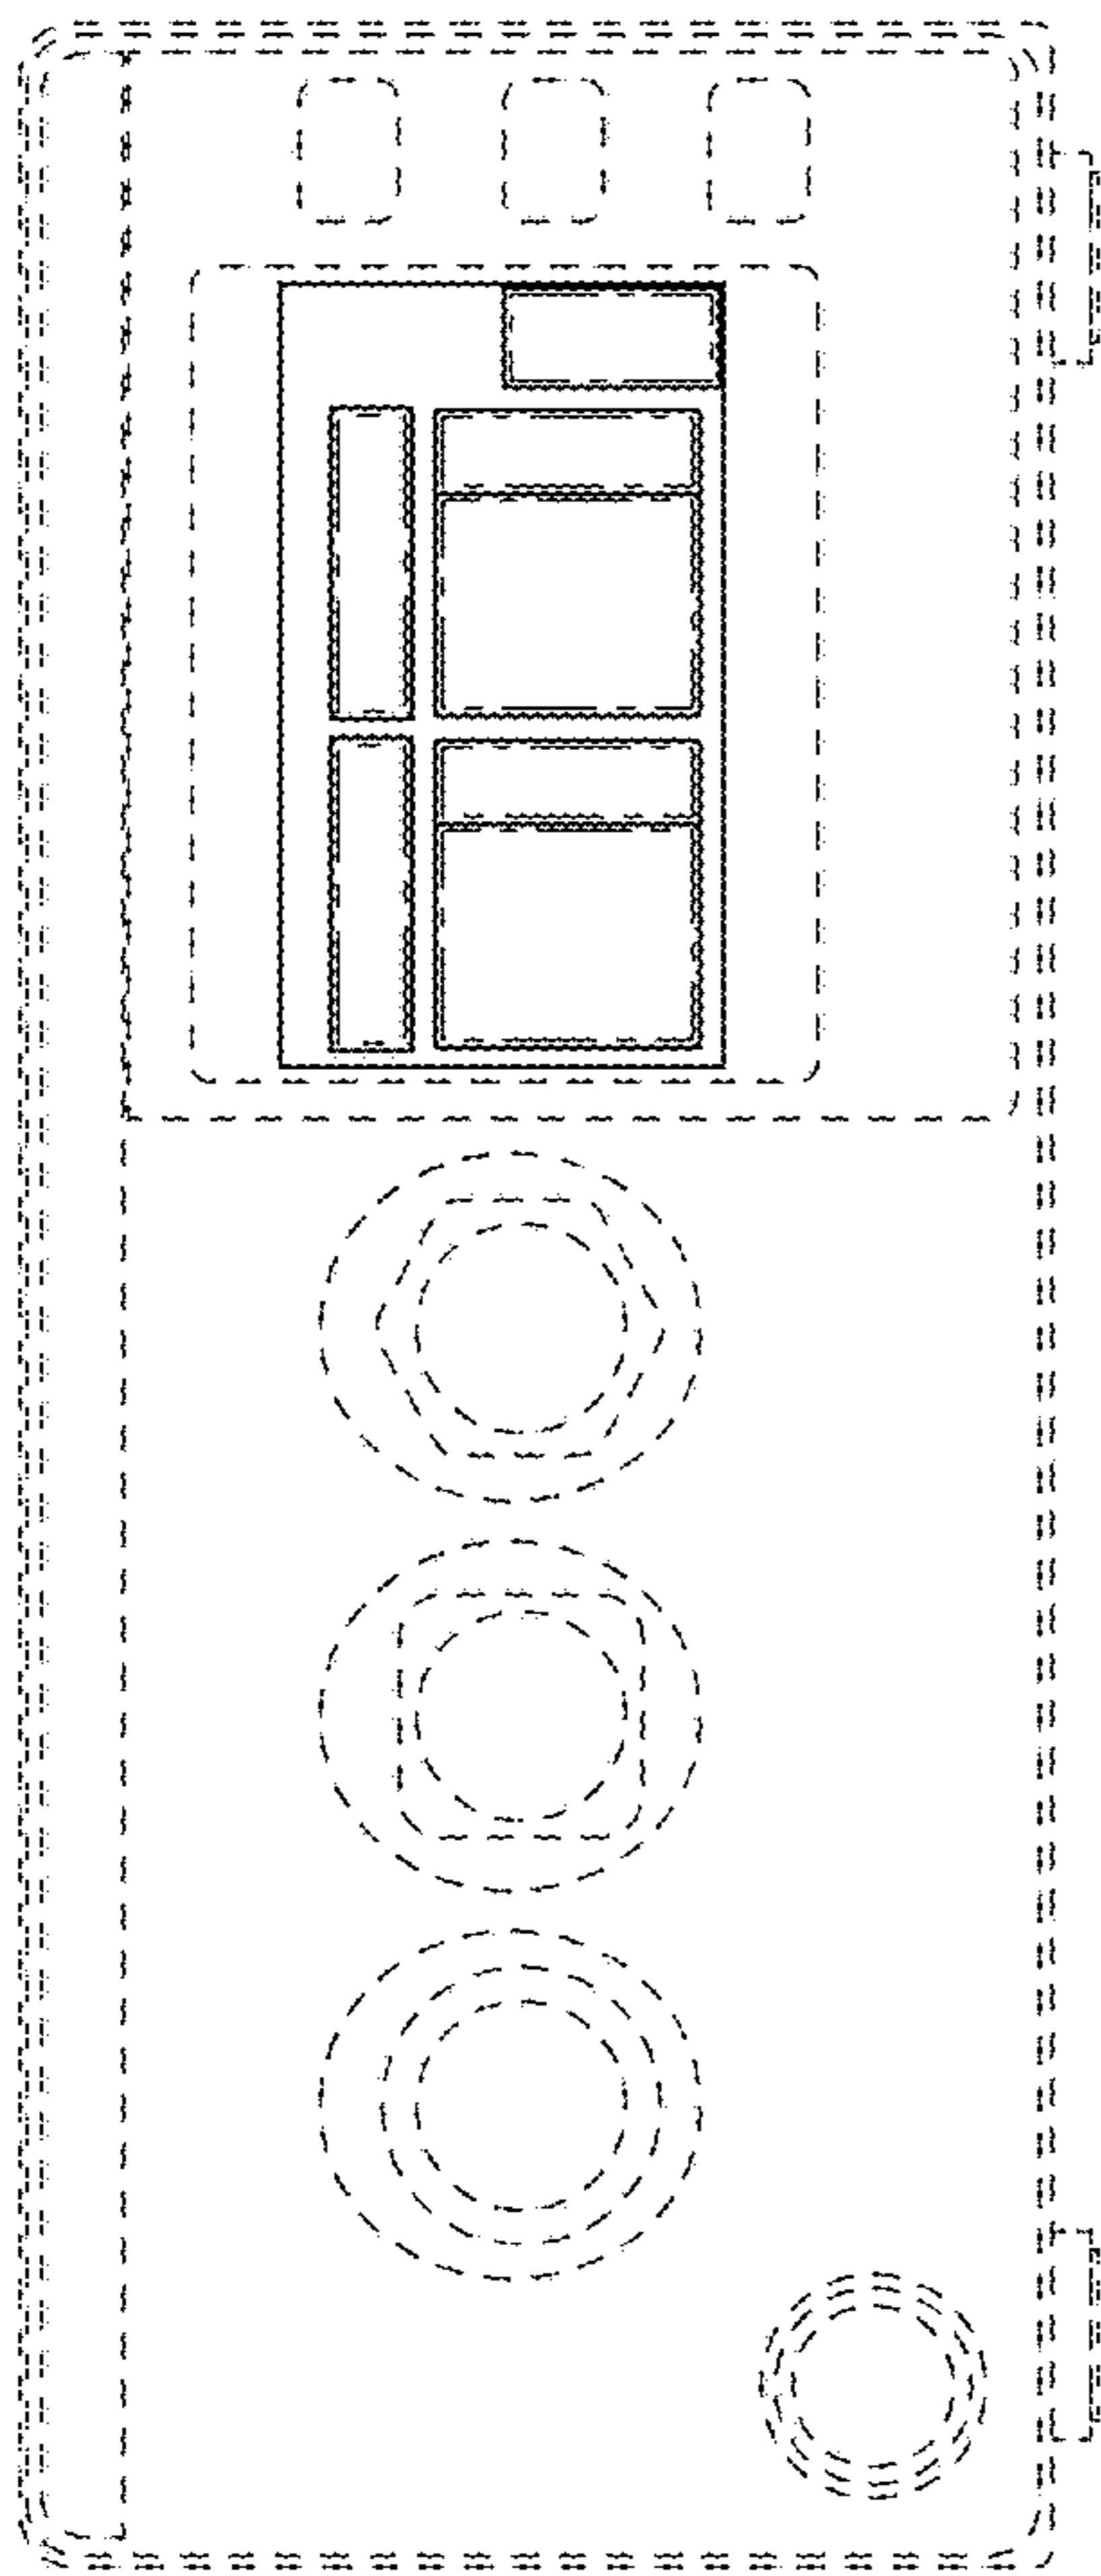


Fig. 1

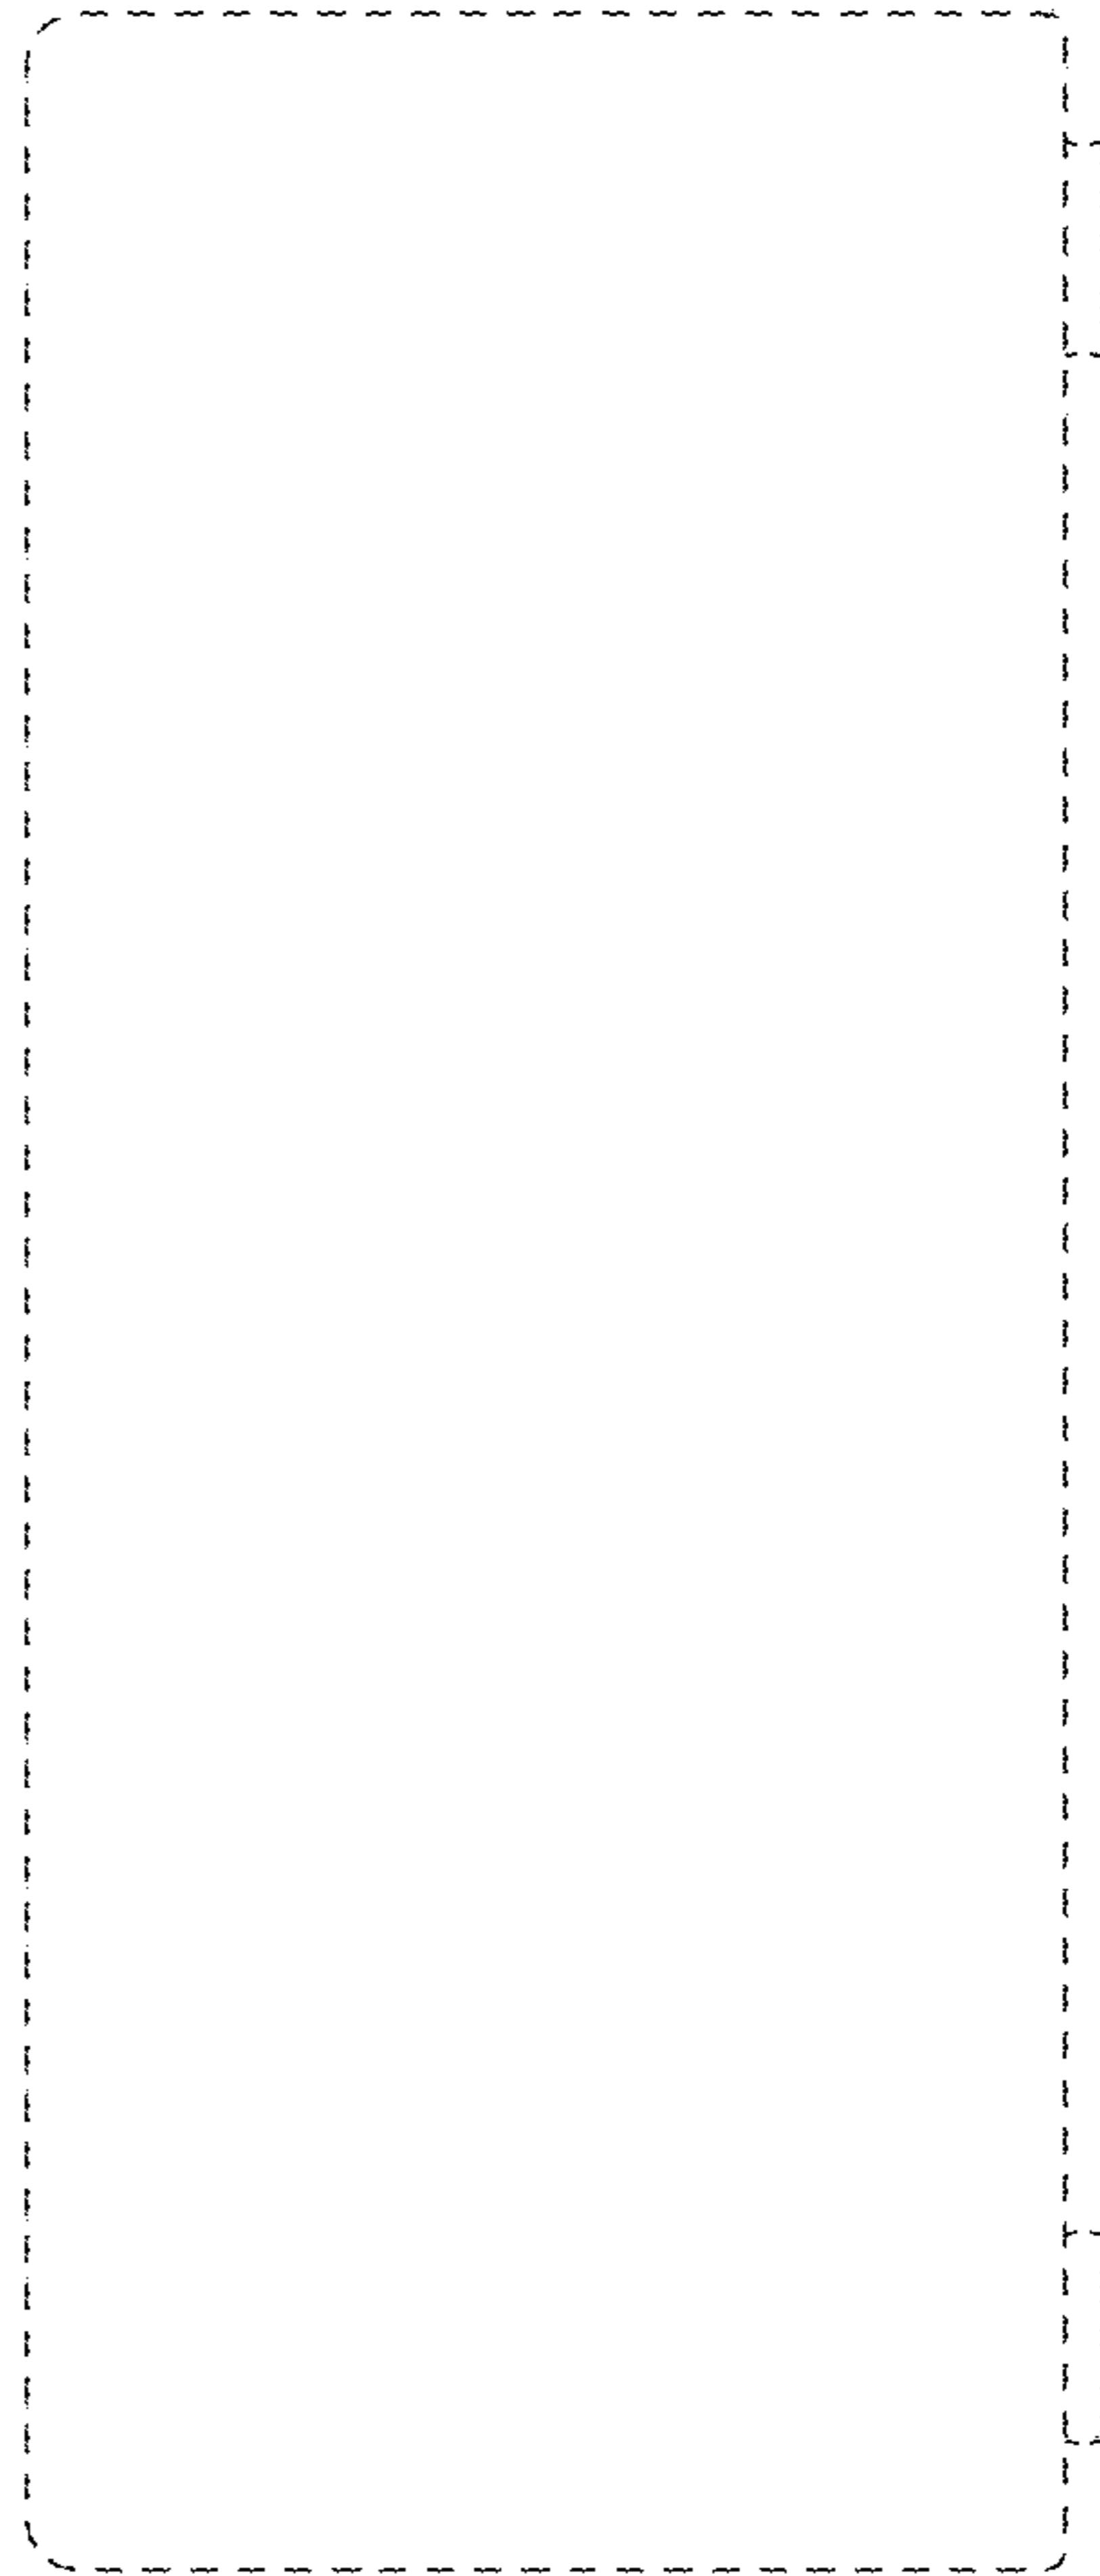


Fig. 2

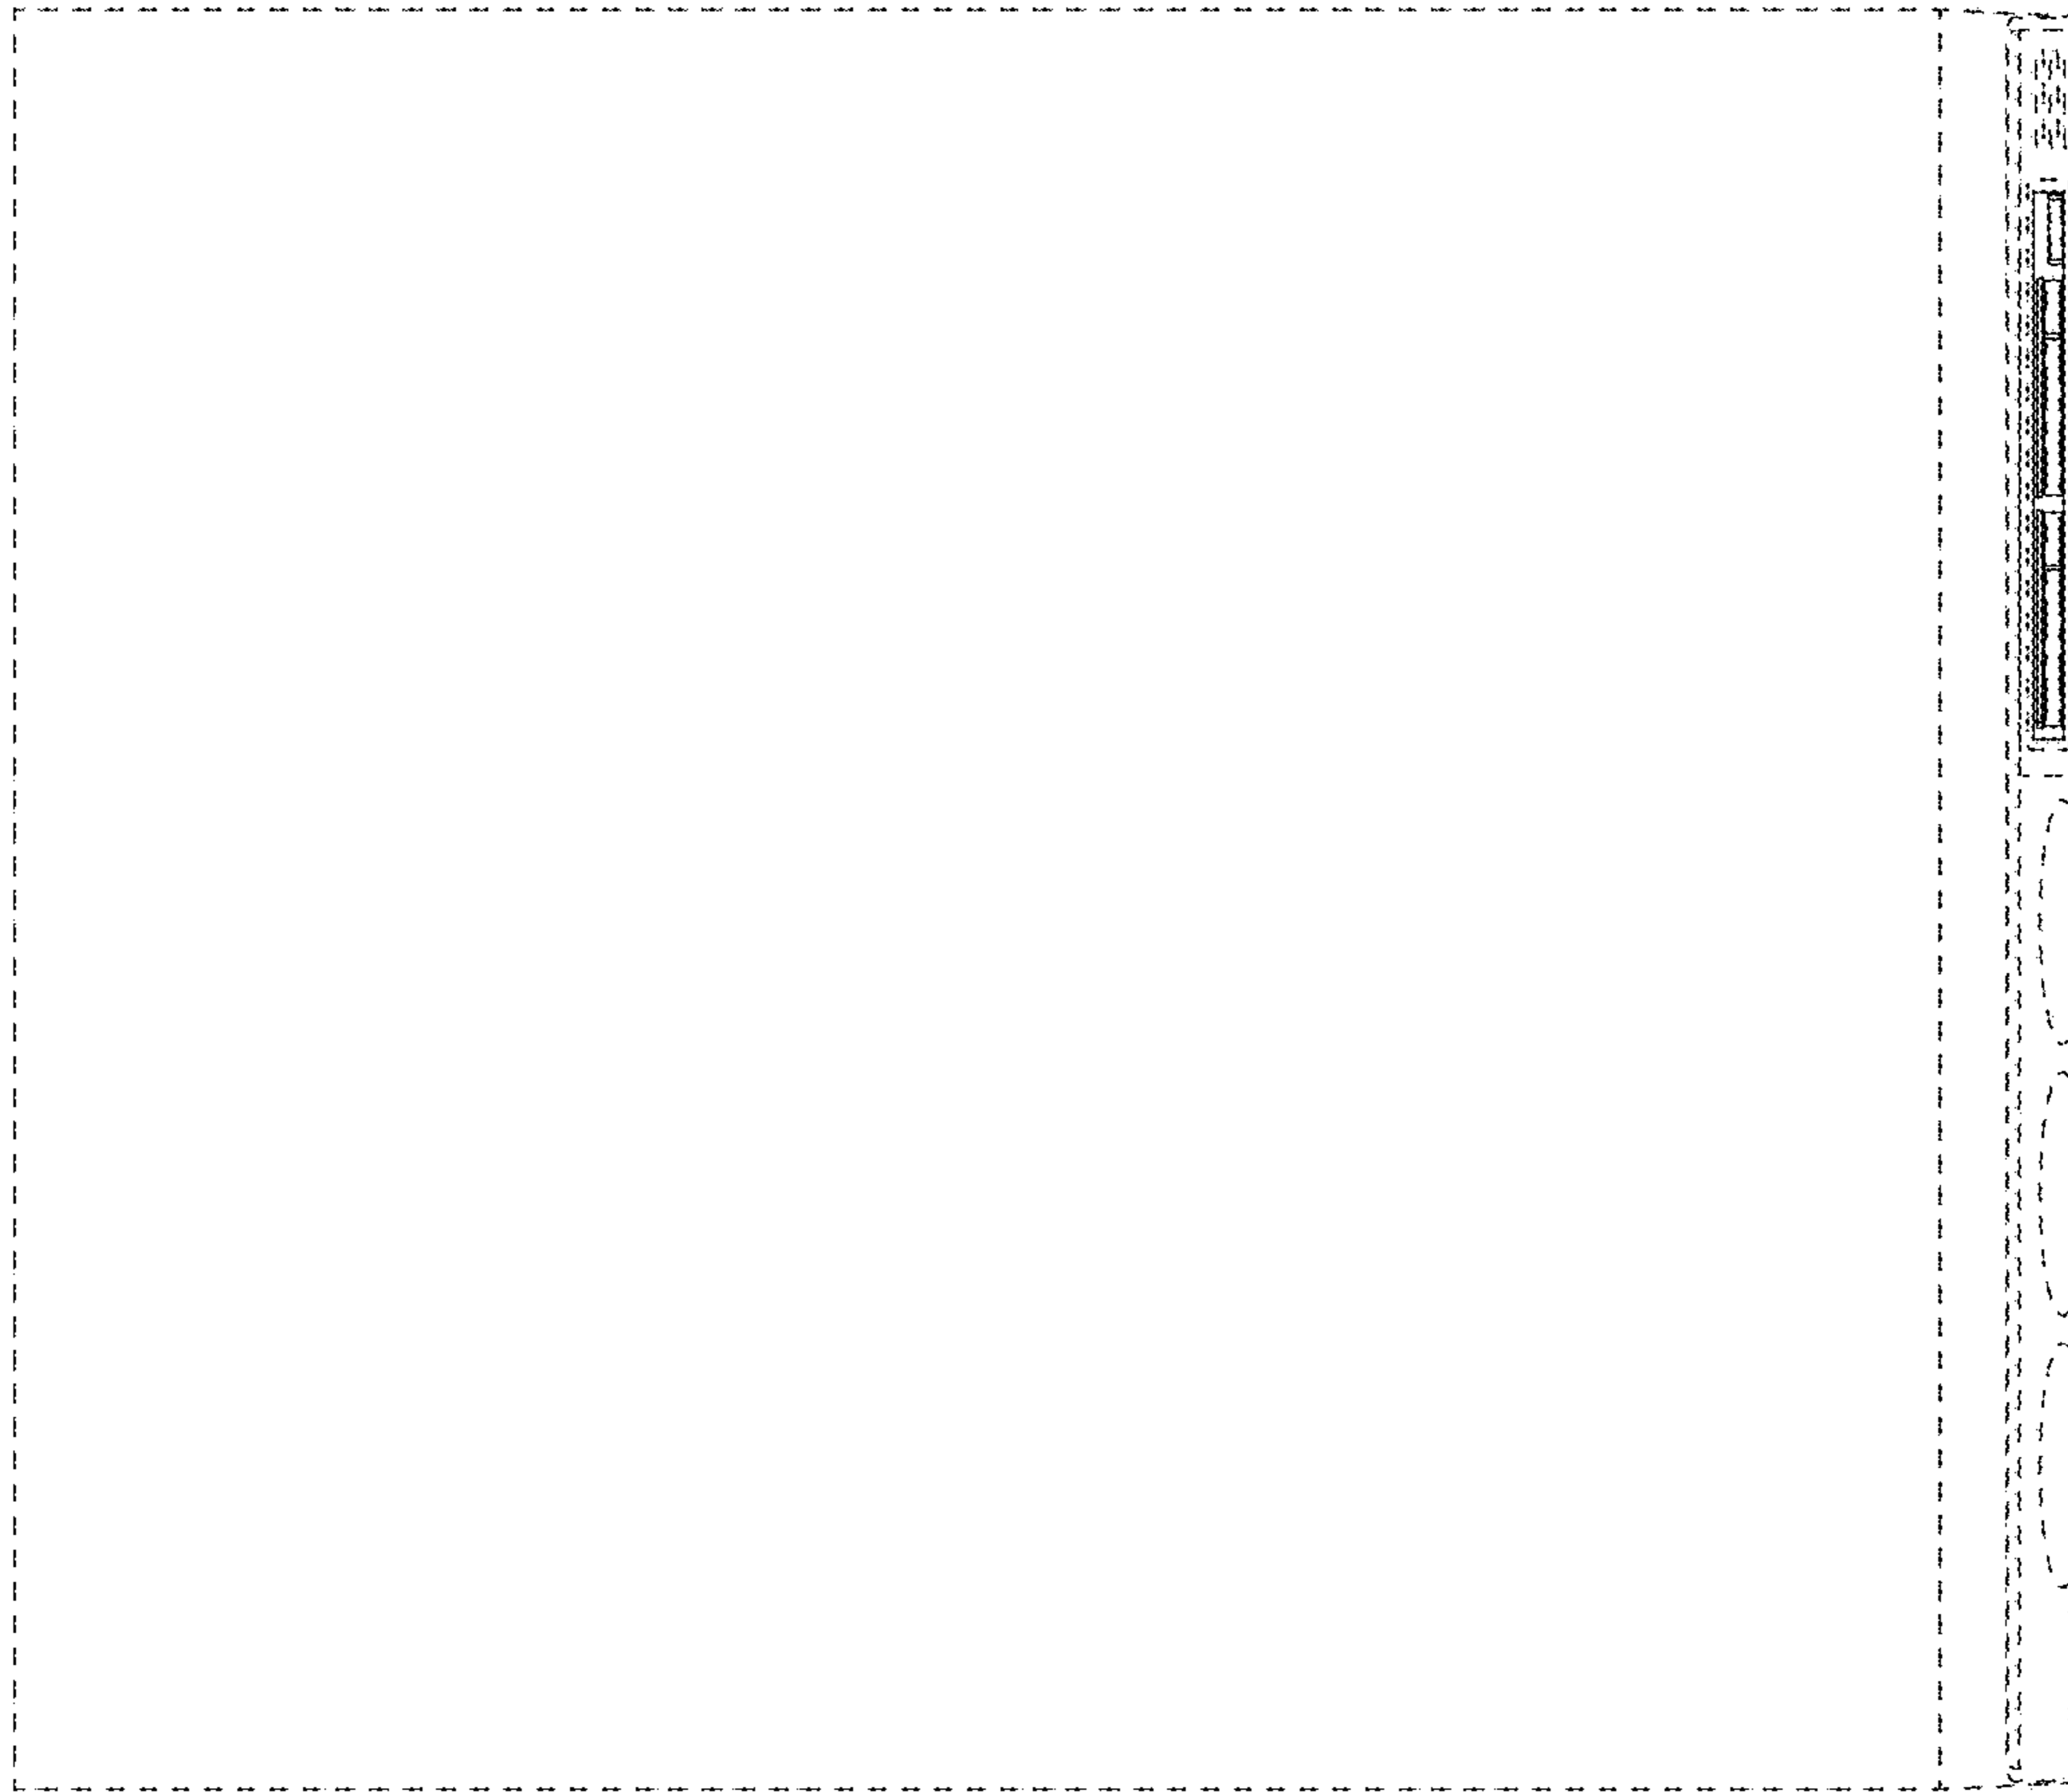


Fig. 3

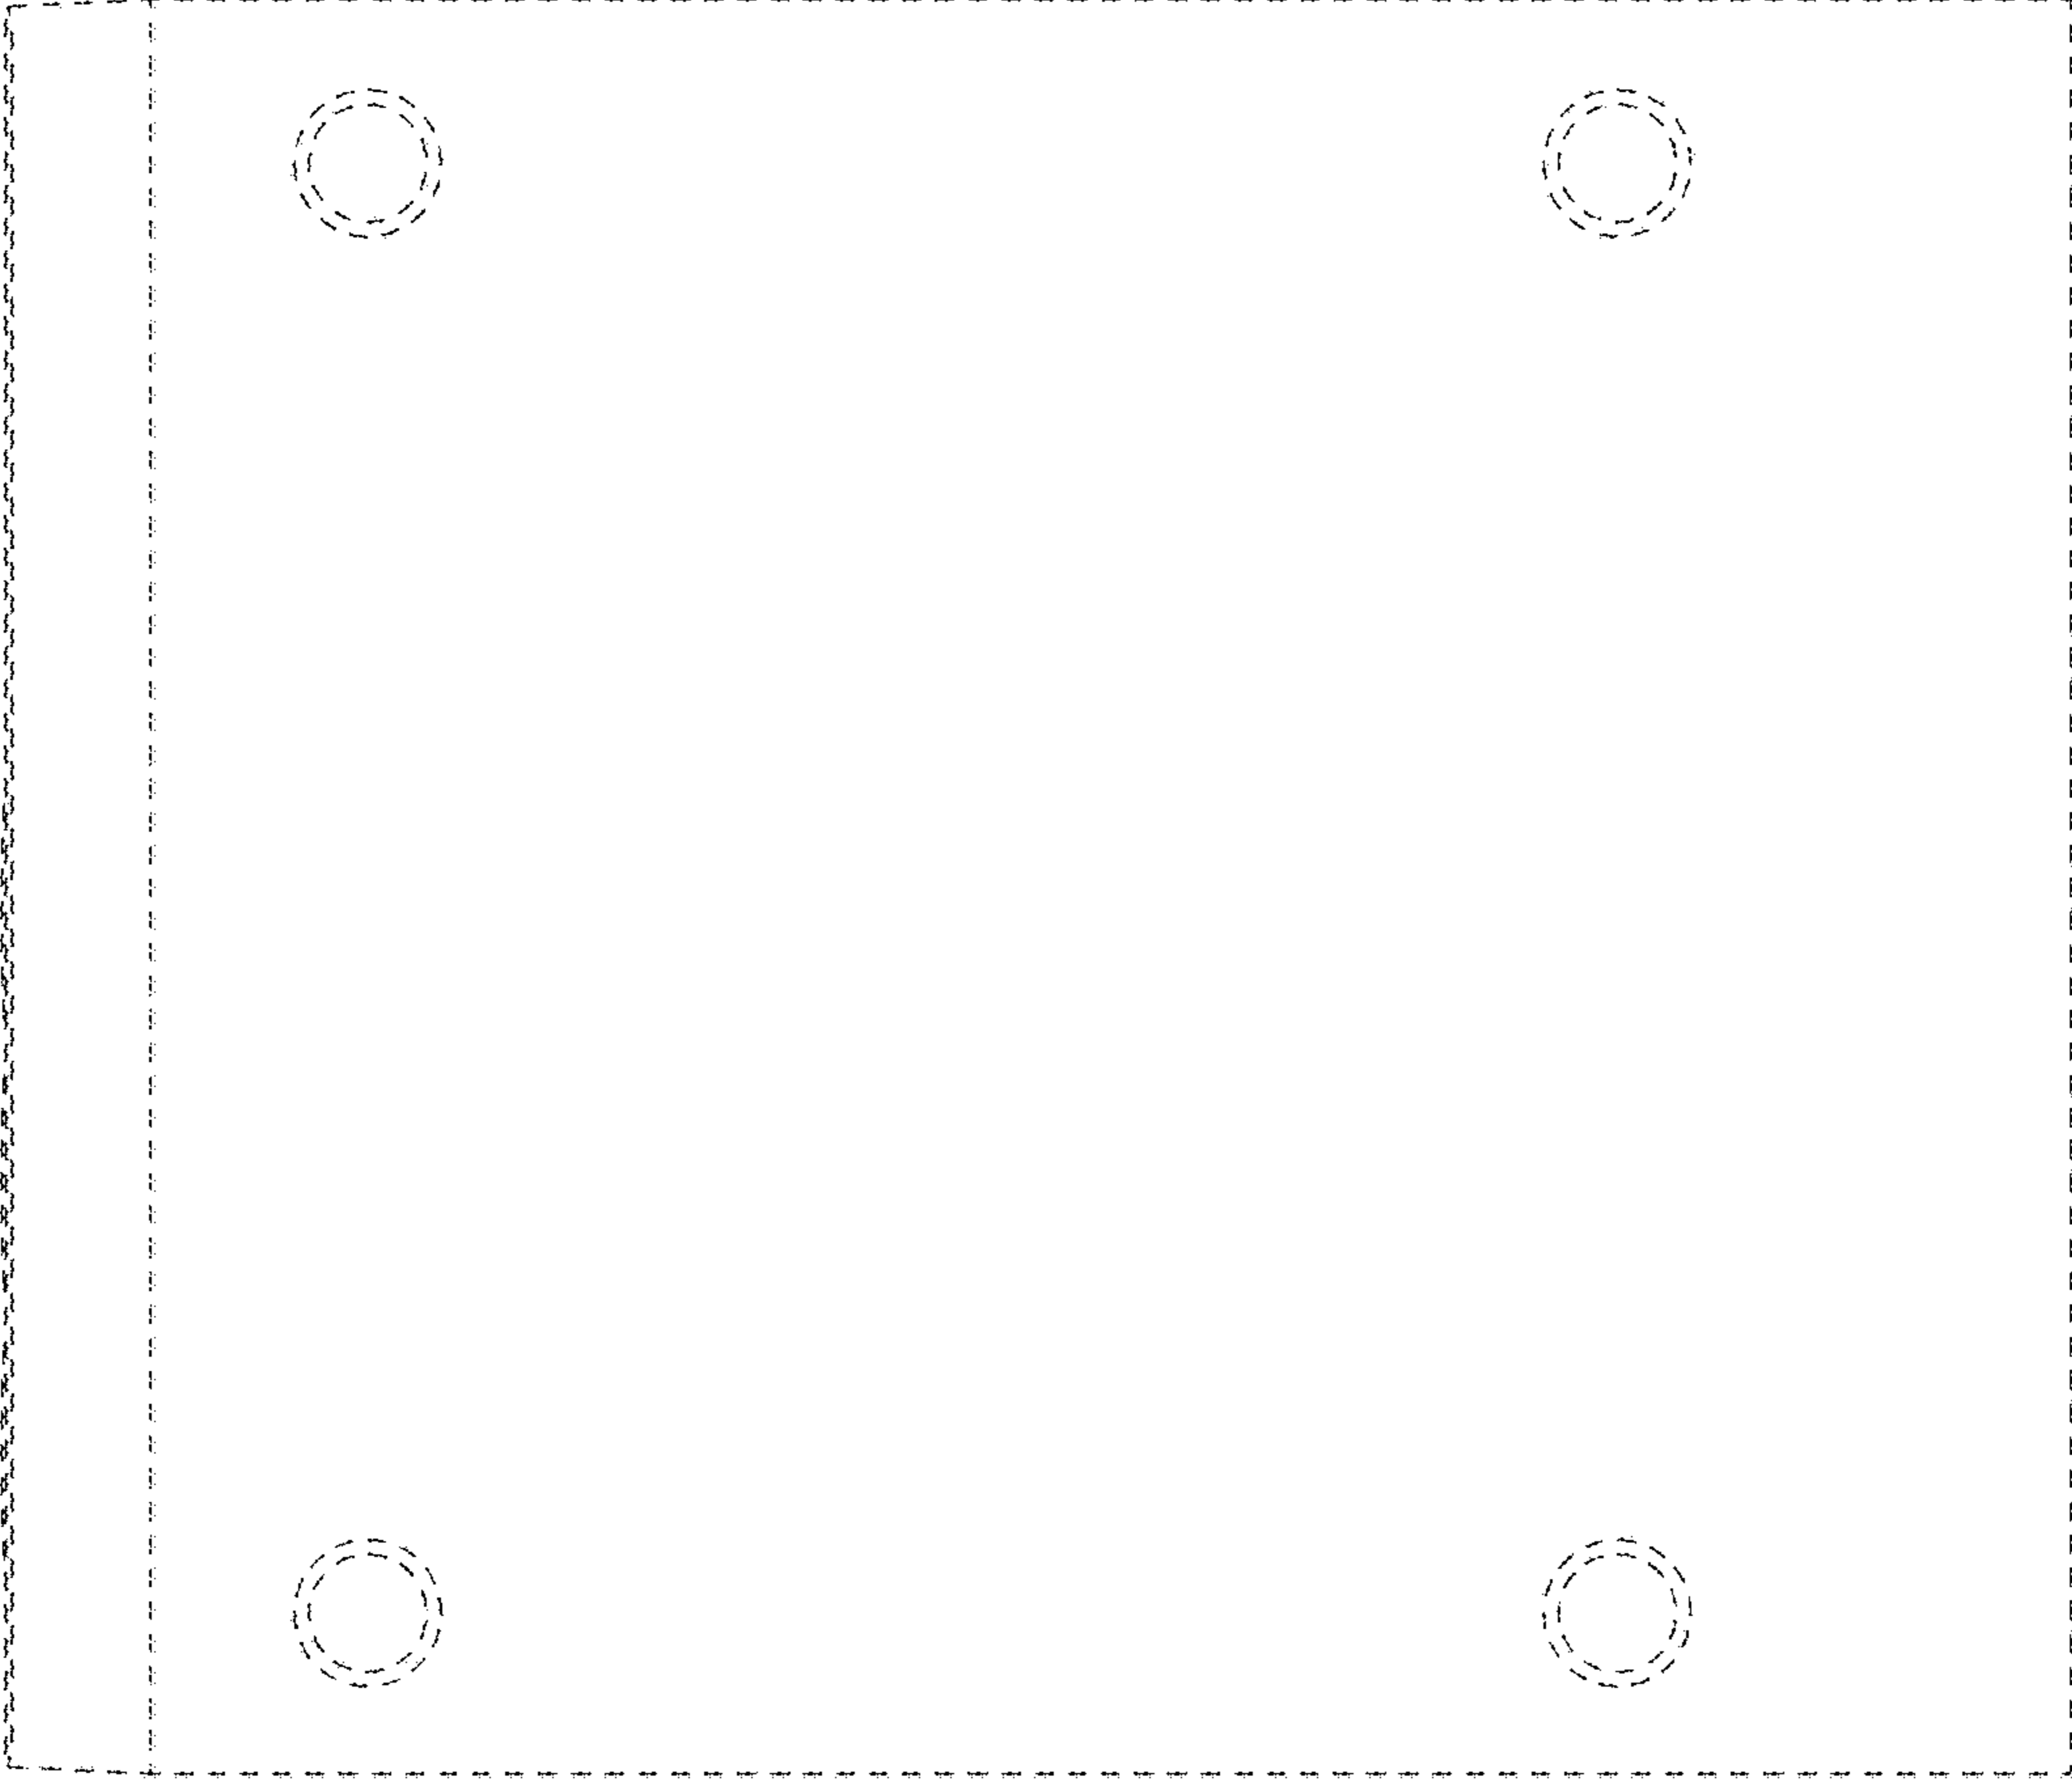


Fig. 4

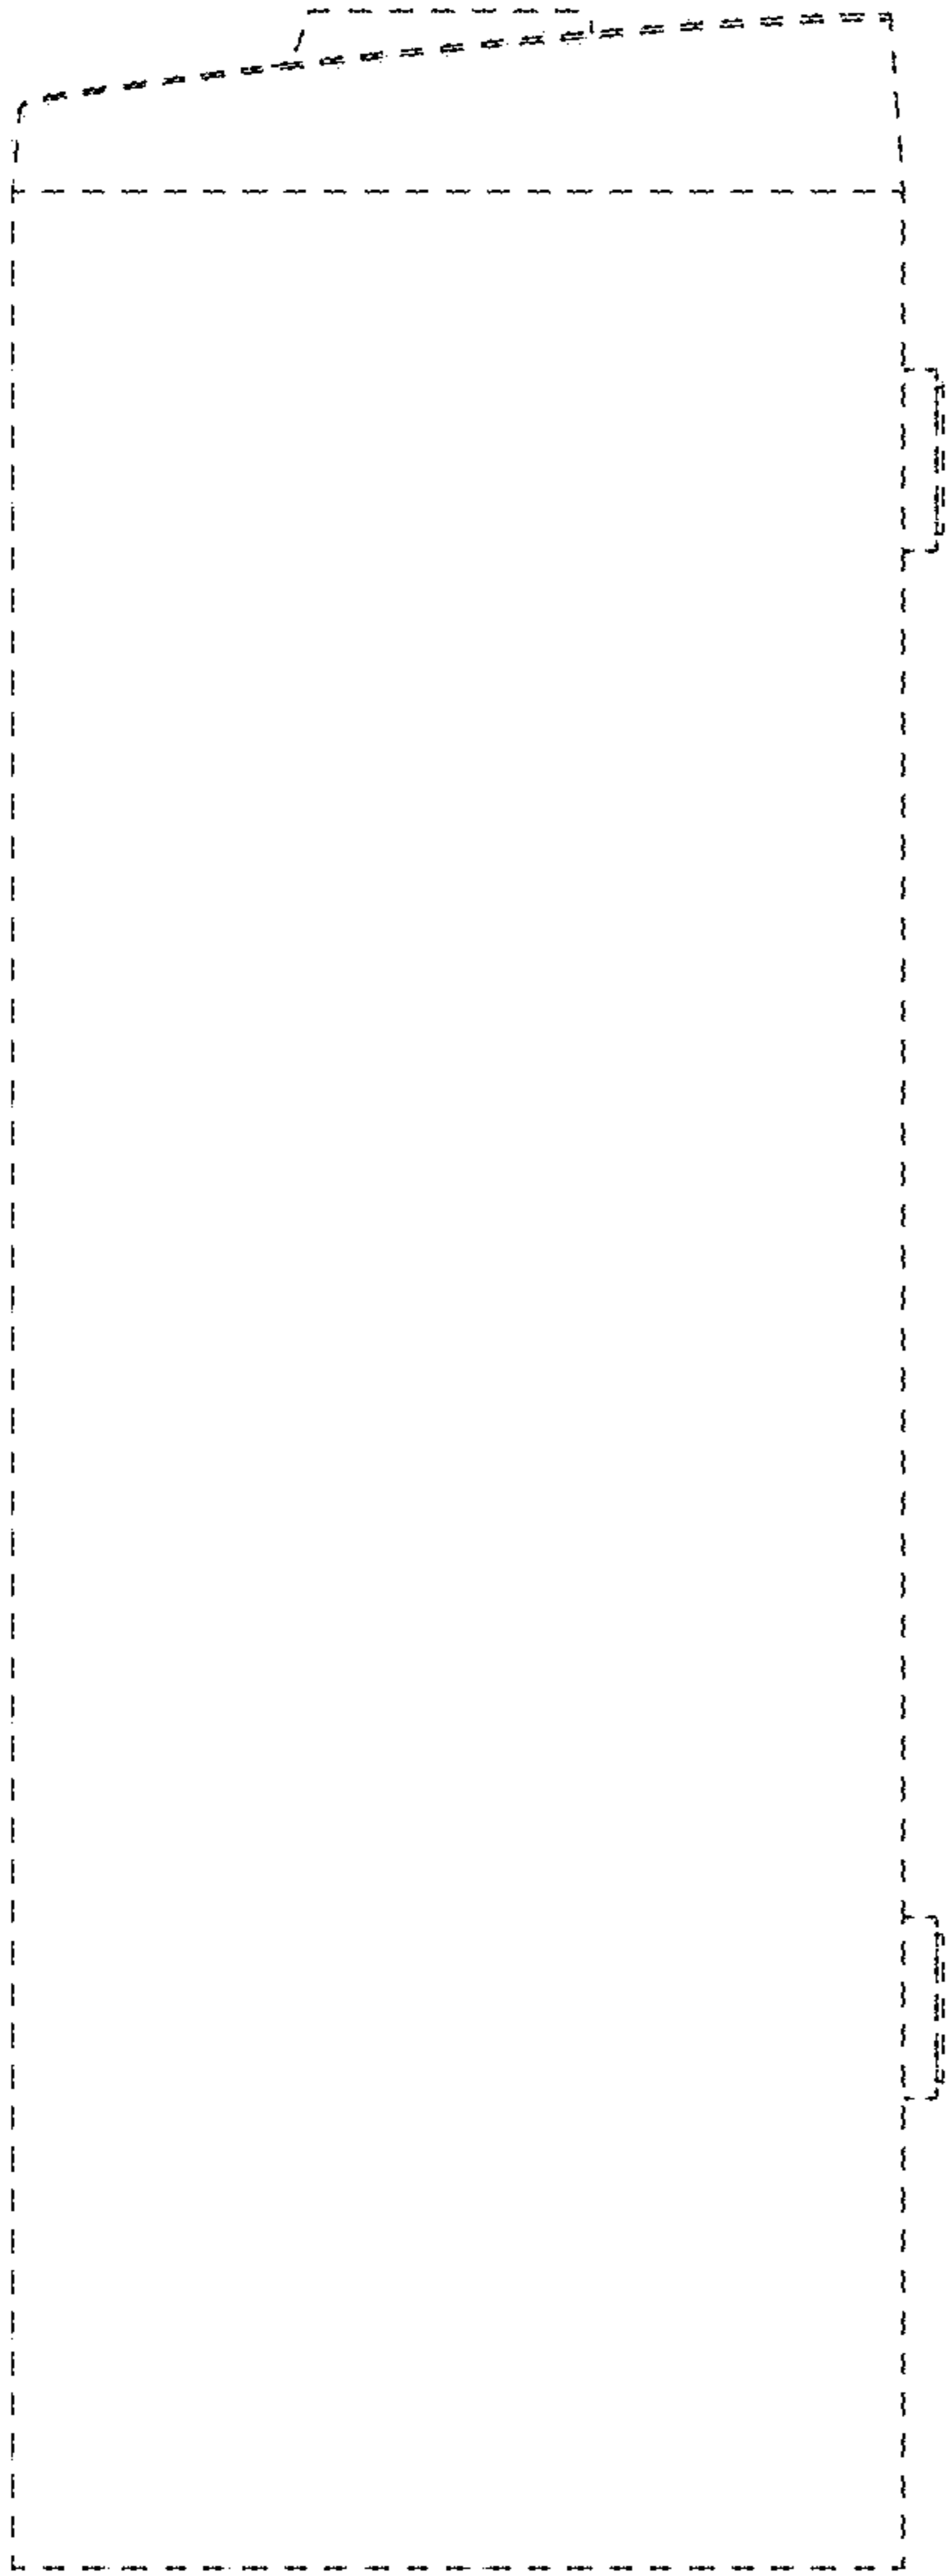


Fig. 5

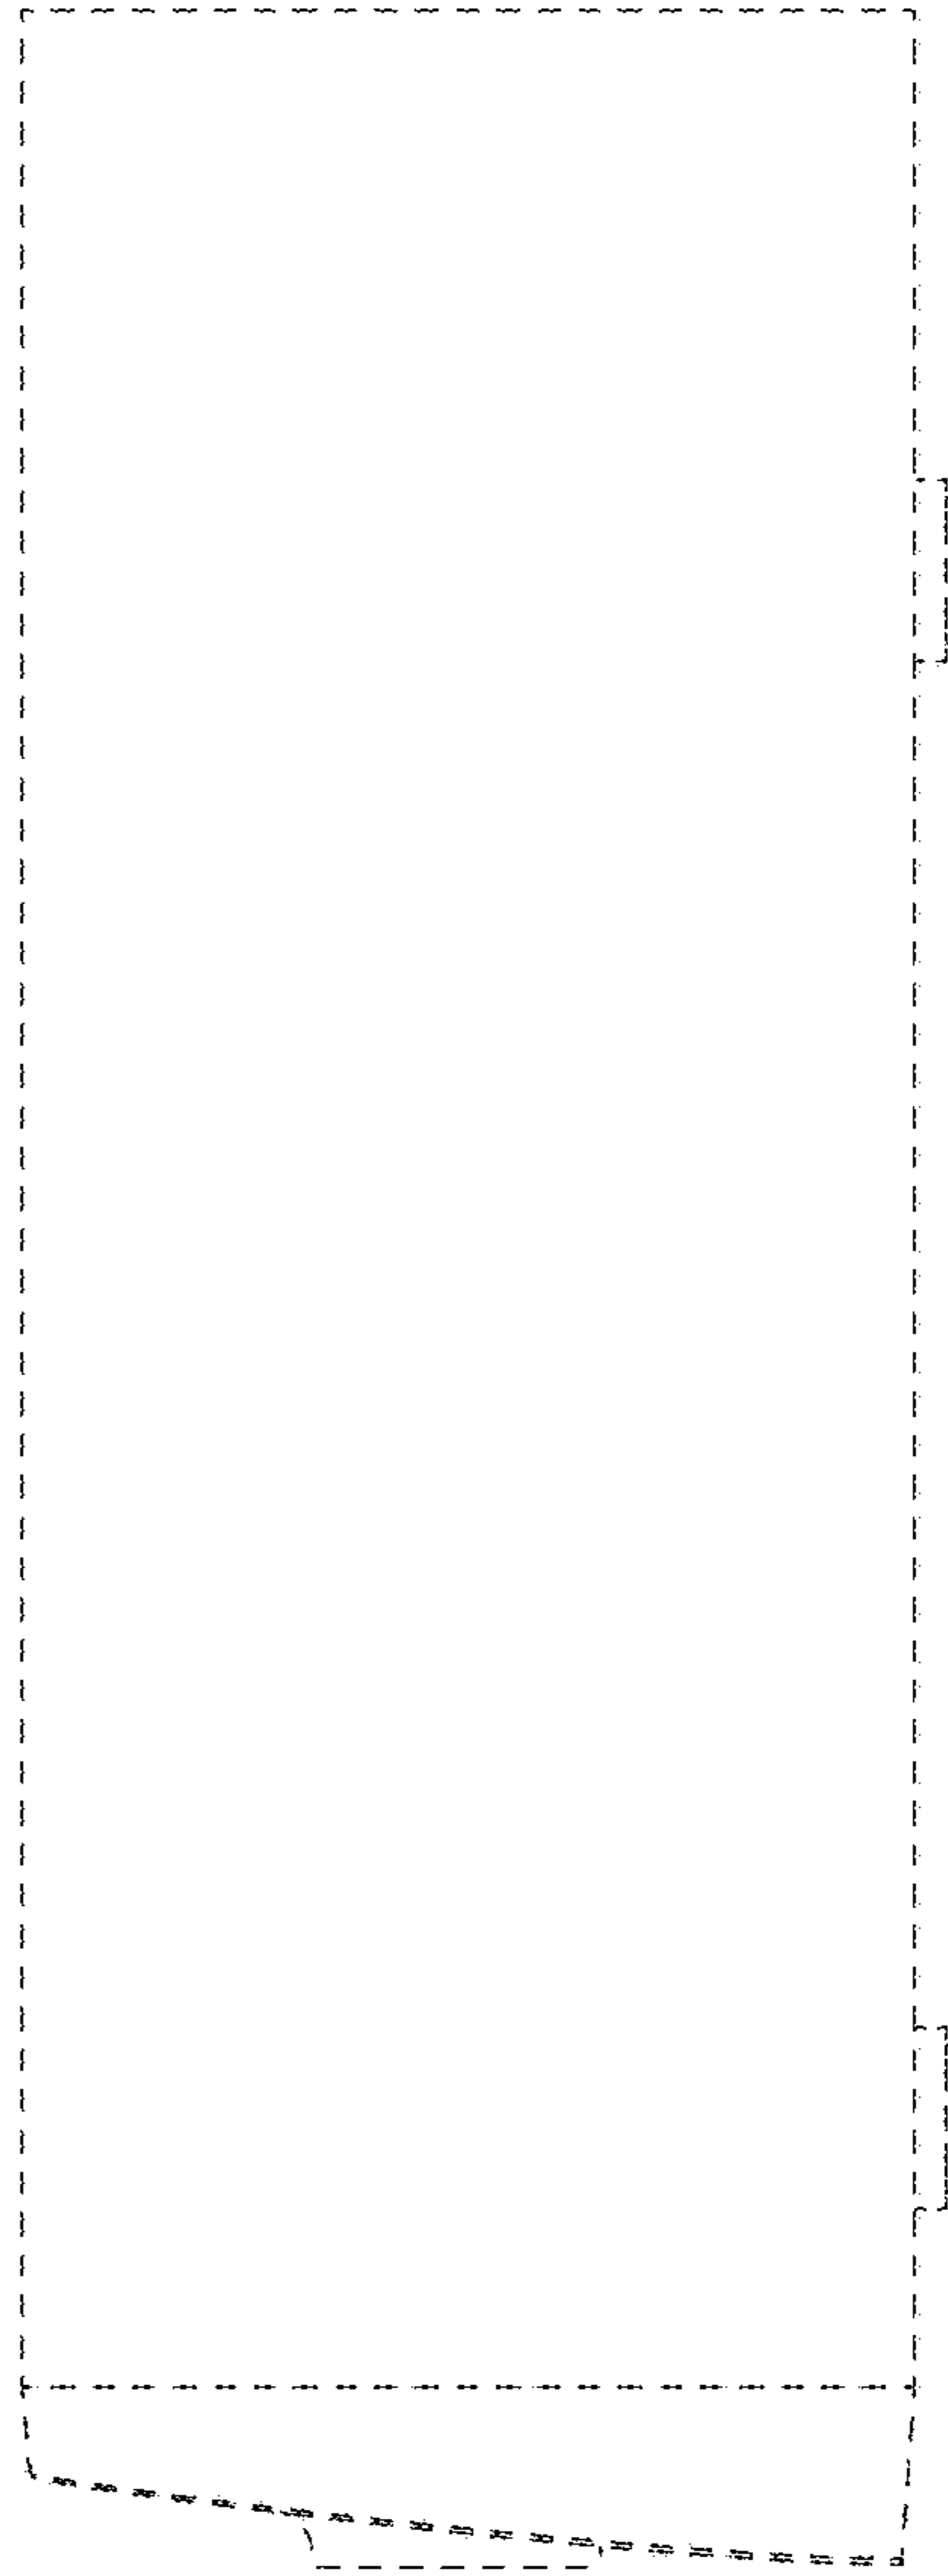


Fig. 6

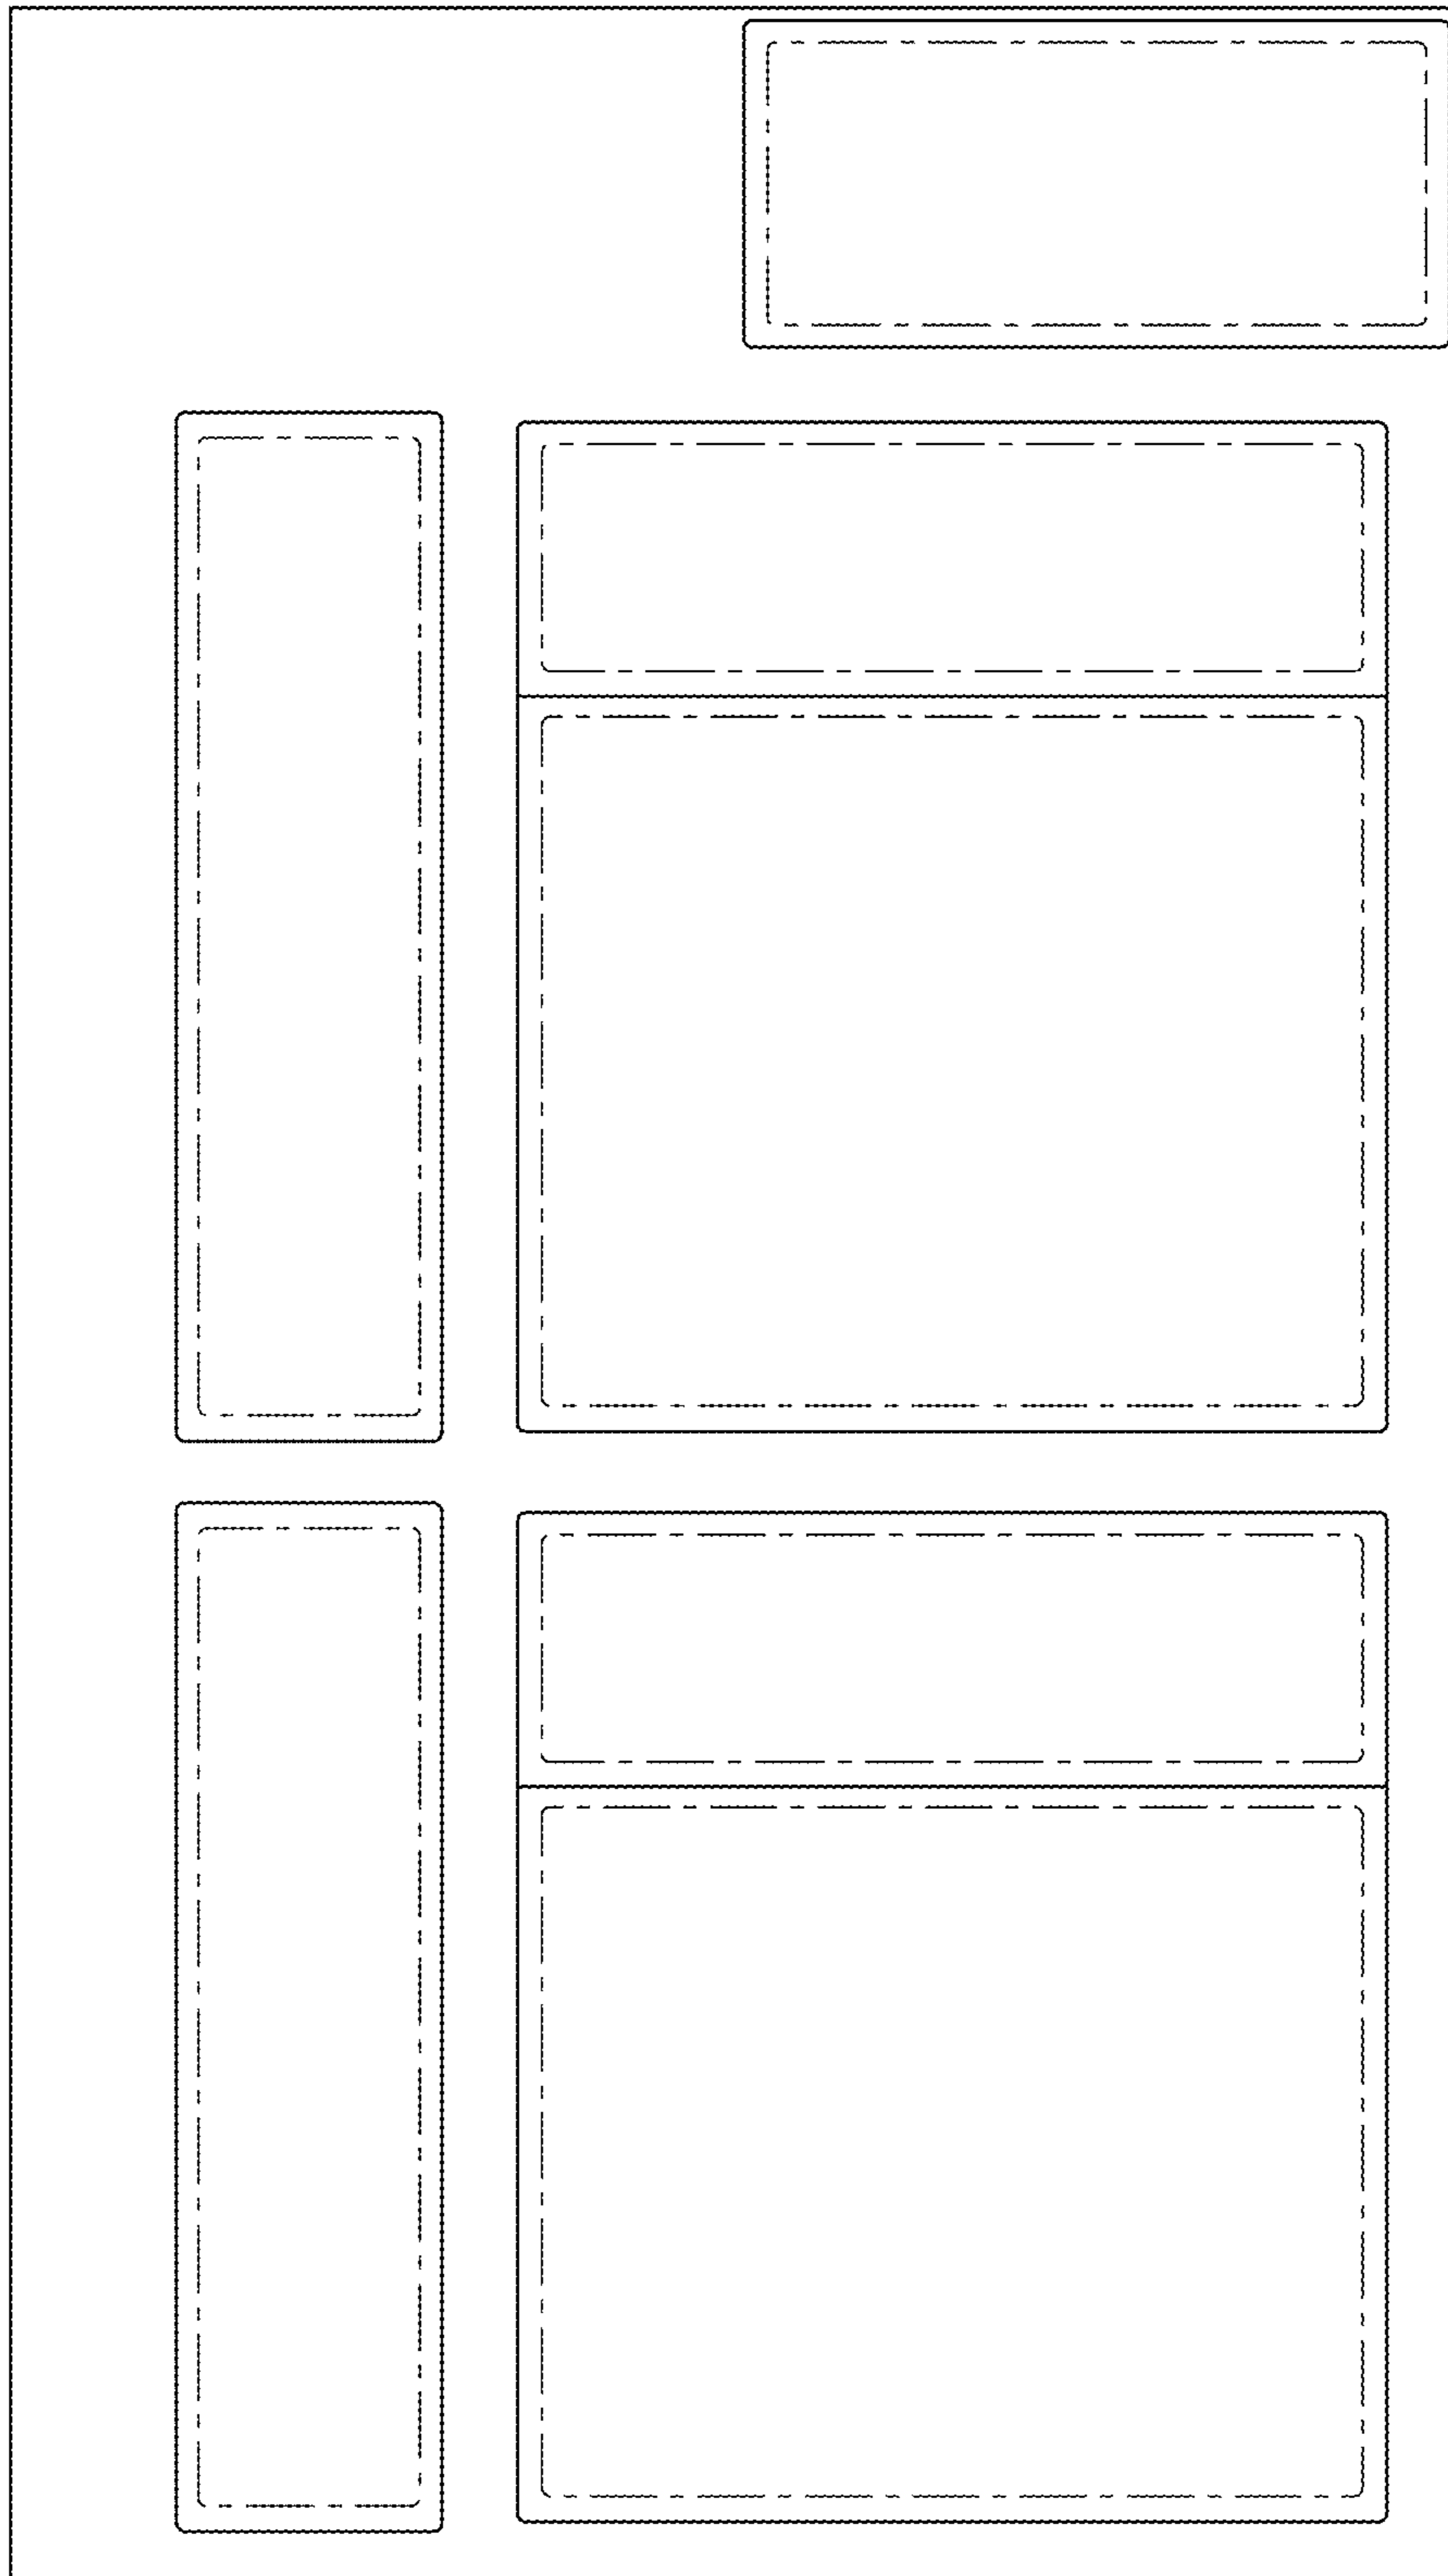


Fig. 7