



US00D869664S

(12) **United States Design Patent** (10) **Patent No.:** **US D869,664 S**
de Jonge et al. (45) **Date of Patent:** **** Dec. 10, 2019**

(54) **ULTRASOUND PROBE**
(71) Applicant: **Butterfly Network, Inc.**, Guilford, CT (US)
(72) Inventors: **Matthew de Jonge**, New York, NY (US); **Christopher Thomas McNulty**, Guilford, CT (US); **David Elgena**, Brooklyn, NY (US); **Stephen Christopher**, Philadelphia, PA (US); **Paul Maxted**, Guilford, CT (US); **Jonathan C. Schultz**, Guilford, CT (US); **Benjamin Chopra**, Guilford, CT (US)

D703,821 S * 4/2014 Moon D24/187
D704,844 S 5/2014 Saeki
9,072,487 B2 7/2015 Hebrard et al.
D745,175 S 12/2015 Kitayama
D749,224 S * 2/2016 Iritani D24/187
(Continued)

FOREIGN PATENT DOCUMENTS

JP D1457814 12/2012
JP D1515349 1/2015
(Continued)

OTHER PUBLICATIONS

[No Author Listed], HDI 5000 Transducer Listing, Publically known prior to Oct. 27, 2017, 6 pages.
(Continued)

(73) Assignee: **Butterfly Network, Inc.**, Guilford, CT (US)
(**) Term: **15 Years**
(21) Appl. No.: **29/677,068**
(22) Filed: **Jan. 16, 2019**

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Wolf, Greenfield & Sacks, P.C.

Related U.S. Application Data

(62) Division of application No. 29/623,977, filed on Oct. 27, 2017, now Pat. No. Des. 846,749.
(51) **LOC (12) Cl.** **24-01**
(52) **U.S. Cl.**
USPC **D24/187**
(58) **Field of Classification Search**
USPC D24/152, 158, 160, 161, 186, 187, 231;
D10/78; D14/420, 426
CPC A61B 8/445; A61B 8/4455; A61B 8/4461
See application file for complete search history.

(57) **CLAIM**

The ornamental design for an ultrasound probe, as shown and described.


DESCRIPTION

FIG. 1 is a bottom, rear, left side perspective view of an ultrasound probe showing our new design;
FIG. 2 is a front elevation view thereof;
FIG. 3 is a rear elevation view thereof;
FIG. 4 is a left side elevation view thereof;
FIG. 5 is a right side elevation view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The dot-dash broken lines in the figures represent boundaries of the claimed design and form no part thereof. All other broken lines illustrate portions of the ultrasound probe that form no part of the claimed design.

(56) **References Cited**
U.S. PATENT DOCUMENTS

D545,433 S 6/2007 Messerly et al.
D681,824 S 5/2013 Shinohara et al.
D703,332 S * 4/2014 Saeki D24/187

1 Claim, 4 Drawing Sheets

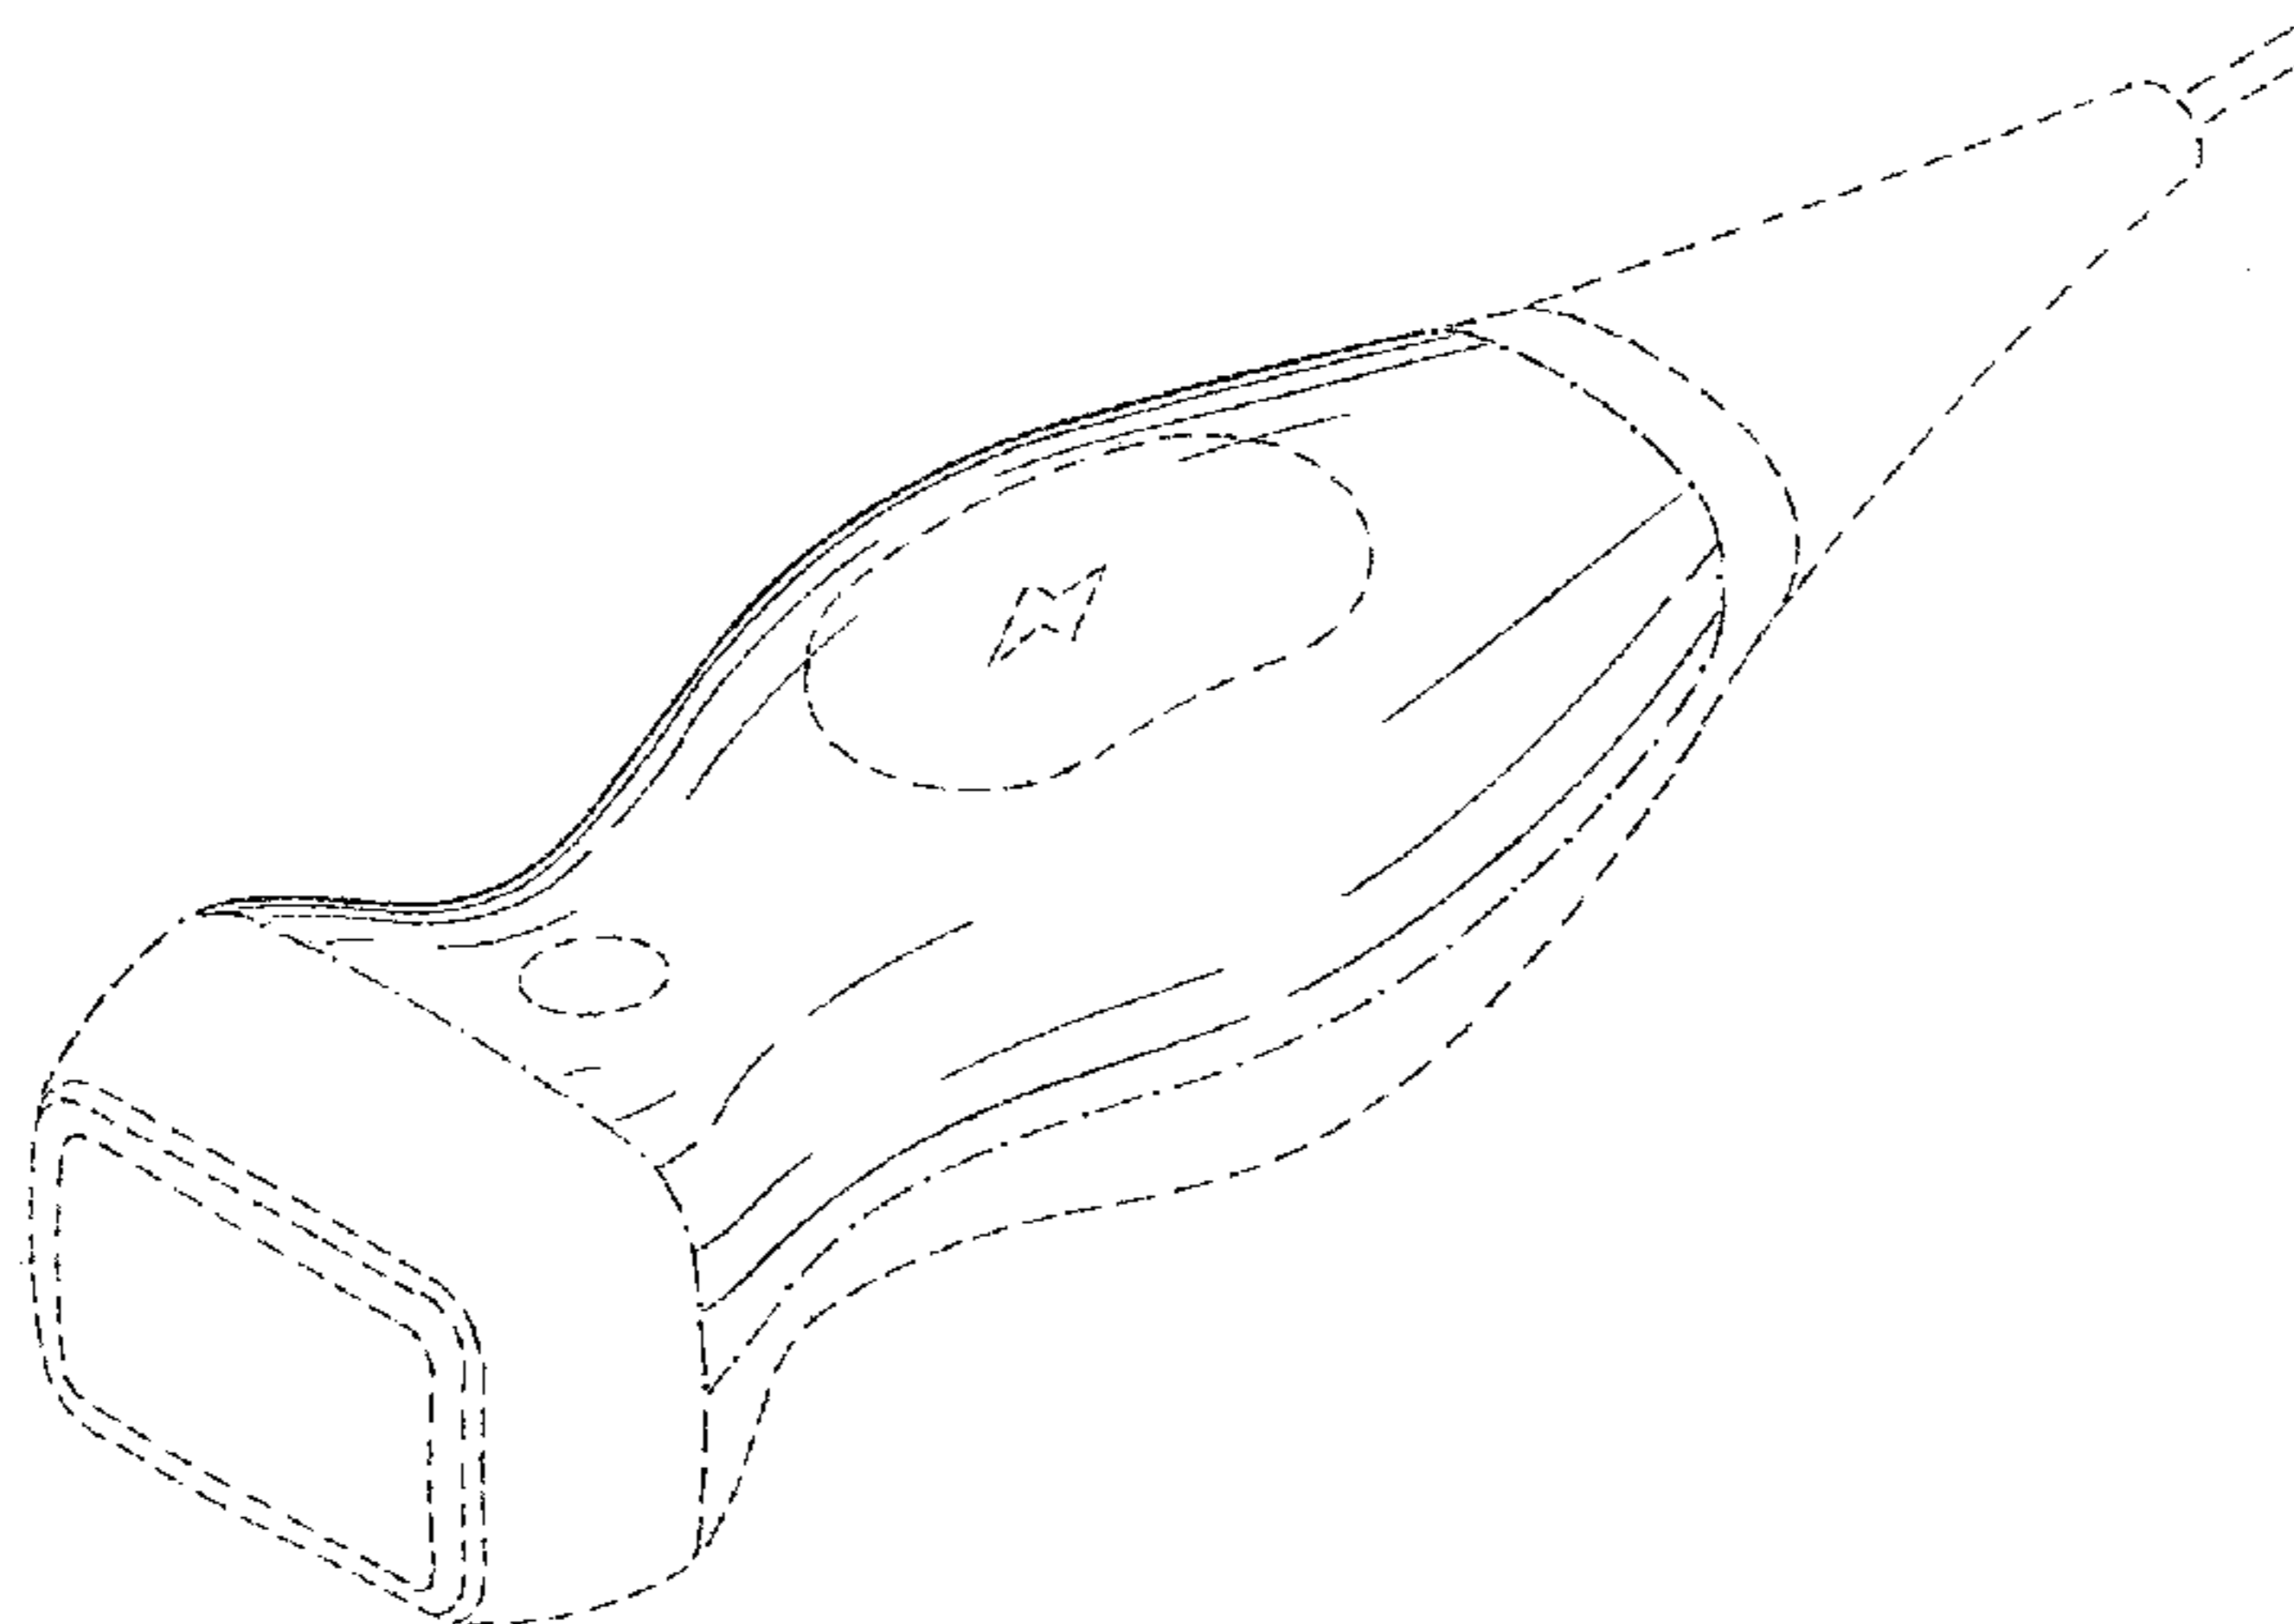

(56)

References Cited

U.S. PATENT DOCUMENTS

D816,850 S 5/2018 Asai et al.
D831,219 S * 10/2018 Henderson D24/187
D846,128 S * 4/2019 de Jonge D24/187
D846,749 S * 4/2019 de Jonge D24/187
2011/0055447 A1 3/2011 Costa
2015/0112200 A1 4/2015 Oberg et al.
2017/0172542 A1 6/2017 Lee et al.
2017/0360397 A1 12/2017 Rothberg et al.
2017/0360401 A1 12/2017 Rothberg et al.
2018/0028159 A1 2/2018 Hageman et al.

FOREIGN PATENT DOCUMENTS

JP D1564542 12/2016
KR 30-0726181 1/2014
KR 30-0726182 1/2014
KR 30-0751362 7/2014
KR 30-0764107 10/2014

OTHER PUBLICATIONS

Declaration of David Elgena, signed May 11, 2018, submitted to the Japanese Patent Office in co-pending application No. JP 2018-009209.

Enriquez et al., An Introduction to Ultrasound Equipment and Knobology. Crit Care Clin. Jan. 2014; 30(1):25-45.

* cited by examiner

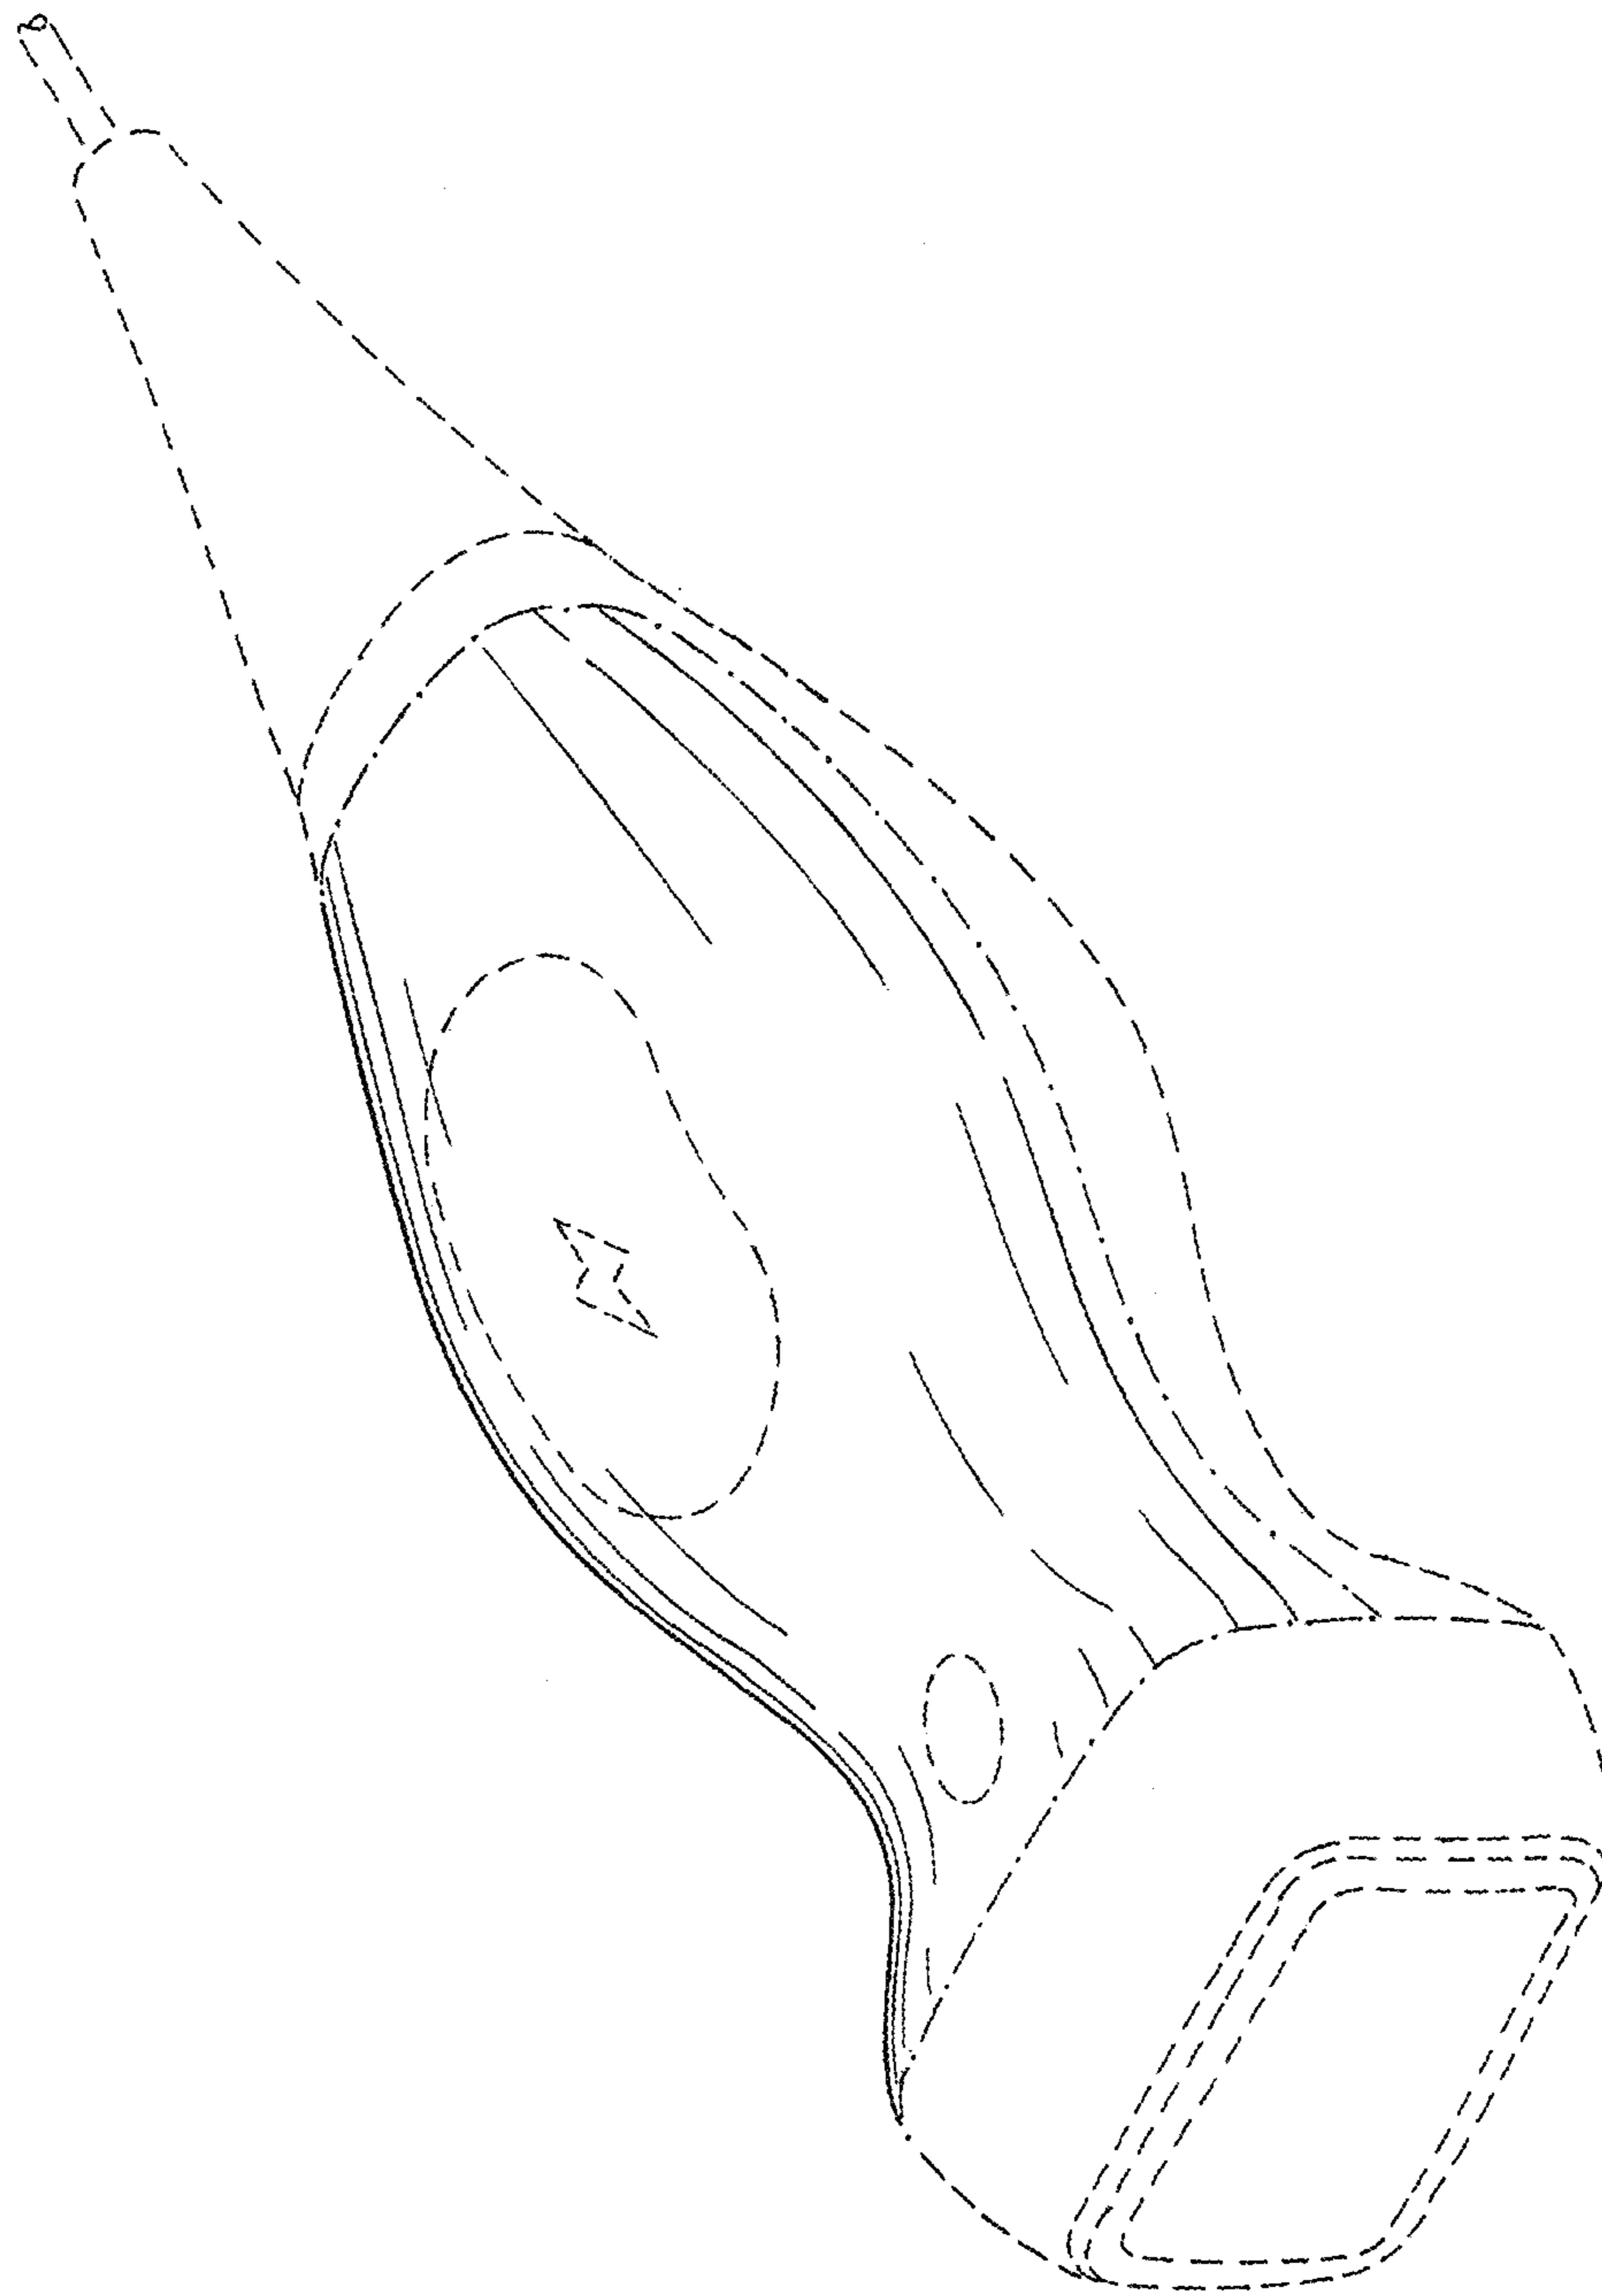


FIG. 1

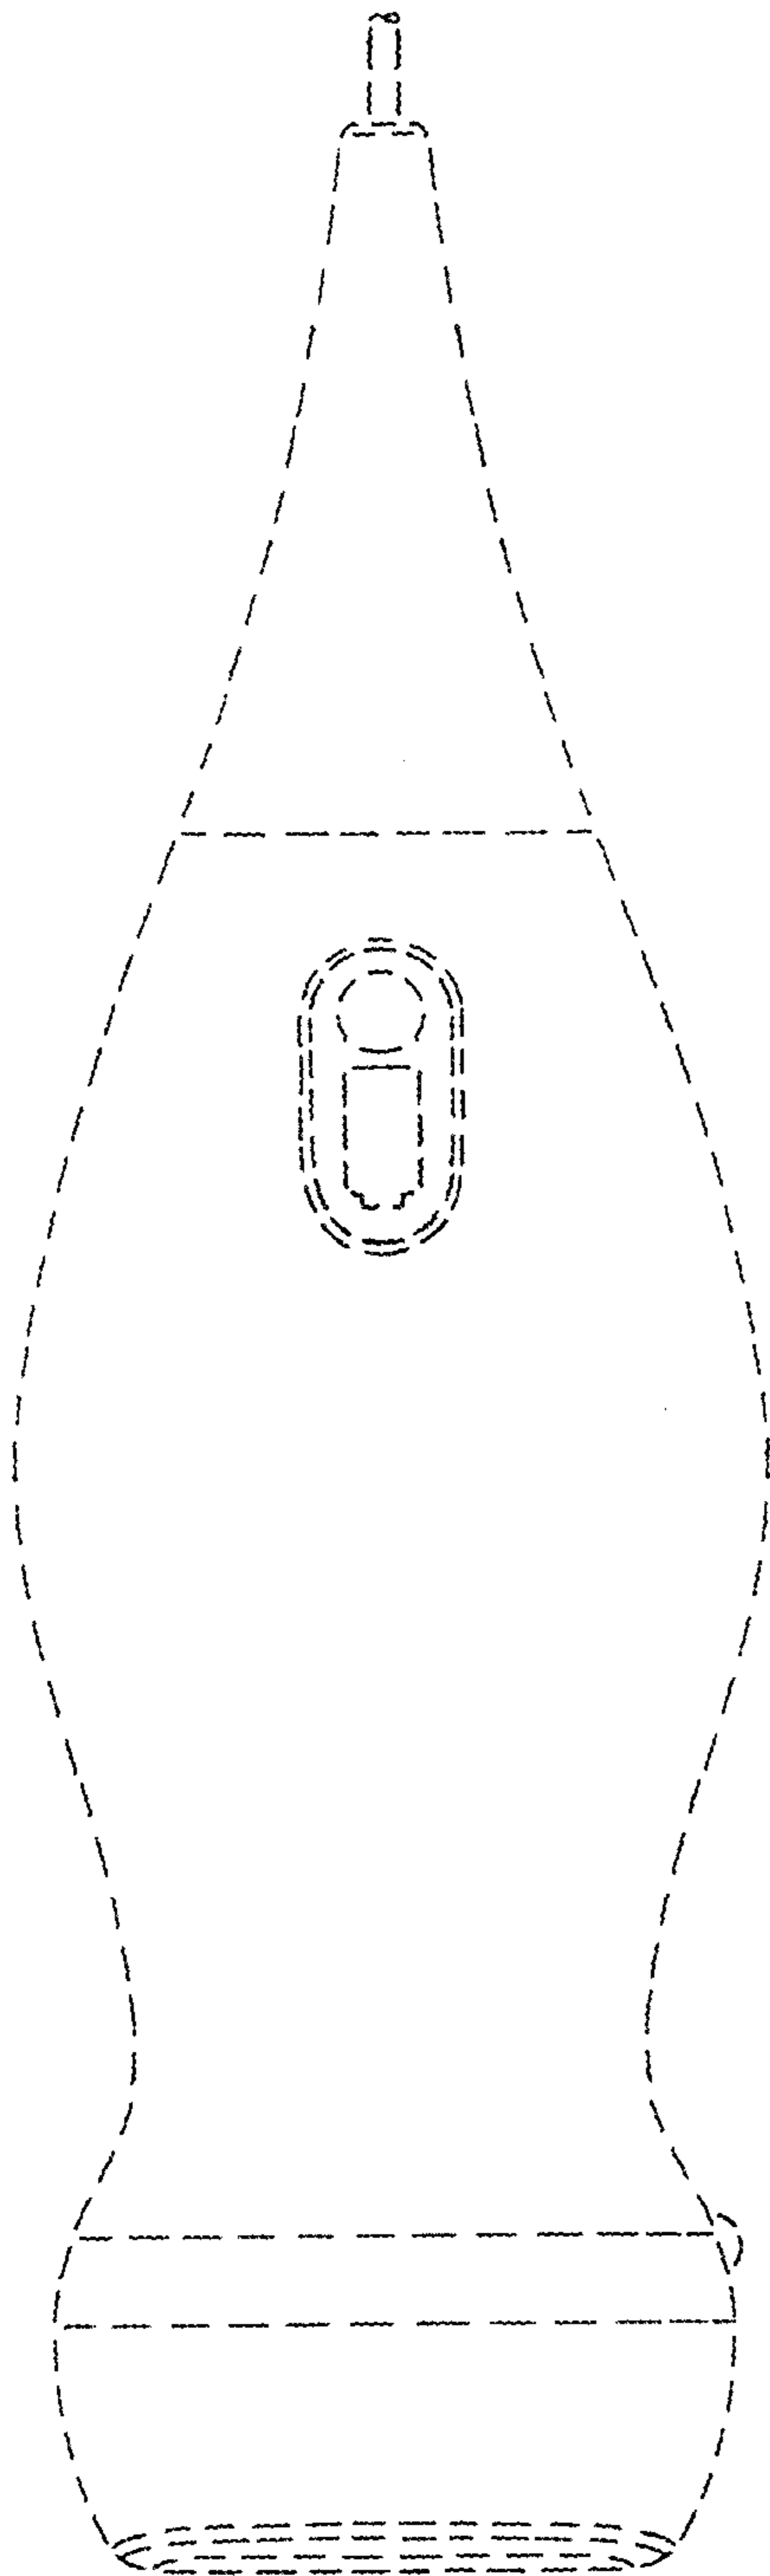


FIG. 2

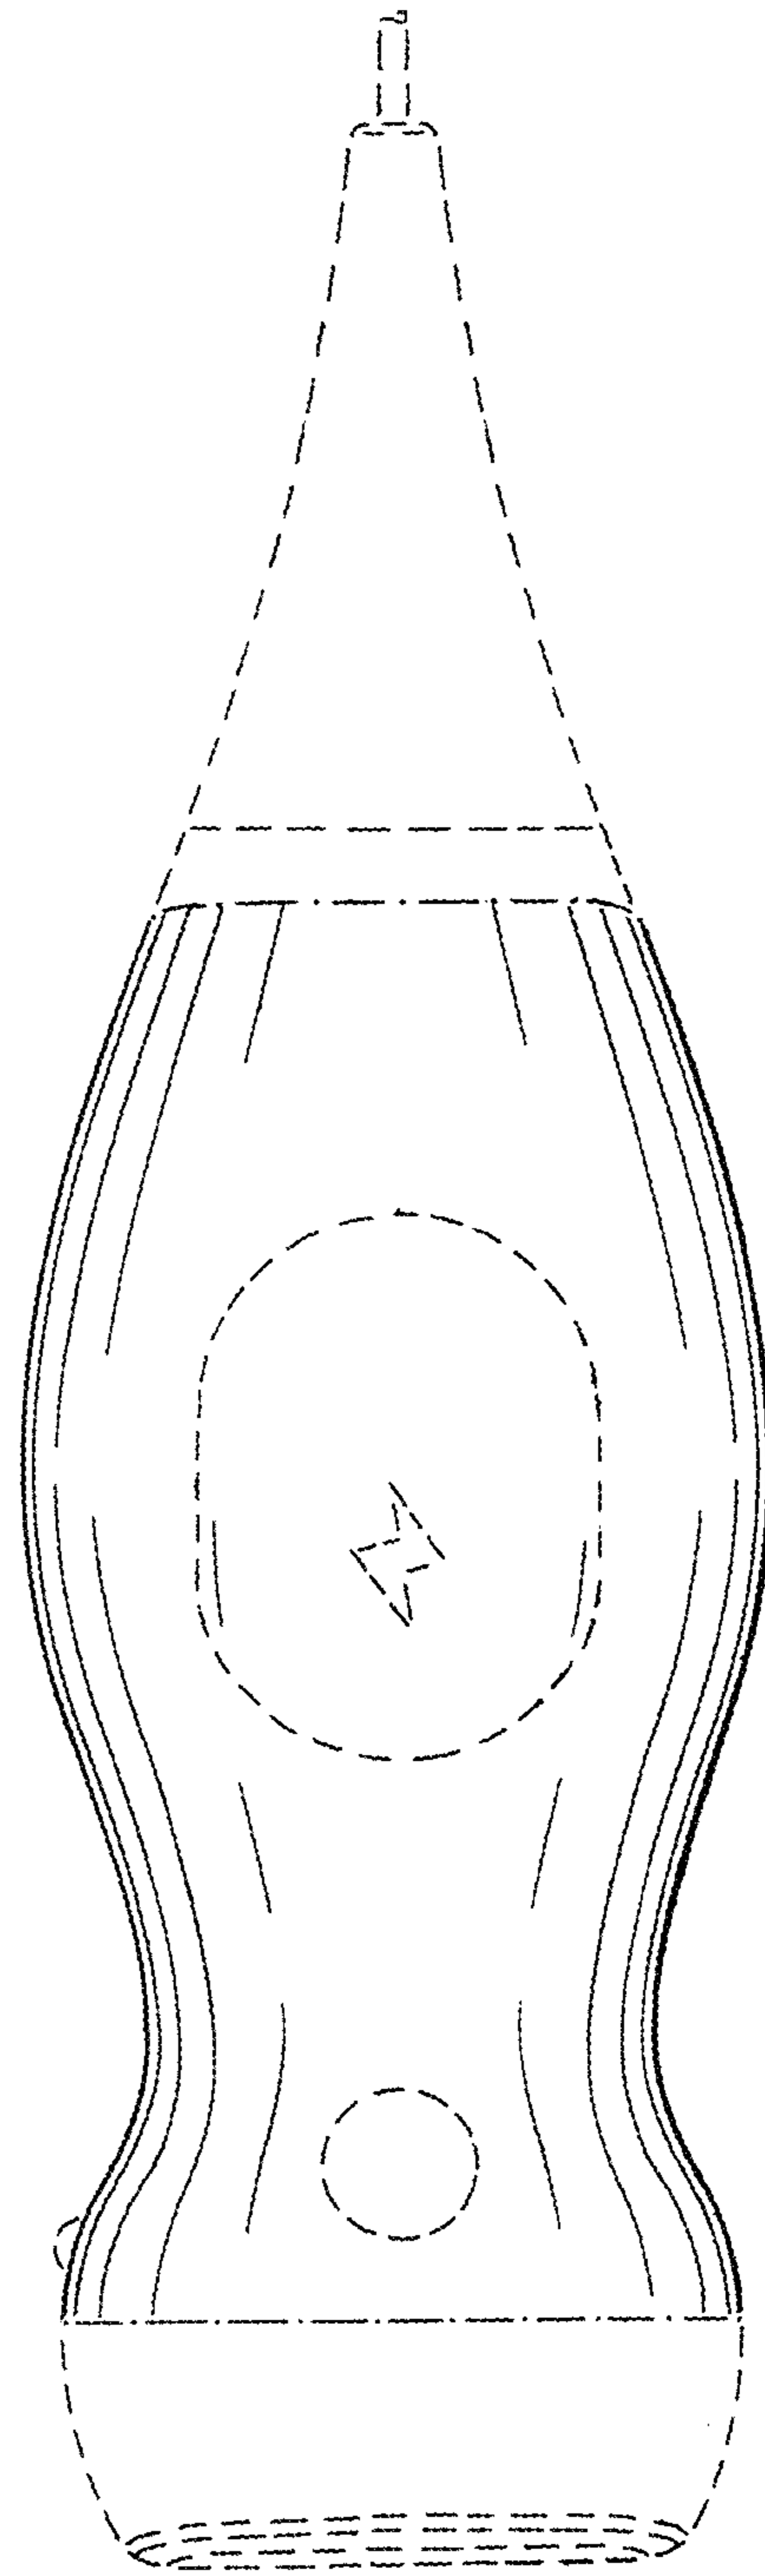


FIG. 3

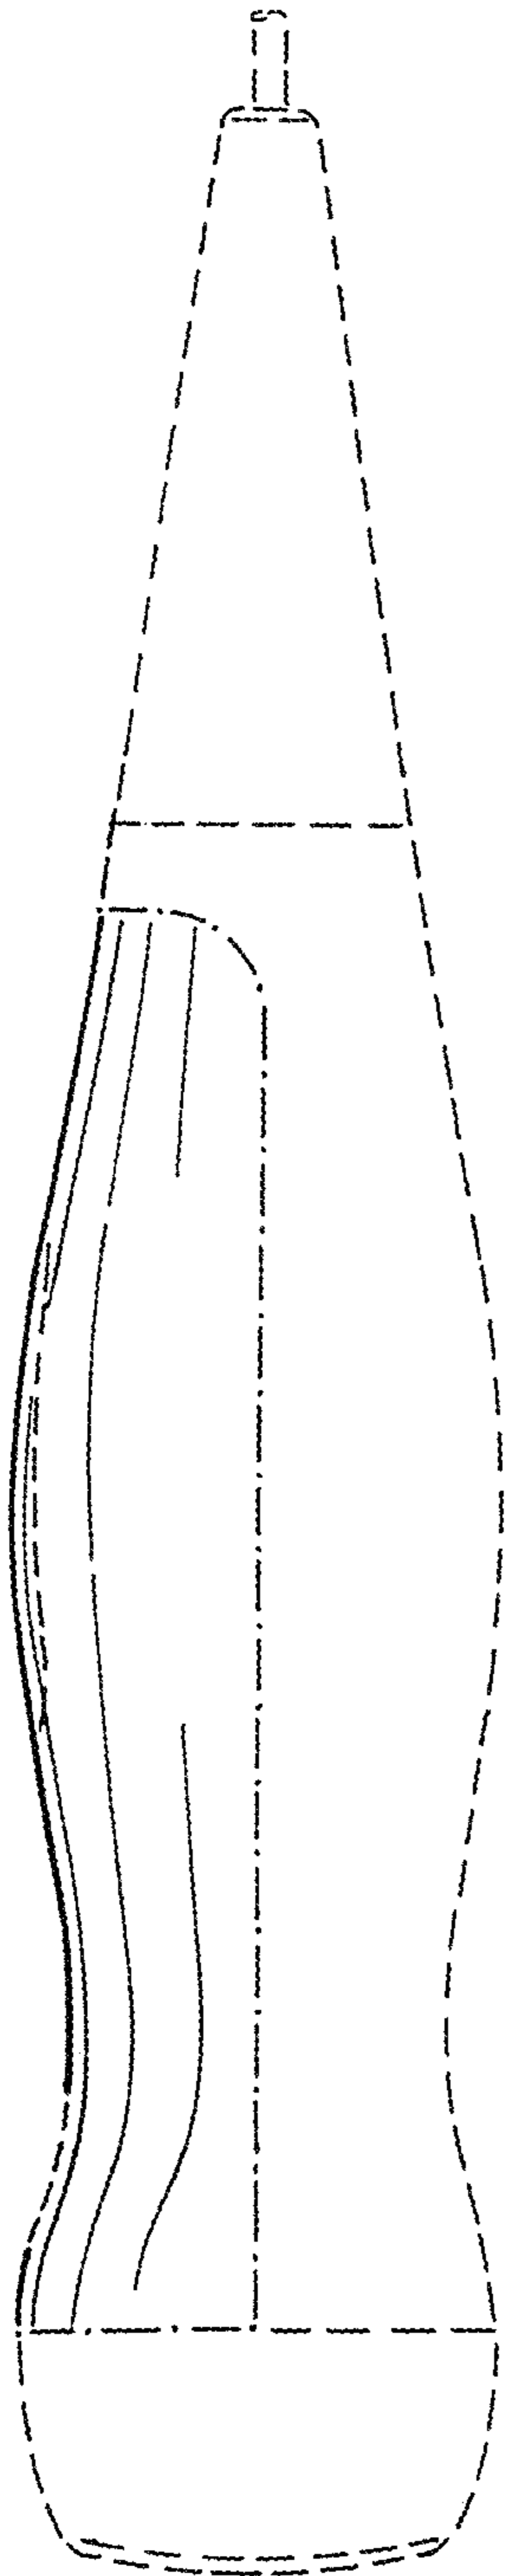


FIG. 4

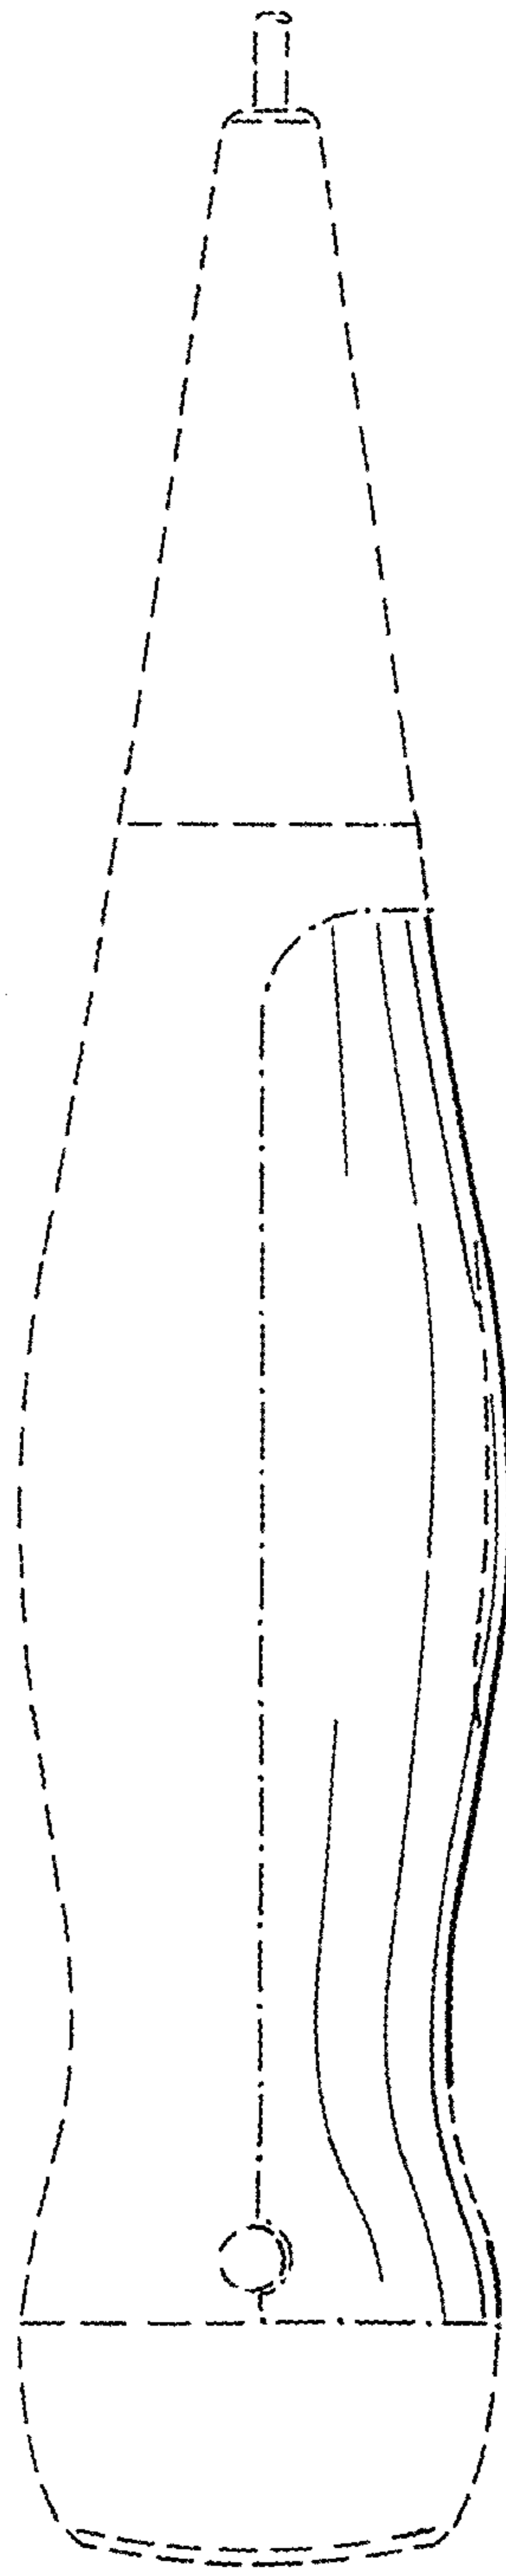


FIG. 5

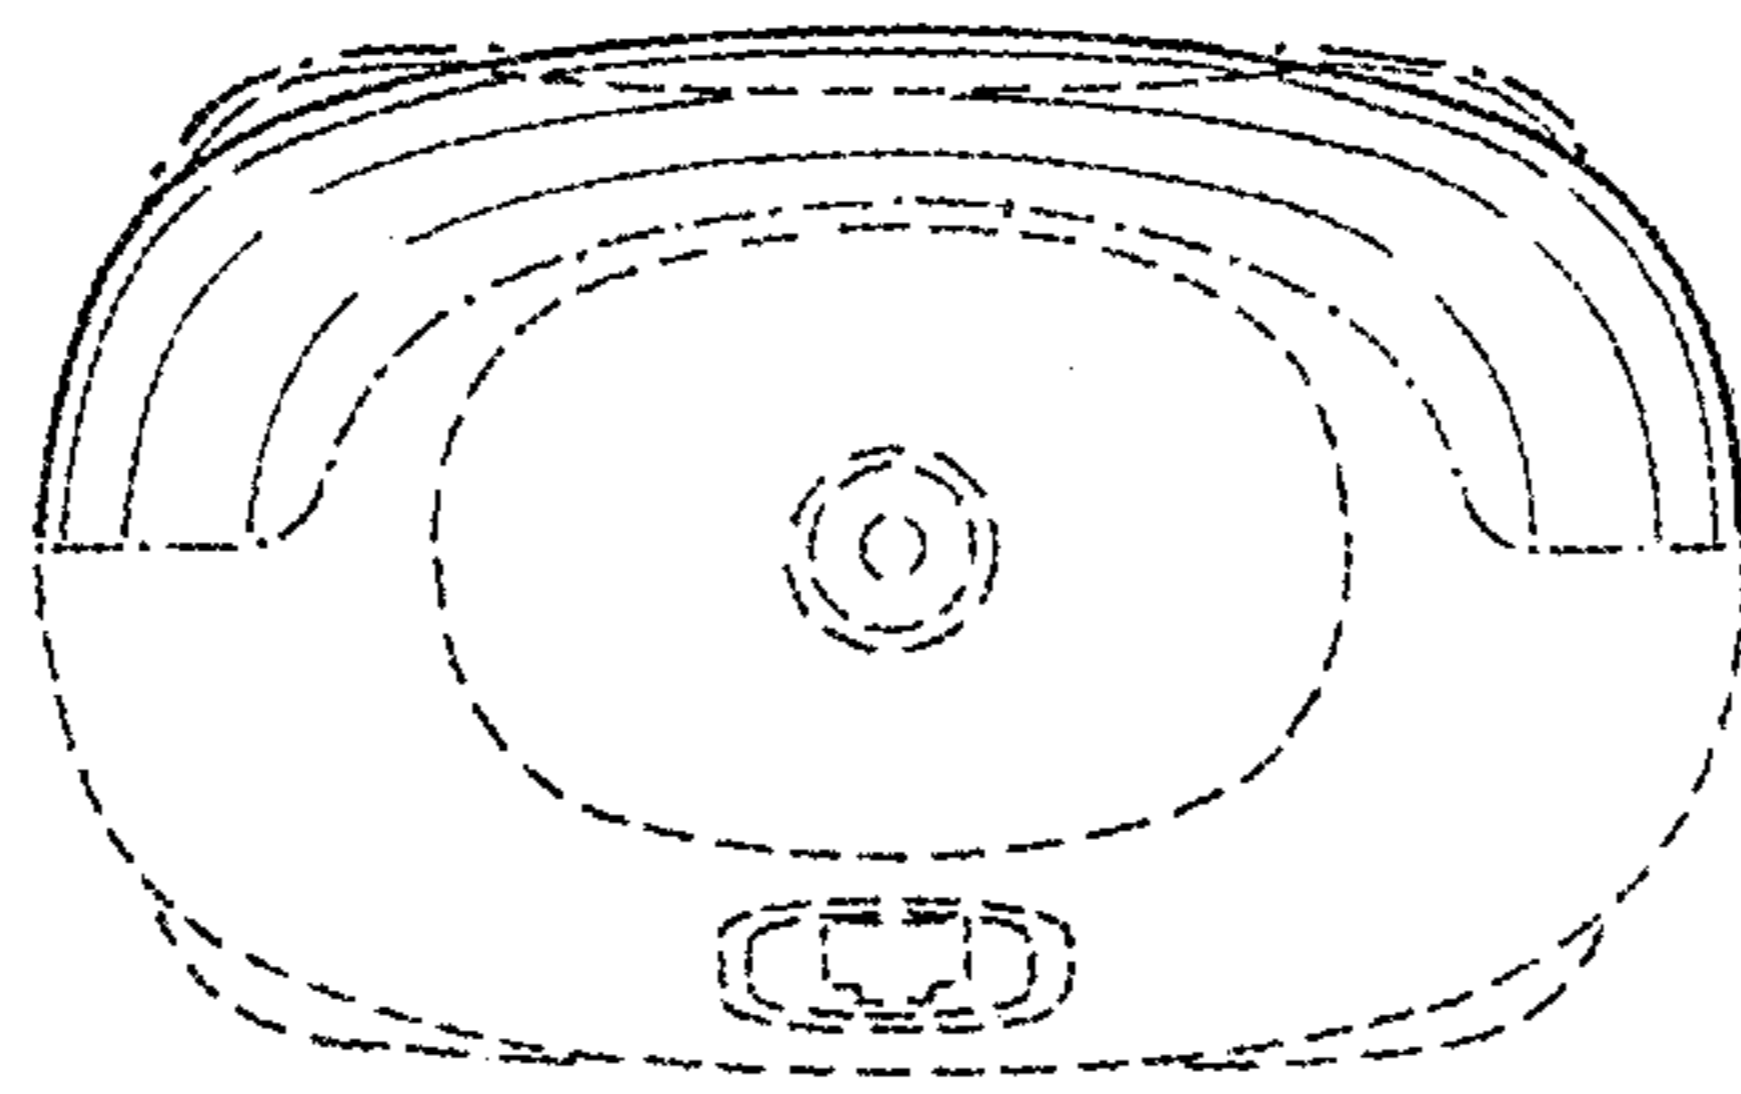


FIG. 6

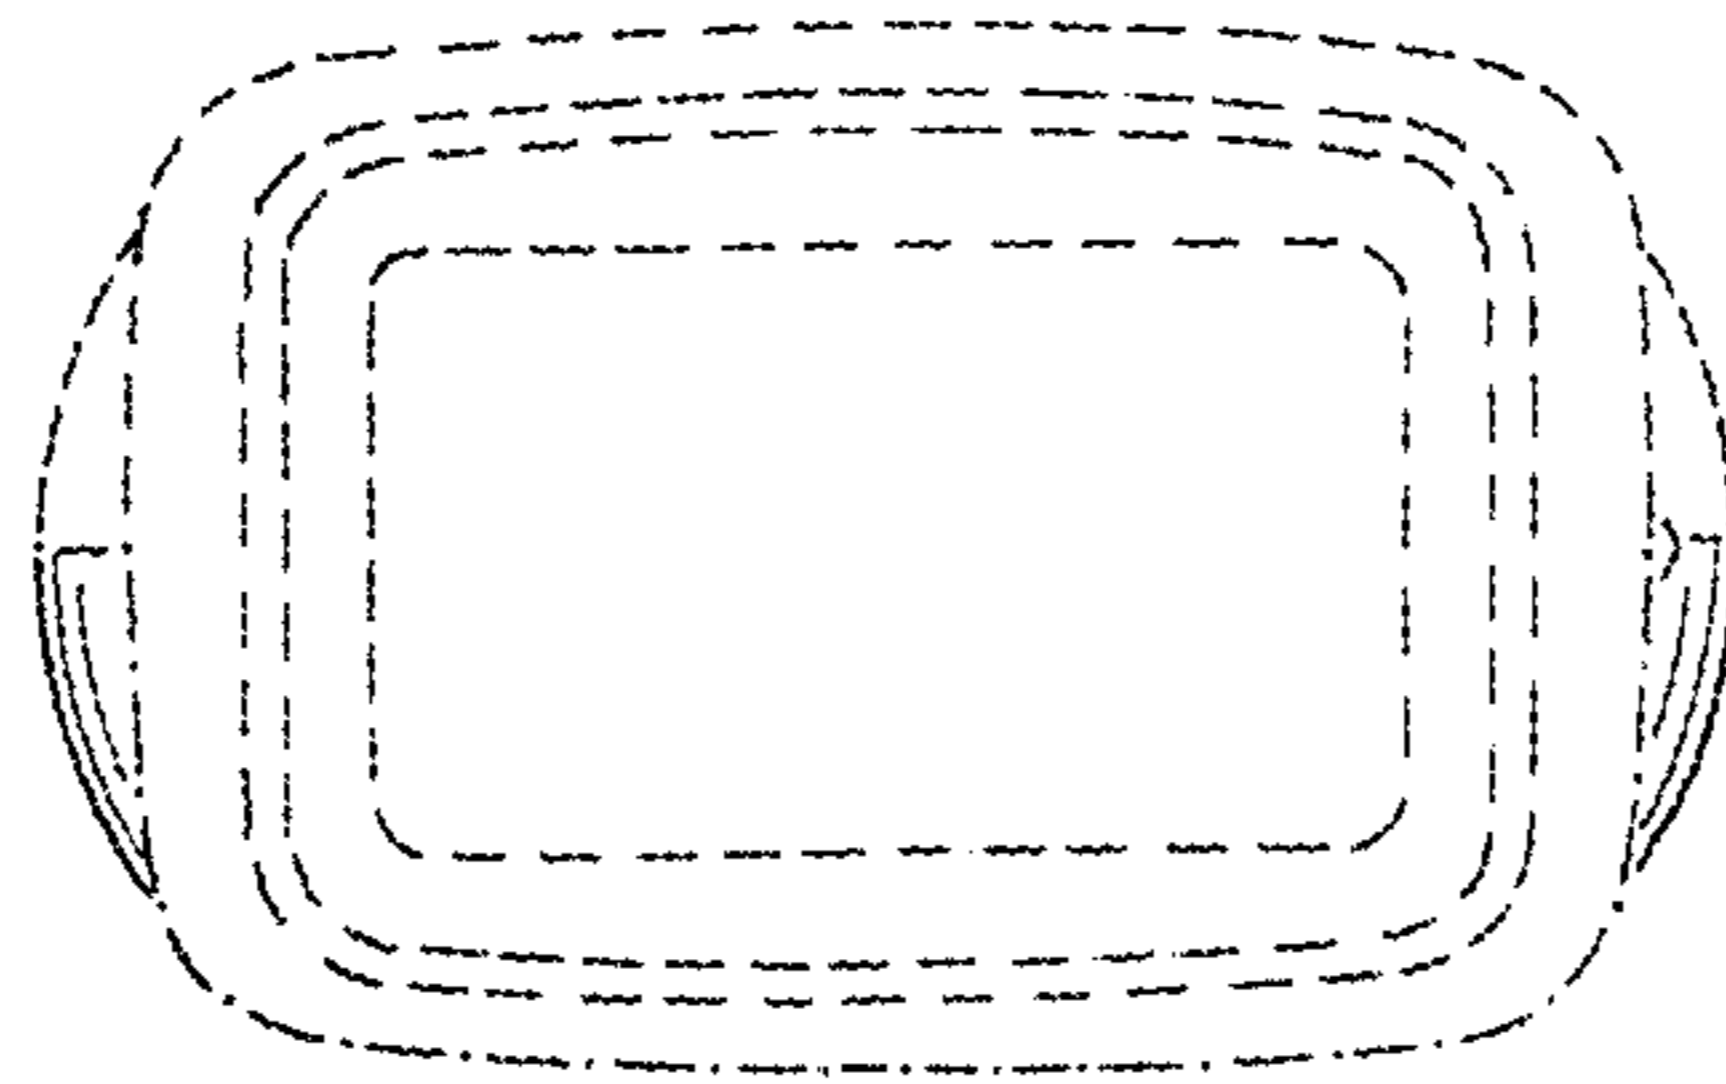


FIG. 7