



US00D870283S

(12) **United States Design Patent** (10) **Patent No.:** **US D870,283 S**
Adams (45) **Date of Patent:** **** *Dec. 17, 2019**

(54) **SINGLE STRAND BI-DIRECTIONAL SUTURE WITH COATING SHIELD**

- (71) Applicant: **Jason P. Adams**, Farmington, NM (US)
- (72) Inventor: **Jason P. Adams**, Farmington, NM (US)
- (*) Notice: This patent is subject to a terminal disclaimer.
- (**) Term: **15 Years**
- (21) Appl. No.: **29/623,747**
- (22) Filed: **Oct. 26, 2017**

Related U.S. Application Data

- (63) Continuation-in-part of application No. 15/096,496, filed on Apr. 12, 2016, now abandoned.
- (51) **LOC (12) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/145**
- (58) **Field of Classification Search**
USPC D24/133, 155, 169, 145, 146, 147, 148
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,720,055 A 3/1973 De Mestral et al.
 - 8,062,363 B2 11/2011 Hirpara et al.
- (Continued)

FOREIGN PATENT DOCUMENTS

- CA 2777345 A1 11/2012
 - EP 2338421 B1 11/2012
- (Continued)

OTHER PUBLICATIONS

John R. Fowler, MD, Tiffany A. Perkins, BS, Bettina A. Buttaro, PhD, and Allan L. Truant, PhD, Clin Ortho Relat Res. Bacteria

Adhere Less to Barbed Monofilament Than Braided Sutures in a Contaminated Wound Model, Feb. 2013; 471(2): 665-671.

(Continued)

Primary Examiner — Cathron C Brooks

Assistant Examiner — Samantha Q Lawrence

(74) *Attorney, Agent, or Firm* — PateBaird, PLLC

(57) **CLAIM**

The ornamental design for a single strand bi-directional suture with coating shield, as shown and described.

DESCRIPTION

FIG. 1 is a side elevation view of a single strand bi-directional suture with coating shield in accordance with the invention, showing the single strand bi-directional suture with coating shield in a first condition of use wherein the strand is shown in a coated condition;

FIG. 2 is an enlarged, partial side elevation of a portion of the single strand bi-directional suture with coating shield taken from FIG. 1;

FIG. 3 is an enlarged partial perspective view of top-most portion of the single strand bi-directional suture with coating shield, as shown in FIG. 1;


FIG. 4 is a cross-section view thereof, showing the single strand bi-directional suture with coating shield taken along line 4-4 of FIG. 2; and,

FIG. 5 is another cross-section view thereof, showing the single strand bi-directional suture with coating shield in a second condition of use wherein the strand is in a non-coated condition.

The single strand bi-directional suture with coating shield is shown with a symbolic break in its length, i.e., FIG. 1. The appearance of any portion of the article between the break lines forms no part of the claimed design.

The single strand bi-directional suture with coating shield contains a repeating pattern of barbs, wherein the pattern of barbs repeats along the length of the suture filaments forming a single-stranded suture. Before and during use, the single-stranded suture contains coating. Once the single strand bi-directional suture with coating shield is installed, the coating on the strand dissolves.

(Continued)

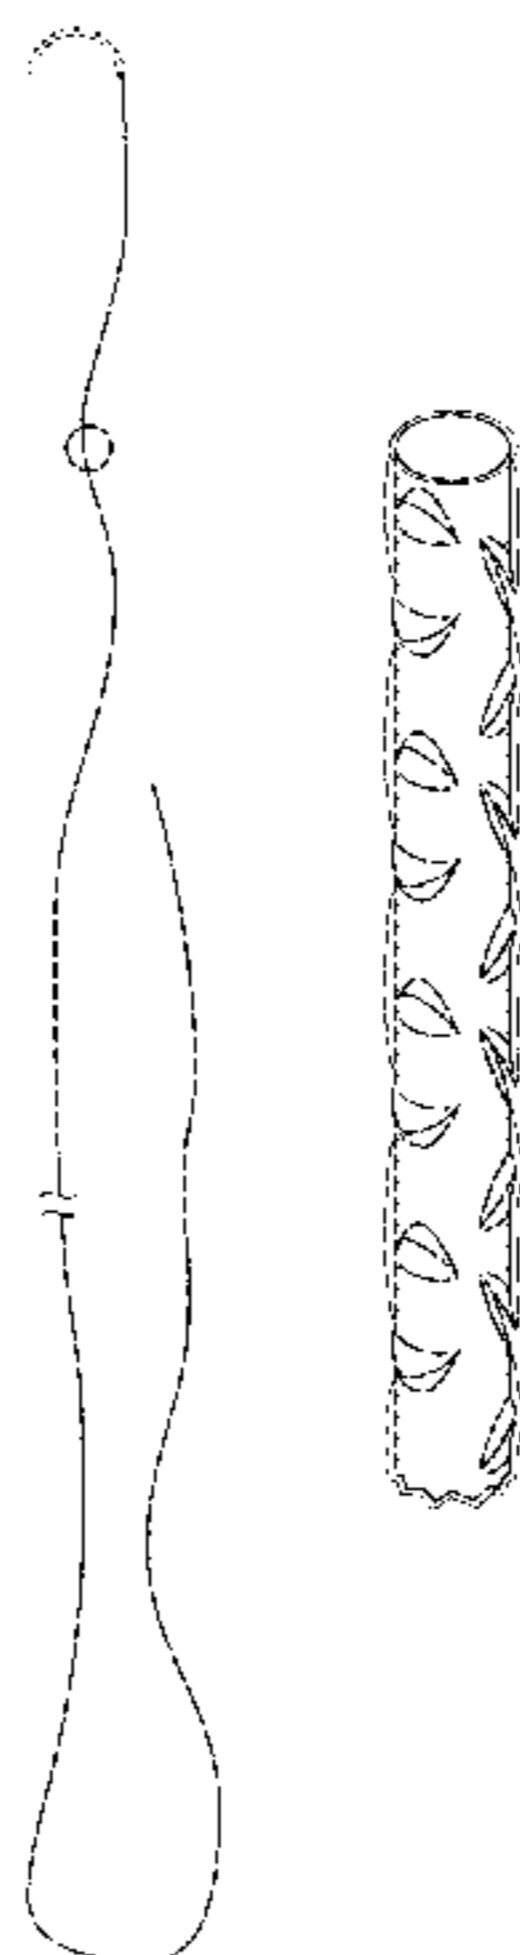

The broken lines showing selected features are for the purpose of illustrating environment and context of the article and form no part of the claimed design.

1 Claim, 2 Drawing Sheets

(58) **Field of Classification Search**

CPC A61B 17/06166; A61B 17/0401; A61B 2017/00526; A61B 2017/06176; A61B 17/06066; A61B 17/04; A61B 2017/0417; A61B 2017/0608; A61B 17/0469; A61B 17/0483; A61B 17/0485; A61B 17/062; A61B 17/0046; A61F 2002/075; B21G 1/08

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

8,353,931	B2	1/2013	Stopek et al.	
8,562,644	B2	10/2013	Yuan et al.	
9,125,647	B2 *	9/2015	Goraltchouk	A61B 17/06166
9,248,580	B2 *	2/2016	Leung	B26D 3/08
2010/0298878	A1 *	11/2010	Leung	A61B 17/0401 606/232
2012/0130406	A1 *	5/2012	Odermatt	A61B 17/06166 606/151
2012/0277793	A1 *	11/2012	Marczyk	A61B 17/06166 606/228
2013/0066369	A1	3/2013	Collier et al.	
2013/0165971	A1	6/2013	Leung et al.	
2014/0213966	A1 *	7/2014	Ostapoff	A61B 17/06166 604/93.01

2015/0272720	A1 *	10/2015	Marks	A61B 17/00008 623/13.2
2016/0278769	A1 *	9/2016	Kim	D02J 3/10
2017/0189016	A1 *	7/2017	Gross	A61B 17/06166
2017/0281160	A1 *	10/2017	Lin	A61B 17/06166
2017/0319203	A1 *	11/2017	Cohen	A61B 17/06166
2018/0116648	A1 *	5/2018	Kim	A61B 17/06109
2018/0125472	A1 *	5/2018	Dreyfuss	A61B 17/0401
2018/0140291	A1 *	5/2018	Dreyfuss	A61B 17/0401
2018/0177505	A1 *	6/2018	Chu	A61B 17/06166

FOREIGN PATENT DOCUMENTS

EP	2447040	A3	12/2013
JP	61171998		2/1986

OTHER PUBLICATIONS

James A. Greenberg, MD, US National Library of Medicine National Institute of Health, The Use of Barbed Sutures in Obstetrics and Gynecology, v.3(3); Summer 2010.

Dr. R.K. Mishra, Barbed Suture in Laparoscopic Surgery, Feb. 9, 2016.

Angiotech Puerto Rico, Inc., Quill™ Knotless Tissue-Closure Device Product Catalog, 2007-2013.

Angiotech Pharmaceuticals, Inc. Quill™ SRS Product Catalog, 2009.

Covidien, V-Loc™ Wound Closure Devices Product Overview, 2011.

Covidien, V-Loc™ Wound Closure Device (the secure advantage), 2013.

DePuy Mitek, a Johnson & Johnson Company, MicroFix Absorbable QuickAnchor® Plus, Massachusetts, 2005.

* cited by examiner

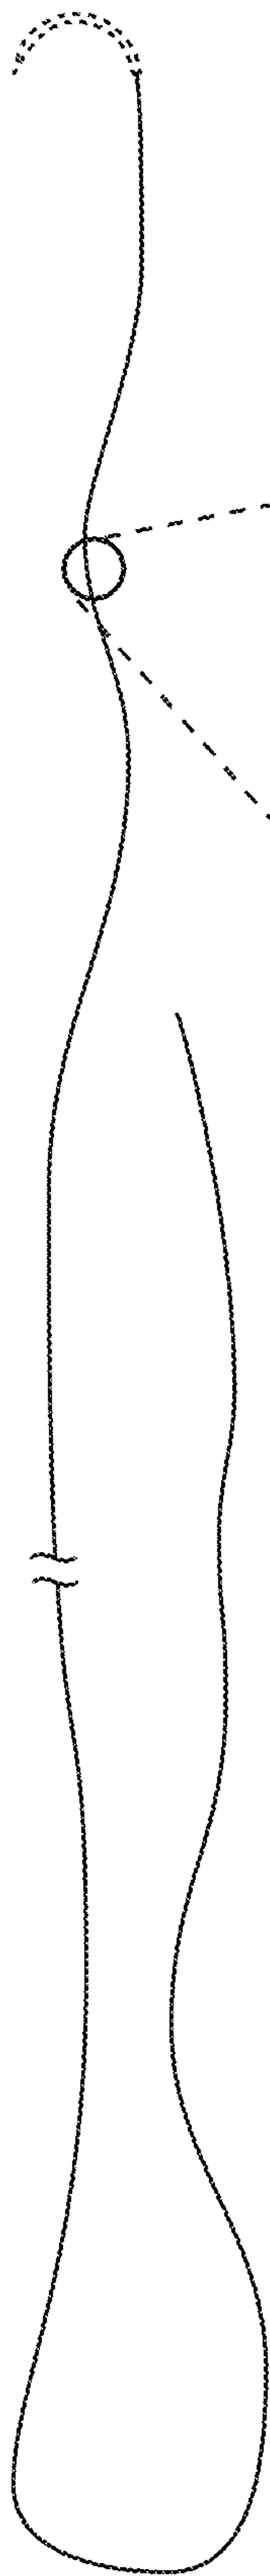


FIG. 1

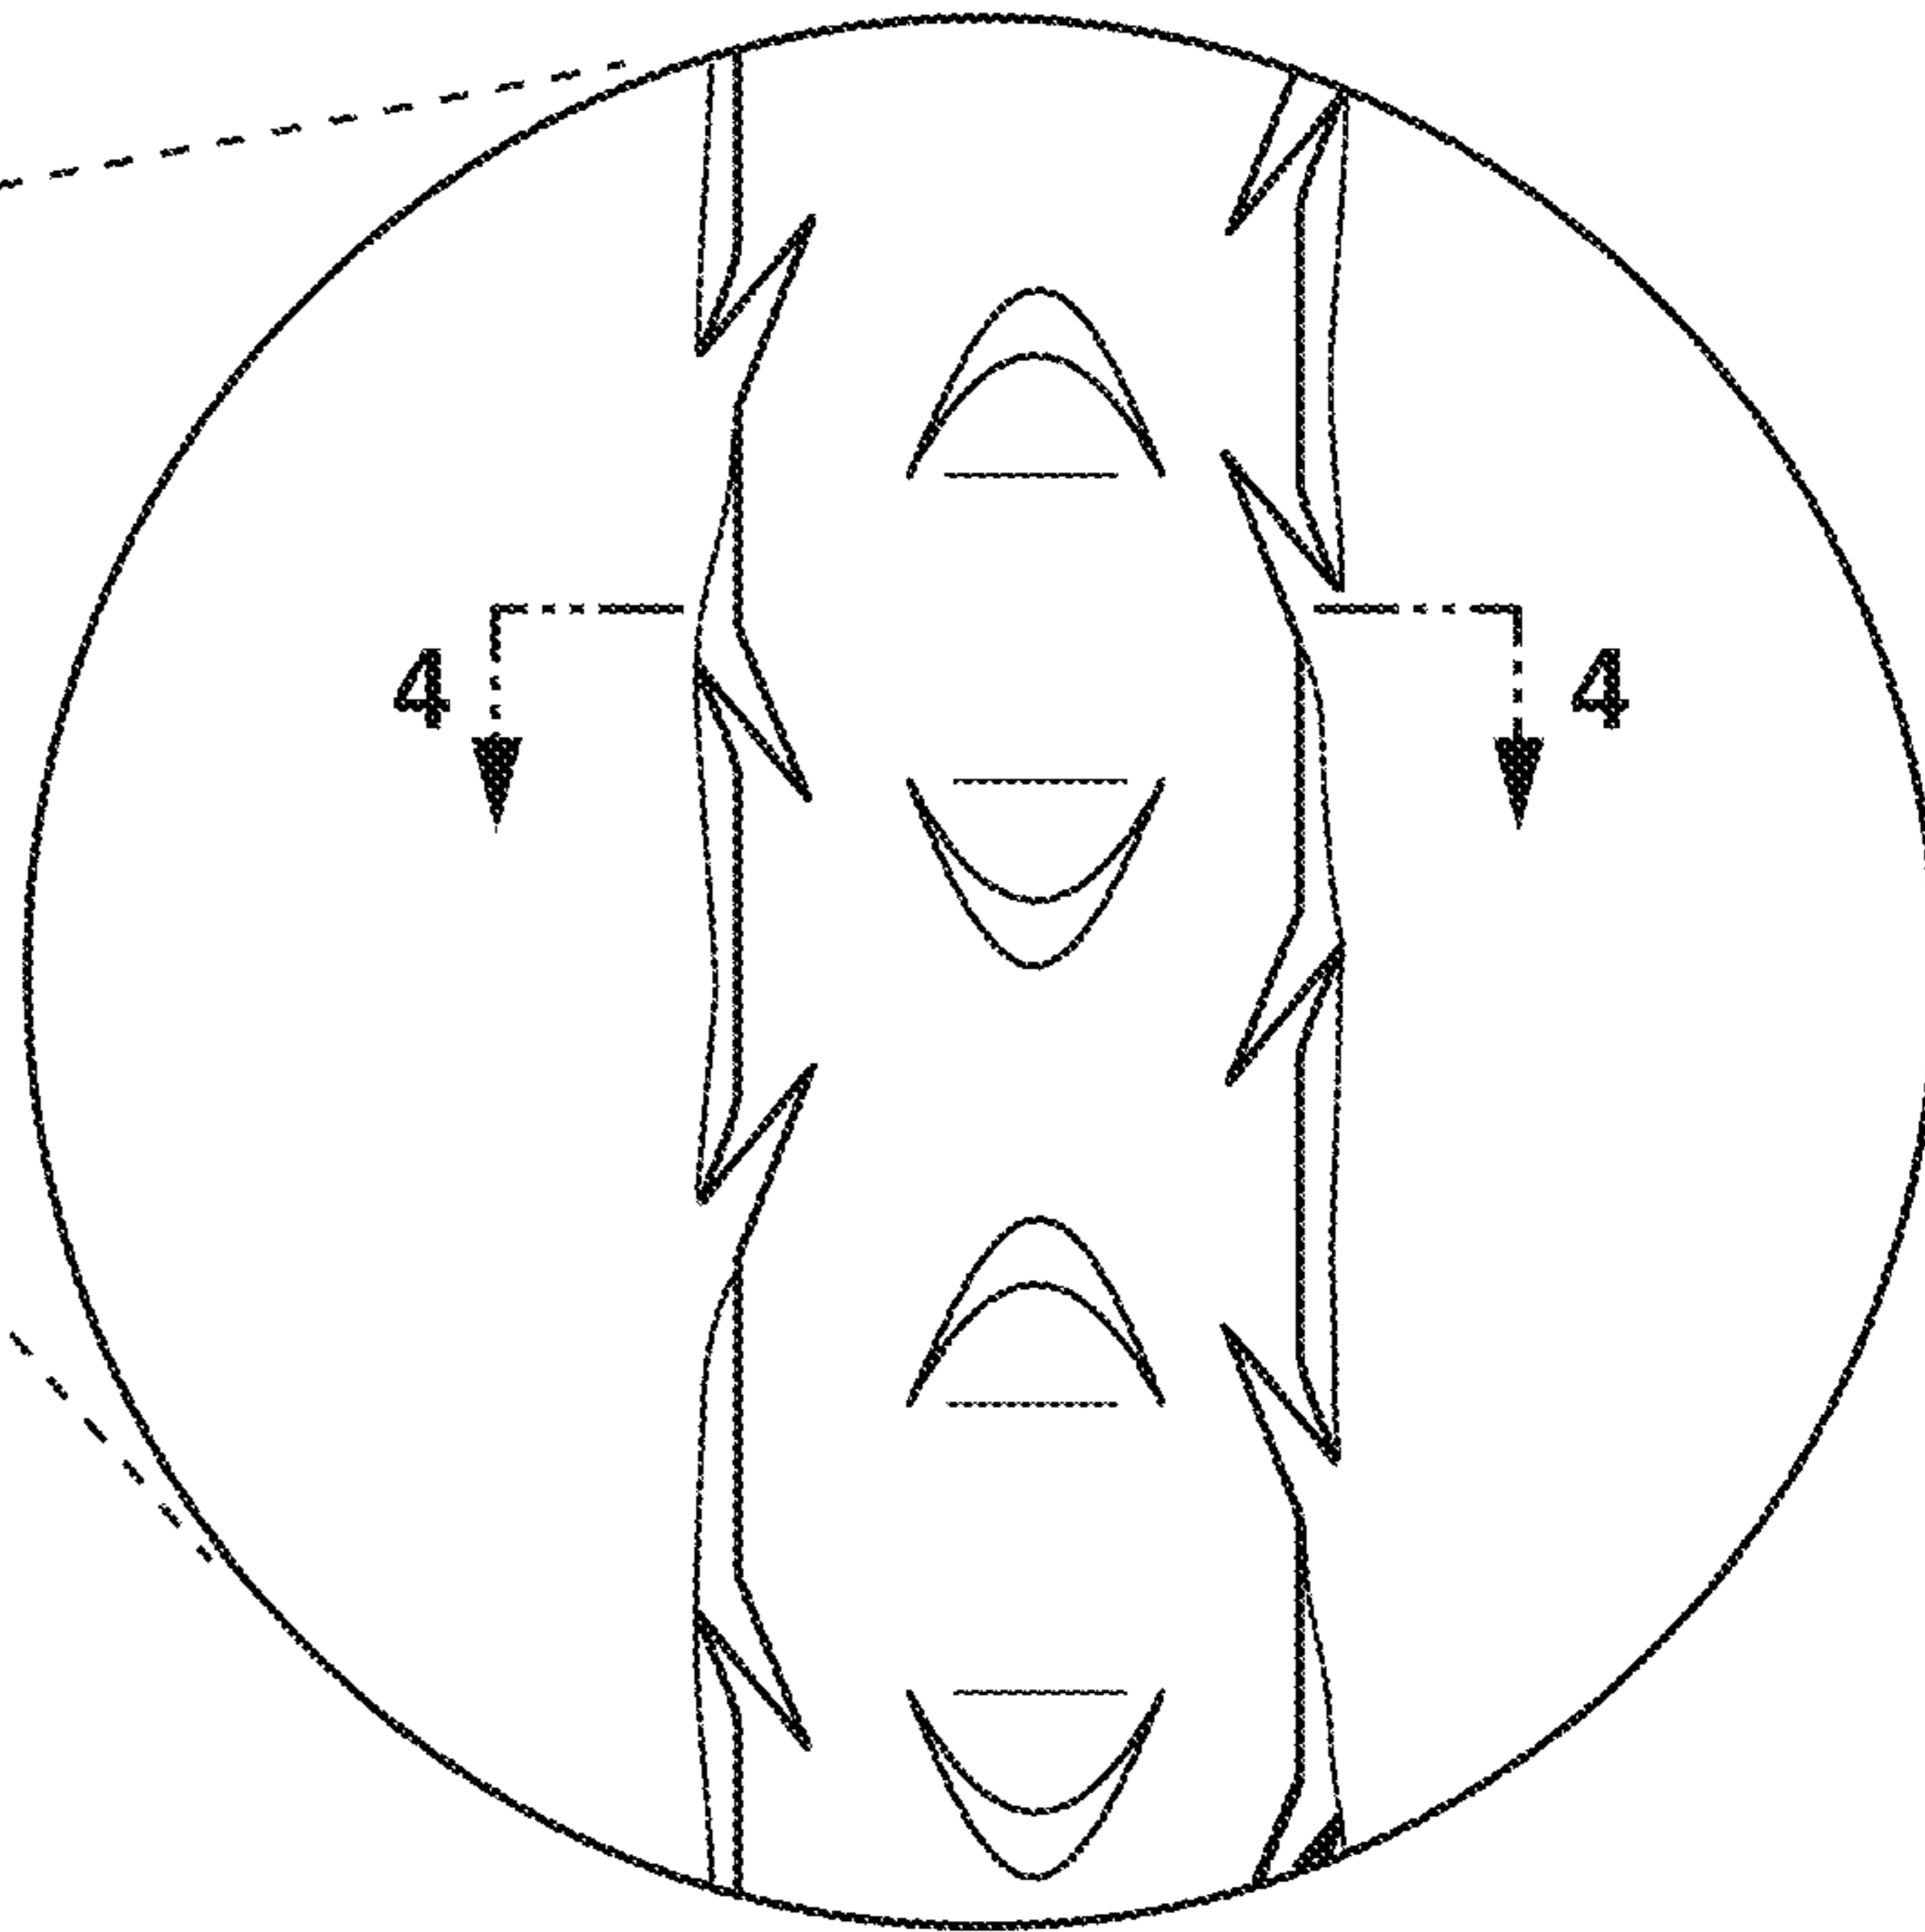


FIG. 2



FIG. 3

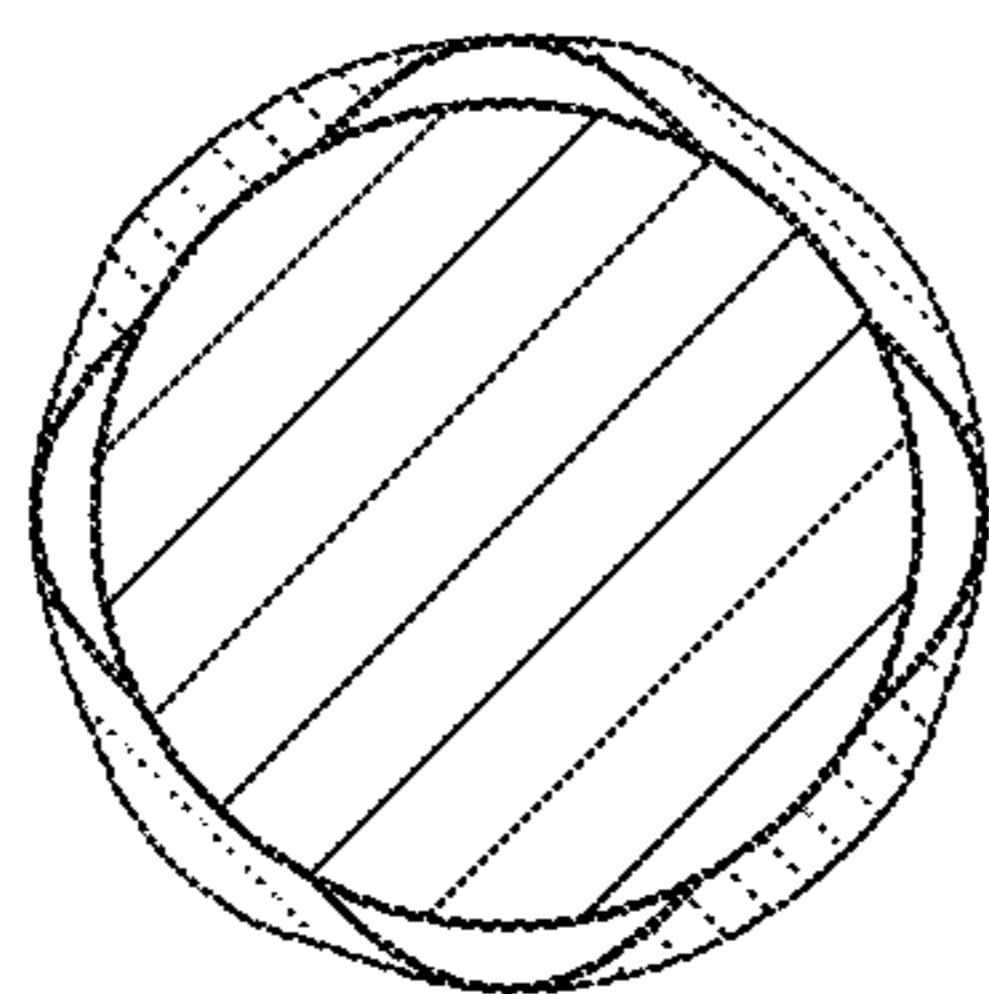


FIG. 4

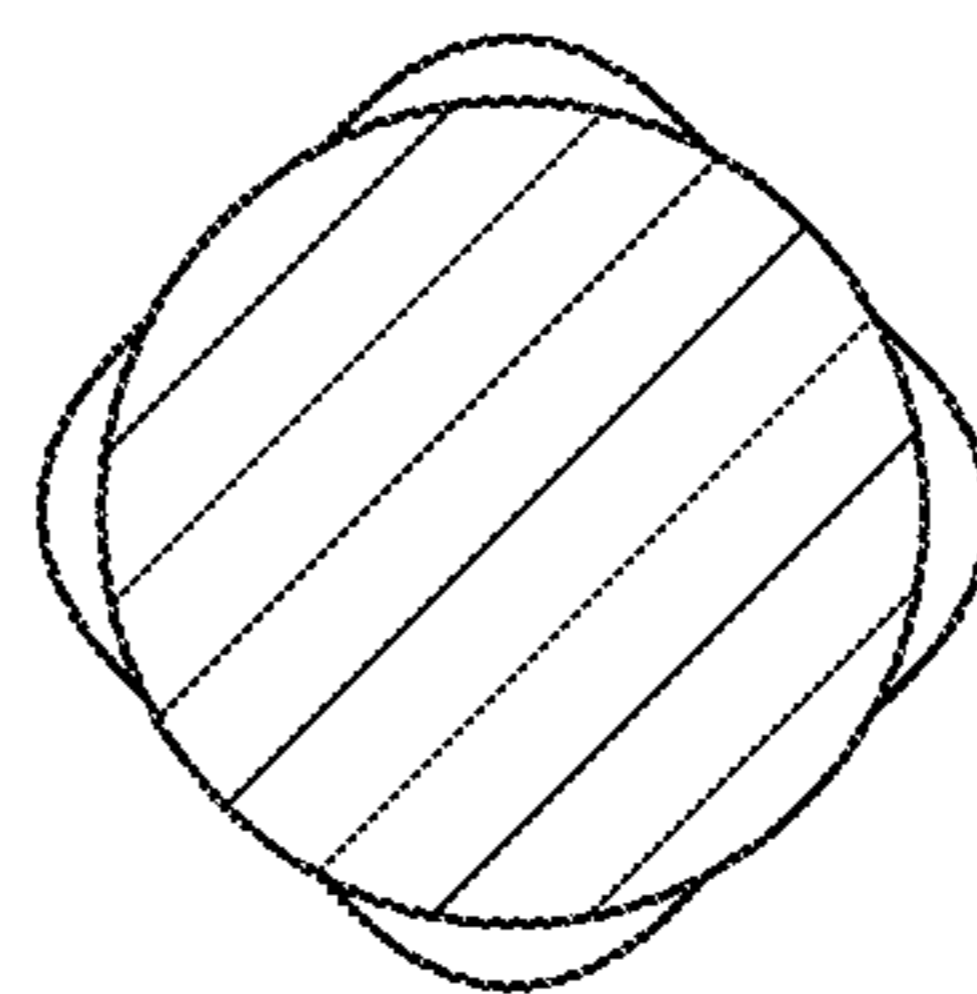


FIG. 5