



US00D870897S

(12) **United States Design Patent** (10) **Patent No.:** **US D870,897 S**
Katzberg (45) **Date of Patent:** **** Dec. 24, 2019**

- (54) **MEDICAL PROBE**
- (71) Applicant: **Oral Diagnostix LLC**, Clinton, SC (US)
- (72) Inventor: **Richard W. Katzberg**, Clinton, SC (US)
- (73) Assignee: **Oral Diagnostix LLC**, Clinton, SC (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/654,191**
- (22) Filed: **Jun. 21, 2018**
- (51) **LOC (12) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/187**
- (58) **Field of Classification Search**
USPC D24/107, 133, 137, 138, 141, 158–161,
D24/164, 165, 167, 170, 185–187;
D10/57, 60, 78, 80; D6/709
CPC ... A61B 8/0437; A61B 8/0883; A61B 8/4405;
A61B 8/4427; A61B 8/445
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D211,675 S *	7/1968	Murcott	D24/183
D349,160 S *	7/1994	Pellegrino	D24/158
5,425,637 A *	6/1995	Whitehouse	A61C 17/08 433/95
D372,781 S *	8/1996	Reif	D24/133
5,690,113 A	11/1997	Sliwa, Jr. et al.		
D387,162 S *	12/1997	Zeimer	D24/133
5,779,639 A	7/1998	Yeung		
5,931,788 A	8/1999	Keen et al.		
5,984,913 A *	11/1999	Kritzinger	A61F 9/00804 604/541
D533,270 S *	12/2006	Kierce	D24/112
D540,952 S *	4/2007	Colvin	D24/215
D565,191 S *	3/2008	Nan	D24/105

D650,901 S *	12/2011	Ghosh	D24/115
D765,245 S *	8/2016	Kamal	D24/141
9,532,857 B2 *	1/2017	Ronto	A61C 17/08
D785,176 S *	4/2017	Tseng	D16/208
D798,447 S *	9/2017	Leather	D24/135

(Continued)

OTHER PUBLICATIONS

OMNI Replacement Angled Bars. Online, published date Oct. 10, 2014. Retrieved on Oct. 19, 2019 from URL: <https://www.speedymoto.com/products/handle-bars/omni-bars/>.
(Continued)

Primary Examiner — Susan Bennett Hattan
Assistant Examiner — Omeed Agilee
(74) *Attorney, Agent, or Firm* — Blank Rome LLP


(57) **CLAIM**

The ornamental design for a medical probe, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a medical probe in accordance with the present design;
FIG. 2 is a front elevational view of the medical probe illustrated in FIG. 1;
FIG. 3 is a rear elevational view of the medical probe illustrated in FIG. 1;
FIG. 4 is a right side elevational view of the medical probe illustrated in FIG. 1;
FIG. 5 is a left side elevational view of the medical probe illustrated in FIG. 1;
FIG. 6 is a top plan view of the medical probe illustrated in FIG. 1; and,
FIG. 7 is a bottom plan view of the medical probe illustrated in FIG. 1.
The broken lines in the drawings depict portions of the medical probe that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

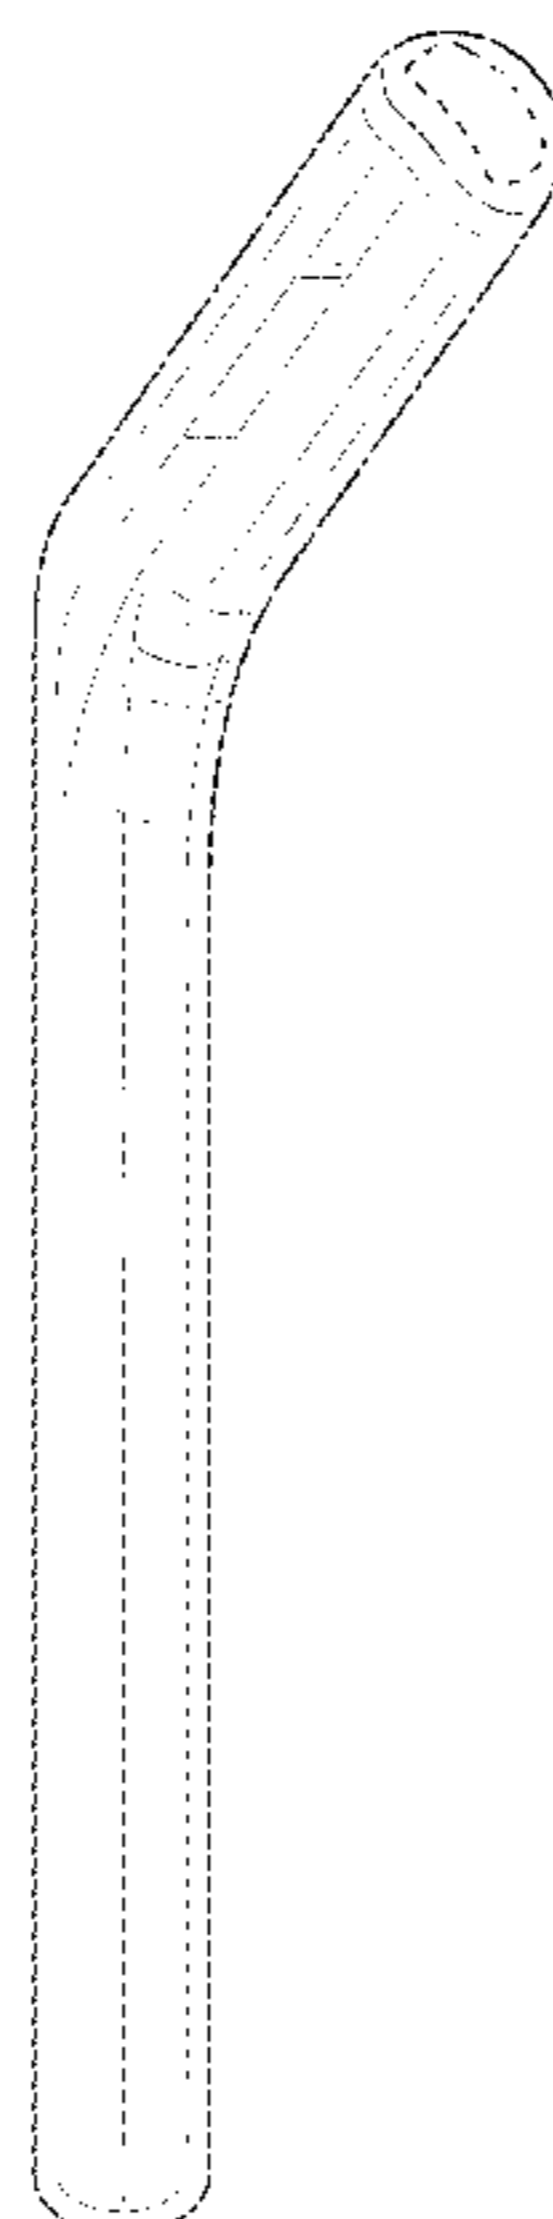

(56)

References Cited

U.S. PATENT DOCUMENTS

D808,702 S * 1/2018 Hollander D7/300.2
 D813,392 S * 3/2018 Wang D24/152
 D822,218 S * 7/2018 Asai D24/187
 D826,421 S * 8/2018 Janapol D24/215
 D831,397 S * 10/2018 Diorio D7/300.2
 D837,391 S * 1/2019 Naka D24/187
 2004/0143186 A1 7/2004 Anisimov et al.
 2010/0198069 A1 8/2010 El-Khorassani
 2013/0060144 A1 3/2013 Culjat et al.
 2015/0374331 A1 12/2015 Cho et al.
 2018/0368912 A1* 12/2018 Katzberg A61B 18/1477

OTHER PUBLICATIONS

Bent curve Durable Stainless Steel Drinking Straw Straws 8 inch Metal for Bar Family kitchen. Online, published date unknown. Retrieved on Oct. 19, 2019 from URL: <https://www.dhgate.com/product/brand-new-excurved-durable-stainless-steel1/252444216.html>.*

Schiffman E, Ohrbach R, Truelor E et al. Diagnostic Criteria for Temporomandibular Disorders (DC/TMD) for Clinical and Research Applications: Recommendations of the International RDC/TMD Consortium Network and Orofacial Pain Special Interest Group. *J Oral Facial Pain Headache* 2014; 28: 6-27.

Detamore MS, Athanasiou KA. A call to action for bioengineers and dental professionals: Directives for the future of TMJ bioengineering. *Annals of Biomedical Engineering* 2017; 35: 1301-1311.

Ahmad M, Hollender L, Anderson Q et al. Research diagnostic criteria for temporomandibular disorders (RDC/TMD): development of image analysis criteria and examiner reliability for image analysis. *Oral Surg Oral Med Oral Pathol Radiol Endod* 2009; 107: 844-860.

Westesson P-L. Are high-resolution ultrasonic signs of disc displacement valid? *J Oral Maxillofac Surg* 2002; 60: 628.

Dupuy-Bonafé I, Picot M-C, Maldonado IL, et al. Internal derangement of the temporomandibular joint: is there still a place for ultrasound? *Oral Surg Oral Med Oral Pathol Oral Radiol* 2012; 113: 832-840.

Harms SE, Wilk RM, Wolford LM et al. The Temporomandibular joint: magnetic resonance using surface coils. *Radiology* 1985; 157: 133-136.

Emshoff R, Jank S, Rudisch A, et al. Are high-resolution ultrasonic signs of disc displacement valid. *J Oral Maxillofac Surg*. 2002; 60: 623.

Melis M, Secci, Coneviz C. Use of ultrasonography for the diagnosis of temporomandibular disorders: A review. *Am J Dent* 2007; 20: 73.

Landis JR, Koch GG. The measurement of observer agreement for categorical data. *Biometrics* 1977; 33: 159-174.

Kundu H, Basavaraj P, Kote S, et al. Assessment of TMJ disorders using ultrasonography as a diagnostic tool: a review. *J Clin Diagn Res*. 2013; 7: 3116-3120.

Schiffman E. et al., "Effects of four treatment strategies for temporomandibular joint closed lock" *Int. J. Oral Maxillofac Surg.*, 2014; 43(2):217-226.

* cited by examiner

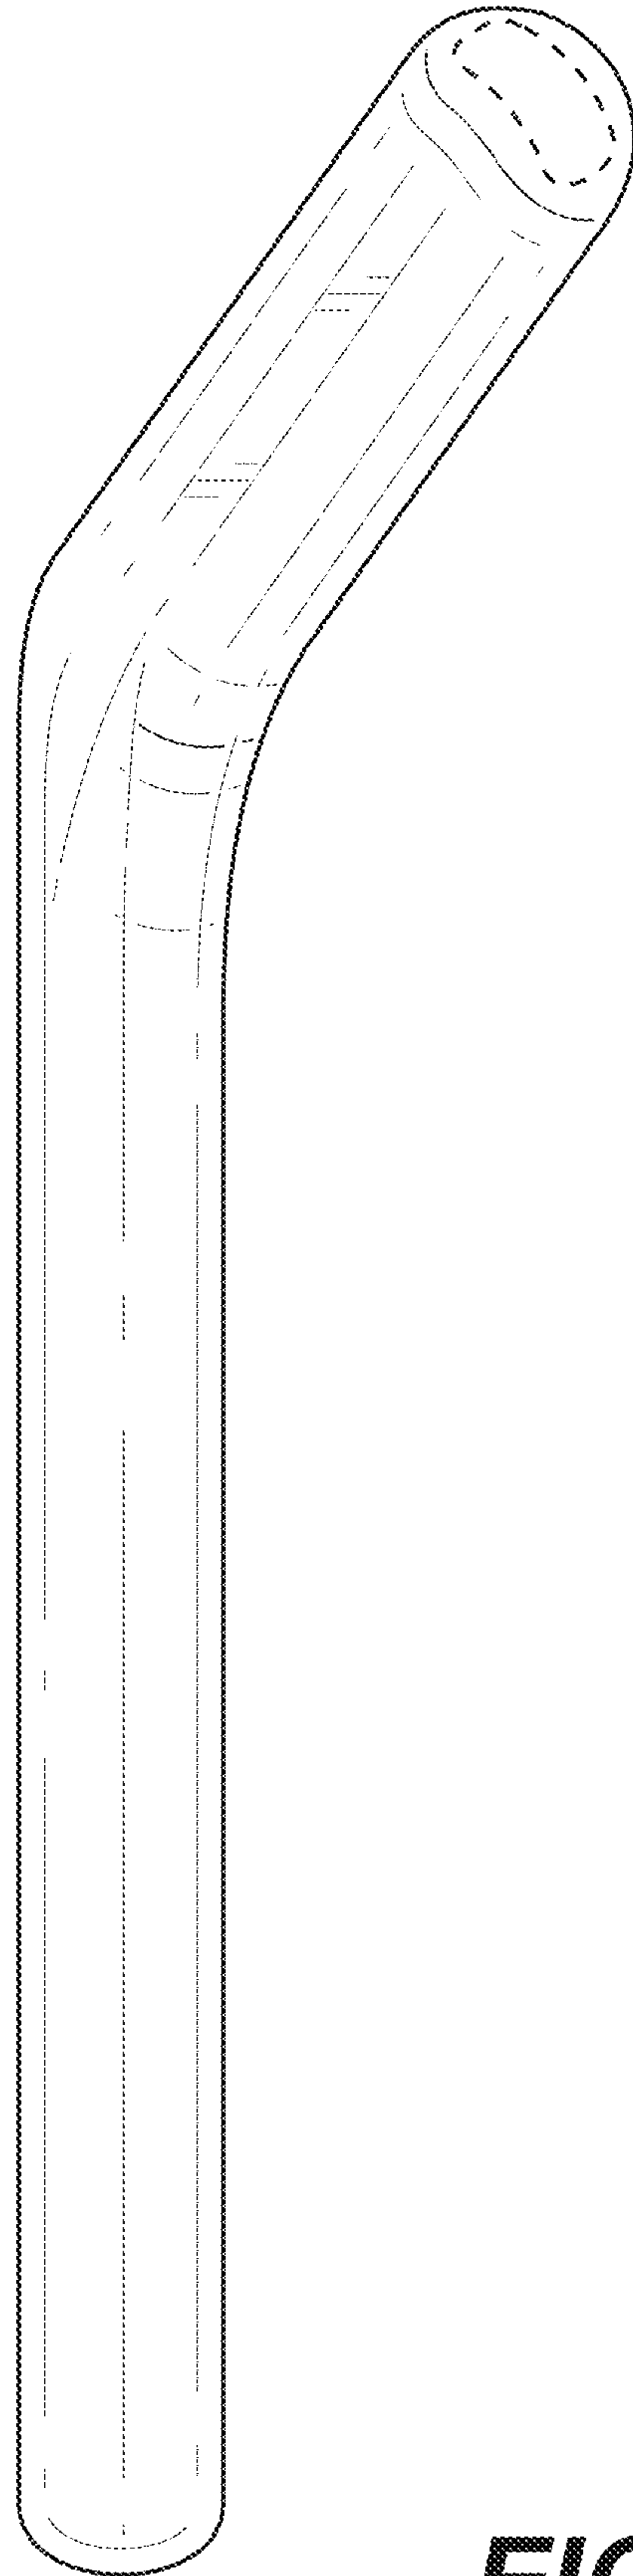


FIG. 1

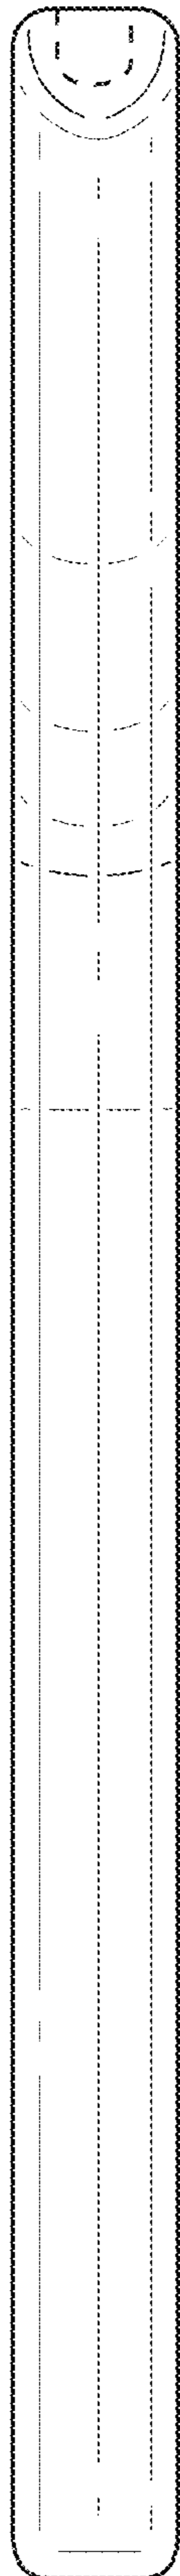


FIG. 2

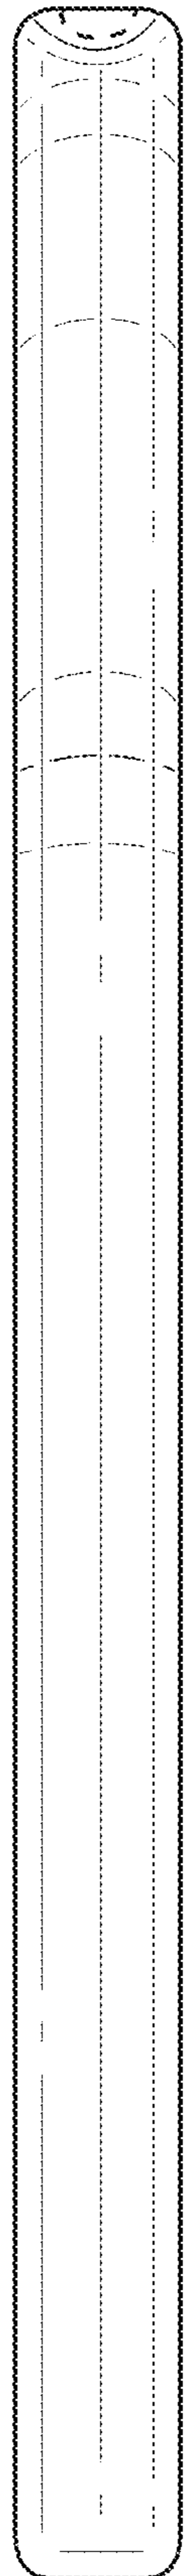


FIG. 3

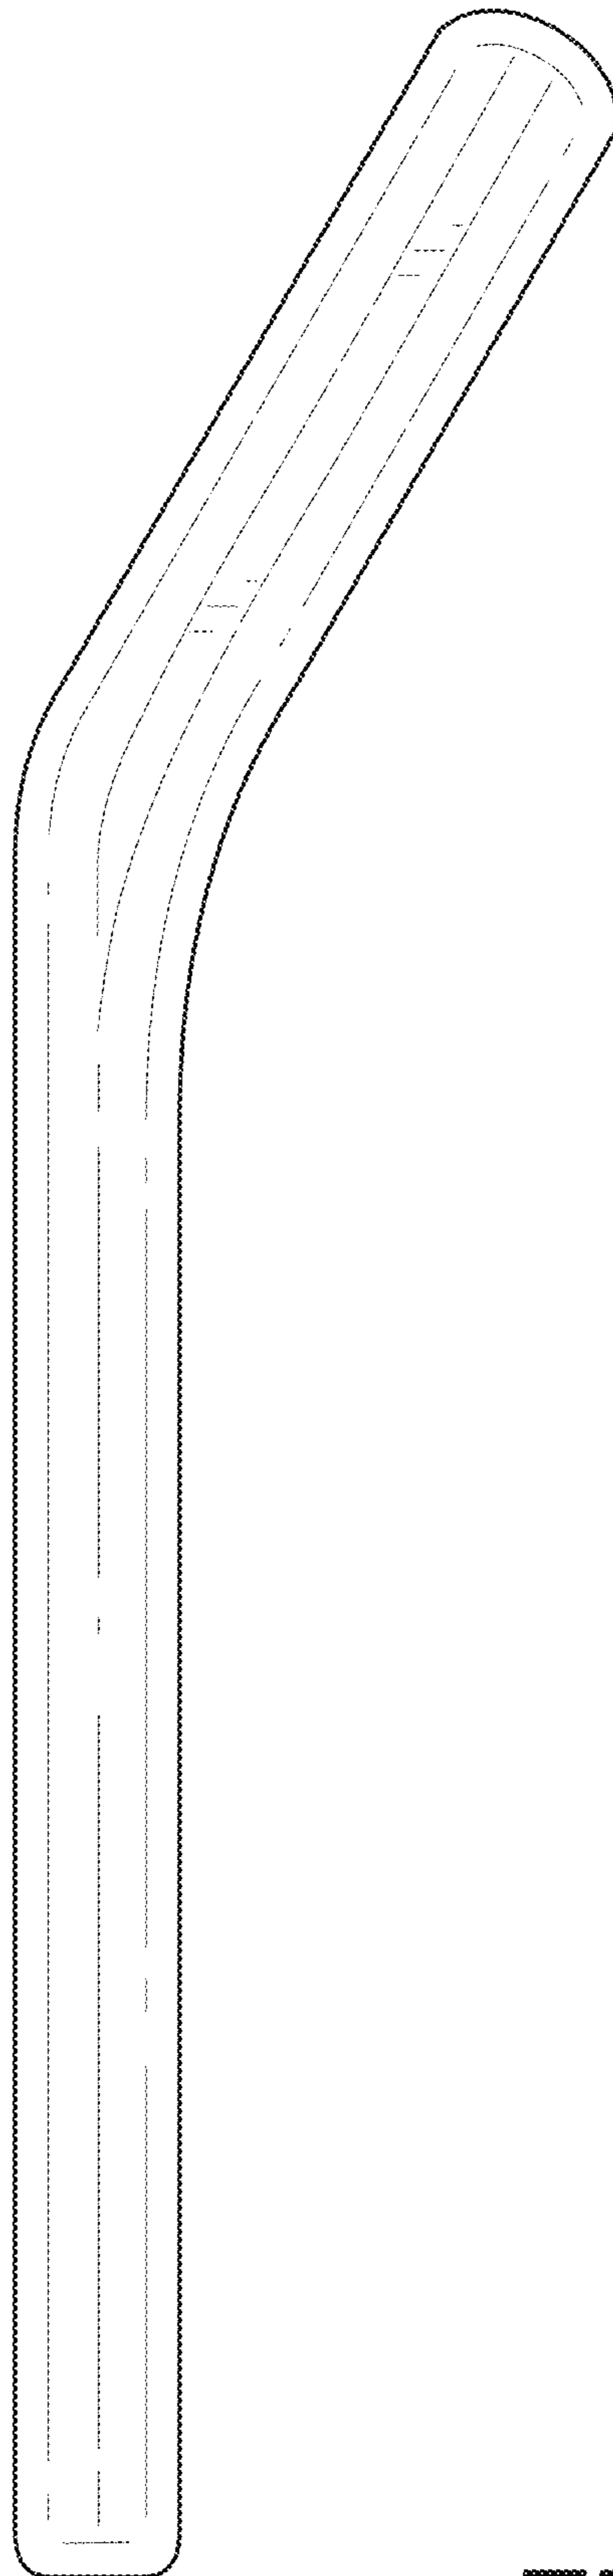


FIG. 4

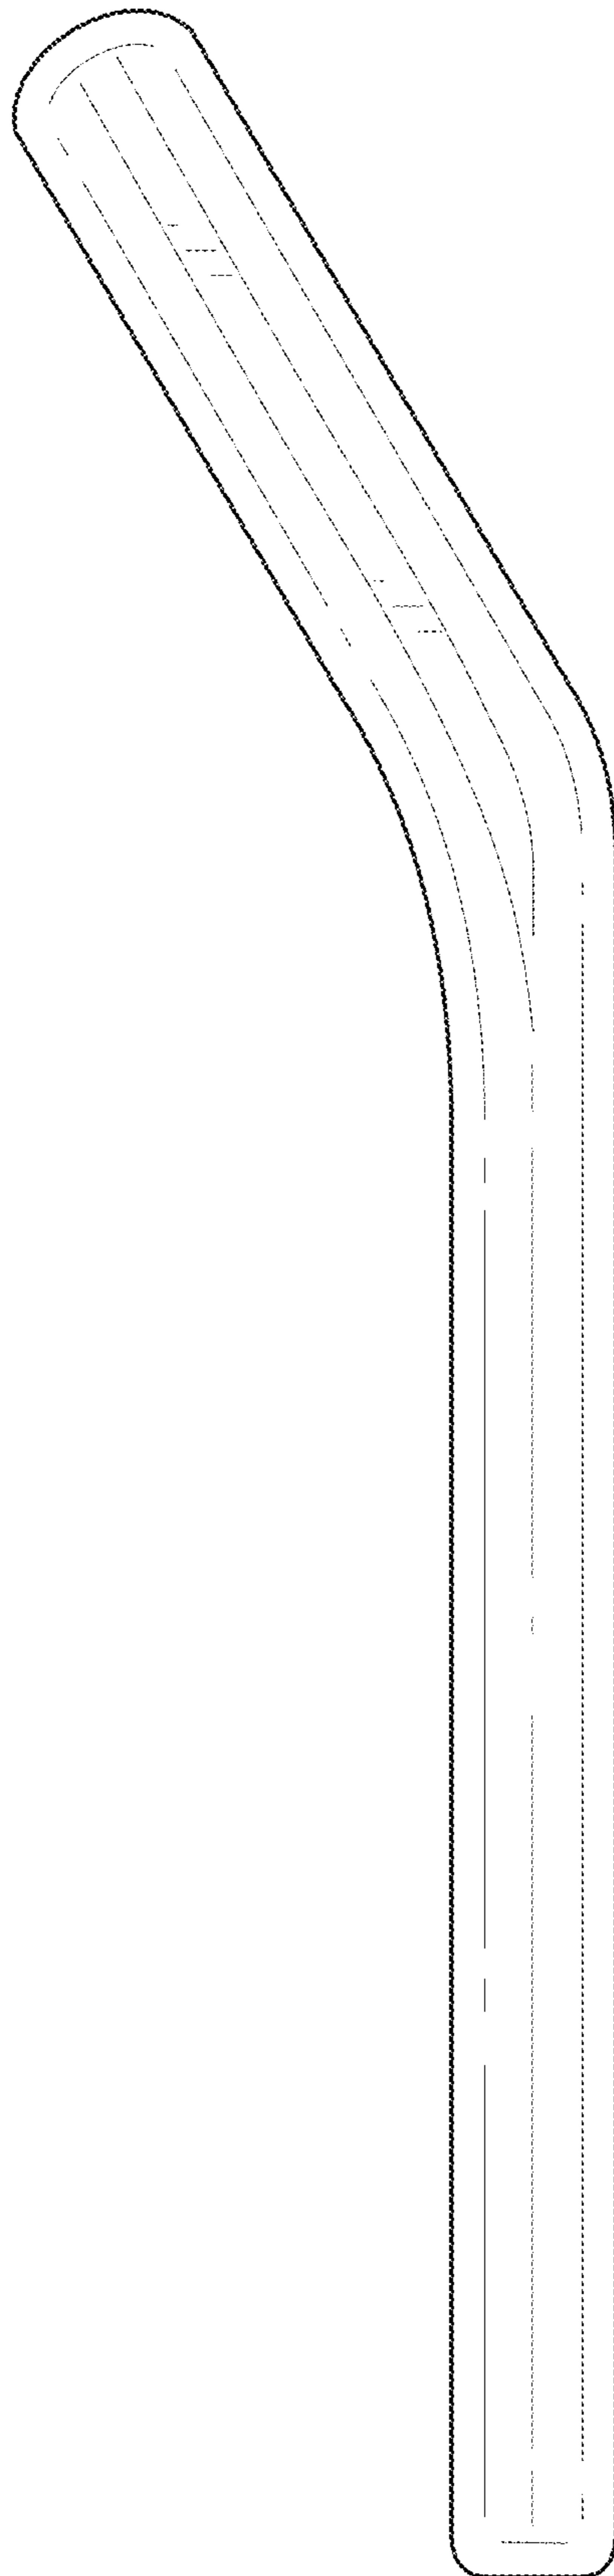


FIG. 5

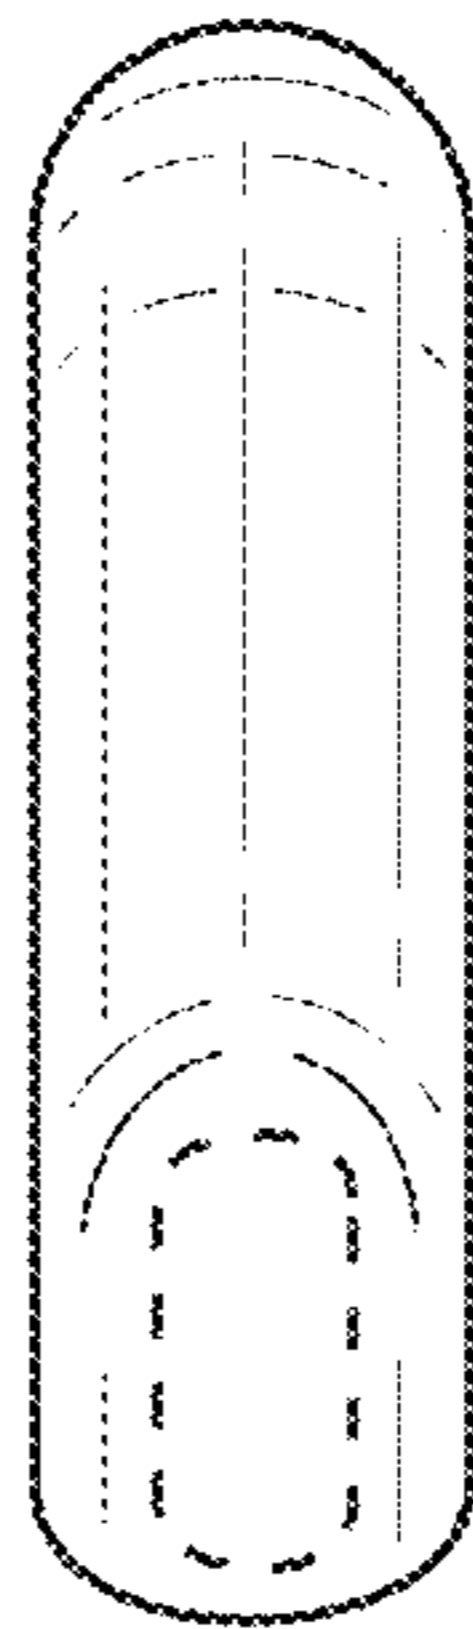


FIG. 6

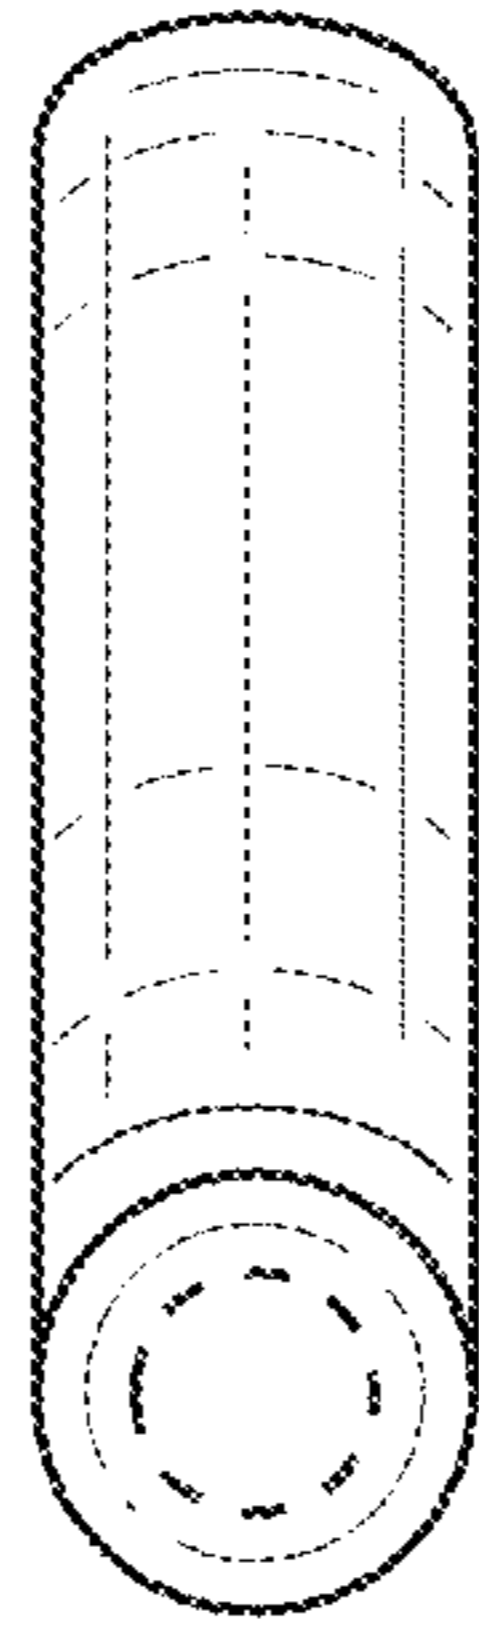


FIG. 7