



US00D871439S

(12) **United States Design Patent**  
**Peeters et al.**

(10) **Patent No.:** **US D871,439 S**

(45) **Date of Patent:** **\*\* Dec. 31, 2019**

(54) **DISPLAY SCREEN WITH ANIMATED GRAPHICAL USER INTERFACE**

D692,444 S \* 10/2013 Lee ..... D14/486  
D730,366 S \* 5/2015 Brush ..... D14/485

(Continued)

(71) Applicant: **KONINKLIJKE PHILIPS N.V.**,  
Eindhoven (NL)

(72) Inventors: **Harold Johannes Antonius Peeters**,  
Eindhoven (NL); **Pieter Frank De Jong**,  
Eindhoven (NL); **Rudolf Theodoor Springorum**,  
Eindhoven (NL); **Willem Christiaan Constantijn Furster**,  
Eindhoven (NL)

(73) Assignee: **KONINKLIJKE PHILIPS N.V.**,  
Eindhoven (NL)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/656,266**

(22) Filed: **Jul. 11, 2018**

(30) **Foreign Application Priority Data**

Jan. 11, 2018 (EM) ..... 004662500-0001

(51) **LOC (12) Cl.** ..... **14-04**

(52) **U.S. Cl.**  
USPC ..... **D14/487**

(58) **Field of Classification Search**

USPC ..... D14/485-495; D20/11; D21/324, 325  
CPC .... G06F 3/048; G06F 3/0481; G06F 3/04817;  
G06F 3/0482; G06F 3/0483; G06F  
3/04842; G06F 3/0485; G06F 3/04855;  
G06F 3/0486; G06F 3/0488; G06F  
3/04886; G06F 9/4443; G06F 17/211;  
G06F 17/212; G06F 19/321; A61B 90/90;  
A61J 7/04; G01R 33/543; G01R 33/546;  
G06Q 30/06; G07C 1/08

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D575,792 S \* 8/2008 Benson ..... D14/486  
8,336,917 B2 \* 12/2012 Doiron ..... A61J 7/04  
283/115

OTHER PUBLICATIONS

“Warning Sign” Aug. 4, 2017, posted at dribbble.com, [site visited Aug. 20, 2019]. <https://dribbble.com/shots/3712534-Warning-Sign>.\*

(Continued)

*Primary Examiner* — Jack Reickel  
*Assistant Examiner* — John M Otte

(57) **CLAIM**

The ornamental design for a display screen with animated graphical user interface, as shown and described.

**DESCRIPTION**


FIG. 1 is a front view of a first image in a sequence of a display screen with animated graphical user interface, showing our new design;

FIG. 2 is a front view of a second image thereof; and, FIG. 3 is a front view of a third image thereof.

The appearance of the animated graphical user interface sequentially transitions between the images shown in FIGS. 1-3. The process or period in which an image transitions to another forms no part of the claimed design.

The broken lines of uneven length show the display screen and form no part of the claimed design. The long-dash broken lines illustrate portions of the display screen with animated graphical user interface that form no part of the claimed design. The short-dash broken lines surrounding the torso of the unclaimed human figure in FIGS. 1 and 3 form part of the claimed design.

**1 Claim, 3 Drawing Sheets**

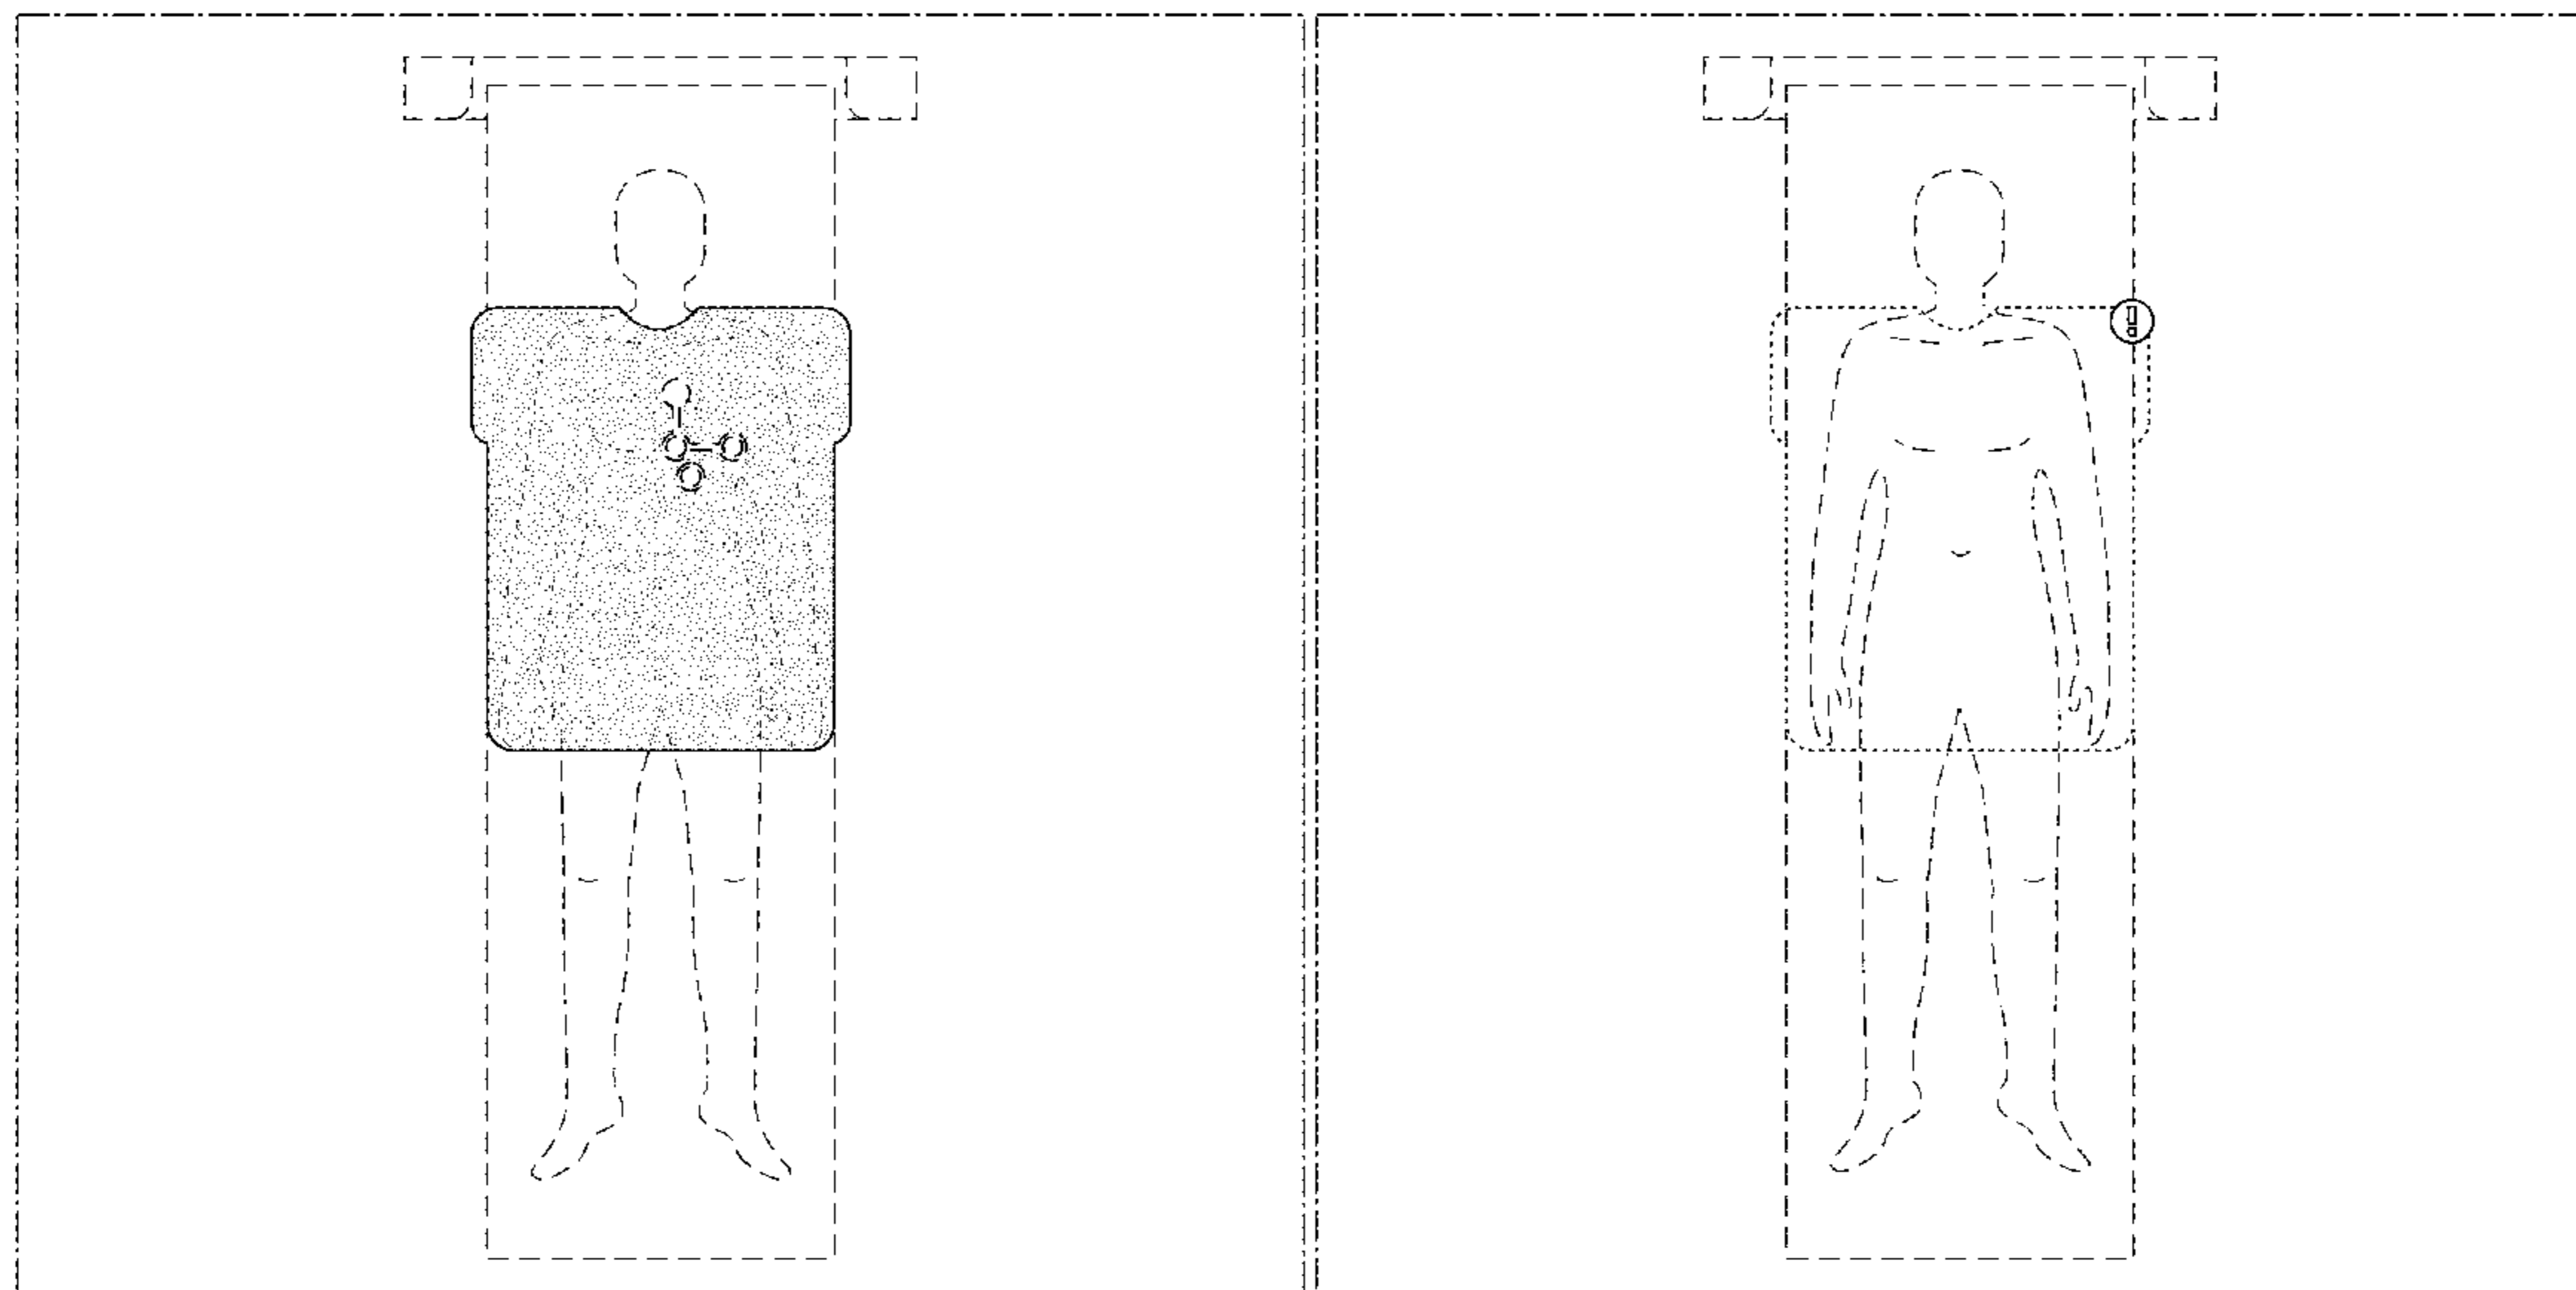

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D750,126 S \* 2/2016 Lee ..... D14/489  
D754,198 S \* 4/2016 Moon ..... D14/492  
D772,891 S \* 11/2016 Nook ..... D14/485  
D837,231 S \* 1/2019 Nook ..... D14/485  
2017/0193712 A1 \* 7/2017 Keller ..... G07C 1/08  
2018/0089727 A1 \* 3/2018 Neville ..... G06Q 30/06  
2018/0356482 A1 \* 12/2018 Kaufholz ..... G01R 33/543  
2019/0154780 A1 \* 5/2019 Traverso ..... G01R 33/546


OTHER PUBLICATIONS

“Images GIF” May 13, 2017, posted at [gfycat.com](http://gfycat.com), [site visited Aug. 20, 2019]. <https://gfycat.com/presentheavenlyharvestmouse>.\*


“MRI revealed that the human brain partially stops when too many security warnings are seen.” Mar. 23, 2015, posted at [gigazine.net](http://gigazine.net), [site visited Aug. 20, 2019]. [https://gigazine.net/gsc\\_news/en/20150323-brains-shutdown-security-prompt](https://gigazine.net/gsc_news/en/20150323-brains-shutdown-security-prompt).\*

Frauenrath, Tobias, “Fig 3” Jan. 2012, posted at [researchgate.net](http://researchgate.net), [site visited Aug. 15, 2019]. [https://www.researchgate.net/figure/Basic-setup-for-ECG-monitoring-in-a-clinical-MRI-environment-Patient-preparation-such-as\\_fig3\\_221923127](https://www.researchgate.net/figure/Basic-setup-for-ECG-monitoring-in-a-clinical-MRI-environment-Patient-preparation-such-as_fig3_221923127).\*


\* cited by examiner

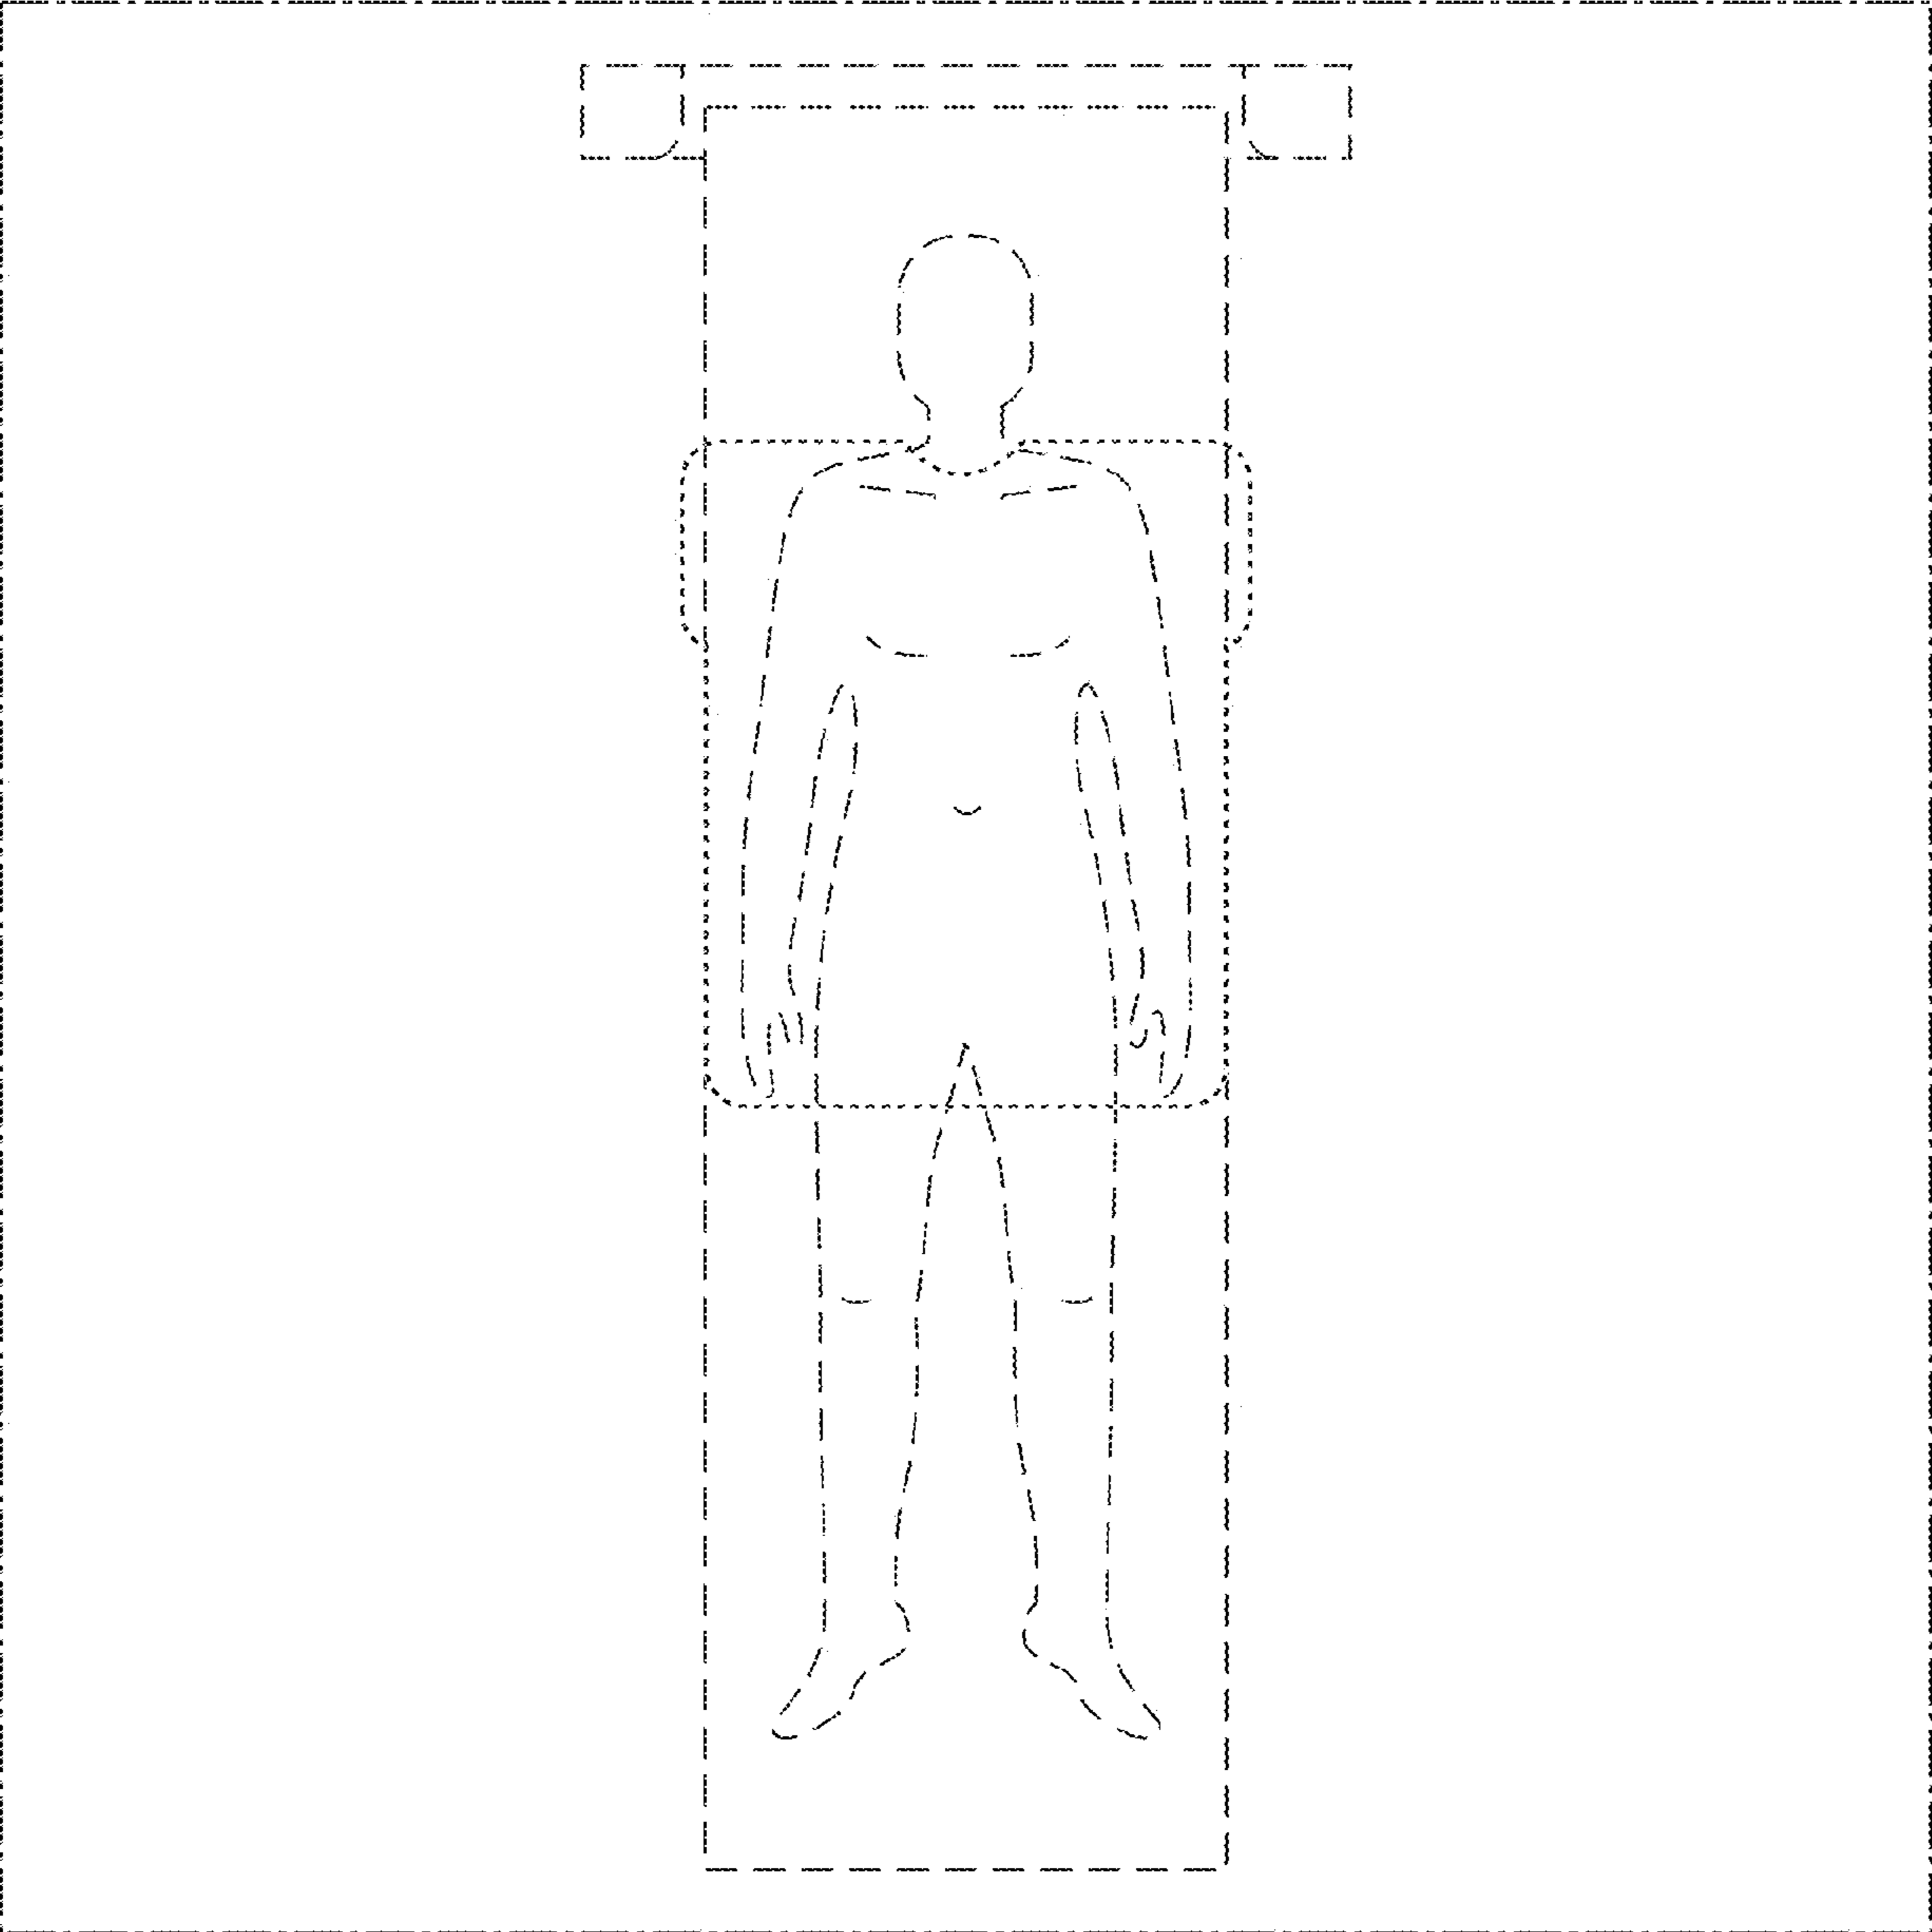

**FIG. 1**

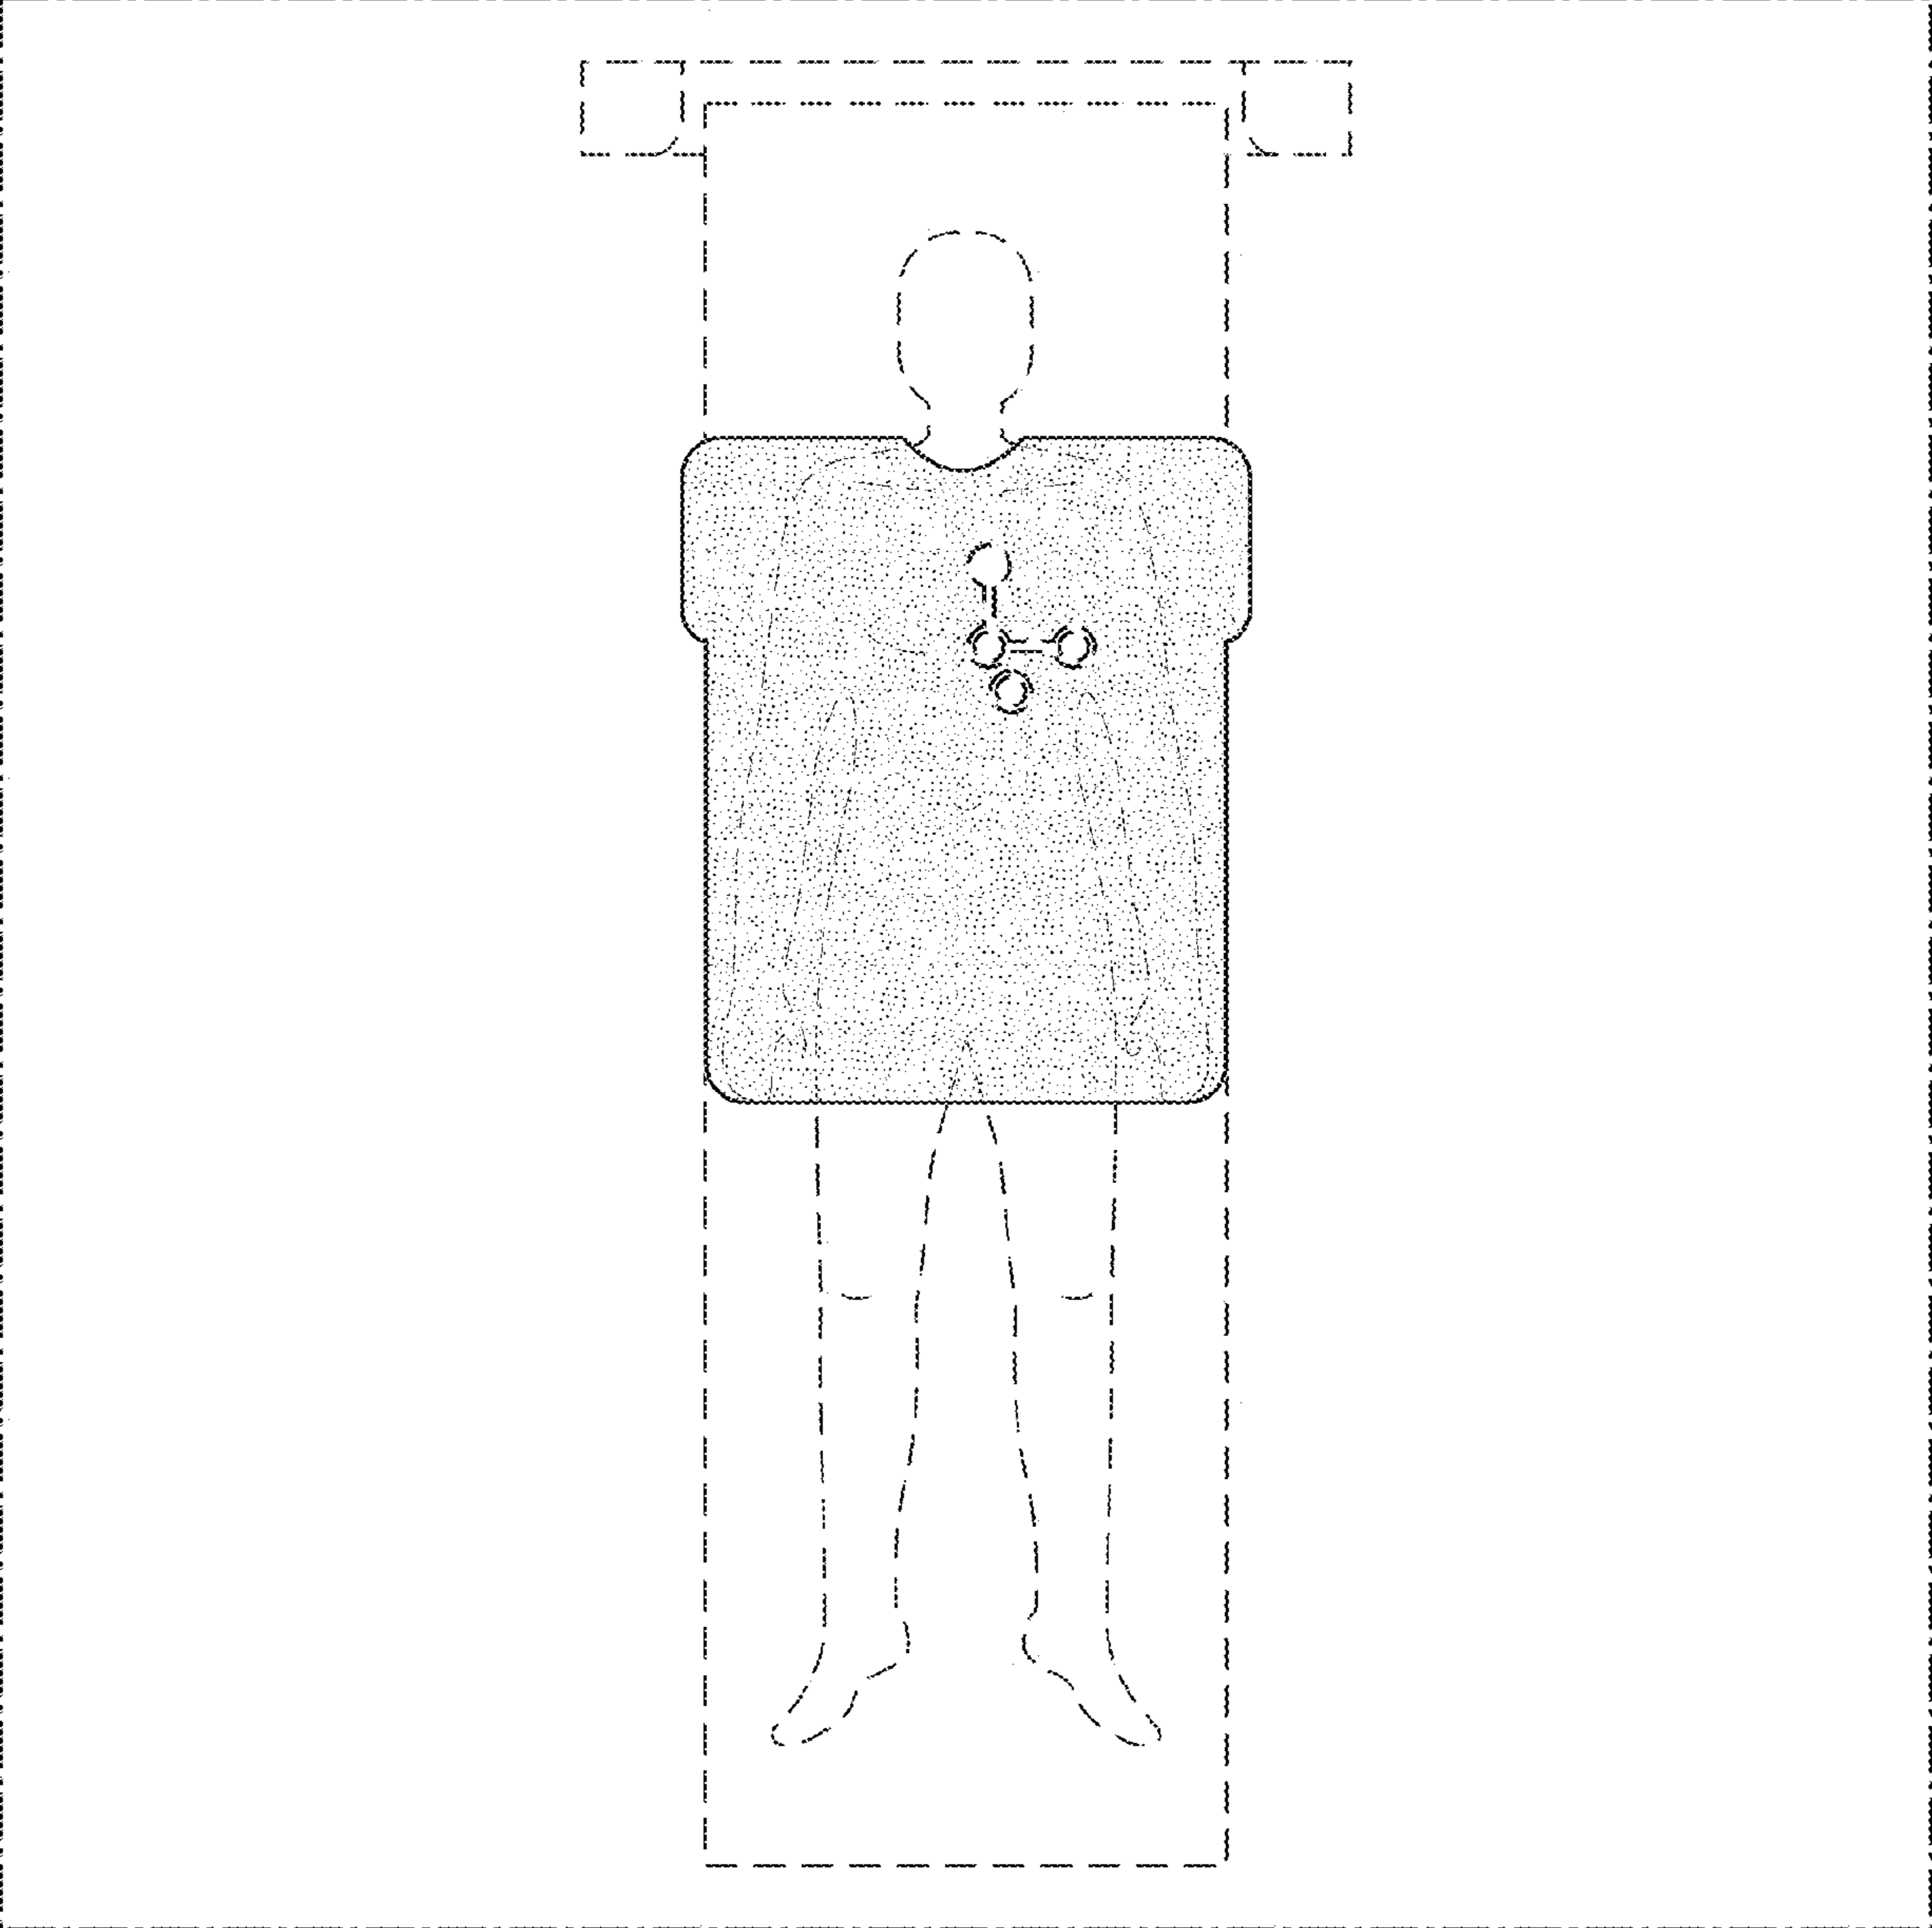

**FIG. 2**

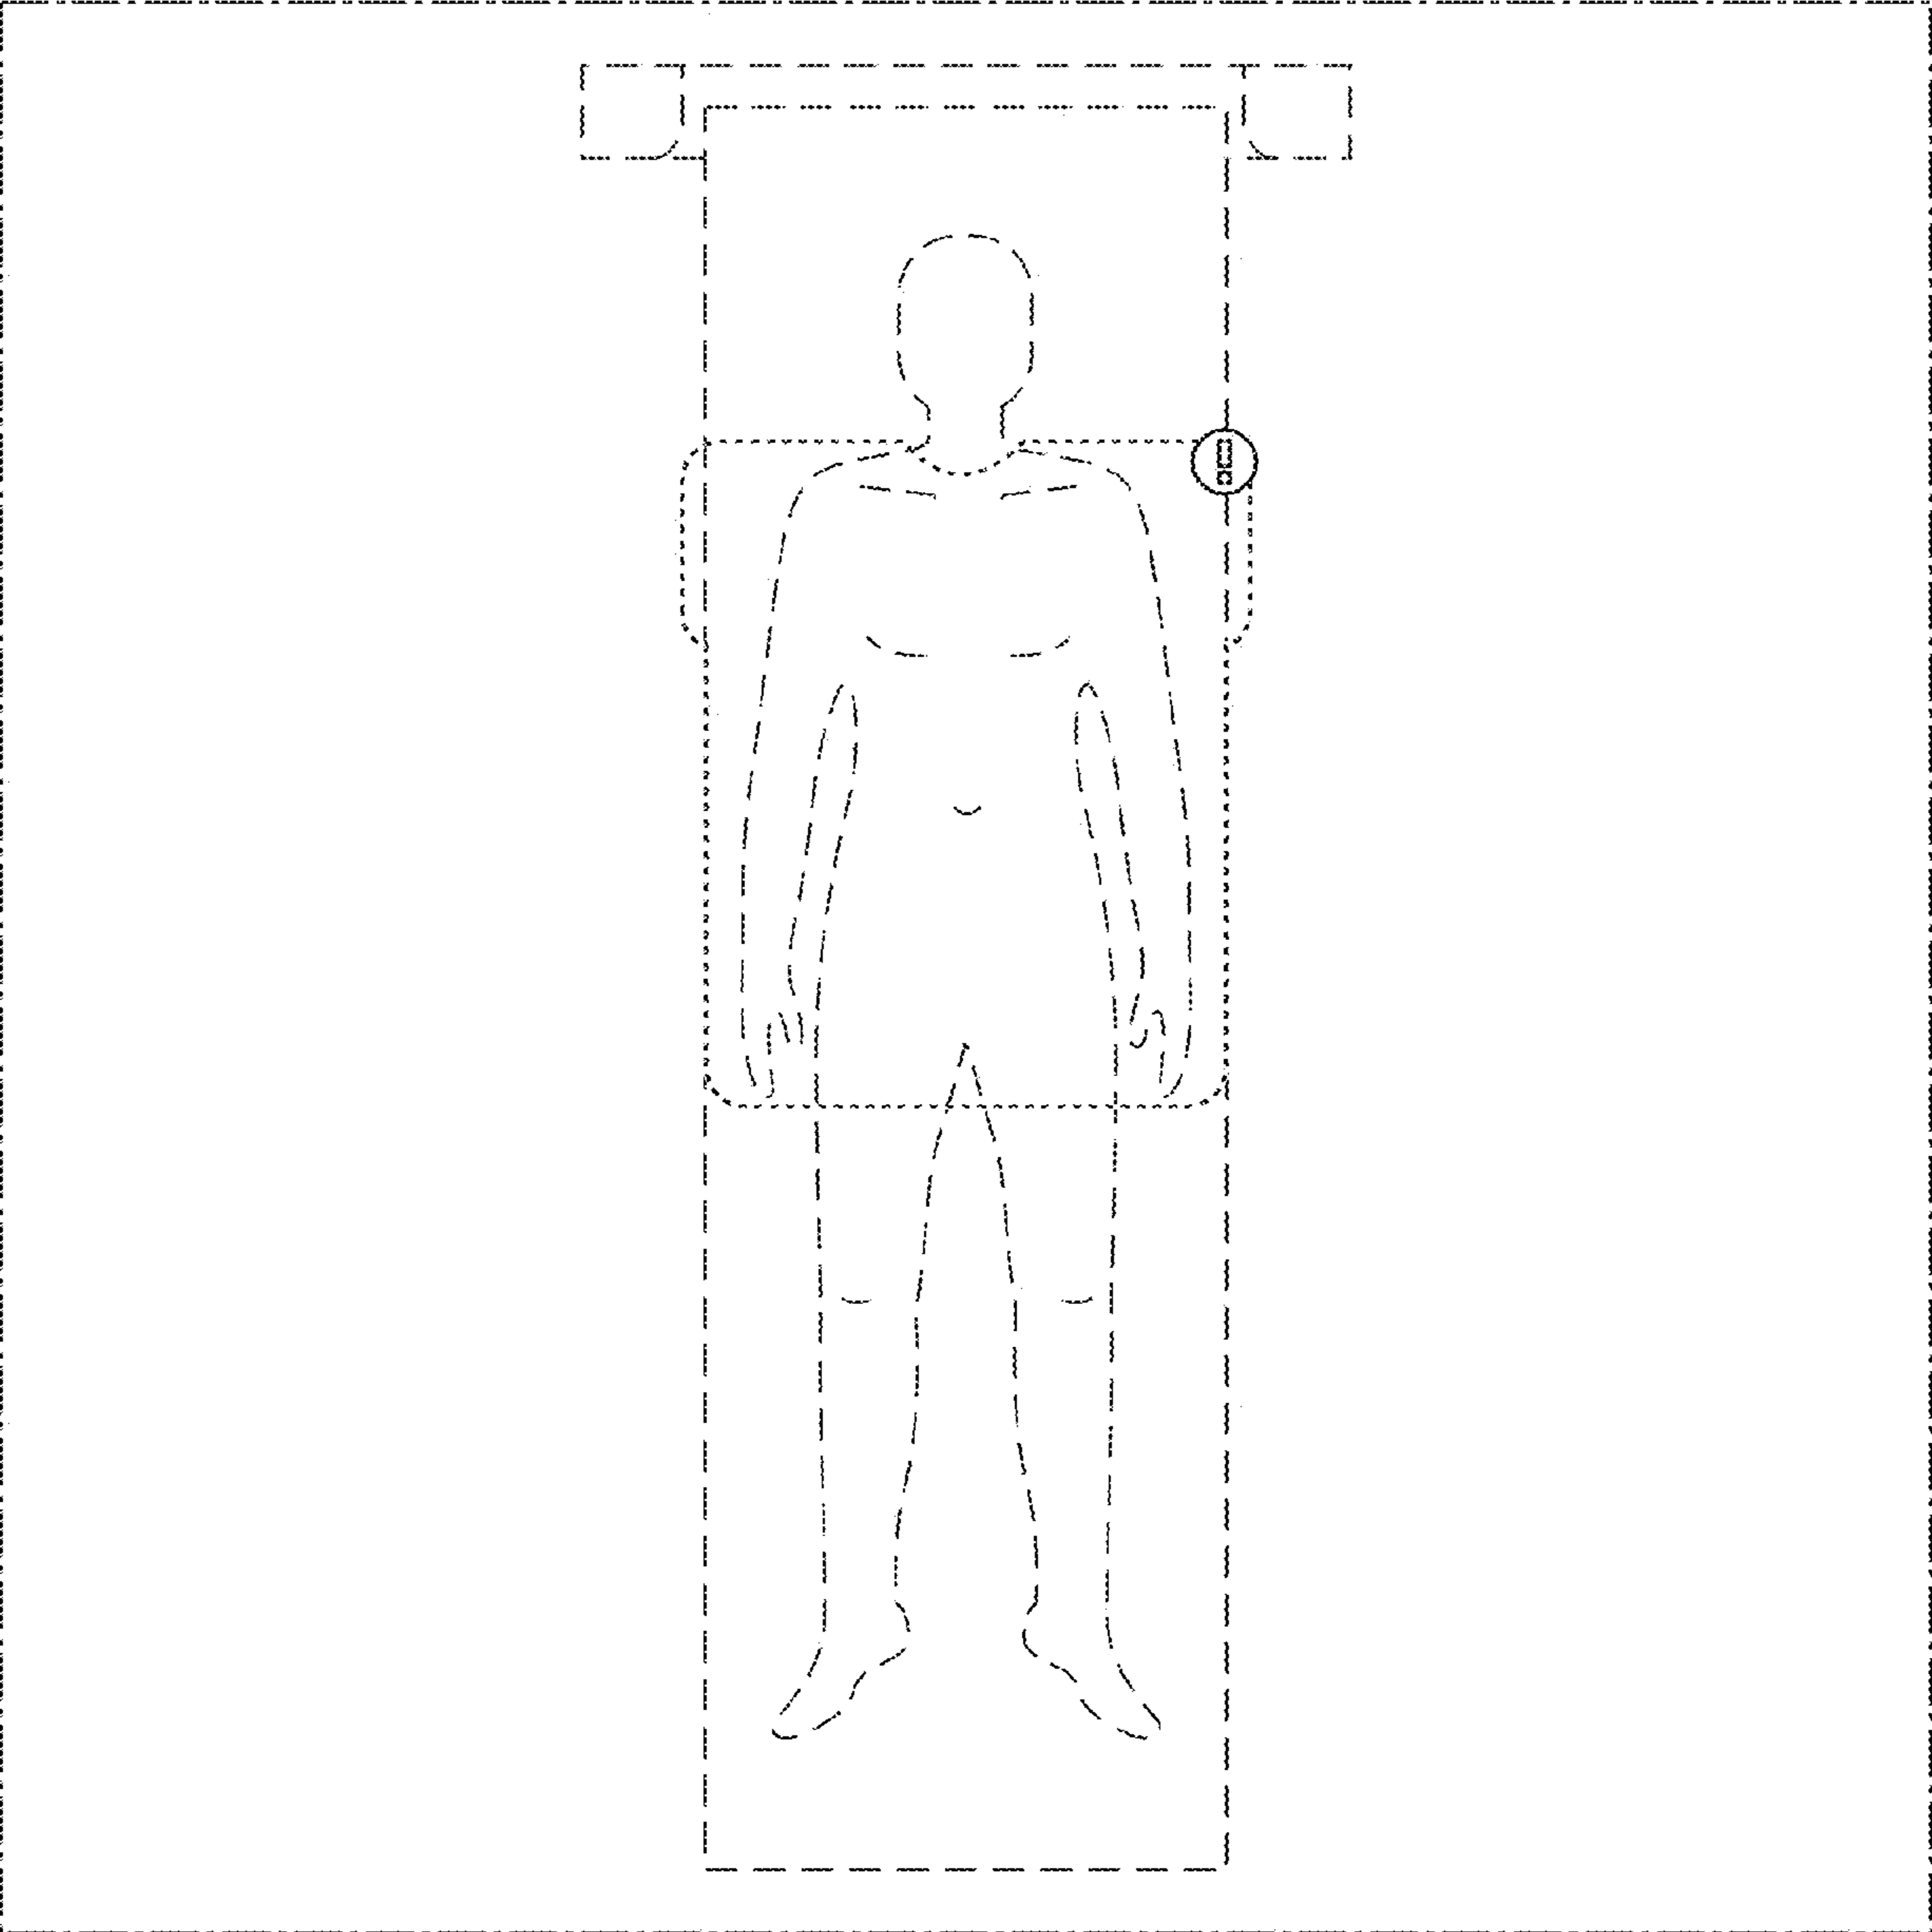

**FIG. 3**