



US00D871578S

(12) **United States Design Patent** (10) **Patent No.:** **US D871,578 S**
Shah et al. (45) **Date of Patent:** **** Dec. 31, 2019**

(54) **PROXIMAL HUMERAL FRACTURE PLATE**(71) Applicants: **Anup A. Shah**, Sugar Land, TX (US);
Joshua T. Woody, Houston, TX (US)(72) Inventors: **Anup A. Shah**, Sugar Land, TX (US);
Joshua T. Woody, Houston, TX (US)(**) Term: **15 Years**(21) Appl. No.: **29/645,975**(22) Filed: **Apr. 30, 2018****Related U.S. Application Data**

(62) Division of application No. 29/524,660, filed on Apr. 22, 2015, now Pat. No. Des. 816,840.

(51) **LOC (12) Cl.** **24-03**(52) **U.S. Cl.**USPC **D24/155**(58) **Field of Classification Search**USPC D24/155-157
CPC A61B 17/8061; A61B 17/7059; A61B 17/8052; A61B 17/8605; A61B 17/8085; A61B 17/809; A61B 17/8014; A61B 17/8033; A61B 17/8004; A61B 17/888; A61B 17/842; A61B 17/8023; A61B 17/8009; A61B 17/86; A61B 17/1739; A61B 17/8066; A61B 17/1671; A61B 17/1757; A61B 17/8071; A61B 17/176; A61B 2017/1782; A61B 2017/1775

See application file for complete search history.

(56)

References Cited**U.S. PATENT DOCUMENTS**

4,919,670 A	4/1990	Dale et al.
5,066,296 A	11/1991	Chapman et al.
5,112,333 A	5/1992	Fixel
5,489,309 A	2/1996	Lackey et al.
5,507,517 A	4/1996	Krawczak
5,776,194 A	7/1998	Mikol et al.
6,096,040 A	8/2000	Esser
6,468,278 B1	10/2002	Muckter
7,001,388 B2	2/2006	Orbay et al.


D576,731 S	*	9/2008	Strnad	D24/155
D589,148 S	*	3/2009	Strnad	D24/155
D589,149 S	*	3/2009	Strnad	D24/155
7,655,029 B2		2/2010	Niederberger et al.	
7,731,718 B2		6/2010	Schwammberger et al.	
D646,785 S	*	10/2011	Milford	D24/155
RE43,482 E		6/2012	Mikol et al.	
D664,253 S	*	7/2012	Pech	D24/155
D665,082 S	*	8/2012	Milford	D24/155
8,287,538 B2		10/2012	Brenzel et al.	
8,337,534 B2		12/2012	Celli et al.	
D700,334 S	*	2/2014	Borostyankoi	D24/155
8,906,070 B2		12/2014	Medoff	
D816,840 S	*	5/2018	Shah	D24/155
2004/0167522 A1		8/2004	Niederberger et al.	
2005/0085818 A1*		4/2005	Huebner	A61B 17/1728 606/281
2005/0245931 A1*		11/2005	Orbay	A61B 17/1728 606/291
2007/0088360 A1*		4/2007	Orbay	A61B 17/8057 606/287
2008/0021477 A1*		1/2008	Strnad	A61B 17/8033 606/287
2009/0281578 A1		11/2009	Spencer	
2011/0224736 A1		9/2011	Humphrey	
2011/0313422 A1		12/2011	Schwager et al.	
2012/0016366 A1		1/2012	Eglseder	
2012/0136396 A1		5/2012	Baker et al.	
2012/0179208 A1		7/2012	Geissler et al.	
2012/0226323 A1		9/2012	Gonzalez-Hernandez	
2013/0096629 A1		4/2013	Rollinghof et al.	
2016/0022336 A1		1/2016	Bateman	

FOREIGN PATENT DOCUMENTS

CN	201020679245.9	U	12/2010
DE	102005043285	B3	12/2002
EP	2474278	A2	11/2012
WO	2014110421	A1	7/2014

OTHER PUBLICATIONS

Jayakumar, Prakash, et al. , A Pittfall in Fixation of Distal Humeral Fractures with Pre-Contoured Locking Plate Compression, Case Report, Apr. 2015, pp. 130-133, vol. 2015:3(2), The Archives of Bone and Joint Surgery, Mashhad University of Medical Sciences, Iranian Society of Knee Surgery, Arthroscopy and Sports Traumatology, Iranian Orthopedic Association, Mashhad, Iran.
Makins, Surgeon-General, Sir George H., K.C.M.G., C.B., F.R.C.S., The Development of British Surgery in the Hospitals on the Lines

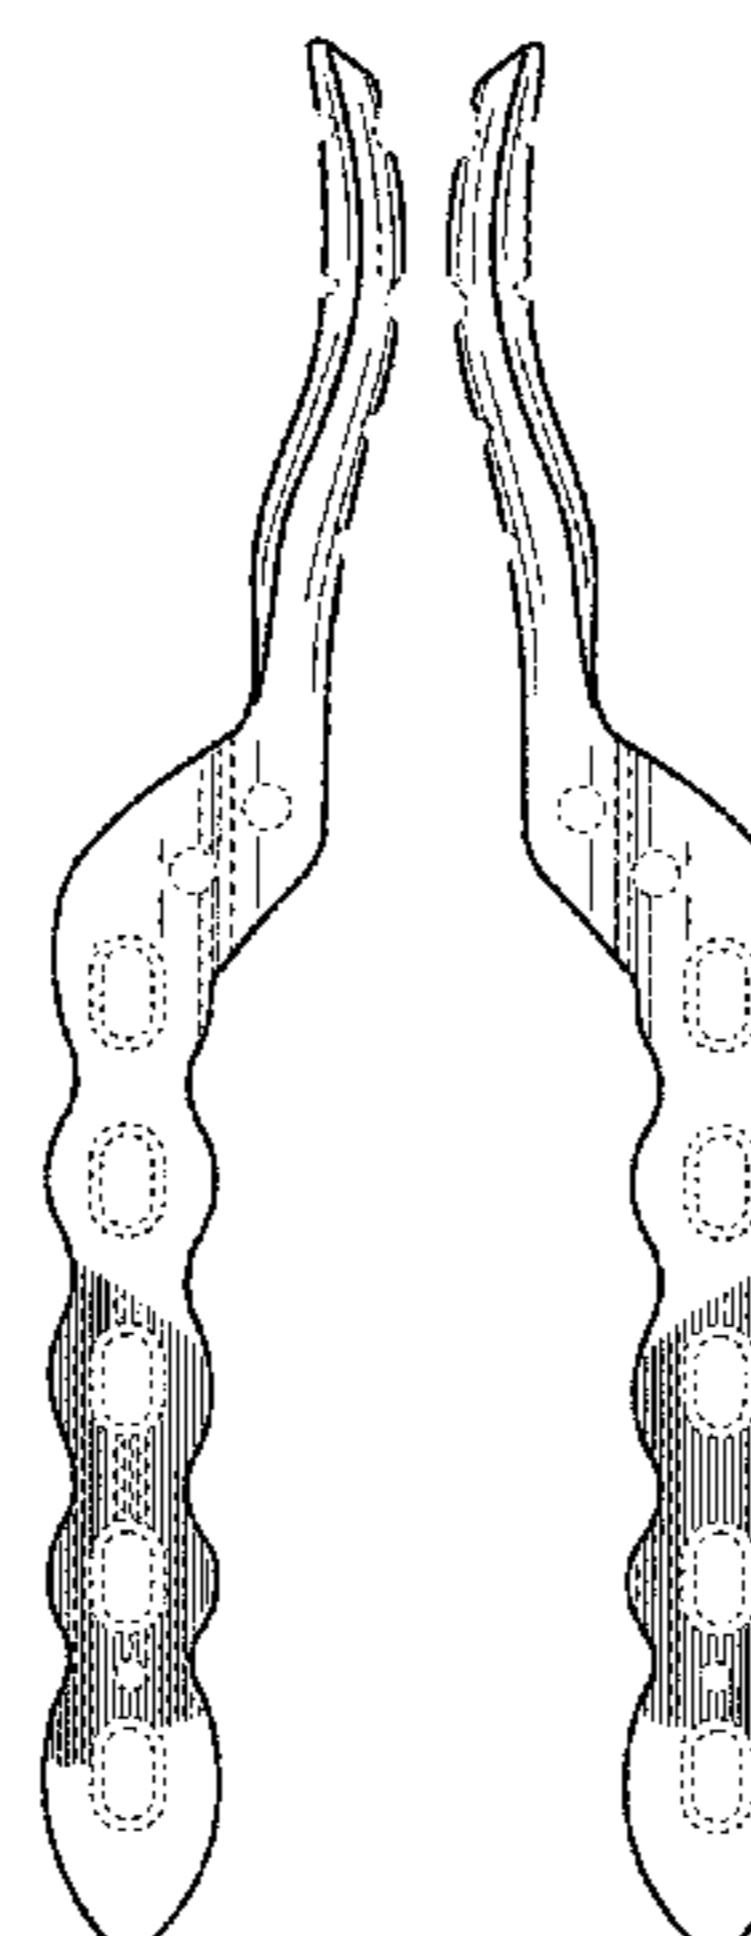

- of Communication in France, Journal, Jun. 16, 1917, pp. 789-806, vol. 2946, The British Medical Journal, London, England, United Kingdom.
- Babhulkar, Sudhir, et al., Controversies in the Management of Intra-articular Fractures of the Distal Humerus in Adults, Journal, May-Jun. 2011, pp. 216-225, vol. 45(3), Indian Journal of Orthopedics, New Dehli, India.
- Boulton, Christina, MD, et al., Do Locking Screws Work in Plates Bent at Holes?, Journal, Apr. 2014, pp. 189-194, vol. 28, No. 4, Journal of Orthopedic Trauma, Rosemont, Illinois, United States.
- Martolla, Martta et al., Fracture of Titanium Plates Used for Mandibular Reconstruction Following Ablative Tumor Surgery, Journal, Jul. 18, 2006, pp. 345-352, Volume unknown, Wiley InterScience, Helsinki, Finland.
- Sterba, William, et al., Biomechanical Analysis of Differing Pedicle Screw Insertion Angles, Journal, May 2007, pp. 385-391, vol. 22, Issue 4, Clinical Biomechanics, Bristol, Avon.
- Singh Gurjinder, Dr. et al., Outcome of Precontoured Locking Plate Fixation in Distal Humerus Fractures, Journal, 2017, pp. 145-148, vol. 3, Issue 1, International Journal of Orthopaedics Sciences, Dehli, India.
- Ricchetti, Eric T., et al., The Use of Precontoured Humeral Locking Plates in the Management of Displaced Proximal Humeral Fracture, Journal, 2009, pp. 582-590, vol. 17, No. 9, Journal of American Academy of Orthopedic Surgeons, Philadelphia, Pennsylvania, United States.
- Gallagher, Bethany, MD, Effect of Off-Axis Screw Insertion, Insertion Torque, and Plate Contouring on Locking Screw Strength, Journal, Jul. 2014, pp. 427-432, vol. 28, No. 7, Journal of Orthopedic Trauma, Saint Louis, Missouri, United States.
- Koukakis, Athanasios, et al., Fixatation of Proximal Humerus Fractures Using Philos Plate: Early Experience, Journal, Jan. 2006, pp. 115-120, vol. 442, Clinical Orthopaedics and Related Research, A Publication of the Association of Bone and Joint Surgeons, Lippencott Williams and Wilkins, Philadelphia, Pennsylvania, United States.
- Jabran, Ali, et al., Biomedical Analysis of Plate Systems for Proximal Humerus Fractures: A Systematic Literature Review, Biomedical Engineering Online, available online Apr. 27, 2018, pp. 1-30, 17:47, unknown city and unknown country.
- Gottschalk, Andre, et al., Is Anesthesia Dangerous?, 2011, pp. 469-474, vol. 108, No. 27, Deutsches Arzteblatt International, unknown city, Federal Republic of Germany.
- Zimmer Periarticular Locking Plate System Brochure, undated. Produced by Zimmer Trauma, (18 pages).
- AxSOS Locking Plate System Brochure, copyrighted 2011. Produced by Stryker, (24 pages).
- Fernandez, Dell'Oca, "Helical Implants," Injury, International Journal of the Care of the Injured, 33-SA-29-40, published by Elsevier Science, Inc. (2002), unknown city and/or country (12 pages).
- Gardener, Michael et al., "Helical Plating of the Proximal Humerus," Injury, International Journal of the Care of the Injured, 36-1197-1200, published by Elsevier Science, Inc. (2005), unknown city and/or country (4 pages).
- Hanchen, Marc et al., "Mono-versus polyaxial locking plates in distal femur fractures: a prospective randomized multicenter clinical trial," 38-857-863, International Orthopedics published online on Dec. 11, 2013, Springer-Verlag, Berlin Heidelberg (7 pages).
- Apivatthalkakul, T. et al., "Danger zone for locking screw placement in minimally invasive plate osteosynthesis," Injury, International Journal of the Care of the Injured, 41-169-172, published by Elsevier Science, Inc. (2010), unknown city and/or country (4 pages).
- Yang, Kyu Hyun, "Helical plate fixation for treatment of comminuted fractures of the proximal and middle one-third of the humerus," Injury, International Journal of the Care of the Injured, 36-75-80, published by Elsevier Science, Inc. (2005), unknown city and/or country (6 pages).
- Tan, James Chung Hai et al., "Minimally Invasive Helical Plating for Shaft of Humerus Fractures: Technique and Outcome," The Open Orthopedics Journal, 2012, vol. 6, 184-188, published by Bentham Open 2012, unknown city and/or country (5 pages).
- Apivatthalkakul, T. et al., Minimally invasive plate osteosynthesis (MIPO) of the humeral shaft fracture Is it possible? A cadaveric study and preliminary report, International Journal of the Care of the Injured, 36-530-538, published by Elsevier Science, Inc. (2005), unknown city and/or country (9 pages).
- Fernandez, Dell'Oca, "The principle of helical implants Unusual ideas worth considering," Injury, International Journal of the Care of the Injured, 33-SA 1 27, published by Elsevier Science, Inc. (2002), unknown city and/or country (27 pages).
- Valdez, Victor, "Minimally Invasive Plate Osteosynthesis Using a Helical Plate for Metadiaphyseal Complex Fractures of the Proximal Humerus," Ortopedia Pediatrica y Cirugia Articular, published online at www.helio.com and dated Mar. 27, 2014, unknown city and/or country (9 pages).
- Smith & Nephew, Peri-Loc Locked Plating System—Proximal Humerus Fracture with Shaft Extension Case Study, Produced by Smith & Nephew, Inc. copyright 2010, (4 pages).
- Smith & Nephew, Peri-Loc Locked Plating System, Produced by Smith & Nephew, Inc. copyright 2014, (68 pages).
- Advanced Orthopedic Solutions, Proximal Humeral Plating System, webpage printed as a PDF on Oct. 30, 2019, date: unknown, pages: n/a, volume: n/a, volume-issue number: n/a, published by Advanced Orthopedic Solutions and "Copyright Advanced Orthopedic Solutions 2018," city and/or country where published: n/a. (13 pages).
- Advanced Orthopedic Solutions, Proximal Humeral Plating System, downloaded from Advanced Orthopedic Solution's website as a PDF on Oct. 30, 2019, date: unknown, pages: n/a, volume: n/a, volume-issue number: n/a, published by Advanced Orthopedic Solutions and "Copyright Advanced Orthopedic Solutions 2018 P/N 9023 Rev. B," city and/or country where published: n/a. (6 pages).
- Advanced Orthopedic Solutions, Mirror Images Alpha Plate Versus the Reverse Shoulder , downloaded from Advanced Orthopedic Solution's website as a PDF on Oct. 30, 2019, date: unknown, pages: n/a, volume: n/a, volume-issue number: n/a, published by Advanced Orthopedic Solutions, city and/or country where published: n/a. (2 pages).
- Advanced Orthopedic Solutions, Proximal Humeral Plating System including the PHP, 95° and Alpha Plate Systems Surgical Technique, PDF downloaded from Advanced Orthopedic Solution's website on Oct. 30, 2019, date: unknown, pages: n/a, volume: n/a, volume-issue number: n/a, published by Advanced Orthopedic Solutions and "Copyright Advanced Orthopedic Solutions 201 P/N 9023 Rev. B," city and/or country where published: n/a. (14 pages).

* cited by examiner

Primary Examiner — Charles D Hanson

(74) *Attorney, Agent, or Firm* — Malcolm E. Whittaker; Whittaker Law Firm

(57)

CLAIM

The ornamental design for the proximal humeral fracture plate, as shown and described.

DESCRIPTION

FIG. 1 is an environmental perspective view of a proximal humeral fracture plate for repairing a fracture of a patient's left humerus, screw holes disclaimed.

FIG. 2 is an anterior view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus, screw holes disclaimed.

FIG. 3 is a lateral view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus, screw holes disclaimed.

FIG. 4 is a medial view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus, screw holes disclaimed.

FIG. 5 is a posterior view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus, screw holes disclaimed.

FIG. 6 is a superior view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus, screw holes disclaimed.

FIG. 7 is an inferior view of the proximal humeral fracture plate for repairing a fracture of a patient's left humerus, screw holes disclaimed.

FIG. 8 is an environmental perspective view of a proximal humeral fracture plate for repairing a fracture of a patient's right humerus, screw holes disclaimed.

FIG. 9 is an anterior view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus, screw holes disclaimed.

FIG. 10 is a lateral view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus, screw holes disclaimed.


FIG. 11 is a medial view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus, screw holes disclaimed.

FIG. 12 is a posterior view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus, screw holes disclaimed.

FIG. 13 is a superior view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus, screw holes disclaimed; and,

FIG. 14 is an inferior view of the proximal humeral fracture plate for repairing a fracture of a patient's right humerus, screw holes disclaimed.

1 Claim, 4 Drawing Sheets

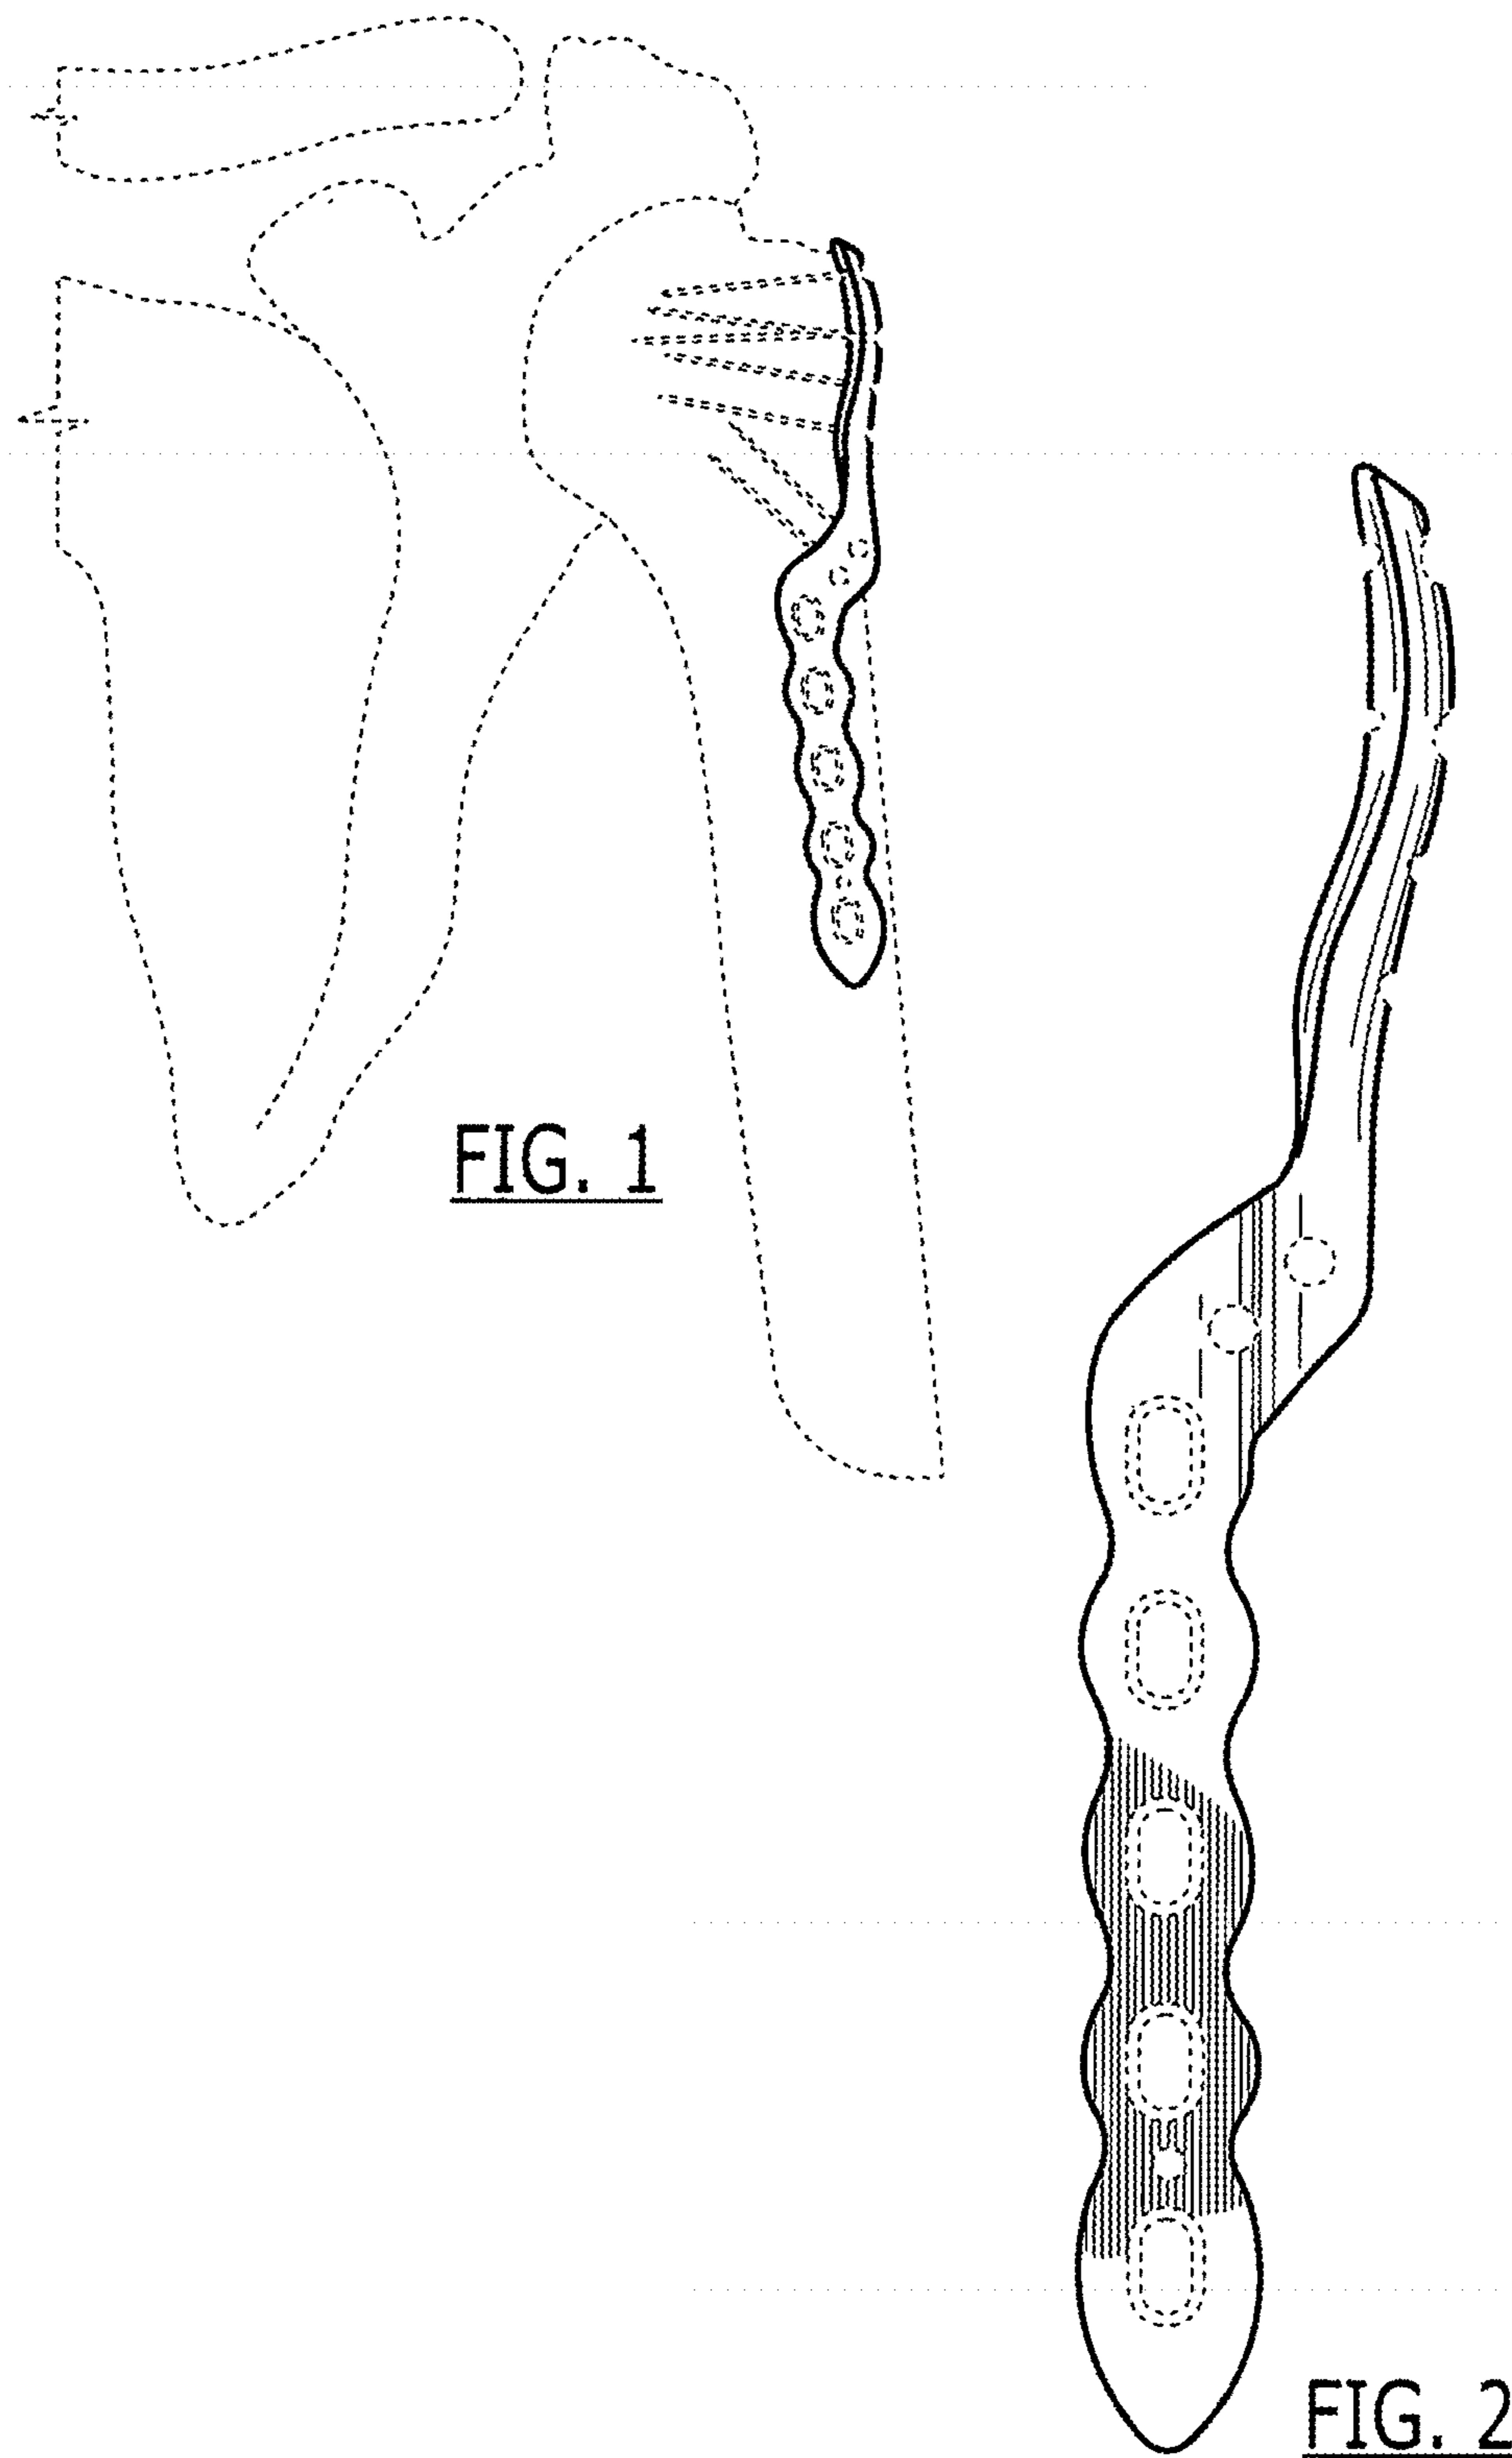

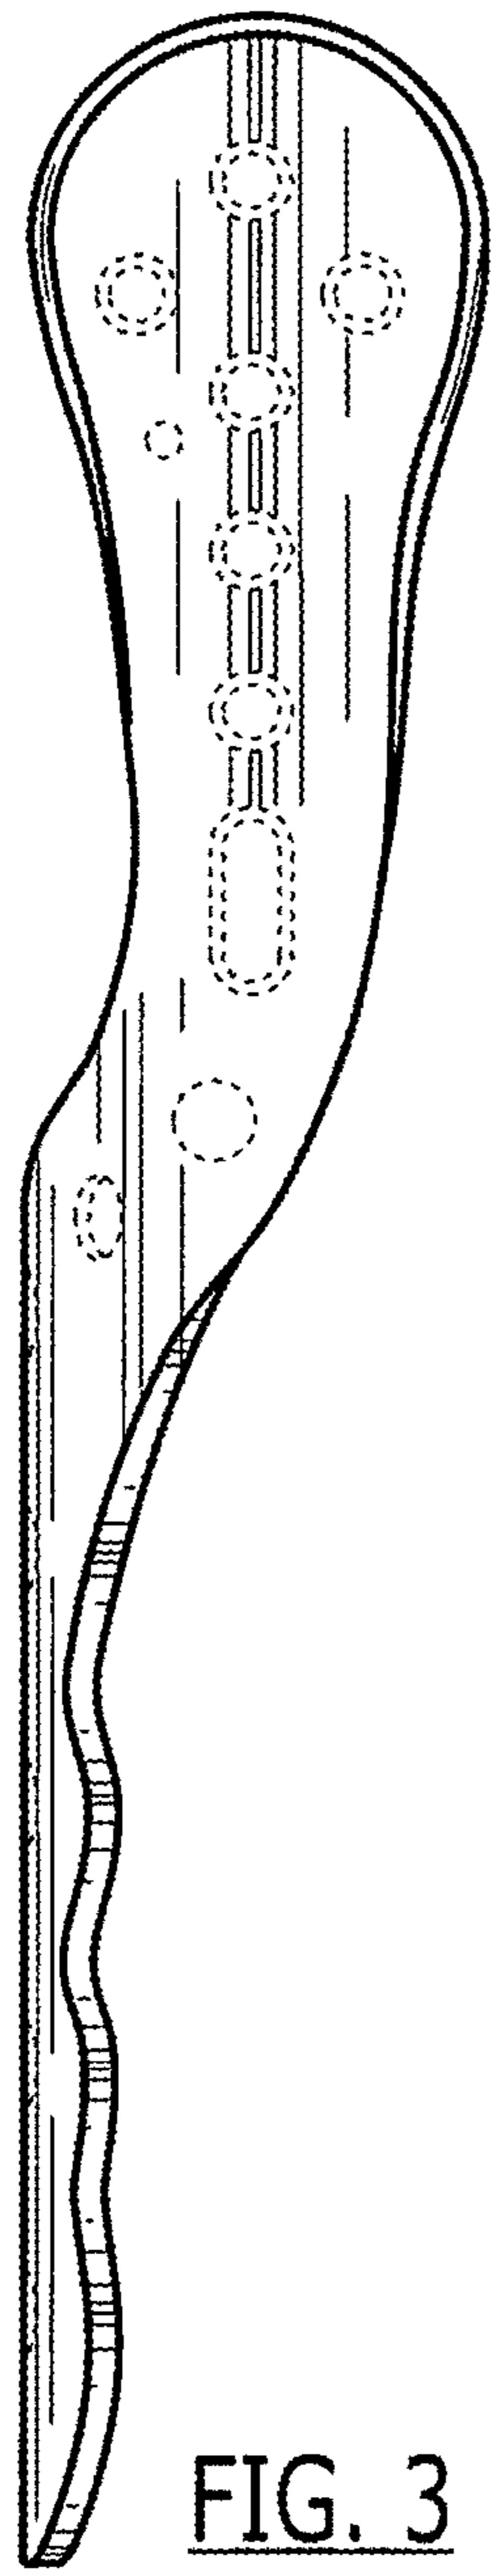


FIG. 3

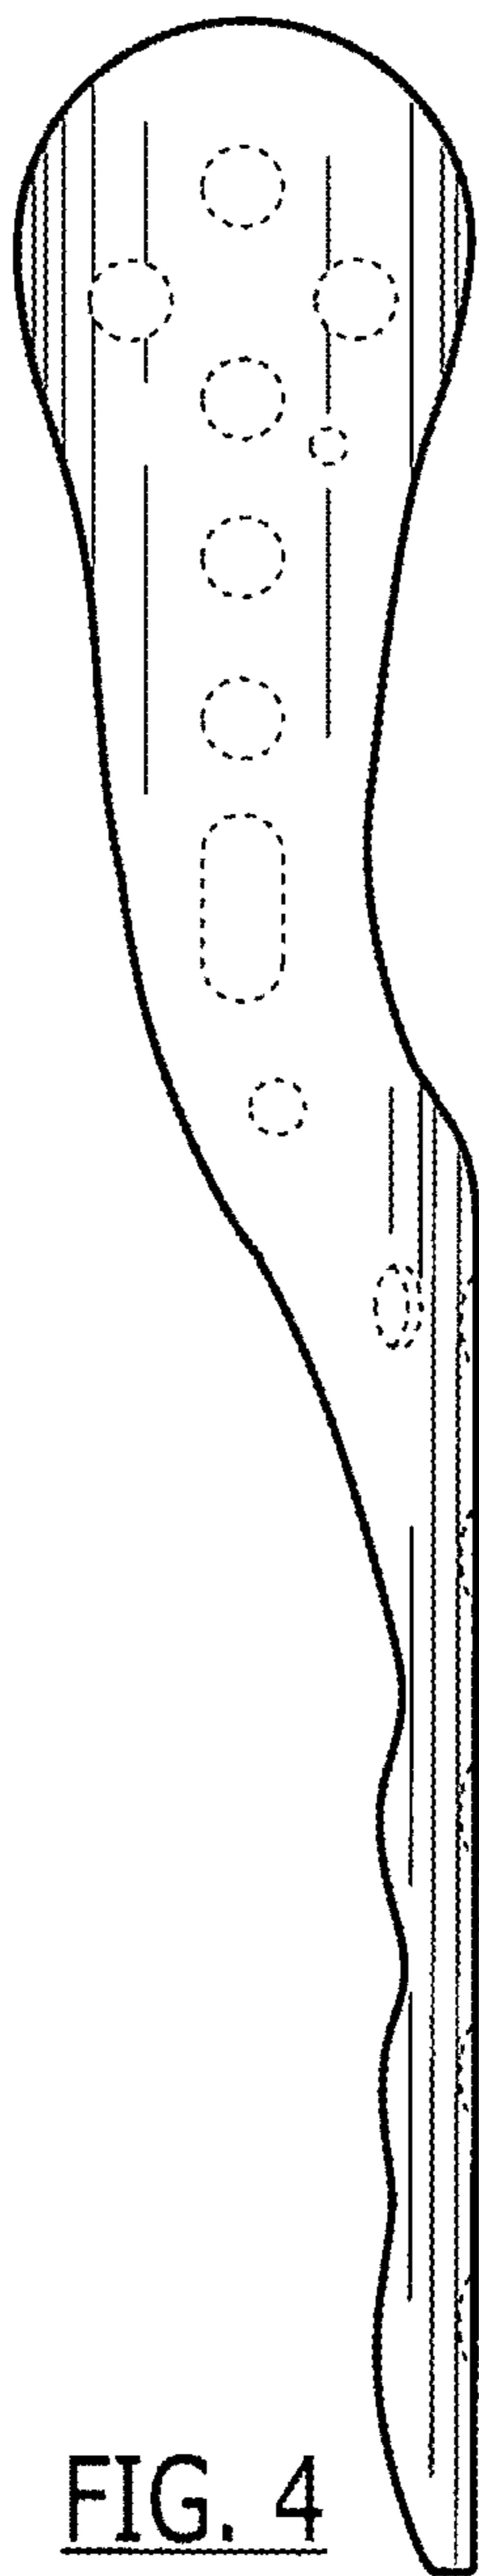


FIG. 4

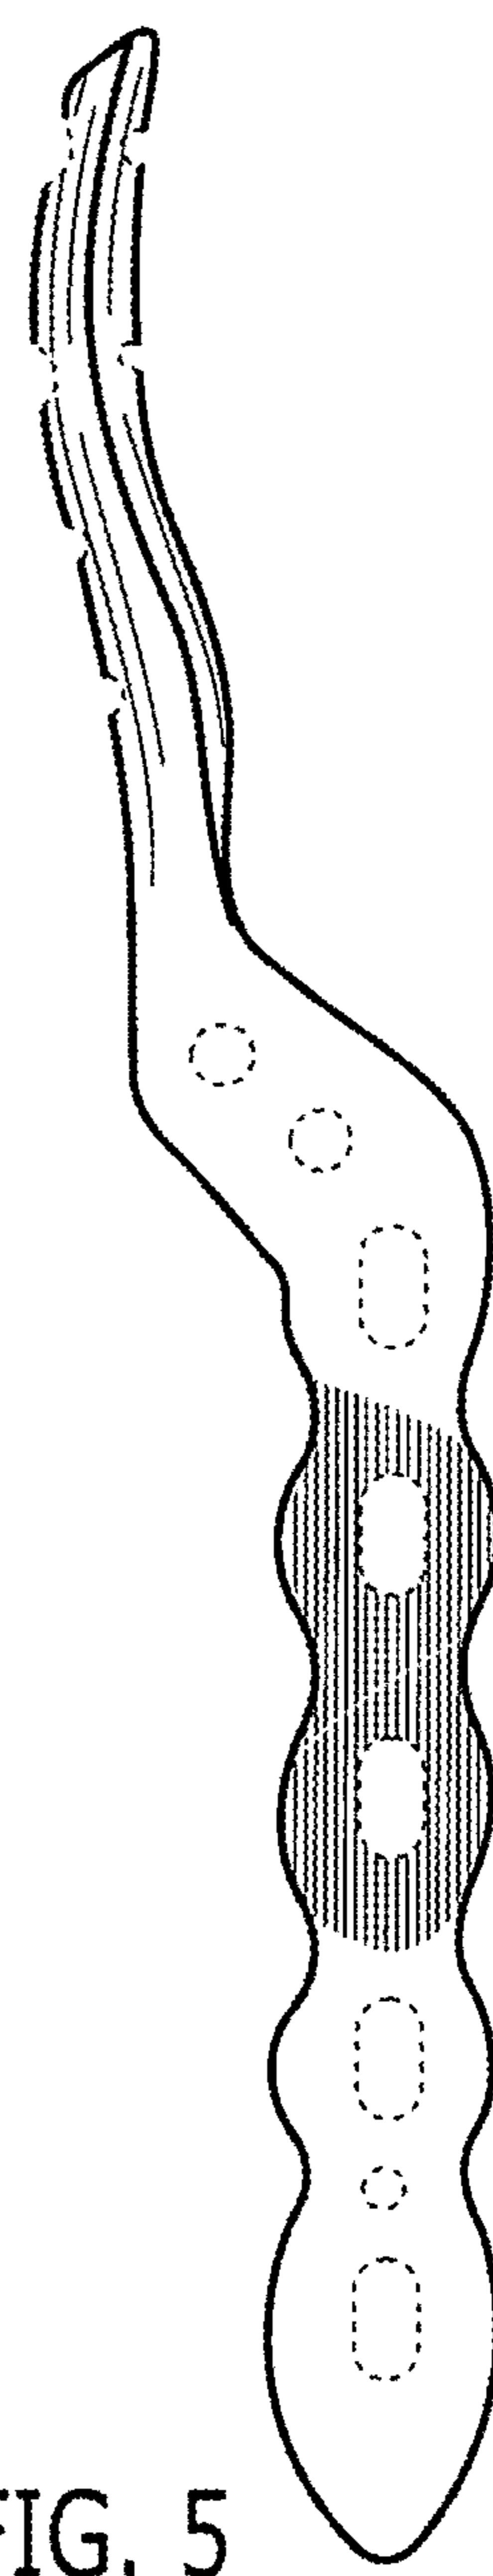


FIG. 5

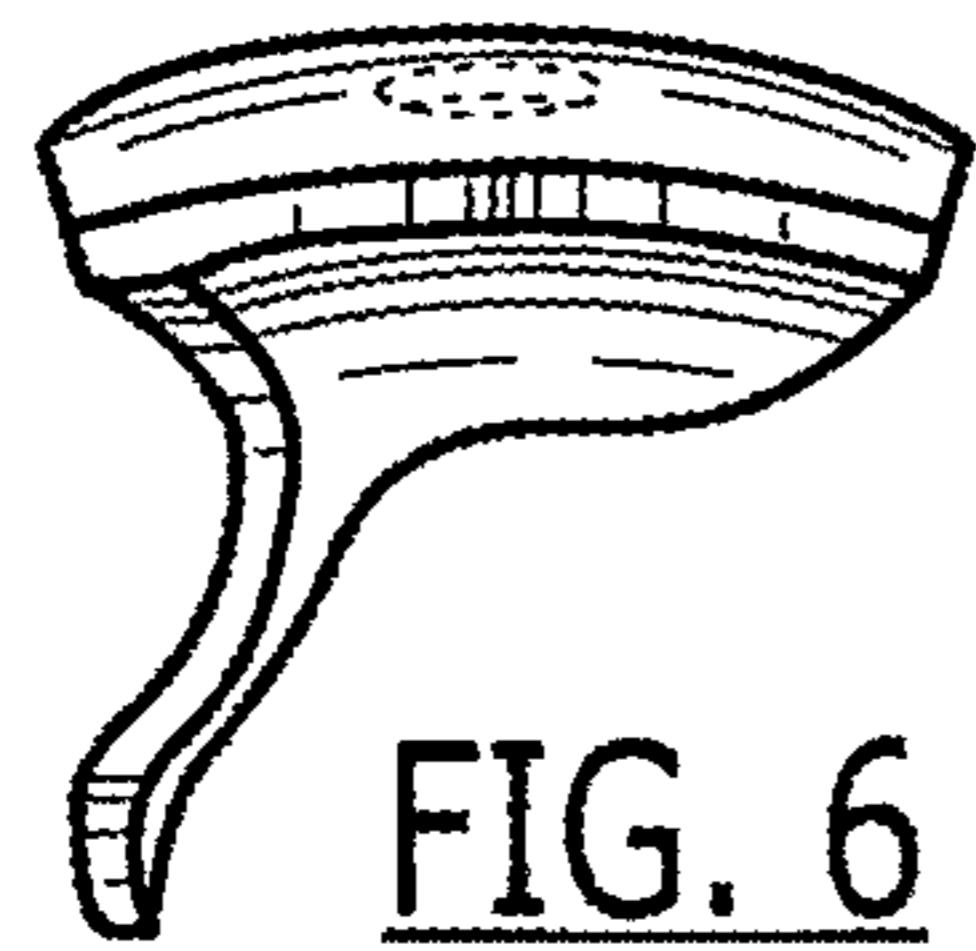


FIG. 6

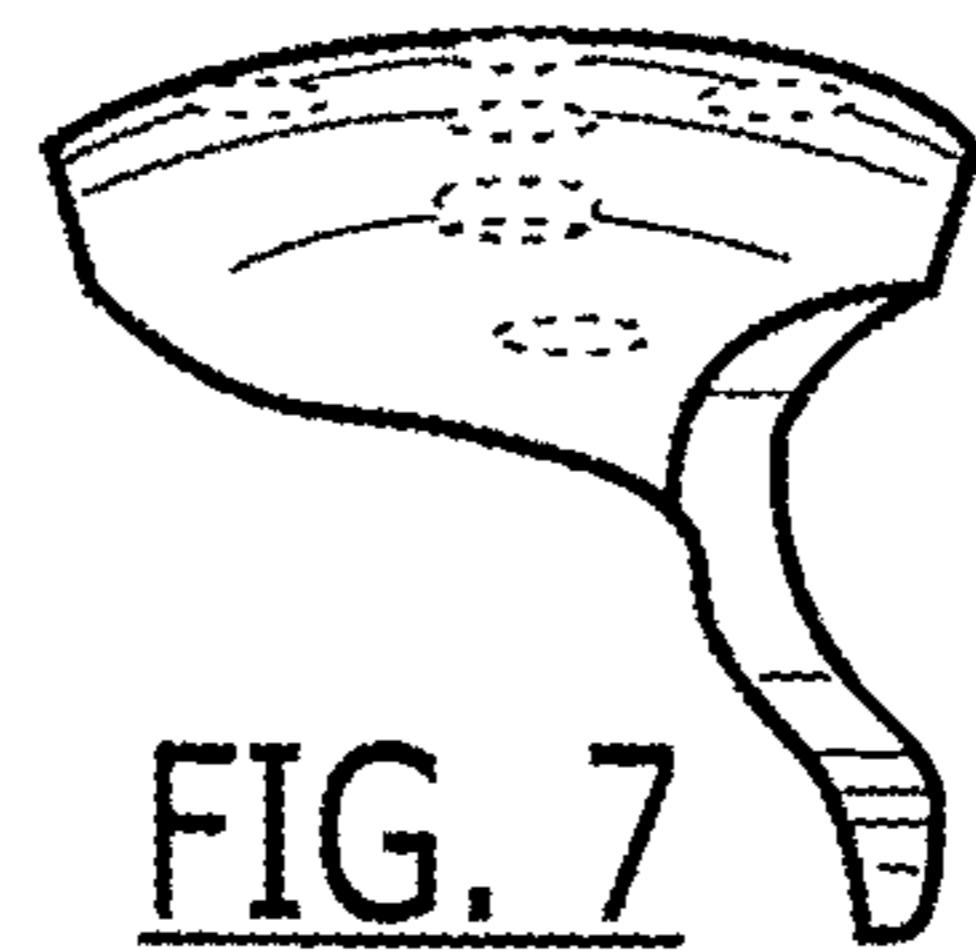


FIG. 7

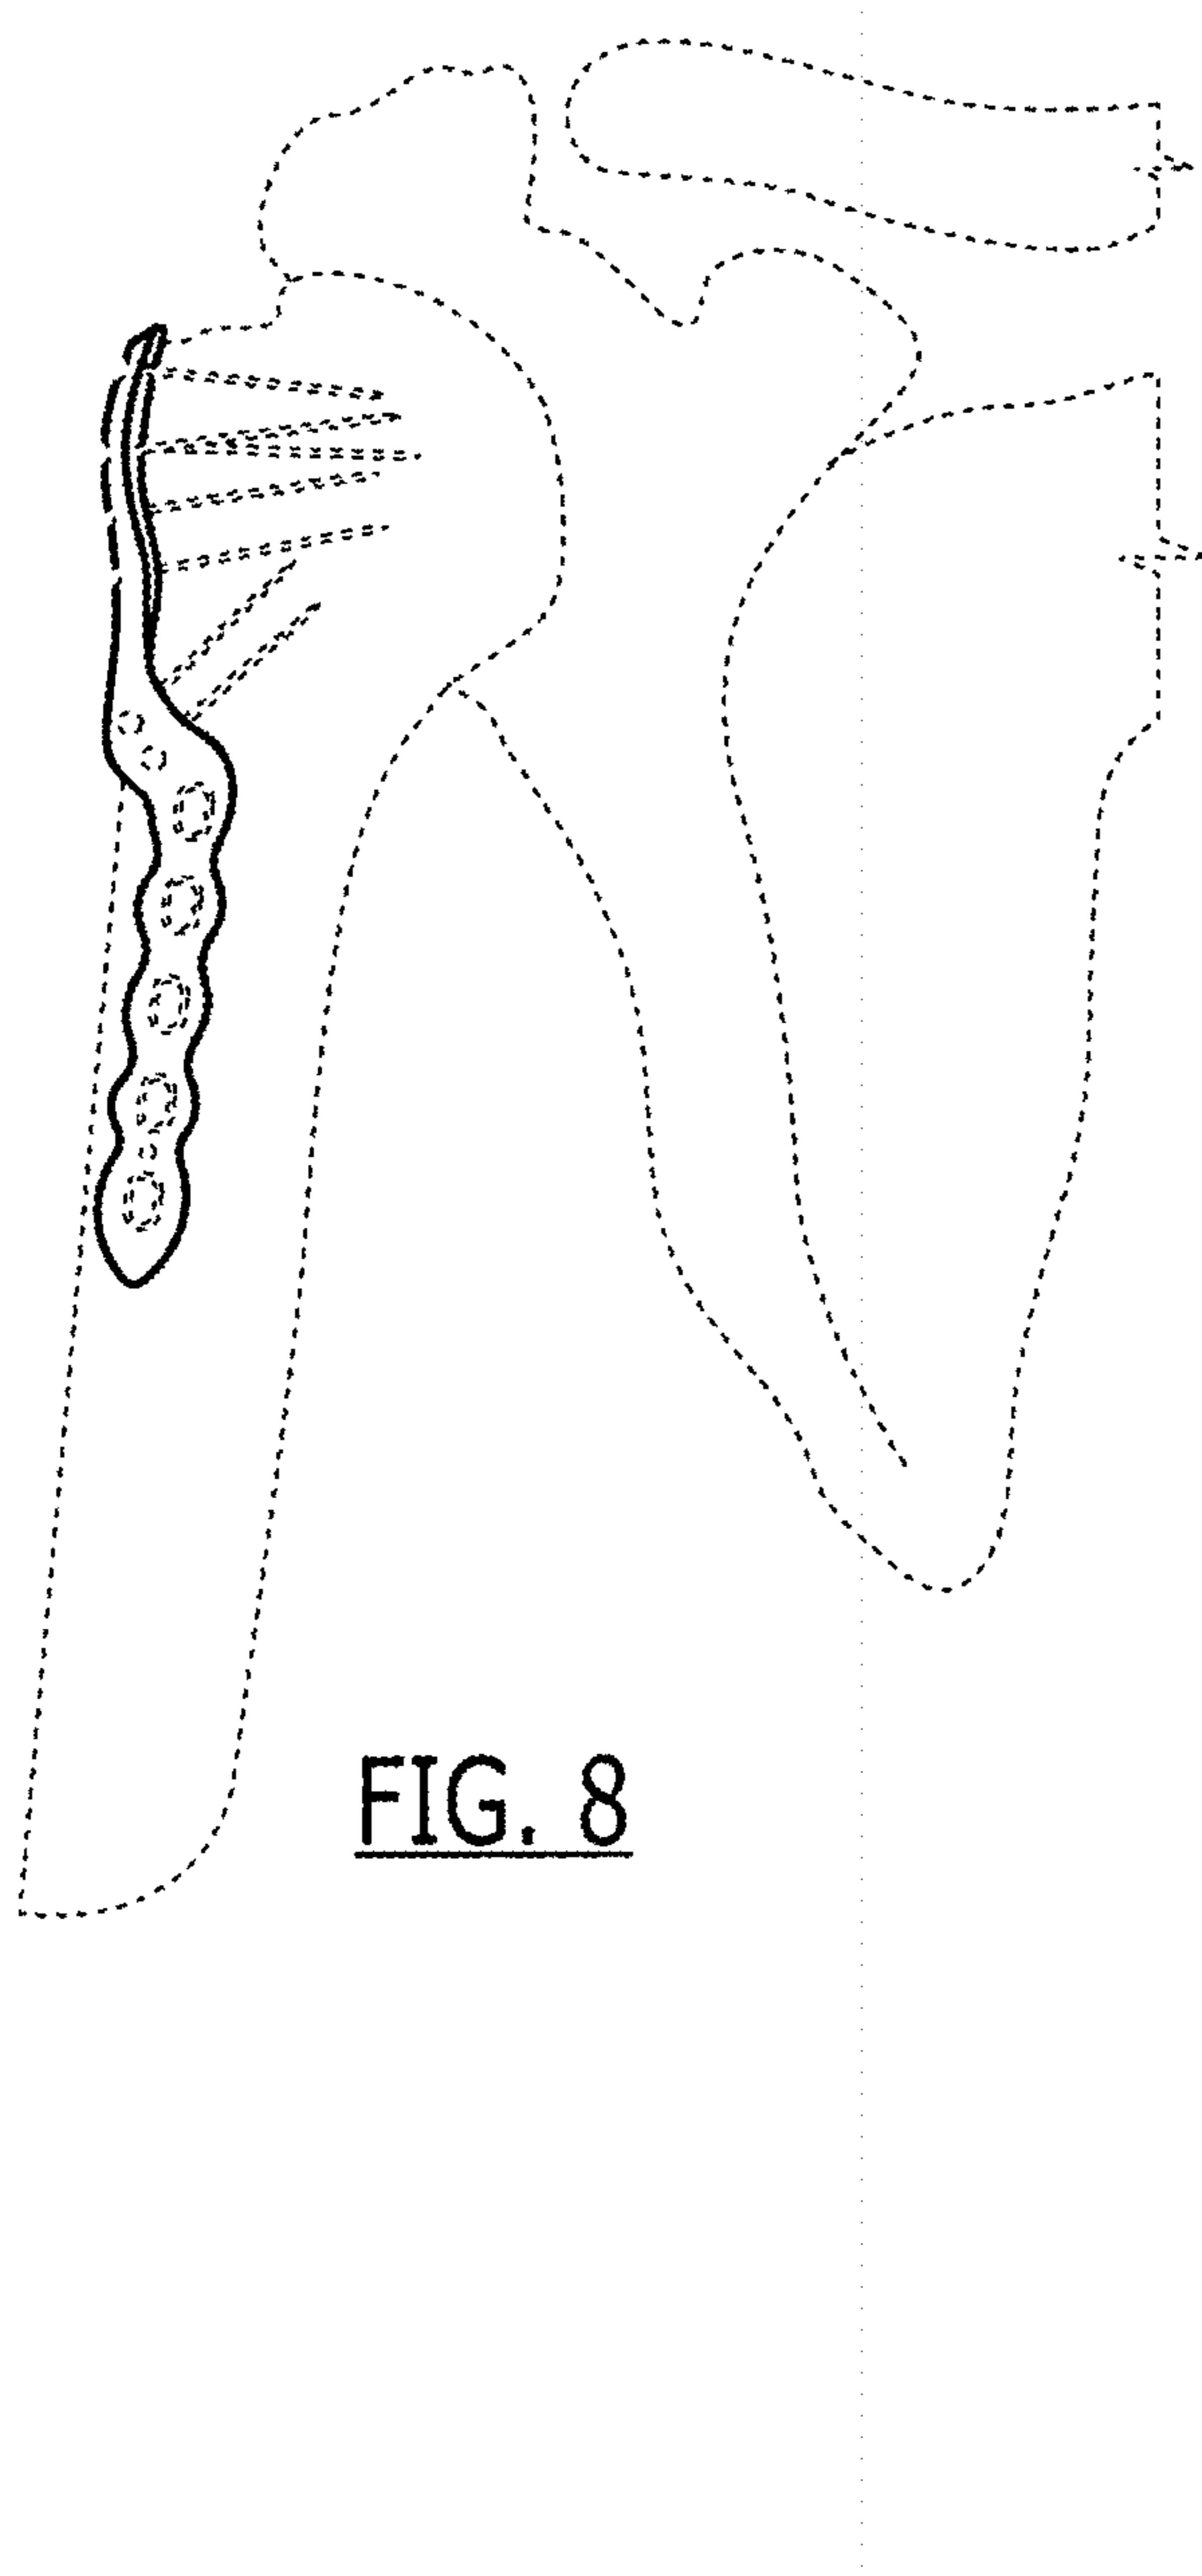


FIG. 8

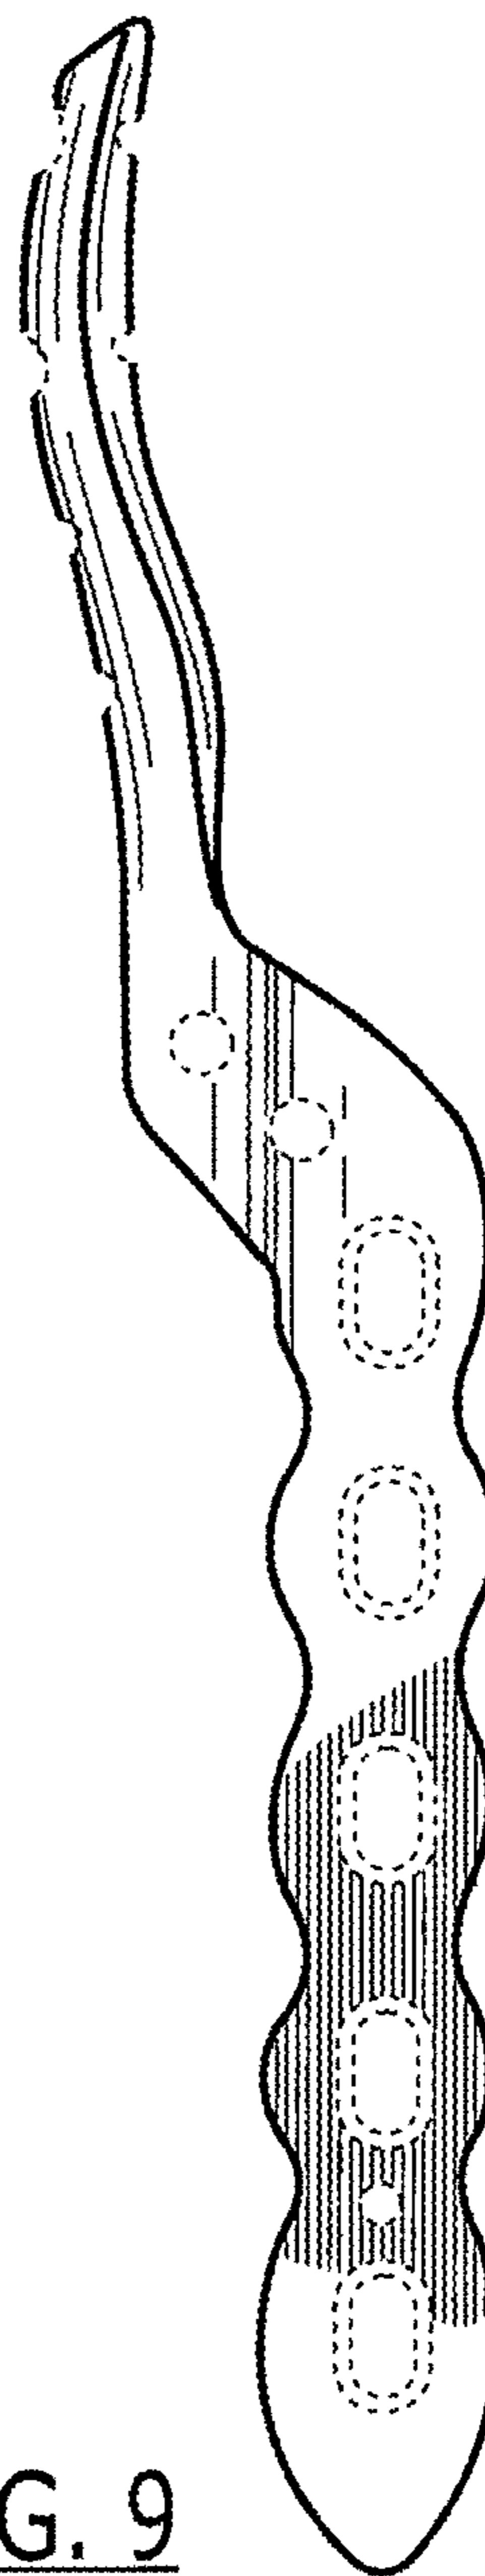


FIG. 9

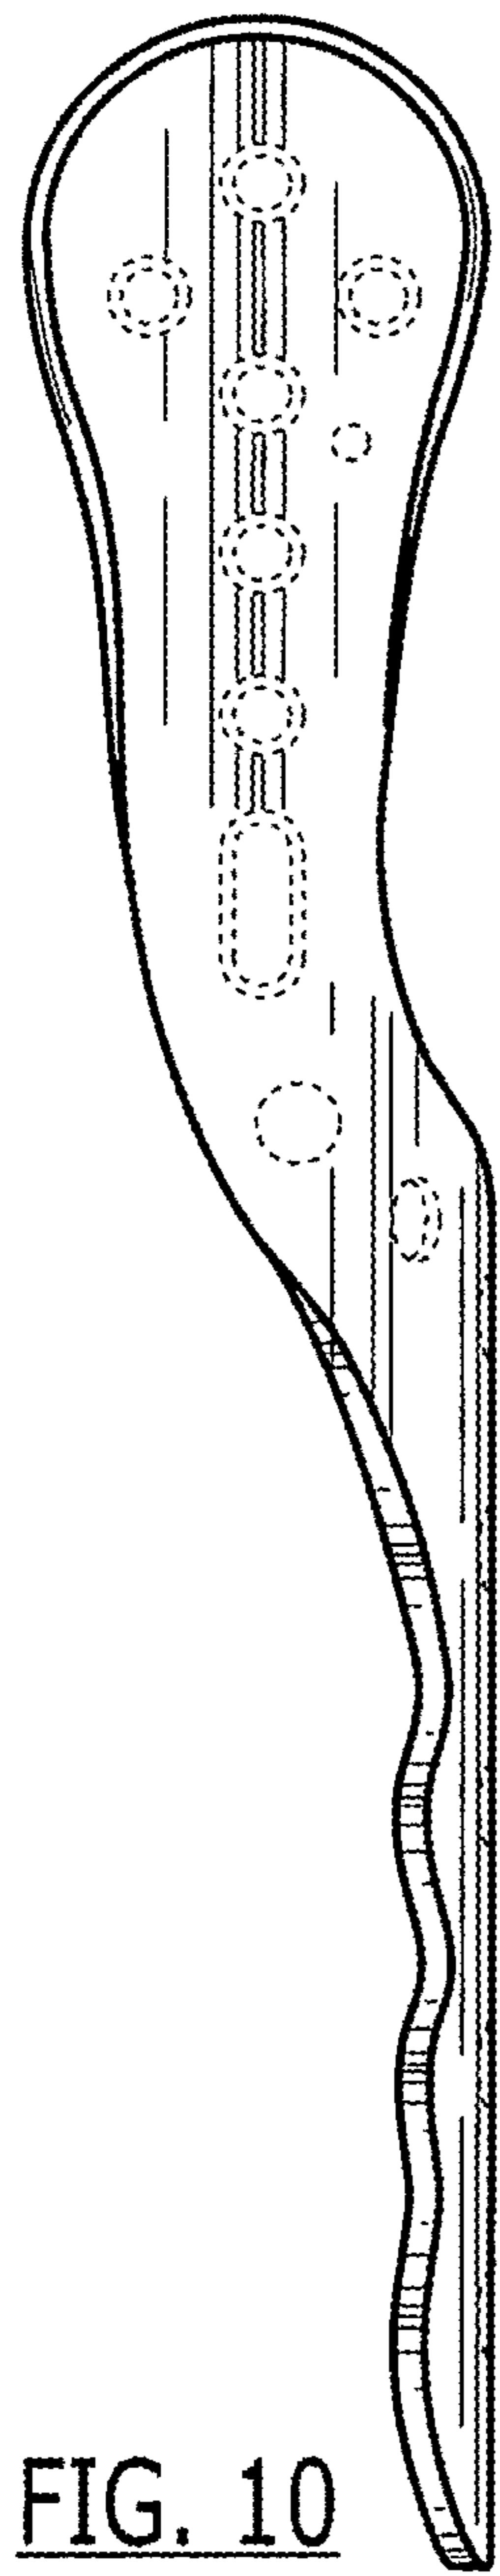


FIG. 10

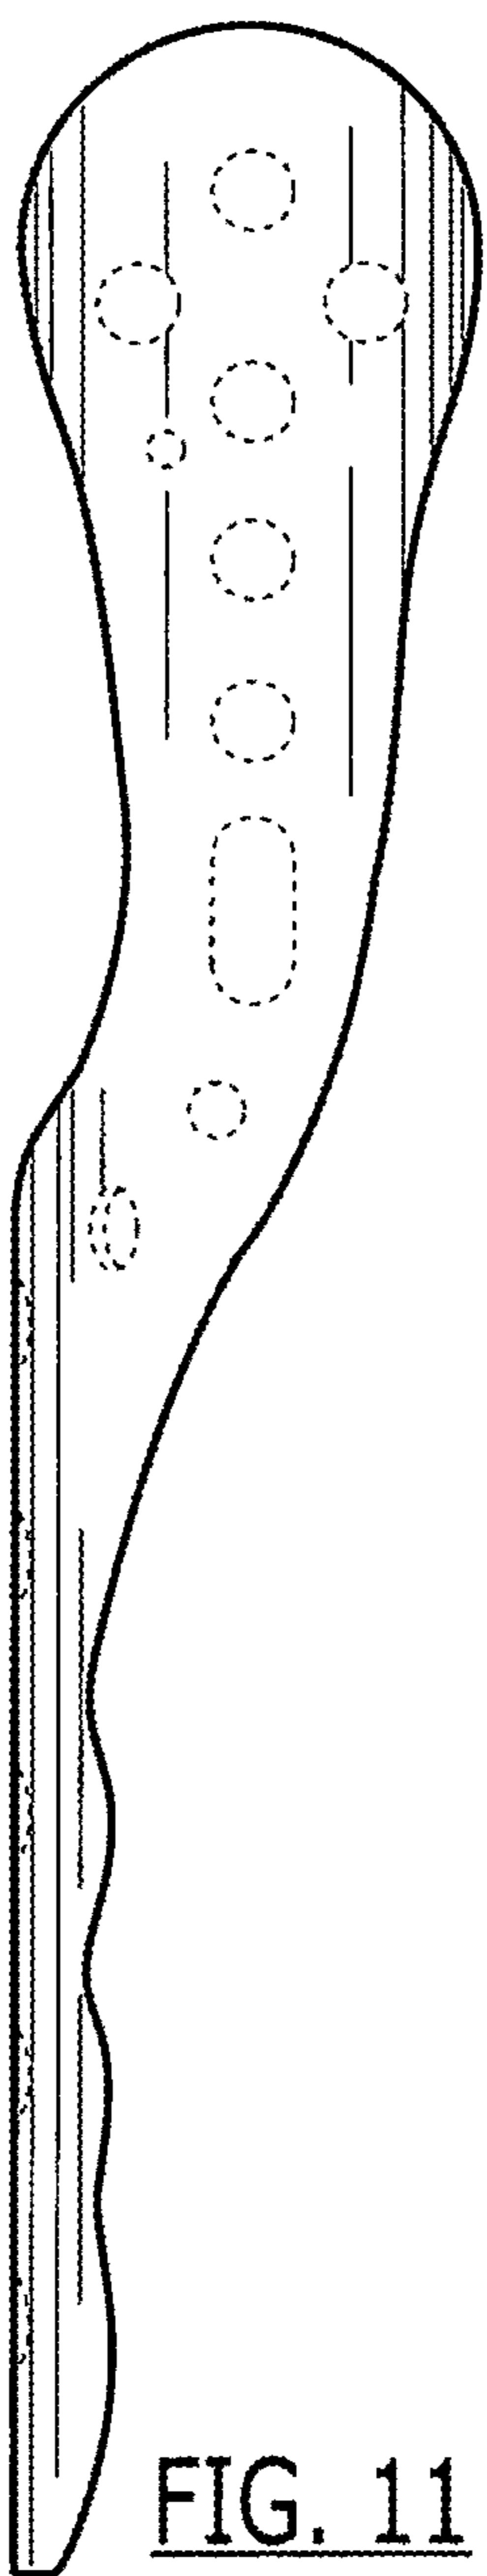


FIG. 11

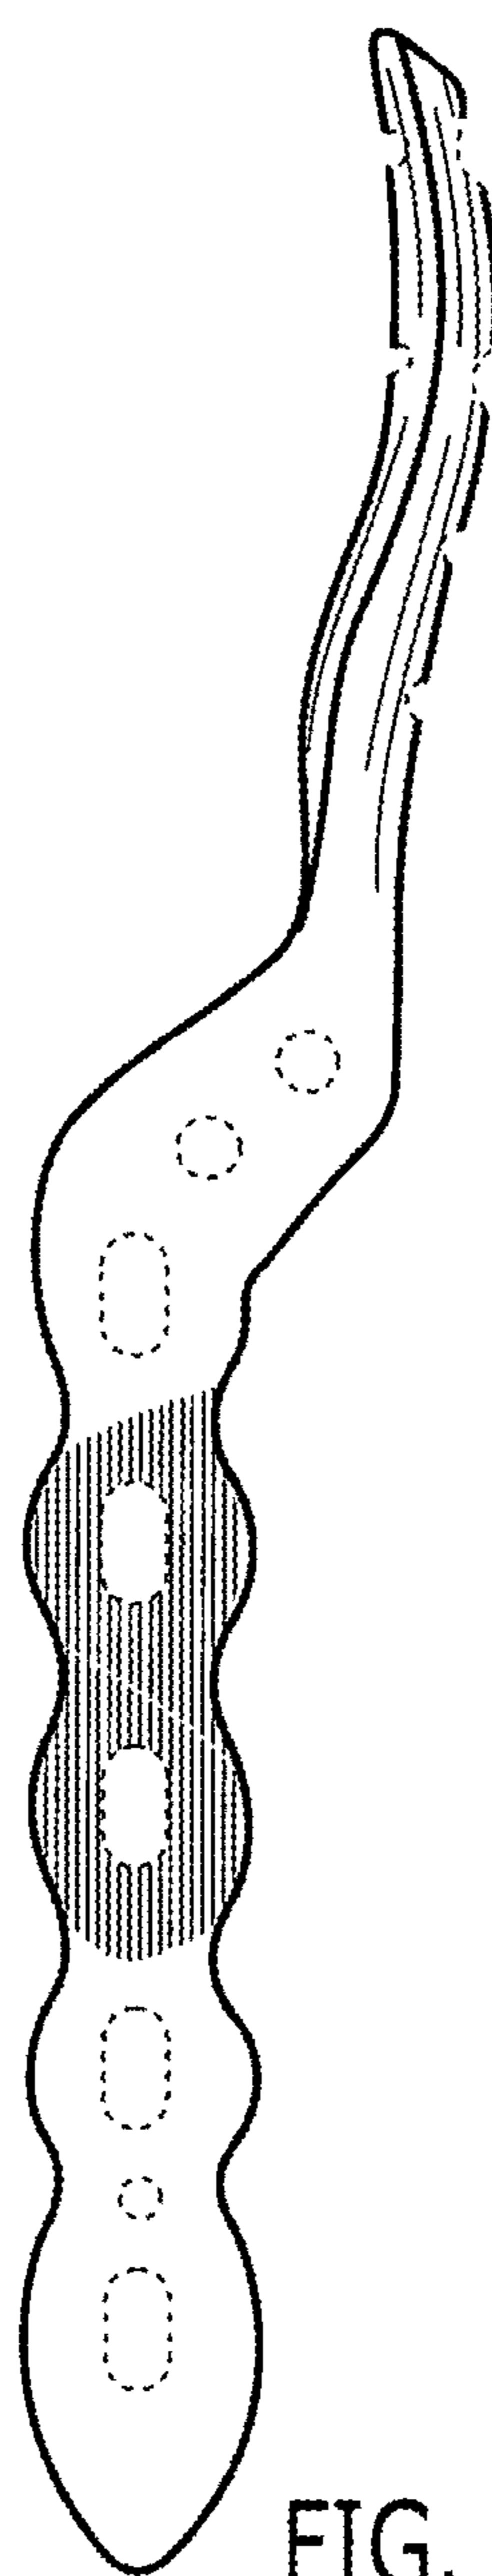


FIG. 12



FIG. 13

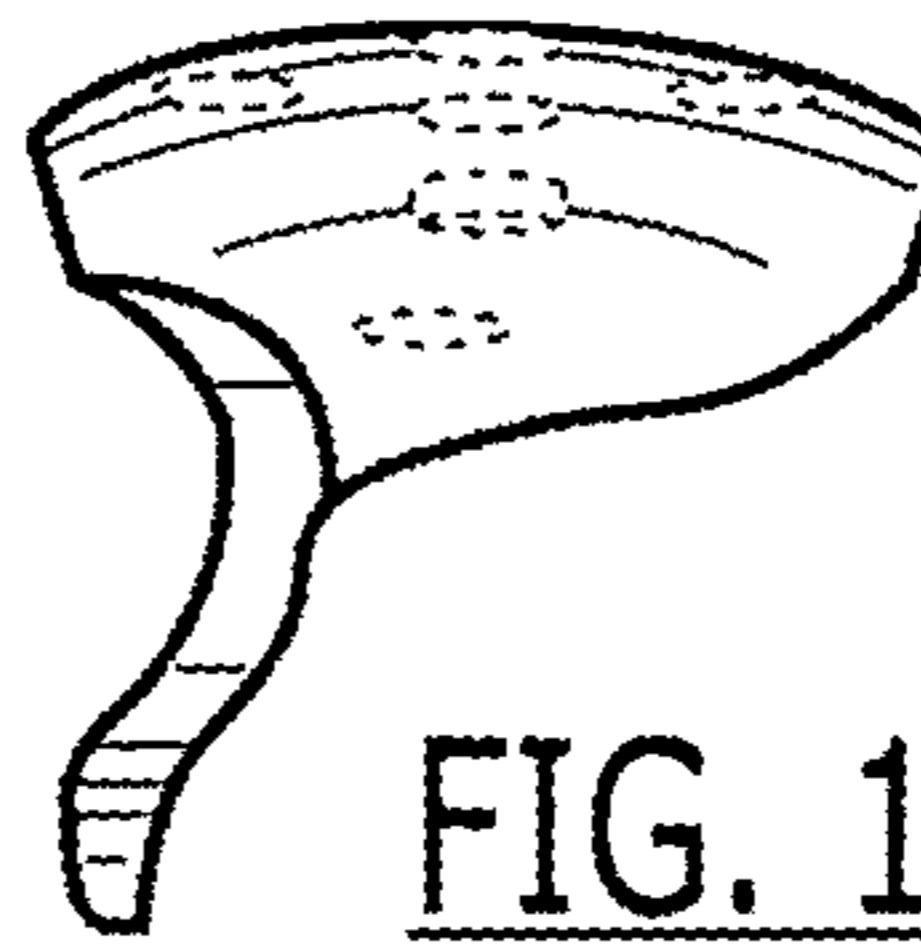


FIG. 14