



US00D872275S

(12) **United States Design Patent**
Frenkler et al.

(10) **Patent No.:** **US D872,275 S**
(45) **Date of Patent:** **** Jan. 7, 2020**

(54) **DISPLAY PANEL OF MEDICAL X-RAY
PHOTOGRAPHING APPARATUS WITH
GRAPHICAL USER INTERFACE**

CPC .. A61B 5/05; A61B 5/055; A61B 6/03; A61B
6/035; A61B 6/4405; A61B 6/4411; A61B
6/4435; A61B 6/4441; A61B 6/4447;
A61B 6/14; G06T 2207/30036
See application file for complete search history.

(71) Applicant: **J. MORITA MFG. CORP.**, Kyoto-shi,
Kyoto (JP)

(56) **References Cited**

(72) Inventors: **Fritz Frenkler**, Munich (DE); **Anette
Ponholzer**, Munich (DE); **Junji
Kawabe**, Munich (DE)

U.S. PATENT DOCUMENTS

(73) Assignee: **J. MORITA MFG. CORP.**, Kyoto (JP)

D661,313 S * 6/2012 Nenoki D14/487
D664,554 S * 7/2012 Nenoki D14/487
D824,935 S * 8/2018 Boutoussov D14/486
2002/0122537 A1* 9/2002 Yoshimura A61B 6/0478
378/208
2011/0064188 A1* 3/2011 Suzuki A61B 6/14
378/21

(**) Term: **15 Years**

(Continued)

(21) Appl. No.: **29/656,715**

Primary Examiner — Anhdao Doan

(22) Filed: **Jul. 16, 2018**

(74) *Attorney, Agent, or Firm* — Oliff PLC

Related U.S. Application Data

(57) **CLAIM**

(62) Division of application No. 29/600,722, filed on Apr.
14, 2017, now Pat. No. Des. 839,427.

The ornamental design for a display panel of medical X-ray
photographing apparatus with graphical user interface, as
shown and described.

DESCRIPTION

(30) **Foreign Application Priority Data**

Oct. 14, 2016 (JP) 2016-022437
Oct. 14, 2016 (JP) 2016-022438
Oct. 14, 2016 (JP) 2016-022439
Oct. 14, 2016 (JP) 2016-022440
Oct. 14, 2016 (JP) 2016-022441
Oct. 14, 2016 (JP) 2016-022442
Oct. 14, 2016 (JP) 2016-022443
Oct. 14, 2016 (JP) 2016-022444


FIG. 1 is a front view of a display panel of medical X-ray
photographing apparatus with graphical user interface of the
present design;
FIG. 2 is a rear view thereof;
FIG. 3 is a left side view thereof;
FIG. 4 is a right side view thereof;
FIG. 5 is a top view thereof;
FIG. 6 is a bottom view thereof; and,
FIG. 7 is an enlarged view of 7-7 portion of FIG. 3 thereof.
The broken lines shown in the drawings represent portions
of display panel of medical X-ray photographing apparatus
with graphical user interface that form no part of the claimed
design. The long dashed and short dashed lines indicate only
boundaries of the claimed subject matter and form no part of
the claimed design.

(51) **LOC (12) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/158**; D14/485

1 Claim, 6 Drawing Sheets

(58) **Field of Classification Search**
USPC D24/158-161, 185, 186, 107, 152, 176,
D24/177; D14/485, 486, 487

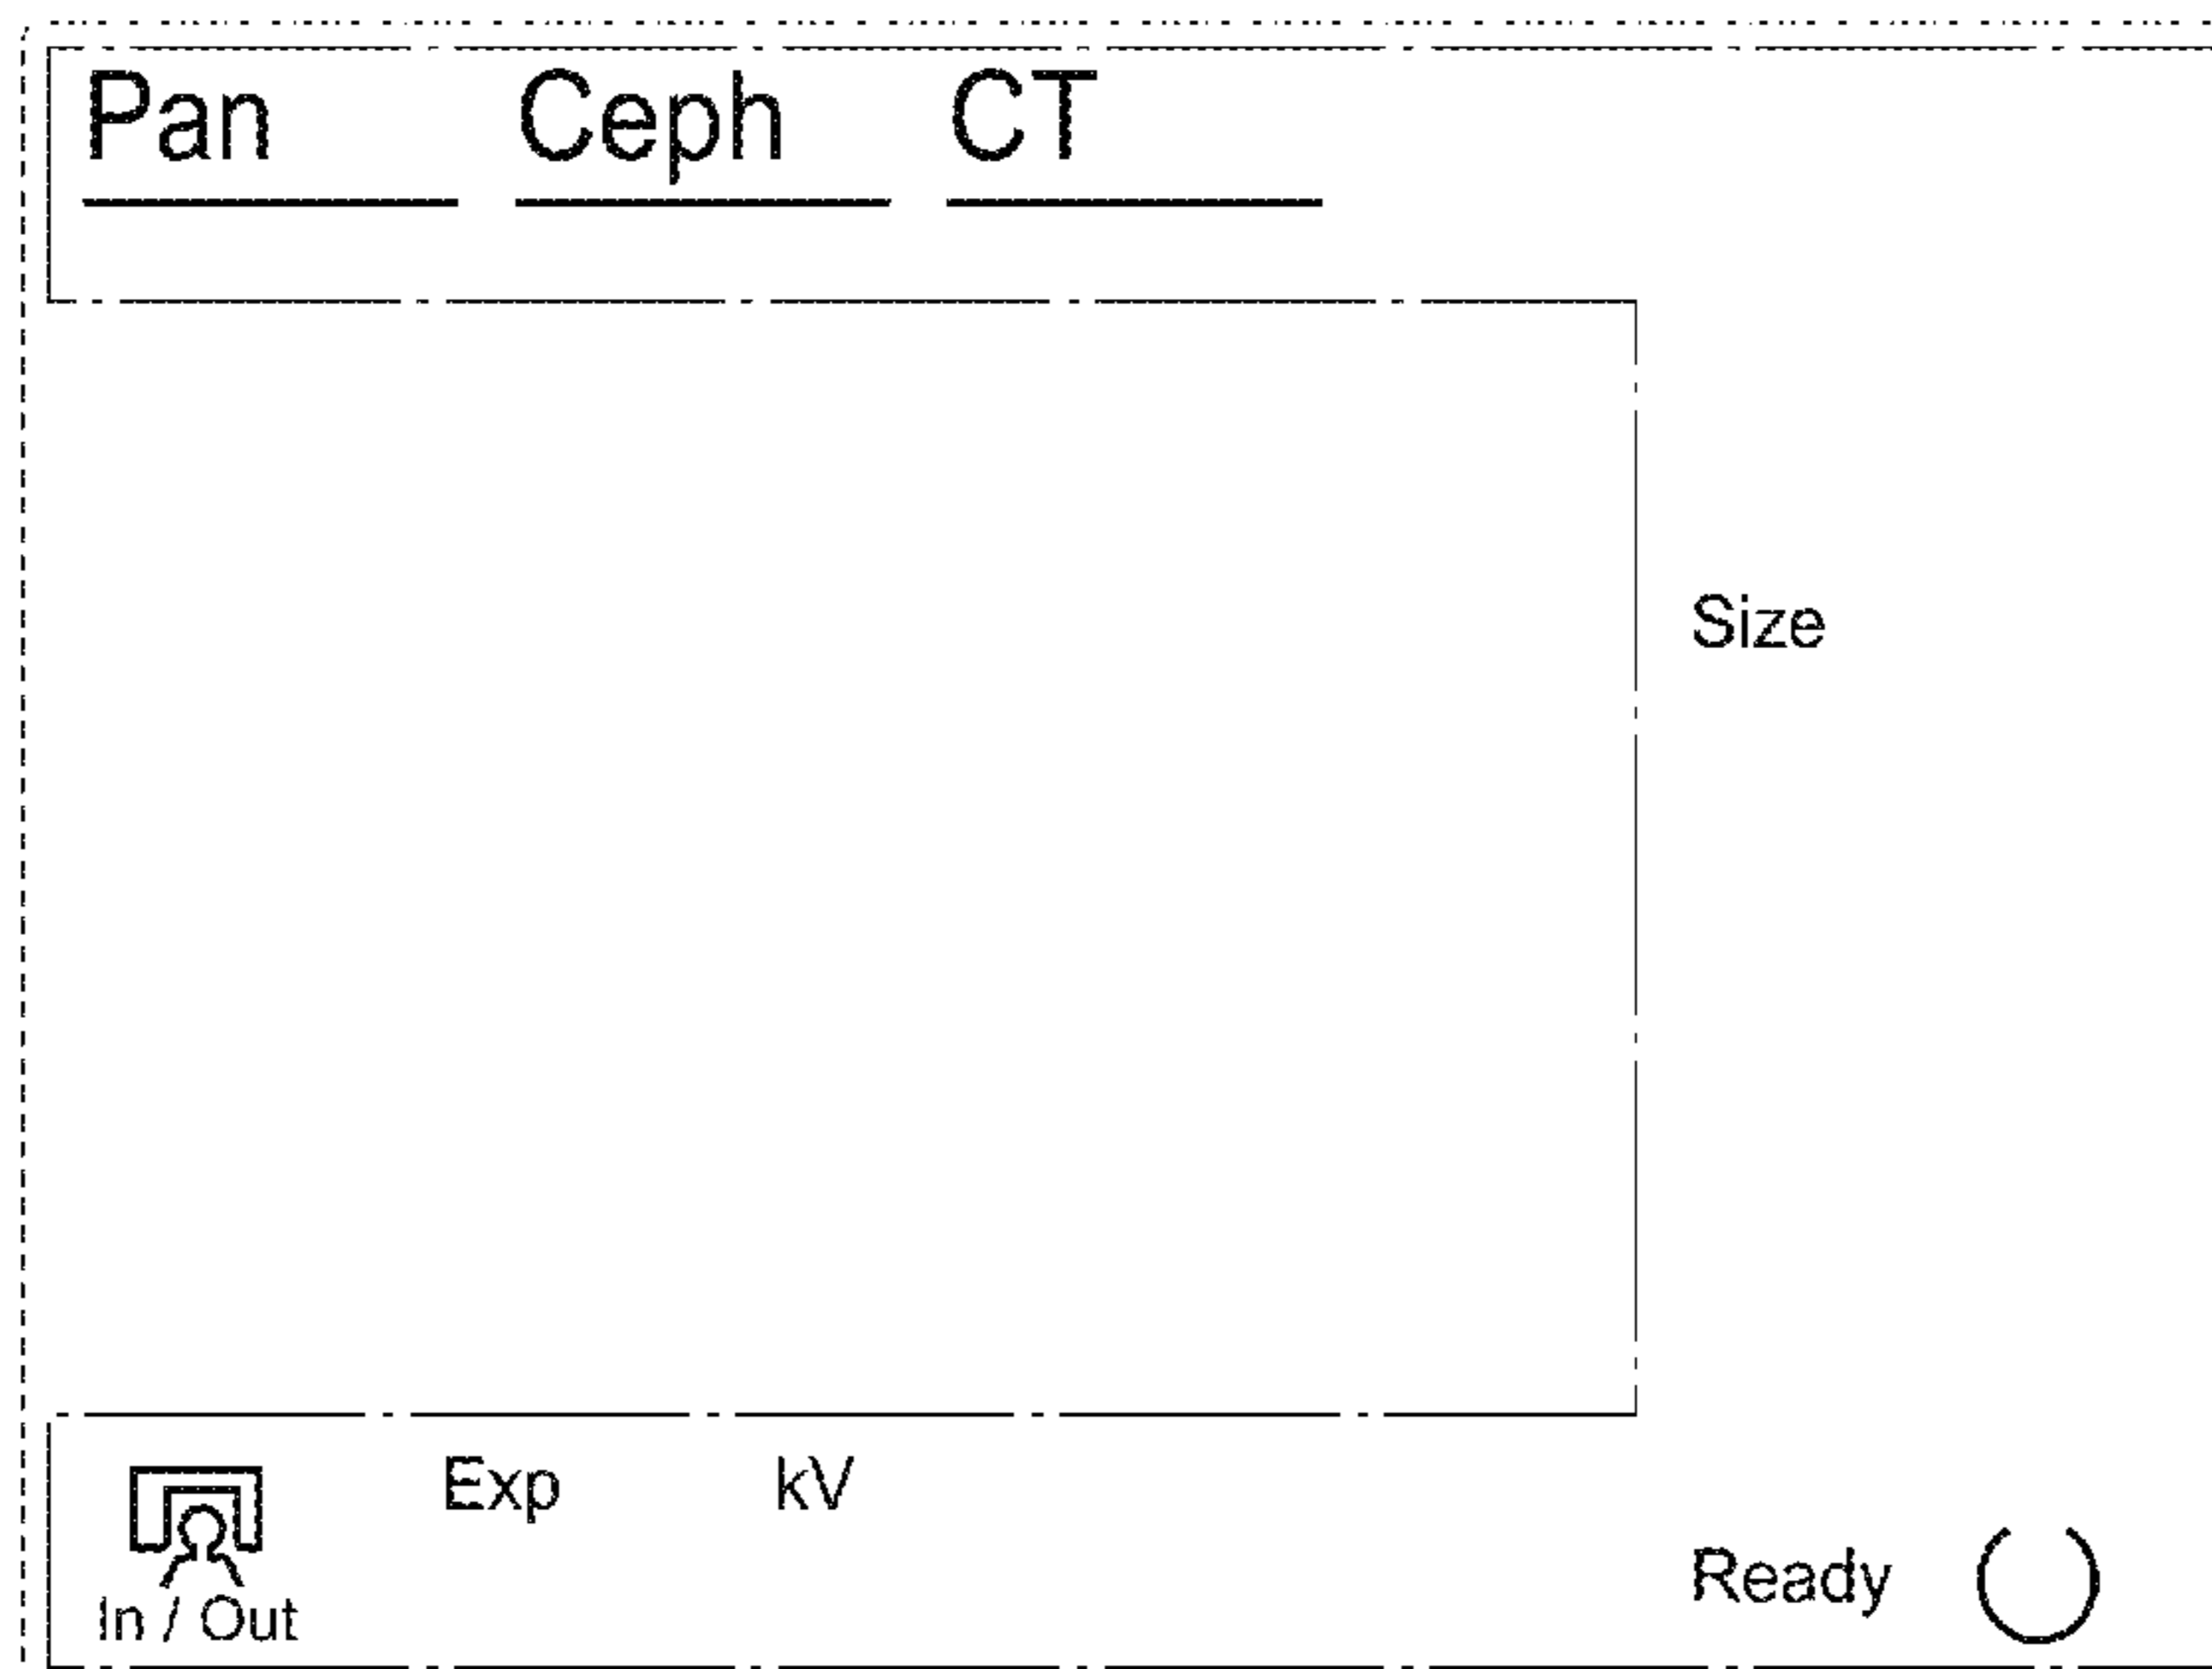

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0108011 A1* 5/2013 Sadakane A61B 6/03
378/19
2015/0351638 A1* 12/2015 Amato A61B 6/14
433/245
2015/0359501 A1* 12/2015 Eronen A61B 6/032
378/62
2018/0103920 A1* 4/2018 Ito A61B 6/032
2018/0325475 A1* 11/2018 Choi A61B 6/463

* cited by examiner

FIG. 1

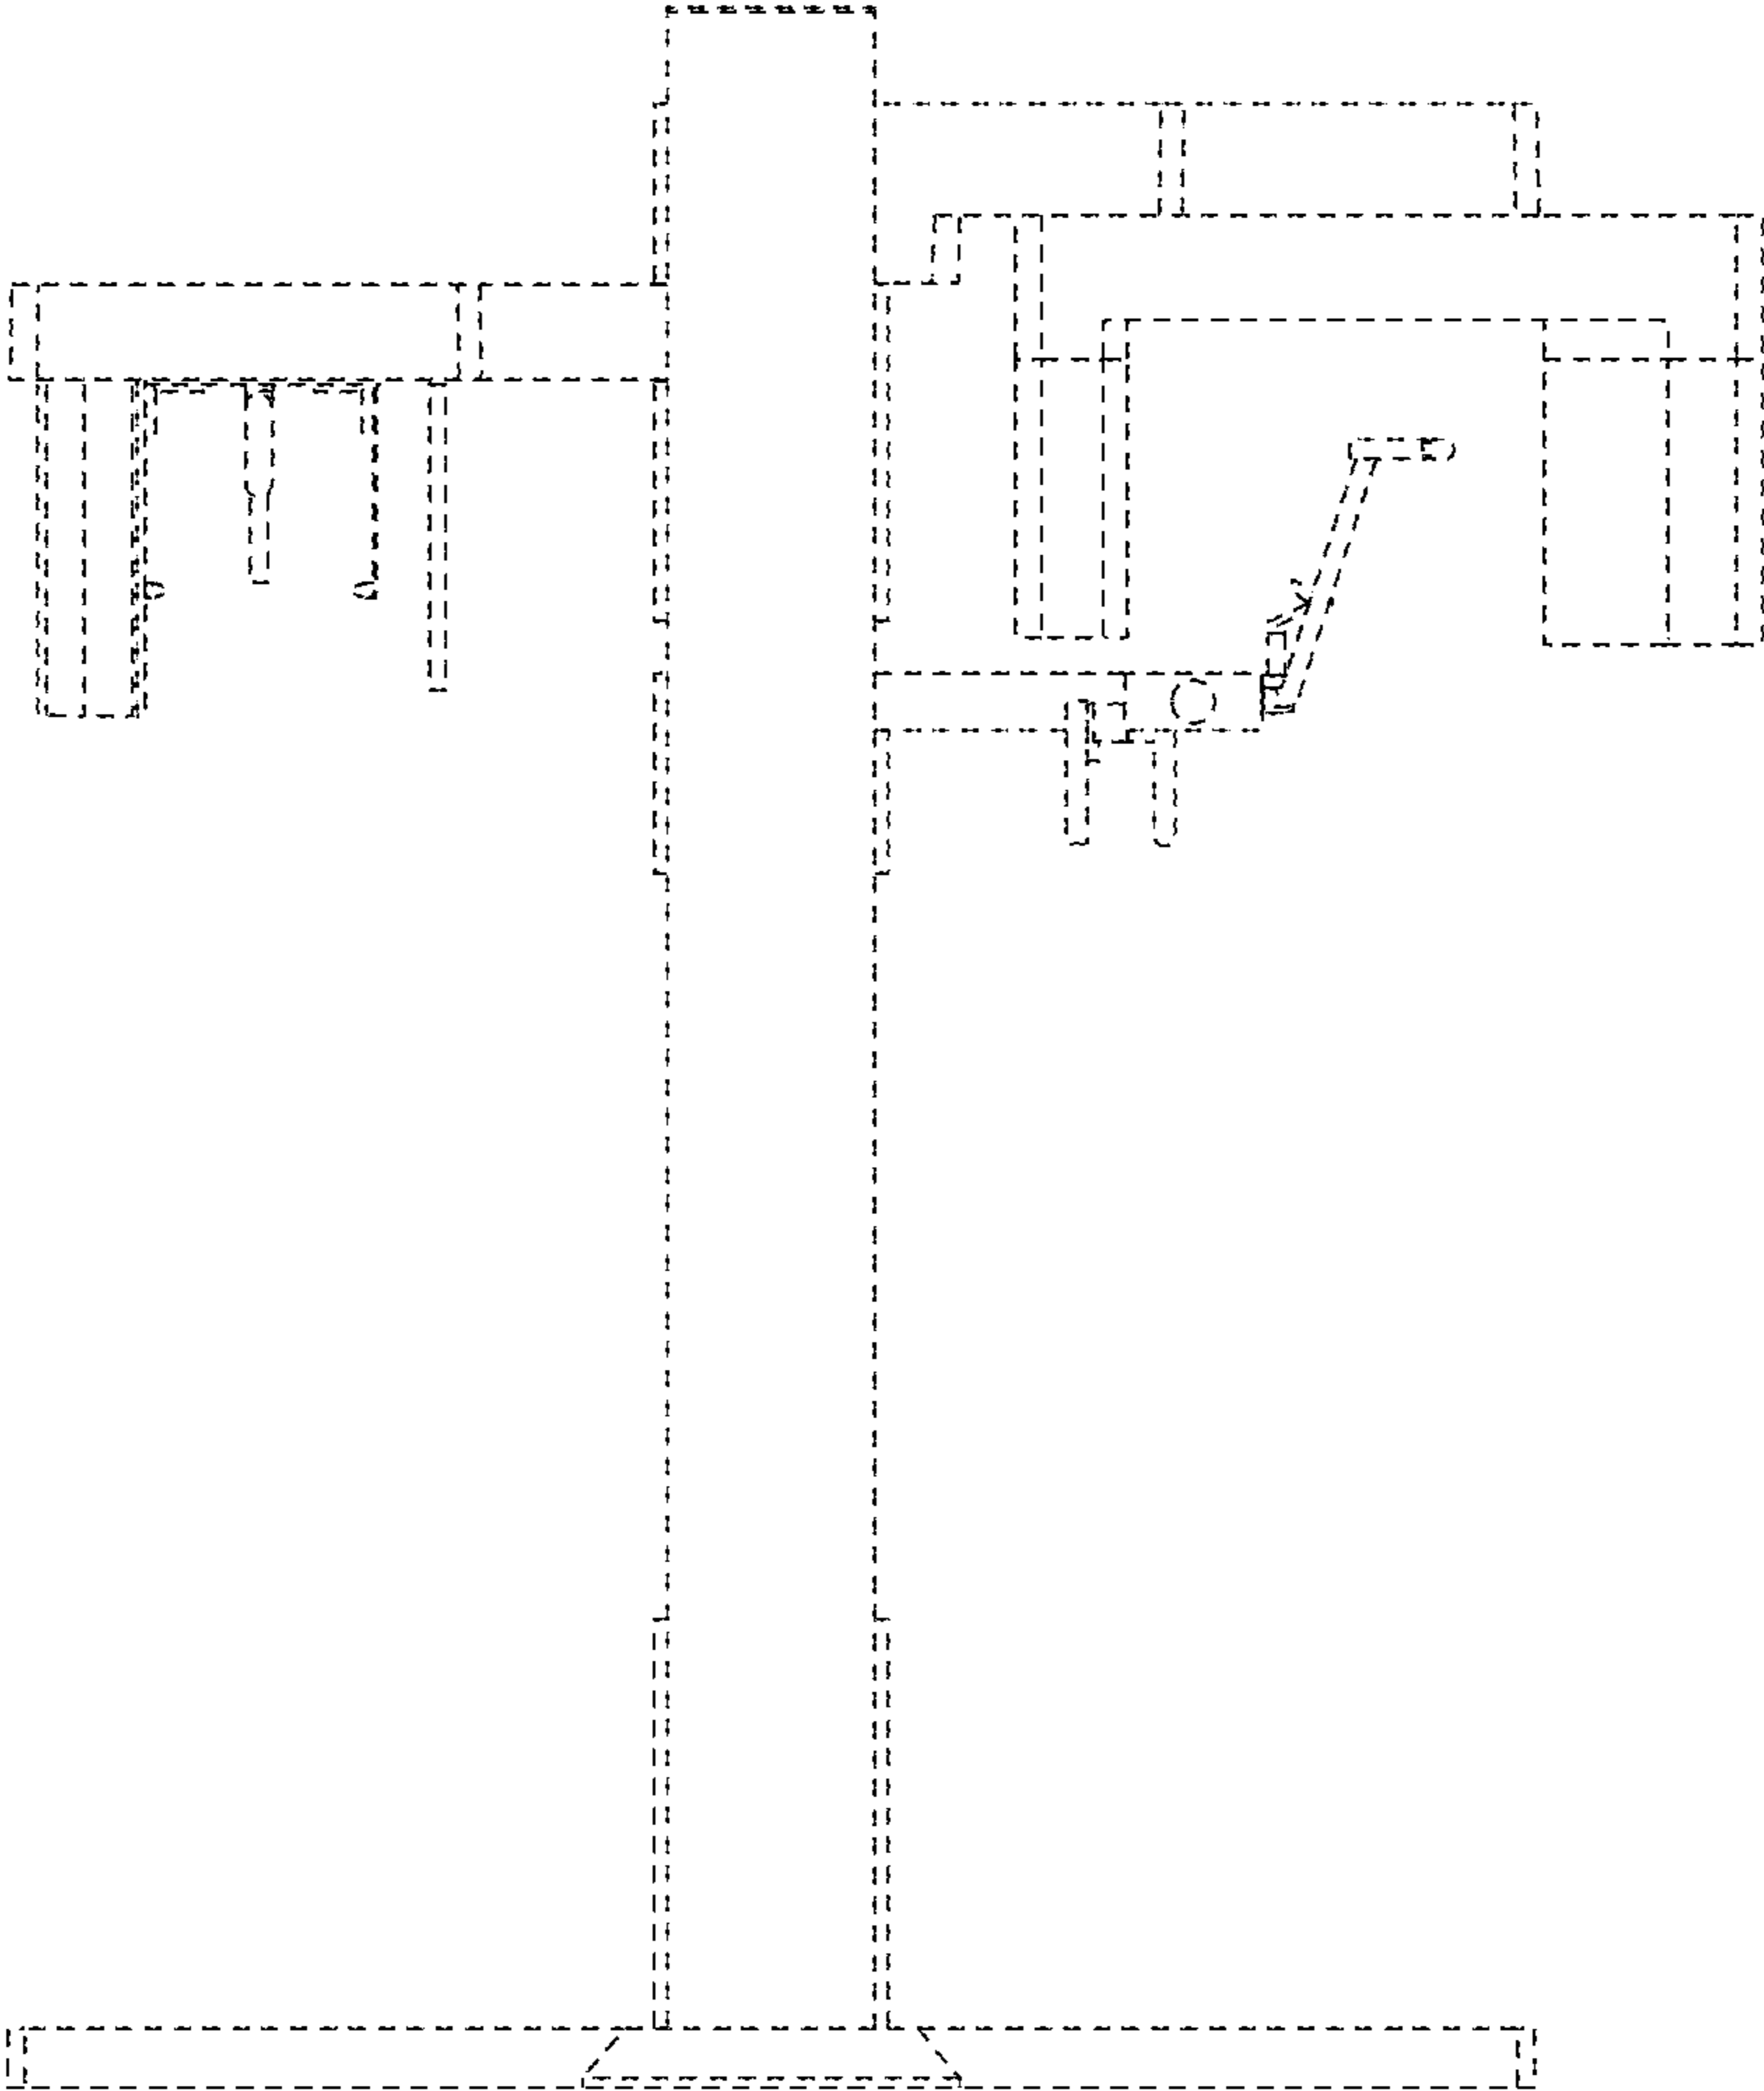


FIG. 2

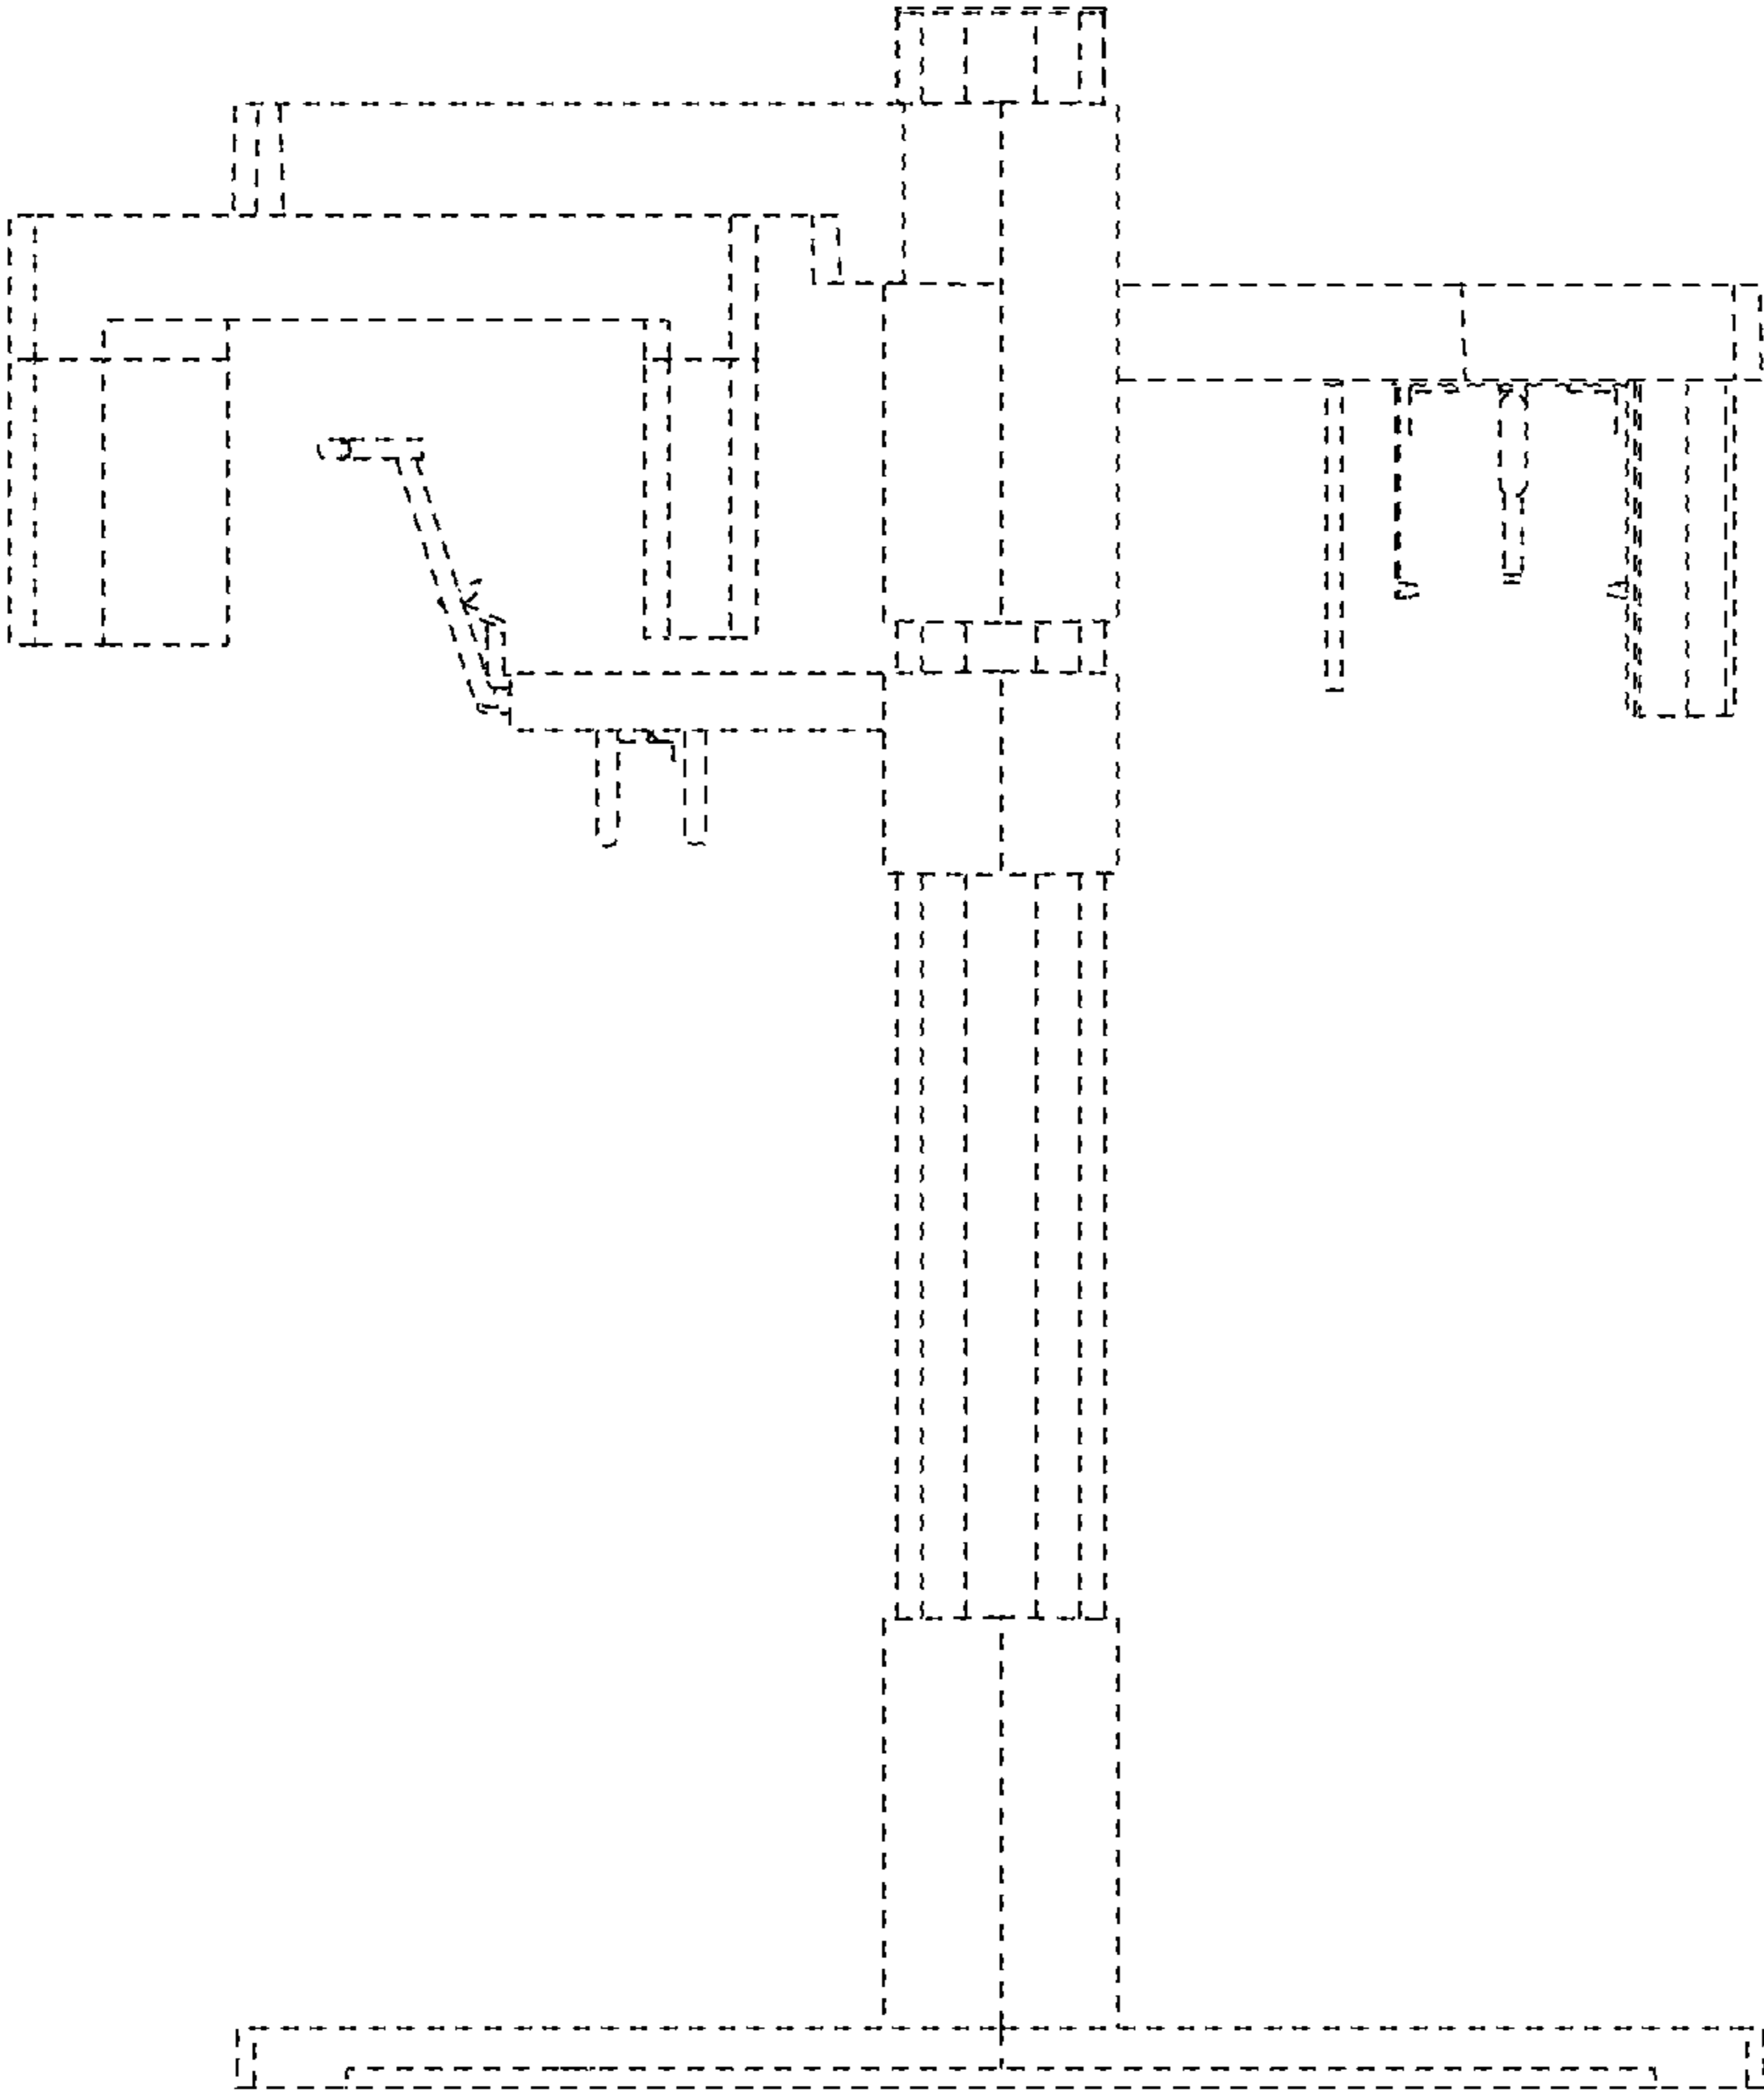


FIG. 3

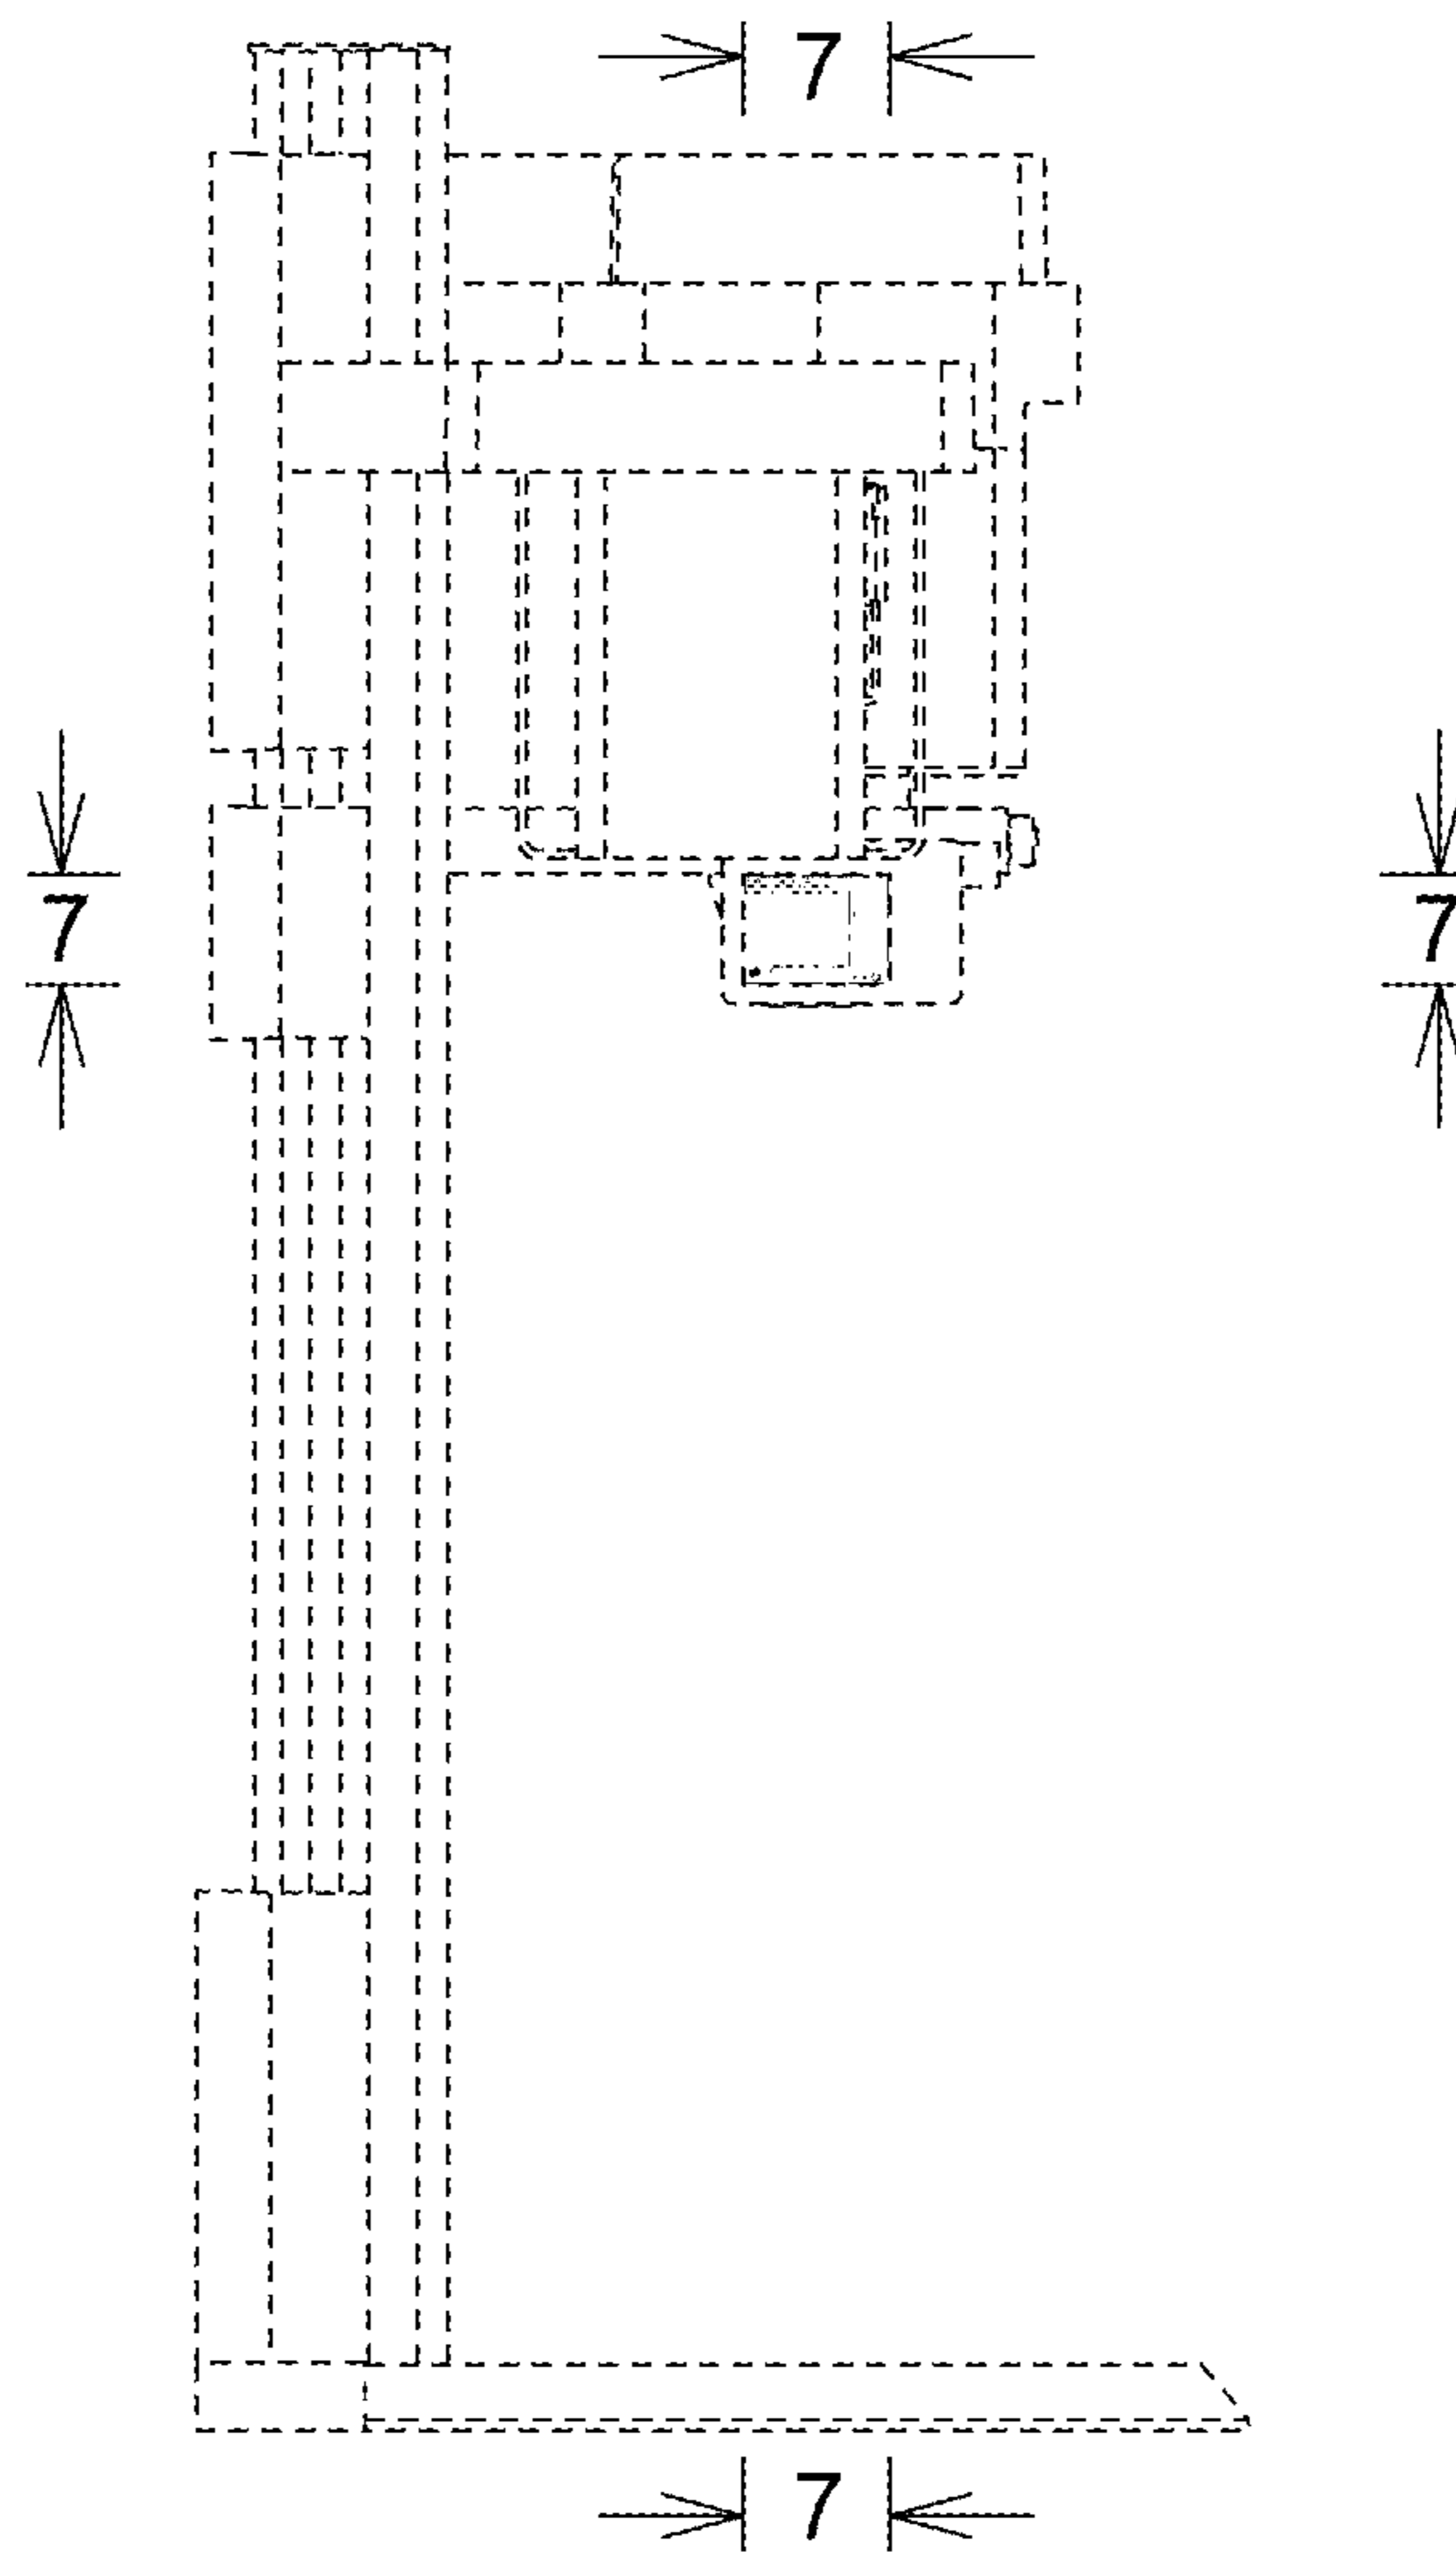


FIG. 4

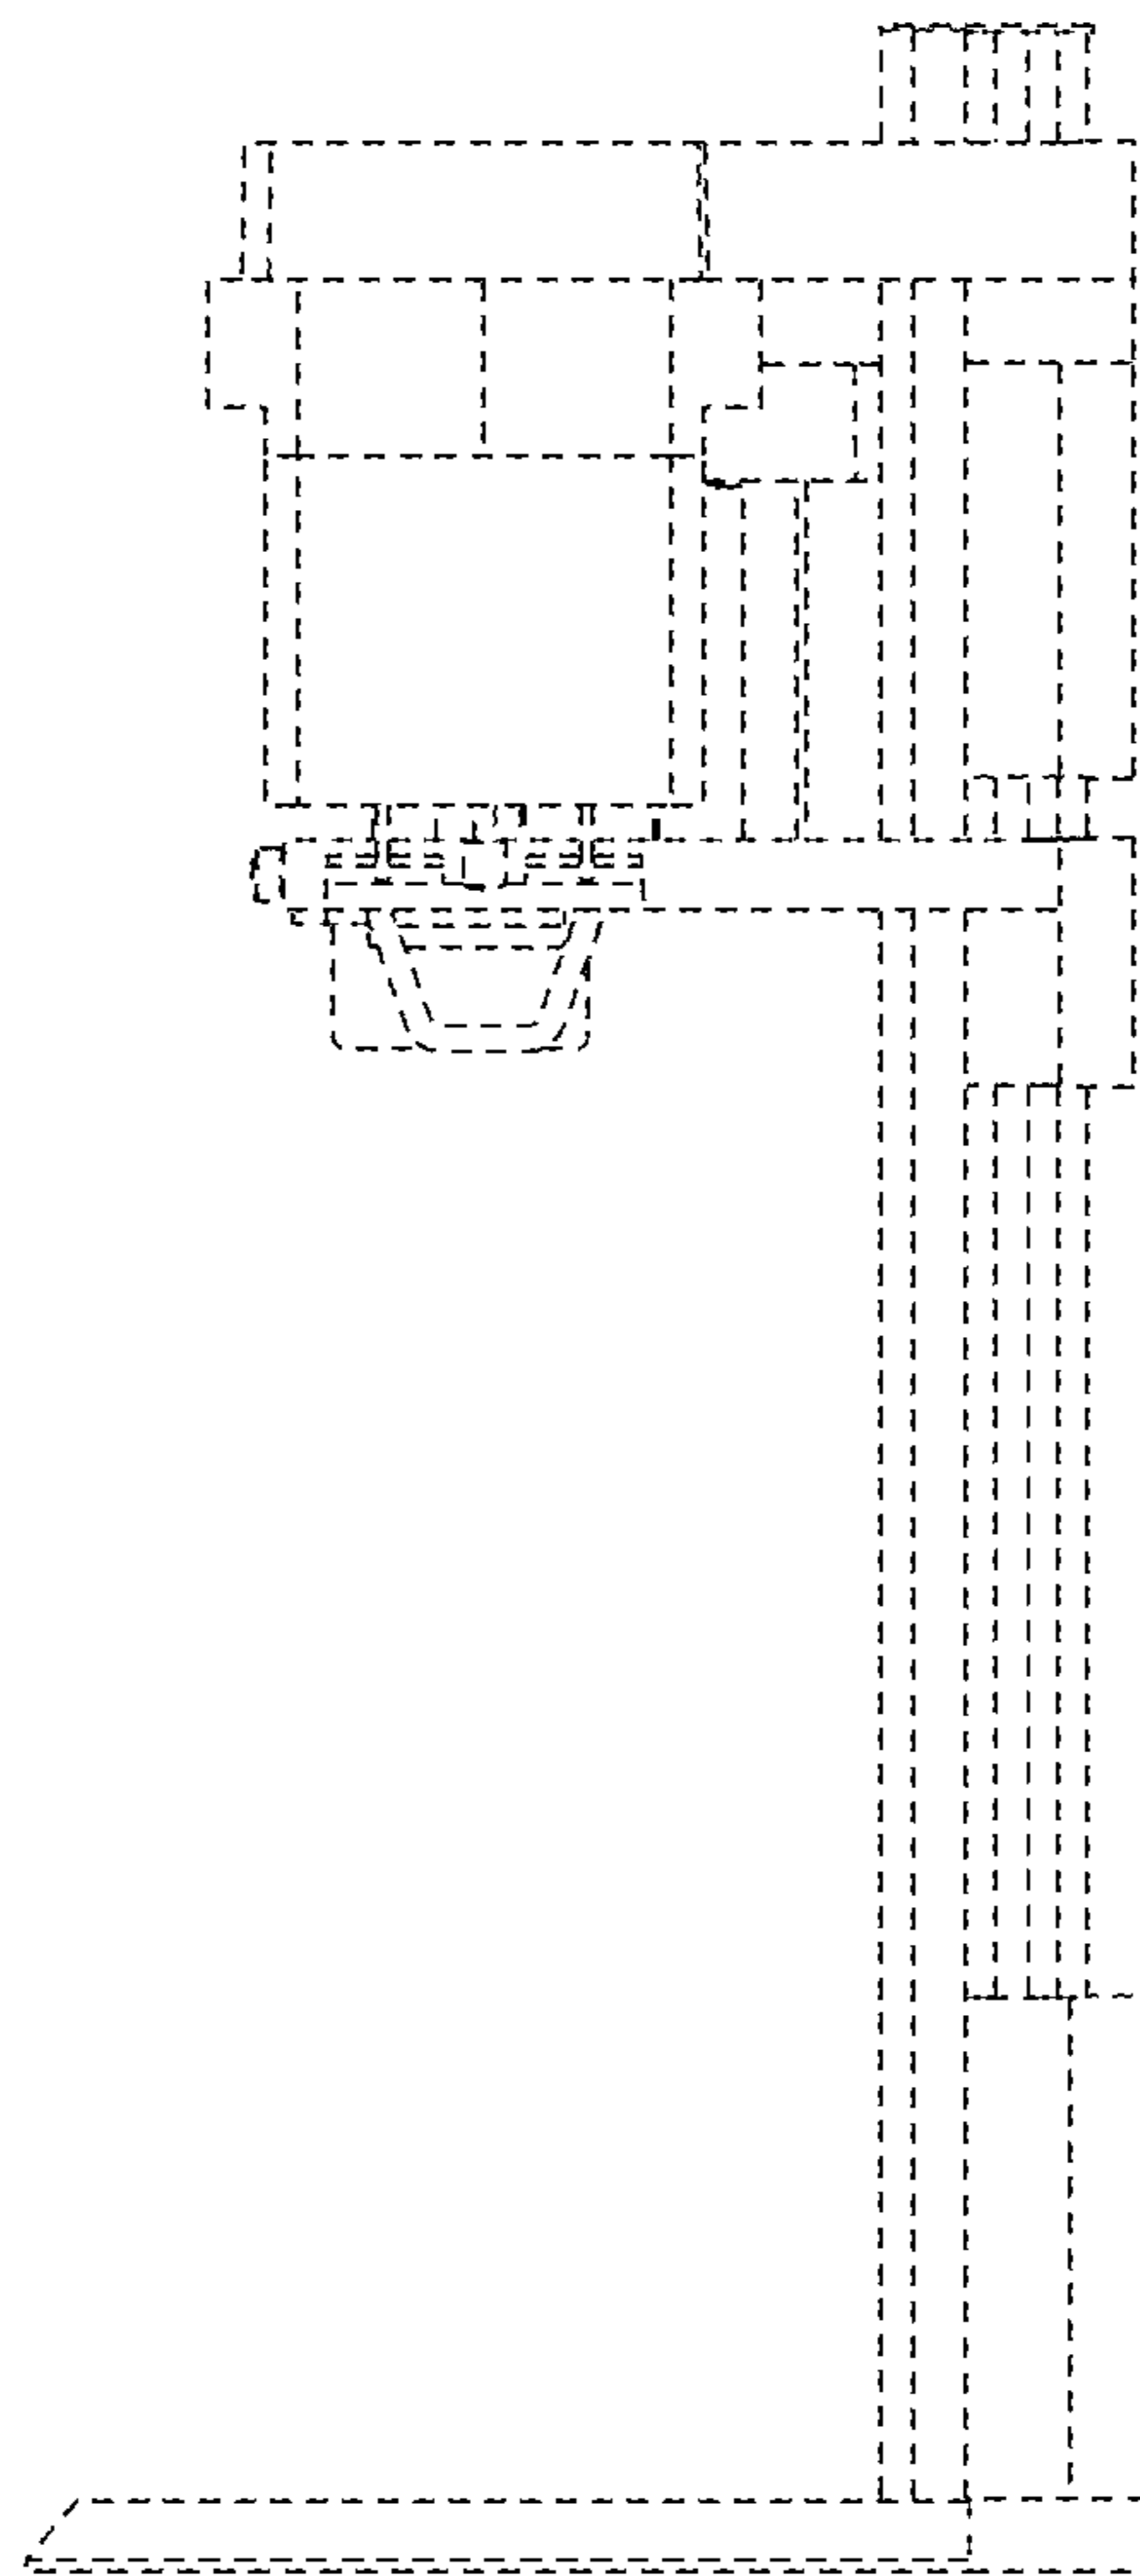


FIG. 5

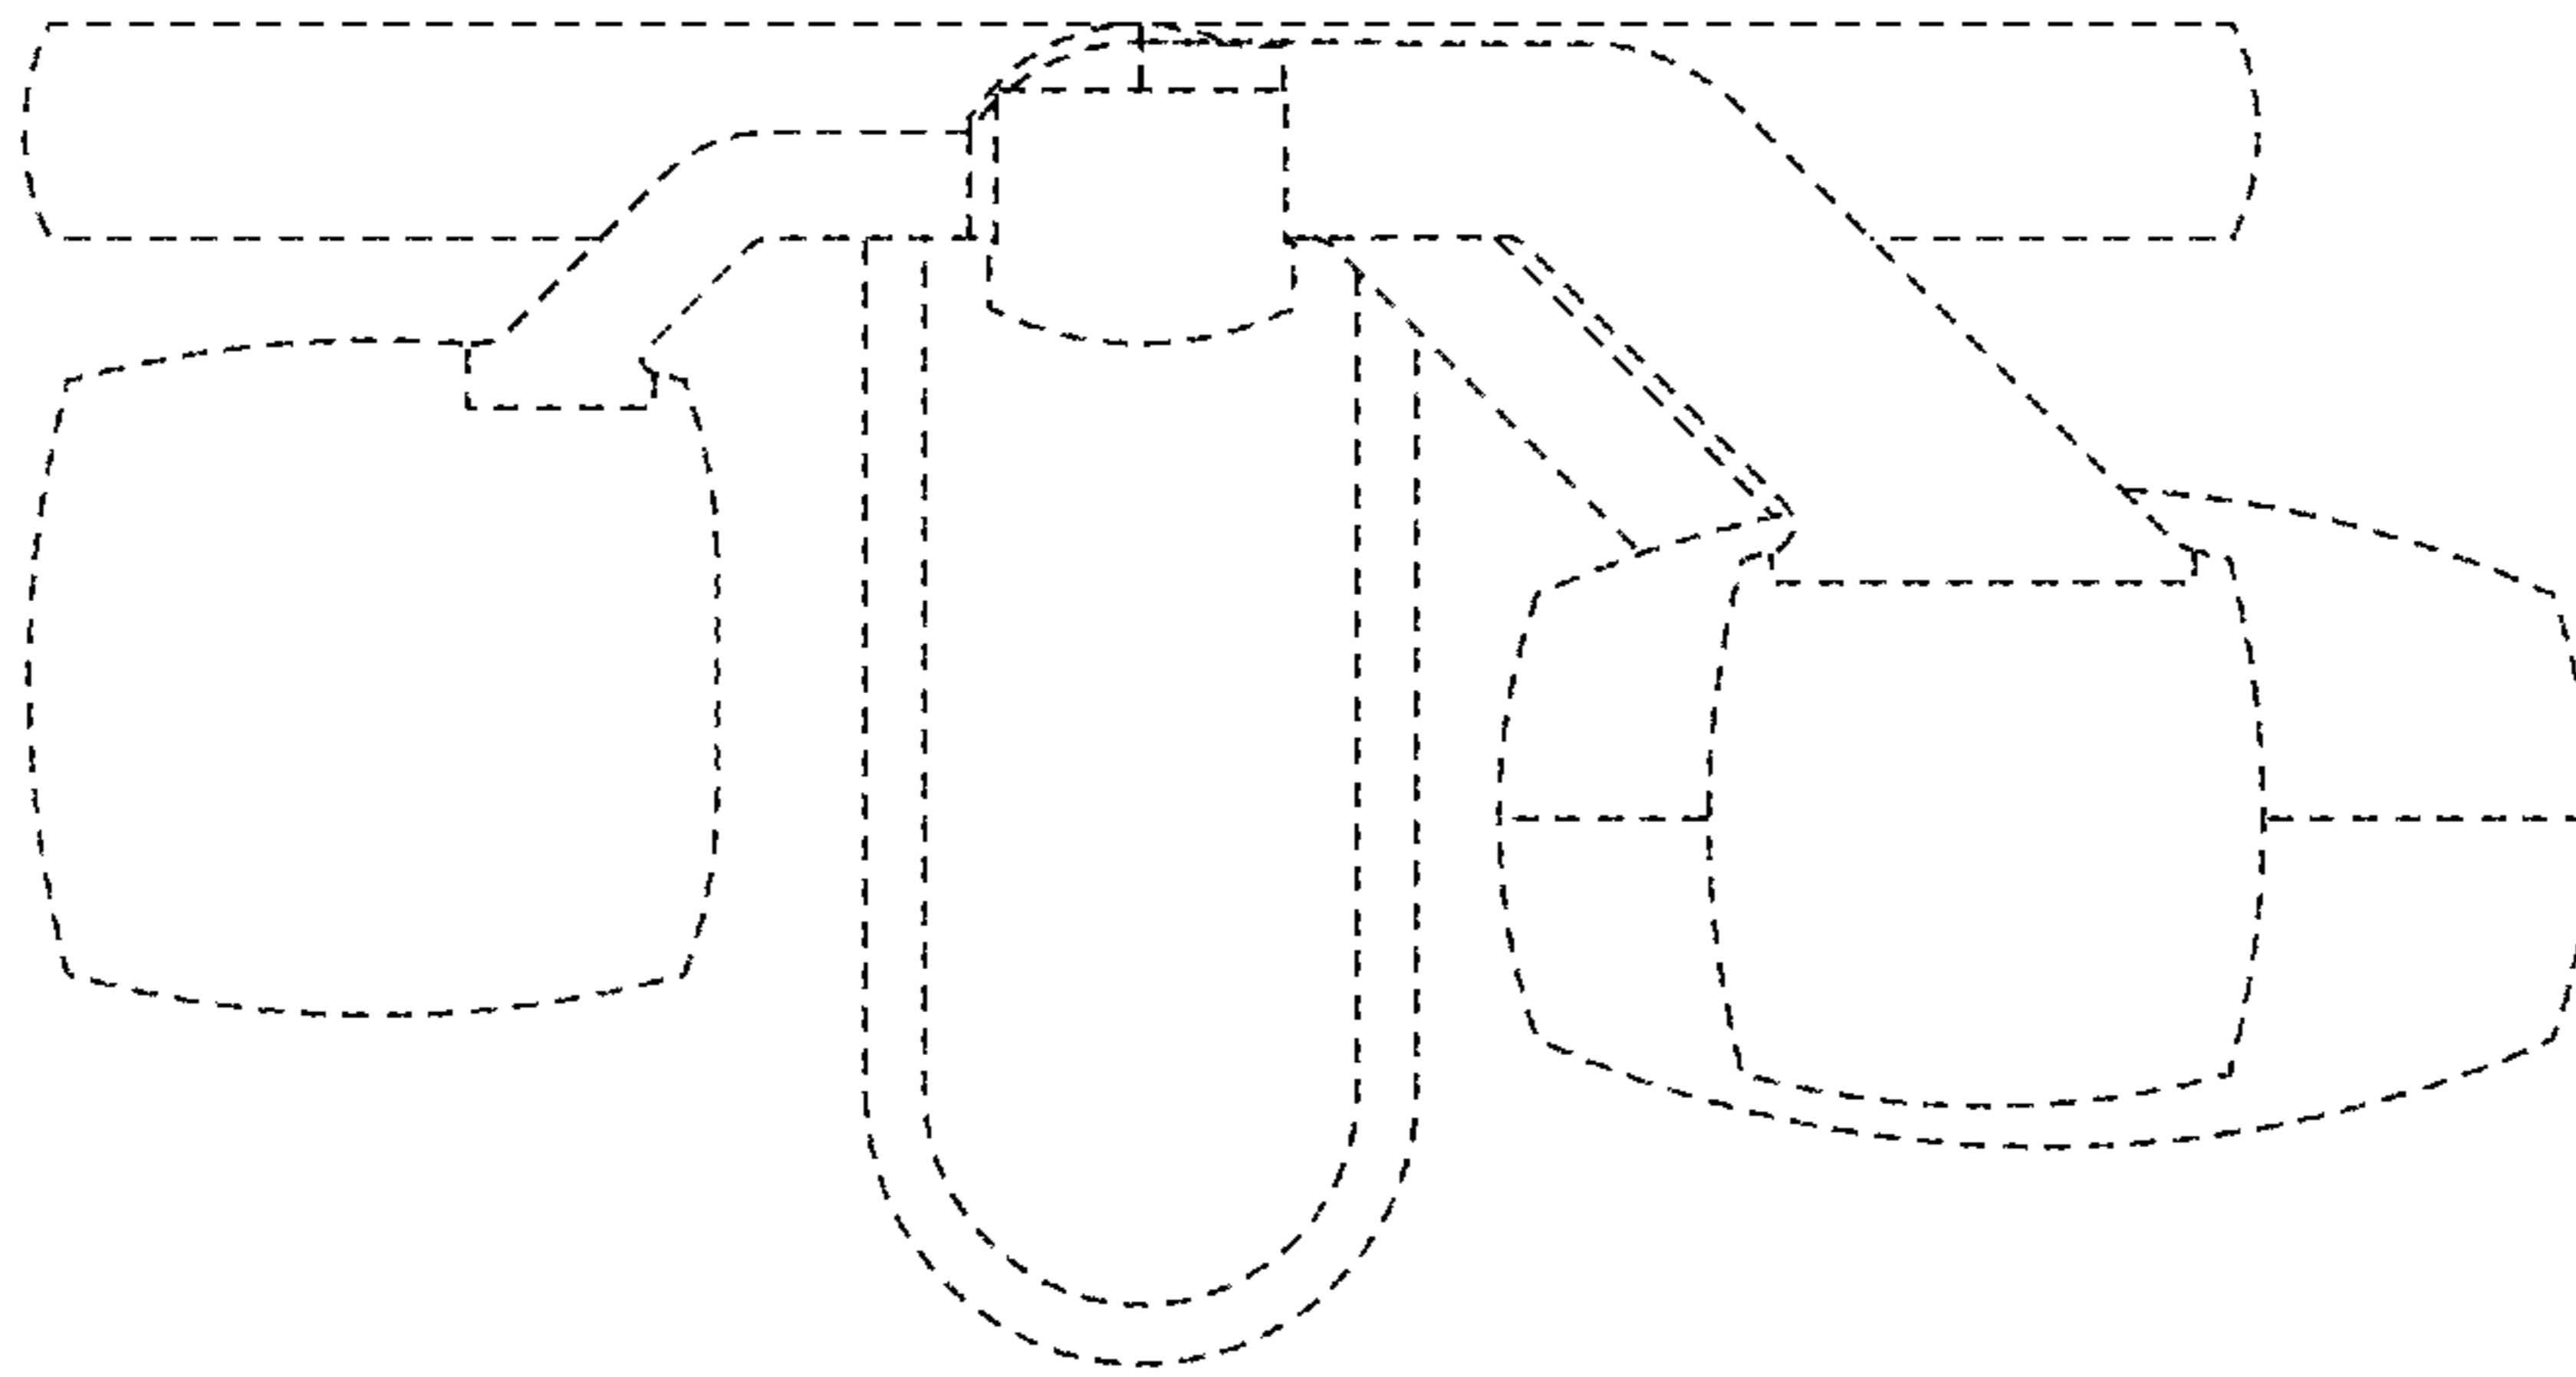


FIG. 6

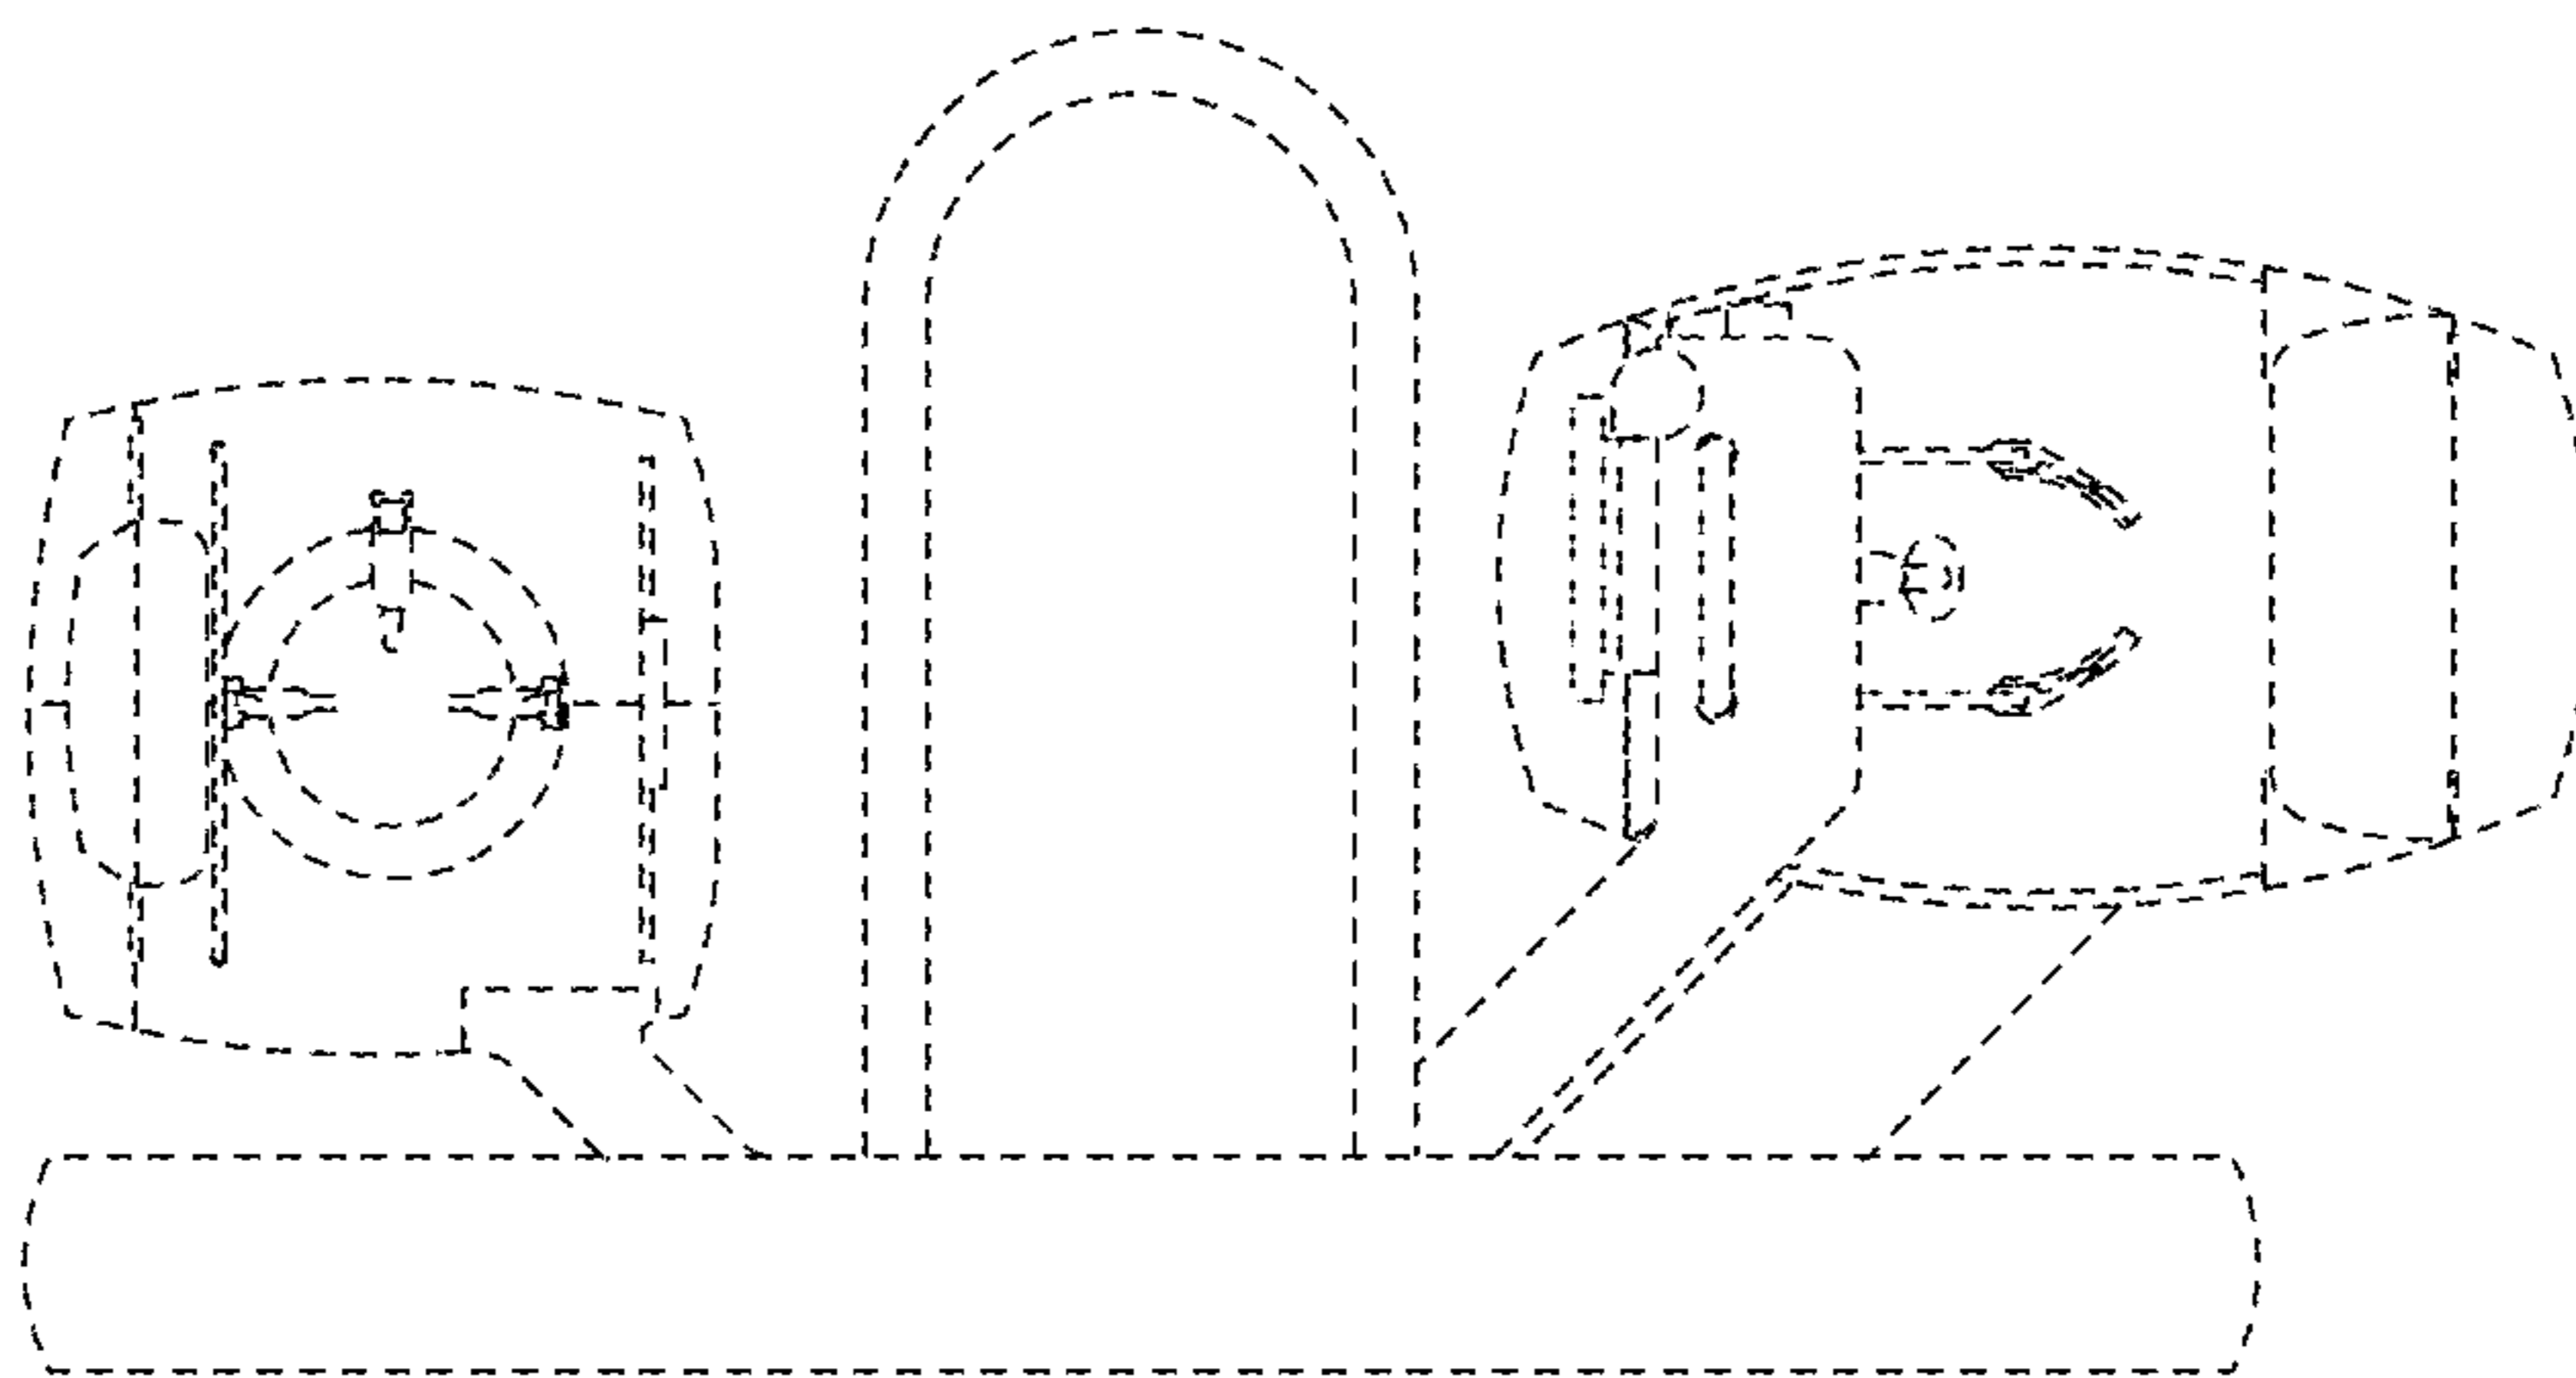


FIG. 7

