



(12) **United States Design Patent** (10) **Patent No.:** **US D872,300 S**
Demsia (45) **Date of Patent:** **** Jan. 7, 2020**

(54) **LABORATORY PIPETTE STAND**

(71) Applicant: **MTC Bio, Inc.**, Sayreville, NJ (US)
 (72) Inventor: **Walter Demsia**, Holmdel, NJ (US)
 (73) Assignee: **MTC BIO, INC.**, Sayreville, NJ (US)
 (**) Term: **15 Years**

(21) Appl. No.: **29/642,613**

(22) Filed: **Mar. 30, 2018**

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
 USPC **D24/227**

(58) **Field of Classification Search**
 USPC D24/222, 227–230, 107, 121, 133, 216;
 D19/86, 87, 88, 89, 90, 91, 92; D16/244
 CPC B01L 9/00; B01L 9/54
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|---------------|---------|-----------|-------|----------------------|
| D221,191 S * | 7/1971 | Nutt | | D19/91 |
| 4,095,697 A * | 6/1978 | Matthaei | | B01L 9/00 211/134 |
| D271,501 S * | 11/1983 | Manning | | D19/86 |
| D279,674 S * | 7/1985 | Harley | | D14/251 |
| D437,600 S * | 2/2001 | Calfee | | D14/447 |
| D501,513 S * | 2/2005 | Linyear | | D19/88 |
| D524,448 S * | 7/2006 | Telimaa | | D24/227 |
| D633,149 S * | 2/2011 | Parshad | | D19/91 |
| D660,912 S * | 5/2012 | Denzinger | | D19/91 |
| D754,872 S * | 4/2016 | Li | | D24/227 |
| D756,346 S * | 5/2016 | Kim | | D14/253 |
| D806,450 S * | 1/2018 | Seong | | D6/672 |
| D814,653 S * | 4/2018 | Shedlosky | | D24/229 |

(Continued)

OTHER PUBLICATIONS

SureStand™ Multi-Channel Capable Pipette Rack—Patent Pending. Online, published date May 28, 2018. Retrieved on Jun. 2, 2019 from URL: <https://mtcbiotech.com/product/surestand-multi-channel-capable-pipette-rack/>.*

(Continued)

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Fox Rothschild LLP


(57) **CLAIM**

The ornamental design for a laboratory pipette stand, as shown and described.

DESCRIPTION

FIG. 1 is a left, front, top perspective view of the first embodiment of a laboratory pipette stand showing my new design;
 FIG. 2 is a right, front, top perspective view thereof;
 FIG. 3 is a front elevation view thereof;
 FIG. 4 is a rear elevation view thereof;
 FIG. 5 is a left side elevation view thereof;
 FIG. 6 is a right side elevation view thereof;
 FIG. 7 is a top plan view thereof;
 FIG. 8 is a bottom plan view thereof;
 FIG. 9 is a left, front, top perspective view of the second embodiment of a laboratory pipette stand;
 FIG. 10 is a right, front, top perspective view thereof;
 FIG. 11 is a front elevation view thereof;
 FIG. 12 is a rear elevation view thereof;
 FIG. 13 is a left side elevation view thereof;
 FIG. 14 is a right side elevation view thereof;
 FIG. 15 is a top plan view thereof; and,
 FIG. 16 is a bottom plan view thereof.
 The broken lines in the drawings depict portions of the laboratory pipette stand that form no part of the claimed design.

1 Claim, 12 Drawing Sheets

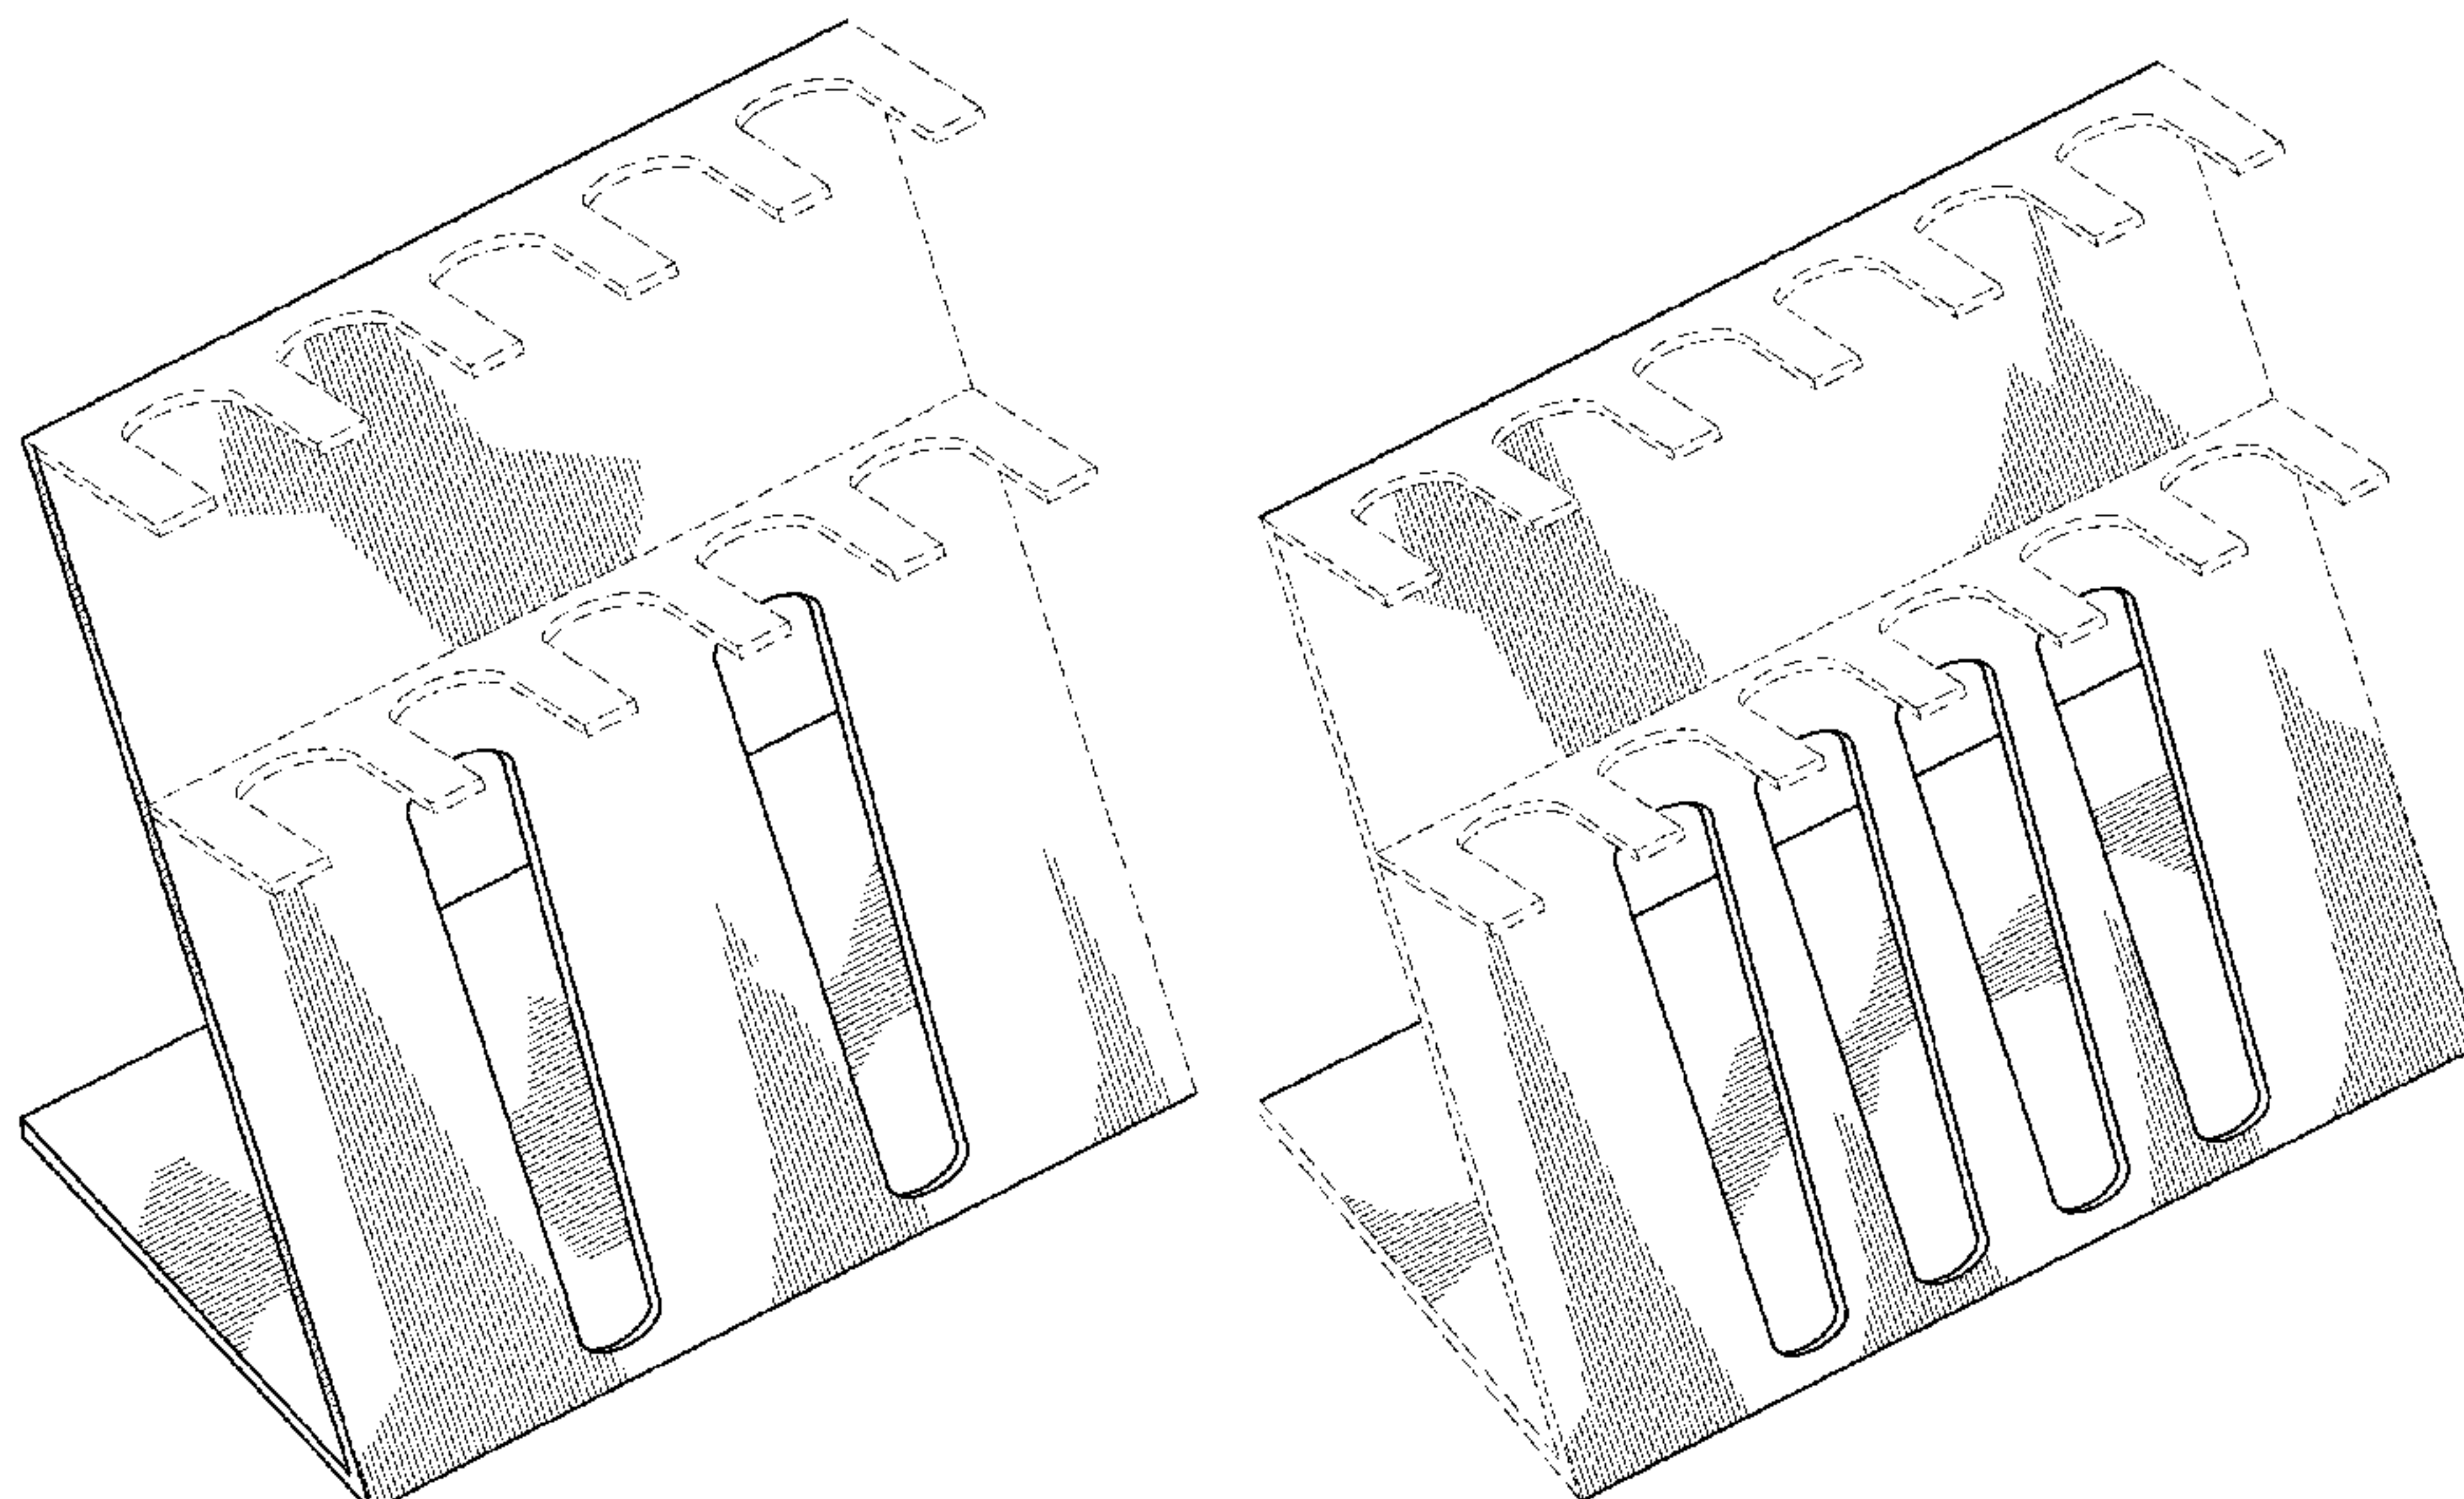

(56)

References Cited

U.S. PATENT DOCUMENTS

2016/0069508 A1* 3/2016 Haymond F16M 11/38
29/857

2016/0346783 A1* 12/2016 Moroney B01L 9/54

OTHER PUBLICATIONS

Heathrow Scientific® “Acrylic and ABS Pipette Stands” printed on Apr. 3, 2018, available at http://www.heathrowscientific.com/acrylic-and-abs-pipette-stands-i-hea206203-group?_vsrefdom=adwords&gclid=Cj0KCQjwqYfWBRDPARIsABjQRYwEuUIFW5n9v6KS9gMTL01yhXkajMsoalENERT_X8ZmT8MfKzCE4PMaAm8EALw_wcB.

Yahoo.com Image search for “pipette stand”, printed on Apr. 3, 2018, available at https://images.search.yahoo.com/search/images;_ylt=AwrE189hpMJJaHKUAxC5XNyoA;_ylu=X3oDMTB0N2Noc211BGNvbG8DYmYxBHBvcwMxBHZ0aWQDBHNIYwNwaXZz?

p=pipette+stand&fr2=piv-web&fr=yfp-t#id=0&iurl=http%3A%2F%2Fflabreco.com%2Fdata%2Fcatalog%2Fproducts%2F1847%2Fmain%2F6-Place%2520Pipettor%2520Stand.png&action=click.

Yahoo.com image search for “pipette stand” printed on Apr. 3, 2018, available at https://images.search.yahoo.com/search/images;_ylt=AwrE189hpMJJaHKUAxC5XNyoA;_ylu=X3oDMTB0N2Noc211BGNvbG8DYmYxBHBvcwMxBHZ0aWQDBHNIYwNwaXZz?p=pipette+stand&fr2=piv-web&fr=yfp-t#id=0&iurl=http%3A%2F%2Fflabreco.com%2Fdata%2Fcatalog%2Fproducts%2F1847%2Fmain%2F6-Place%2520Pipettor%2520Stand.png&action=close.

Yahoo.com Image search for “pipette stand”, printed on Apr. 3, 2018, available at https://images.search.yahoo.com/search/images;_ylt=AwrE189hpMJJaHKUAxC5XNyoA;_ylu=X3oDMTB0N2Noc211BGNvbG8DYmYxBHBvcwMxBHZ0aWQDBHNIYwNwaXZz?p=pipette+stand&fr2=piv-web&fr=yfp-t#id=190&iurl=http%3A%2F%2Fblog.universalmedicalinc.com%2Fwp-content%2Fuploads%2Fsites%2F136%2Fgallery%2Fpostimages%2F6-Place-Blue-ABS-Pipette-Stand.jpg&action=click.

* cited by examiner

FIG. 1

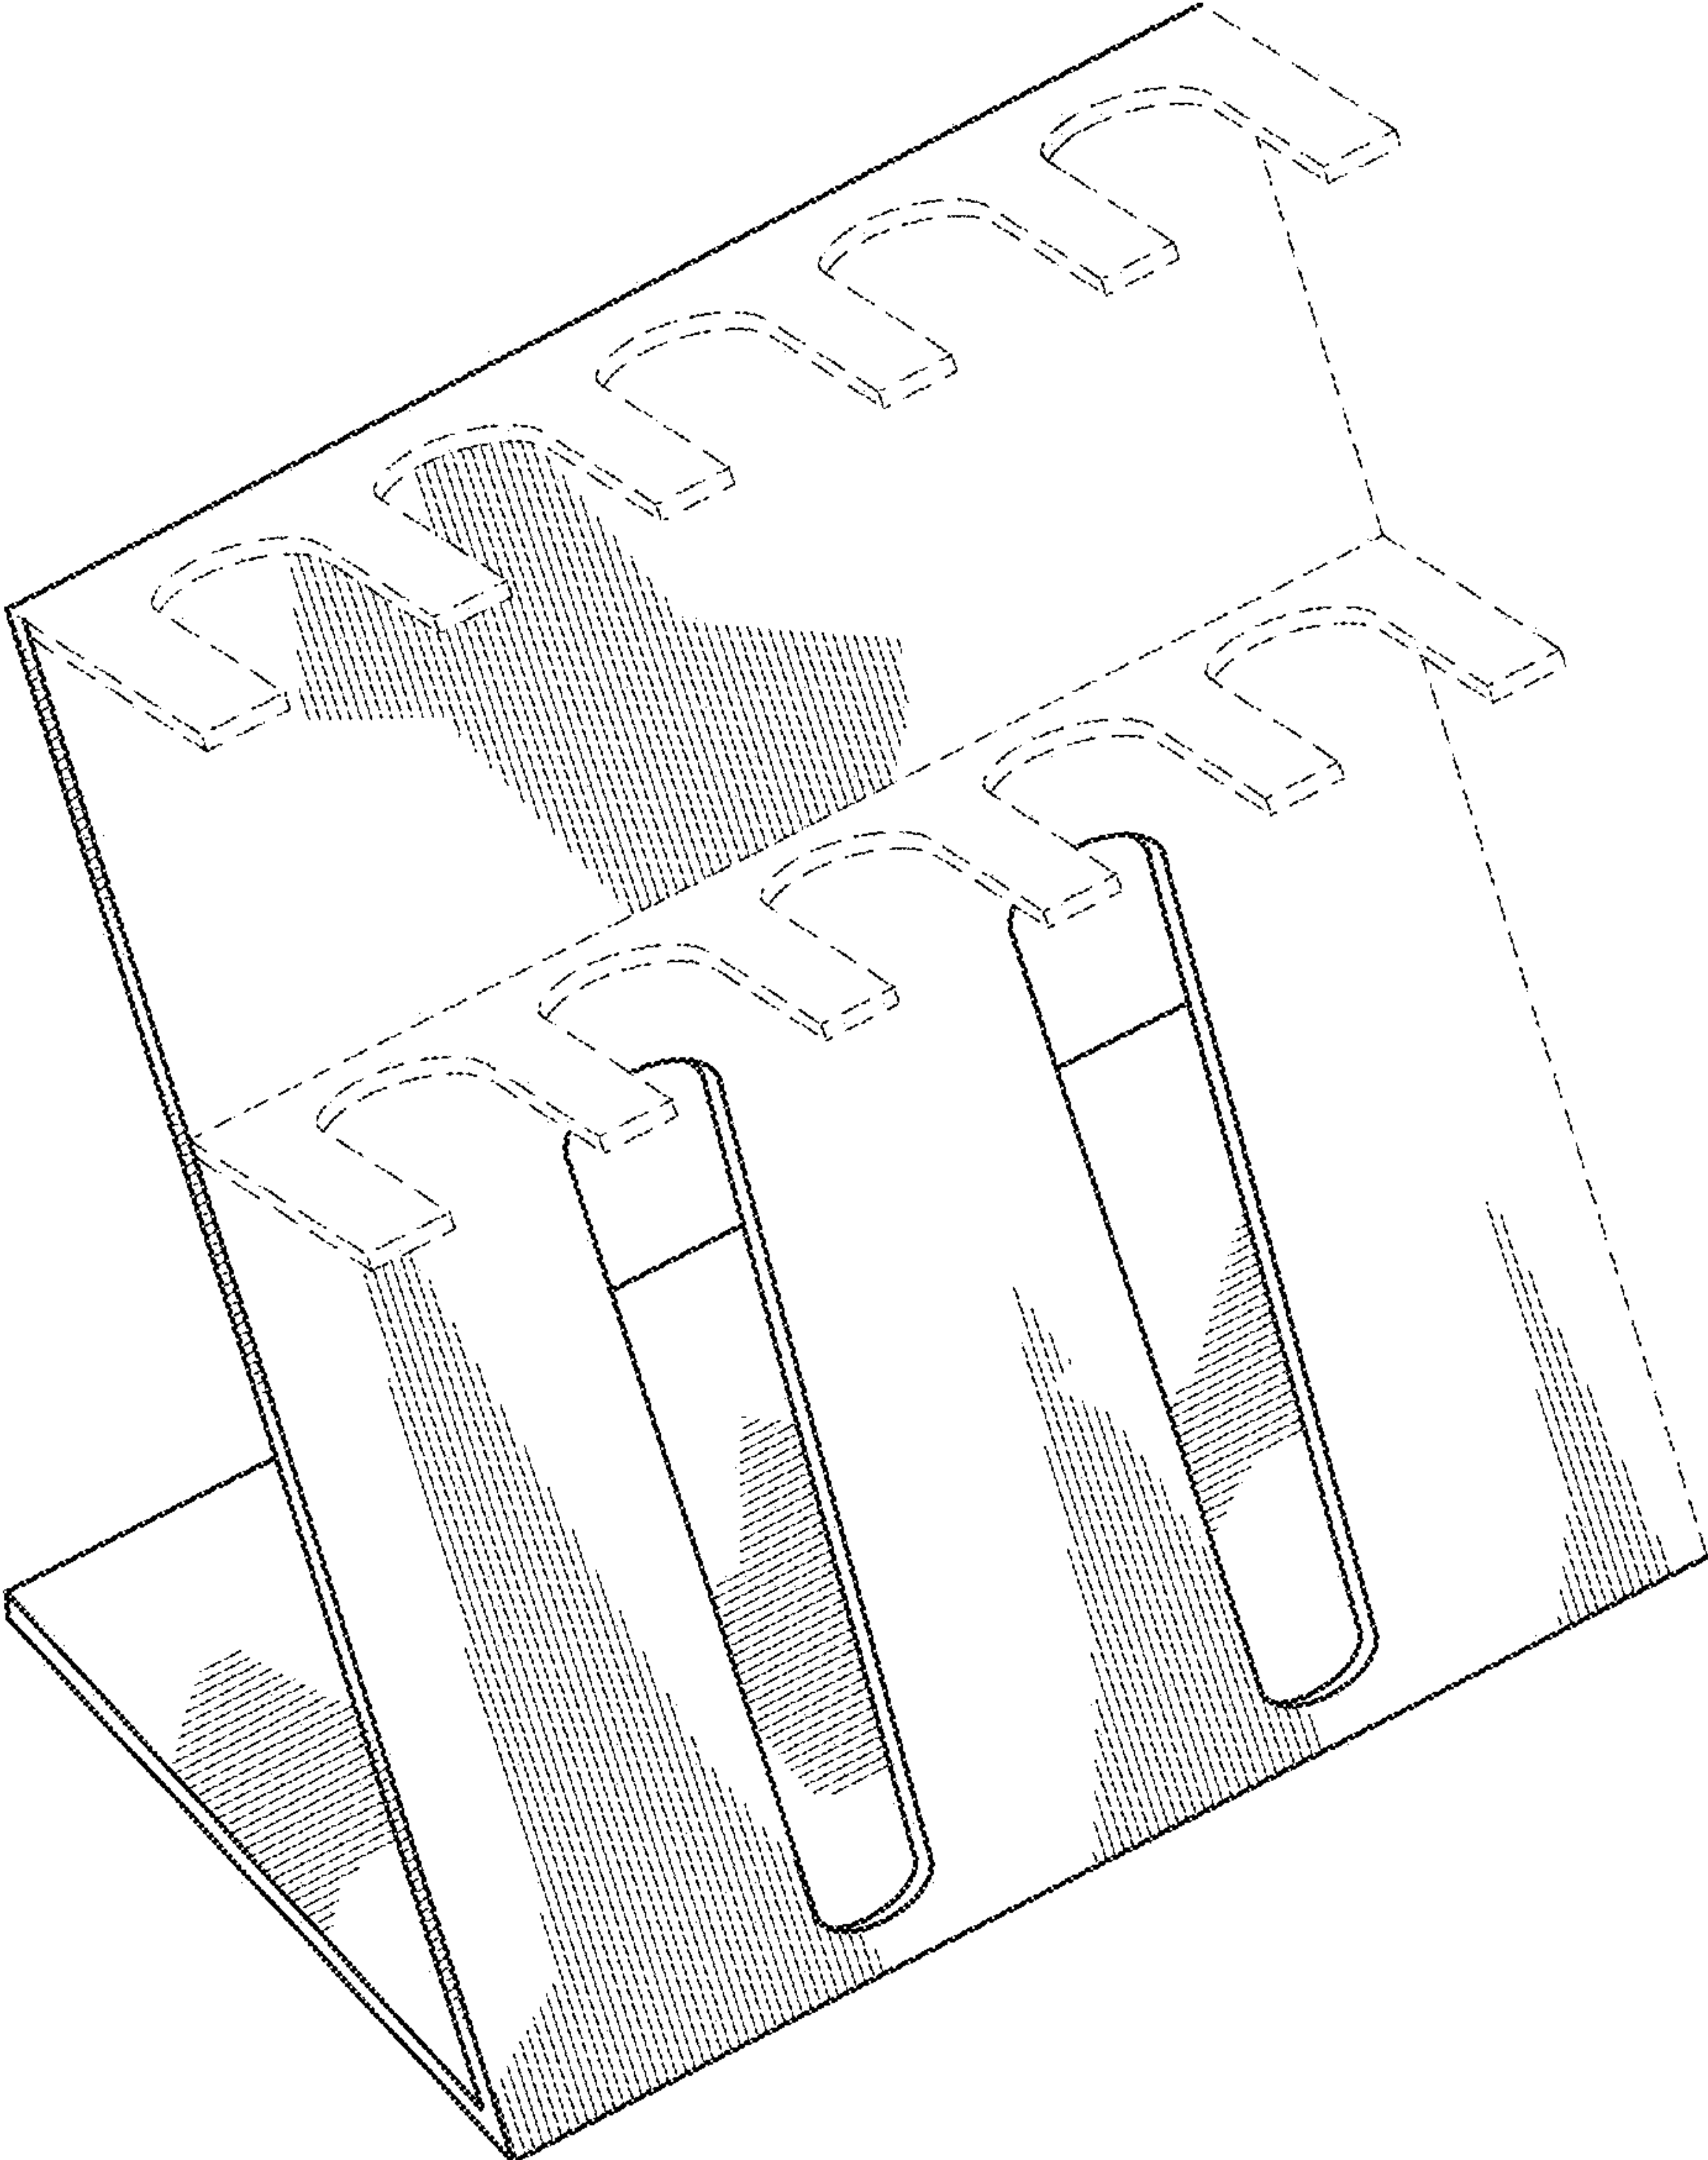
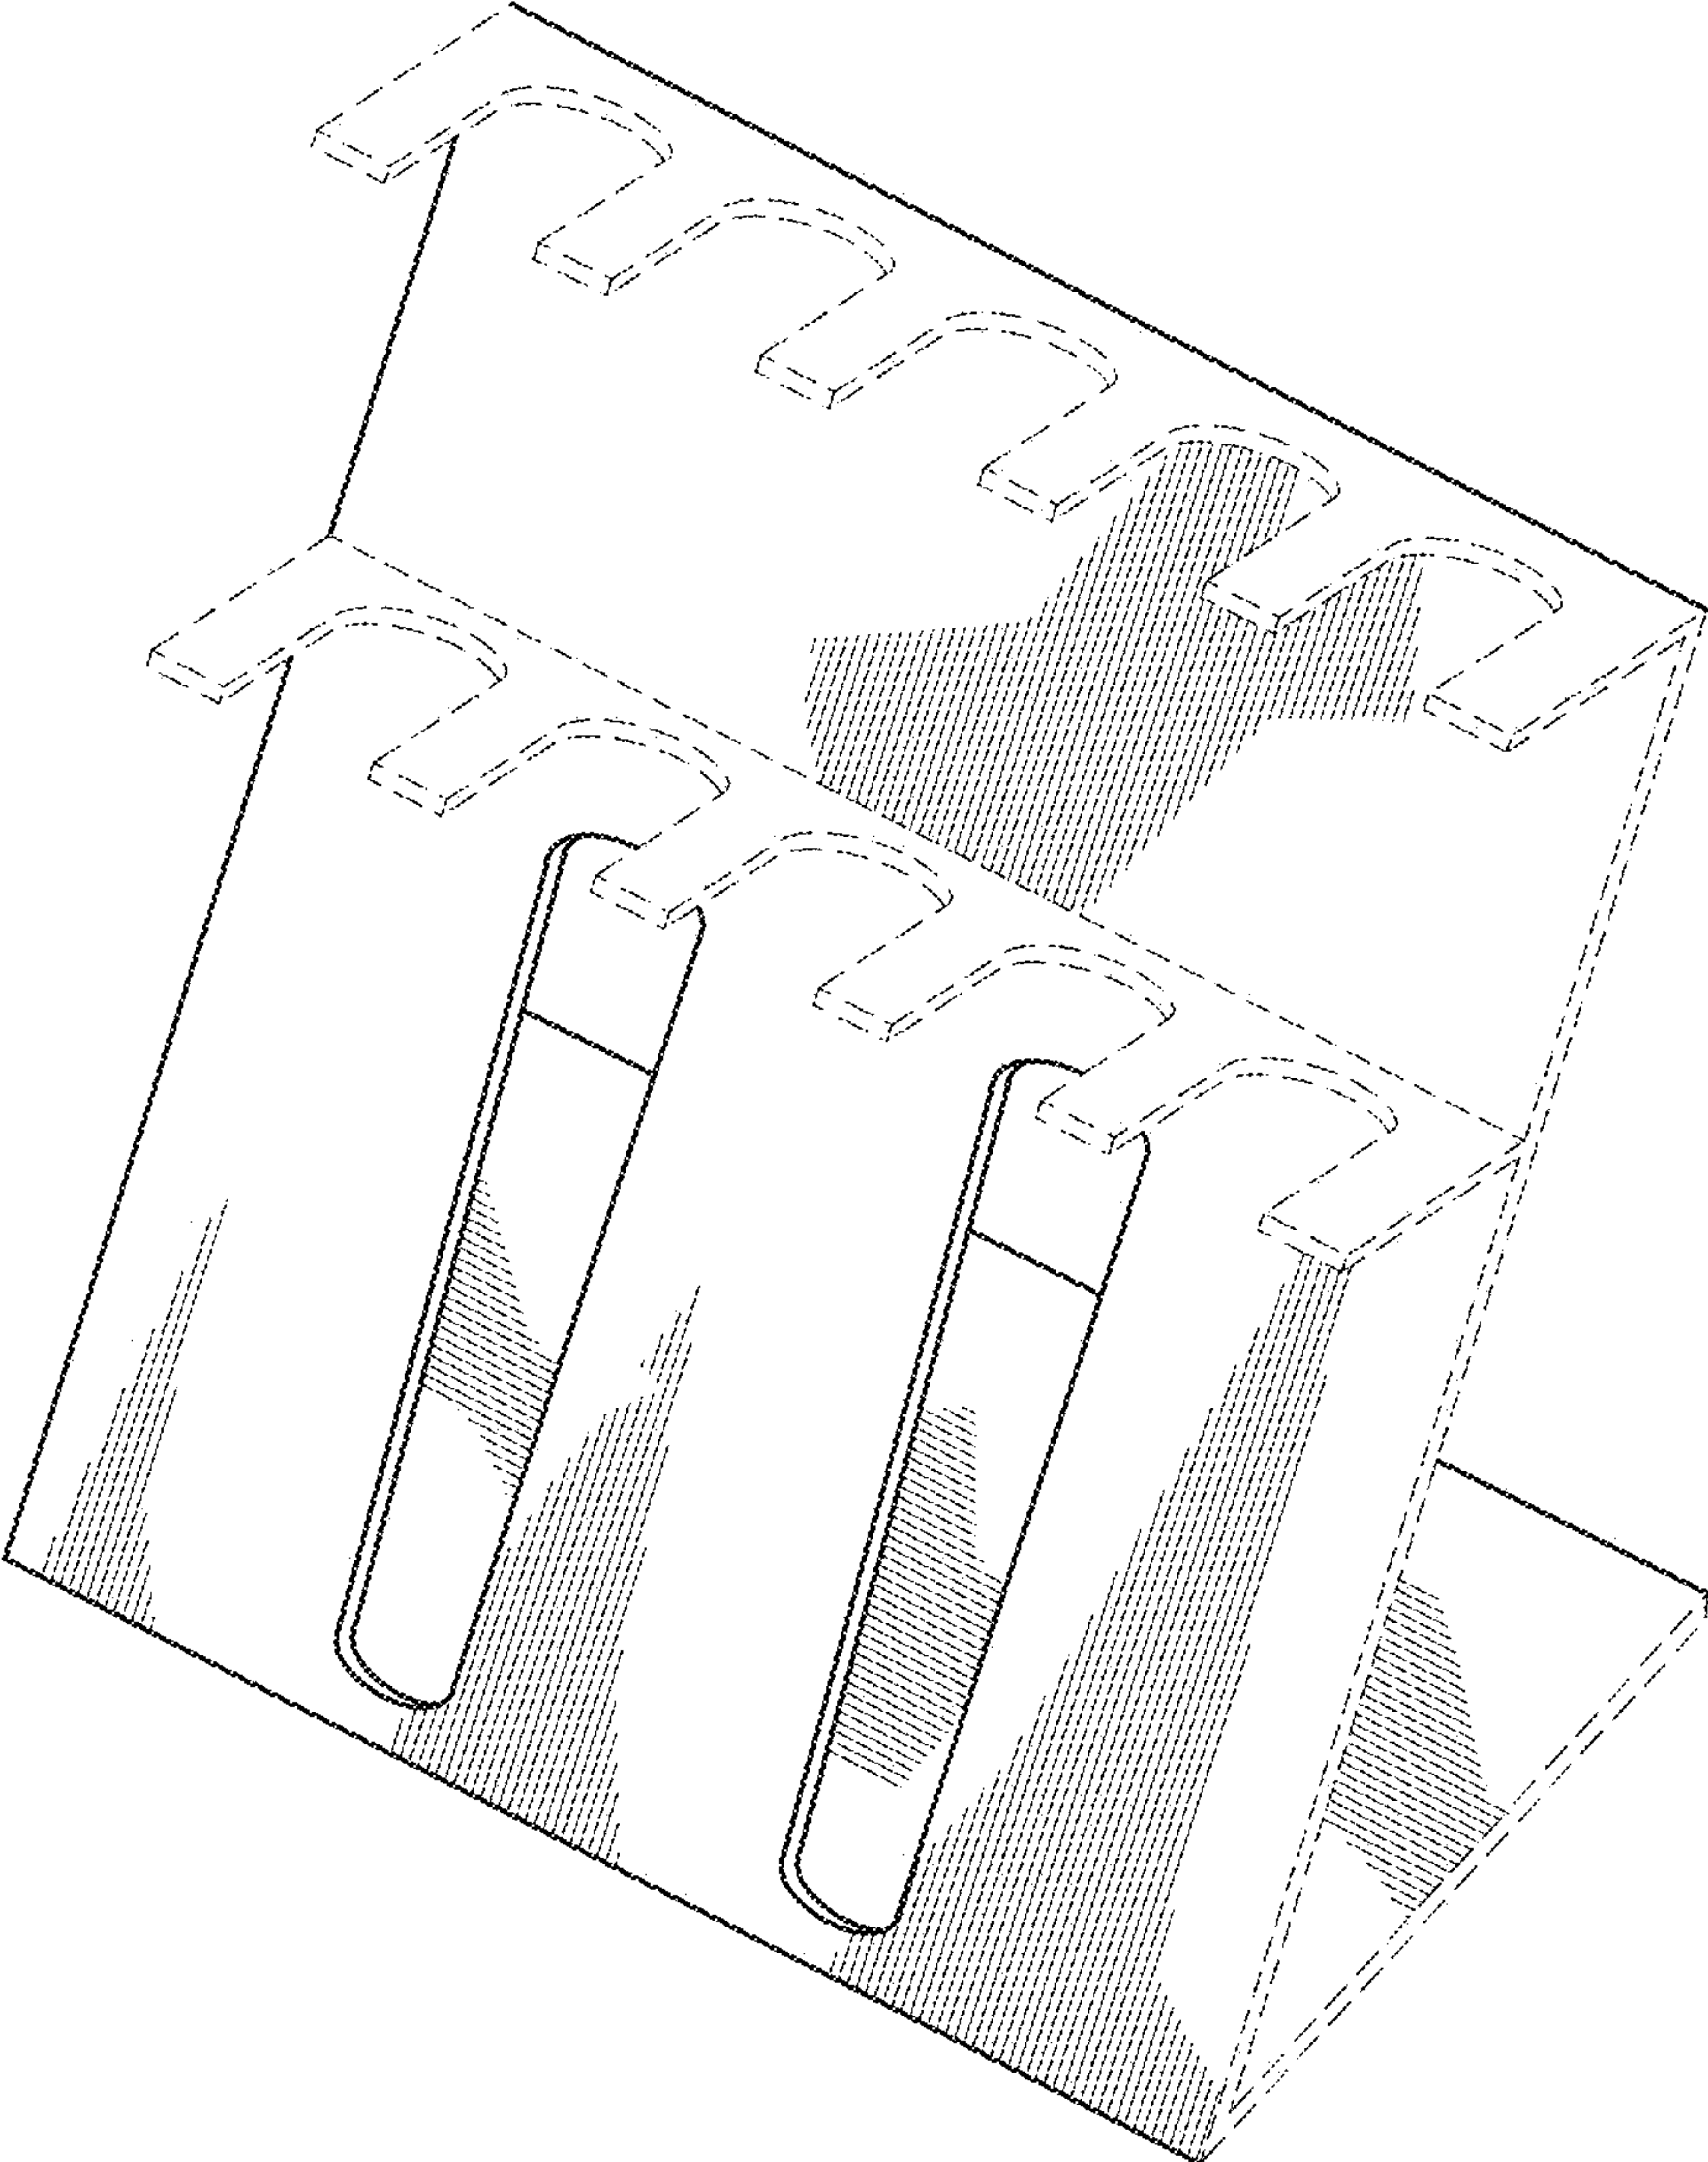


FIG. 2



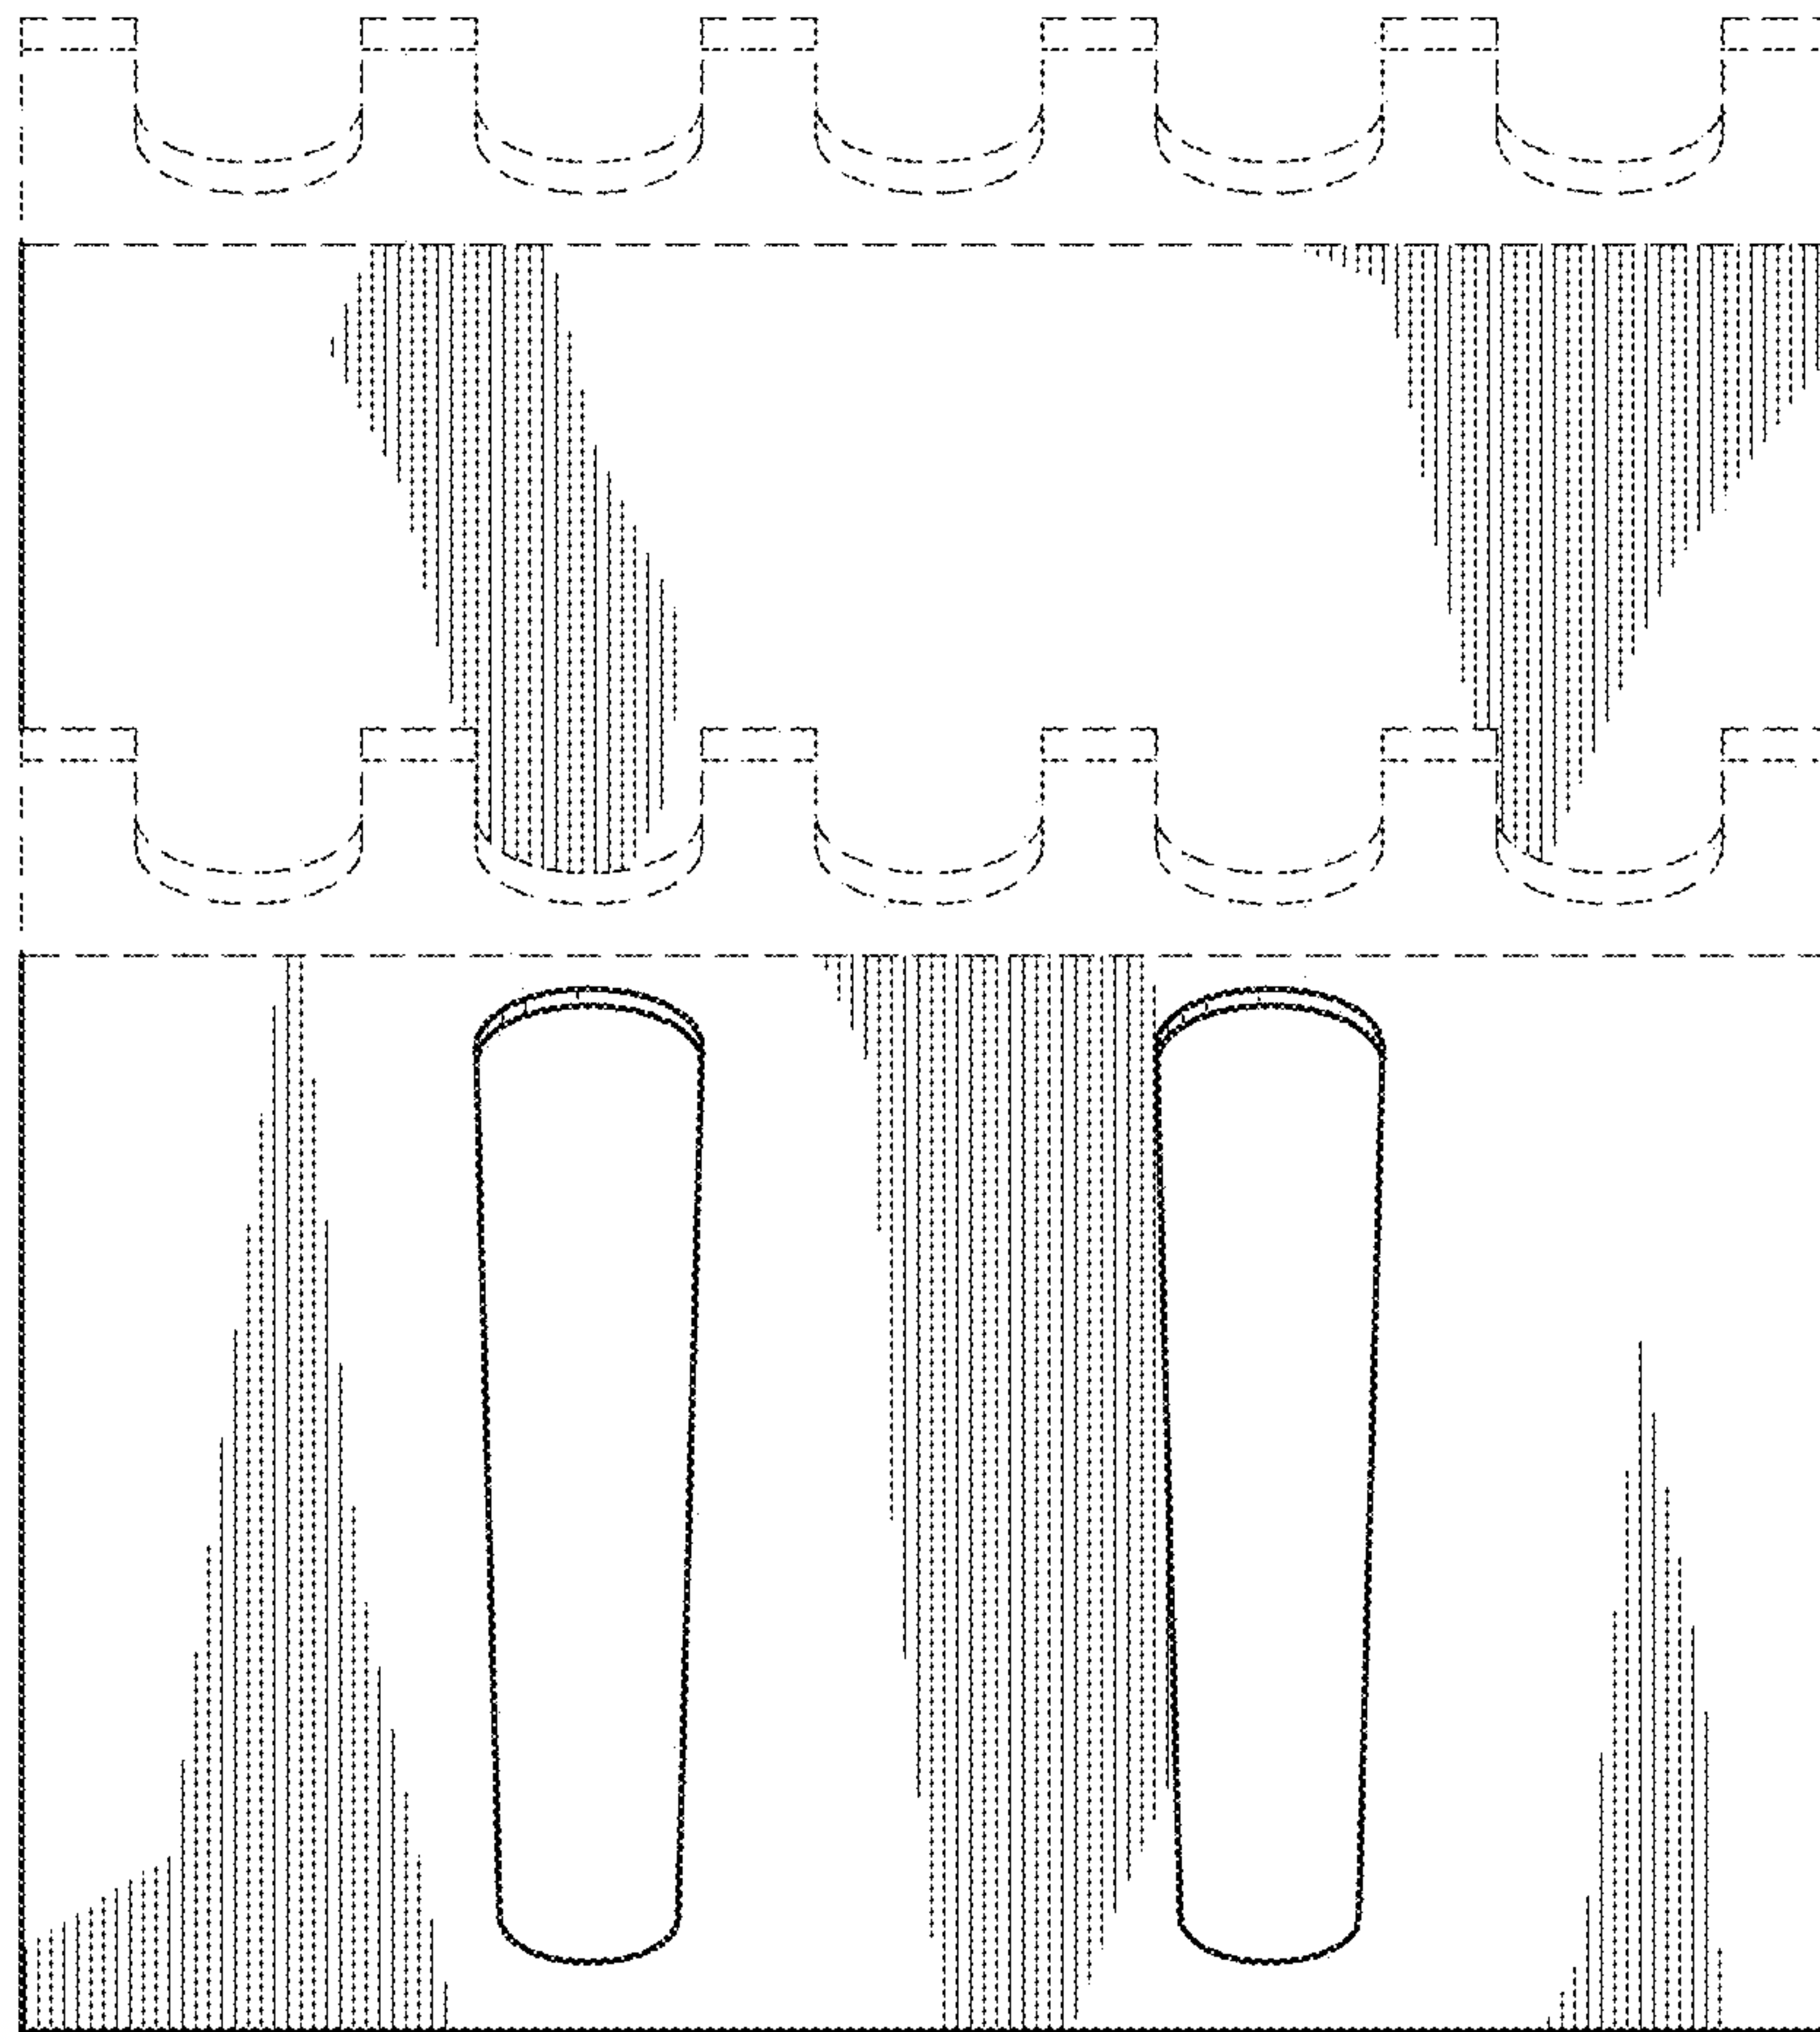


FIG. 3

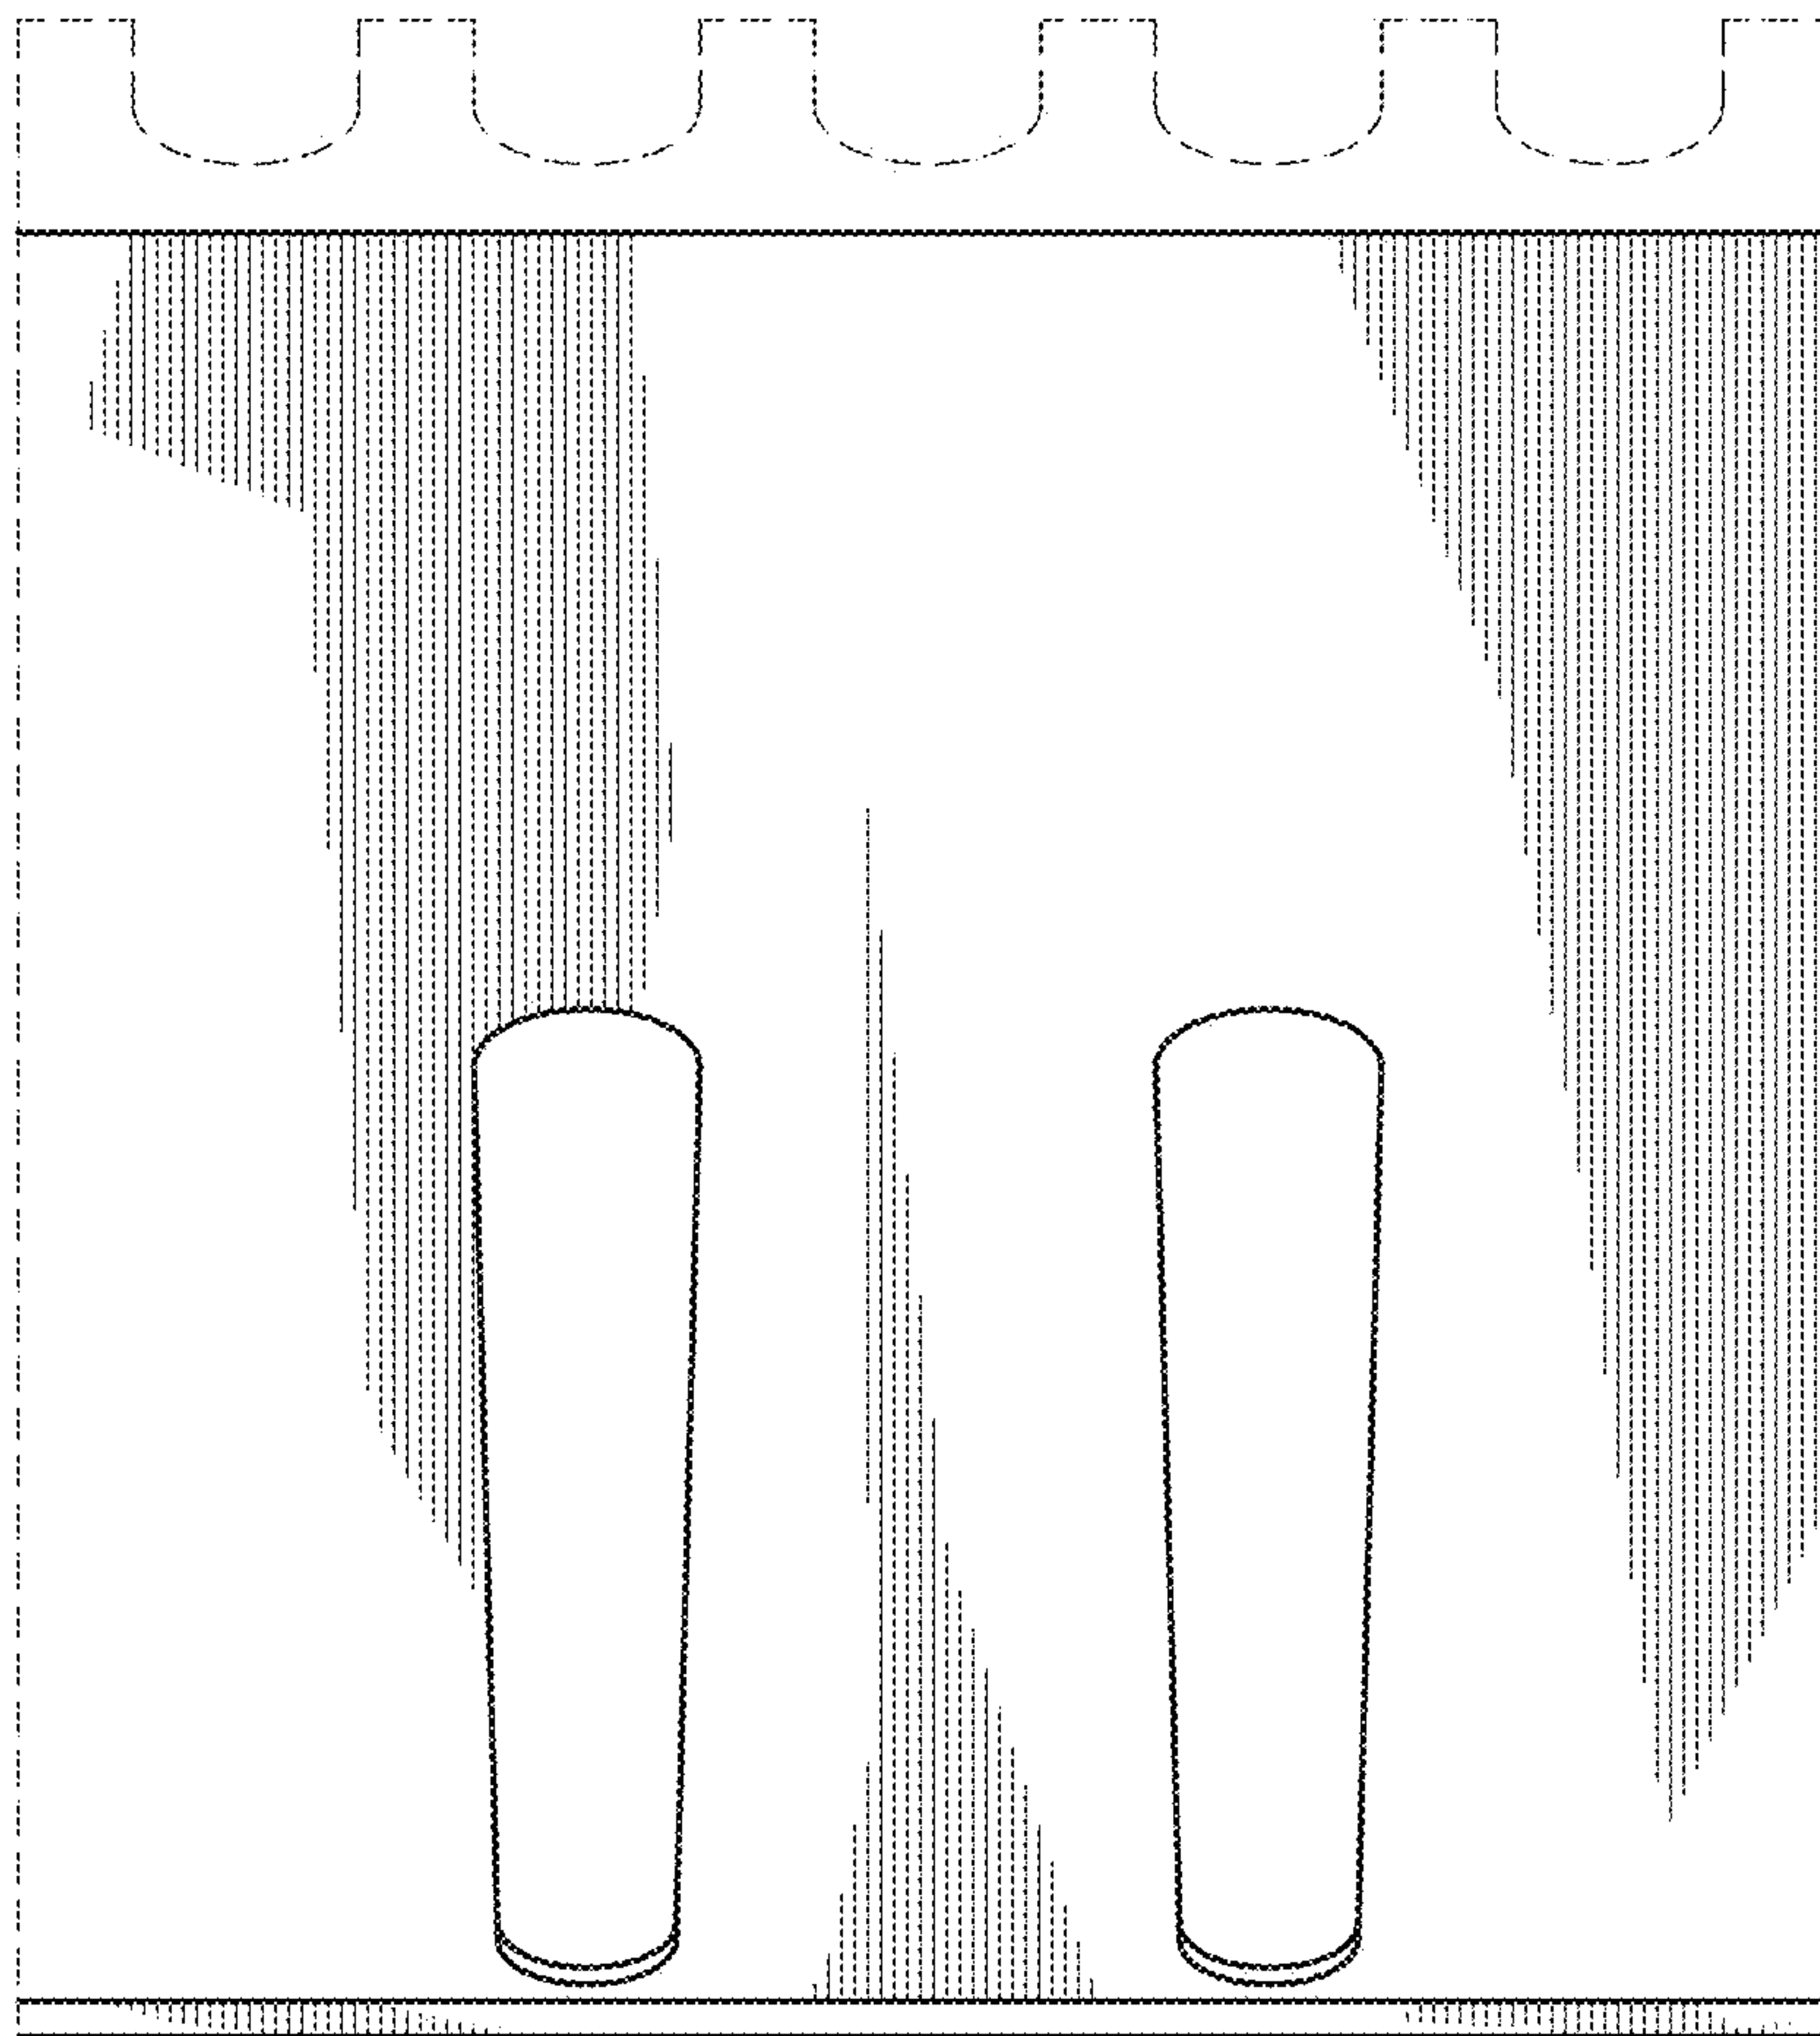


FIG. 4

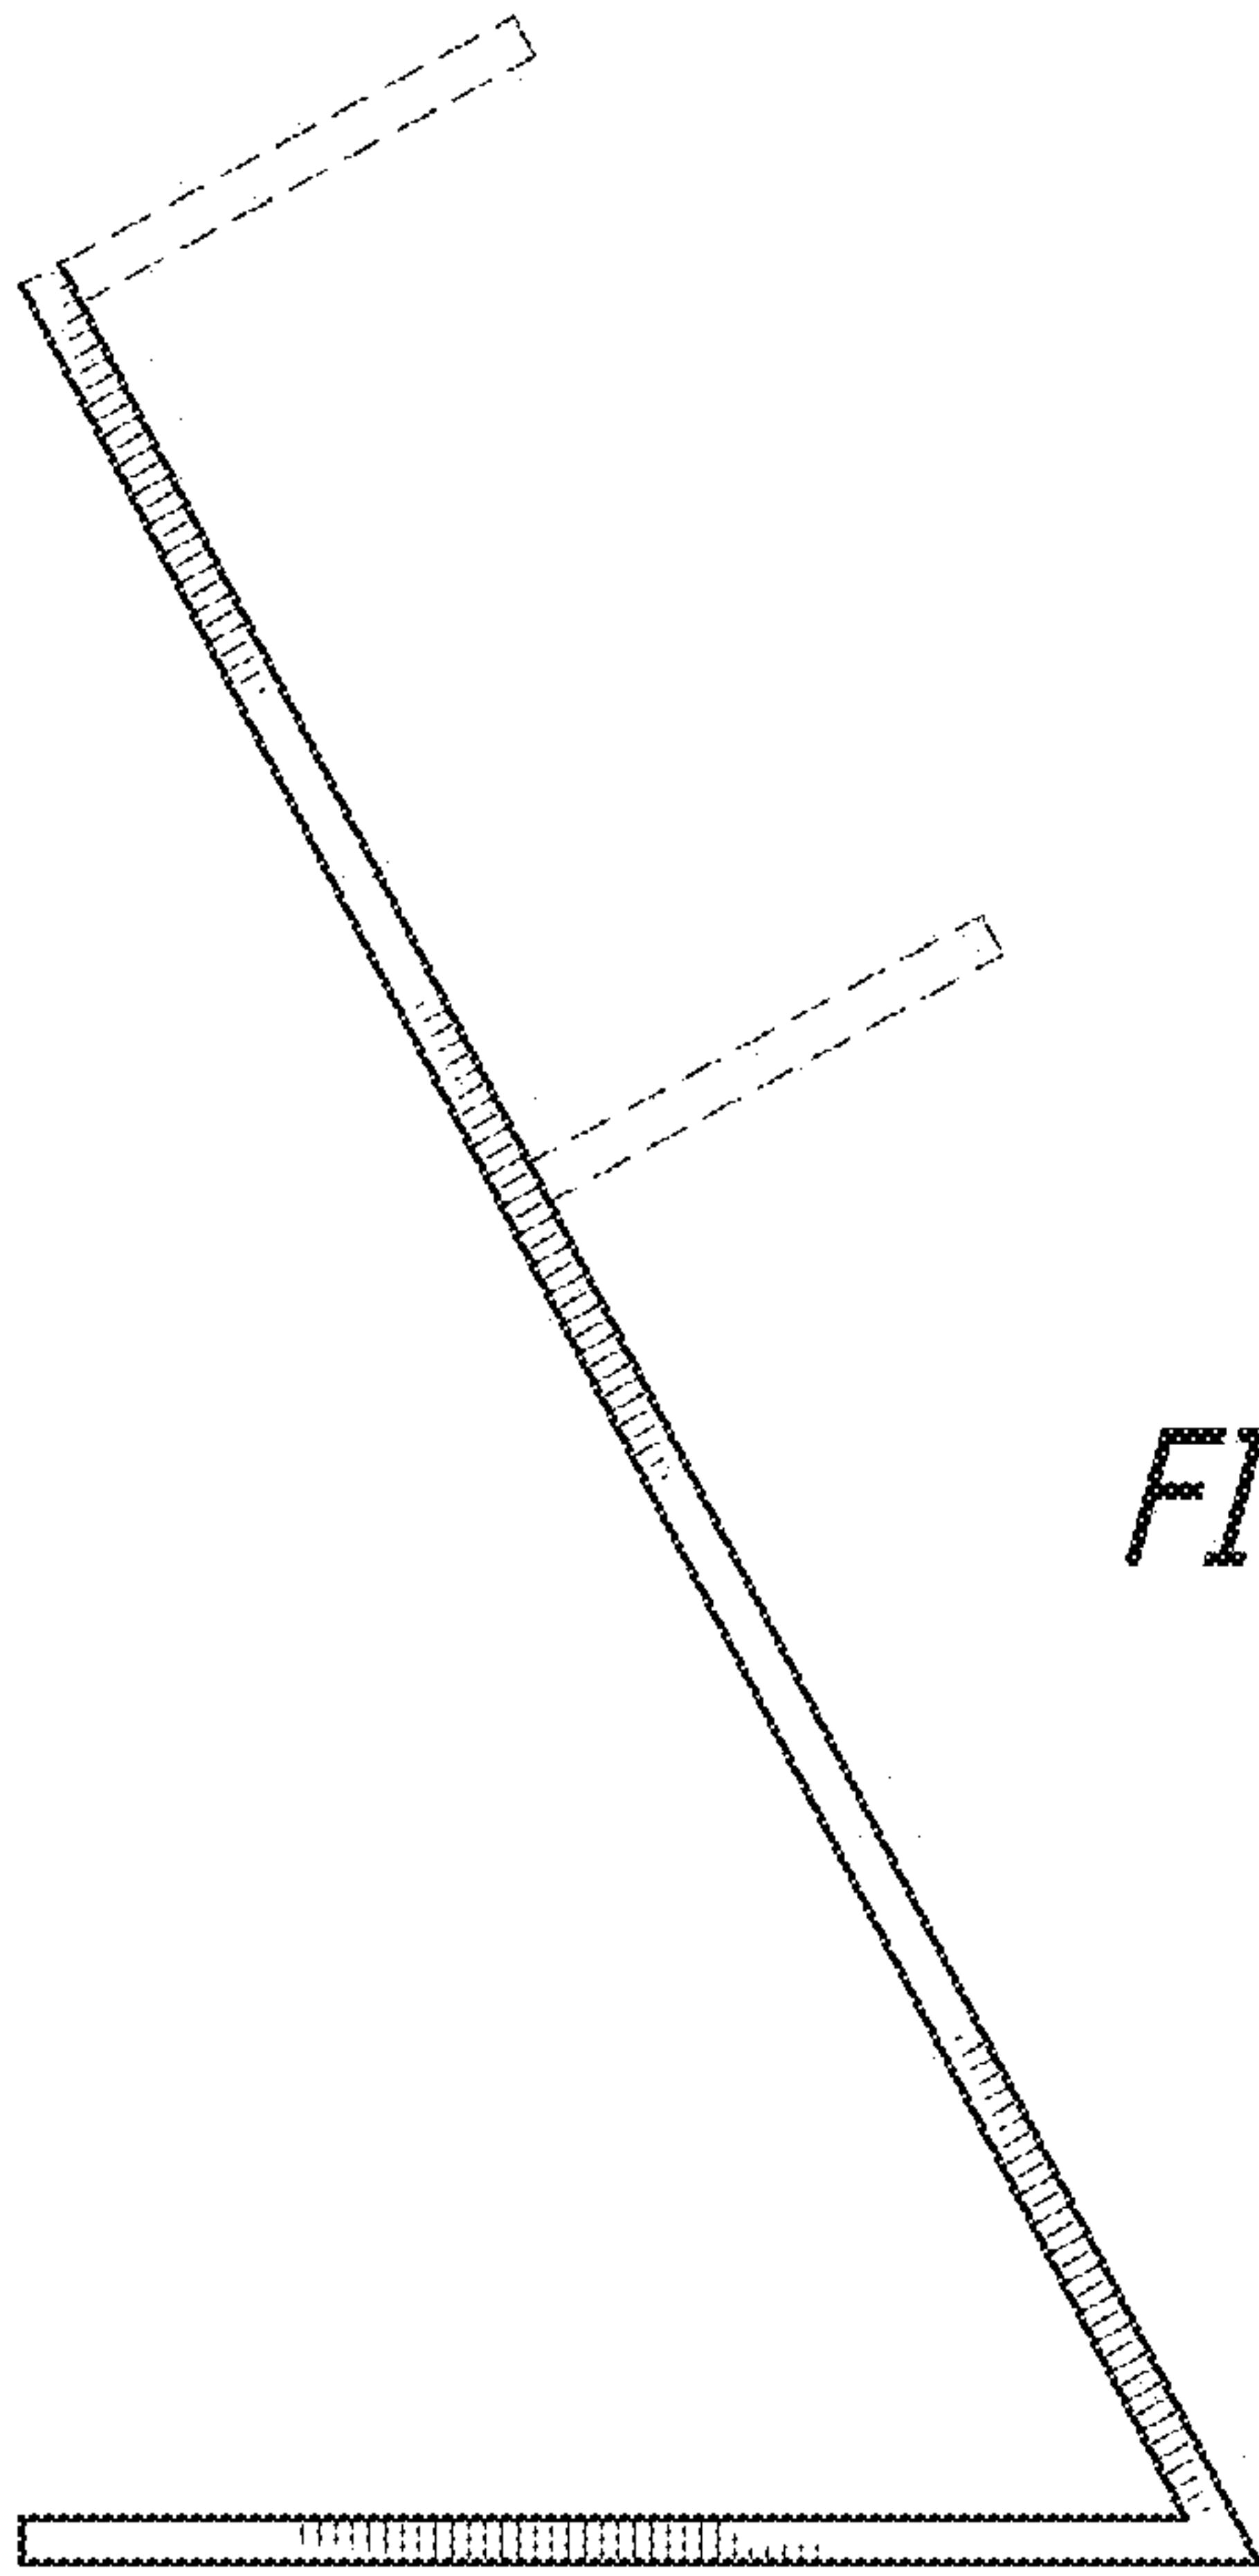


FIG. 5

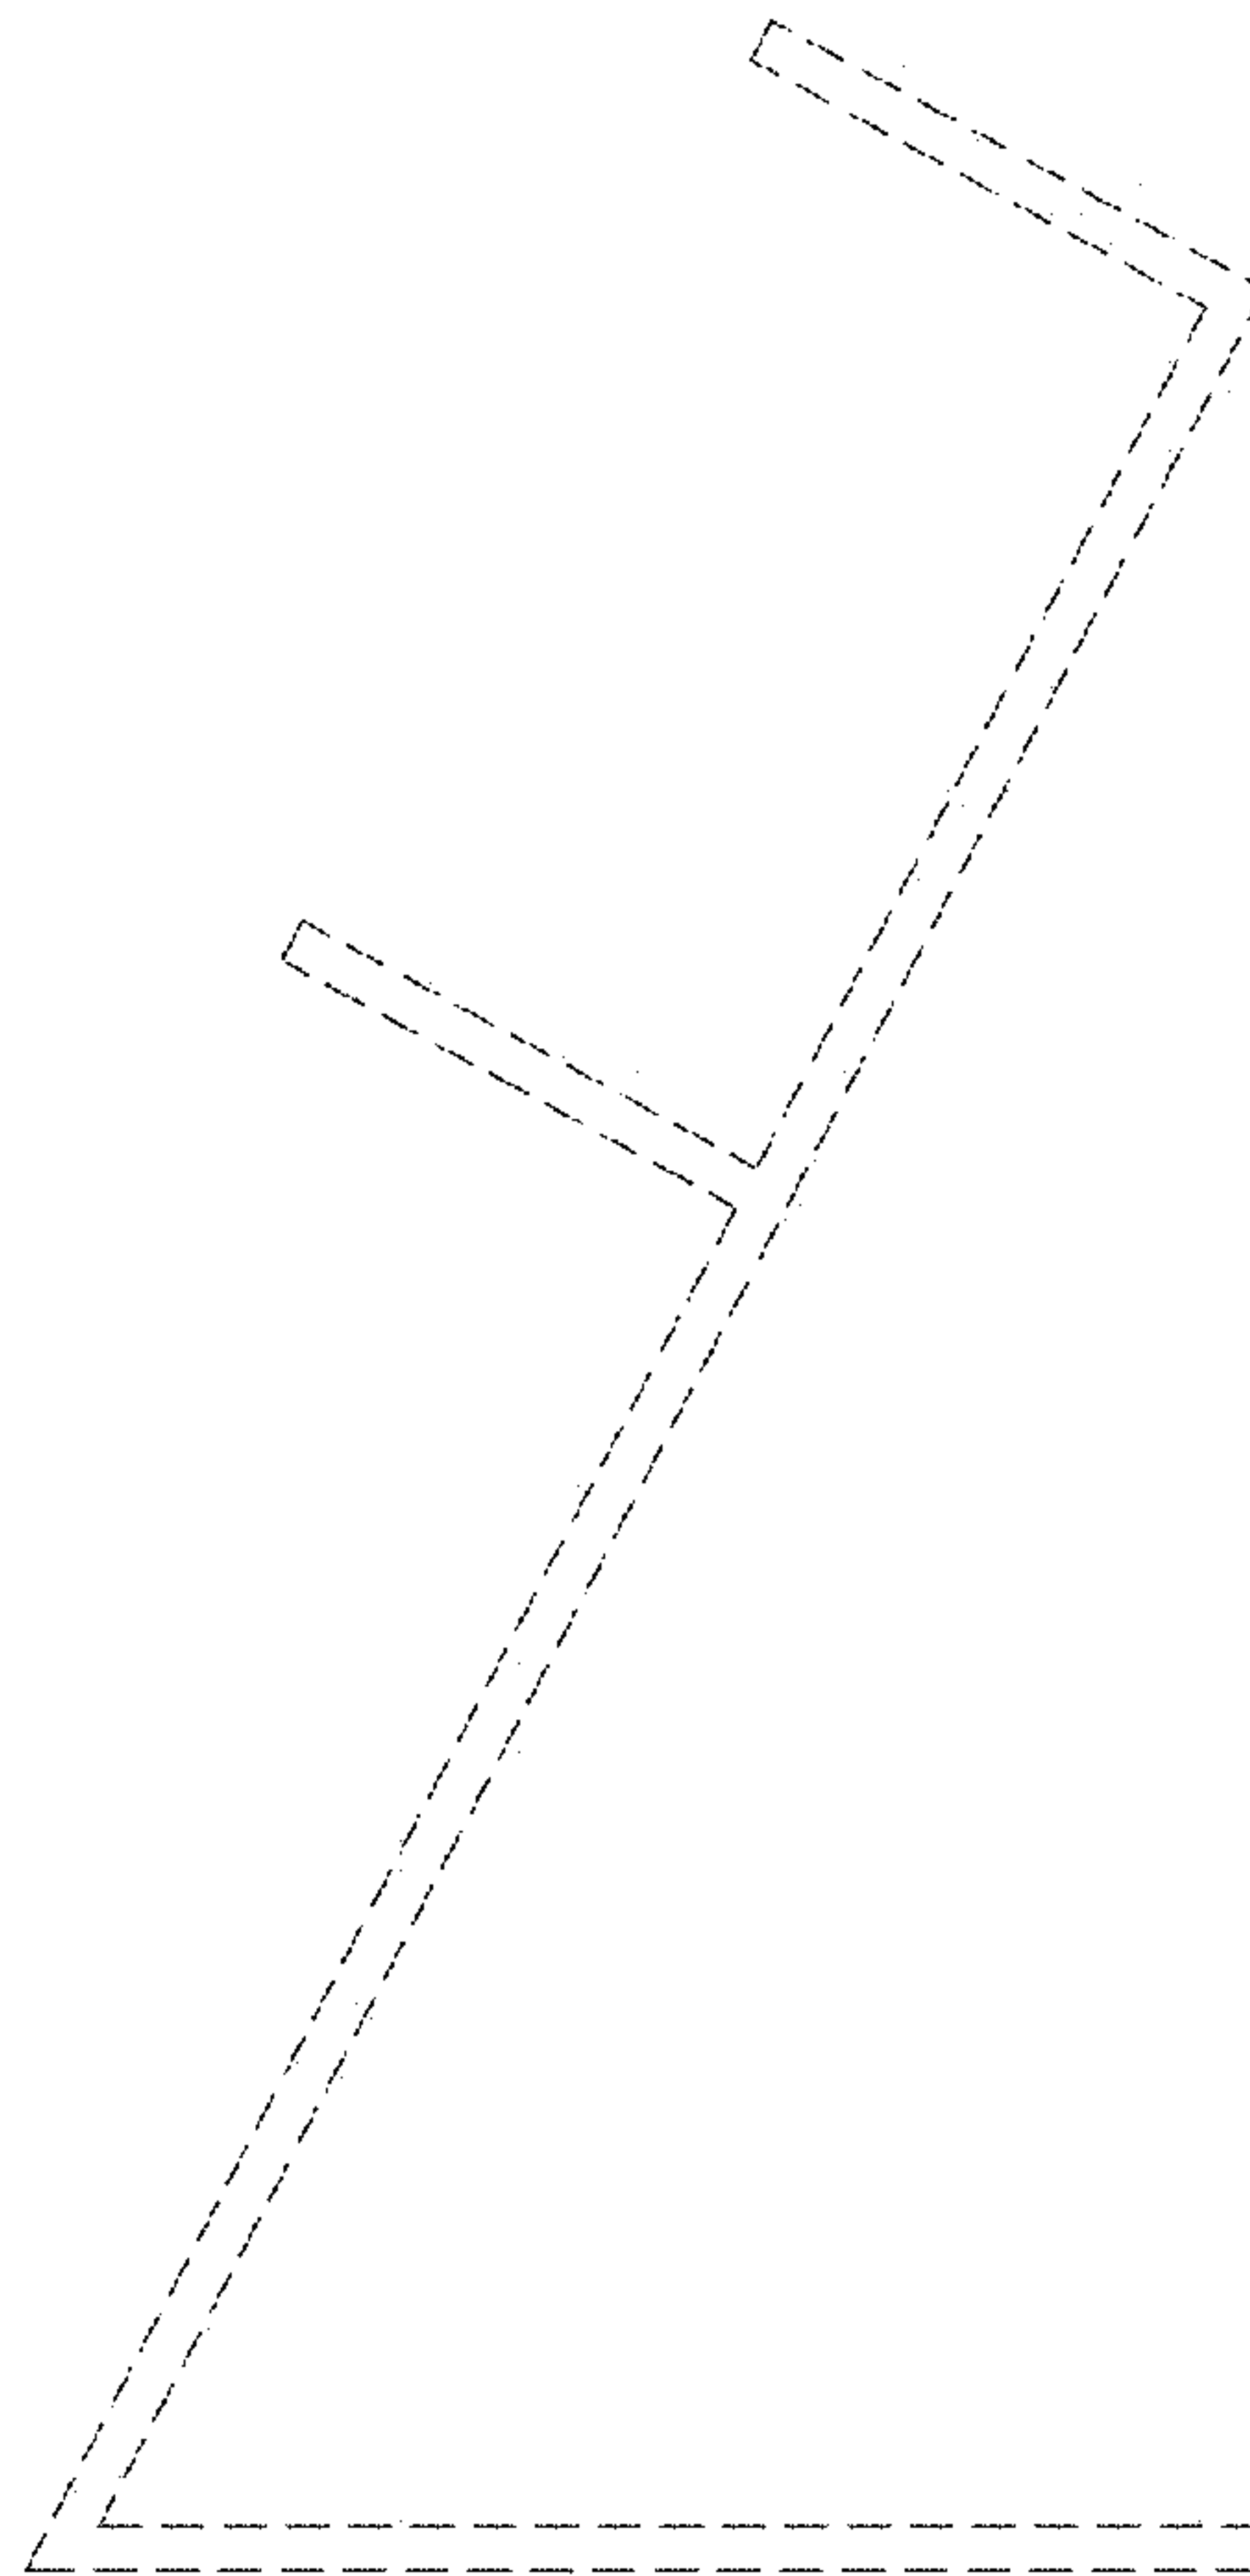


FIG. 6

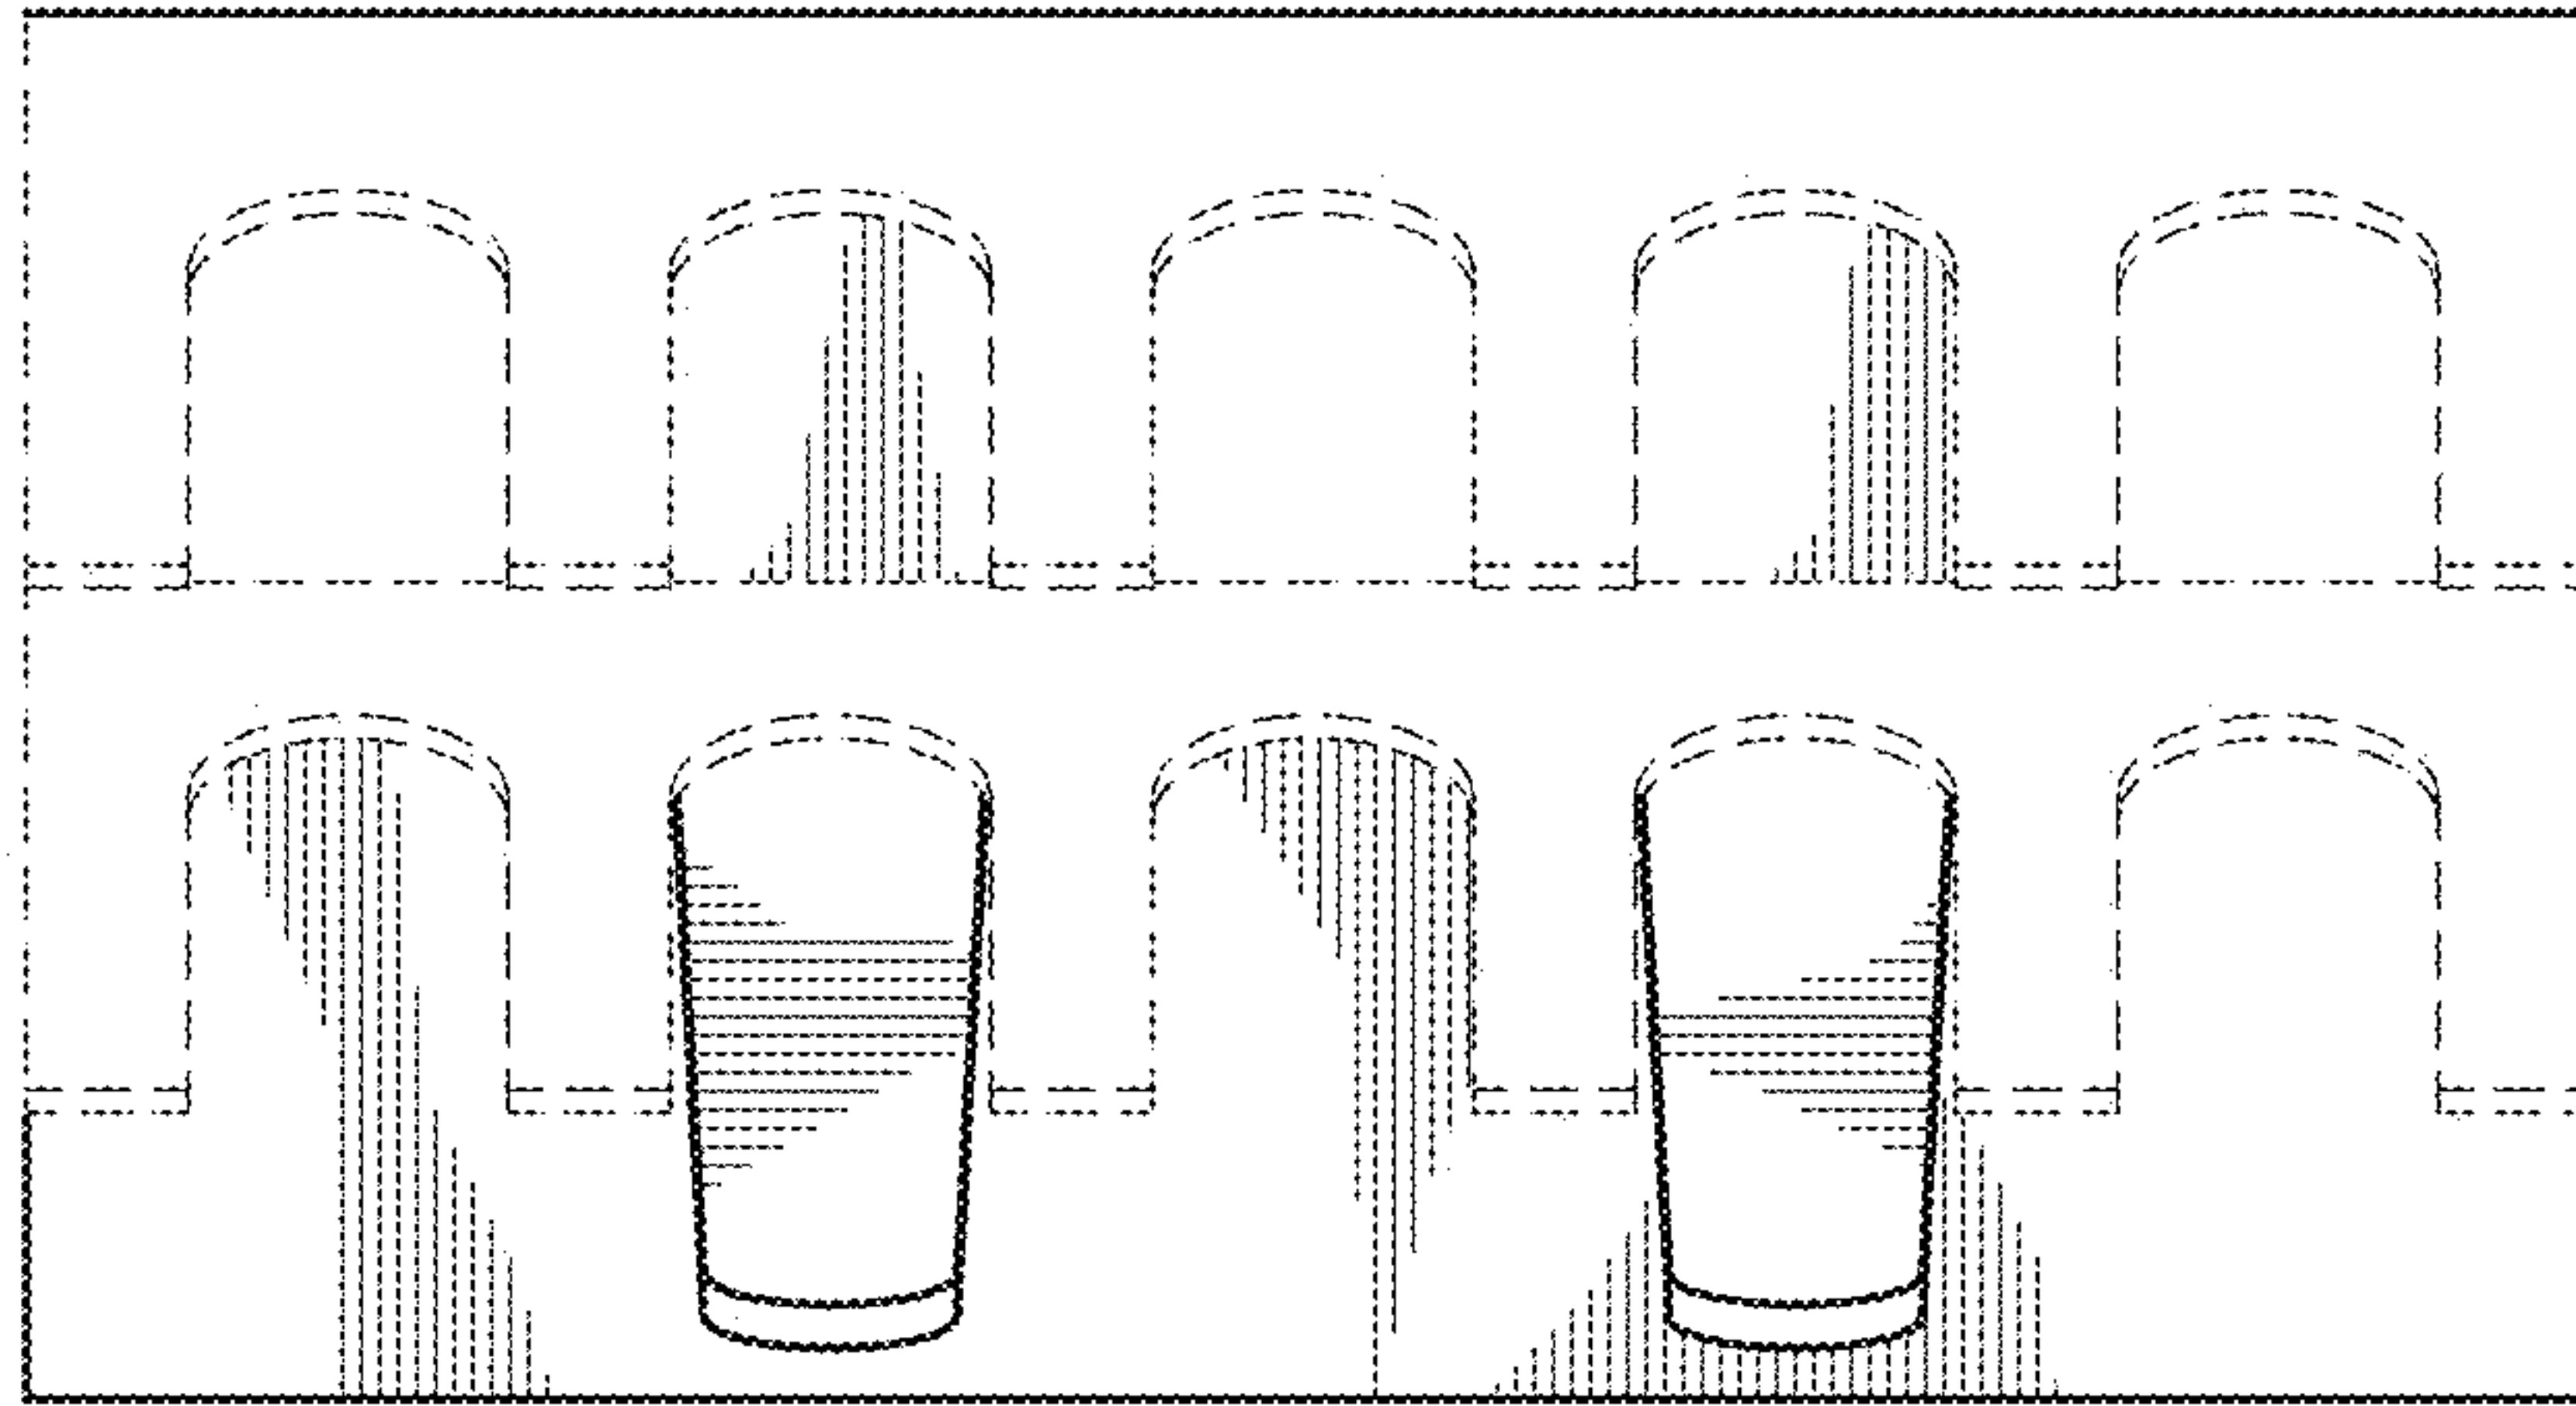


FIG. 7

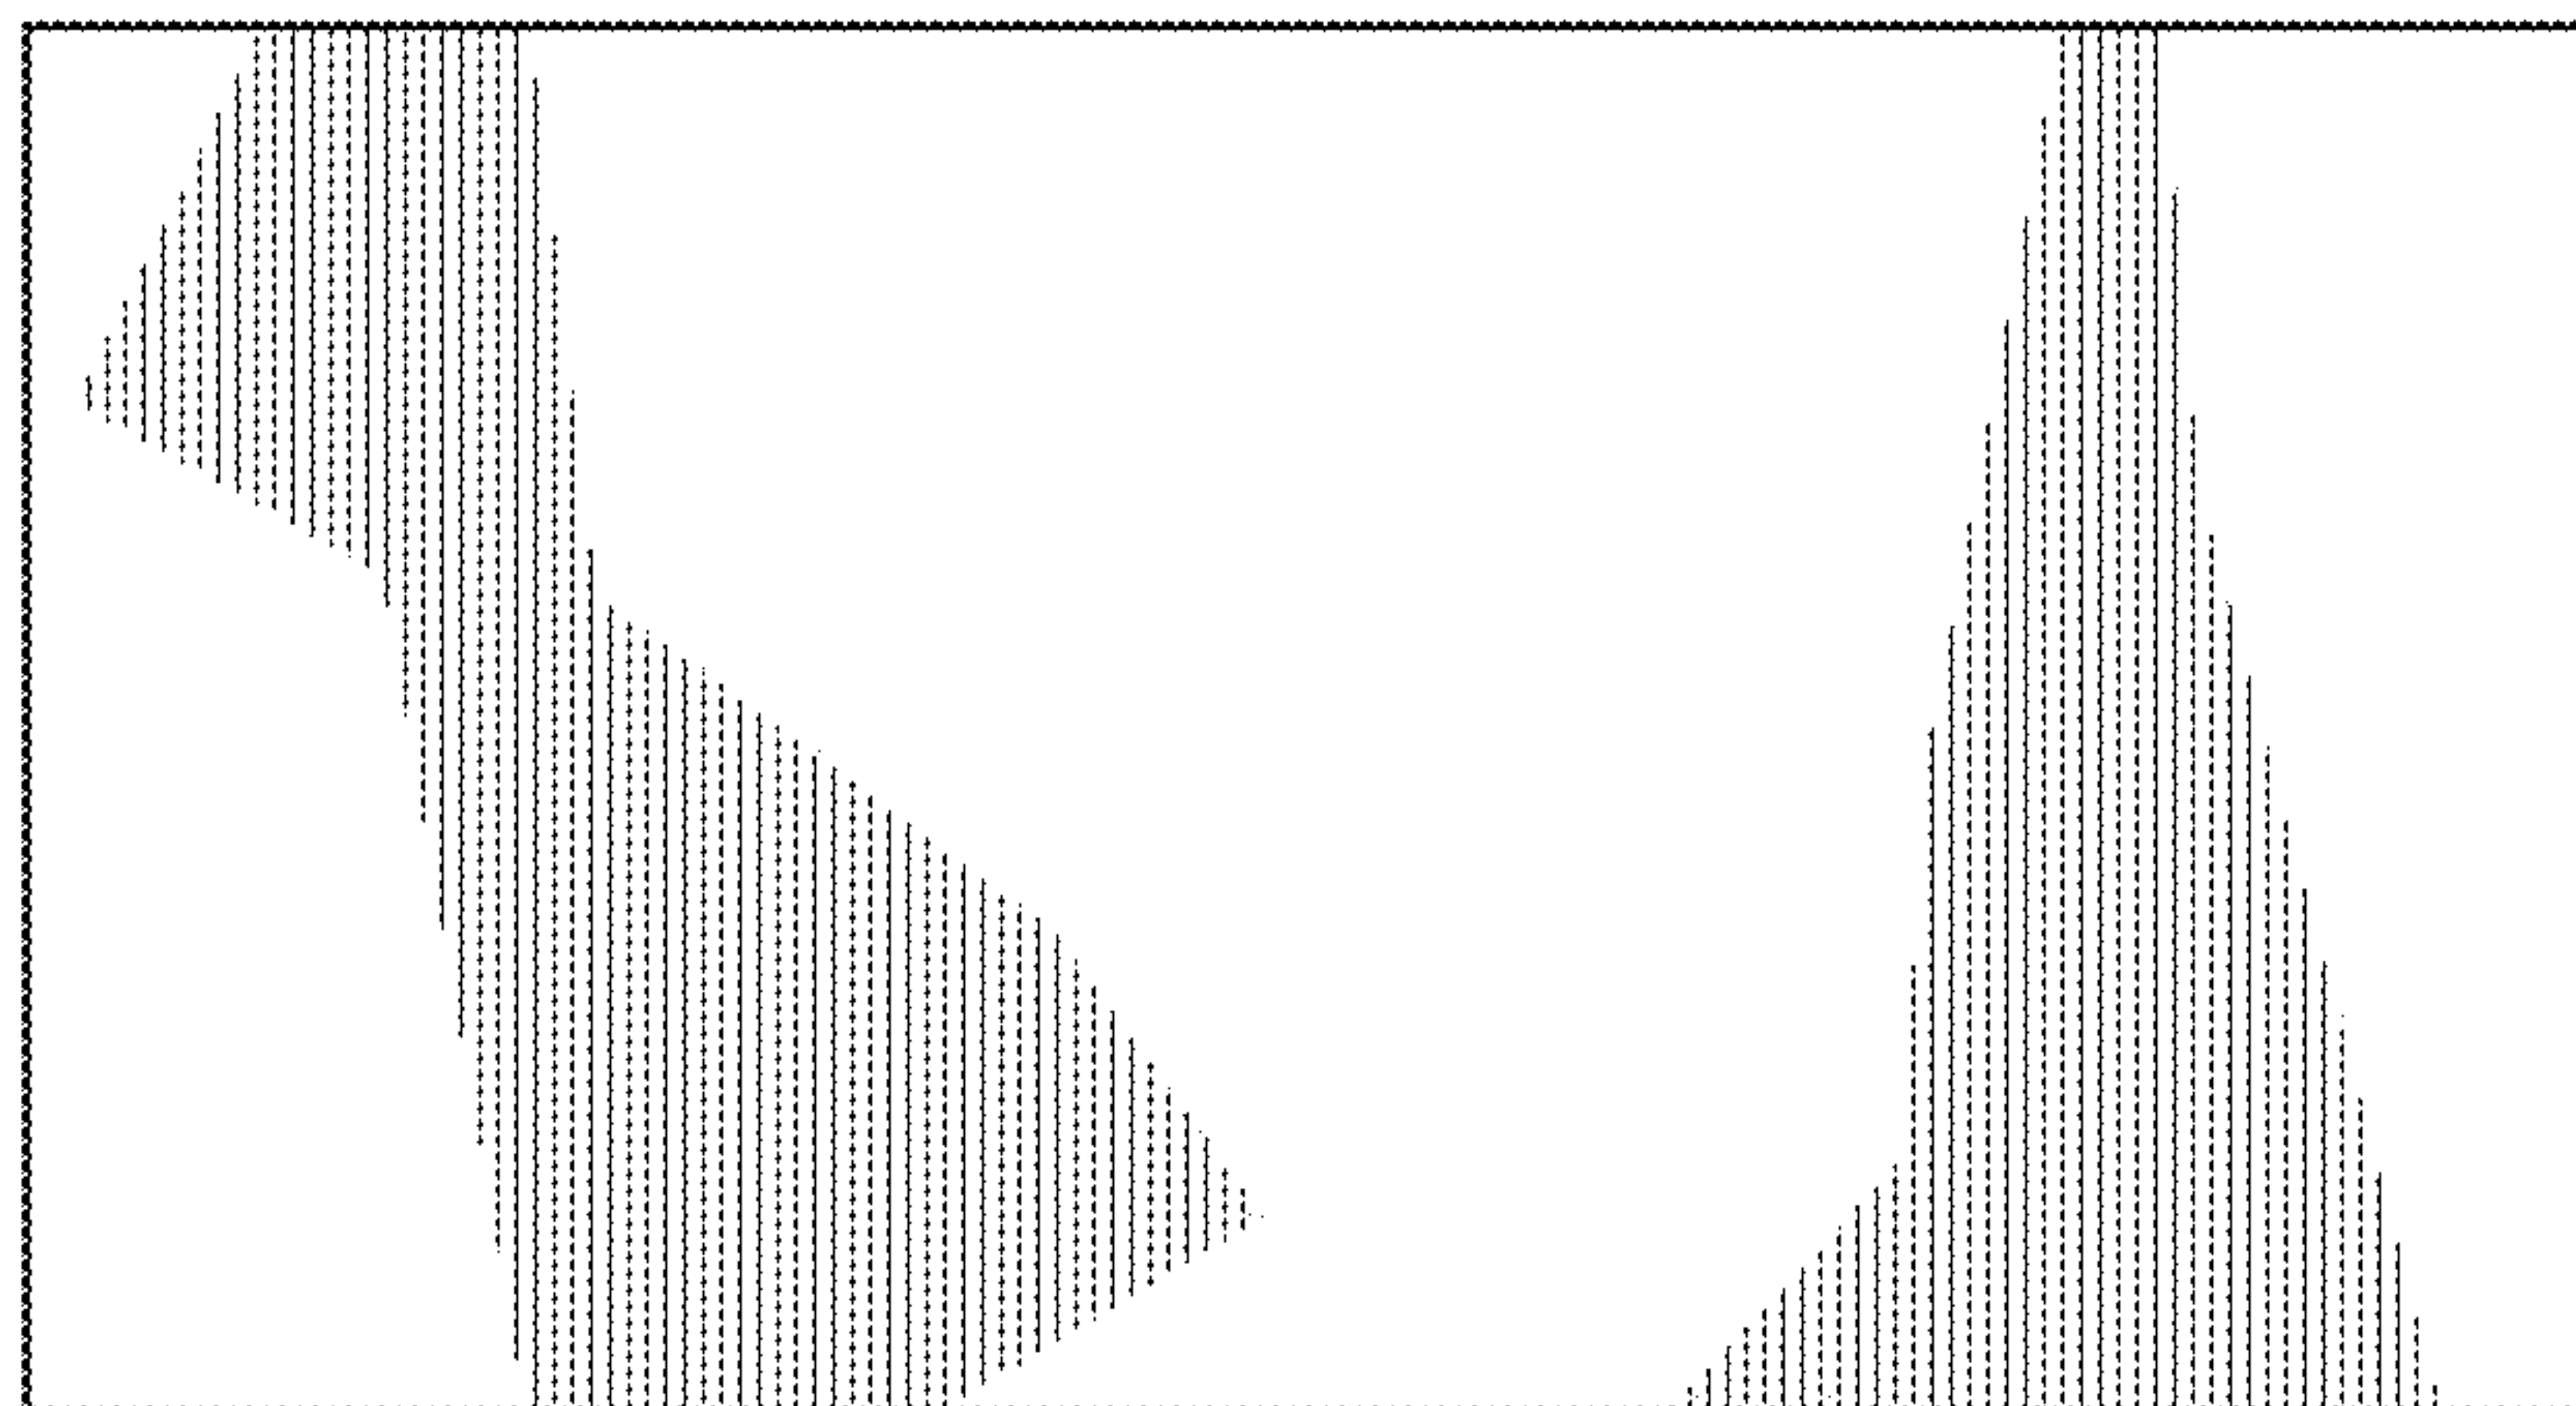


FIG. 8

FIG. 9

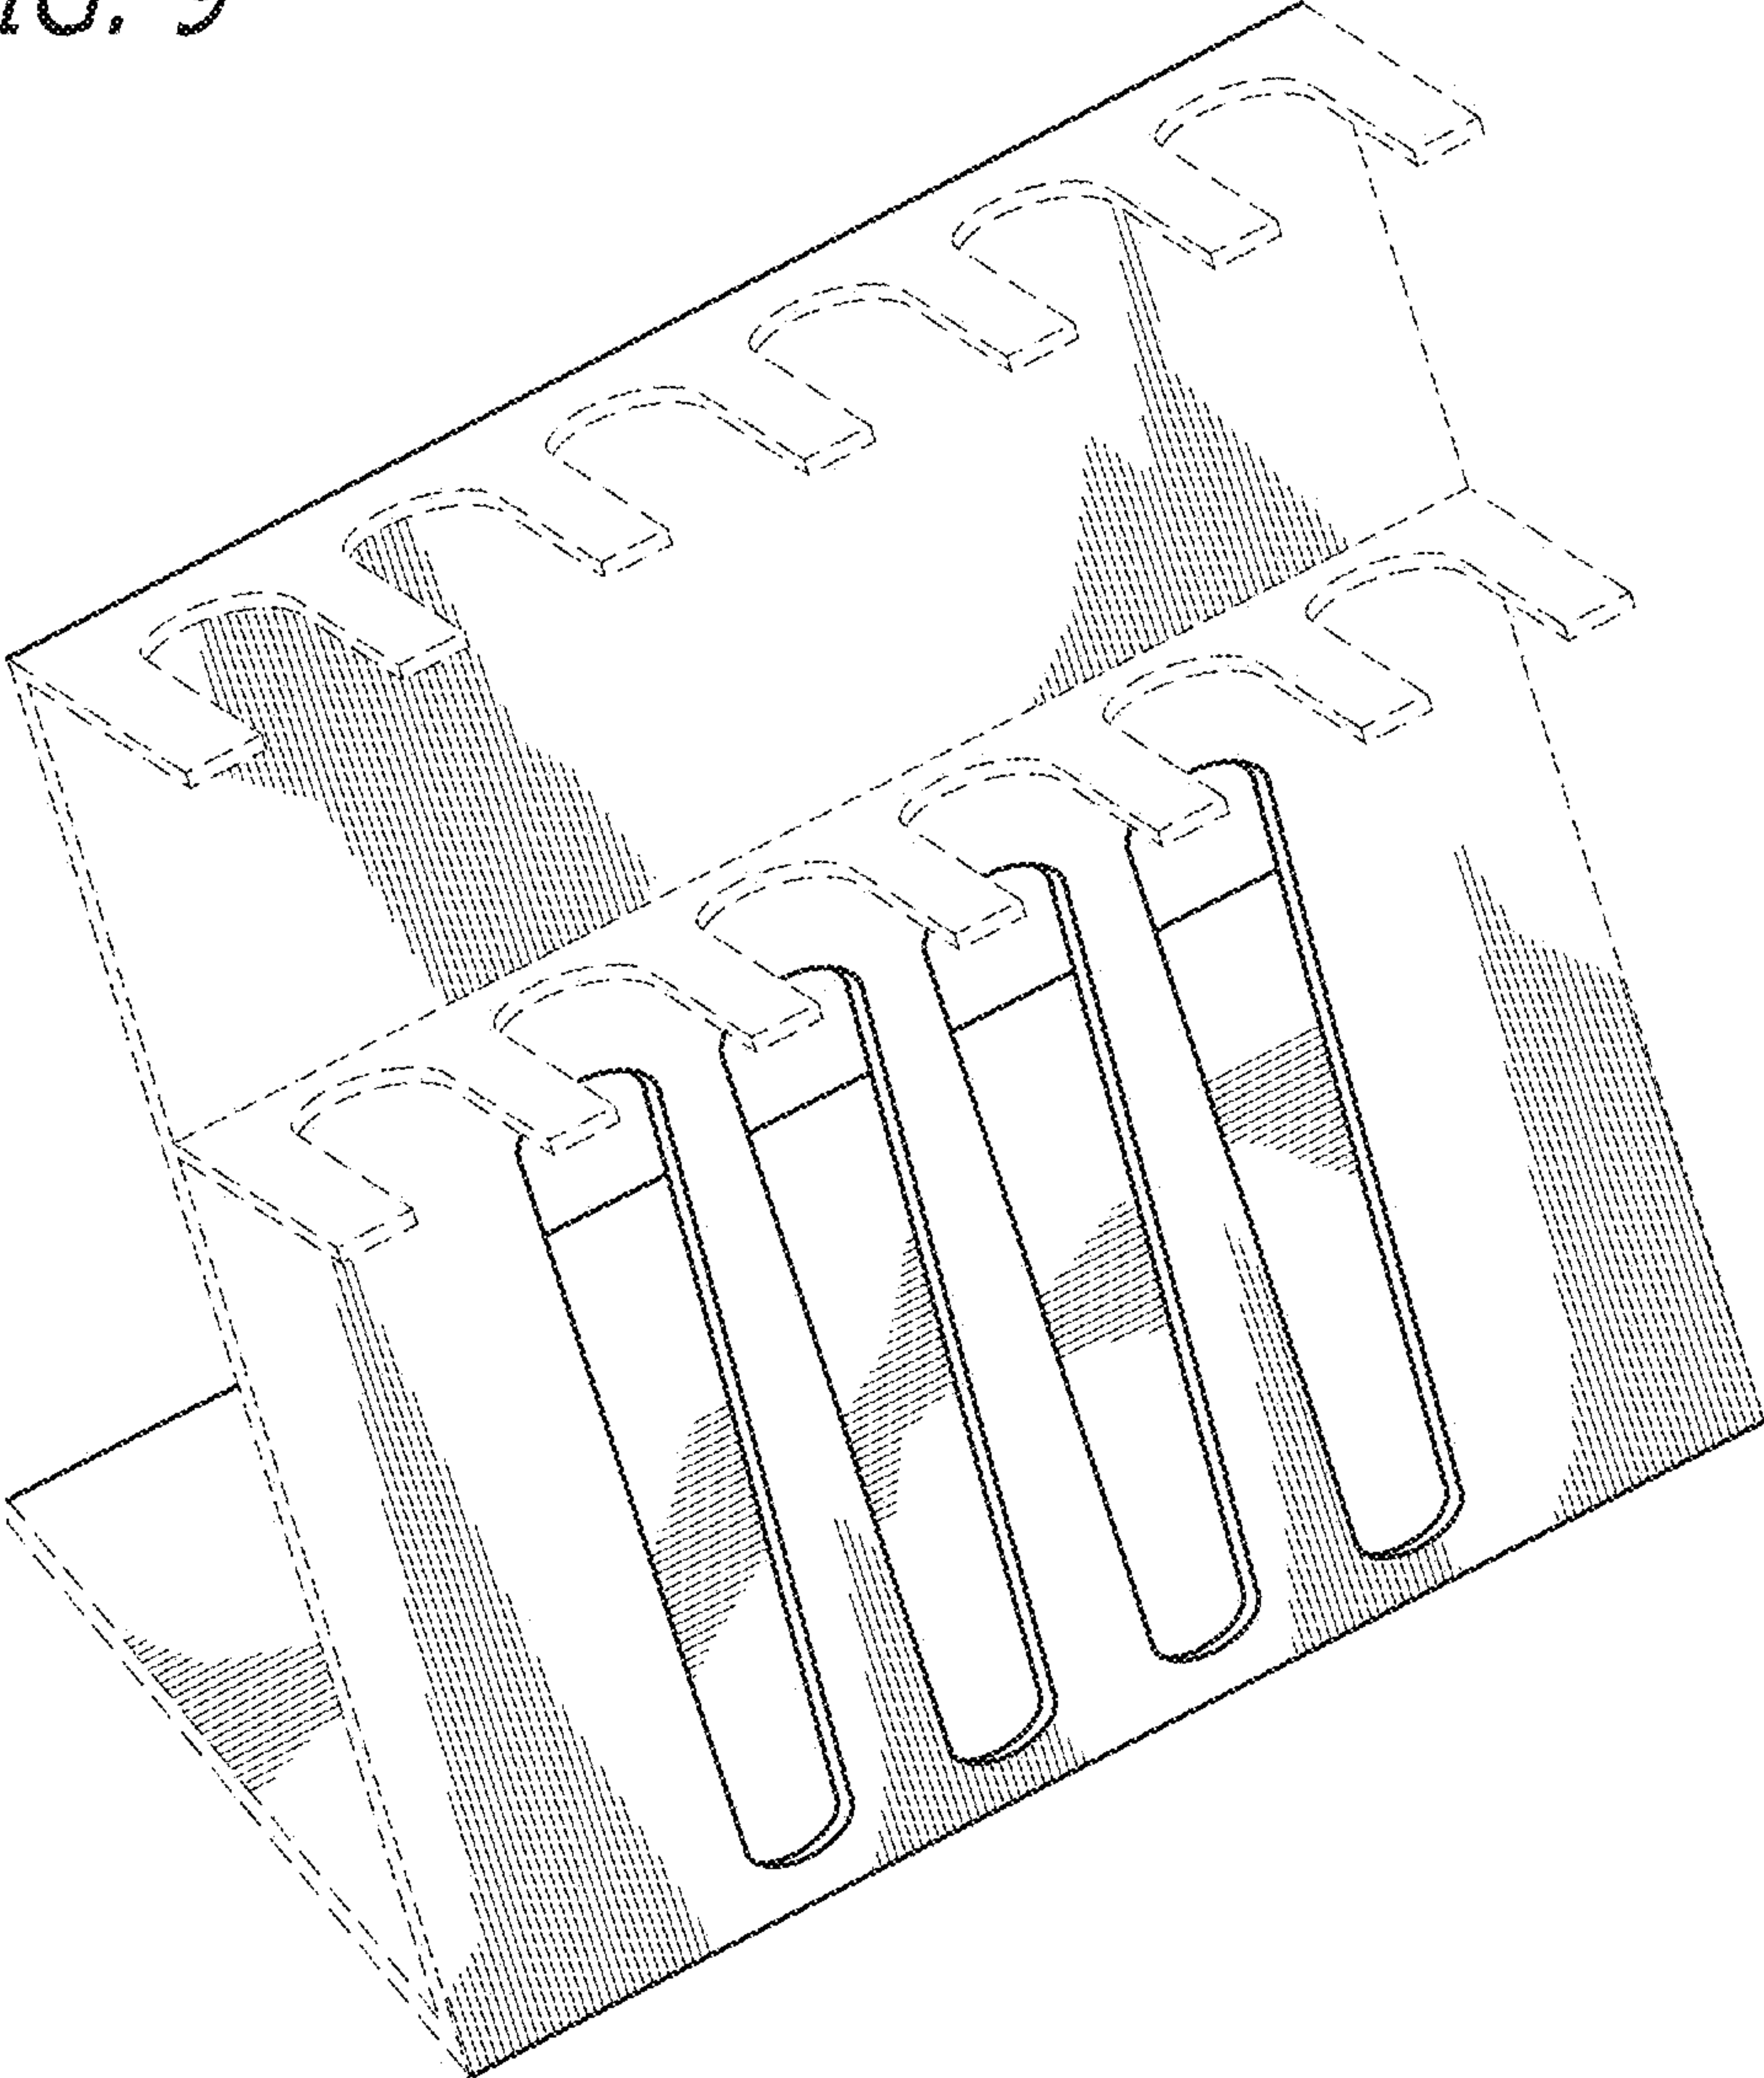
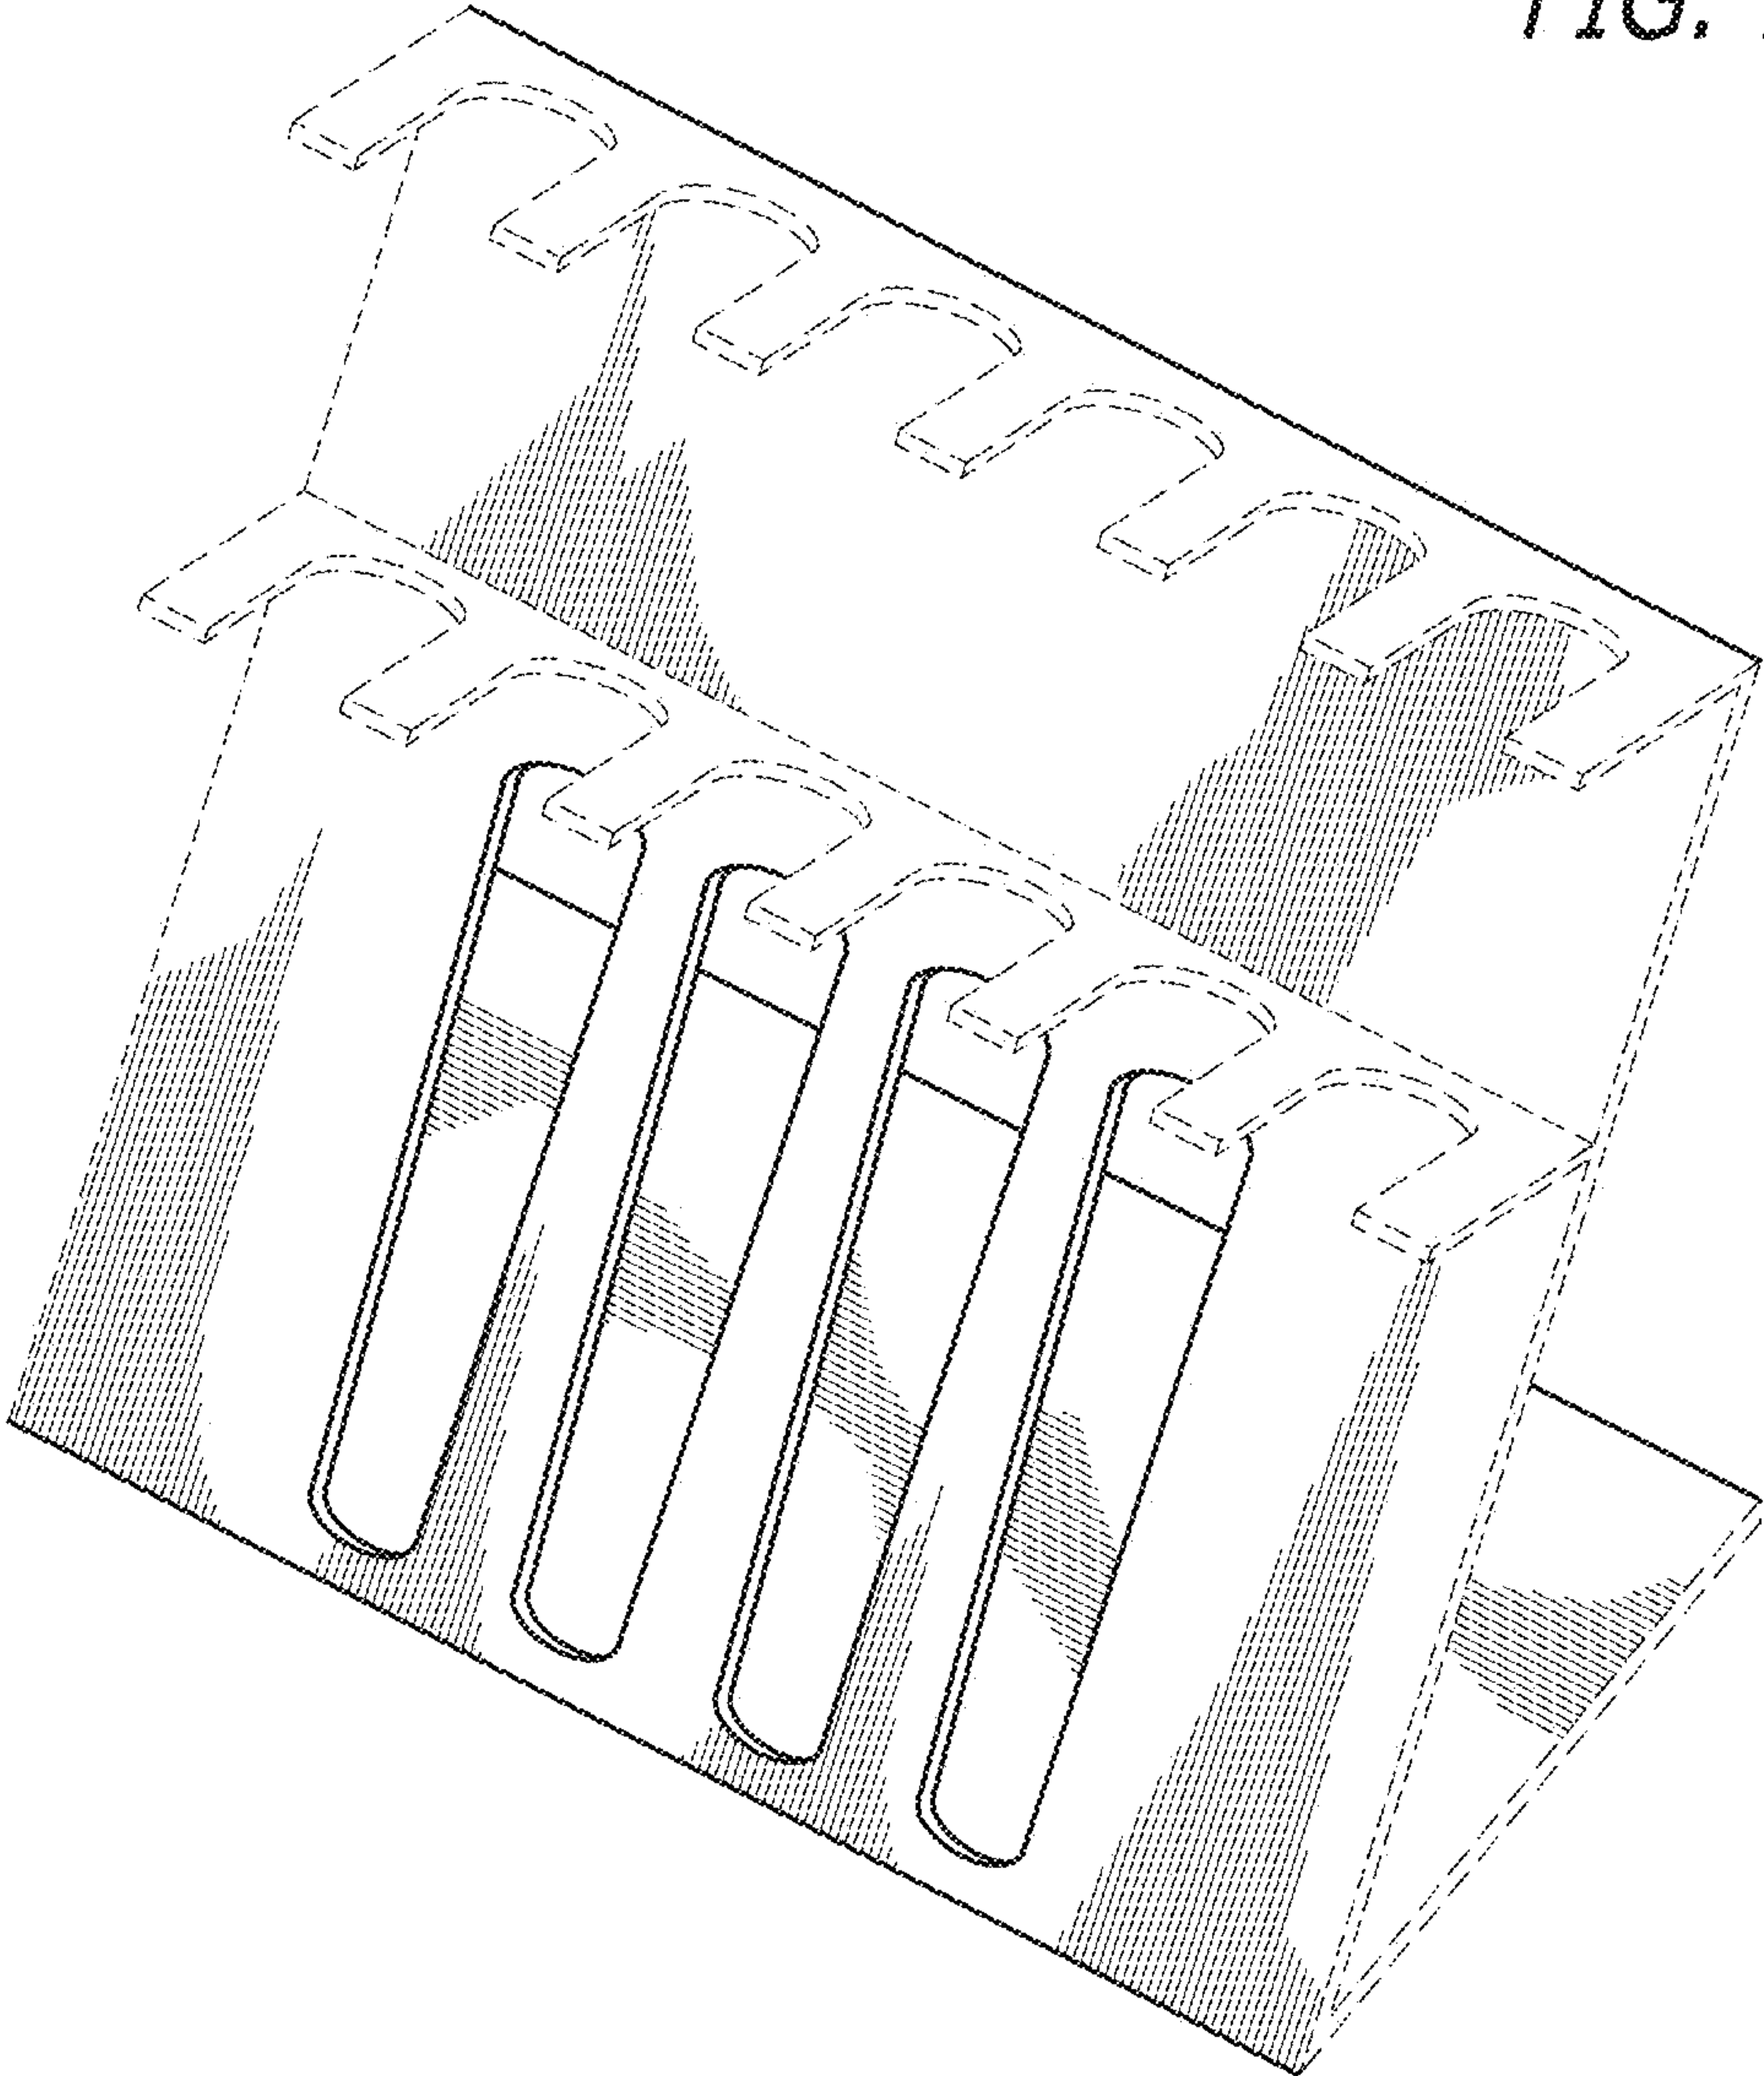


FIG. 10



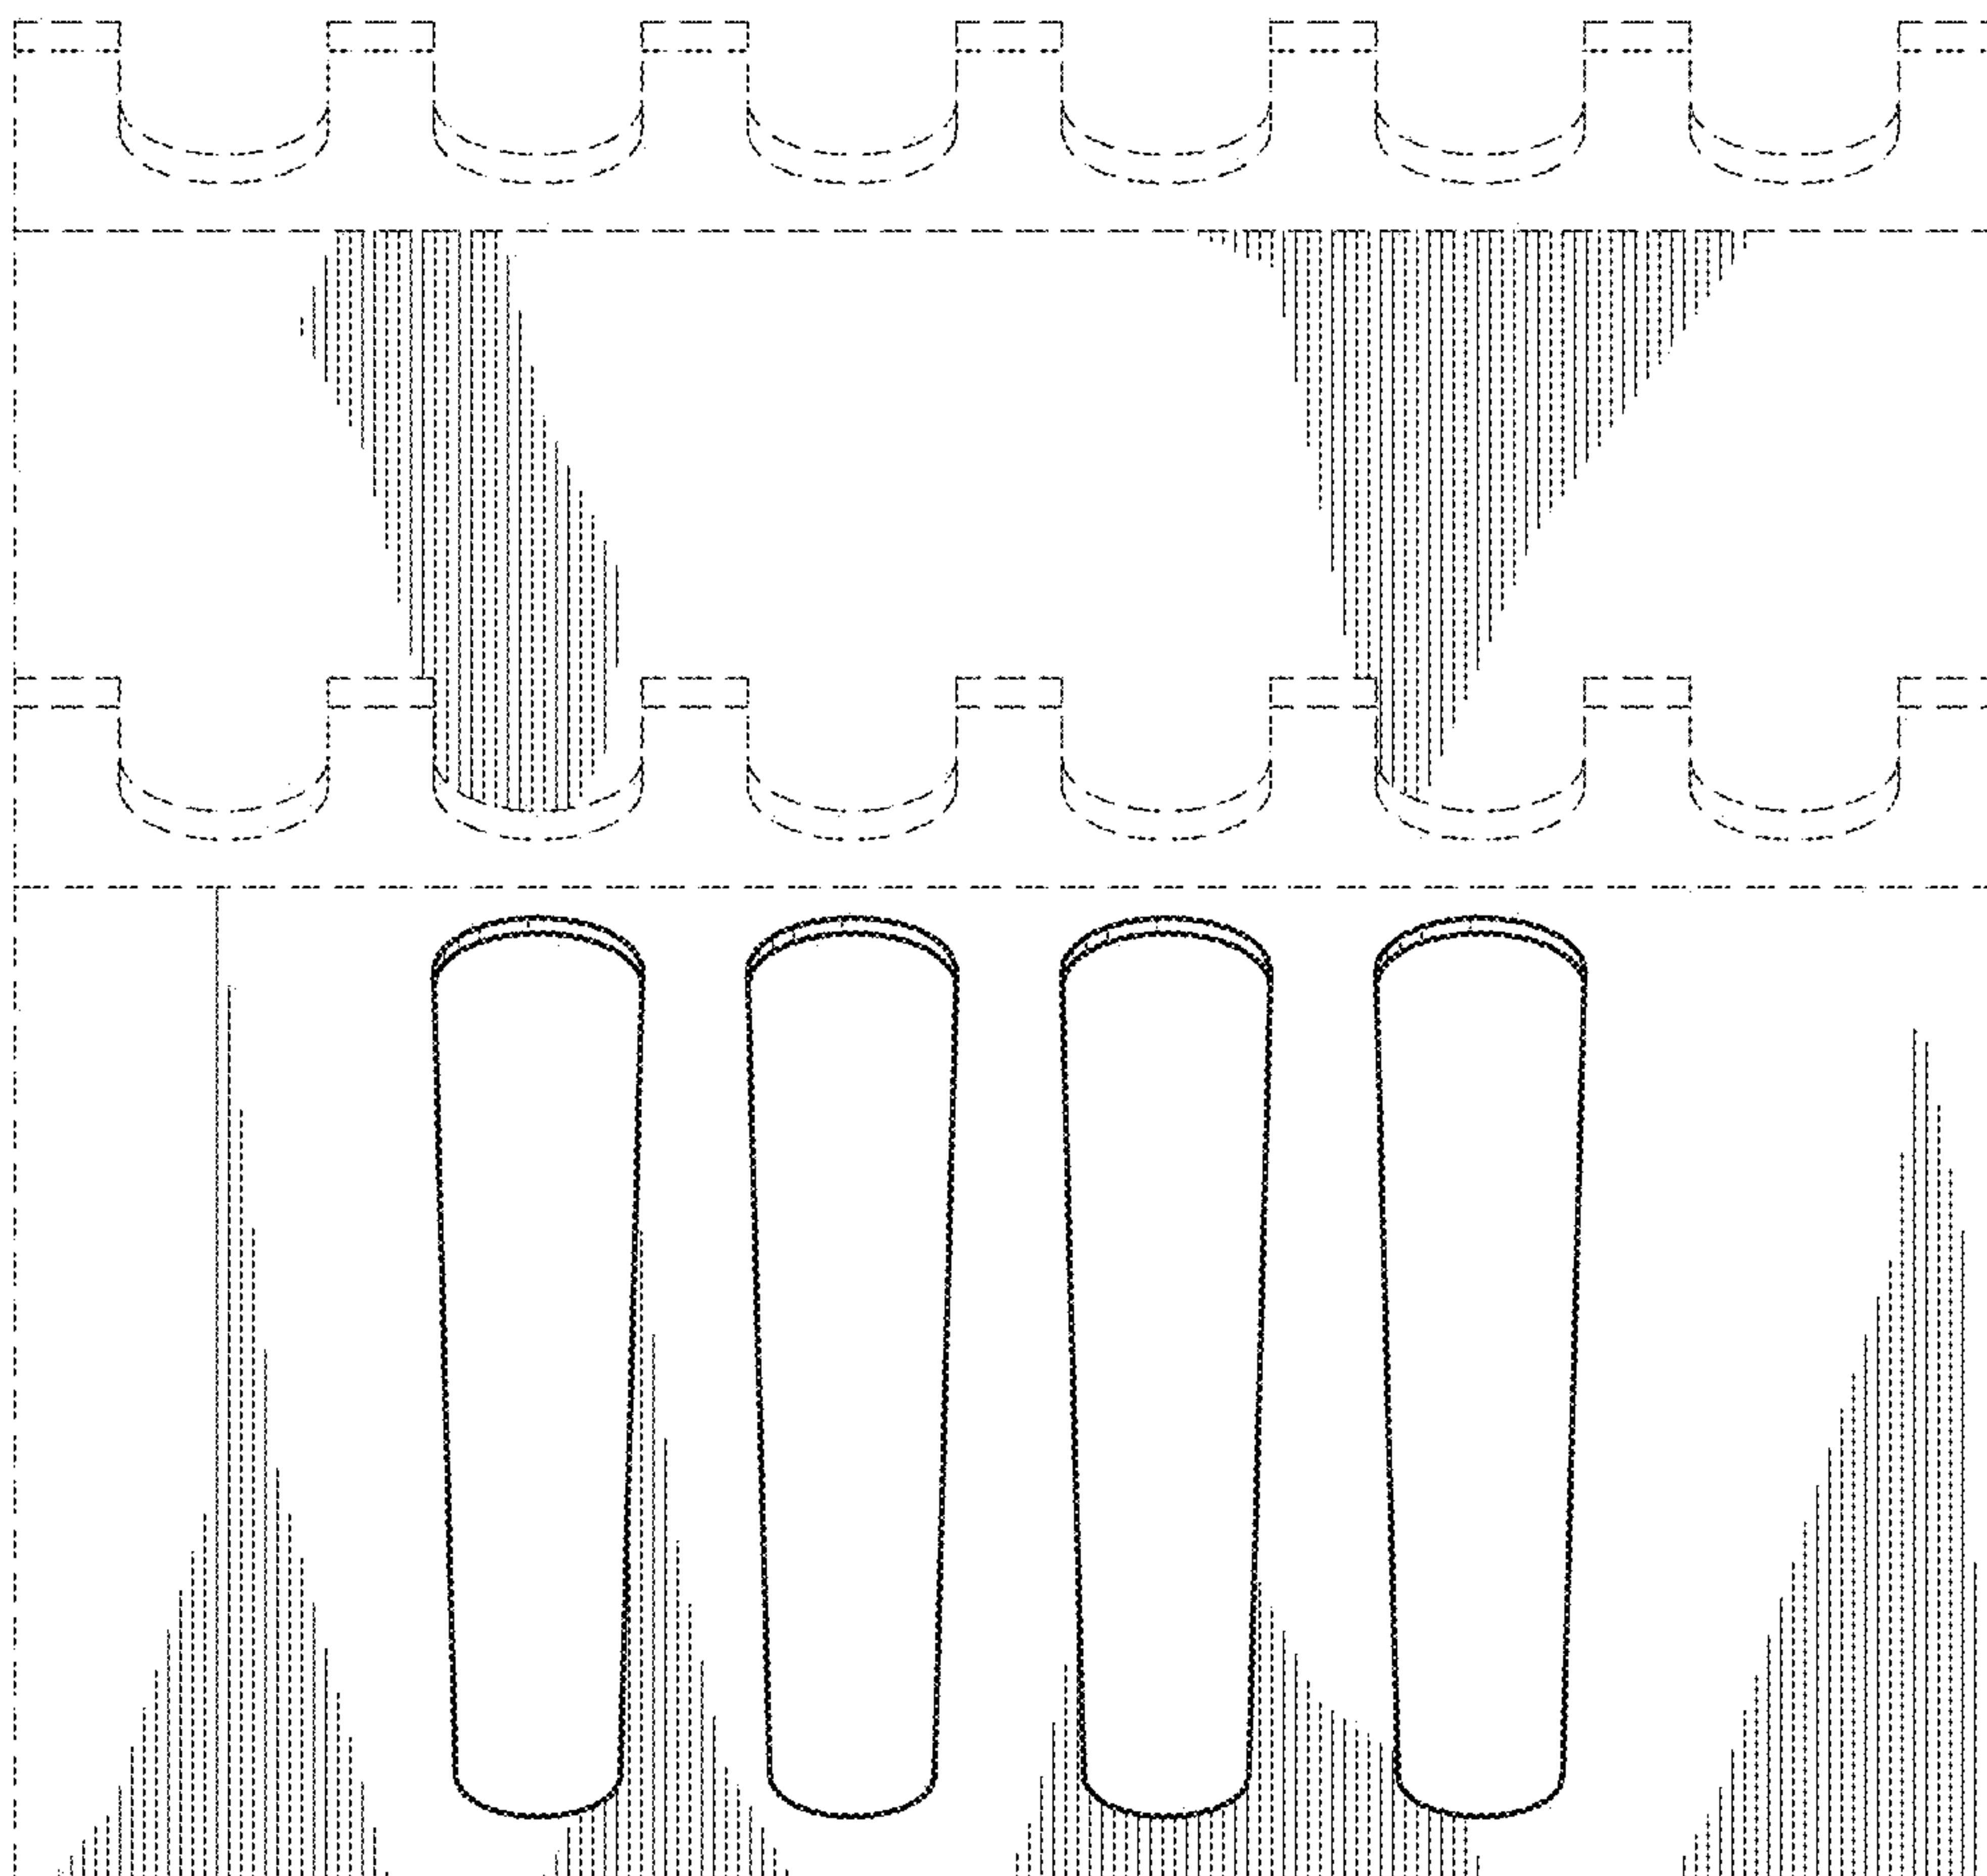


FIG. 11

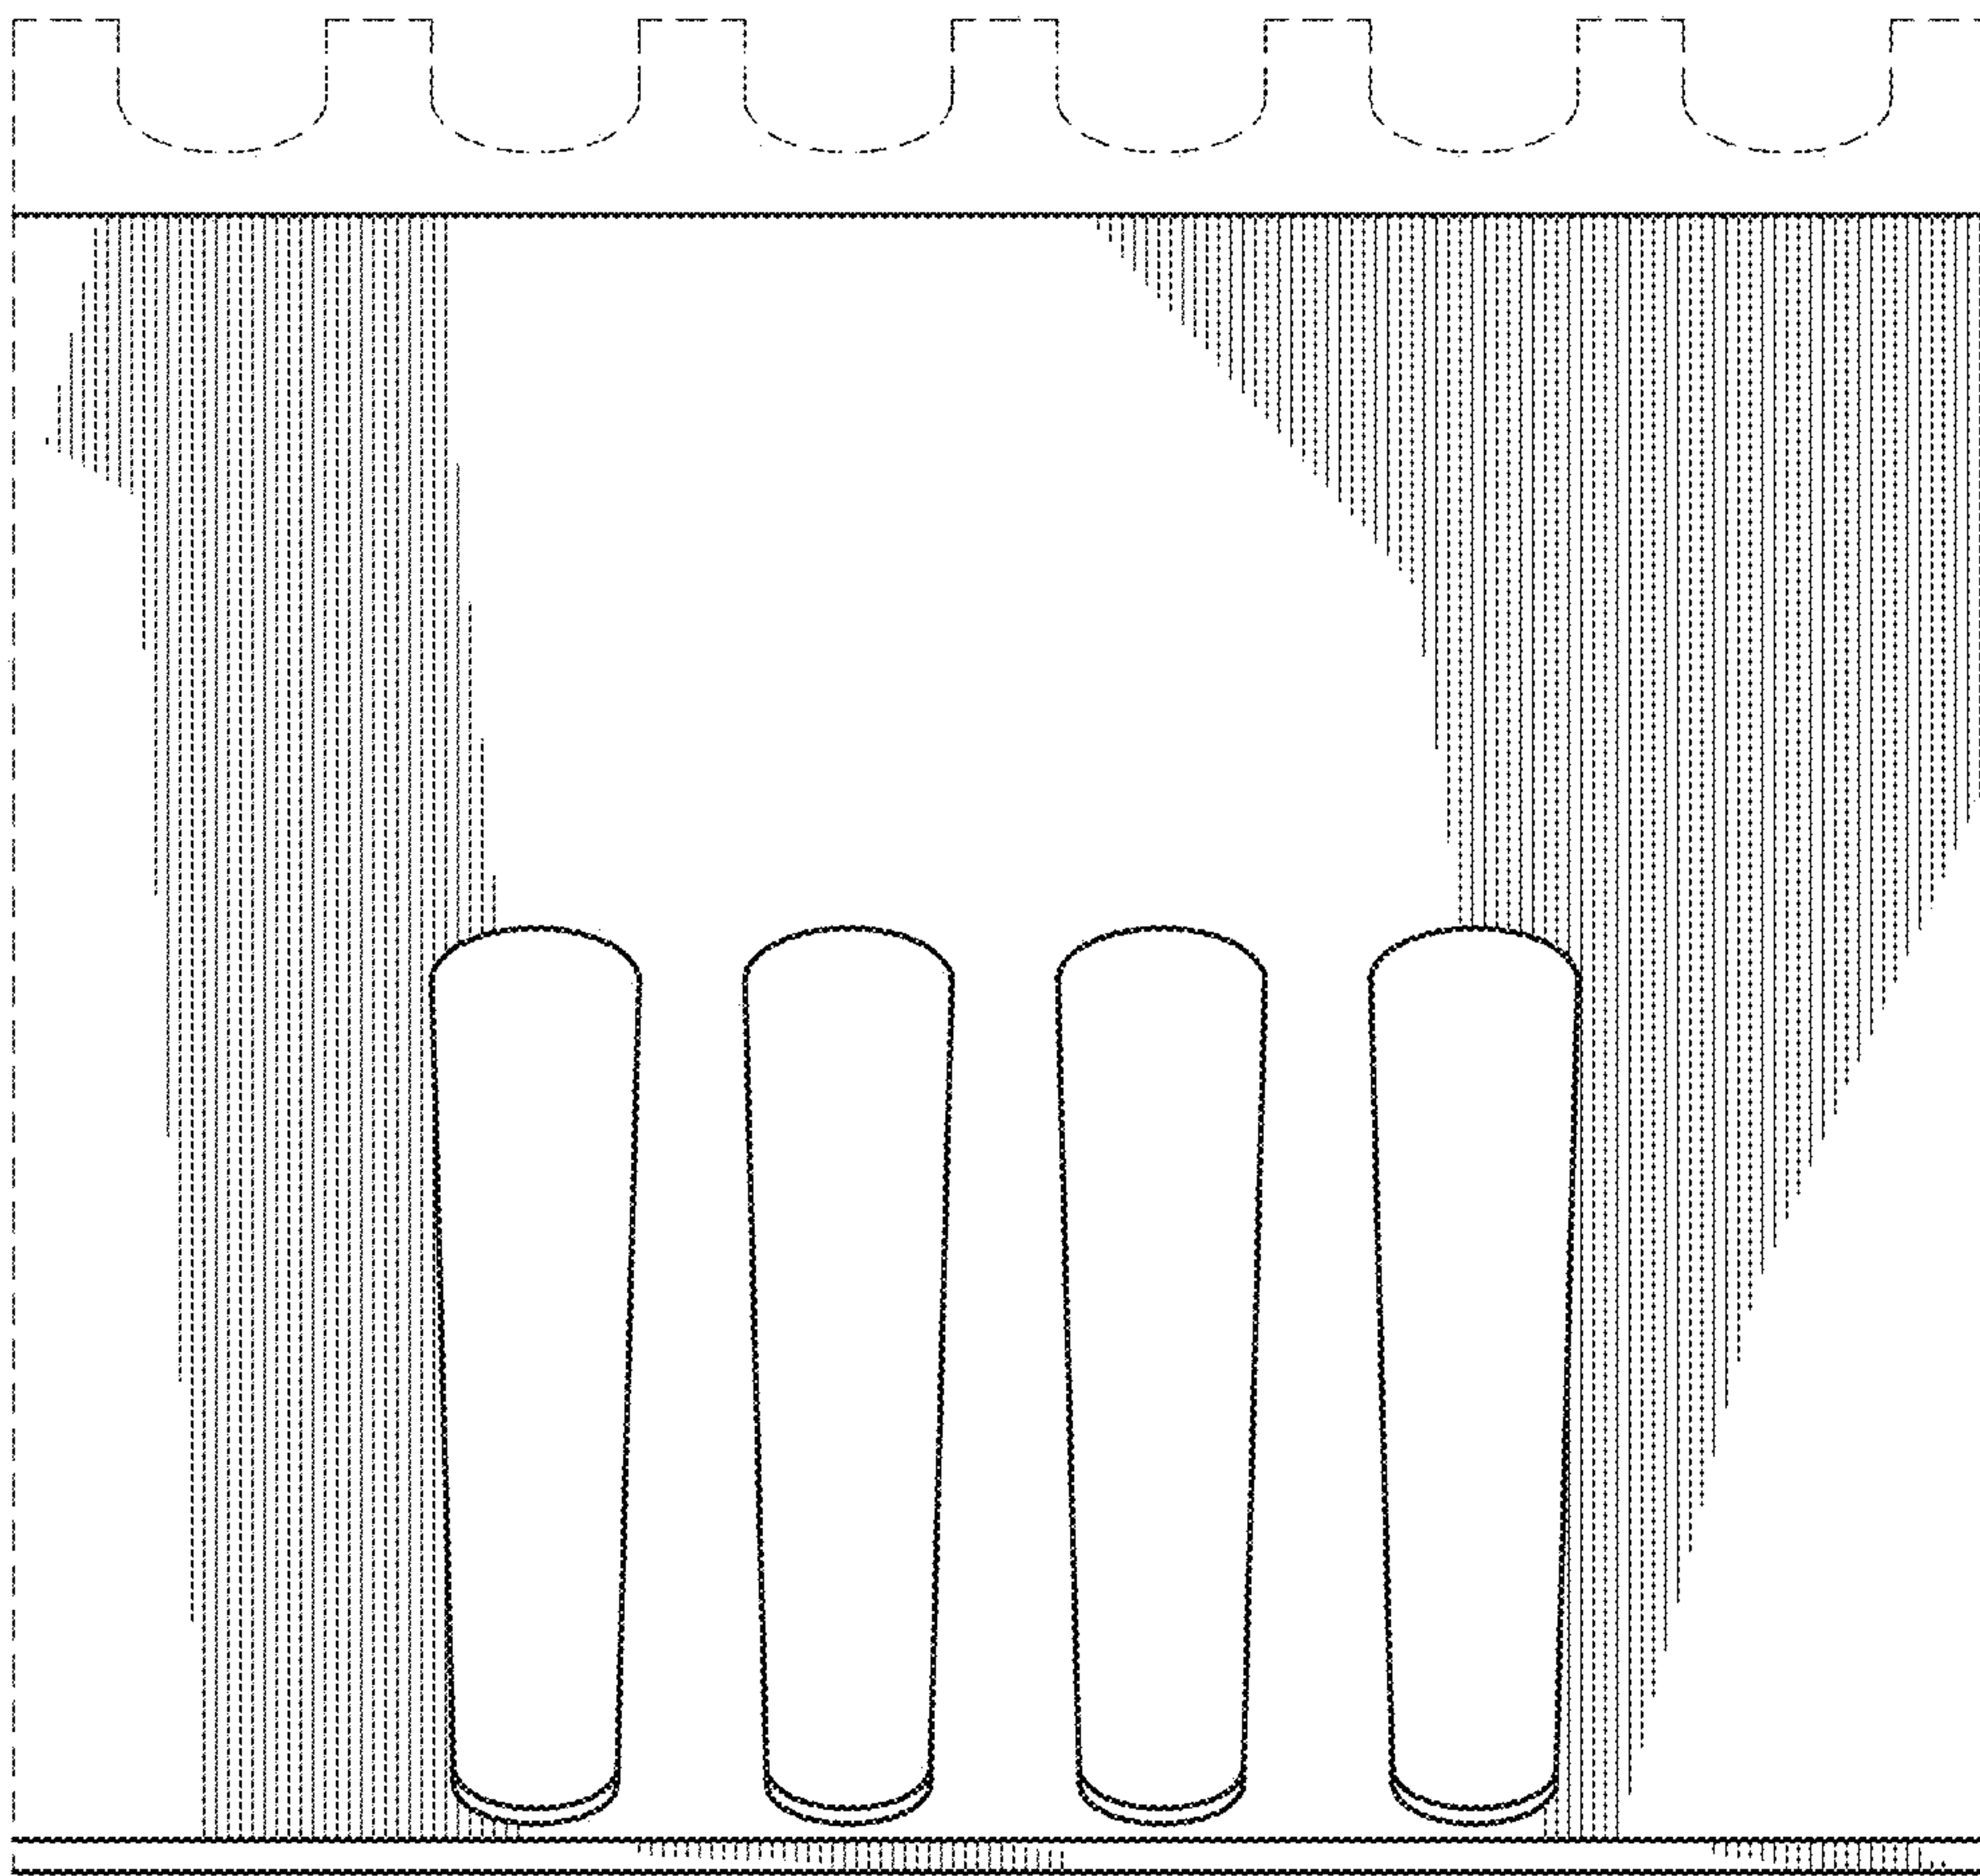


FIG. 12

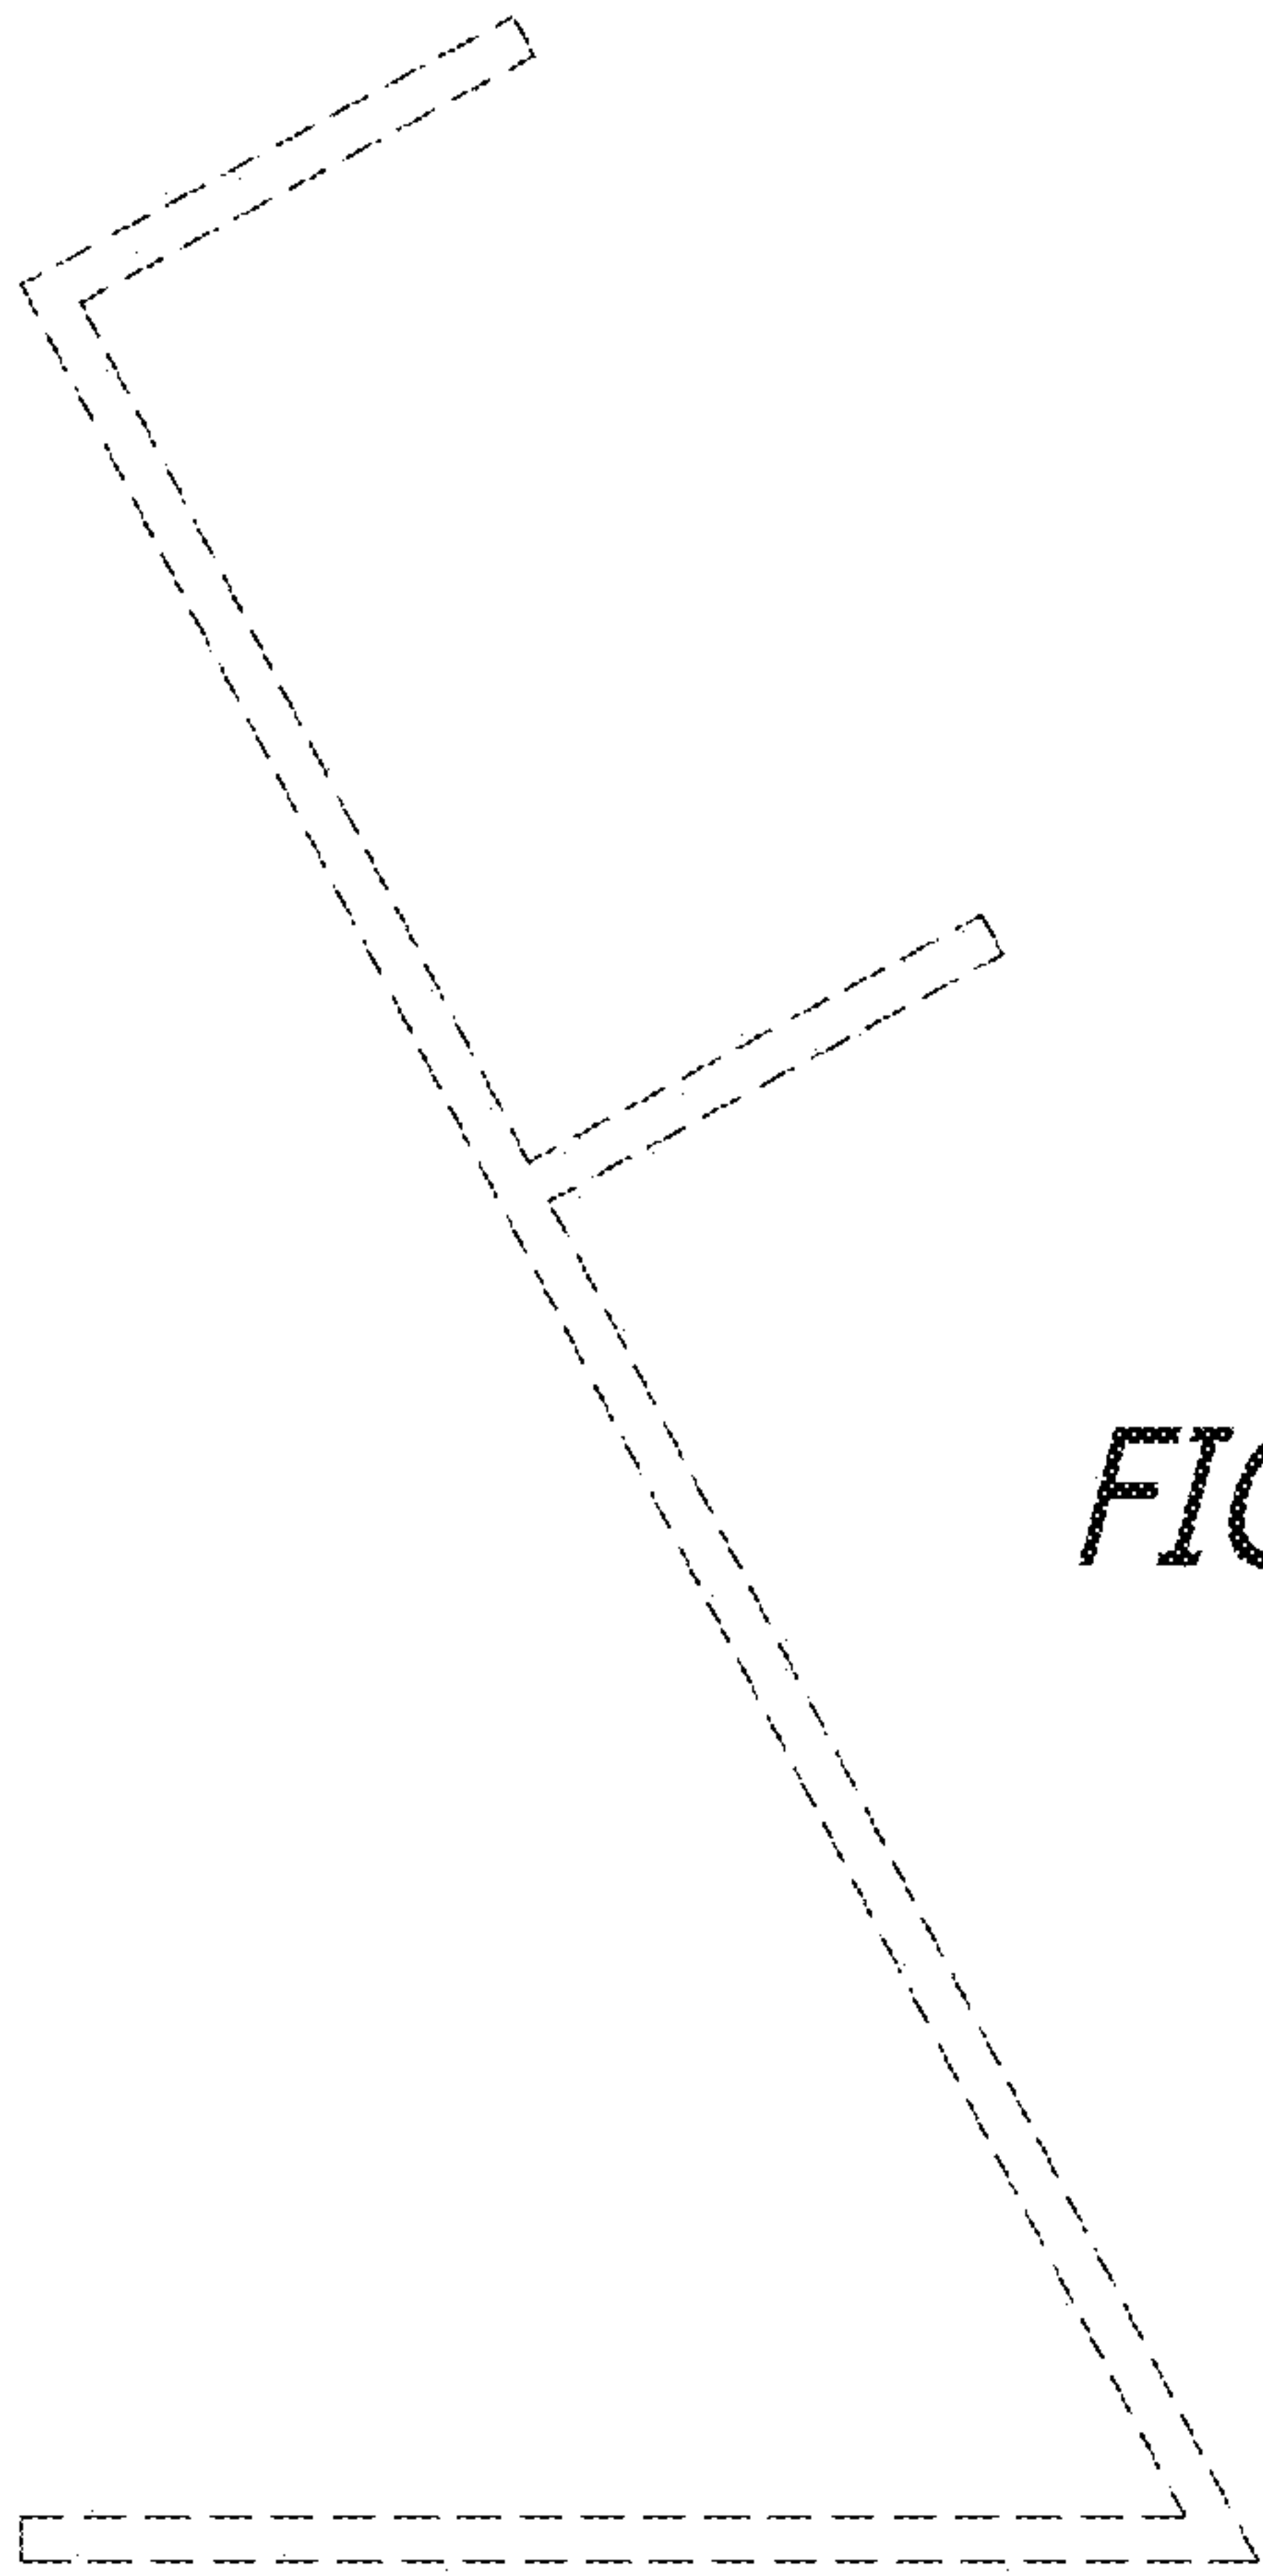


FIG. 13

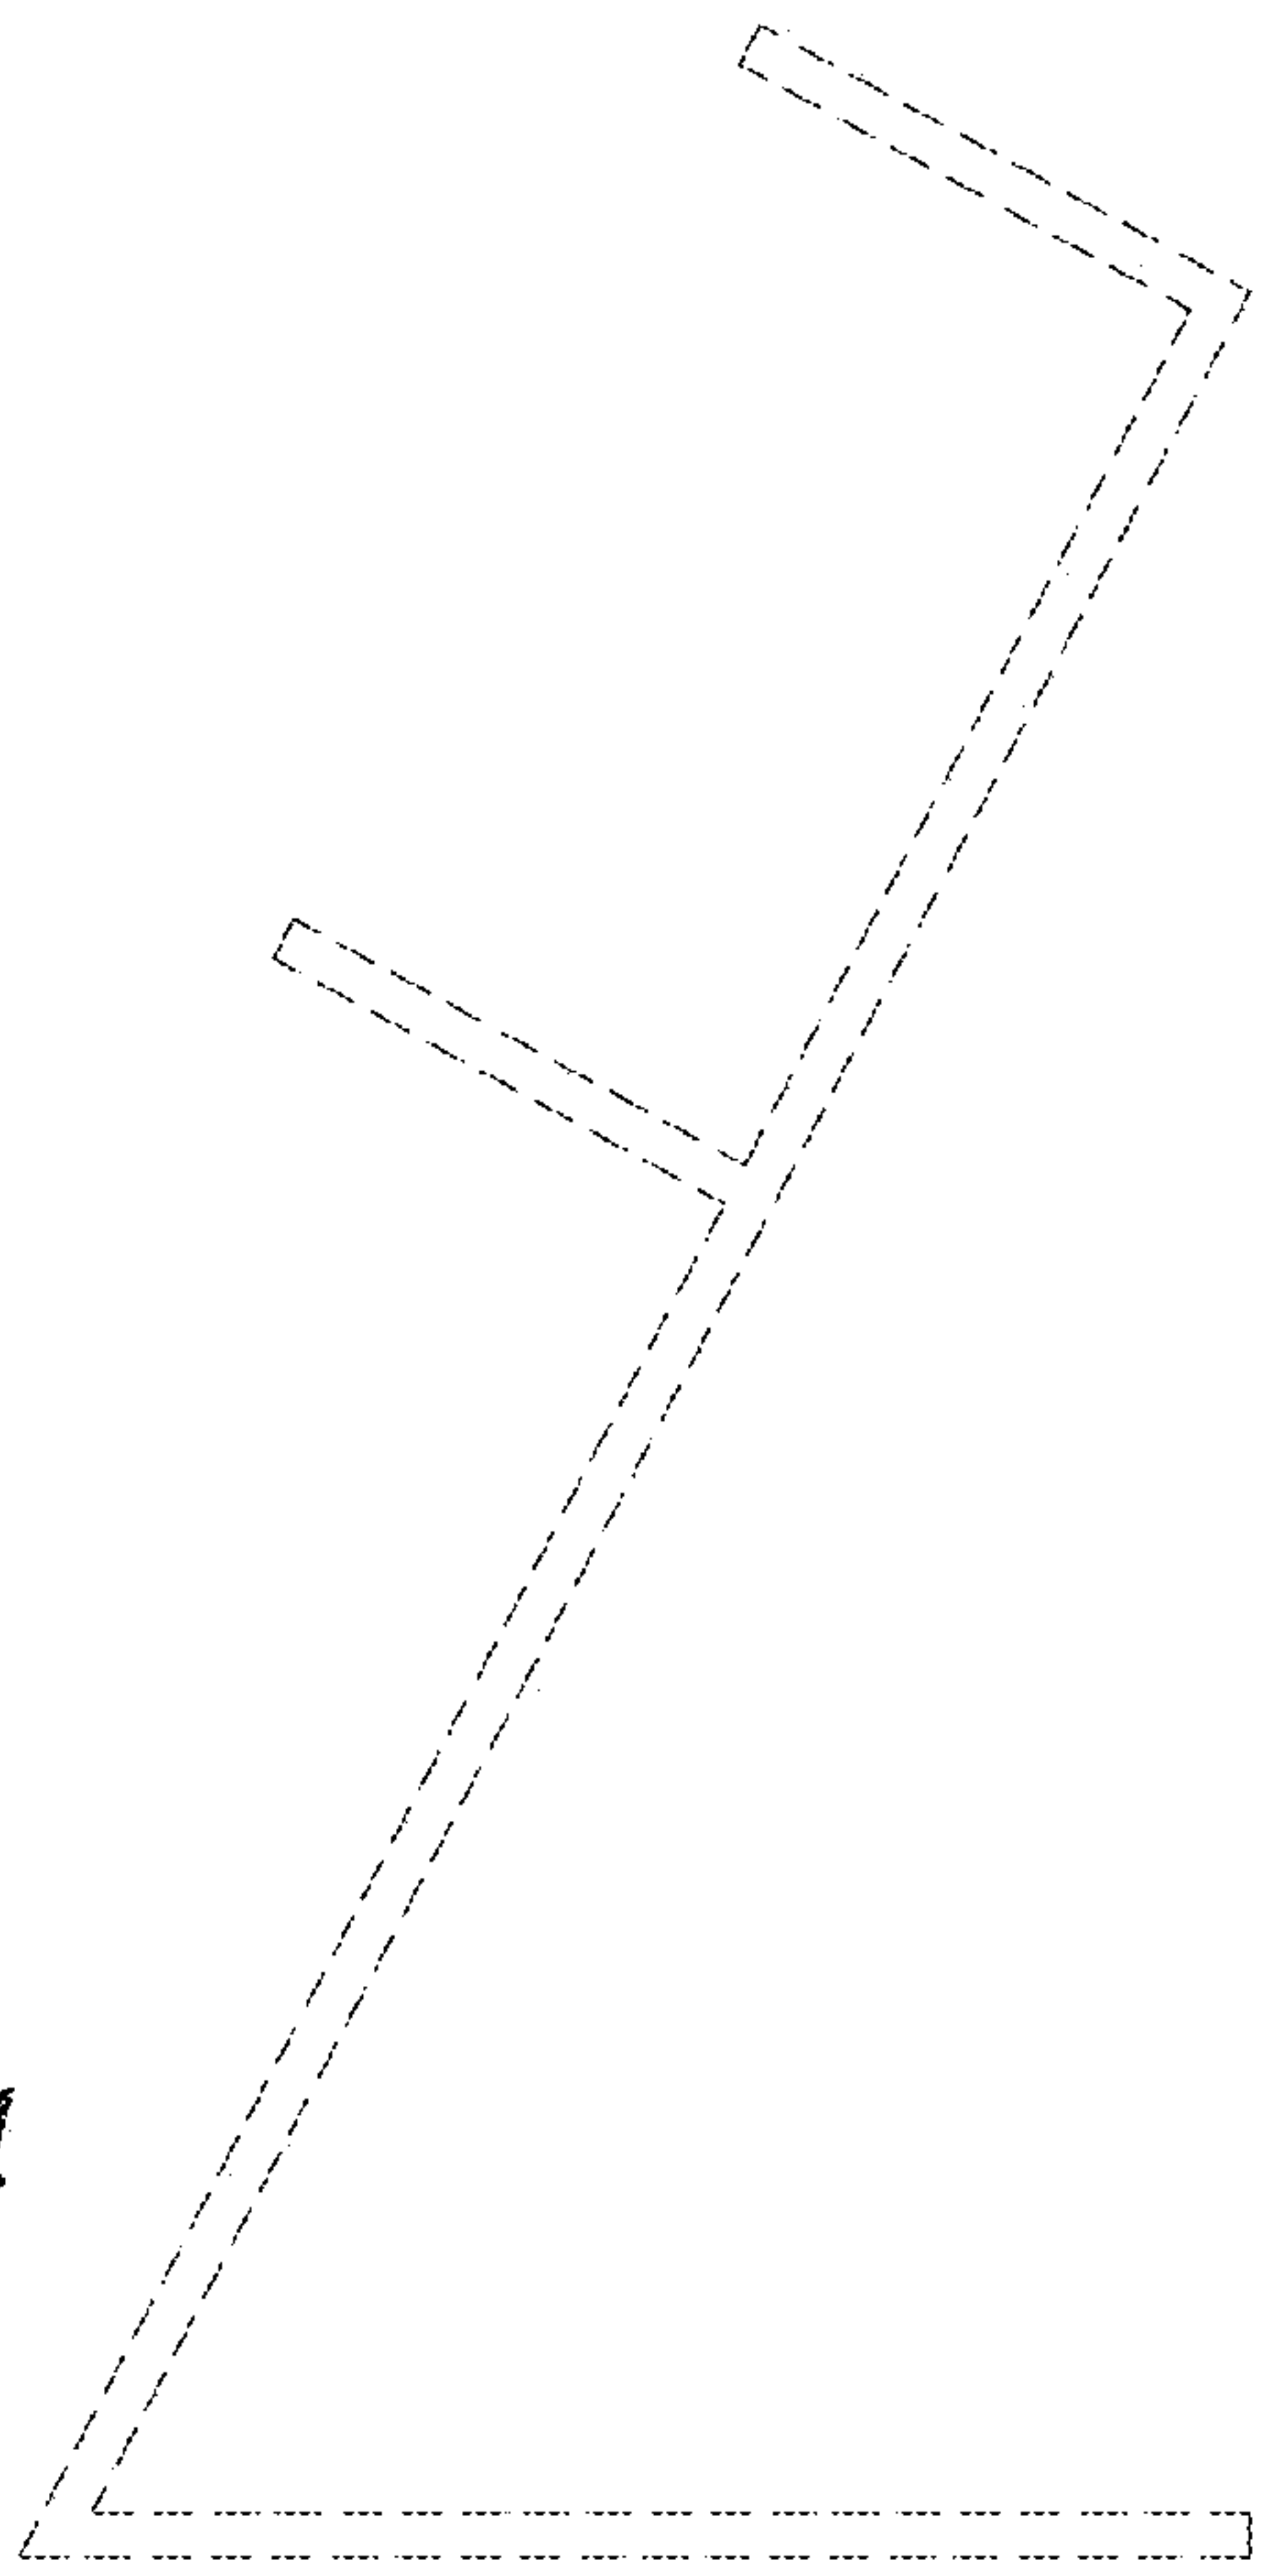


FIG. 14

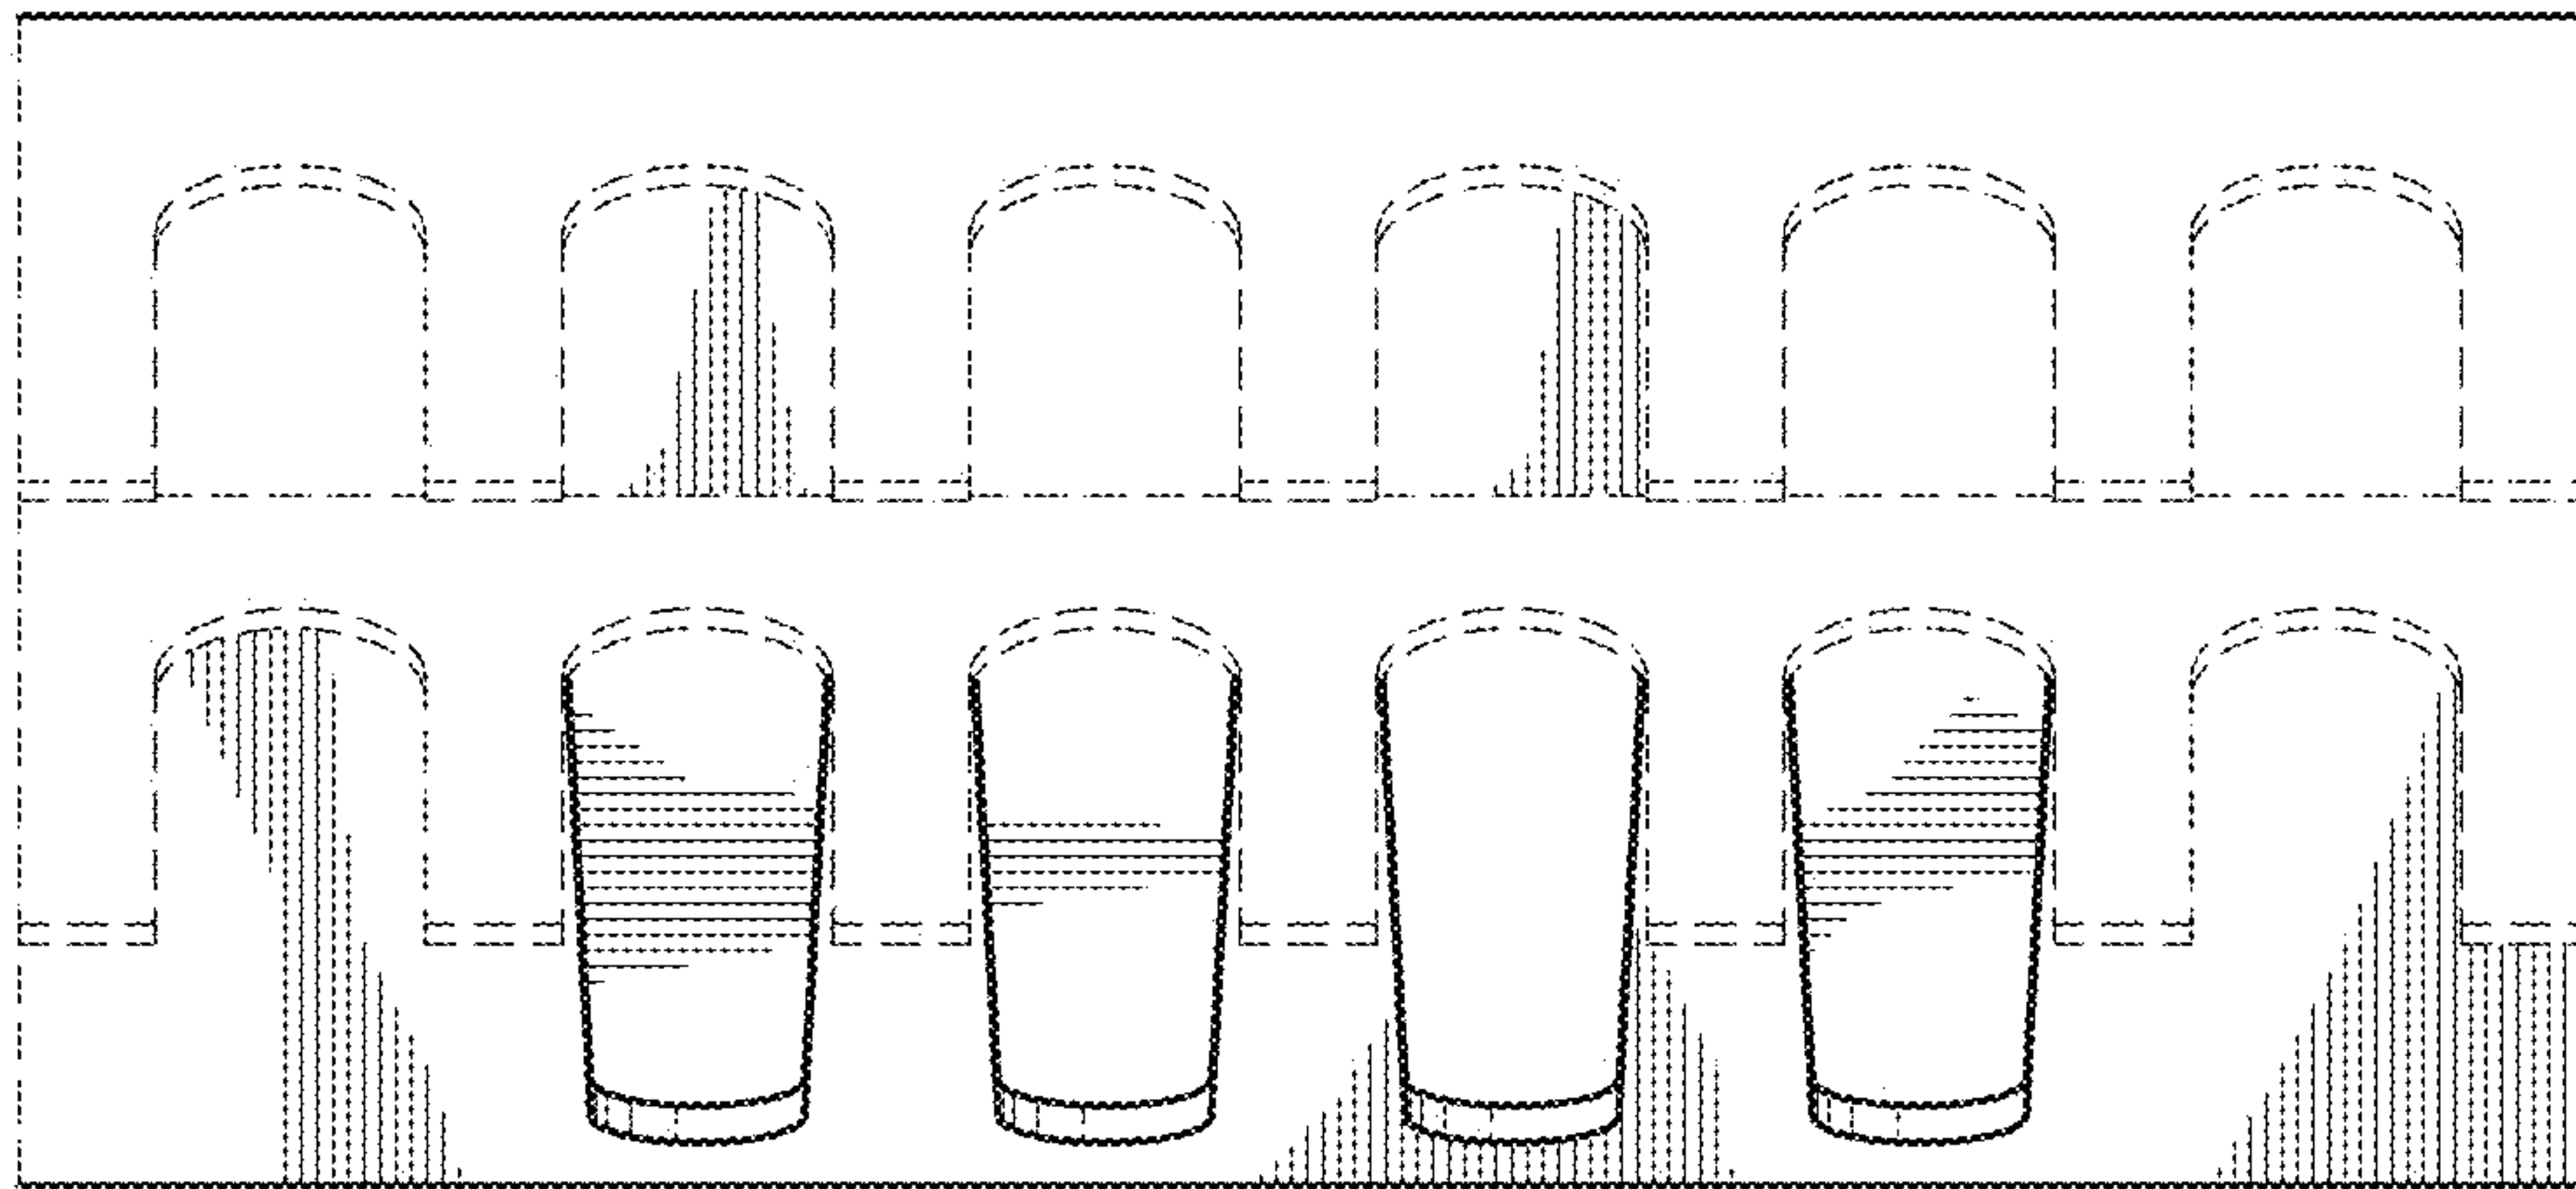


FIG. 15

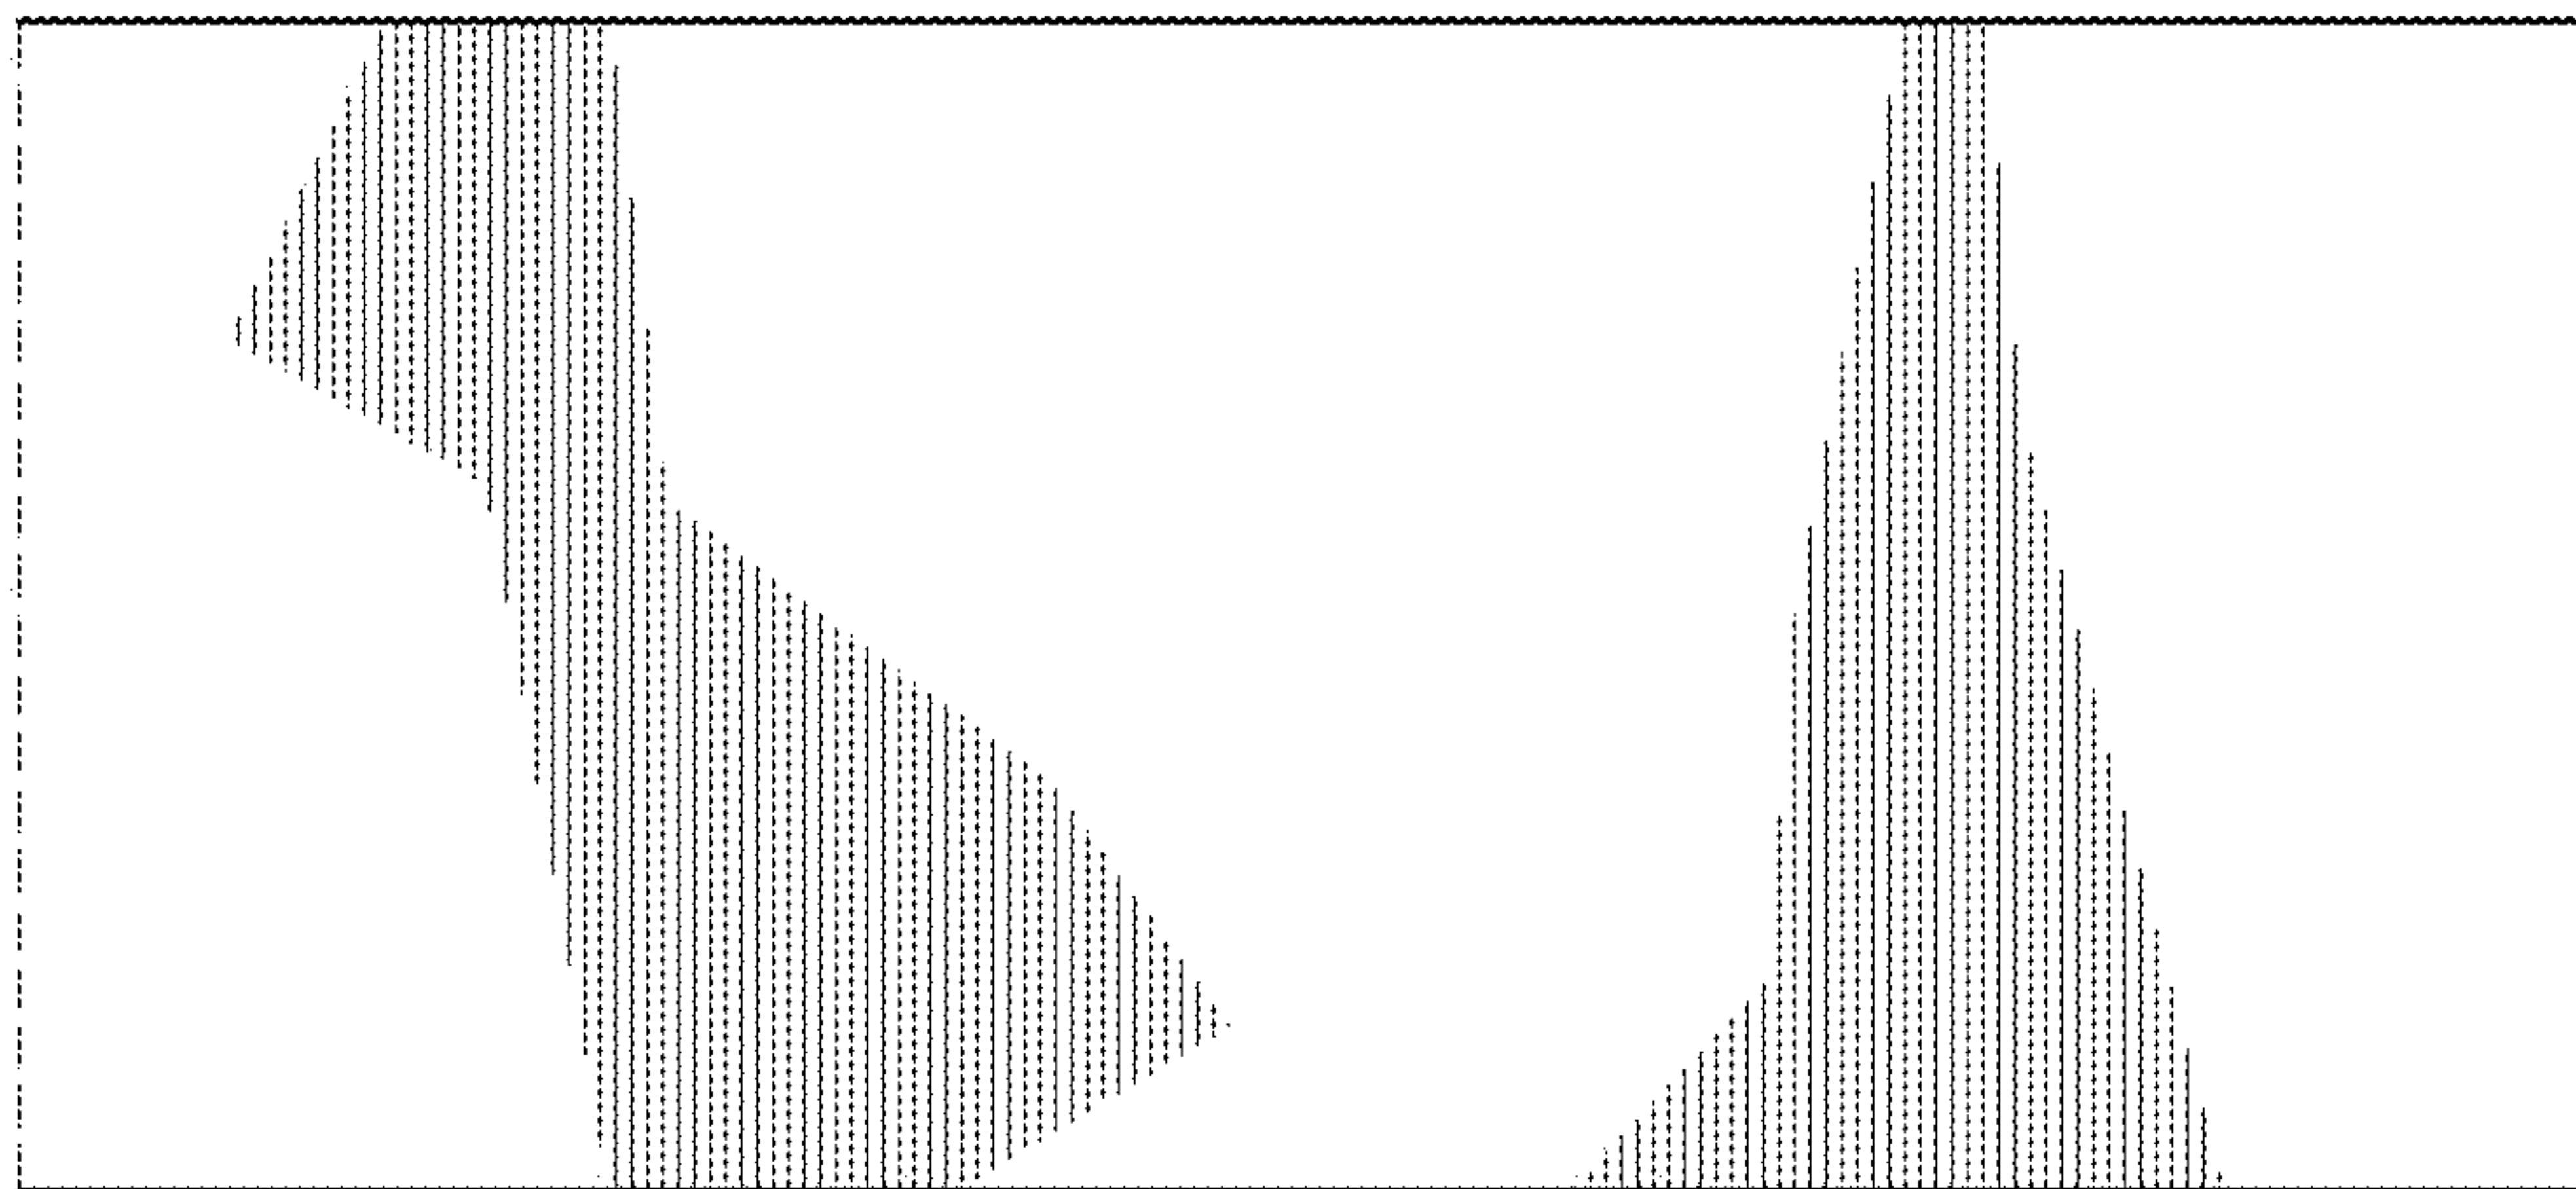


FIG. 16