



US00D872861S

(12) **United States Design Patent** (10) **Patent No.:** **US D872,861 S**
Adams (45) **Date of Patent:** **** Jan. 14, 2020**

(54) **DOUBLE STRAND TWIST BI-DIRECTIONAL BARB SUTURE WITH SINGLE COATING SHIELD**

FOREIGN PATENT DOCUMENTS

CA 2777345 A1 11/2012
EP 2338421 B1 11/2012

(Continued)

(71) Applicant: **Jason P. Adams**, Farmington, NM (US)

(72) Inventor: **Jason P. Adams**, Farmington, NM (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/623,778**

(22) Filed: **Oct. 26, 2017**

Related U.S. Application Data

(63) Continuation-in-part of application No. 15/096,496, filed on Apr. 12, 2016, now abandoned.

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/145**

(58) **Field of Classification Search**
USPC D24/145, 146, 147, 148, 133, 155, 169;
D11/1, 3, 13, 15
CPC A61B 17/06166; A61B 17/0401; A61B
2017/00526; A61B 2017/06176; A61B
17/06066; A61B 17/04; A61B 2017/0417;
A61B 2017/0608; A61B 17/0469; A61B
17/0483; A61B 17/0485; A61B 17/062;
A61B 2017/0046; A61B 2017/047; A61F
2002/075; B21G 1/08

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,720,055 A 3/1973 De Mestral et al.
4,622,777 A * 11/1986 Greene, Jr. A01G 9/022
47/67
D398,271 S * 9/1998 Wang D12/193
D398,551 S * 9/1998 Kupelian D11/18

(Continued)

OTHER PUBLICATIONS

John R. Fowler, MD, Tiffany A. Perkins, BS, Bettina A. Buttaro, PhD, and Allan L. Truant, PhD, Clin Ortho Relat Res. Bacteria Adhere Less to Barbed Monofilament Than Braided Sutures in a Contaminated Wound Model, Feb. 2013; 471(2): 665-671.

(Continued)

Primary Examiner — Cathron C Brooks

Assistant Examiner — Samantha Q Lawrence

(74) *Attorney, Agent, or Firm* — Pate Baird, PLLC

(57) **CLAIM**

The ornamental design for a double strand twist bi-directional barb suture with single coating shield, as shown and described.

DESCRIPTION

FIG. 1 is a side elevation view of a double strand twist bi-directional barb suture with single coating shield in accordance with the invention, in a first condition of use, with the strands having a clear coating, with all other side views are substantially the same, as based on the repeating pattern of the barb;

FIG. 2 is a perspective view thereof;

FIG. 3 is a cross-section view thereof taken along line 3-3, the bottom view being a mirror image thereof; and,

FIG. 4 is a cross-section view of the double strand twist bi-directional barb suture with single coating shield taken along line 3-3 in a second condition of use, with the coating dissolved, the bottom view being a mirror image thereof.

1 Claim, 1 Drawing Sheet



(56)

References Cited

U.S. PATENT DOCUMENTS

D462,633 S * 9/2002 Chia D11/13
 D539,550 S * 4/2007 Ping Sheng D5/99
 8,062,363 B2 11/2011 Hirpara et al.
 8,353,931 B2 1/2013 Stopek et al.
 8,562,644 B2 10/2013 Yuan et al.
 D734,459 S * 7/2015 Arnett D24/145
 D745,964 S * 12/2015 Ponganis D24/133
 D745,965 S * 12/2015 Anderson D24/133
 D746,449 S * 12/2015 Ponganis D24/133
 D746,450 S * 12/2015 Anderson D24/133
 D747,996 S * 1/2016 Bridges D11/3
 D749,726 S * 2/2016 Ponganis D24/133
 D844,140 S * 3/2019 Adams D24/145
 2012/0277793 A1 * 11/2012 Marczyk A61B 17/06166
 606/228
 2013/0066369 A1 3/2013 Collier et al.
 2013/0165971 A1 6/2013 Leung et al.
 2015/0272720 A1 * 10/2015 Marks A61B 17/00008
 623/13.2
 2016/0120543 A1 * 5/2016 Nawrocki A61B 17/06166
 606/230
 2016/0278769 A1 * 9/2016 Kim D02J 3/10
 2017/0189016 A1 * 7/2017 Gross A61B 17/06166
 2017/0281160 A1 * 10/2017 Lin A61B 17/06166
 2017/0319195 A1 * 11/2017 Denham A61F 2/0811
 2017/0319203 A1 * 11/2017 Cohen A61B 17/06166
 2017/0360543 A1 * 12/2017 Rosenblatt A61F 2/0045

2018/0103944 A9* 4/2018 Sauer A61B 17/0401
 2018/0116648 A1 * 5/2018 Kim A61B 17/06166
 2018/0125472 A1 * 5/2018 Dreyfuss A61B 17/0401
 2018/0140291 A1 * 5/2018 Dreyfuss A61B 17/0401

FOREIGN PATENT DOCUMENTS

EP 2447040 A3 12/2013
 JP 61171998 2/1986

OTHER PUBLICATIONS

James A. Greenberg, MD, US National Library of Medicine National Institute of Health, The Use of Barbed Sutures in Obstetrics and Gynecology, v.3(3); Summer 2010.
 Dr. R.K. Mishra, Barbed Suture in Laparoscopic Surgery, Feb. 9, 2016.
 Angiotech Puerto Rico, Inc., Quill™ Knotless Tissue-Closure Device Product Catalog, 2007-2013.
 Angiotech Pharmaceuticals, Inc. Quill™ SRS Product Catalog, 2009.
 Covidien, V-Loc™ Wound Closure Devices Product Overview, 2011.
 Covidien, V-Loc™ Wound Closure Device (the secure advantage), 2013.
 DePuy Mitek, a Johnson & Johnson Company, MicroFix Absorbable QuickAnchor® Plus, Massachusetts, 2005.

* cited by examiner

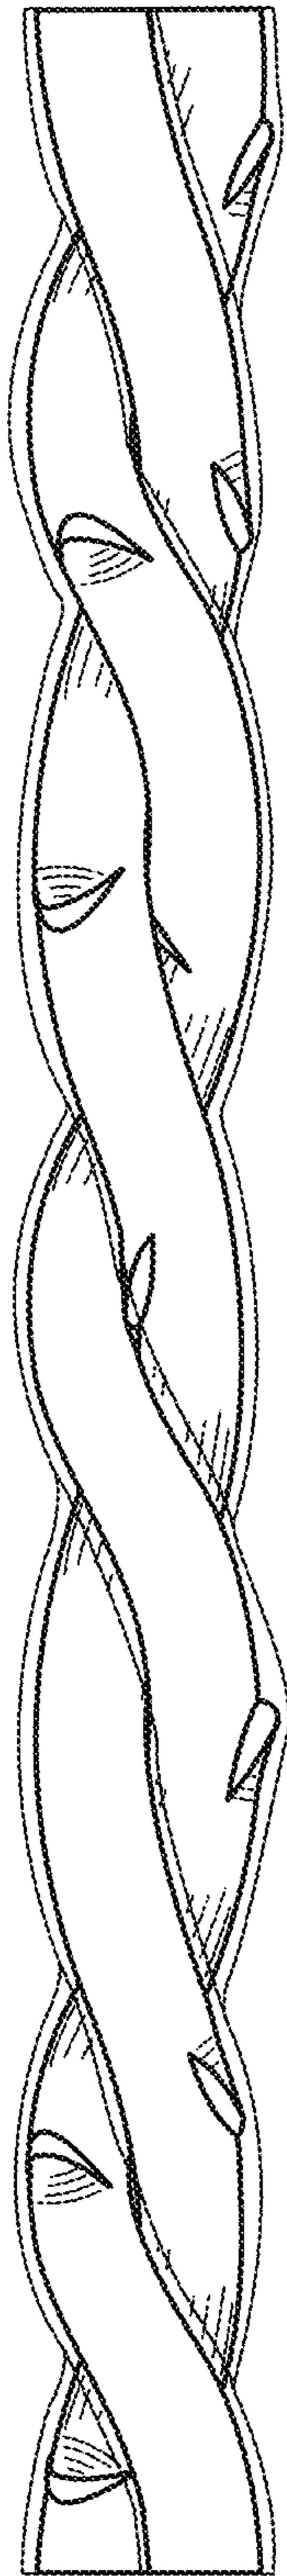


FIG. 1

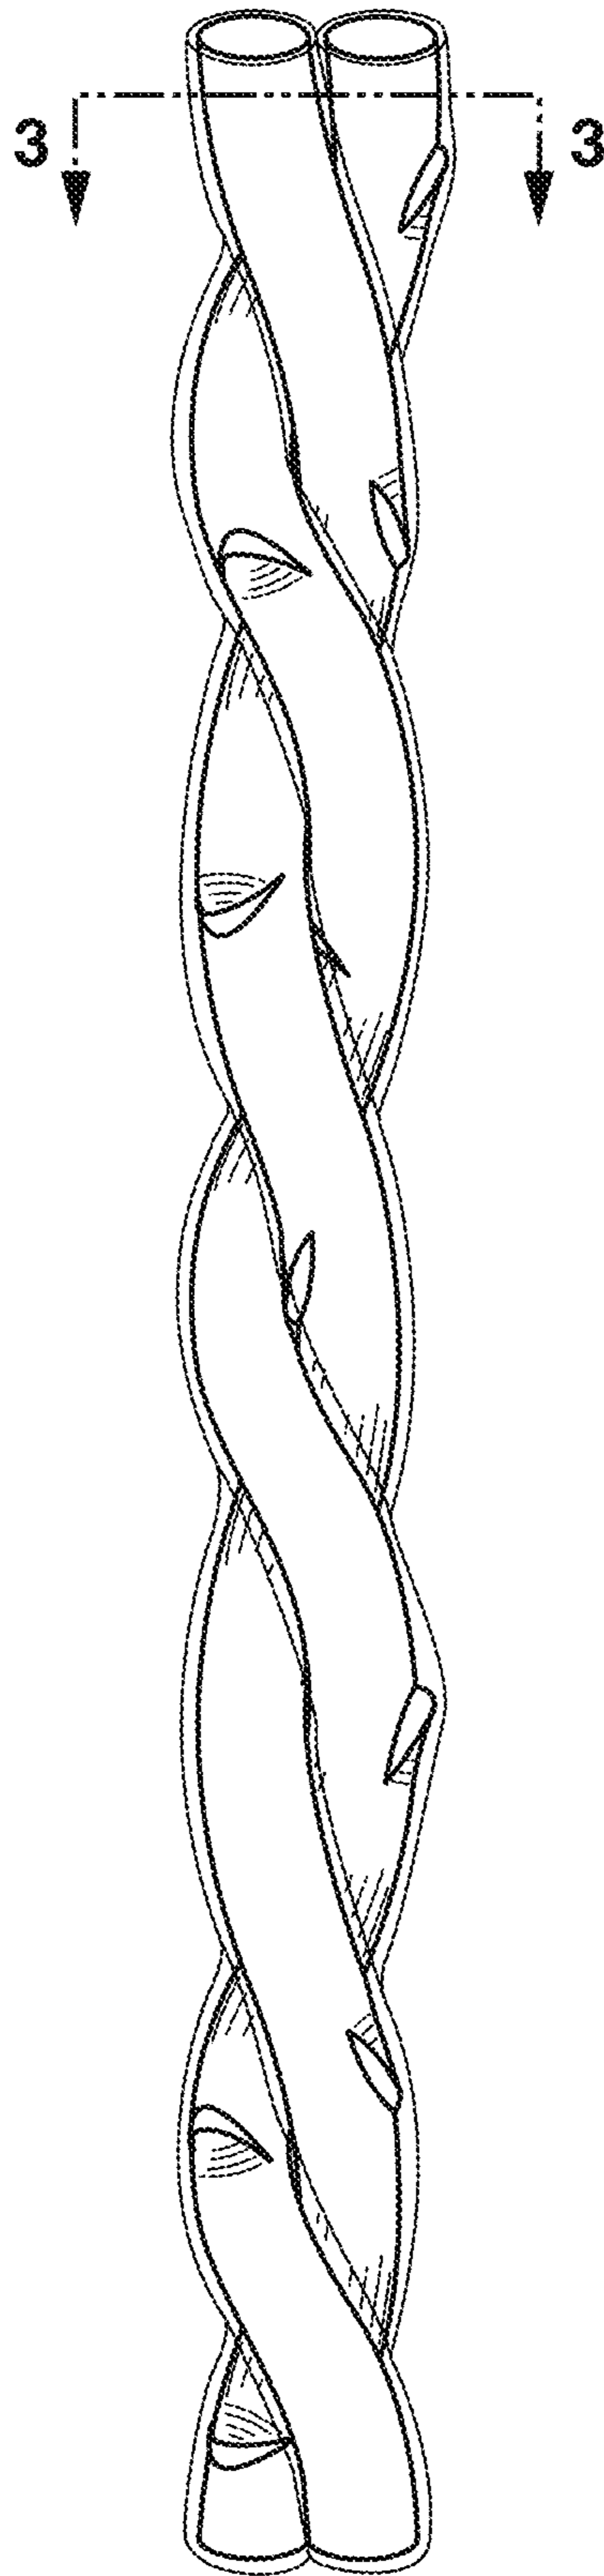


FIG. 2

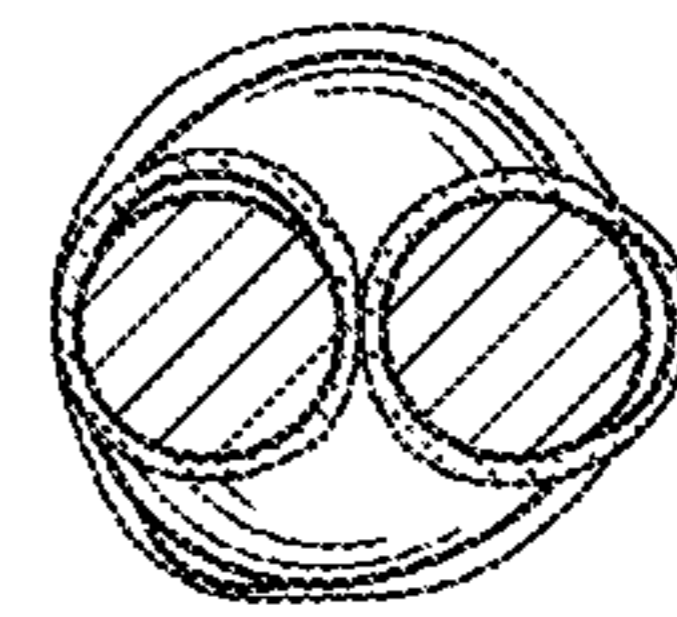


FIG. 3

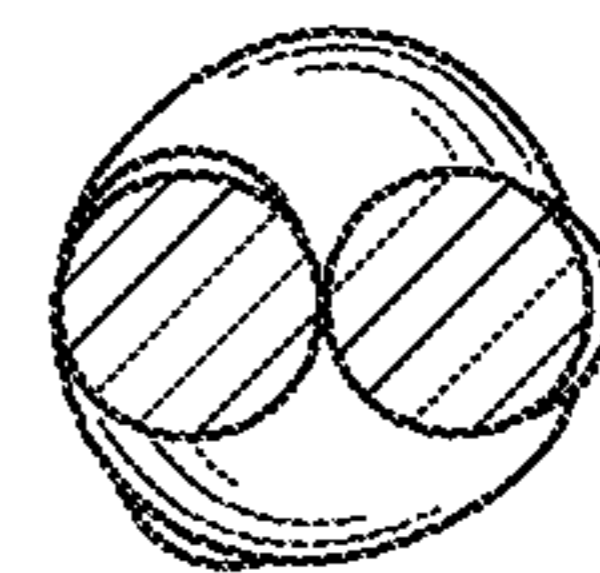


FIG. 4