



US00D873416S

(12) **United States Design Patent**
Köppel et al.

(10) **Patent No.:** **US D873,416 S**
(45) **Date of Patent:** **** Jan. 21, 2020**

(54) **PEDAL FOR OPHTHALMOLOGIC APPARATUS**

D761,675 S * 7/2016 Thaveeprungsriporn D10/38
D766,841 S * 9/2016 Alvarez D13/167
2014/0135785 A1* 5/2014 Tran H01H 21/26
606/107

(71) Applicant: **THIS AG**, Heerbrugg (CH)

(72) Inventors: **Thomas Köppel**, Widnau (CH); **Marco Zünd**, Widnau (CH); **Marco Cafadér**, Bruges (CH); **Hanspeter Kersten**, Bruges (CH); **Raimund Erdmann**, Bruges (CH)

(73) Assignee: **THIS AG**, Heerbrugg (CH)

(**) Term: **15 Years**

(21) Appl. No.: **29/600,184**

(22) Filed: **Apr. 10, 2017**

(51) **LOC (12) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/172**

(58) **Field of Classification Search**
USPC D24/144, 107, 127, 167, 169–170, 172, D24/179, 185; D13/167
CPC A61B 2017/00973; A61C 1/0023; H01H 3/14; H01H 13/16; H01H 21/26
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D586,919 S * 2/2009 Nielsen D13/167
D599,746 S * 9/2009 Long D13/167
D609,801 S * 2/2010 Egorov D24/107
D623,209 S * 9/2010 Matuschek D13/167
D669,441 S * 10/2012 Naef D13/167
D708,593 S * 7/2014 Lynn D13/179
D713,529 S * 9/2014 Li D13/167
D715,924 S * 10/2014 Green D24/127
D727,498 S * 4/2015 Creed D13/167
D751,706 S * 3/2016 Chambers D13/167

FOREIGN PATENT DOCUMENTS

CN 304614414 * 5/2018

* cited by examiner

Primary Examiner — Barbara Fox

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Nutter McClennen & Fish LLP

(57) **CLAIM**

The ornamental design for a pedal for ophthalmologic apparatus, as shown and described.

DESCRIPTION

This application is related to U.S. design application Ser. No. 29/600,172 entitled “Ophthalmologic Apparatus”.

This application is related to U.S. design application Ser. No. 29/600,176 entitled “Cassette for Ophthalmologic Apparatus”.

The contents of these related applications are incorporated herein by reference in their respective entireties.

FIG. 1 is a right-front perspective view of a pedal for ophthalmologic apparatus in accordance with the present invention.

FIG. 2 is a left-rear perspective view thereof.

FIG. 3 is a right elevation view thereof.

FIG. 4 is a front elevation view thereof.


FIG. 5 is a left elevation view thereof.

FIG. 6 is a back elevation view thereof; and,

FIG. 7 is a top view thereof.

The broken lines depict portions of the pedal for ophthalmologic apparatus that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

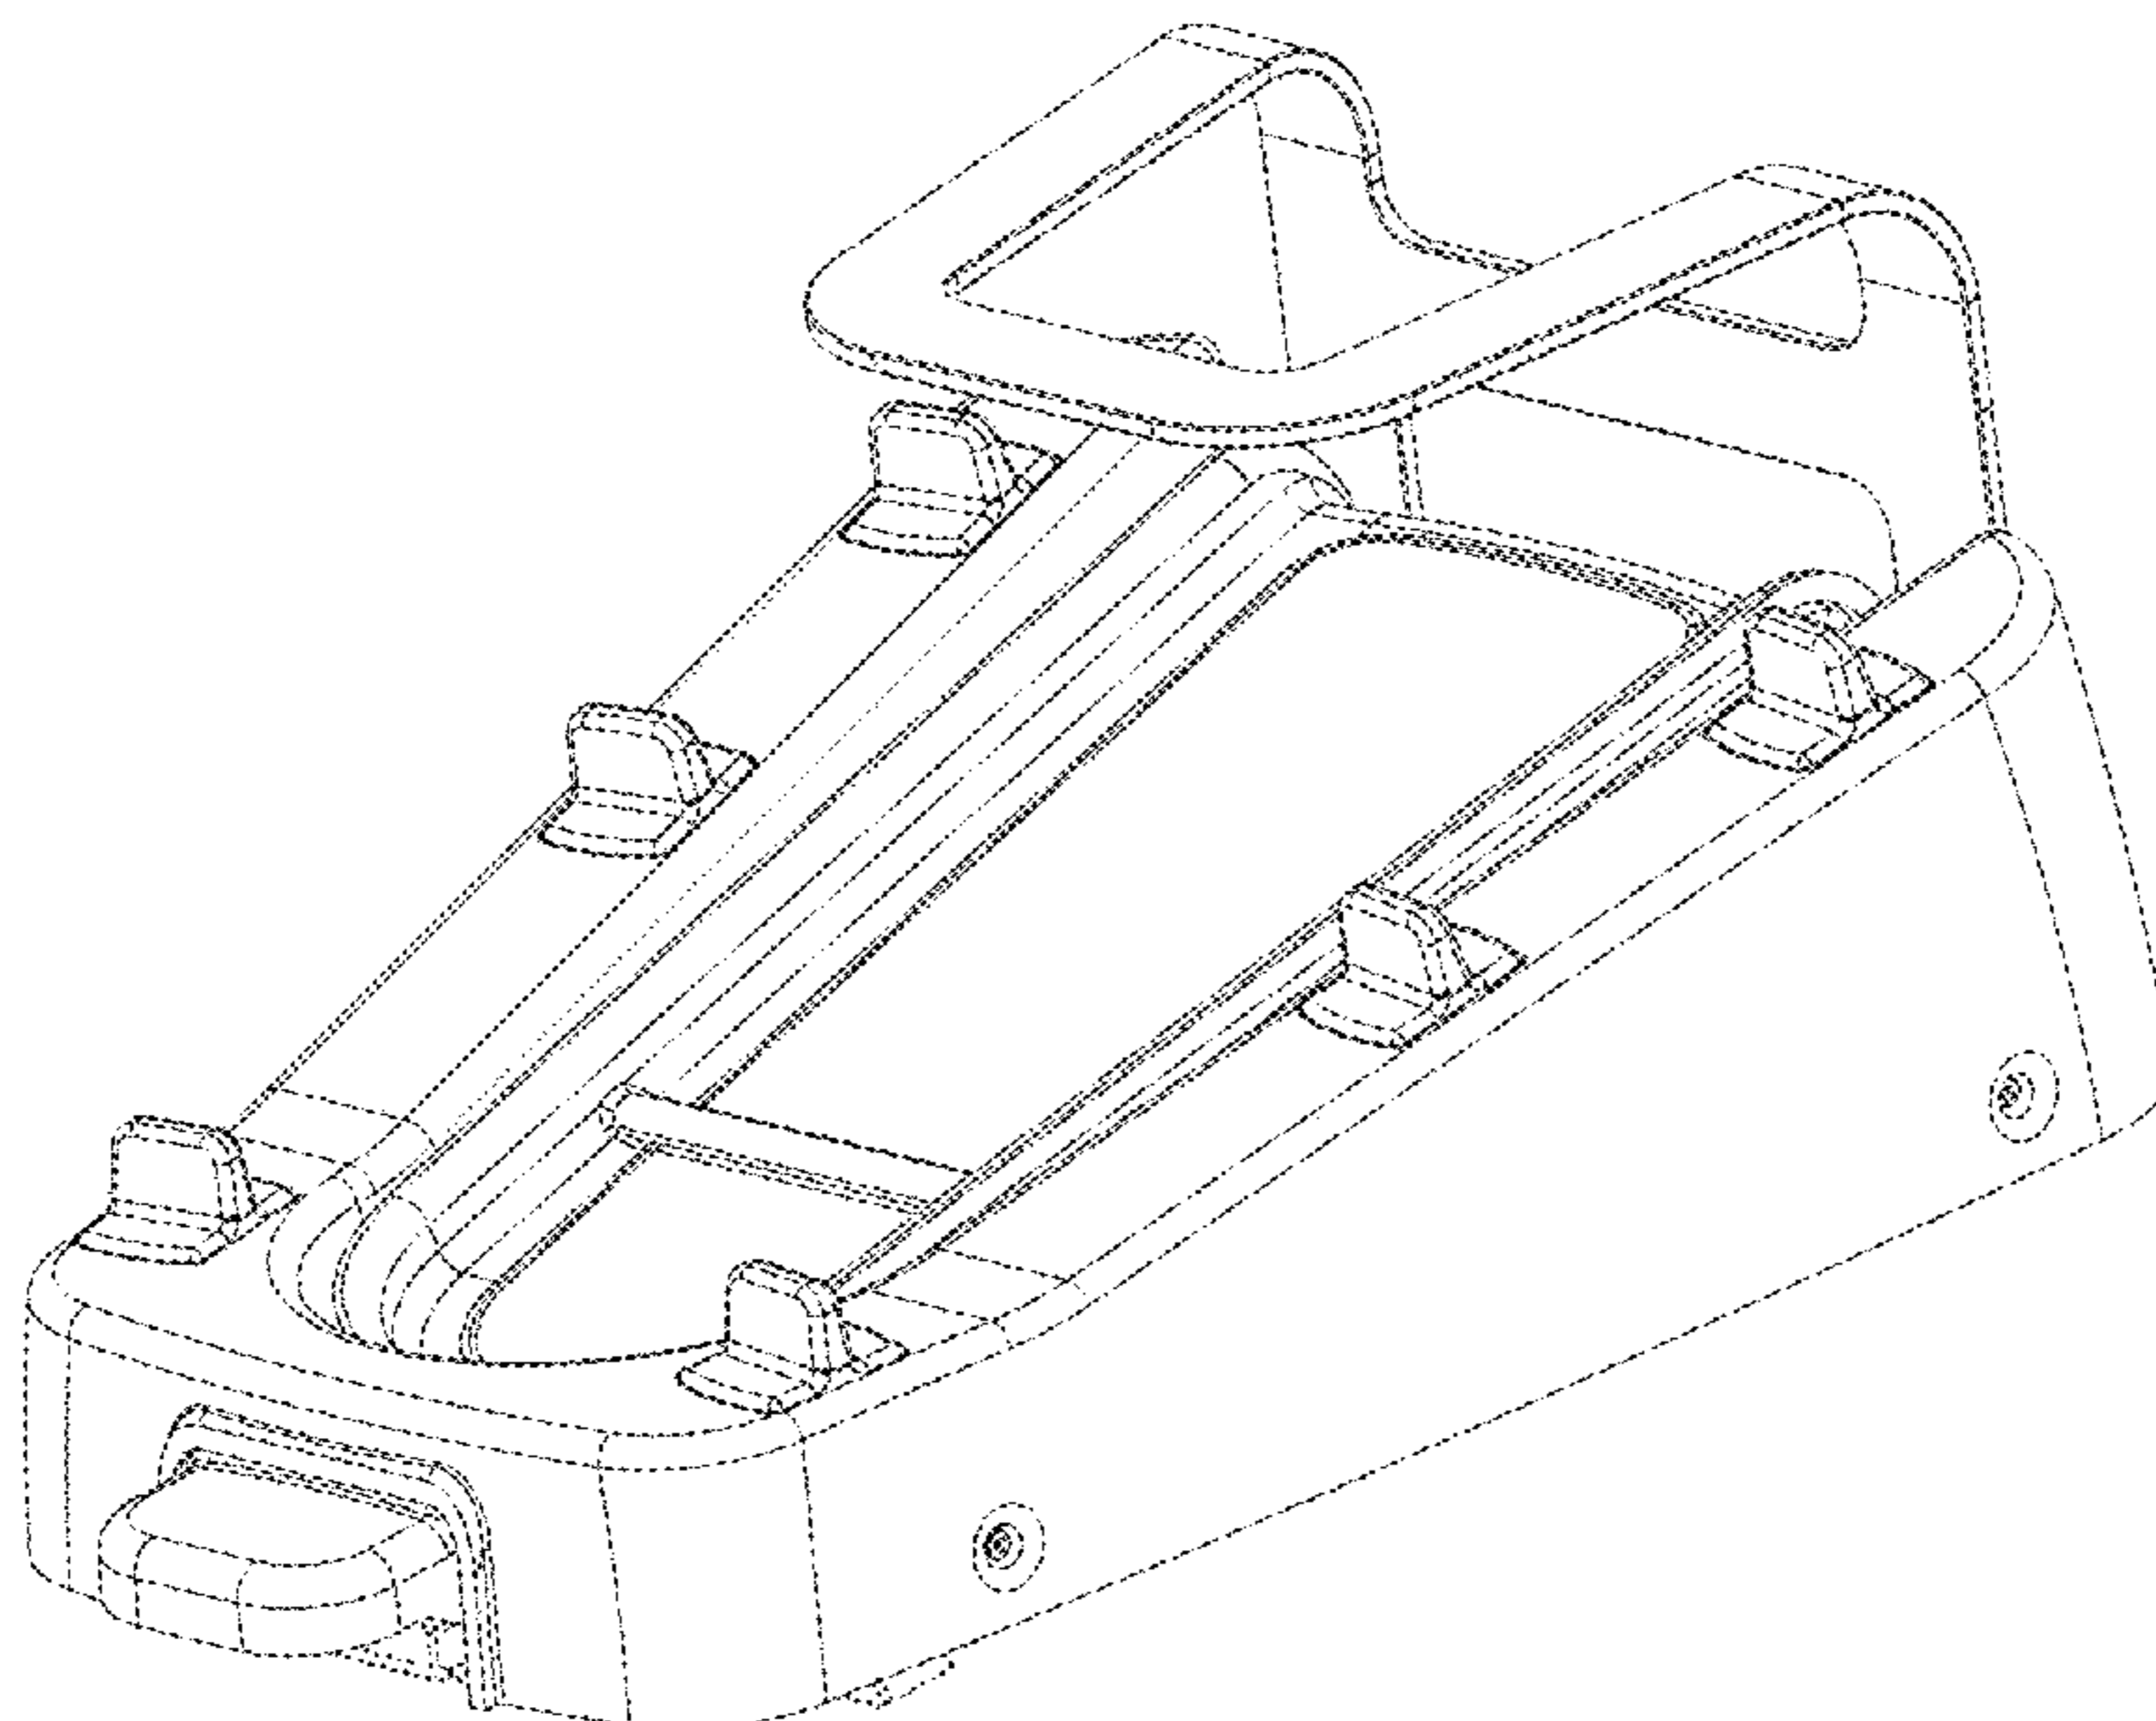

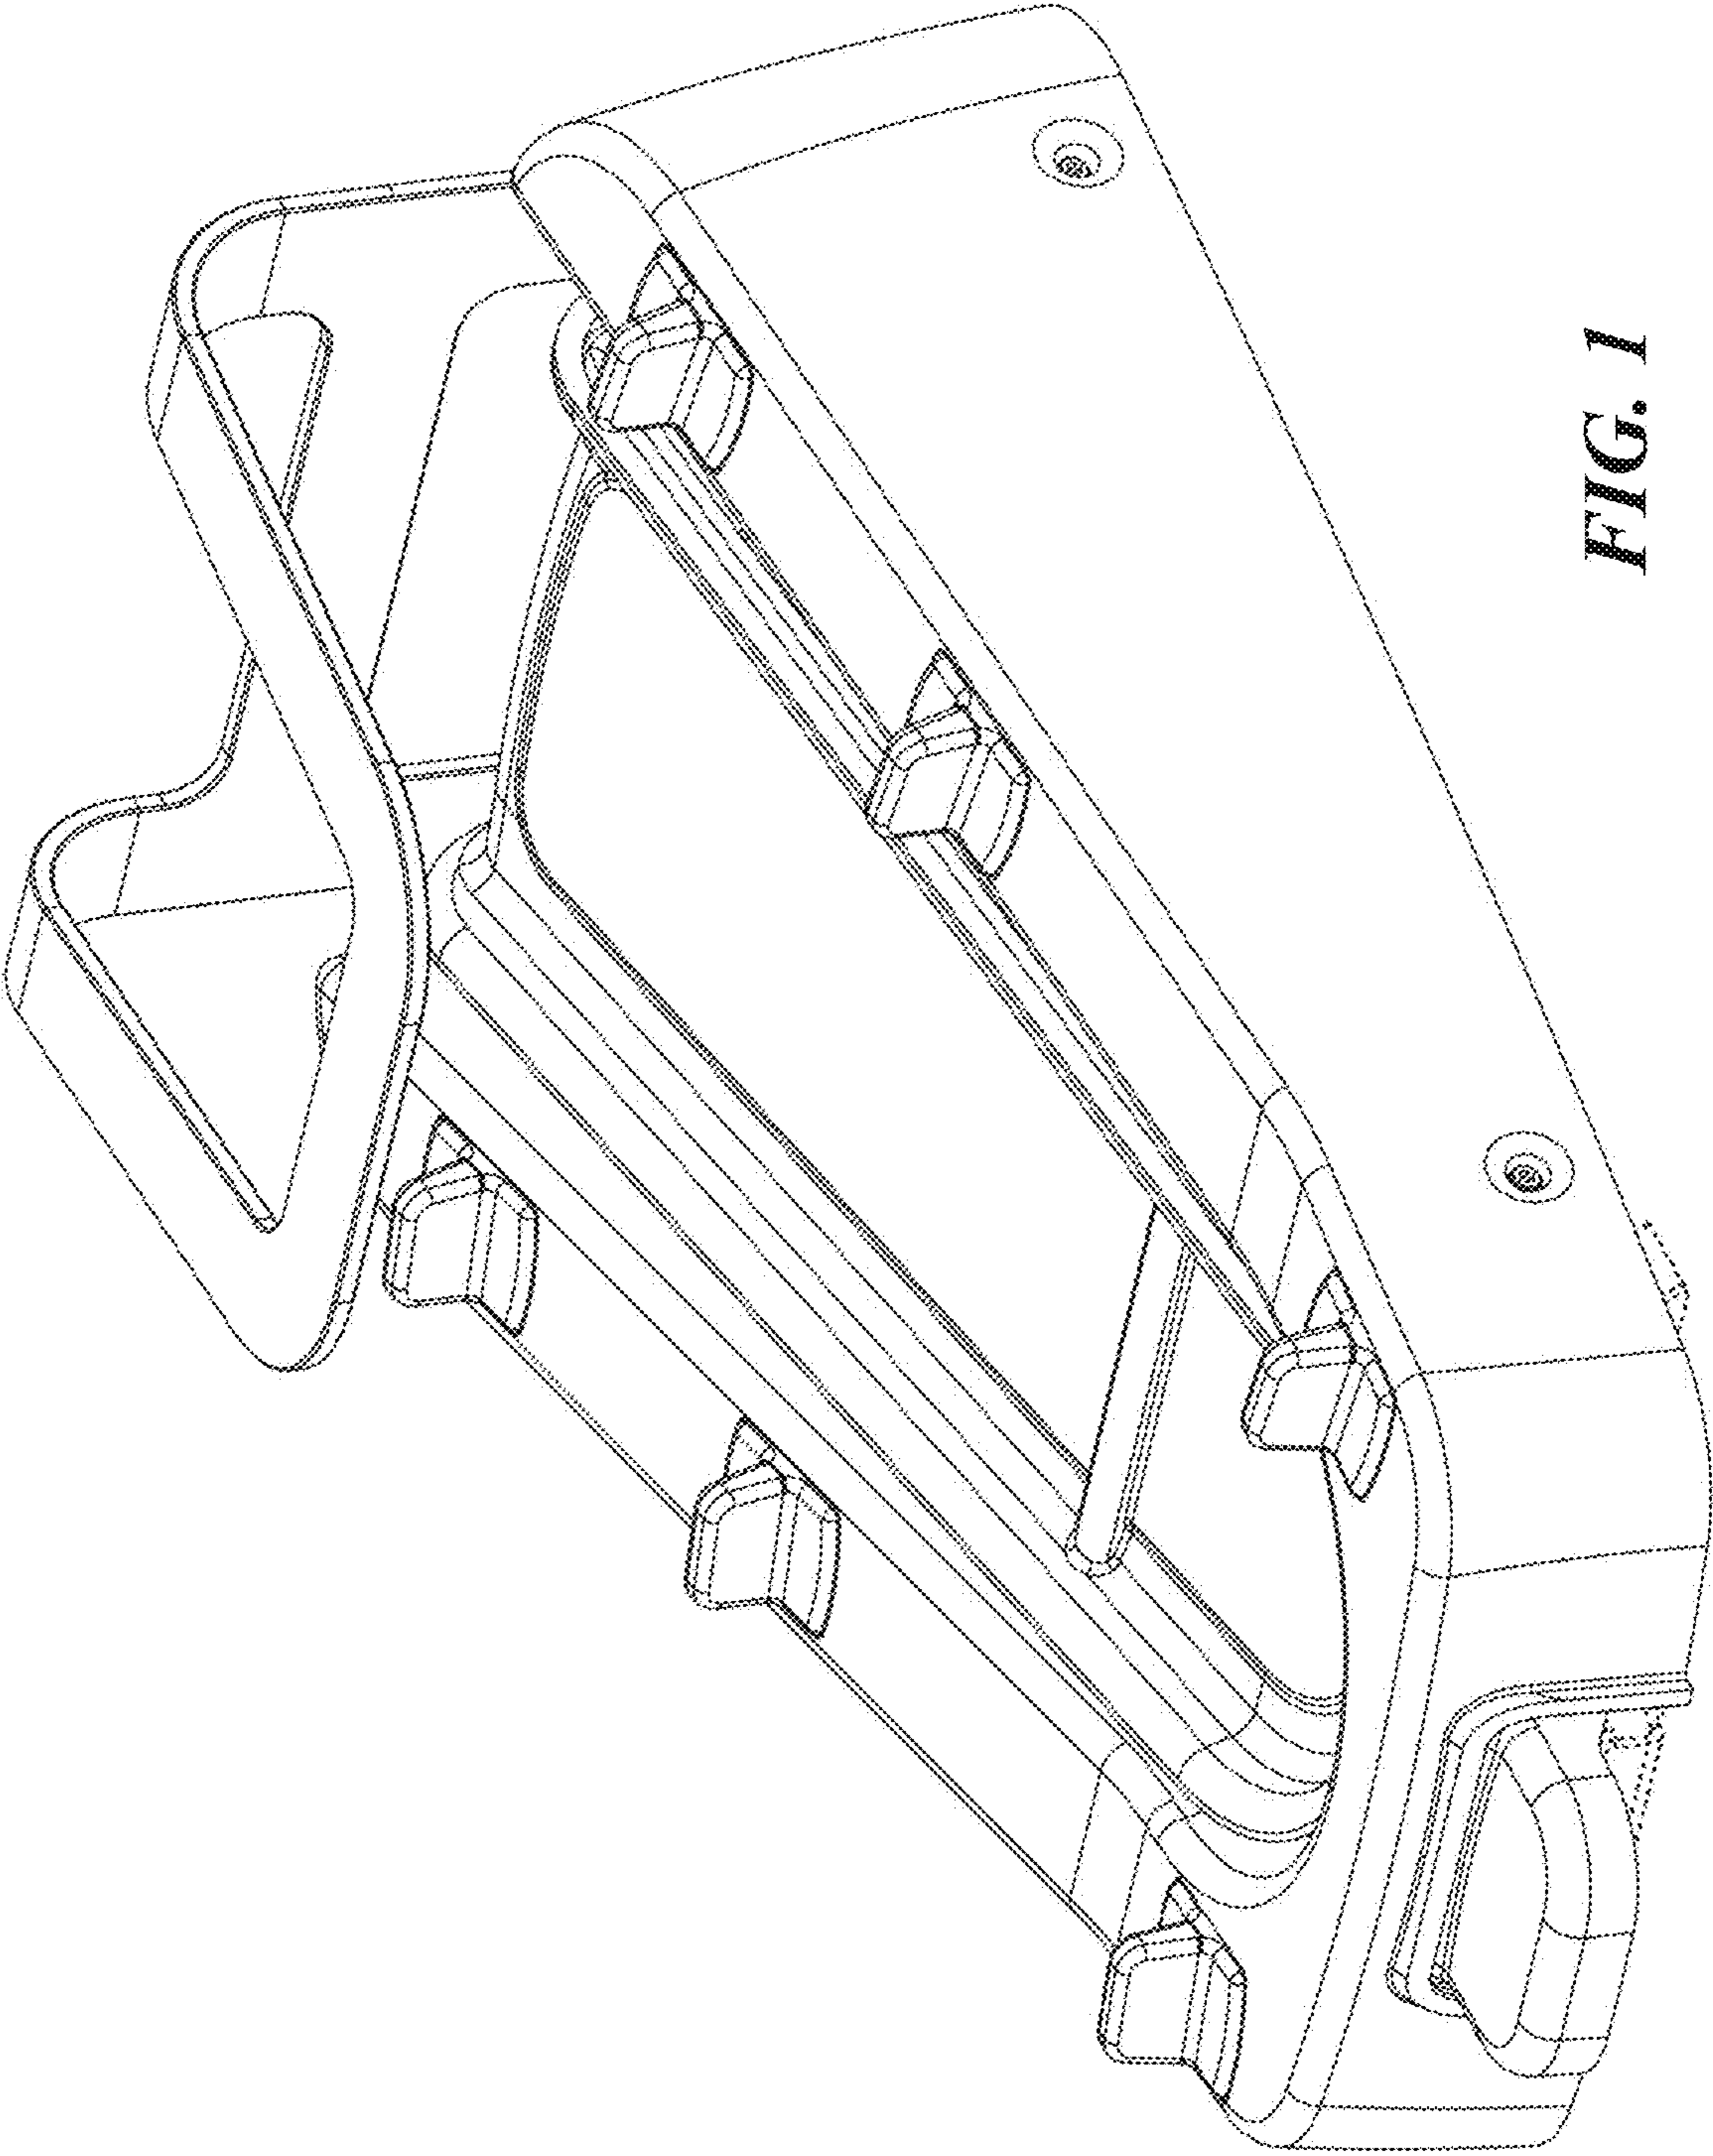


FIG. 1

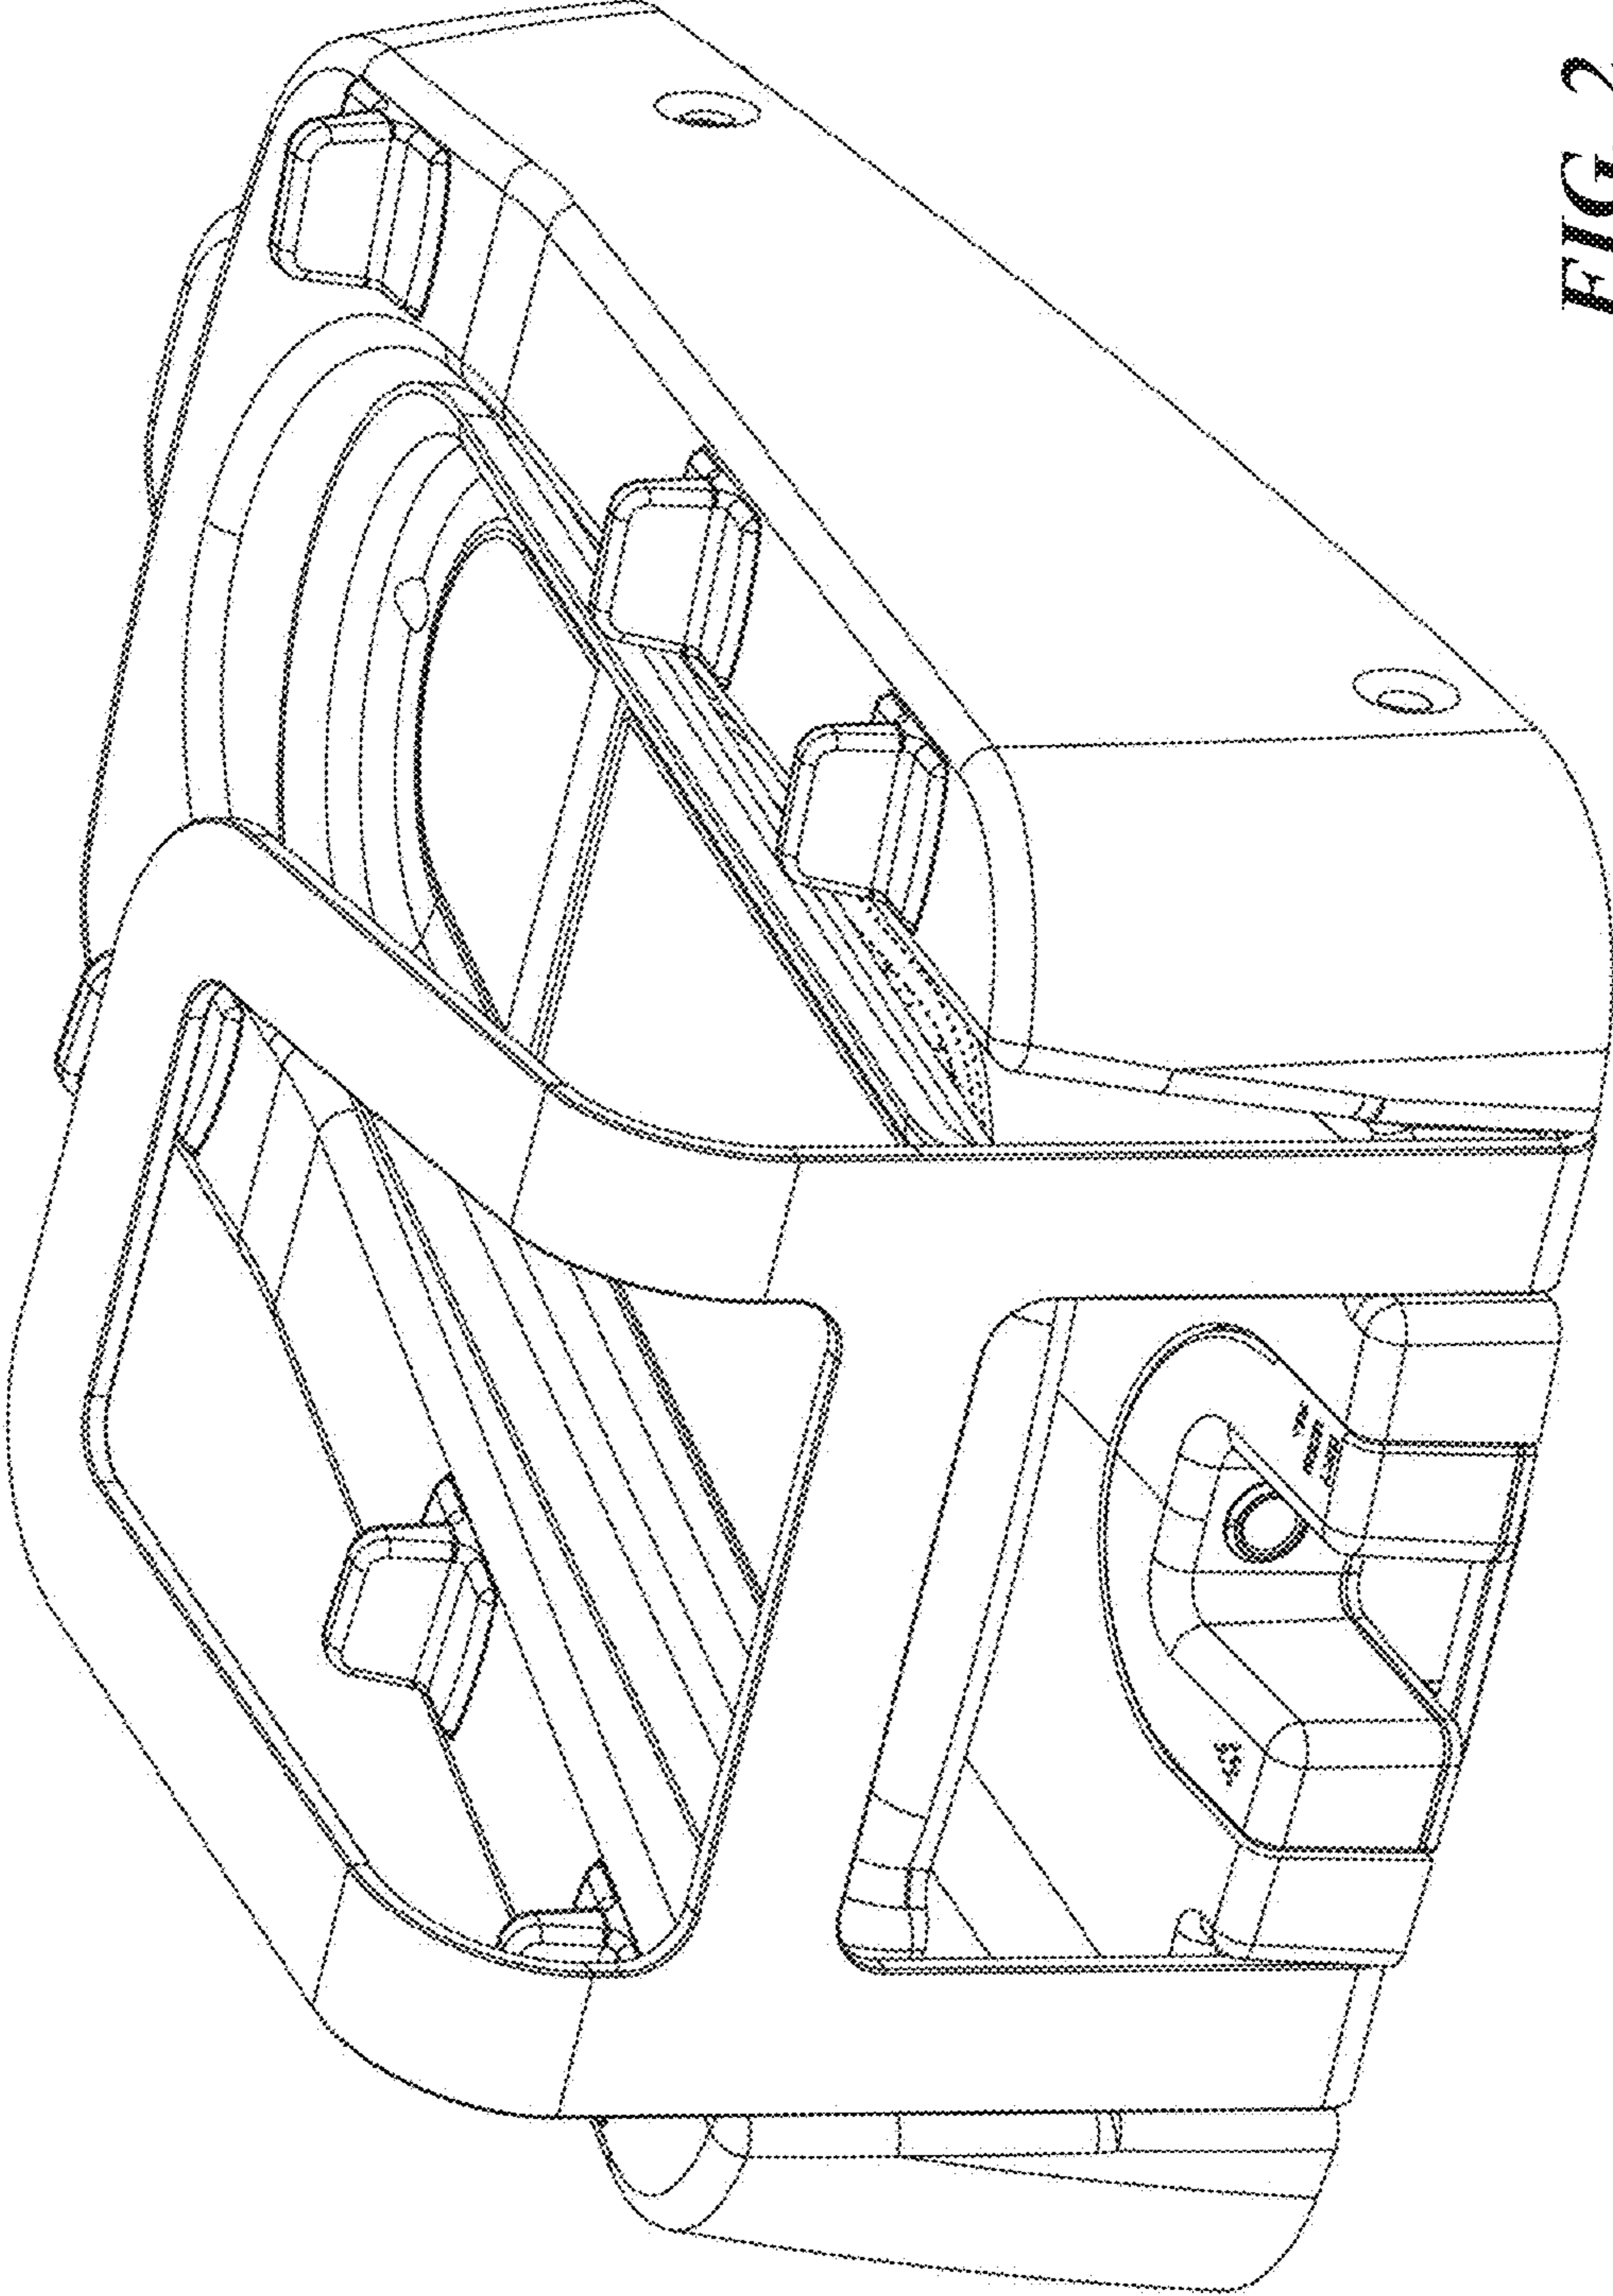


FIG. 2

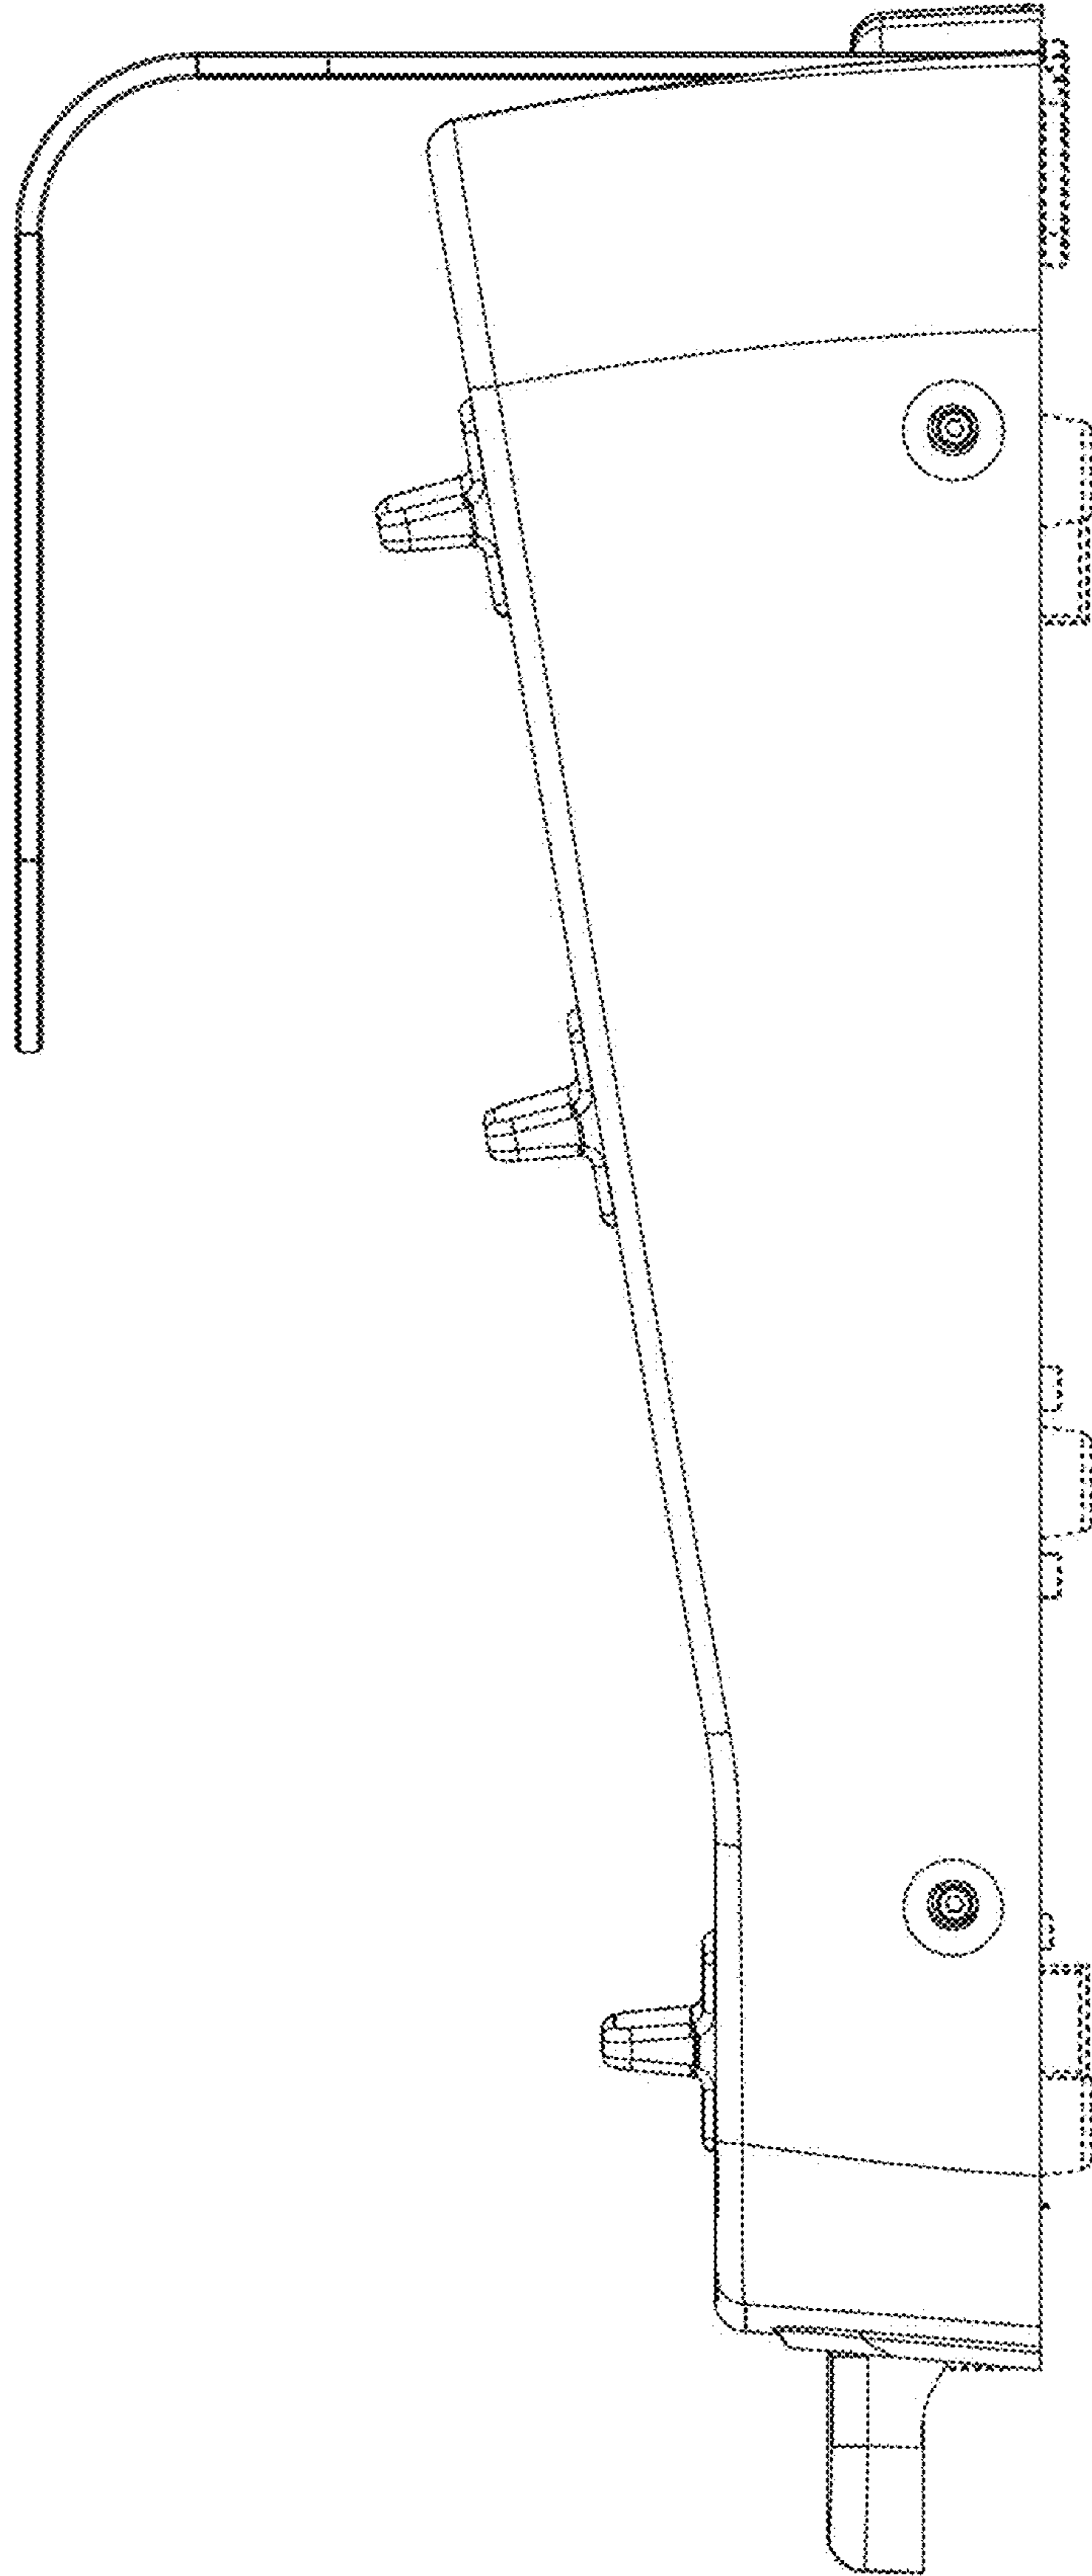


FIG. 3

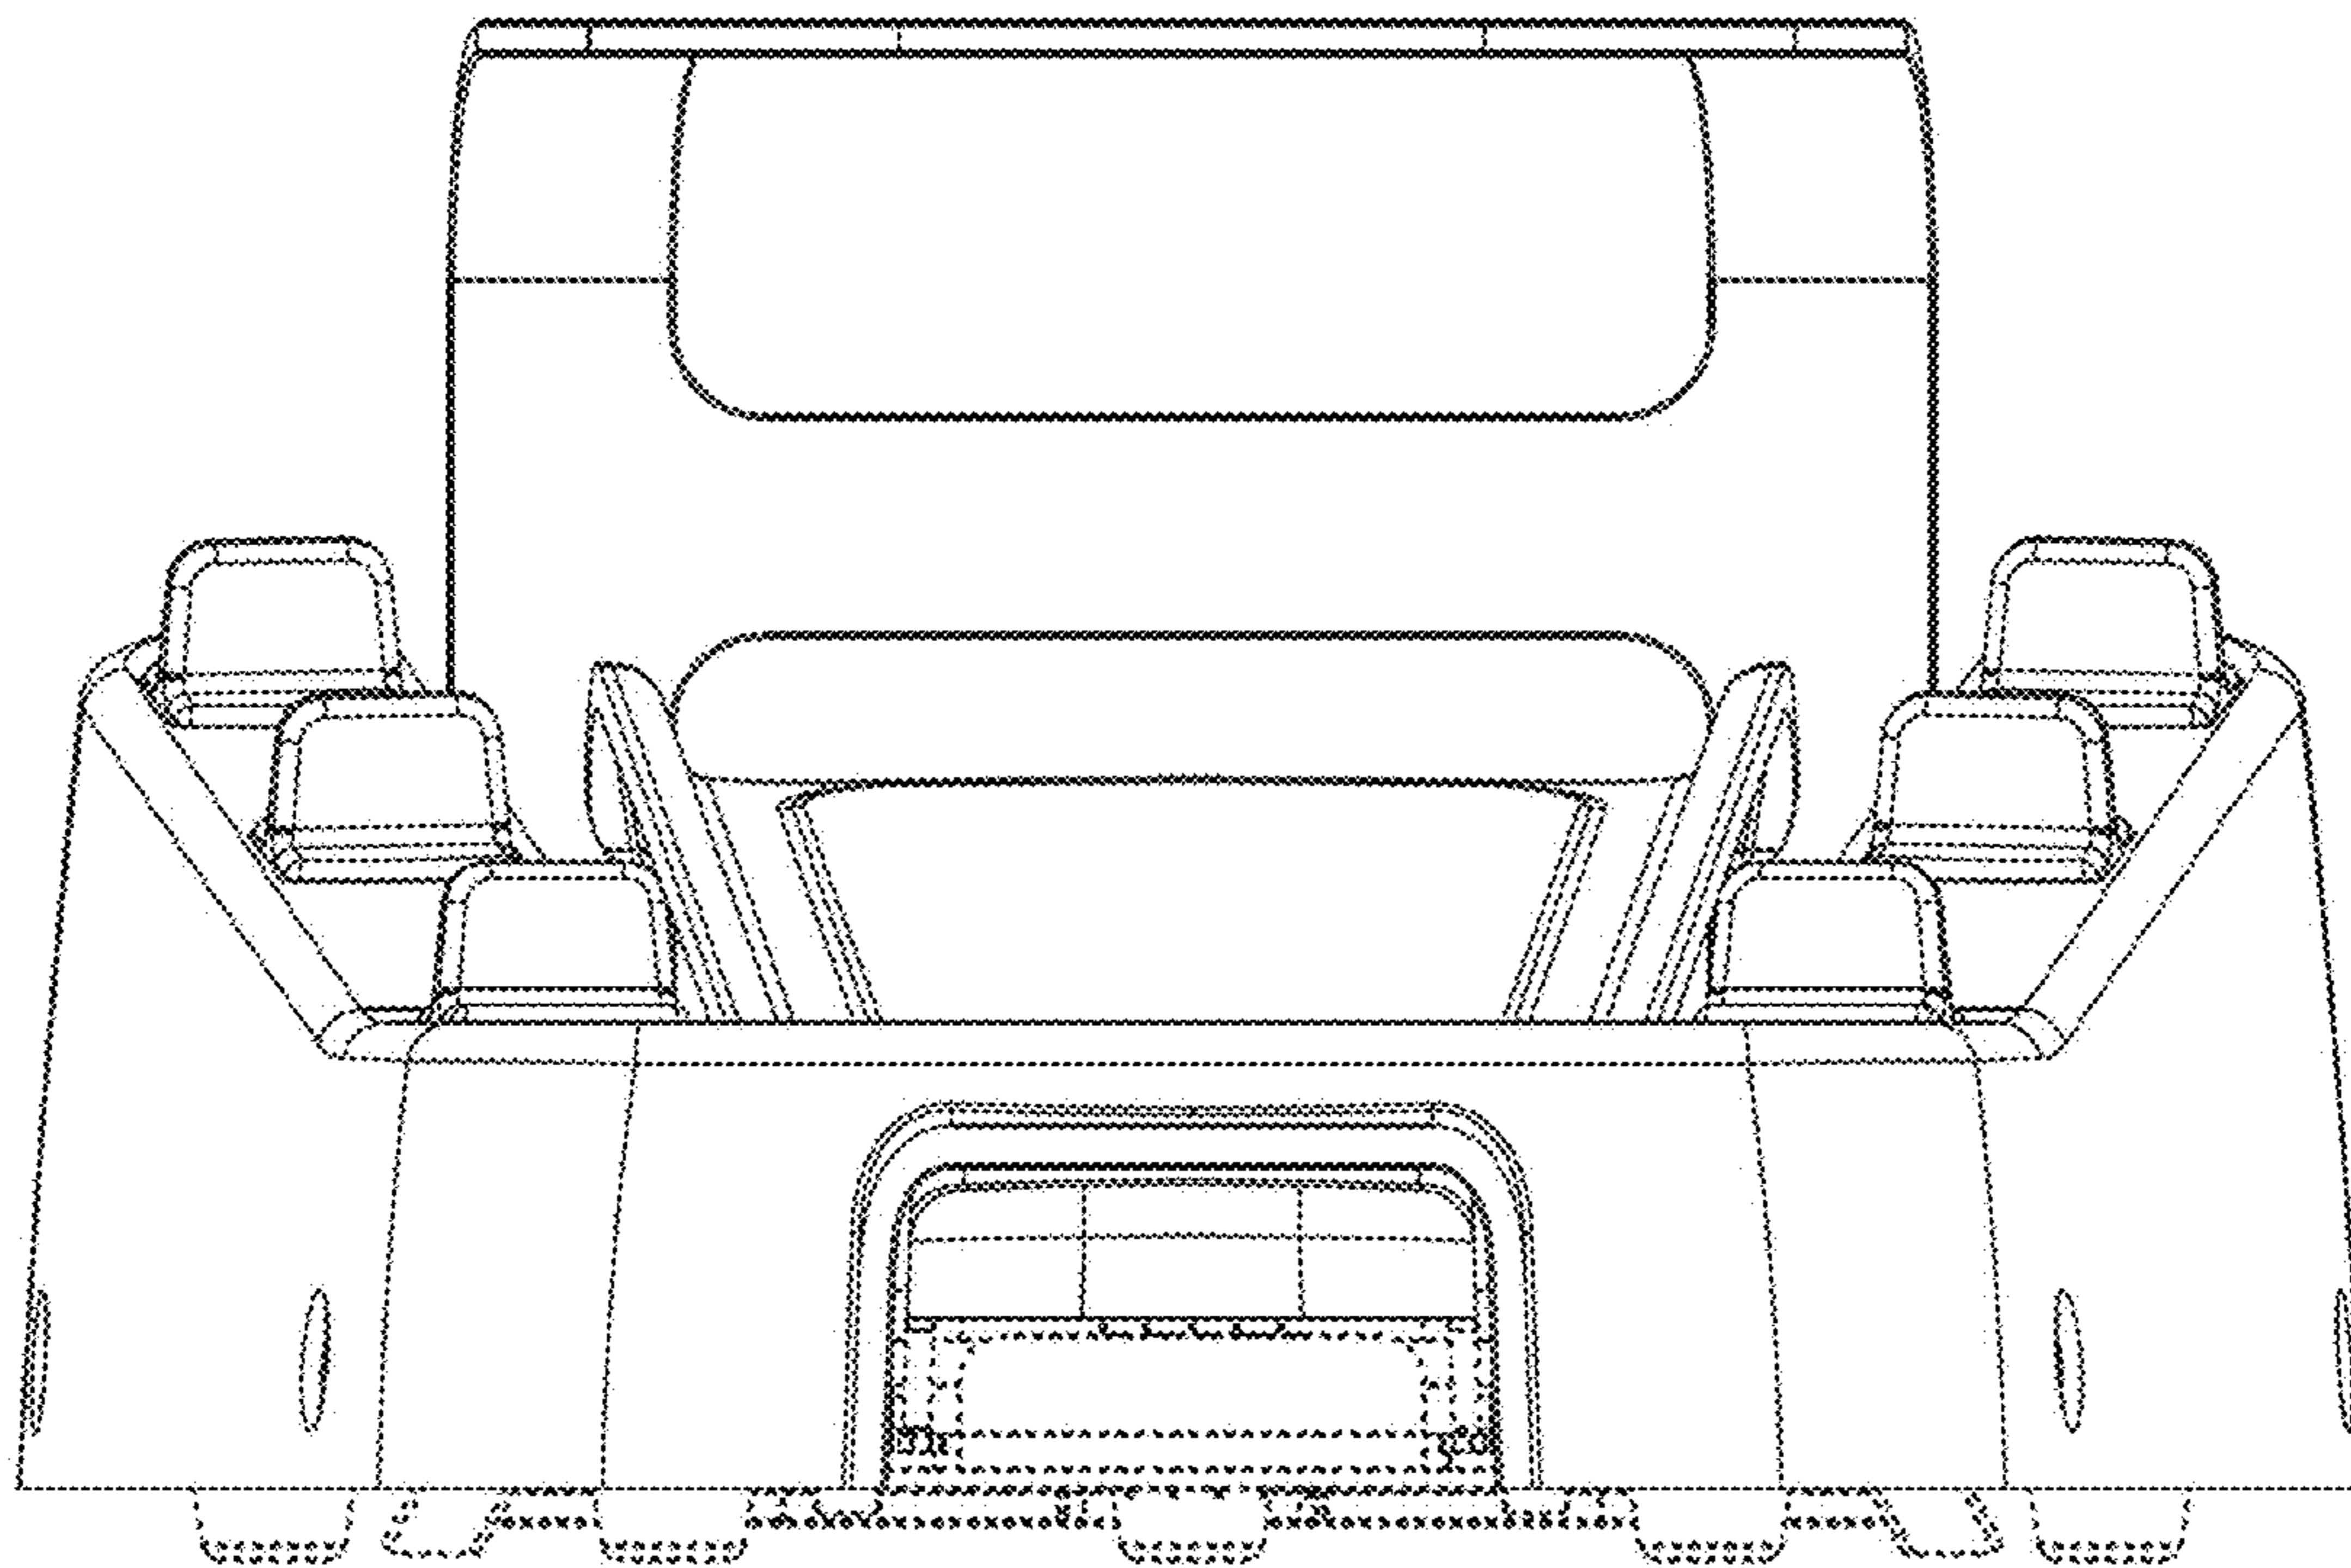


FIG. 4

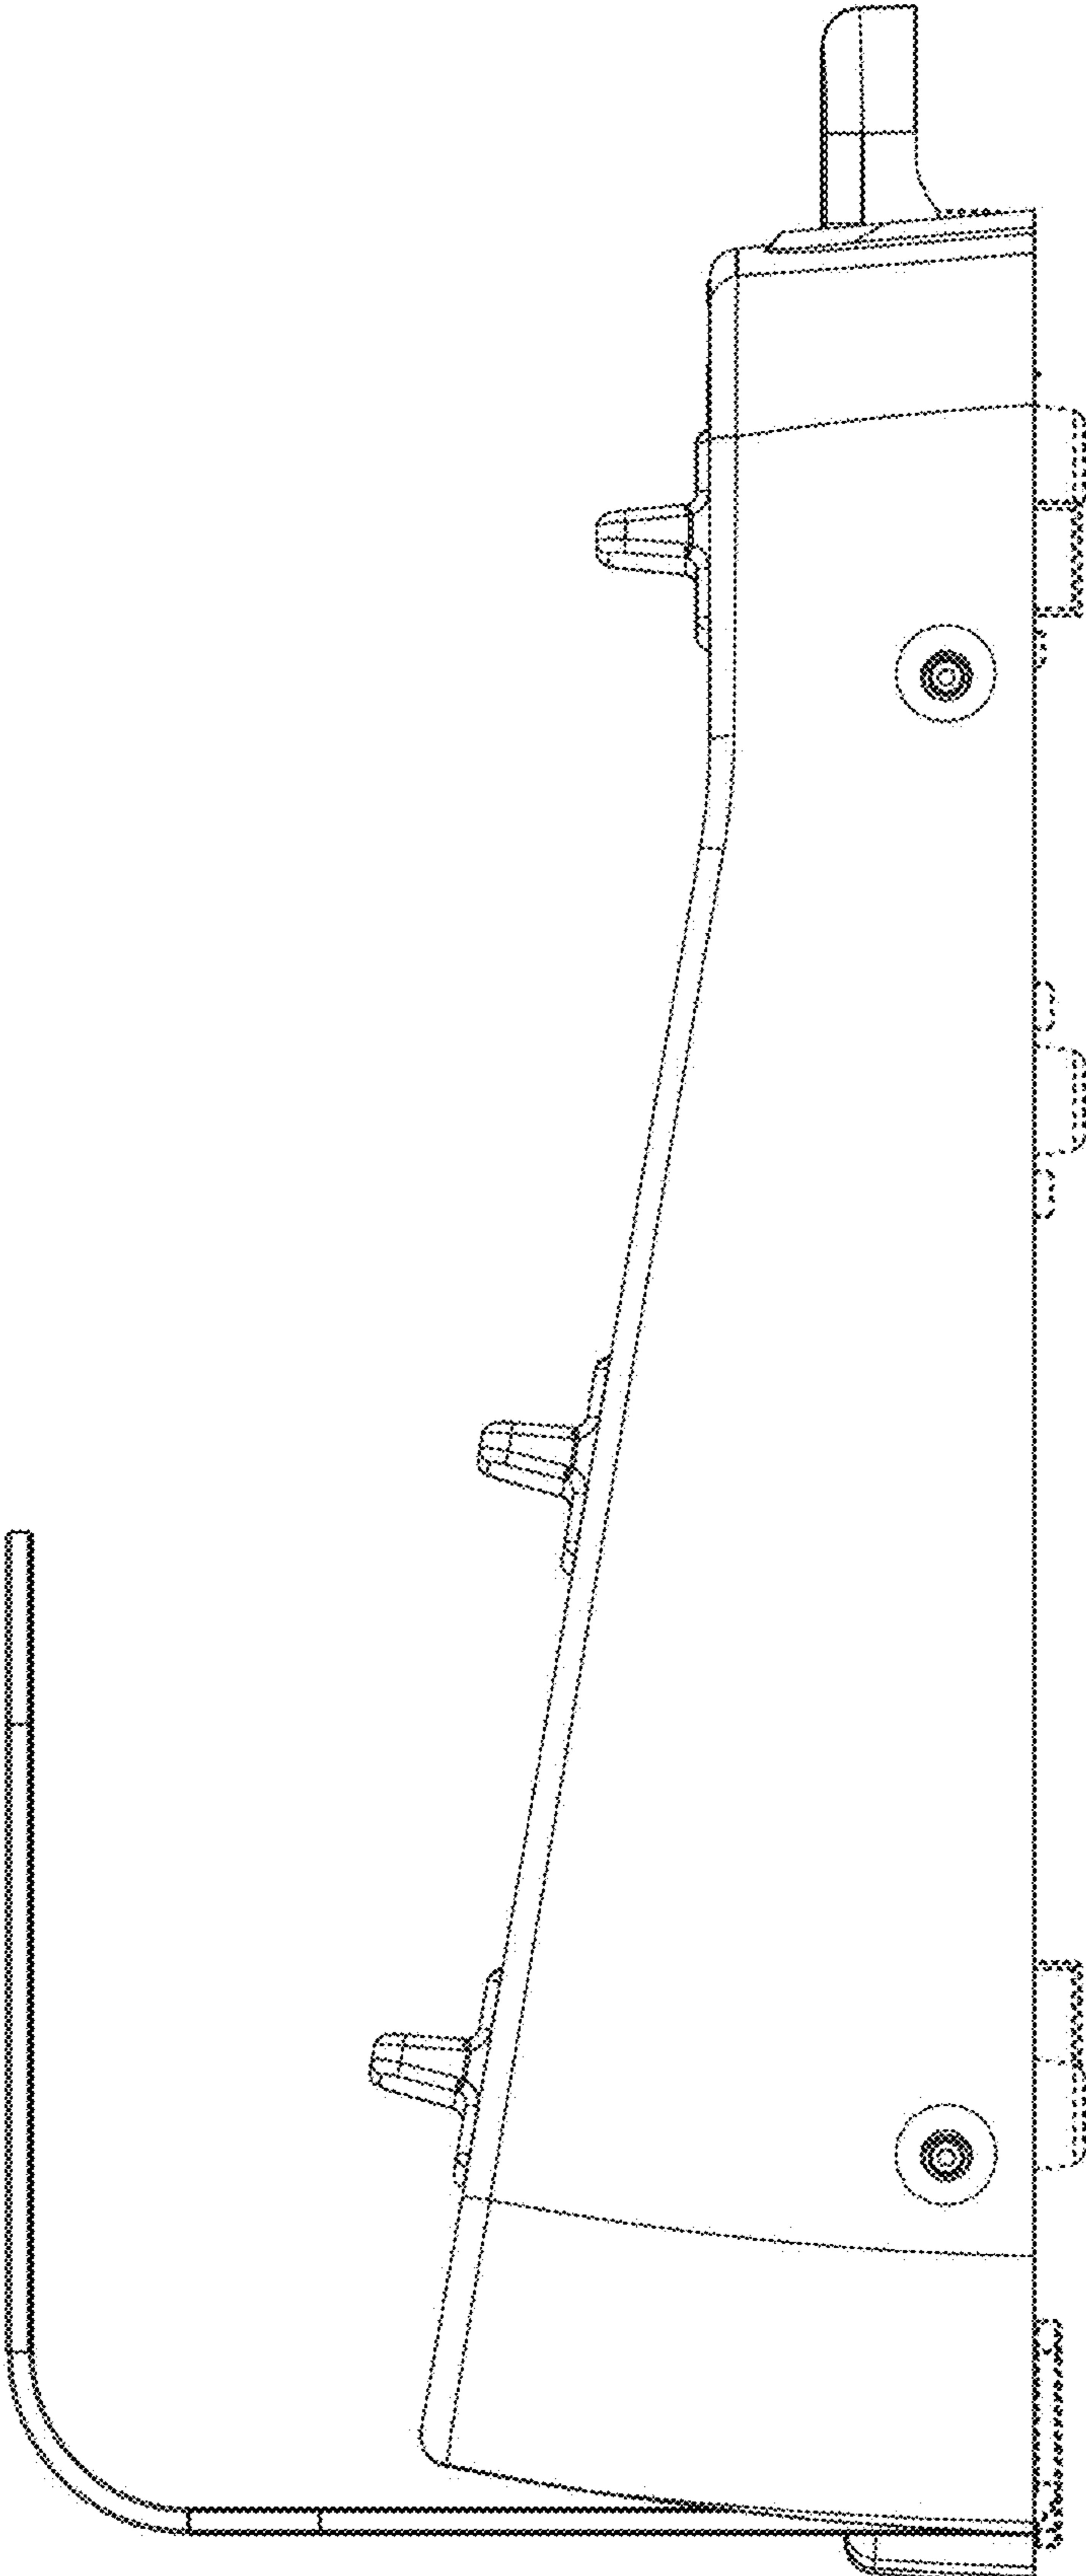


FIG. 5

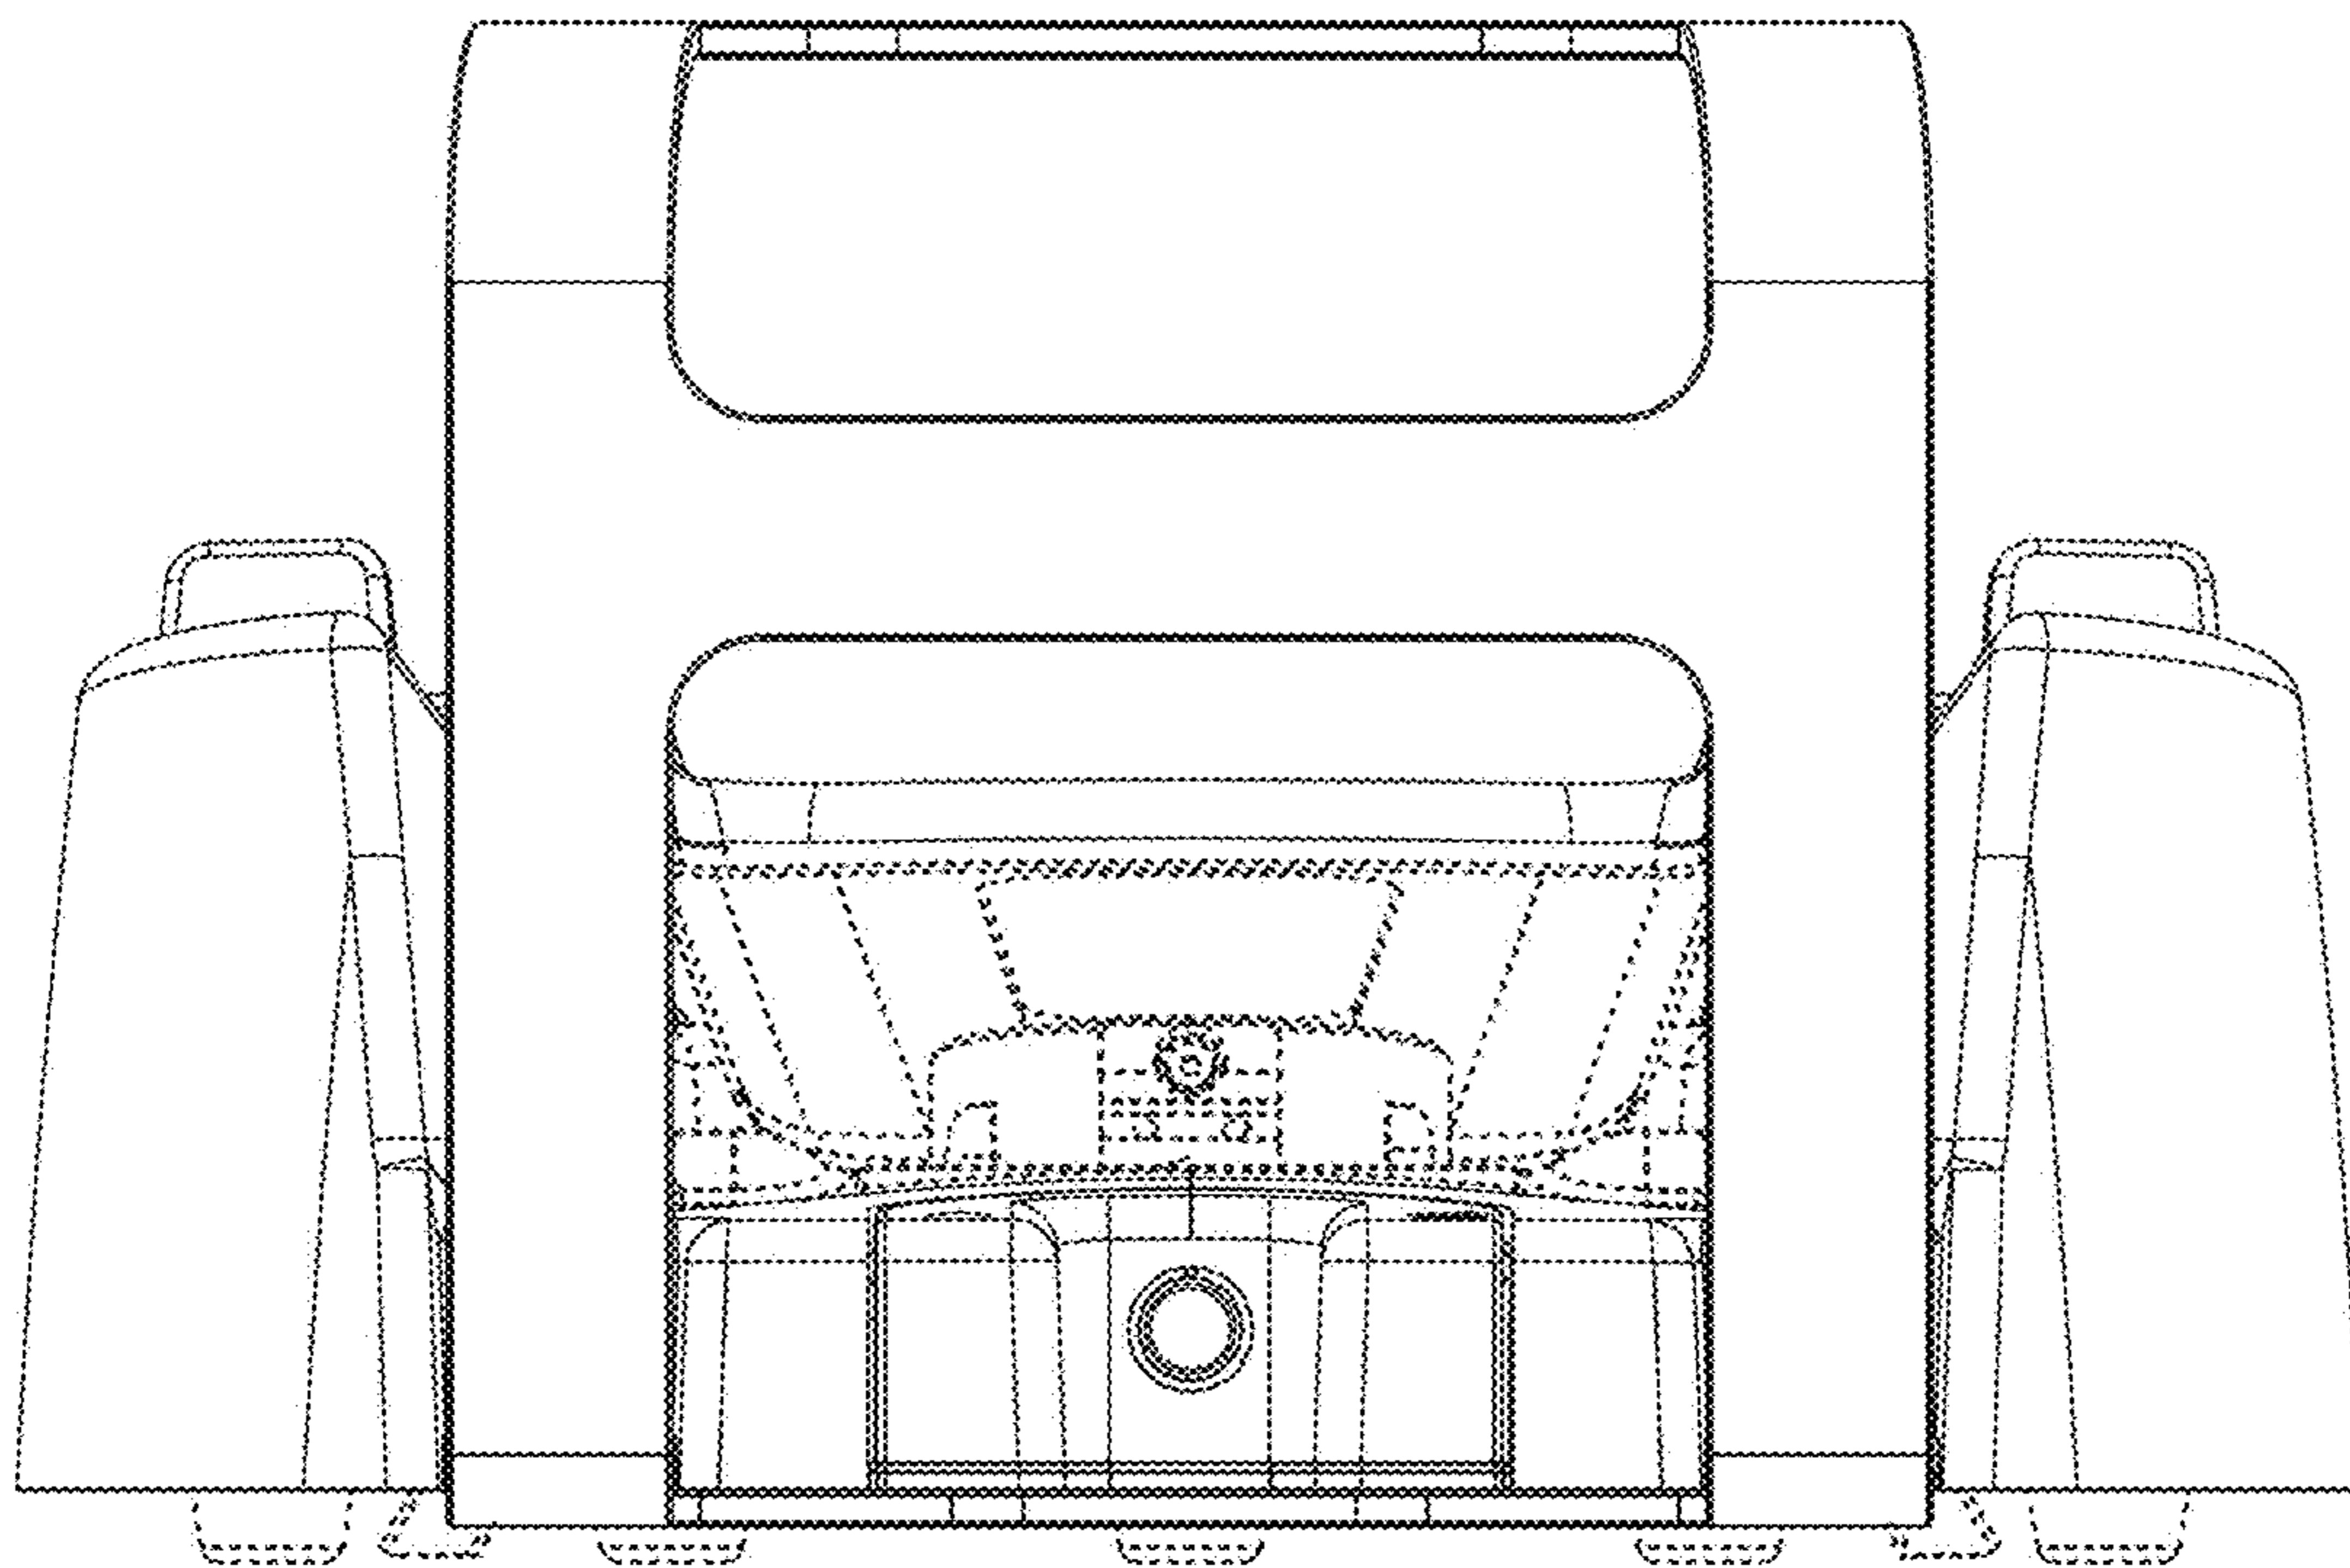


FIG. 6

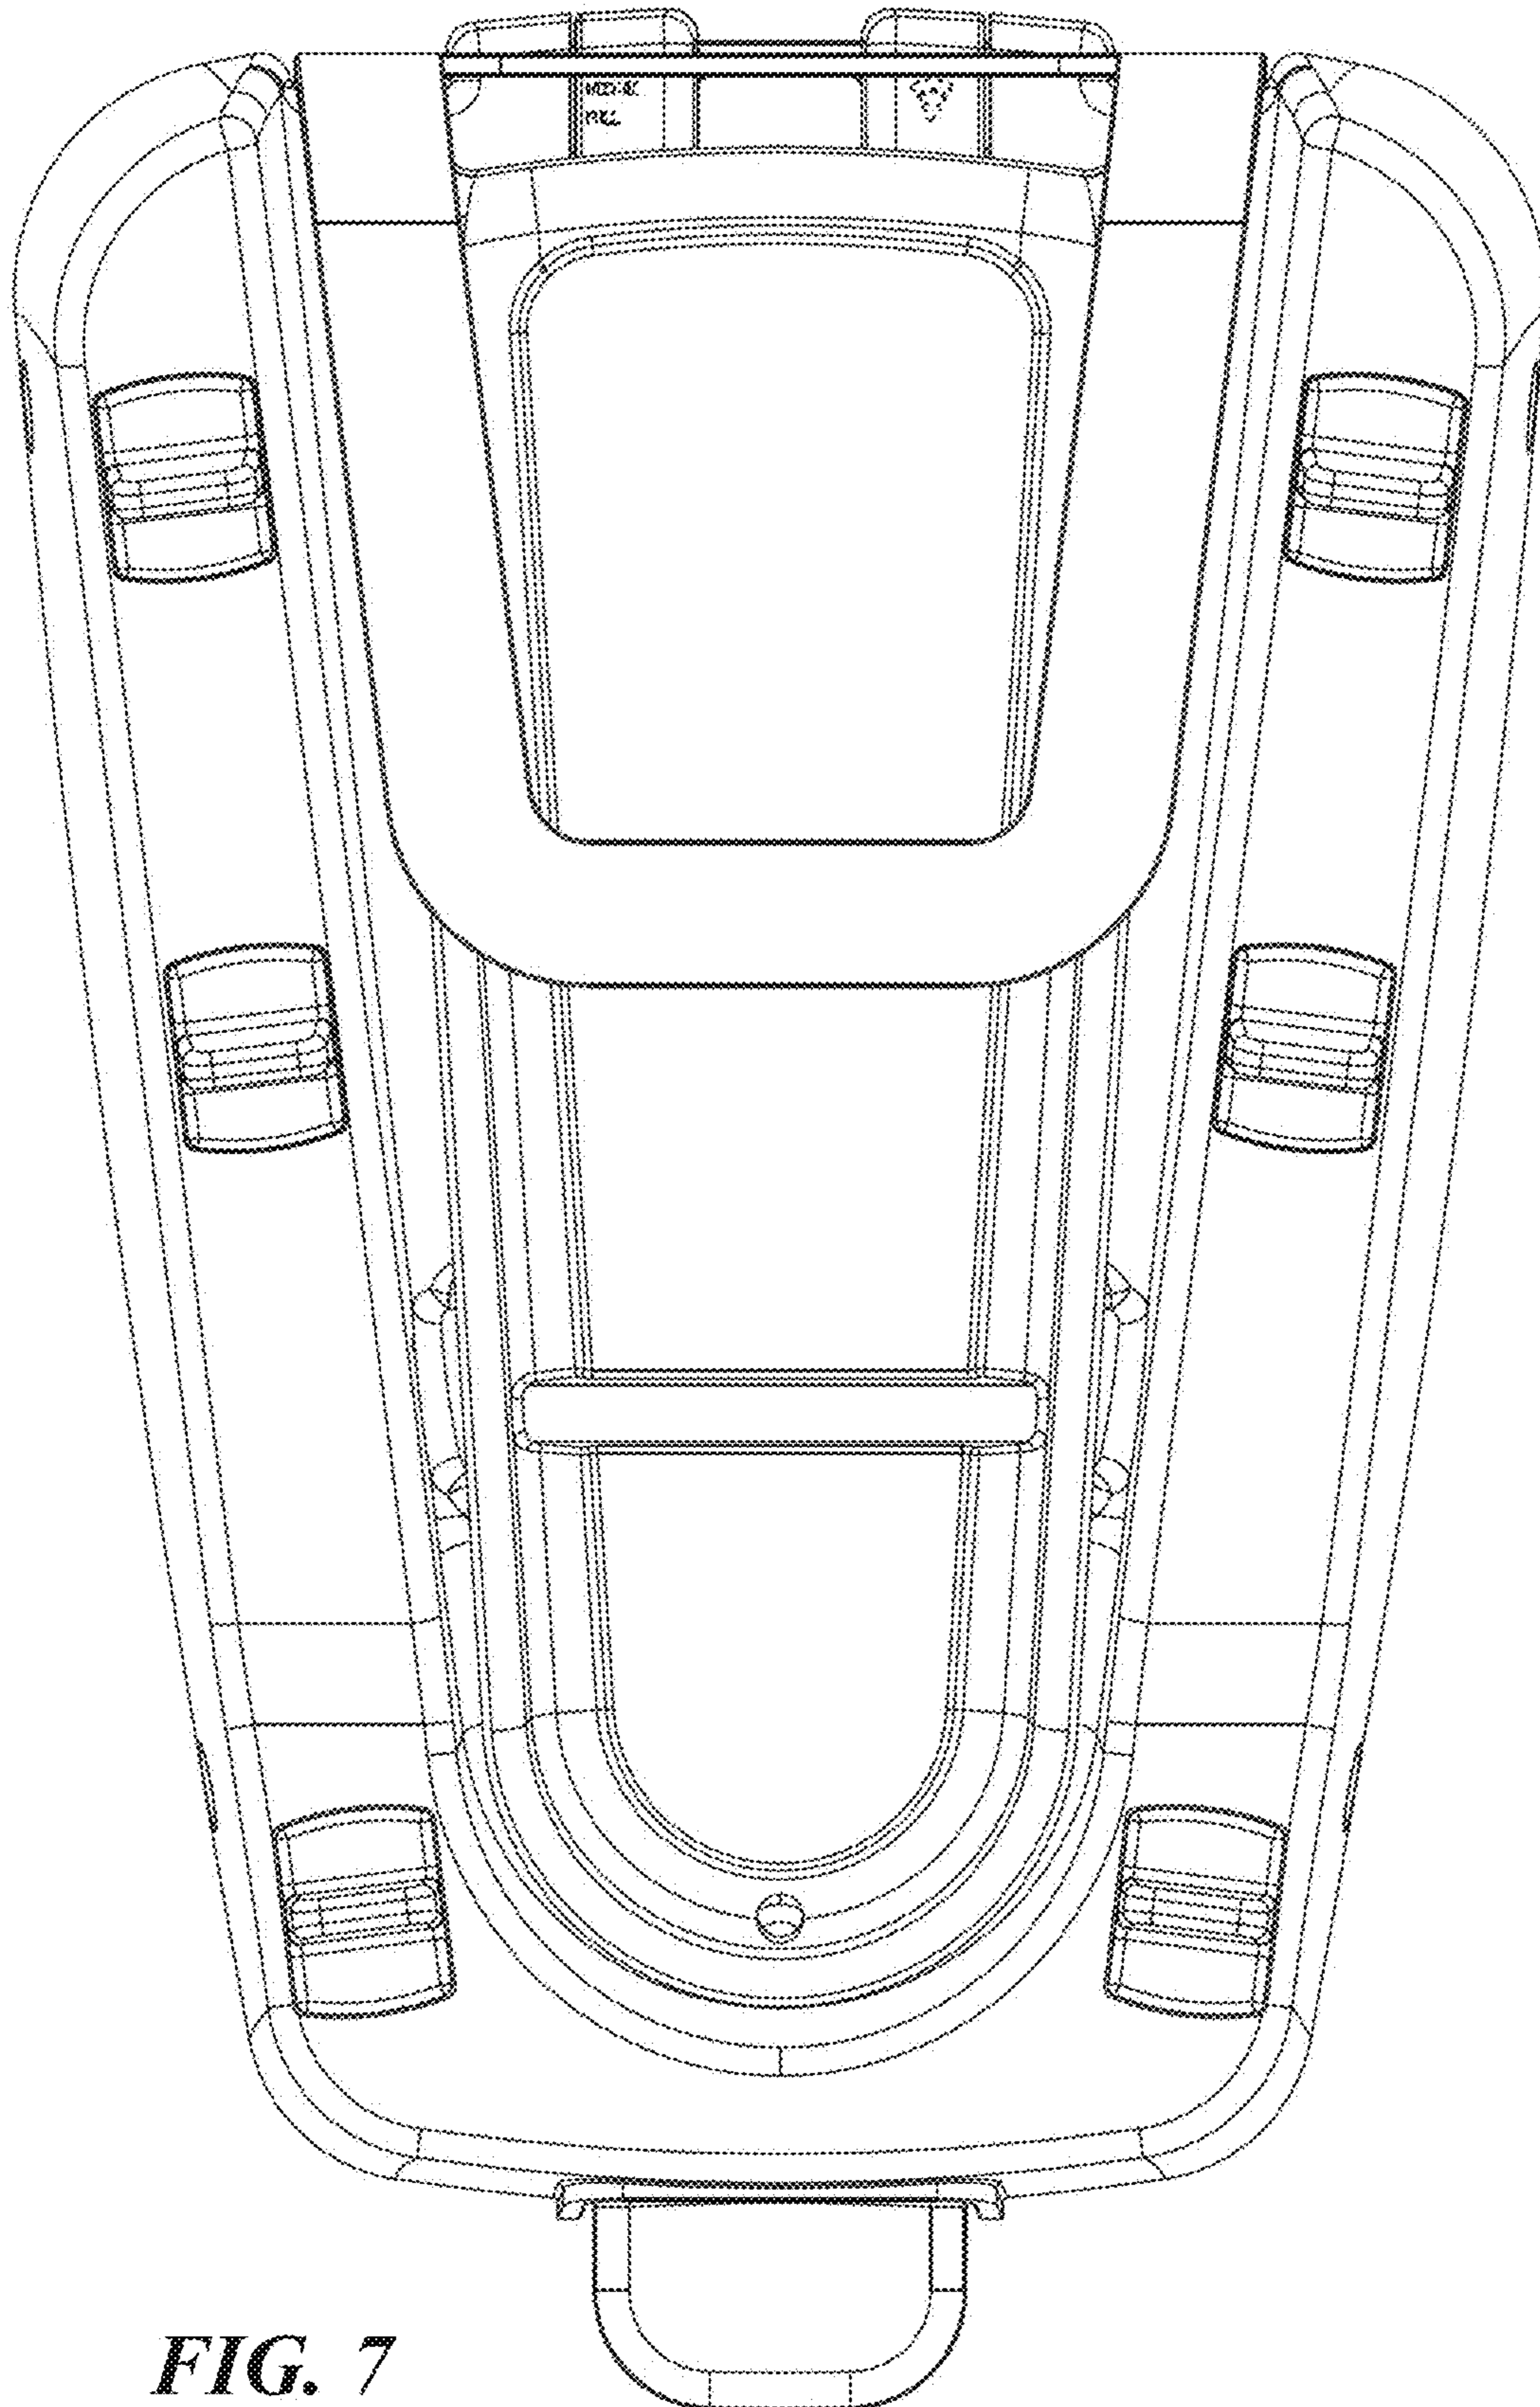


FIG. 7