



US00D873430S

(12) **United States Design Patent**
Accolla

(10) **Patent No.:** **US D873,430 S**
(45) **Date of Patent:** **** Jan. 21, 2020**

(54) **BIO-SPECTRUM THERAPEUTIC APPARATUS**

(71) Applicant: **Lin Zhou**, Beijing (CN)
(72) Inventor: **Avril Accolla**, Shanghai (CN)
(73) Assignee: **Lin Zhou**, Beijing (CN)
(**) Term: **15 Years**

(21) Appl. No.: **29/633,443**

(22) Filed: **Jan. 13, 2018**

(30) **Foreign Application Priority Data**

Jul. 13, 2017 (CN) 2017 3 0308591

(51) **LOC (12) Cl.** **28-03**

(52) **U.S. Cl.**
USPC **D24/209**

(58) **Field of Classification Search**
USPC D24/107, 186, 158, 231, 200, 209, 210,
D24/214, 215; D26/37-39; D10/81
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D240,082 S * 5/1976 Garwood D24/210
D259,738 S * 6/1981 Boschetti D24/210
(Continued)

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Gokalp Bayramoglu

(57) **CLAIM**


The ornamental design for a bio-spectrum therapeutic apparatus, as shown and described.

DESCRIPTION

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application

publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee. The color shown on the claimed design forms no part thereof. FIG. 1 is a front view of a bio-spectrum therapeutic apparatus showing the new design; FIG. 2 is a rear view of the bio-spectrum therapeutic apparatus; FIG. 3 is a left side view of the bio-spectrum therapeutic apparatus; FIG. 4 is a right side view of the bio-spectrum therapeutic apparatus; FIG. 5 is a top view of the bio-spectrum therapeutic apparatus; FIG. 6 is a bottom view of the bio-spectrum therapeutic apparatus; FIG. 7 is a perspective view of the bio-spectrum therapeutic apparatus; FIG. 8 is a perspective view of the bio-spectrum therapeutic apparatus in close state; FIG. 9 is a perspective view of the bio-spectrum therapeutic apparatus in open state; FIG. 10 is a perspective view of the bio-spectrum therapeutic apparatus when the light is on; FIG. 11 is a perspective view of the bio-spectrum therapeutic apparatus showing the remote control and the bio-spectrum therapeutic apparatus separately; FIG. 12 is another perspective view of the bio-spectrum therapeutic apparatus; FIG. 13 is another perspective view of the bio-spectrum therapeutic apparatus in close state; FIG. 14 is another perspective view of the bio-spectrum therapeutic apparatus in open state; FIG. 15 is another perspective view of the bio-spectrum therapeutic apparatus when the light is on; FIG. 16 is an enlarged view of portion 16 shown in FIG. 11; and, FIG. 17 is an enlarged view of portion 17 shown in FIG. 11.

1 Claim, 17 Drawing Sheets
(17 of 17 Drawing Sheet(s) Filed in Color)

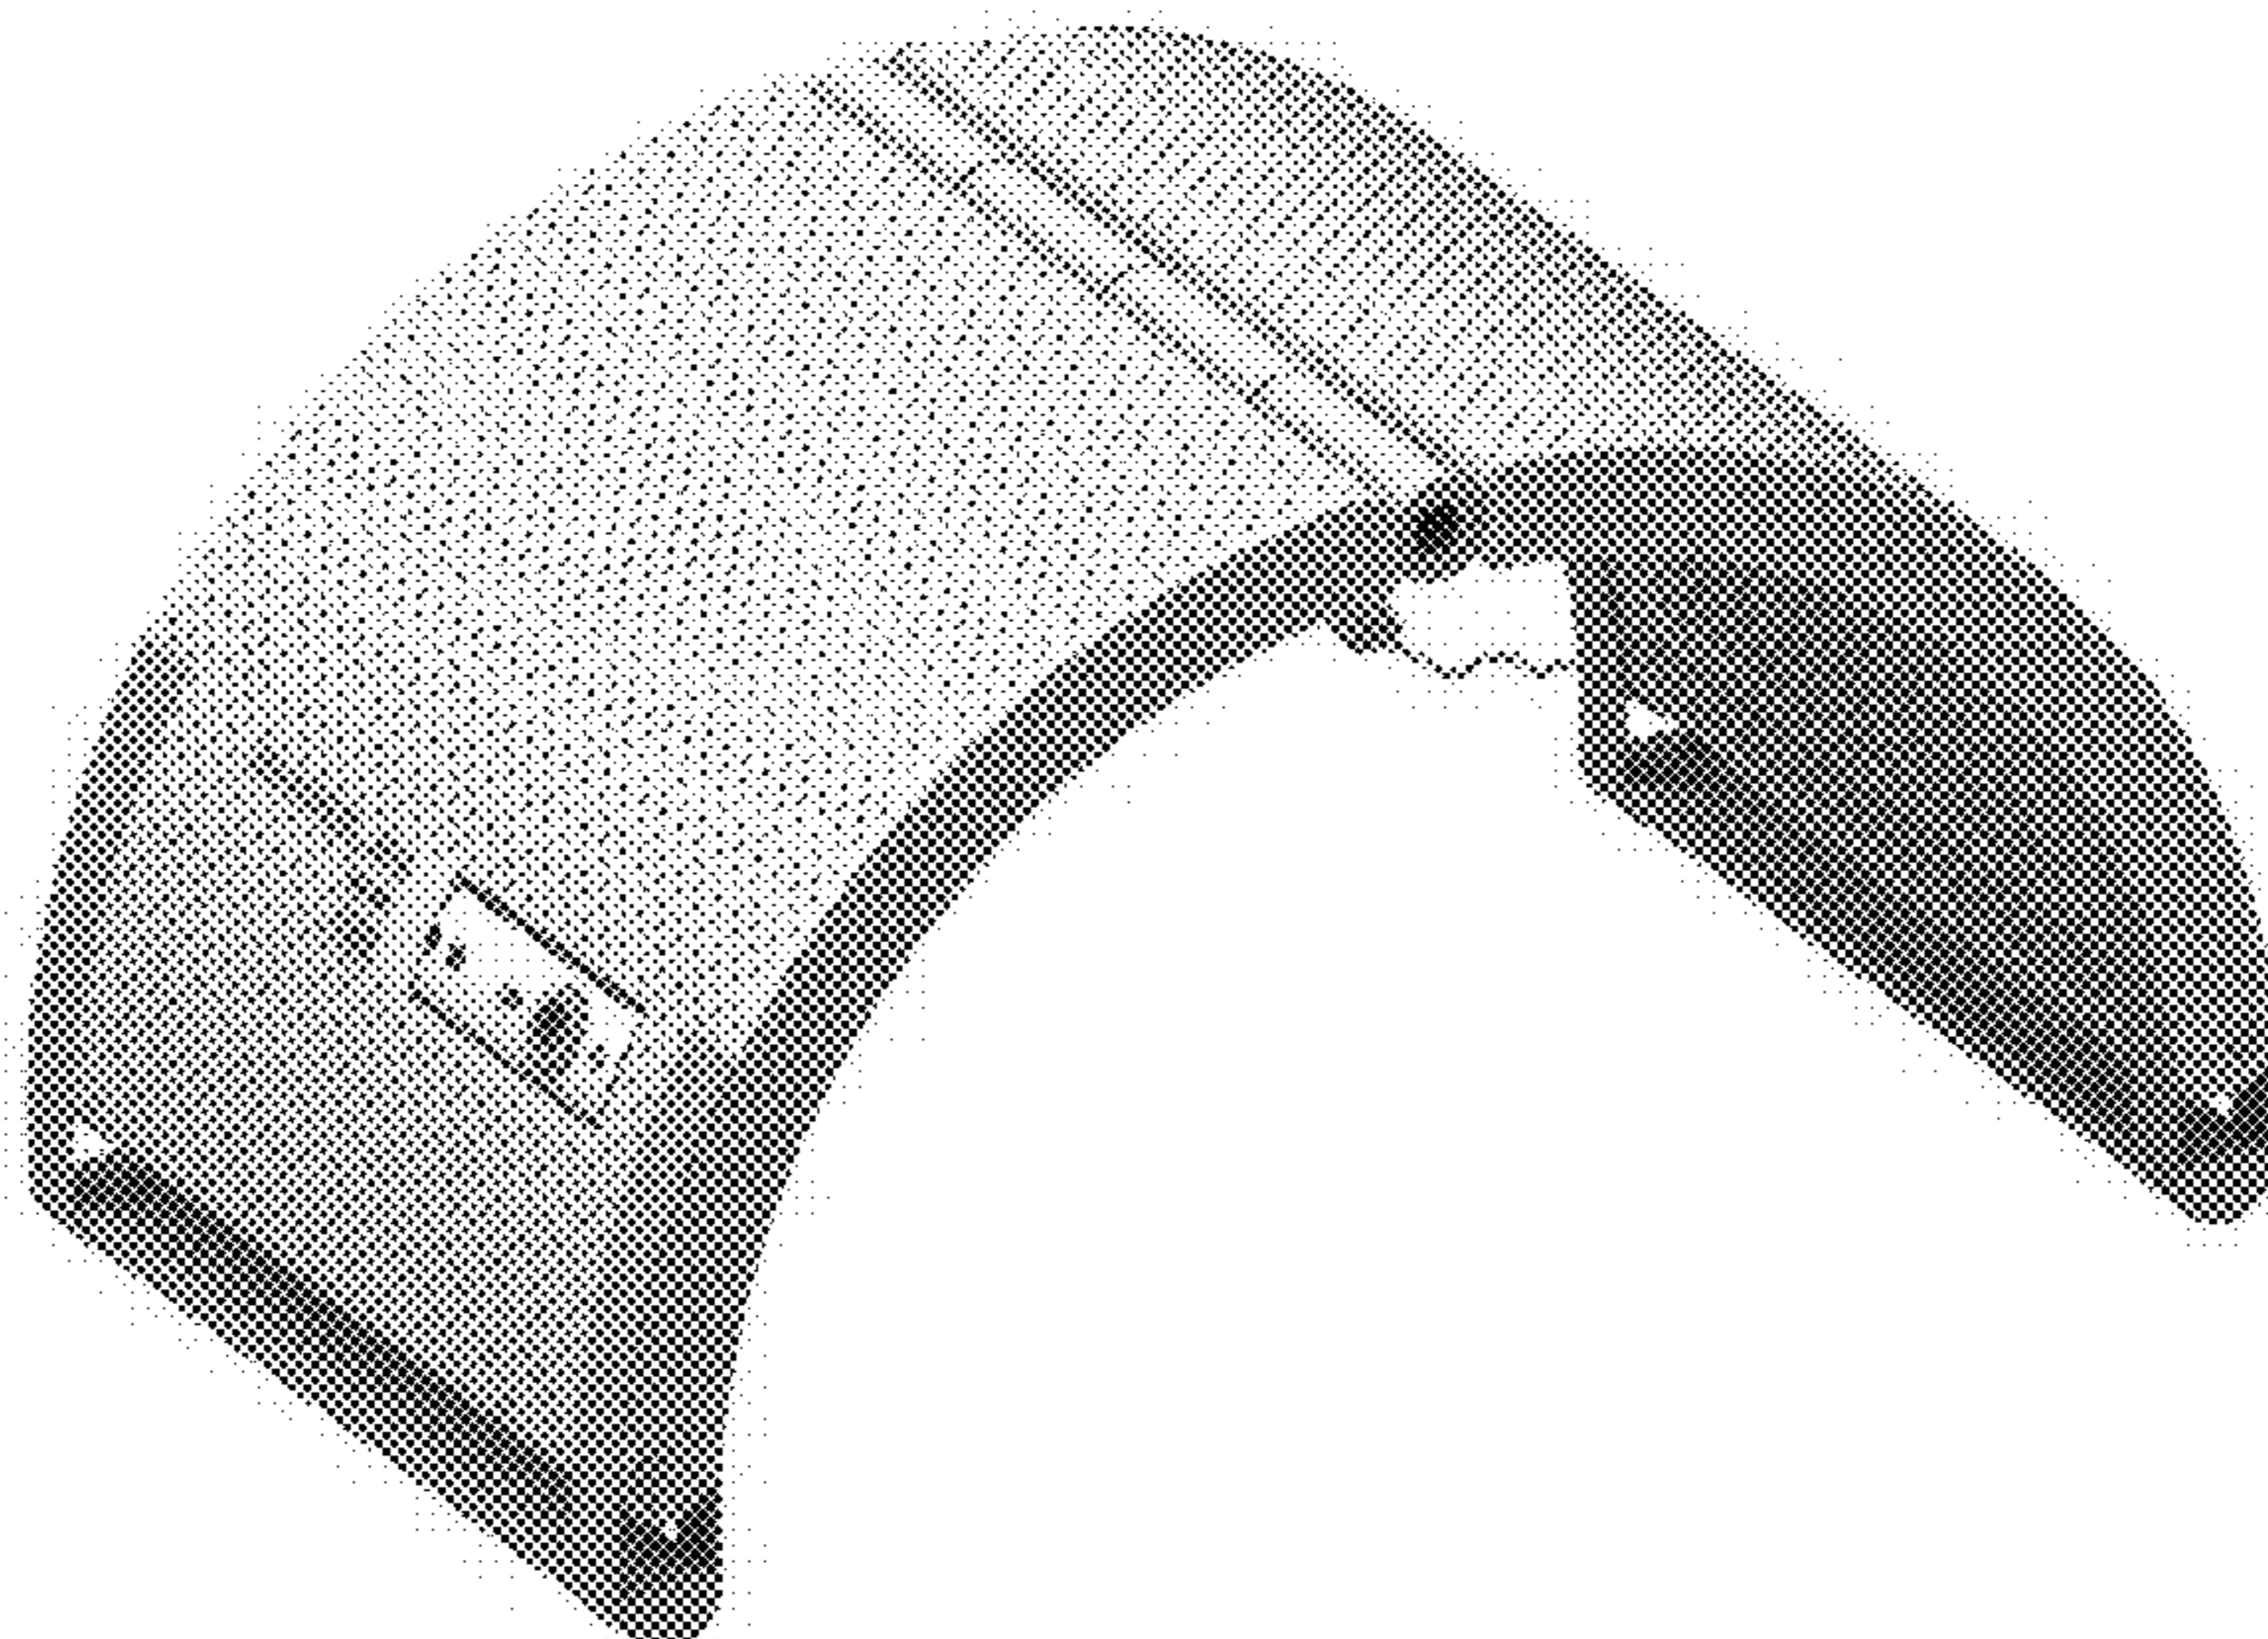

(58) **Field of Classification Search**

CPC .. A61N 5/0616; A61N 5/0617; A61N 5/0618;
A61N 5/062; A61N 5/0627; A61N
5/0624; A61N 5/0625; A61N 2005/0643;
A61N 2005/0644; A61N 2005/0645;
A61N 2005/0647; A61N 2005/0651;
A61N 2005/0652; A61N 2005/0654;
A61N 2005/0662; A61B 2018/00452;
A61B 2018/1807

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D260,176 S * 8/1981 Boschetti D24/210
6,598,994 B1 * 7/2003 Tait G01B 11/00
362/11
D505,207 S * 5/2005 Waldmann D24/210
D517,699 S * 3/2006 Lansohn D24/210
D650,486 S * 12/2011 Cowan D24/209
D711,545 S * 8/2014 Soltész-Nagy D24/210
D712,560 S * 9/2014 Soltész-Nagy D24/209
D804,047 S * 11/2017 Michaels D24/209
D831,839 S * 10/2018 Pelletier D24/209
2004/0122492 A1 * 6/2004 Harth A61N 5/0613
607/88
2009/0005839 A1 * 1/2009 Griffith A61N 5/0614
607/91

* cited by examiner

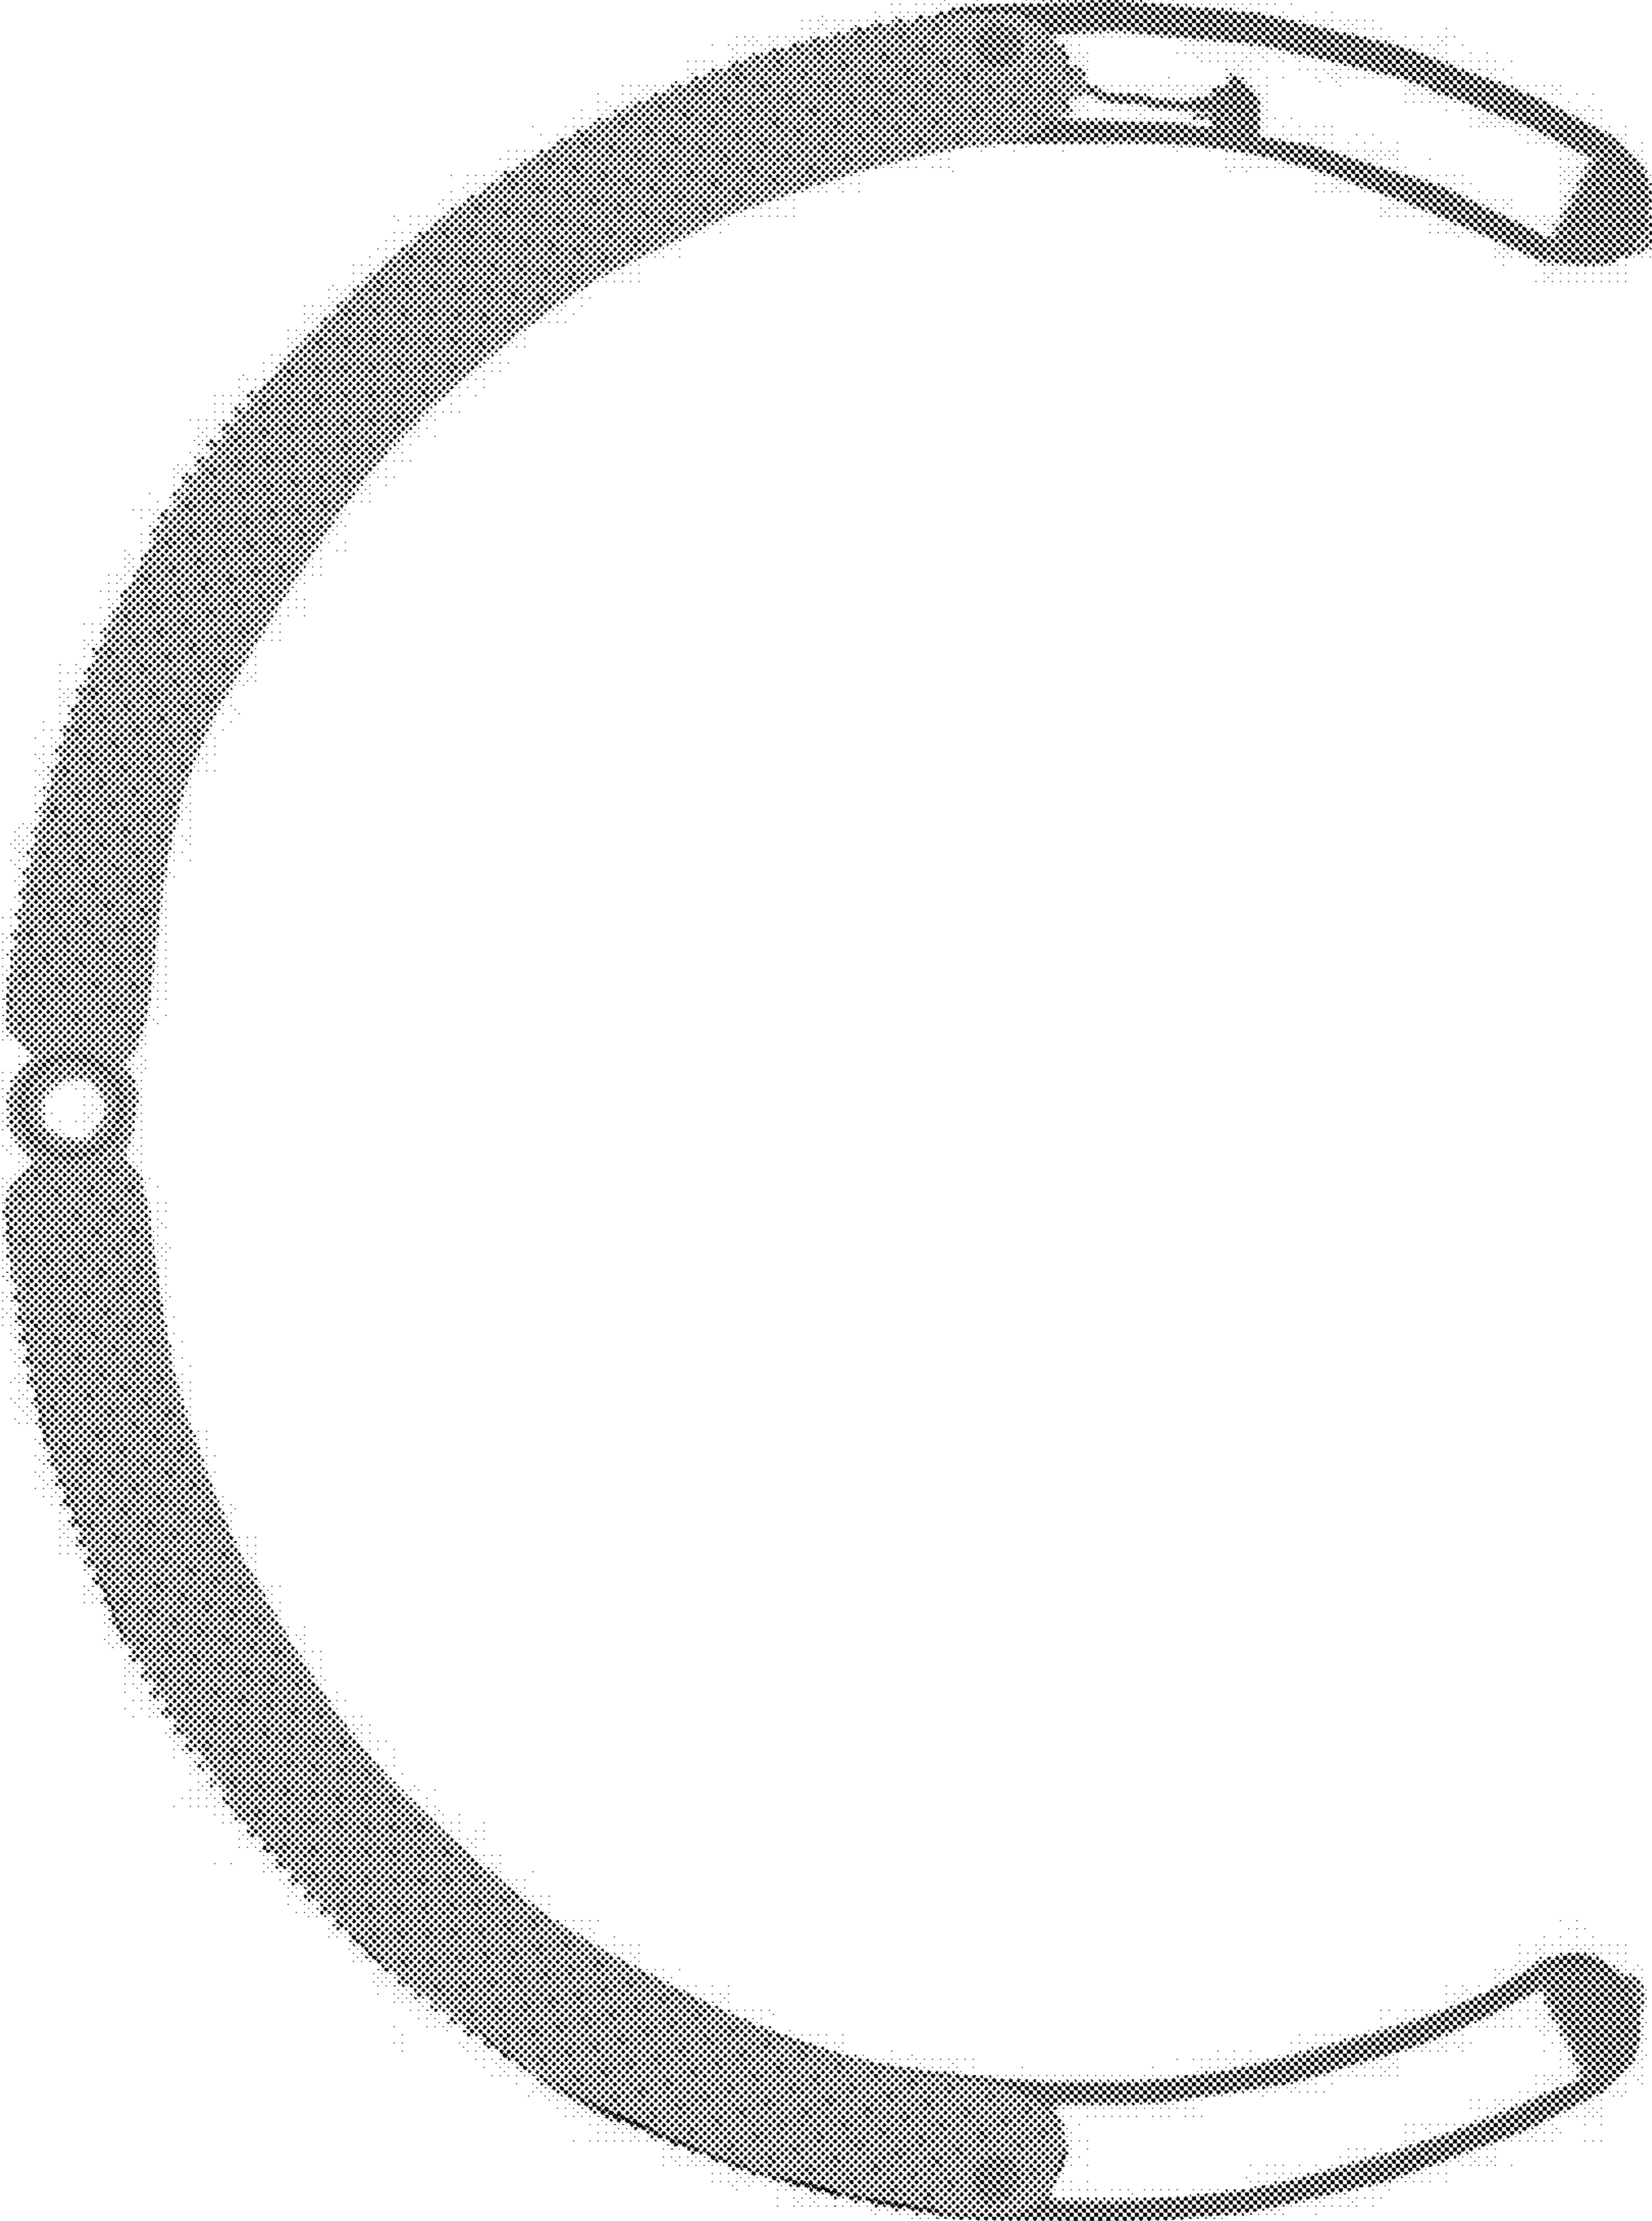


FIG. 1

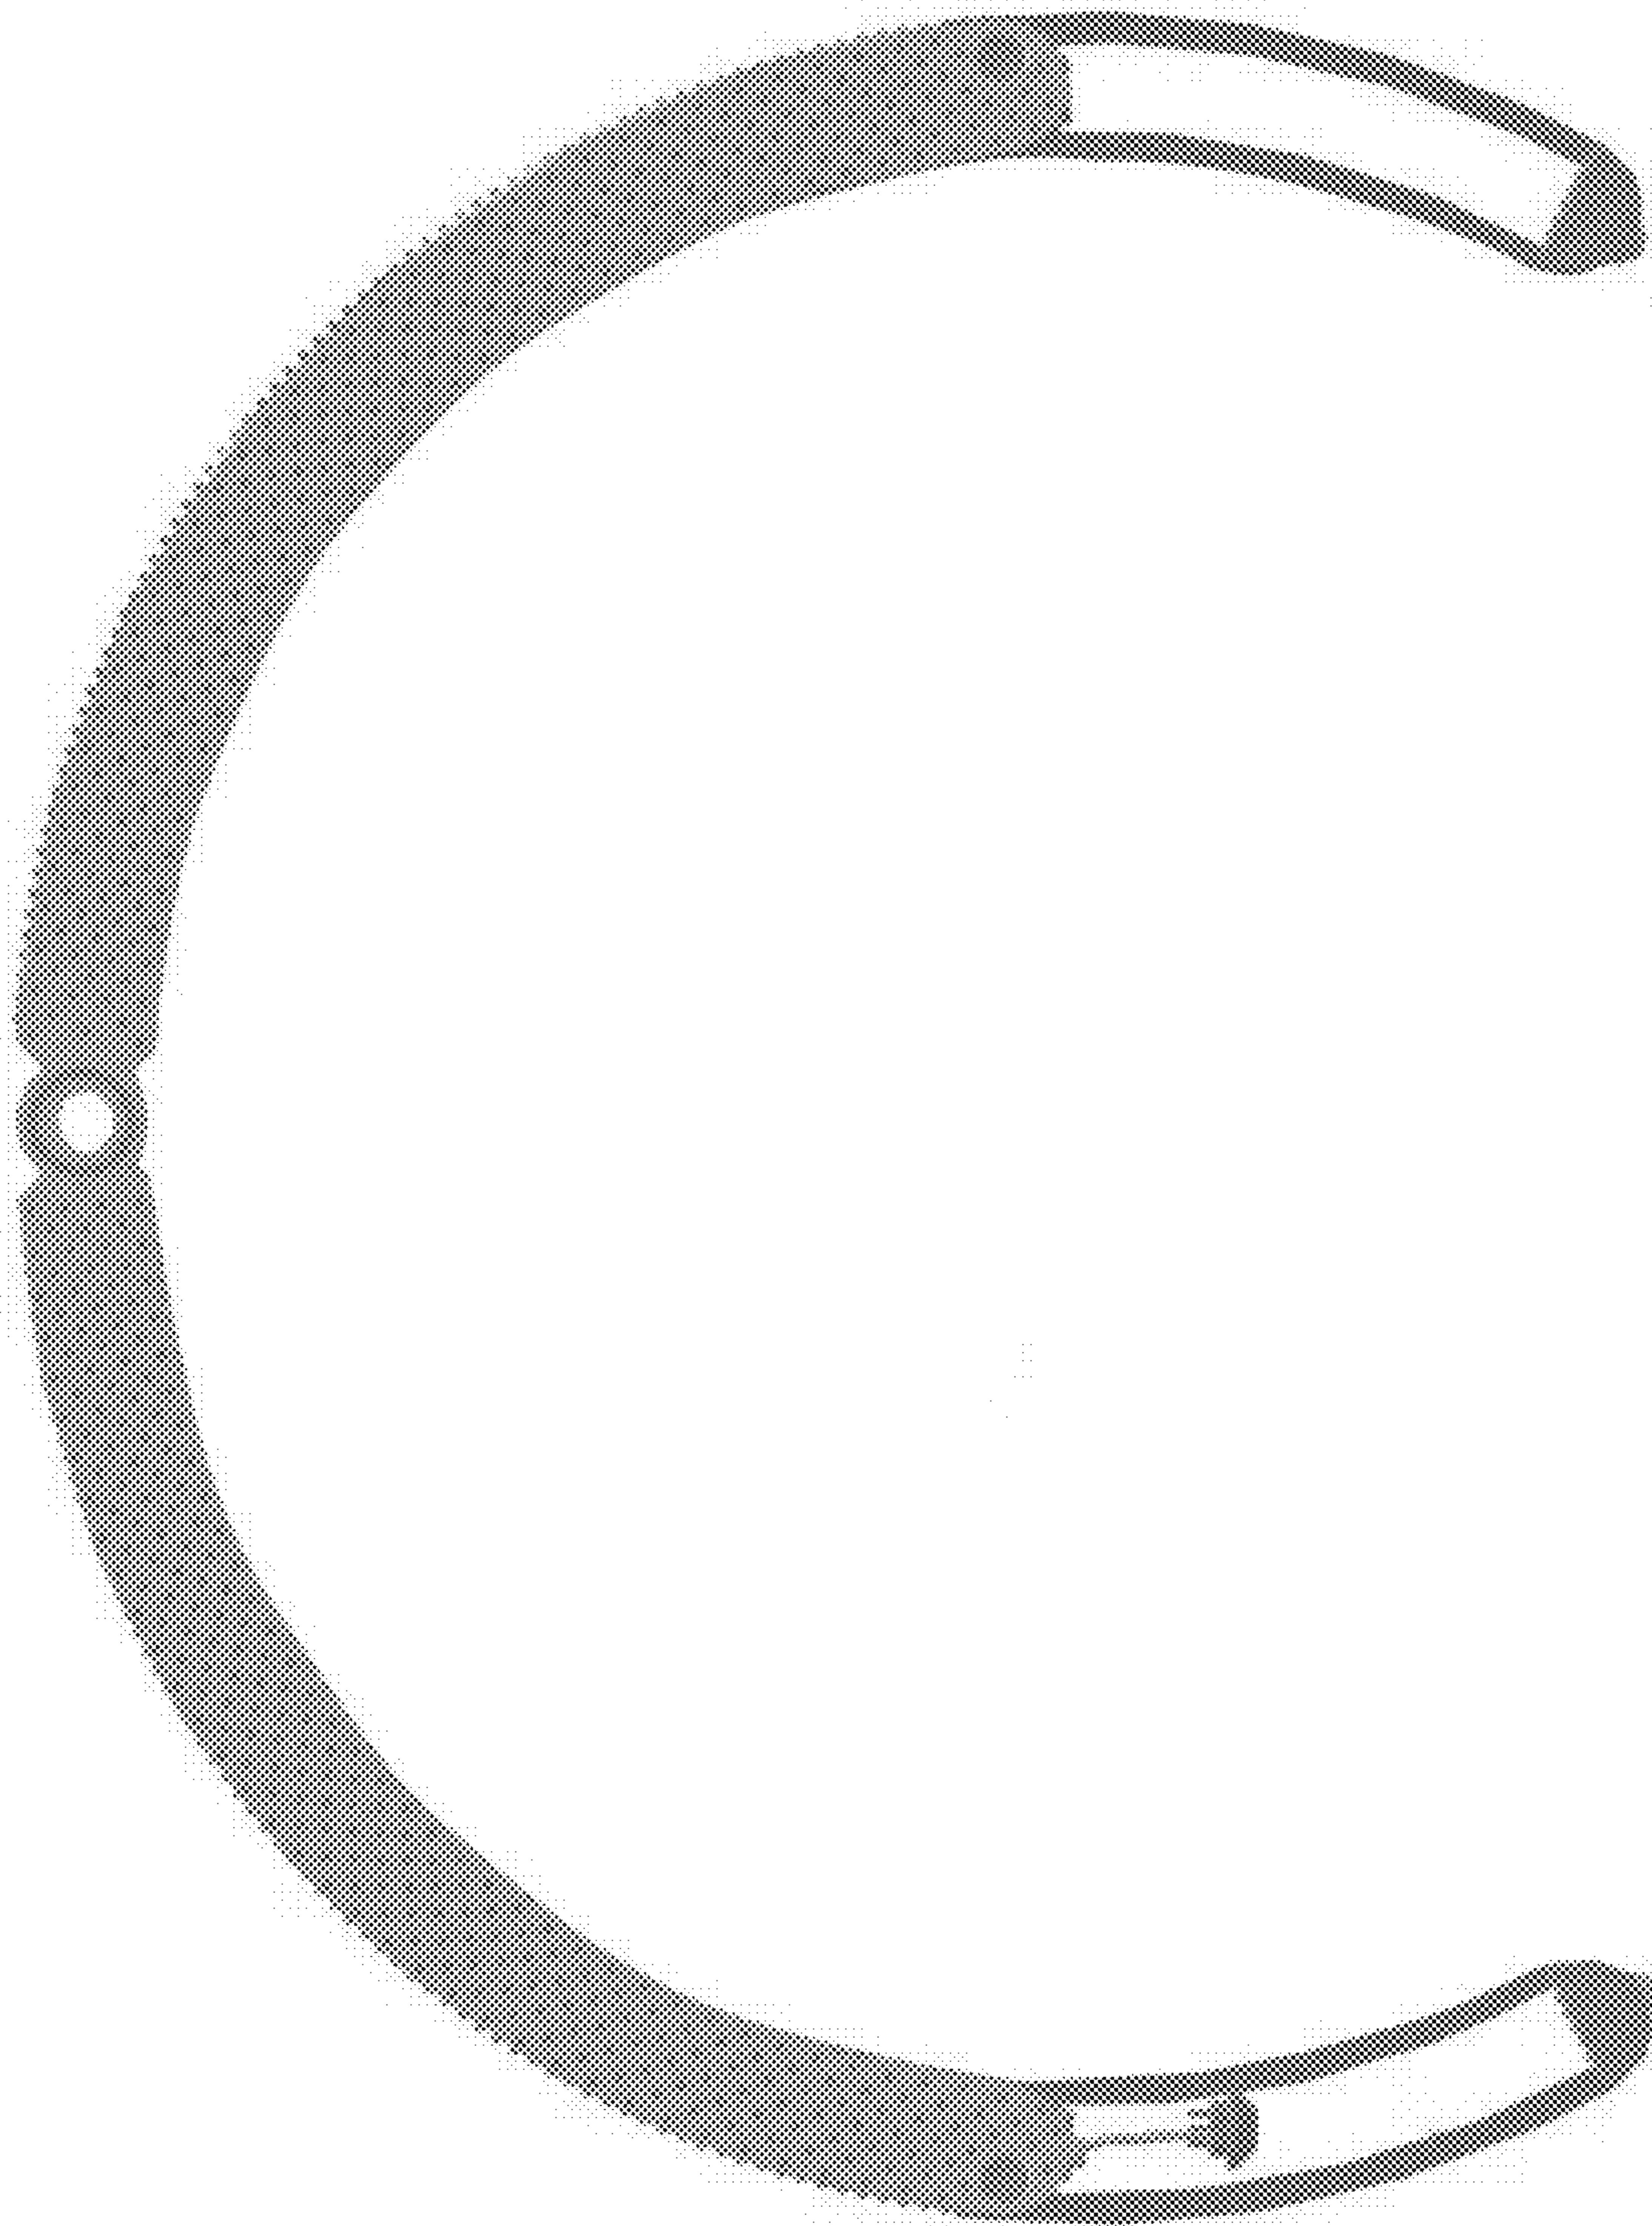


FIG. 2

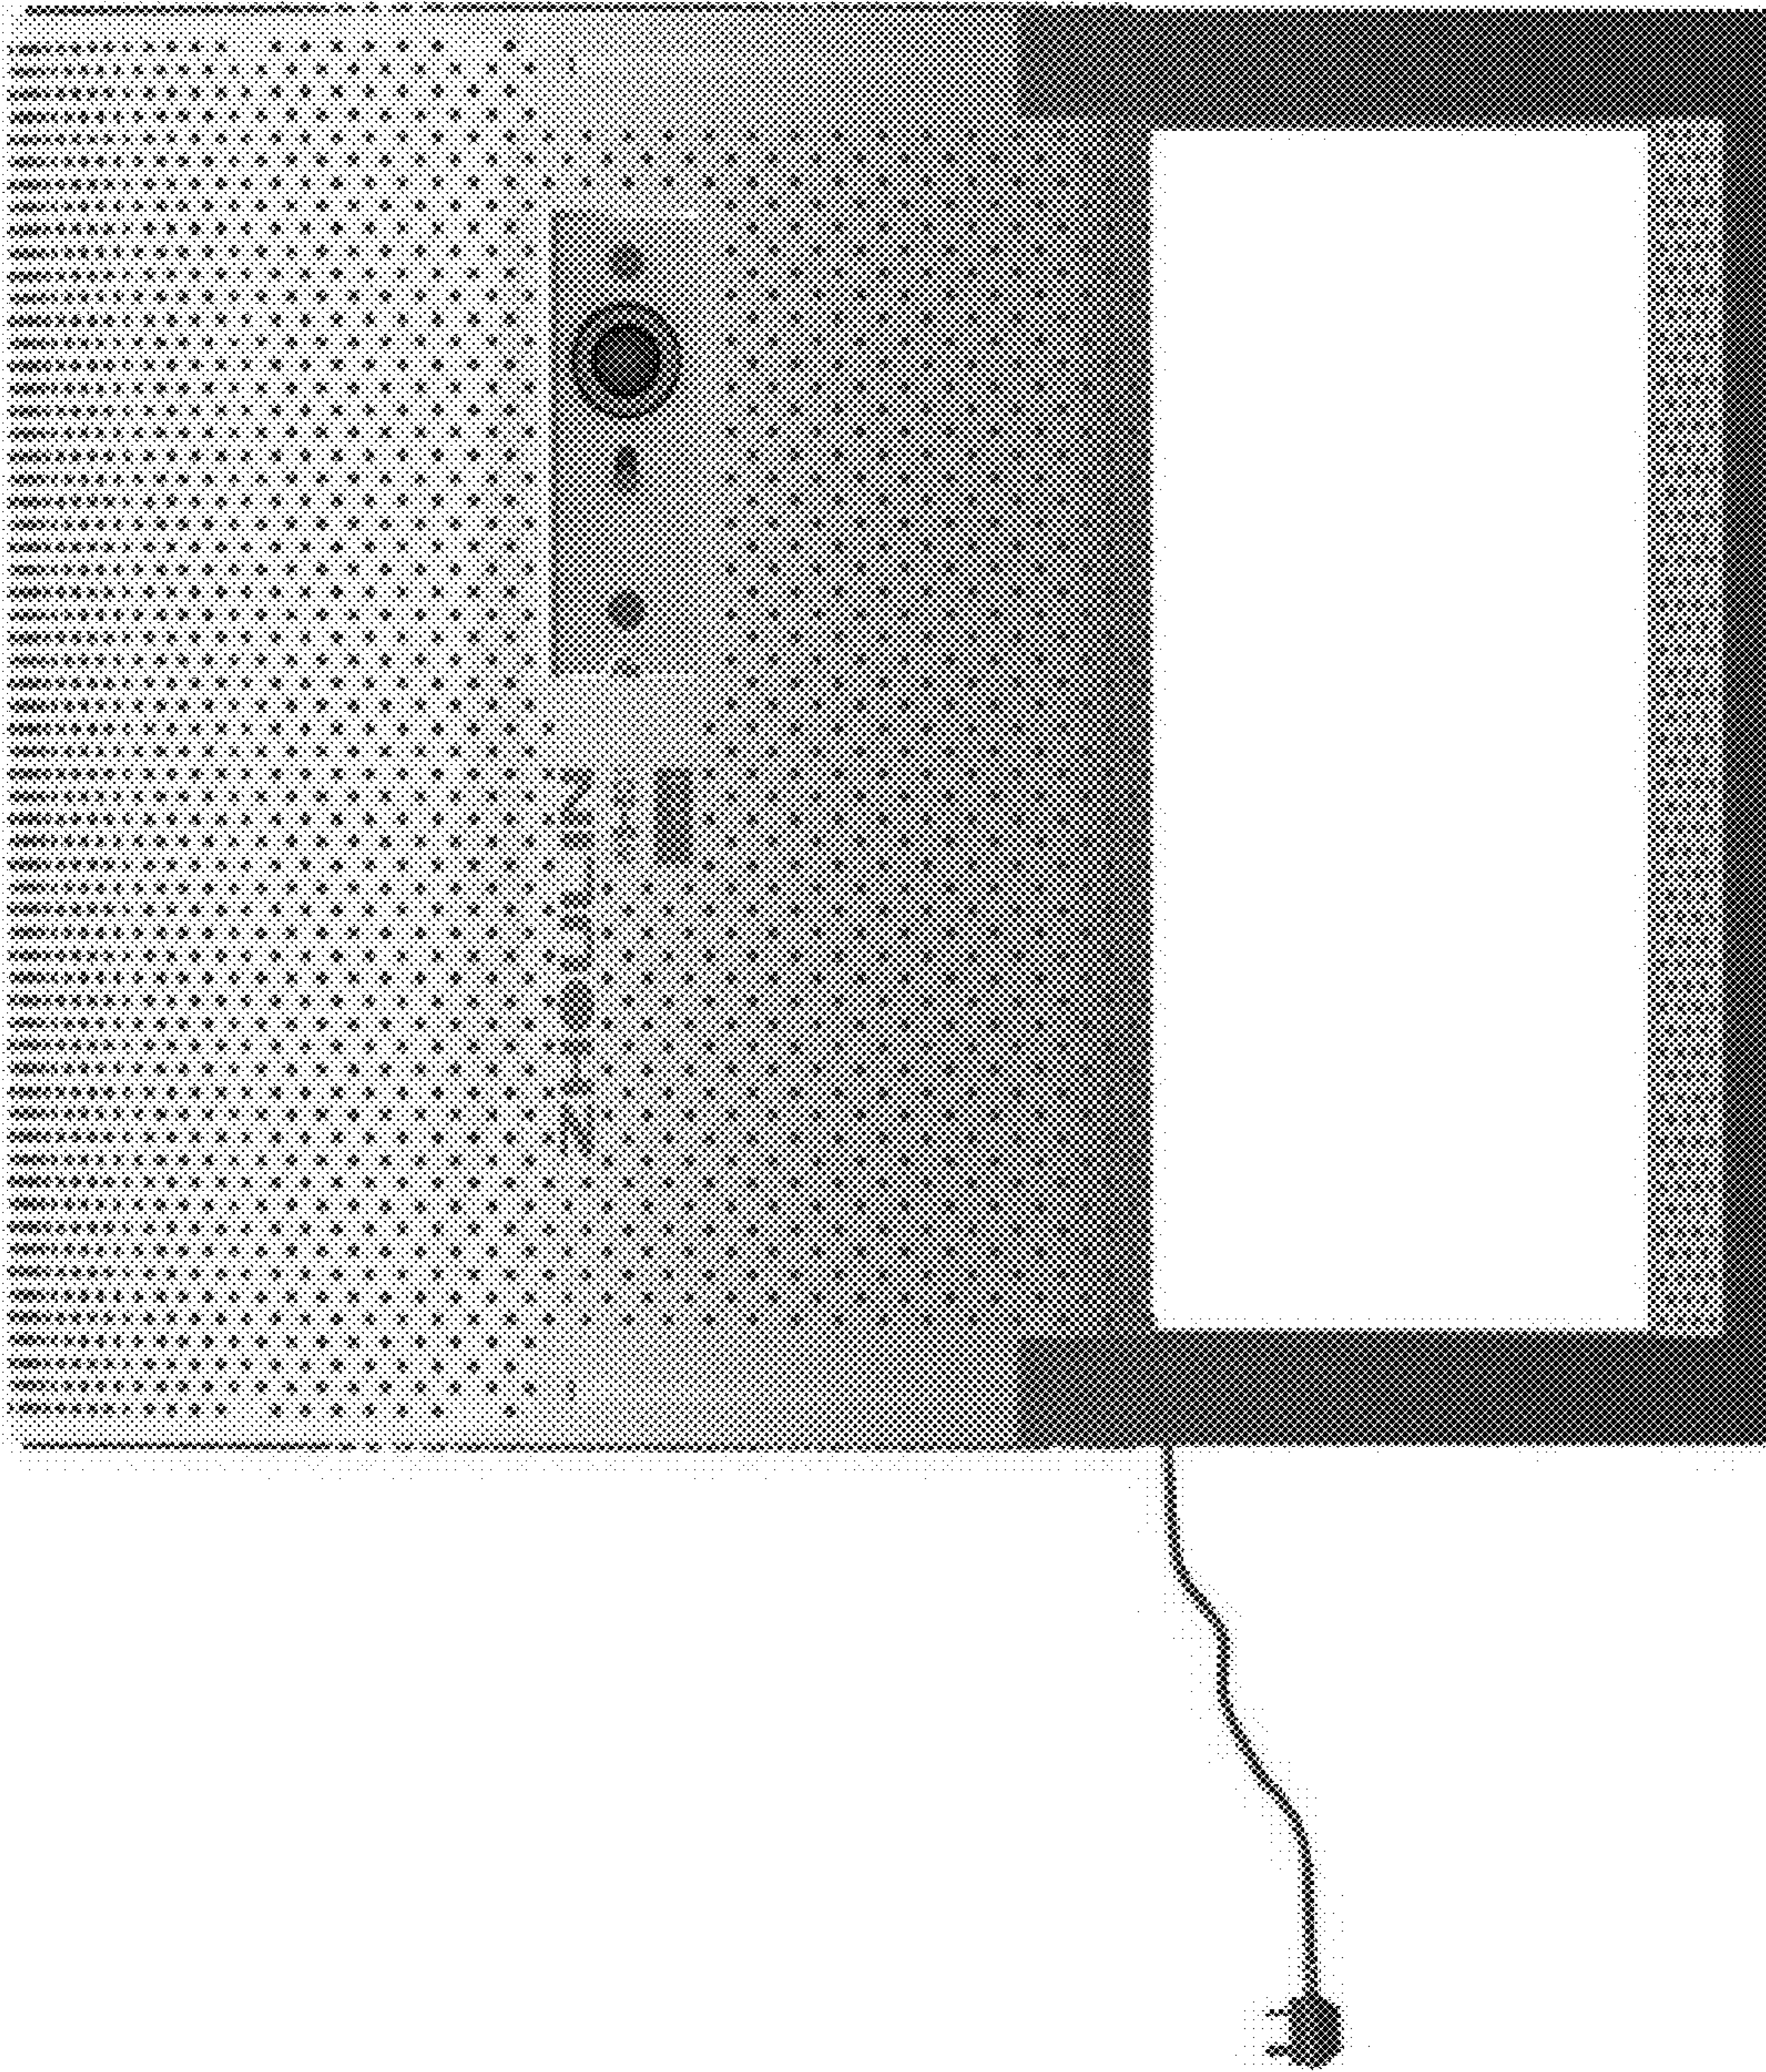


FIG. 3

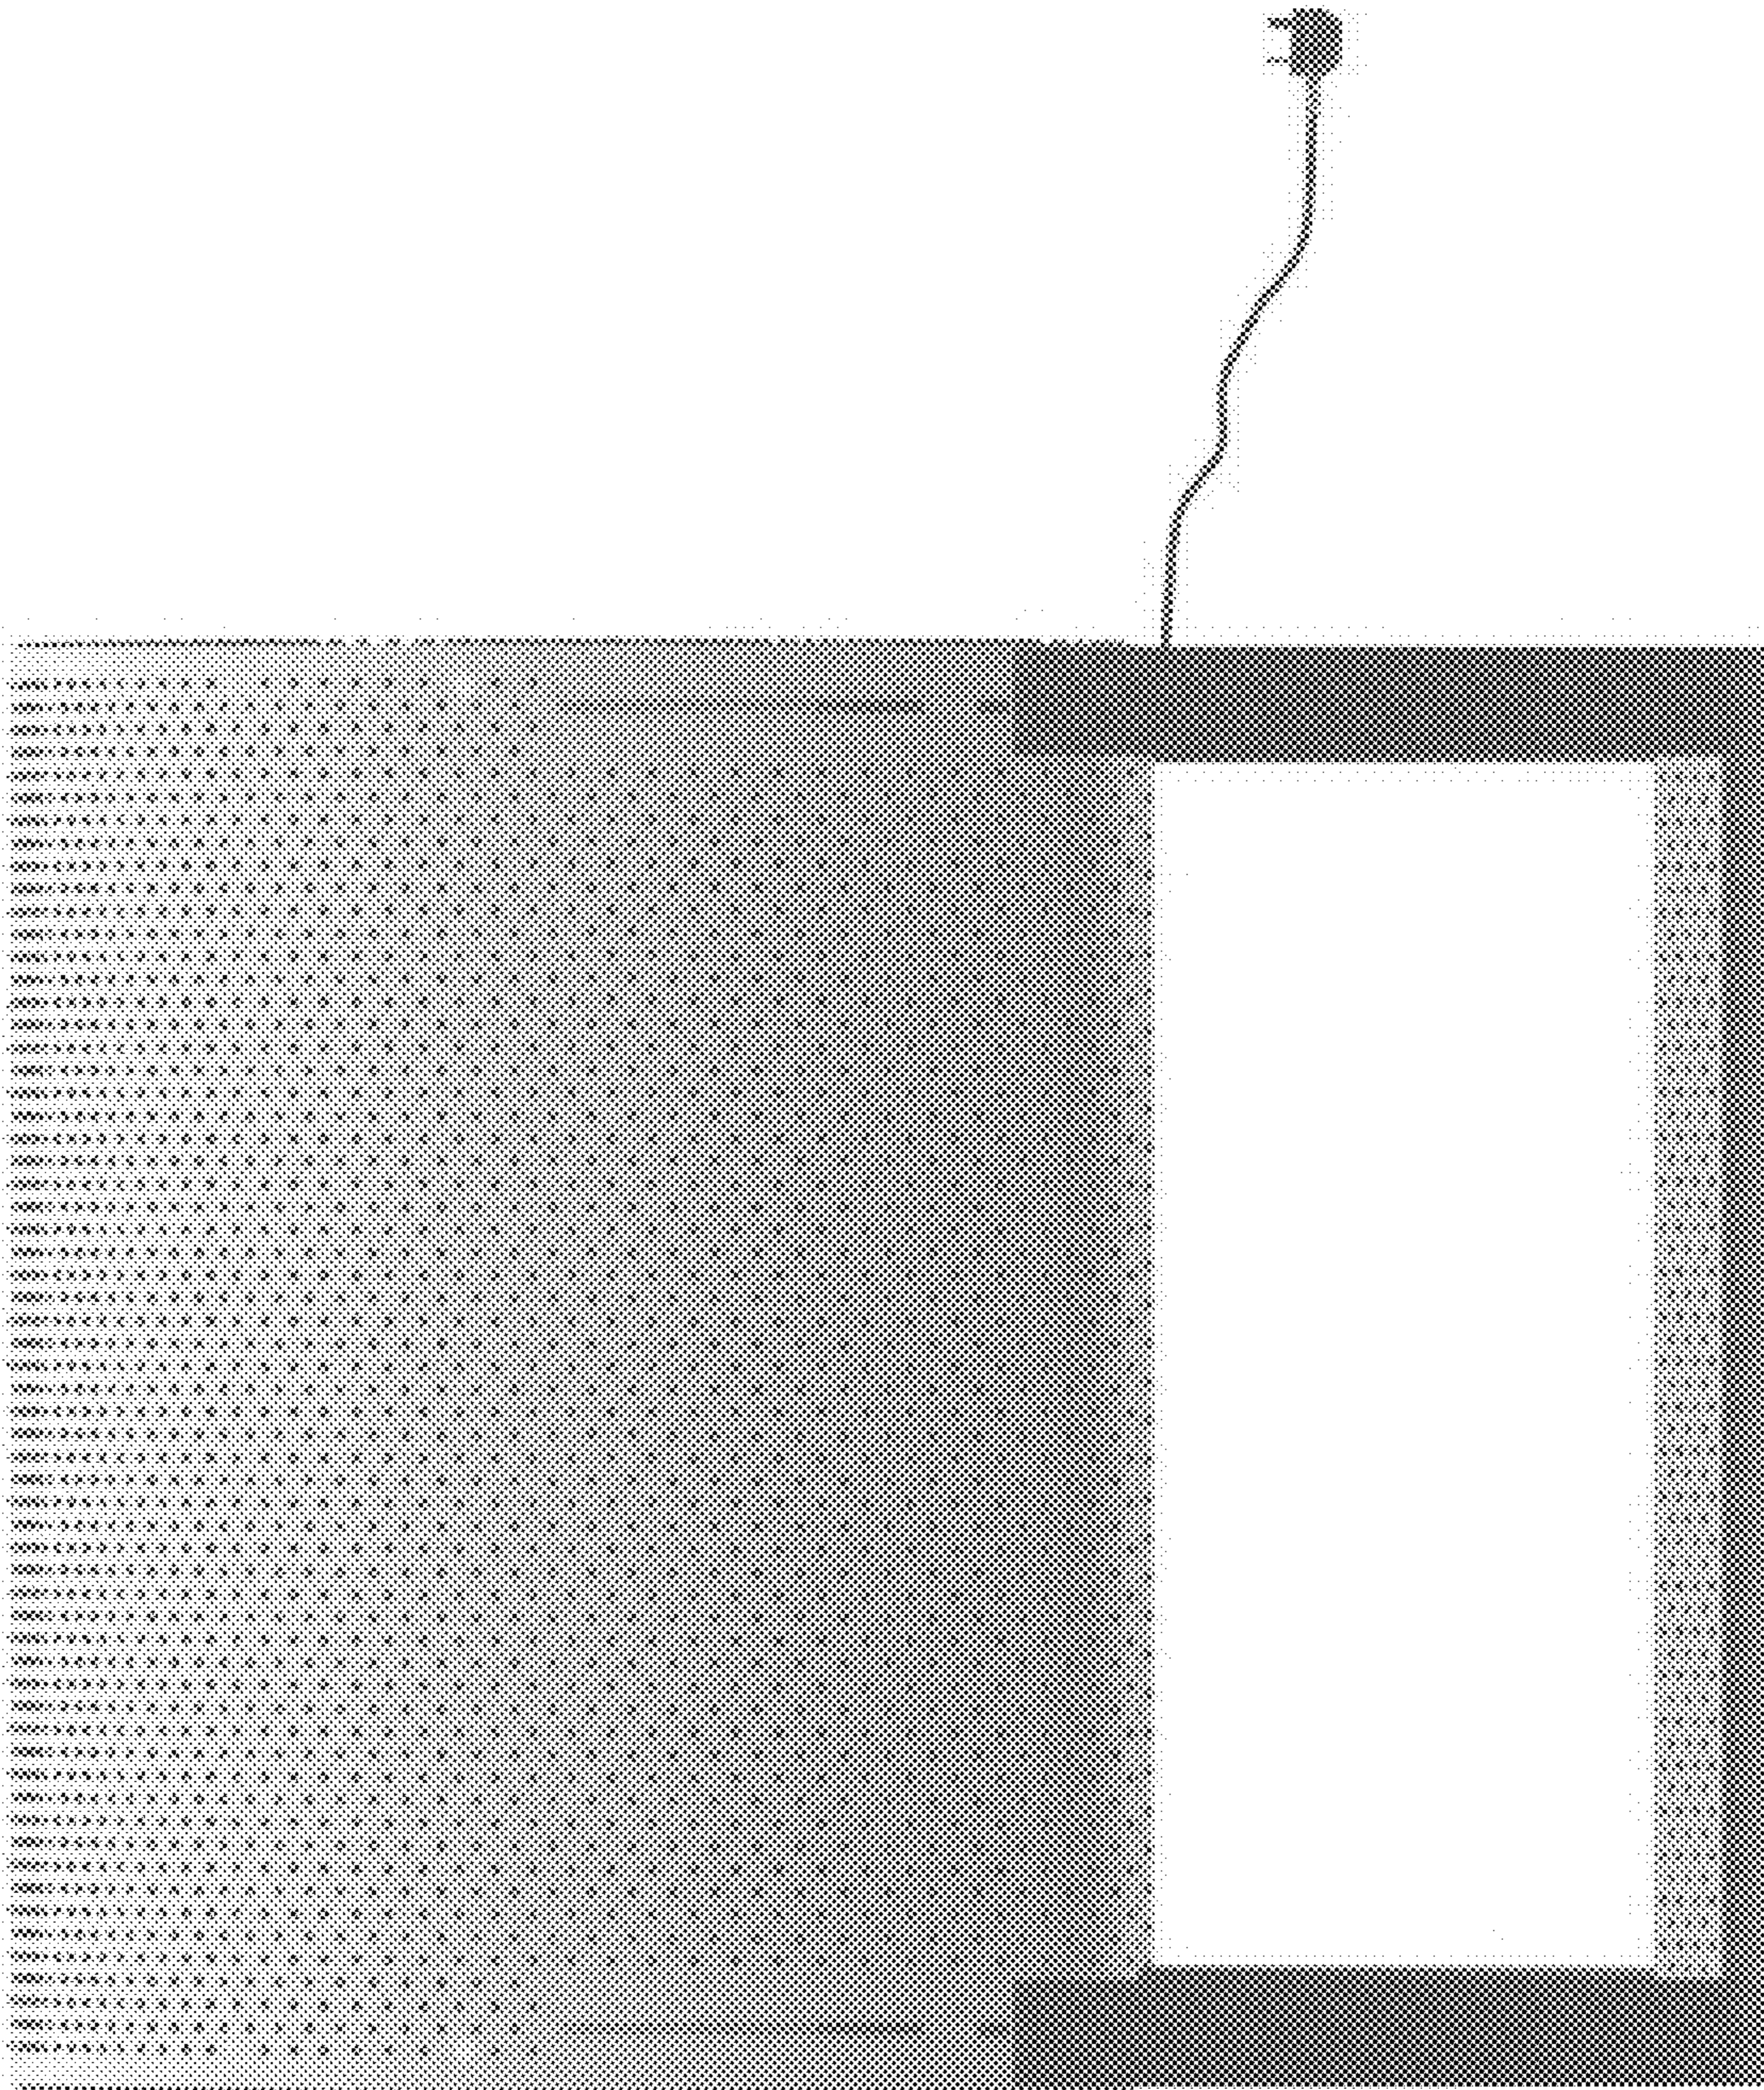


FIG. 4

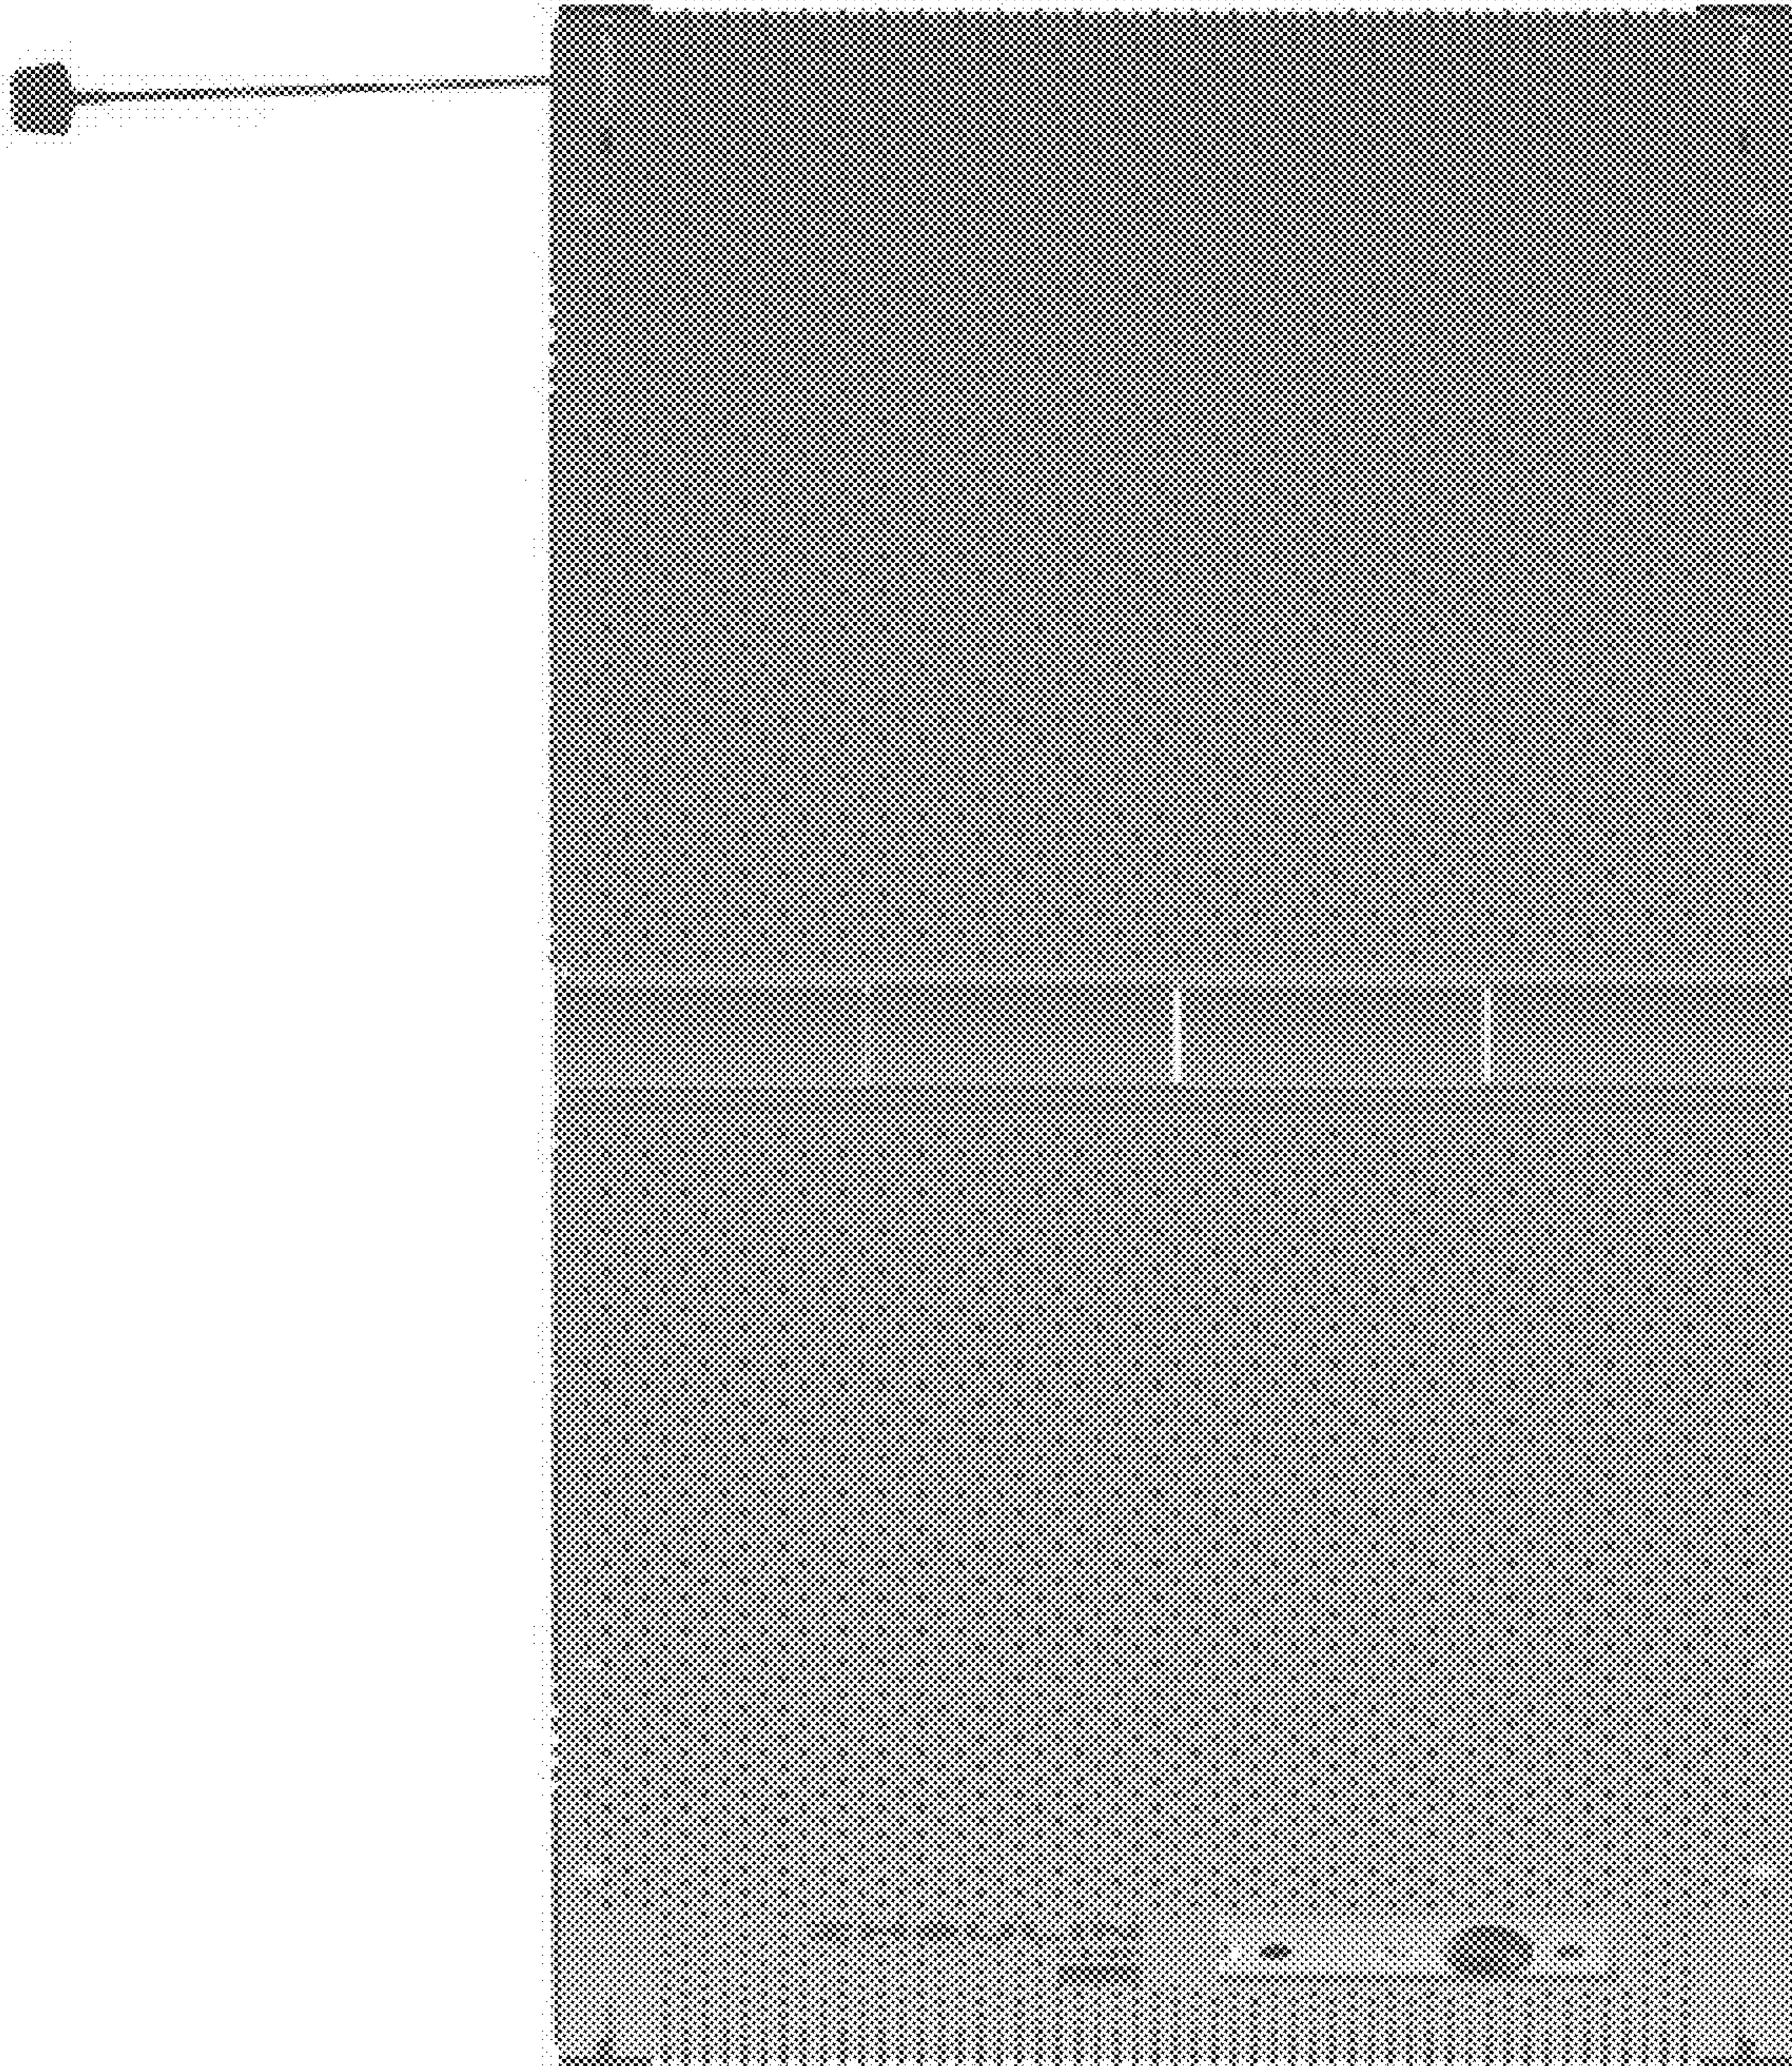


FIG. 5

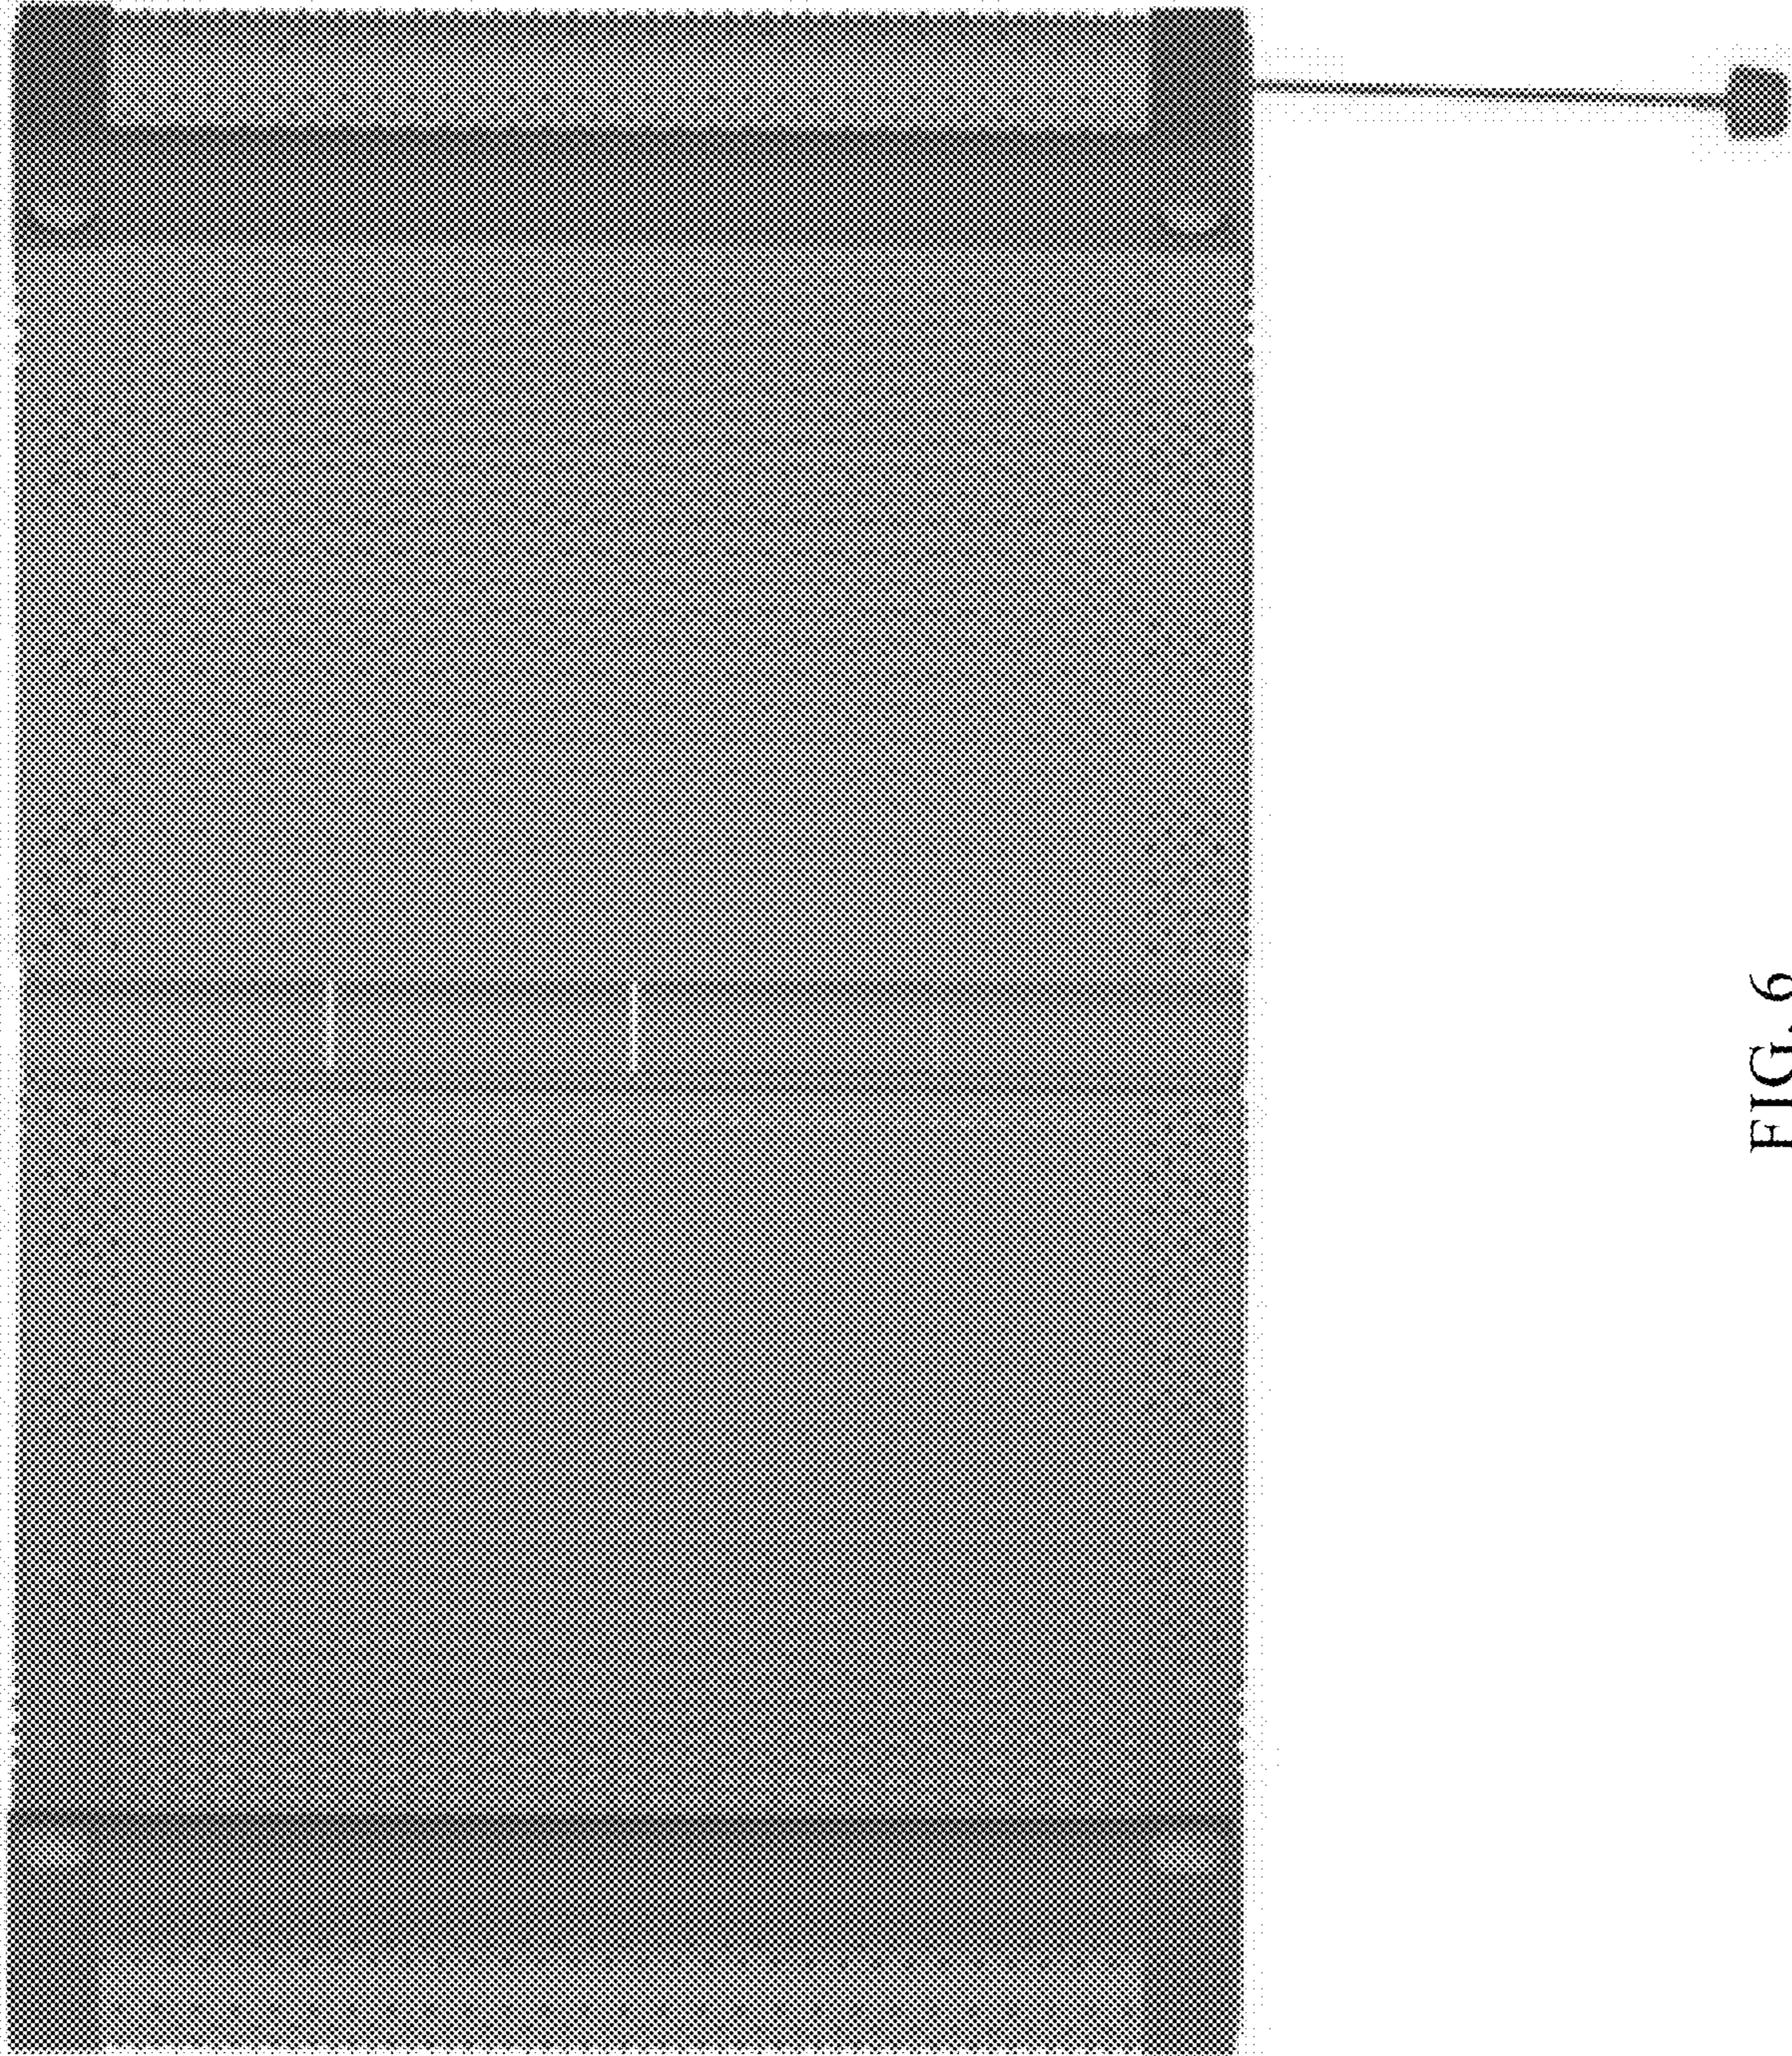


FIG. 6

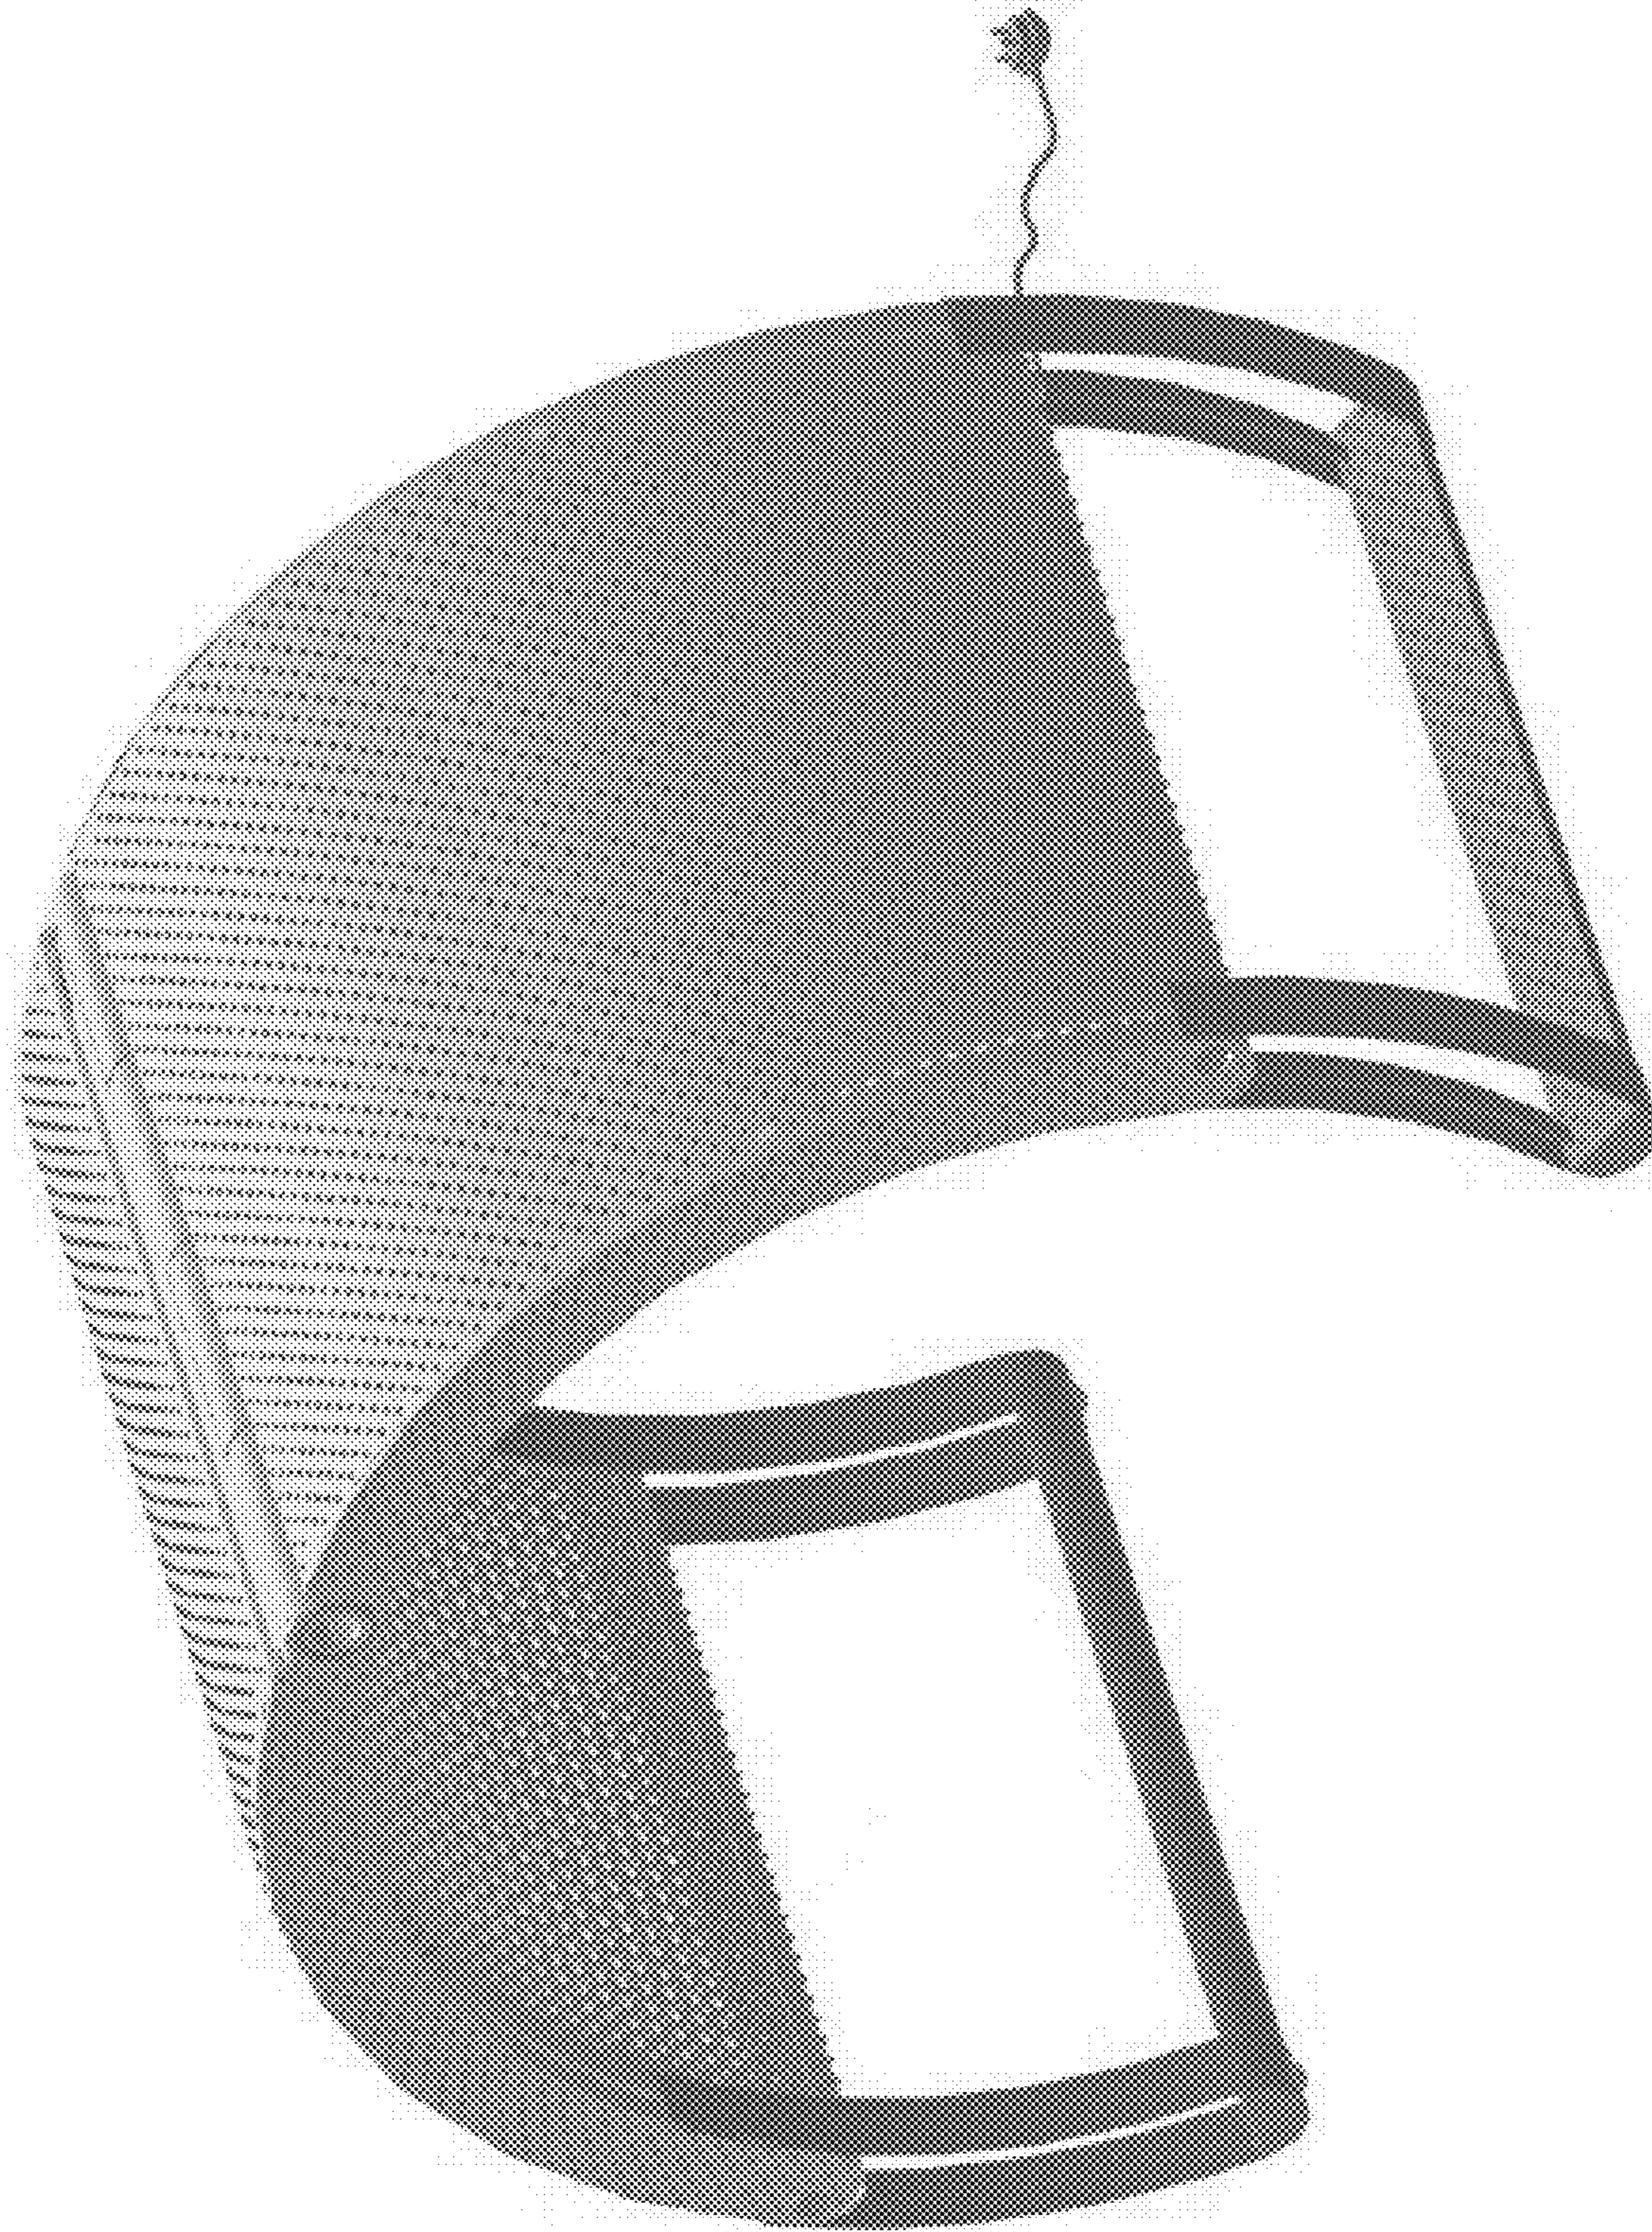


FIG. 7



FIG. 8

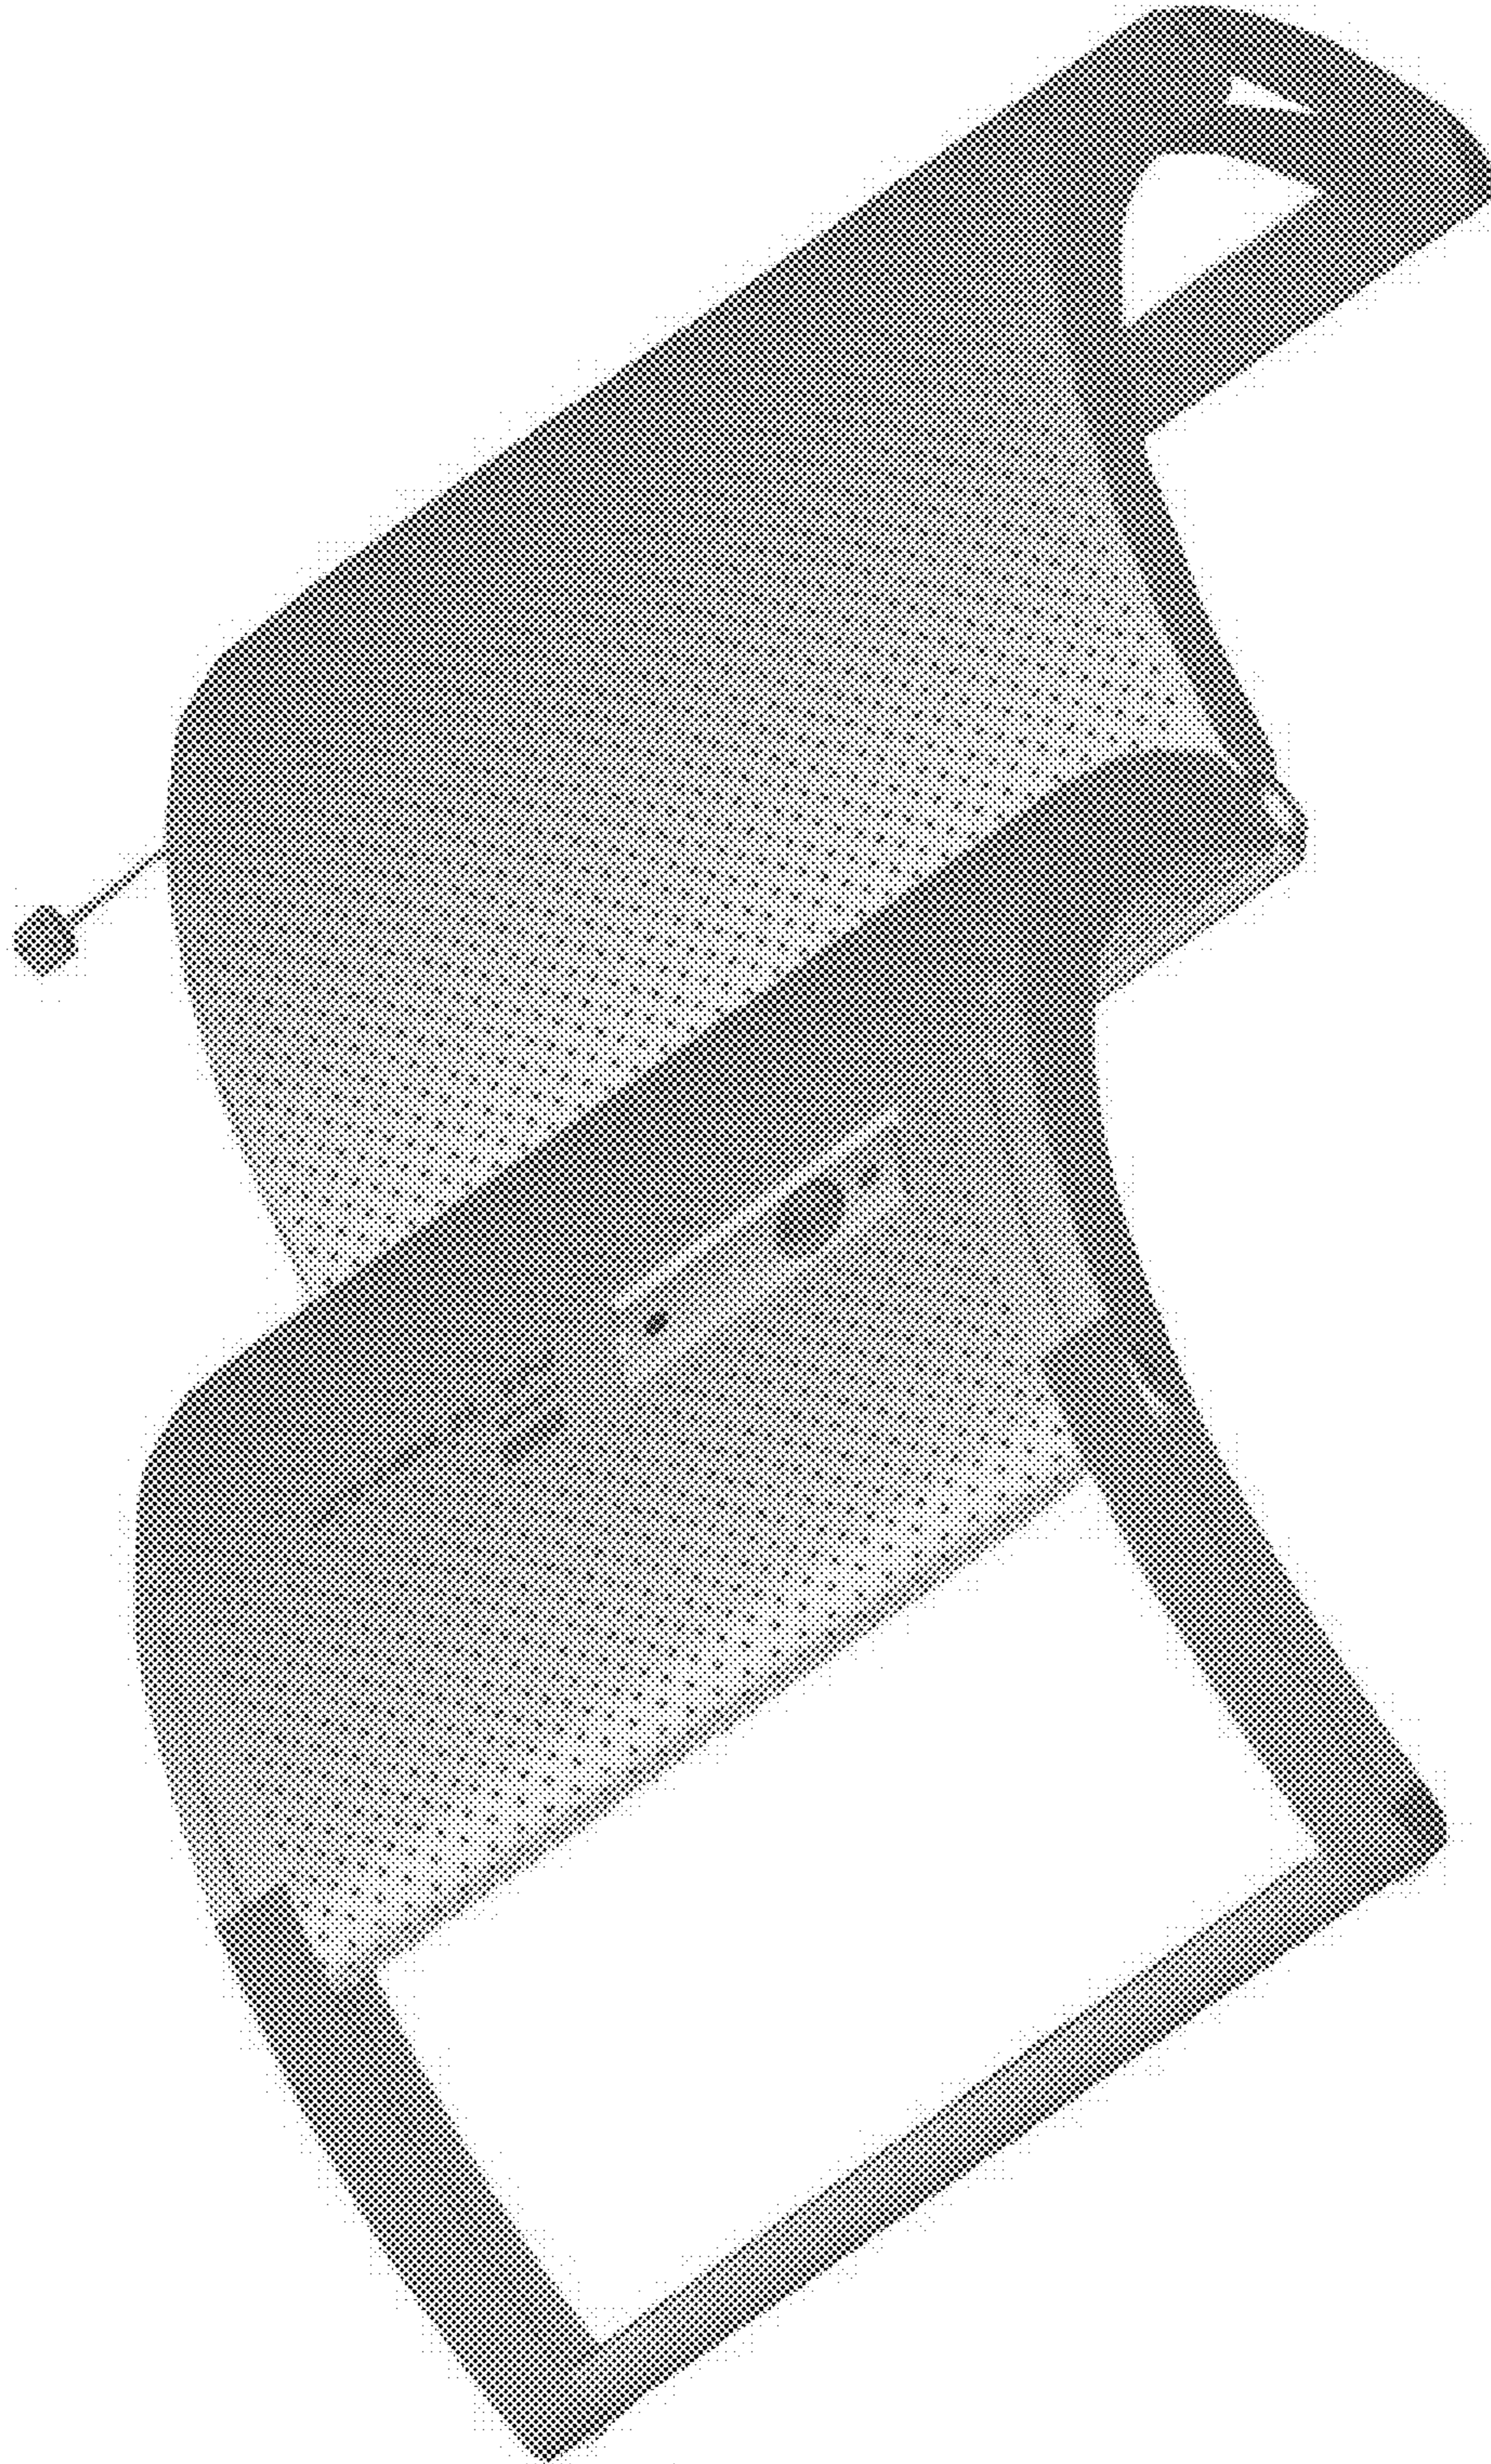


FIG. 9



FIG. 10

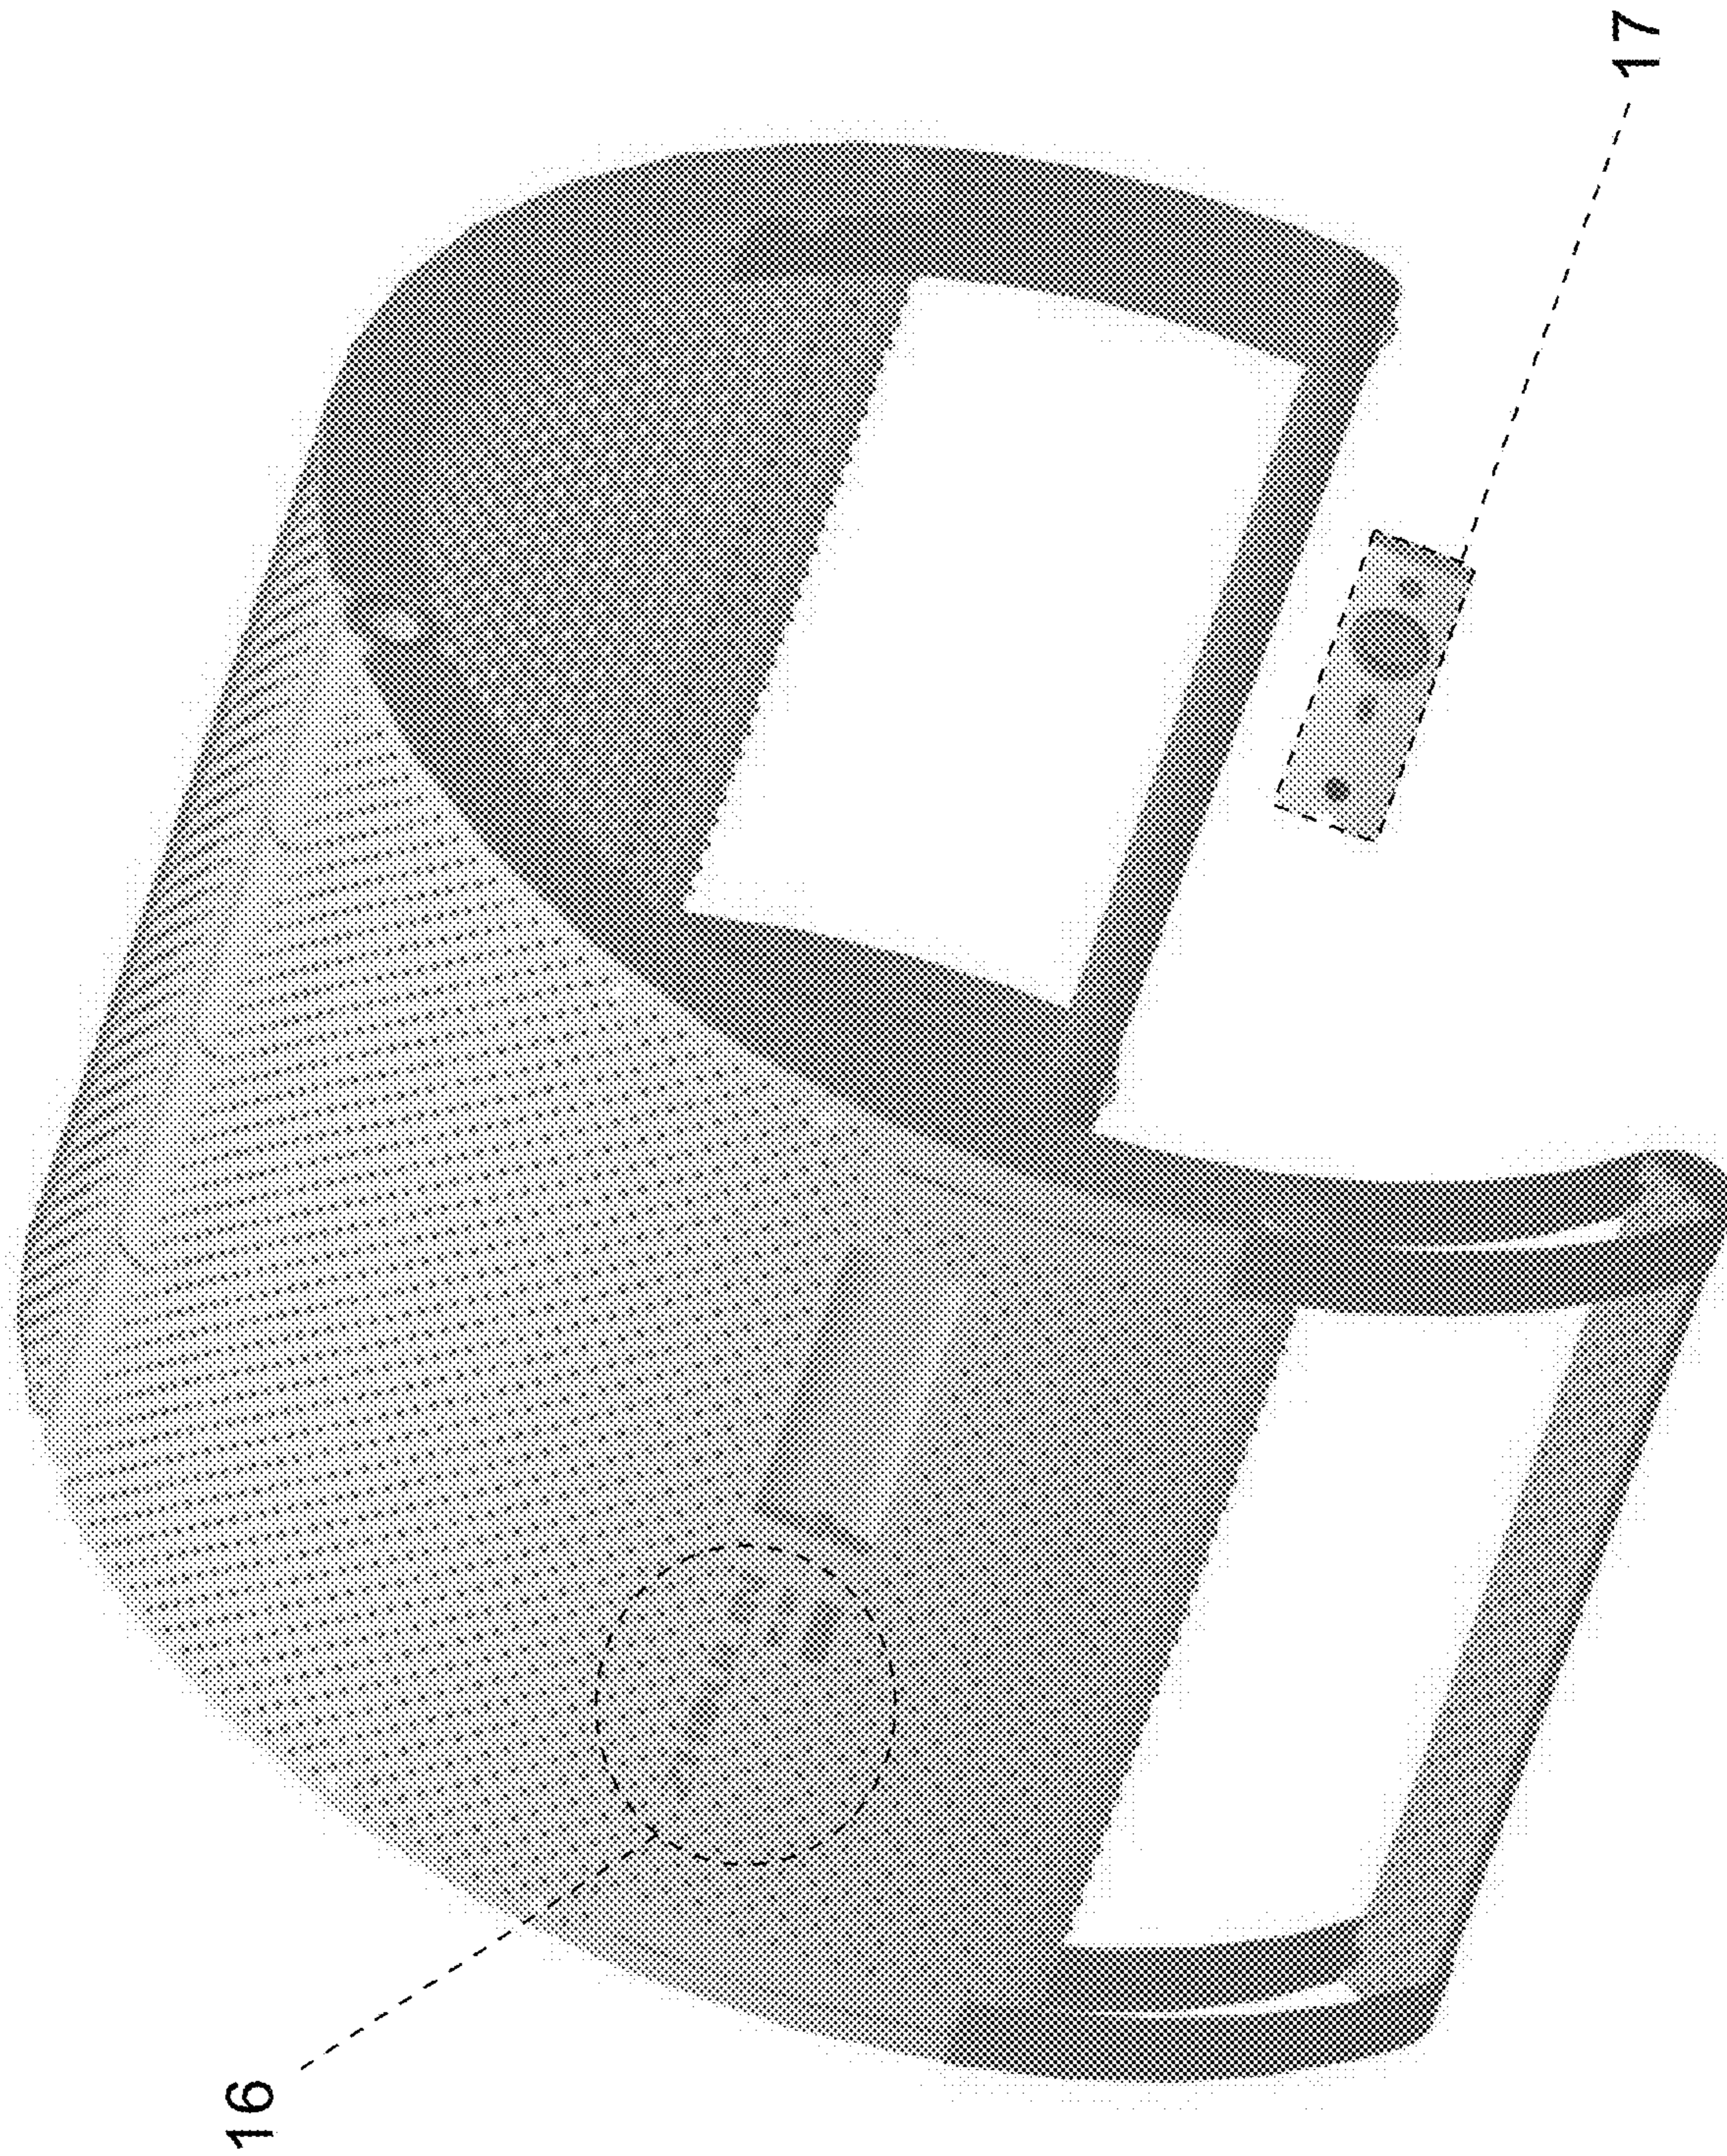


FIG. 11

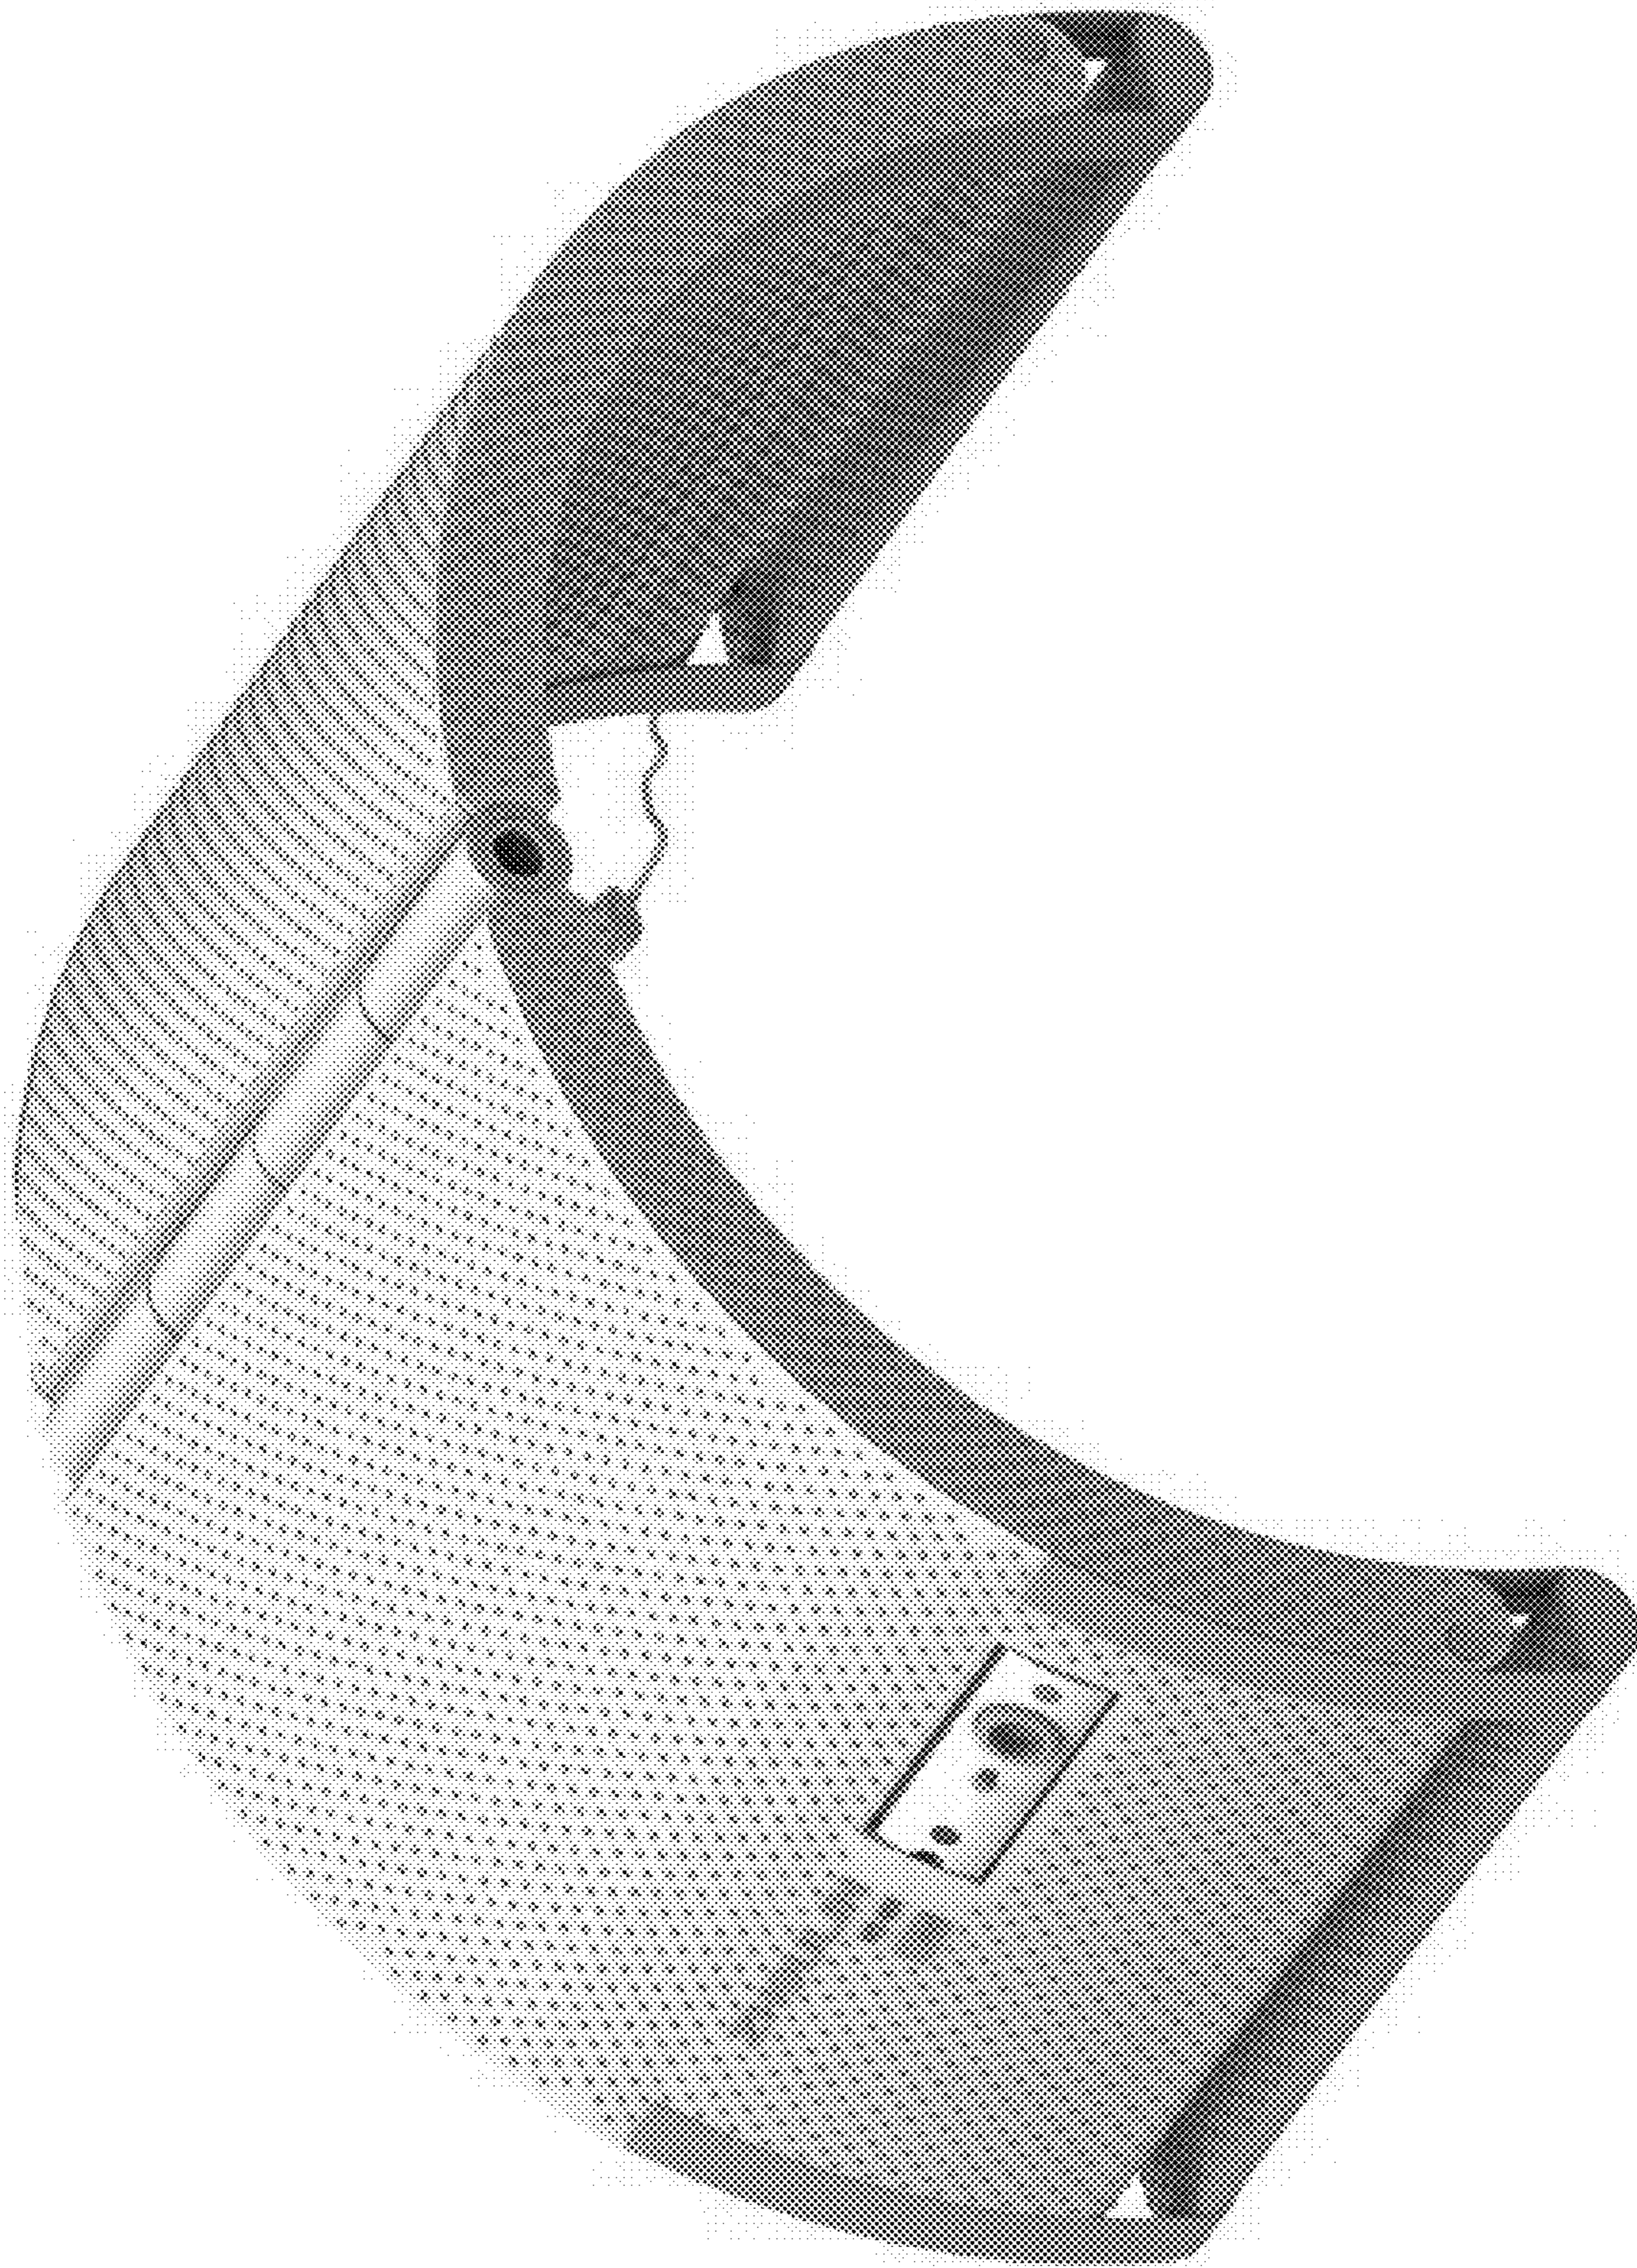


FIG. 12

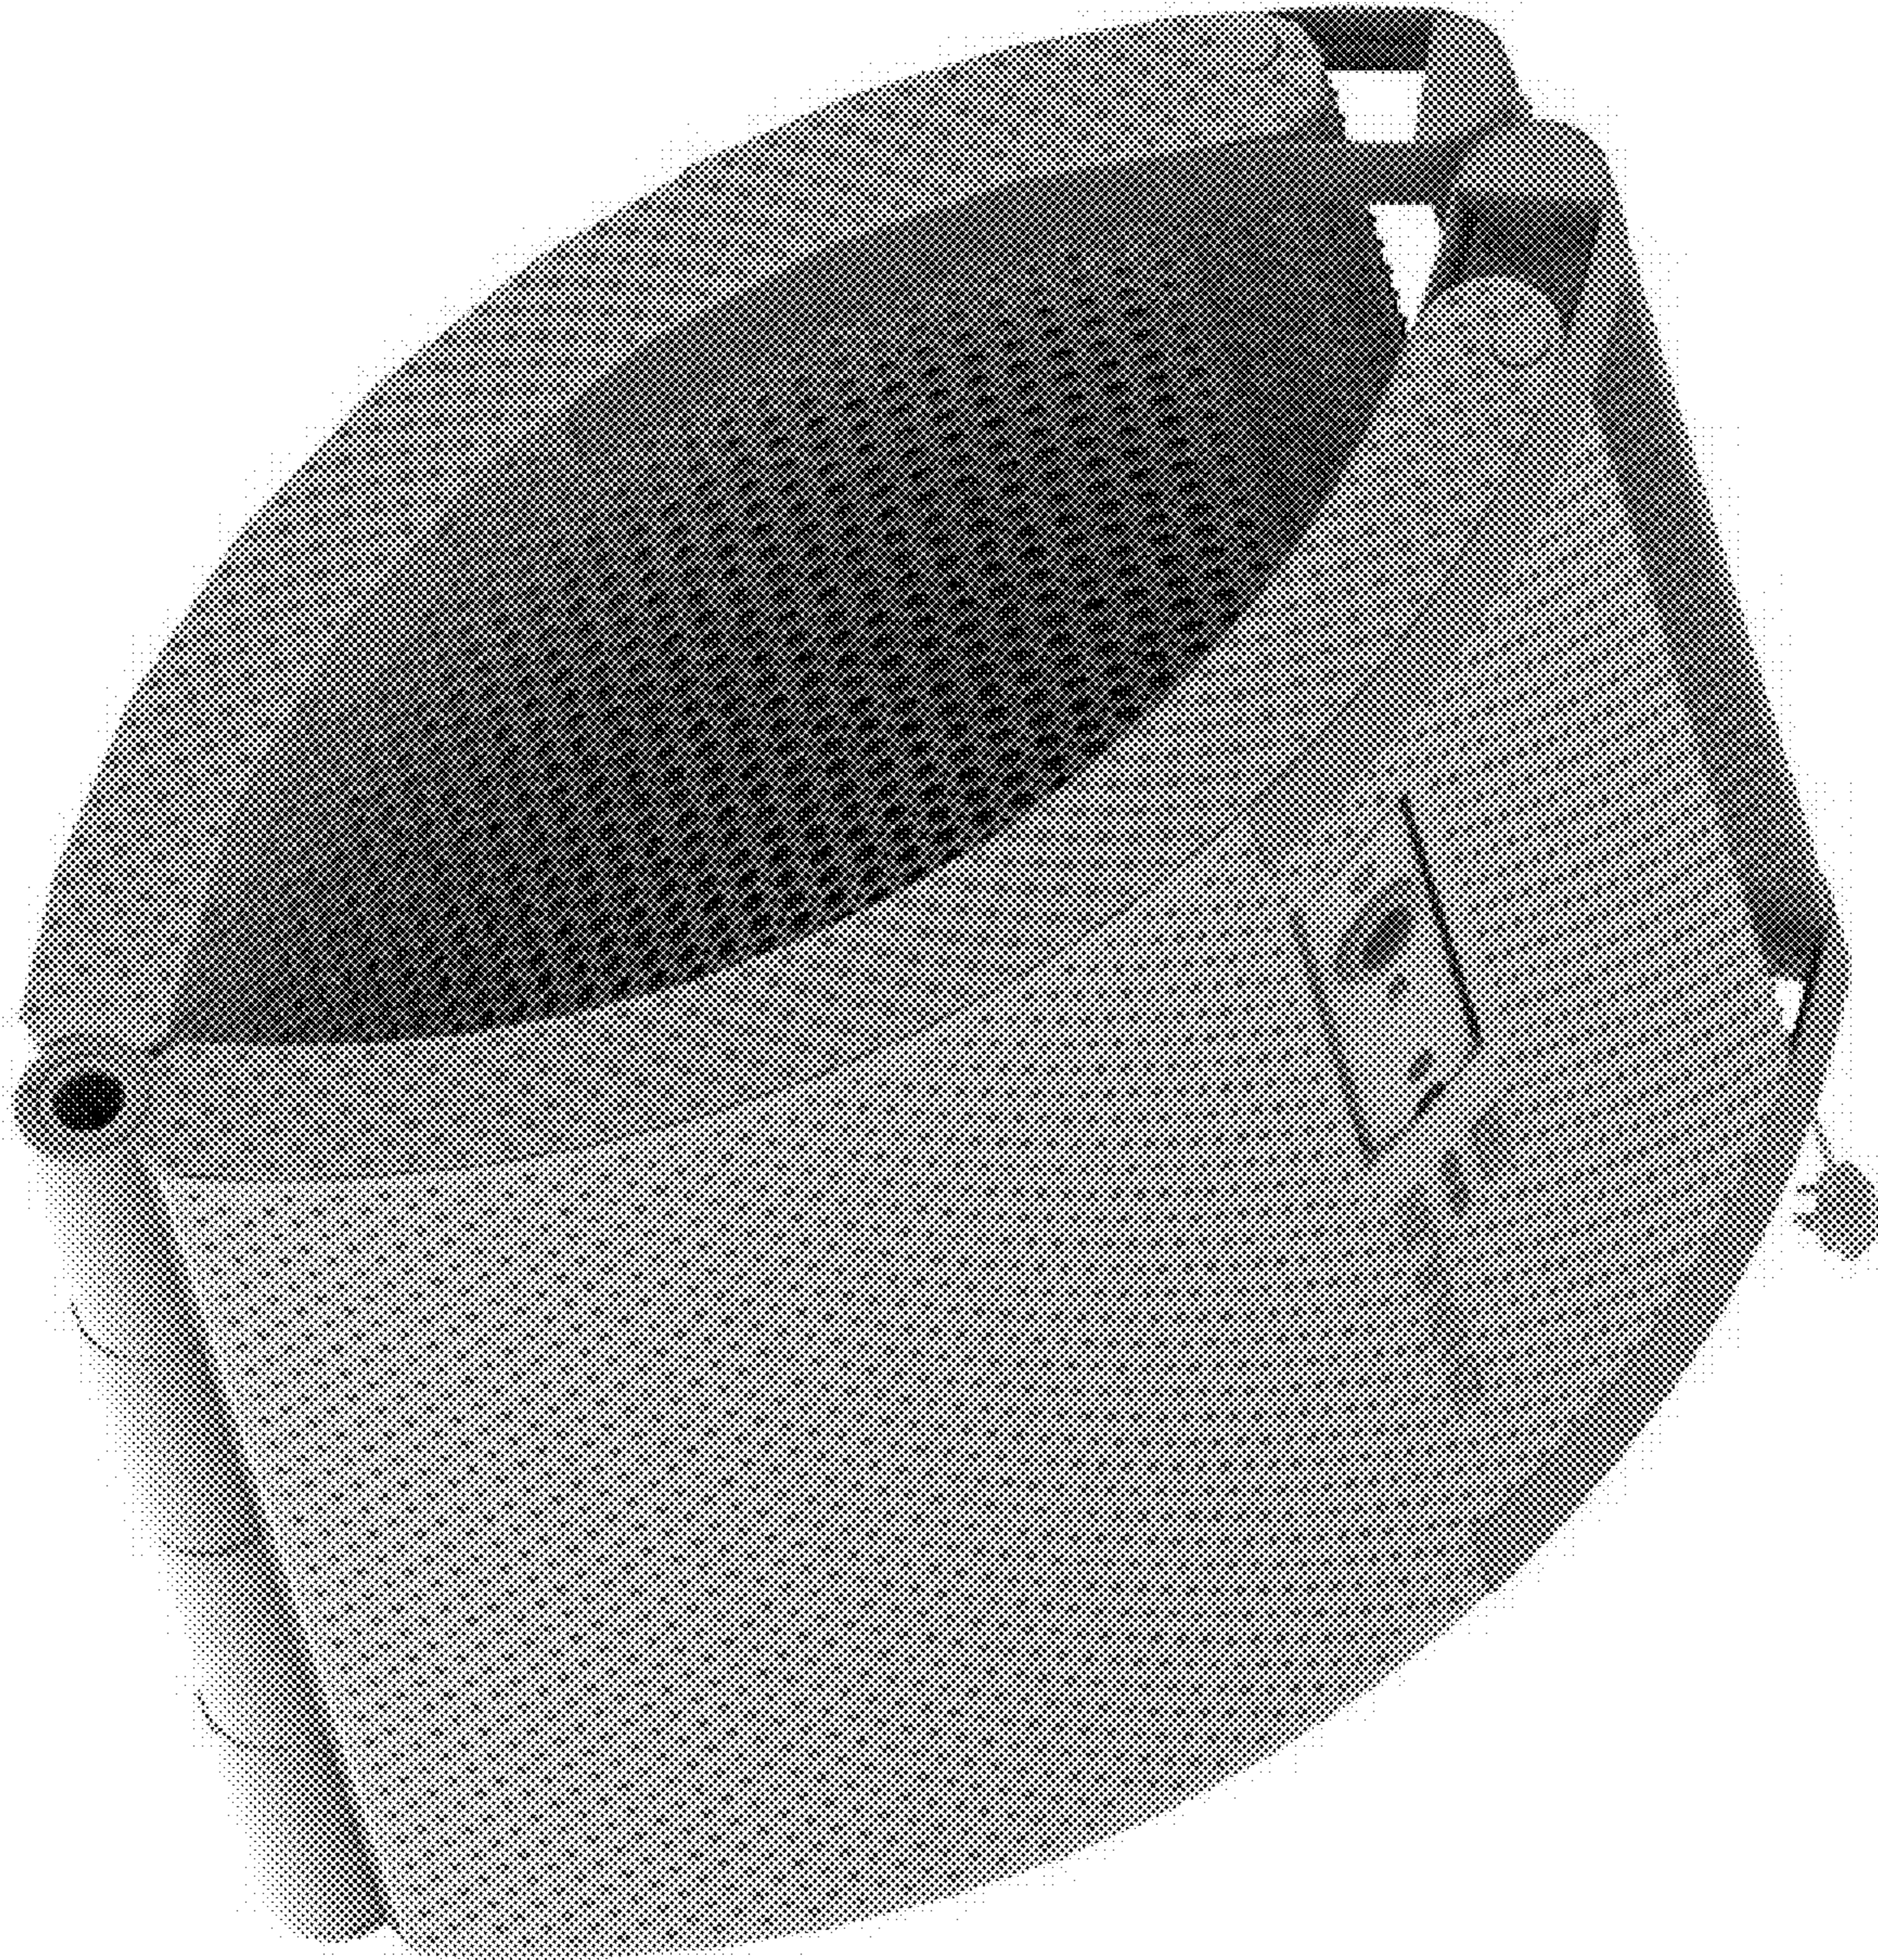


FIG. 13



FIG. 14

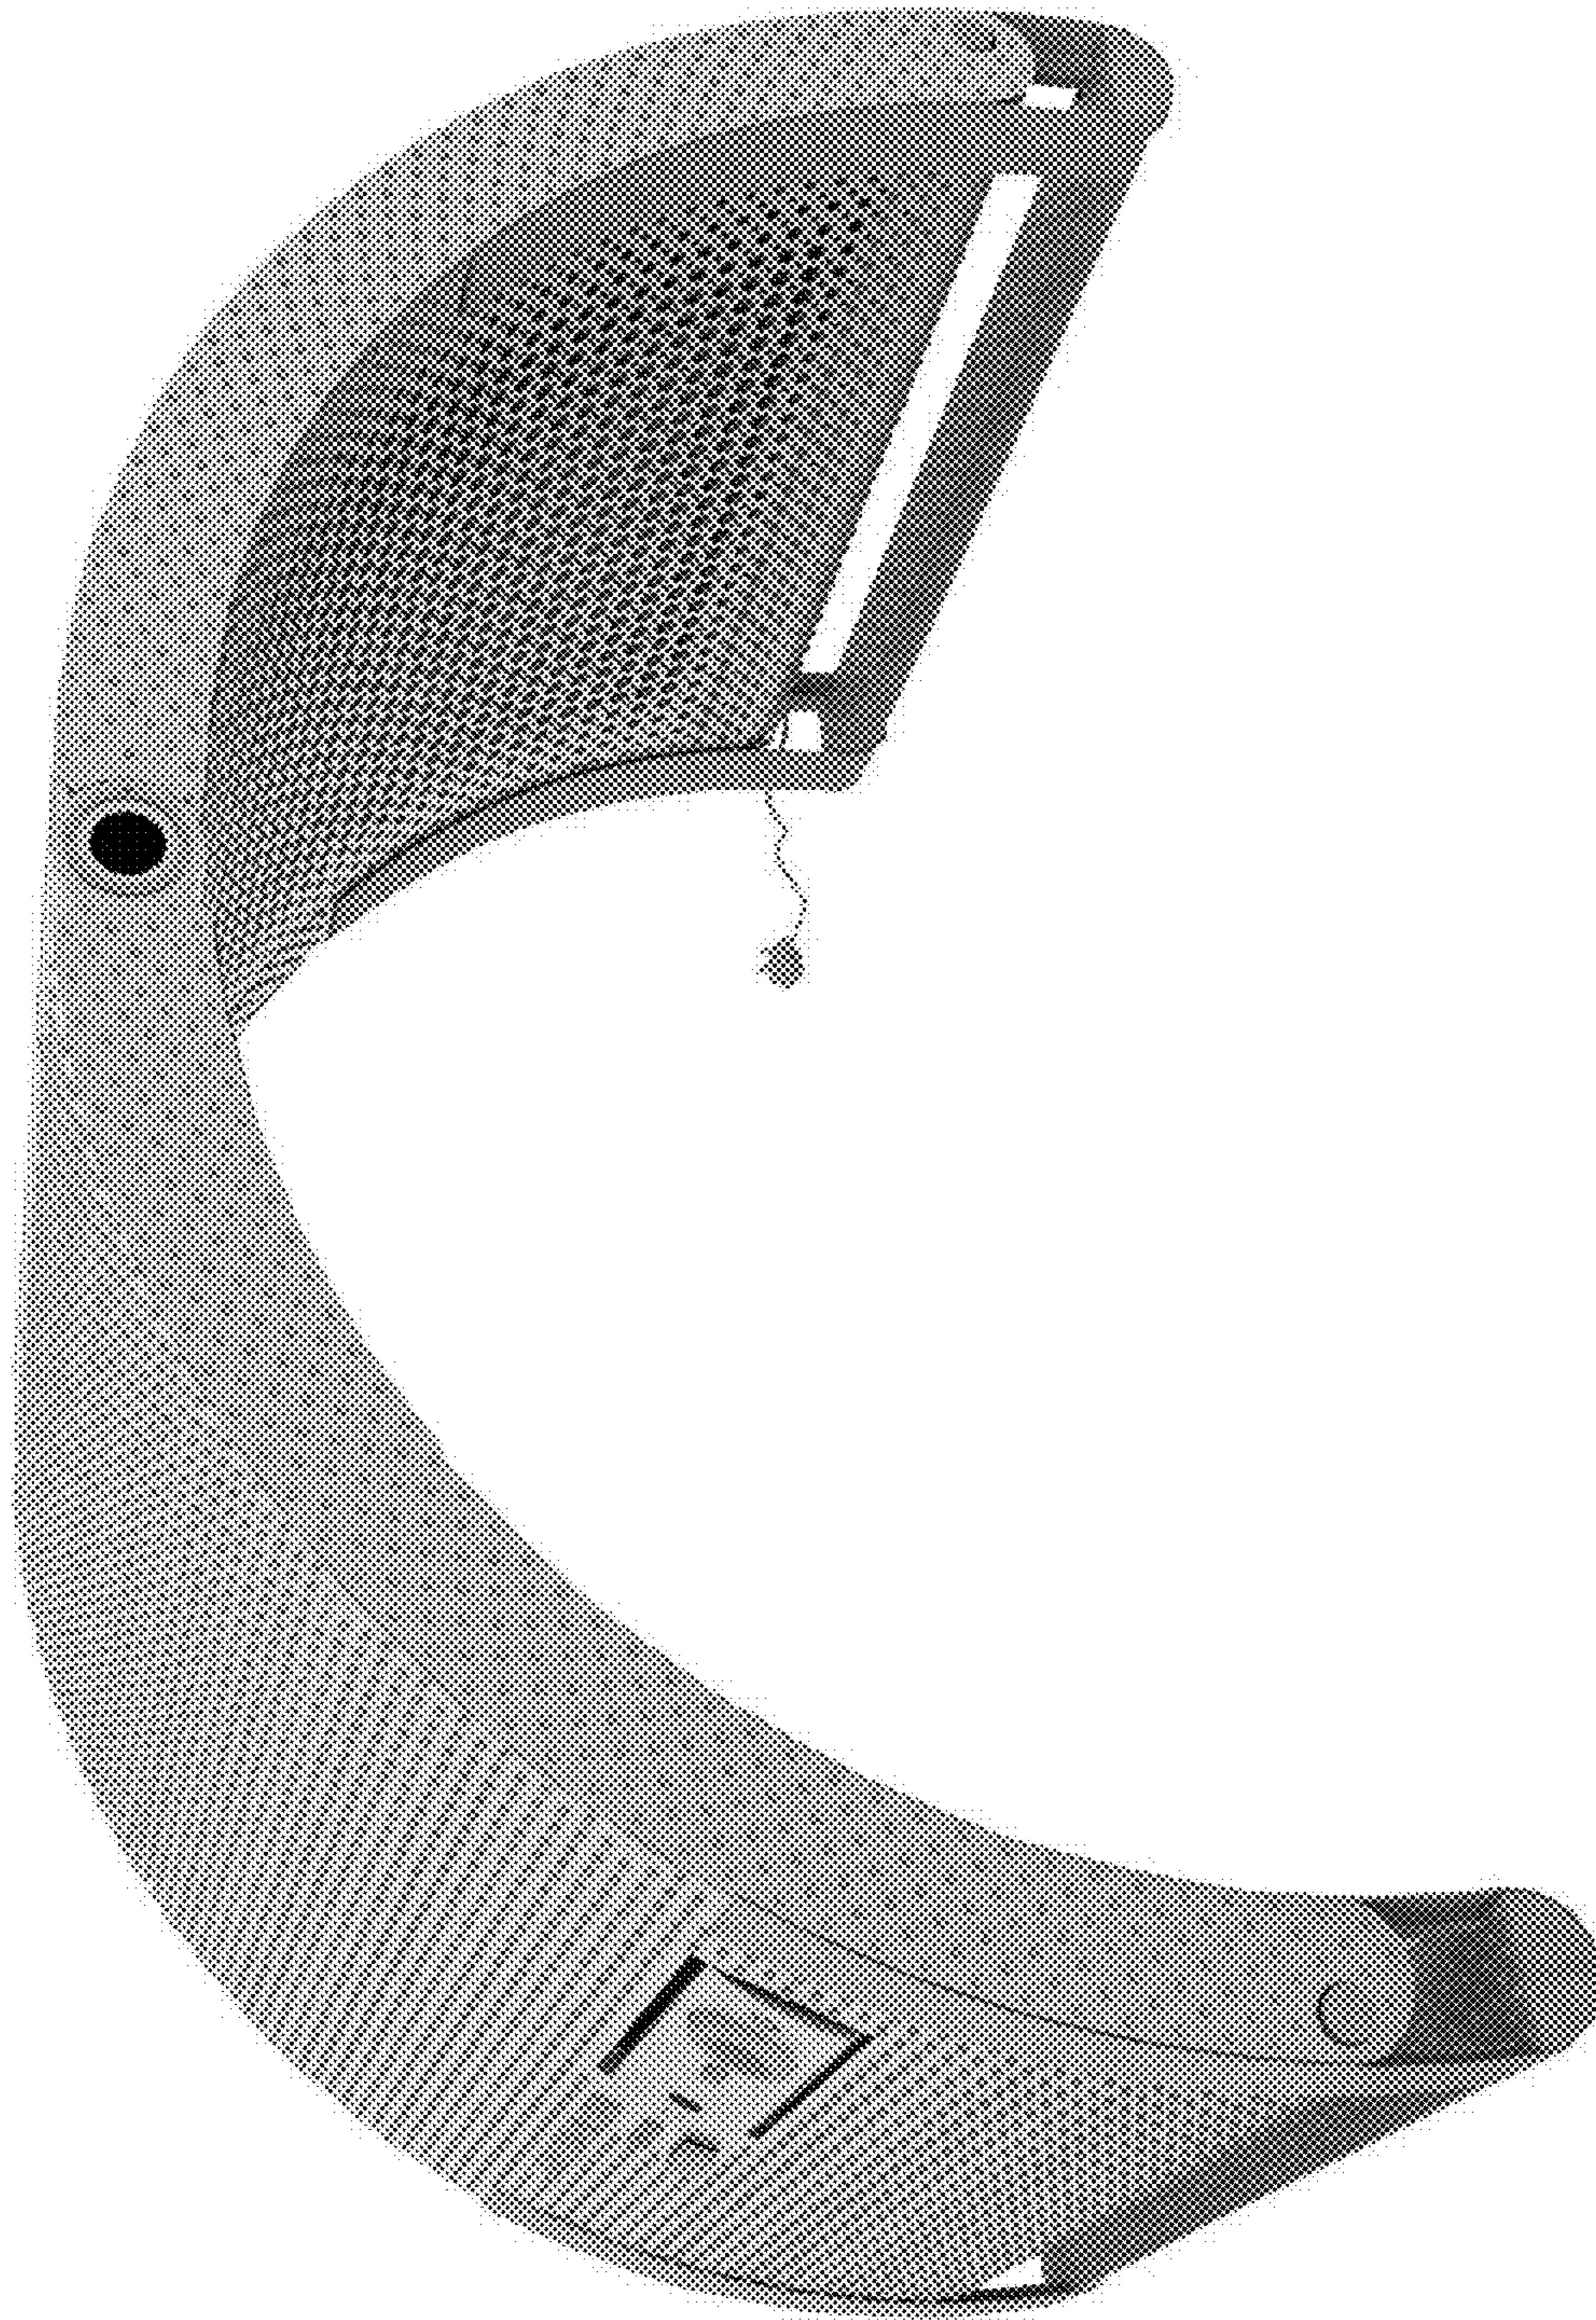


FIG. 15

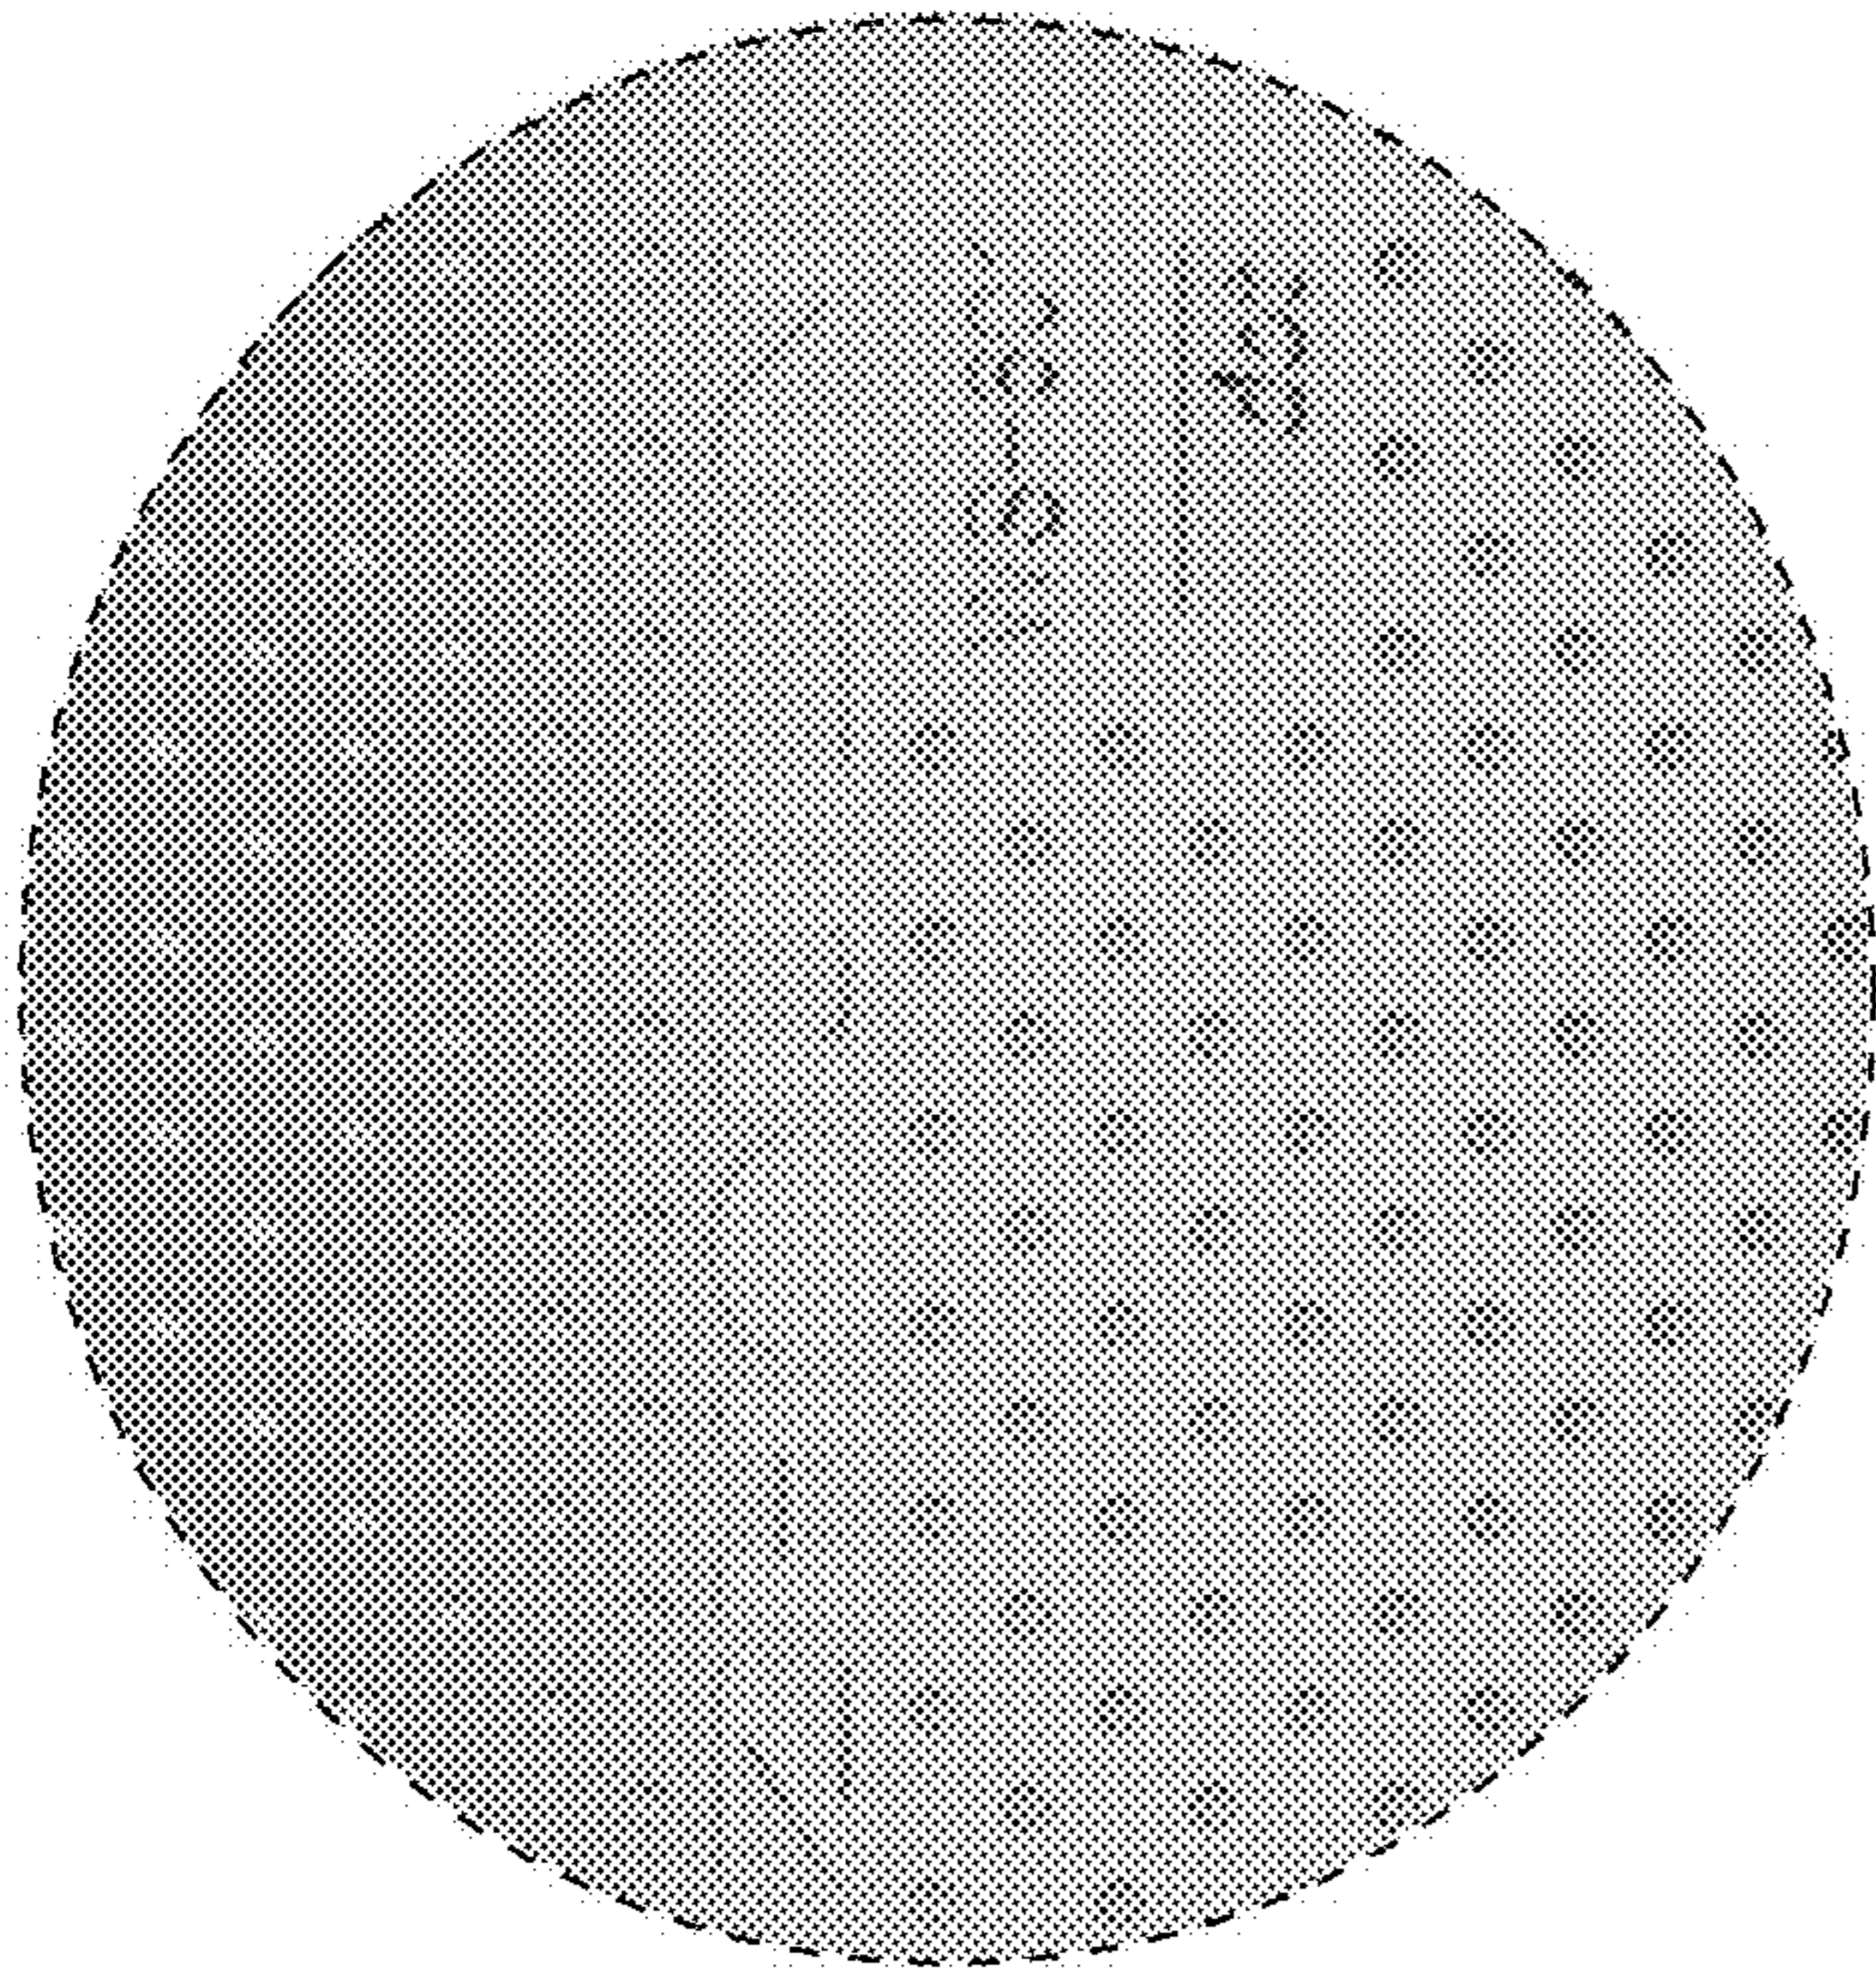


FIG. 16

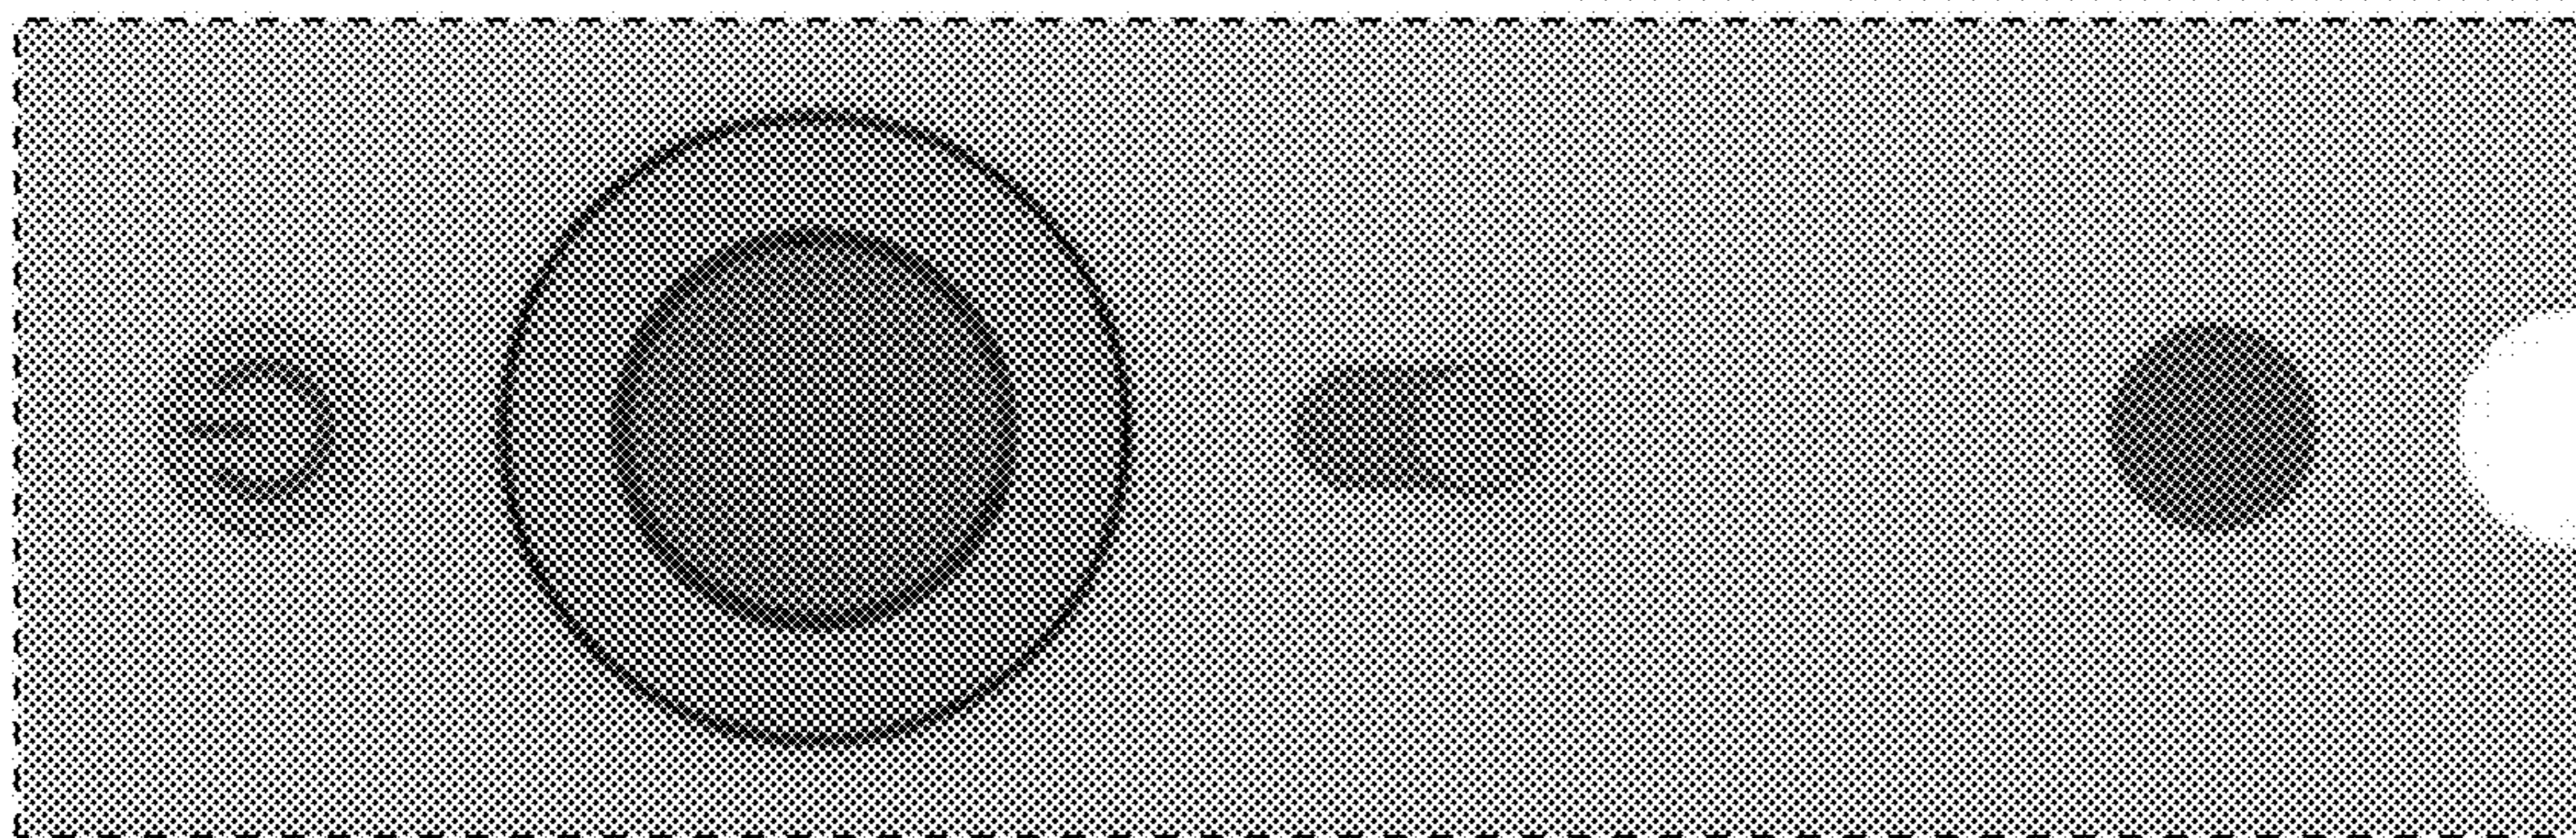


FIG. 17