



US00D875052S

(12) **United States Design Patent** (10) **Patent No.:** **US D875,052 S**  
**Zhou et al.** (45) **Date of Patent:** **\*\* Feb. 11, 2020**

(54) **CONTROL PANEL**

- (71) Applicant: **LEICA MICROSYSTEMS LTD., SHANGHAI**, Shanghai (CN)
- (72) Inventors: **Gang Zhou**, Shanghai (CN); **Zheguang Fan**, Shanghai (CN); **Jingtian Zhang**, Shanghai (CN); **Xiang Liang**, Shanghai (CN)
- (73) Assignee: **LEICA MICROSYSTEMS LTD., SHANGHAI**, Shanghai (CN)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/635,586**
- (22) Filed: **Jan. 31, 2018**
- (30) **Foreign Application Priority Data**

Nov. 30, 2017 (CN) ..... 2017 3 0601149

- (51) **LOC (12) Cl.** ..... **13-03**
- (52) **U.S. Cl.**  
USPC ..... **D13/164**
- (58) **Field of Classification Search**  
USPC ..... D13/162, 164, 168; D24/216, 232  
CPC ..... G05B 19/409; G05B 2219/23406; H05K 5/00; H05K 5/0017; H05K 5/02; H05K 5/0217; H05K 5/03; G01N 1/06  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,447,594	A *	6/1969	Andrews	.....	G01N 1/06 165/263
D256,230	S *	8/1980	Beale	.....	D13/164
D352,025	S *	11/1994	Dellavecchia	.....	D13/164
D549,184	S *	8/2007	Riley	.....	D13/164
D579,800	S *	11/2008	Mobley	.....	D10/57
D608,302	S *	1/2010	Liu	.....	D13/164
D776,627	S *	1/2017	Shimohama	.....	D13/164
D788,716	S *	6/2017	Ewringmann	.....	D13/164
D802,540	S *	11/2017	Kurokawa	.....	D13/164
D807,306	S *	1/2018	Suwa	.....	D13/164

**OTHER PUBLICATIONS**

Leica RM Rotary Microtome with controller; prior to Jan. 31, 2018; 1 pg. 1; [https://www.google.com/search?q=controller+for+microtome&hl=en&biw=1536&bih=813&source=Int&tbs=cdr%3A1%2Ccd\\_min%3A%2Ccd\\_max%3A1%2F31%2F2018&tbs=isch#imgrc=G9dE8LkxHuL59M:&spf=1561485663238.\\*](https://www.google.com/search?q=controller+for+microtome&hl=en&biw=1536&bih=813&source=Int&tbs=cdr%3A1%2Ccd_min%3A%2Ccd_max%3A1%2F31%2F2018&tbs=isch#imgrc=G9dE8LkxHuL59M:&spf=1561485663238.*)

Leica RM2255 Microtome; prior to Jan. 31, 2018; 1 pg. 1; [https://www.google.com/search?q=controller+for+microtome&hl=en&biw=1536&bih=813&source=Int&tbs=cdr%3A1%2Ccd\\_min%3A%2Ccd\\_max%3A1%2F31%2F2018&tbs=isch#imgrc=gevAFoeqOcj-nM:&spf=1561485663243.\\*](https://www.google.com/search?q=controller+for+microtome&hl=en&biw=1536&bih=813&source=Int&tbs=cdr%3A1%2Ccd_min%3A%2Ccd_max%3A1%2F31%2F2018&tbs=isch#imgrc=gevAFoeqOcj-nM:&spf=1561485663243.*)

Leica RM2145 Microtome; prior to Jan. 31, 2017; 1 pg.; [https://www.google.com/search?q=controller+for+microtome&hl=en&biw=1536&bih=813&source=Int&tbs=cdr%3A1%2Ccd\\_min%3A%2Ccd\\_max%3A1%2F31%2F2017&tbs=isch#imgrc=CeonZuevd5S\\_tM:&spf=1561486237241.\\*](https://www.google.com/search?q=controller+for+microtome&hl=en&biw=1536&bih=813&source=Int&tbs=cdr%3A1%2Ccd_min%3A%2Ccd_max%3A1%2F31%2F2017&tbs=isch#imgrc=CeonZuevd5S_tM:&spf=1561486237241.*)

Cole Parmer, TBS SC4500; prior to Jan. 31, 2017; 1 pg.; [https://www.google.com/search?q=controller+for+microtome&hl=en&biw=1536&bih=813&source=Int&tbs=cdr%3A1%2Ccd\\_min%3A%2Ccd\\_max%3A1%2F31%2F2017&tbs=isch#imgrc=ok9DwQQPJM\\_ATM:&spf=1561486477574.\\*](https://www.google.com/search?q=controller+for+microtome&hl=en&biw=1536&bih=813&source=Int&tbs=cdr%3A1%2Ccd_min%3A%2Ccd_max%3A1%2F31%2F2017&tbs=isch#imgrc=ok9DwQQPJM_ATM:&spf=1561486477574.*)

\* cited by examiner

*Primary Examiner* — Selina Sikder  
(74) *Attorney, Agent, or Firm* — Hodgson Russ LLP


(57) **CLAIM**

The ornamental design for a control panel, as shown and described.

**DESCRIPTION**

FIG. 1 is perspective view of a first embodiment of a control panel showing our new design;  
 FIG. 2 is a front elevation view thereof;  
 FIG. 3 is a rear elevation view thereof;  
 FIG. 4 is a right side elevation view thereof;  
 FIG. 5 is a left side elevation view thereof;  
 FIG. 6 is a bottom plan view thereof; and,  
 FIG. 7 is a top plan view thereof.  
 The broken lines illustrate unclaimed portions of the control panel that form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

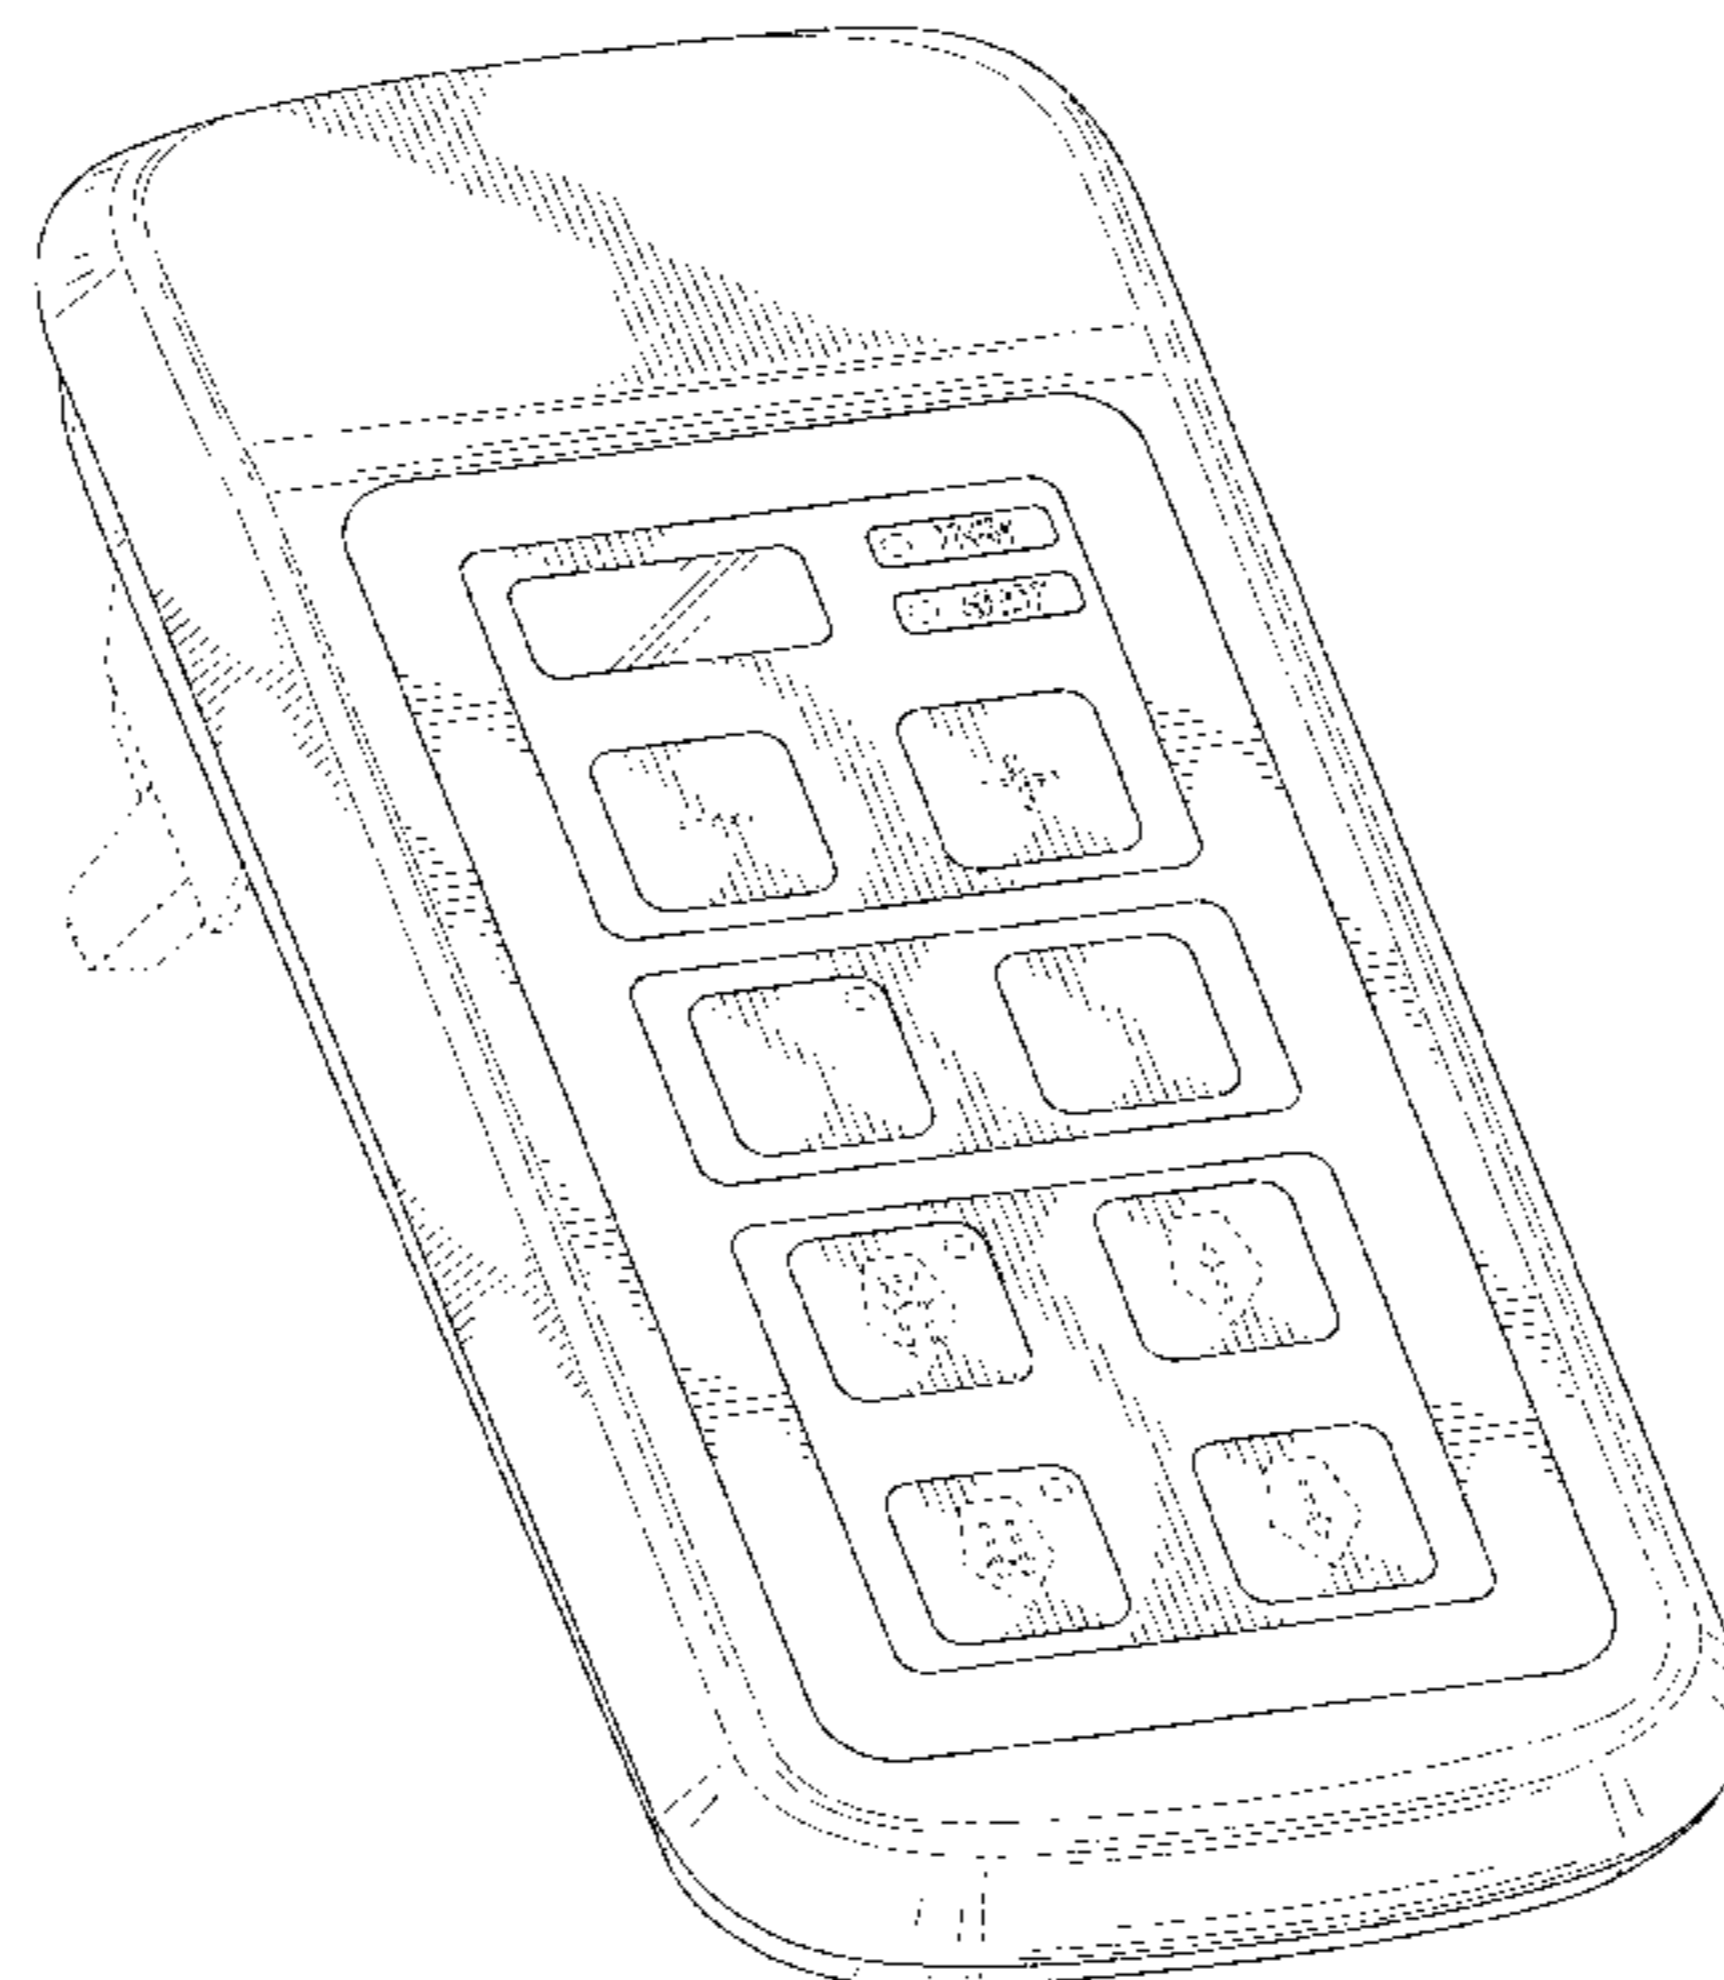

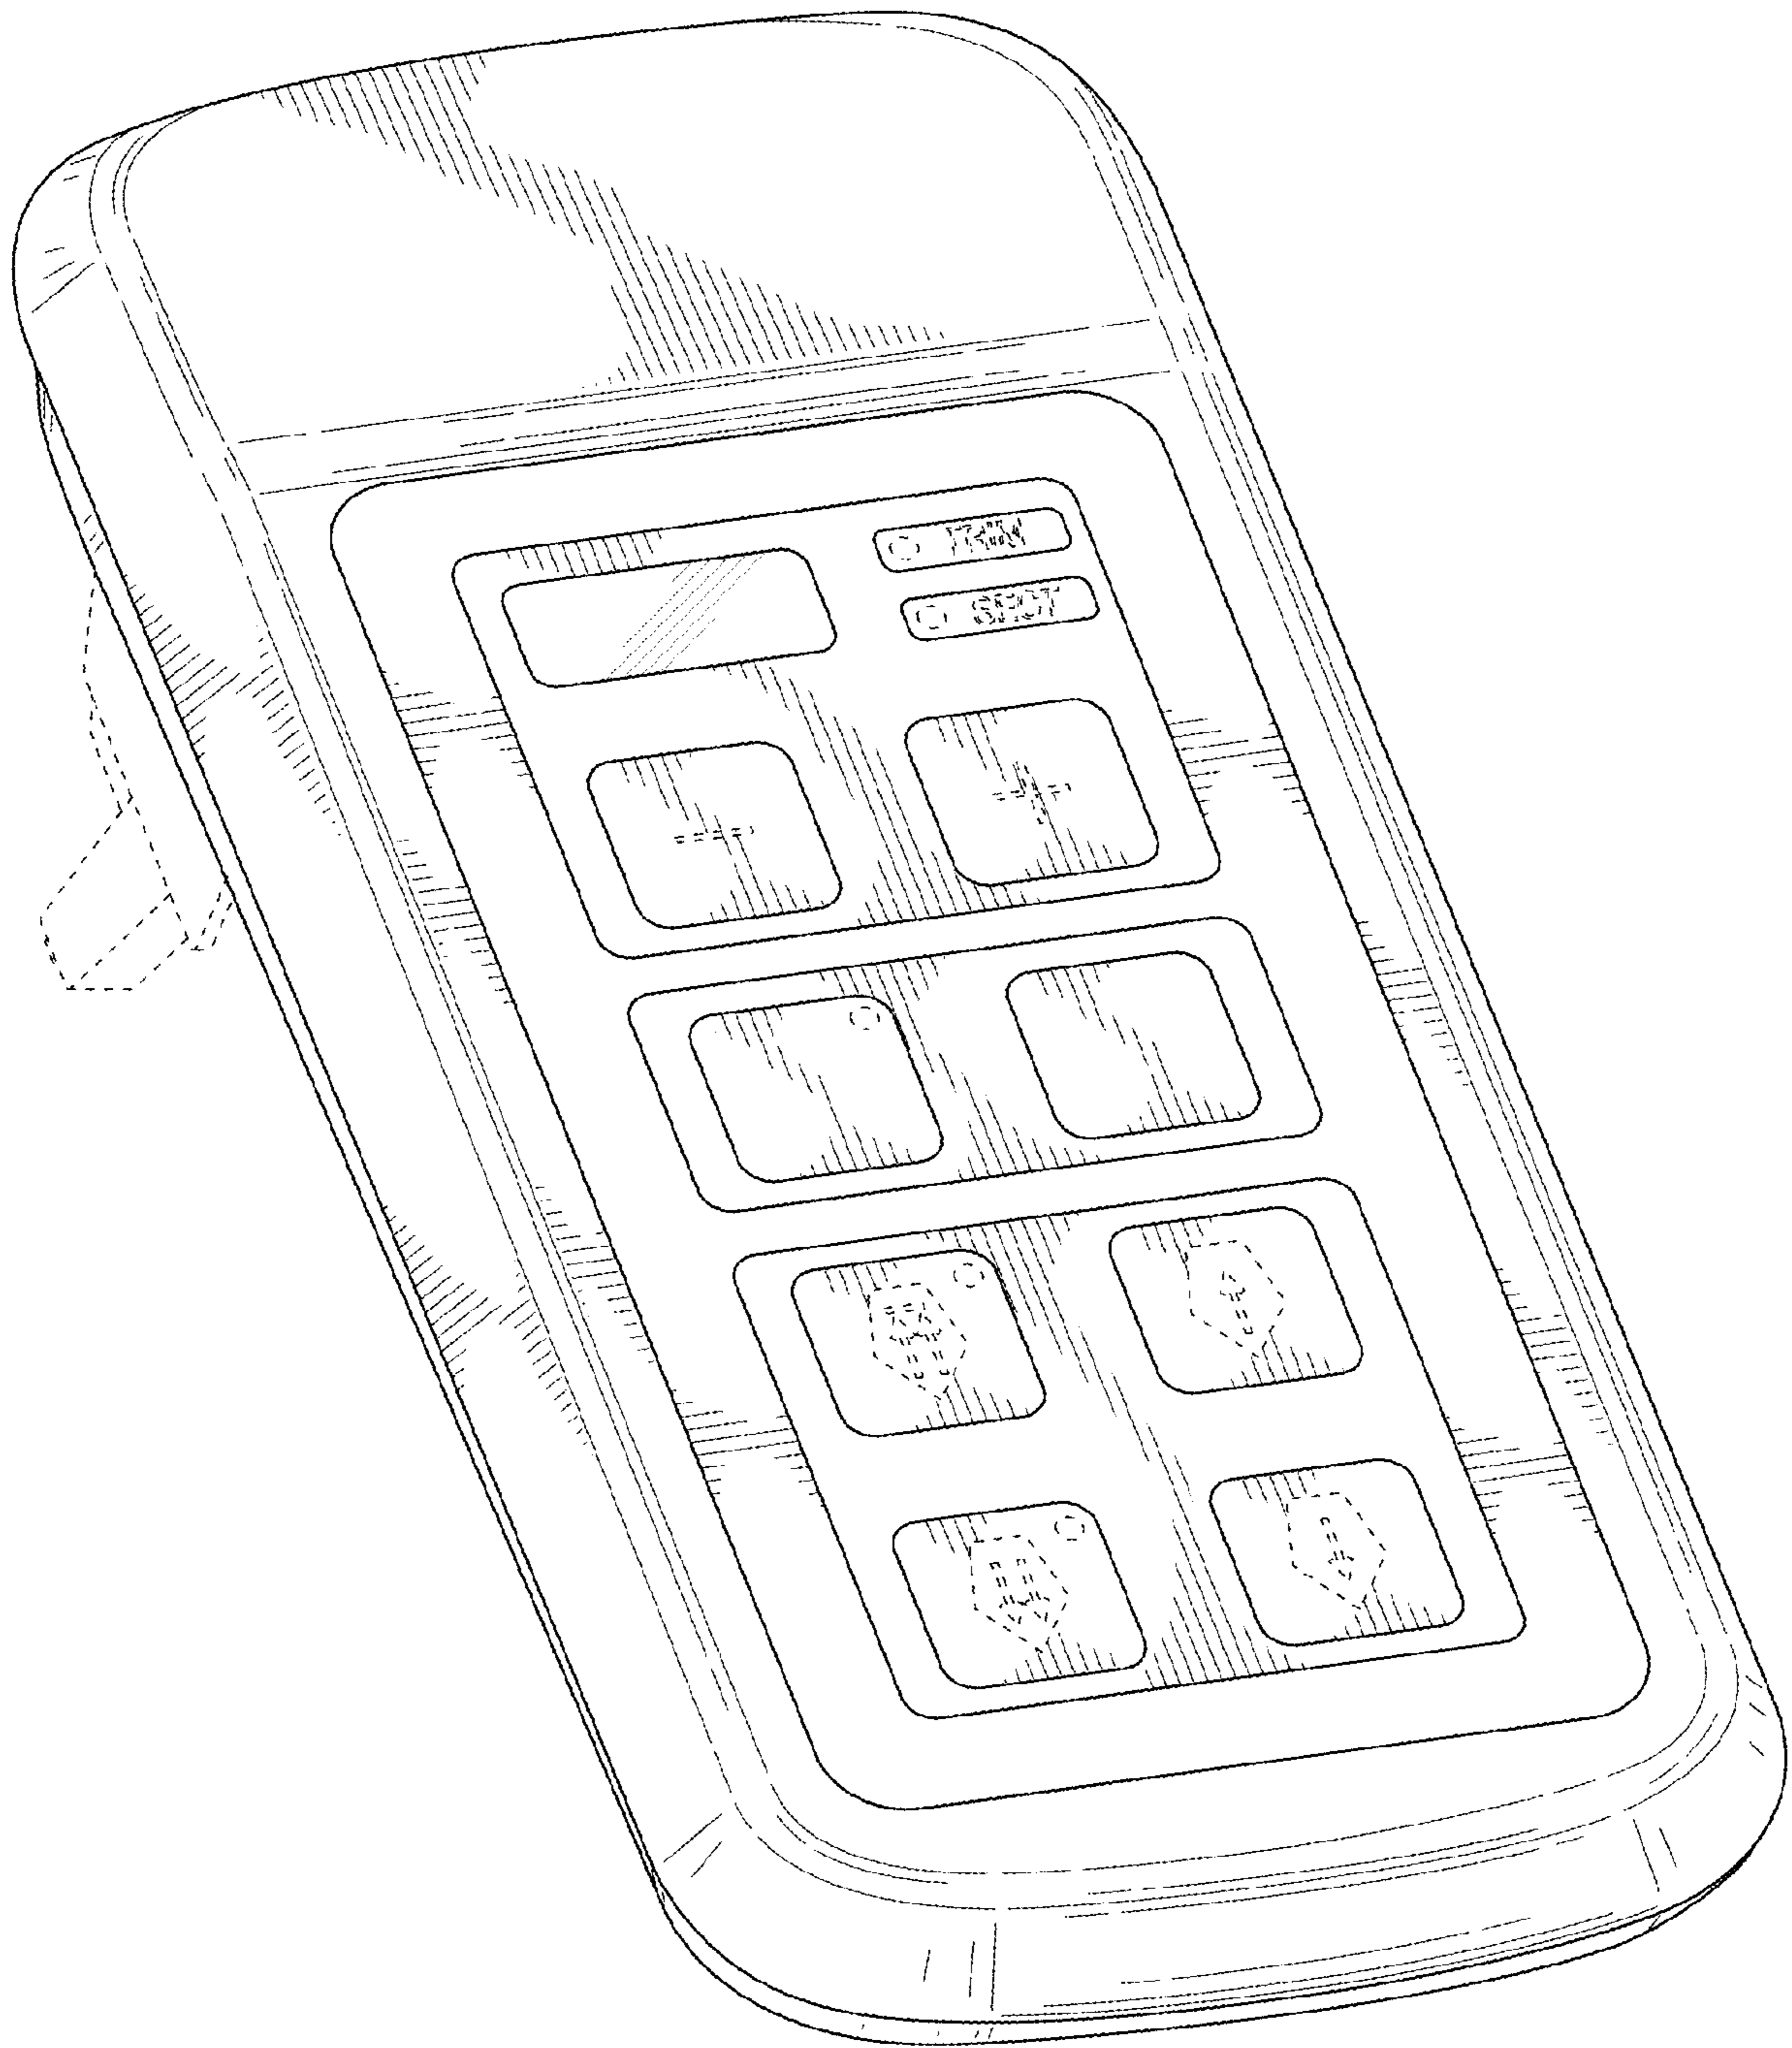


FIG. 1

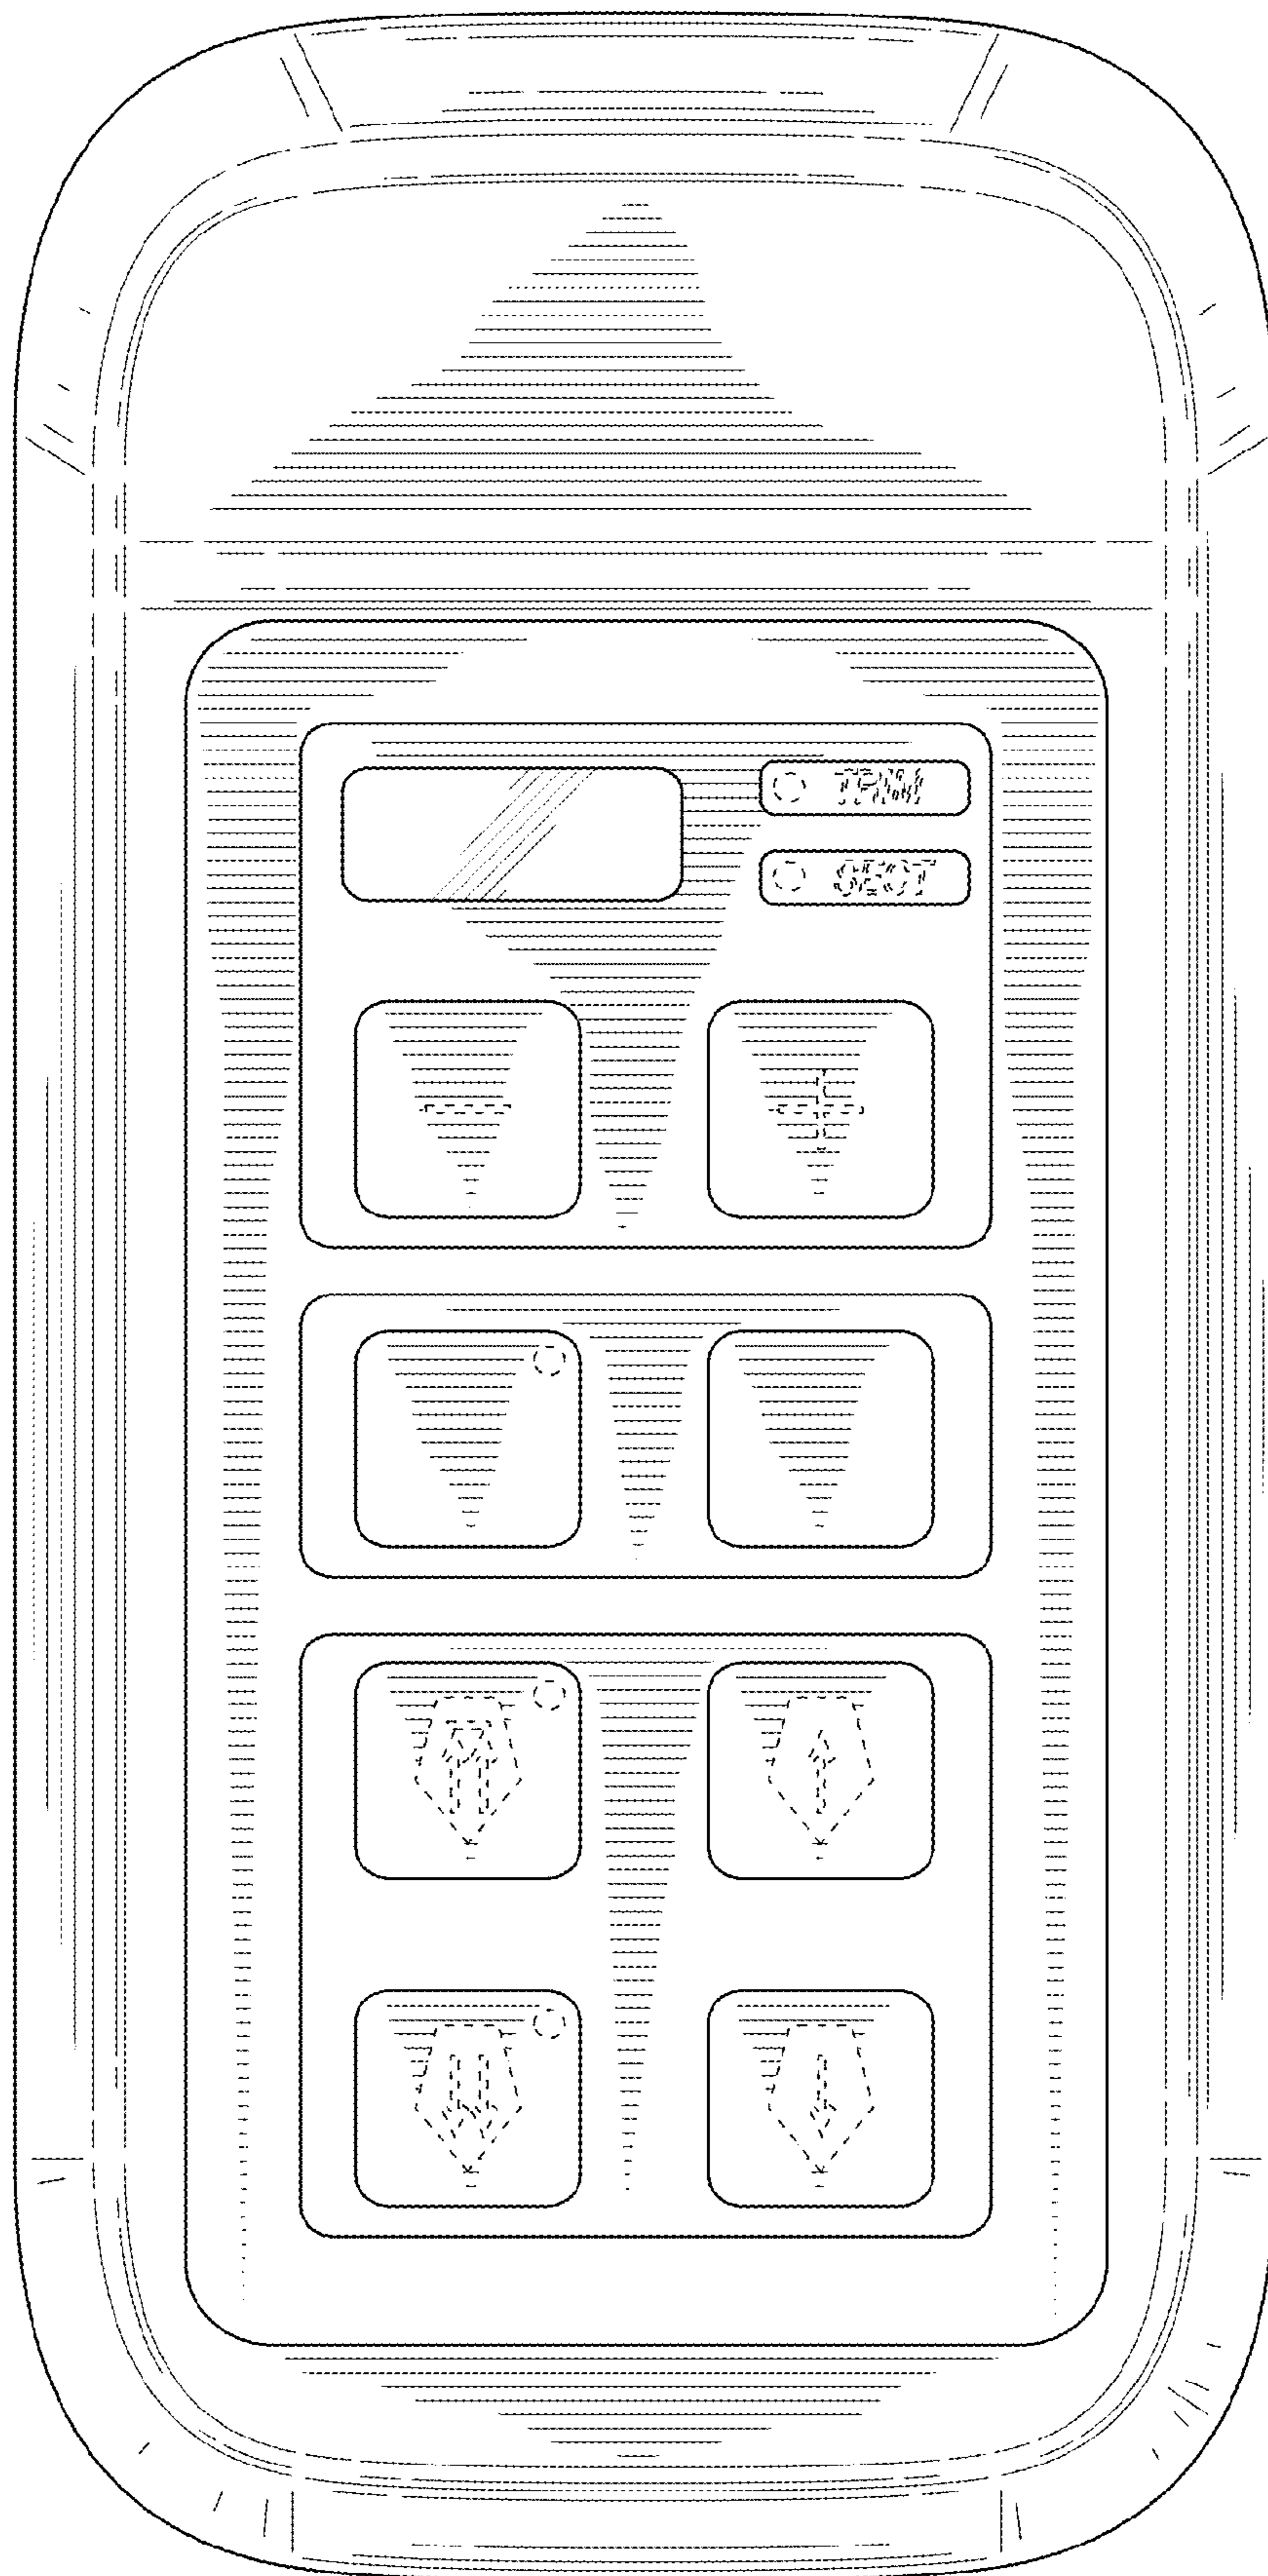


FIG. 2

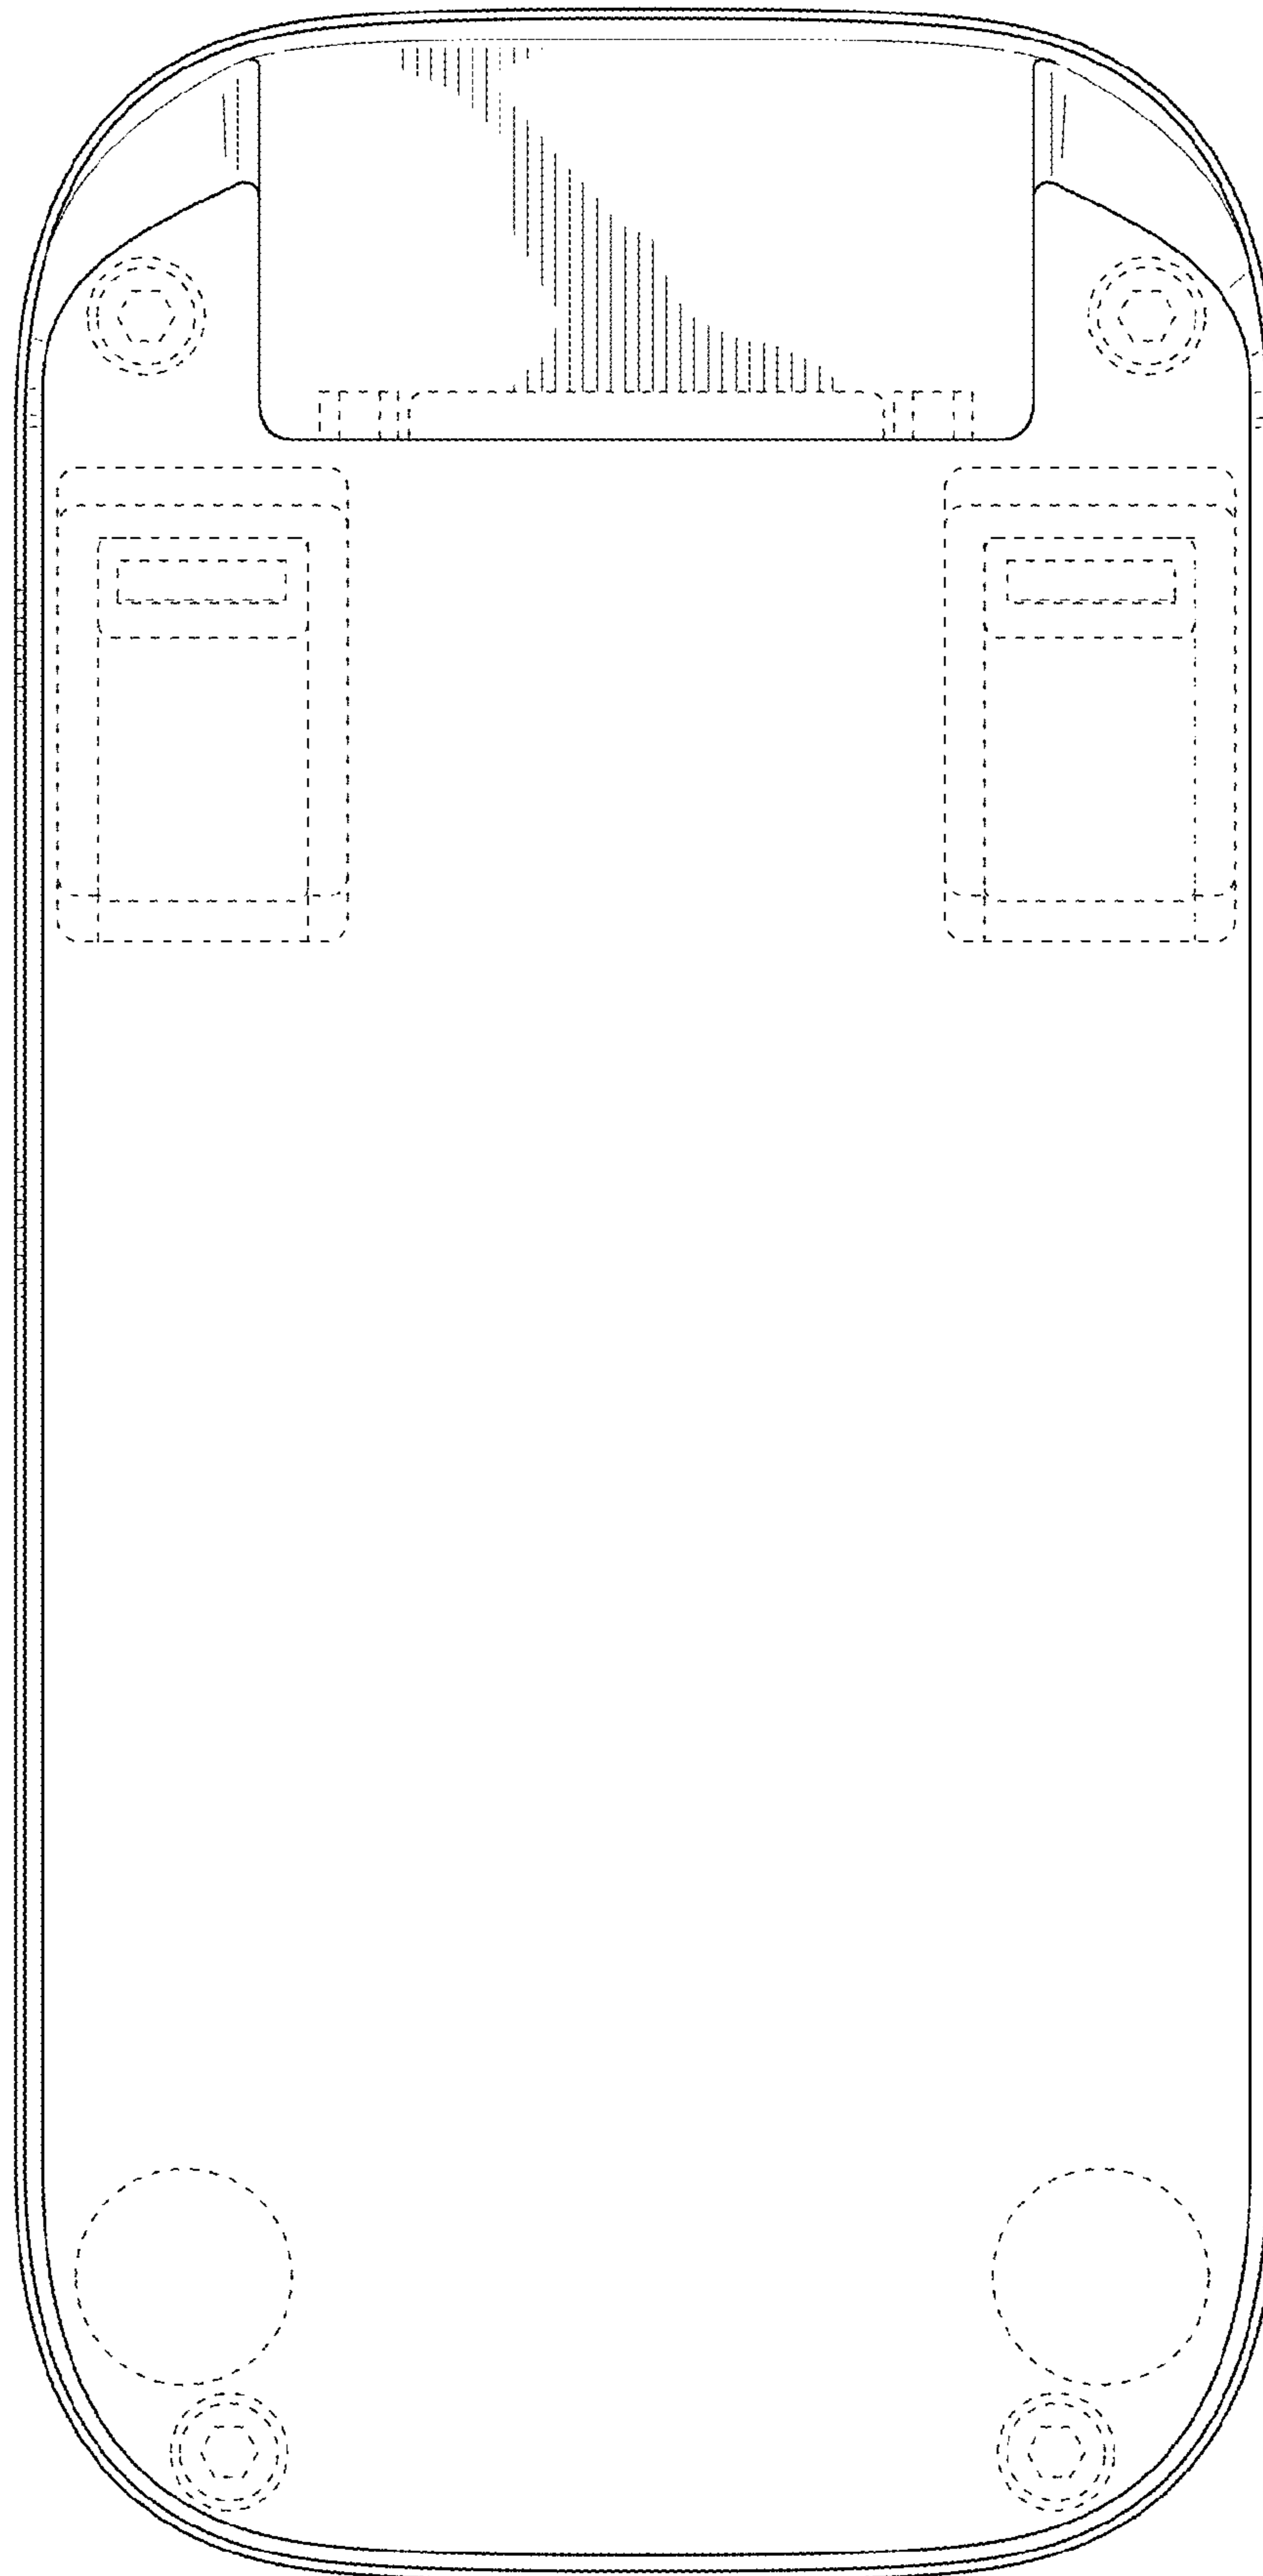


FIG. 3

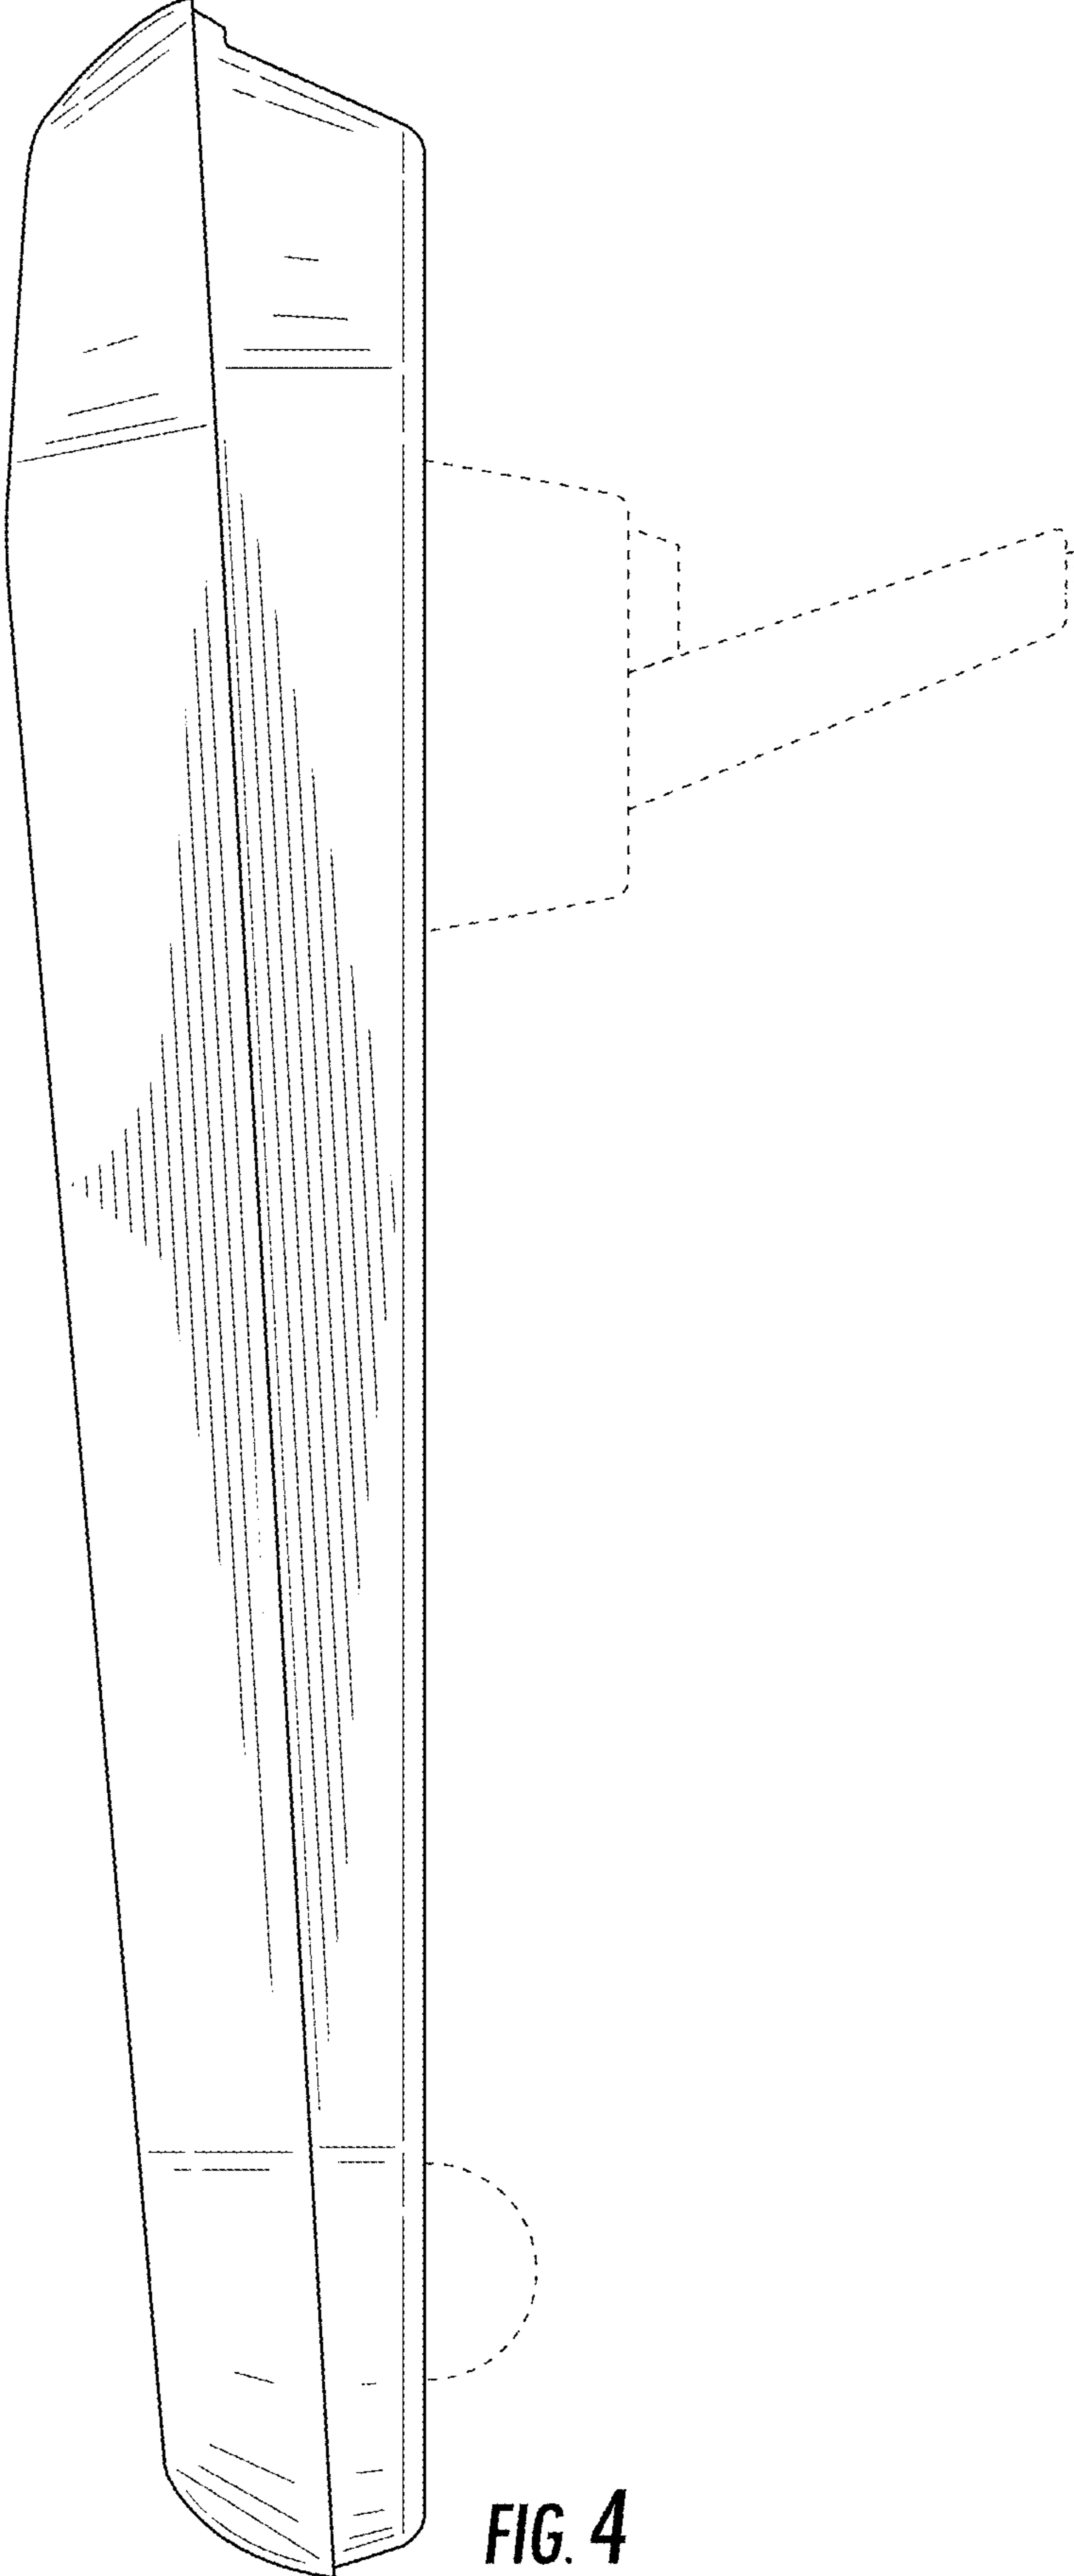


FIG. 4

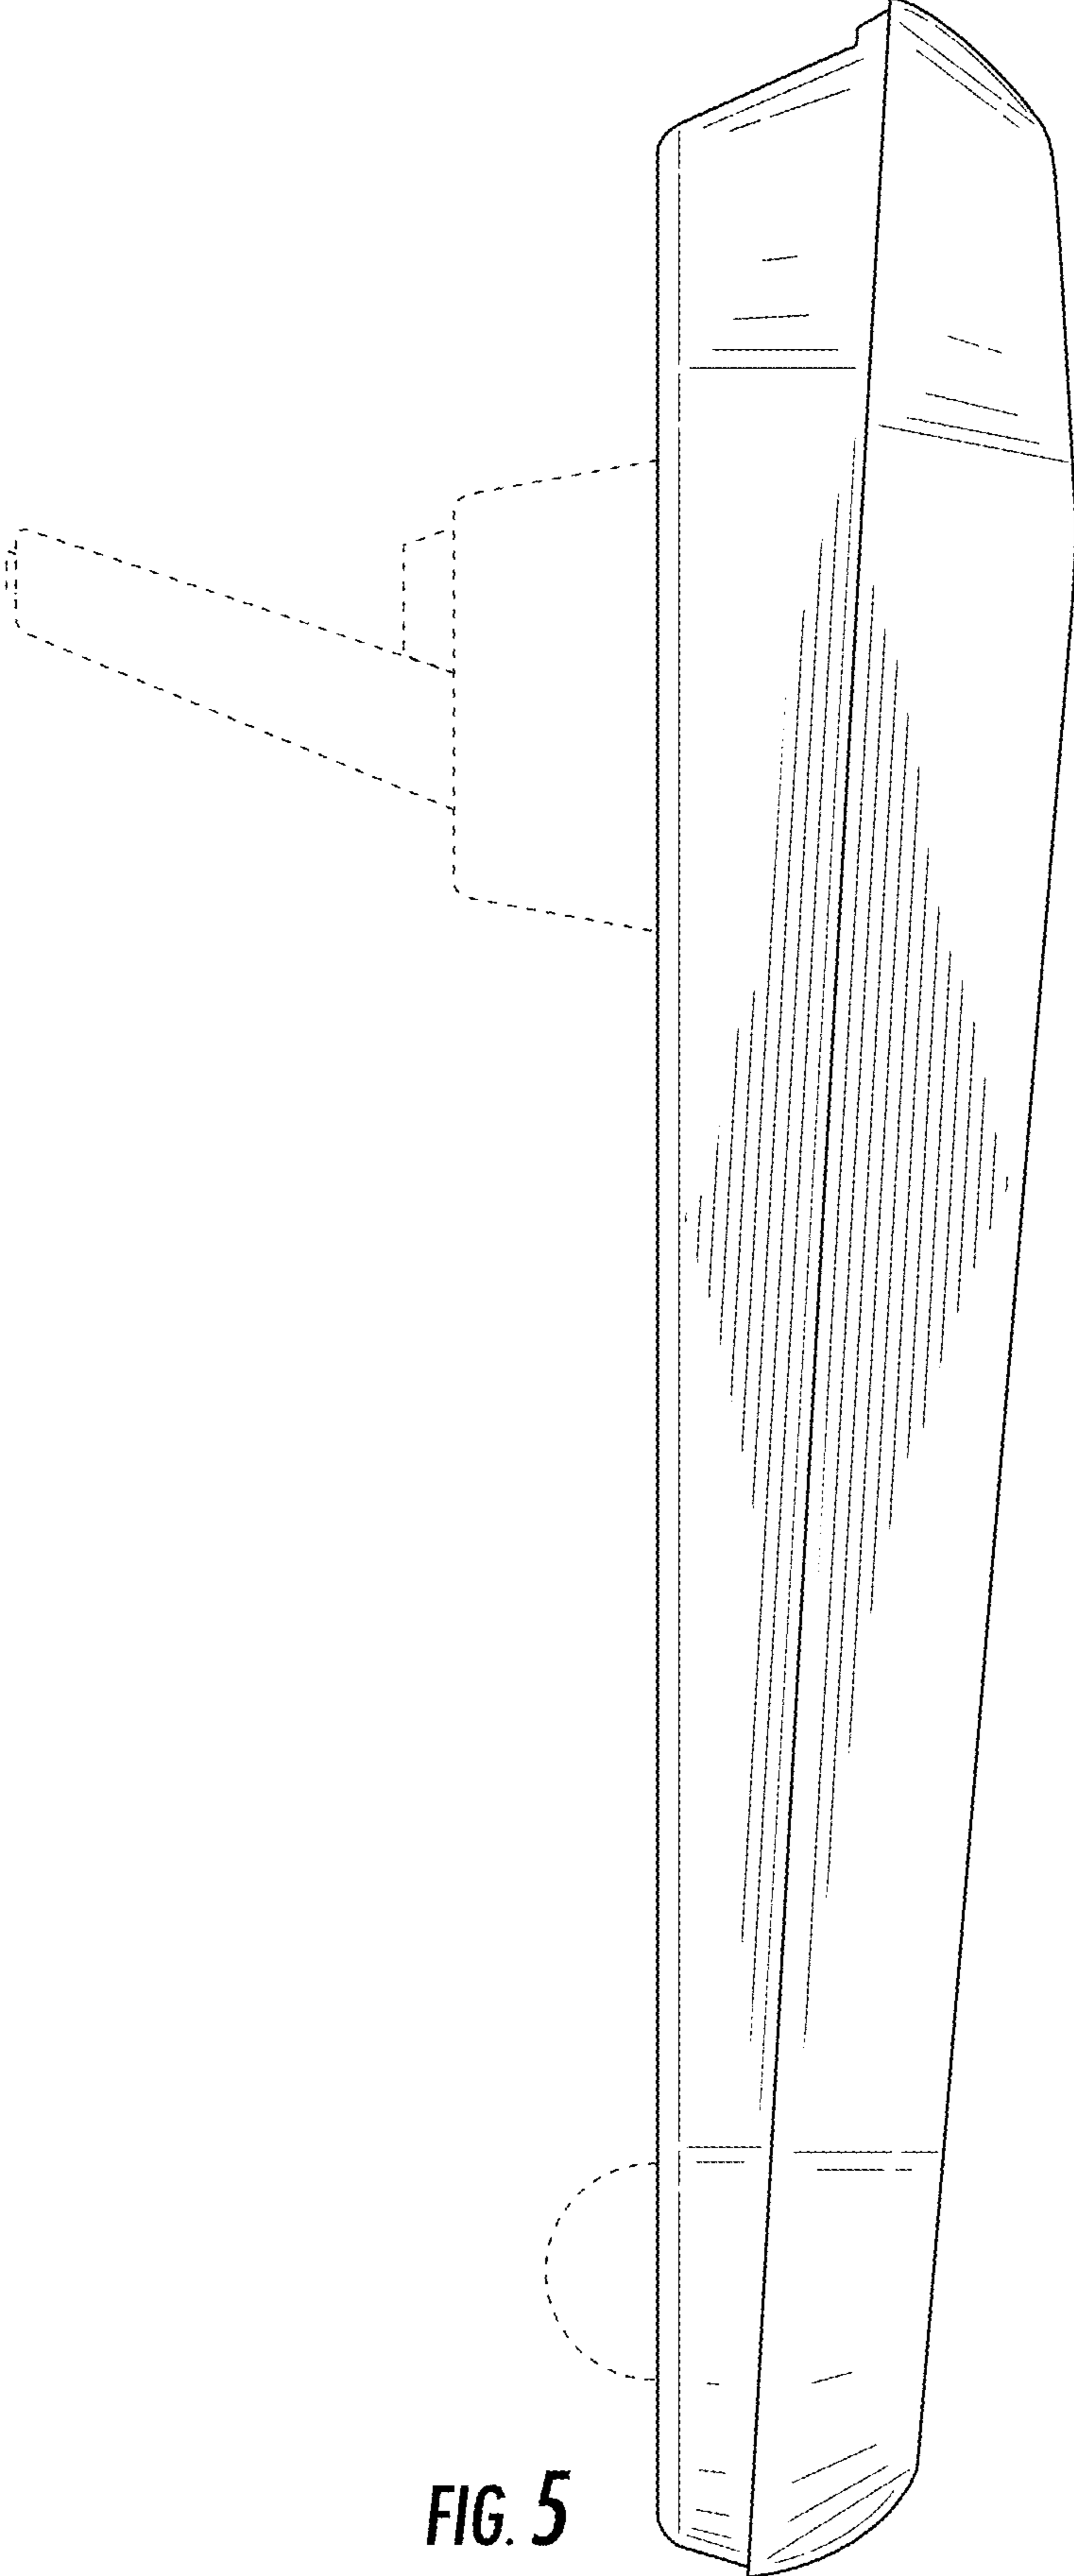


FIG. 5

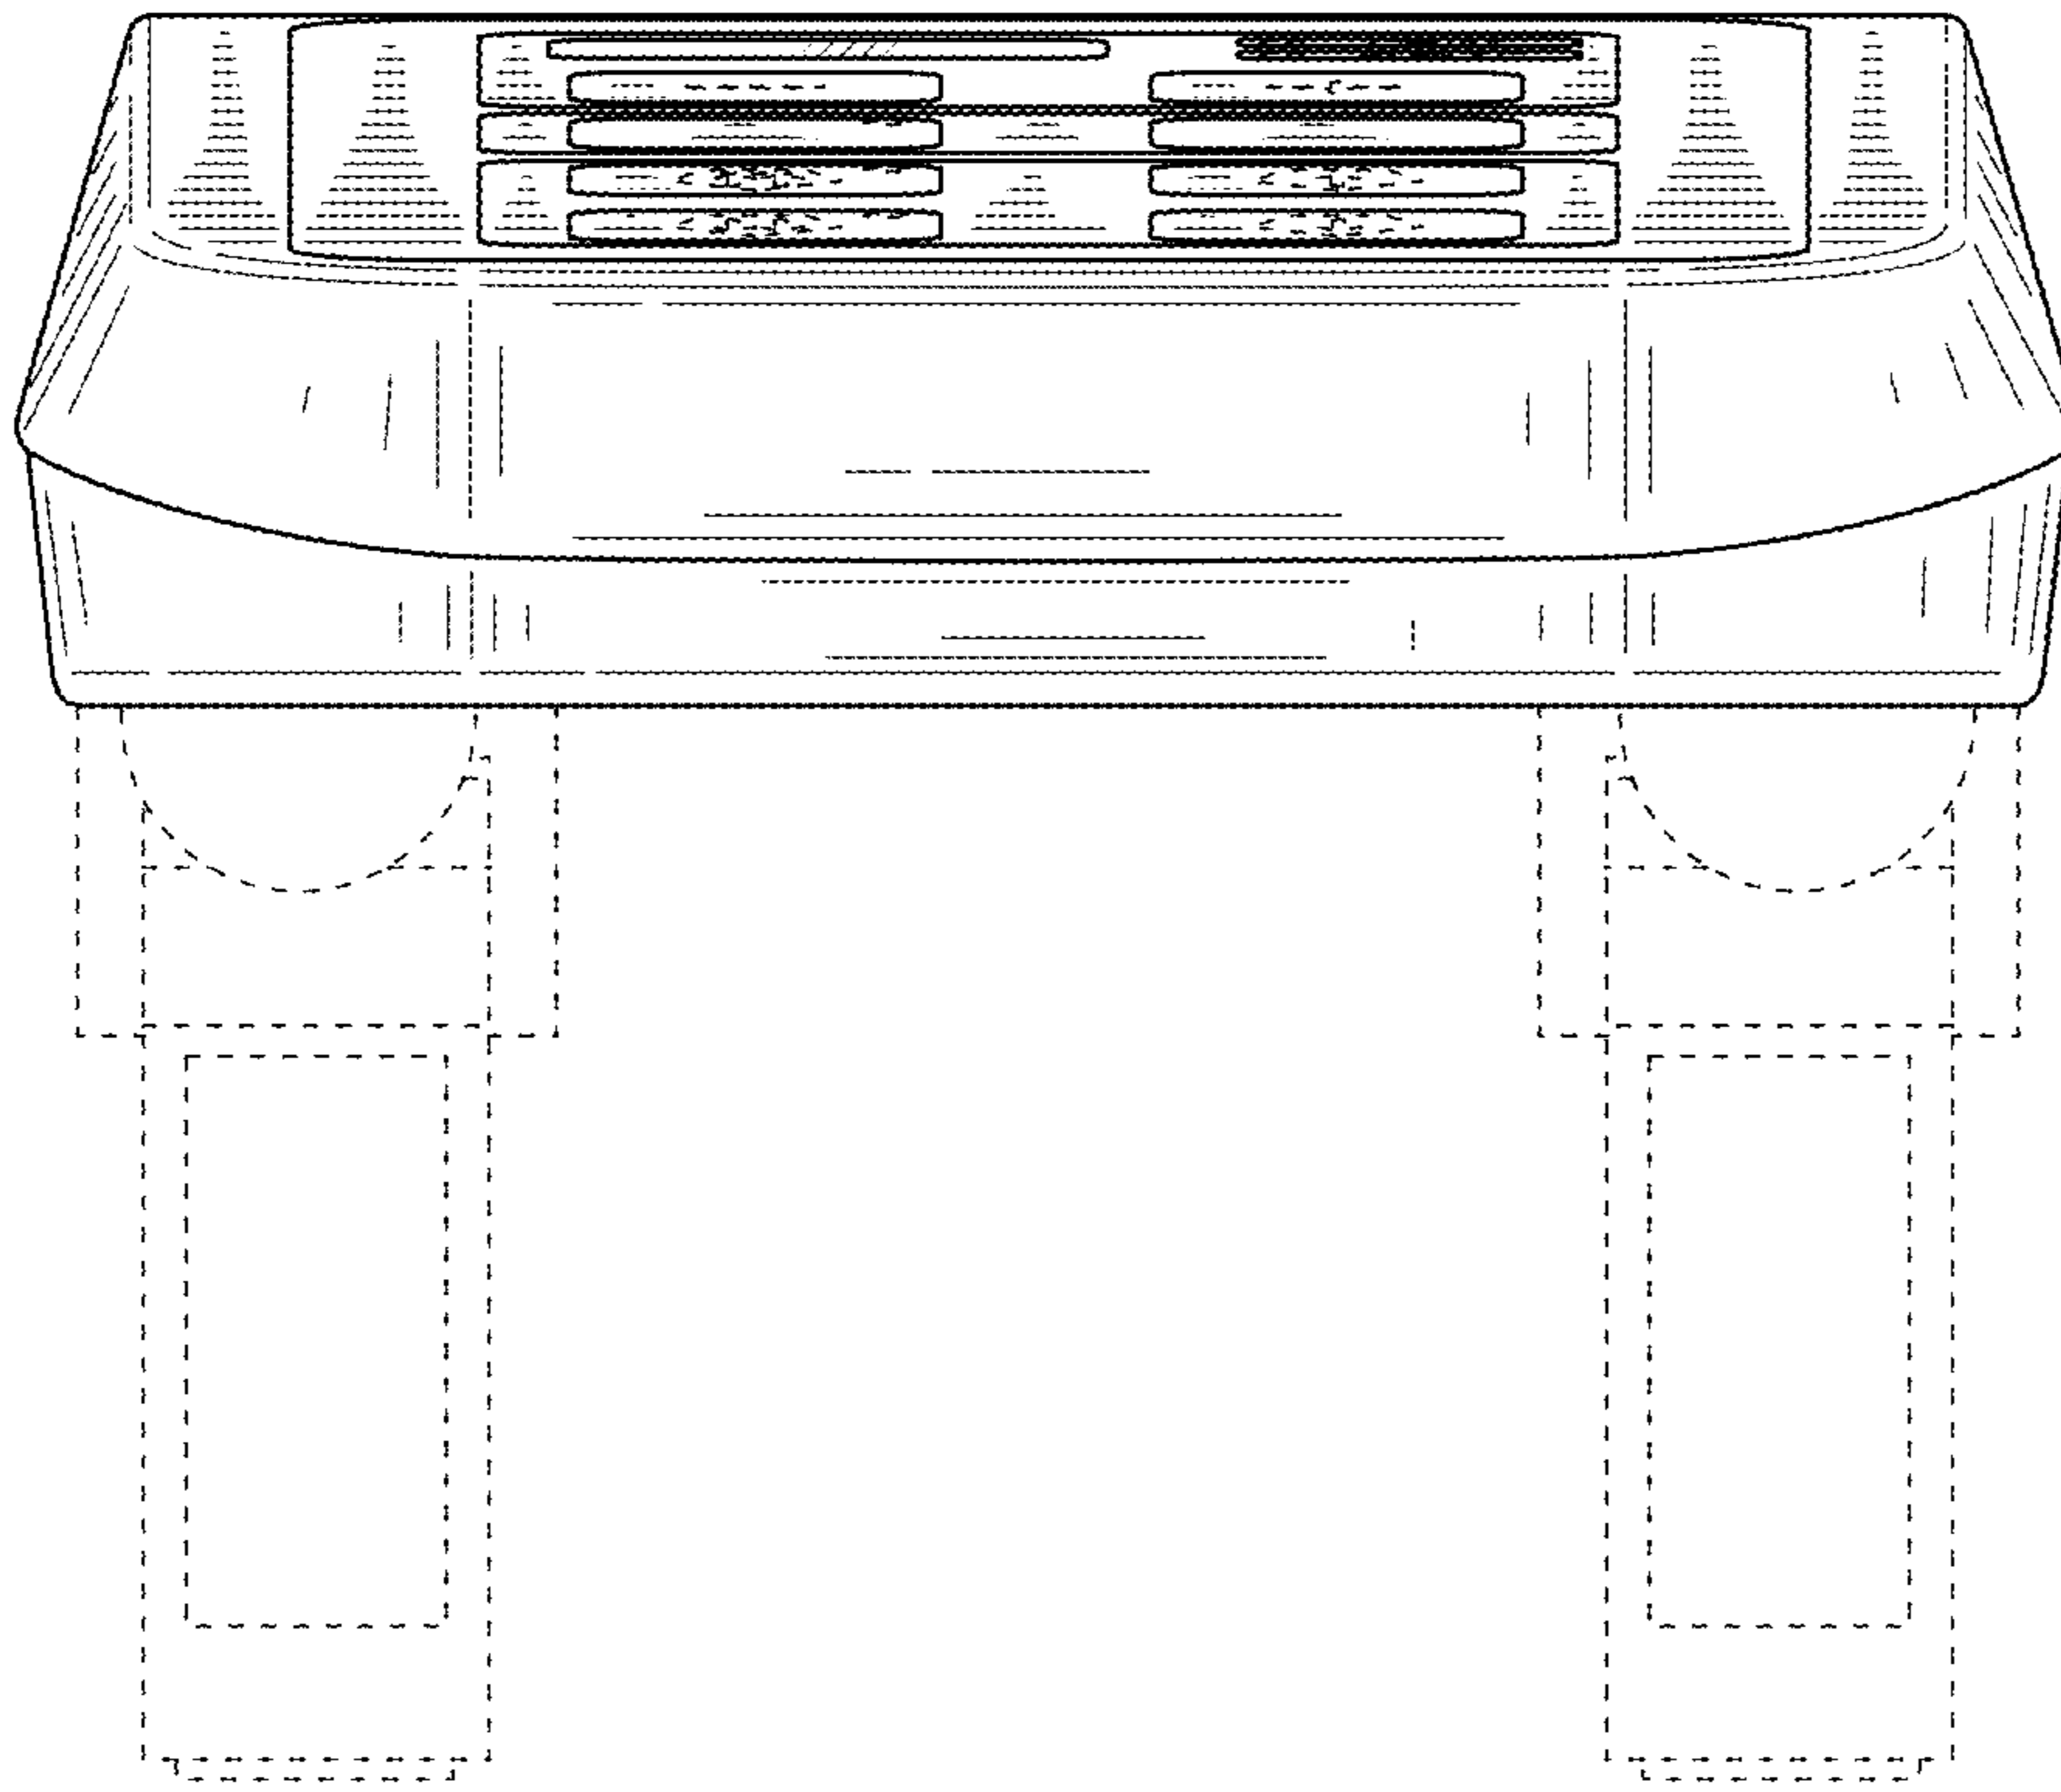


FIG. 6

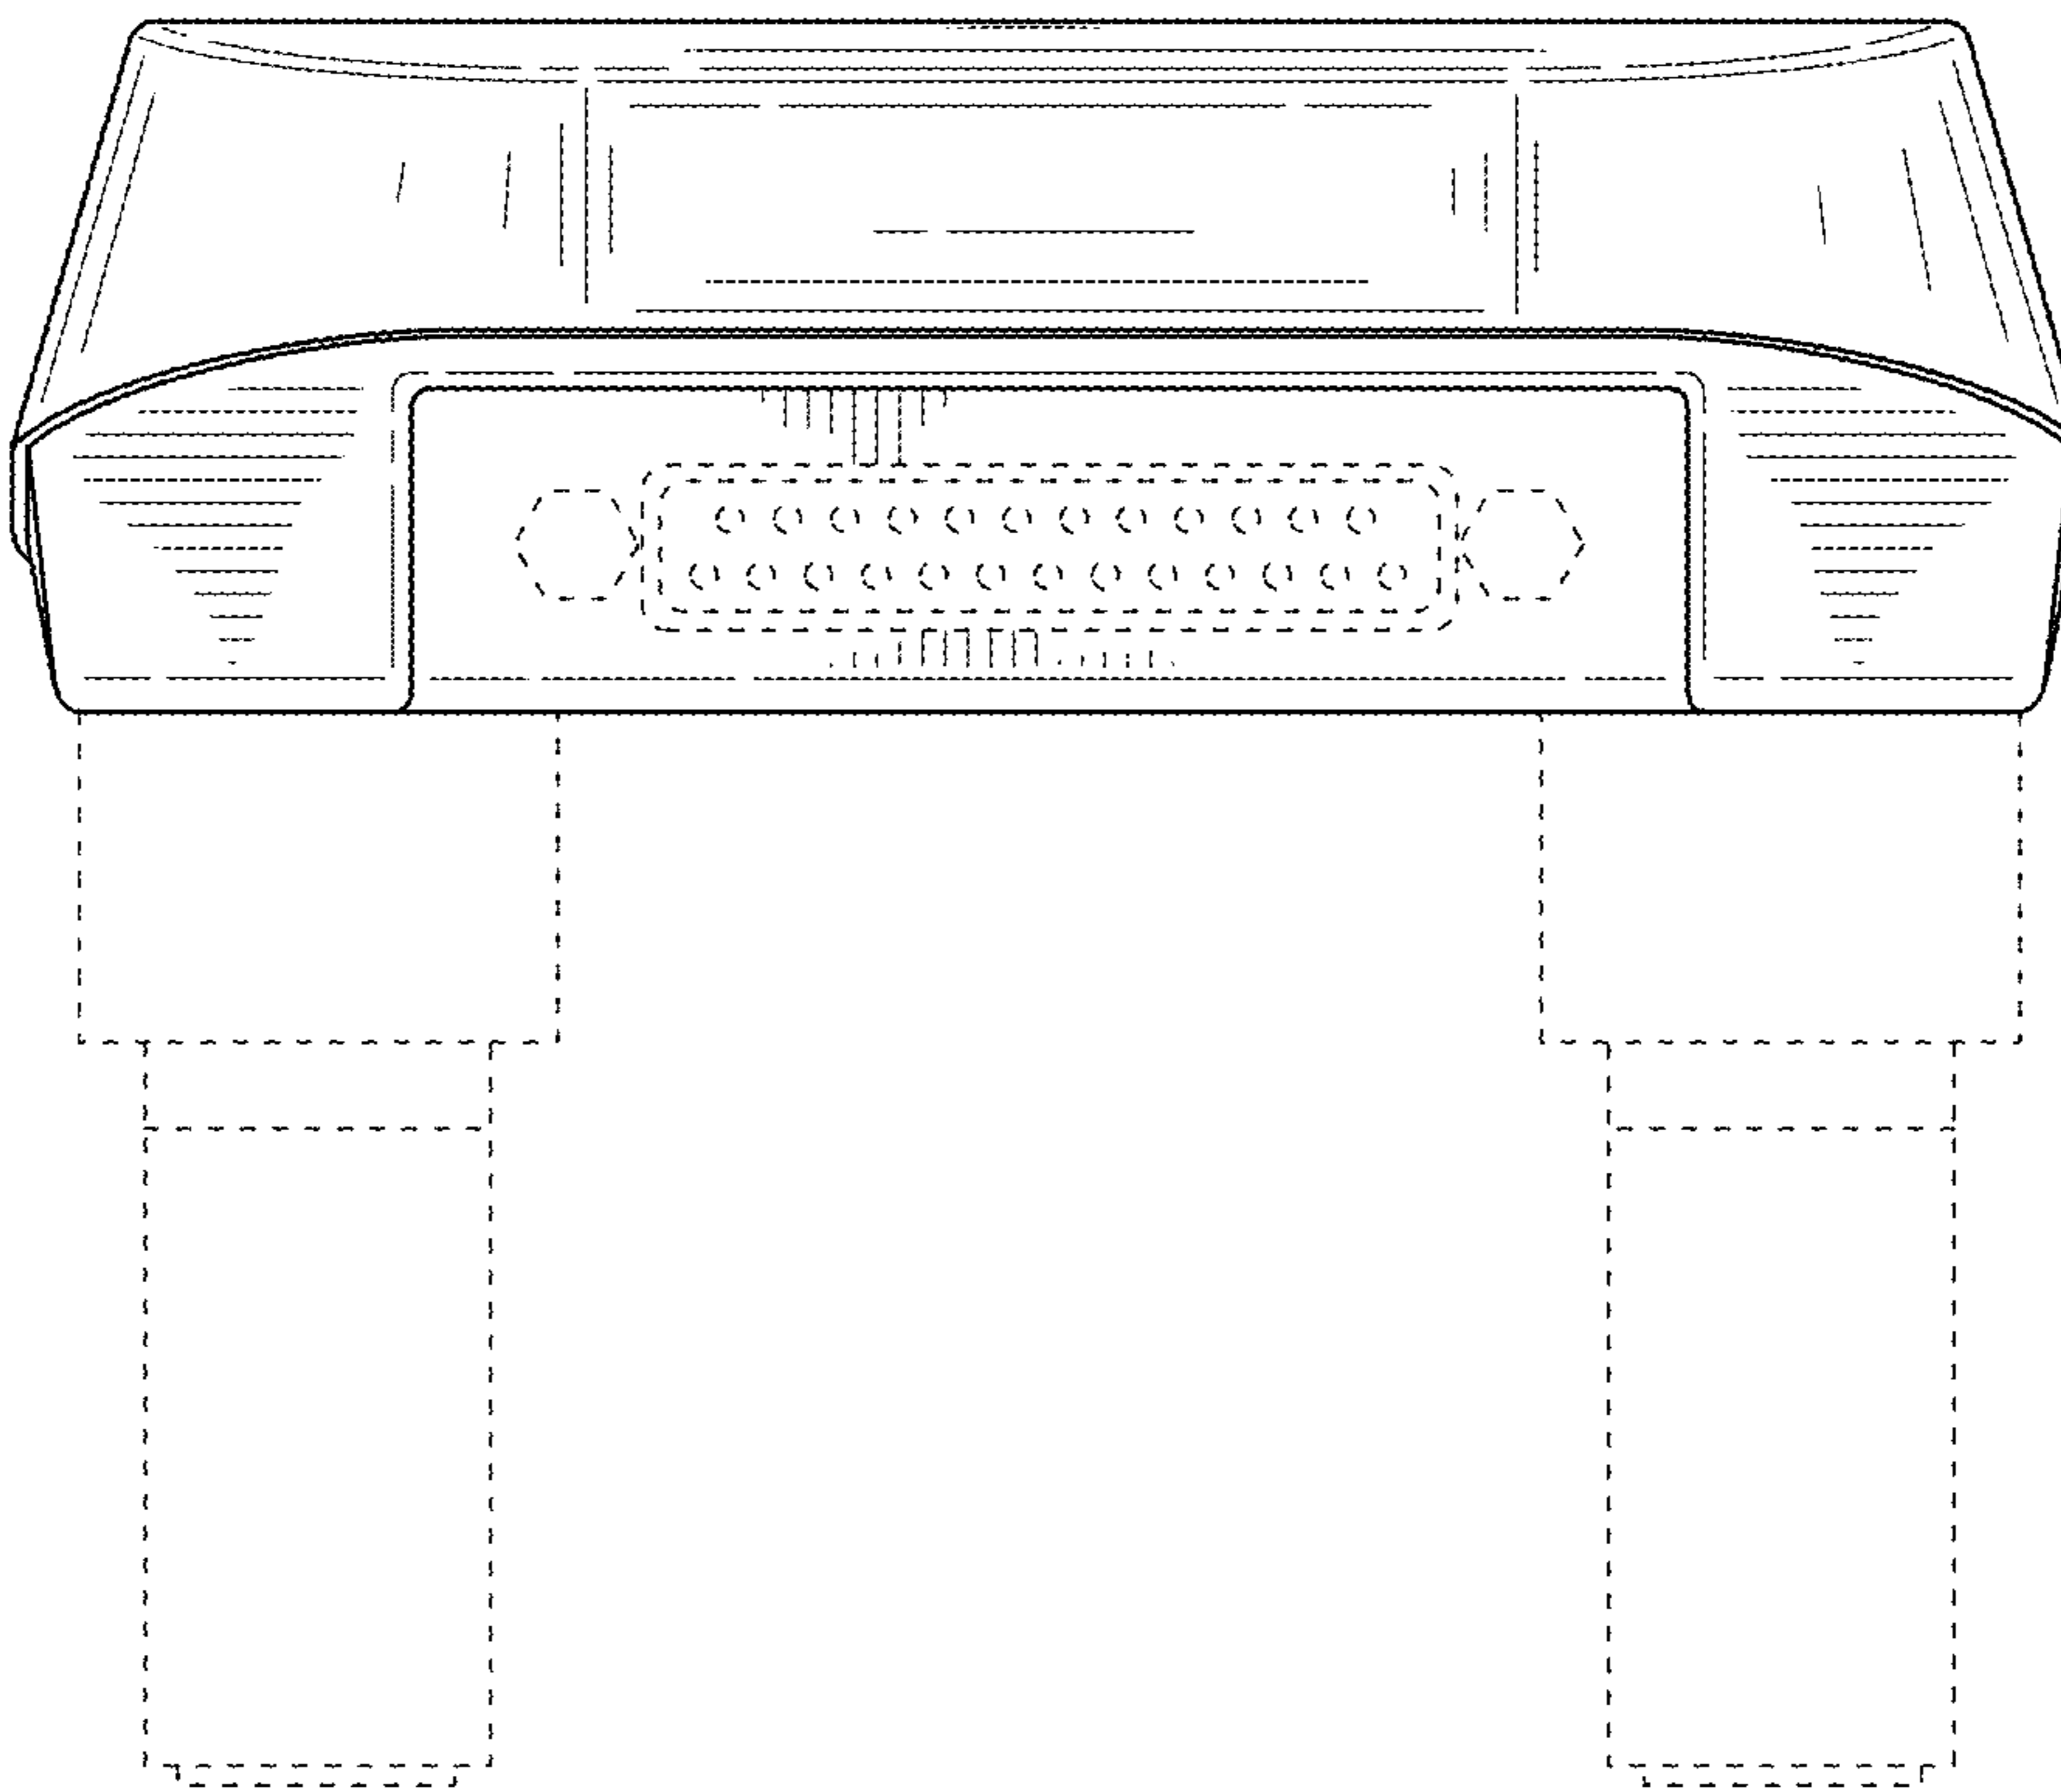


FIG. 7