



US00D875254S

(12) **United States Design Patent** (10) **Patent No.:** **US D875,254 S**
Cooke et al. (45) **Date of Patent:** **** Feb. 11, 2020**

(54) **INTRADERMAL BIOSENSOR**
(71) Applicant: **Biolinq, Inc.**, San Diego, CA (US)
(72) Inventors: **Cory Cooke**, San Francisco, CA (US);
Joshua Windmiller, Del Mar, CA (US); **Jared Rylan Tangney**, Encinitas, CA (US)

6,284,126 B1 9/2001 Kurnik et al.
6,413,396 B1 7/2002 Yang et al.
6,471,903 B2 10/2002 Sherman et al.
6,603,987 B2 8/2003 Whitson
6,814,845 B2 11/2004 Wilson et al.
6,862,466 B2 3/2005 Ackerman
6,908,453 B2 6/2005 Fleming et al.
7,097,776 B2 8/2006 Raju

(Continued)

(73) Assignee: **Biolinq, Inc.**, San Diego, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/650,794**

(22) Filed: **Jun. 8, 2018**

(51) **LOC (12) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/169**

(58) **Field of Classification Search**
USPC D24/164-169, 186, 187, 107, 216;
D10/70, 75, 78, 98, 103; D14/344,
D14/138 R, 138 AA
CPC A61B 5/14532; A61B 5/14865; A61B
2560/0412; A61B 2560/0443; A61B
2560/0462; A61M 25/0606; A61M
25/0631

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,305,401 A 12/1981 Reissmueller et al.
4,323,996 A 4/1982 Ganter
4,407,295 A 10/1983 Steuer et al.
5,131,390 A 7/1992 Sakaguchi et al.
5,279,543 A 1/1994 Glikfeld et al.
5,286,364 A 2/1994 Yacynych et al.
5,540,828 A 7/1996 Yacynych
5,730,714 A 3/1998 Guy et al.
5,766,132 A 6/1998 Yasukawa et al.
6,036,055 A 3/2000 Mogadam et al.
6,139,718 A 10/2000 Kurnik et al.
6,269,053 B1 7/2001 Kawata et al.

OTHER PUBLICATIONS

The Intelligent Continuous Glucose Monitoring System, posted at biolinq.me, no posting date, online, URL:https://www.biolinq.me/ (Year: 2019).*

Primary Examiner — Barbara Fox

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Clause Eight IPS; Michael Catania

(57) **CLAIM**


The ornamental design for an intradermal biosensor, as shown and described.

DESCRIPTION

FIG. 1 is a top plan view of an intradermal biosensor, showing our new design;
FIG. 2 is a bottom plan view thereof;
FIG. 3 is a front elevation view thereof;
FIG. 4 is a rear elevation view thereof;
FIG. 5 is a side elevation view thereof;
FIG. 6 is a side elevation view thereof;
FIG. 7 is an exploded view thereof; and,
FIG. 8 is a perspective view showing the intradermal biosensor worn by a user.

The broken lines showing a human figure and the internal components of an intradermal biosensor are for the purpose of depicting environmental subject matter that forms no part of the claimed design.

1 Claim, 4 Drawing Sheets

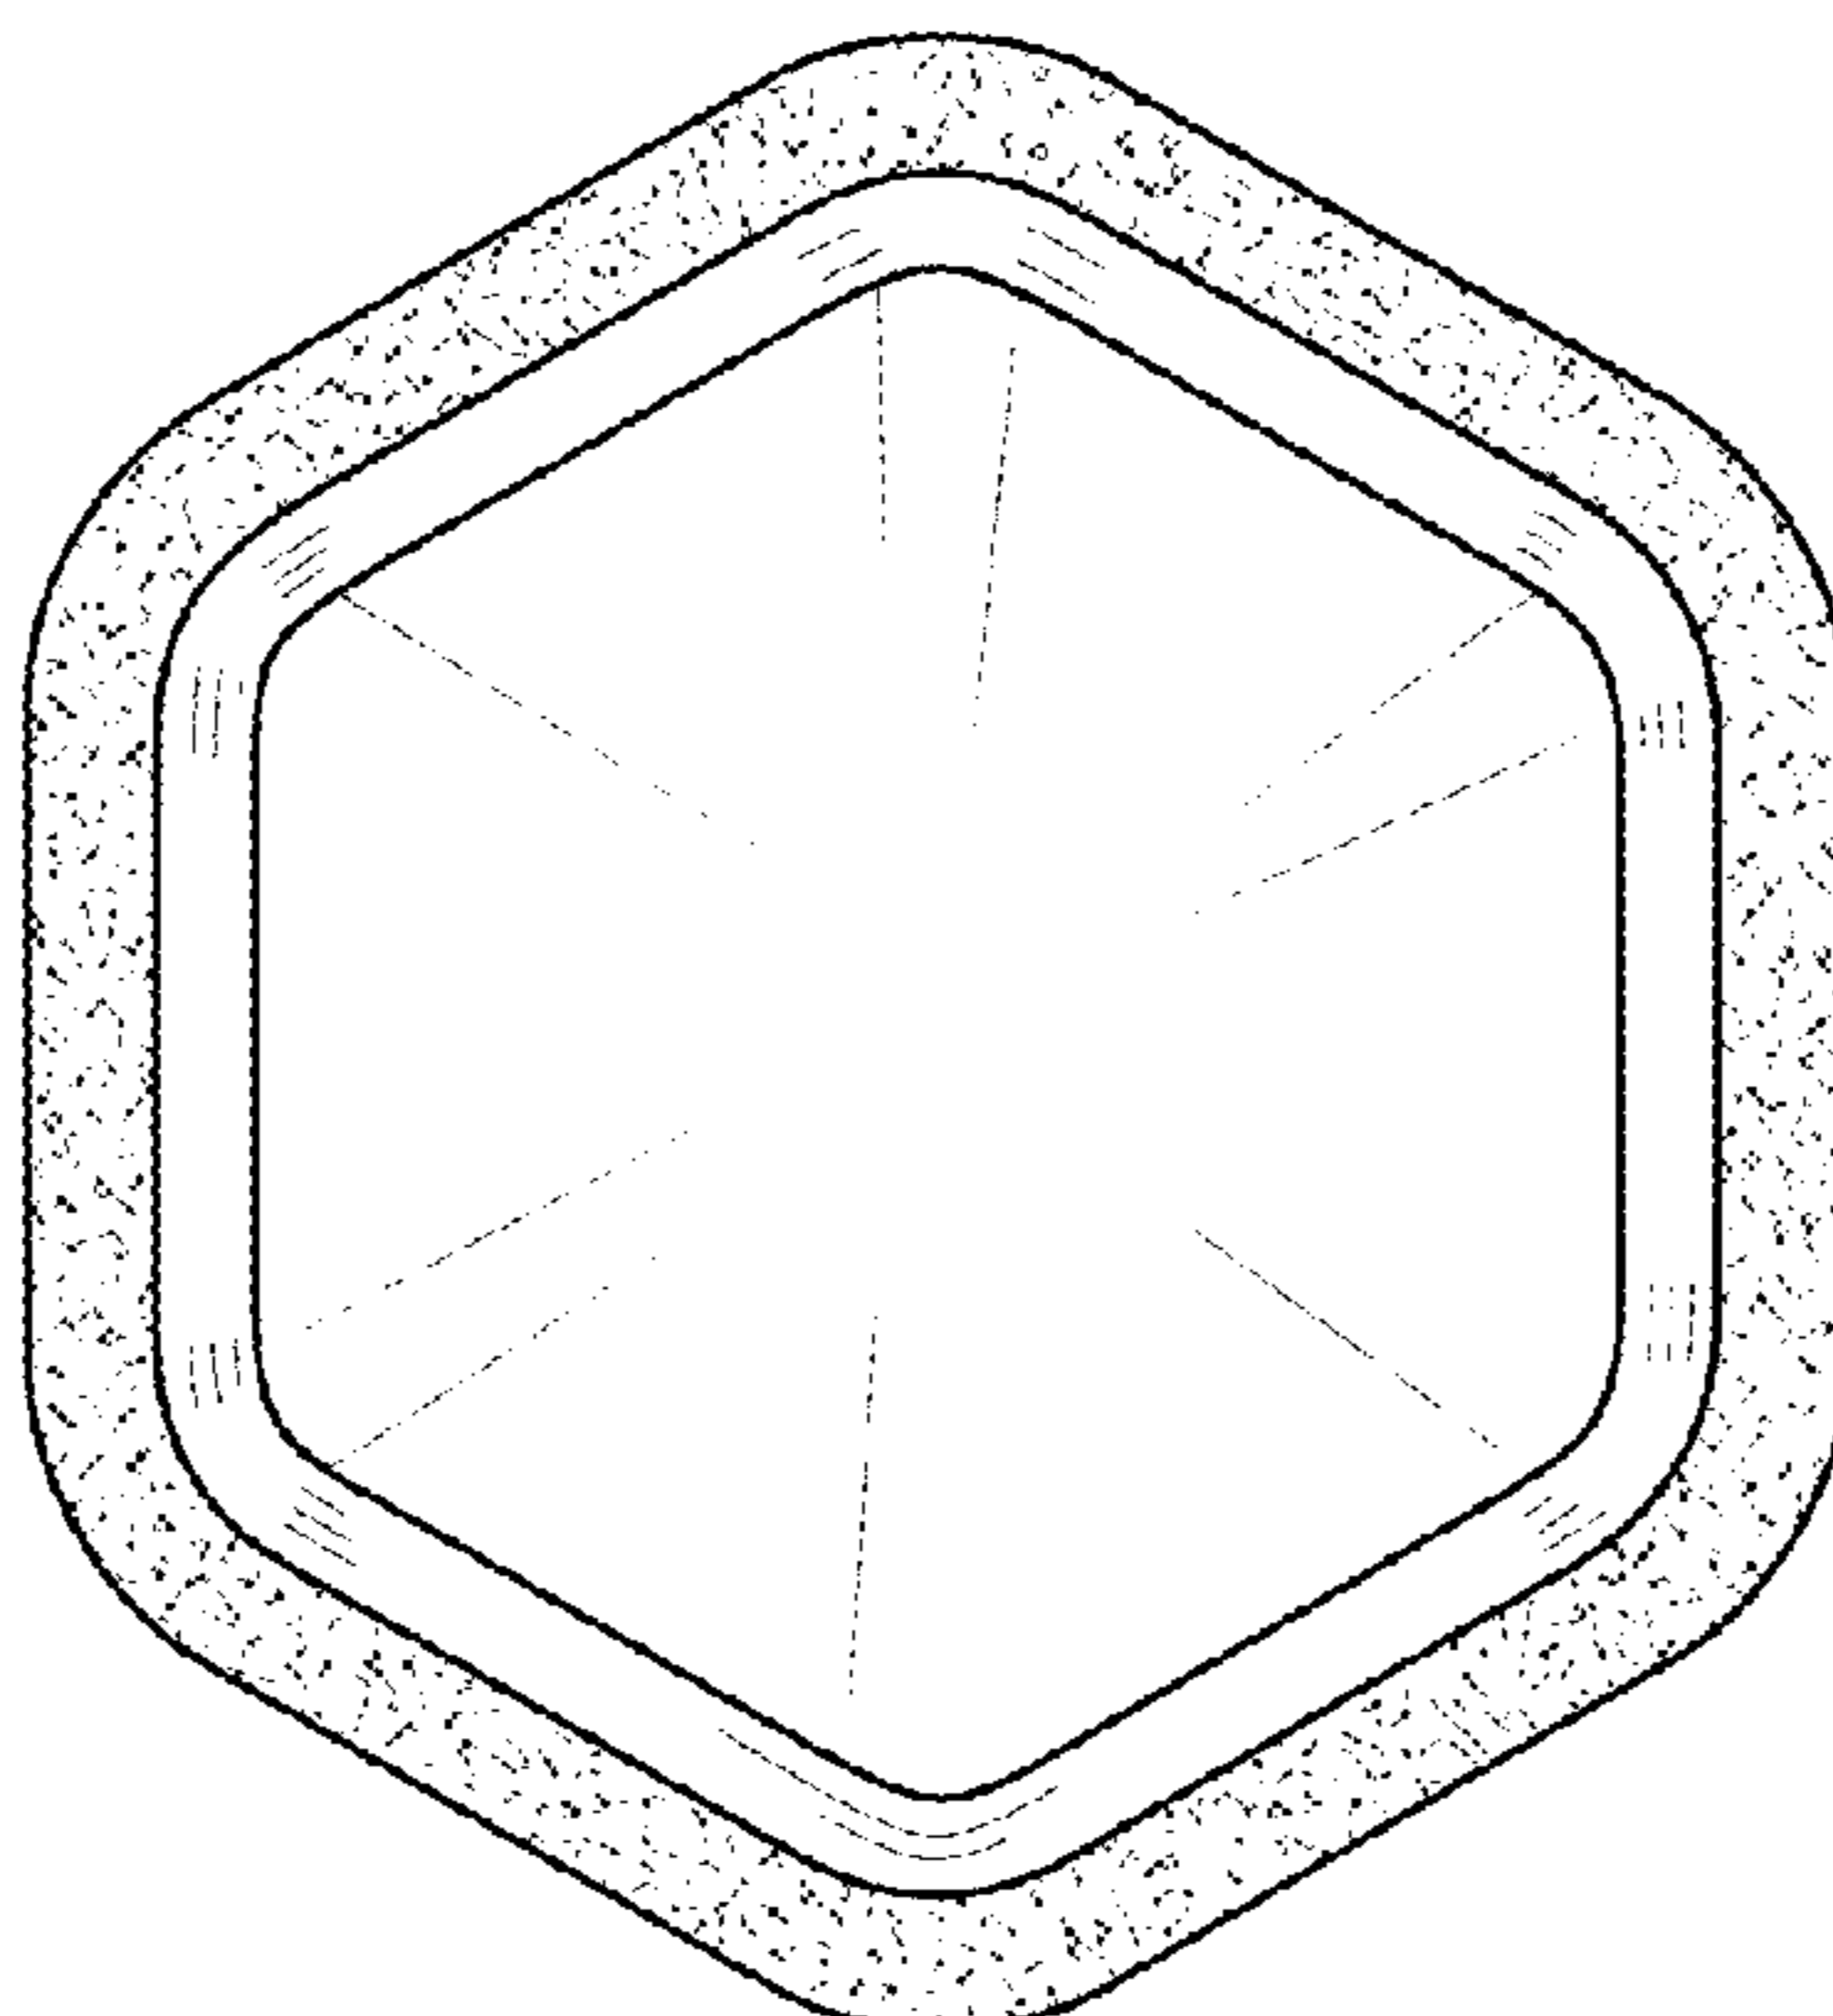

(56)

References Cited

U.S. PATENT DOCUMENTS

7,132,054 B1 11/2006 Kravitz et al.
 7,262,068 B2 8/2007 Roy et al.
 7,343,188 B2 3/2008 Sohrab
 7,344,499 B1 3/2008 Prausnitz et al.
 7,429,333 B2 9/2008 Chiou et al.
 7,456,112 B2 11/2008 Lee
 7,493,232 B1 2/2009 Surina
 8,022,292 B2 9/2011 Arianpour et al.
 8,088,321 B2 1/2012 Ferguson et al.
 8,574,165 B2 11/2013 Marsh
 8,798,799 B2 8/2014 Deo et al.
 8,909,543 B2* 12/2014 Tropper A61B 5/1118
 705/14.22
 D722,697 S * 2/2015 Moon D24/169
 D750,786 S * 3/2016 Davies D24/169
 D757,000 S * 5/2016 Lagomarsino D14/344
 9,551,698 B2 1/2017 Huys et al.
 D815,289 S * 4/2018 Evers D24/169
 D816,229 S * 4/2018 Frick D24/169

10,092,207 B1* 10/2018 Windmiller A61N 1/05
 D842,996 S * 3/2019 Frick D24/169
 2003/0225360 A1 12/2003 Eppstein et al.
 2006/0015061 A1 1/2006 Kuo et al.
 2007/0170054 A2 7/2007 Wilsey
 2007/0213044 A1 9/2007 Steingart et al.
 2009/0088652 A1 4/2009 Tremblay
 2009/0143761 A1 6/2009 Cantor et al.
 2009/0259118 A1 10/2009 Feldman et al.
 2010/0286803 A1 11/2010 Tillotson
 2012/0323097 A9 12/2012 Chowdhury
 2013/0065257 A1 3/2013 Wang et al.
 2013/0144131 A1 6/2013 Wang et al.
 2014/0259652 A1 9/2014 Pushpala et al.
 2014/0275897 A1 9/2014 Pushpala et al.
 2014/0336487 A1 11/2014 Wang et al.
 2015/0335272 A1* 11/2015 Natale A61B 5/0022
 600/365
 2017/0055851 A1* 3/2017 Al-Ali A61B 5/7264
 2018/0249937 A1* 9/2018 Wiese G16H 50/20
 2019/0095602 A1* 3/2019 Setlak G06K 9/2027

* cited by examiner

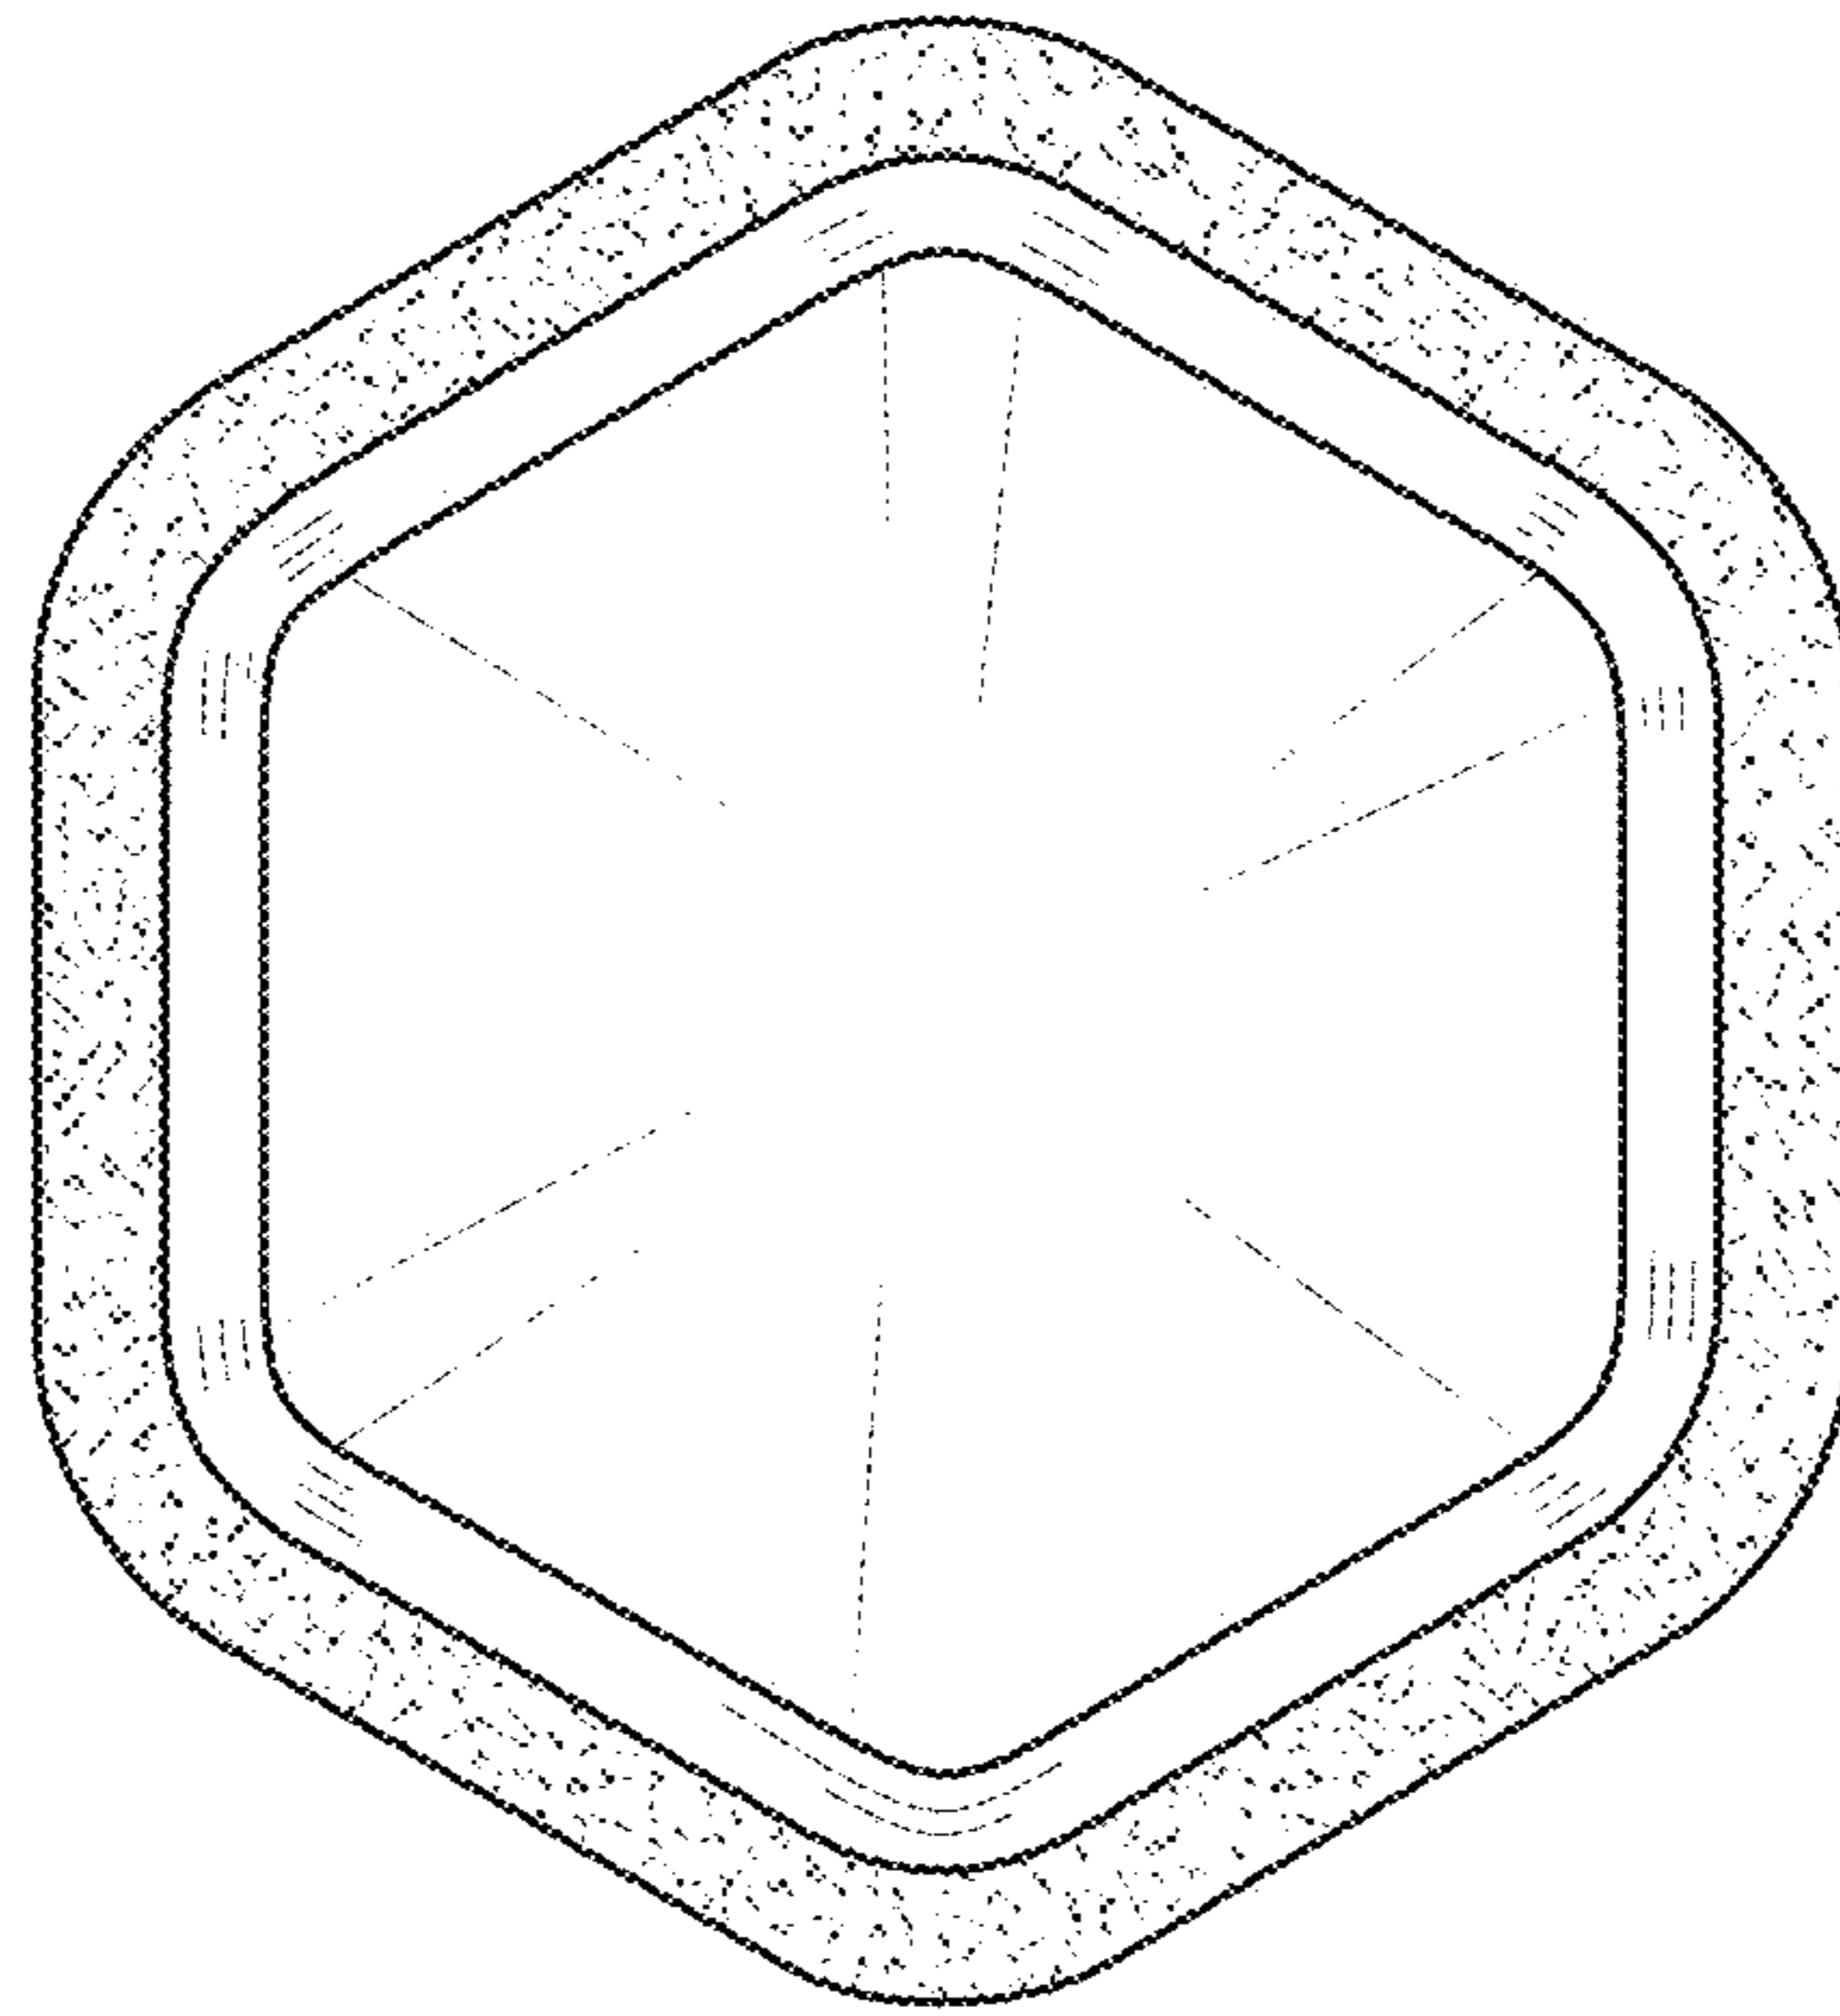


FIG. 1

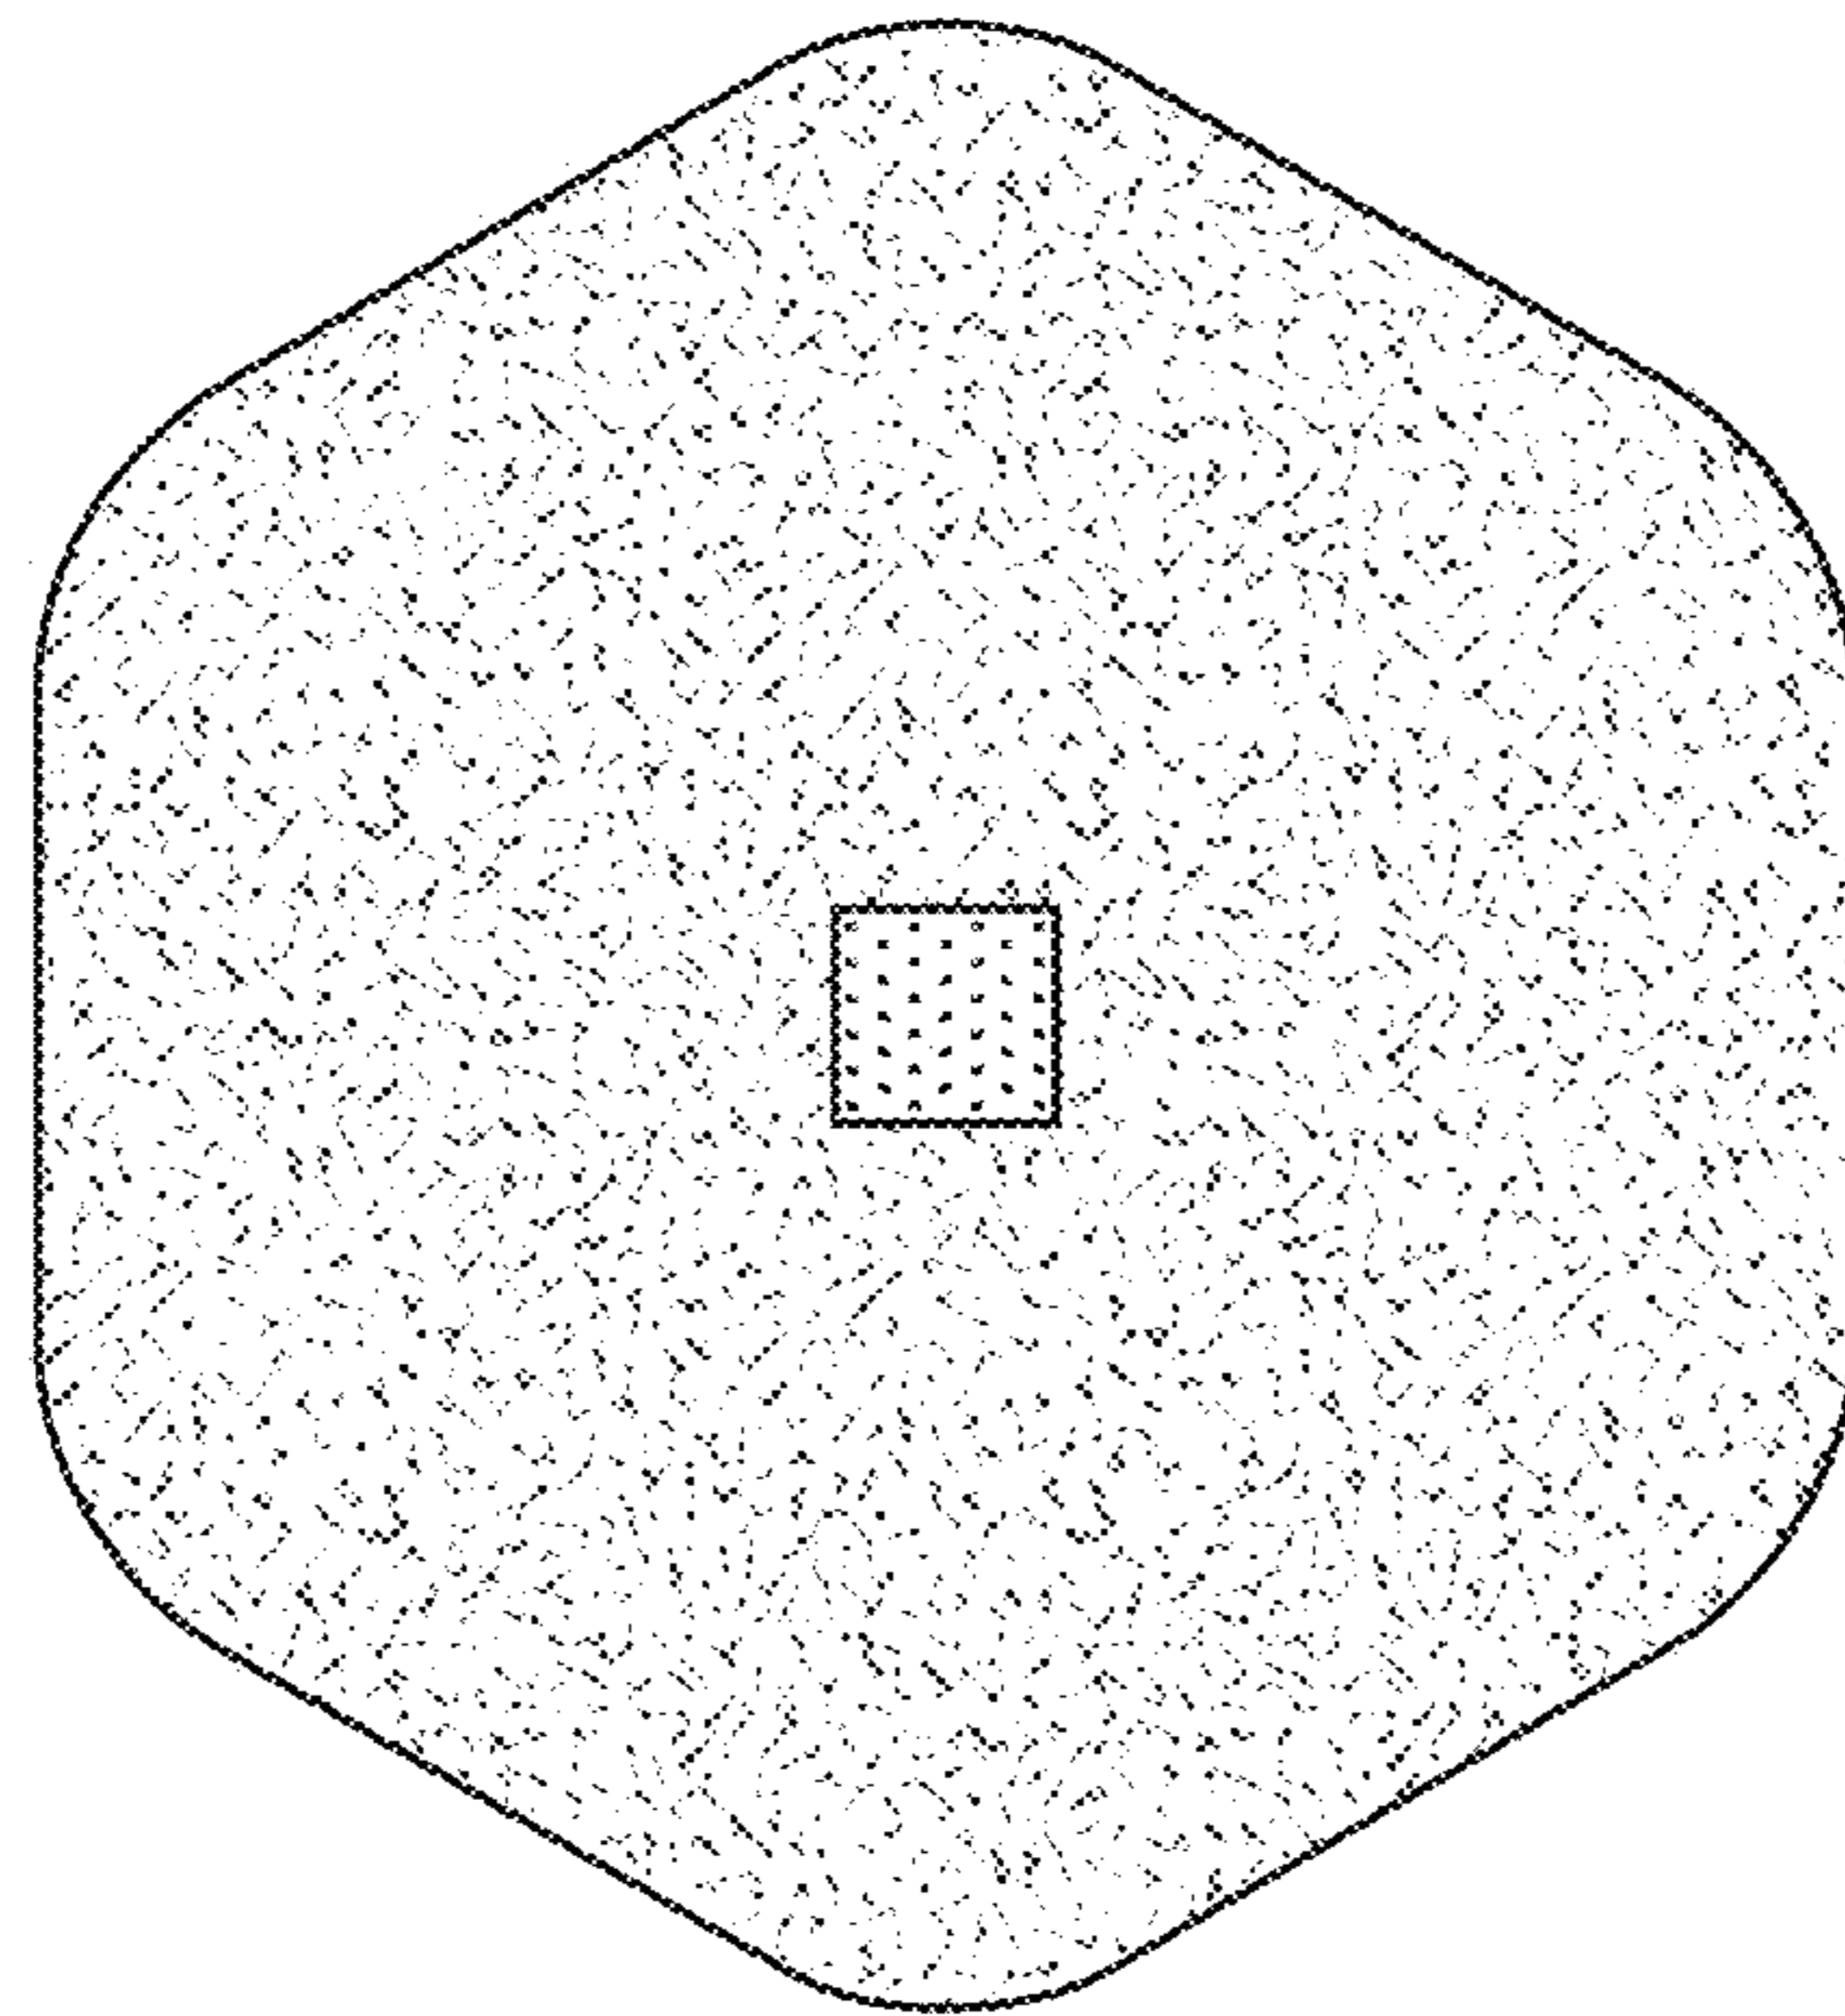


FIG. 2



FIG. 3



FIG. 4



FIG. 5



FIG. 6

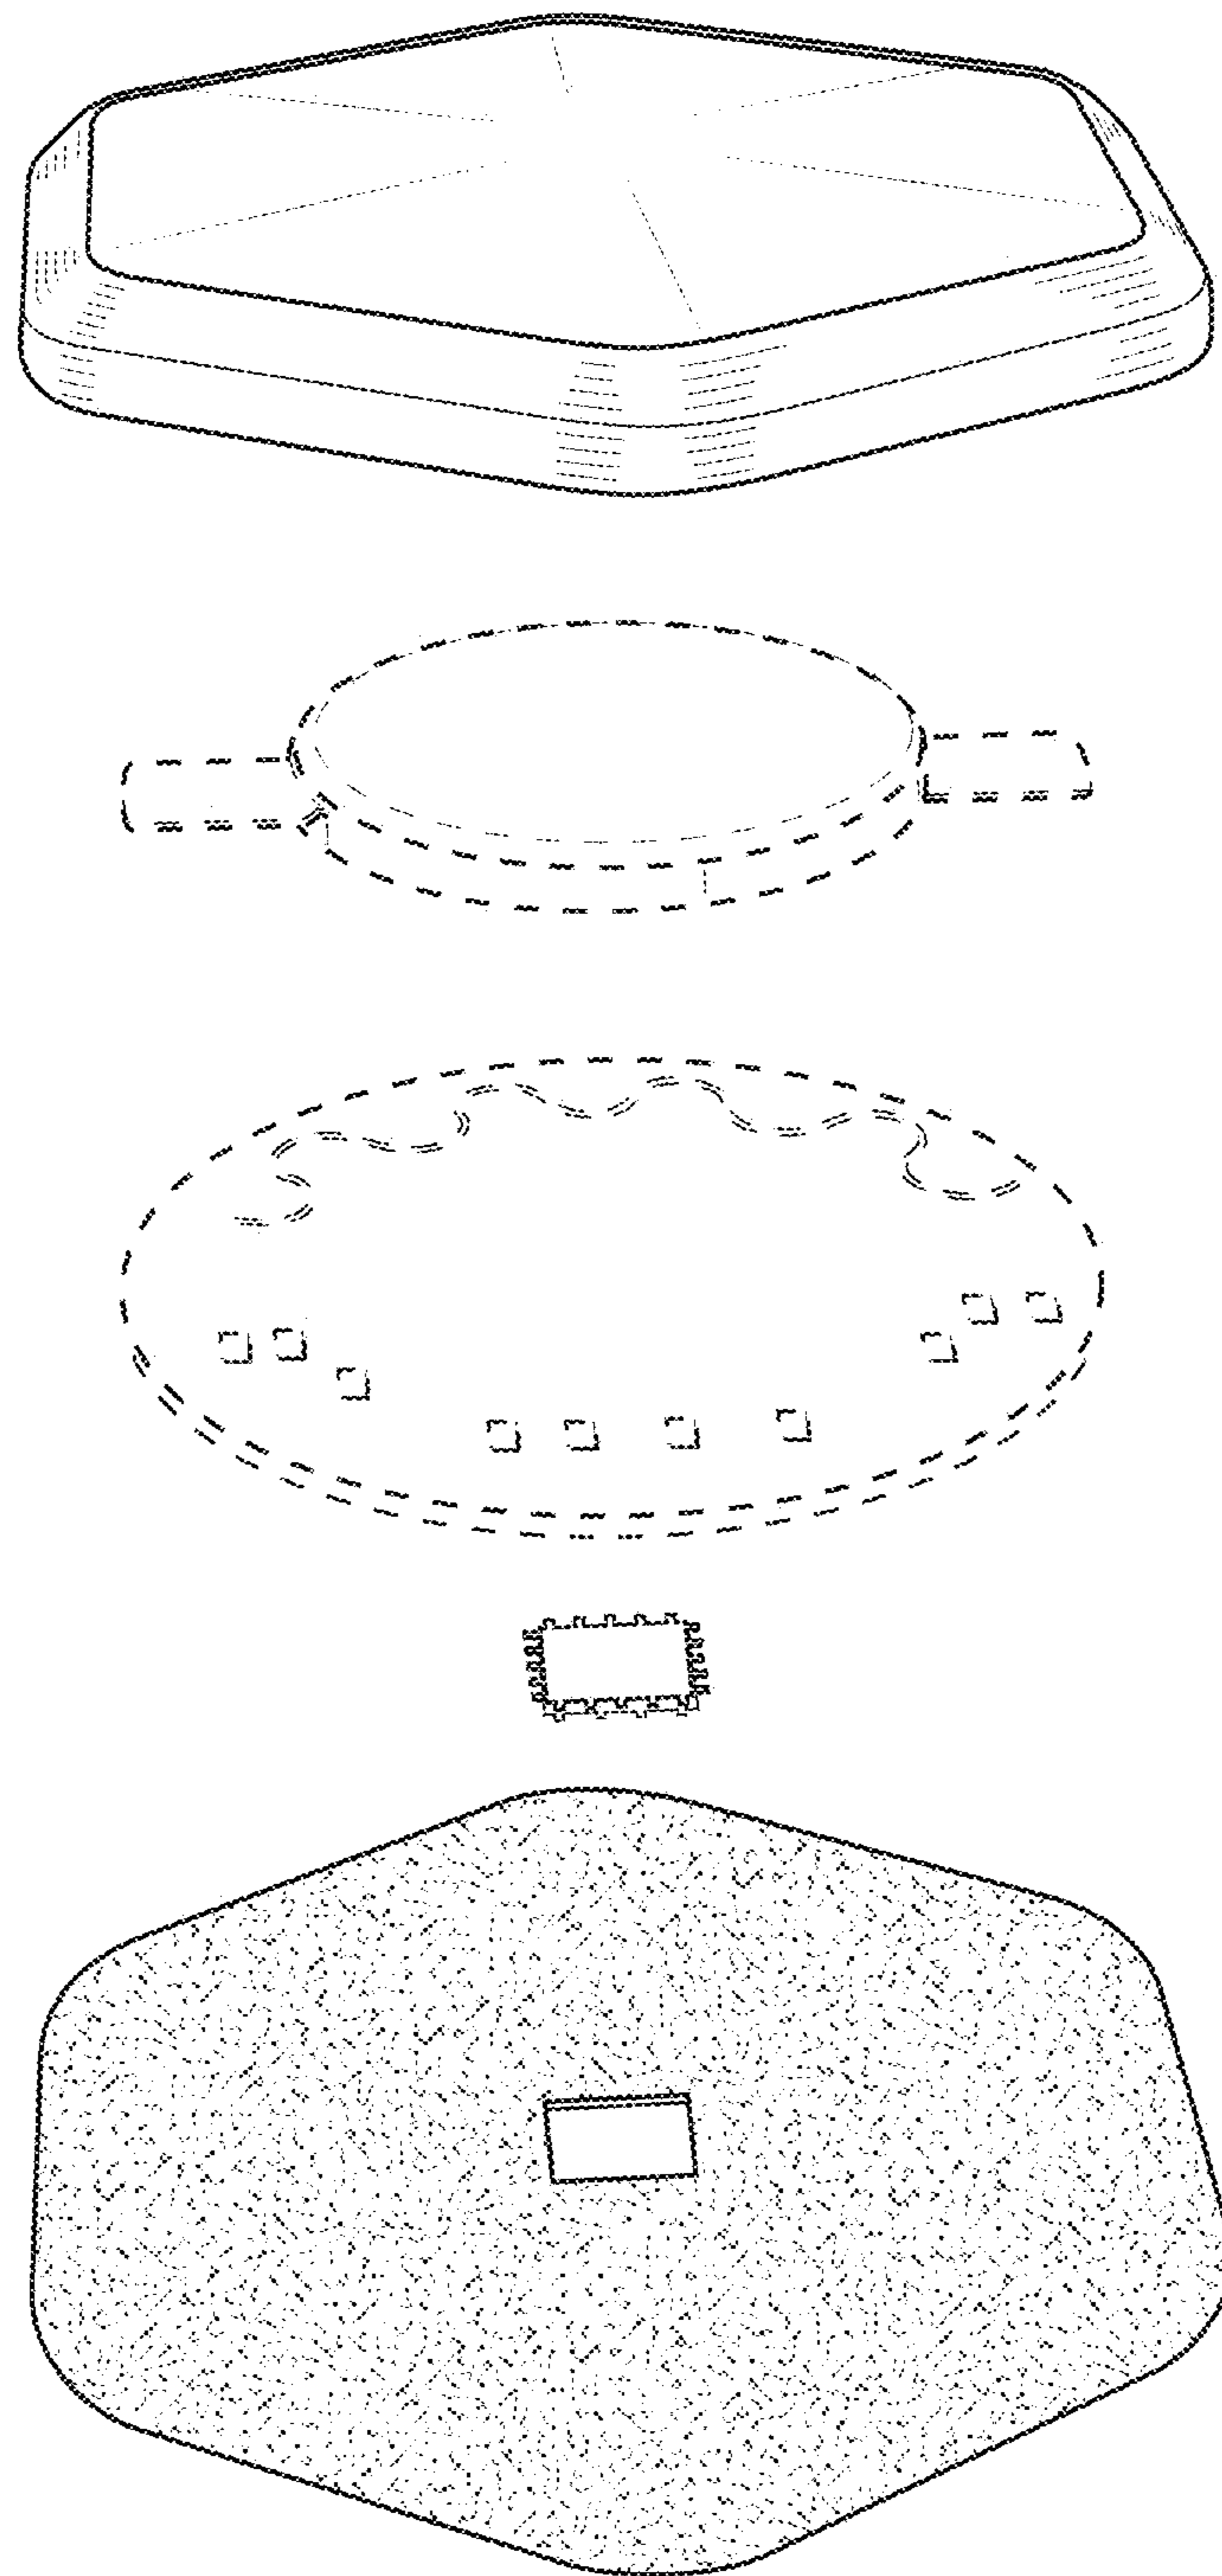


FIG. 7

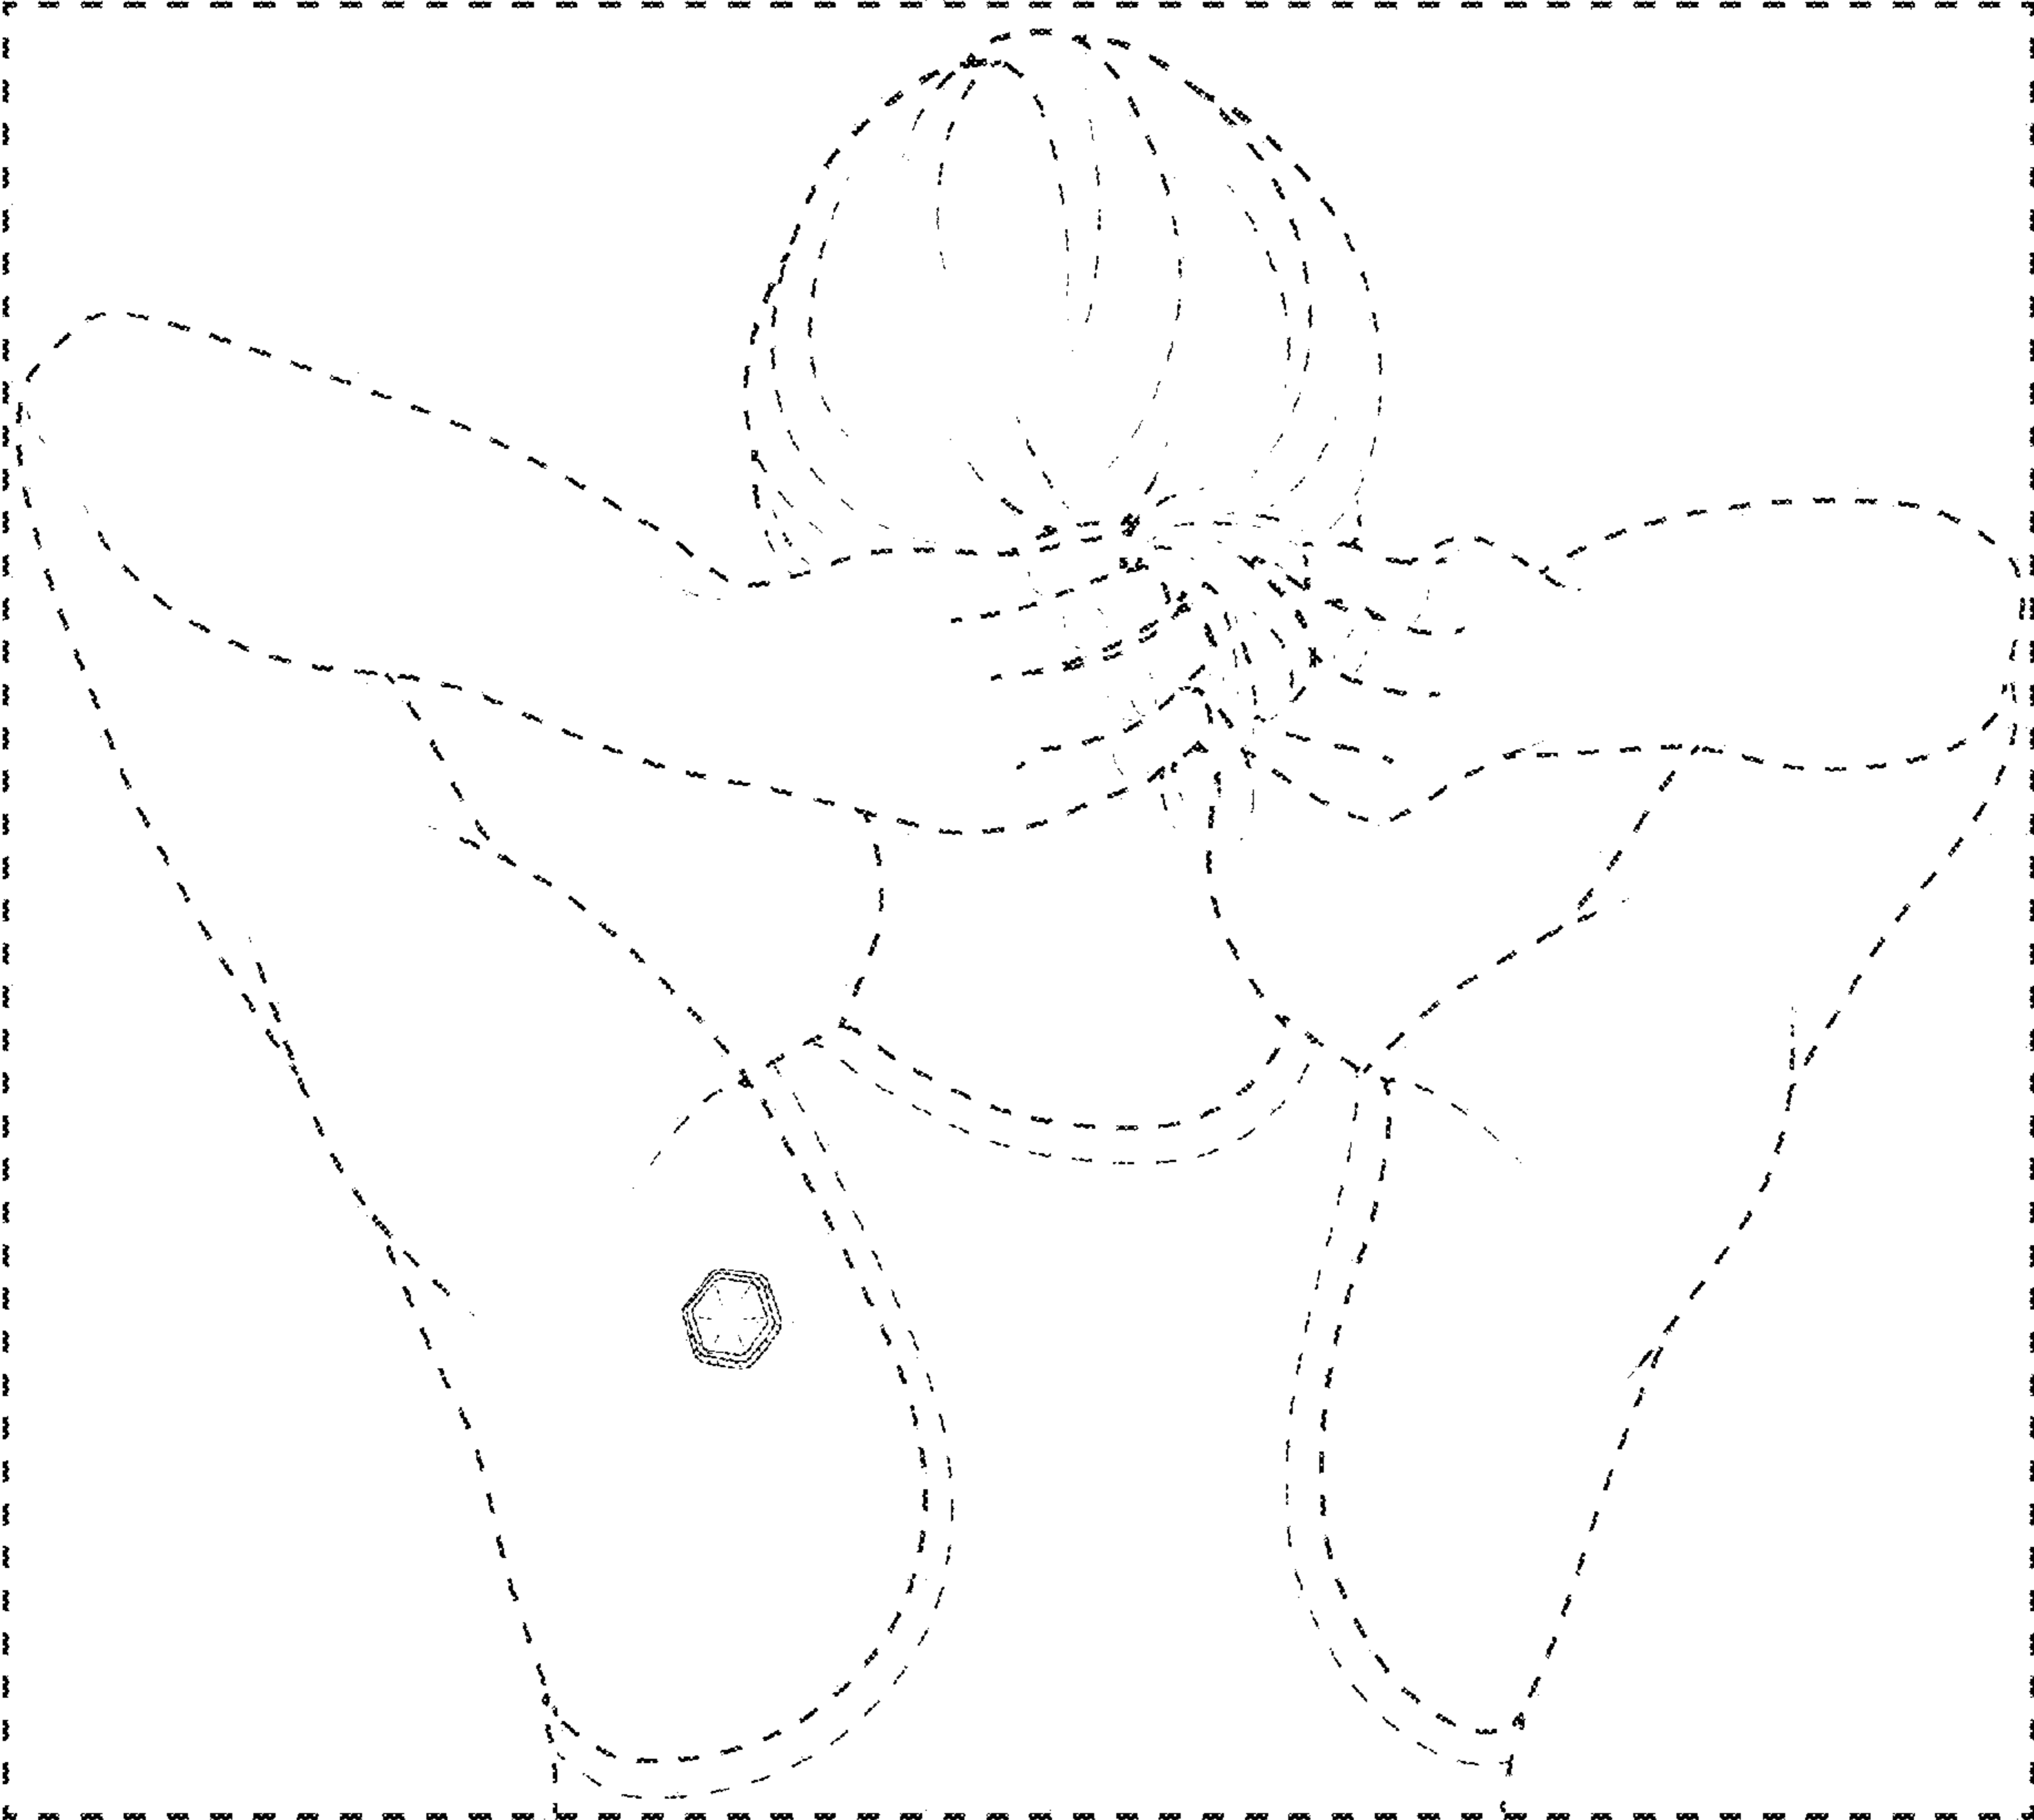


FIG. 8