



US00D875753S

(12) **United States Design Patent**
D'Costa et al.

(10) **Patent No.:** **US D875,753 S**

(45) **Date of Patent:** **** Feb. 18, 2020**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH GRAPHICAL USER INTERFACE FOR BIOLOGICAL SLIDE SCANNING**

(71) Applicant: **Ventana Medical Systems, Inc.,**
Tucson, AZ (US)

(72) Inventors: **Maya D'Costa, Basel (CH); Daniela Pretorius, Lisbon (PT); Pedro de Sousa Couto e Santos, Almada (PT)**

(73) Assignee: **Ventana Medical Systems, Inc.,**
Tucson, AZ (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/639,454**

(22) Filed: **Mar. 6, 2018**

(51) **LOC (12) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486; D14/488**

(58) **Field of Classification Search**
USPC D14/485, 486, 487, 488
CPC H04N 1/00196; H04N 1/00408; H04M 1/2477; G06F 2203/04807; G06F 3/0482; A63F 2300/308; A63F 13/53; A63F 200/66; A63F 2300/8082
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D656,946 S *	4/2012	Judy	D14/486
D698,796 S *	2/2014	Evans	D14/485
D703,688 S *	4/2014	Choi	D14/486
D757,763 S *	5/2016	Lim	G06F 17/3056
				D14/486
D770,493 S *	11/2016	Blank	D14/486
9,613,469 B2 *	4/2017	Fish	G06F 3/04886
D786,910 S *	5/2017	Higuchi	D14/486
D813,248 S *	3/2018	Burton	D14/485
D817,999 S *	5/2018	Ambielli	D14/488

D824,414 S *	7/2018	Peeters	D14/487
D832,302 S *	10/2018	Chu	D14/488
D844,019 S *	3/2019	Keys	D14/486
D847,856 S *	5/2019	Kim	D14/488
D849,765 S *	5/2019	Lee	D14/486
D854,030 S *	7/2019	Dascola	D14/485
D856,362 S *	8/2019	Ibanez Ballesteros	D14/486

(Continued)

OTHER PUBLICATIONS

Huron Digital Pathology. "The Seven Pitfalls of Whole Slide Scanning." News: Medical Life Sciences, posted Jan. 4, 2017 (Retrieved from the Internet Jun. 6, 2019). Internet URL: < https://www.news-medical.net/whitepaper/20170104/The-Seven-Pitfalls-of-Whole-Slide-Scanning.aspx > (Year: 2017) 2017.*

Primary Examiner — Jack Reickel

Assistant Examiner — Rachel A Voorhies

(74) *Attorney, Agent, or Firm* — Kilpatrick Townsend & Stockton LLP


(57) **CLAIM**

The ornamental design for a display screen or portion thereof with graphical user interface for biological slide scanning, as shown and described.

DESCRIPTION

FIG. 1 is a front view of a first embodiment of a display screen or portion thereof with graphical user interface for biological slide scanning showing our new design; and, FIG. 2 is a front view of a second embodiment thereof. The dashed broken line rectangle illustrates a boundary of a display screen or a portion thereof and forms no part of the claimed design. Various texts presented in broken lines form no part of the claimed design. Any trademarks are the property of their respective owners and do not form part of the claimed design. Gradients or degrees of contrast or saturation that impart a tone do not form part of the claimed design.

1 Claim, 2 Drawing Sheets

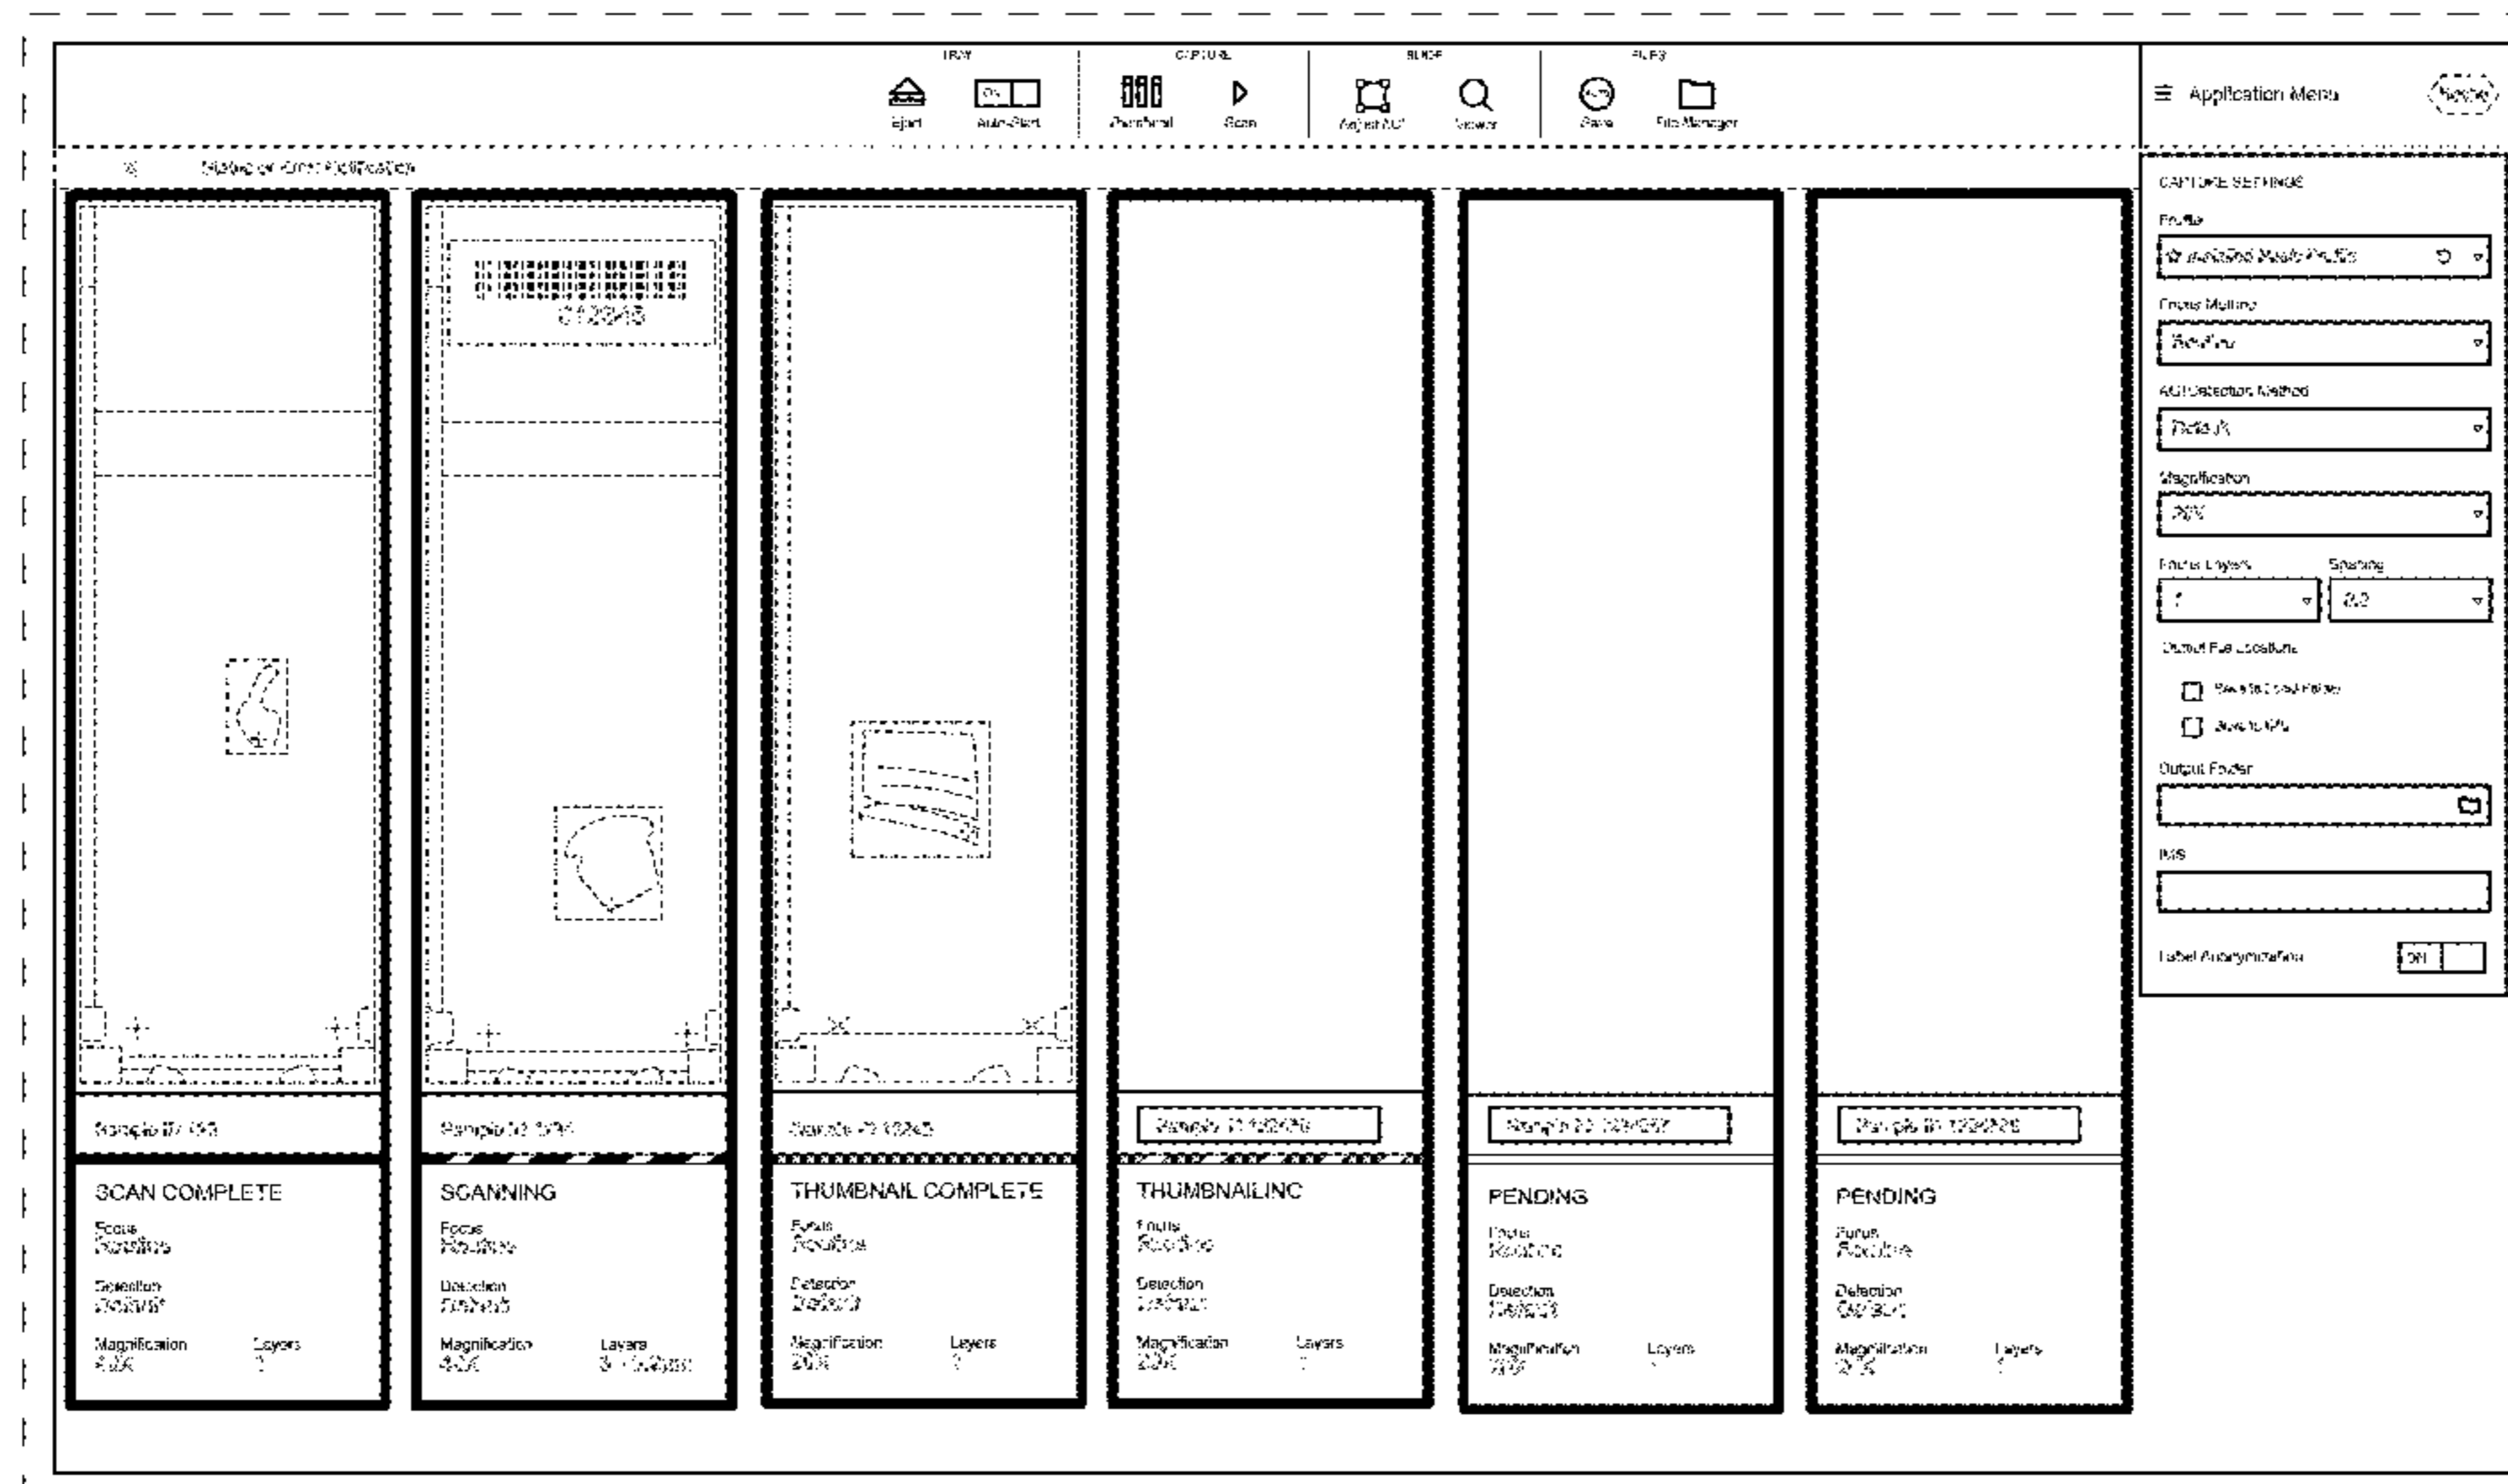

(56)

References Cited

U.S. PATENT DOCUMENTS

2004/0008224 A1* 1/2004 Molander G06F 3/0481
715/764
2015/0177952 A1* 6/2015 Meyer G06F 3/04842
715/739
2016/0019695 A1* 1/2016 Chukka G06T 7/0014
382/128
2016/0110367 A1* 4/2016 Krishnan G06F 17/3056
705/30
2016/0119192 A1* 4/2016 Tanoue H04L 41/22
715/735
2016/0321809 A1* 11/2016 Chukka G06K 9/0014
2017/0185744 A1* 6/2017 Okabe G06F 19/00
2018/0012355 A1* 1/2018 Sarkar G06K 9/00127
2018/0148788 A1* 5/2018 Bracken C12Q 1/6886

* cited by examiner

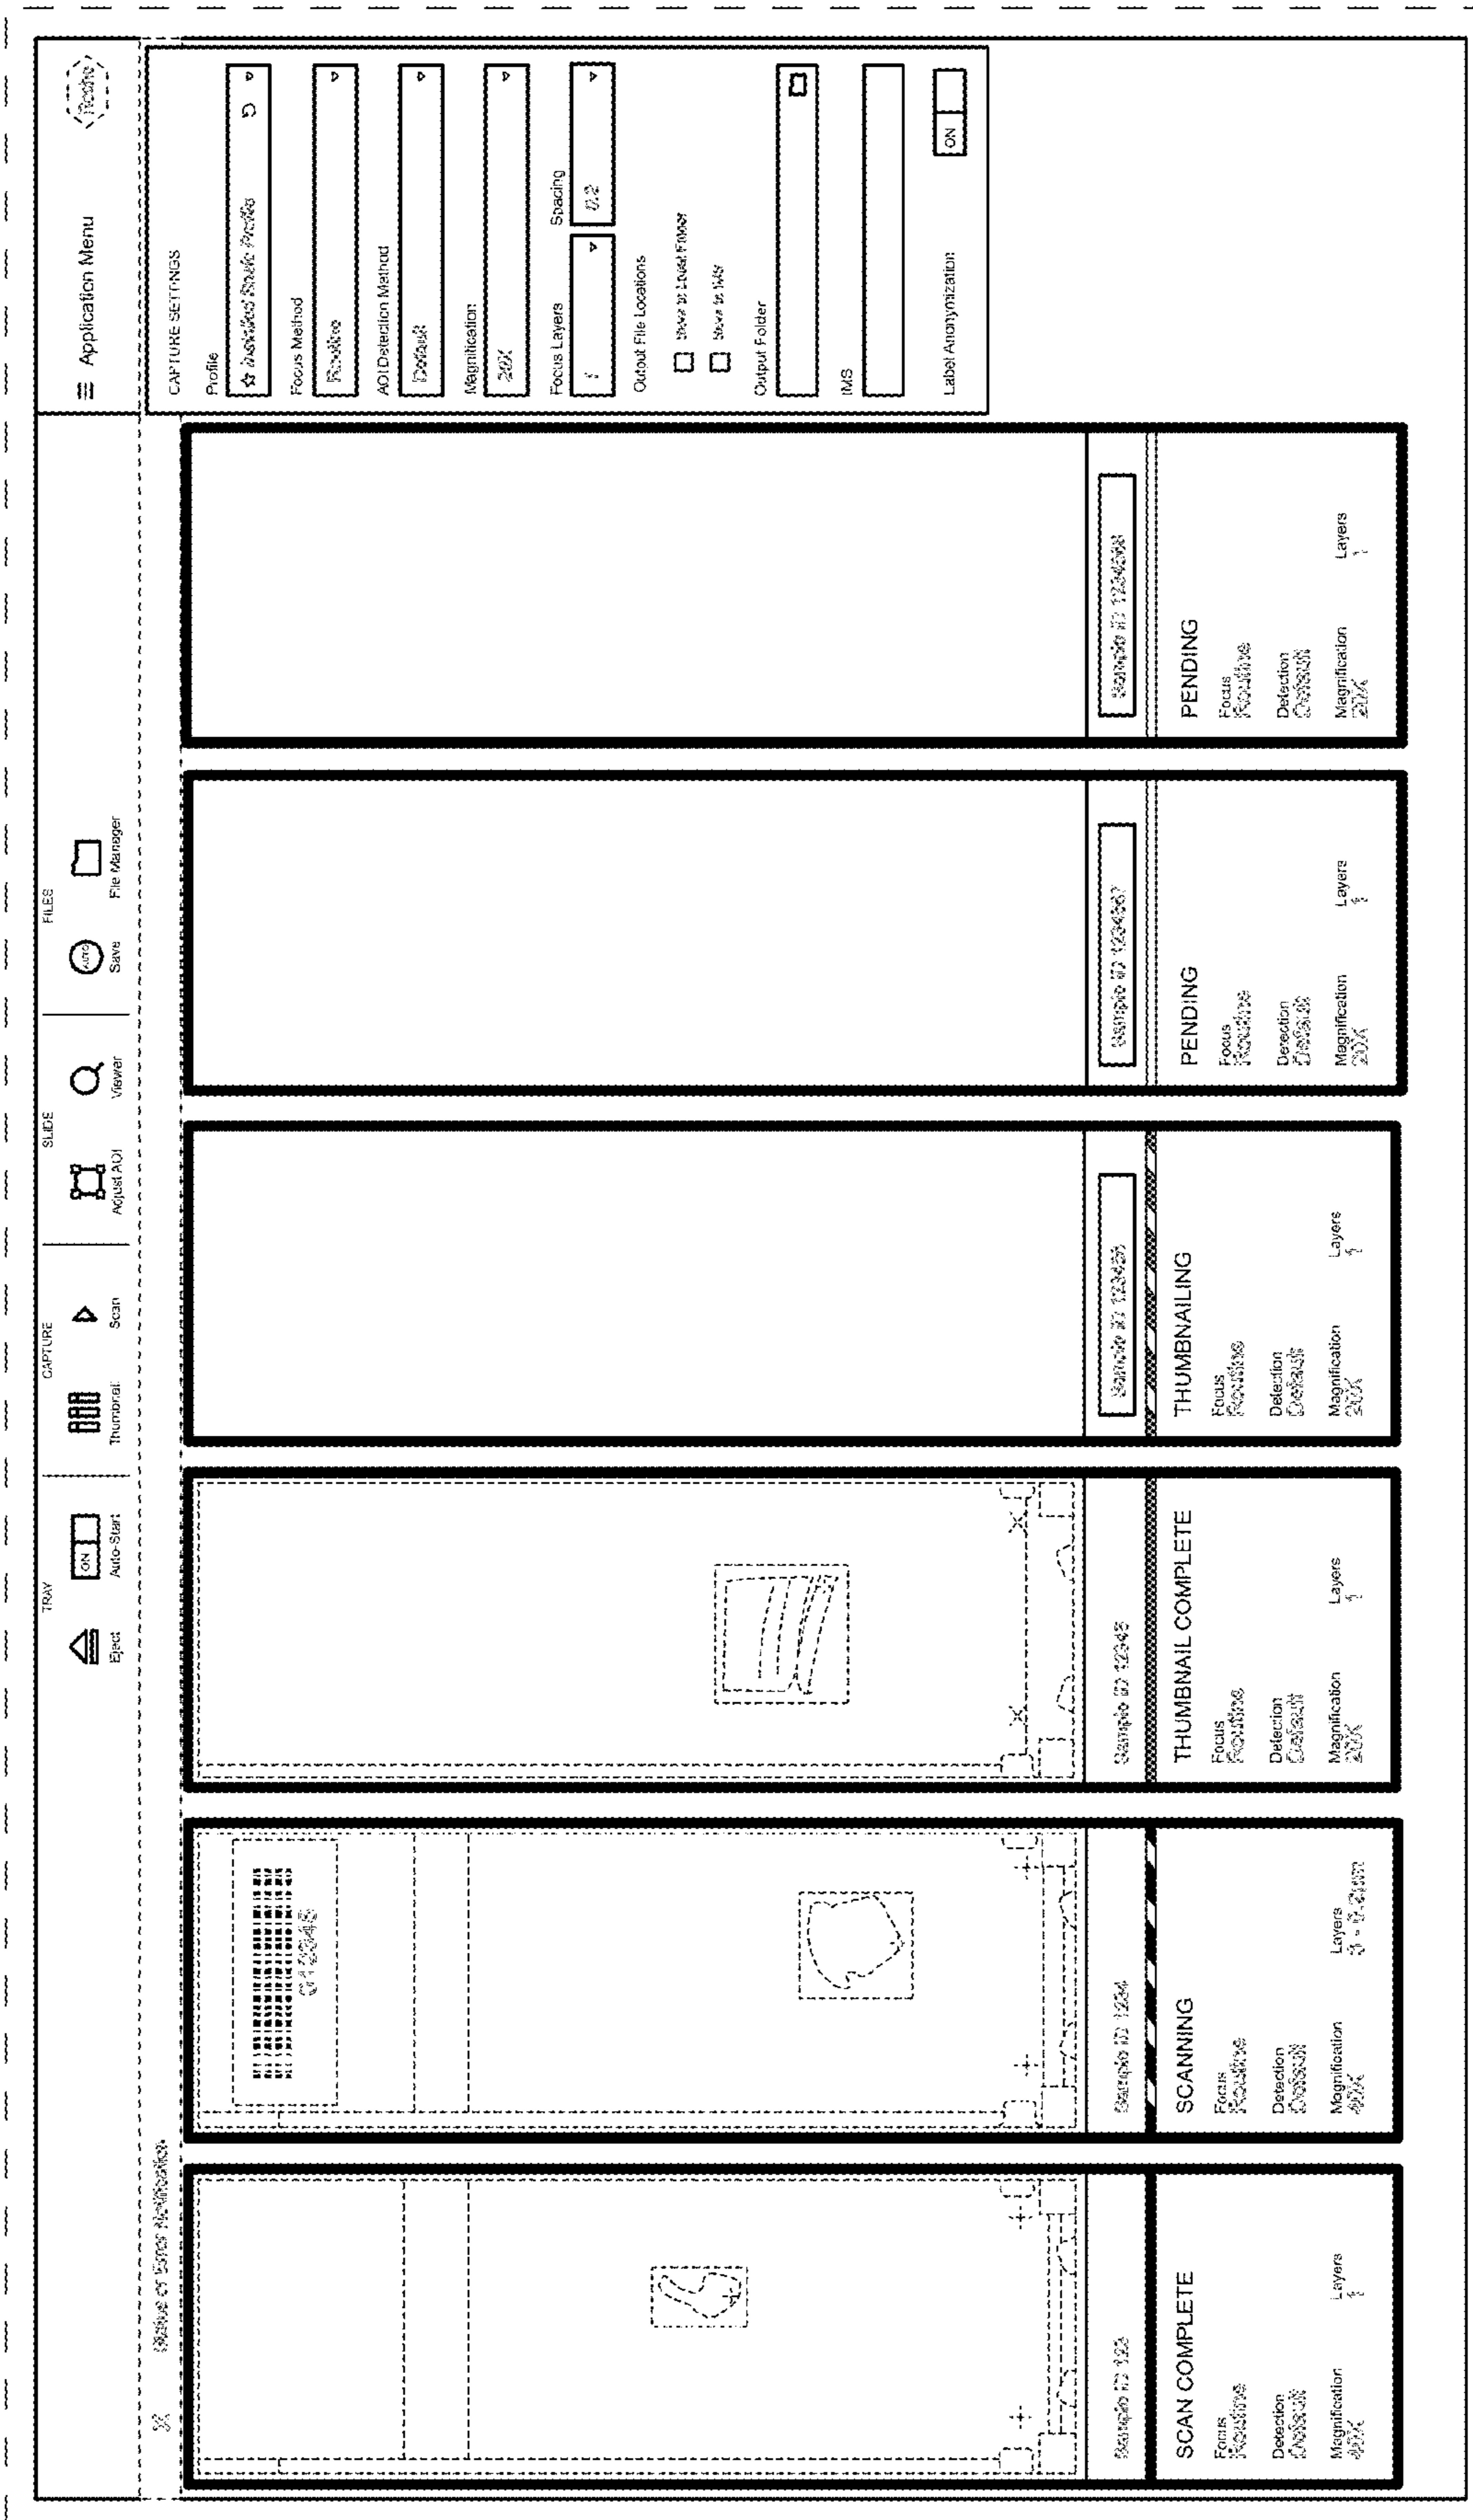


FIG. 1

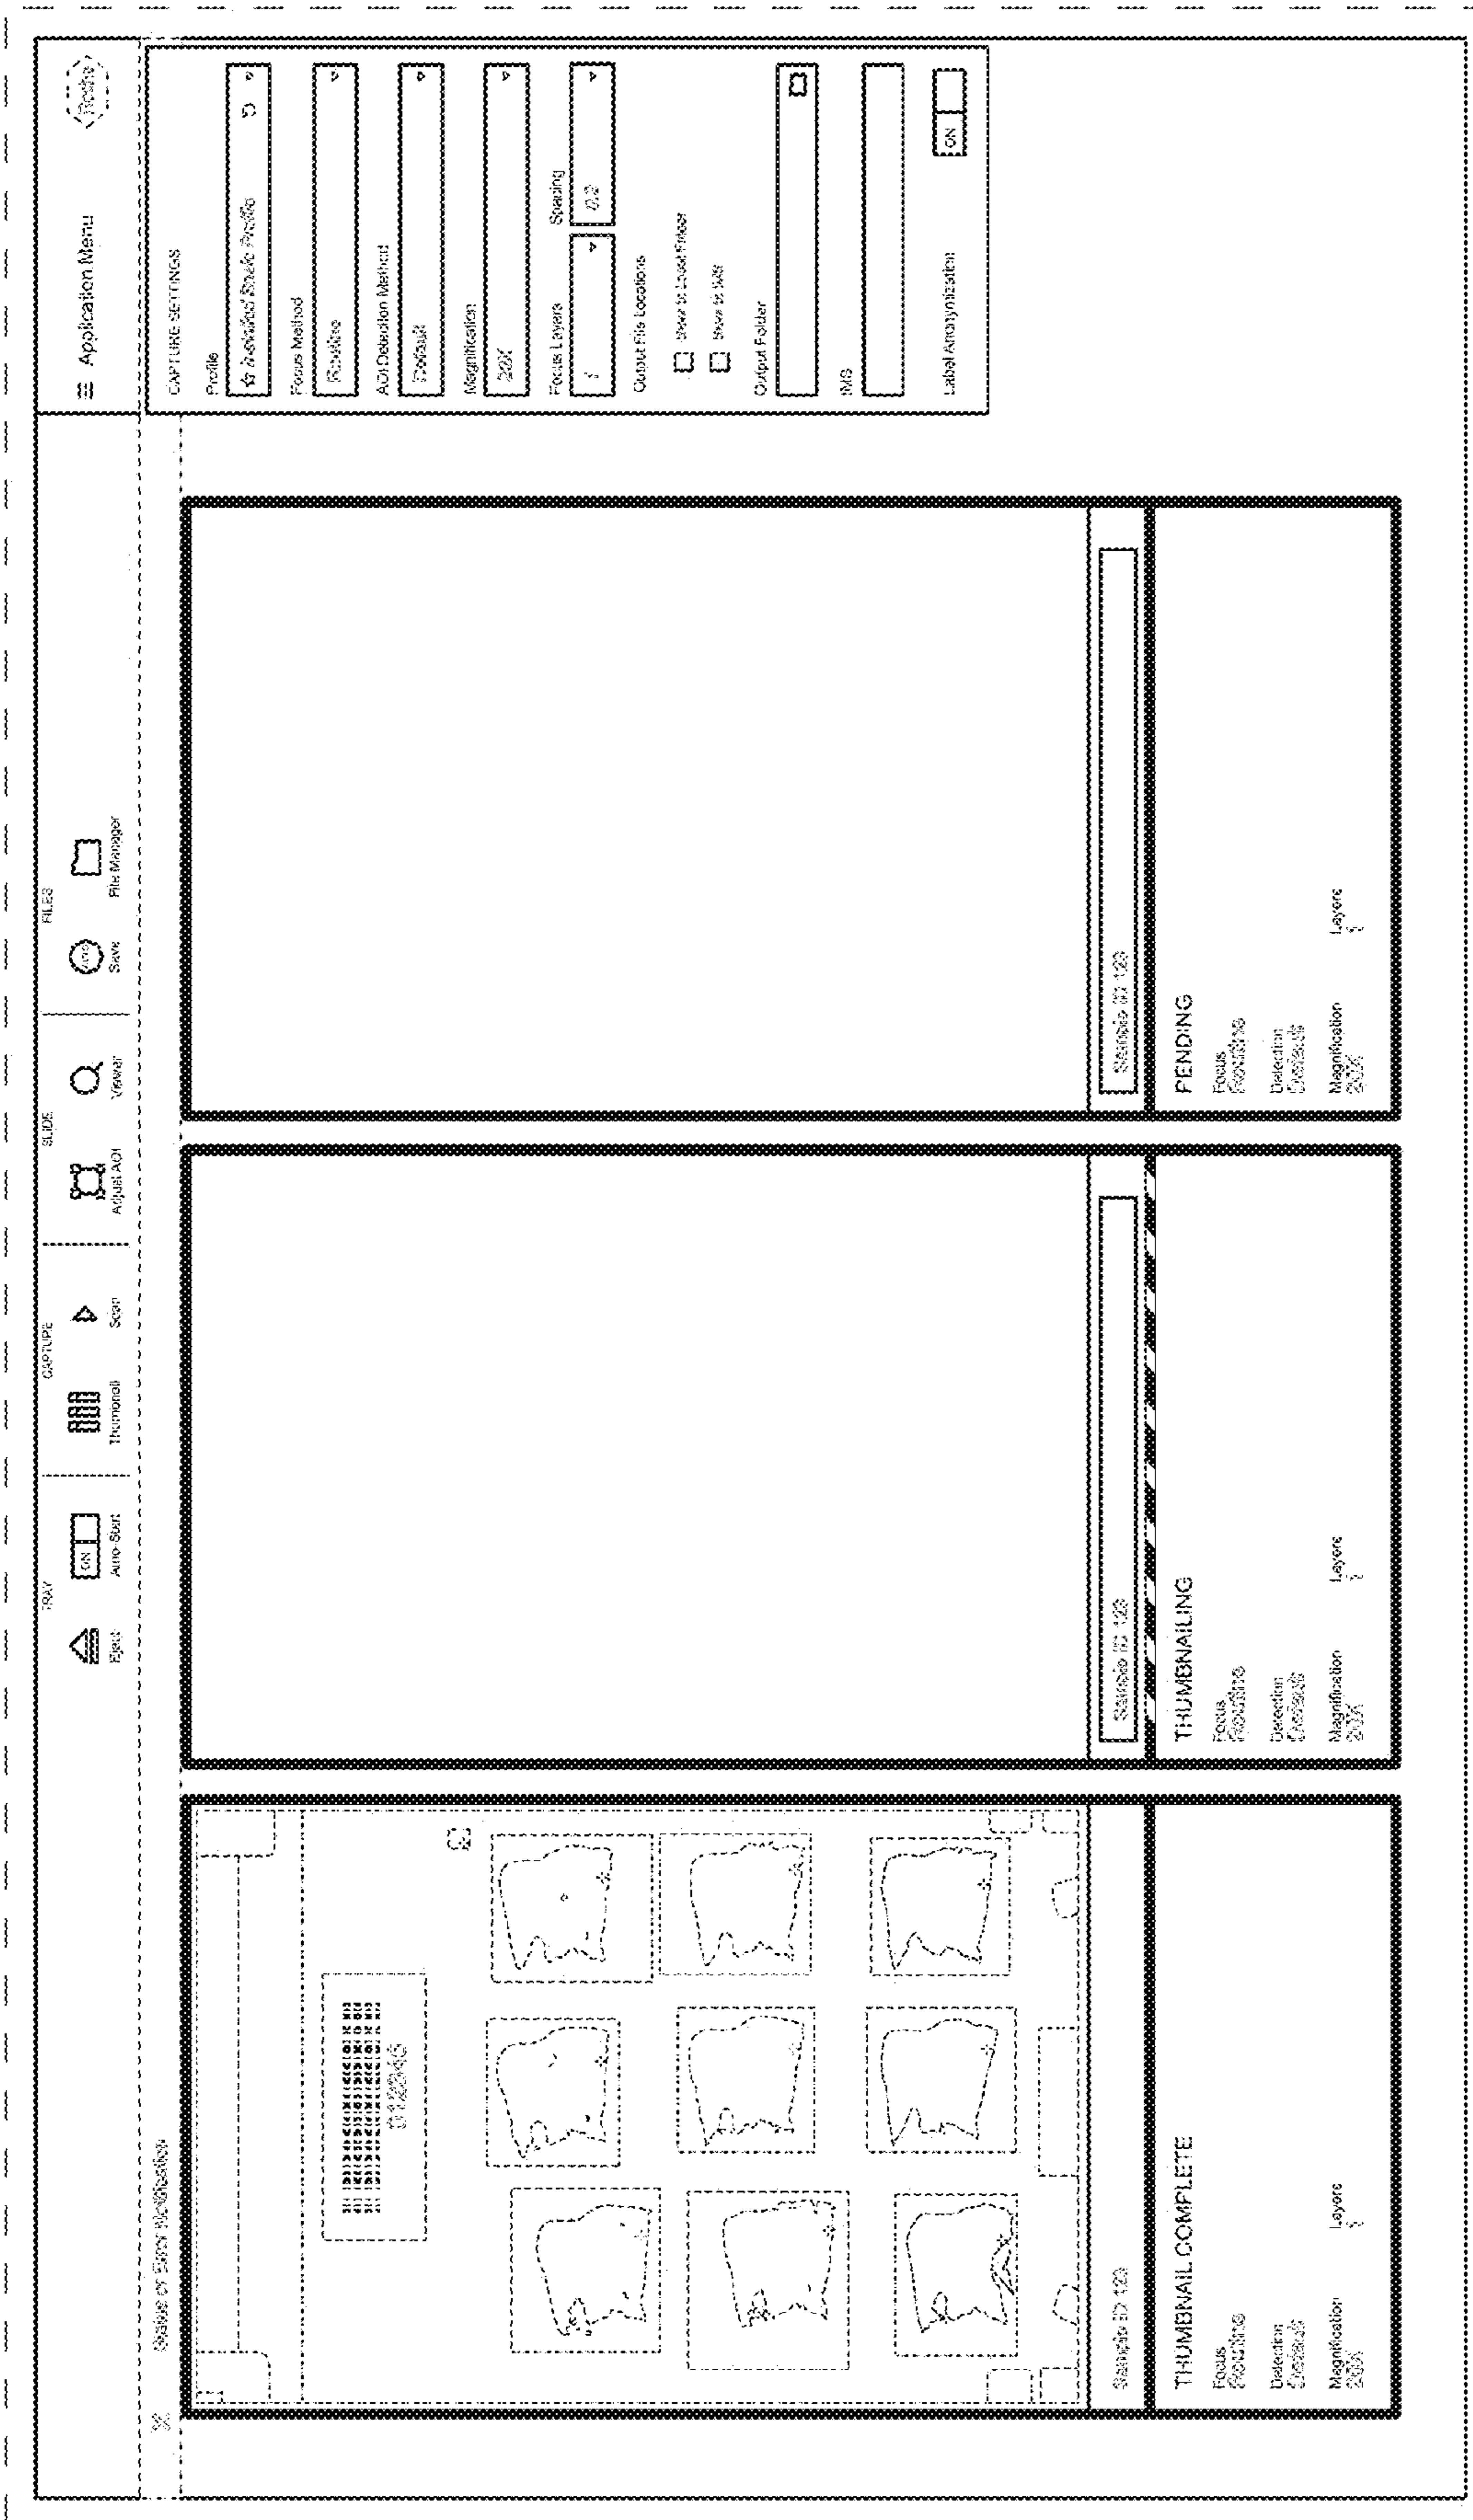


FIG. 2