



US00D876259S

(12) **United States Design Patent**  
**Barton et al.**

(10) **Patent No.:** **US D876,259 S**  
(45) **Date of Patent:** **\*\* Feb. 25, 2020**

(54) **DIAGNOSTIC ANALYZER**

- (71) Applicant: **Abbott Laboratories**, Abbott Park, IL (US)
- (72) Inventors: **Christina A. Barton**, Irving, TX (US); **Vladlena Belozero**, Philadelphia, PA (US); **Ami Marie Verhalen**, Sun Prairie, WI (US); **Jesse Charles Darley**, Madison, WI (US); **Sherry Sue Eckholm**, Sun Prairie, WI (US)
- (73) Assignee: **Abbott Laboratories**, Abbott Park, IL (US)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/692,206**
- (22) Filed: **May 23, 2019**

**Related U.S. Application Data**

- (63) Continuation of application No. 29/633,292, filed on Jan. 12, 2018, now Pat. No. Des. 850,955, which is a (Continued)
- (51) **LOC (12) Cl.** ..... **10-04**
- (52) **U.S. Cl.**  
USPC ..... **D10/81; D24/216**
- (58) **Field of Classification Search**  
USPC ..... **D10/81; D24/216, 219, 220, 232, 233, D24/234**

(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- D662,431 S 6/2012 Kimura
  - D724,753 S 3/2015 Gutmann et al.
- (Continued)

**OTHER PUBLICATIONS**

Japanese Patent Office, "Notice of Reason for Rejection," issued in connection with Japanese Design Application No. 2016-19293, dated Nov. 8, 2016, 3 pages.

(Continued)

*Primary Examiner* — Antoine Duval Davis  
(74) *Attorney, Agent, or Firm* — Hanley, Flight & Zimmerman, LLC


(57) **CLAIM**

The ornamental design for "diagnostic analyzer", as shown and described.

**DESCRIPTION**

FIG. 1 is a front left perspective view of diagnostic analyzer. FIG. 2 is a front view of the diagnostic analyzer of FIG. 1. FIG. 3 is a rear view of the diagnostic analyzer of FIG. 1. FIG. 4 is a right side view of the diagnostic analyzer of FIG. 1. FIG. 5 is a left side view of the diagnostic analyzer of FIG. 1. FIG. 6 is a top view of the diagnostic analyzer of FIG. 1. FIG. 7 is a bottom view of the diagnostic analyzer of FIG. 1. FIG. 8 is a front left perspective view of diagnostic analyzer. FIG. 9 is a front view of the diagnostic analyzer of FIG. 8. FIG. 10 is a rear view of the diagnostic analyzer of FIG. 8. FIG. 11 is a right side view of the diagnostic analyzer of FIG. 8. FIG. 12 is a left side view of the diagnostic analyzer of FIG. 8. FIG. 13 is a top view of the diagnostic analyzer of FIG. 8; and, FIG. 14 is a bottom view of the diagnostic analyzer of FIG. 8. The features shown in broken lines form no part of the claimed design.

**1 Claim, 12 Drawing Sheets**

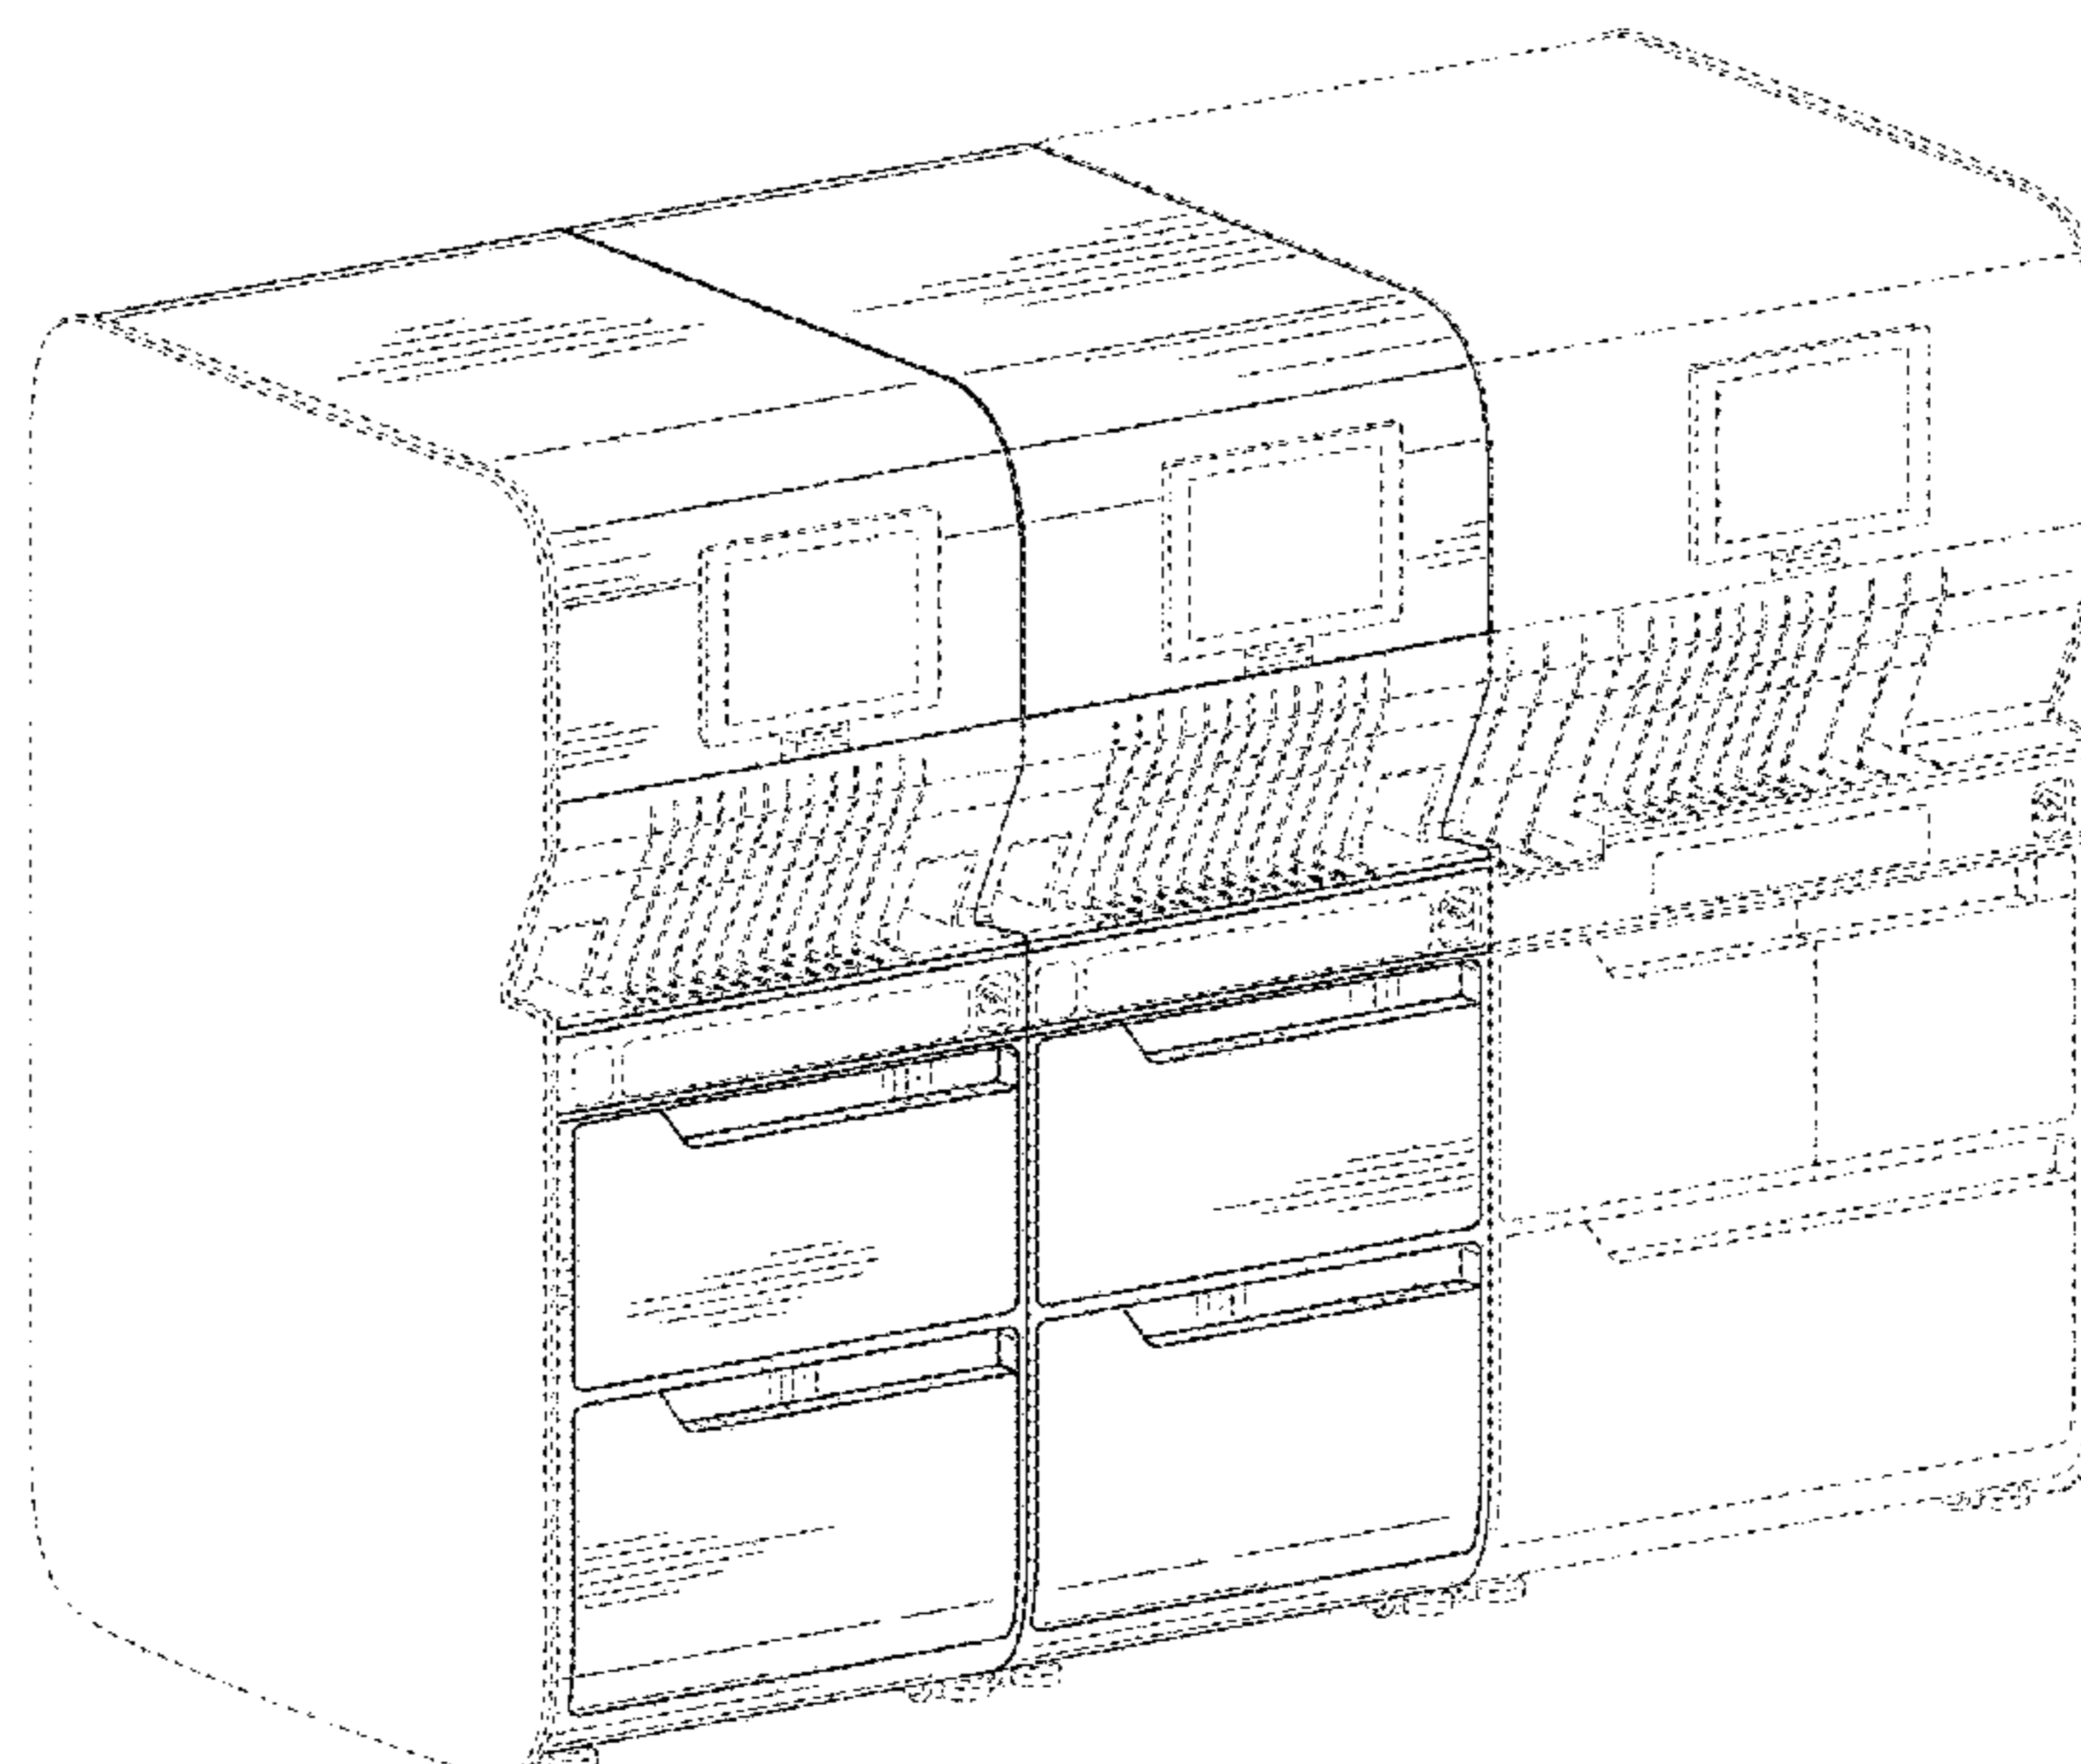

**Related U.S. Application Data**

continuation of application No. 29/587,978, filed on Dec. 16, 2016, now Pat. No. Des. 811,913, which is a continuation of application No. 29/531,578, filed on Jun. 26, 2015, now Pat. No. Des. 777,049.

(58) **Field of Classification Search**

CPC .. G01N 21/00; G01N 21/01; G01N 2201/022; G01N 2201/0221; G01N 2201/0222; G01N 2201/0224; G01N 2201/0225; G01N 2201/0227; G01N 2201/0228; G01N 2201/024; G01N 2201/0245; G01N 2021/0112–21/958; G01N 2021/0106–2021/9586; G01N 35/00–35/1097; G01N 2035/00019–2035/1093; G01N 2204/022–2204/0228

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

|                 |         |               |            |
|-----------------|---------|---------------|------------|
| D773,071 S      | 11/2016 | Hakoda        |            |
| D777,049 S *    | 1/2017  | Barton        | D10/81     |
| D788,617 S *    | 6/2017  | Barton        | D10/81     |
| D799,999 S *    | 10/2017 | Barton        | D10/81     |
| D800,000 S *    | 10/2017 | Barton        | D10/81     |
| D802,156 S *    | 11/2017 | Barton        | D24/216    |
| D811,913 S      | 3/2018  | Barton et al. |            |
| 9,997,266 B2 *  | 6/2018  | Zhang         | G01N 21/65 |
| D824,536 S *    | 7/2018  | Barton        | D24/232    |
| D825,776 S *    | 8/2018  | Quick         | D24/232    |
| D828,575 S *    | 9/2018  | Ohno          | G01N 21/65 |
|                 |         |               | D24/216    |
| D830,210 S *    | 10/2018 | Ihara         | G01N 21/01 |
|                 |         |               | D10/81     |
| 10,220,387 B2 * | 3/2019  | Granier       | G01N 21/01 |
| D850,955 S      | 6/2019  | Barton et al. |            |
| D850,956 S      | 6/2019  | Barton et al. |            |

OTHER PUBLICATIONS

Japanese Patent Office, “Notice of Reason for Rejection,” issued in connection with Japanese Design Application No. 2016-19292, dated Nov. 8, 2016, 3 pages.

Japanese Patent Office, “Notice of Reason for Rejection,” issued in connection with Japanese Design Application No. 2016-19291, dated Nov. 8, 2016, 3 pages.

State Intellectual Property Office of China, “Notice of Grant of Patent Right,” issued in connection with Chinese Patent Application No. 201530555258.3, dated Oct. 20, 2016, 5 pages.

Japanese Patent Office, “Notice of Reason for Rejection,” issued in connection with Japanese Design Application No. 2015-28872 dated Jun. 14, 2016, 5 pages.

Office for Harmonization in the Internal Market, “Notification of the Registration of the Community Designs,” issued in connection with European Community Design Nos. 002930230-0001 through 002930230-0029, dated Mar. 17, 2016, 6 pages.

United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/531,578, dated Sep. 8, 2016, 14 pages.

United States Patent and Trademark Office, “Restriction and/or Election Requirement,” issued in connection with U.S. Appl. No. 29/531,578, dated Jul. 6, 2016, 18 pages.

Japanese Patent Office, “Directive,” issued in connection with Japanese Patent Application No. 2016-19292, dated Mar. 7, 2017, 5 pages.

State Intellectual Property Office of China, “Notice of Grant of Patent Right for a Design,” issued in connection with Chinese Patent Application No. 201630657956.9, dated Jul. 6, 2017, 2 pages.

United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/587,978, dated Nov. 3, 2017, 8 pages.

United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/633,295, dated Jan. 17, 2019, 24 pages.

United States Patent and Trademark Office, “Notice of Allowance and Fee(s) Due,” issued in connection with U.S. Appl. No. 29/633,292, dated Jan. 17, 2019, 25 pages.

\* cited by examiner

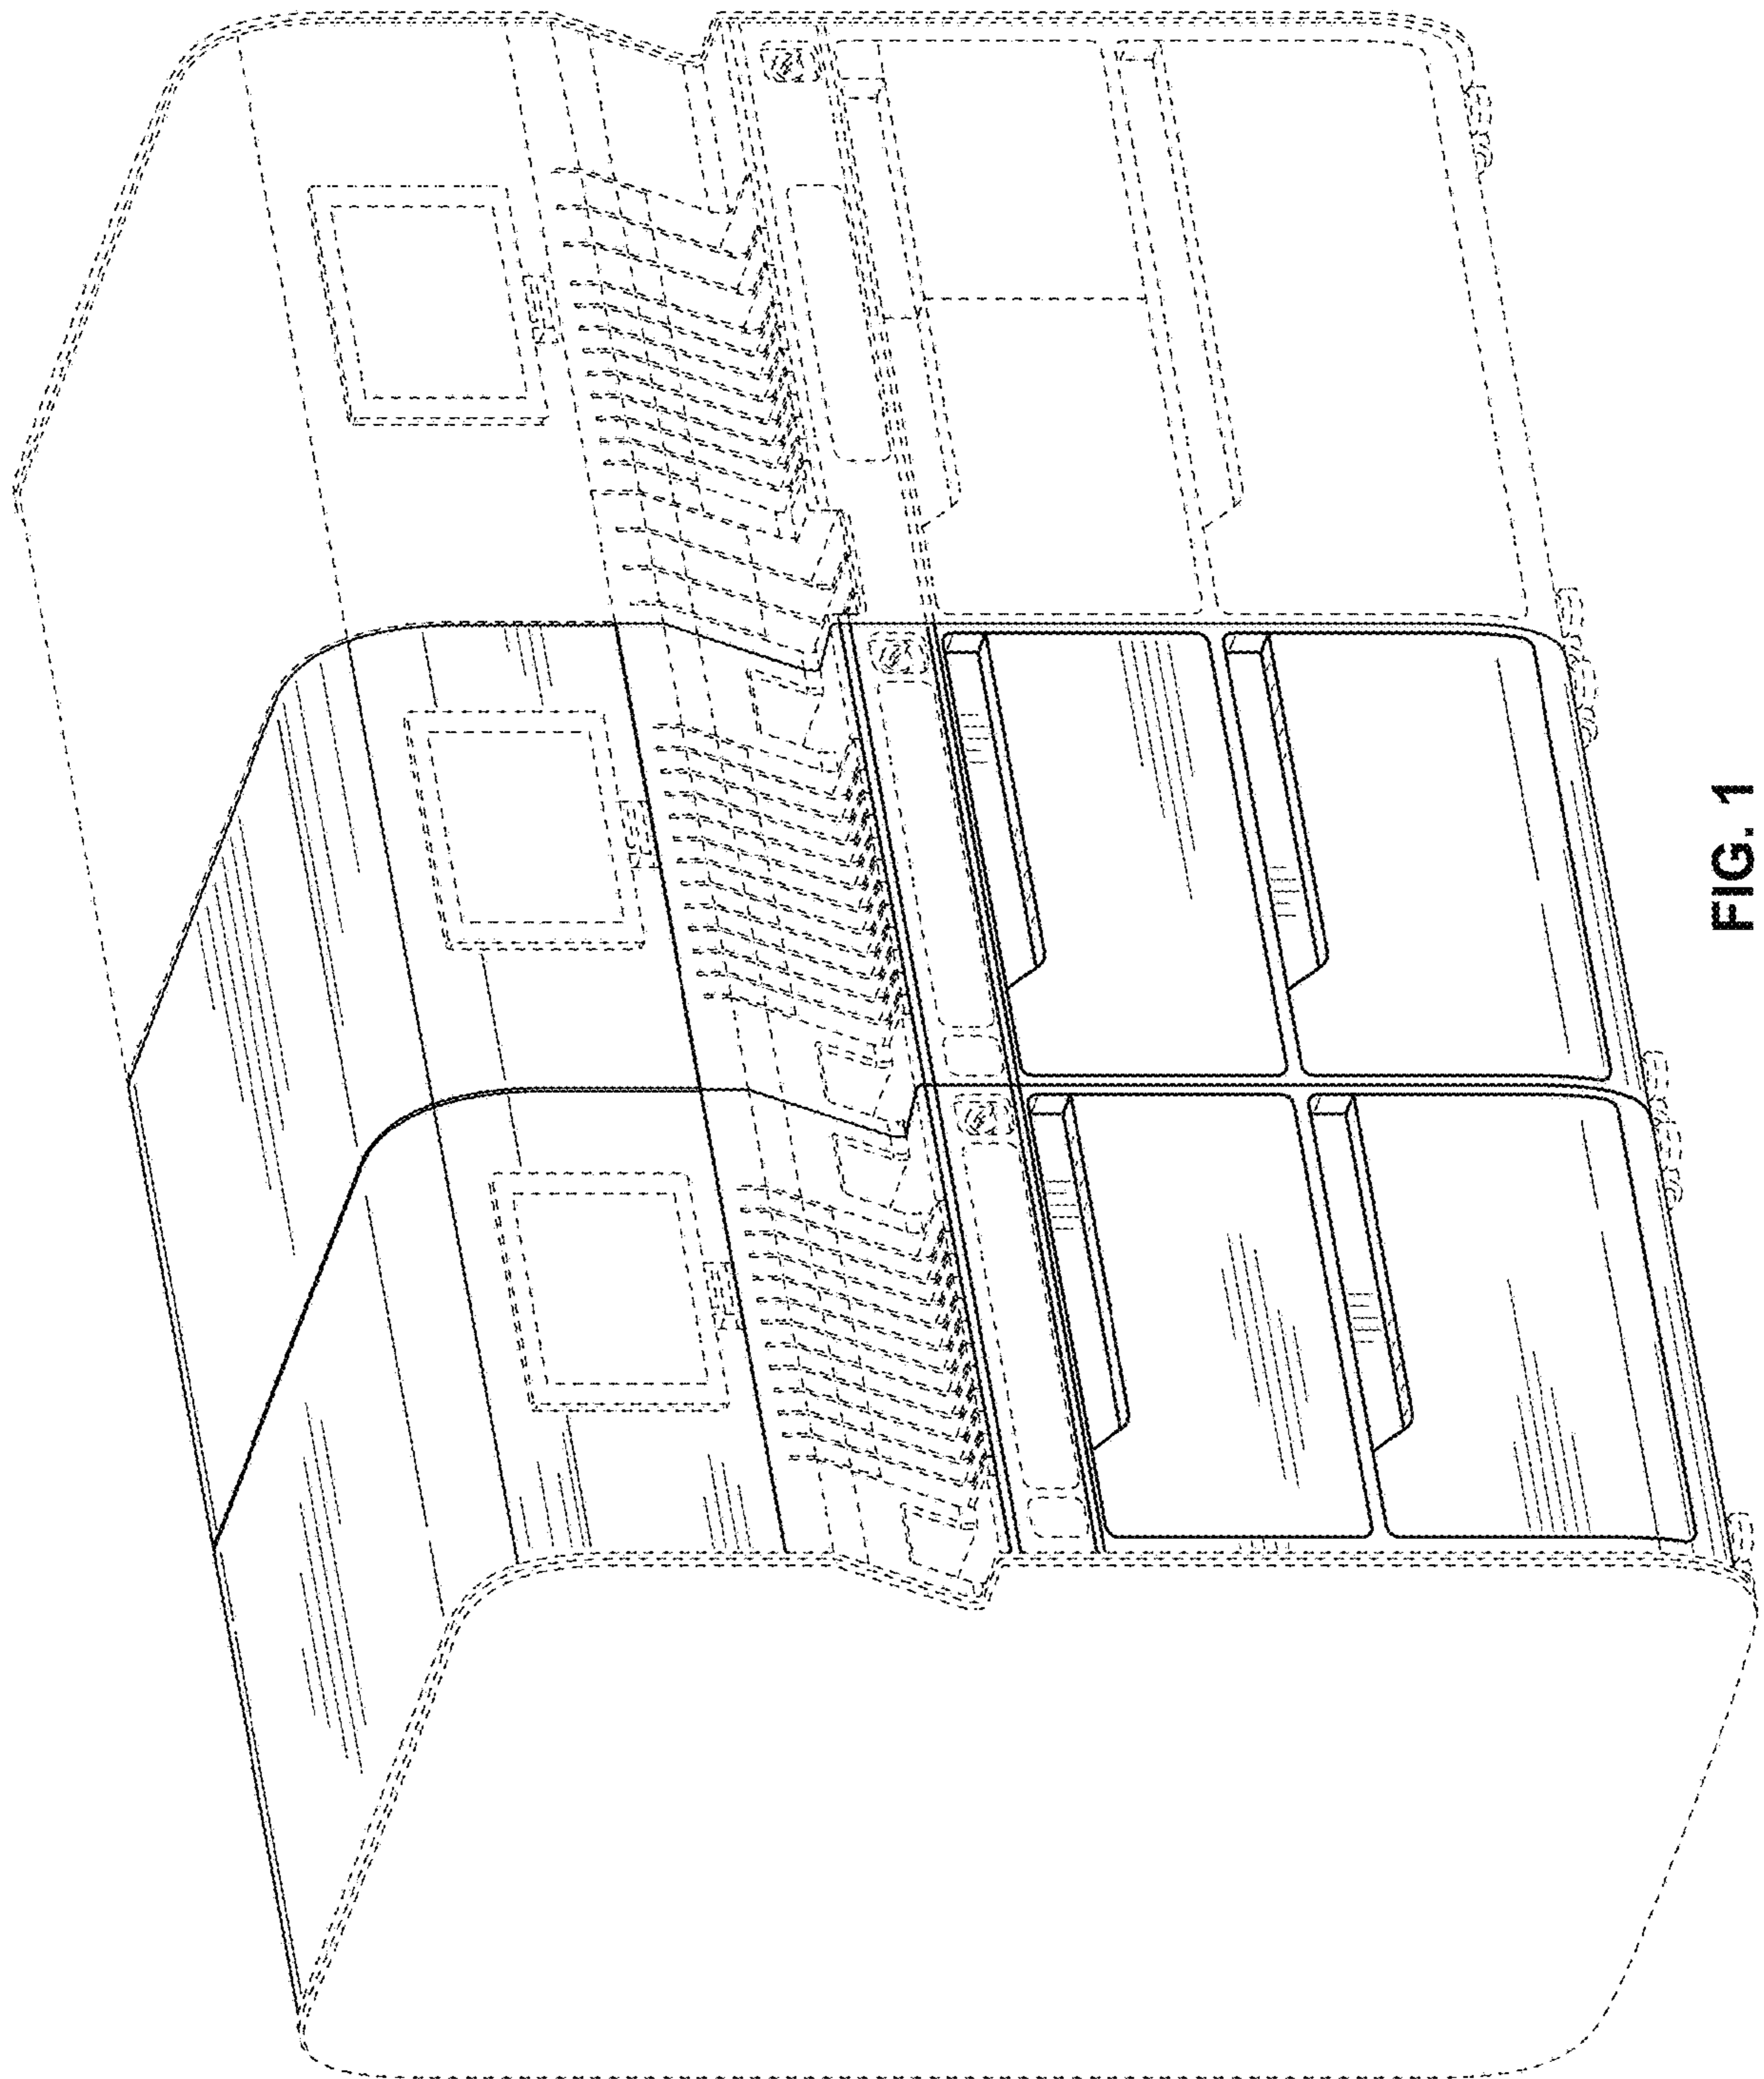


FIG. 1

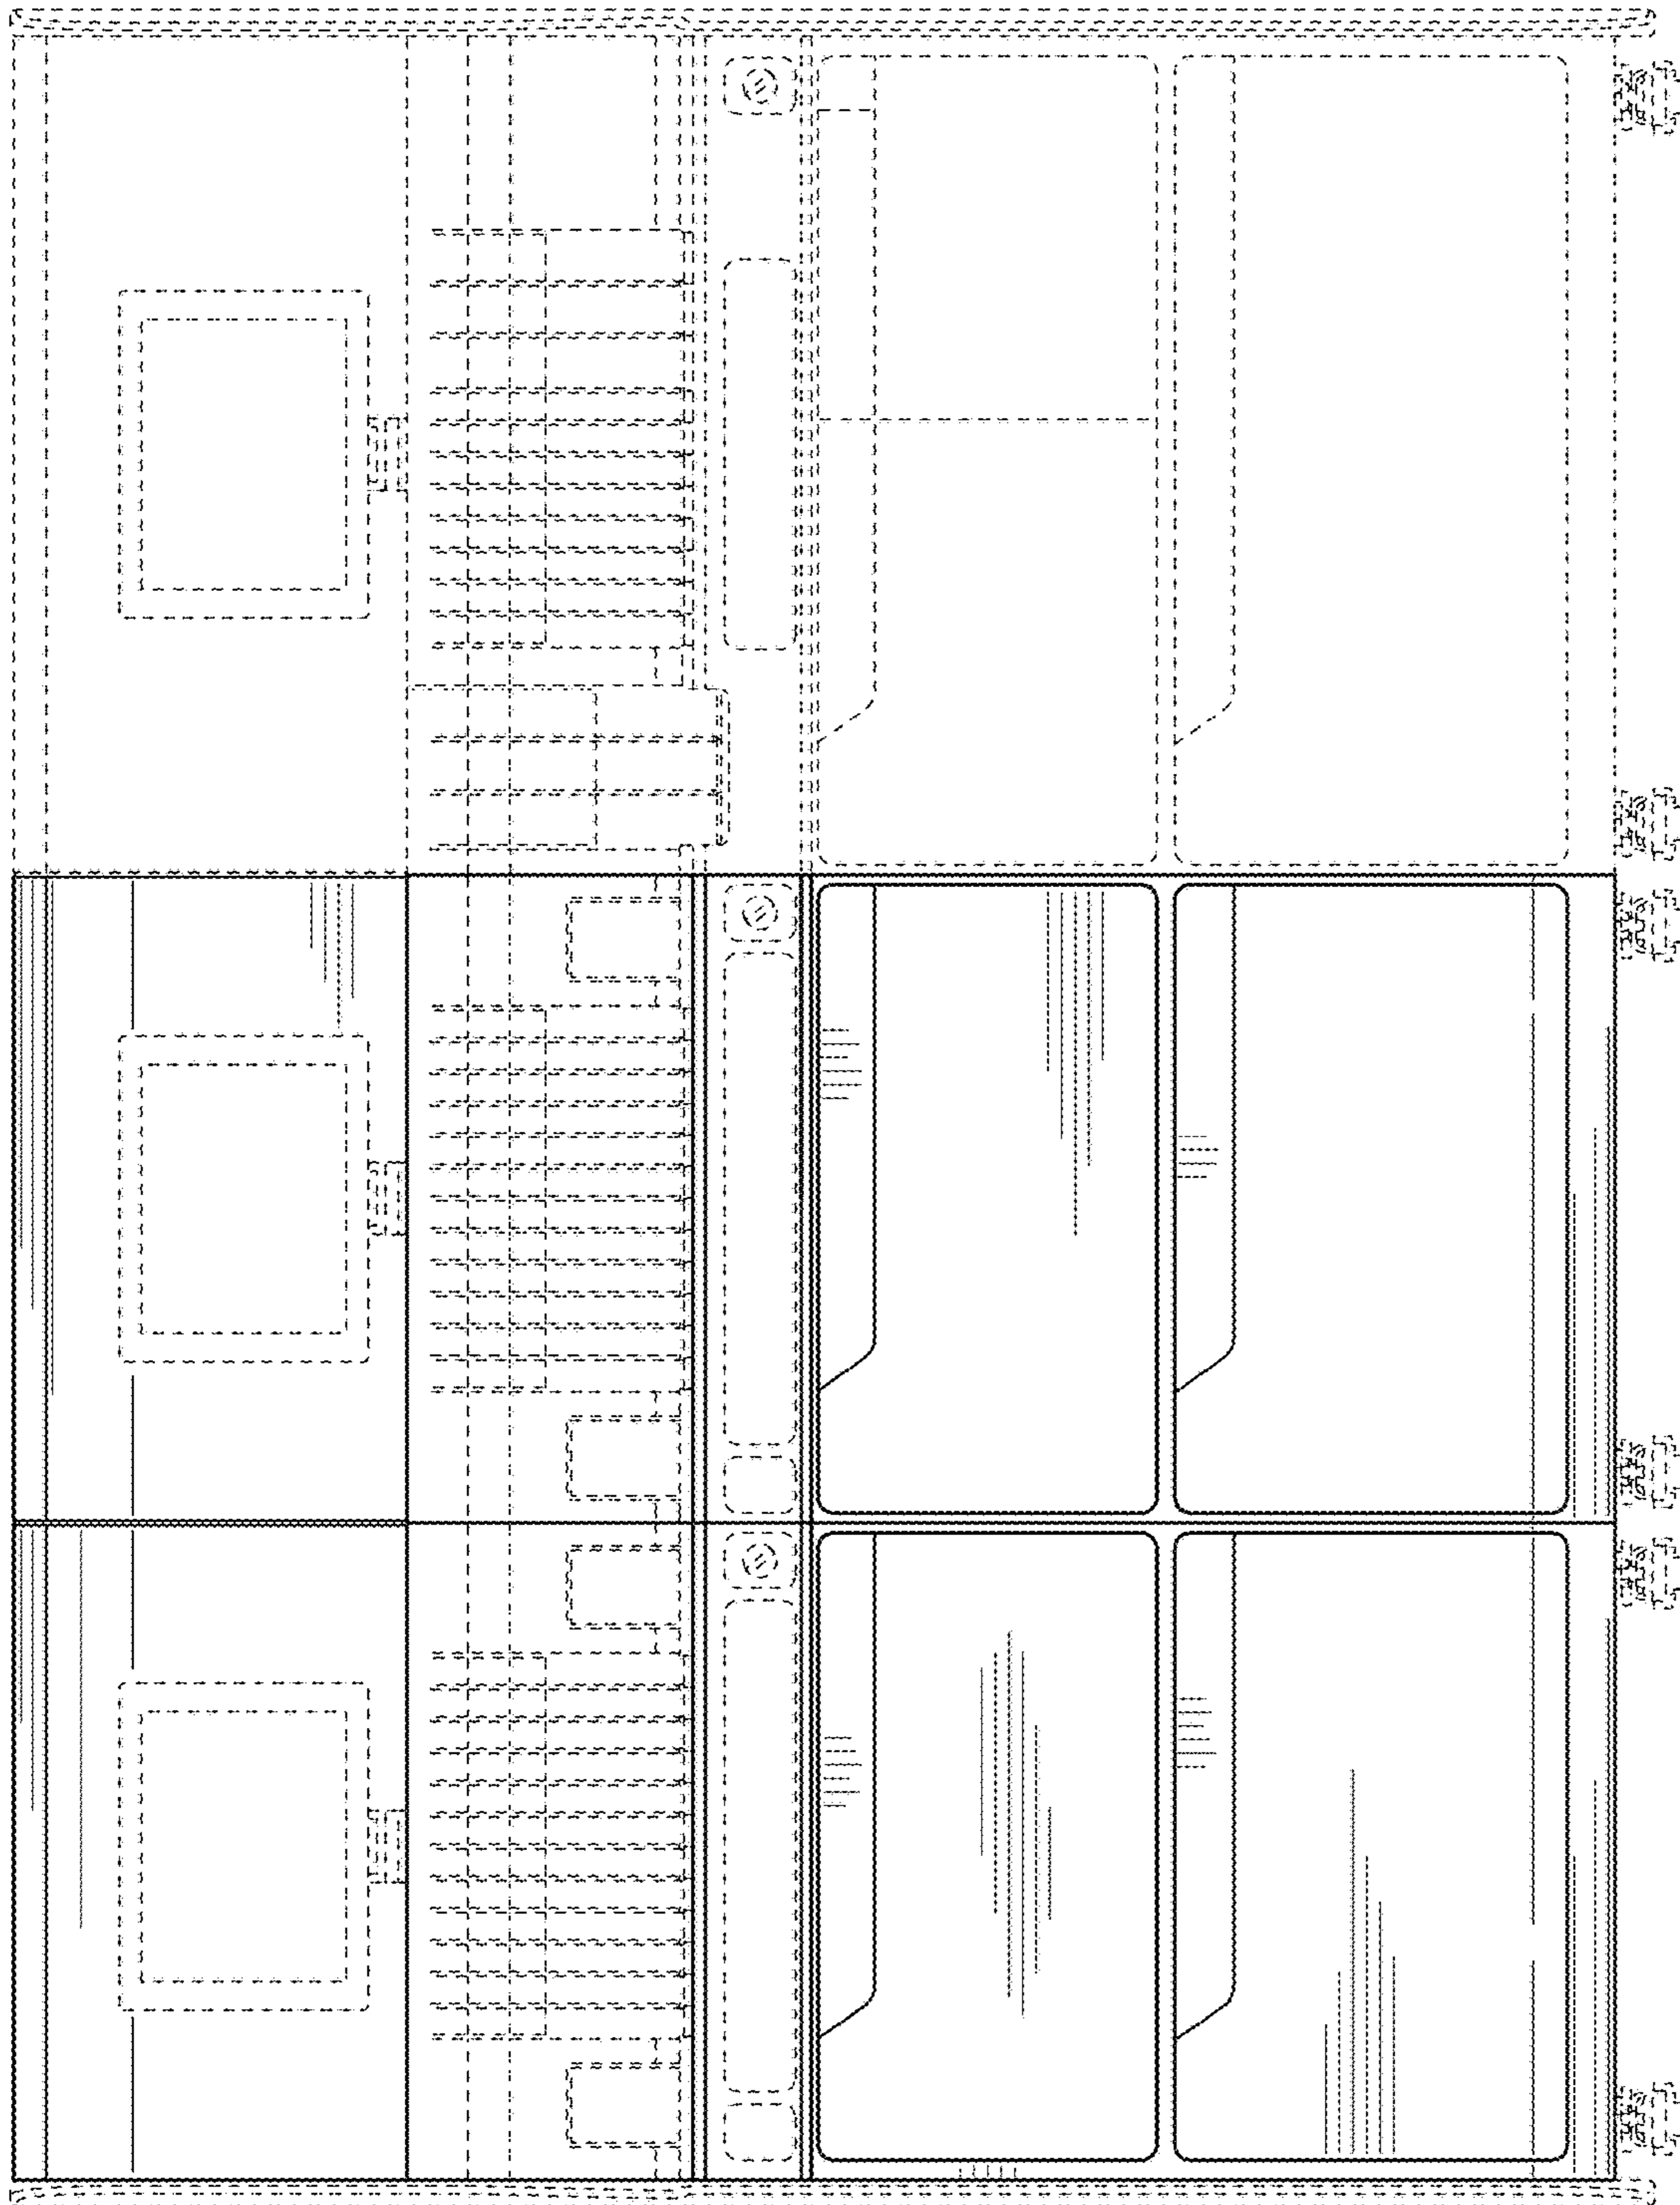


FIG. 2

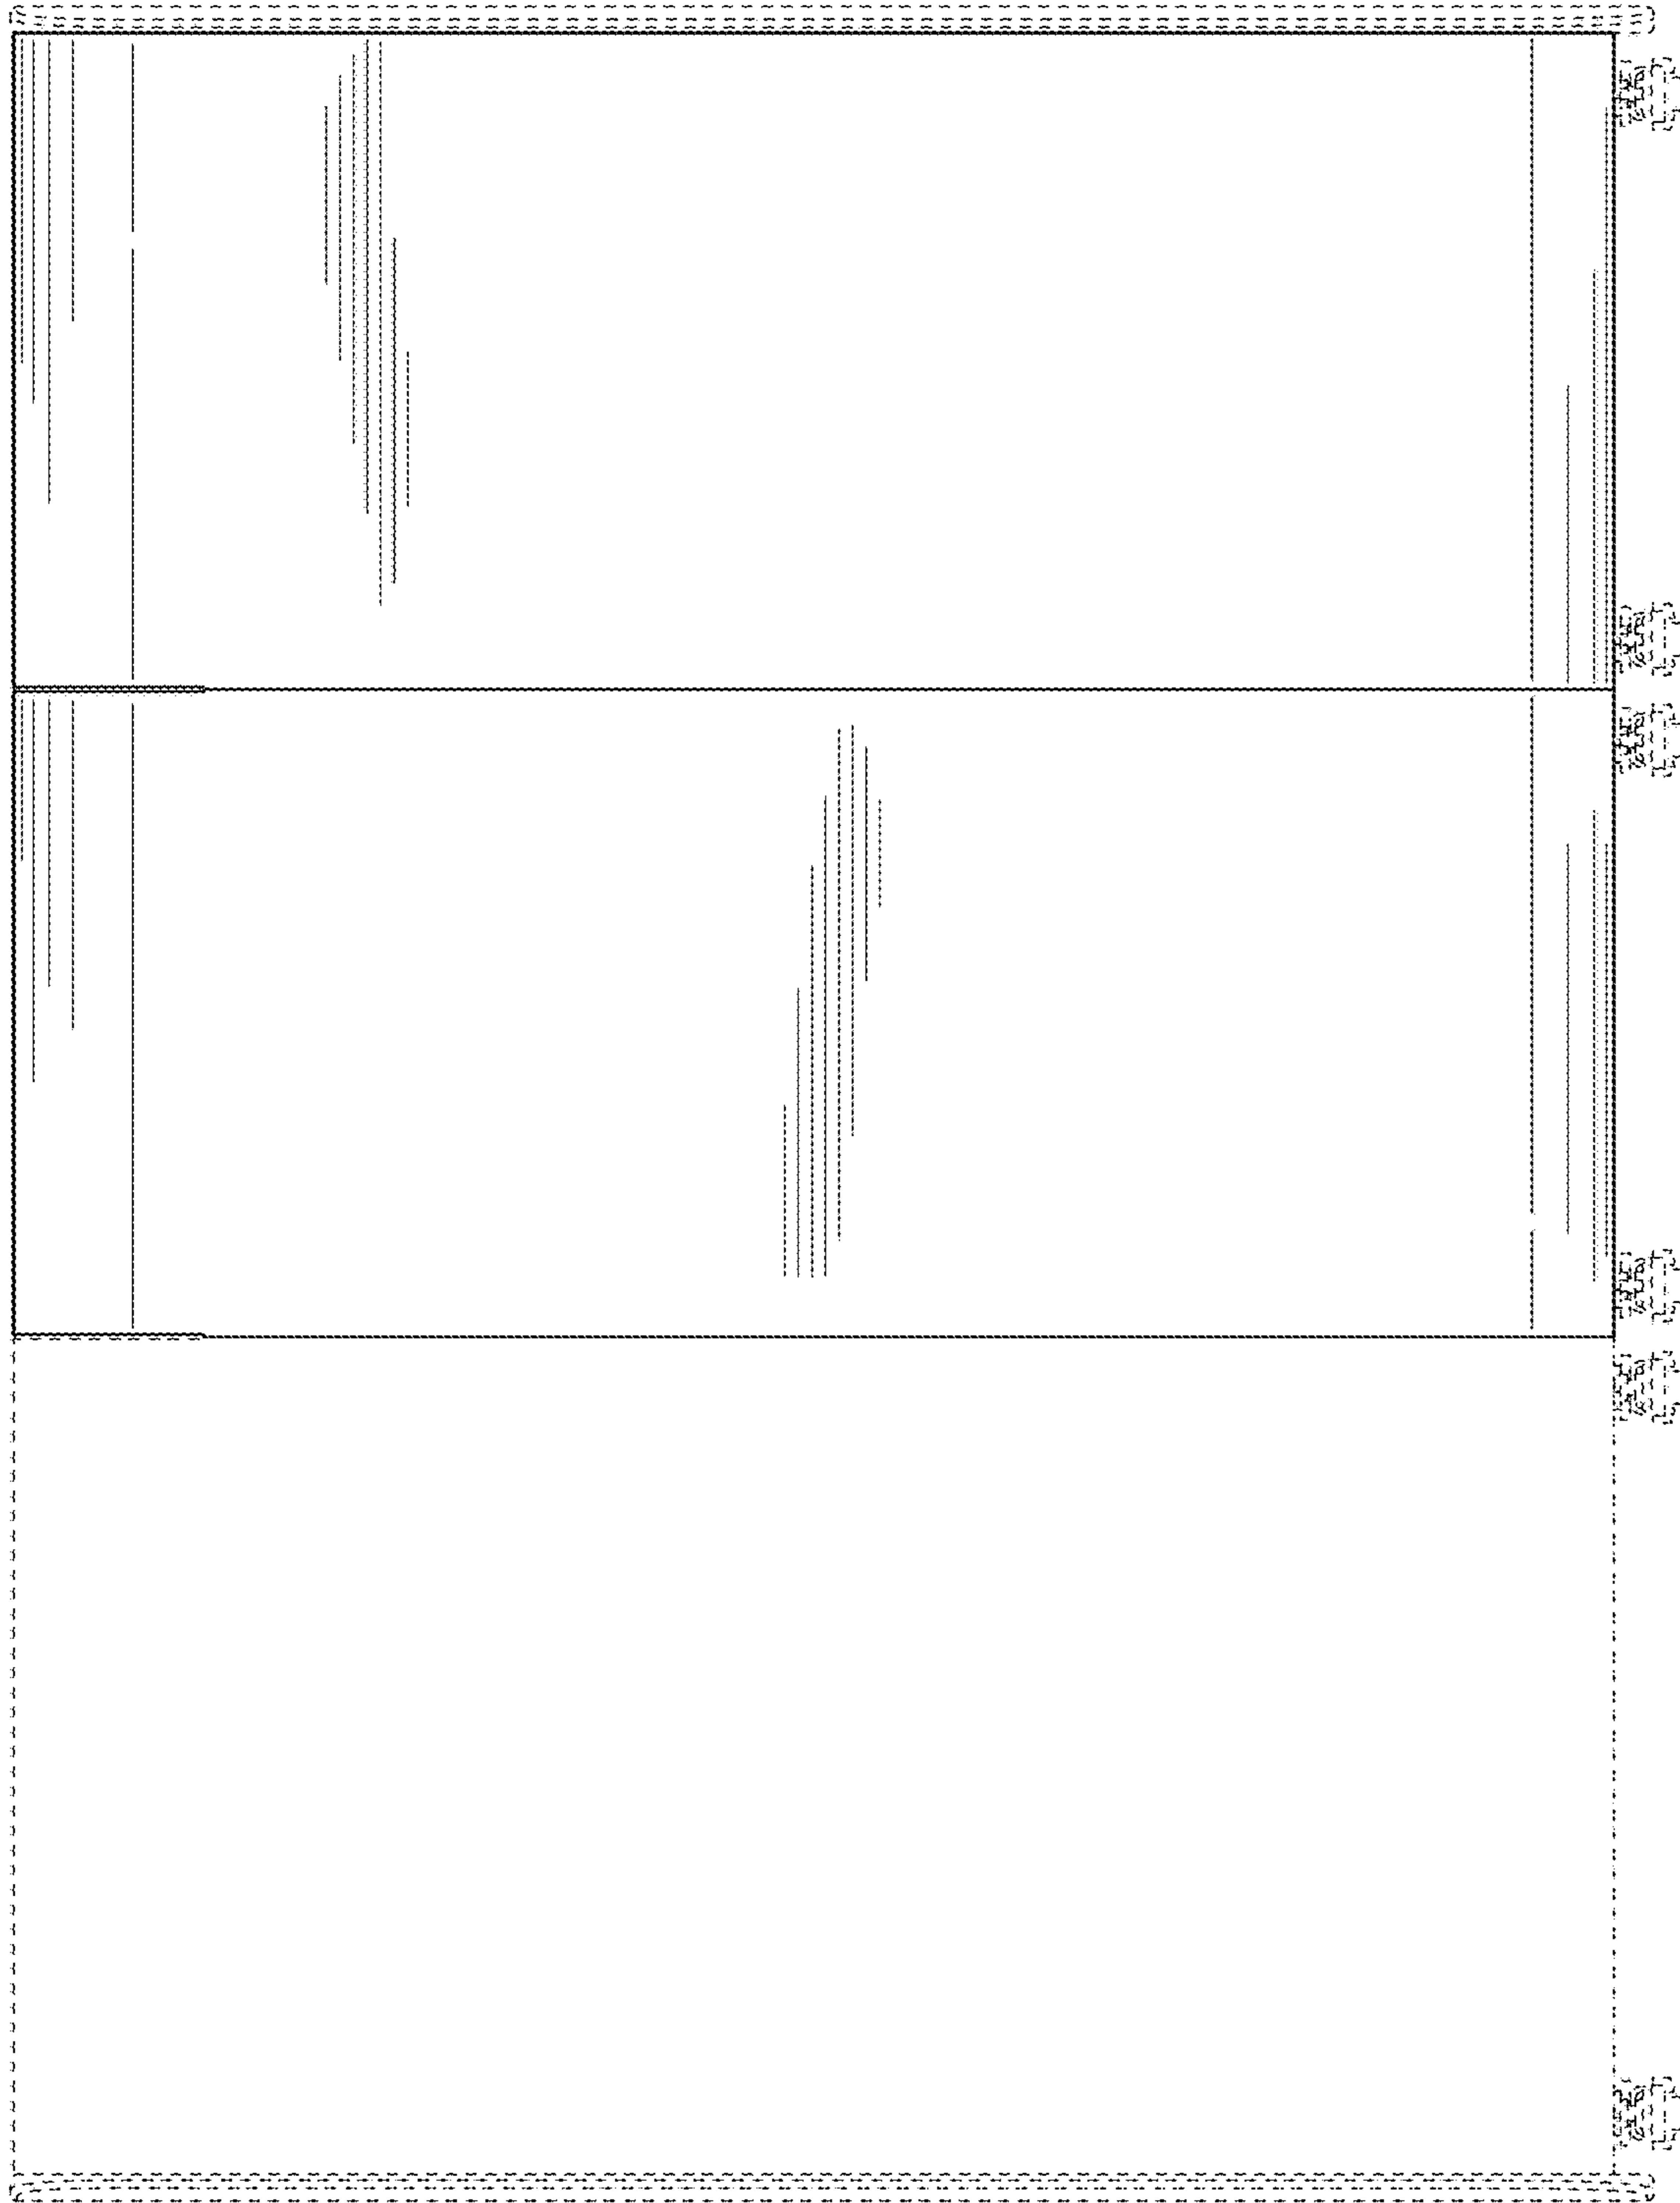


FIG. 3

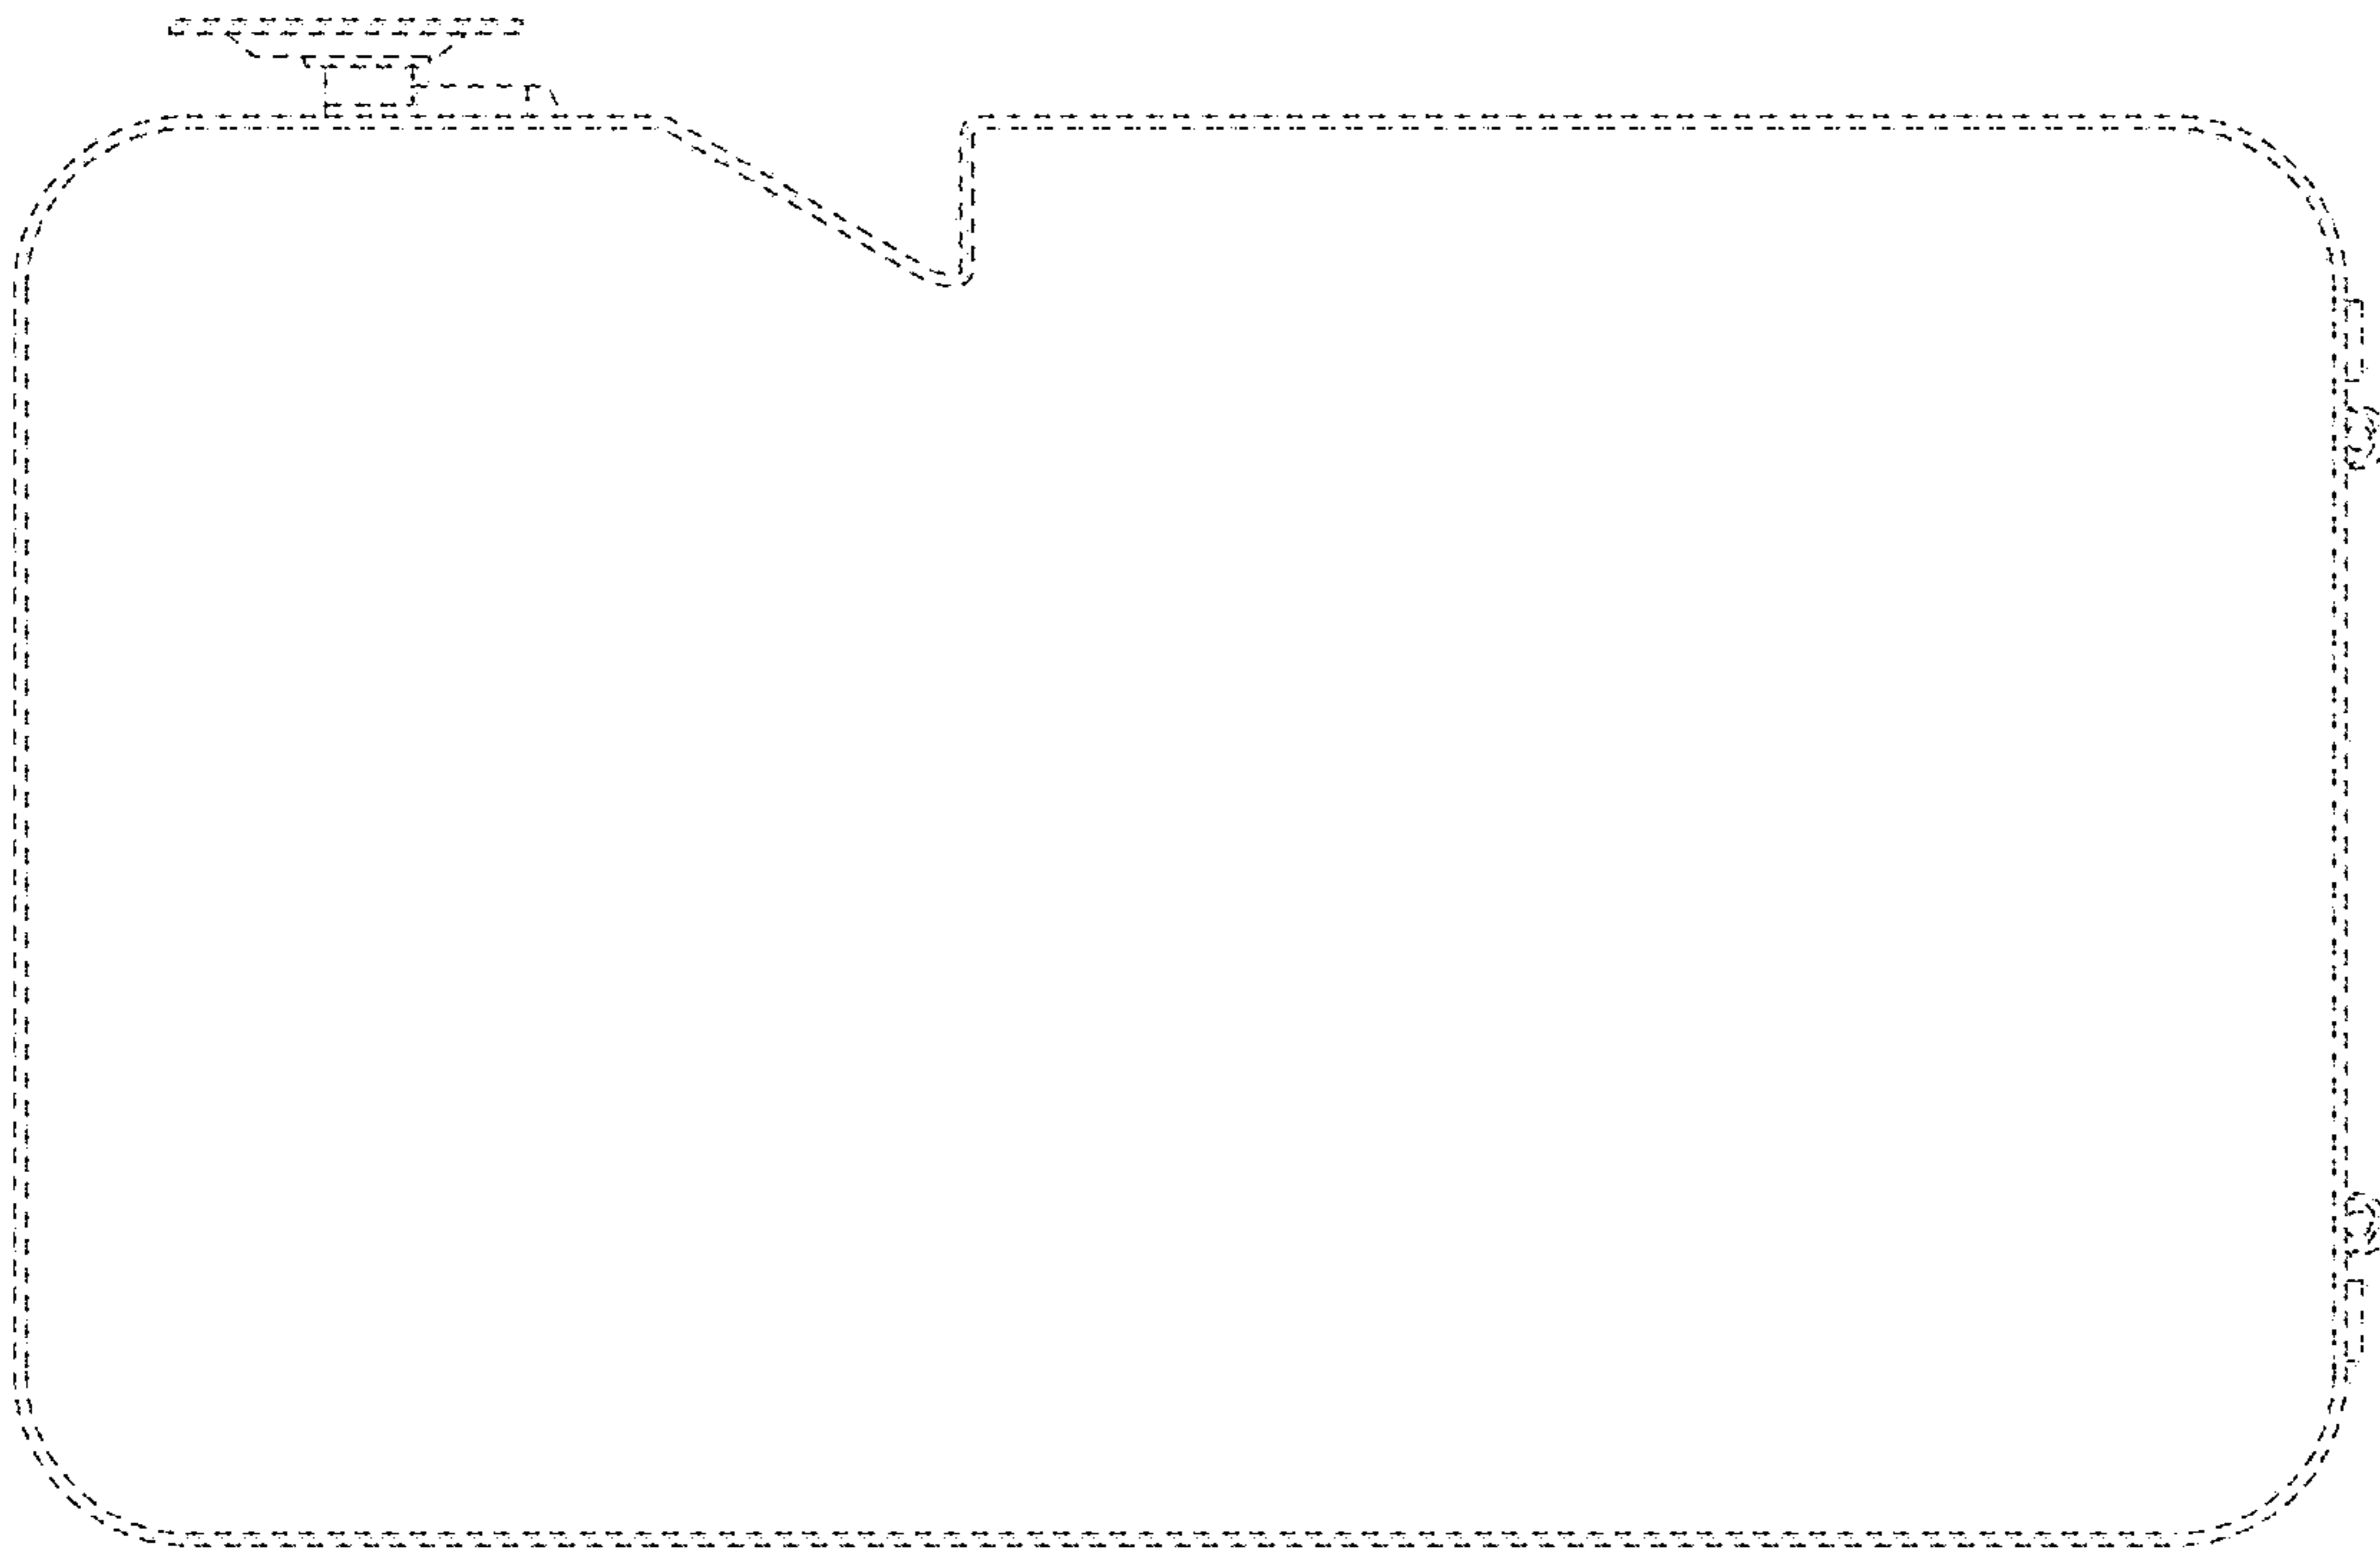


FIG. 5

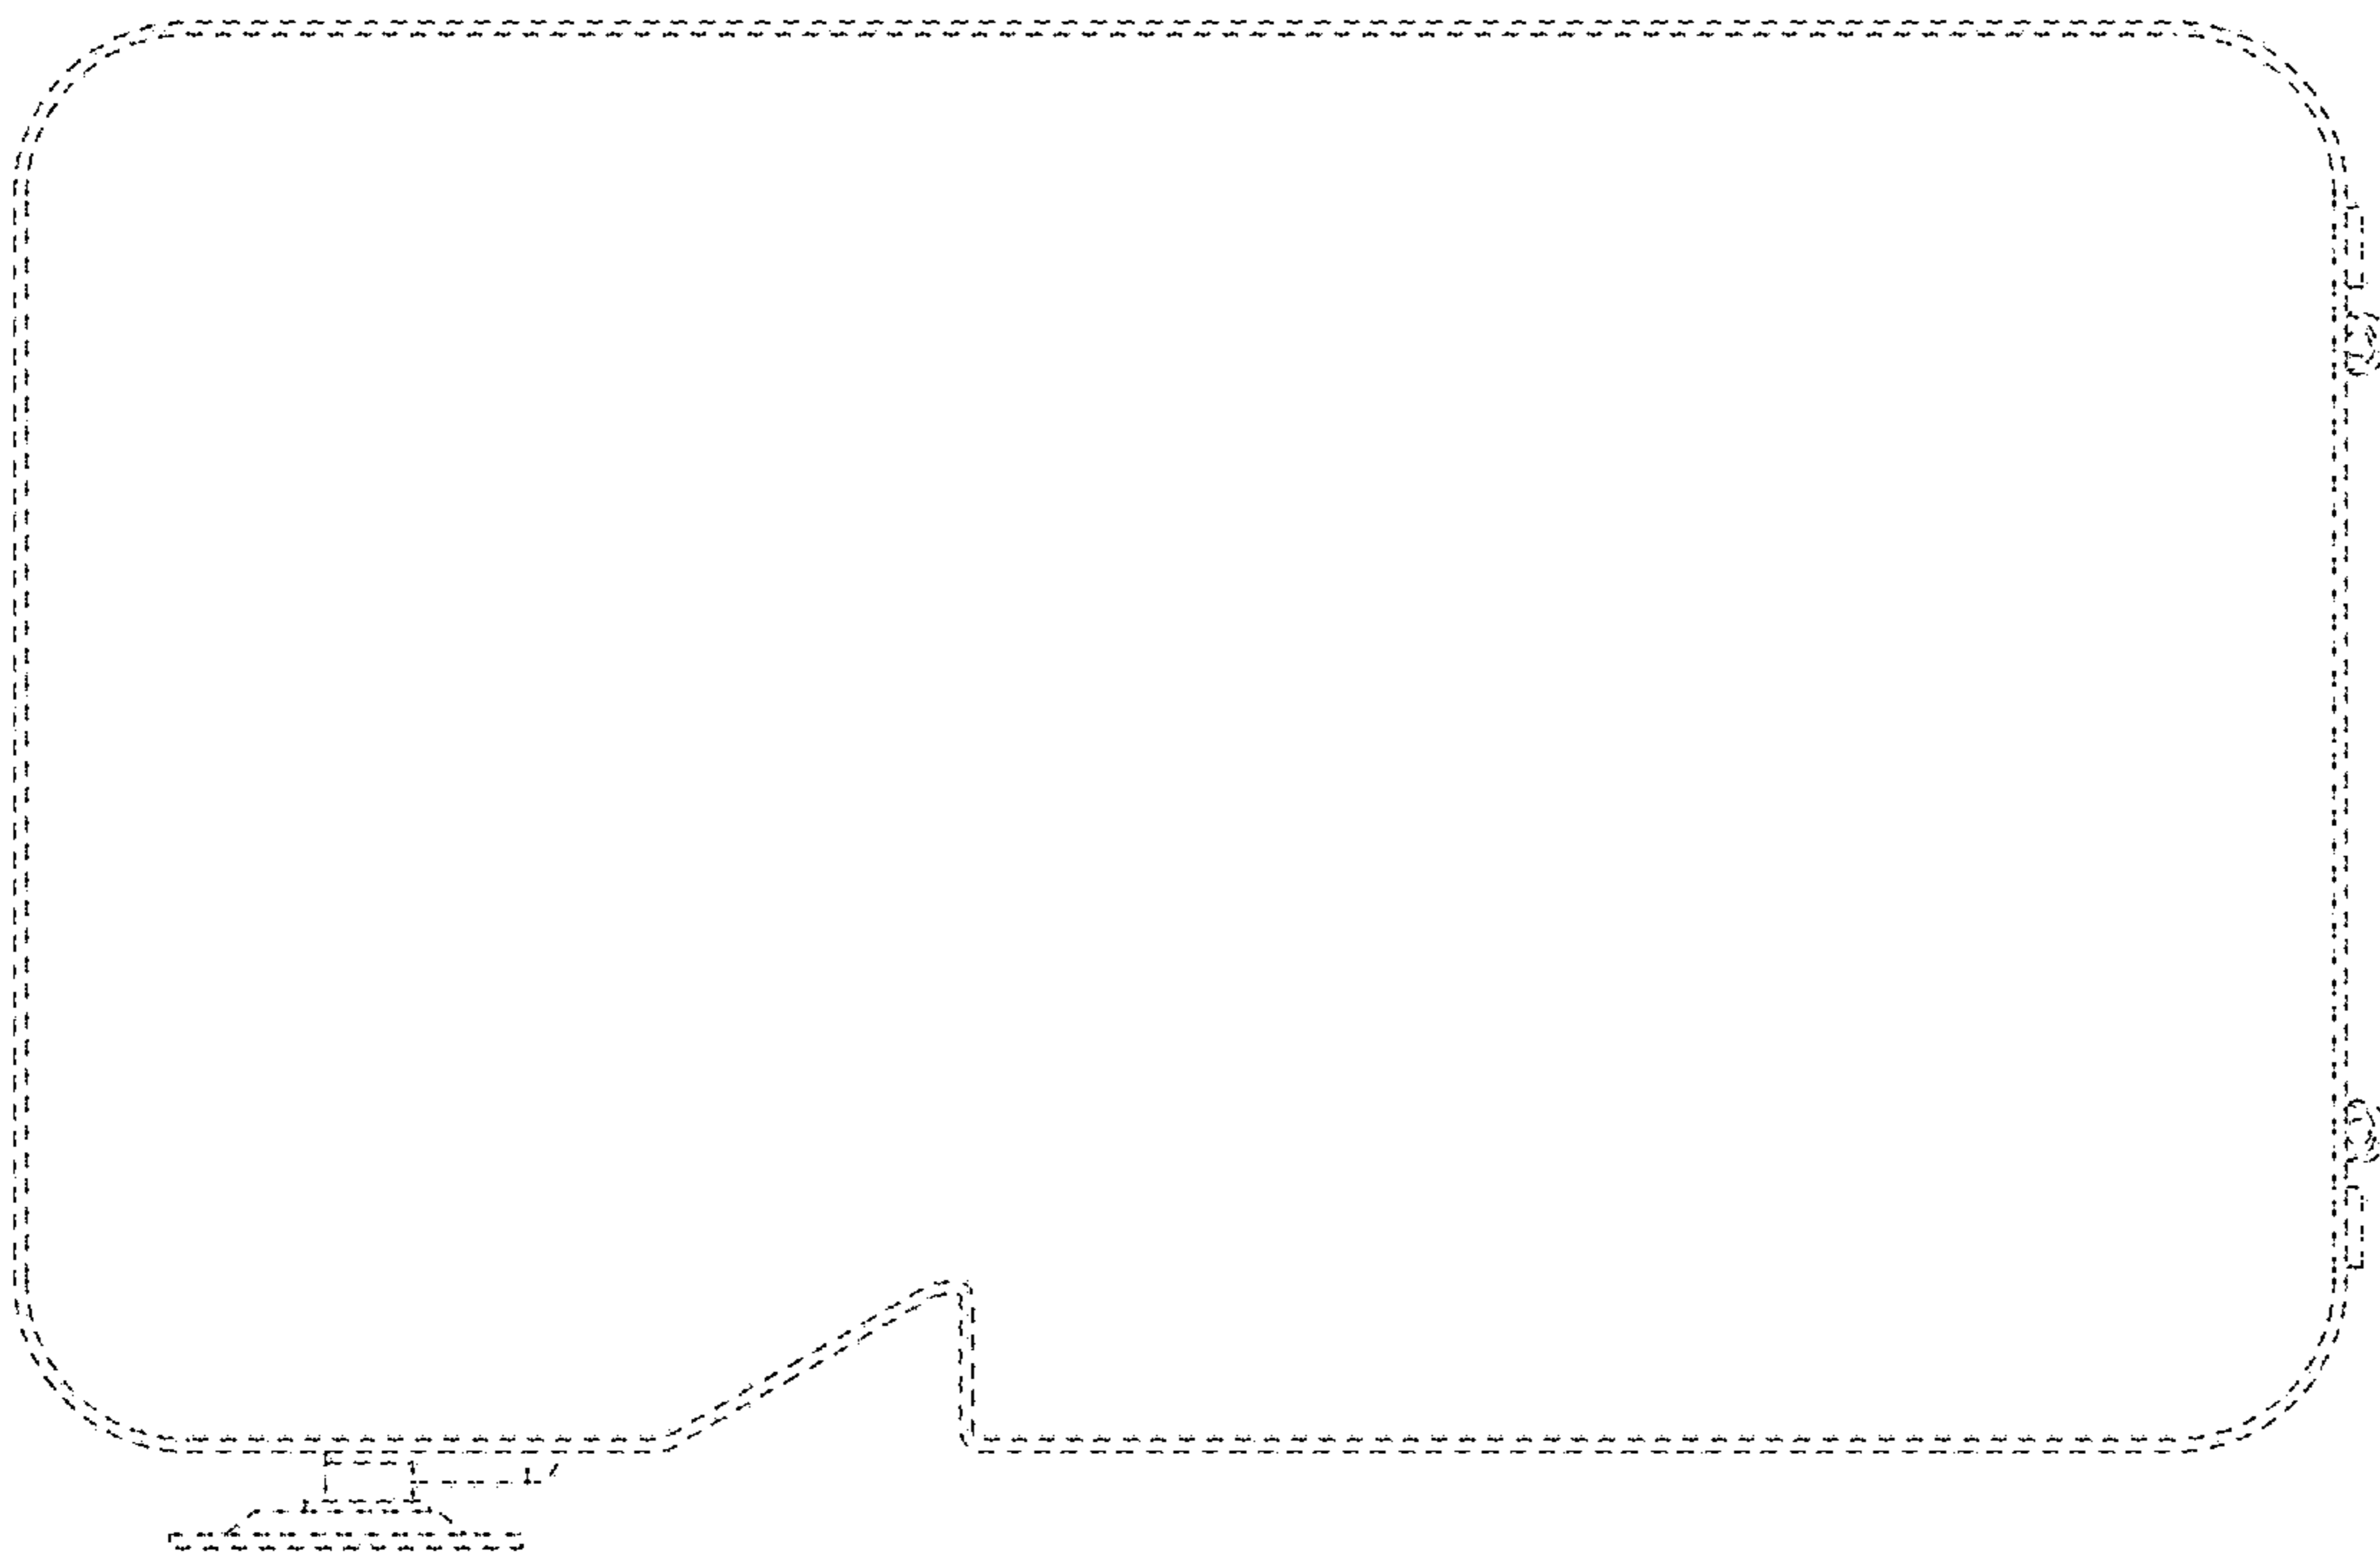


FIG. 4

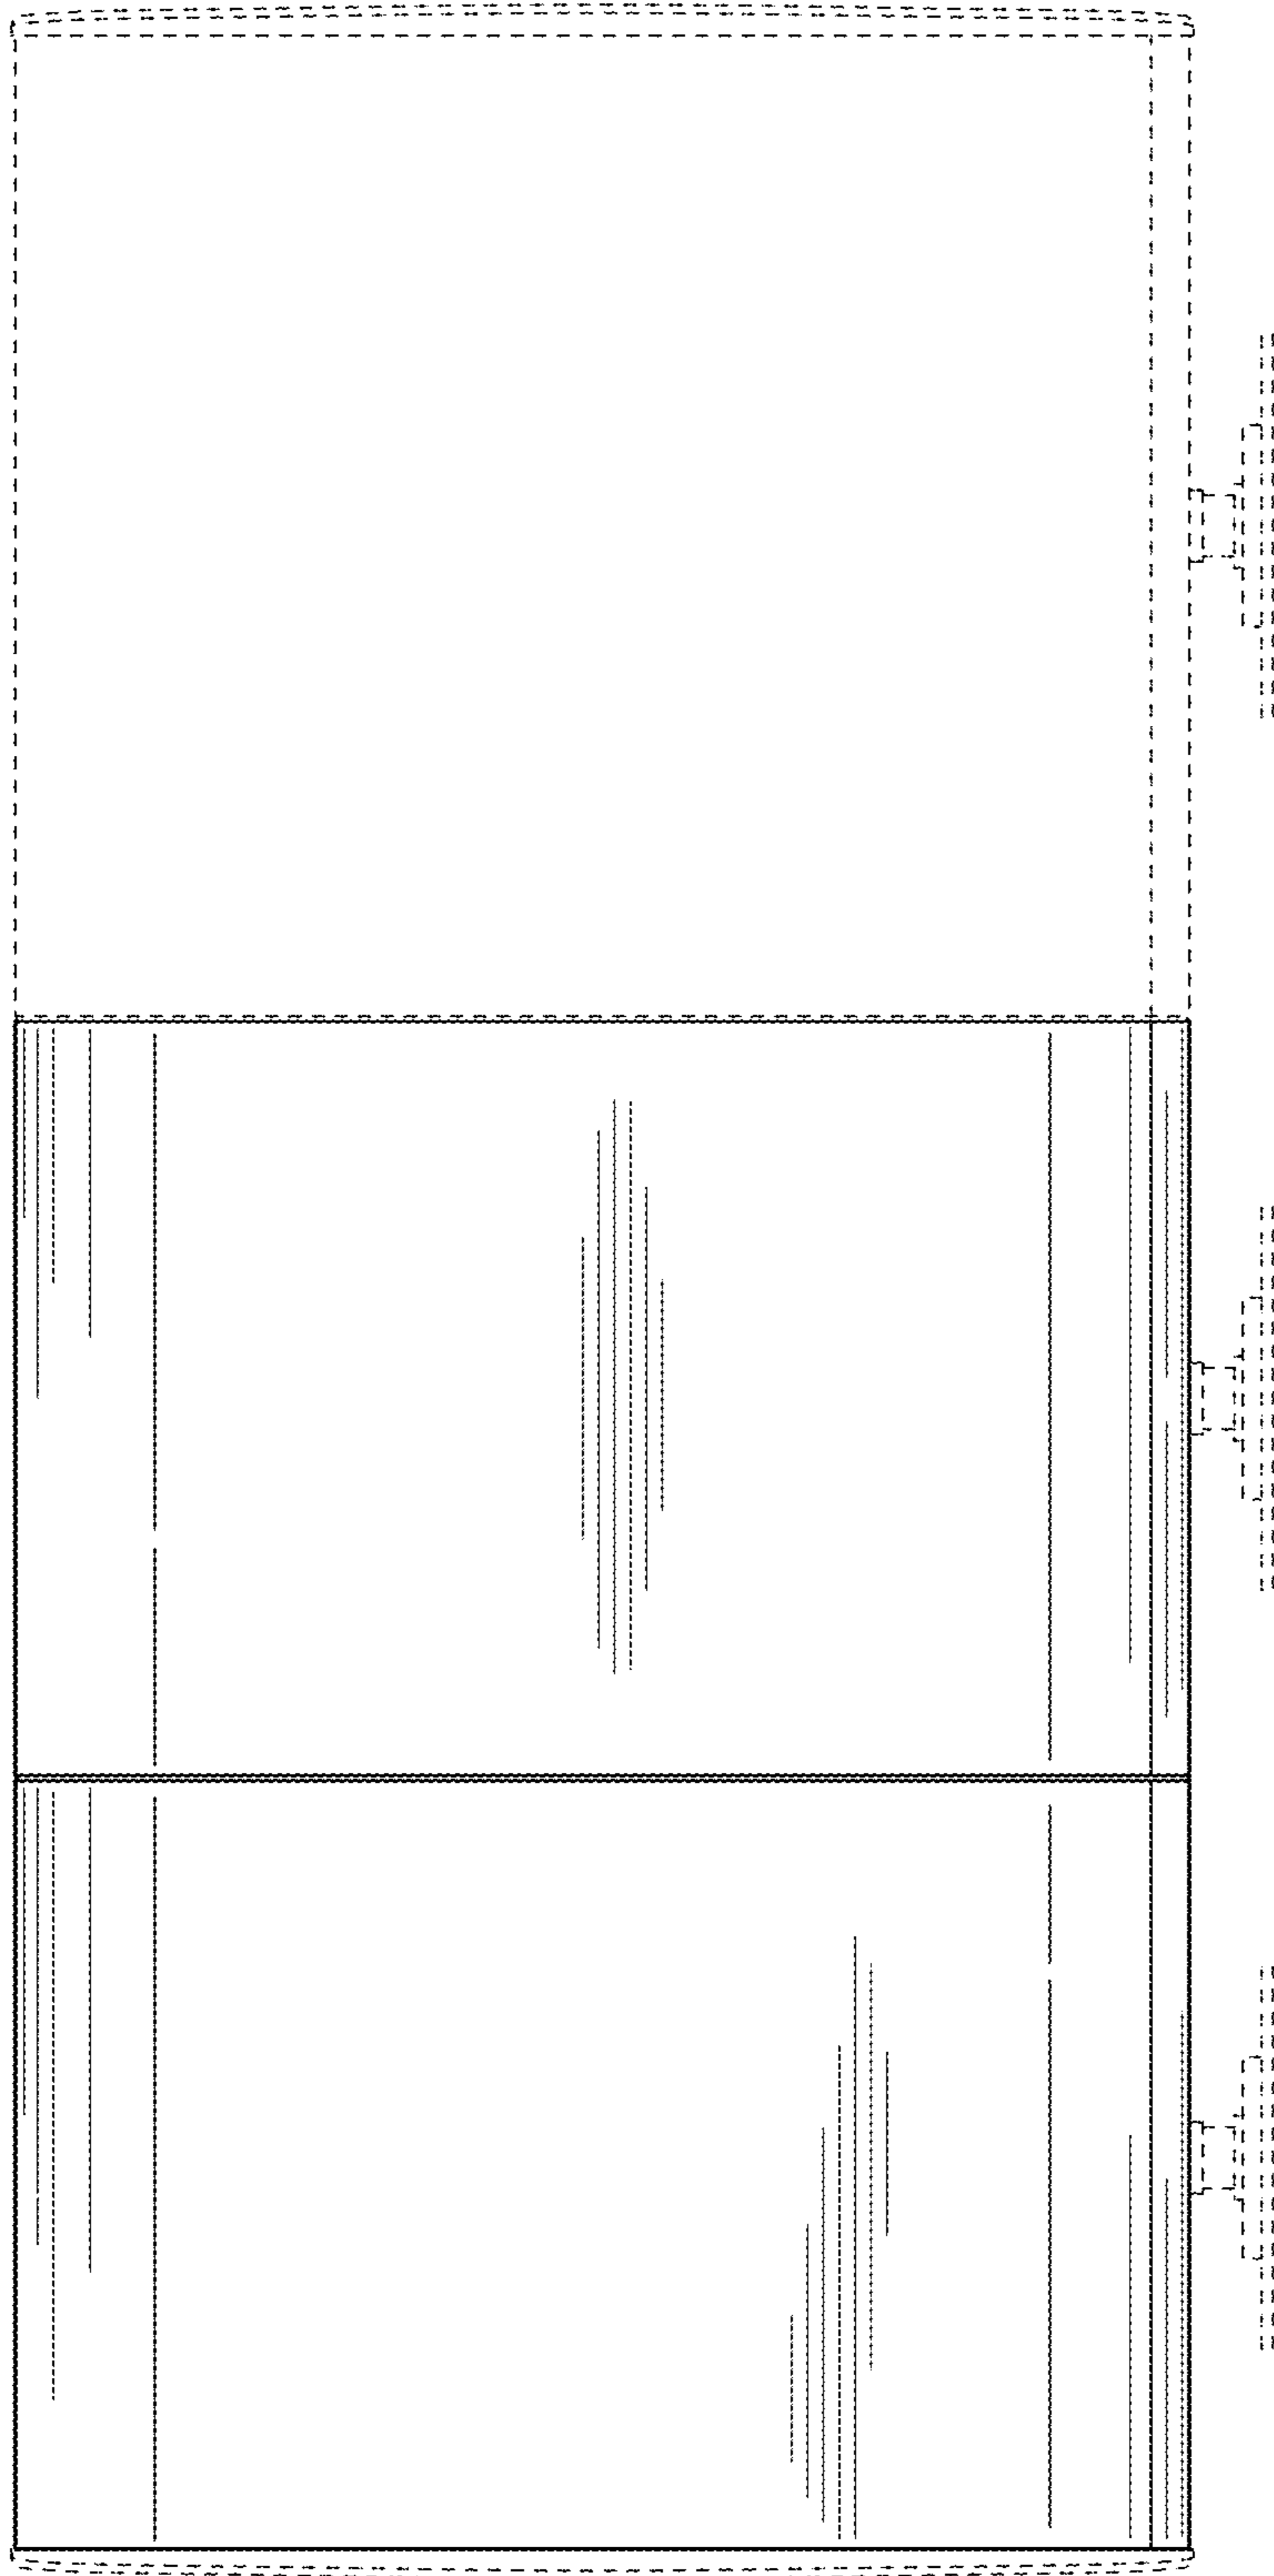


FIG. 6

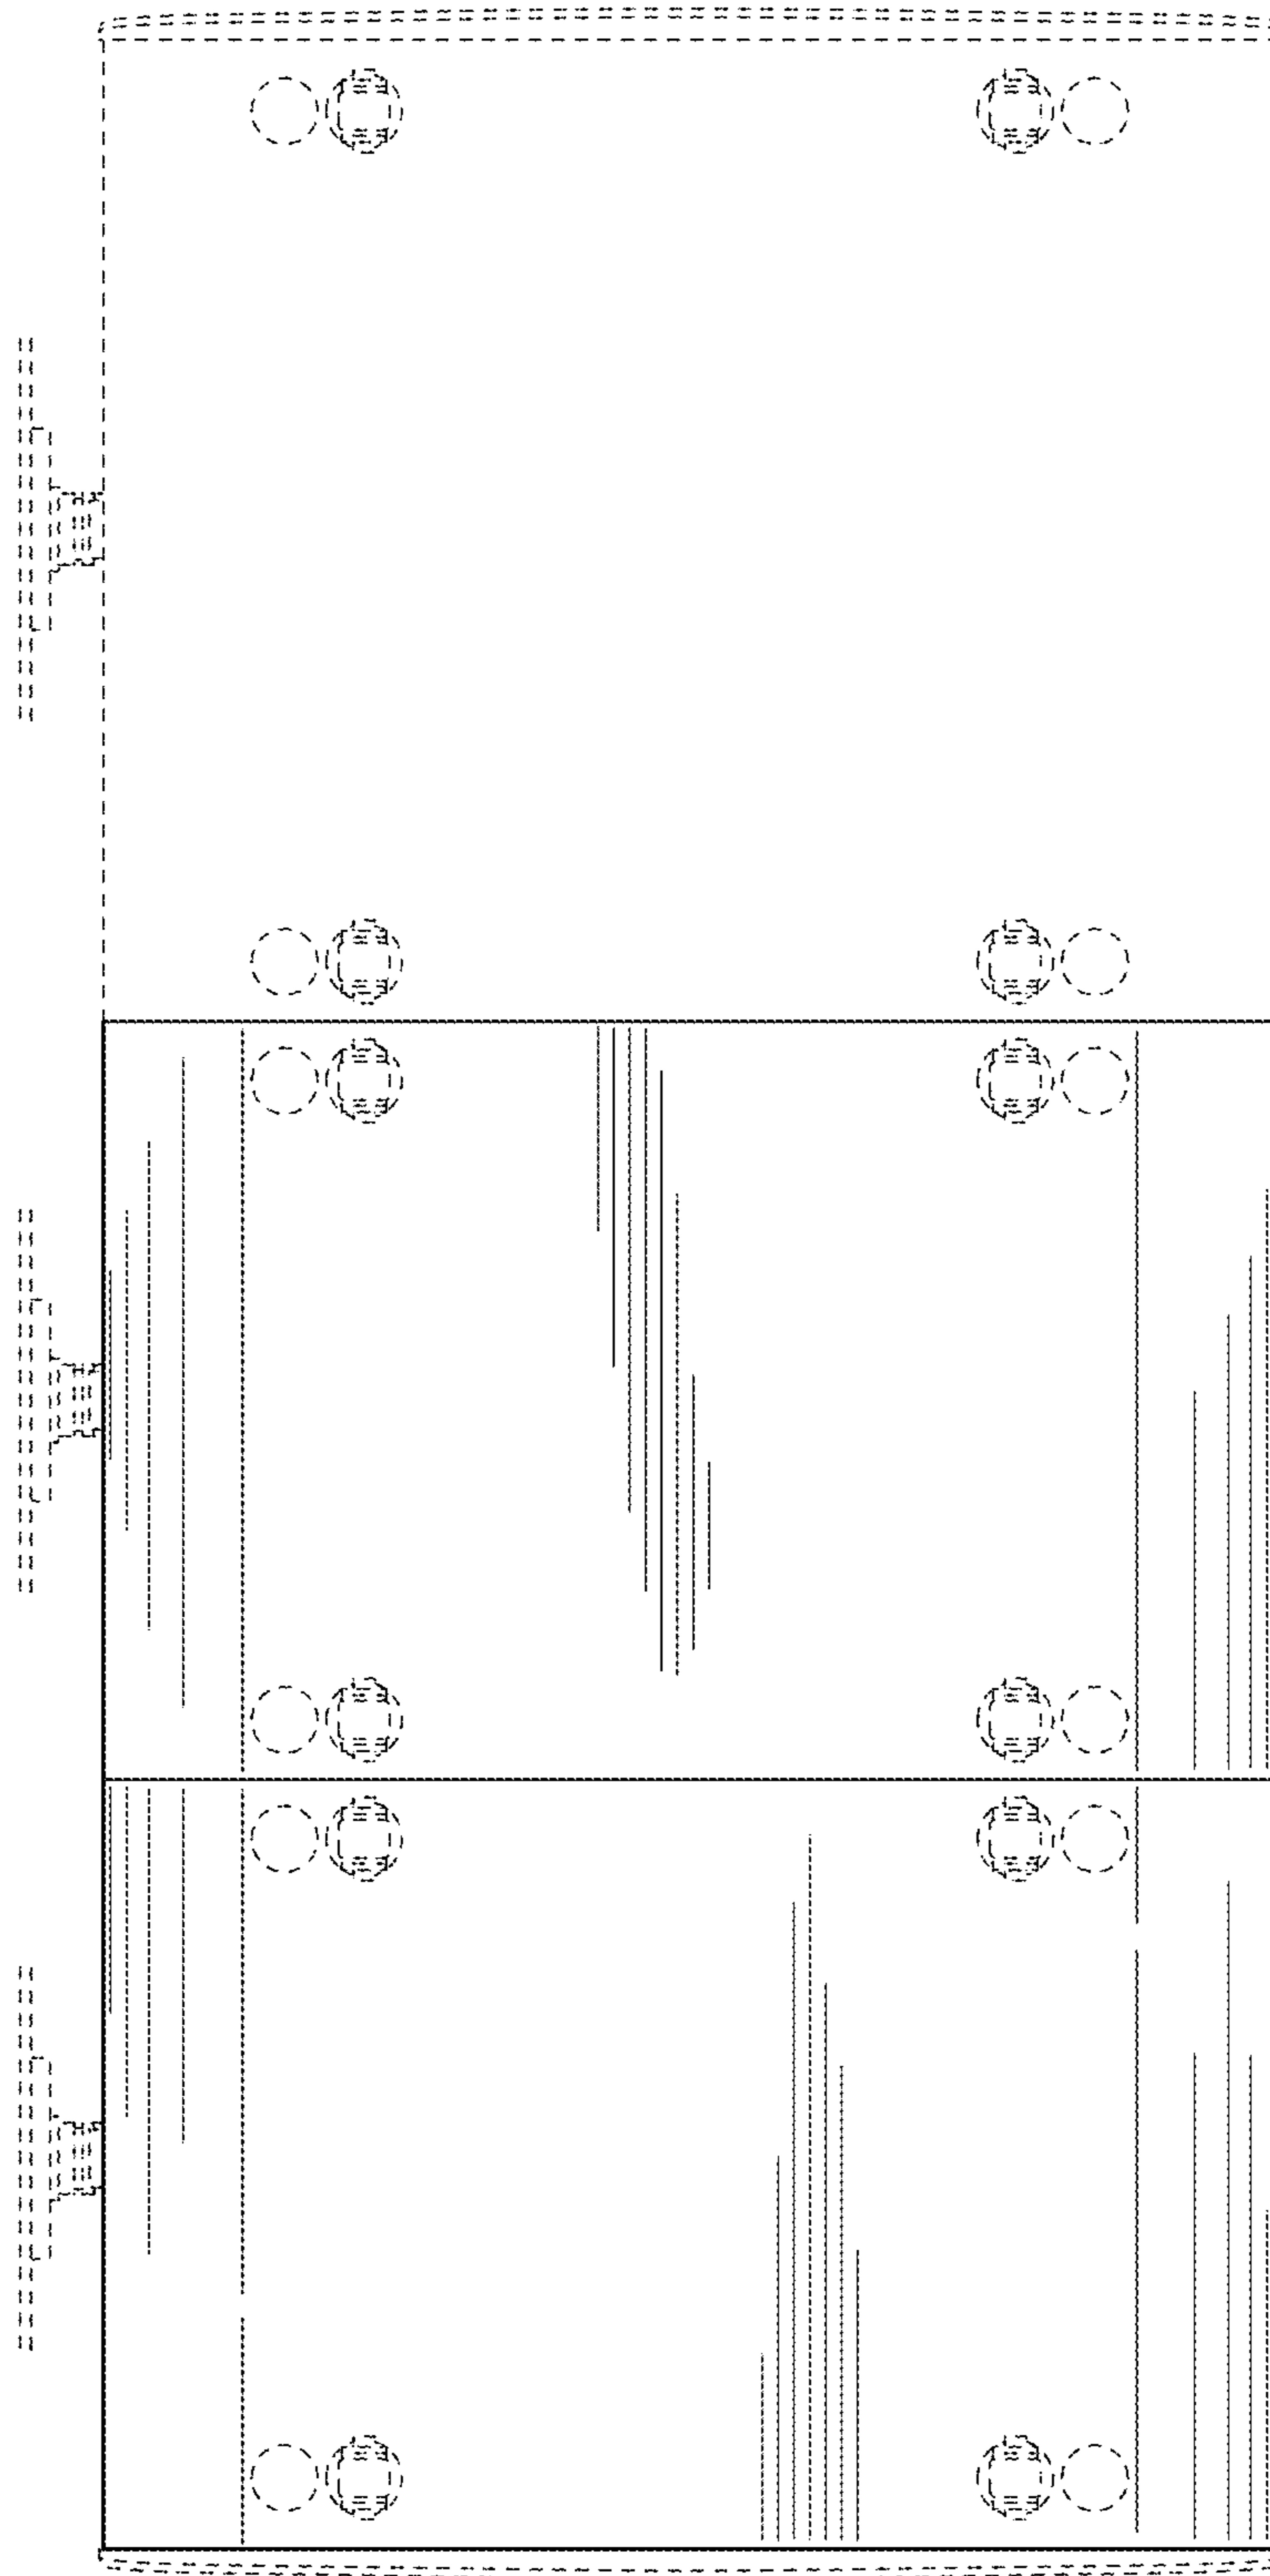


FIG. 7



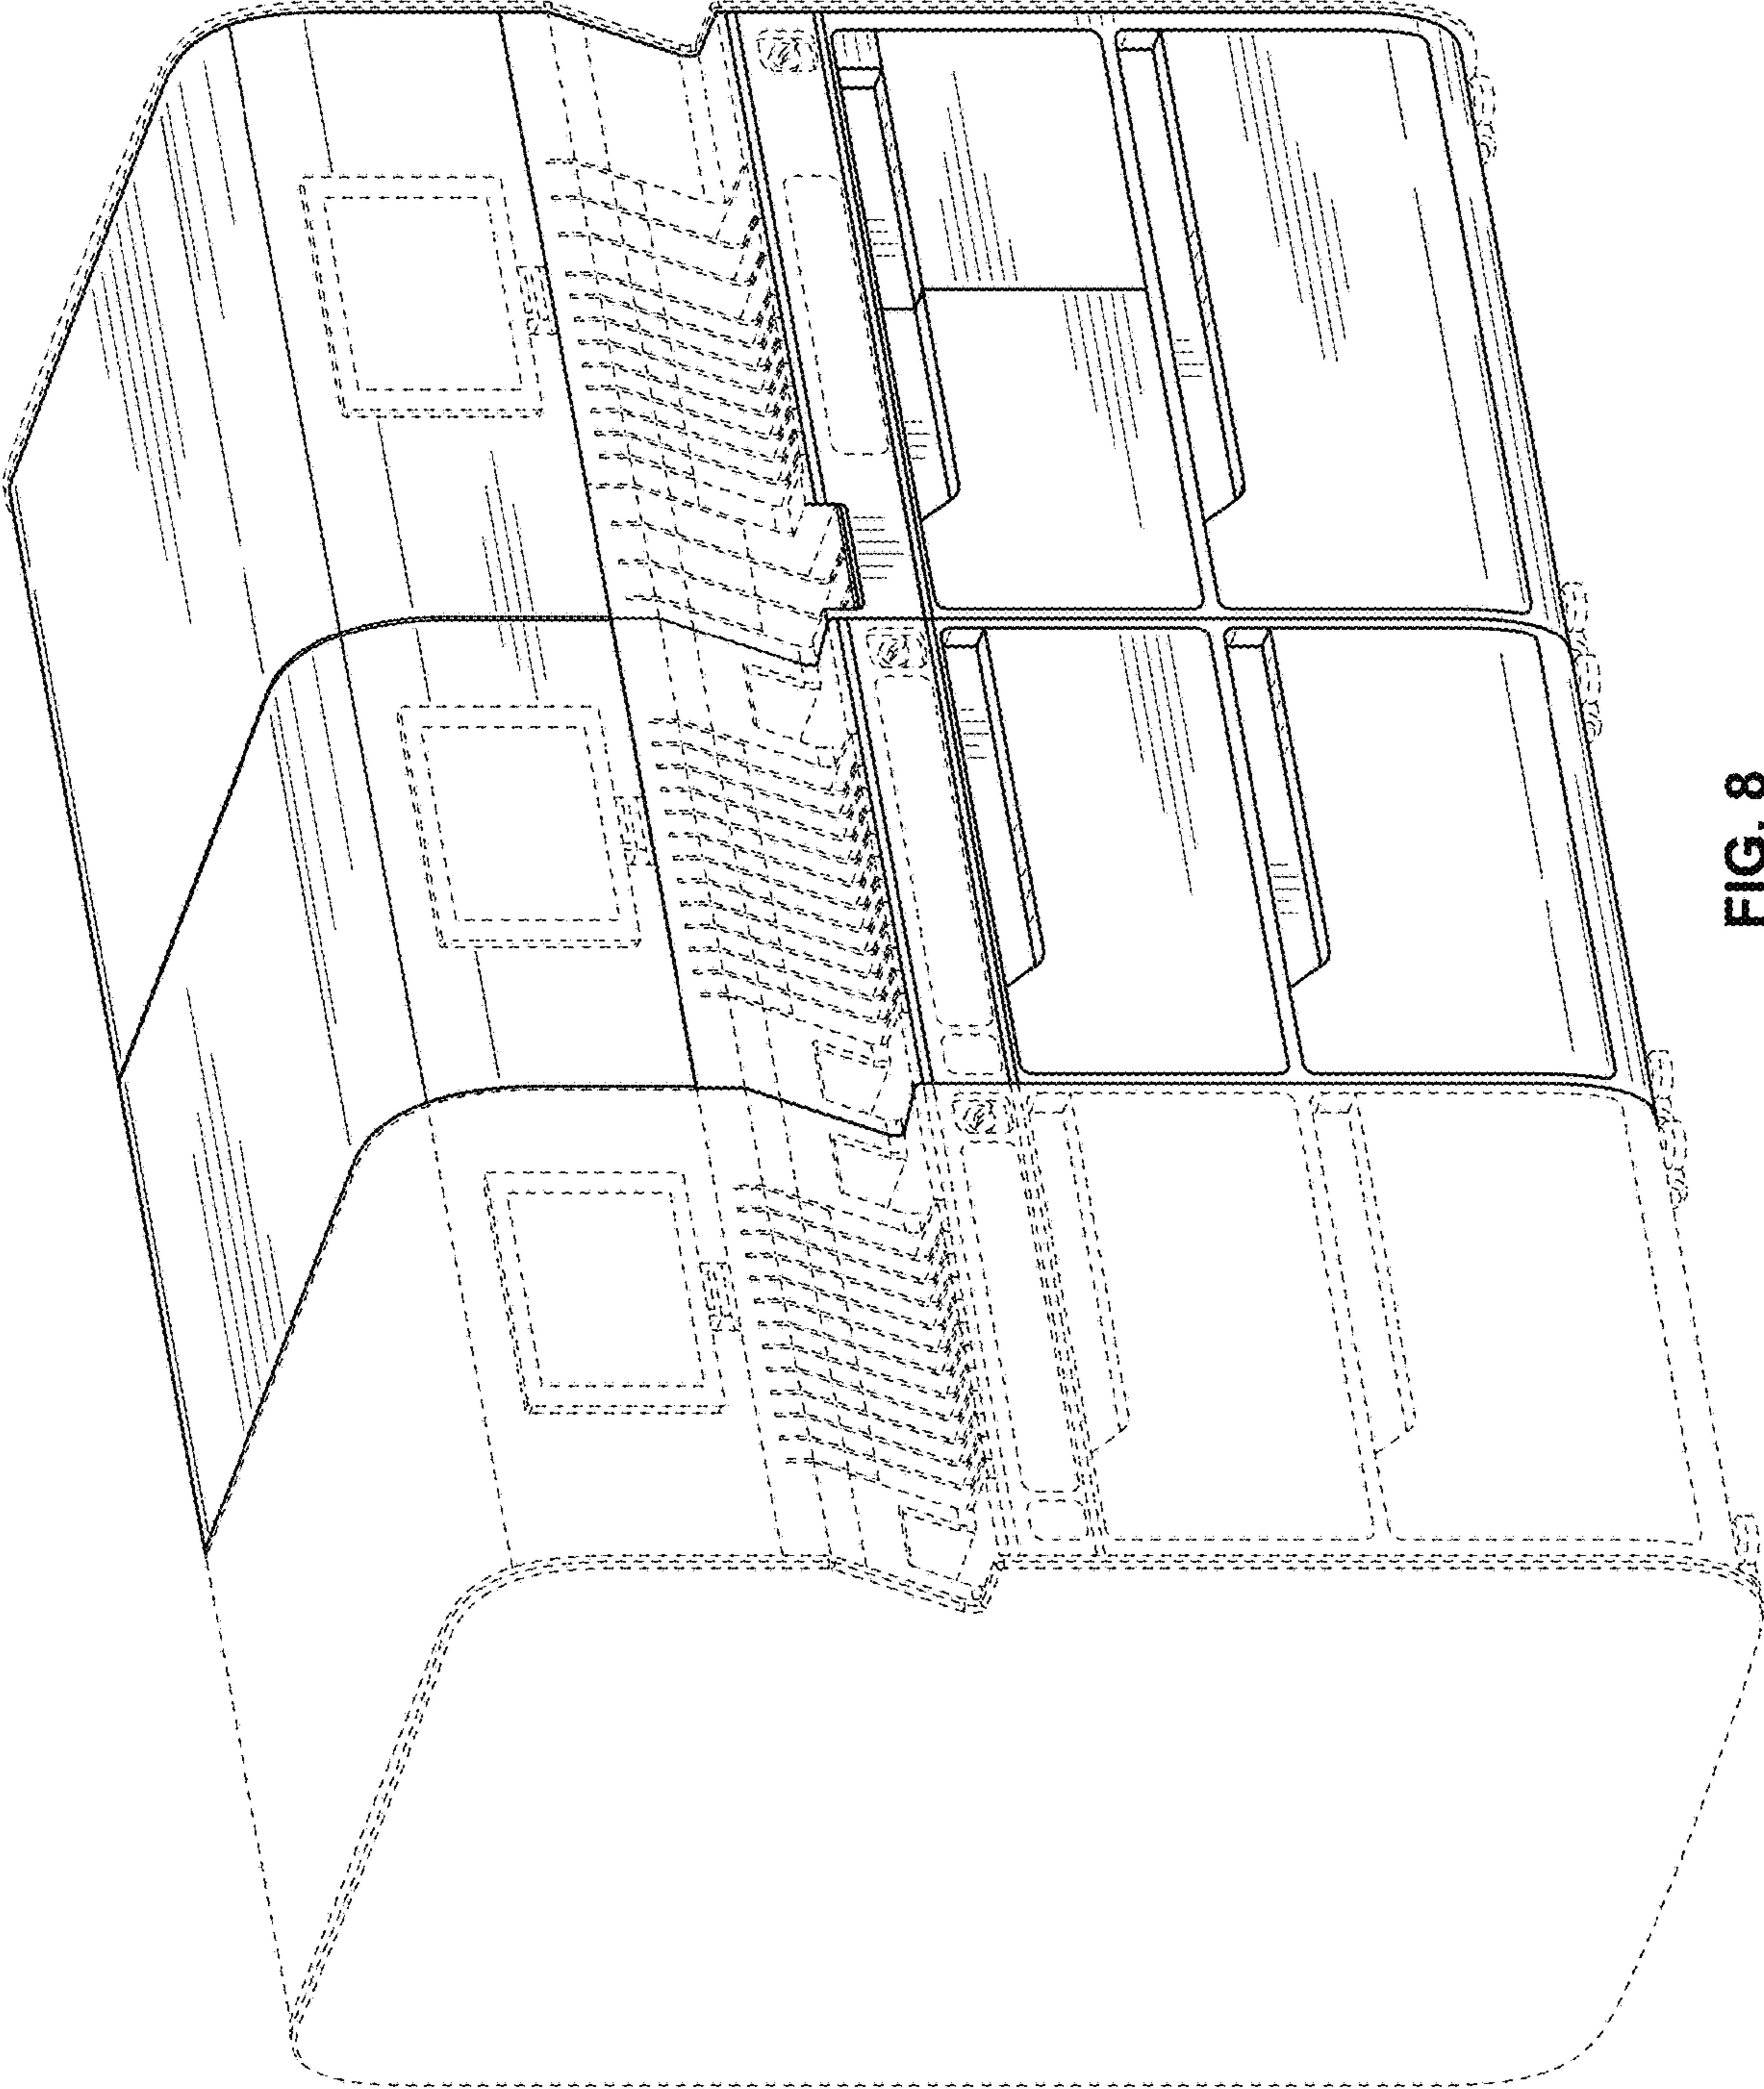


FIG. 8

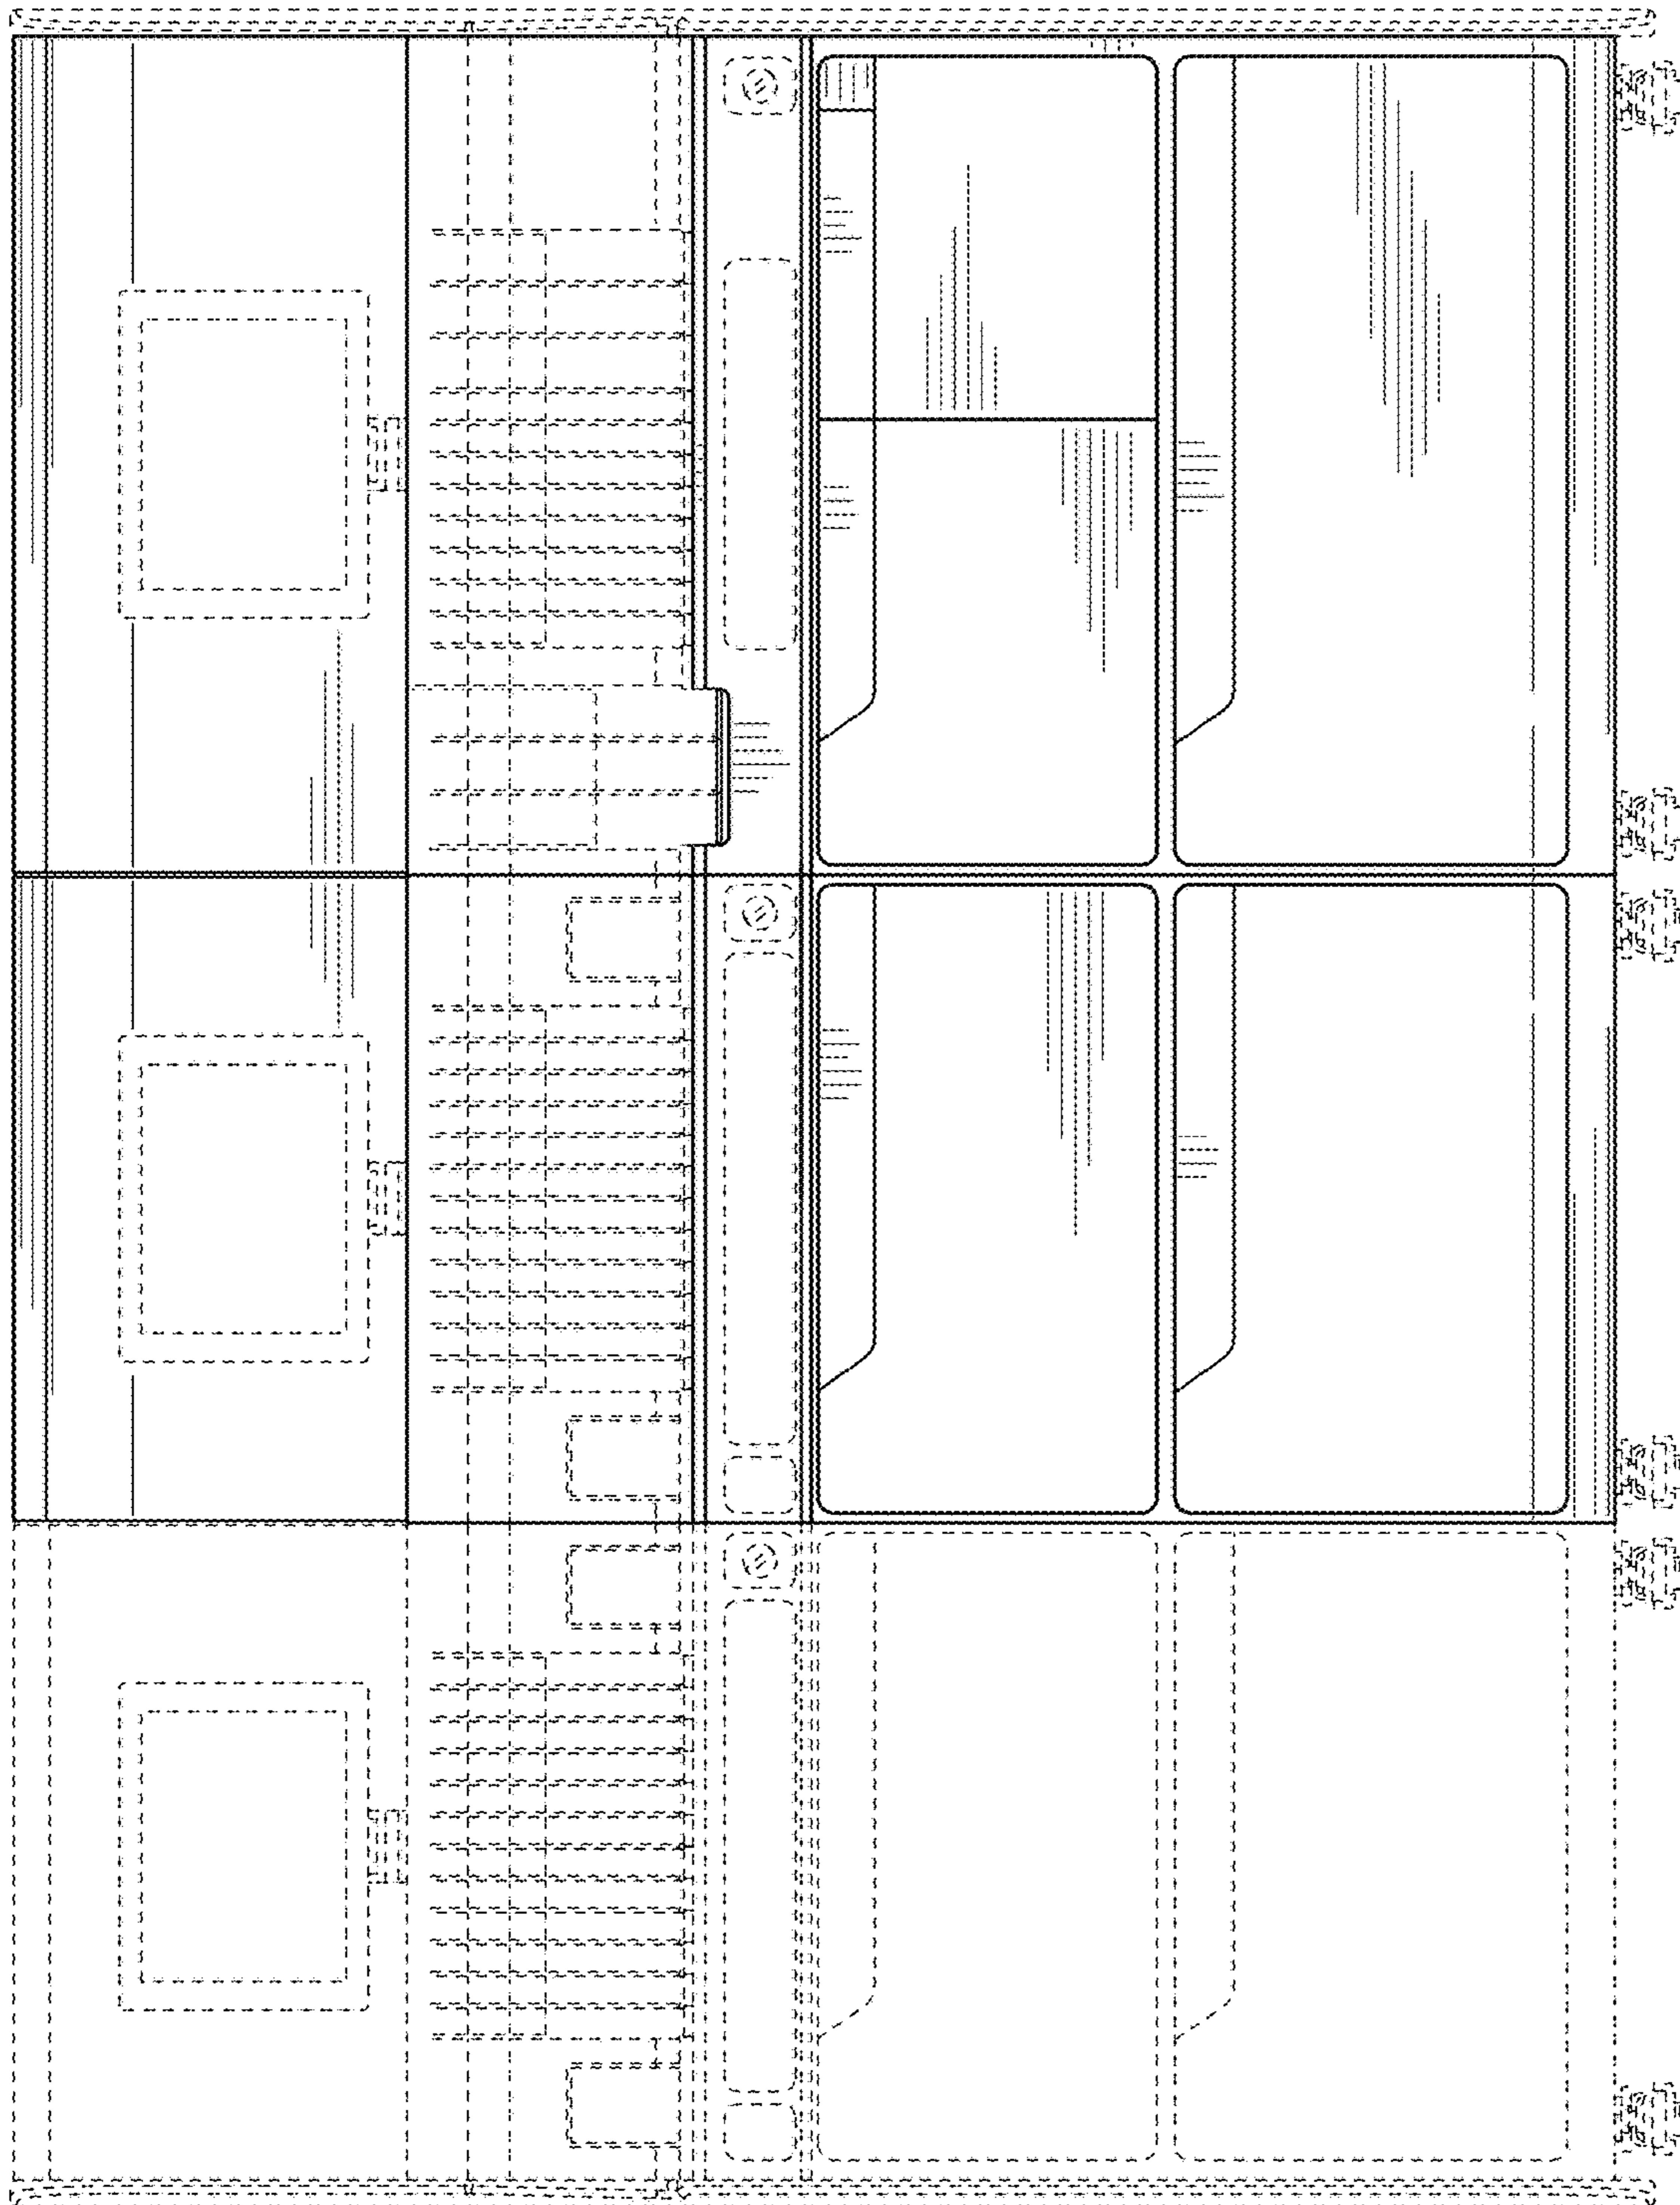


FIG. 9

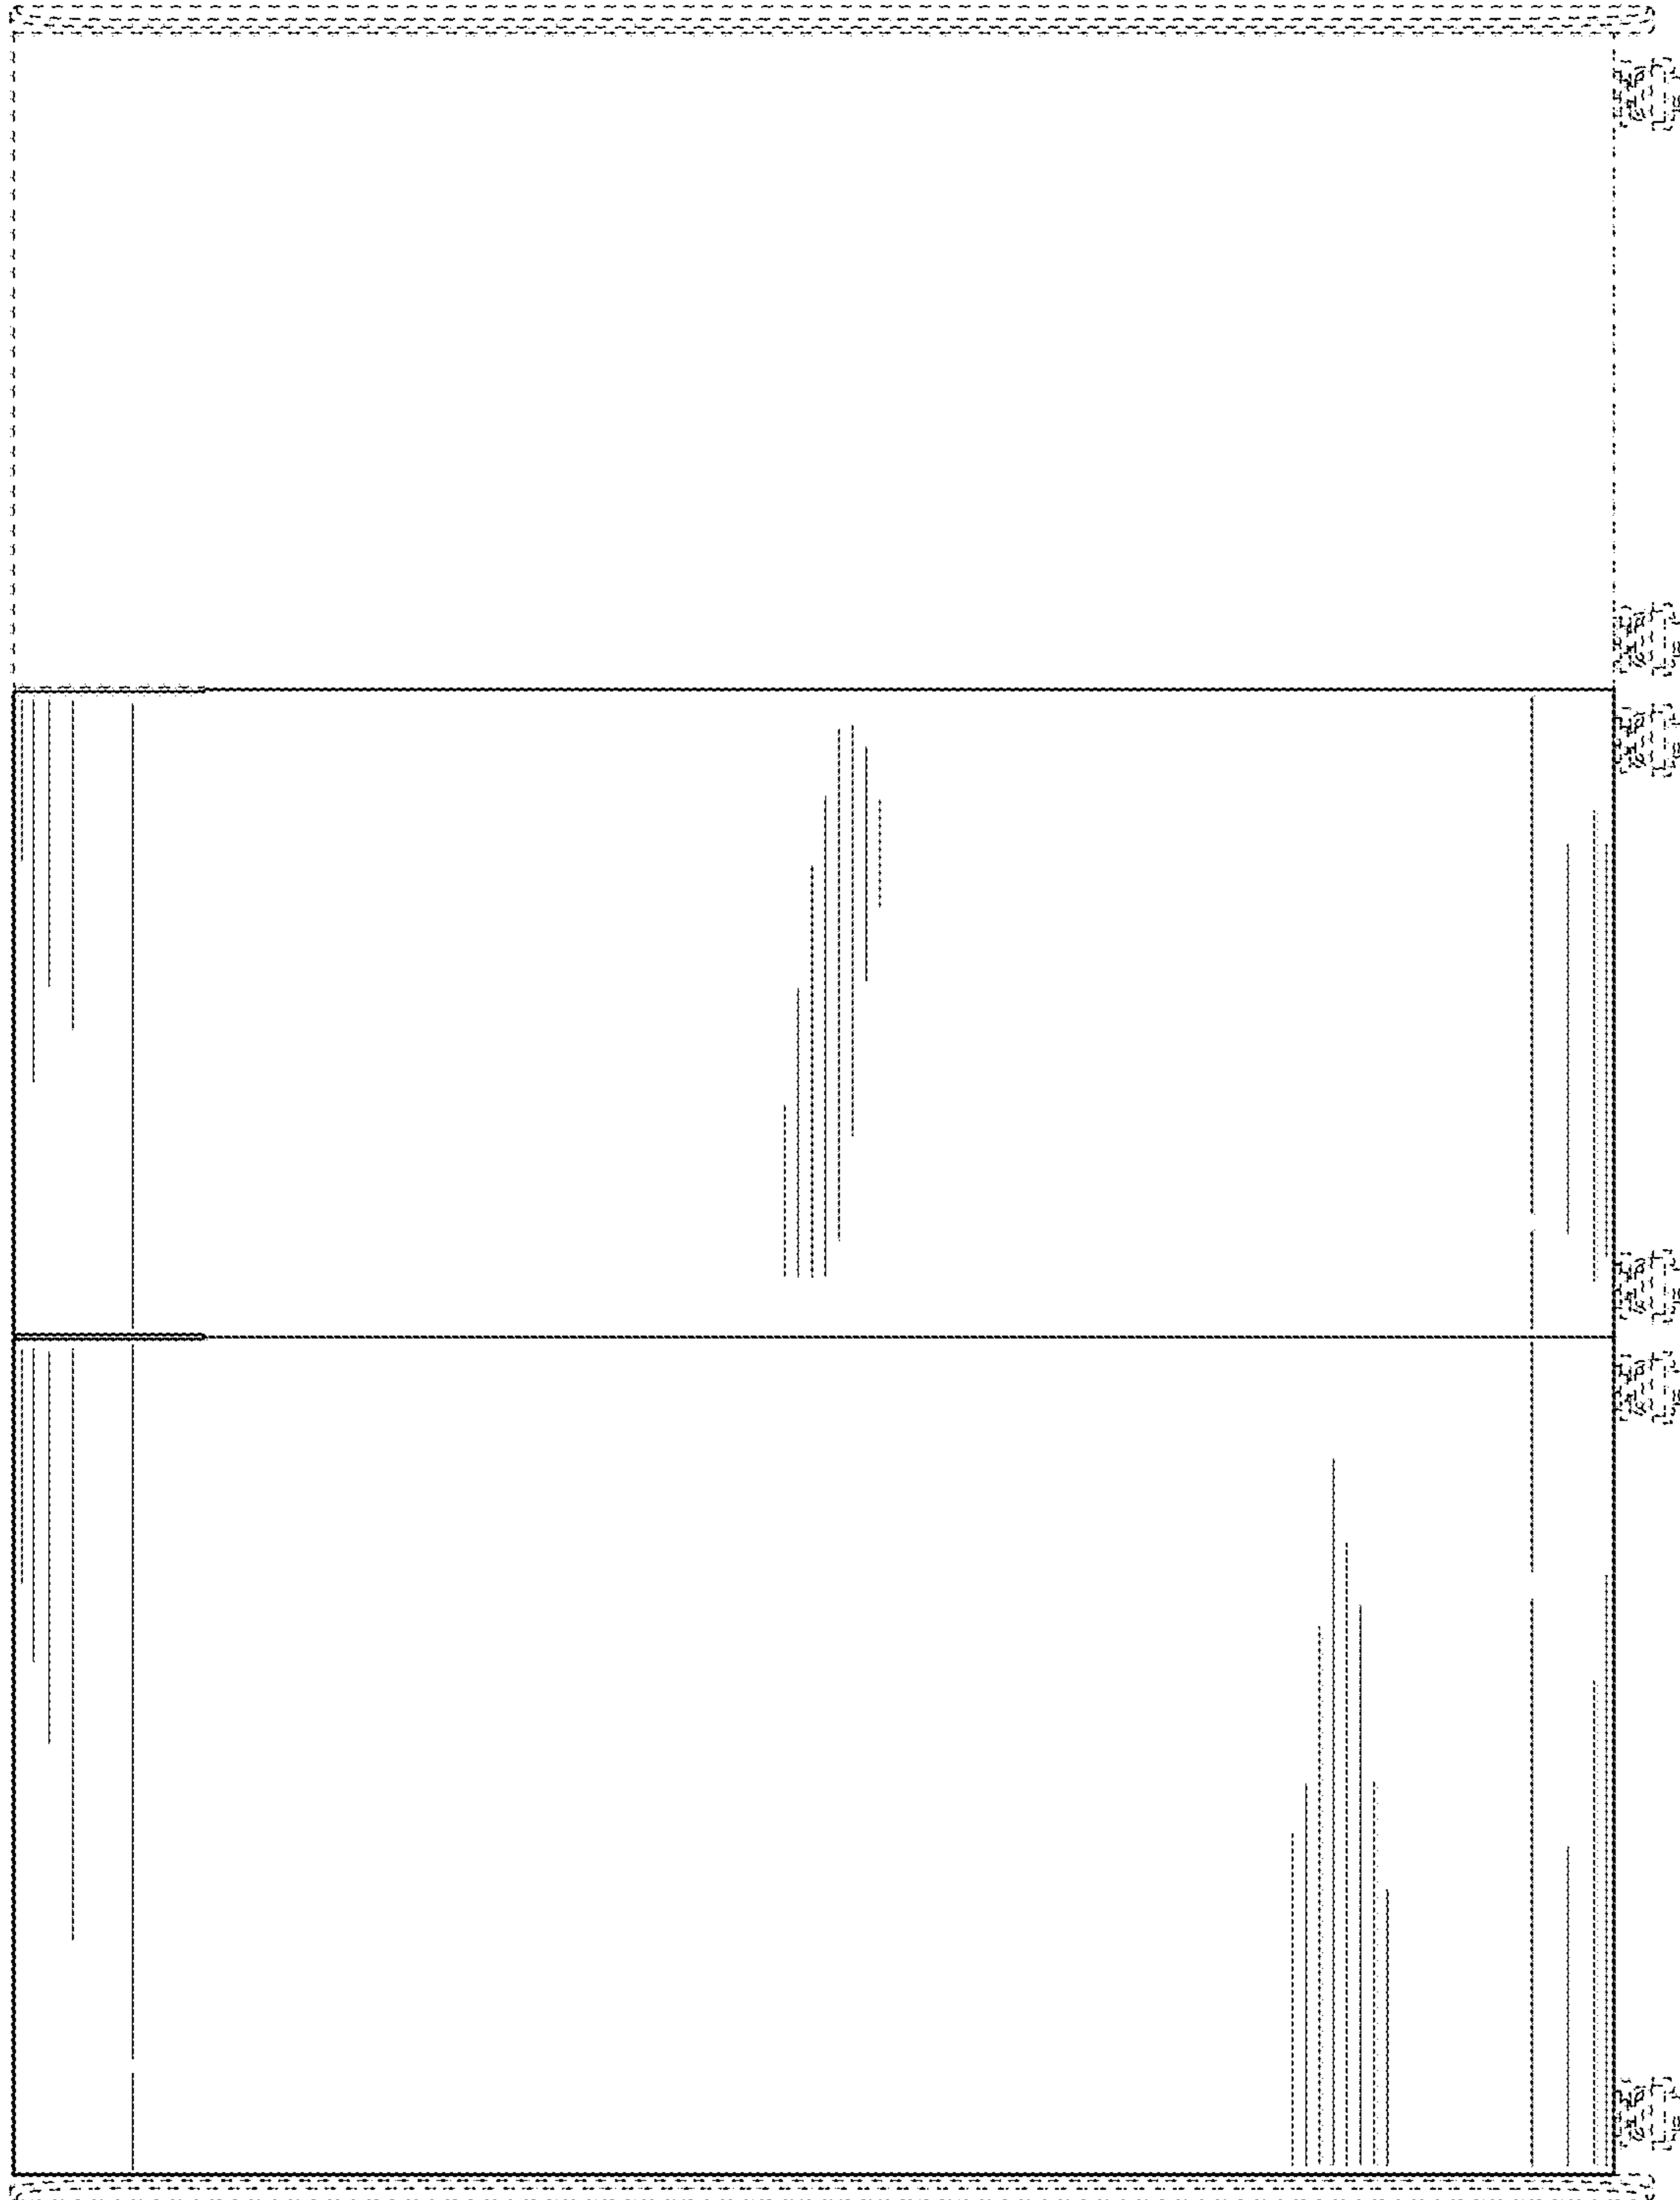


FIG. 10

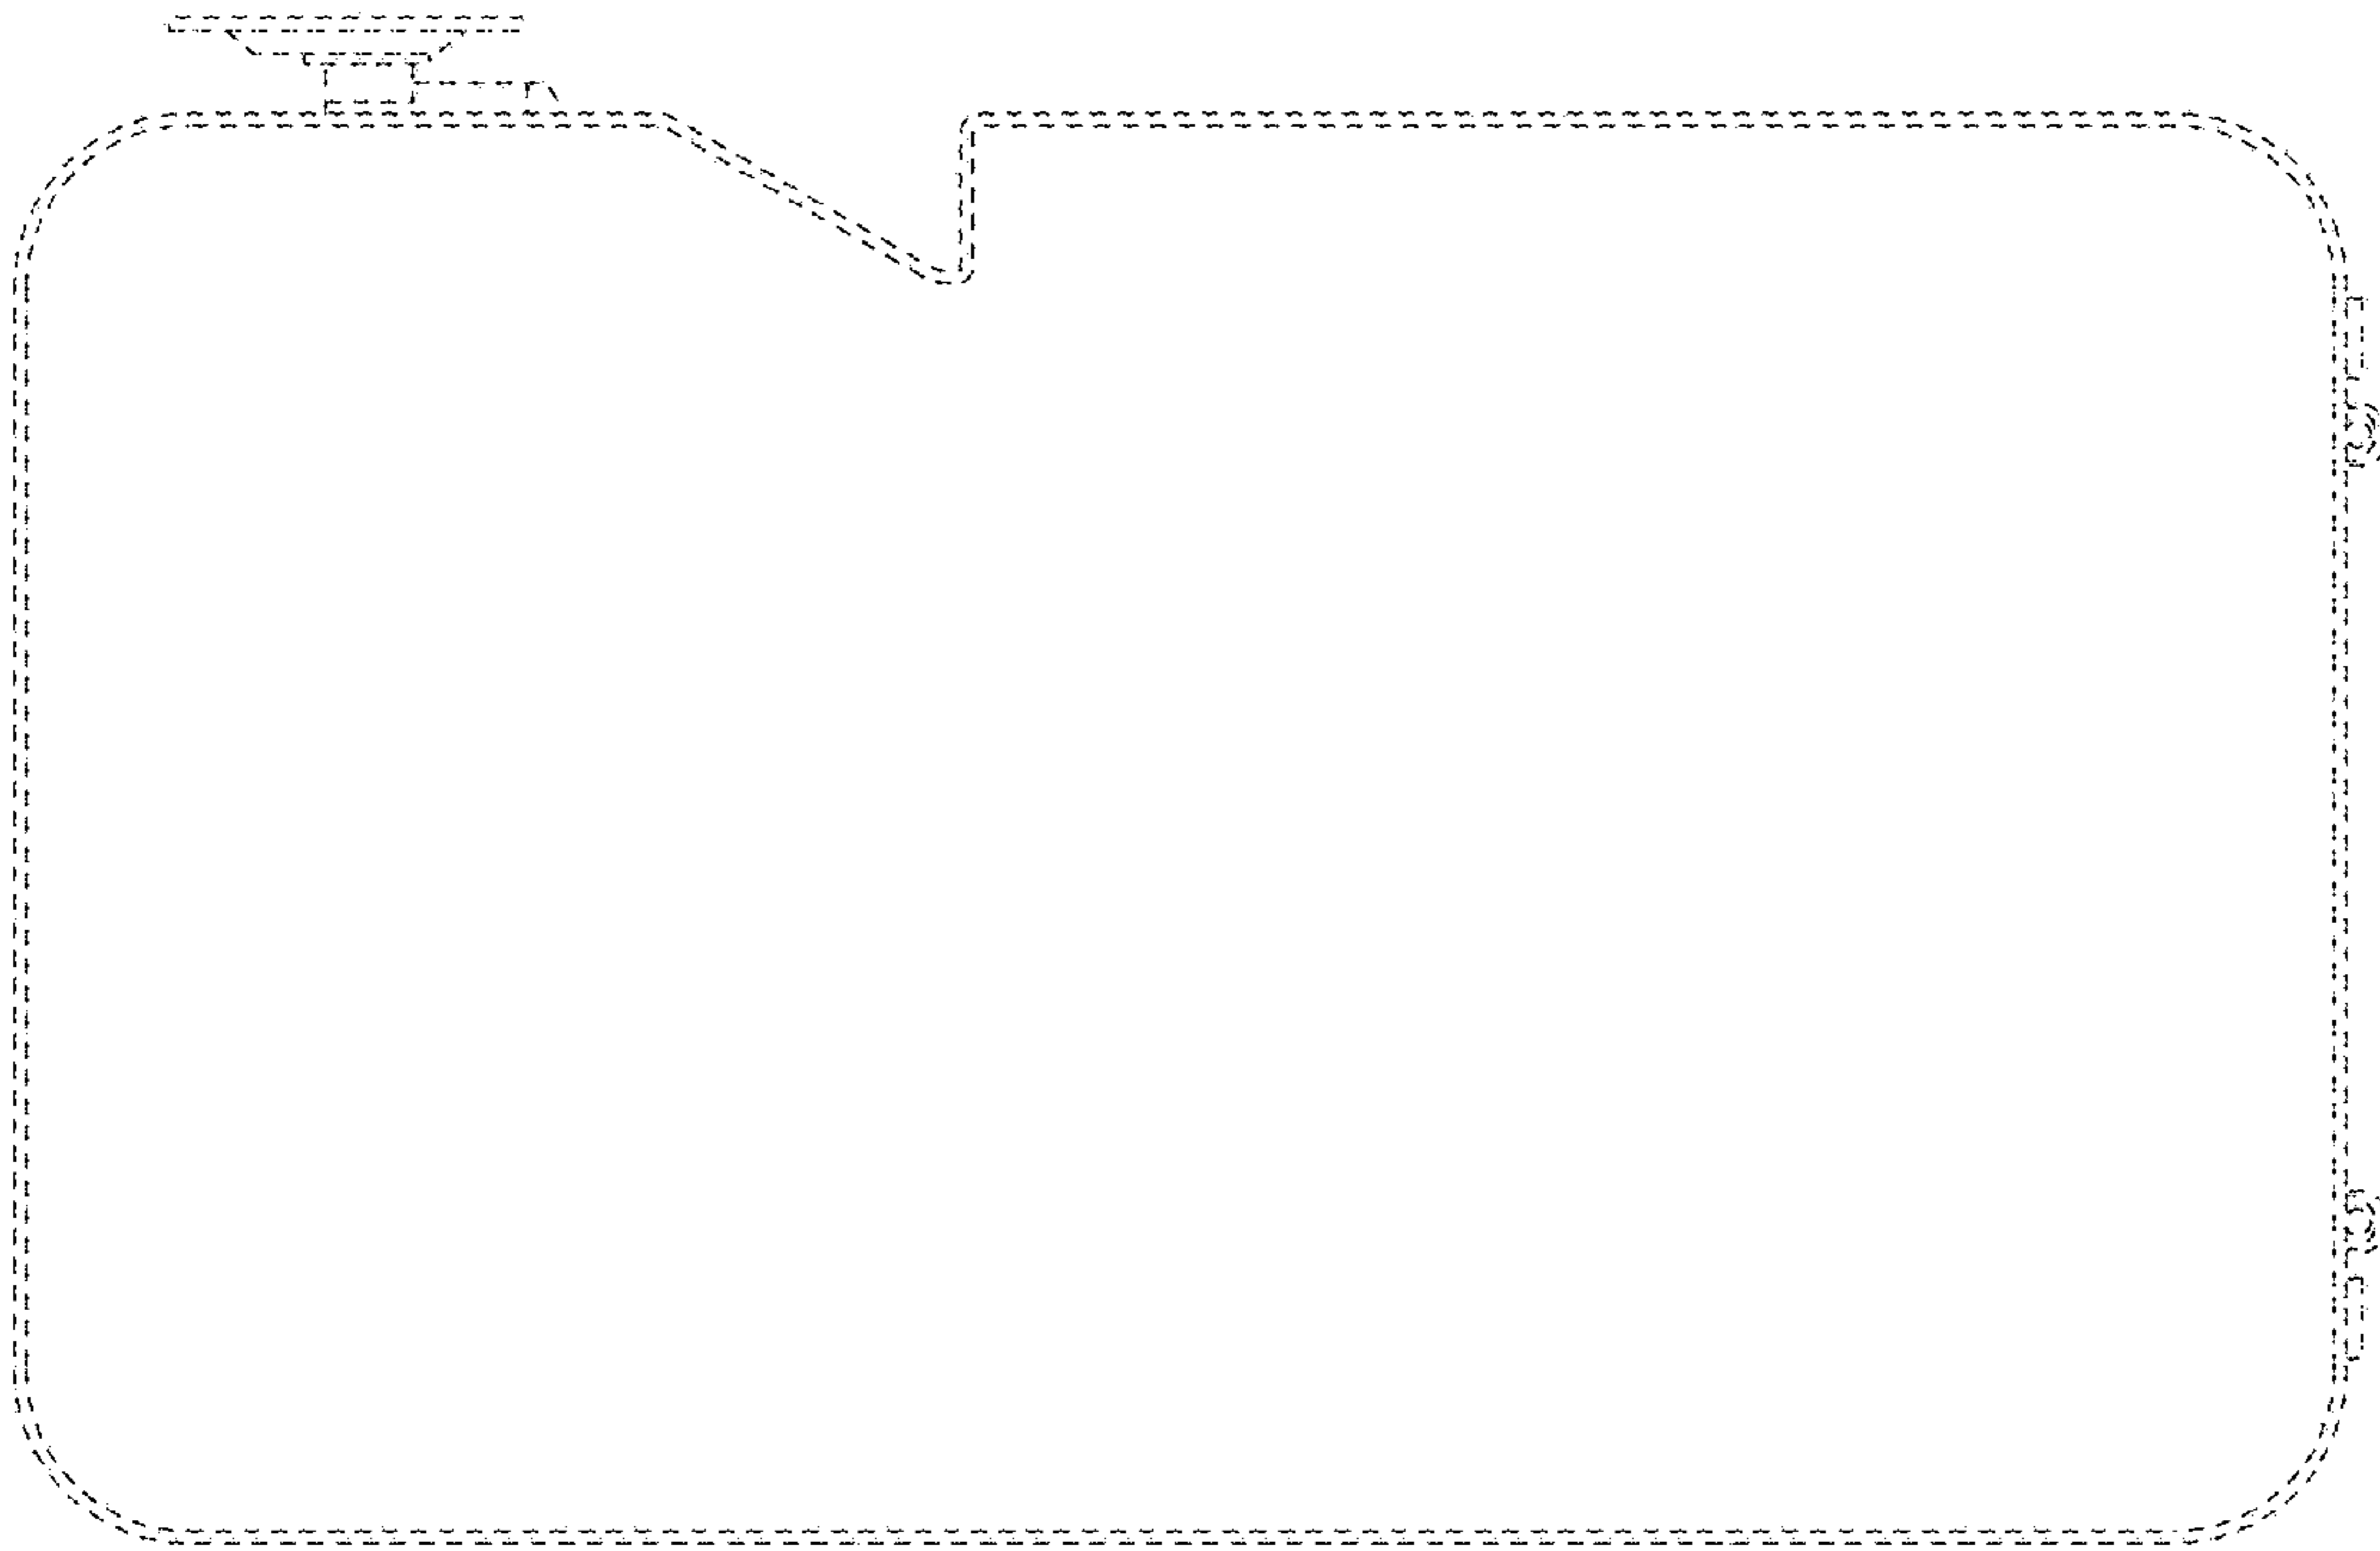


FIG. 12

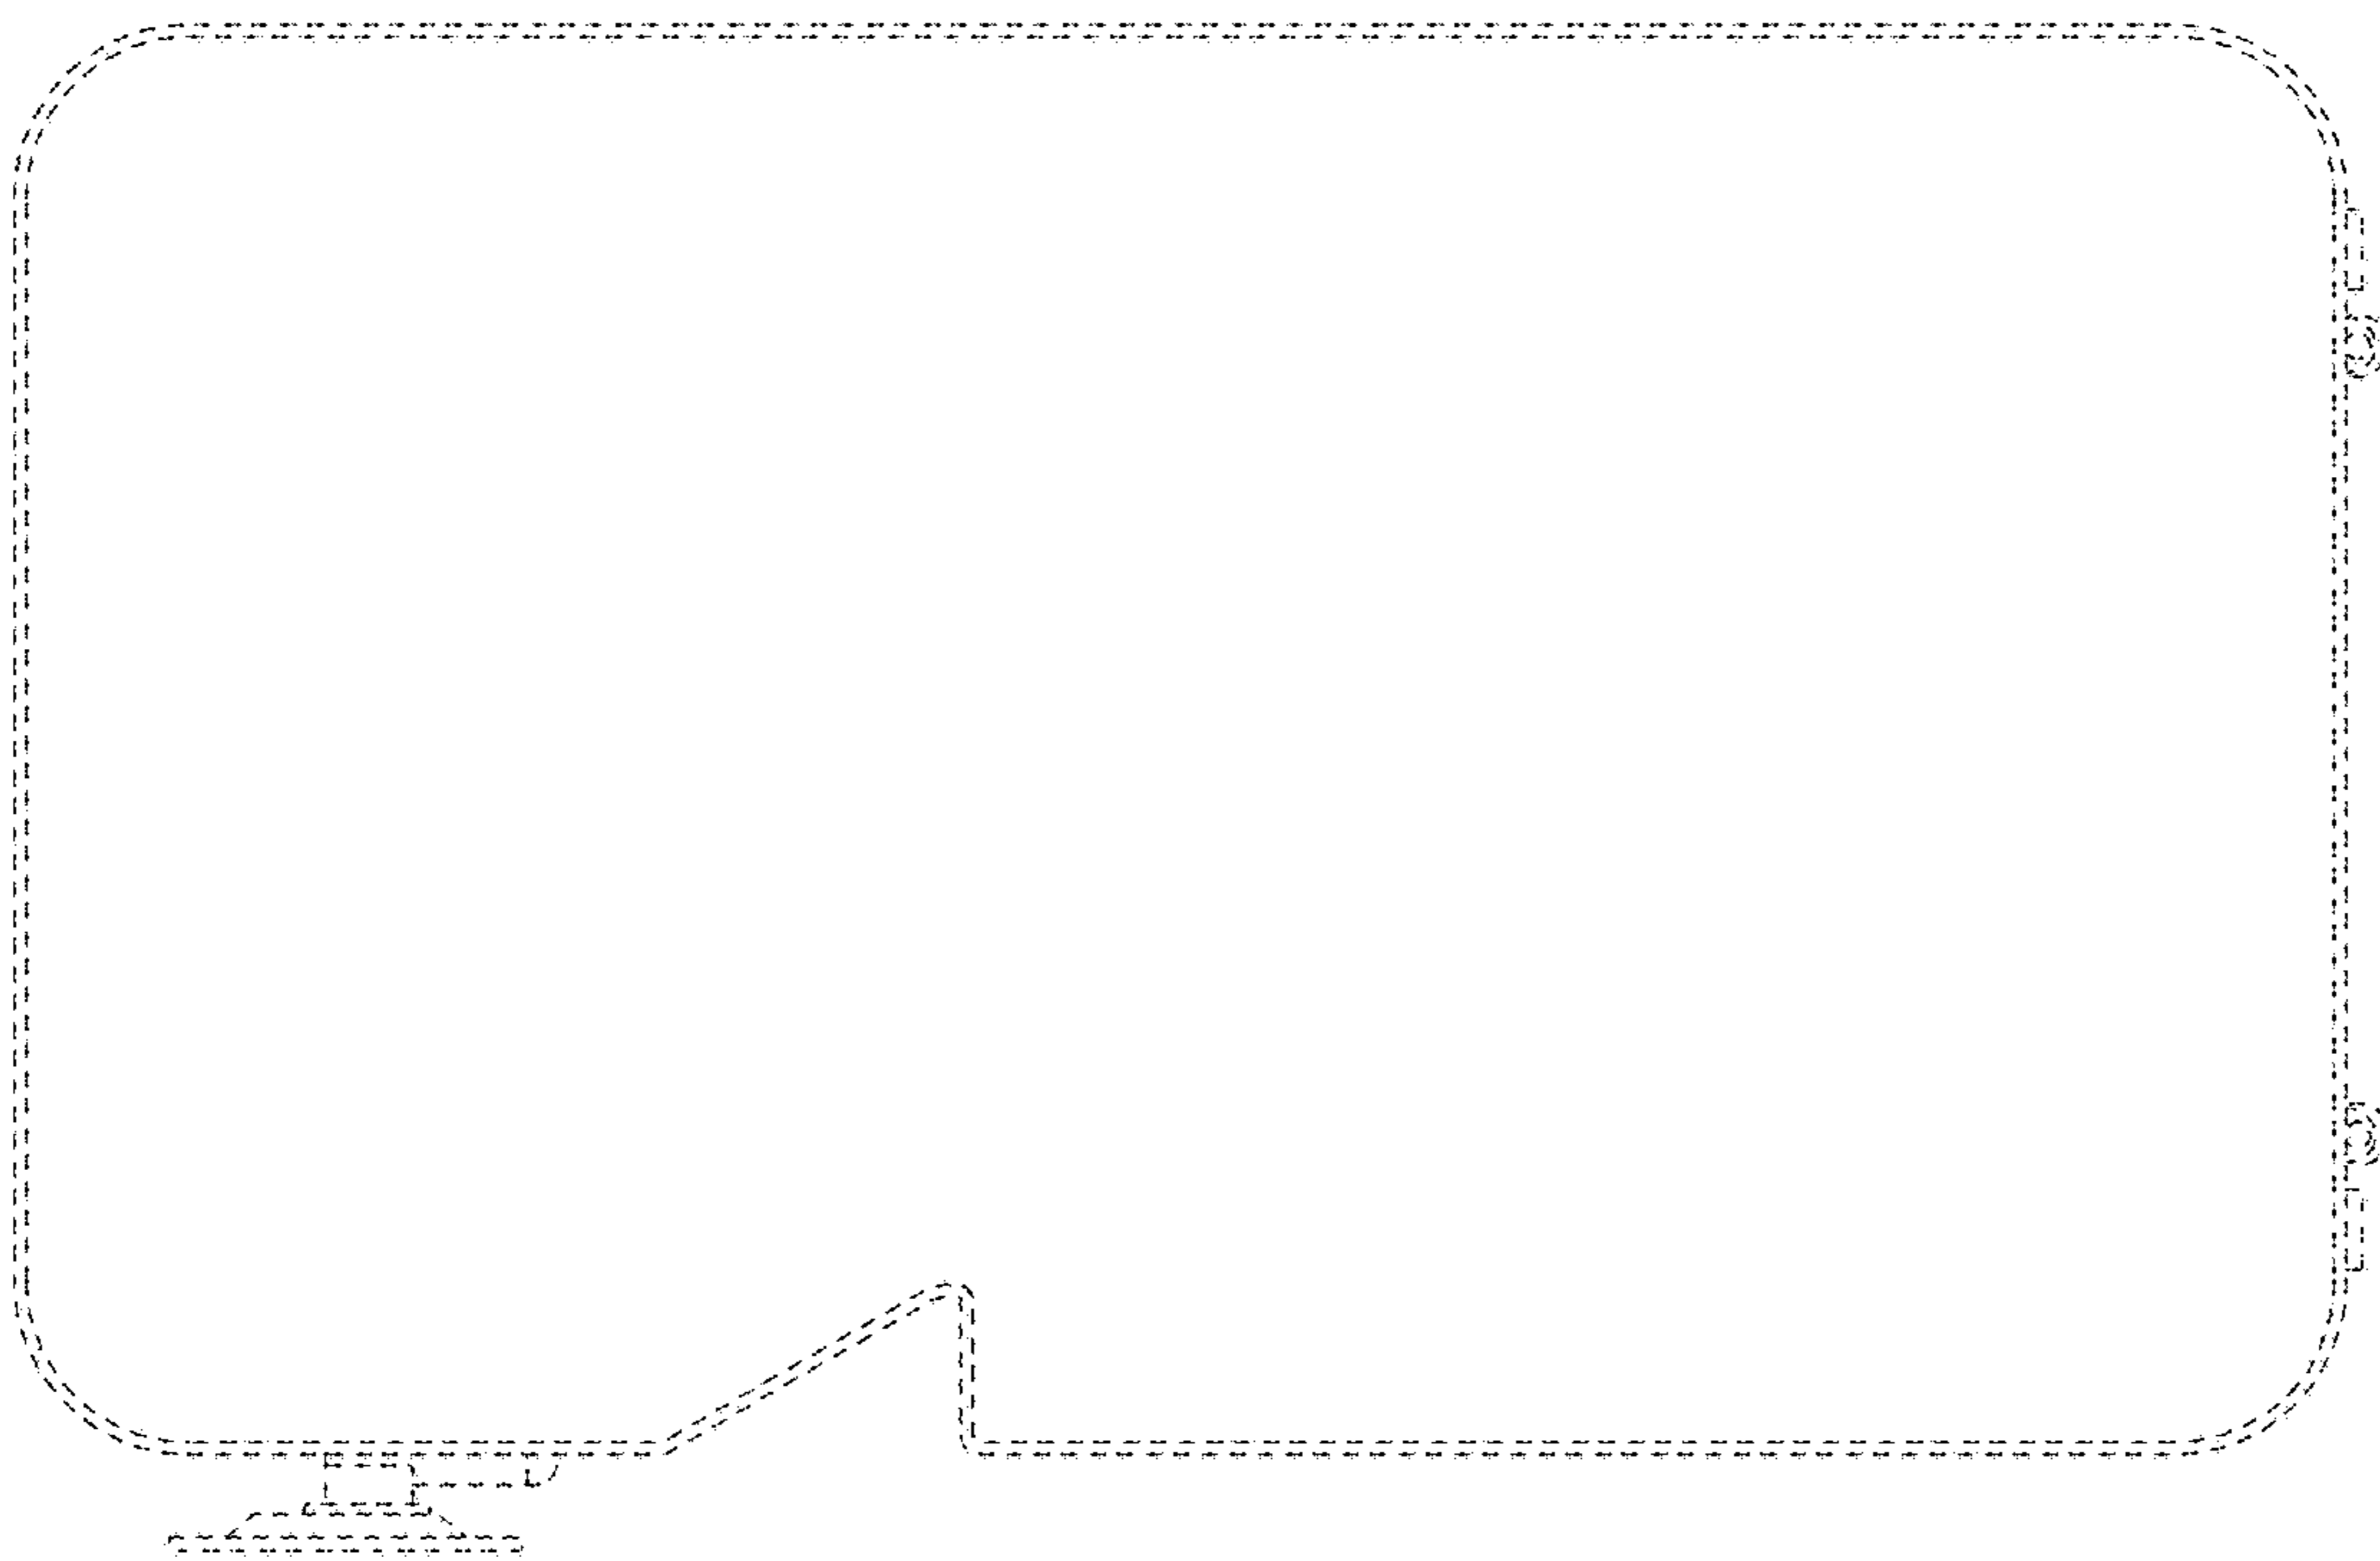


FIG. 11

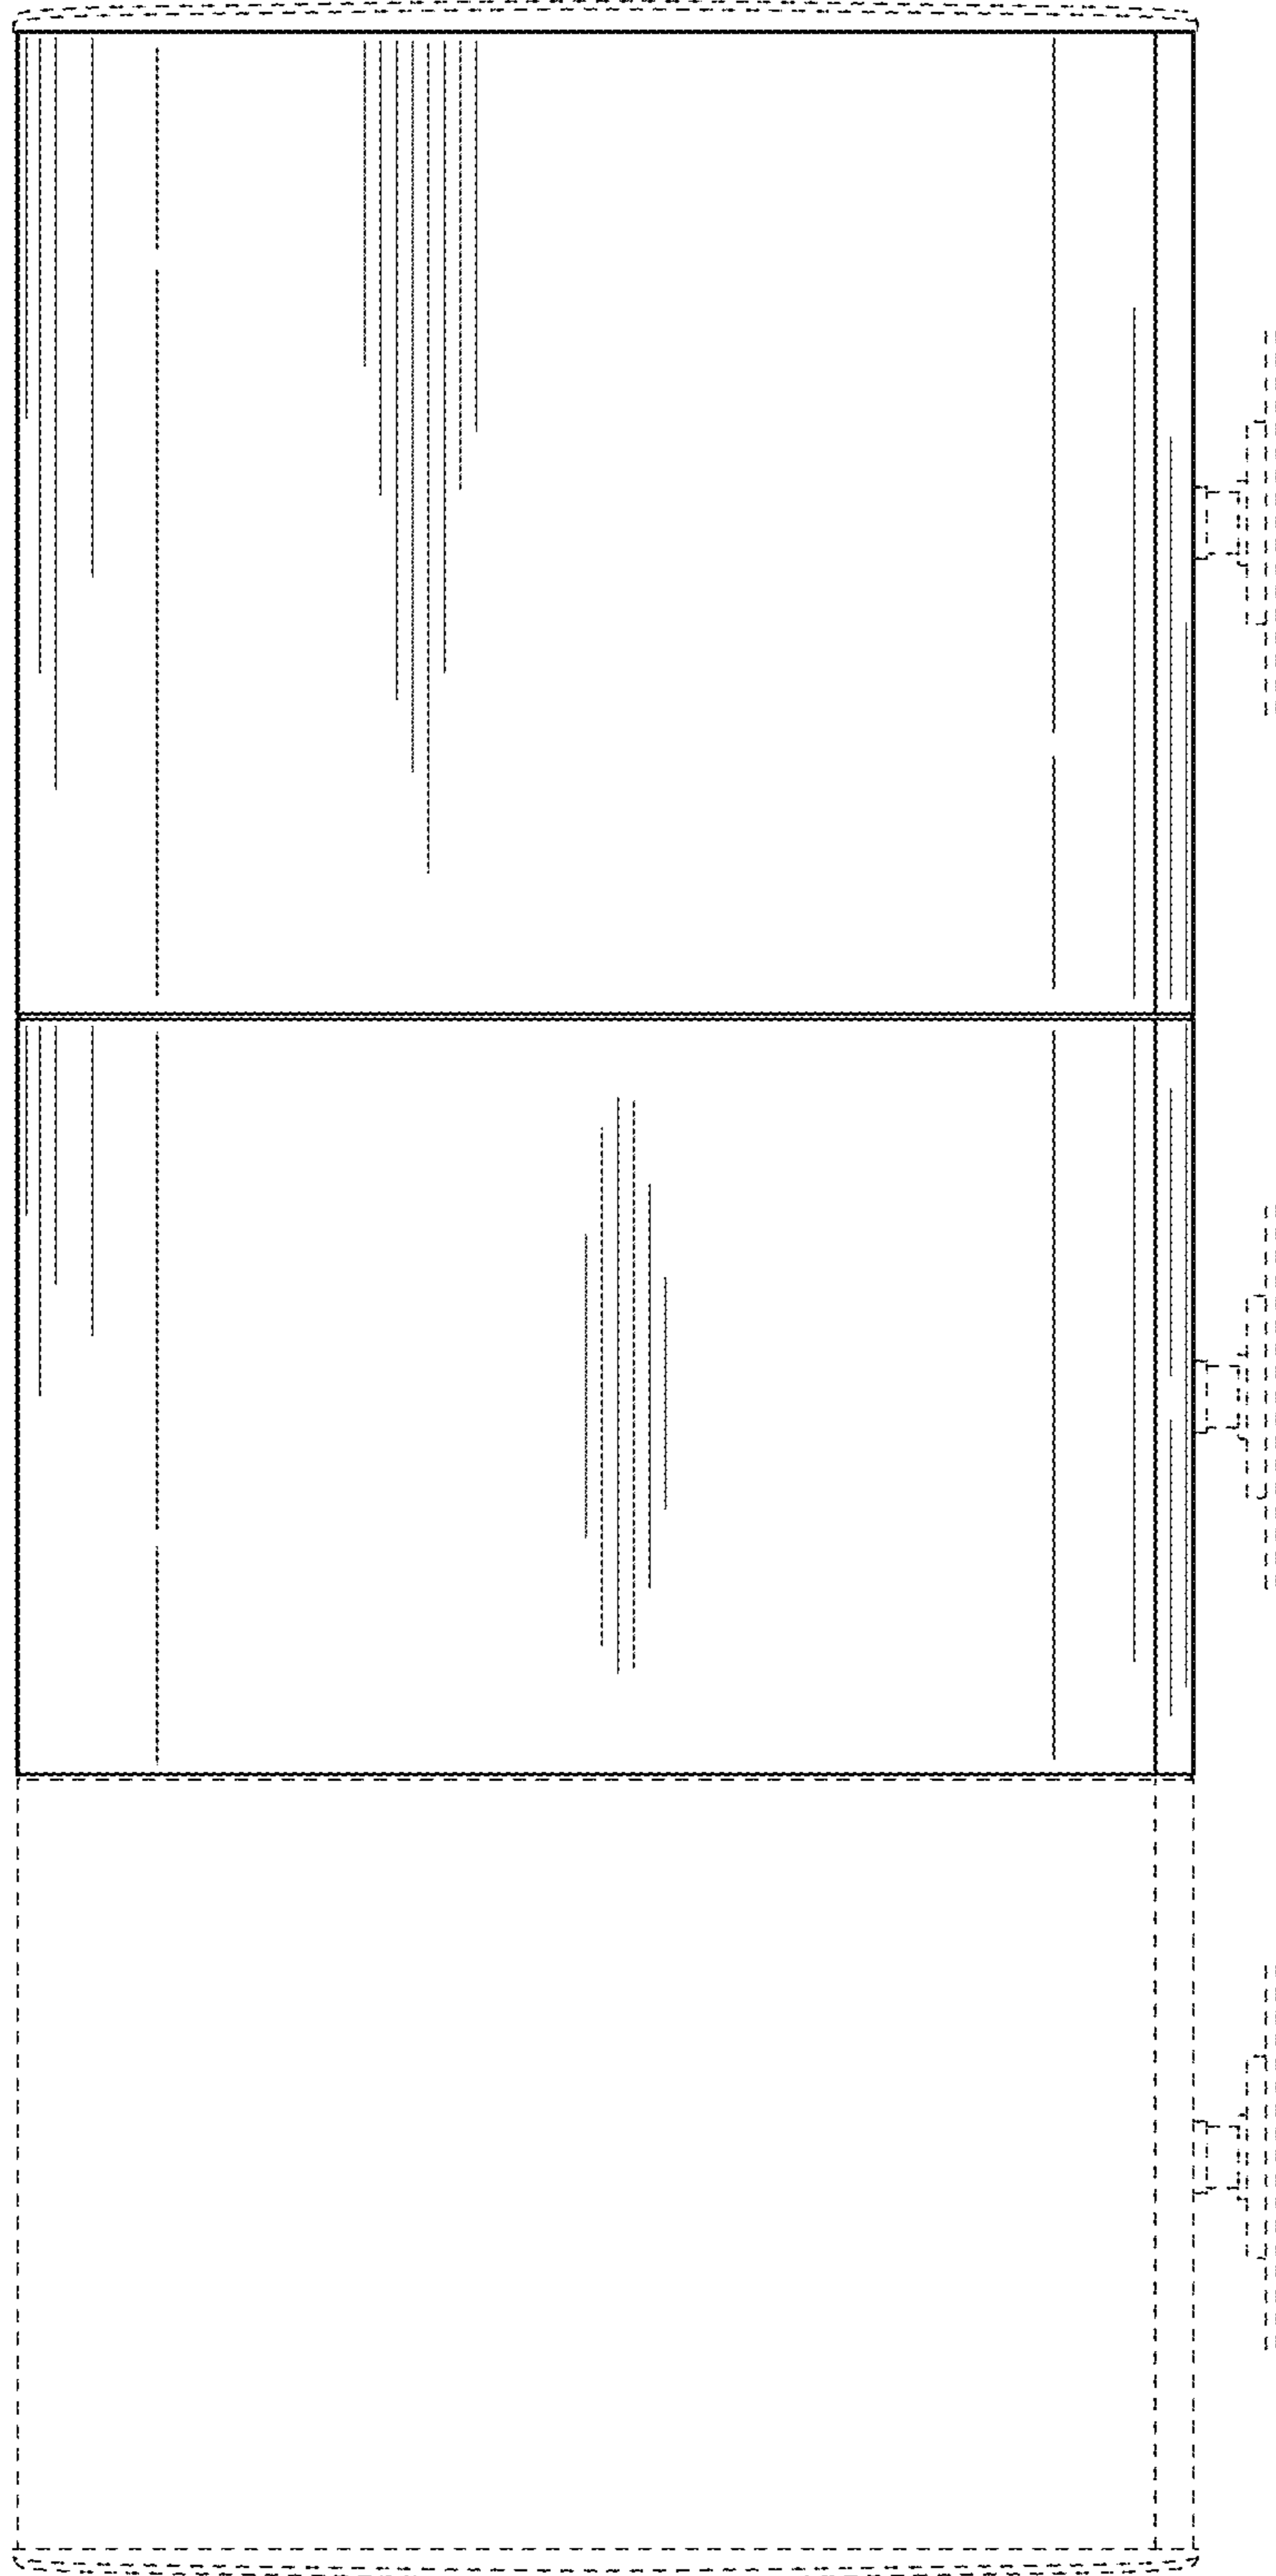


FIG. 13

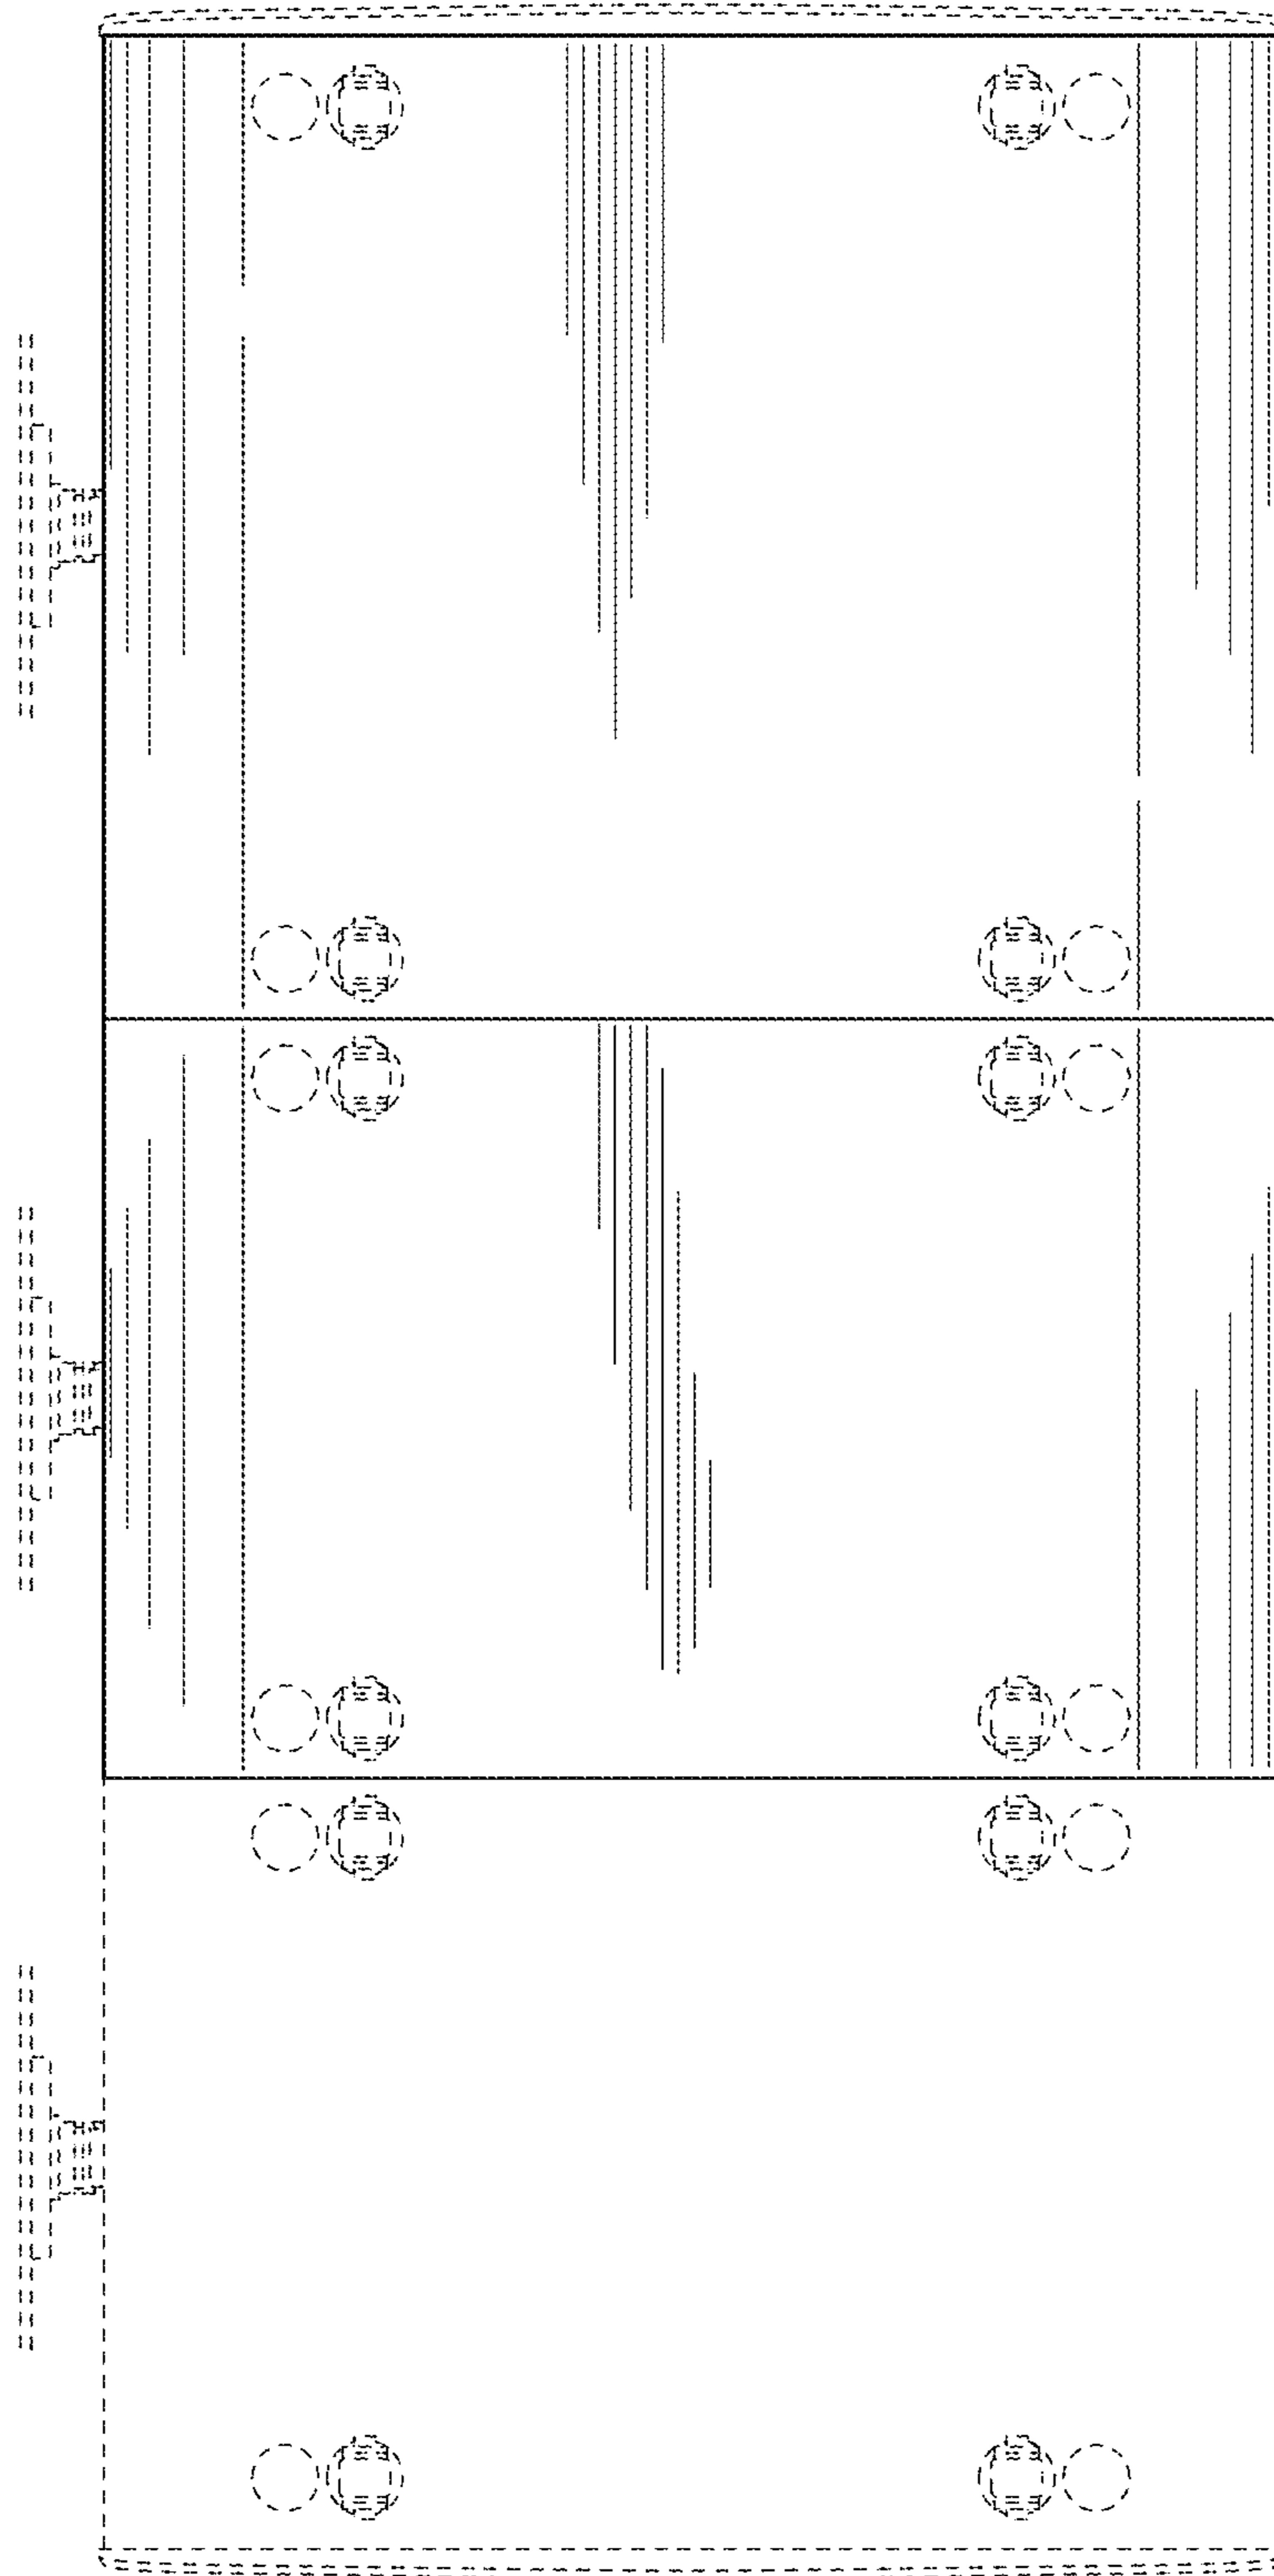


FIG. 14