



US00D877164S

(12) **United States Design Patent** (10) **Patent No.:** **US D877,164 S**
Dieken et al. (45) **Date of Patent:** **** Mar. 3, 2020**

- (54) **DISPLAY SCREEN OR PORTION THEREOF WITH A GRAPHICAL USER INTERFACE** D593,109 S 5/2009 Danton
D752,621 S * 3/2016 Cojuangco D14/486
D778,928 S 2/2017 Bertnick et al.
D780,190 S 2/2017 Kothe et al.
(71) Applicant: **Inspire Medical Systems, Inc.**, Maple Grove, MN (US) D808,408 S * 1/2018 Bombolowsky D14/486
D808,996 S * 1/2018 Ambielli B33Y 40/00 D14/486
(72) Inventors: **David Todd Dieken**, Minneapolis, MN (US); **Maria Isabel Ancona**, Boston, MA (US); **John Rondoni**, Plymouth, MN (US) D813,893 S 3/2018 Tuthill et al.
D820,290 S * 6/2018 Laing D14/486
D832,865 S * 11/2018 Dieken D14/485
D840,422 S * 2/2019 Tuthill D14/486
D840,426 S * 2/2019 Dieken D14/486
(73) Assignee: **Inspire Medical Systems, Inc.**, Golden Valley, MN (US) 2010/0121707 A1 5/2010 Goeldi
2017/0201861 A1 7/2017 Freeman-Baer et al.

* cited by examiner

- (**) Term: **15 Years**
(21) Appl. No.: **29/669,005**
(22) Filed: **Nov. 5, 2018**

Primary Examiner — Richelle G Shelton
(74) *Attorney, Agent, or Firm* — Dicke, Billig & Czaja, PLLC

Related U.S. Application Data

- (63) Continuation of application No. 29/617,334, filed on Sep. 13, 2017, now Pat. No. Des. 832,865.
(51) **LOC (12) Cl.** **14-04**
(52) **U.S. Cl.**
USPC **D14/485**
(58) **Field of Classification Search**
USPC D14/485-488
CPC G06F 3/0482; G06F 16/248
See application file for complete search history.

(57) **CLAIM**

We claim the ornamental design for a display screen or portion thereof with a graphical user interface, as shown and described.

DESCRIPTION


The FIGURE is a front view of a display screen or portion thereof with a graphical user interface showing our new design.
The outermost broken lines show a display screen or portion thereof and form no part of the claimed design. The remaining broken lines show elements of the graphical user interface that form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 6,381,556 B1 4/2002 Kazemi et al.
D591,304 S 4/2009 Banks et al.

1 Claim, 1 Drawing Sheet

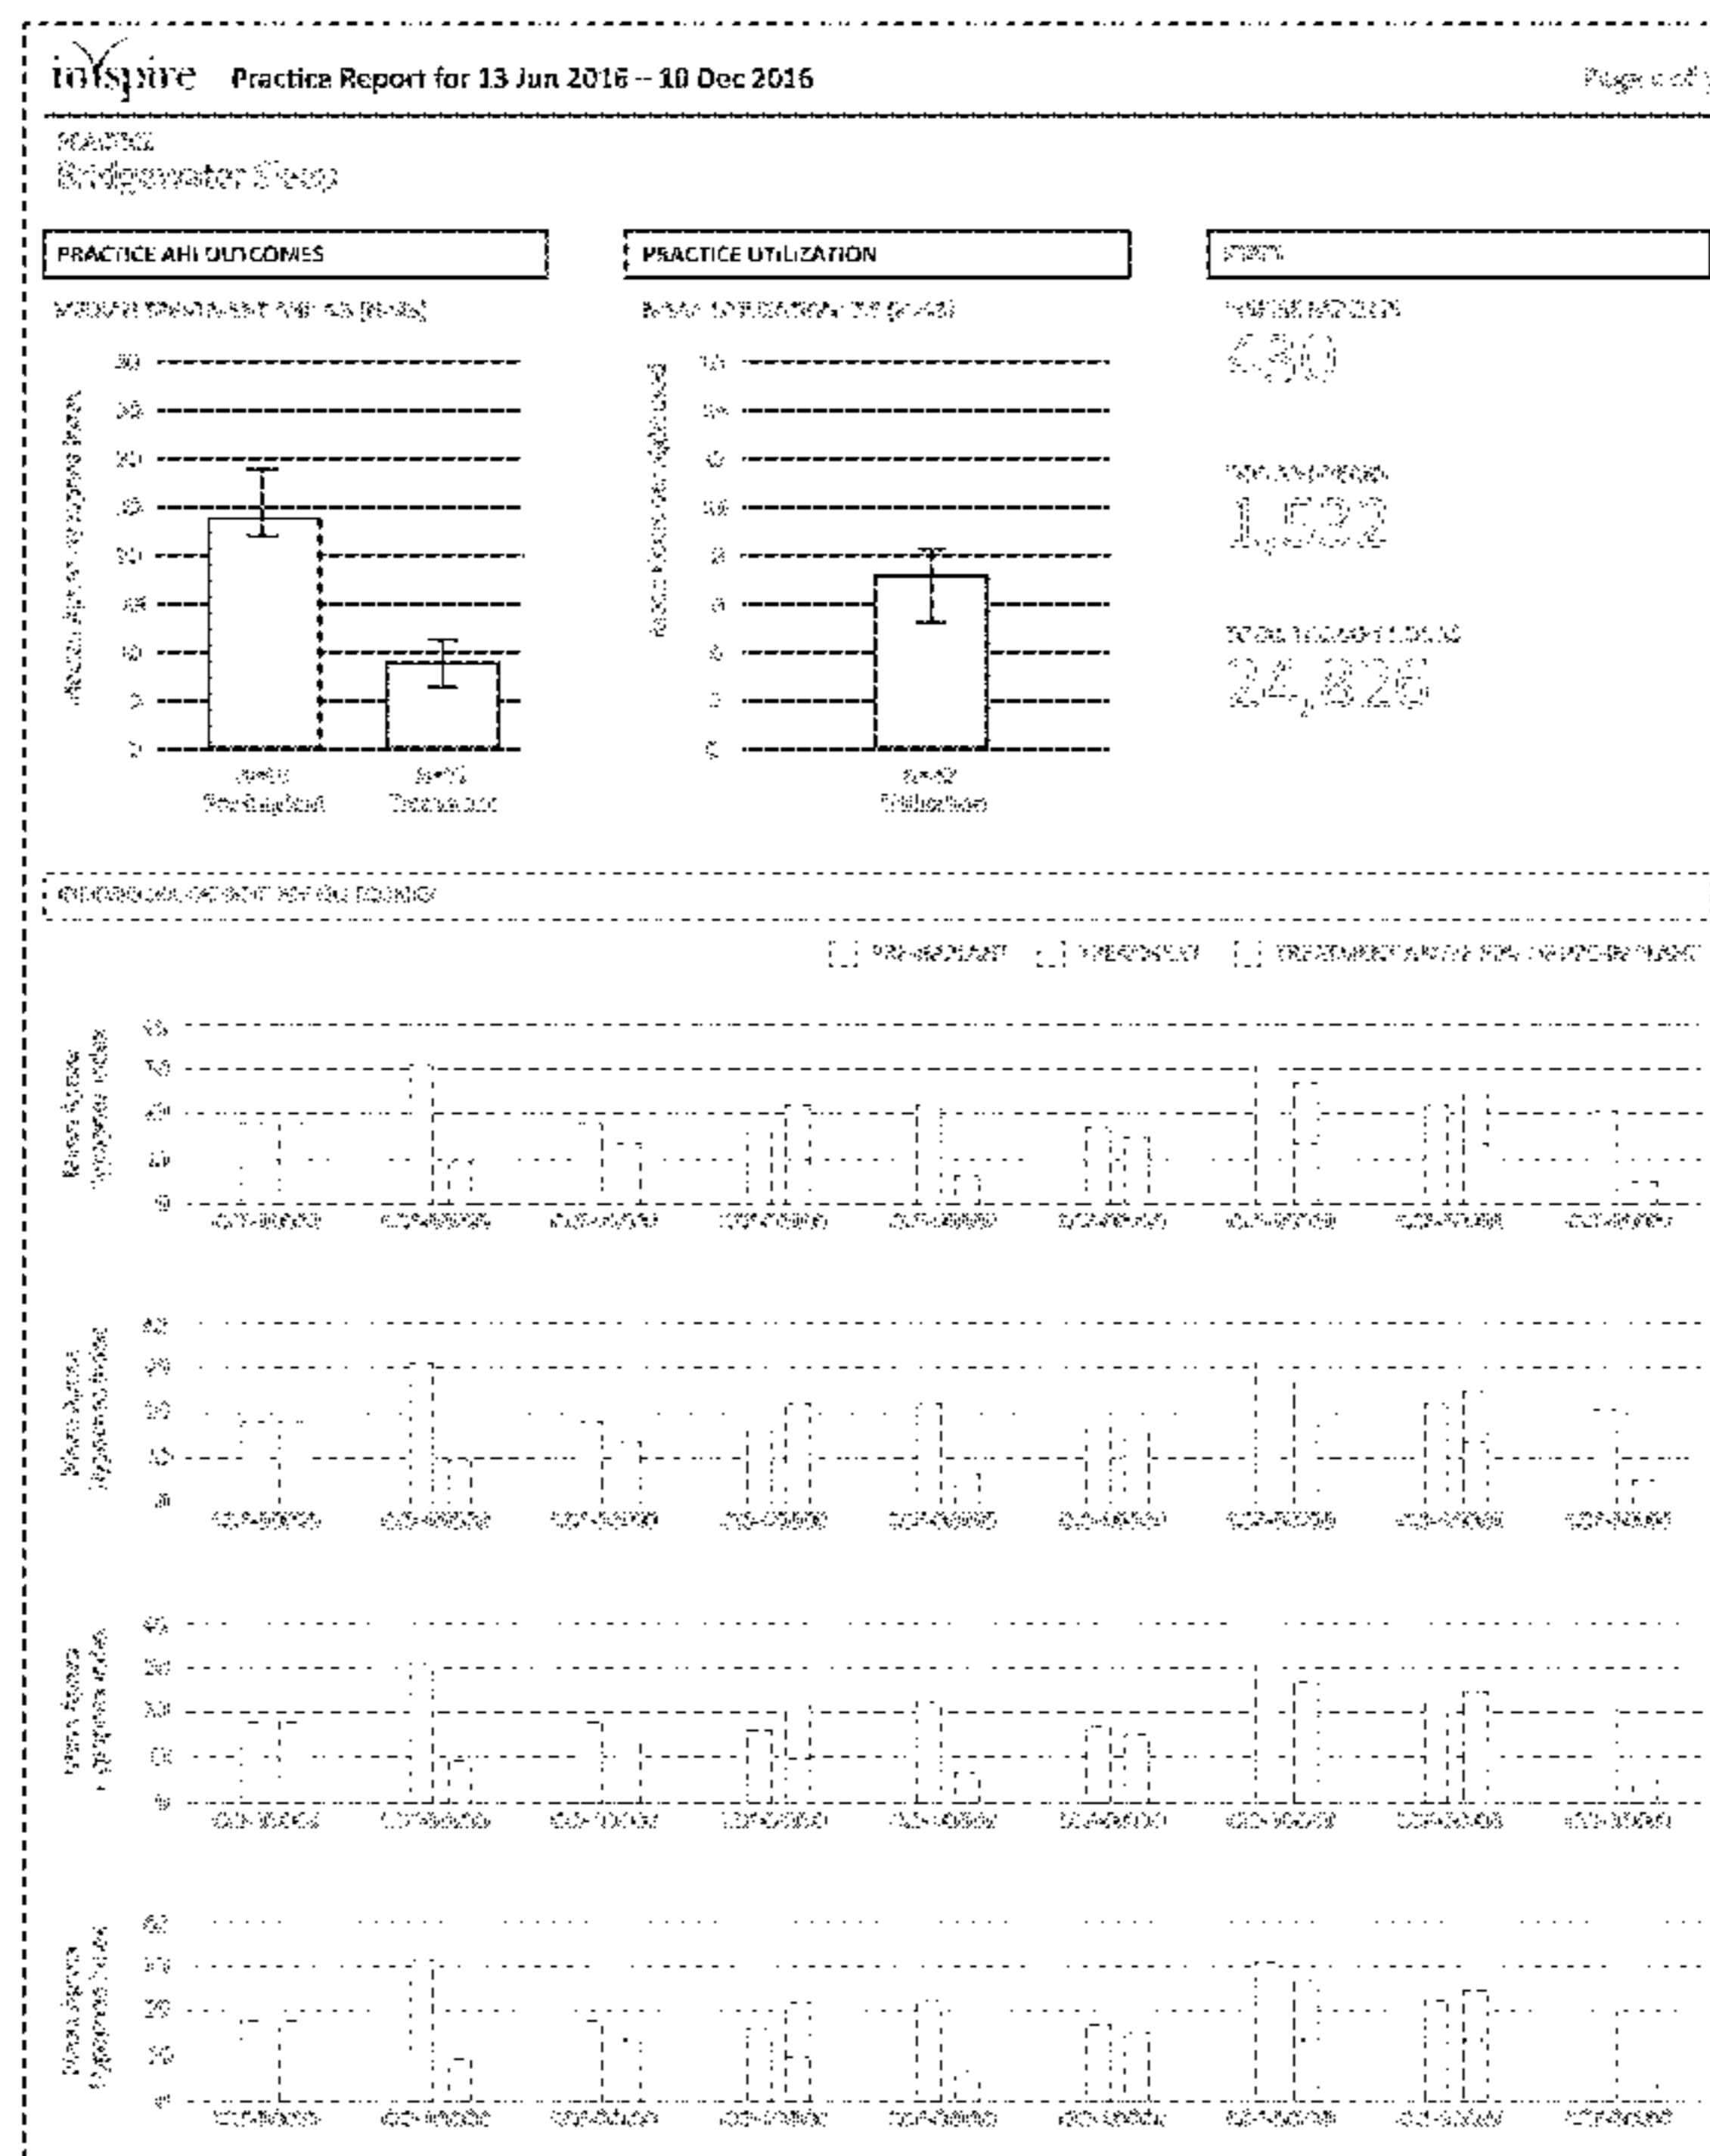




PRACTICE
Bridgewater Sleep


PRACTICE AHI OUTCOMES

MEAN TREATMENT AHI: 4.1 (N=61)

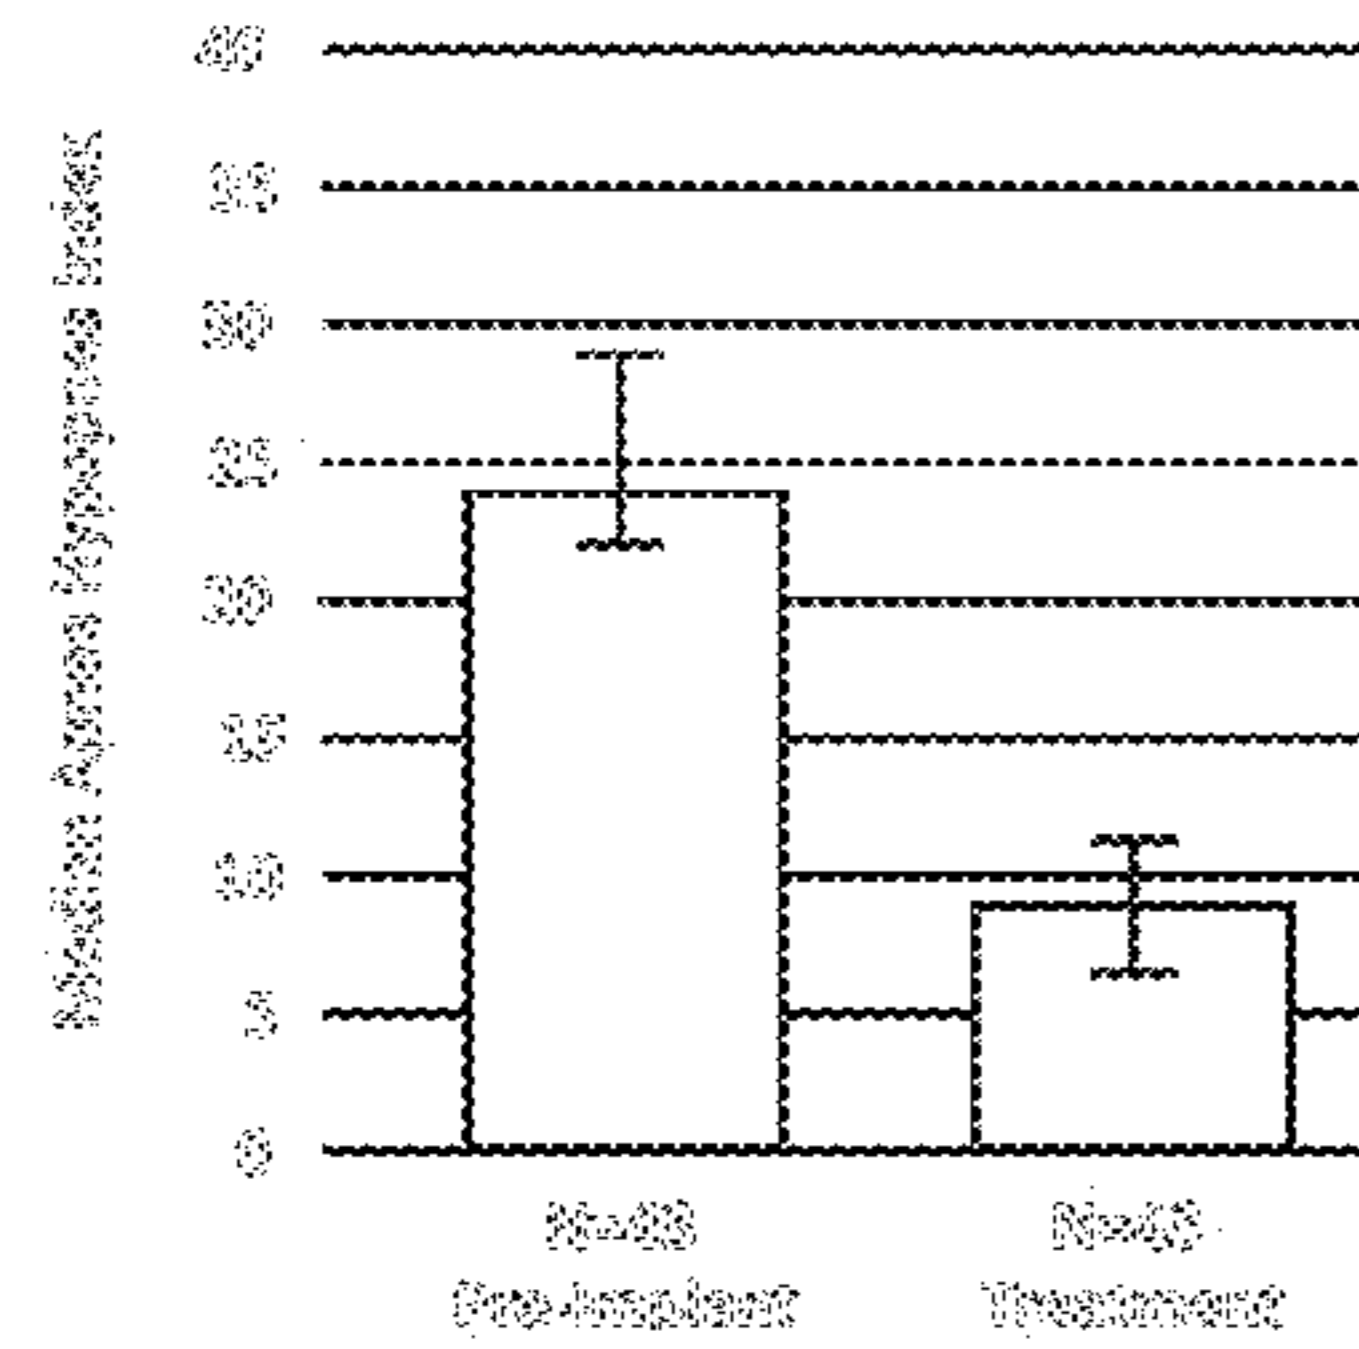

PRACTICE UTILIZATION

MEAN UTILIZATION: 7.5 (N=43)

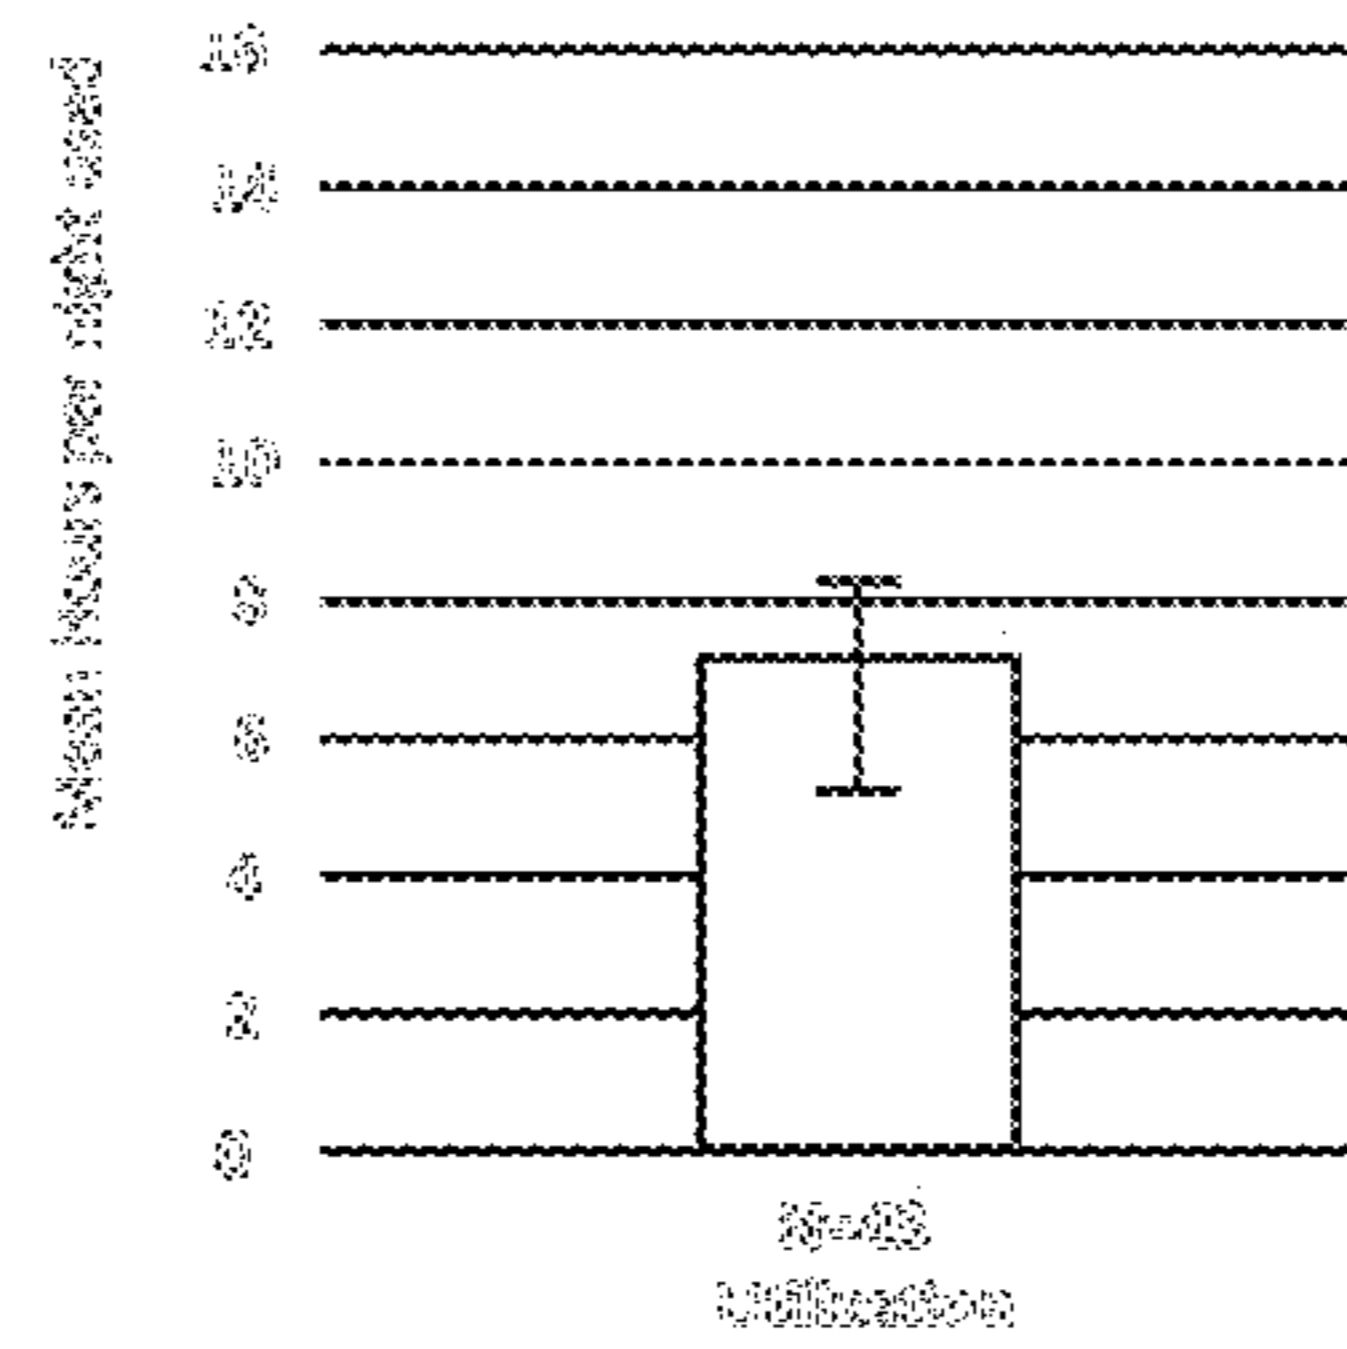

STATS

INSPIRE PATIENTS:

430

IMPLANT YEARS:

1,532

TOTAL THERAPY HOURS:

24,826

INDIVIDUAL PATIENT AHI OUTCOMES

Legend: [] PRE-IMPLANT [] TREATMENT [] TREATMENT ABOVE 50% OF PRE-IMPLANT

