



US00D877166S

(12) **United States Design Patent** (10) **Patent No.:** **US D877,166 S**
Dieken et al. (45) **Date of Patent:** **** Mar. 3, 2020**

(54) **DISPLAY SCREEN OR PORTION THEREOF WITH A GRAPHICAL USER INTERFACE**

(71) Applicant: **Inspire Medical Systems, Inc.**, Maple Grove, MN (US)

(72) Inventors: **David Todd Dieken**, Minneapolis, MN (US); **Maria Isabel Ancona**, Boston, MA (US); **John Rondoni**, Plymouth, MN (US)

(73) Assignee: **Inspire Medical Systems, Inc.**, Golden Valley, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/670,042**

(22) Filed: **Nov. 13, 2018**

Related U.S. Application Data

(63) Continuation of application No. 29/617,338, filed on Sep. 13, 2017, now Pat. No. Des. 833,461.

(51) **LOC (12) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485-488
CPC G06F 3/0482; G06F 16/248
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D593,109 S 5/2009 Danton
D752,621 S * 3/2016 Cojuangco D14/486

D778,928 S 2/2017 Bertnick et al.
D808,408 S * 1/2018 Bombolowsky D14/486
D808,996 S 1/2018 Ambielli
D816,689 S 5/2018 Chalker et al.
D833,461 S * 11/2018 Dieken D14/485
D840,422 S * 2/2019 Tuthill D14/486
D840,426 S * 2/2019 Dieken D14/486
2010/0121707 A1 5/2010 Goeldi
2012/0221589 A1 * 8/2012 Shahar G06F 16/248
707/758
2017/0085436 A1 3/2017 Costa et al.
2017/0140071 A1 5/2017 Coates et al.
2017/0201861 A1 7/2017 Freeman-baer et al.

* cited by examiner

Primary Examiner — Richelle G Shelton

(74) *Attorney, Agent, or Firm* — Dicke, Billig & Czaja, PLLC

(57) **CLAIM**


We claim the ornamental design for a display screen or portion thereof with a graphical user interface, as shown and described.


DESCRIPTION

The FIGURE is a front view of a display screen or portion thereof with a graphical user interface showing our new design.

The outermost broken lines show a display screen or portion thereof and form no part of the claimed design. The remaining broken lines show elements of the graphical user interface that form no part of the claimed design.

1 Claim, 1 Drawing Sheet

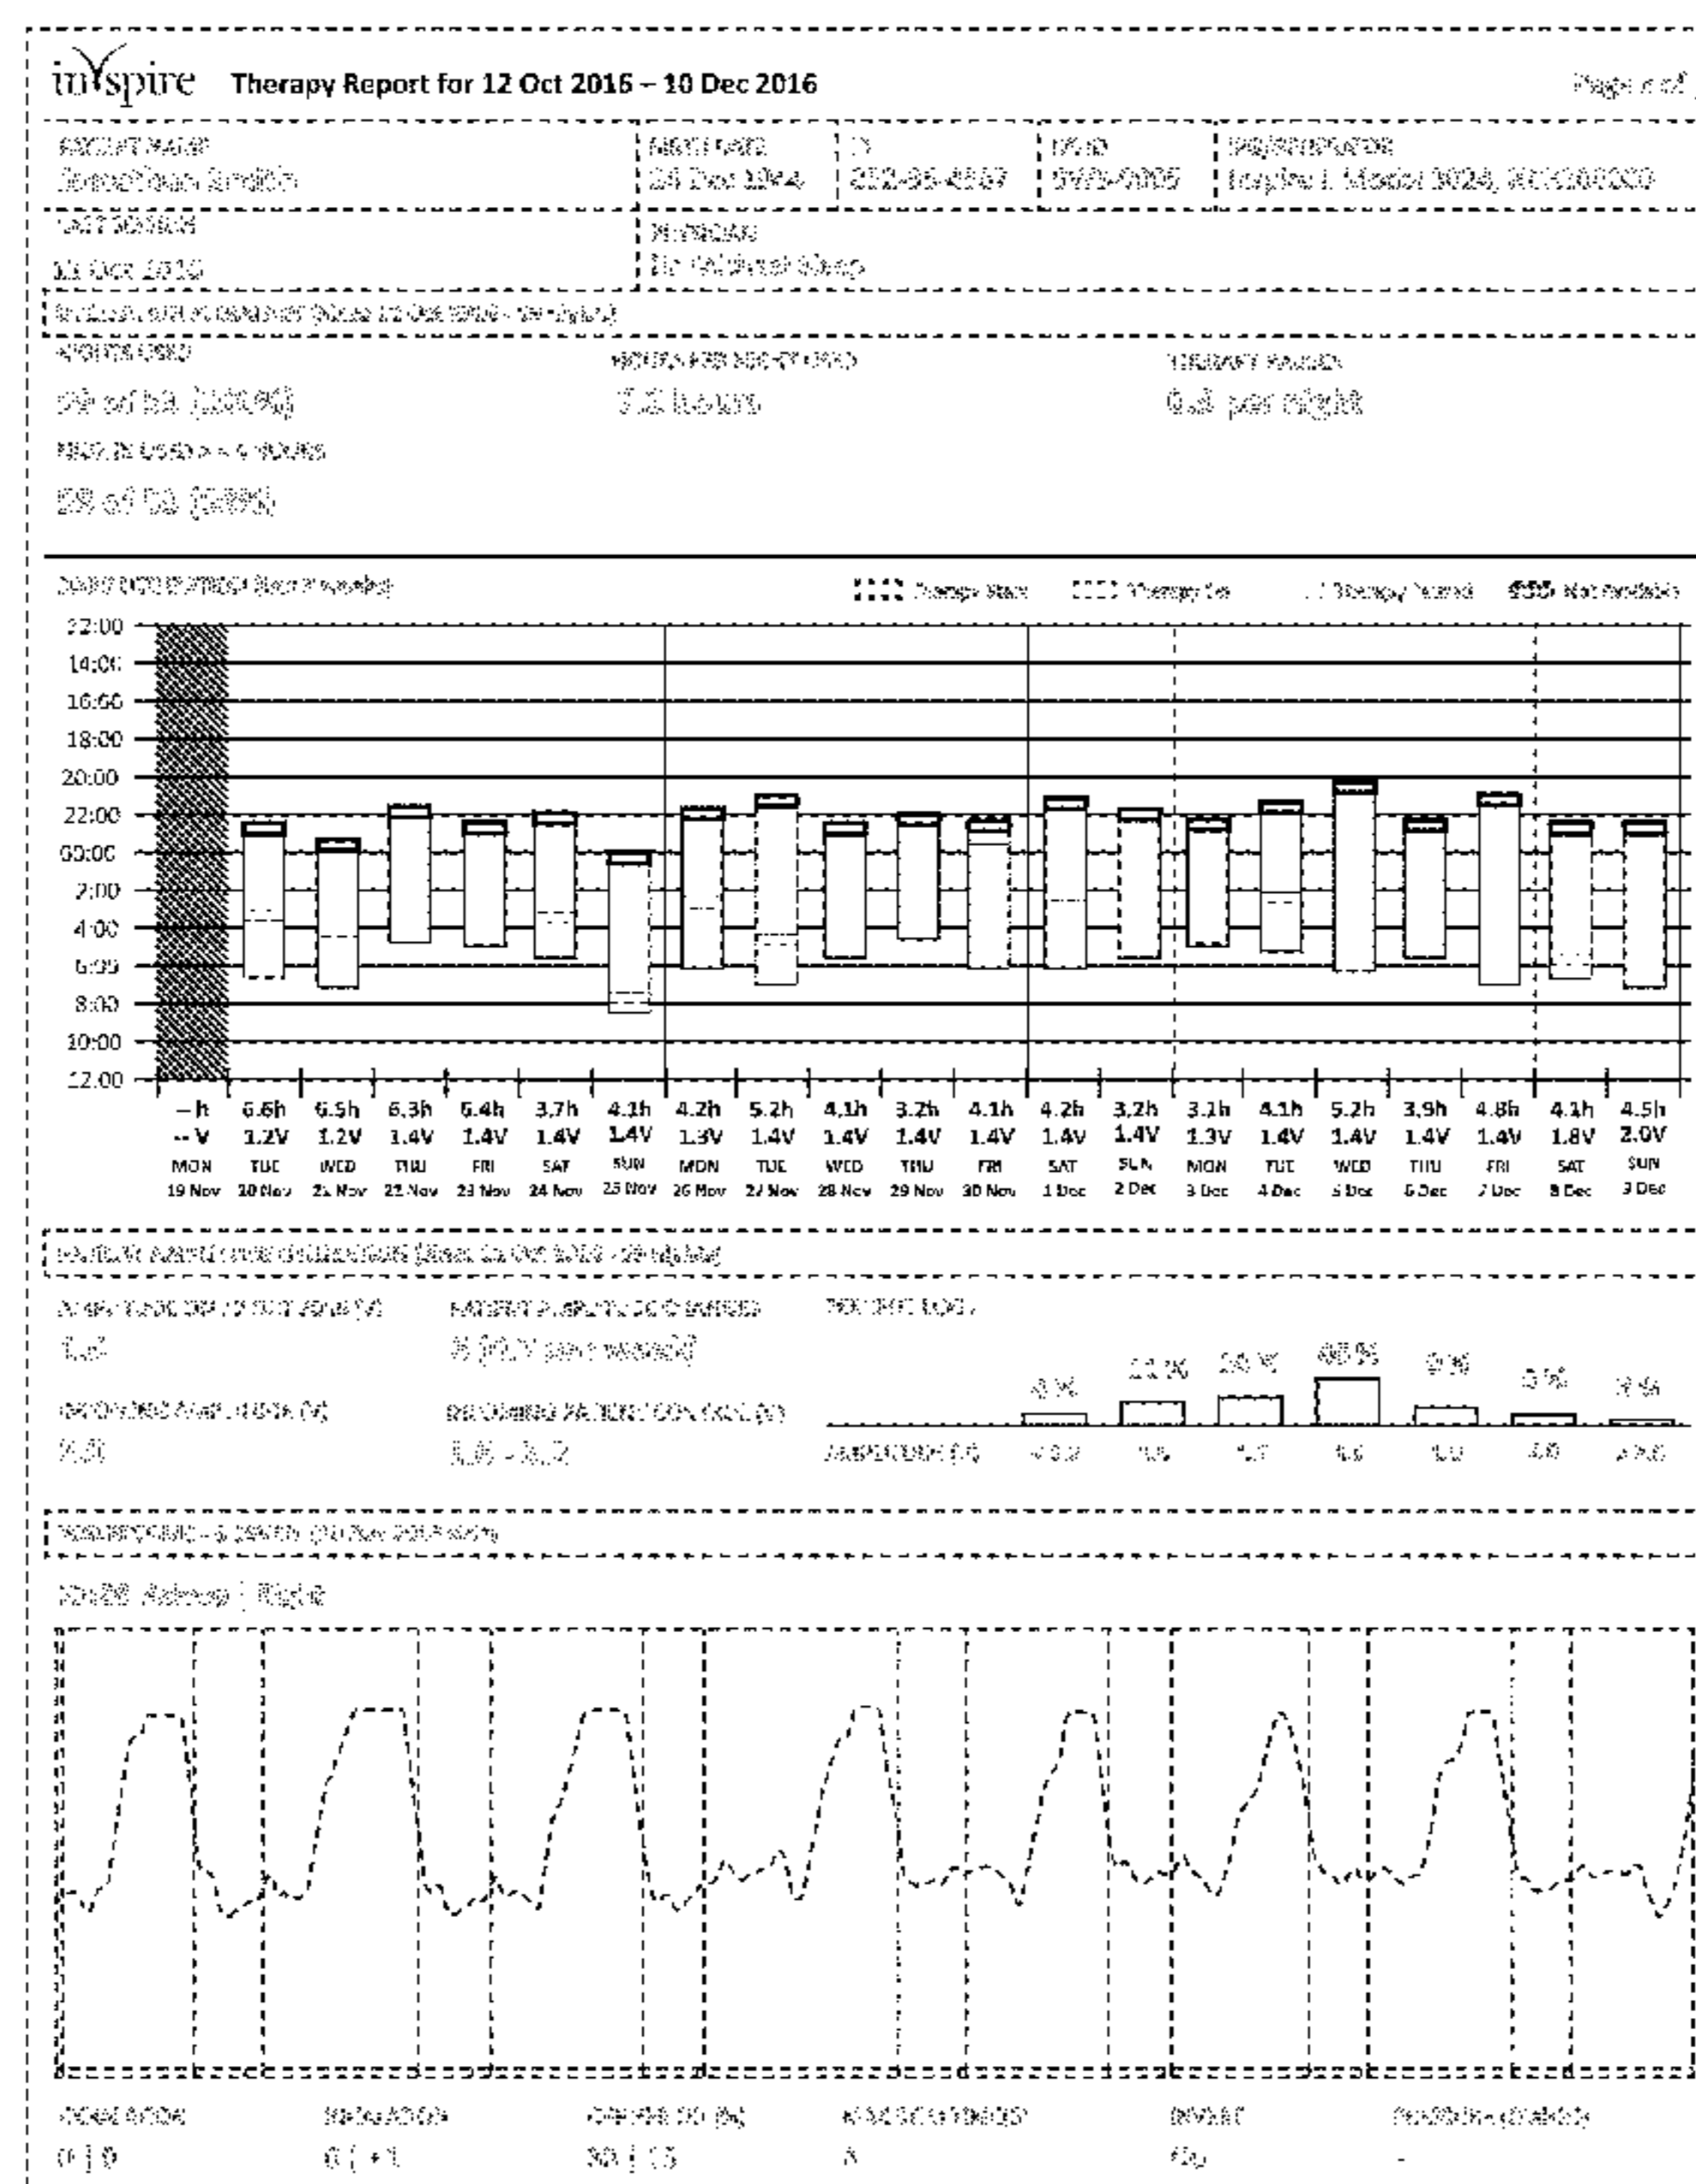



Therapy Report for 12 Oct 2016 – 10 Dec 2016


Page **x** of **y**

PATIENT NAME Jonathan Smith	BIRTH DATE 24 Dec 1944	ID 852-35-4557	DEAD BWS-0005	PG/GENERATOR inspire II Model 3024, NCR200000
LAST SESSION 12 Oct 2016		PHYSICIAN Dr. Michael Sleep		

UTILIZATION SUMMARY (Since 12 Oct 2016 - 59 nights)


NIGHTS USED 59 of 59 (100%)	HOURS PER NIGHT USED 7.2 hours	THERAPY PAUSES 0.9 per night
NIGHTS USED > = 4 HOURS 58 of 59 (98%)		

DAILY UTILIZATION (Last 3 weeks)

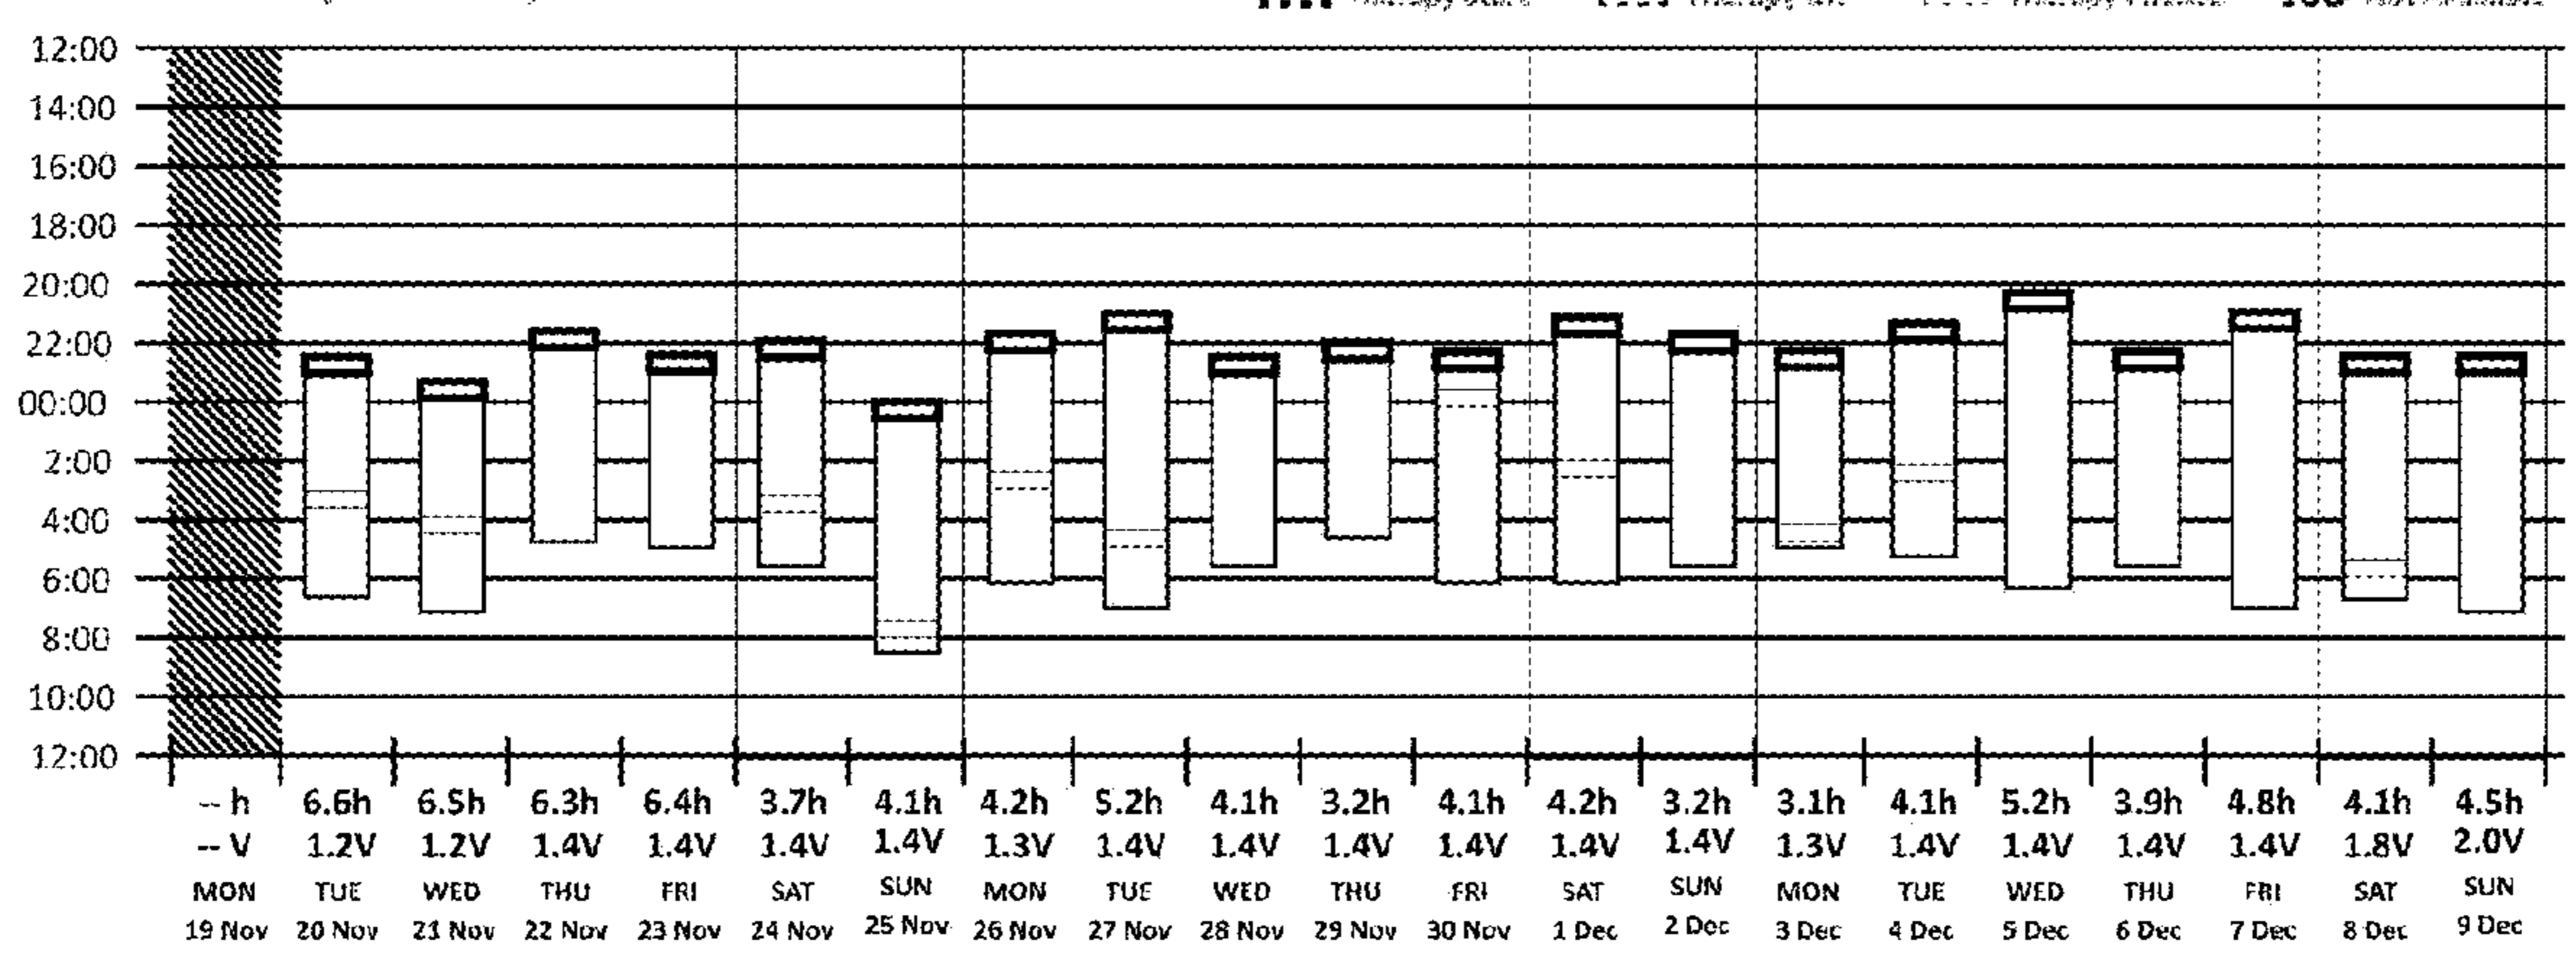


MON 19 Nov	TUE 20 Nov	WED 21 Nov	THU 22 Nov	FRI 23 Nov	SAT 24 Nov	SUN 25 Nov	MON 26 Nov	TUE 27 Nov	WED 28 Nov	THU 29 Nov	FRI 30 Nov	SAT 1 Dec	SUN 2 Dec	MON 3 Dec	TUE 4 Dec	WED 5 Dec	THU 6 Dec	FRI 7 Dec	SAT 8 Dec	SUN 9 Dec
-h	6.6h	6.5h	6.3h	6.4h	3.7h	4.1h	4.2h	5.2h	4.1h	3.2h	4.1h	4.2h	3.2h	3.1h	4.1h	5.2h	3.9h	4.8h	4.1h	4.5h
-v	1.2V	1.2V	1.4V	1.4V	1.4V	1.4V	1.3V	1.4V	1.4V	1.4V	1.4V	1.4V	1.4V	1.3V	1.4V	1.4V	1.4V	1.4V	1.8V	2.0V

PATIENT AMPLITUDE UTILIZATION (Since 12 Oct 2016 - 59 nights)

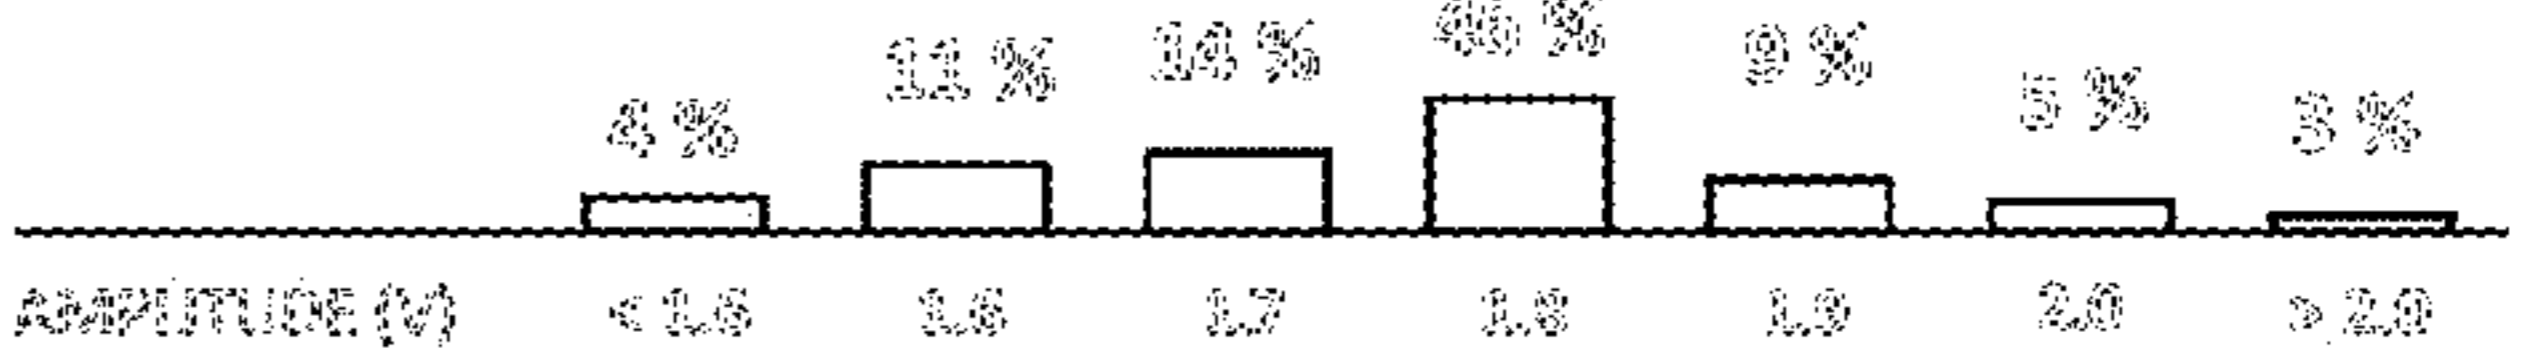AMPLITUDE ON 12 OCT 2016 (V) 1.6	PATIENT AMPLITUDE CHANGES 6 (0.7 per week)	PERCENT USED
INCOMING AMPLITUDE (V) 2.0	INCOMING PATIENT CONTROL (V) 1.5 - 2.2	

WAVEFORMS - 3 SAVED (10 Dec 2016 view)

23:23 Asleep | Right

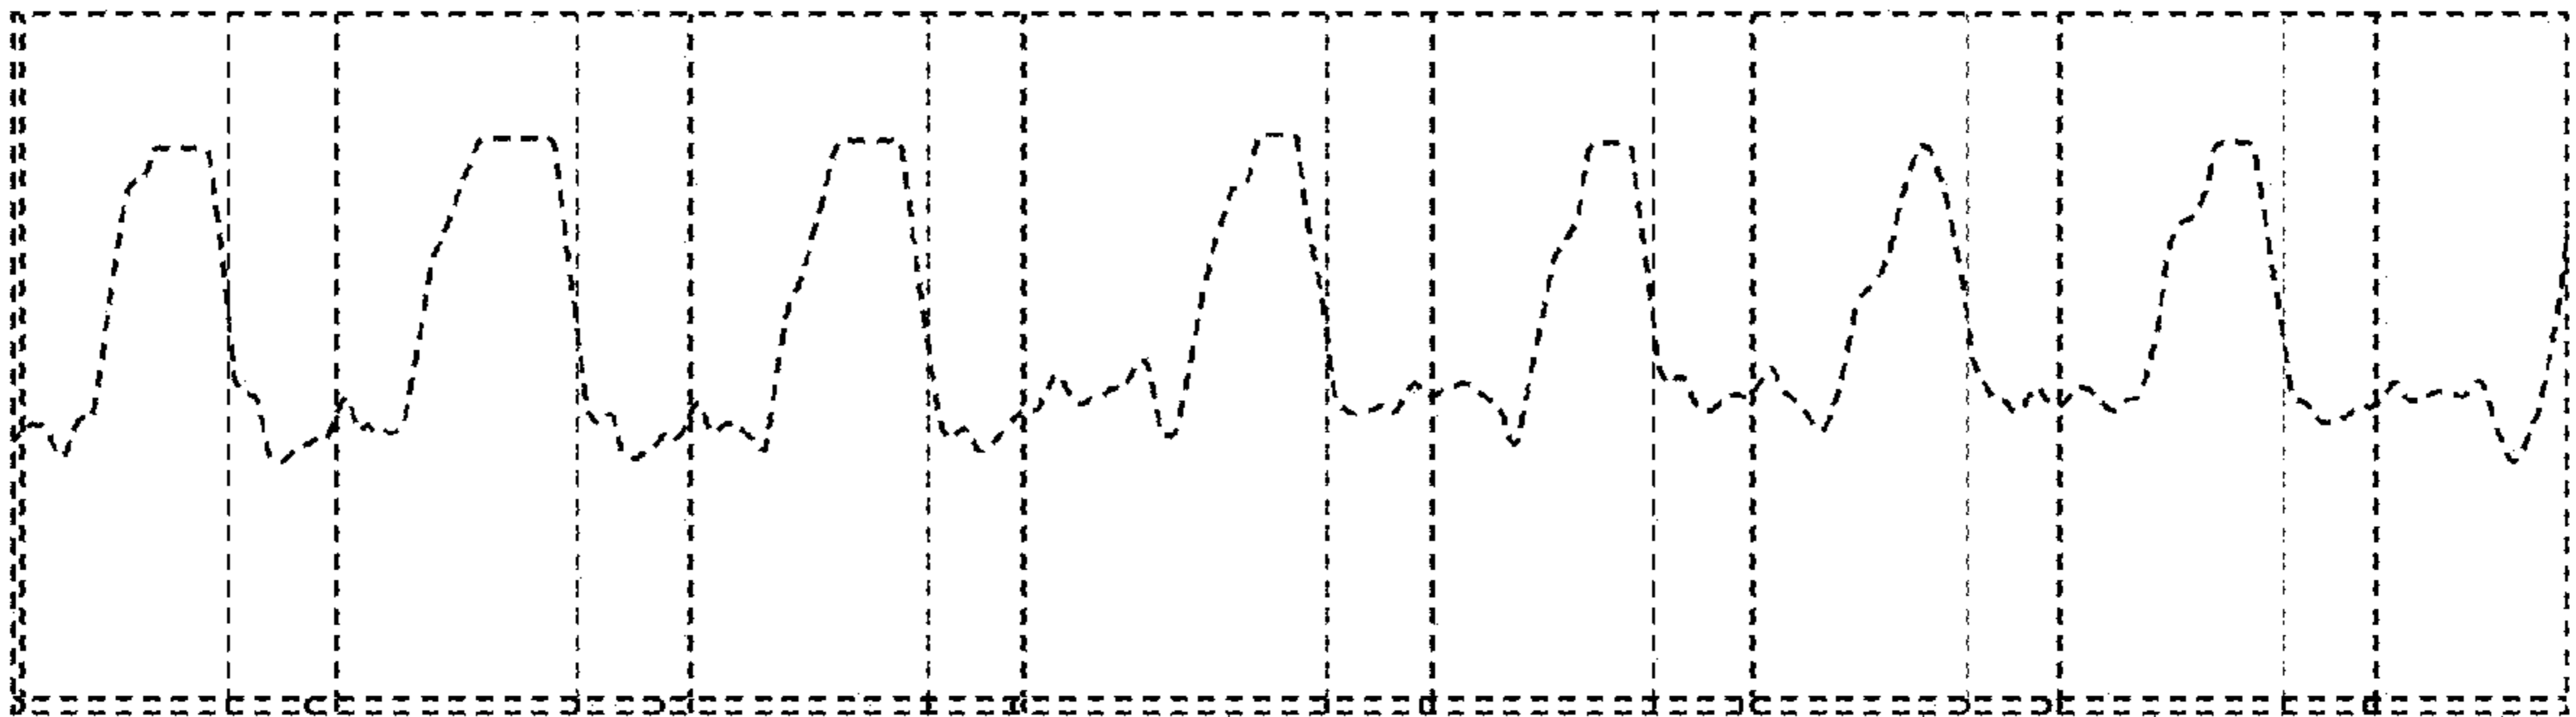

EXHALATION 0 0	INHALATION 0 +1	OFF PERIOD (%) 38 13	MAX STIM TIME(S) 4	INVERT No	PRESSURE (CMH2O) ~
----------------------------	-----------------------------	----------------------------------	------------------------------	---------------------	------------------------------