



US00D877322S

(12) **United States Design Patent**
Jackson et al.

(10) **Patent No.:** **US D877,322 S**
(45) **Date of Patent:** **** Mar. 3, 2020**

(54) **FLIP-TOP METERED-DOSE INHALER**

(71) Applicant: **Optimist Inhaler, LLC**, Flowery Branch, GA (US)

(72) Inventors: **David N Jackson**, Flowery Branch, GA (US); **Russell M Smith**, Flowery Branch, GA (US)

(73) Assignee: **Optimist Inhaler, LLC**, Gainesville, GA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/696,915**

(22) Filed: **Aug. 3, 2019**

(51) **LOC (12) Cl.** **29-02**

(52) **U.S. Cl.**
USPC **D24/110**

(58) **Field of Classification Search**
USPC D24/108, 110, 110.5, 164, 127
CPC A61M 15/009; A61M 2202/064; A61M 15/0065; A61M 15/00; A61M 15/008; A61M 15/0068; A61M 15/0091; A61M 2205/3592; A61M 2205/3553; A61M 15/0021; A61M 15/0025; A61M 15/0026
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D348,929 S * 7/1994 Paton D24/110
D473,640 S * 4/2003 Cuffaro D24/110
(Continued)

FOREIGN PATENT DOCUMENTS

WO WO2016187156 A1 11/2016
WO WO2017182975 A1 10/2017

OTHER PUBLICATIONS

Mhealthspot, <http://mhealthspot.com/2016/02/adherium-smart-inhalers-multicountry-study>, Mar. 18, 2017.
(Continued)


Primary Examiner — Lilyana Bekic
(74) *Attorney, Agent, or Firm* — Mehrman Law Office; Michael J. Mehrman

(57) **CLAIM**
The ornamental design for a flip-top metered-dose inhaler, as shown and described.

DESCRIPTION

FIG. 1 is a right side, front, and top perspective view of a flip-top metered-dose inhaler with its flip cover closed showing the new design.
FIG. 2 is a right side, front, and top perspective view thereof with its flip cover open.
FIG. 3 is a top plan view thereof with its flip cover closed.
FIG. 4 is a top plan view thereof with its flip cover open.
FIG. 5 is a bottom plan view thereof with its flip cover closed.
FIG. 6 is a bottom plan view thereof with its flip cover open.
FIG. 7 is a front elevational view thereof with its flip cover closed.
FIG. 8 is a front elevational view thereof with its flip cover open.
FIG. 9 is a right side elevational view thereof with its flip cover closed.
FIG. 10 is a right side elevational view thereof with its flip cover open.
FIG. 11 is a rear elevational view thereof with its flip cover closed; and,
FIG. 12 is a rear elevational view thereof with its flip cover open.
The broken lines in the drawings depict portions of the flip-top metered-dose inhaler that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

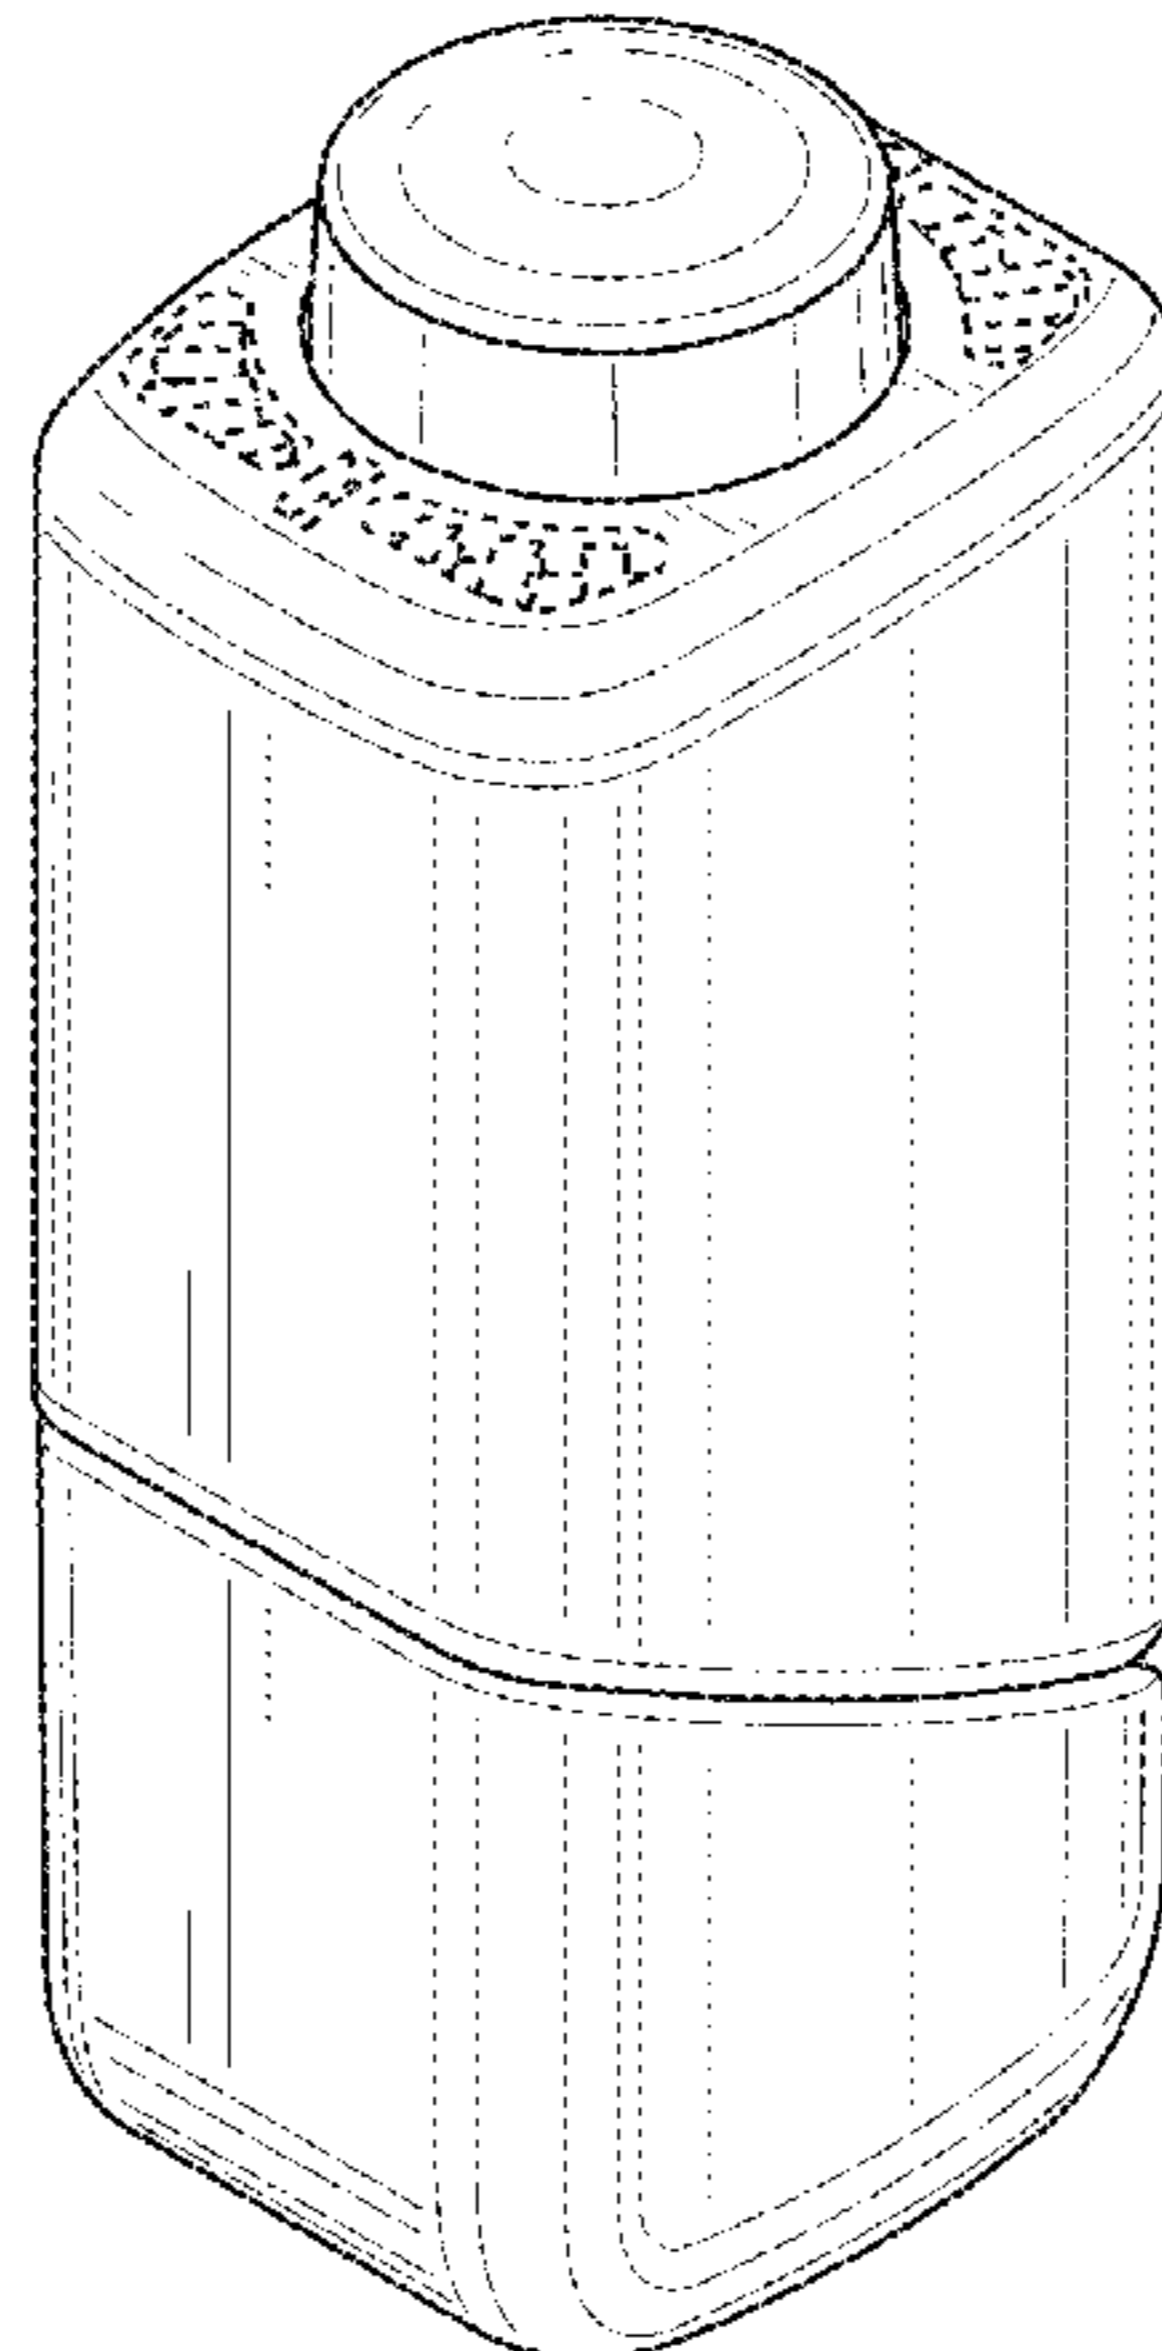

(56)

References Cited

U.S. PATENT DOCUMENTS

D480,474 S * 10/2003 Bowman D24/110
D582,543 S * 12/2008 Lucking D24/110
D582,544 S * 12/2008 Meziere D24/110
D716,936 S * 11/2014 Jensen D24/110
D769,436 S * 10/2016 Walsh D24/110
D769,437 S * 10/2016 Walsh D24/110
D808,515 S * 1/2018 Atkin D24/110
D834,704 S * 11/2018 Atkin D24/110
D863,534 S * 10/2019 Jackson D24/110
10,434,268 B2 * 10/2019 Herder A61M 15/0026
2008/0156321 A1 * 7/2008 Bowman A61M 15/009
128/200.23
2016/0325058 A1 11/2016 Samson et al.
2017/0042215 A1 2/2017 Murison
2017/0319797 A1 11/2017 Germinario et al.
2018/0140788 A1 * 5/2018 Calderon Oliveras
A61M 15/0023
2018/0228988 A1 * 8/2018 Buck A61M 15/00

OTHER PUBLICATIONS

Vaporsmooth, <https://vaporsmooth.com/breeze-smart-inhaler-new-breeze-vaporizer-by-resolve-digital-health>, Jun. 24, 2017.
www.3Ders.org, <http://www.3ders.org/articles/20160314-3d-printed-smart-inhaler-could-help-doctors-better-understand-asthma.html>, Mar. 16, 2016.
Medgadget, <https://www.medgadget.com/2014/06/nexus6-smarttouch-inhaler-monitor-helps-patients-adhere-to-medication-regimens.html>, Jun. 6, 2014.
Syqemmedical, <https://www.syqemmedical.com>, Dec. 1, 2016.
www.vccny.com, <http://www.vccny.com/blog/2016/12/01/albuterol-toxicity-in-pets-where-is-your-inhaler>, Dec. 1, 2016.

* cited by examiner

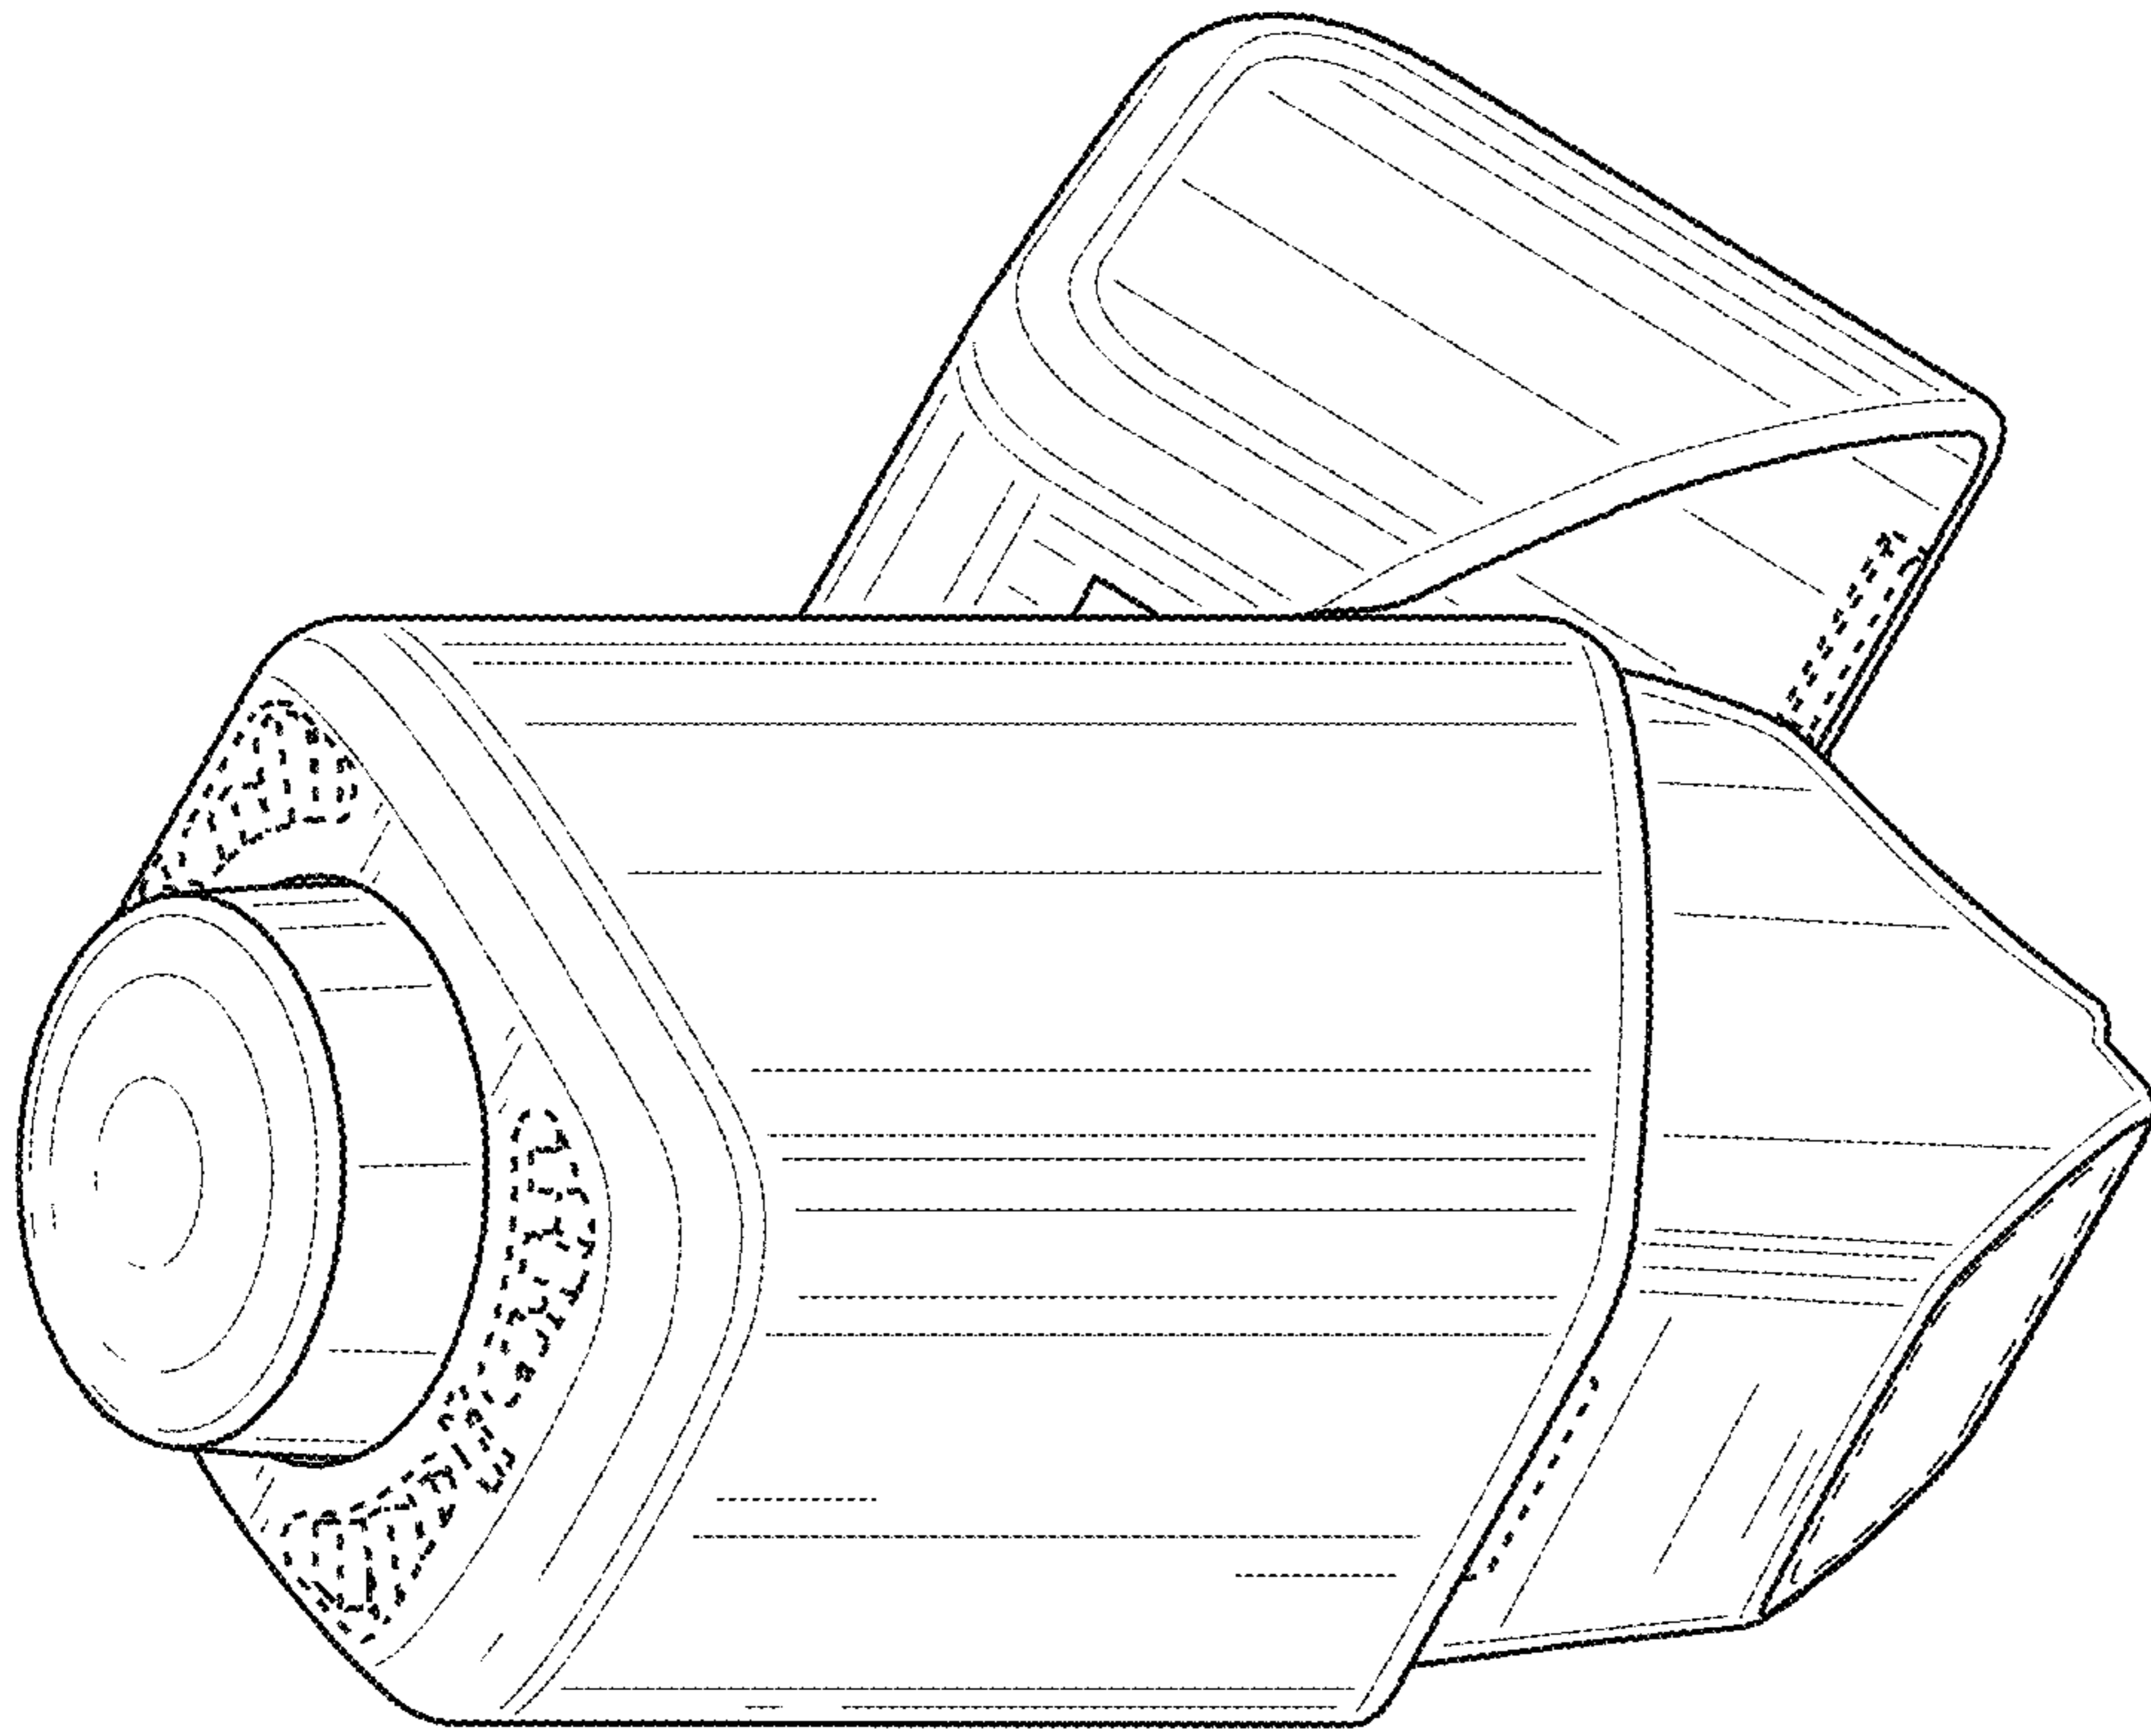


Fig. 1

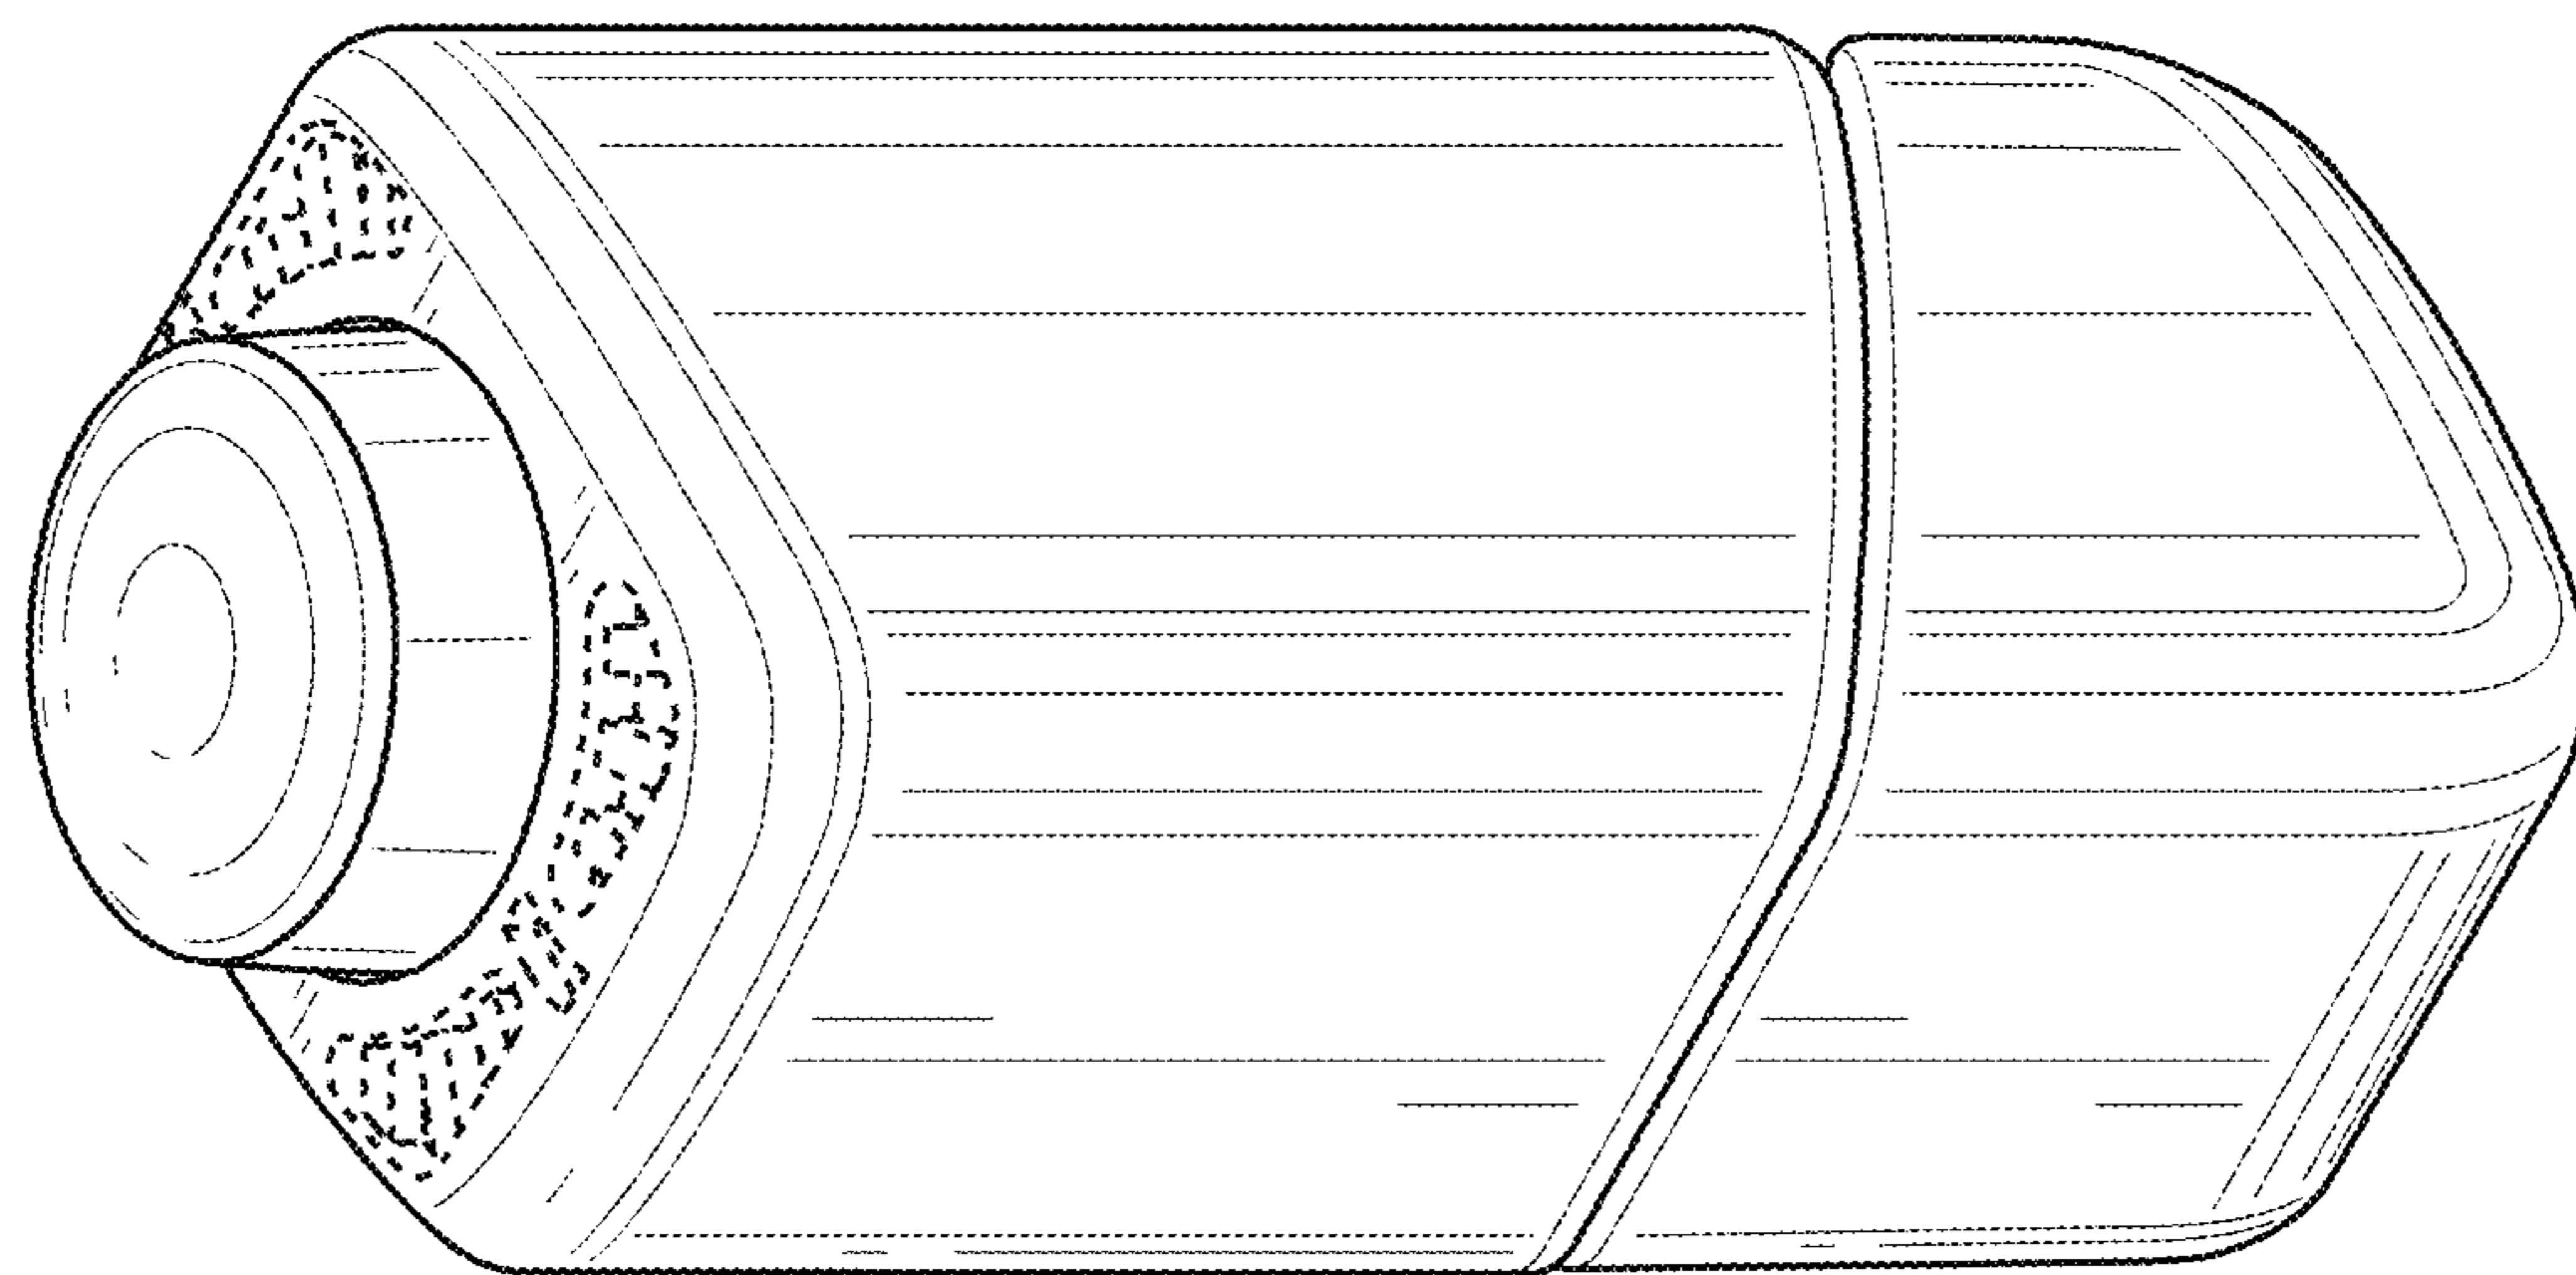


Fig. 2

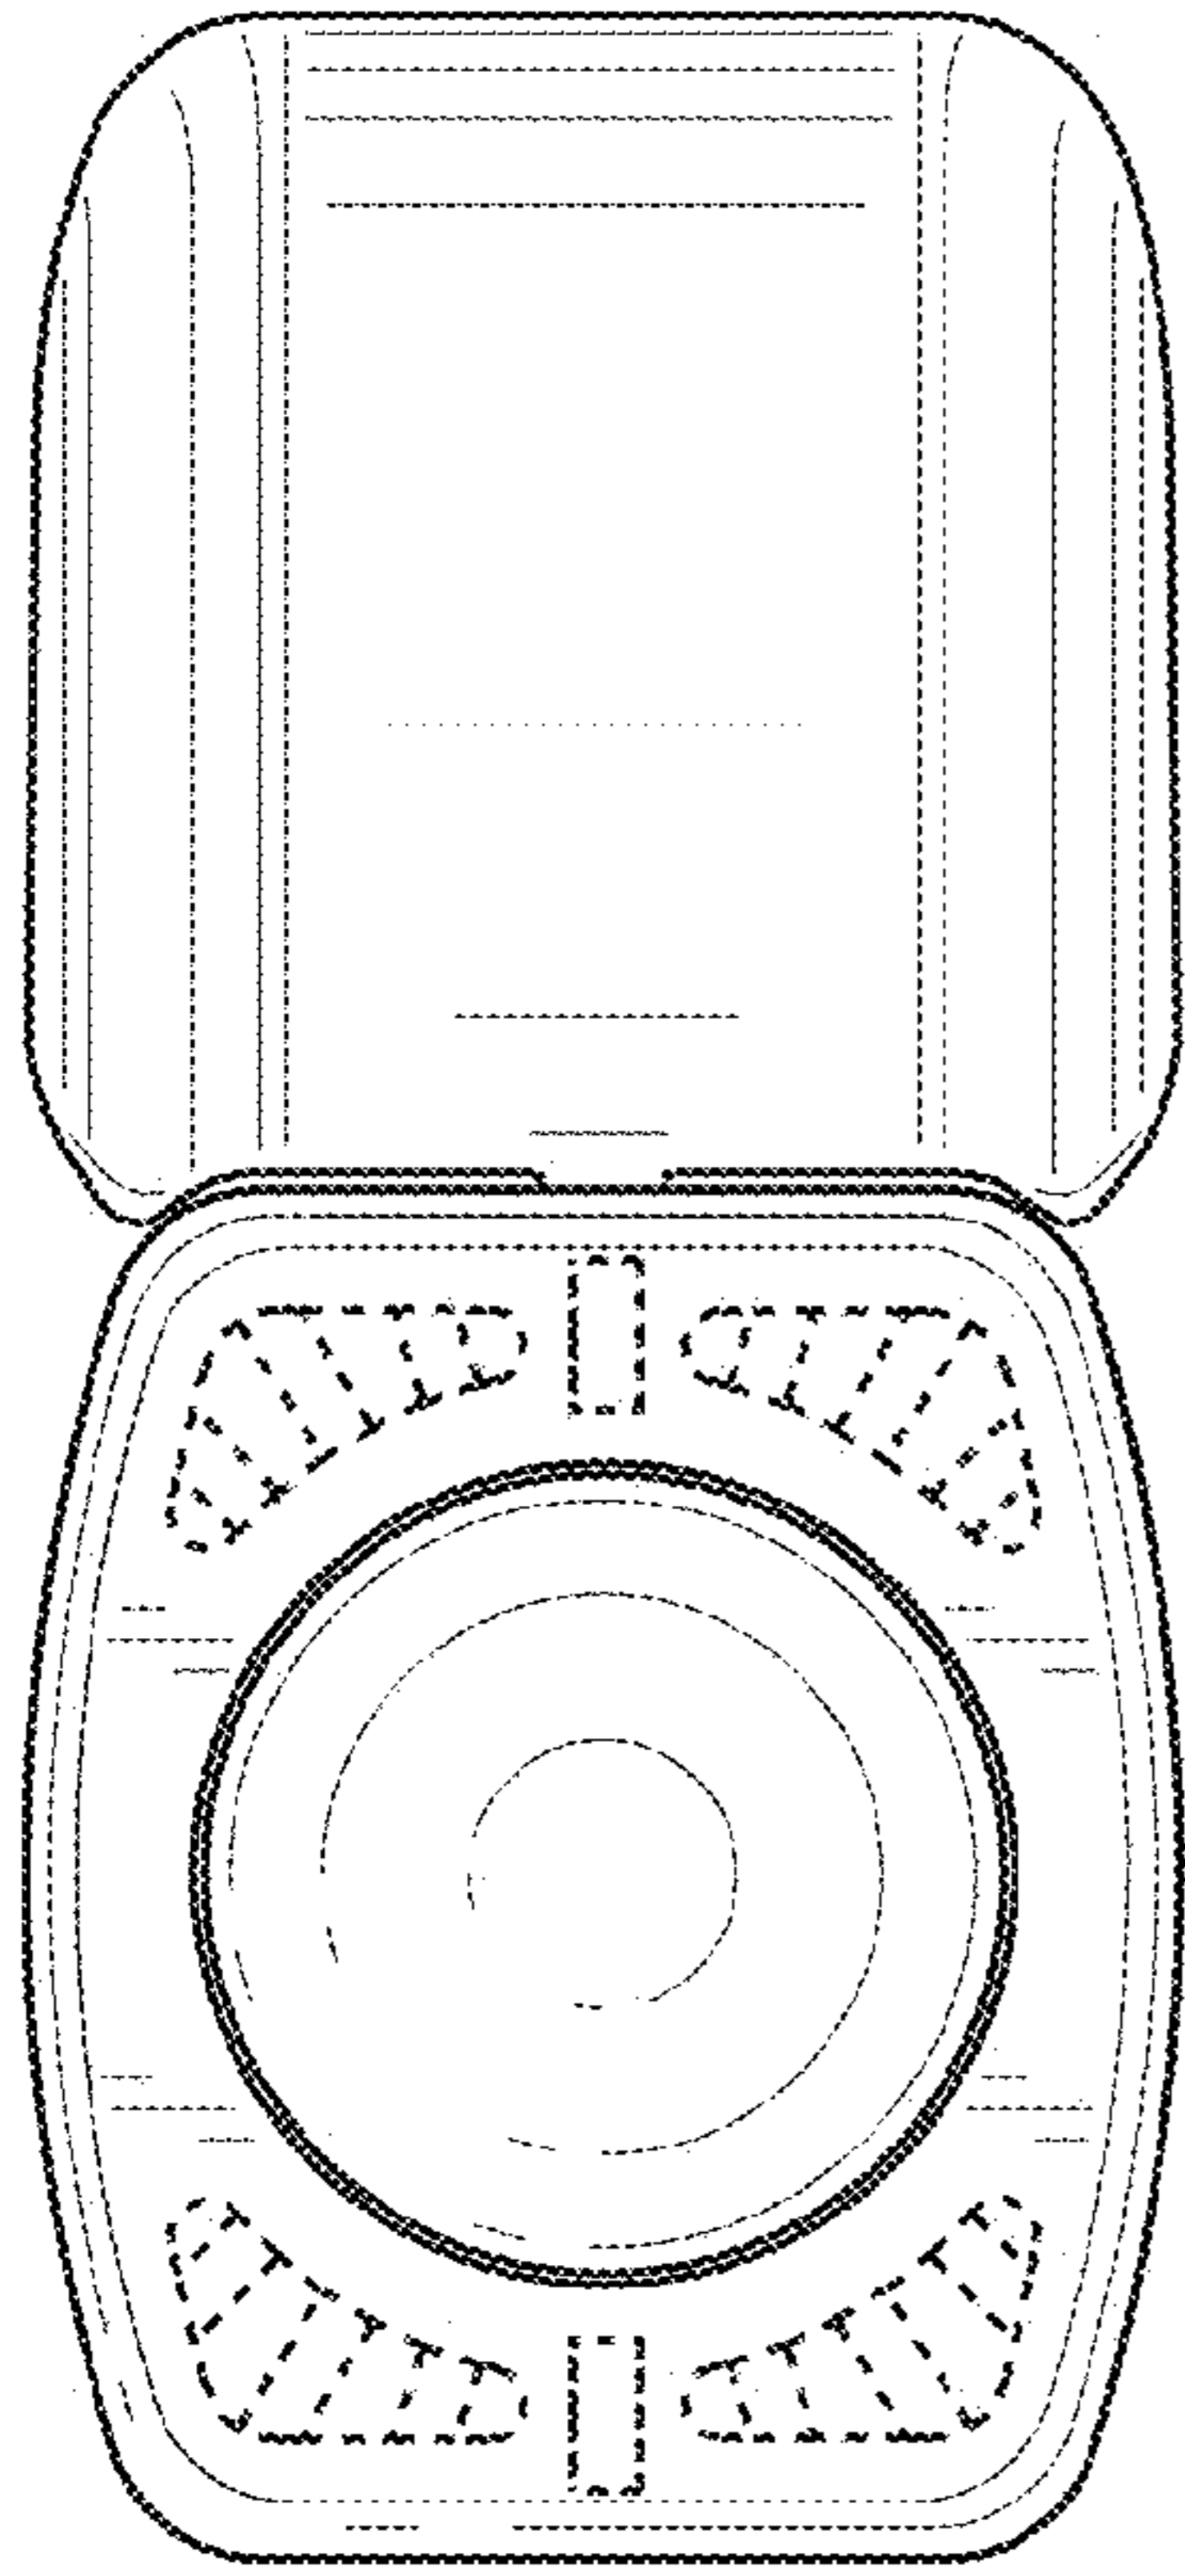


Fig. 4

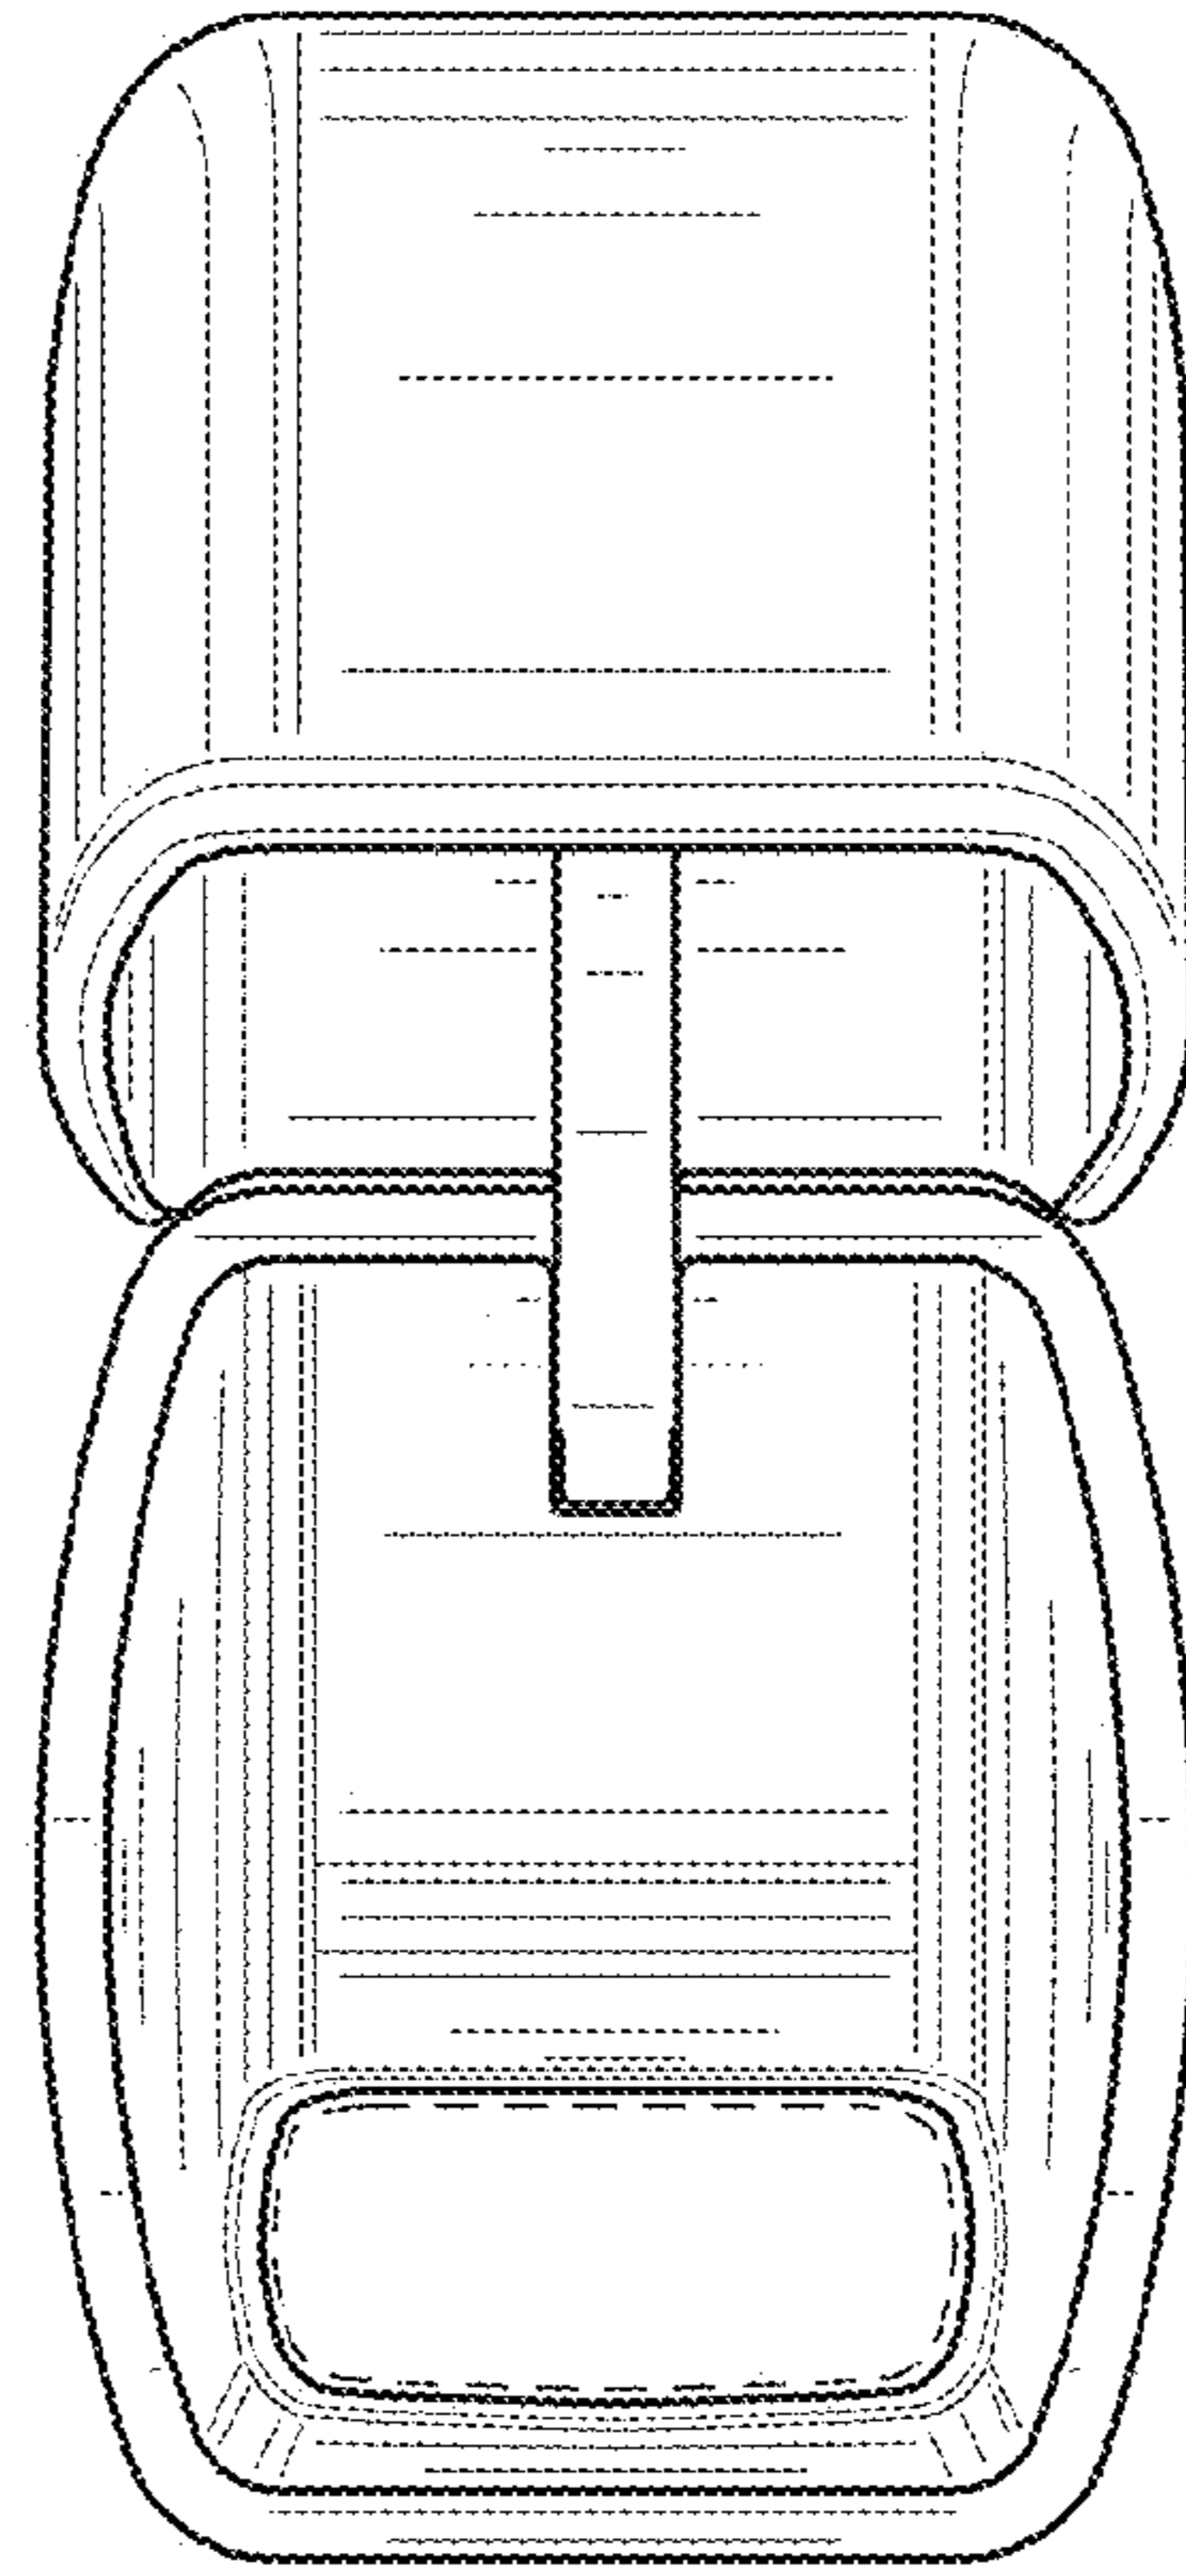


Fig. 6

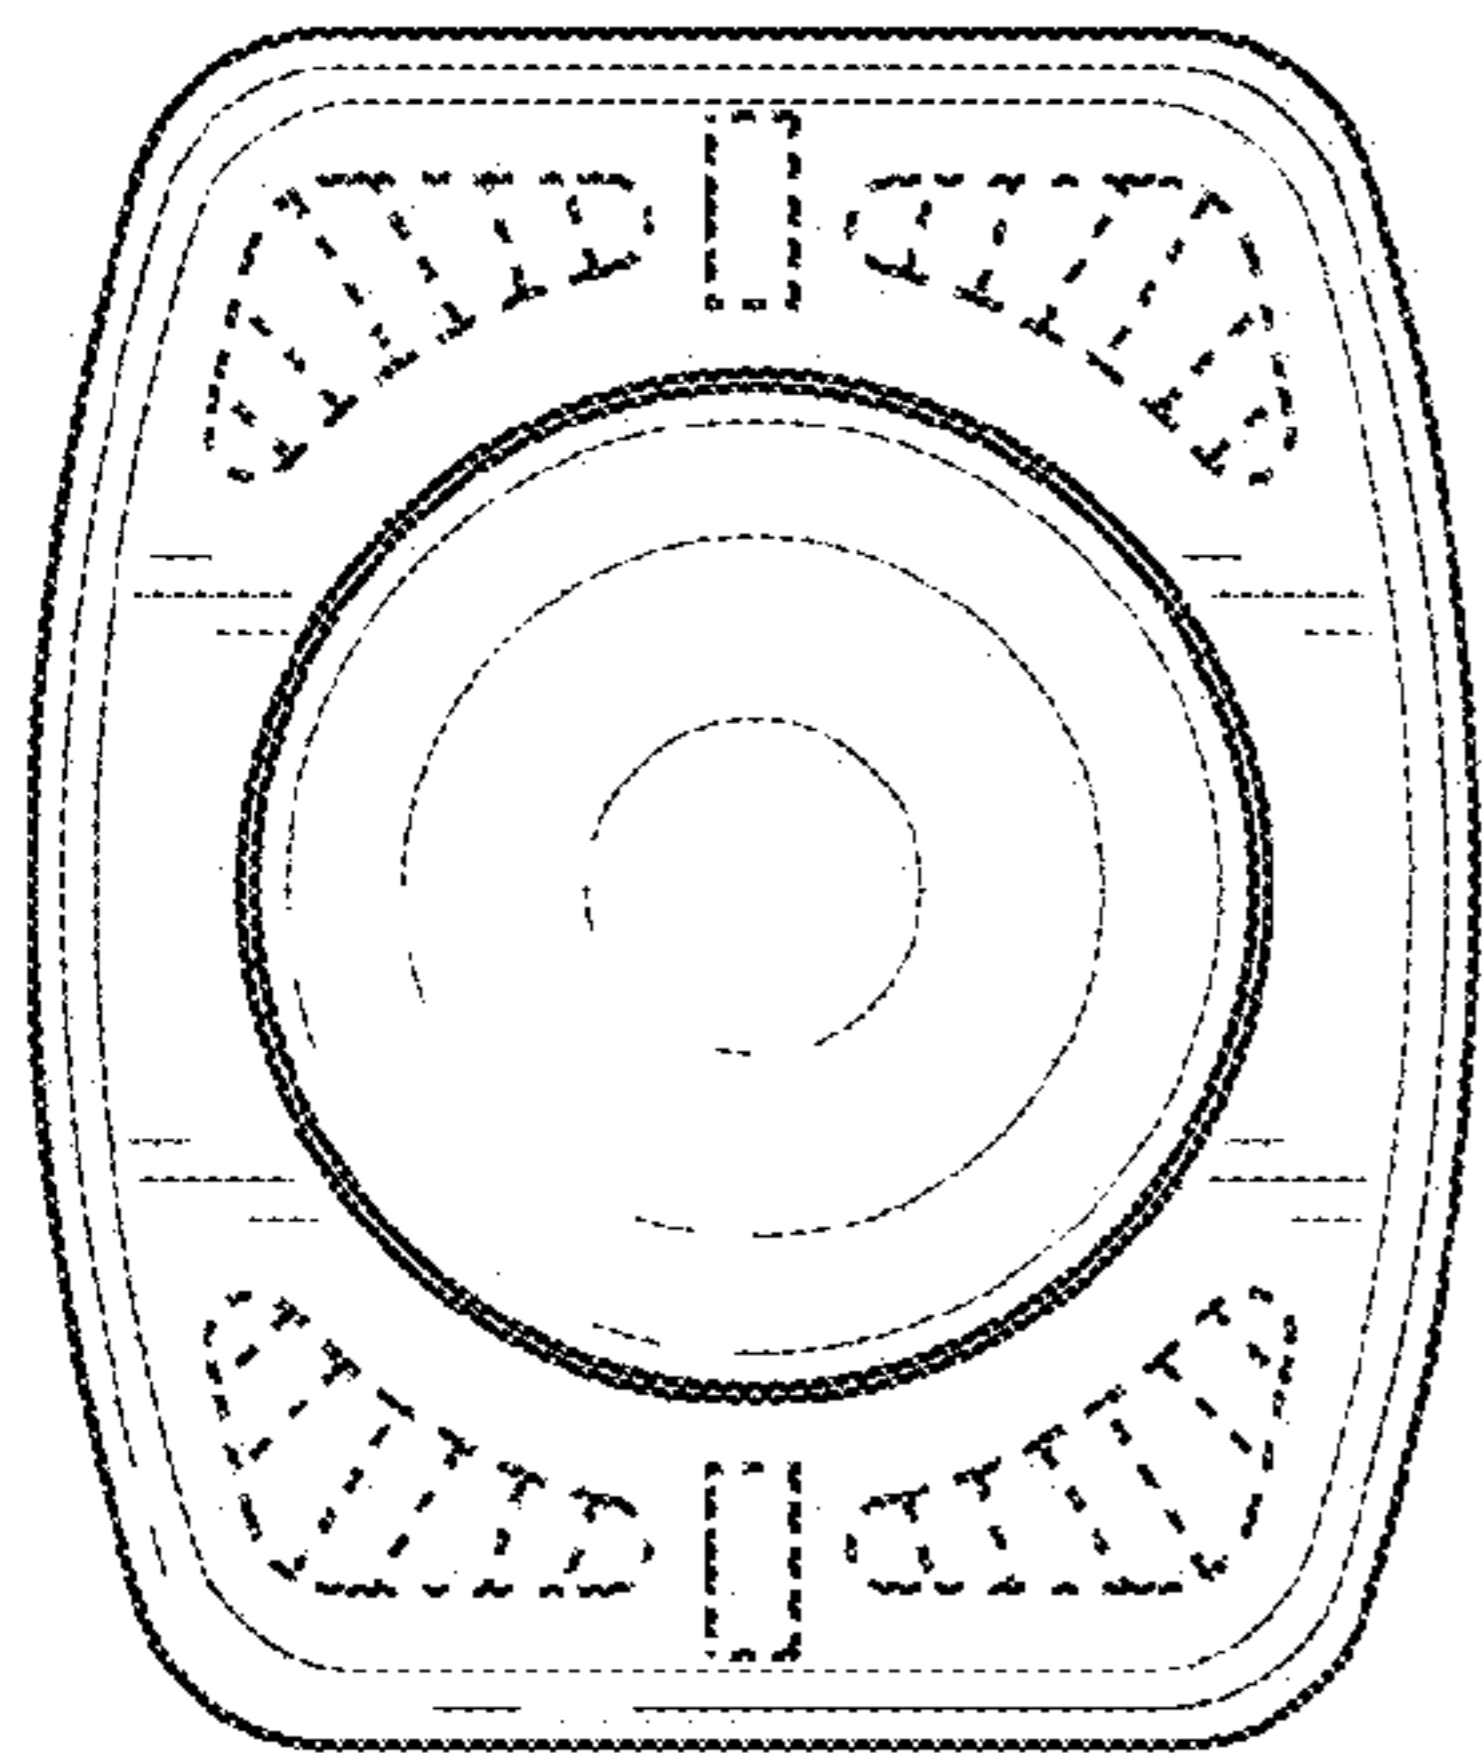


Fig. 3

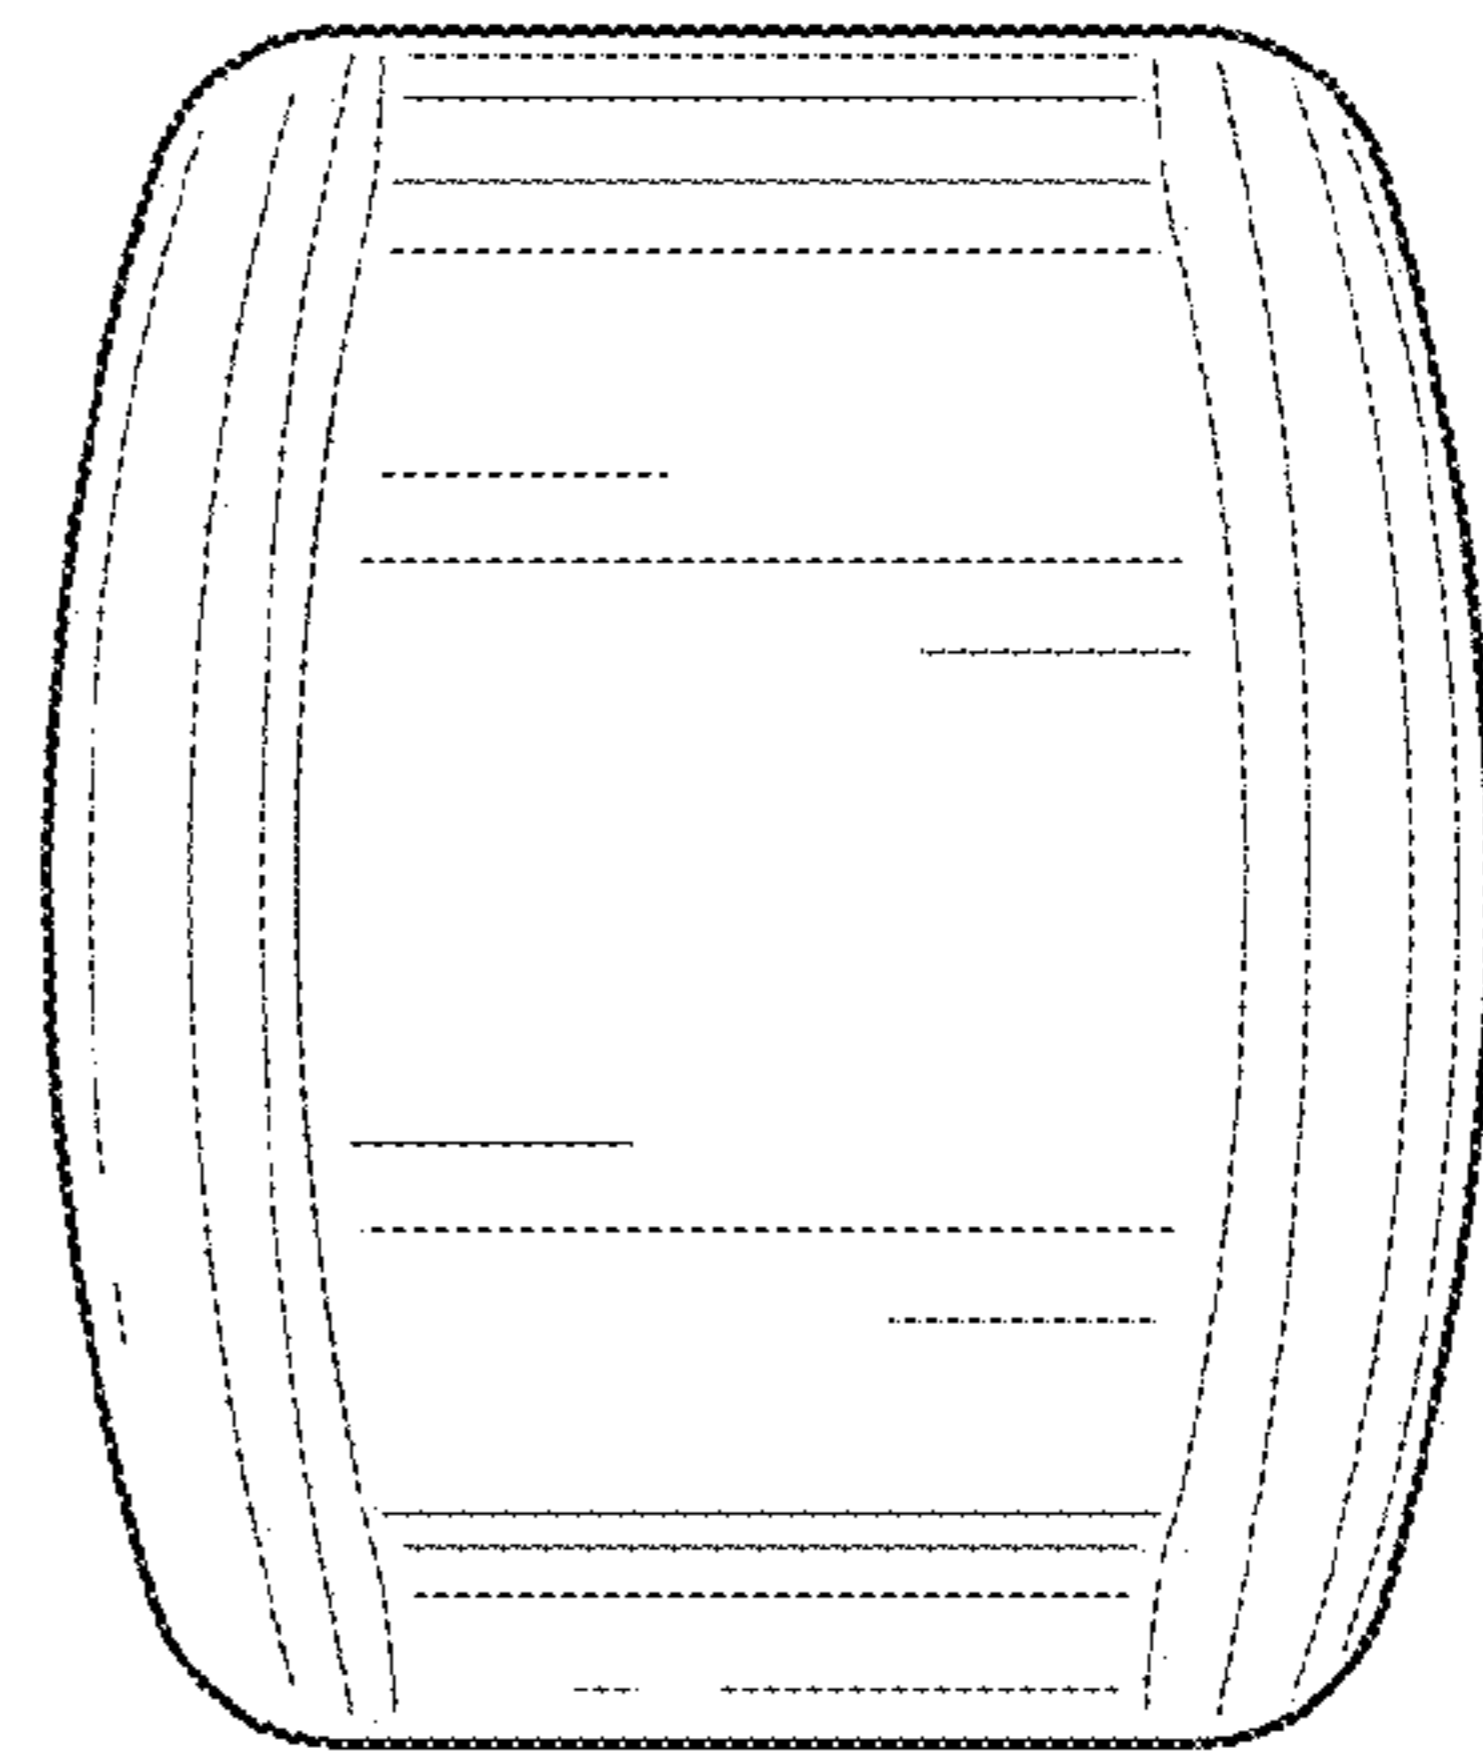


Fig. 5

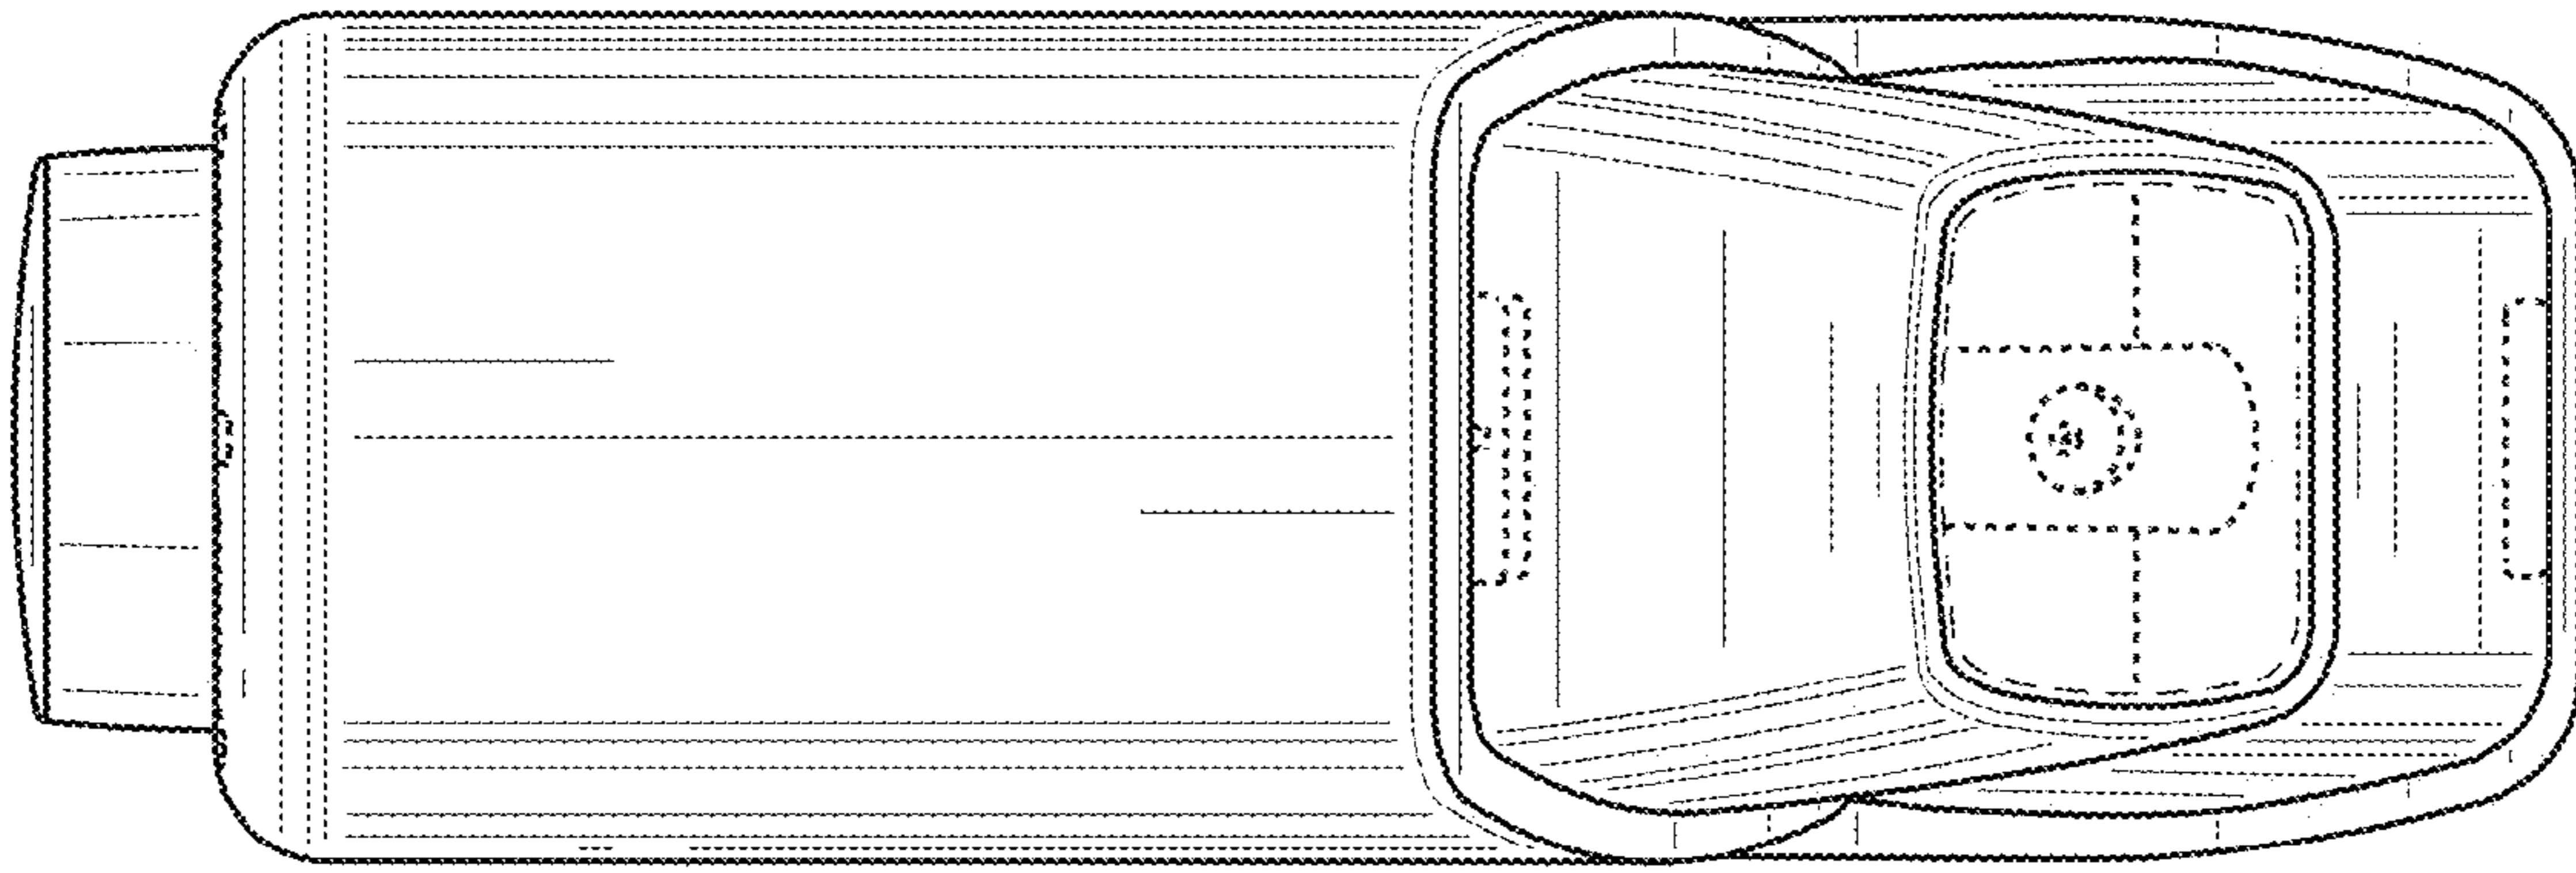


Fig. 8

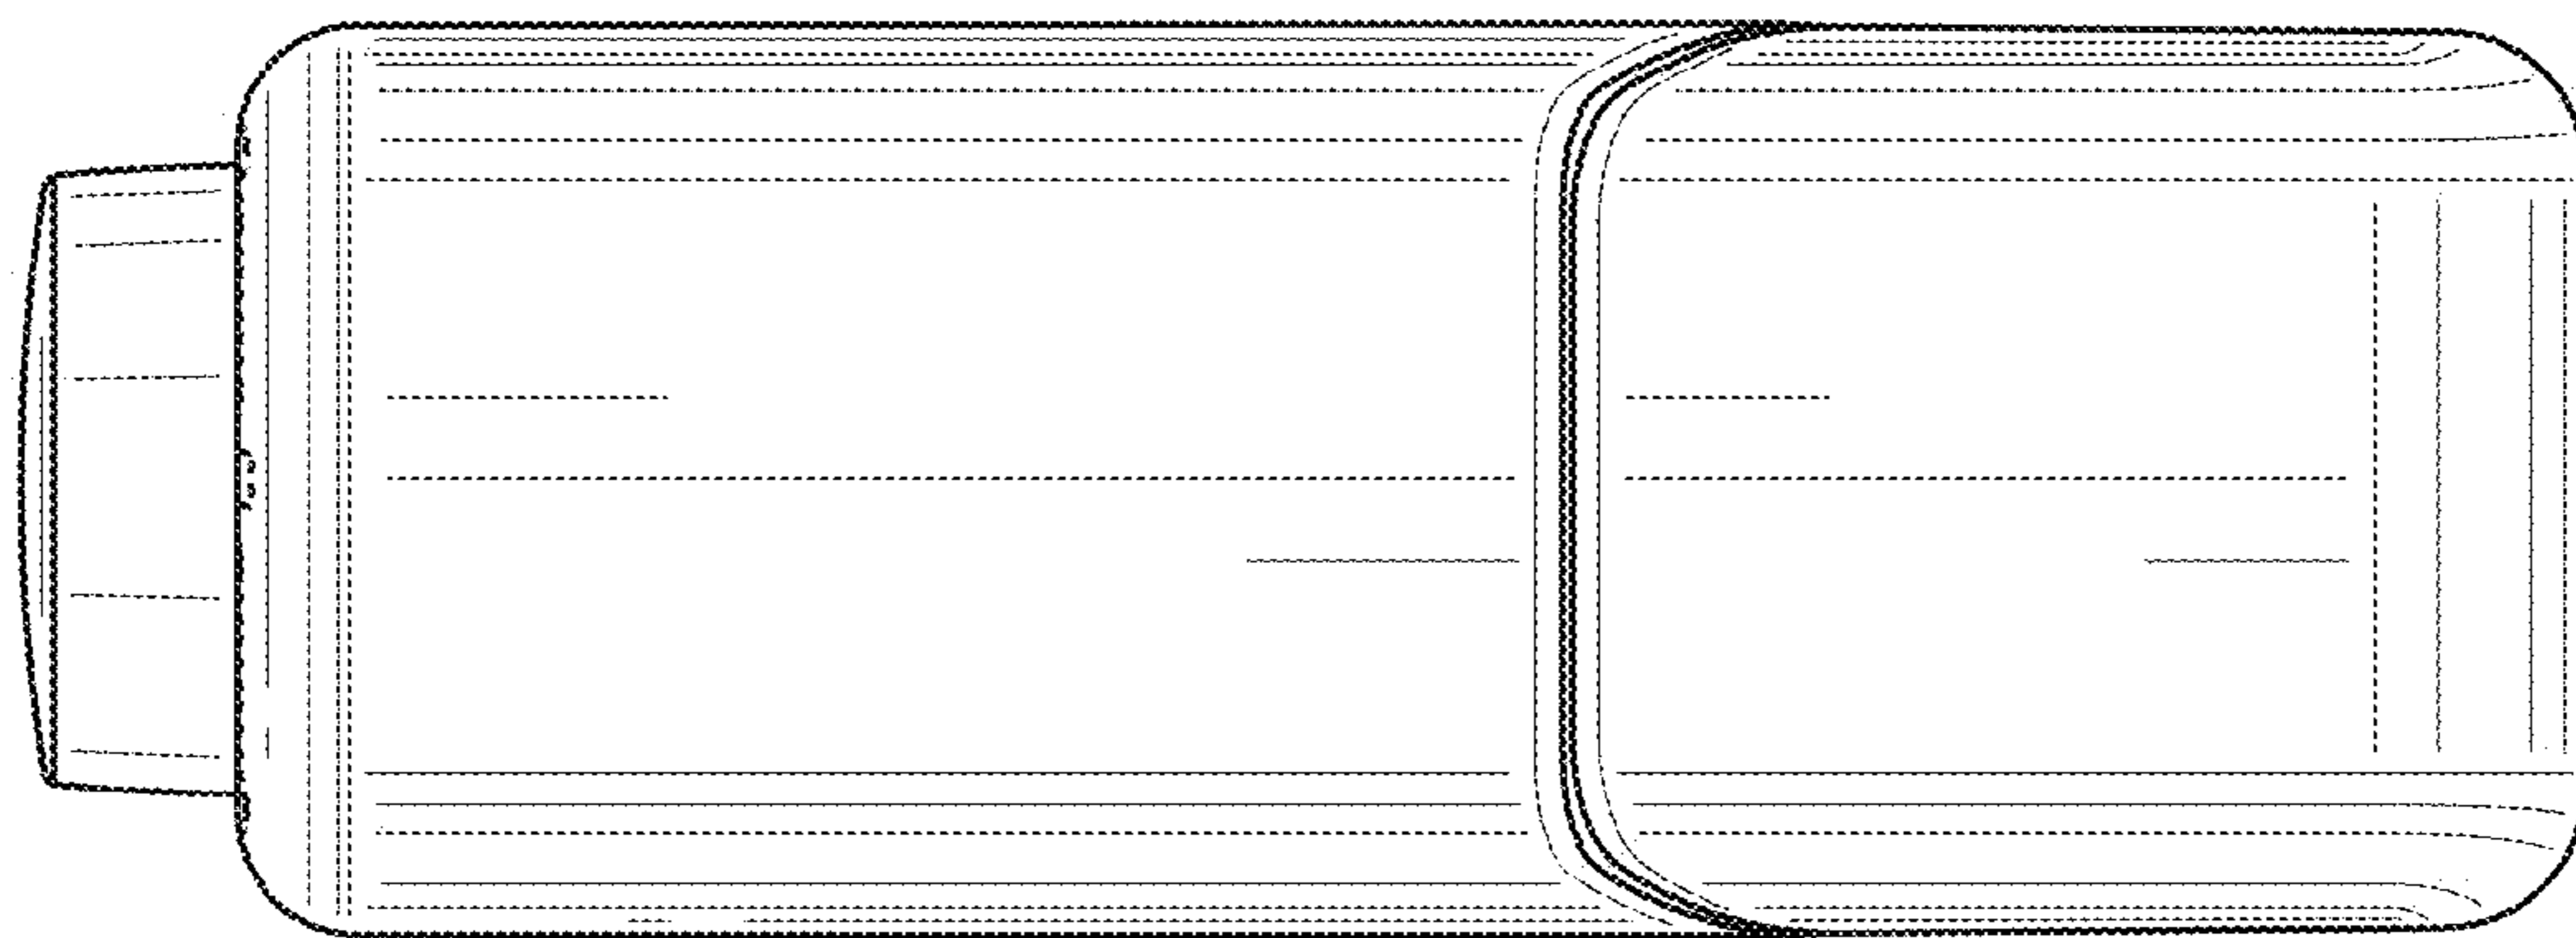


Fig. 7

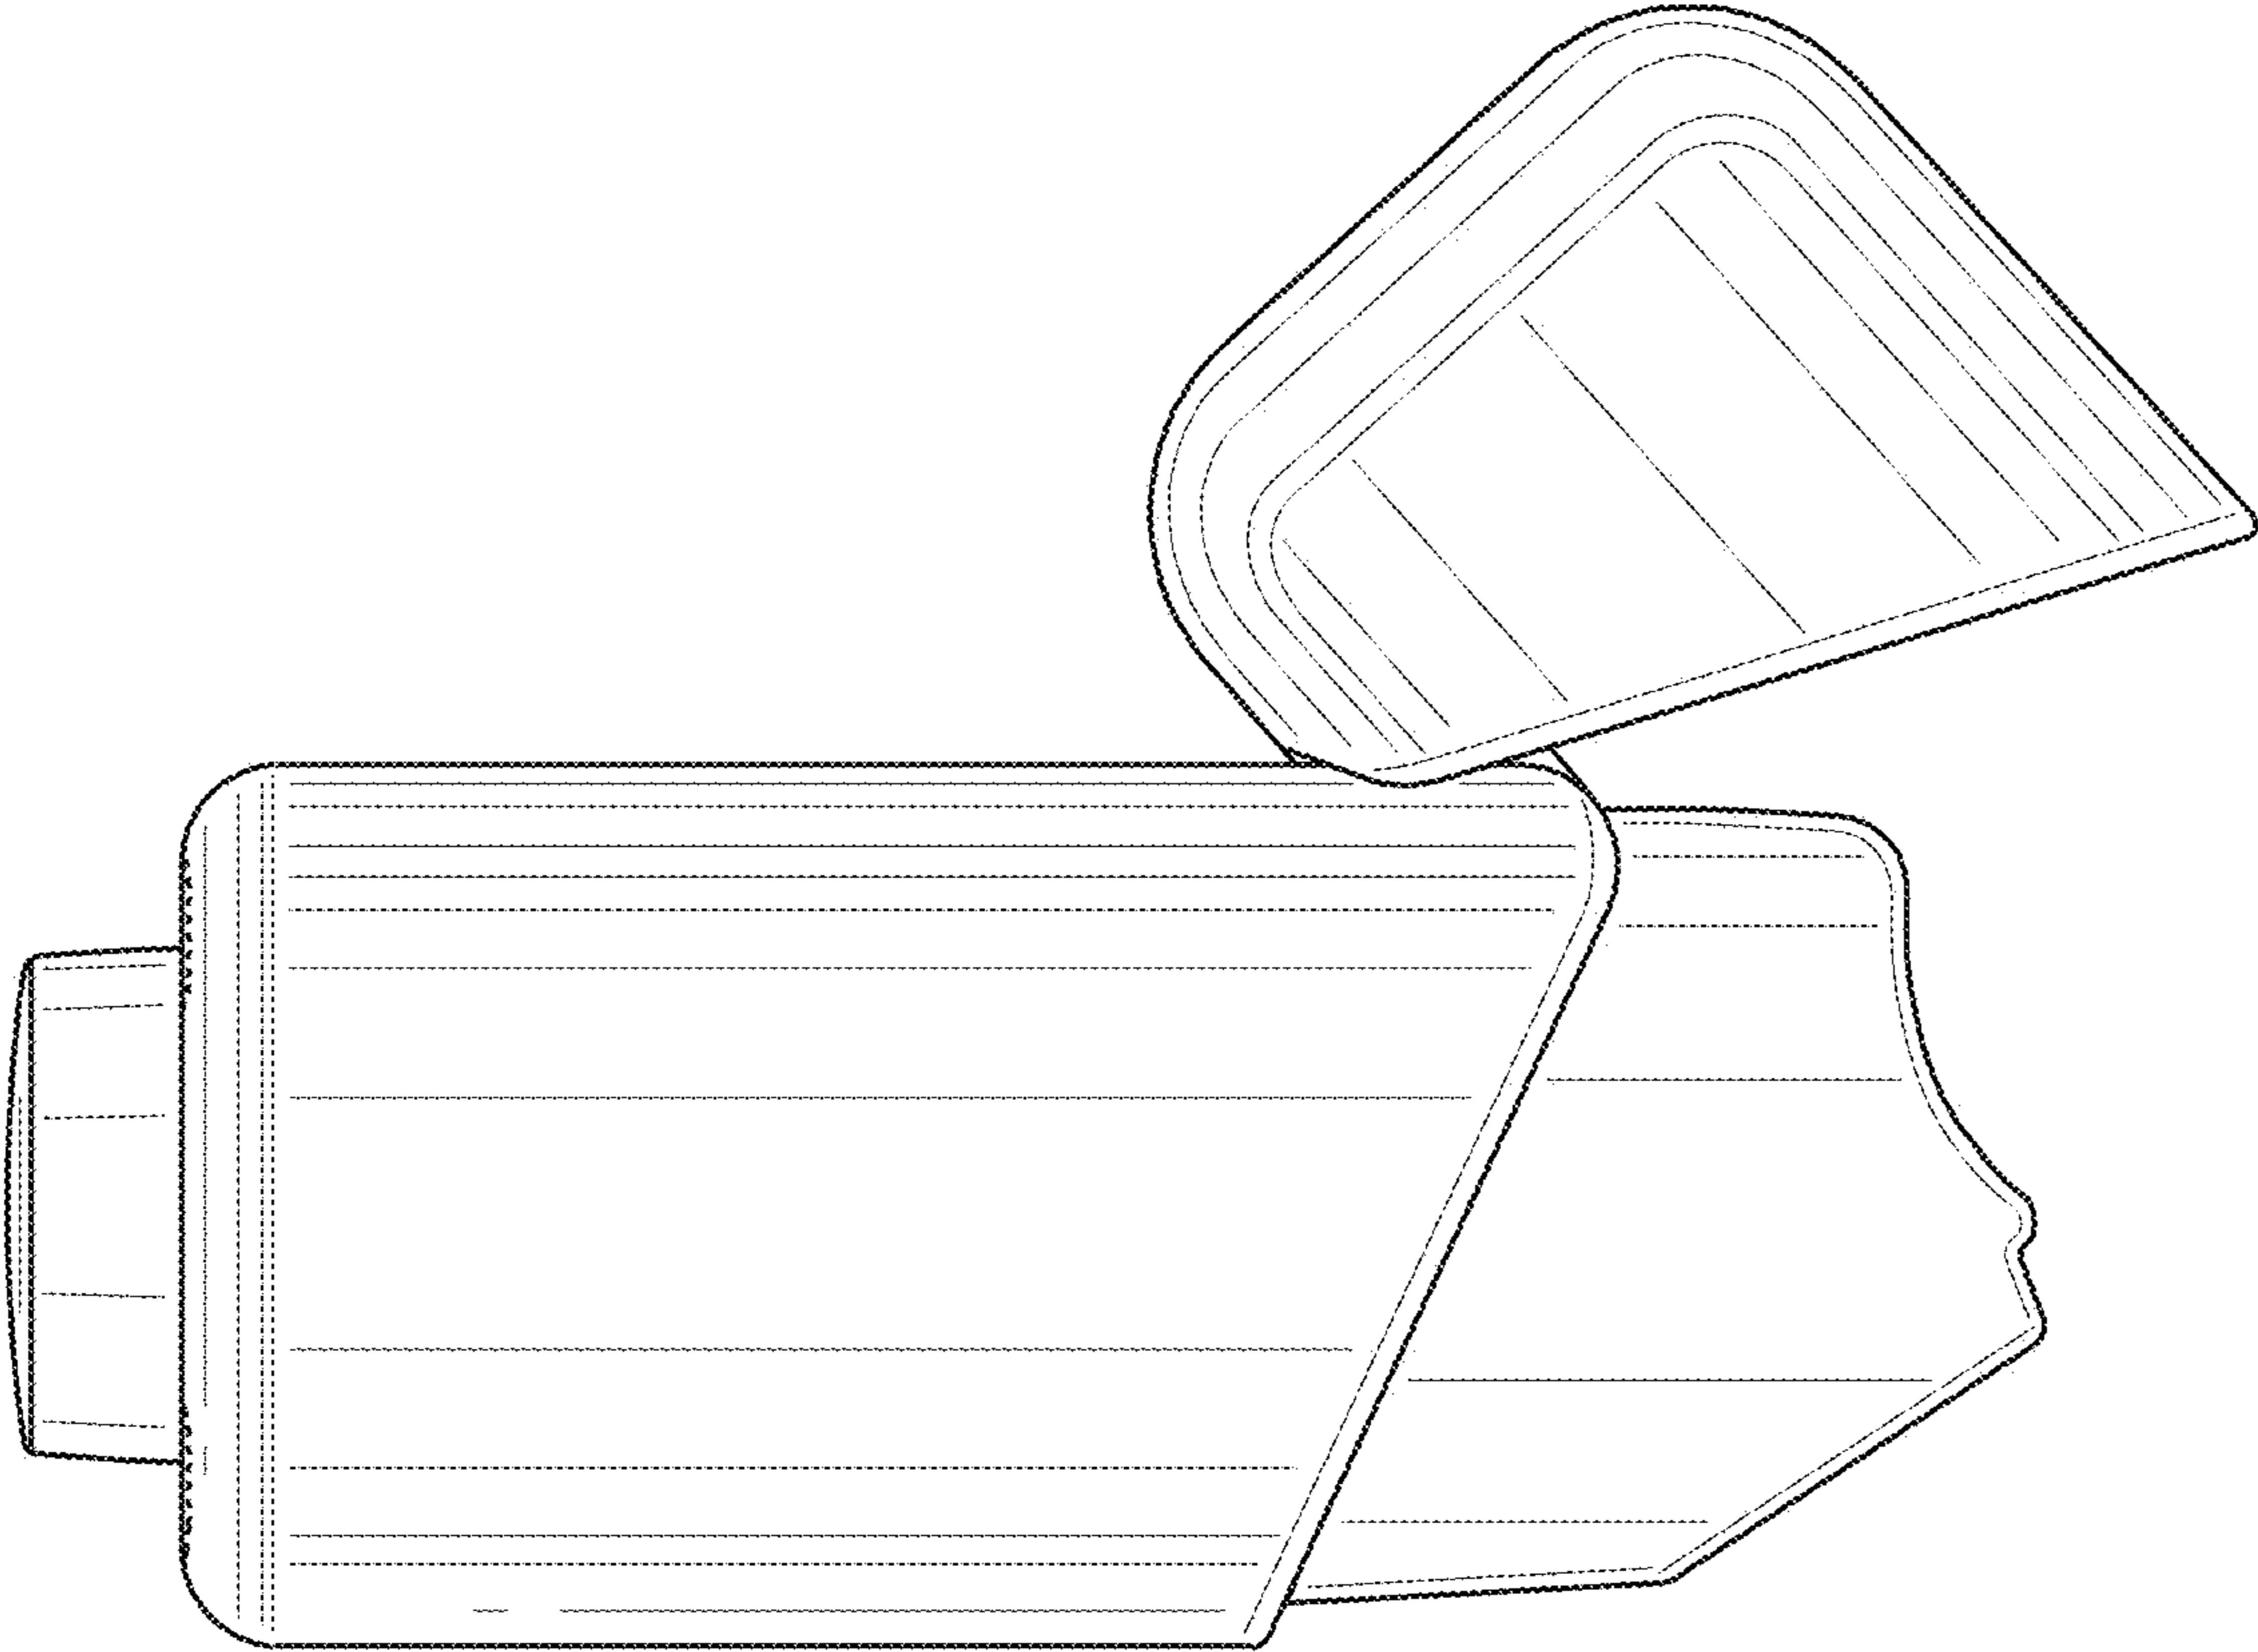


Fig. 9

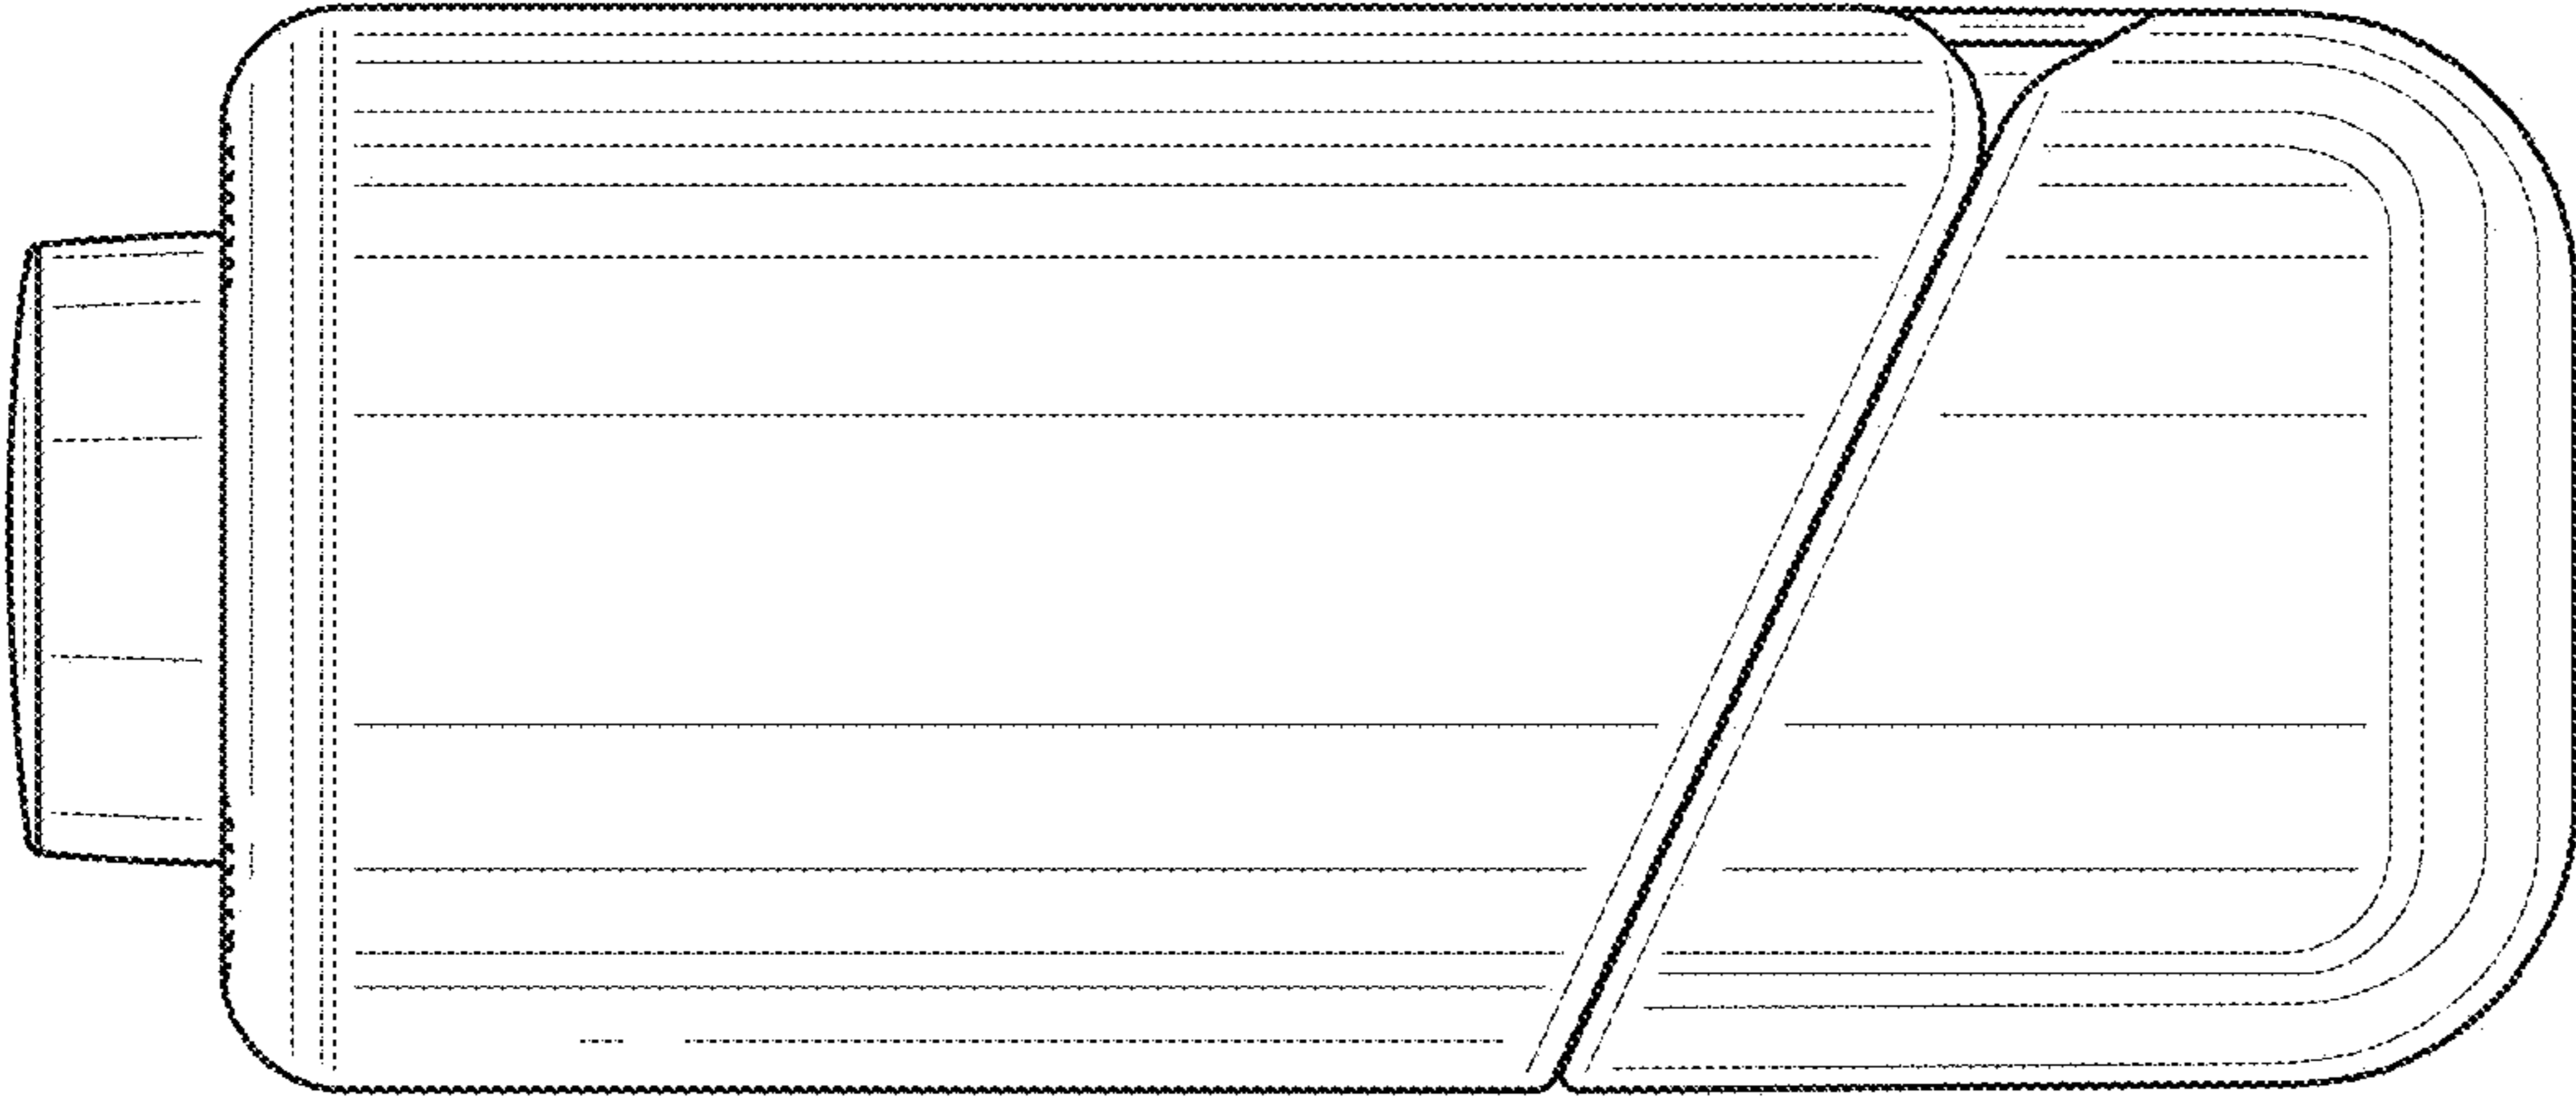


Fig. 10

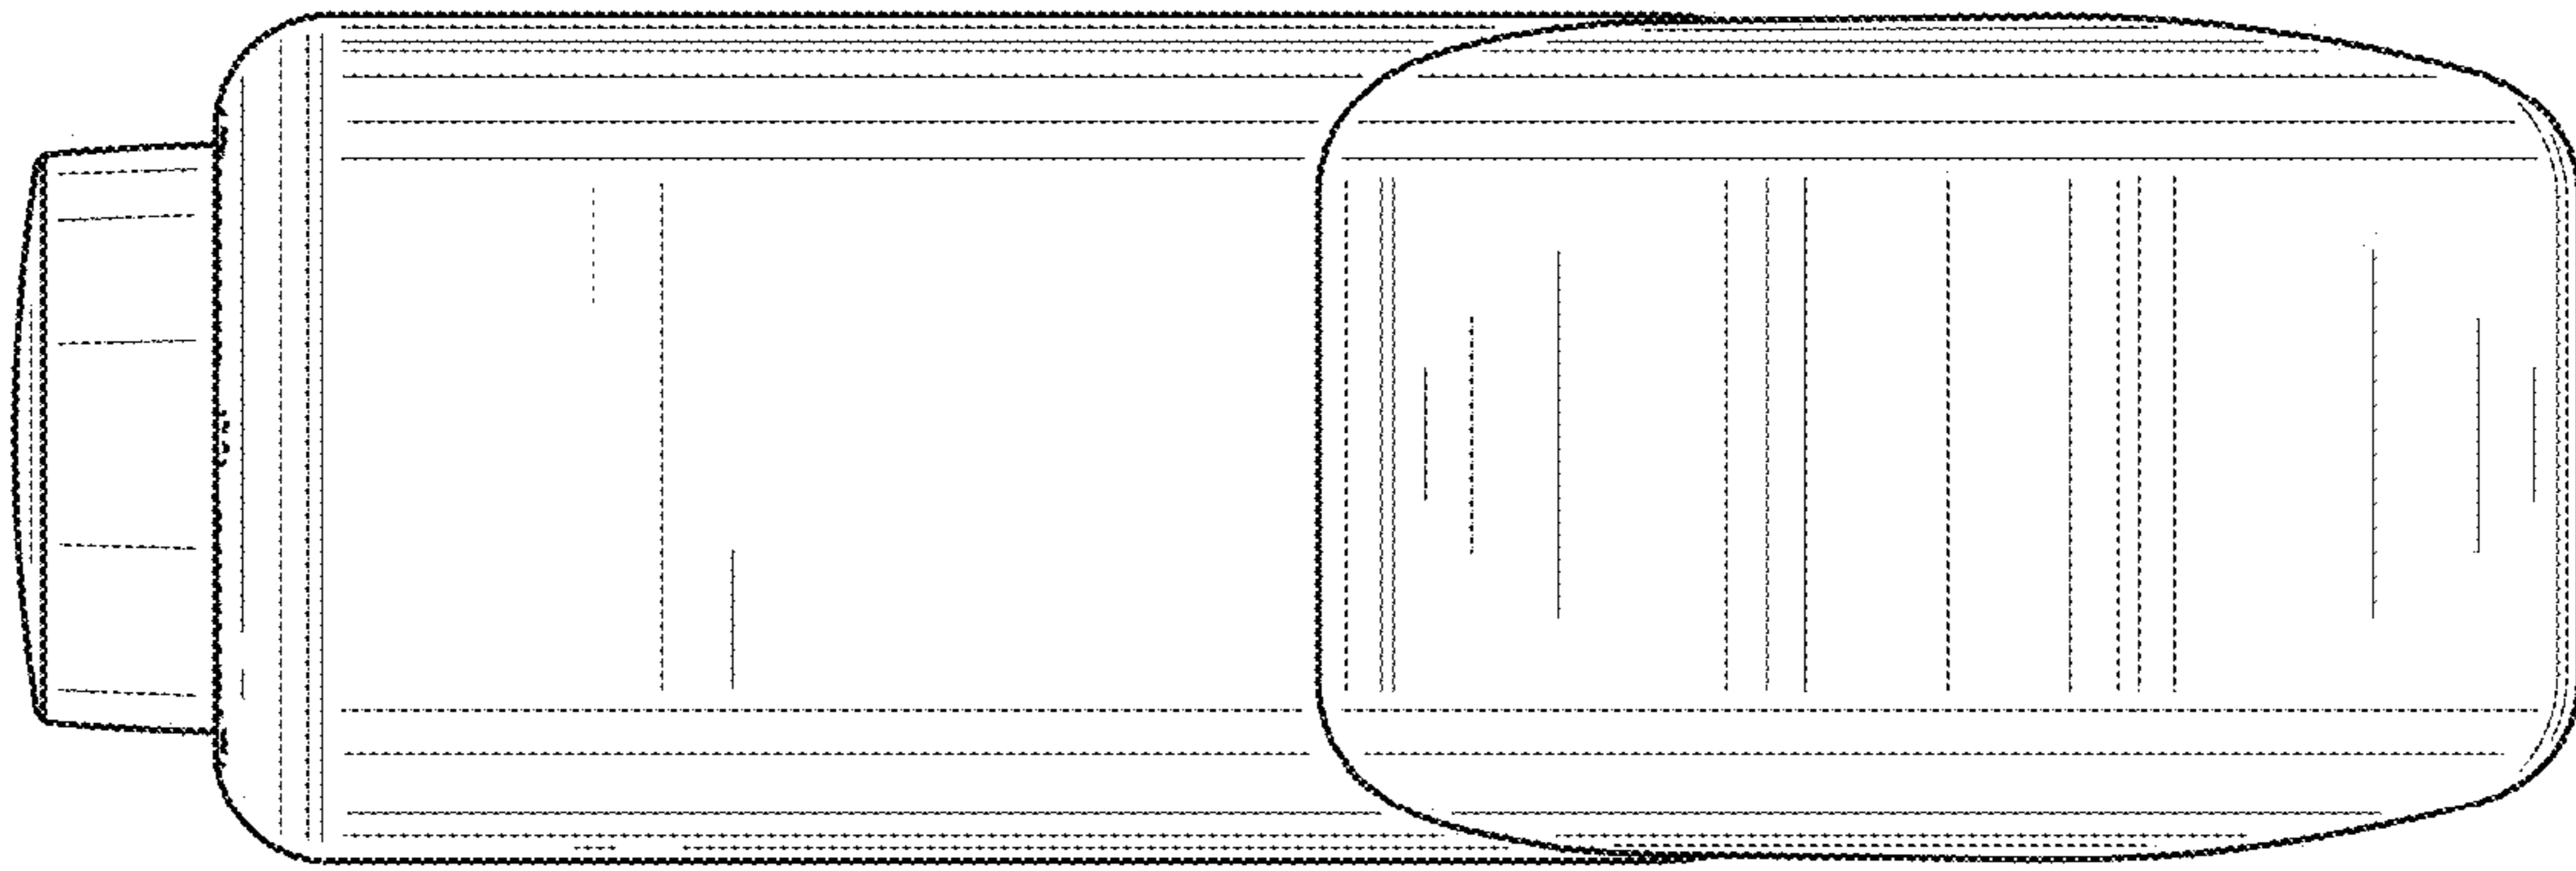


Fig. 12

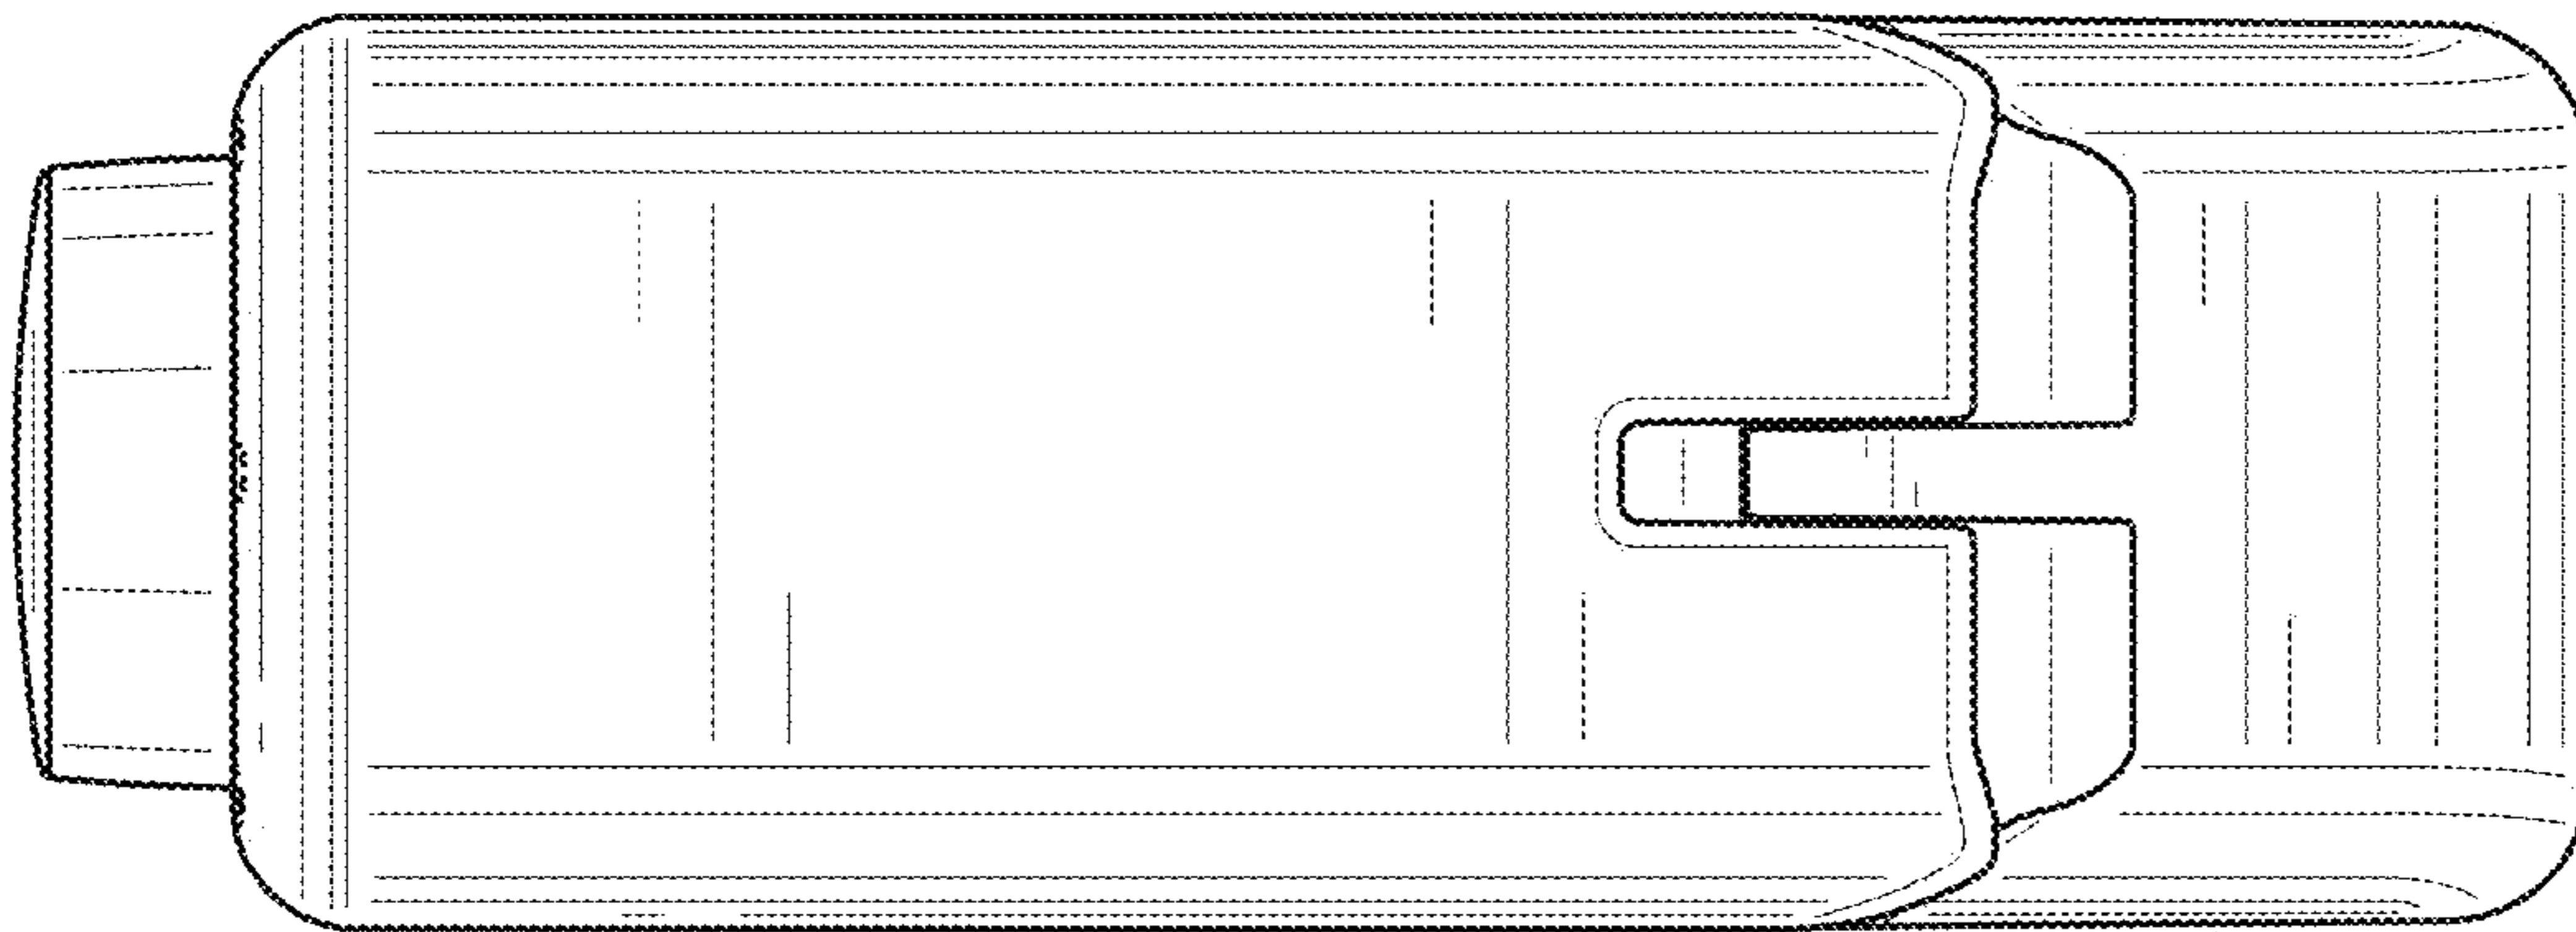


Fig. 11