



US00D877918S

(12) **United States Design Patent**  
**Siff**

(10) **Patent No.:** **US D877,918 S**  
(45) **Date of Patent:** **\*\* Mar. 10, 2020**

(54) **ELECTROTHERAPY AND  
NEUROSTIMULATION MEDICAL DEVICE**

(71) Applicant: **BioWave Corporation**, Norwalk, CT  
(US)

(72) Inventor: **Bradford Siff**, Norwalk, NY (US)

(73) Assignee: **BioWave Corporation**, Norwalk, CT  
(US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/667,557**

(22) Filed: **Oct. 23, 2018**

(51) **LOC (12) Cl.** ..... **28-03**

(52) **U.S. Cl.**  
USPC ..... **D24/200**

(58) **Field of Classification Search**  
USPC ..... D24/200, 214–215, 165, 185–186;  
607/46, 48–50, 51–56, 58, 72  
CPC .. A61N 1/36; A61N 1/36003; A61N 1/36014;  
A61N 1/0404; A61N 1/0456; A61N  
1/36021; A61N 5/0613; A61N 5/0616  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,989,605	A *	2/1991	Rossen	.....	A61N 1/36021 128/907
5,048,523	A *	9/1991	Yamasawa	.....	A61N 1/36021 607/66
D323,561	S *	1/1992	Bartelt	.....	D24/200
D363,553	S *	10/1995	Lee	.....	D24/200
6,393,325	B1 *	5/2002	Mann	.....	A61N 1/36071 607/46
D732,677	S *	6/2015	Kristensen	.....	D24/200

D813,405	S *	3/2018	Ho	.....	D24/200
D861,904	S *	10/2019	Ho	.....	D24/200
2006/0089683	A1 *	4/2006	Hagglof	.....	A61N 1/36021 607/48

\* cited by examiner

*Primary Examiner* — Wan Laymon

(74) *Attorney, Agent, or Firm* — Duane Morris LLP

(57) **CLAIM**

The ornamental design for an electrotherapy and neurostimulation medical device, as shown and described.

**DESCRIPTION**

FIG. 1 is an isometric view for the electrotherapy and neurostimulation medical device showing and embodying our new design;

FIG. 2 is front facing view of FIG. 1;

FIG. 3 is a back facing view of FIG. 1;

FIG. 4 is an enlarged right side view of FIG. 1;

FIG. 5 is an enlarged left side view of FIG. 1.

FIG. 6 is an enlarged top view of FIG. 1.

FIG. 7 is an enlarged bottom view of FIG. 1.

FIG. 8 is an isometric view for the electrotherapy and neurostimulation medical device showing and embodying our new design;

FIG. 9 is front facing view of FIG. 8;

FIG. 10 is a back facing view of FIG. 8;

FIG. 11 is an enlarged right side view of FIG. 8;


FIG. 12 is an enlarged left side view of FIG. 8.

FIG. 13 is an enlarged top view of FIG. 8; and,

FIG. 14 is an enlarged bottom view of FIG. 8.

The broken lines shown in the drawings illustrate portions of the electrotherapy and neurostimulation medical device that form no part of the claimed design. FIGS. 8-14 are identical to FIGS. 1-7 with the exception of additionally claiming five LED lights on the front face of the device.

**1 Claim, 14 Drawing Sheets**

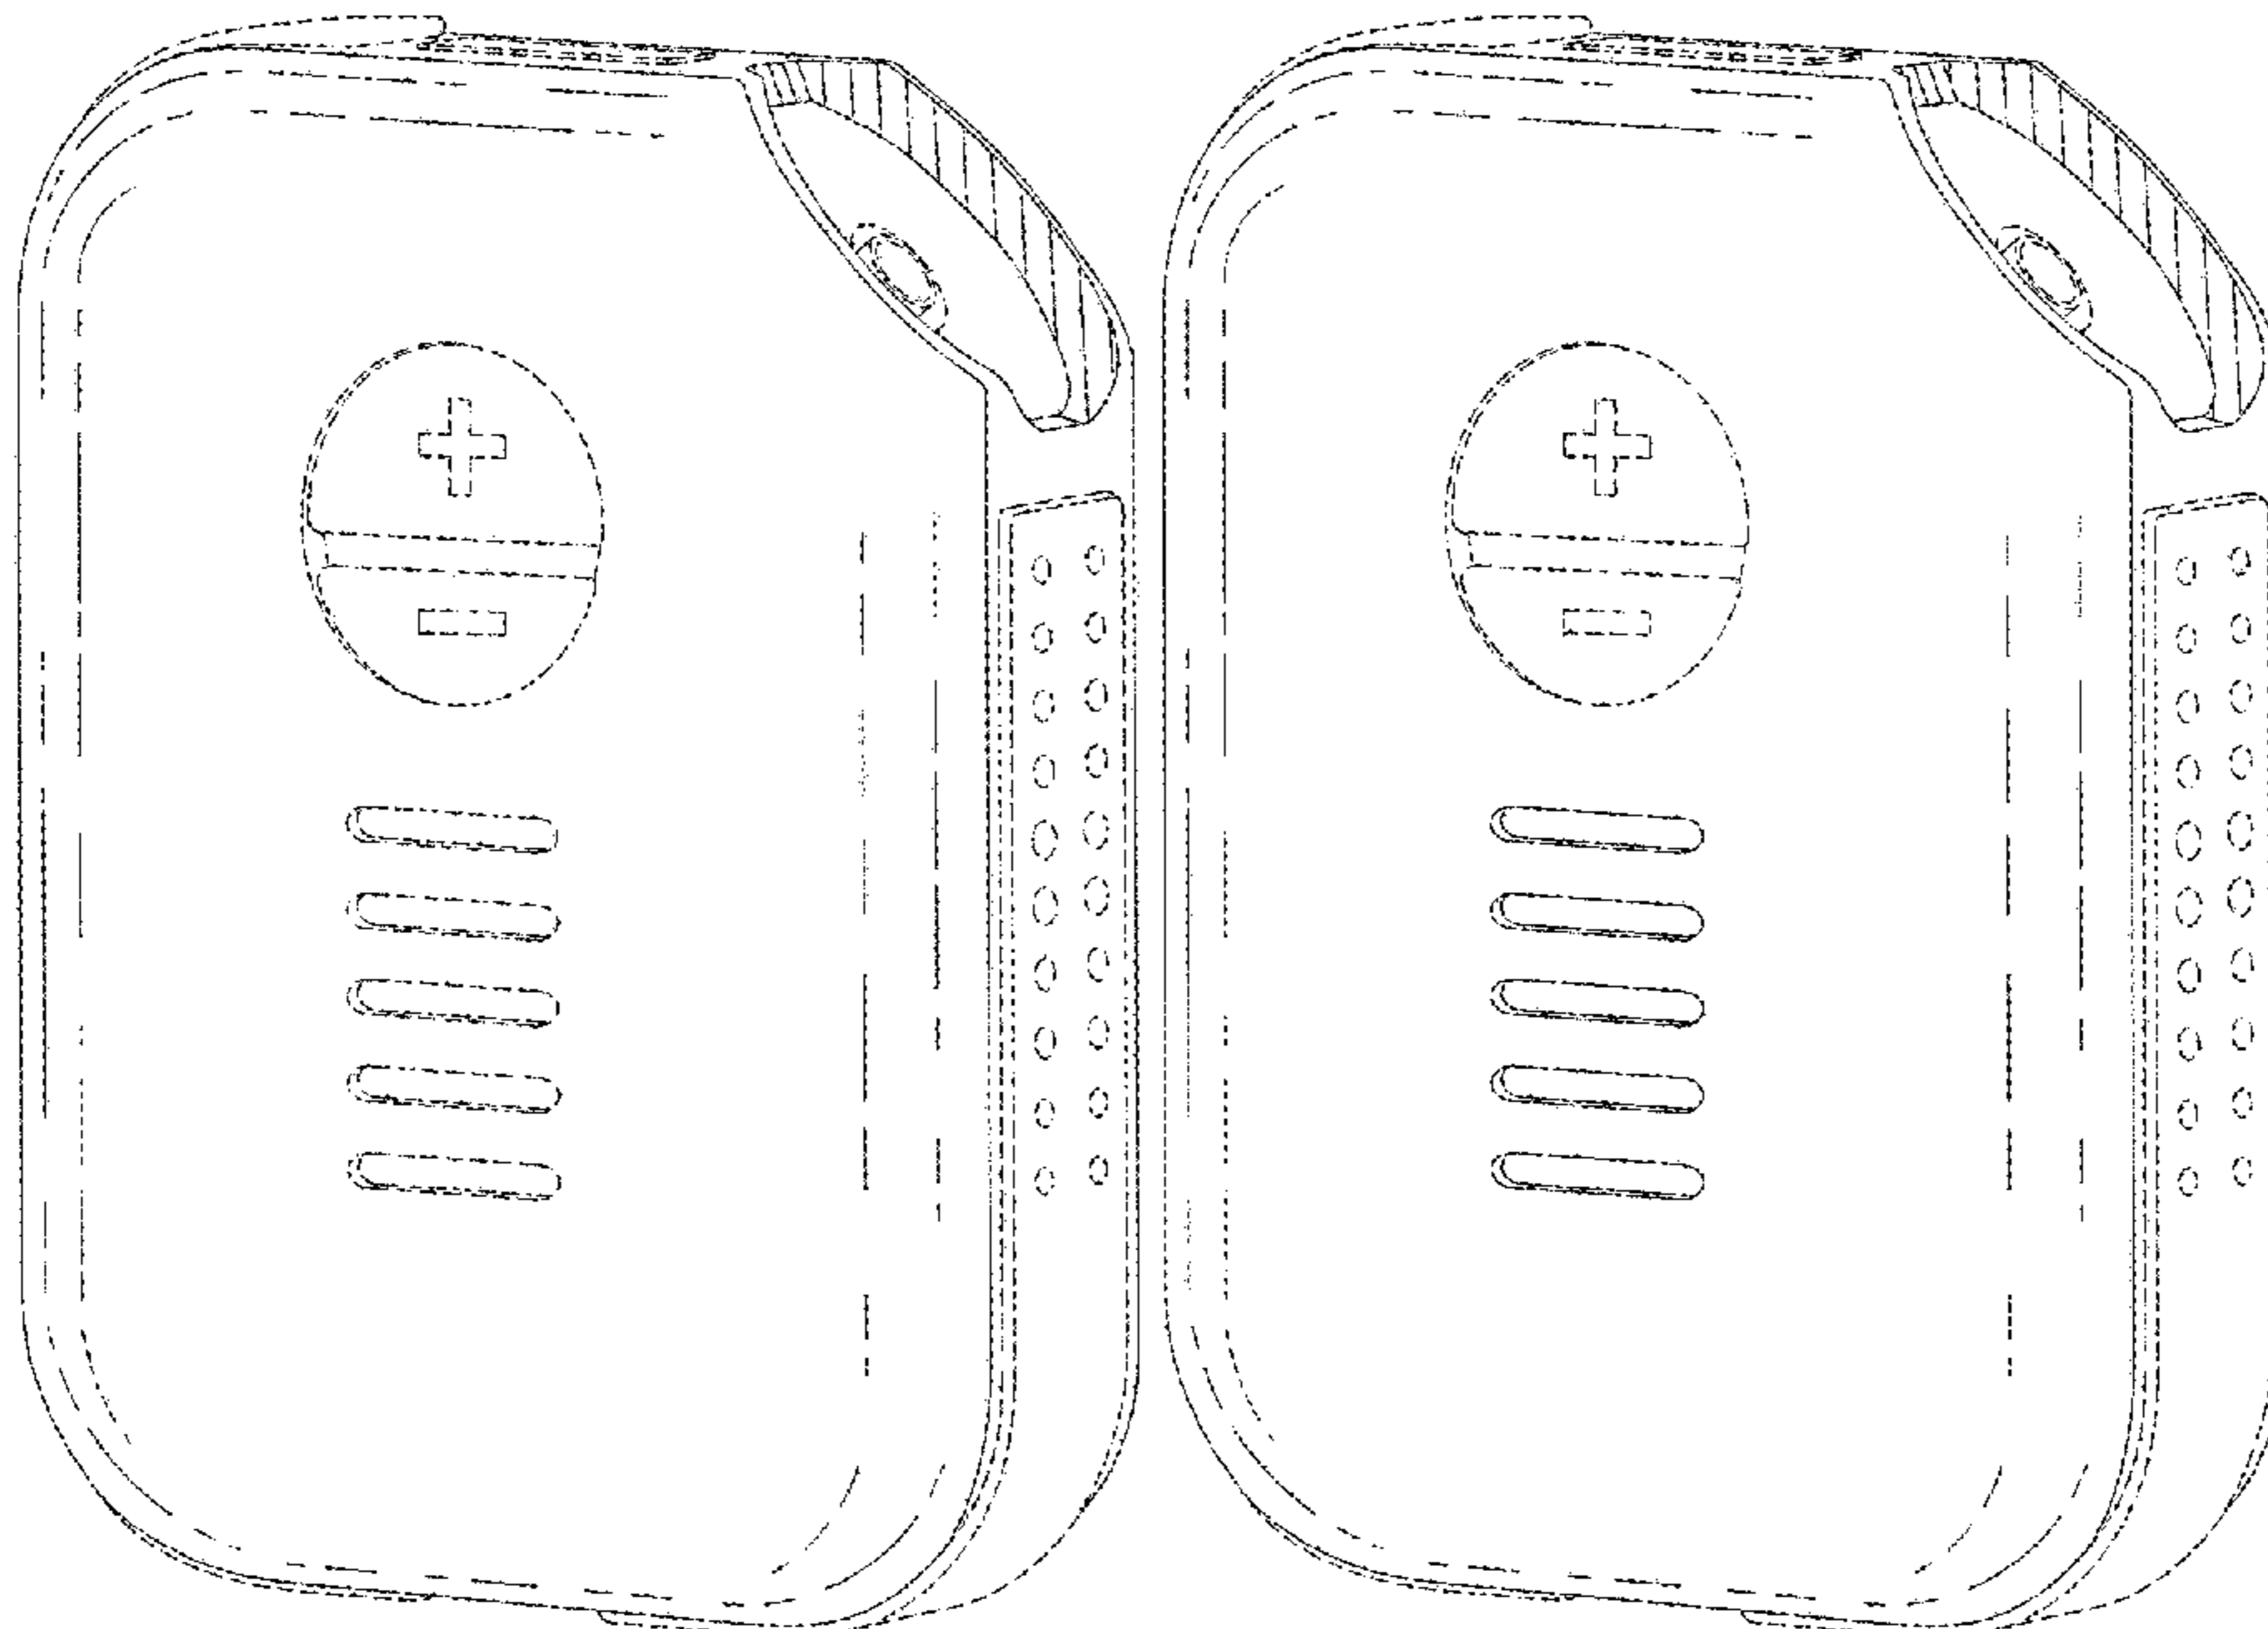

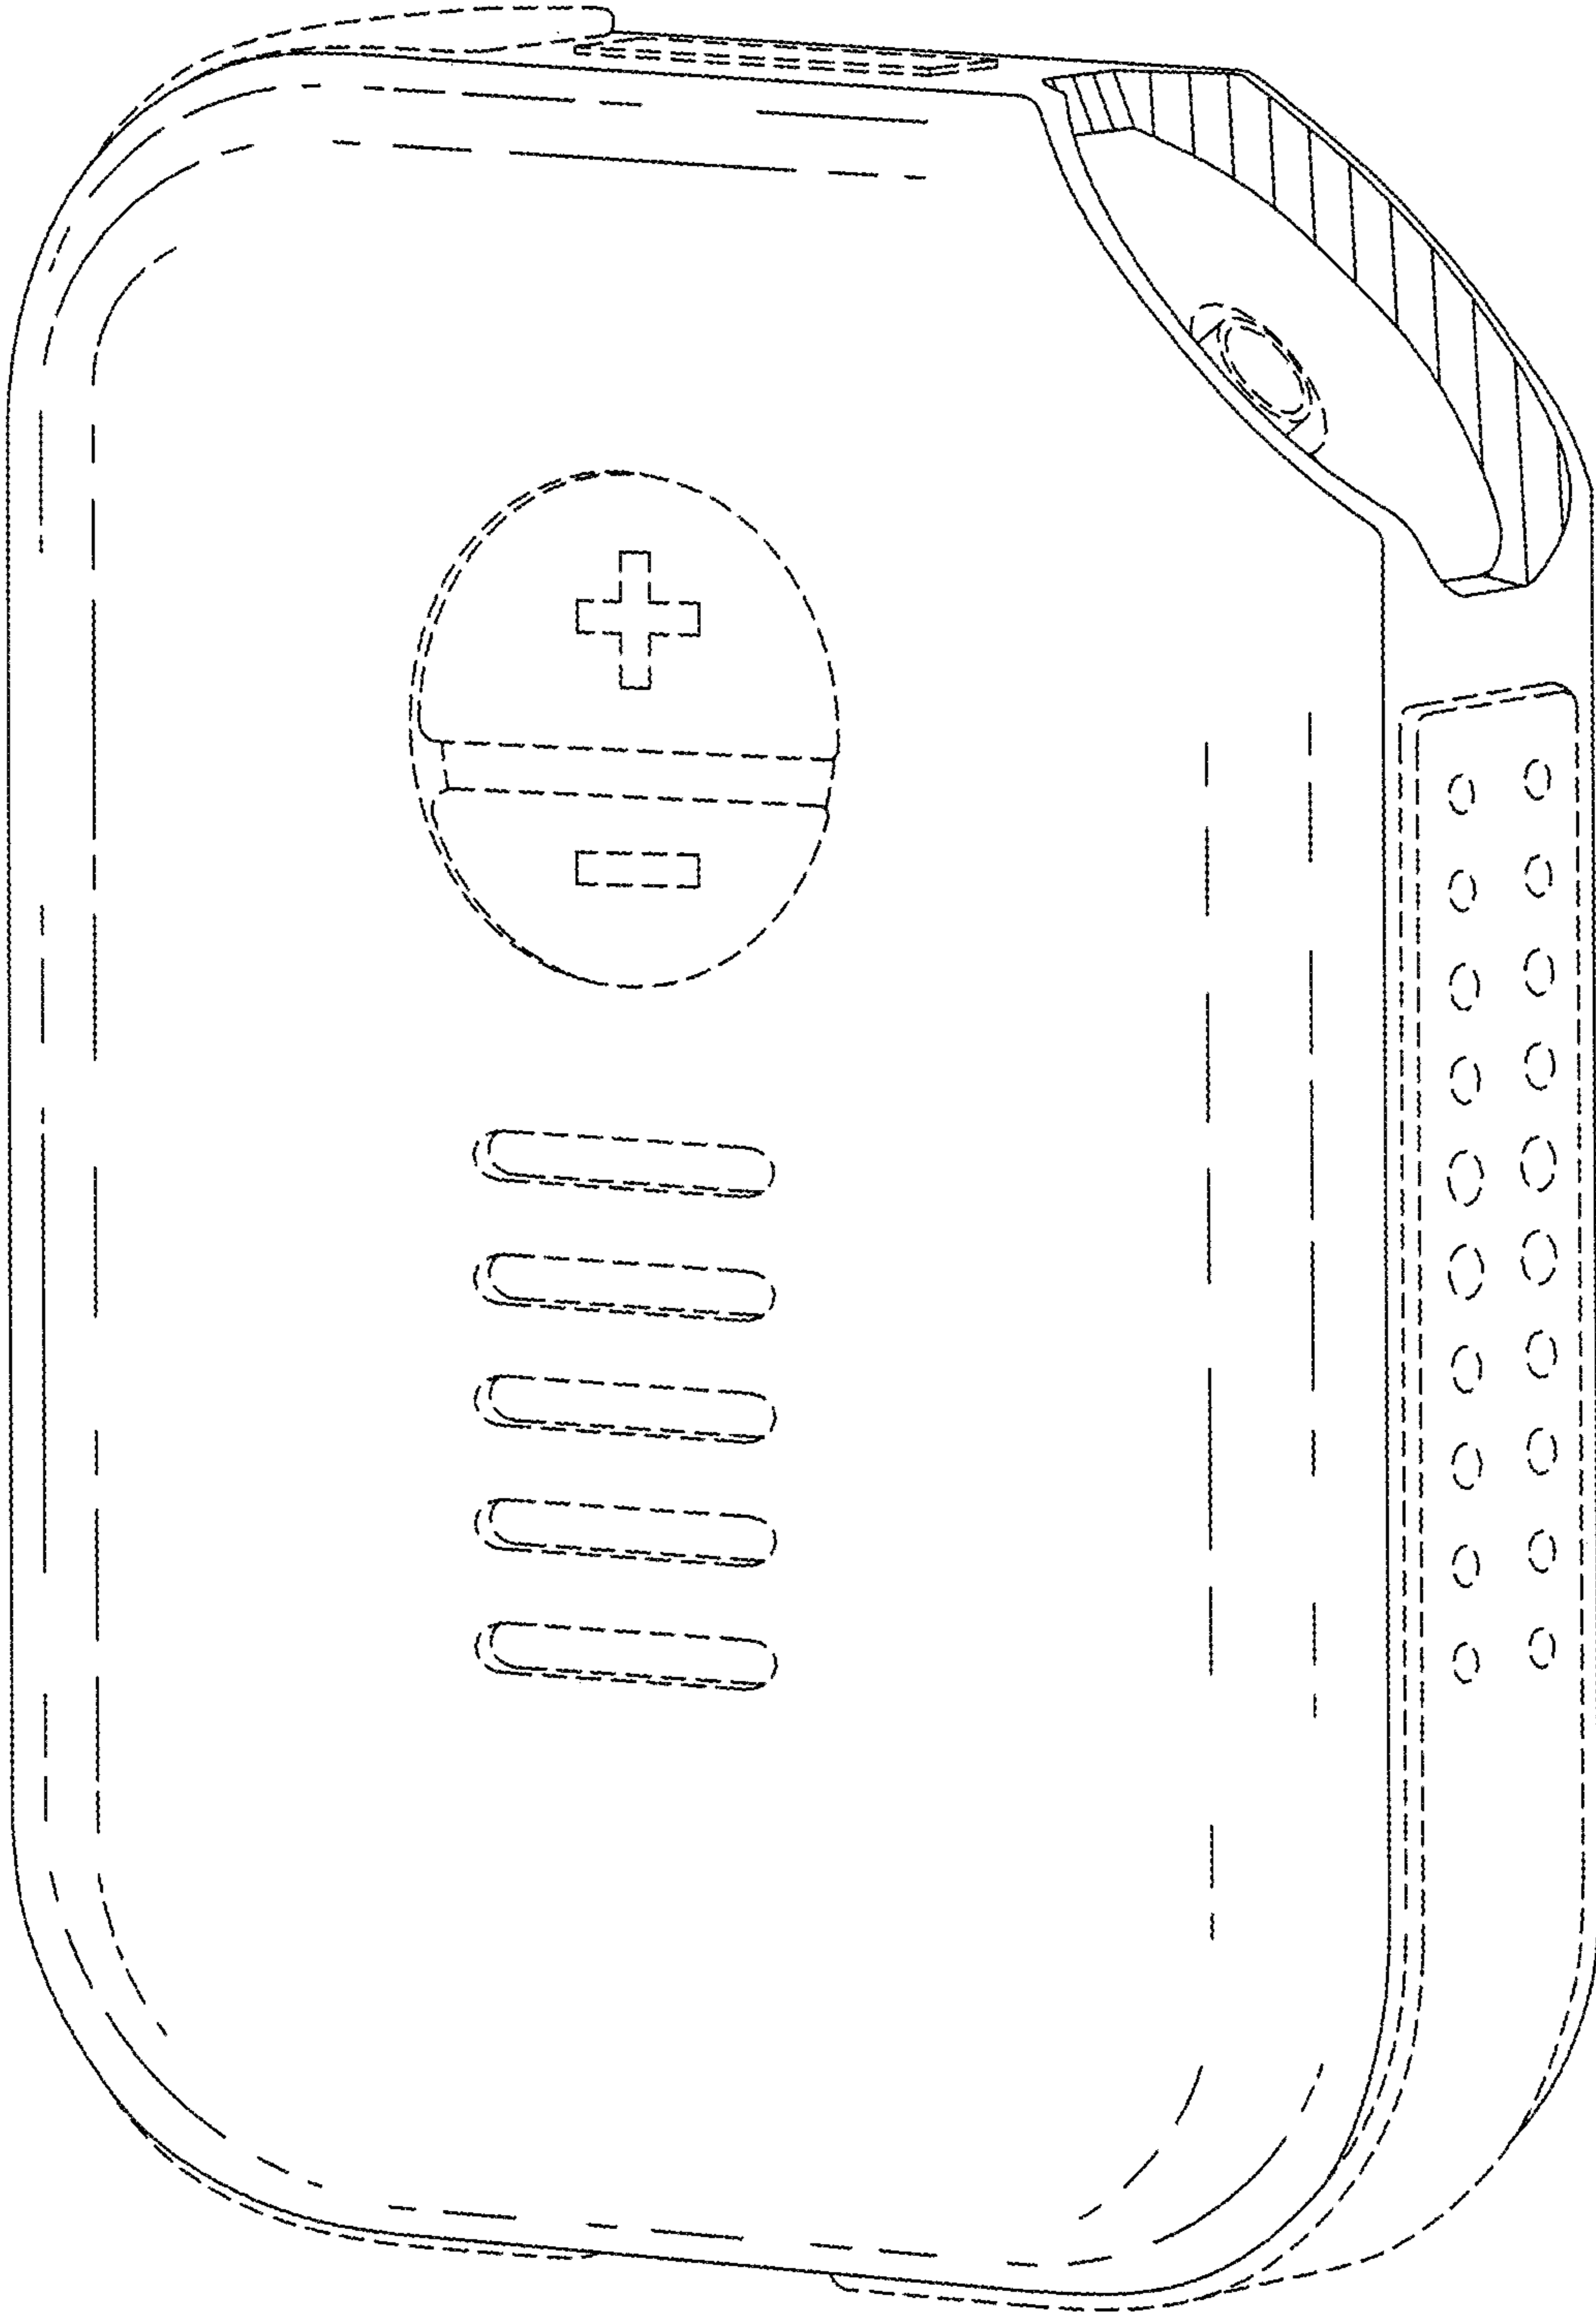


FIG. 1

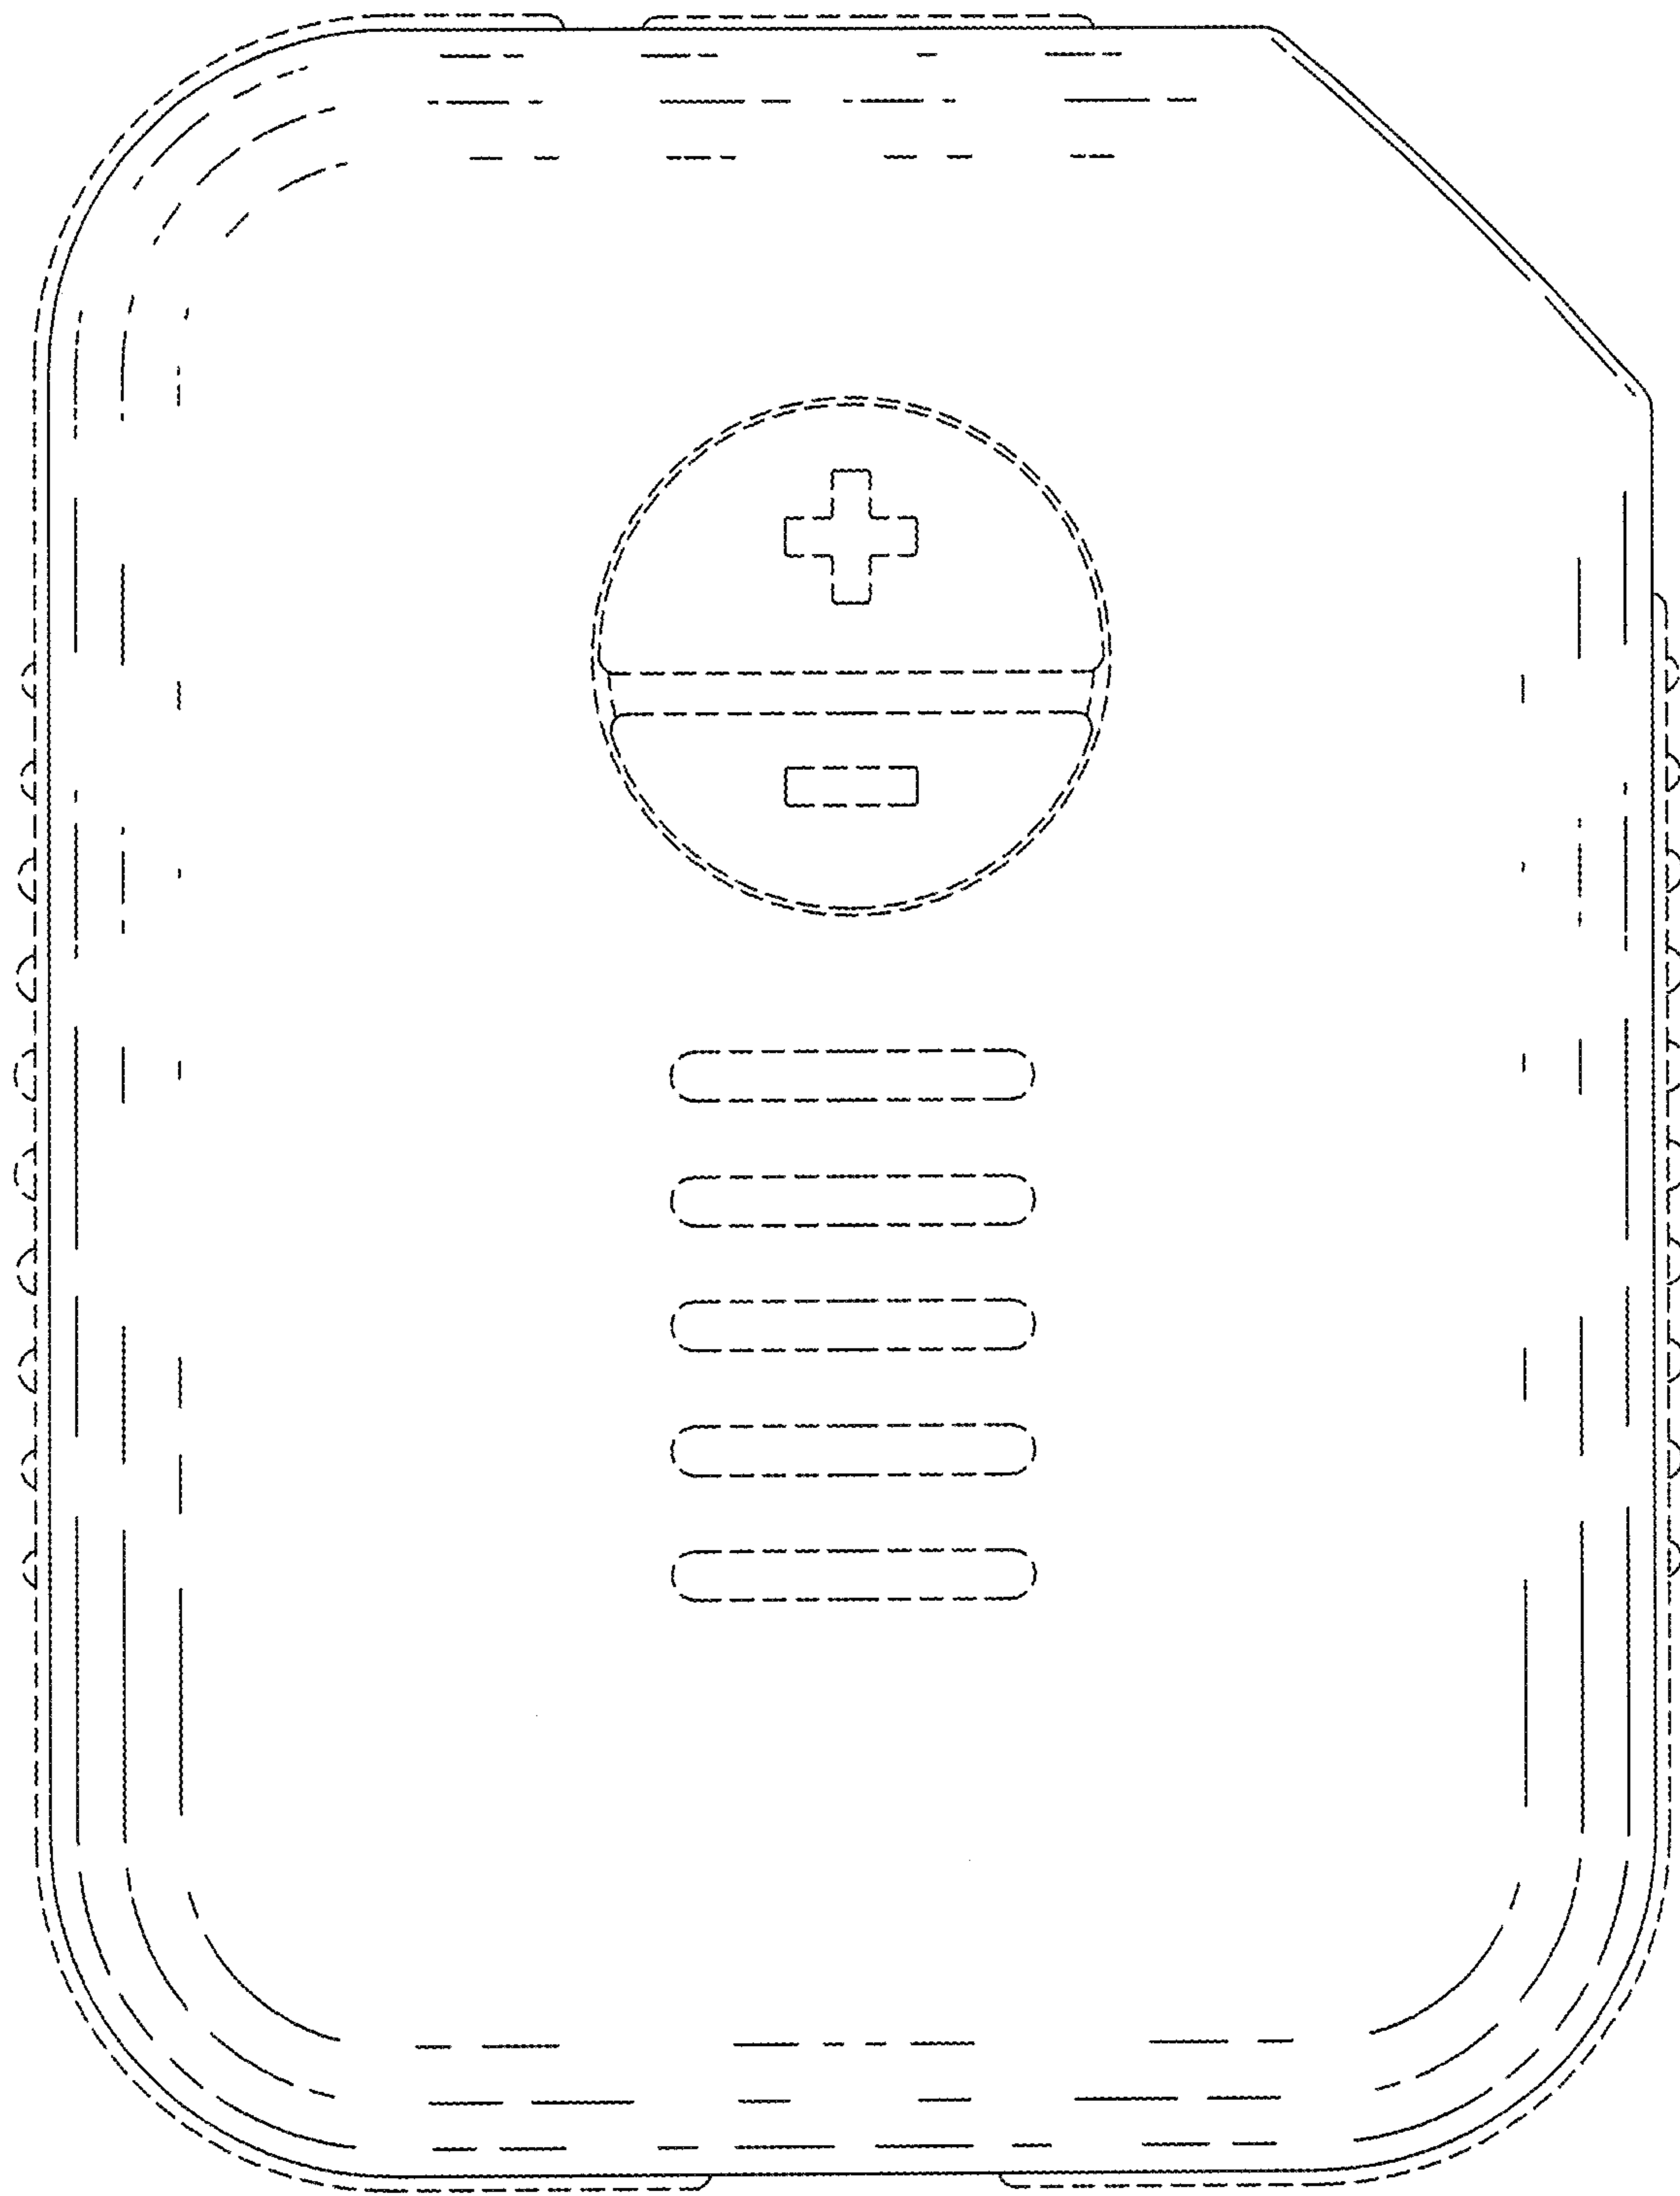


FIG. 2

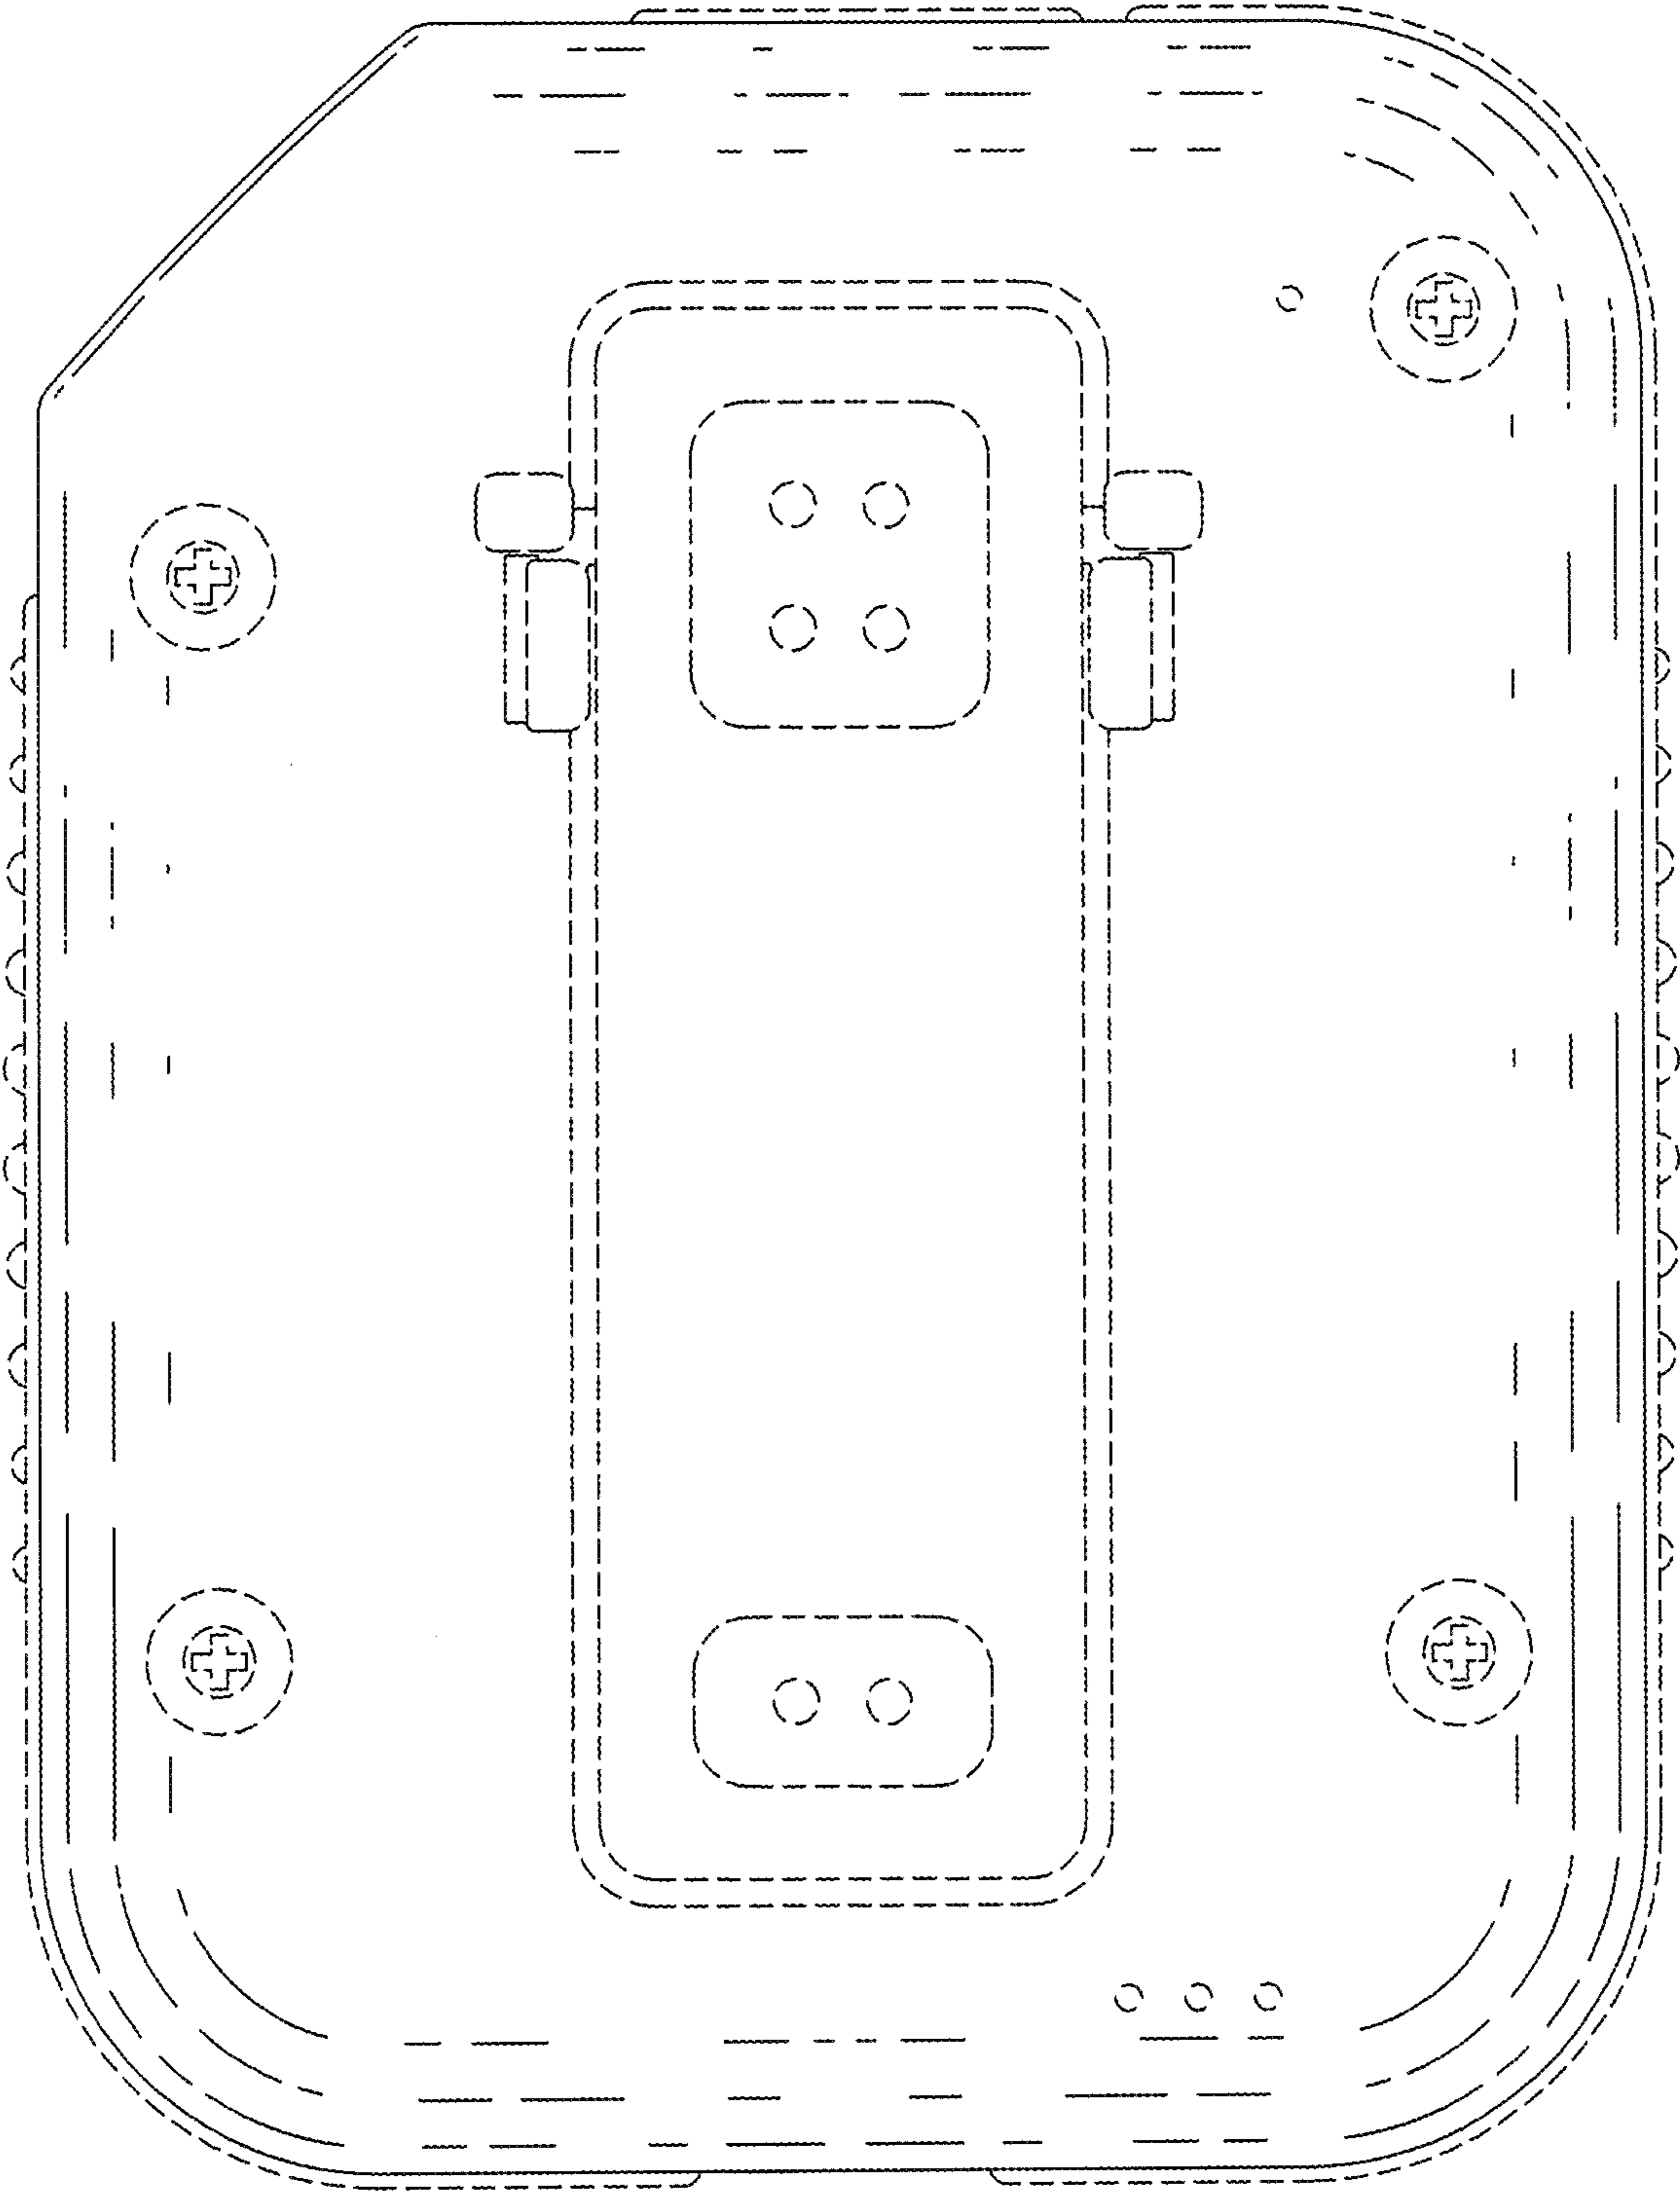


FIG. 3



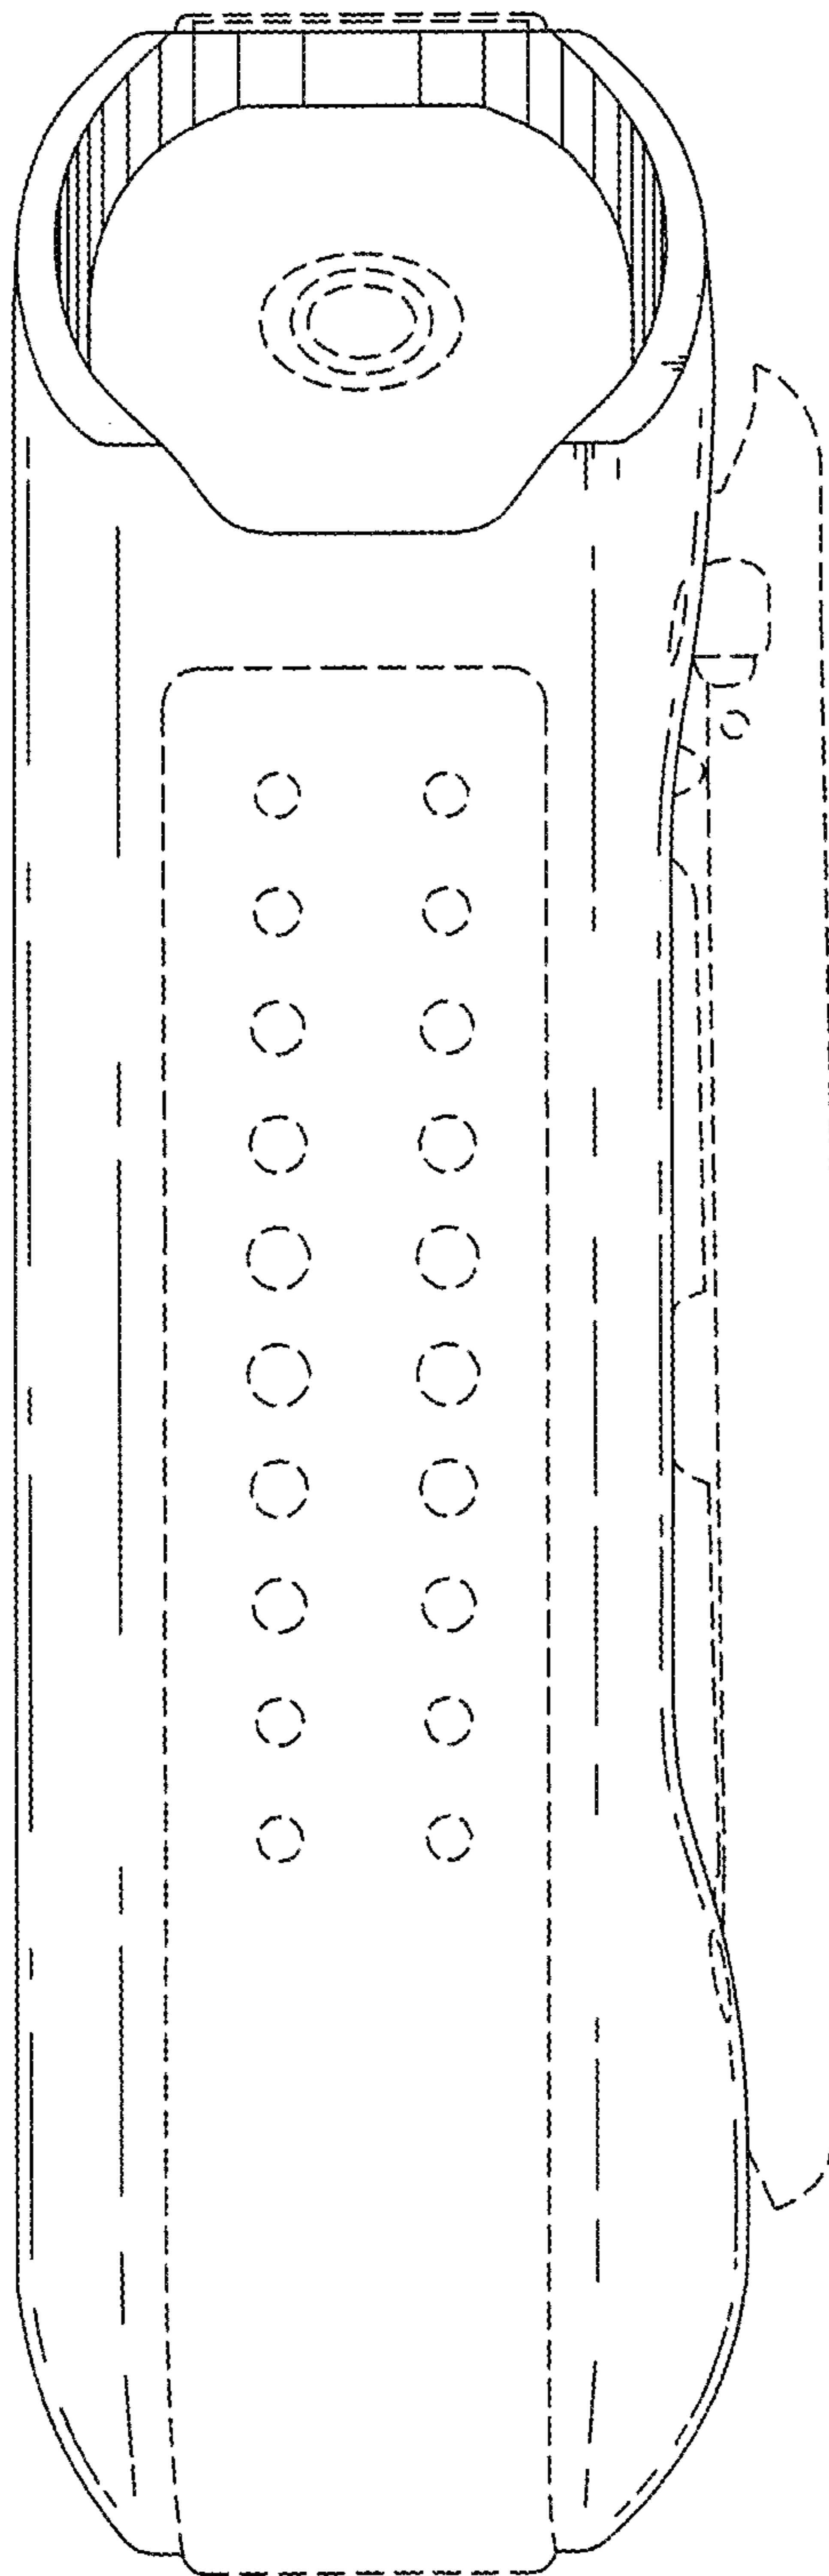


FIG. 4

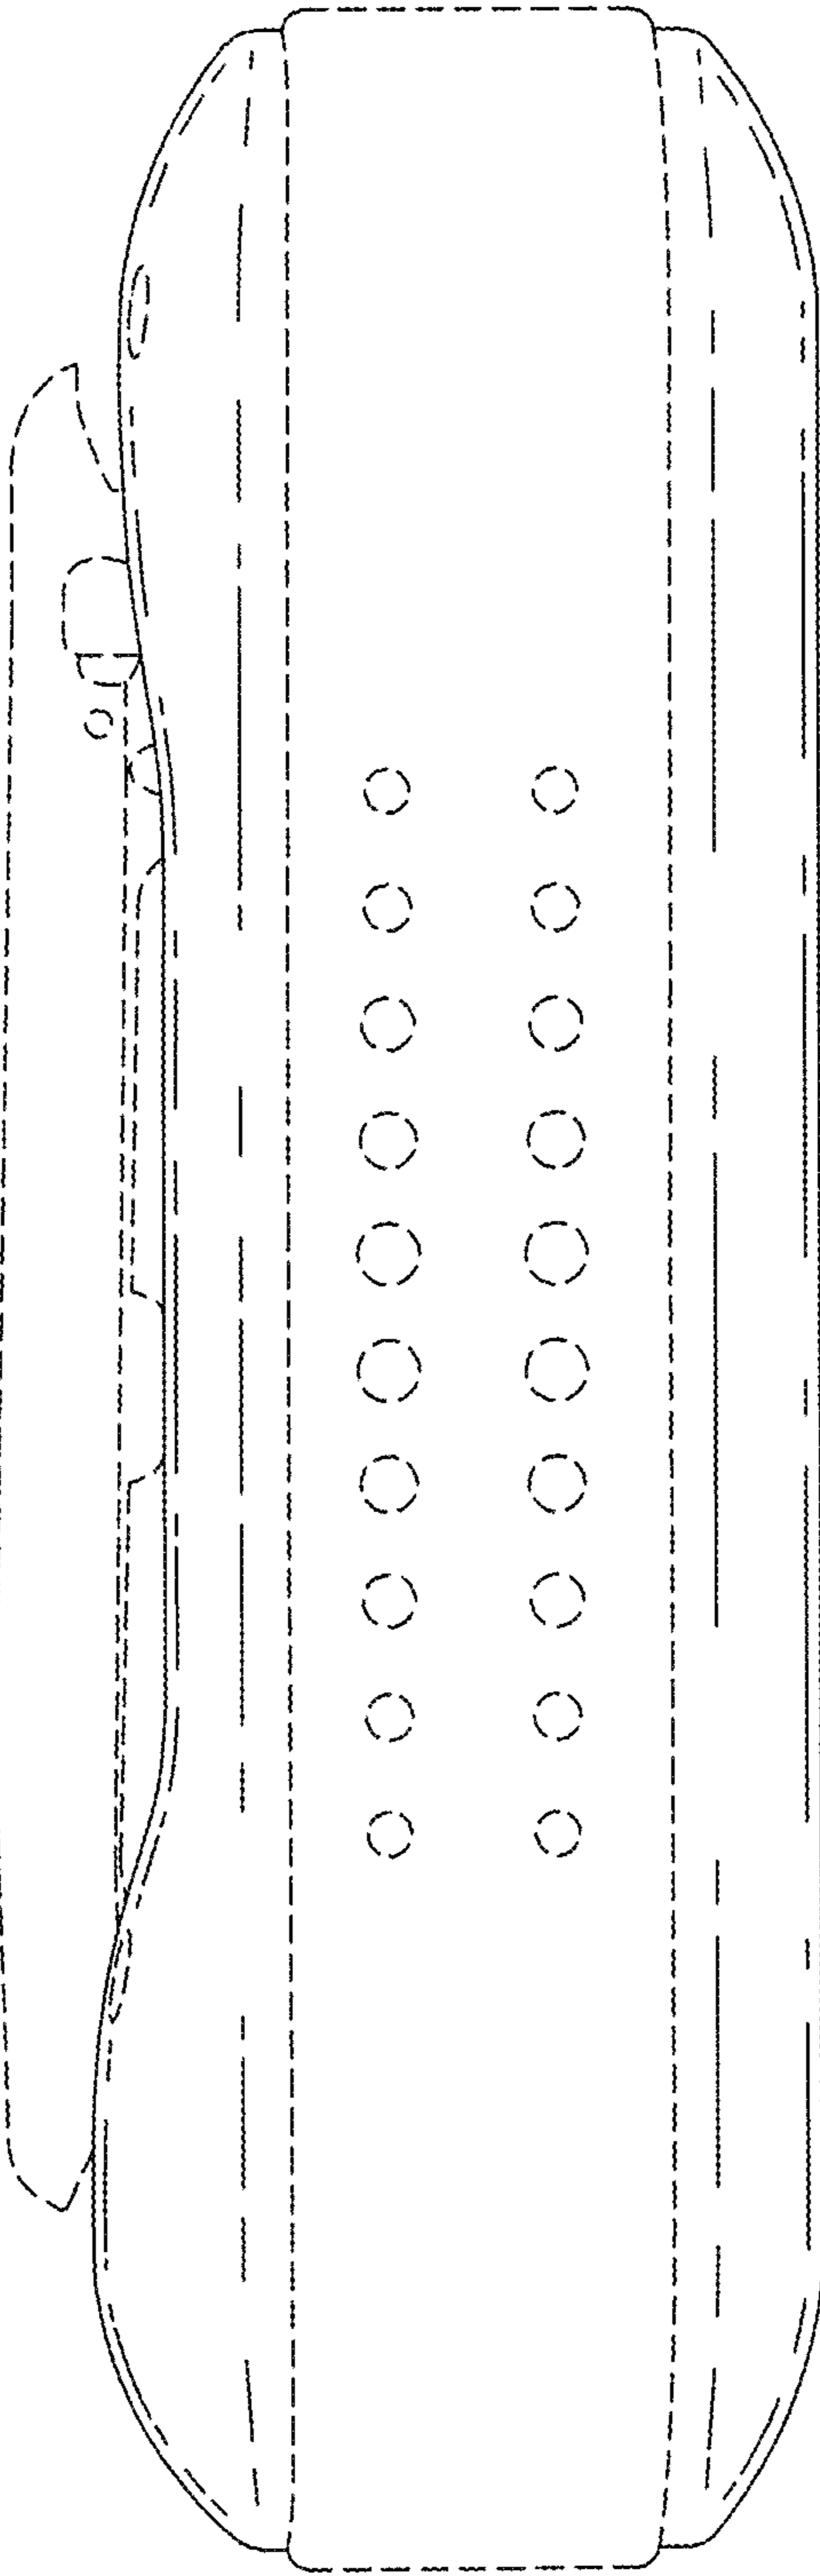


FIG. 5

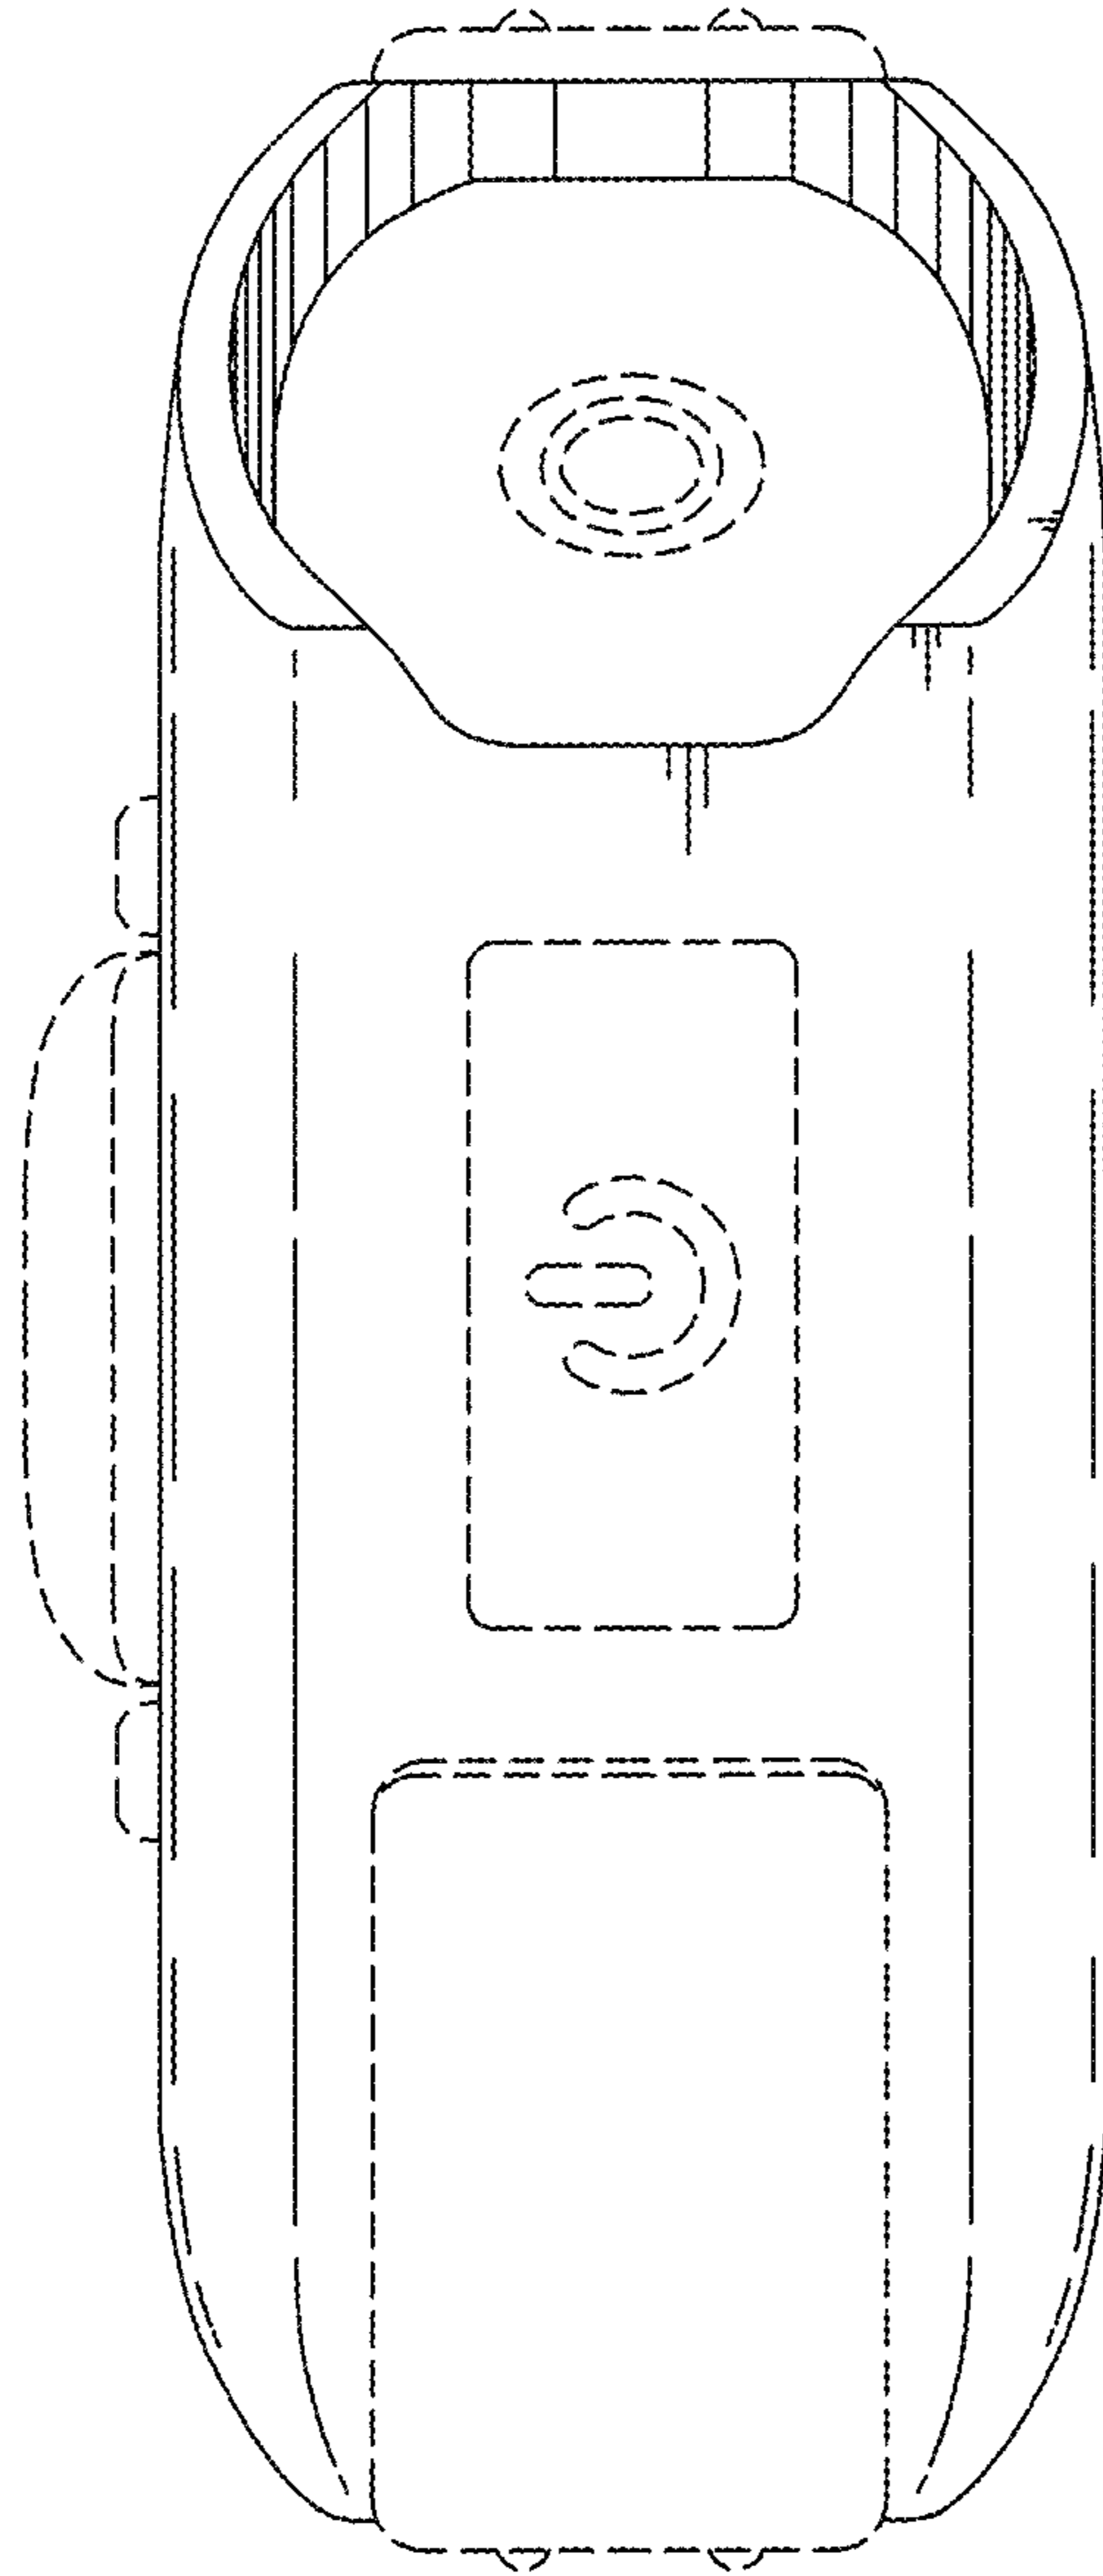


FIG. 6

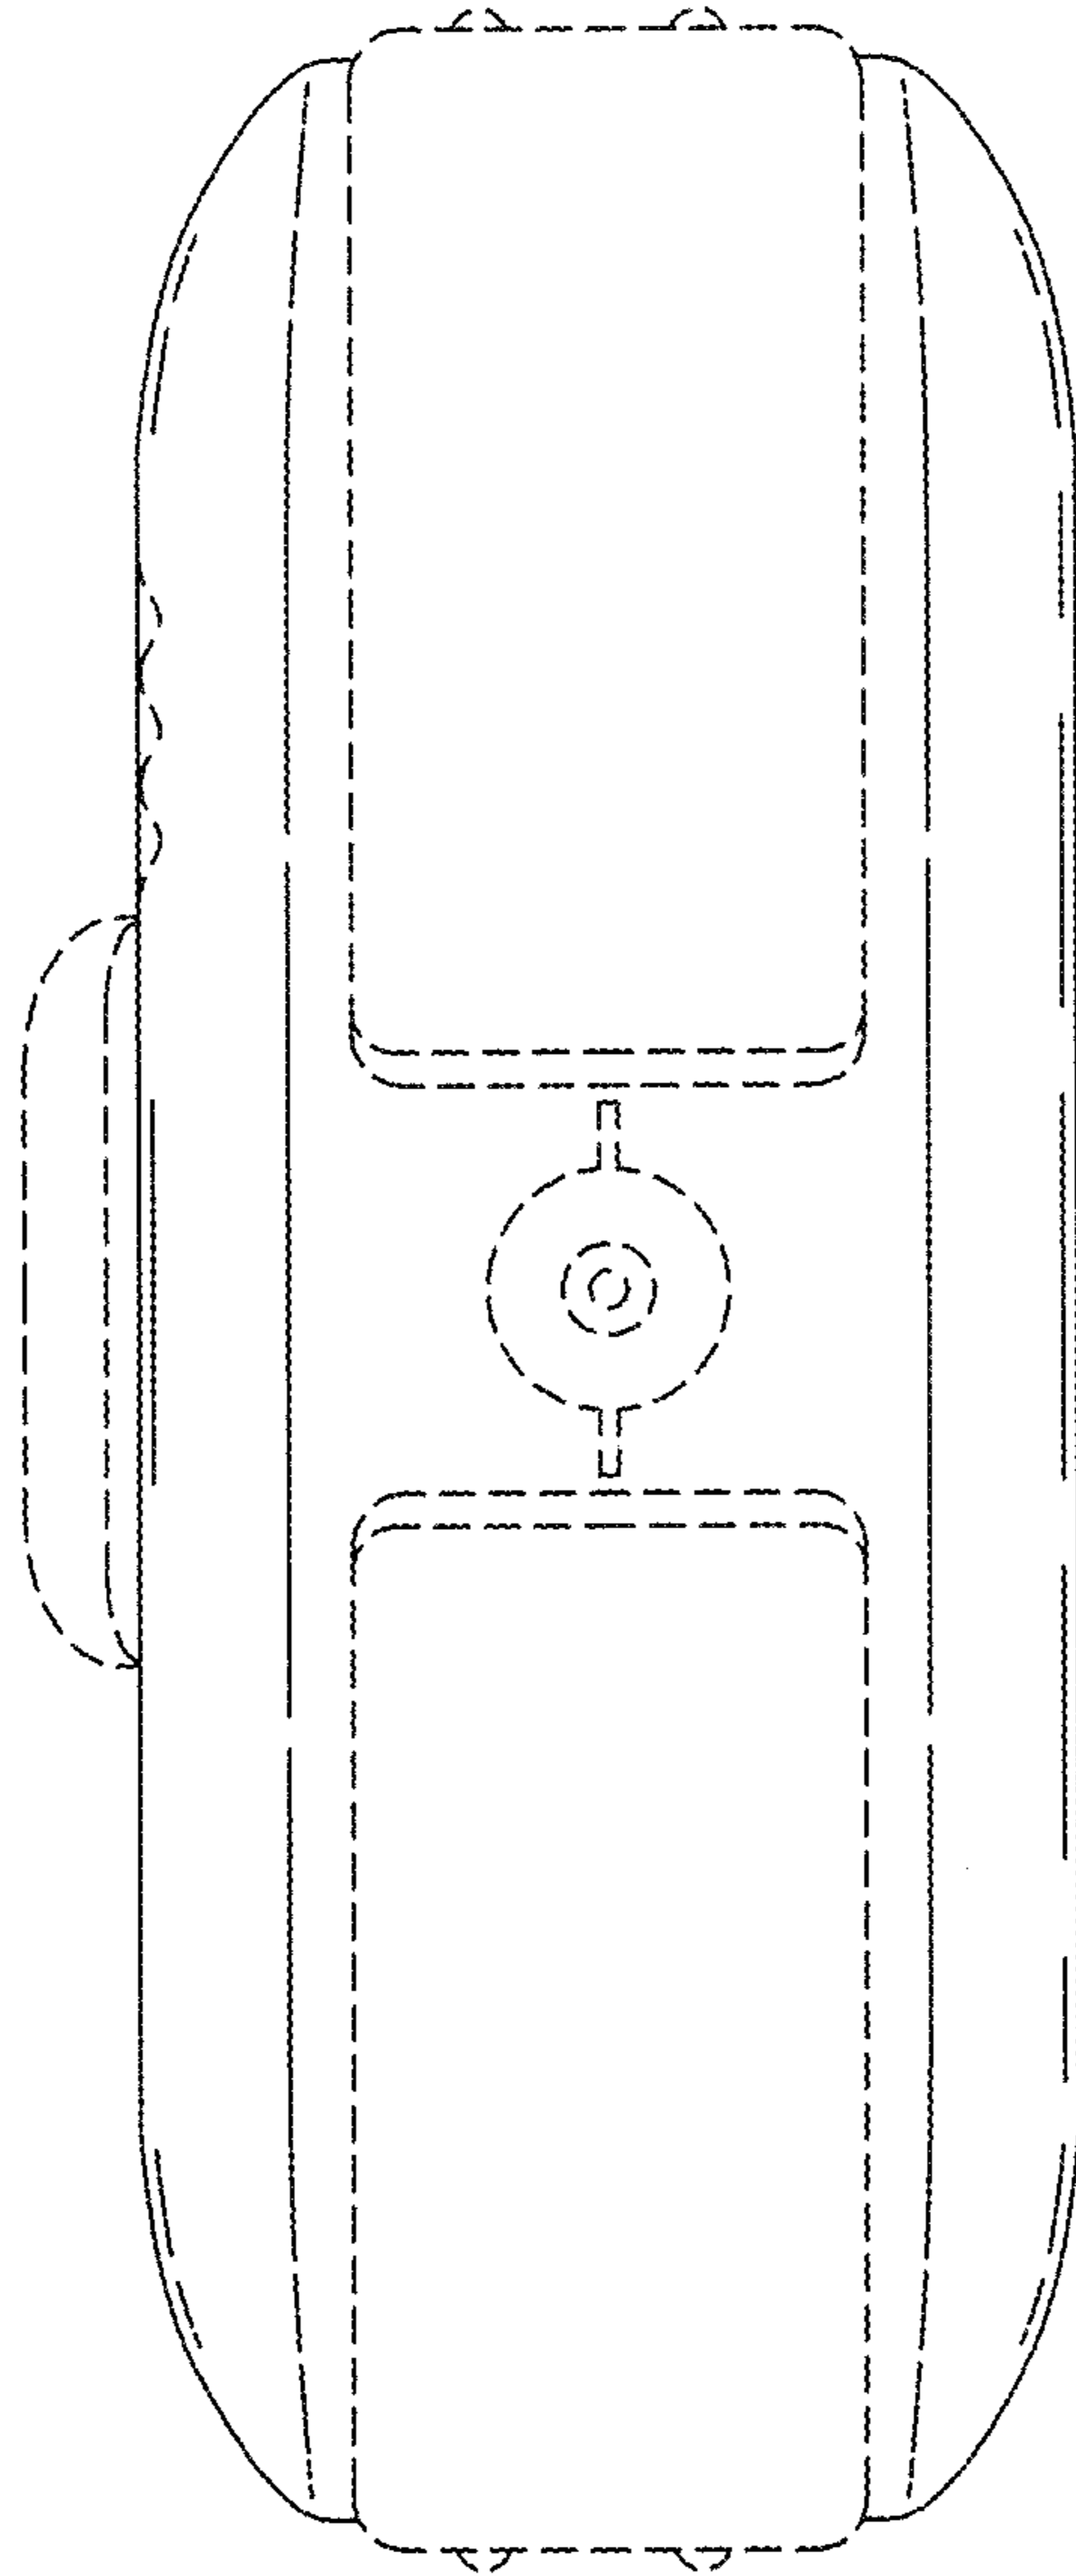


FIG. 7



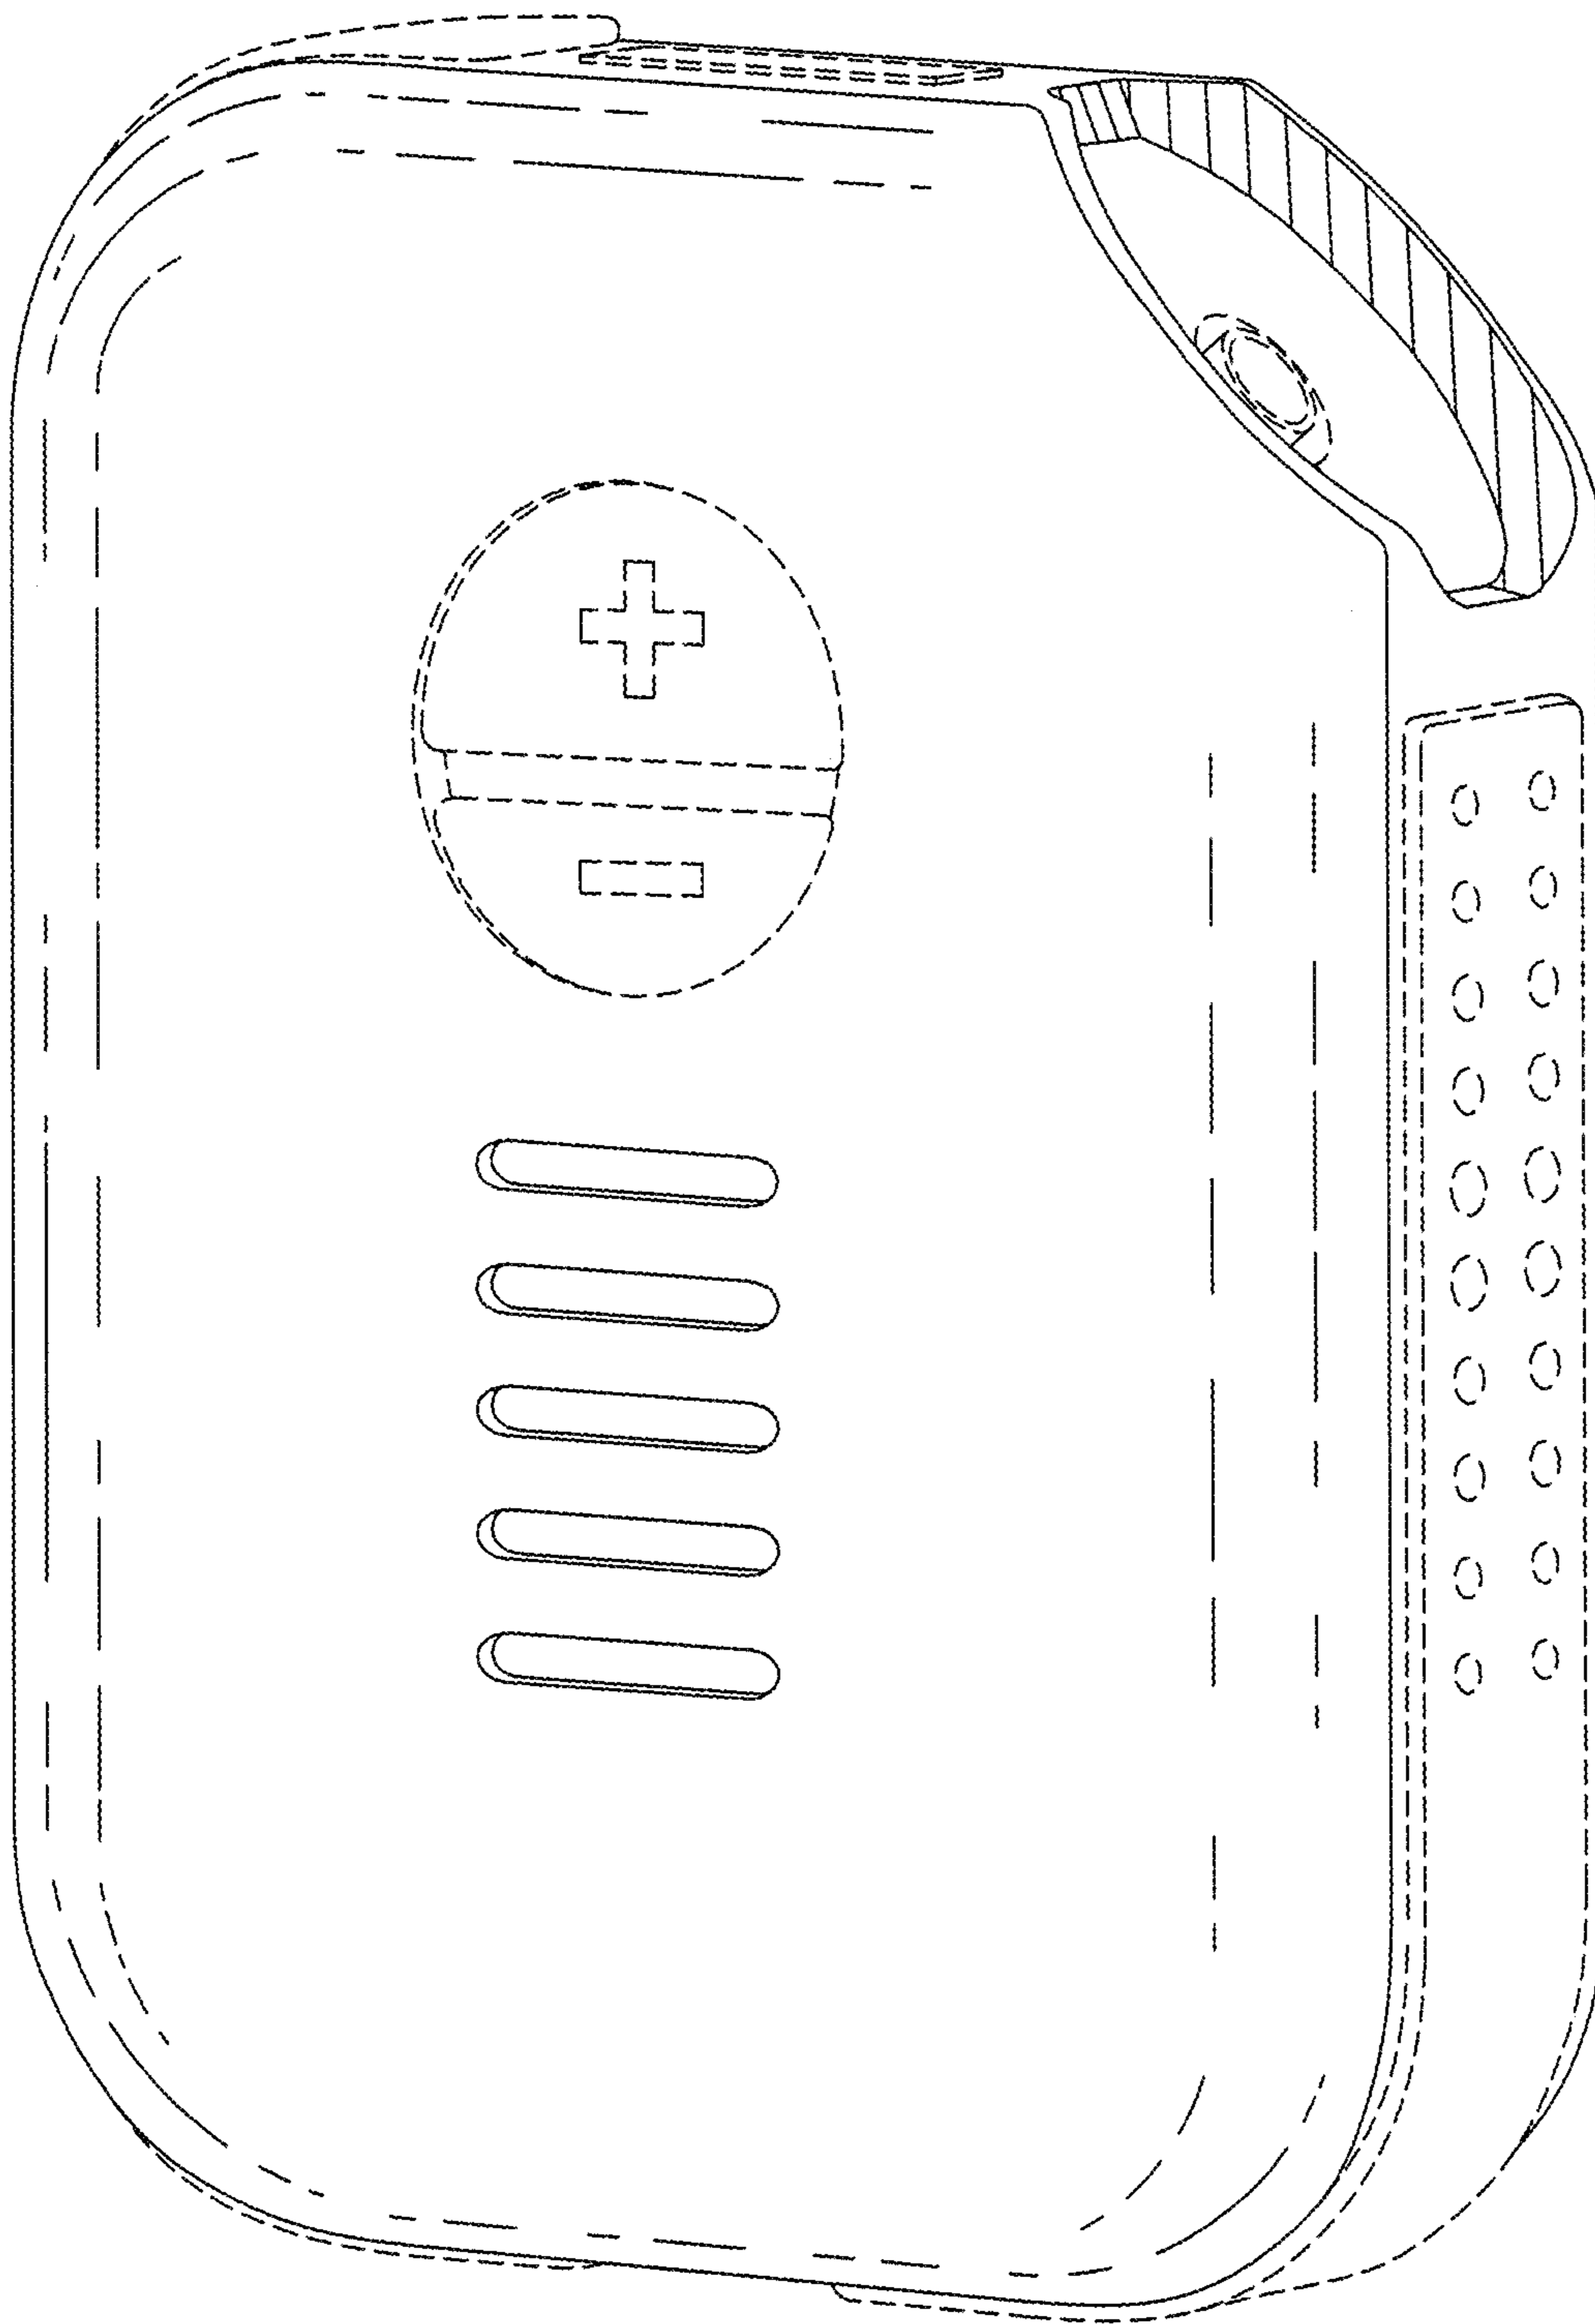


FIG. 8

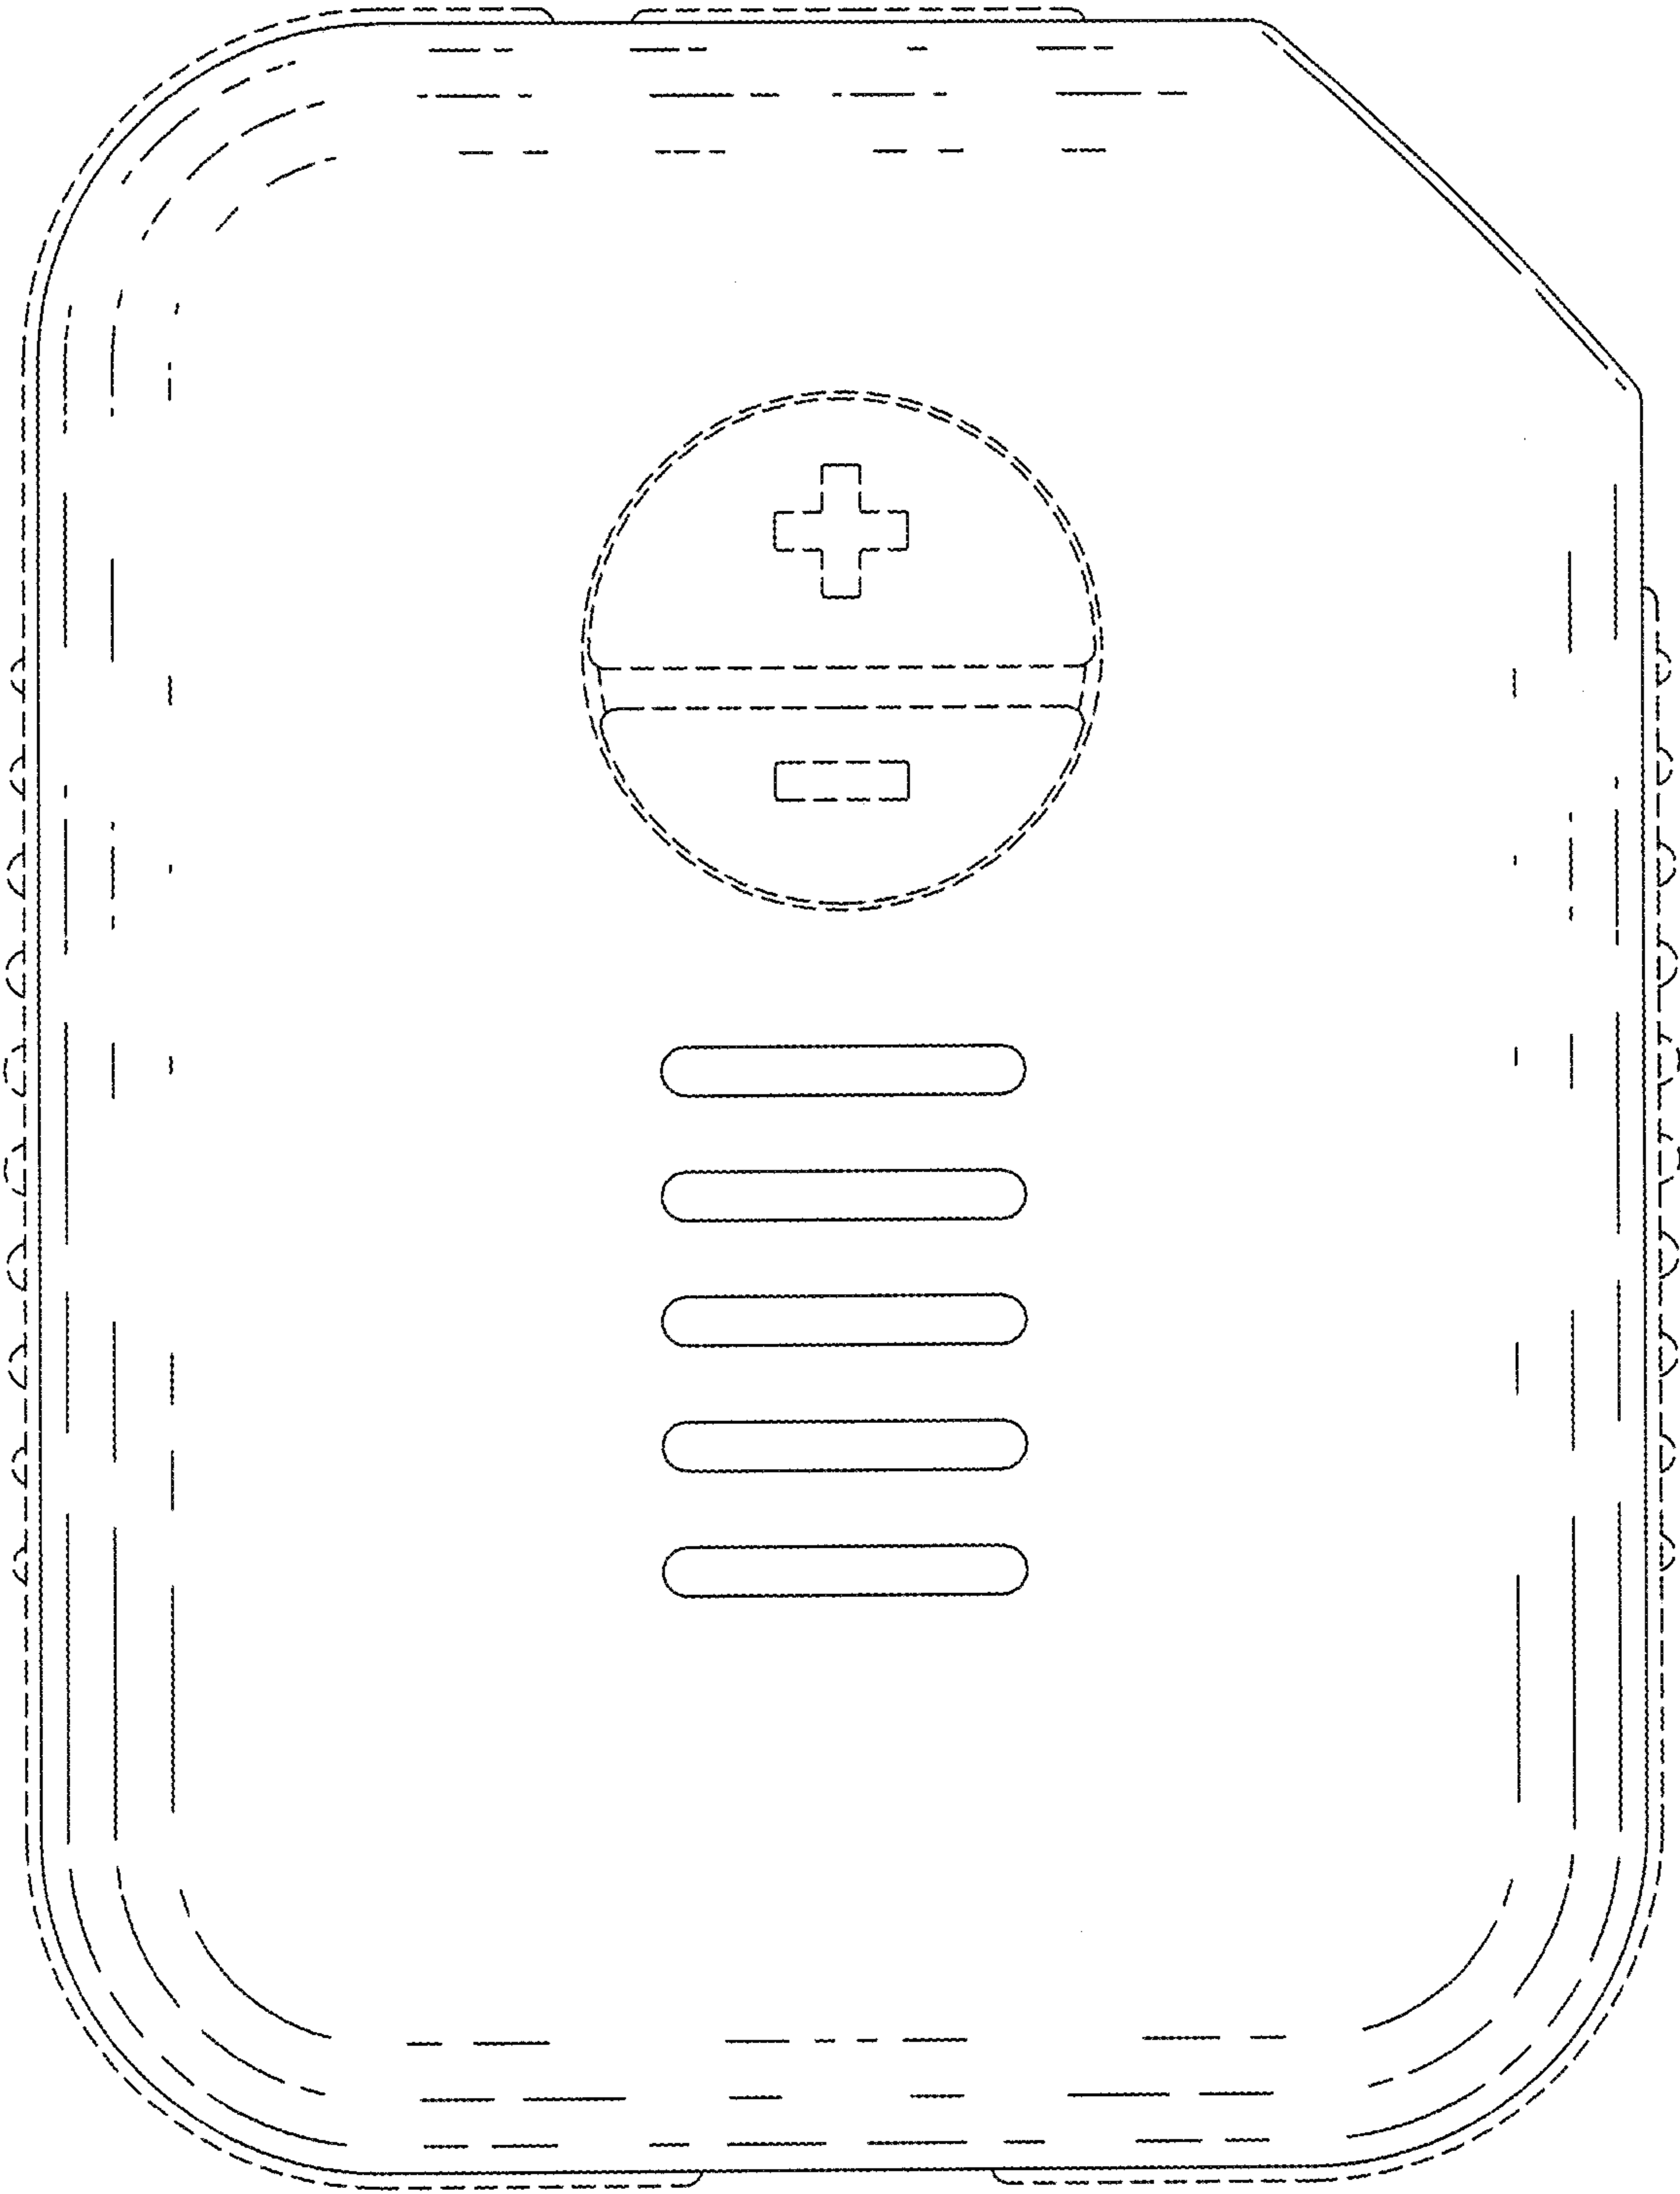


FIG. 9

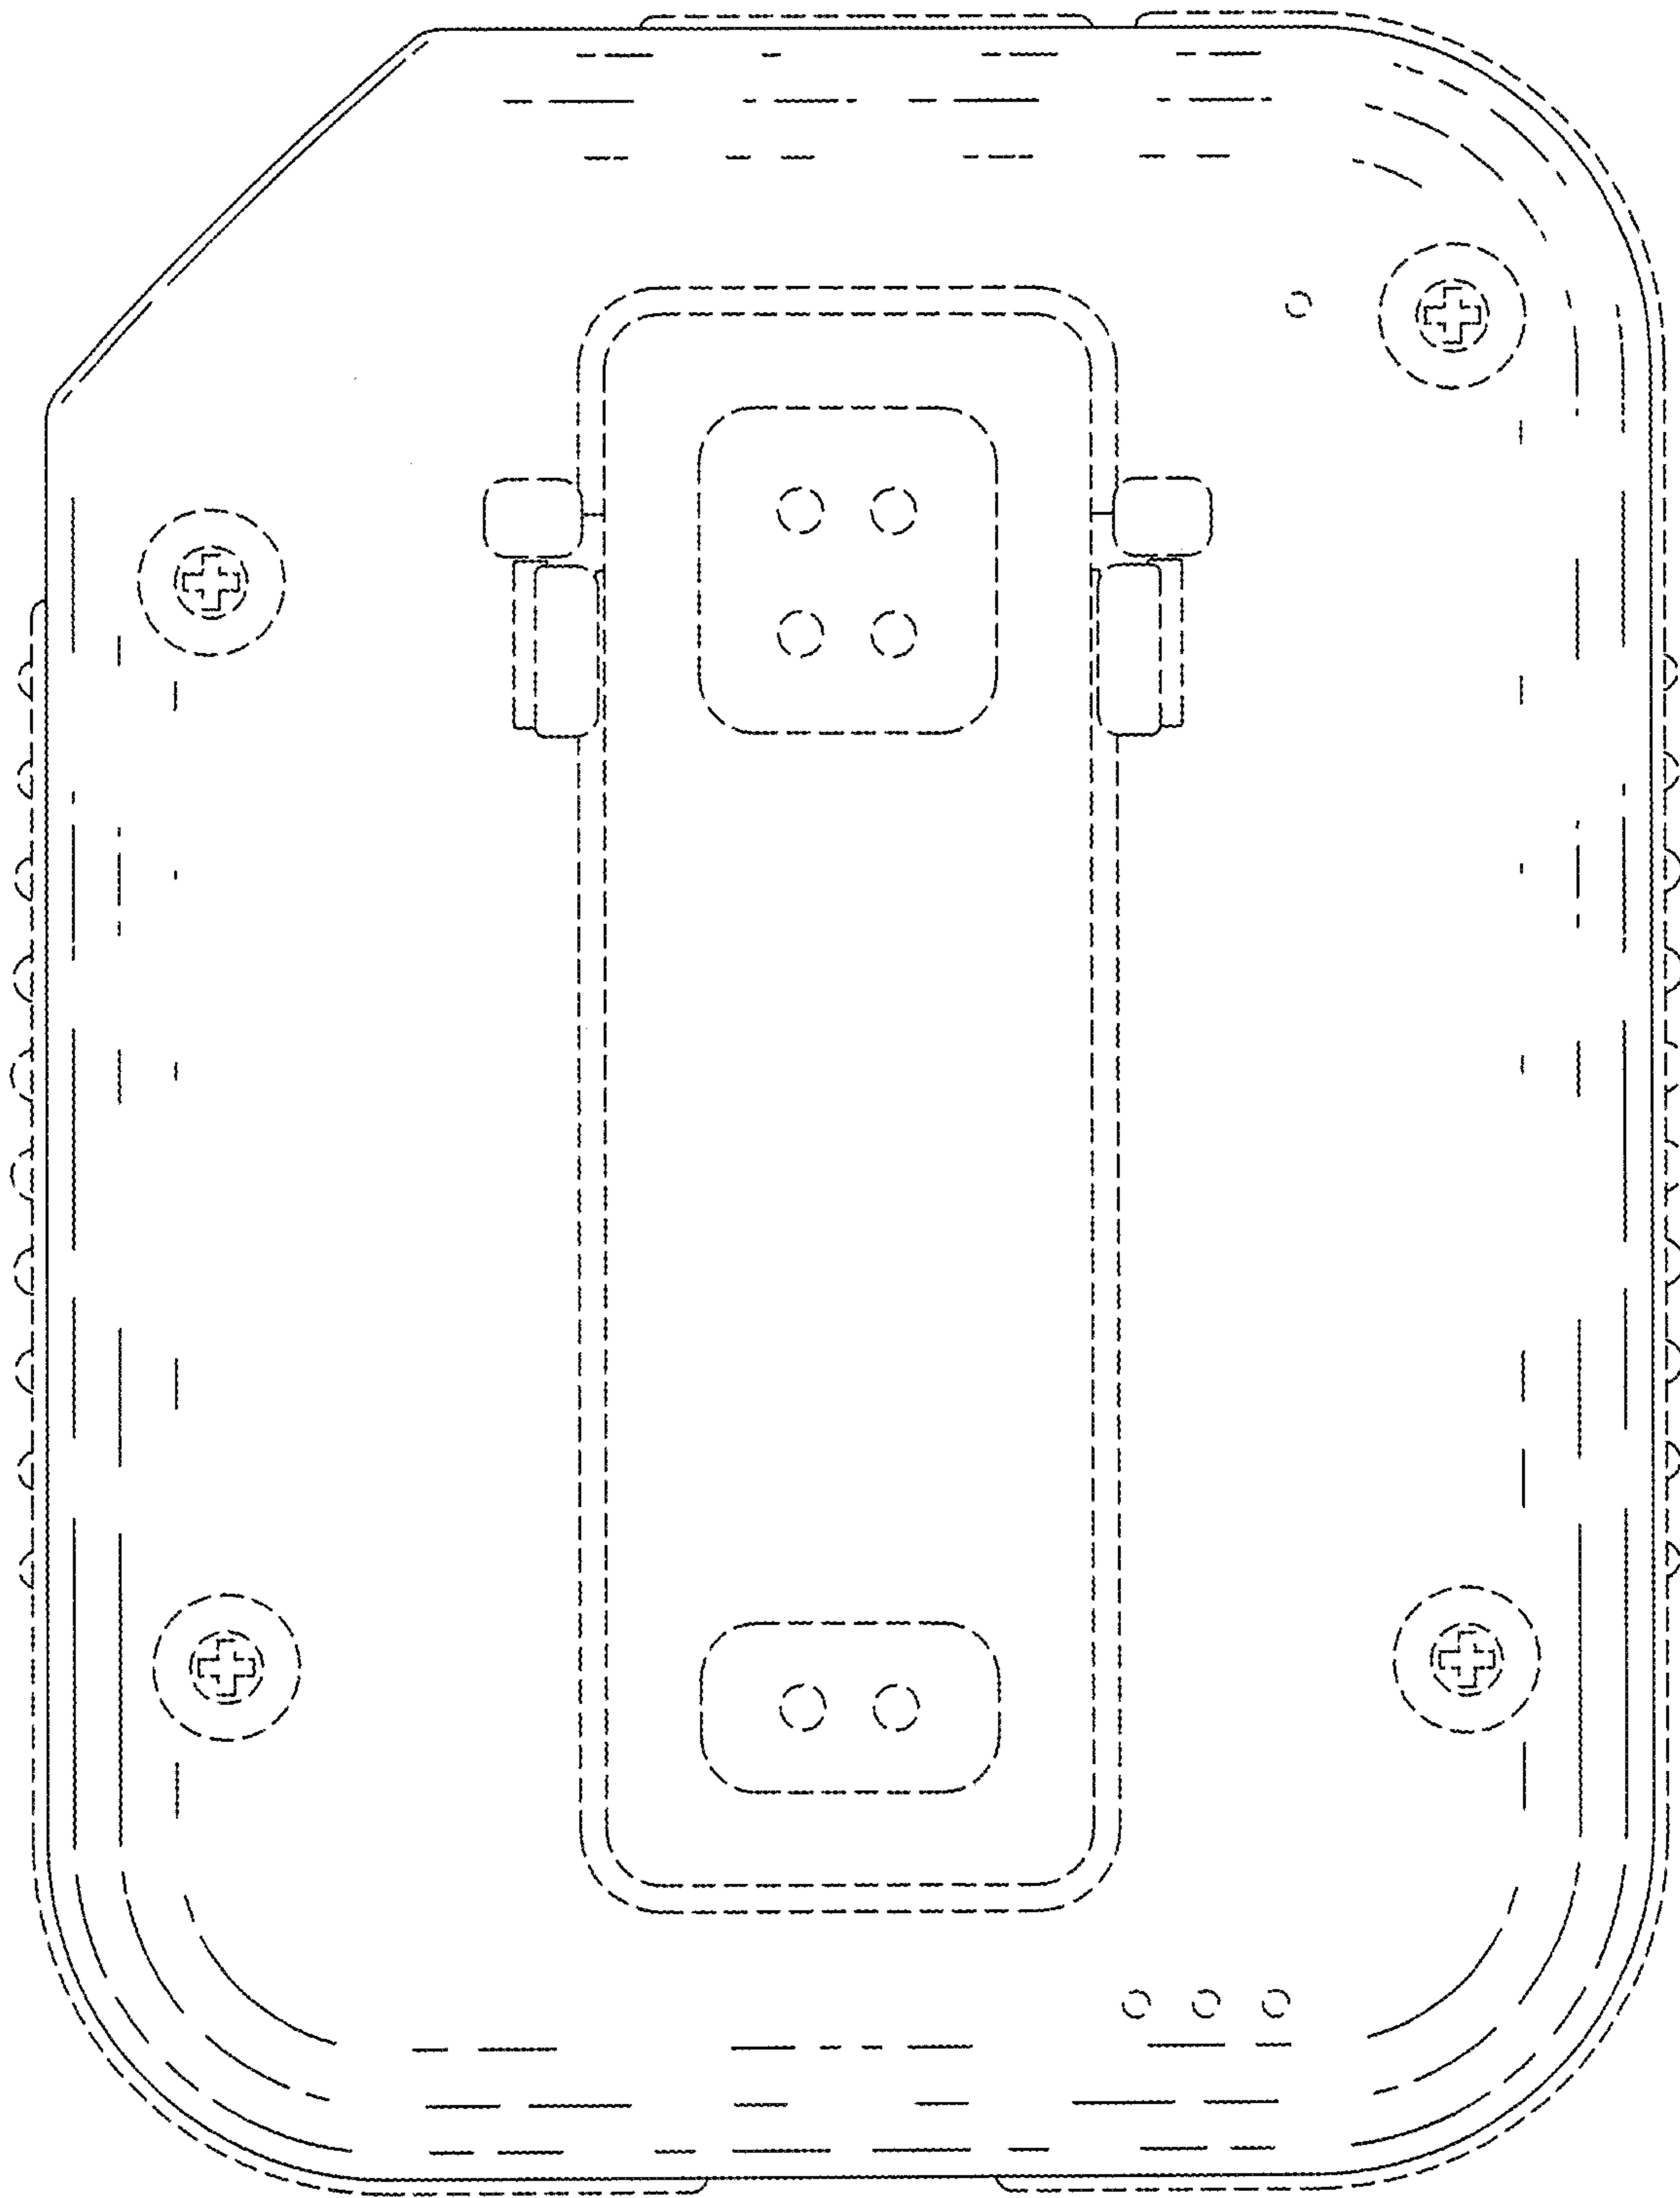


FIG. 10

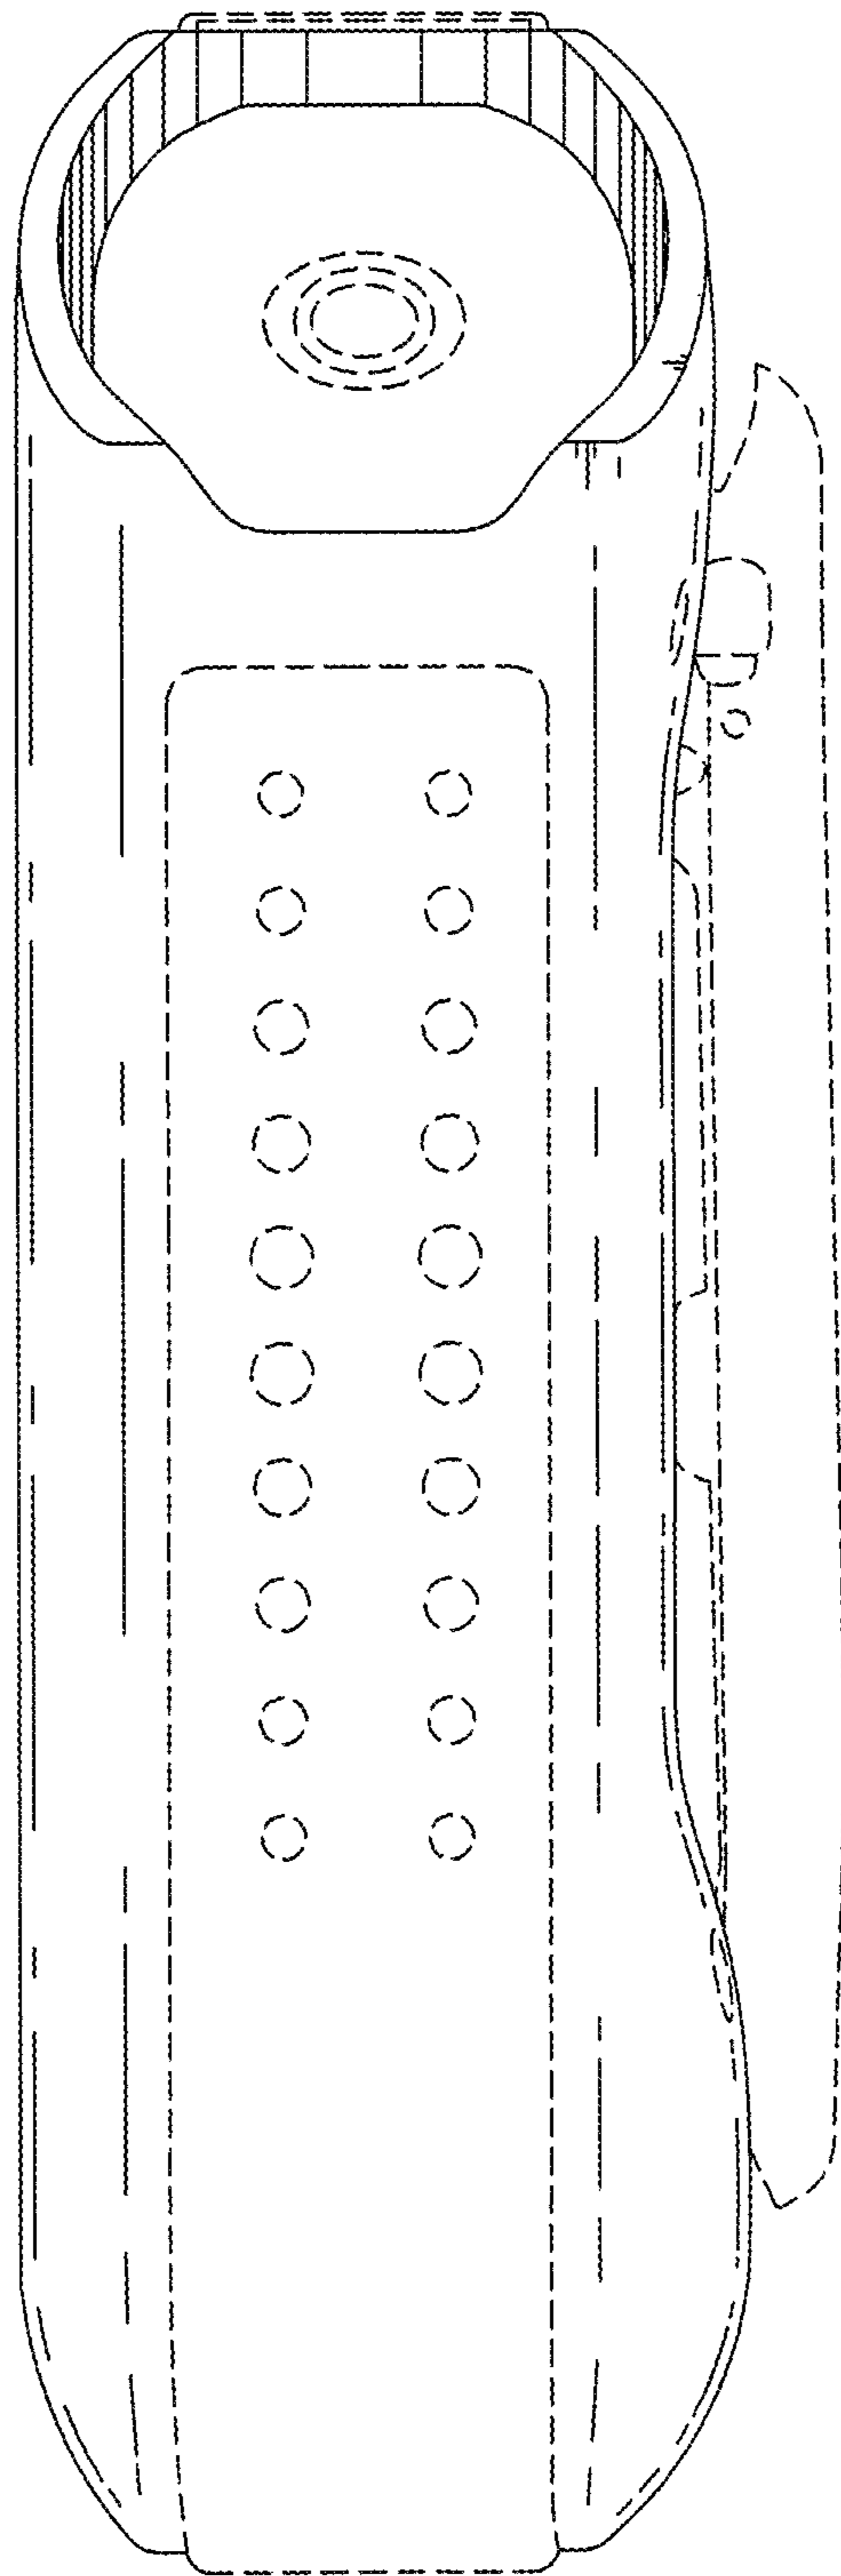


FIG. 11

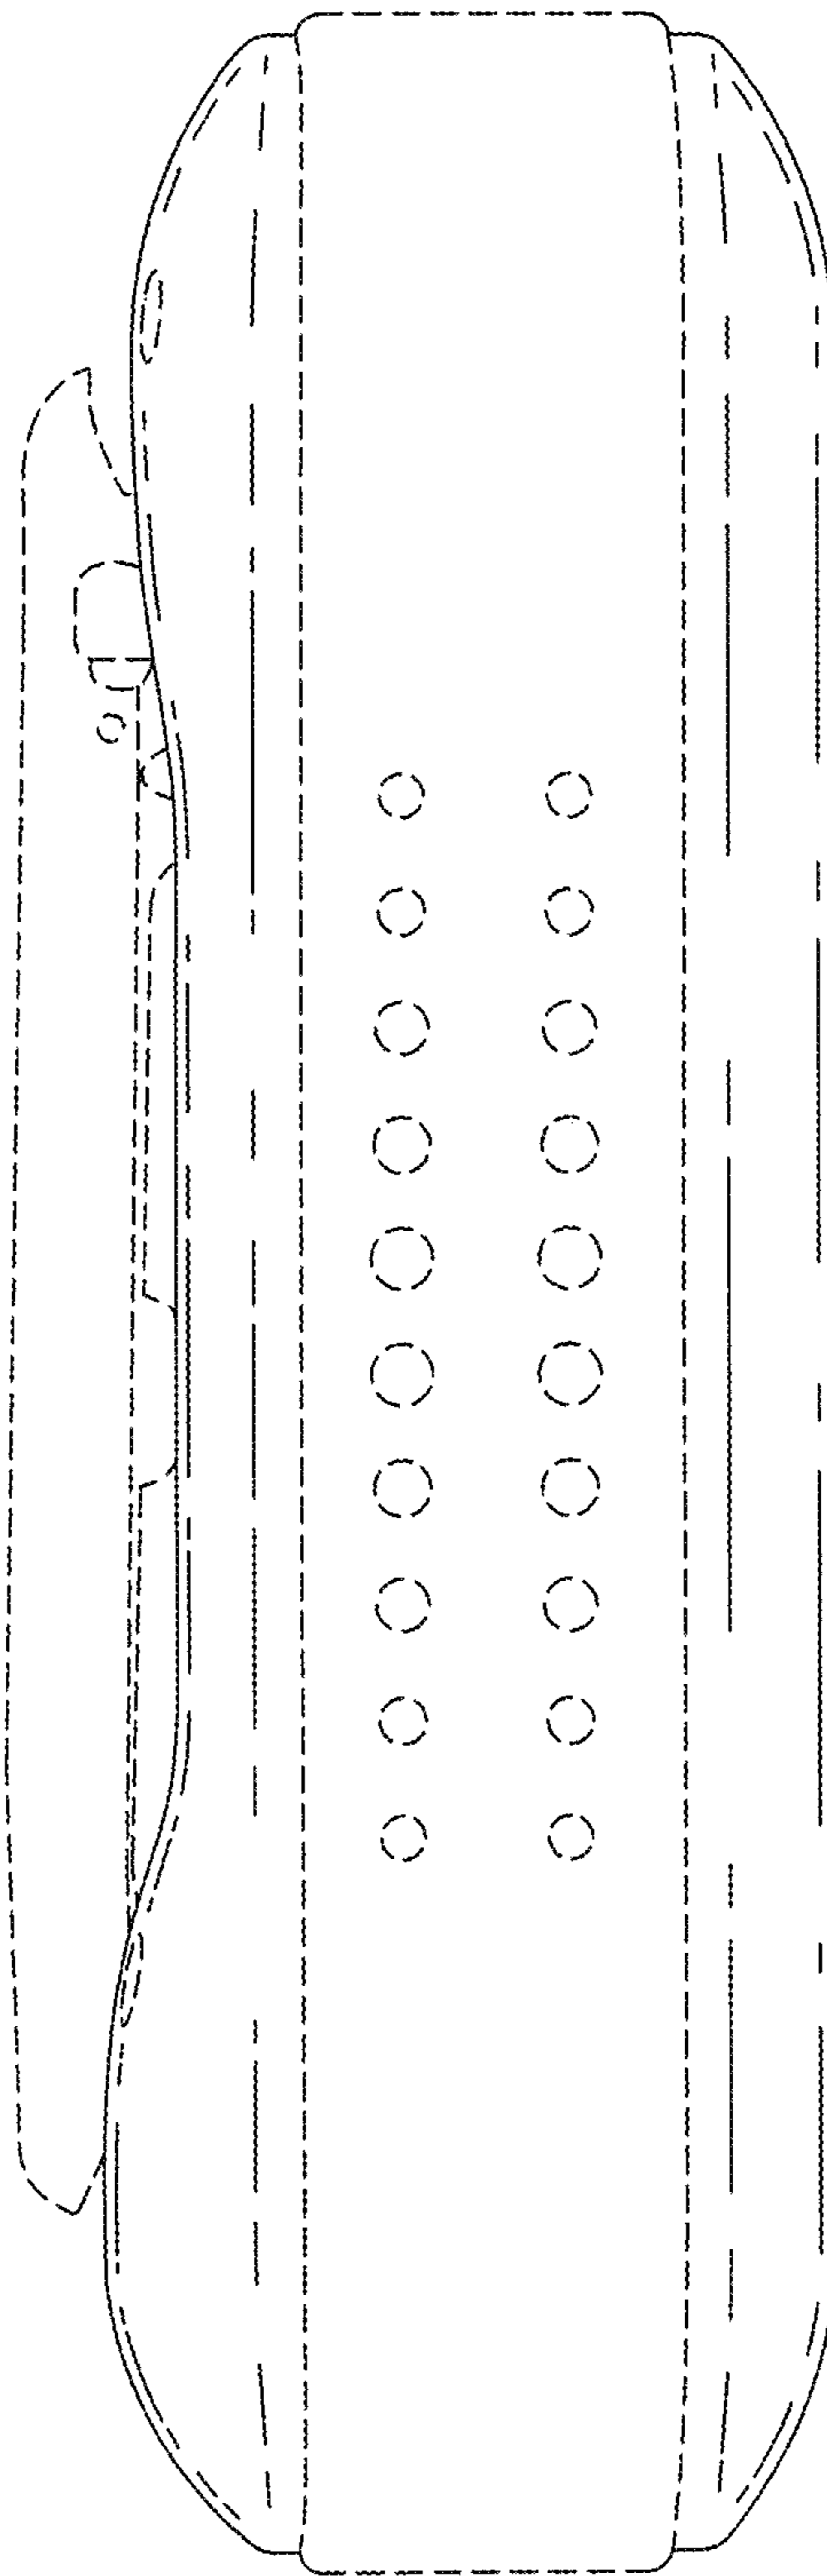


FIG. 12



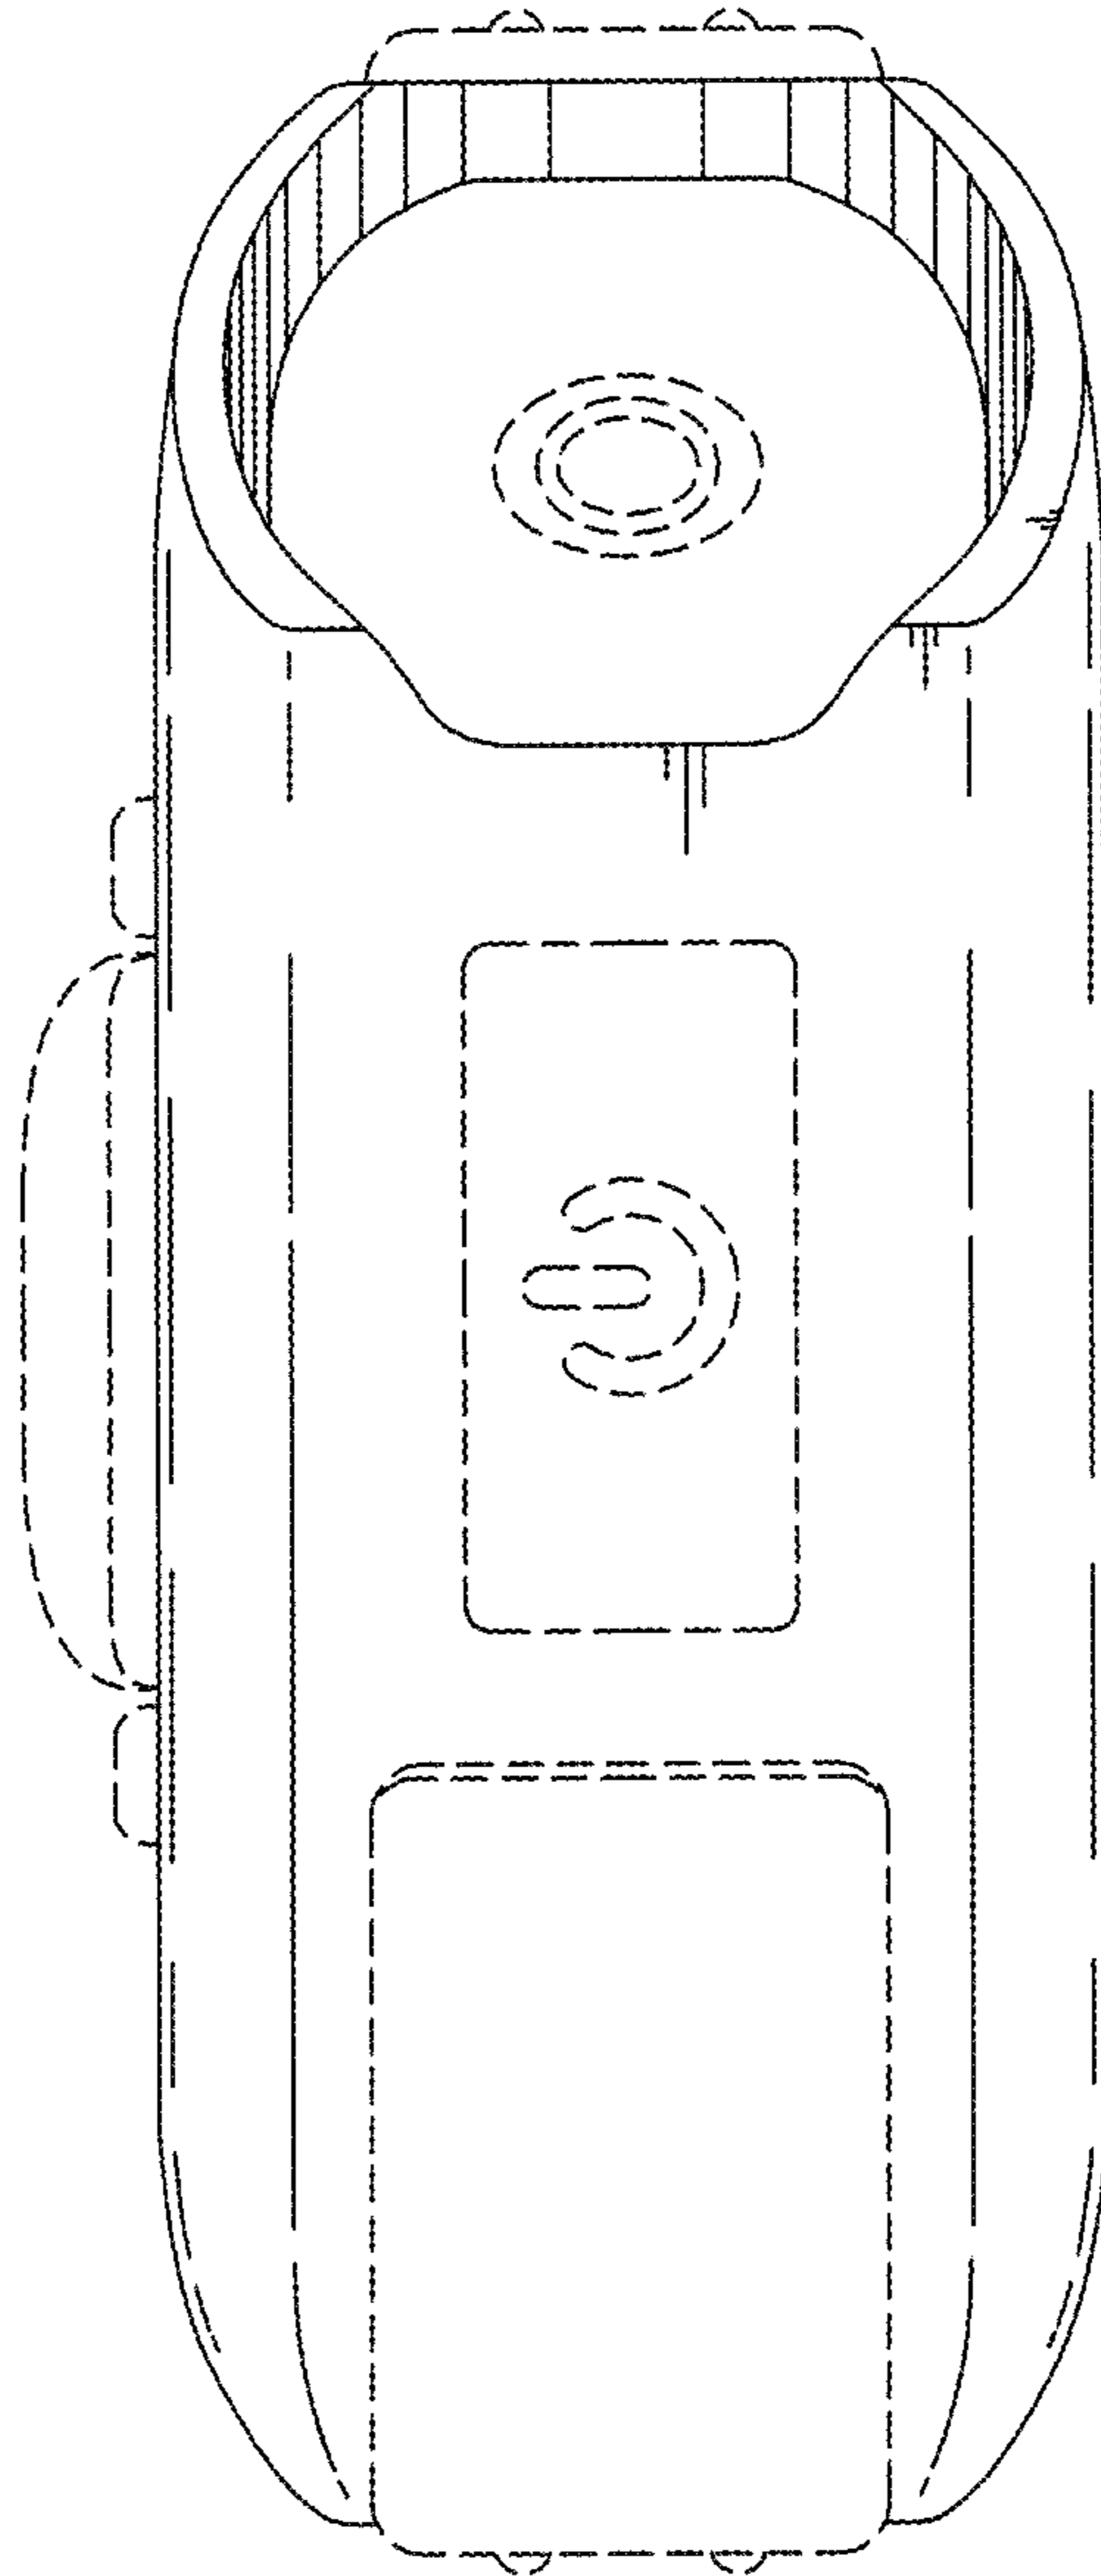


FIG. 13

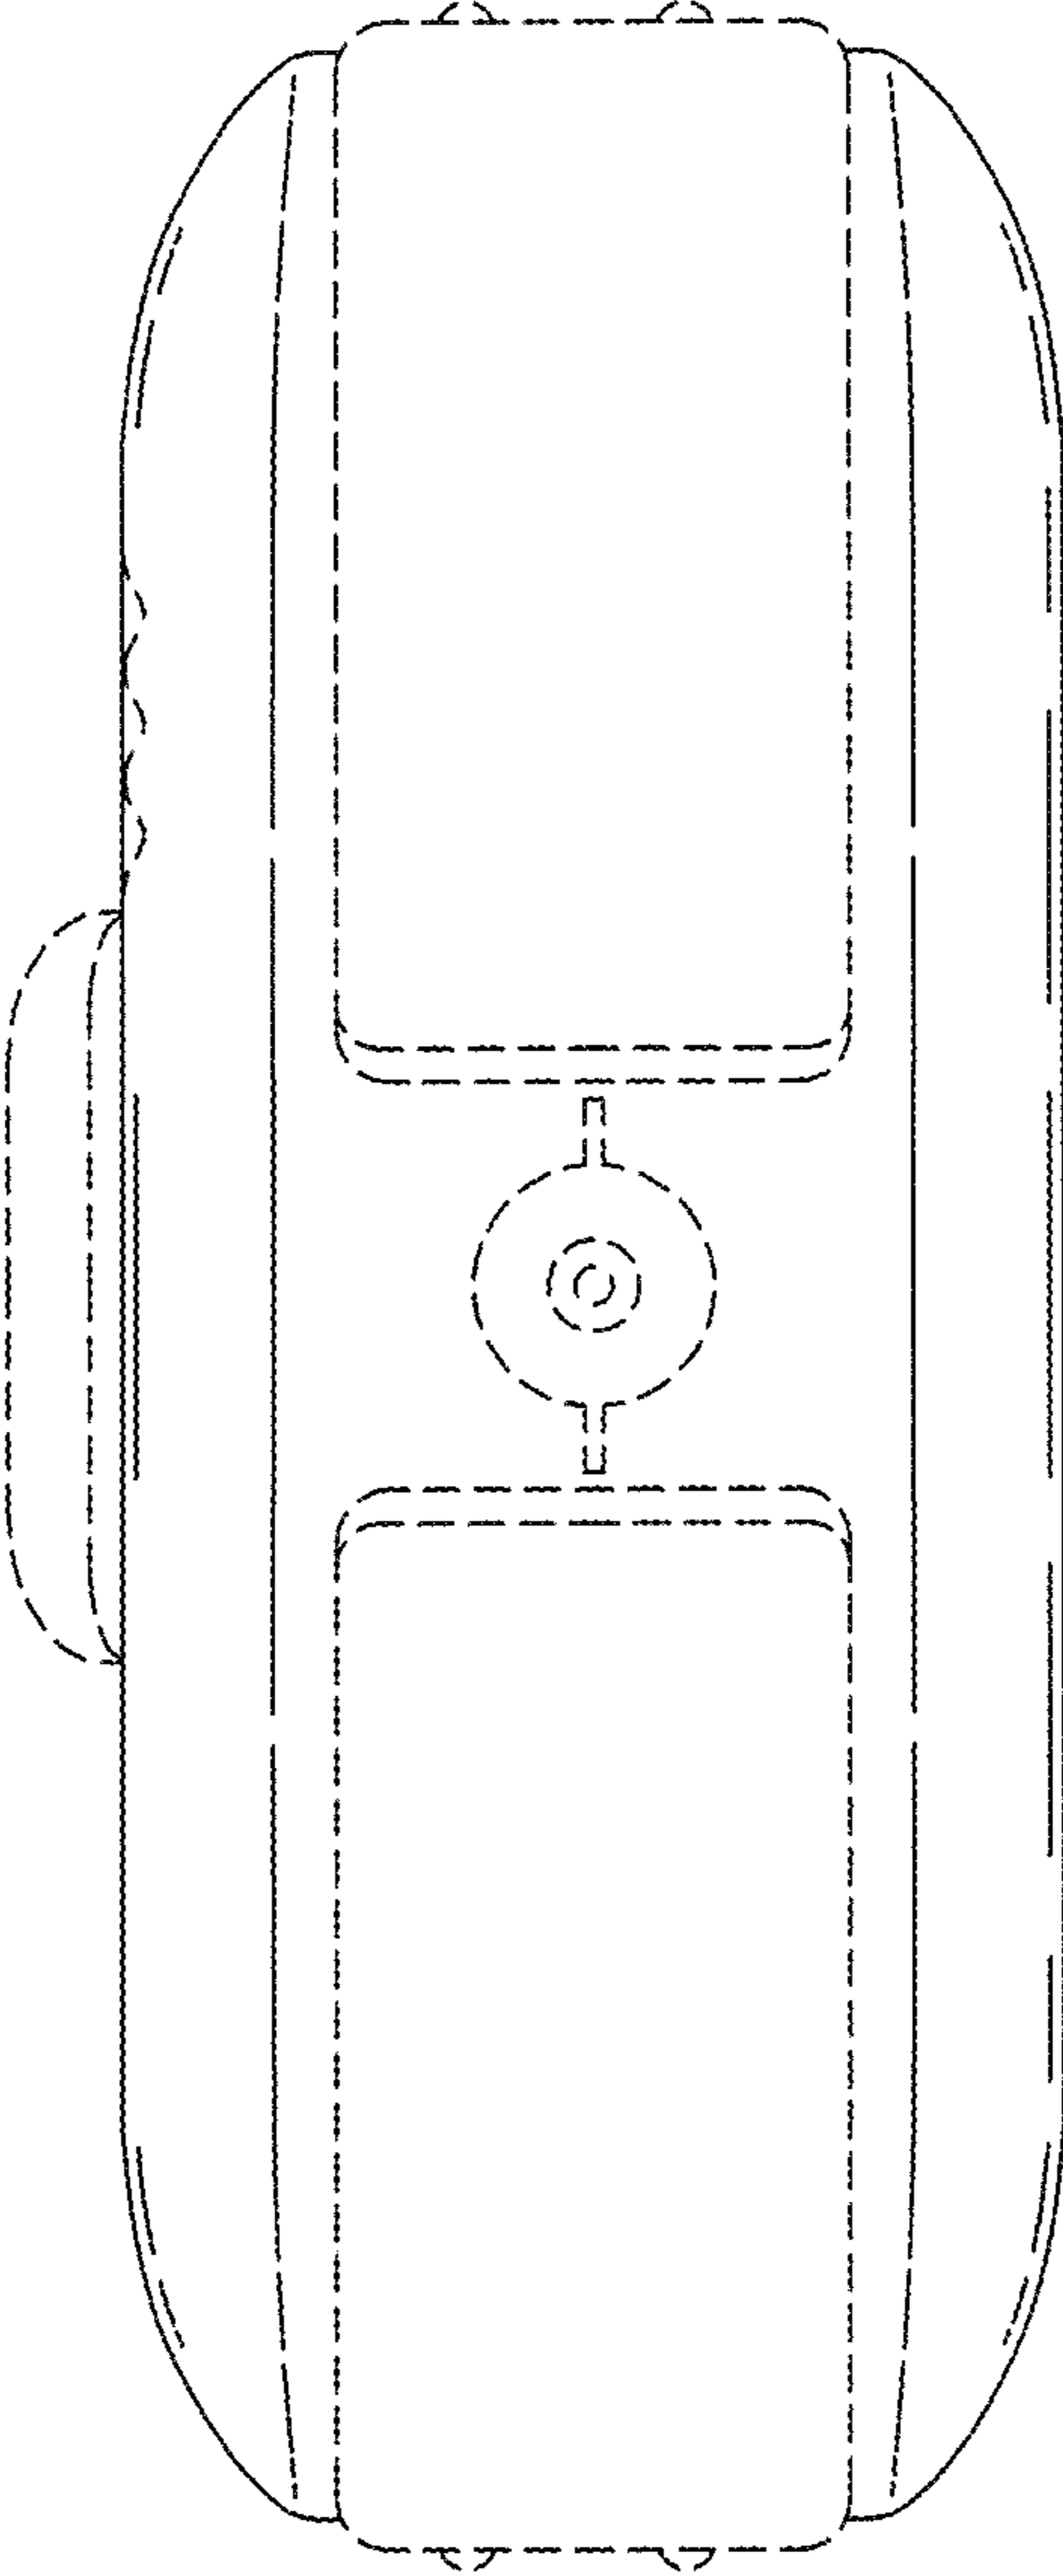


FIG. 14