



US00D877927S

(12) **United States Design Patent**
Nathan

(10) **Patent No.:** **US D877,927 S**

(45) **Date of Patent:** **** Mar. 10, 2020**

- (54) **STERILIZATION DEVICE**
- (71) Applicant: **Violet Defense Technology, Inc.**,
Celebration, FL (US)
- (72) Inventor: **Mark Nathan**, Harmony, FL (US)
- (73) Assignee: **Violet Defense Technology, Inc.**,
Orlando, FL (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/653,557**
- (22) Filed: **Jun. 15, 2018**
- (51) **LOC (12) Cl.** **24-01**
- (52) **U.S. Cl.**
USPC **D24/217**
- (58) **Field of Classification Search**
USPC D24/200, 209–213, 217–219, 224–232,
D24/186, 107, 108; D23/366; D32/1,
D32/25; D28/44, 73; 422/24, 26, 27,
422/307; 250/455.11
CPC A61L 2/26; A61L 2/24; A61L 2/17; A61L
2/18; A61L 2/025; A61L 2/10; A61L
2/084; A61L 2202/122; A61L 2202/10;
A61L 2202/11; A61L 2202/14; A61L
2202/23; A61L 2202/24; A61L 2202/182;
C02F 1/32; C02F 1/325; A61H 15/00;
A61H 15/0007; A61H 2015/0042; A63B
43/06
See application file for complete search history.

- (56) **References Cited**
U.S. PATENT DOCUMENTS
D681,843 S * 5/2013 Nemeth B01L 3/502
D24/224
D837,997 S * 1/2019 Gil D24/217
D848,635 S * 5/2019 Davis D24/217

- 2003/0165398 A1* 9/2003 Waldo A61L 2/0011
422/22
- 2007/0272279 A1* 11/2007 Foster A61L 2/18
134/32
- 2010/0296968 A1* 11/2010 Cady A61L 2/186
422/28
- 2011/0006228 A1* 1/2011 Tow A61L 2/084
250/504 R
- 2013/0142693 A1* 6/2013 Flick A61L 2/18
422/29
- 2014/0299554 A1* 10/2014 Britenstine C02F 1/325
210/748.11
- 2017/0035918 A1* 2/2017 Kassel A61L 2/10
(Continued)

Primary Examiner — Barbara Fox
Assistant Examiner — Mary Shannon Malley
 (74) *Attorney, Agent, or Firm* — Foley & Lardner LLP


(57) **CLAIM**

The ornamental design for a sterilization device, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a sterilization device showing the new design.
 FIG. 2 is a front elevation view of the sterilization device.
 FIG. 3 is a back elevation view of the sterilization device.
 FIG. 4 is a right side elevation view of the sterilization device.
 FIG. 5 is a left side elevation view of the sterilization device.
 FIG. 6 is a top plan view of the sterilization device.
 FIG. 7 is a bottom plan view of the sterilization device; and,
 FIG. 8 is a bottom perspective view of the sterilization device.
 The broken lines in the drawings depict portions of the sterilization device that form no part of the claimed design. The sterilization device is shown with a symbolic break in length, the appearance of any portion of the article between the break lines forms no part of the claimed design.

1 Claim, 6 Drawing Sheets

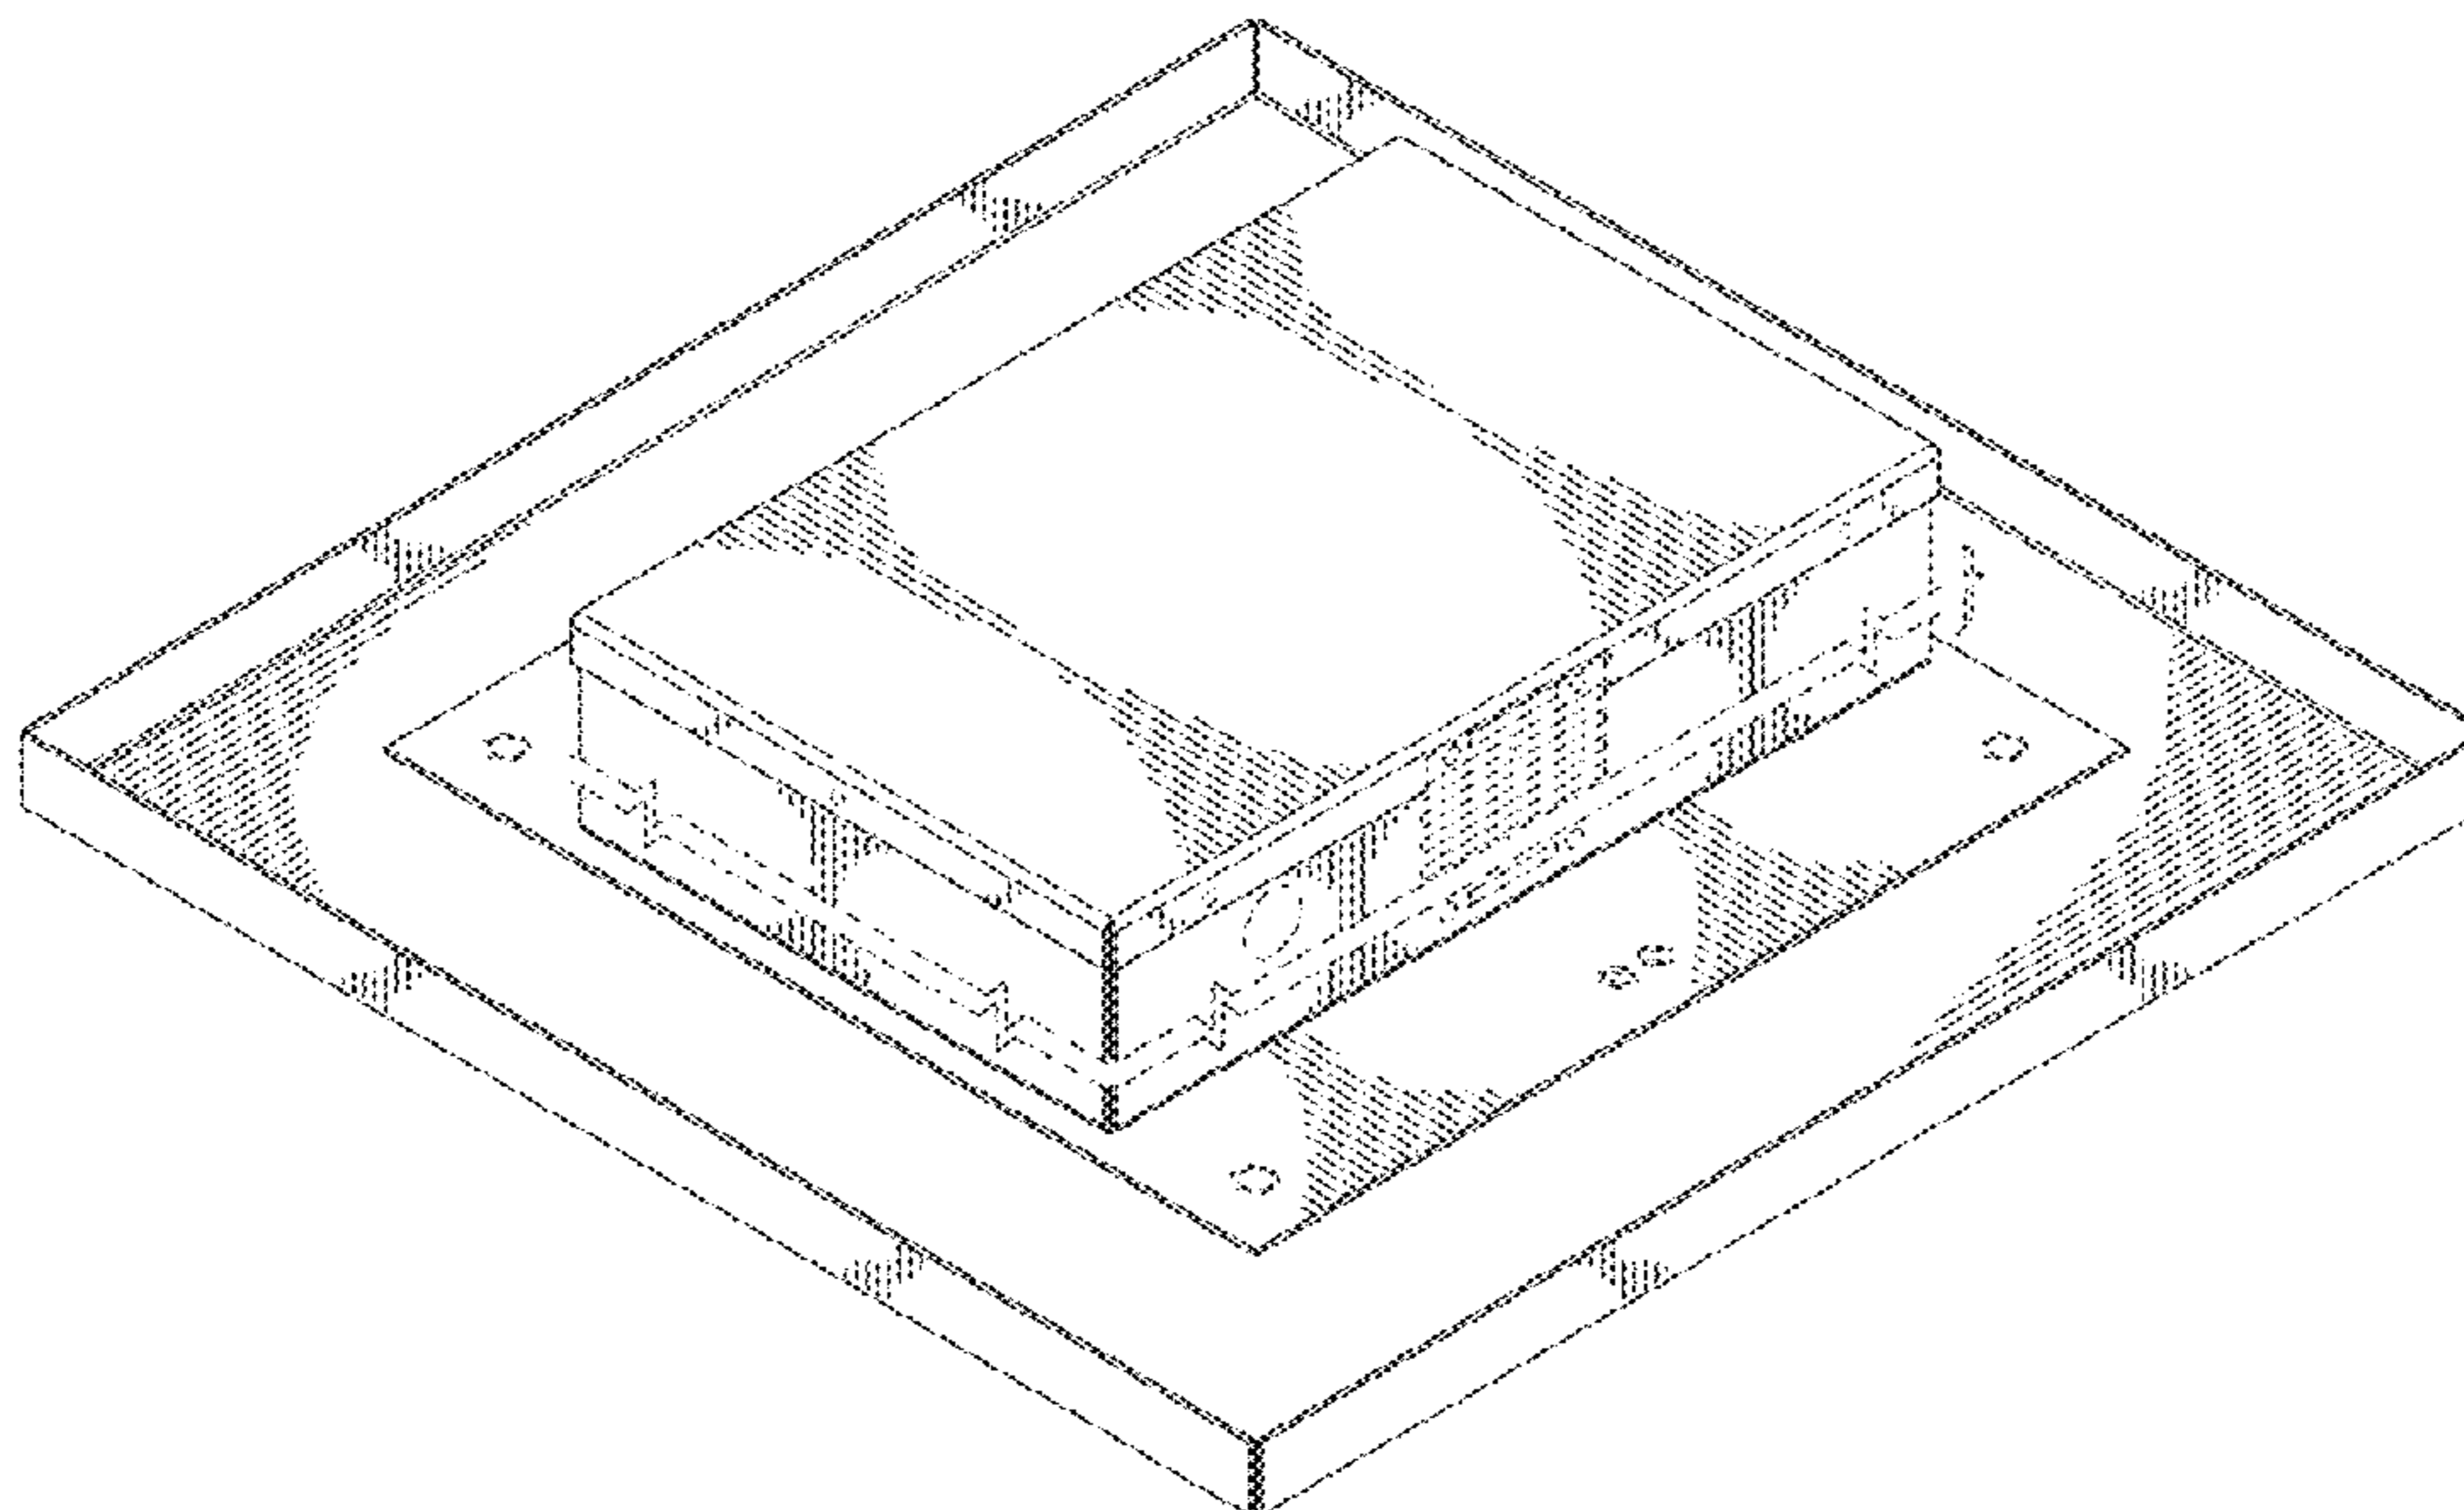

(56)

References Cited

U.S. PATENT DOCUMENTS

2018/0221803 A1* 8/2018 Turbett B01D 46/0002
2018/0311386 A1* 11/2018 Hawkins H05B 33/0857
2018/0353889 A1* 12/2018 Turbett A61L 2/07

* cited by examiner

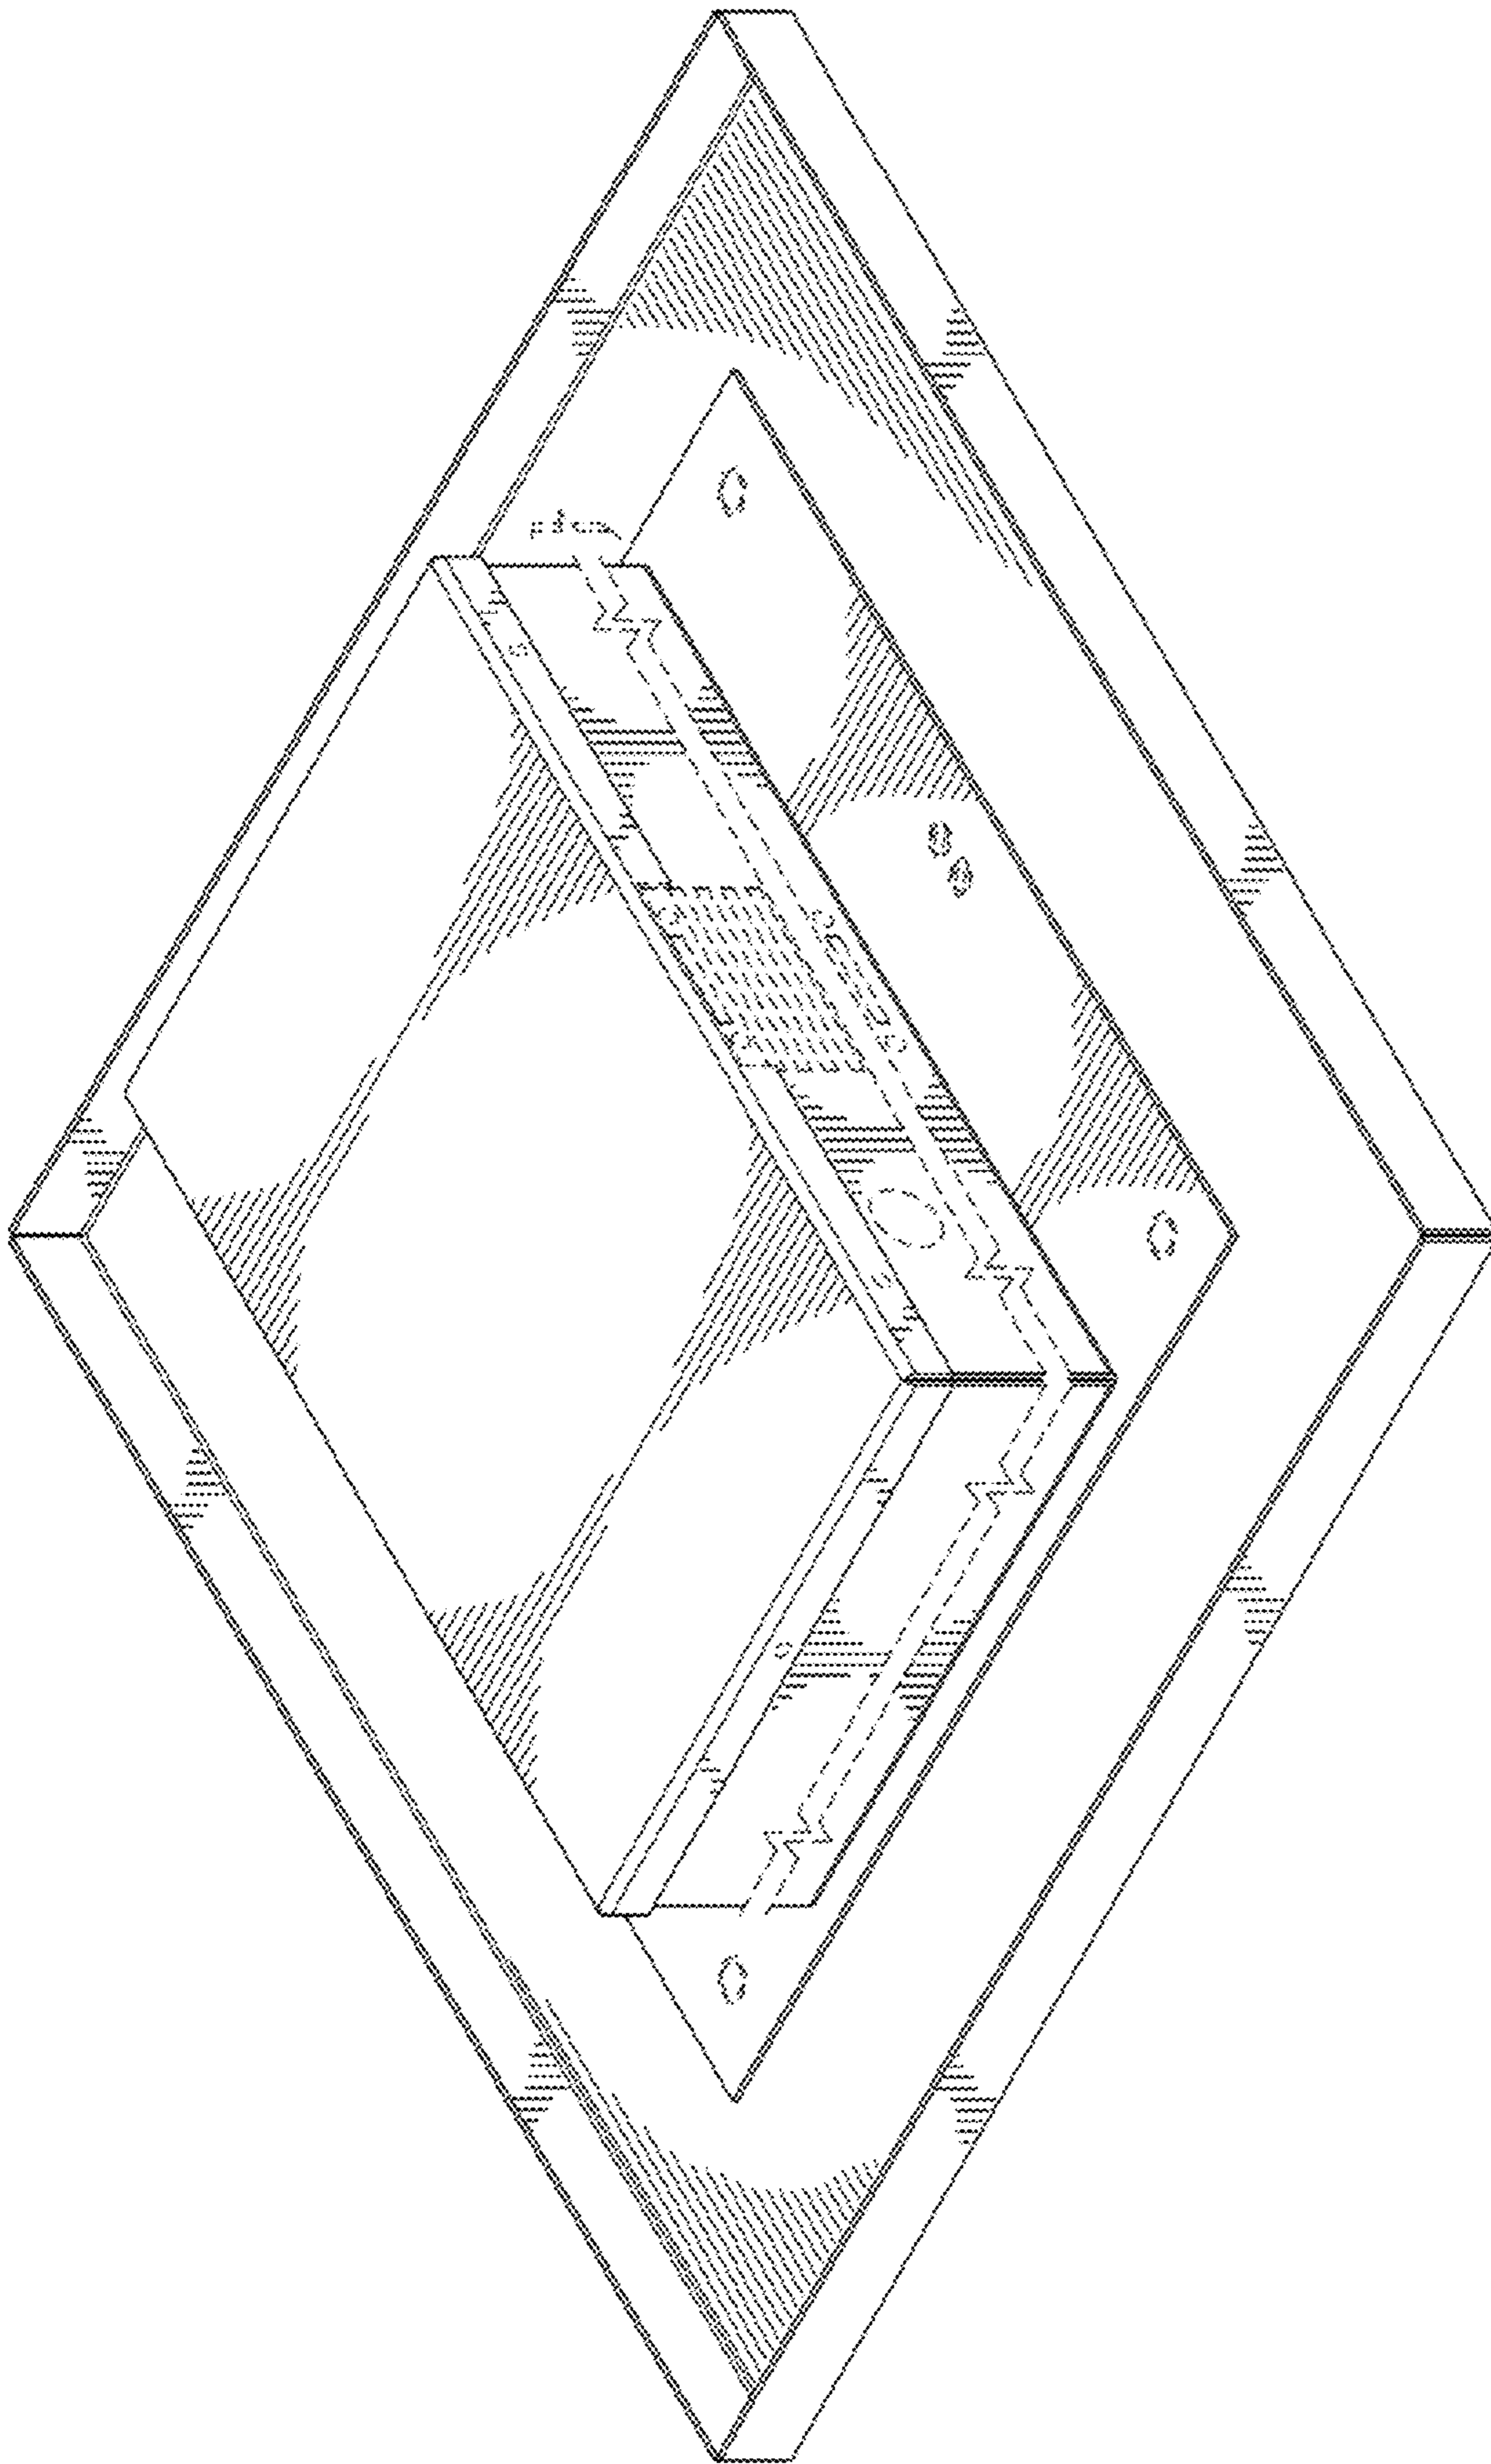


FIG. 1

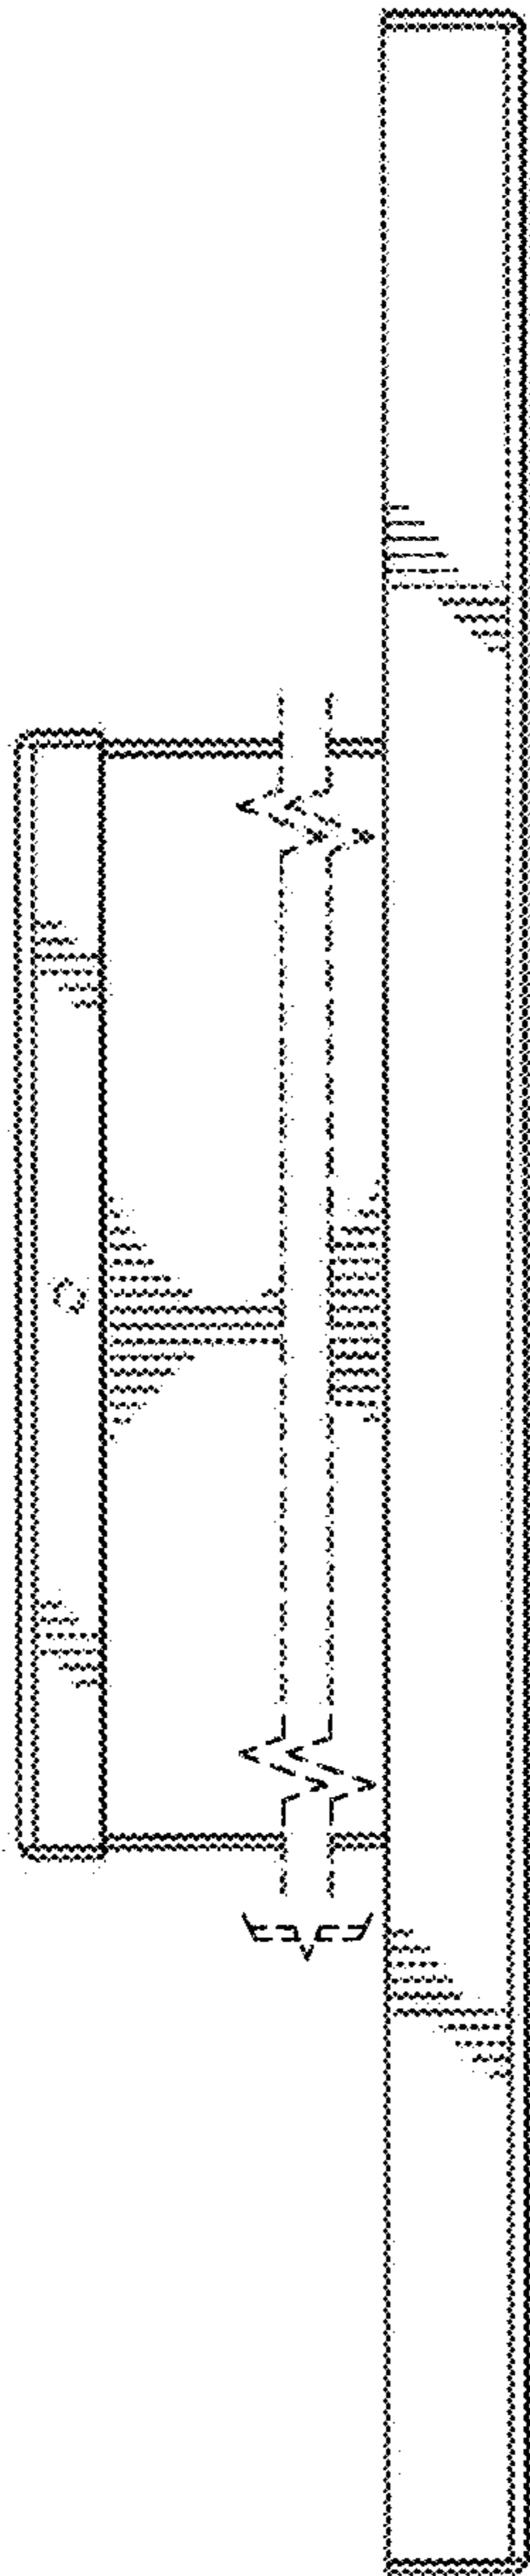


FIG. 2

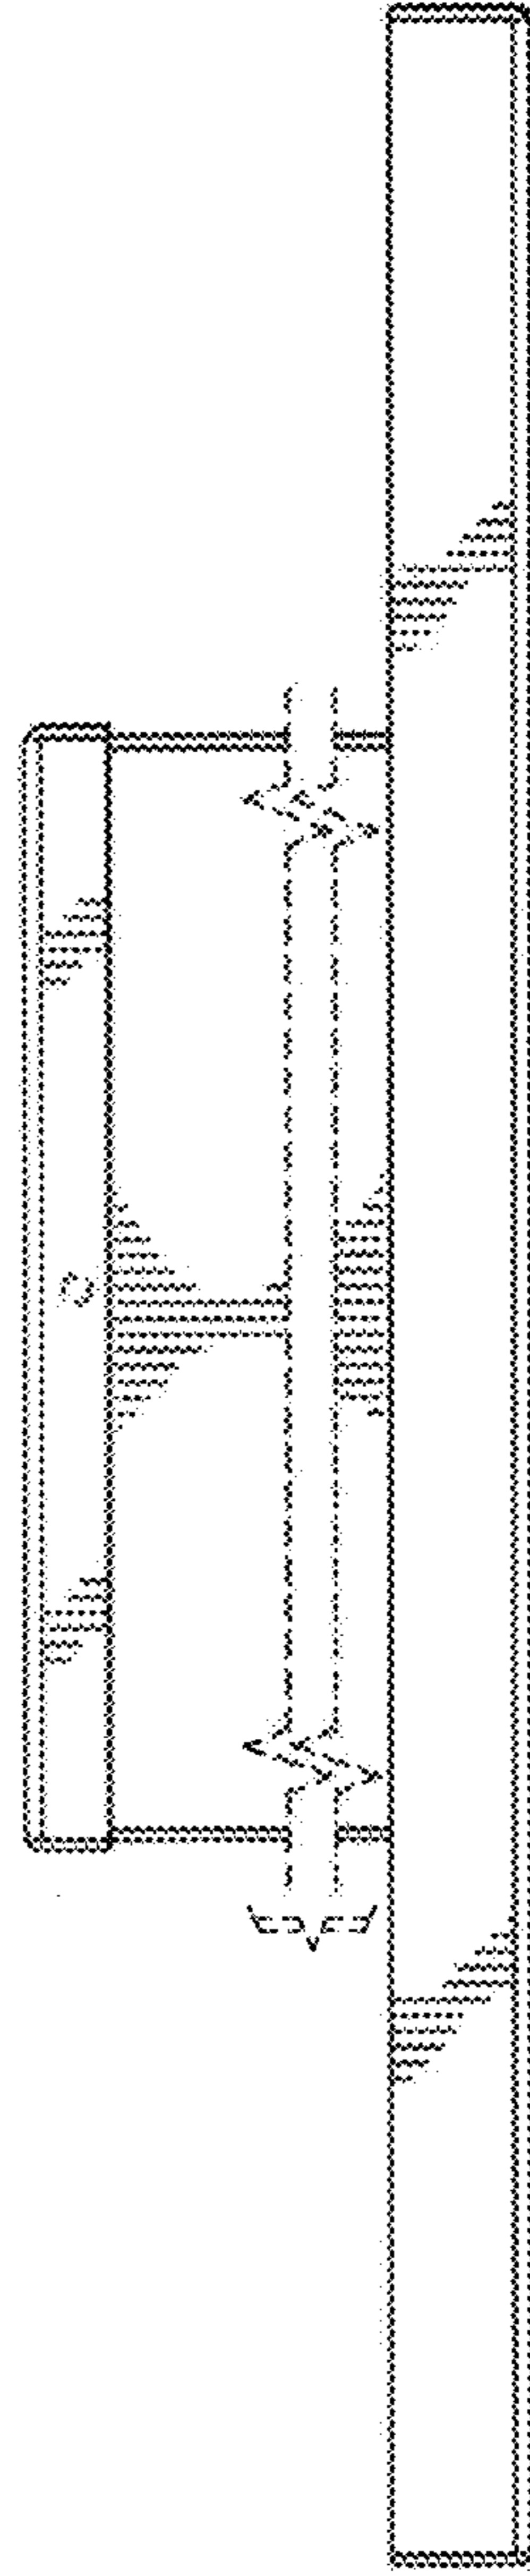


FIG. 3

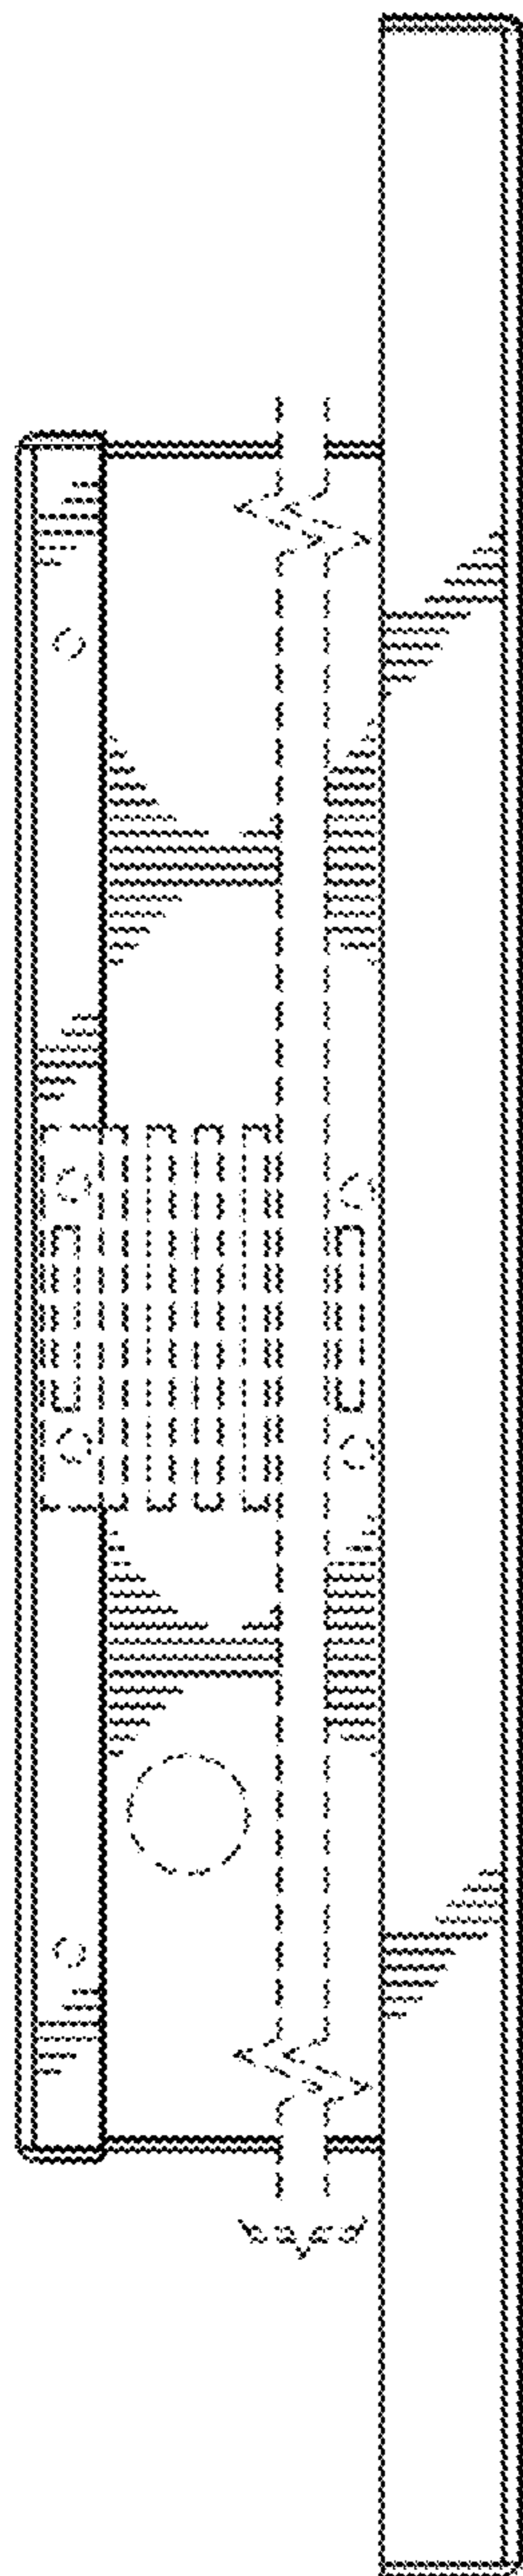


FIG. 4

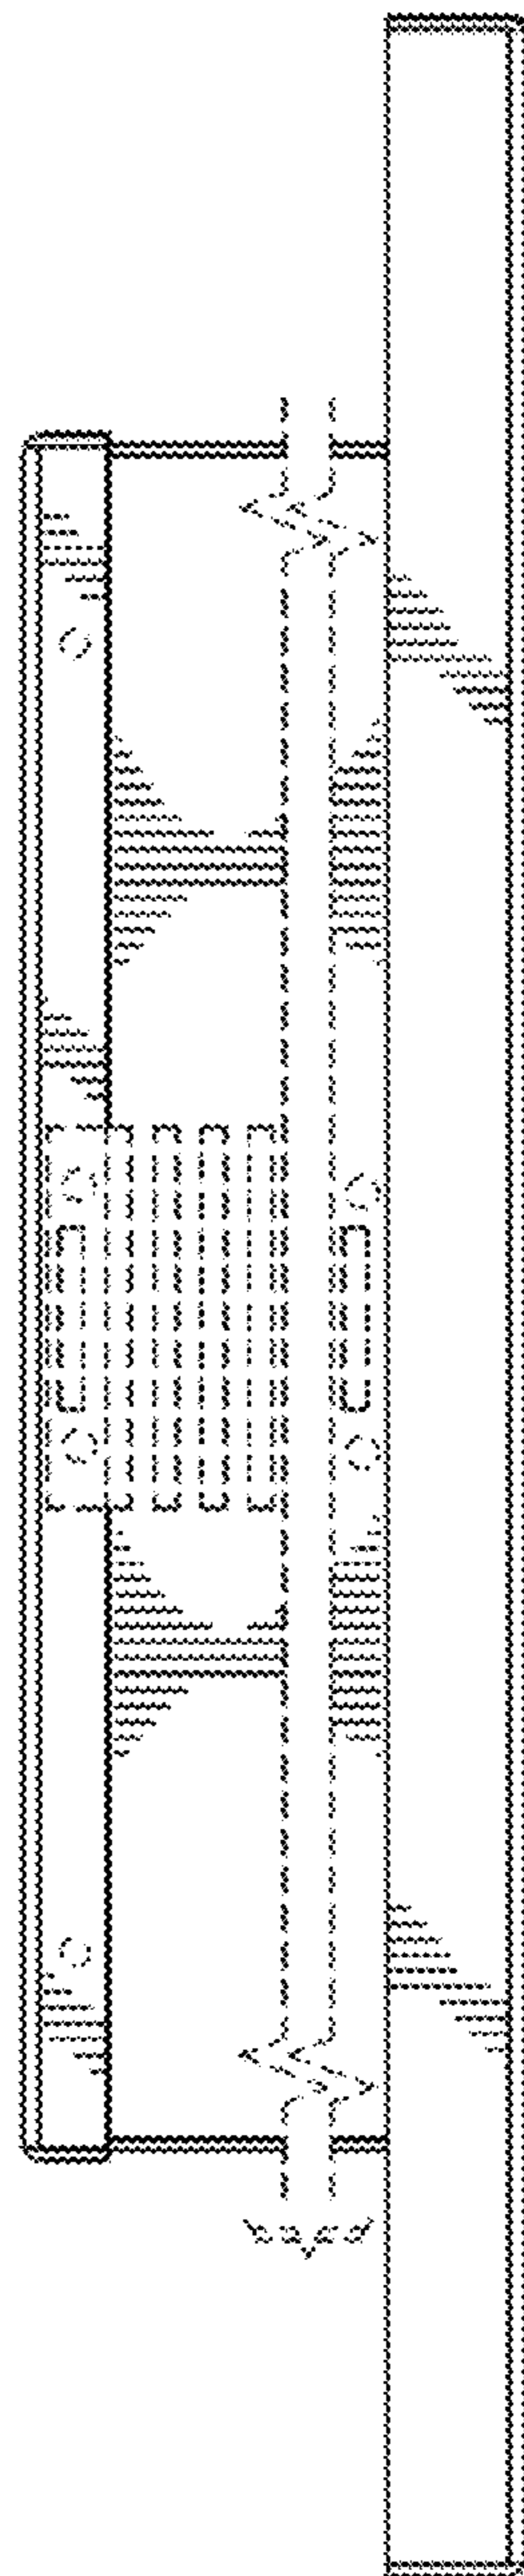


FIG. 5

FIG. 6

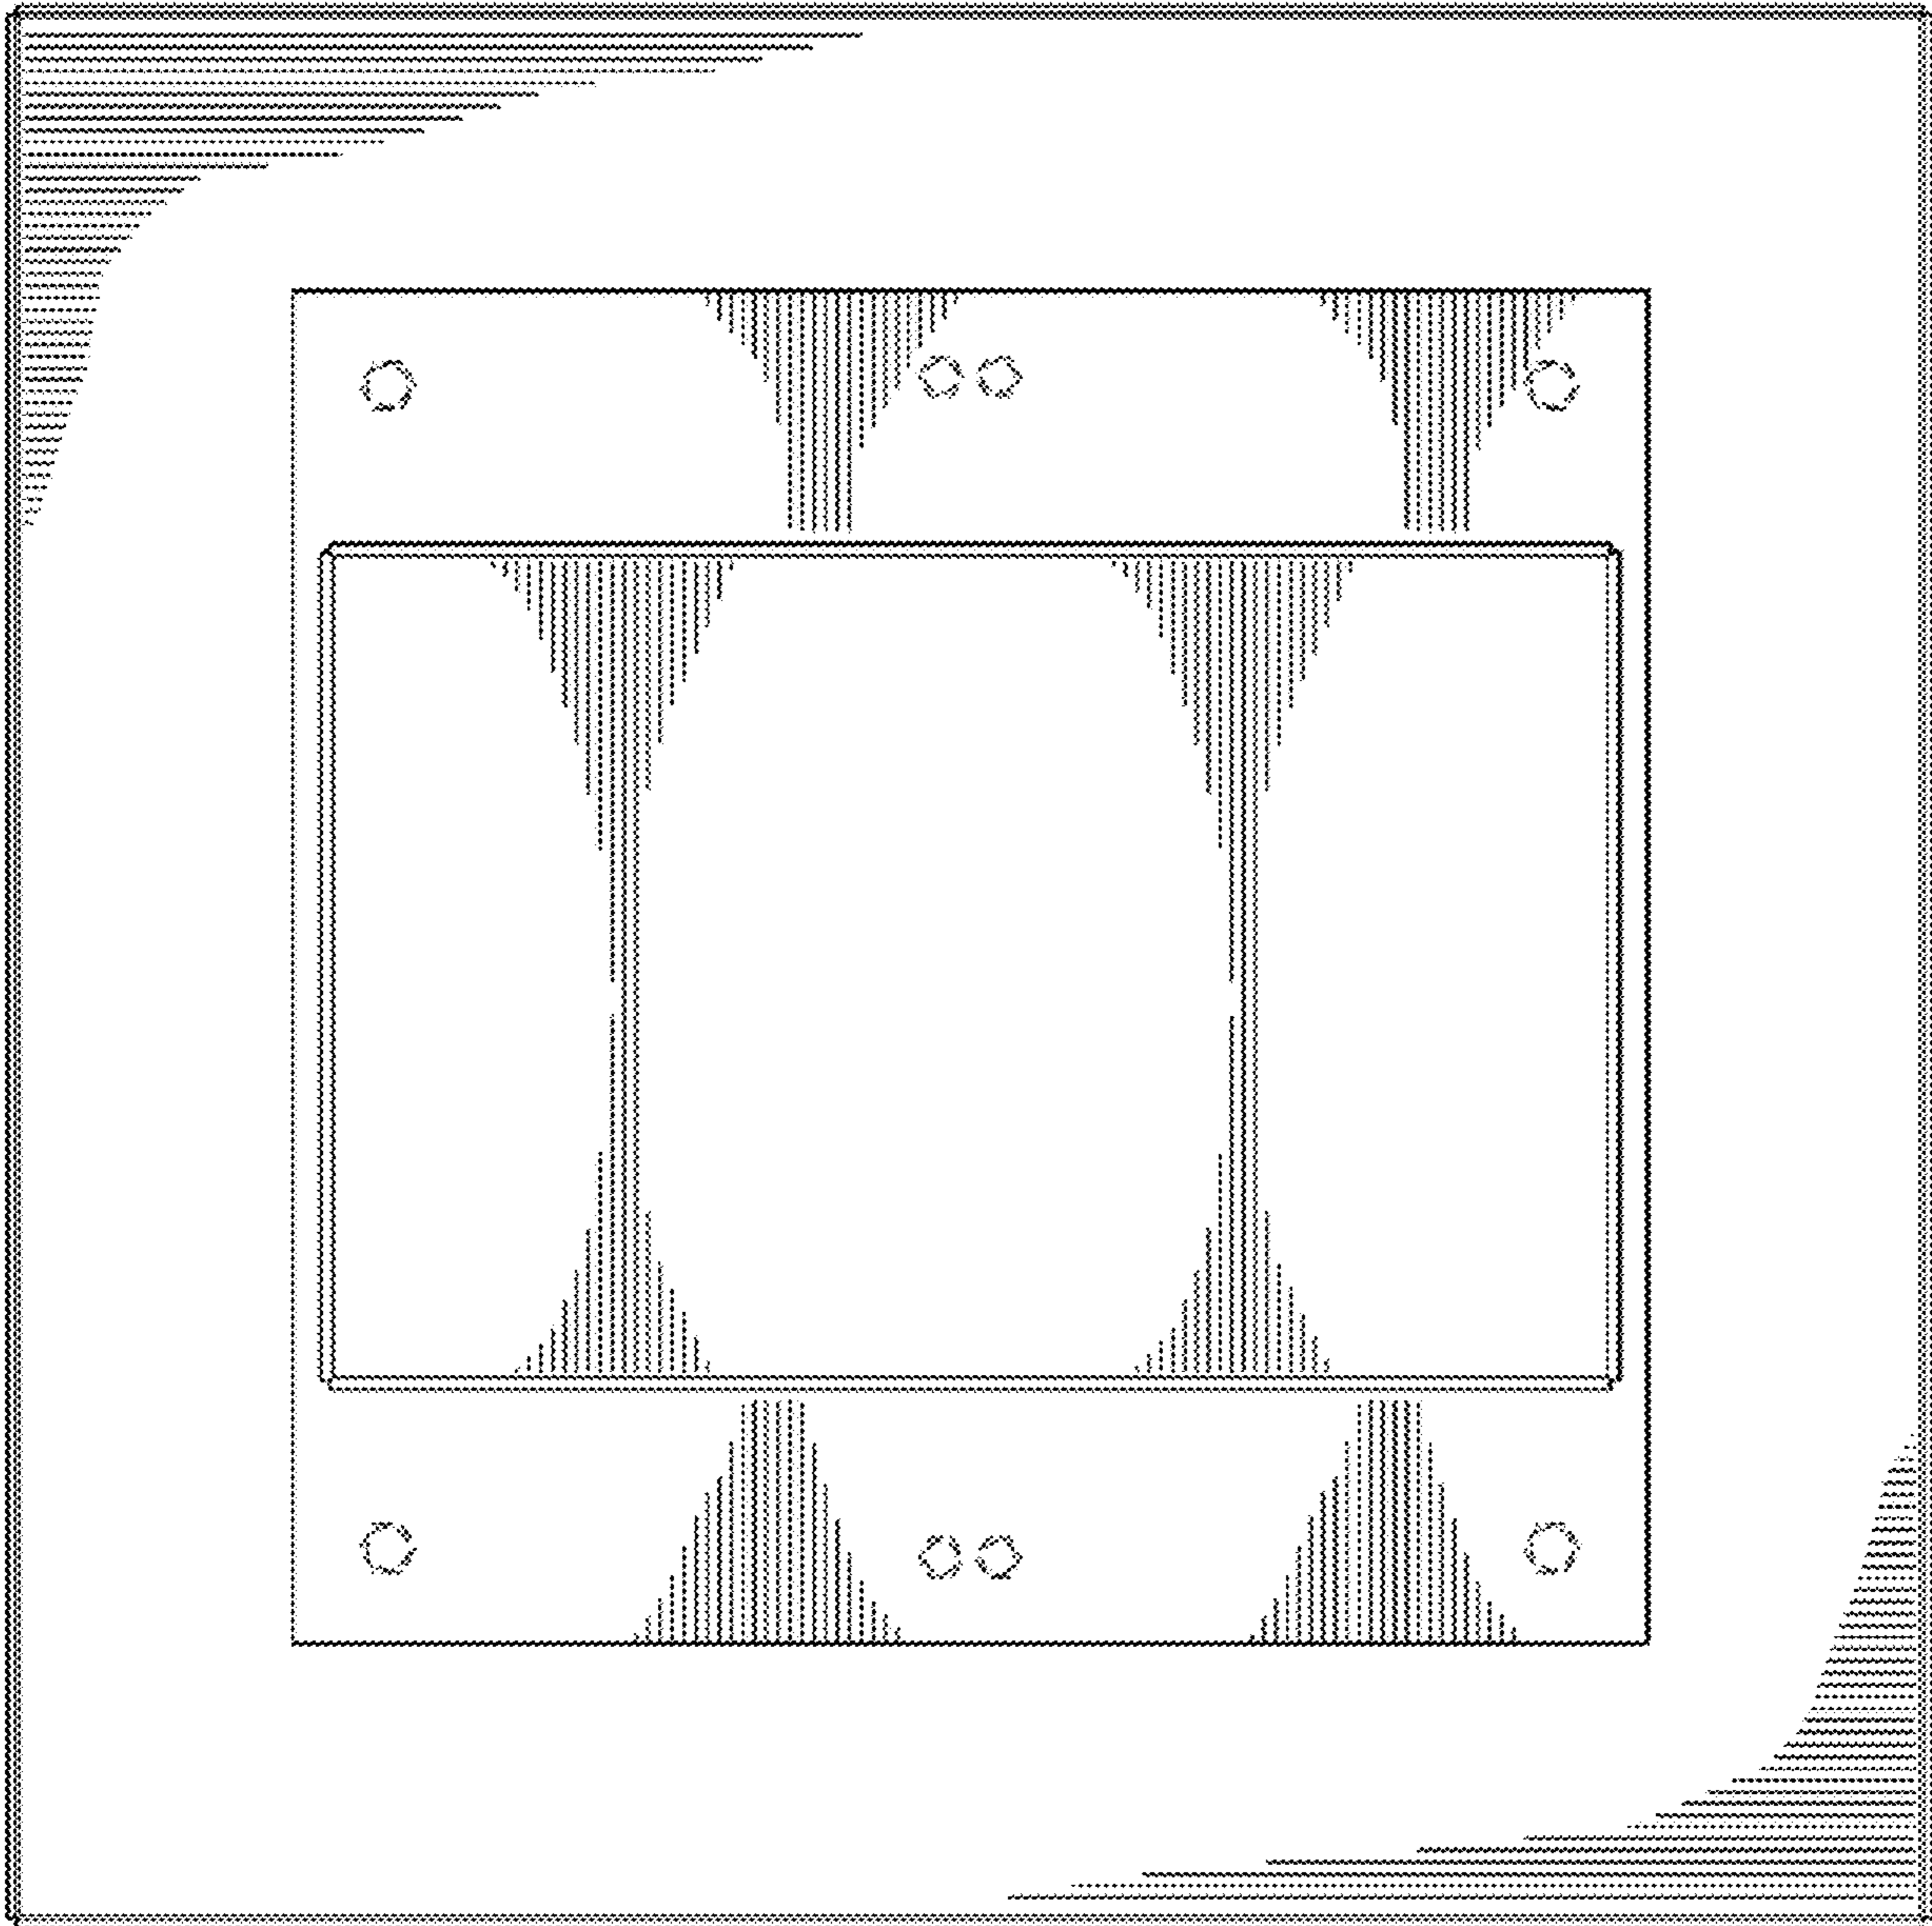
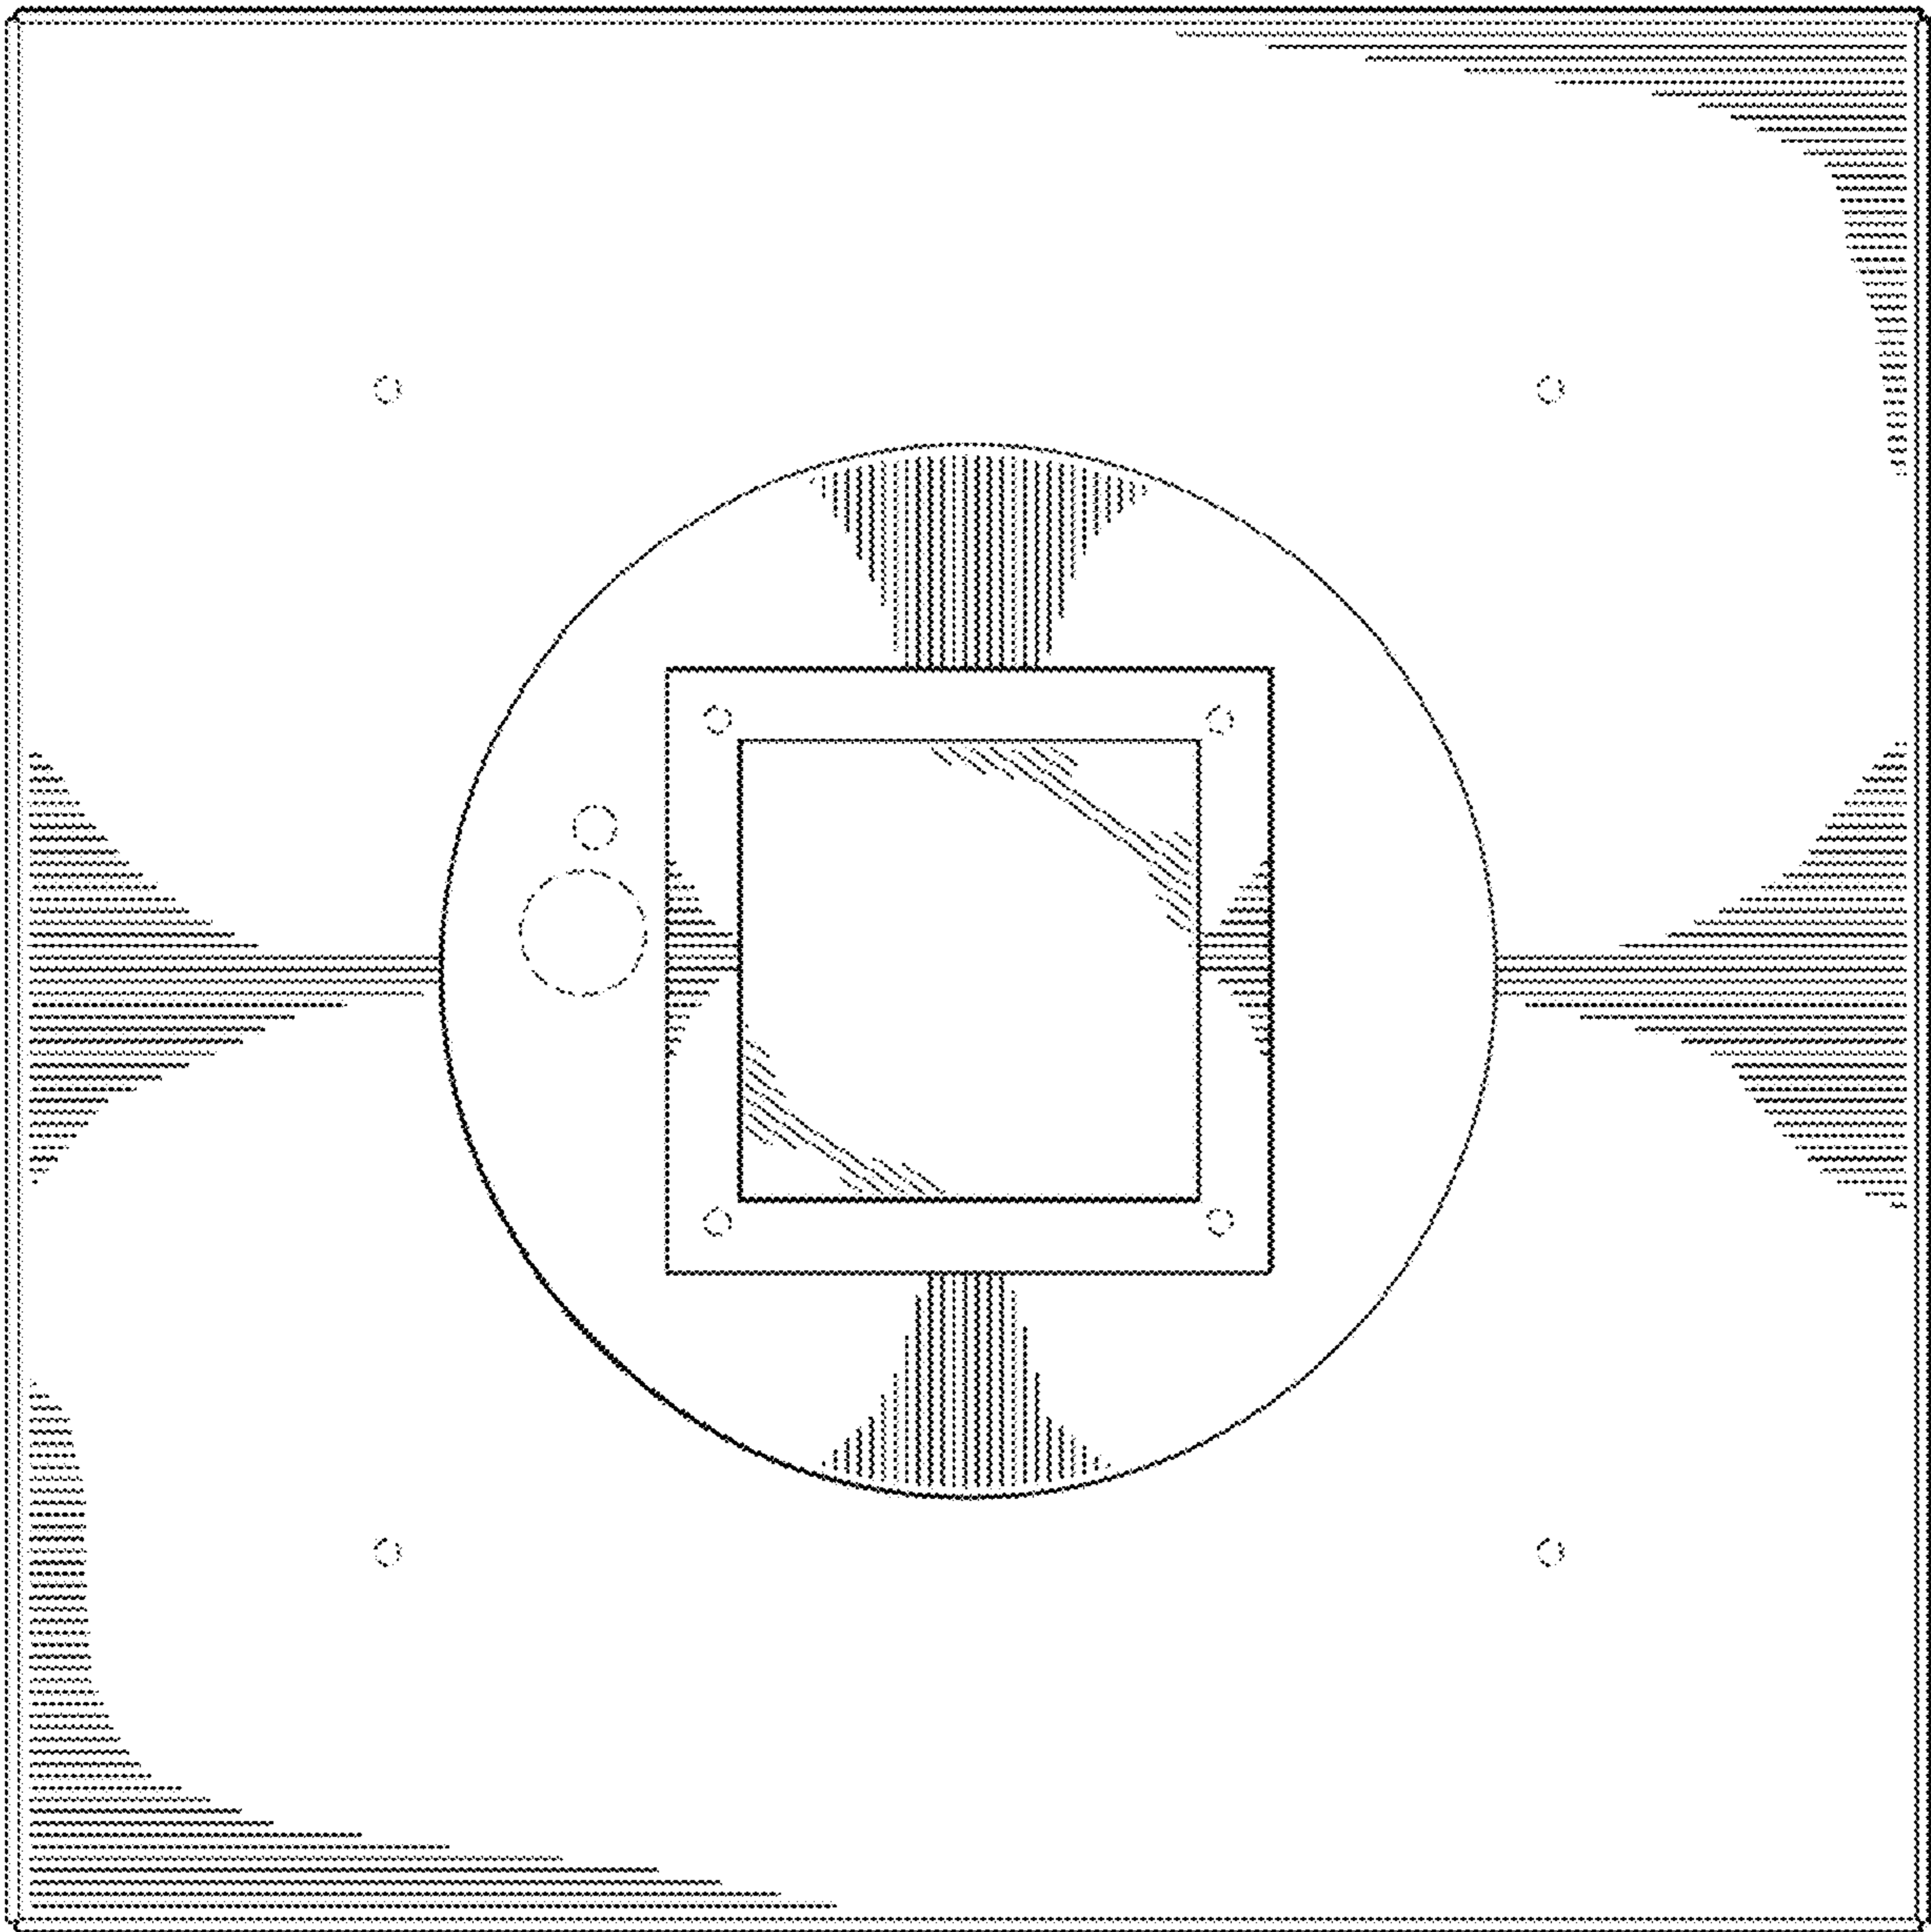


FIG. 7



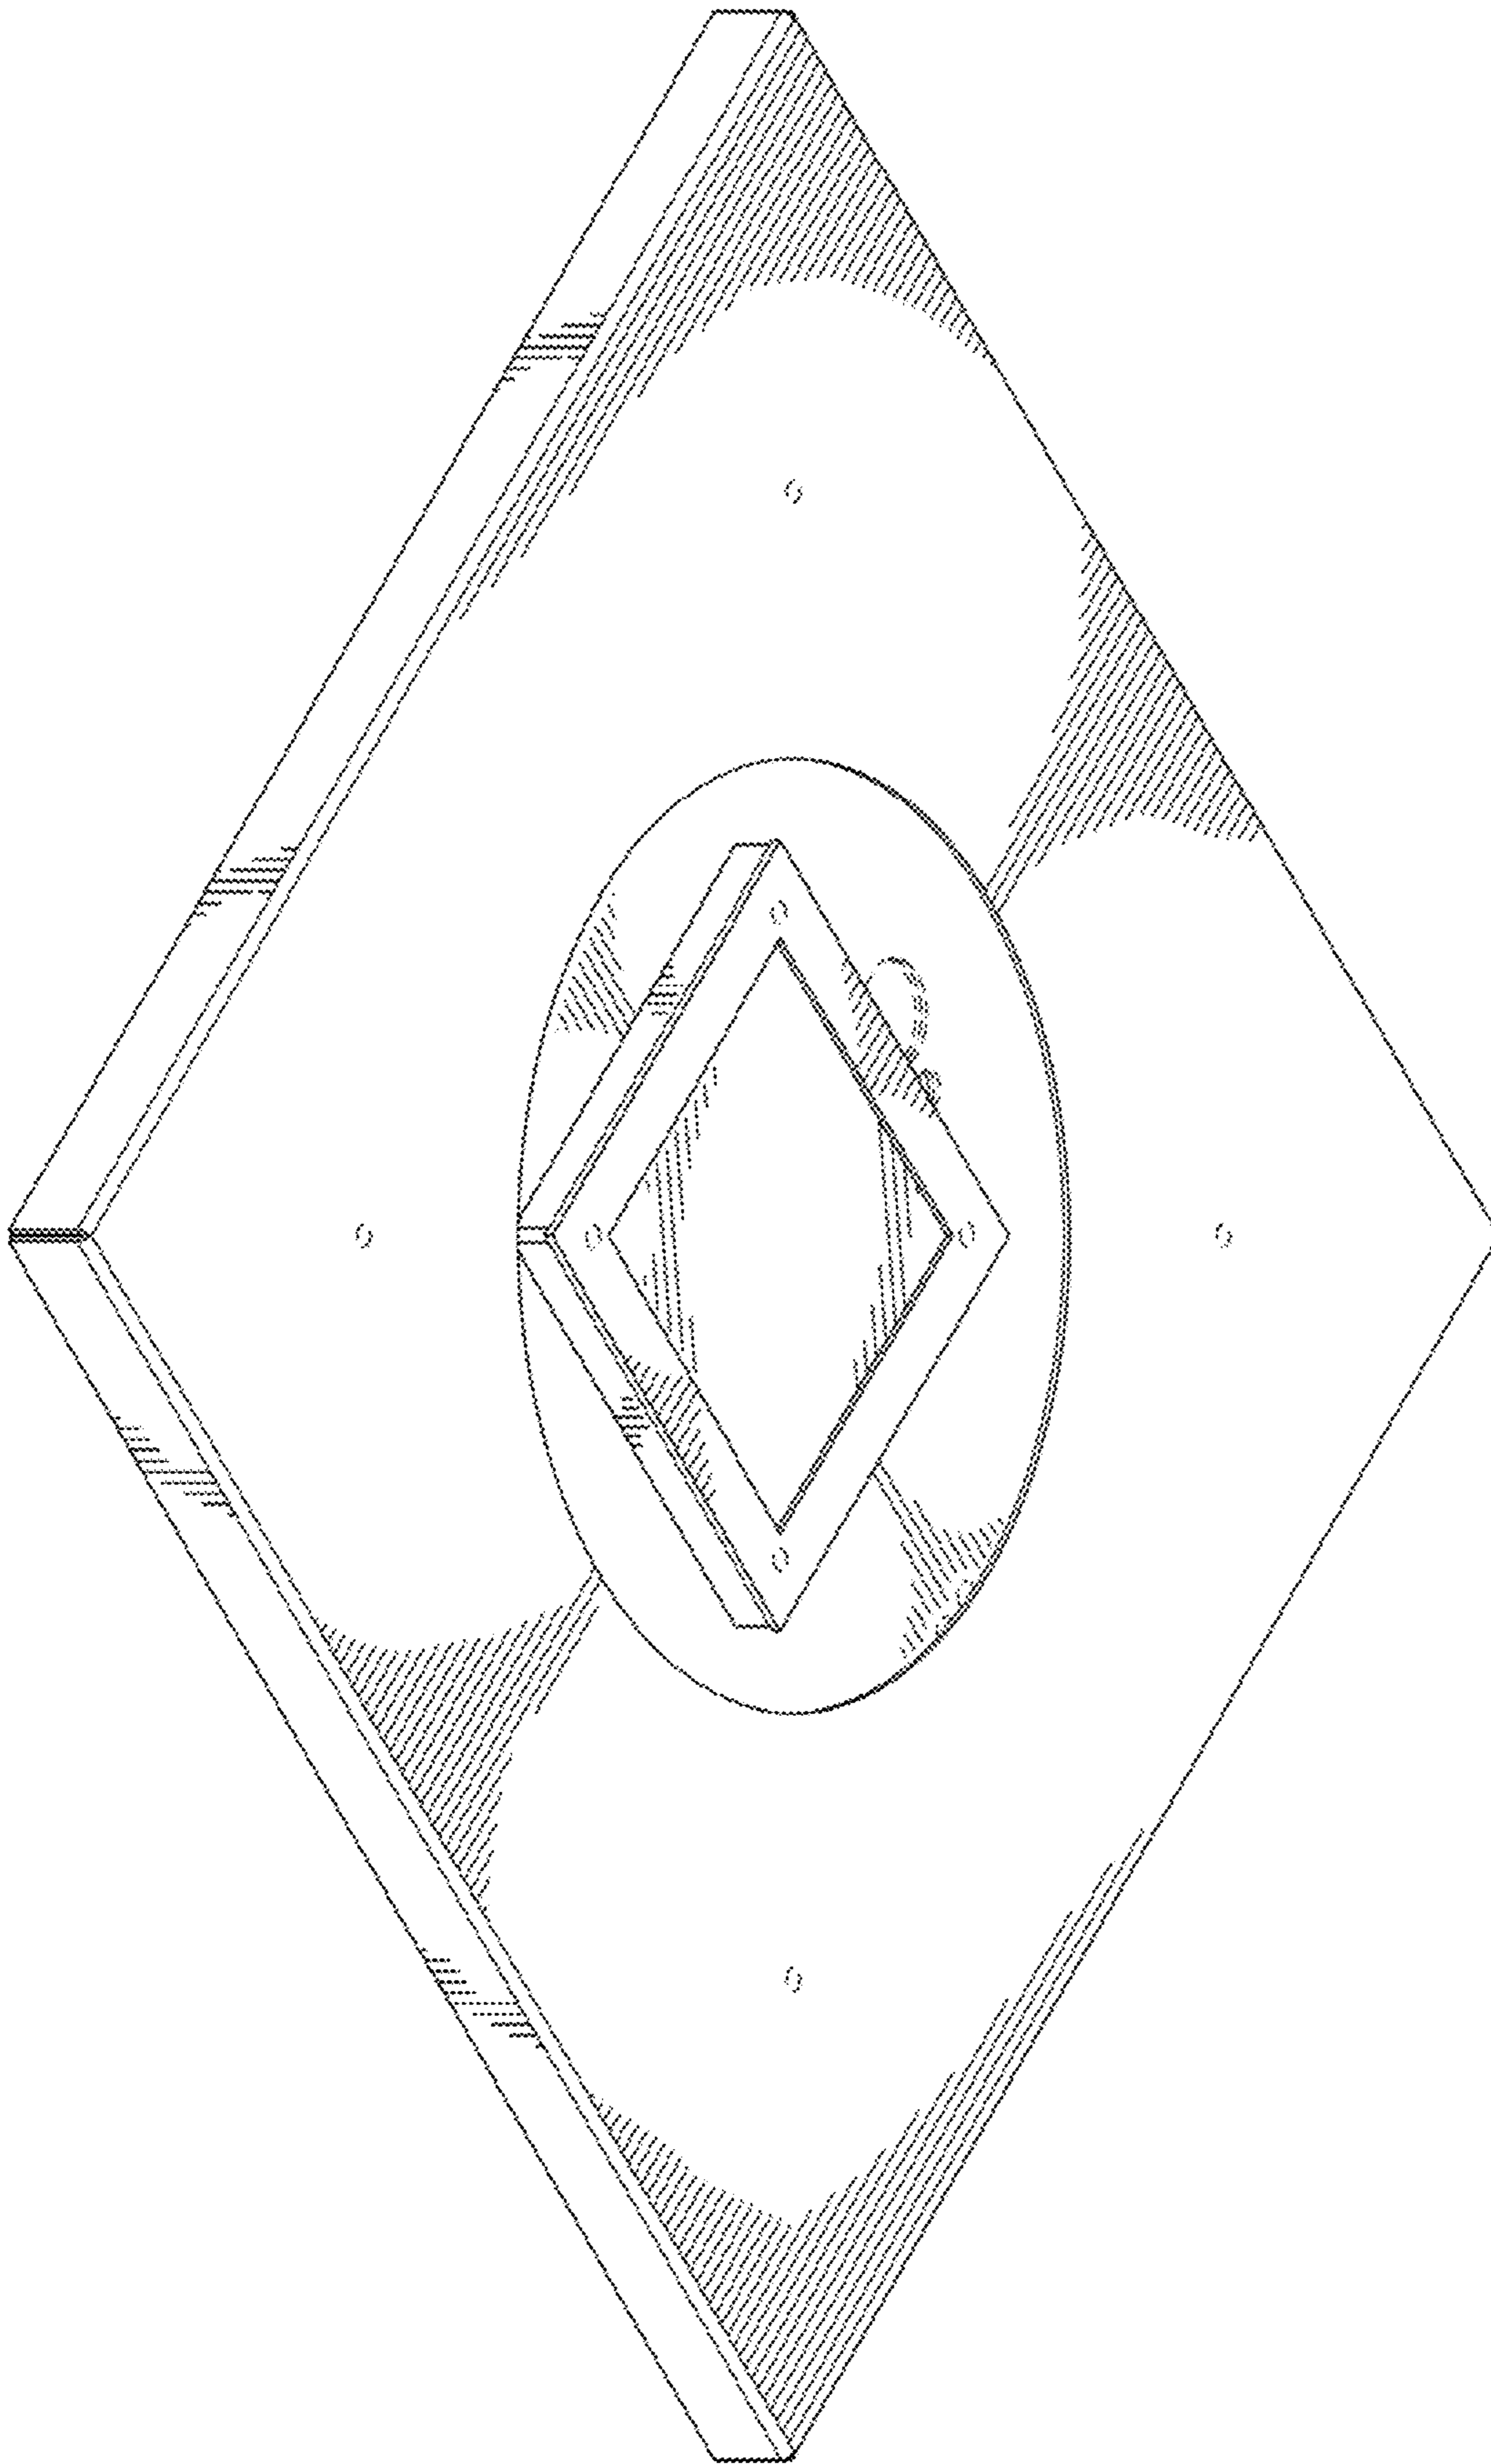


FIG. 8