

US00D878598S

(12) **United States Design Patent**
Hubler et al.

(10) **Patent No.:** **US D878,598 S**
(45) **Date of Patent:** **** Mar. 17, 2020**

(54) **PART OF A CATHETER MANIPULATION DEVICE**

(71) Applicant: **Intuitive Surgical Operations, Inc.**, Sunnyvale, CA (US)

(72) Inventors: **Robert B. Hubler**, Woodinville, WA (US); **Timothy B. Hulford**, San Jose, CA (US)

(73) Assignee: **INTUITIVE SURGICAL OPERATIONS, INC.**, Sunnyvale, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/648,126**

(22) Filed: **May 18, 2018**

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/185; D24/164**

(58) **Field of Classification Search**
USPC D24/185, 164, 110, 128, 165, 107, 129, D24/186; D10/81; D14/154
CPC A61B 17/12022; A61B 1/00098; A61B 10/04; A61H 23/06; A61M 25/0111; A61M 16/0488
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 2,955,592 A * 10/1960 MacLean A61B 10/04 600/569
- 3,316,913 A * 5/1967 Swenson A61M 16/0488 606/108
- 3,335,723 A * 8/1967 Waldman, Jr. A61M 25/0111 604/163
- 3,368,552 A * 2/1968 Bottcher A61B 1/00098 600/107
- 4,745,910 A * 5/1988 Day A61H 23/06 601/107

- 4,950,280 A * 8/1990 Brennan A61B 17/12022 604/1
 - D731,048 S * 6/2015 Winter D24/107
 - D755,392 S * 5/2016 Hwang D24/165
 - D757,242 S * 5/2016 Maksym D24/110
- (Continued)

OTHER PUBLICATIONS

Vertut, Jean and Phillipe Coiffet, Robot Technology: Teleoperation and Robotics Evolution and Development, English translation, Prentice-Hall, Inc., Englewood Cliffs, NJ, USA 1986, vol. 3A, 332 pages.

Primary Examiner — Rhea Shields

(74) *Attorney, Agent, or Firm* — Haynes and Boone, LLP

(57) **CLAIM**

The ornamental design for a part of a catheter manipulation device, as shown and described.

DESCRIPTION


This application is related to U.S. application Ser. No. 29/648,128, filed May 18, 2018, the entire disclosure of which is hereby incorporated herein by reference.

FIG. 1 is a perspective view of a part of a catheter manipulation device showing our new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a right side elevational view thereof;
FIG. 5 is a left side elevational view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof; and,
FIGS. 8, 9, 10, and 11 are additional perspective views thereof.

The broken lines shown in FIGS. 1-11 illustrate unclaimed portions of the part of a catheter manipulation device and form no part of the claimed design.

The part of a catheter manipulation device illustrated in FIGS. 1-11 may be, for example, a catheter manipulation device.

1 Claim, 9 Drawing Sheets

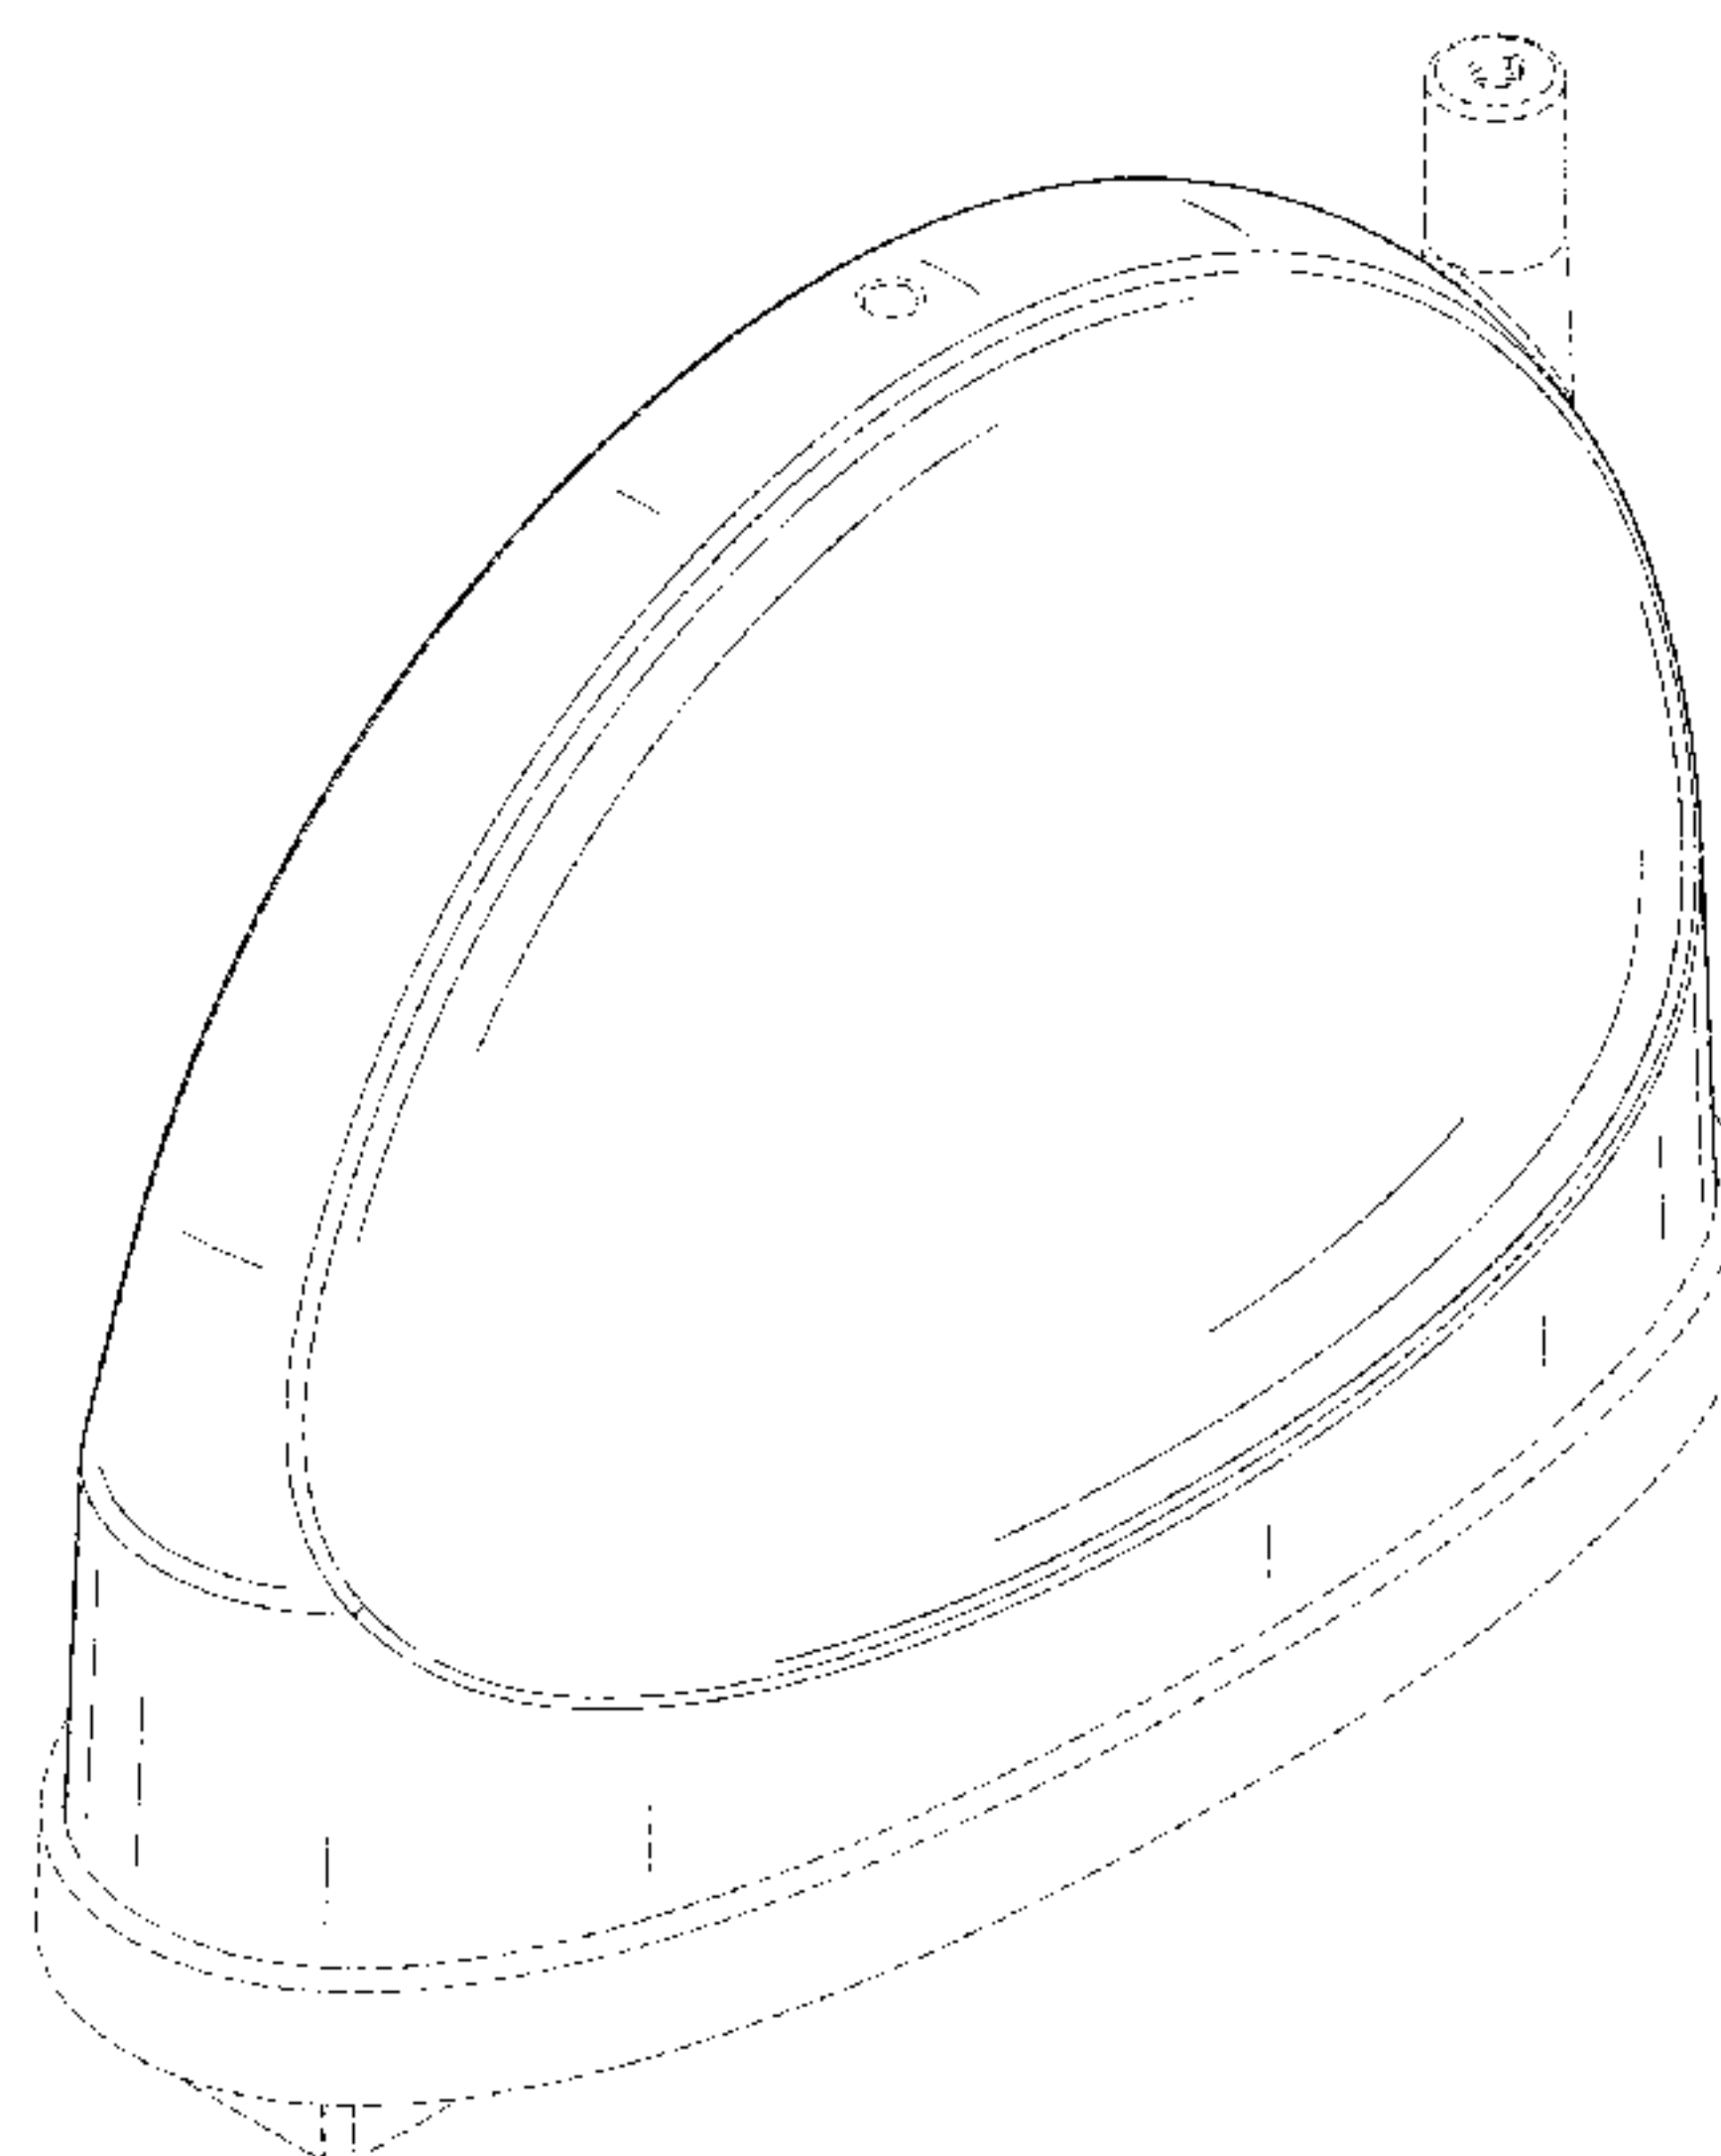

(56)

References Cited

U.S. PATENT DOCUMENTS

D773,034 S	*	11/2016	Allnutt	D24/110
D773,035 S	*	11/2016	Neuner	D24/110
D773,055 S	*	11/2016	Krauss	D10/81
D797,829 S	*	9/2017	Lv	D14/154
D804,659 S	*	12/2017	Hood	D24/128
D805,629 S	*	12/2017	Fiorenza	D24/110
D815,292 S	*	4/2018	Goldman	D24/186
D835,260 S	*	12/2018	Lisberg	D24/110
D837,365 S	*	1/2019	Li	D24/110
D840,529 S	*	2/2019	Steinberg	D24/110
D848,617 S	*	5/2019	Ramstad	D24/129
D855,792 S	*	8/2019	Toksoz	D24/110
D858,745 S	*	9/2019	Kurgan	D24/110

* cited by examiner

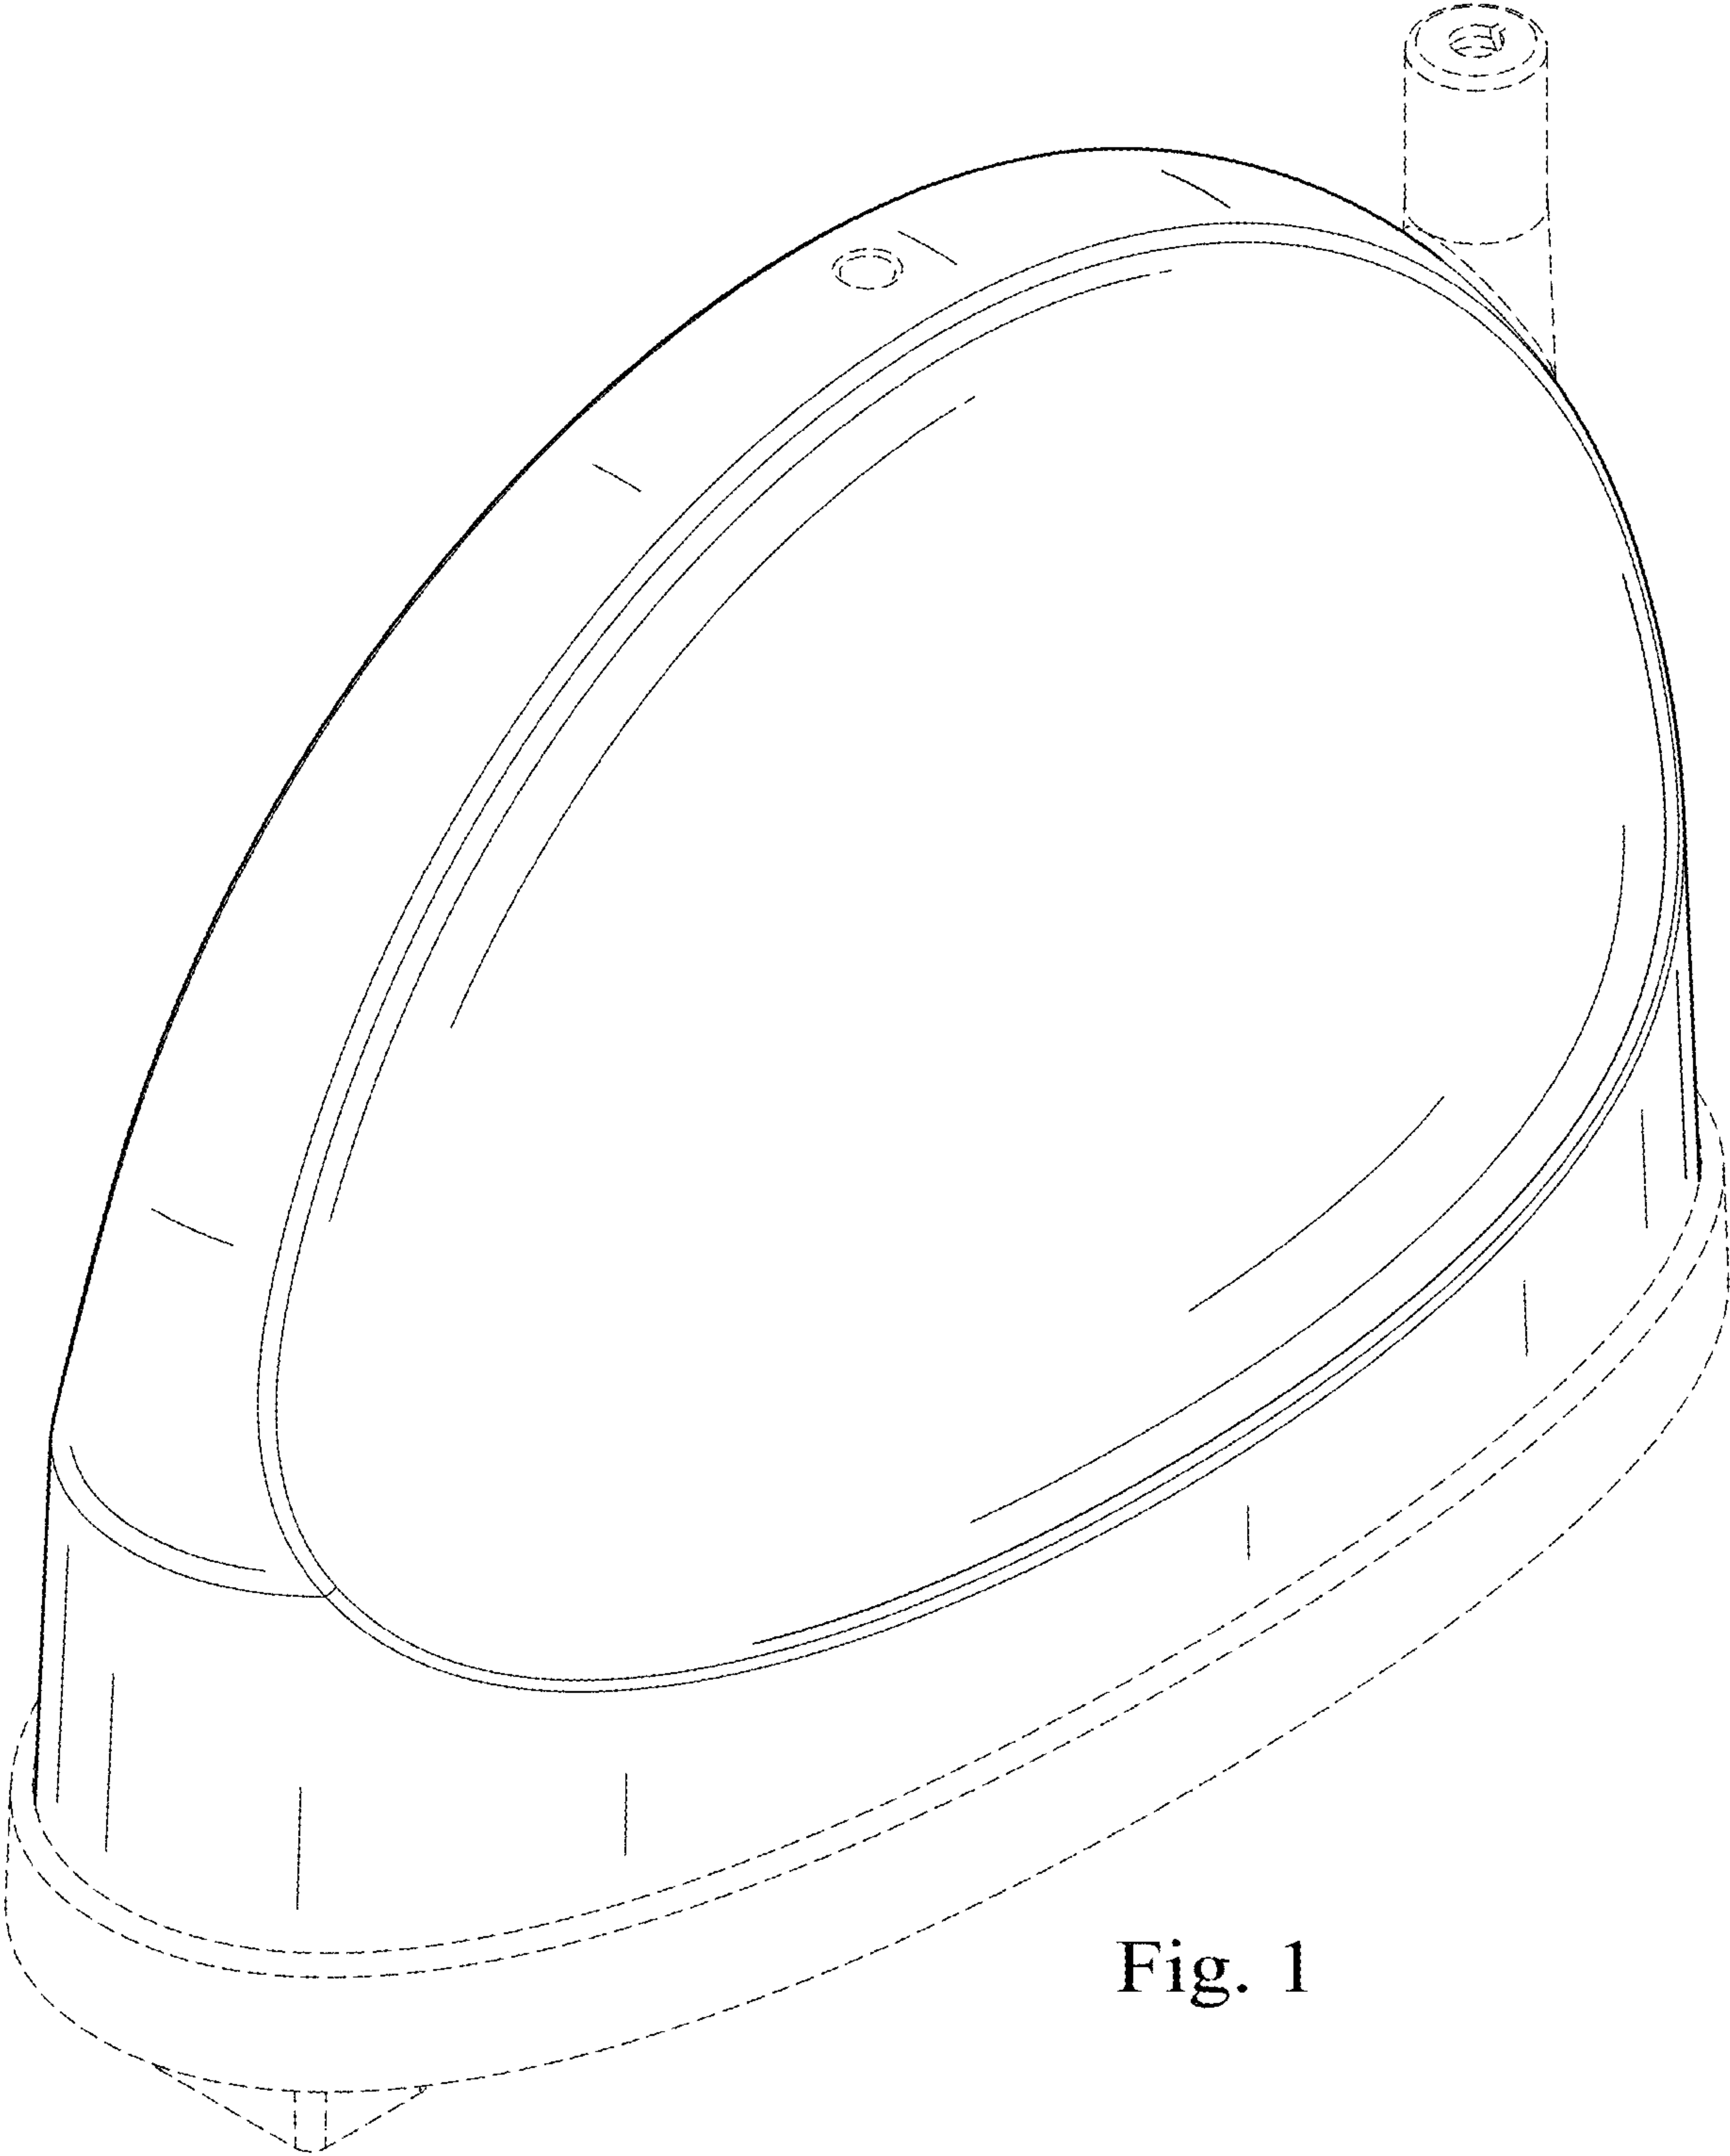


Fig. 1

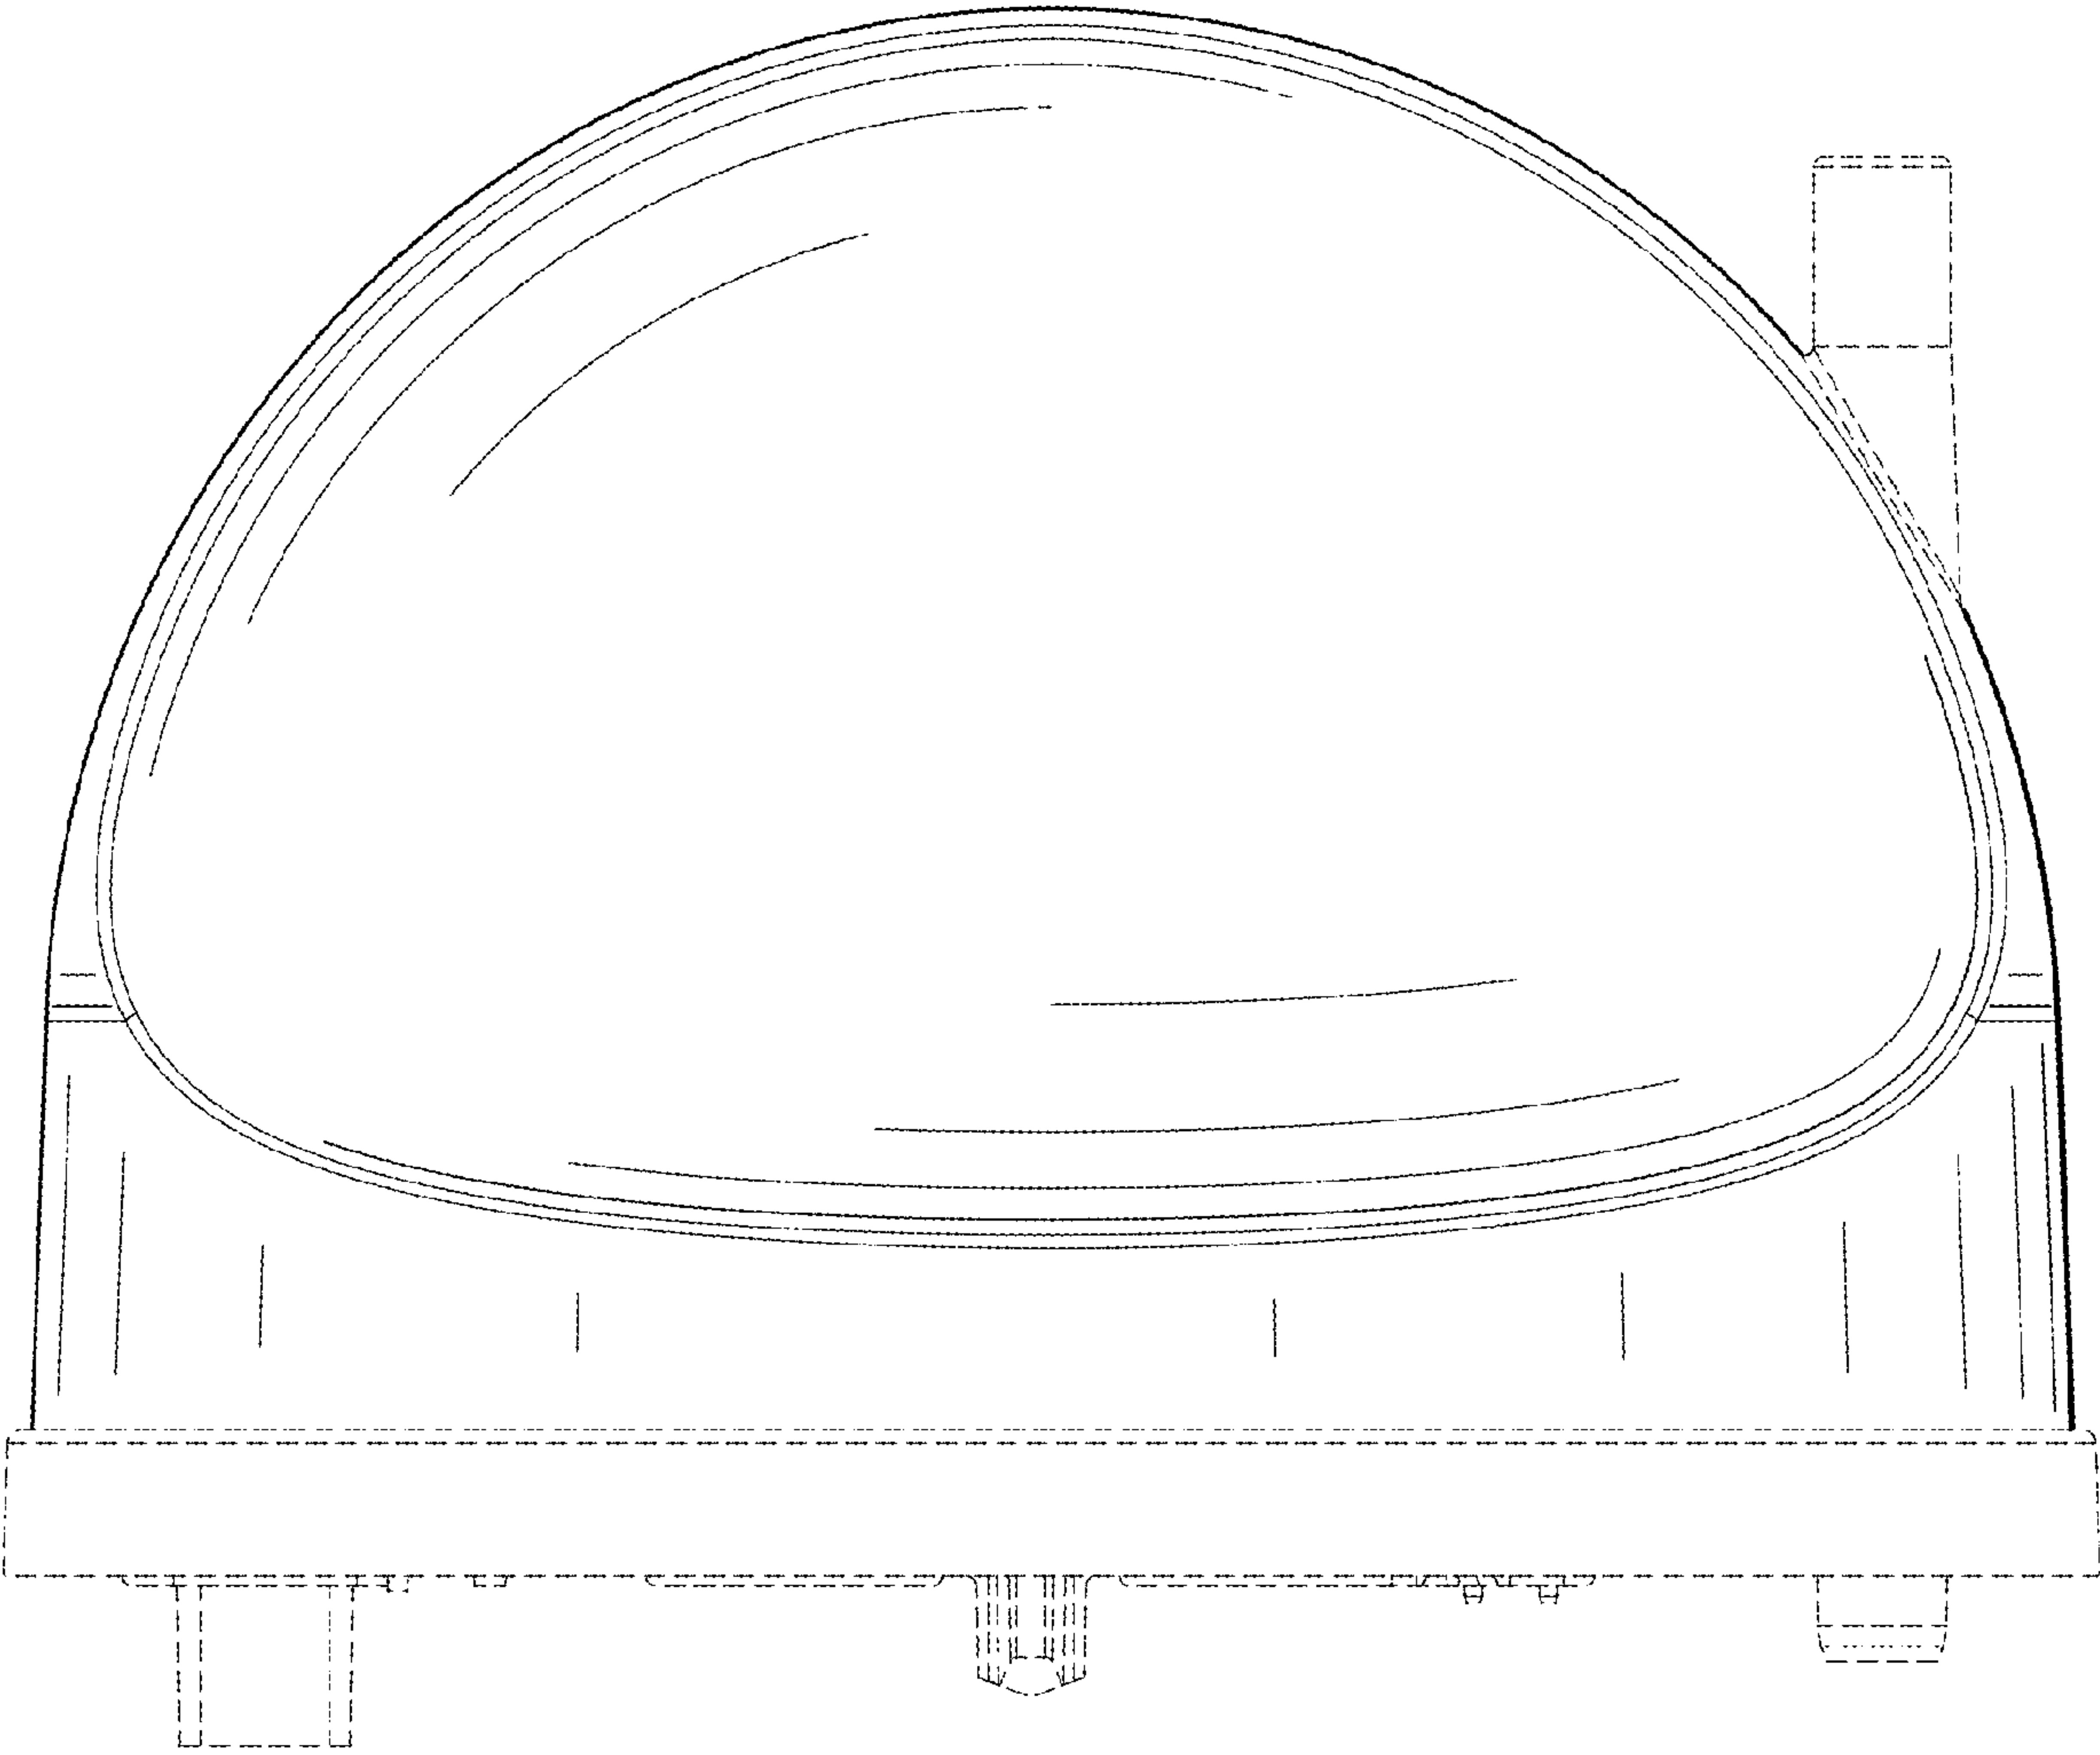


Fig. 2

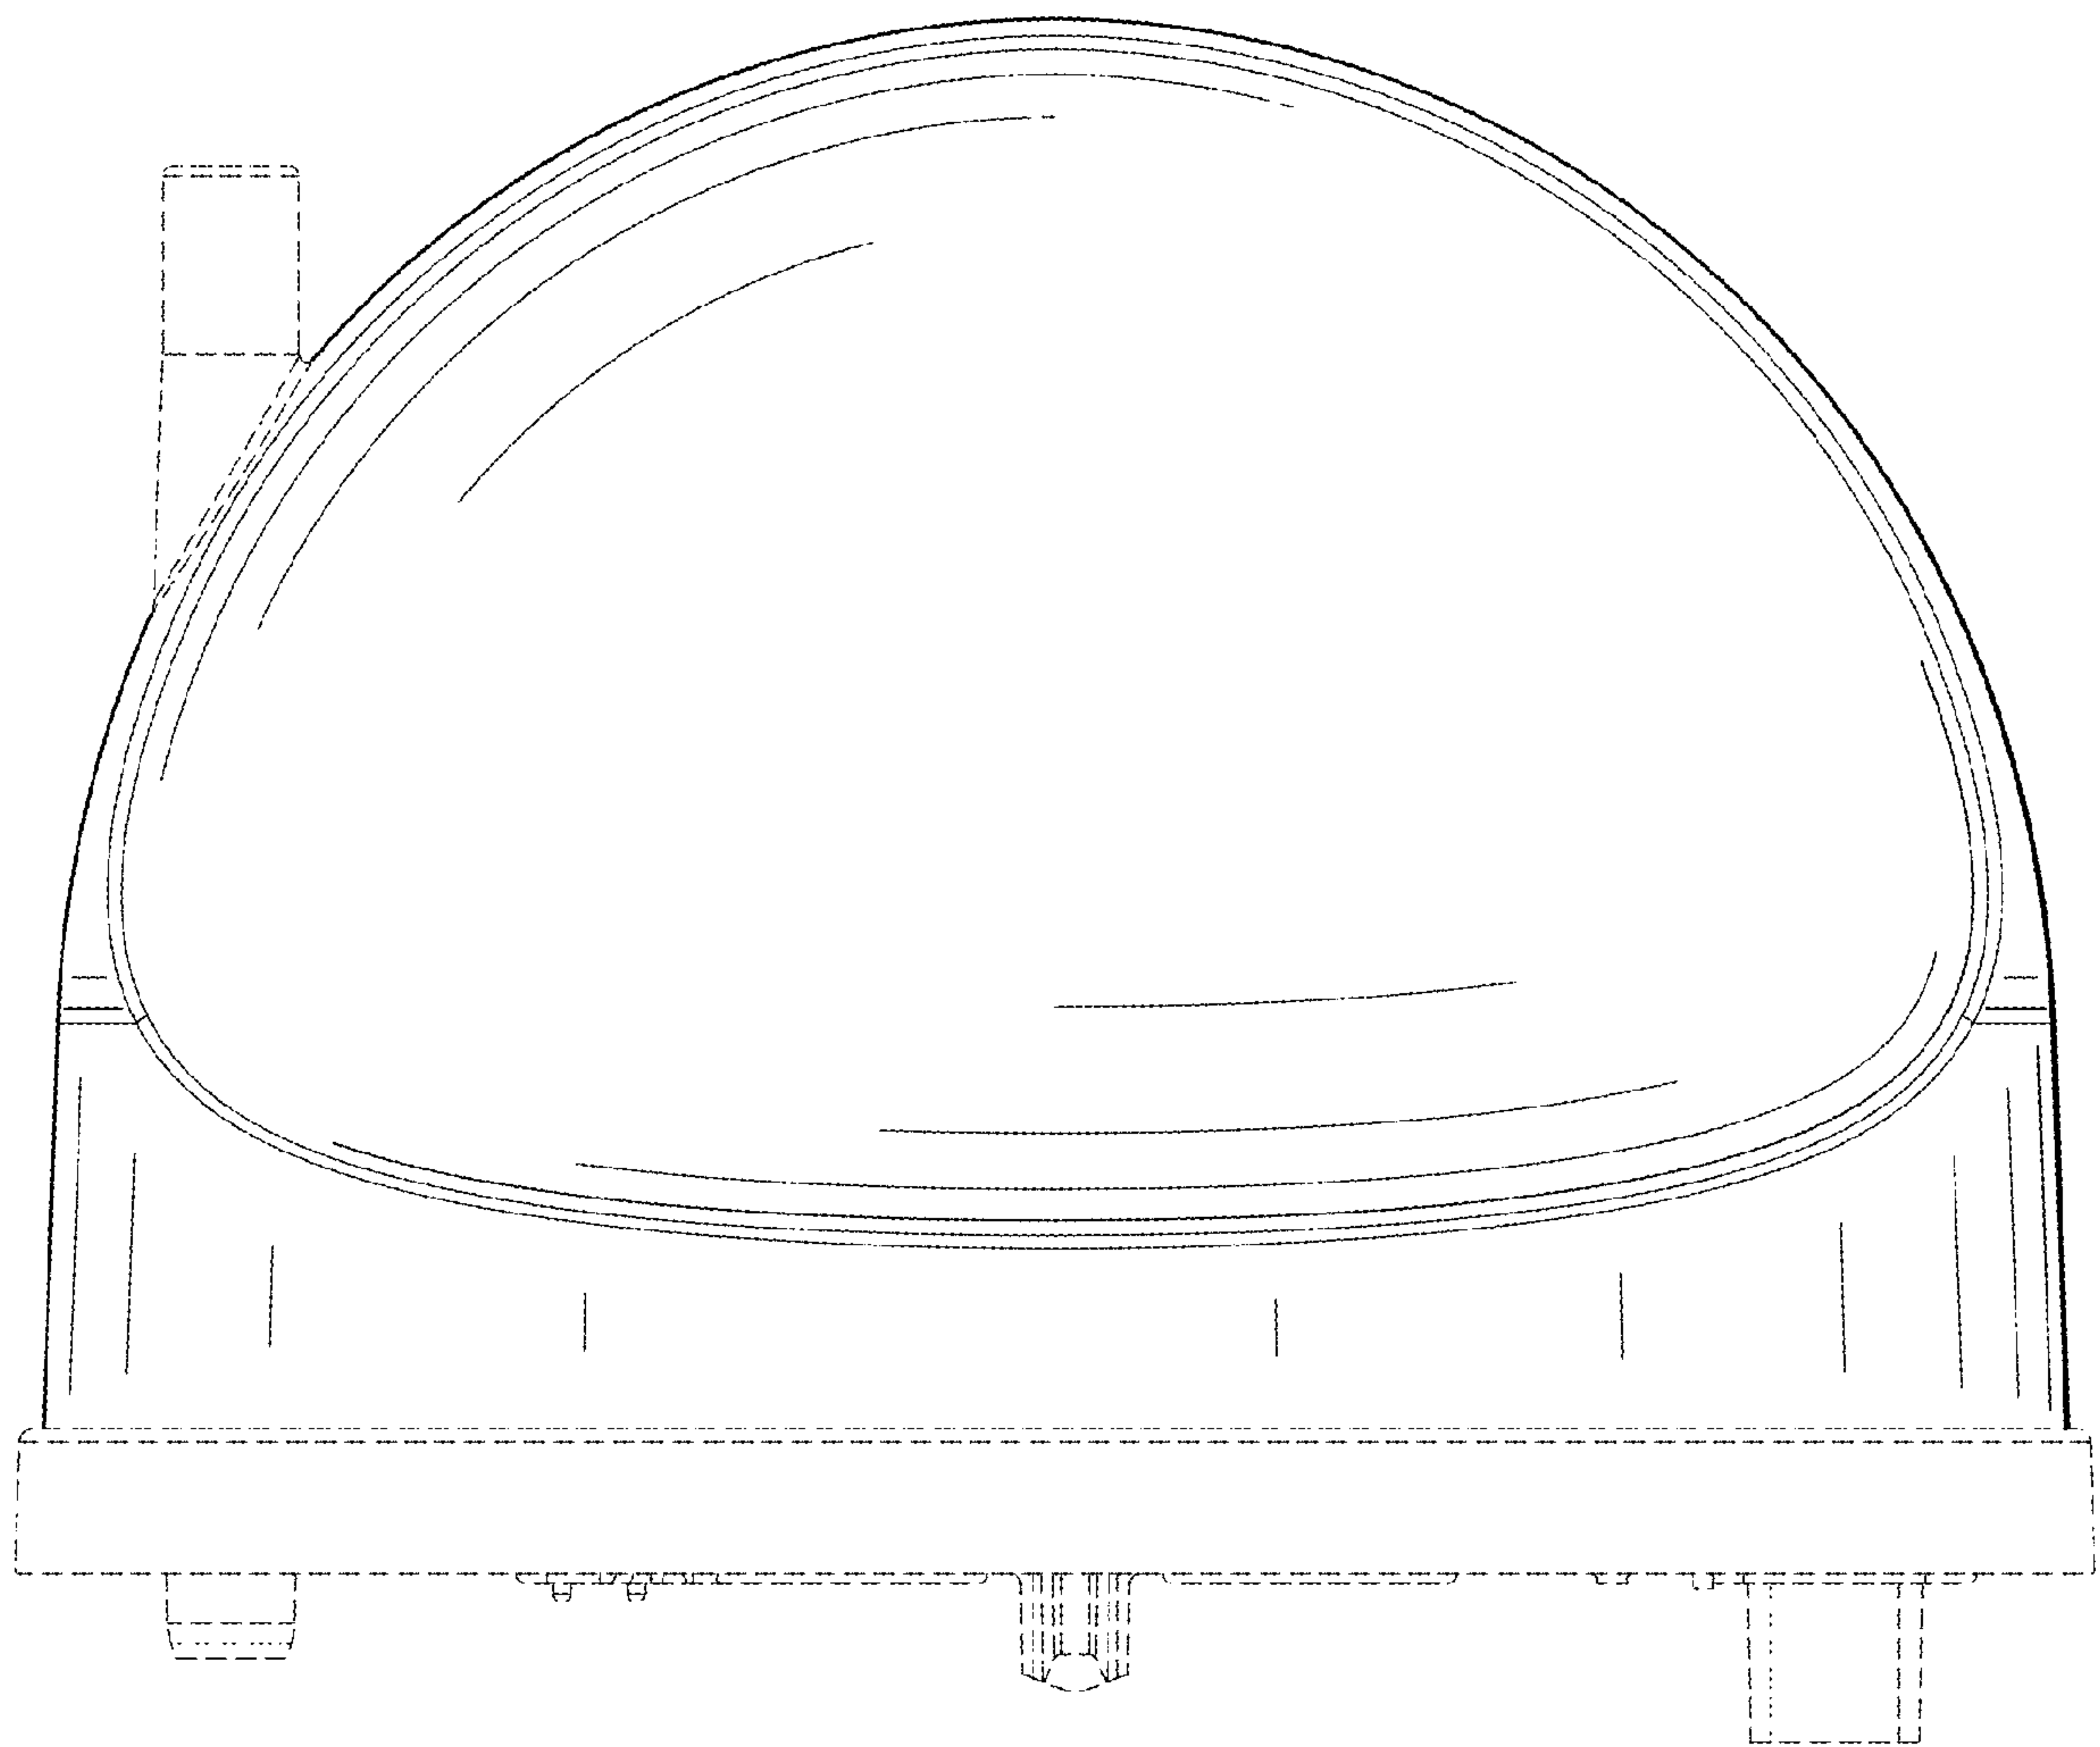


Fig. 3

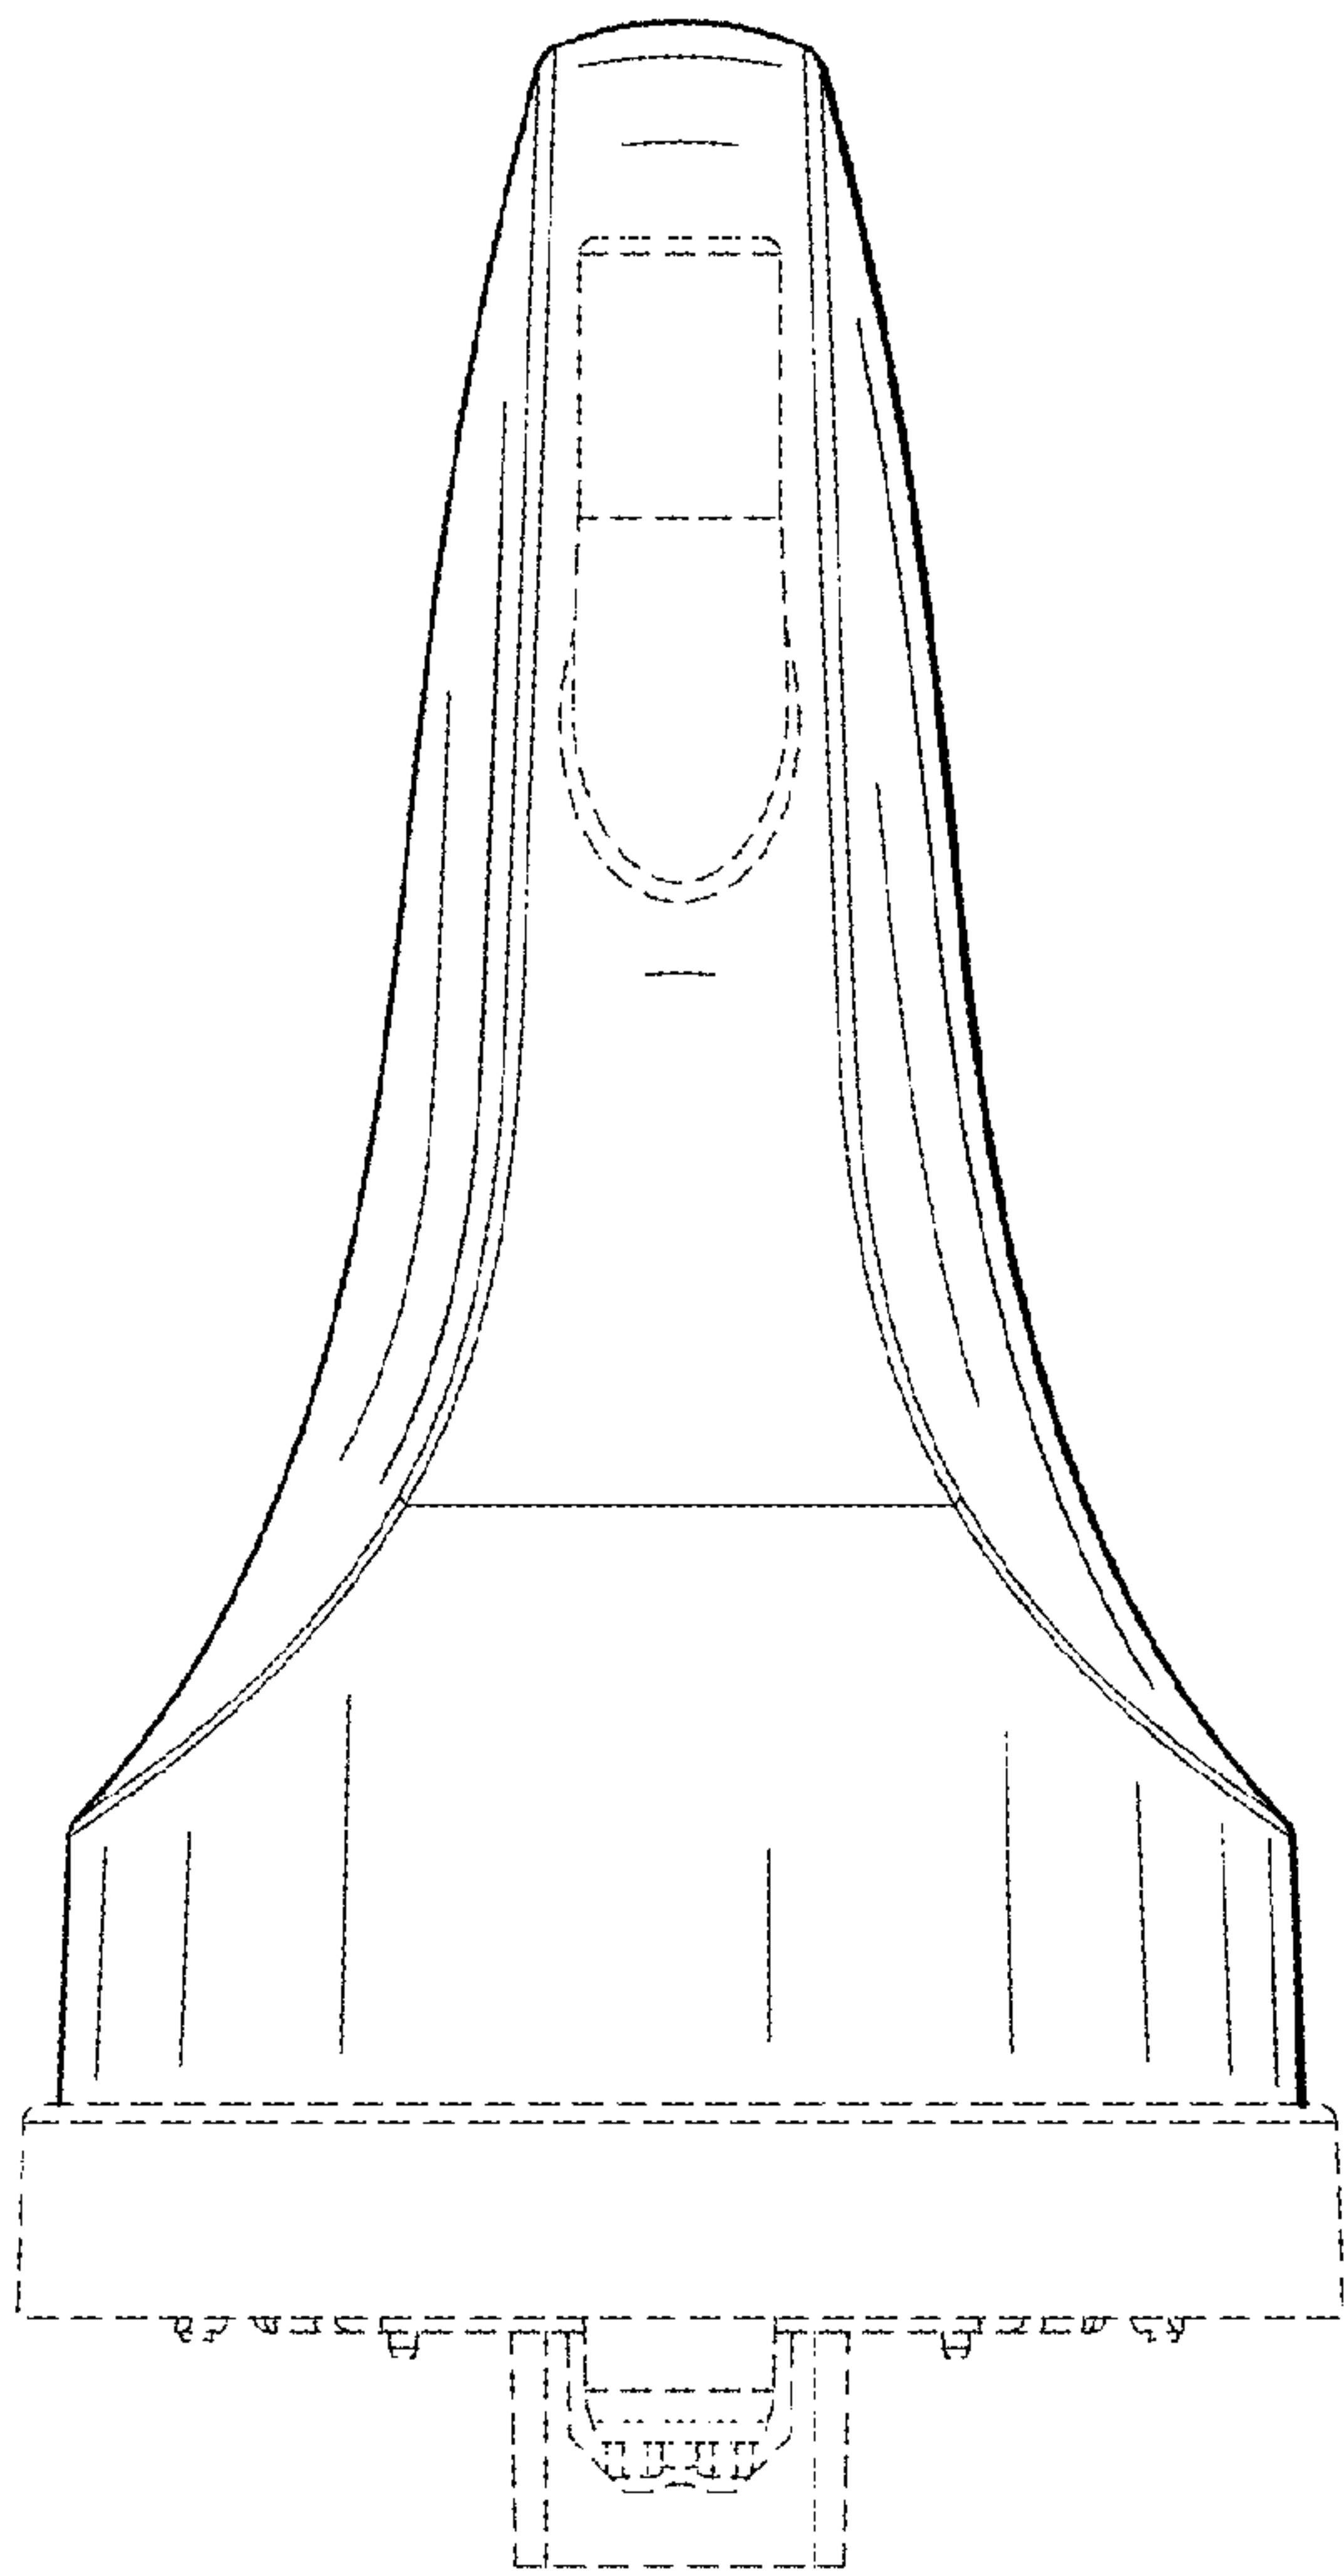


Fig. 4

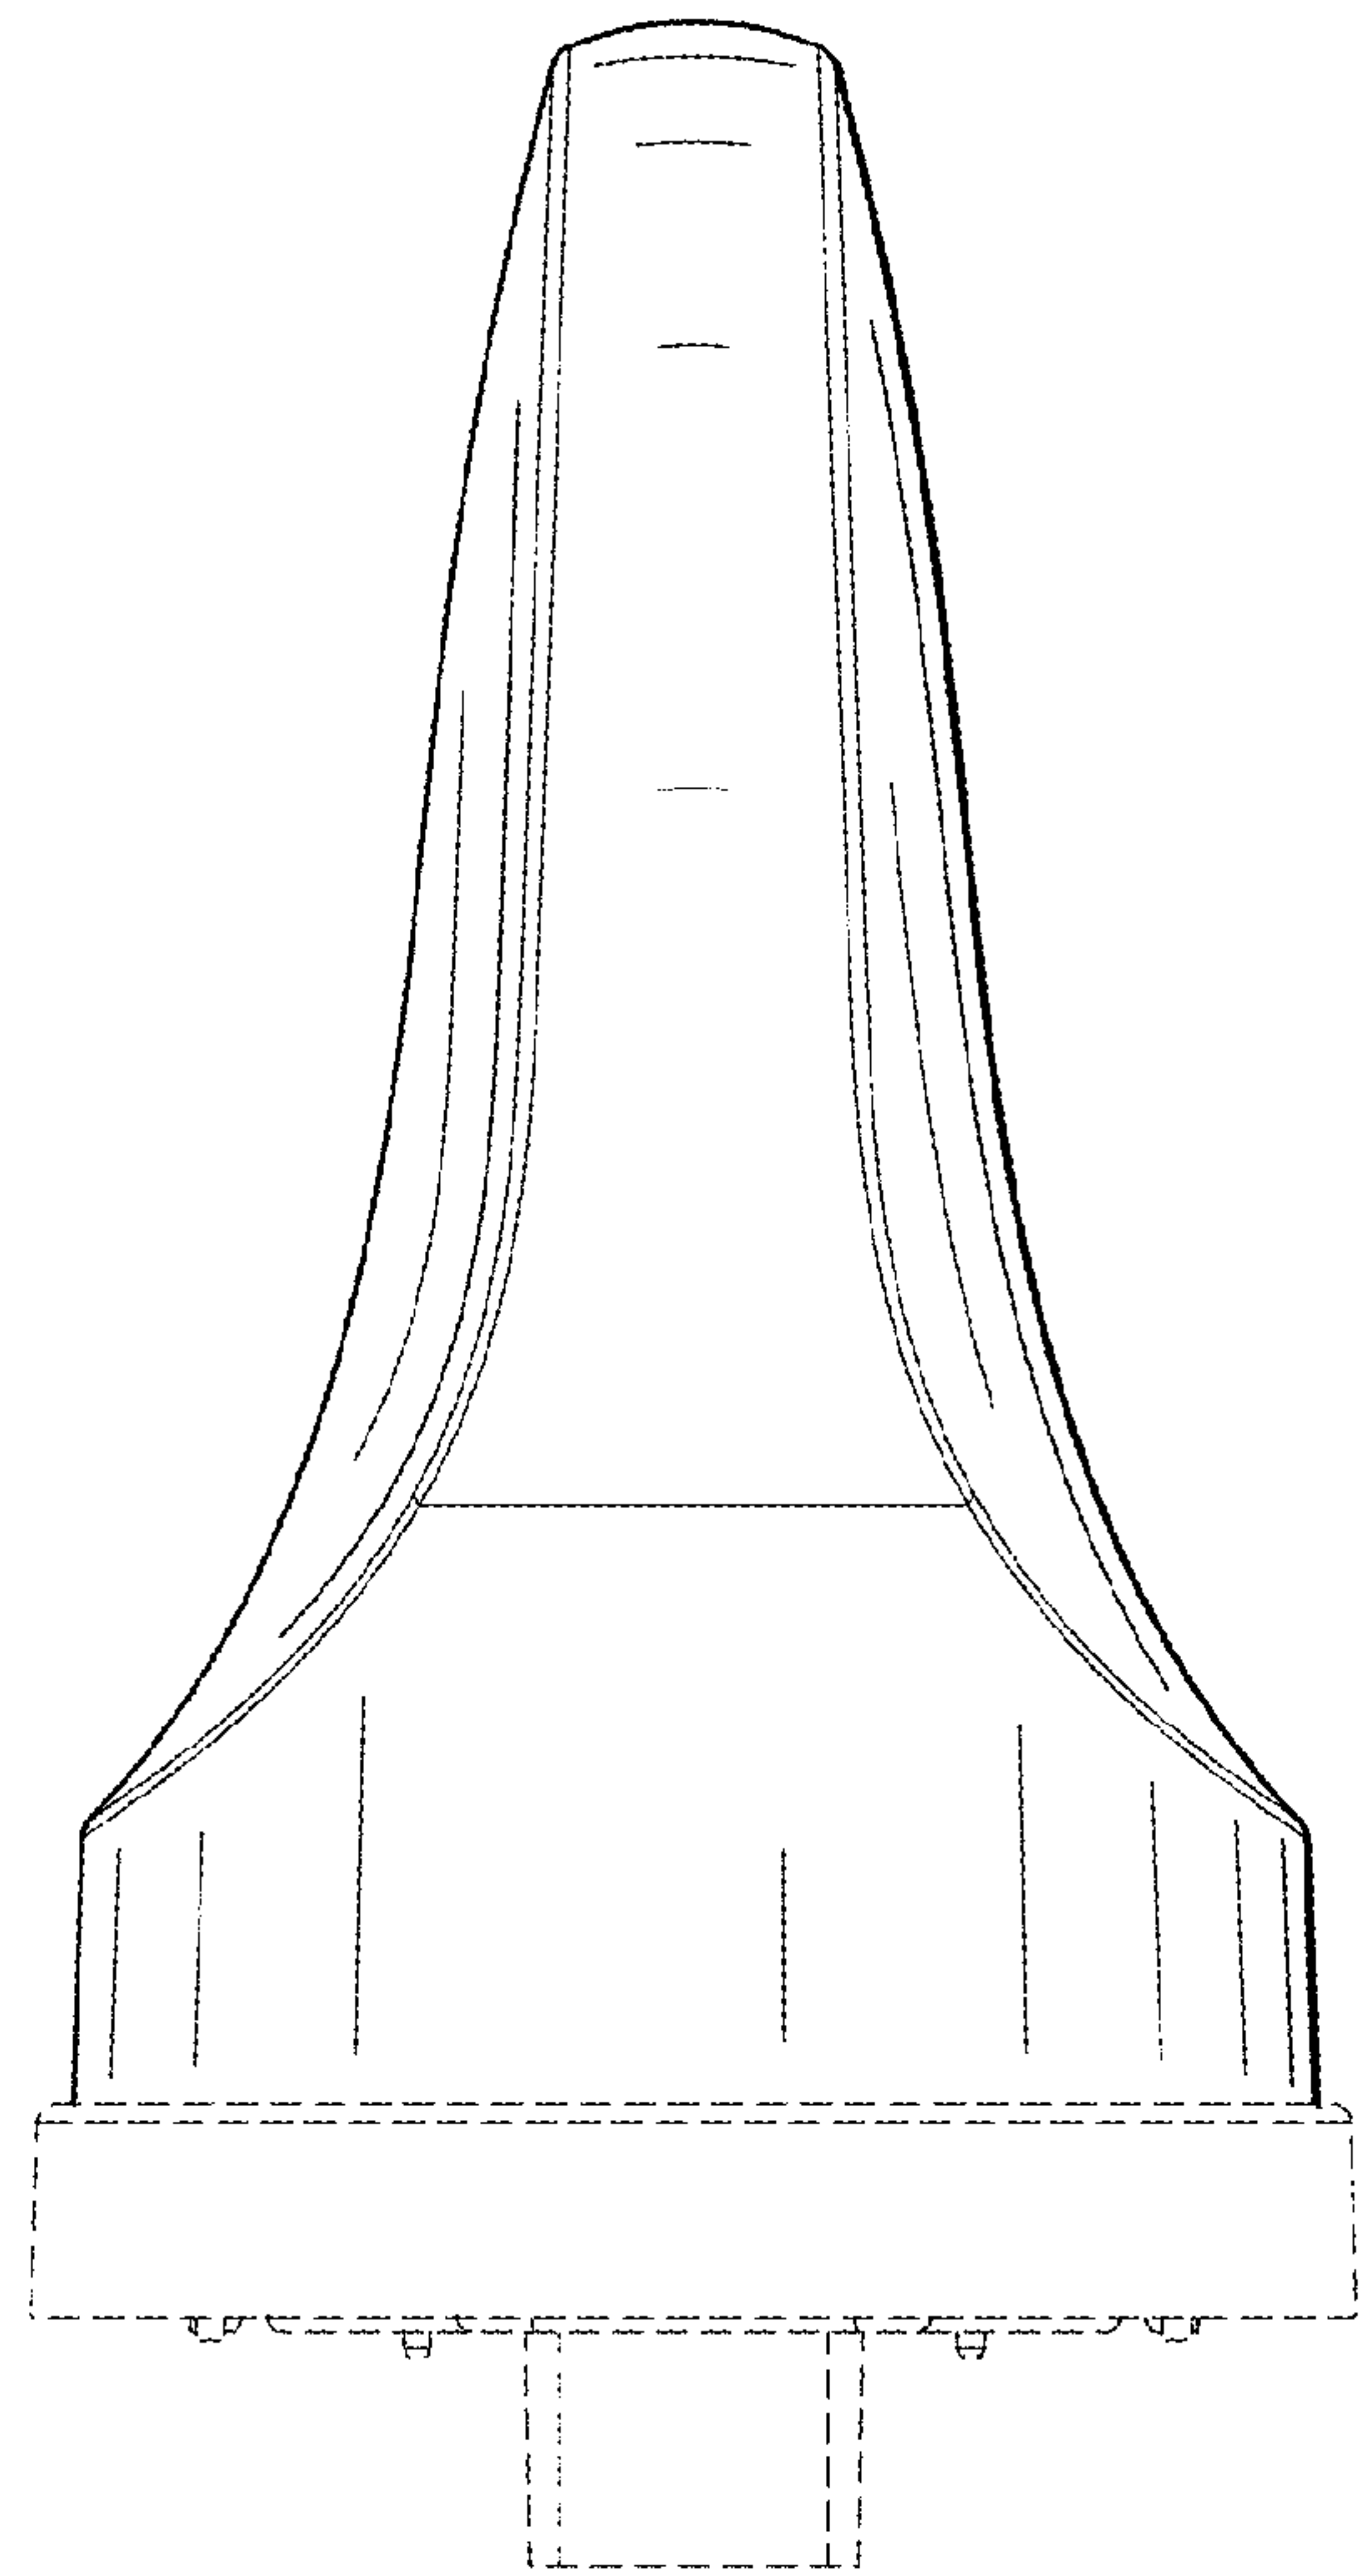


Fig. 5

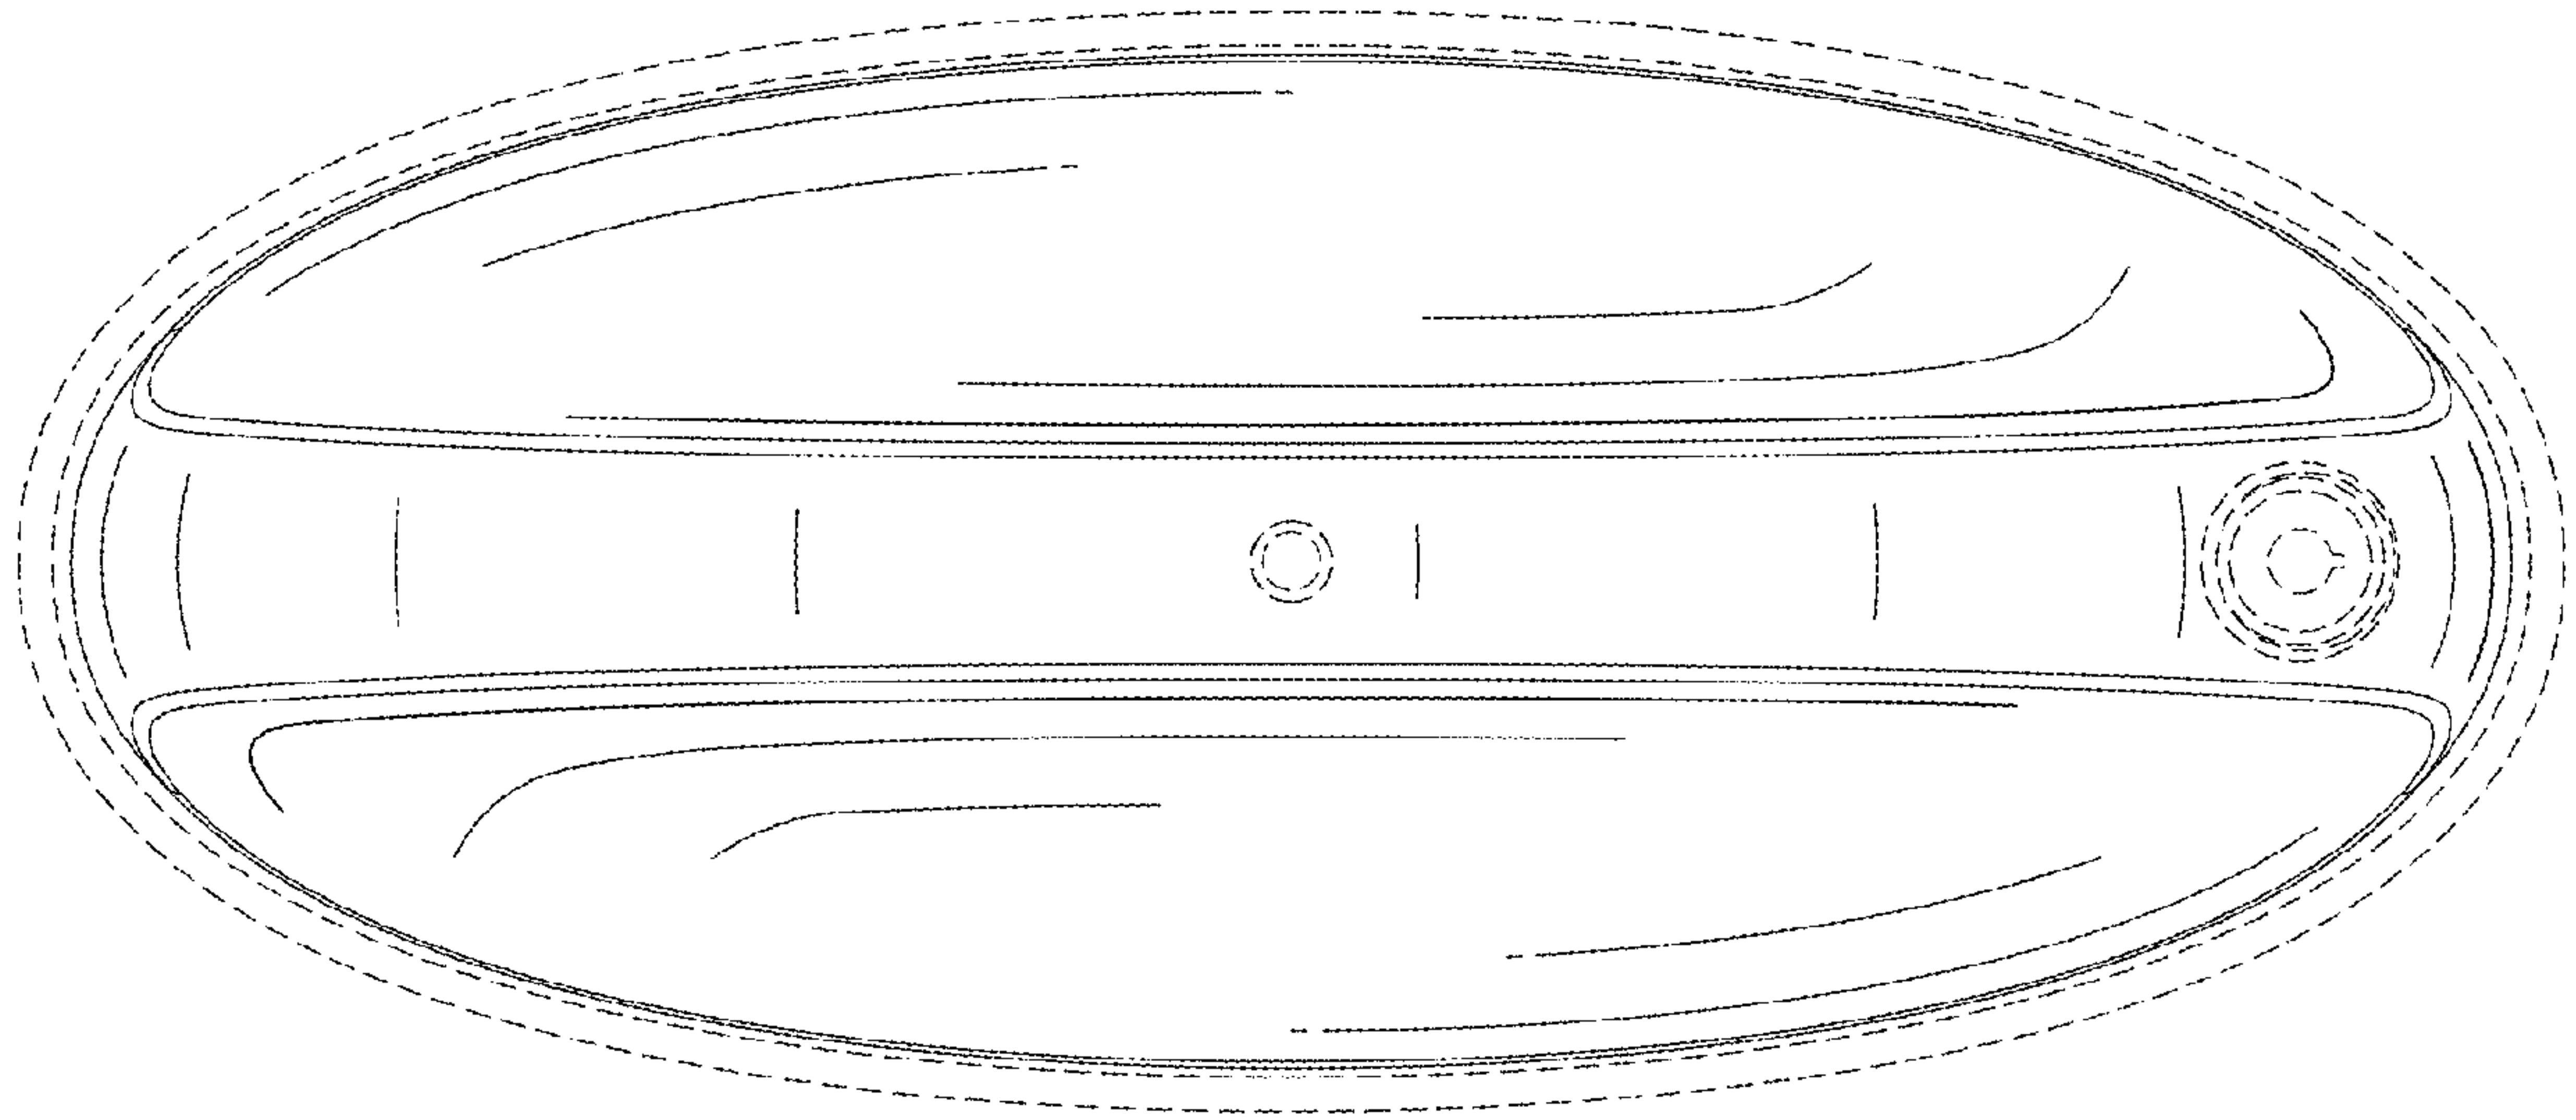


Fig. 6

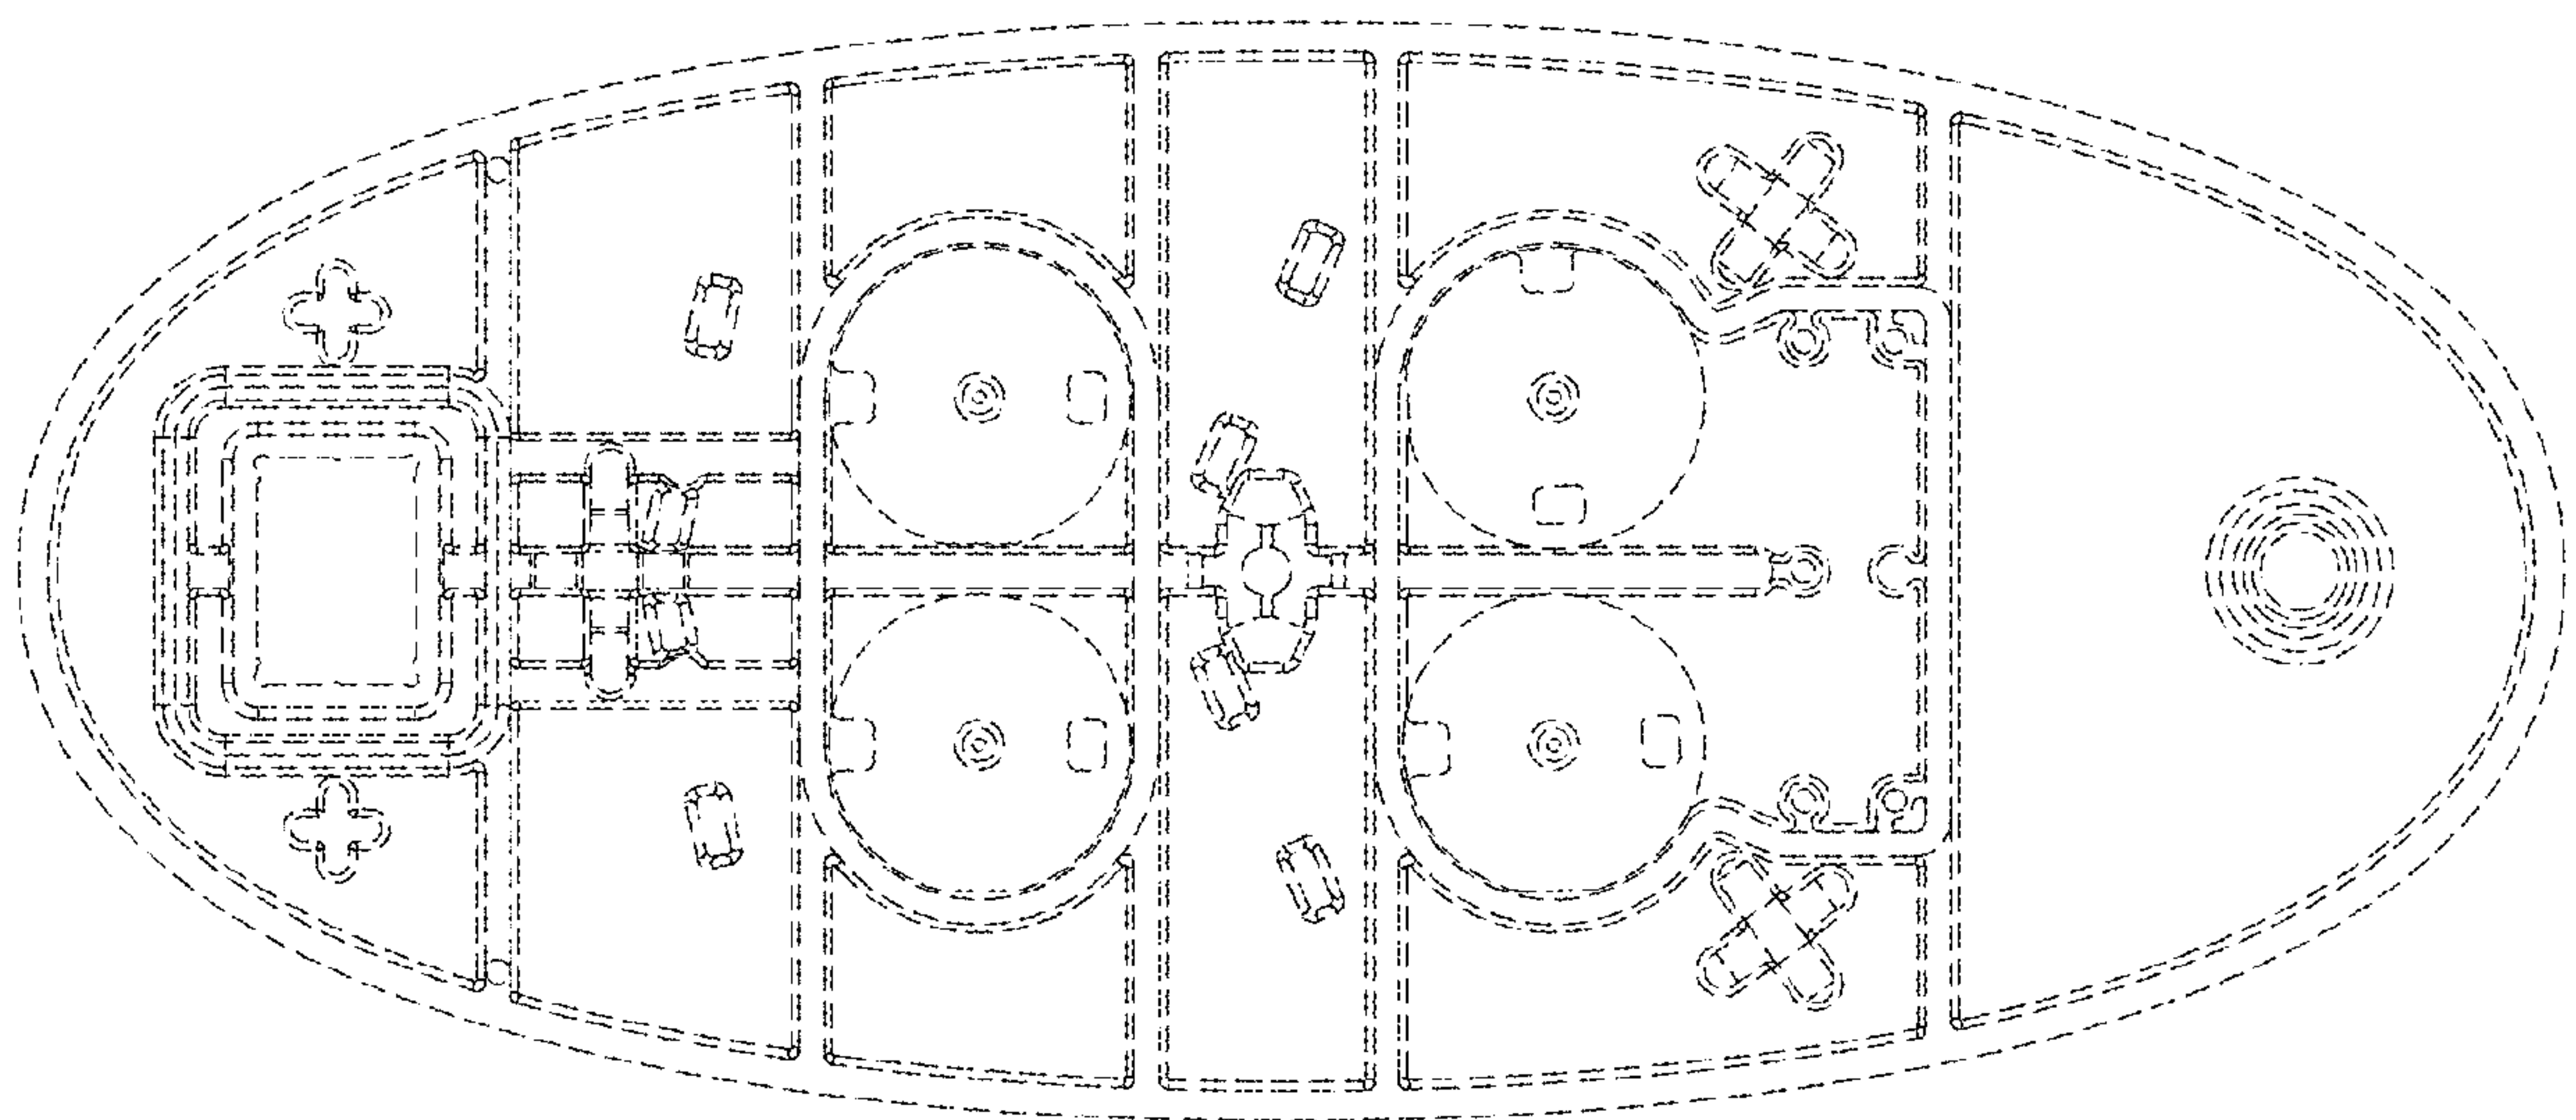


Fig. 7

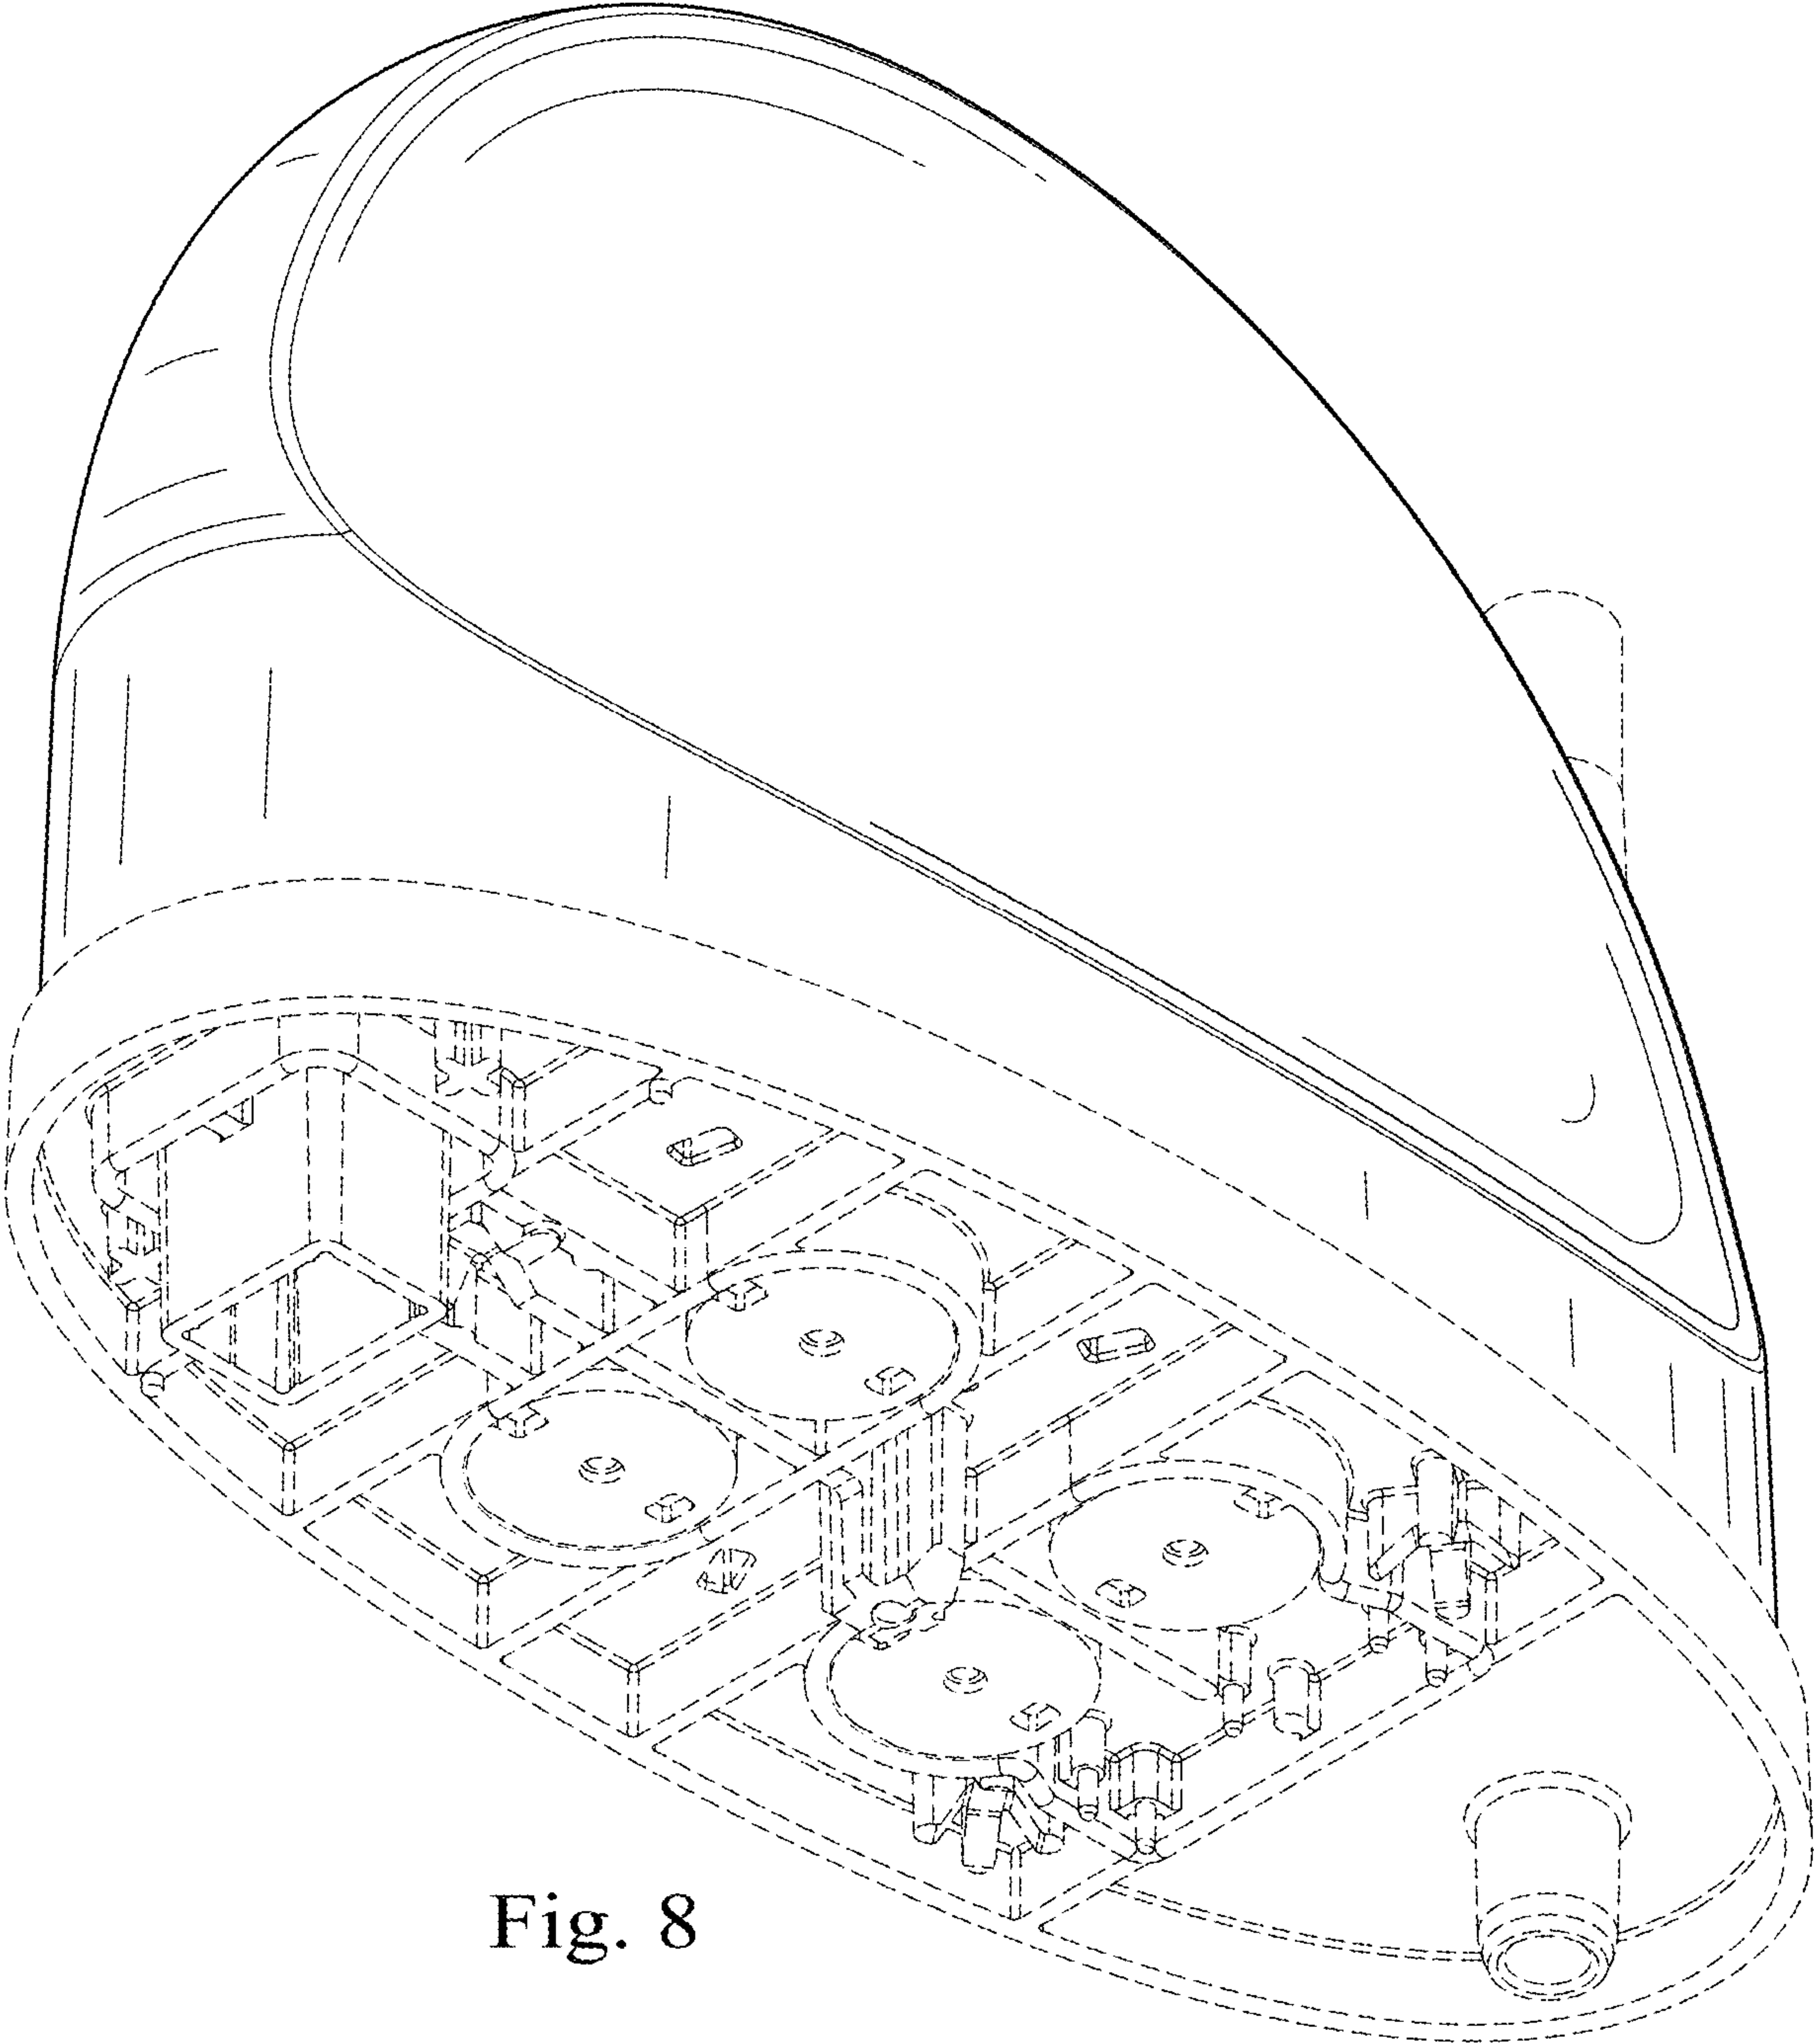


Fig. 8

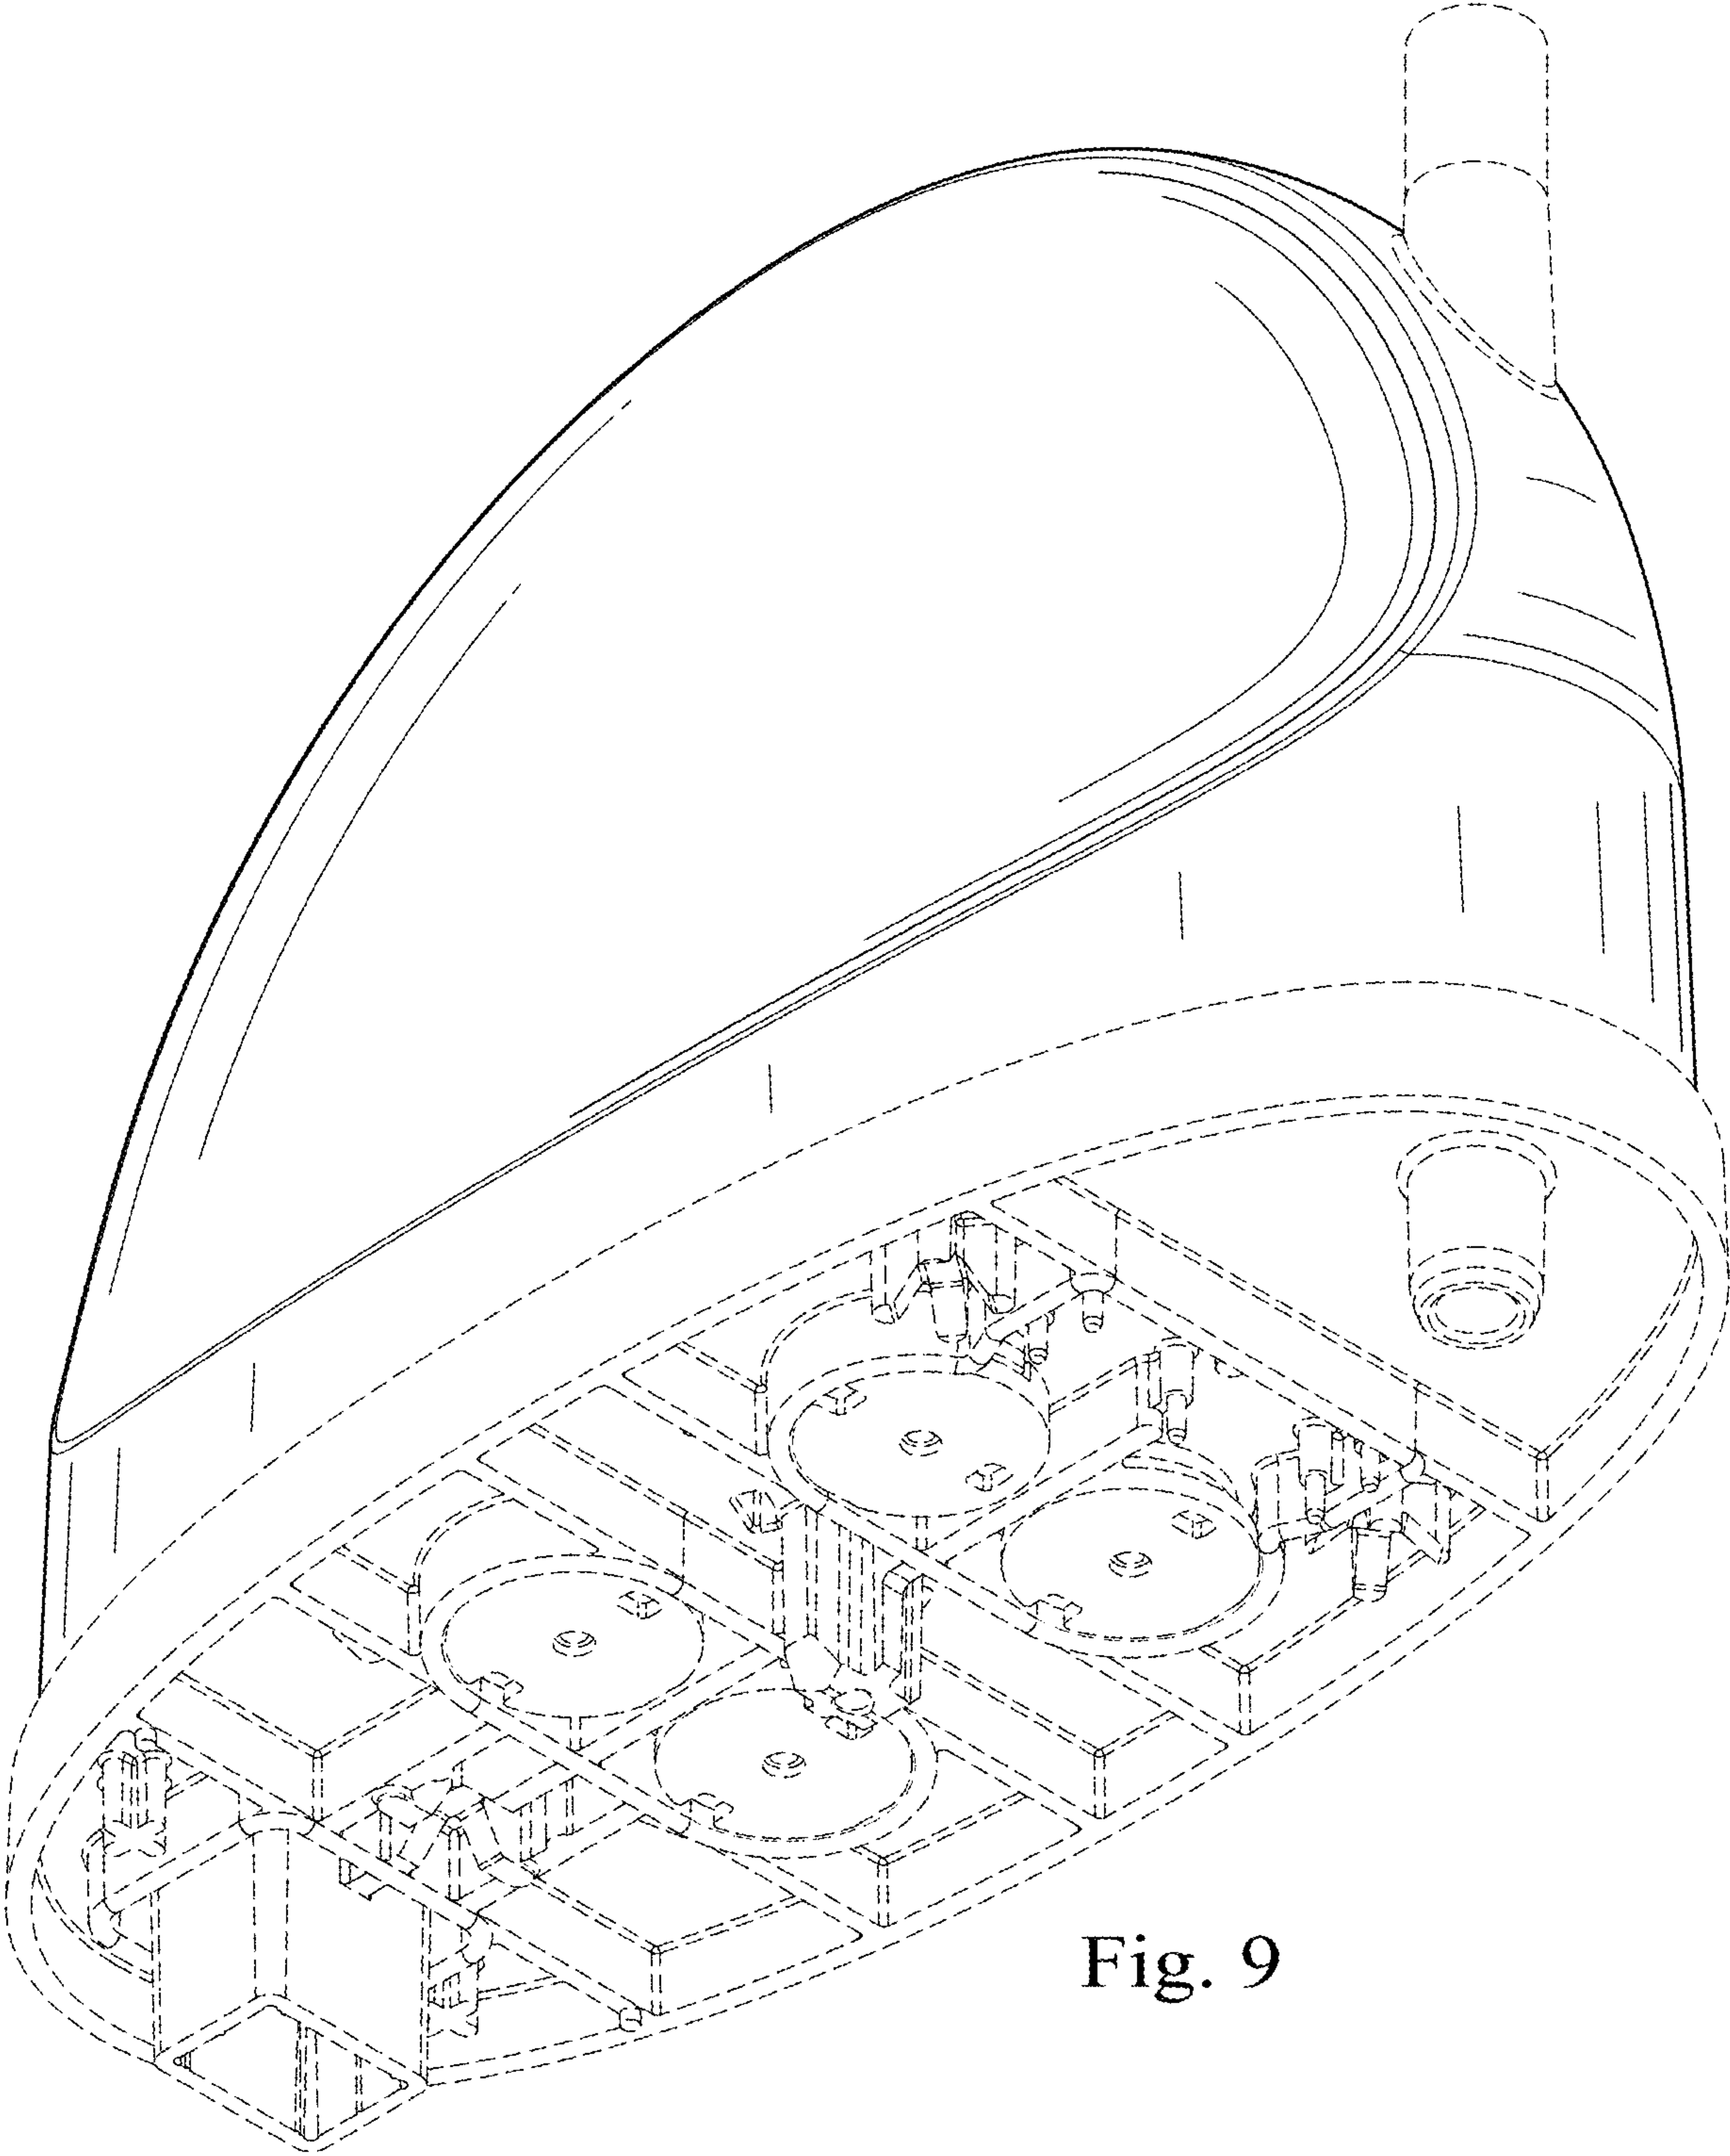


Fig. 9

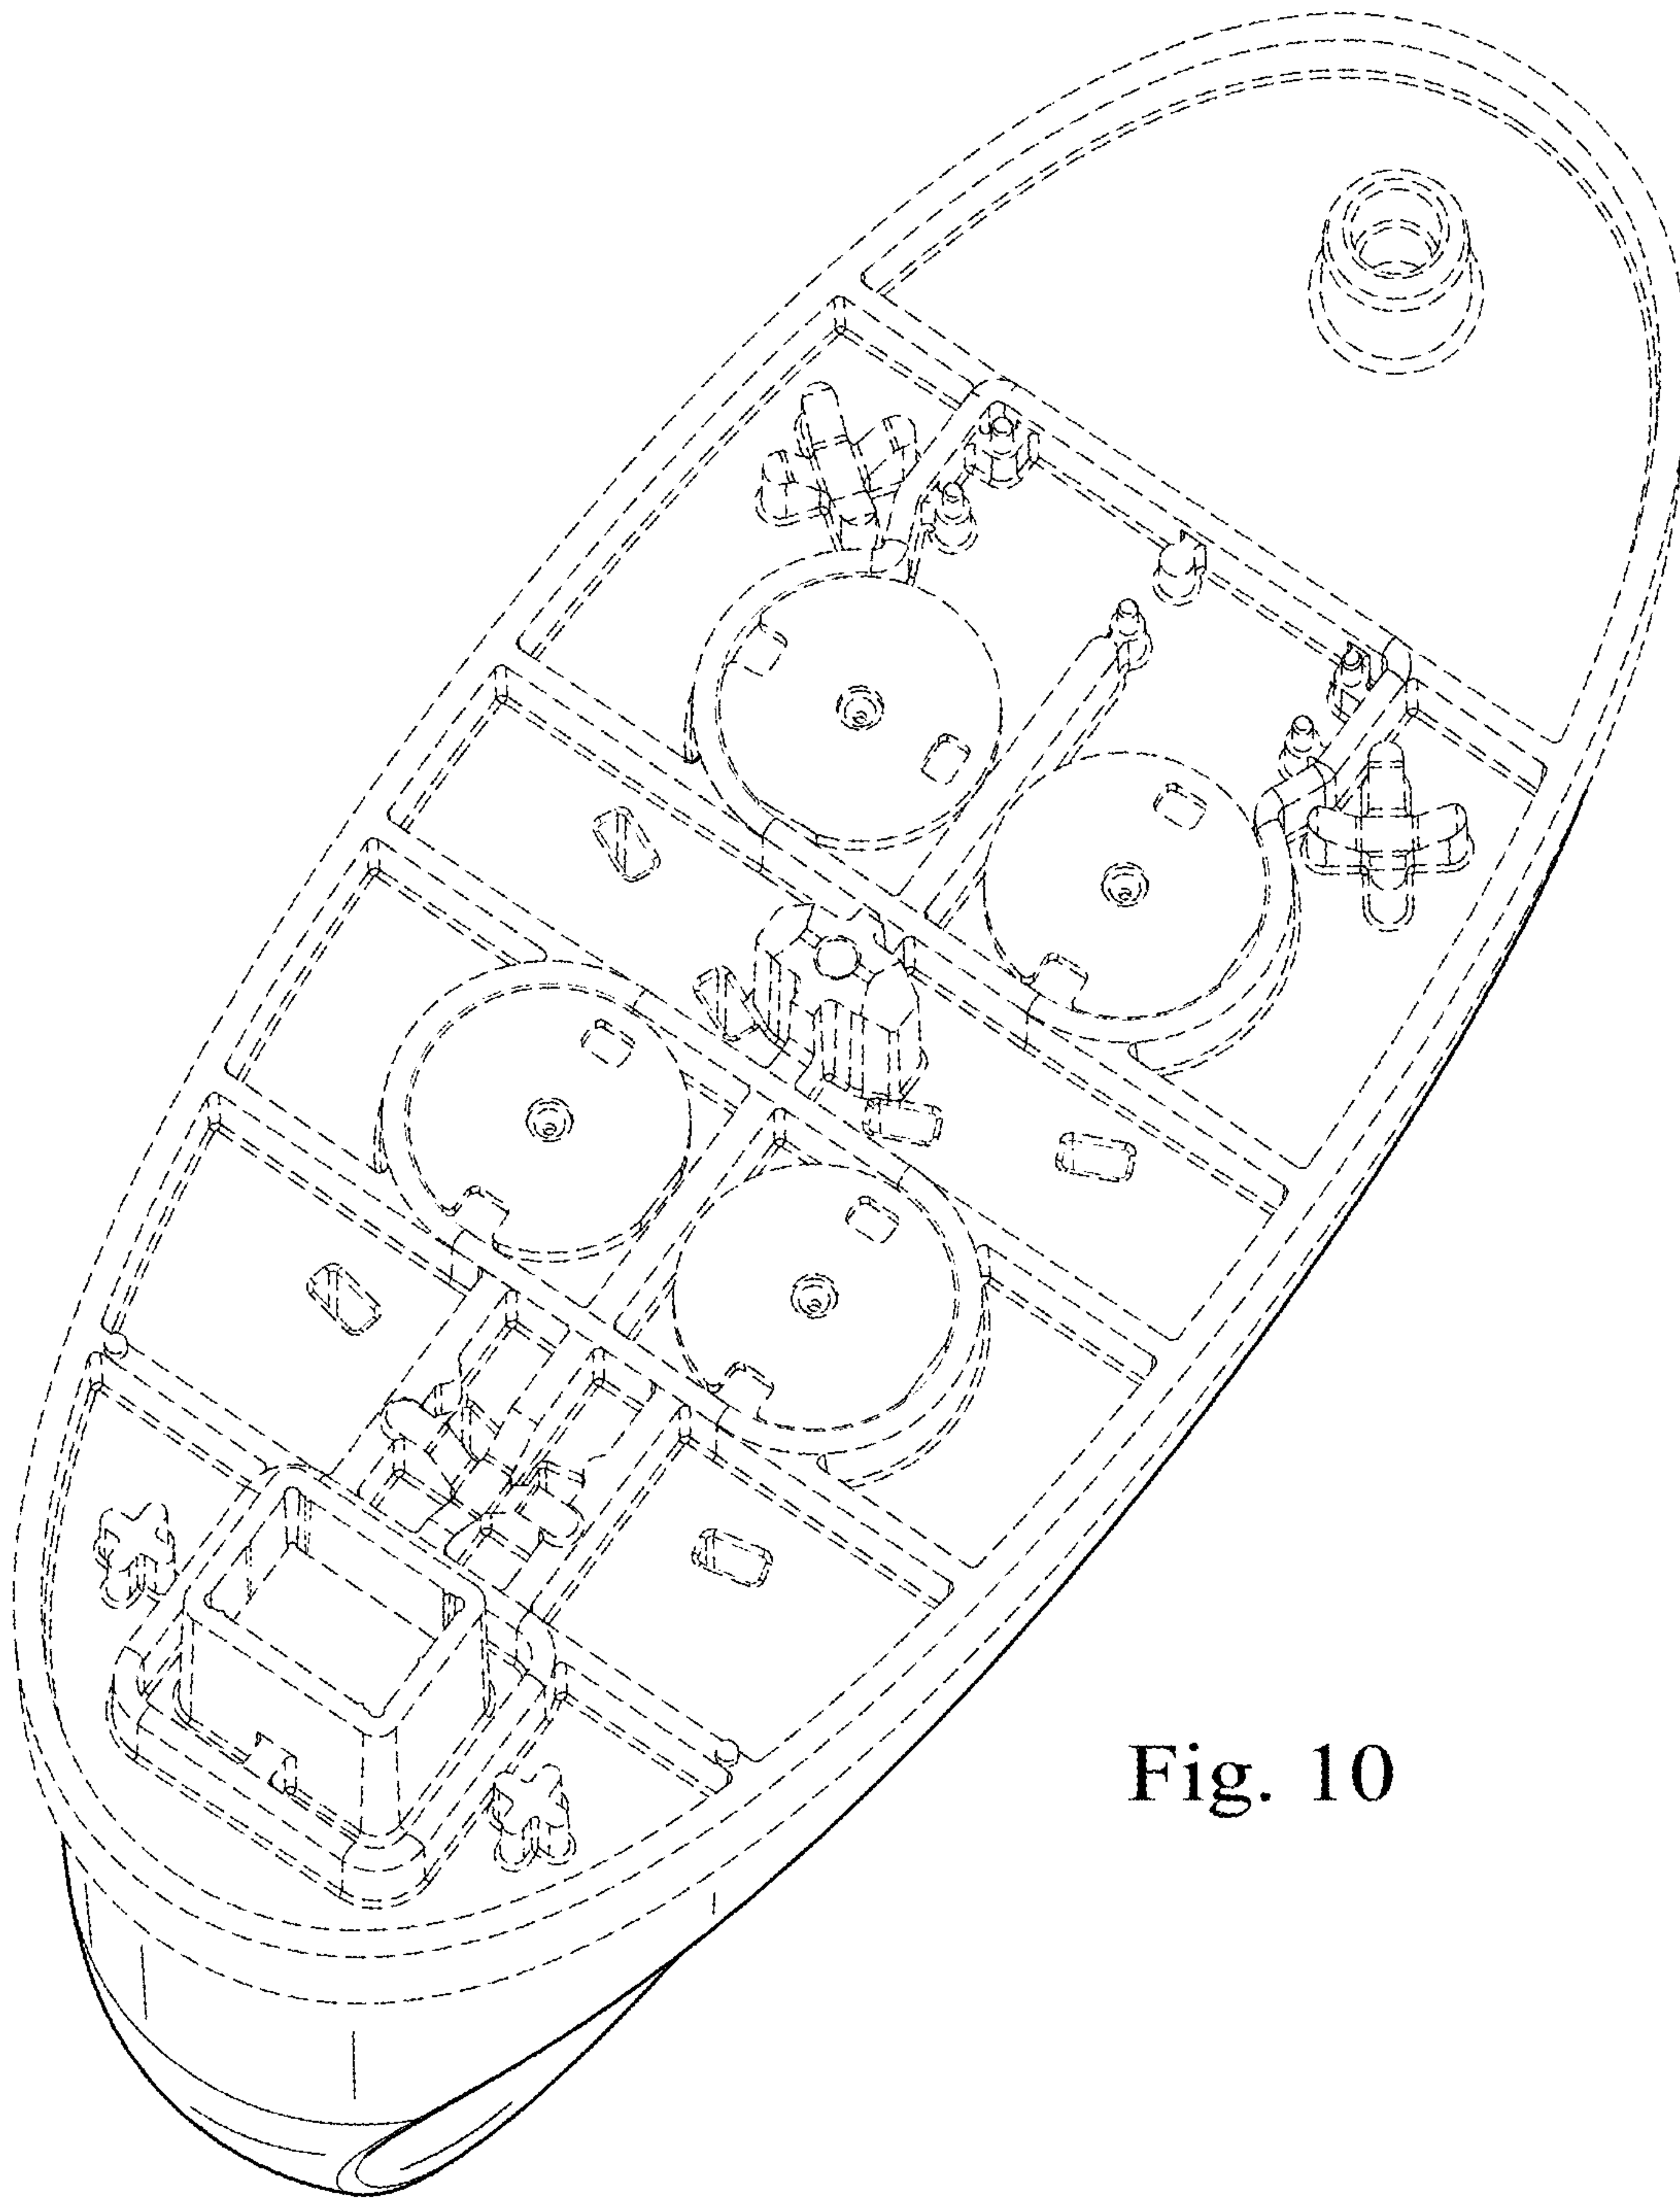


Fig. 10

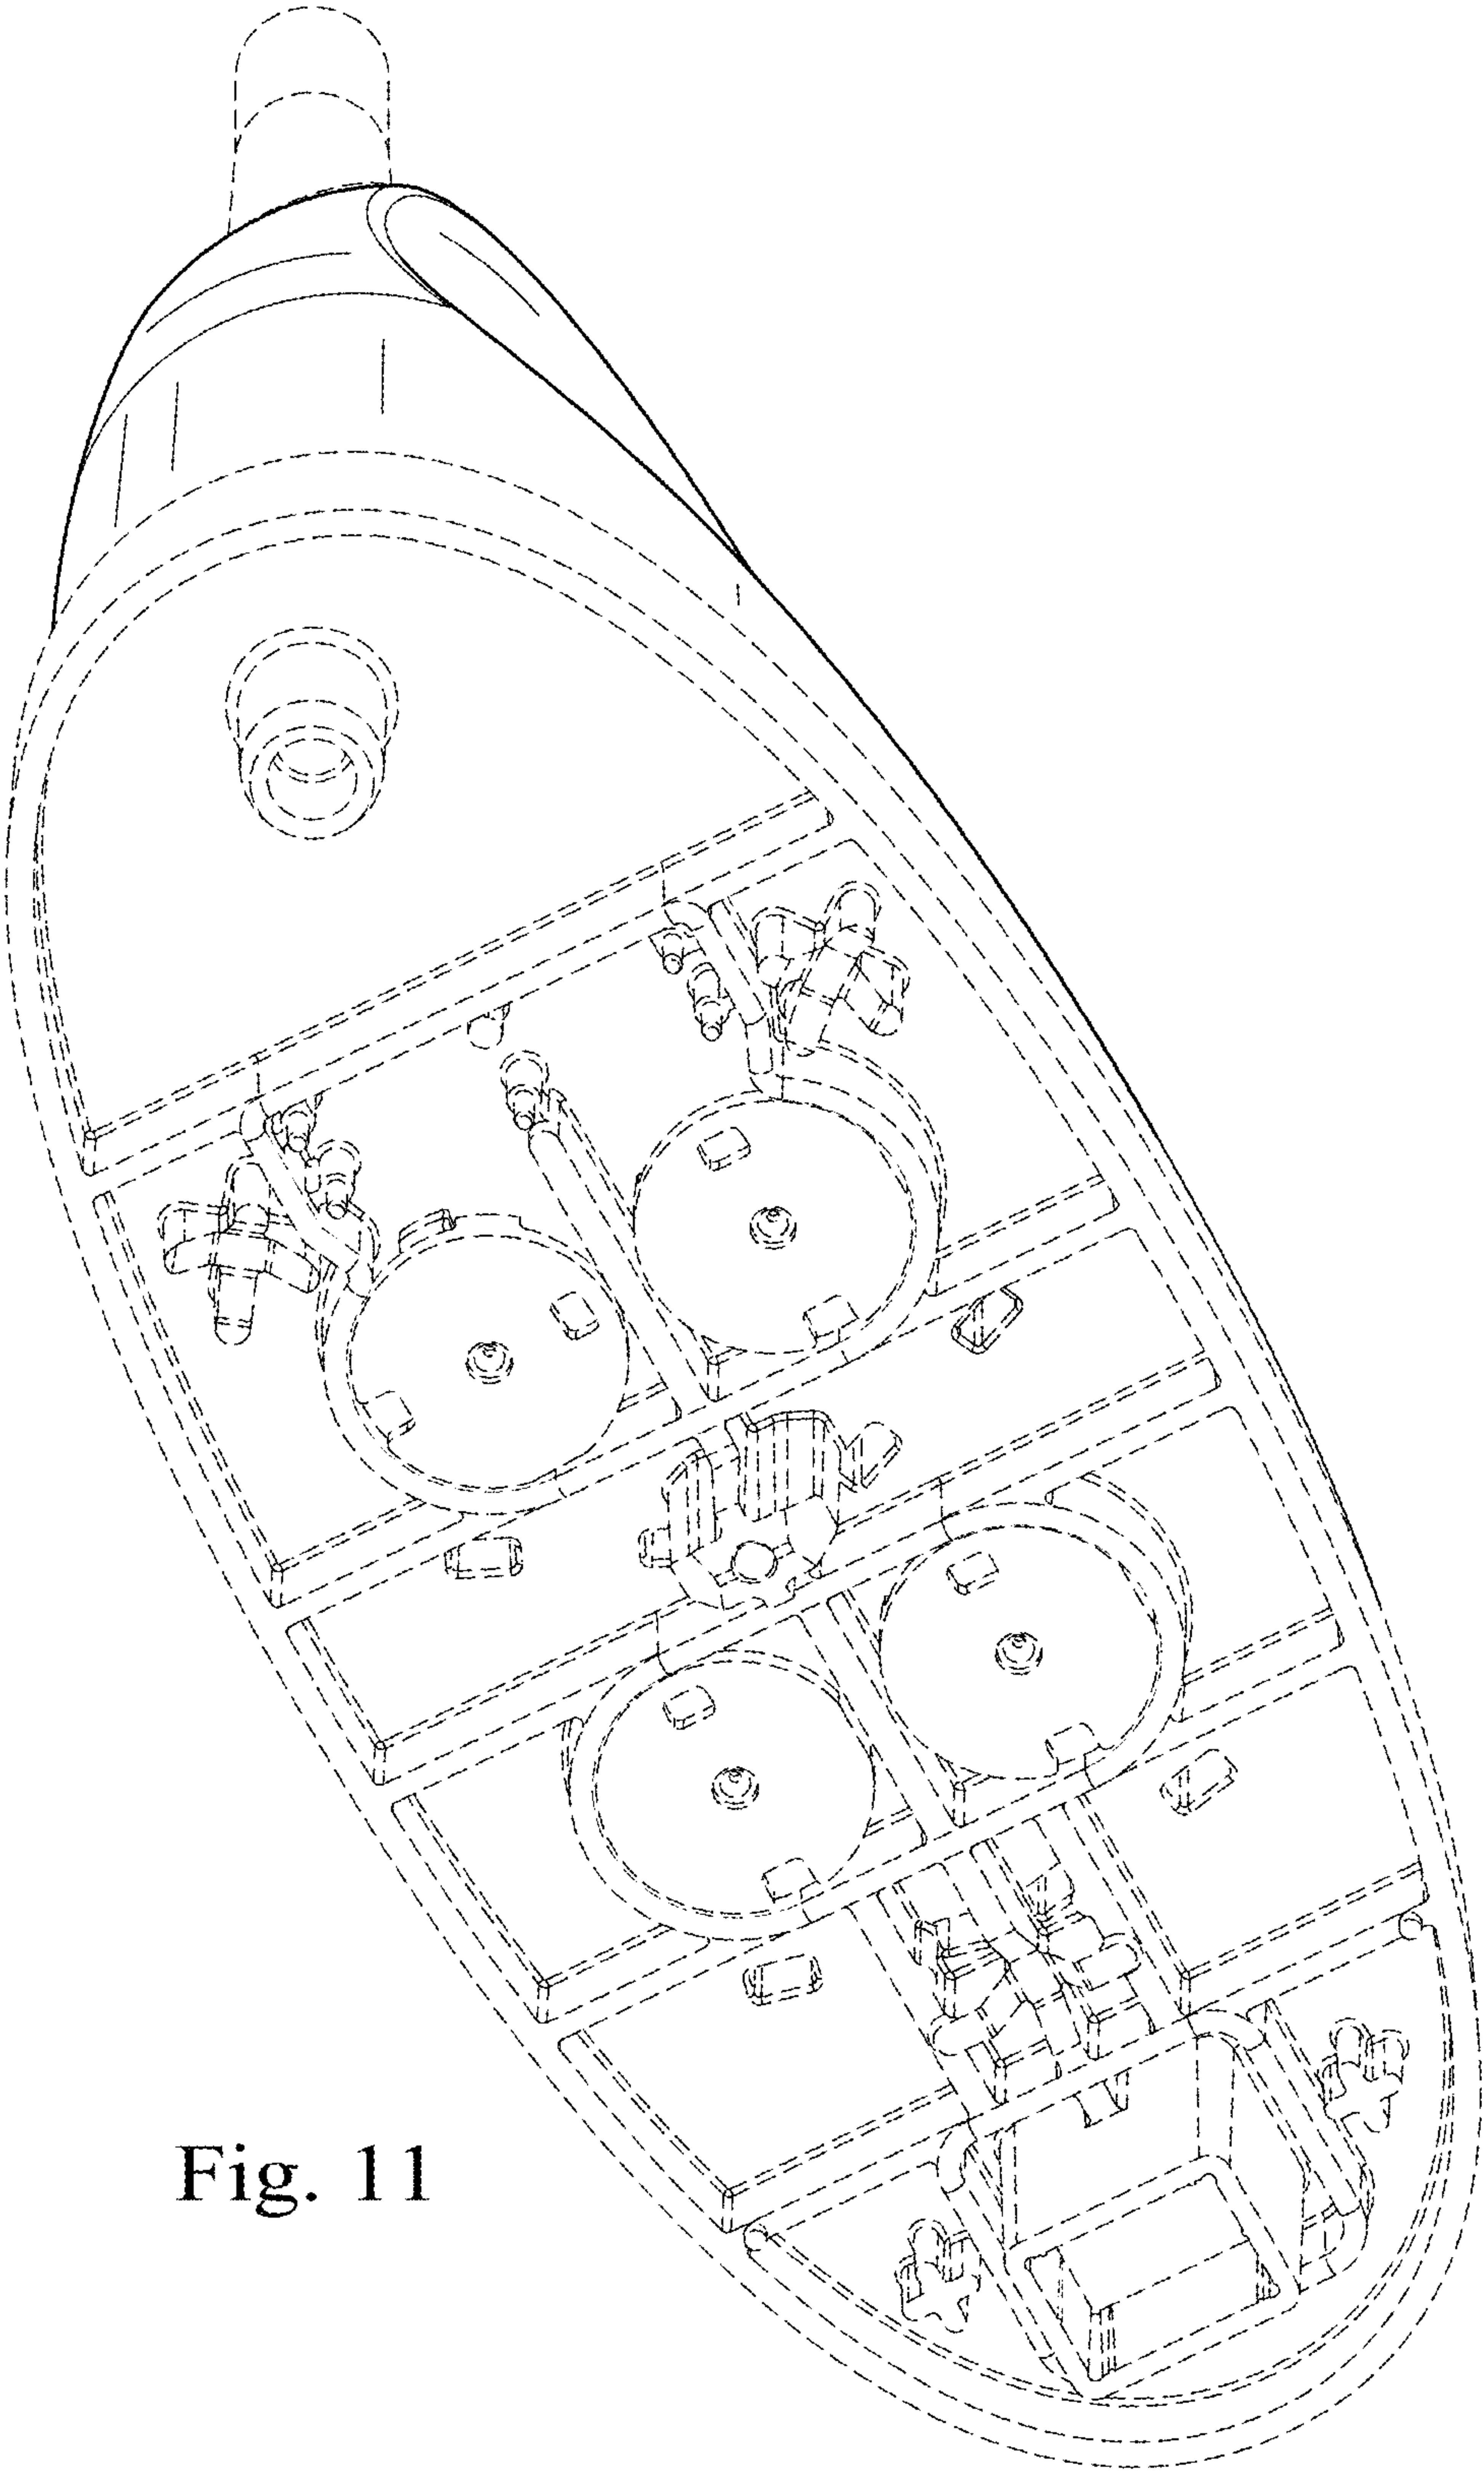


Fig. 11