



US00D878602S

(12) **United States Design Patent**
Chang et al.

(10) **Patent No.:** **US D878,602 S**
(45) **Date of Patent:** **** Mar. 17, 2020**

(54) **PERCUTANEOUS LEAD**

(71) Applicant: **GiMer Medical Co., Ltd.**, New Taipei (TW)

(72) Inventors: **Chi-Heng Chang**, New Taipei (TW);
Mei-Ching Wang, New Taipei (TW)

(73) Assignee: **GIMER MEDICAL CO., LTD.**, New Taipei (TW)

(**) Term: **15 Years**

(21) Appl. No.: **29/655,424**

(22) Filed: **Jul. 3, 2018**

(30) **Foreign Application Priority Data**

Jan. 4, 2018 (CN) 2018 3 0002530

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/187; D24/133**

(58) **Field of Classification Search**
USPC D24/130, 133–136, 140, 146–147, 187;
D23/219, 266
CPC A61N 1/0502
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 4,512,351 A * 4/1985 Pohndorf A61N 1/0551
607/117
- D323,887 S * 2/1992 Picha D24/107
- D478,165 S * 8/2003 Hechel D24/108
- D534,650 S * 1/2007 Inman D24/133
- D593,202 S * 5/2009 Petersen D24/133
- D601,251 S * 9/2009 Horton D24/133
- D628,708 S * 12/2010 Anderson D24/216
- D669,983 S * 10/2012 Dapri D24/133
- D727,527 S * 4/2015 Tao D24/222
- D745,687 S * 12/2015 Kitayama D24/187
- D752,213 S * 3/2016 Paul D24/127
- D752,215 S * 3/2016 Blennow D24/130

(Continued)

OTHER PUBLICATIONS

Infinion™ CX 16-contact Lead. Online, published date unknown. Retrieved on Sep. 23, 2019 from URL: <https://www.bostonscientific.com/en-EU/products/spinal-cord-stimulator-systems/Infinion-CX.html>.*

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Muncy, Geissler, Olds & Lowe, PC

(57) **CLAIM**


The ornamental design for a percutaneous lead, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a percutaneous lead according to our new design;
FIG. 2 is a side elevation thereof;
FIG. 3 is a top enlarged view thereof;
FIG. 4 is an enlarged view of area 4 circumscribed with dash-dot line within FIG. 1;
FIG. 5 is an enlarged view of area 5 circumscribed with dash-dot line within FIG. 1;
FIG. 6 is an enlarged view of area 6 circumscribed with dash-dot line within FIG. 2;
FIG. 7 is an enlarged view of area 7 circumscribed with dash-dot line within FIG. 2; and,
FIG. 8 is a perspective view thereof, shown in a position of use.

The dashed lines in form of a device shown in FIG. 8 depict environmental subject matter and form no part of the claimed design. All the other dashed lines in the drawings depict portions of the percutaneous lead that form no part of the claimed design. The short dash-long dash-short dash broken lines depict boundaries of the enlarged views that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

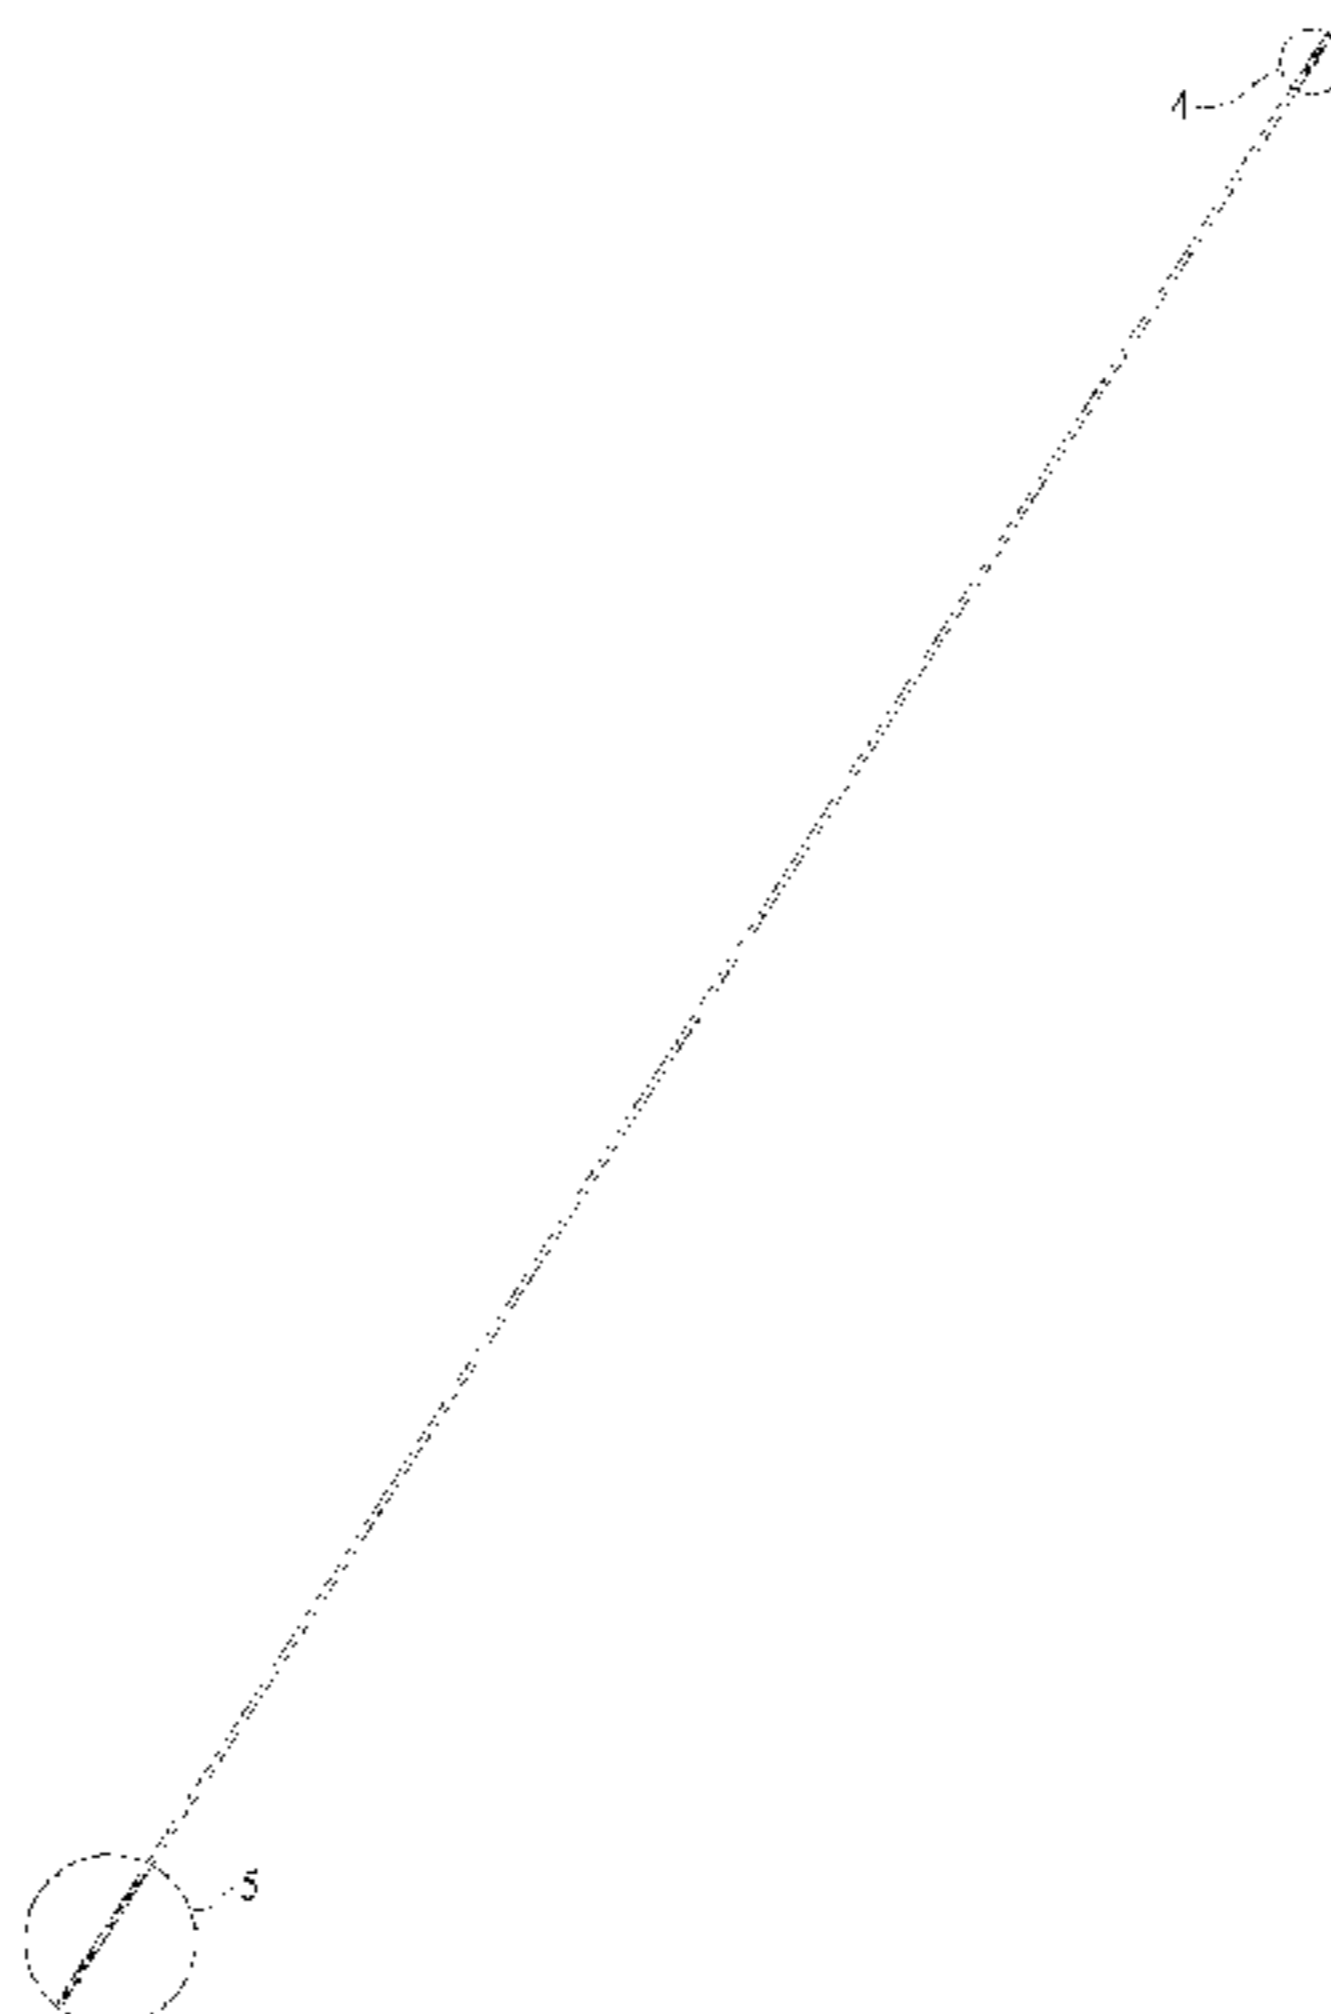

(56)

References Cited

U.S. PATENT DOCUMENTS

D753,289 S * 4/2016 Shimon D24/112
9,456,914 B2 * 10/2016 Longo A61F 2/958
9,764,137 B2 * 9/2017 Lin A61N 1/36071
D810,936 S * 2/2018 Bresco Torras D24/138
D854,680 S * 7/2019 Flores D24/112
2007/0239119 A1 * 10/2007 Lipov A61B 17/3417
604/272
2011/0009933 A1 * 1/2011 Barker A61N 1/0551
607/116
2011/0282424 A1 * 11/2011 De La Rama A61N 1/0558
607/149
2015/0165187 A1 * 6/2015 Liu A61N 1/05
606/129

* cited by examiner

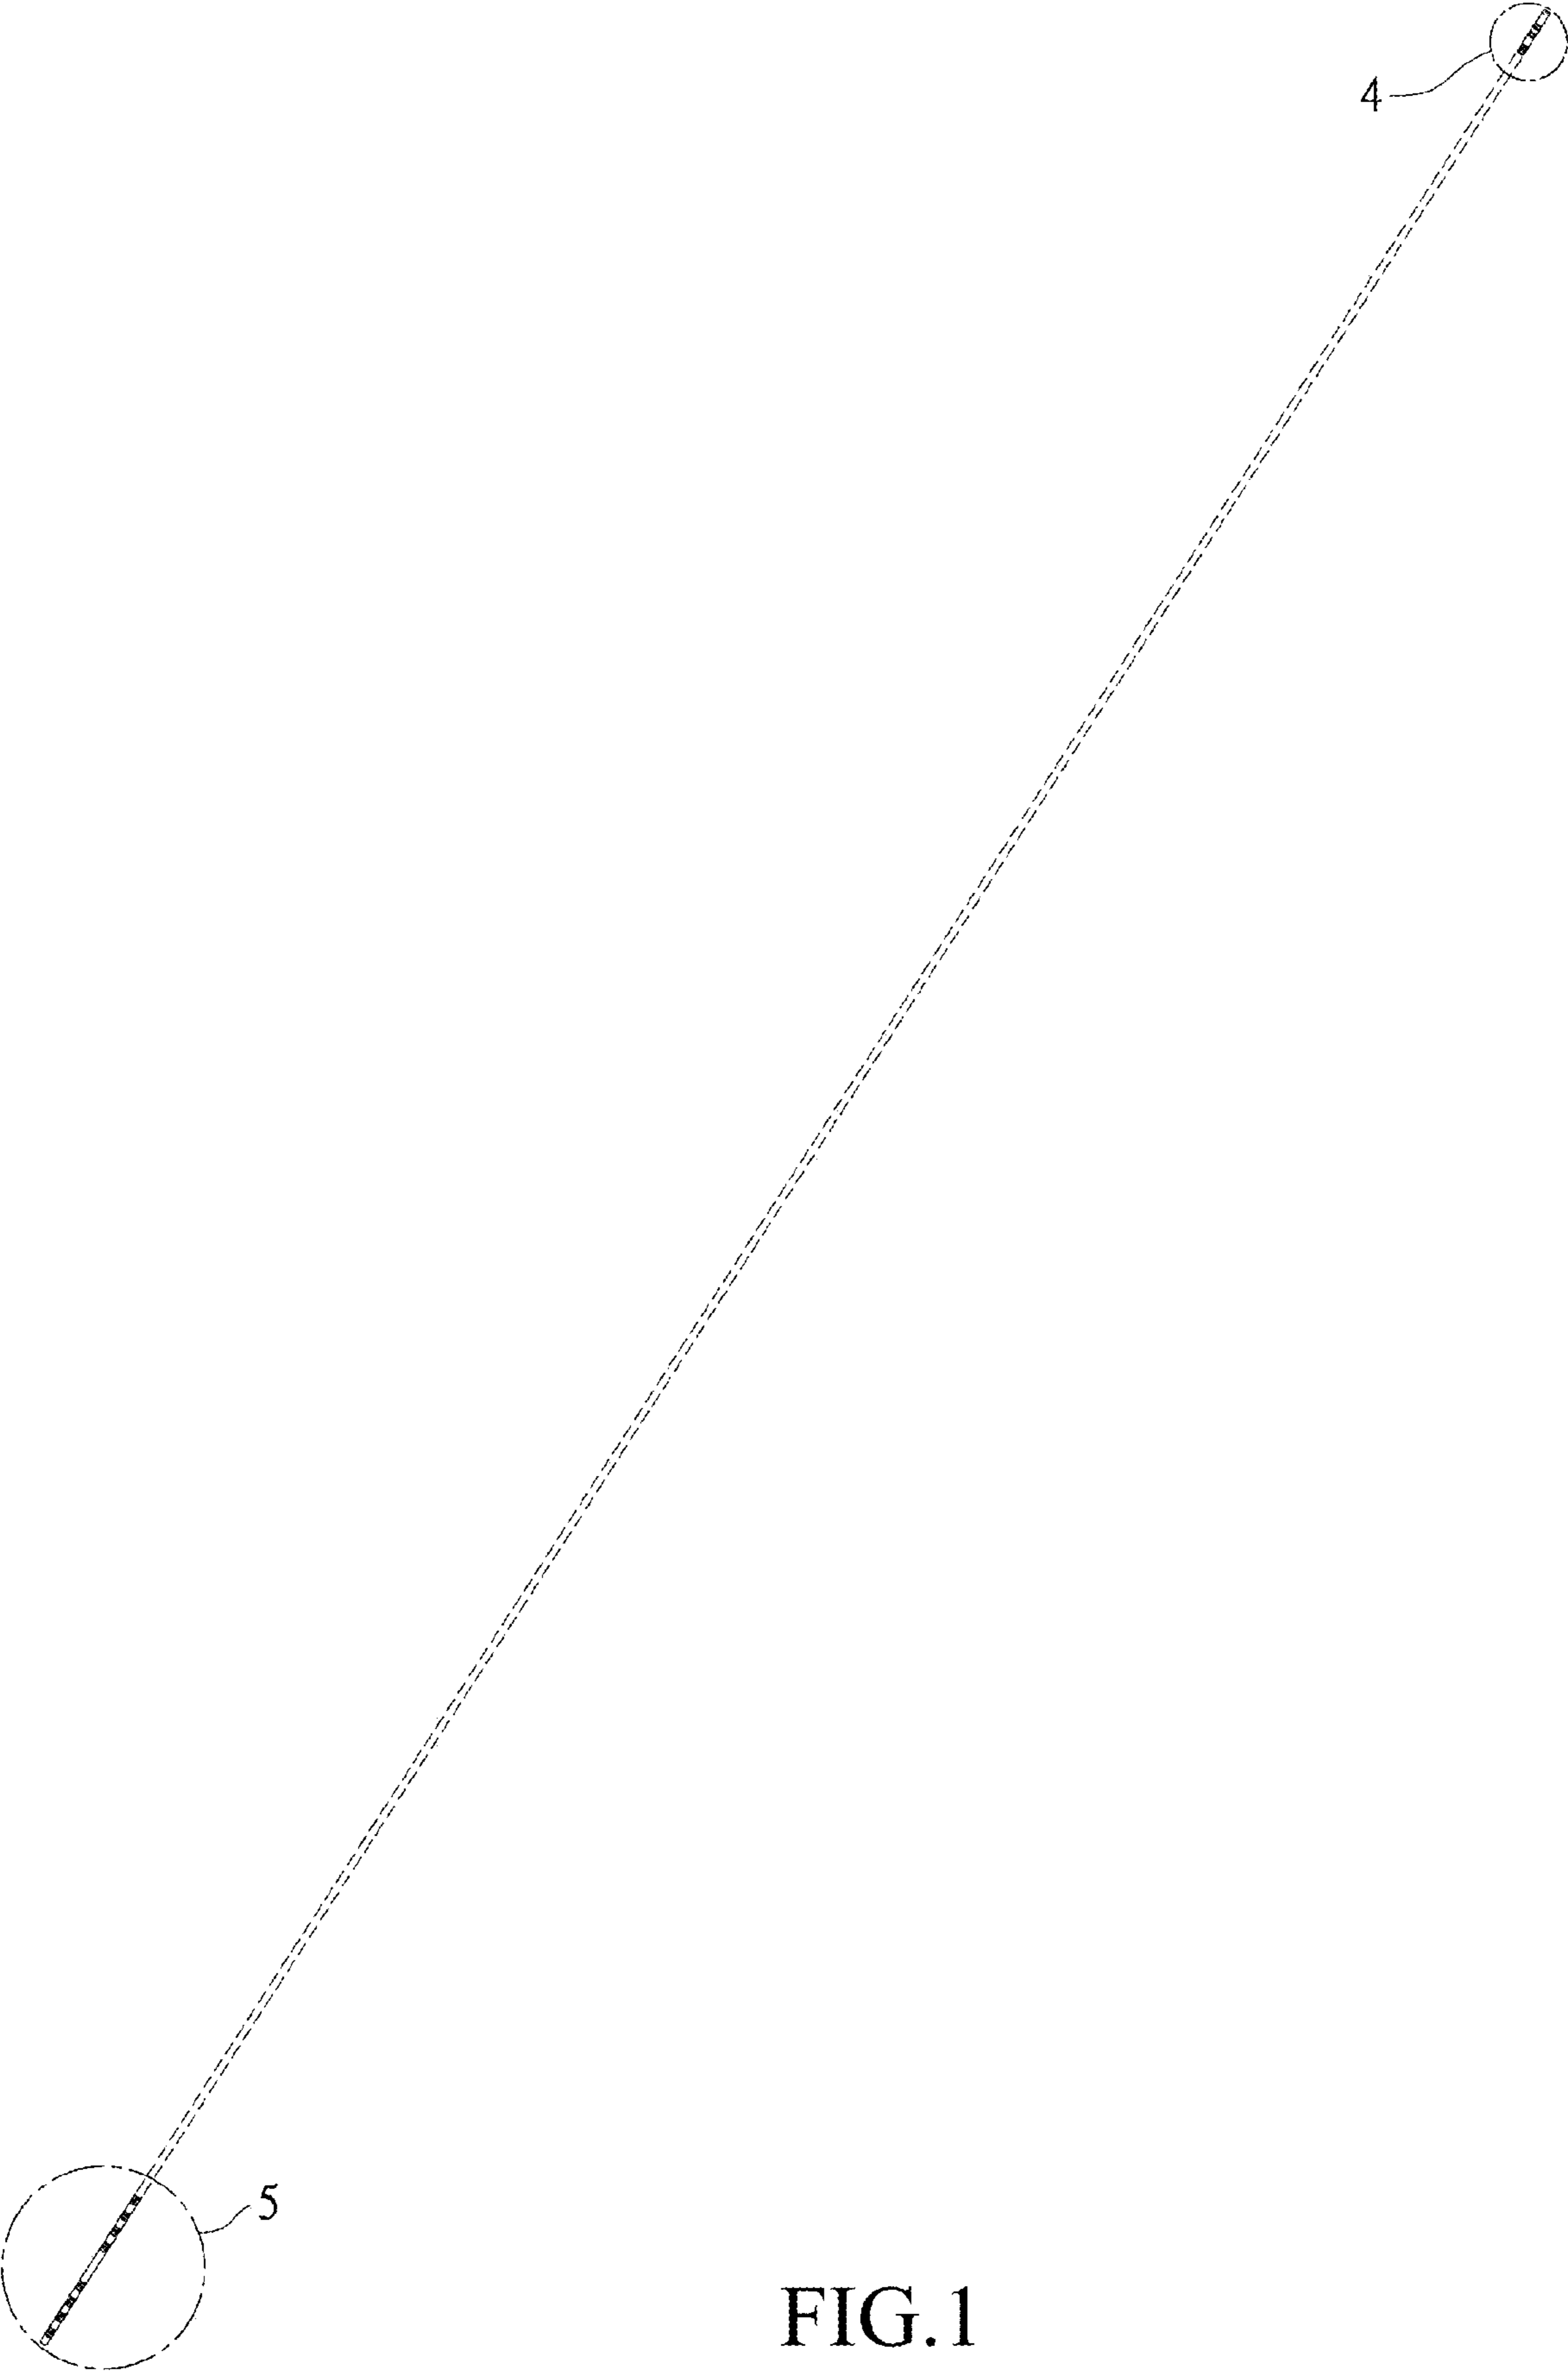


FIG.1

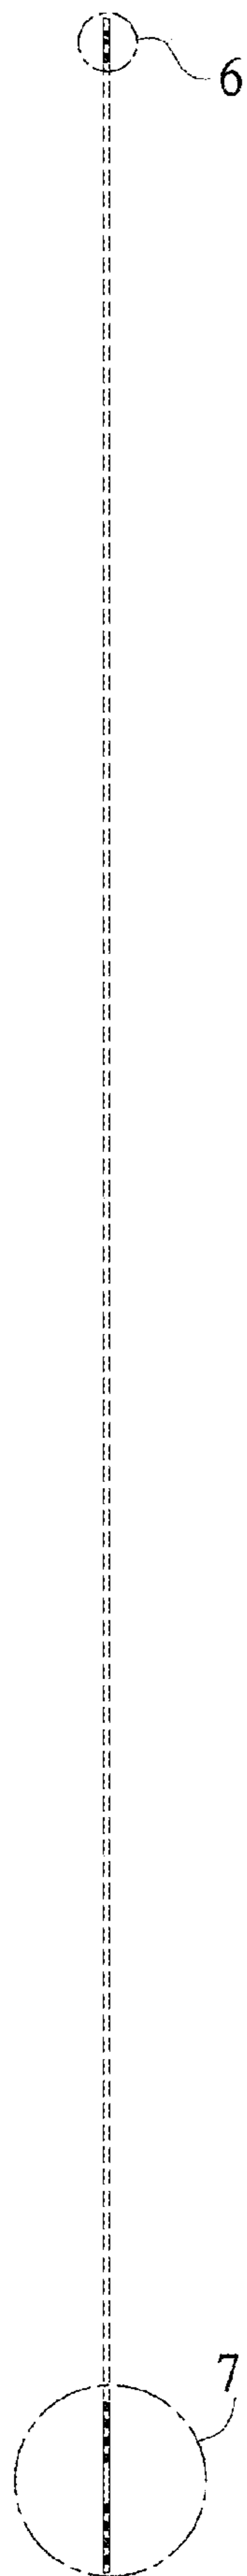


FIG.2

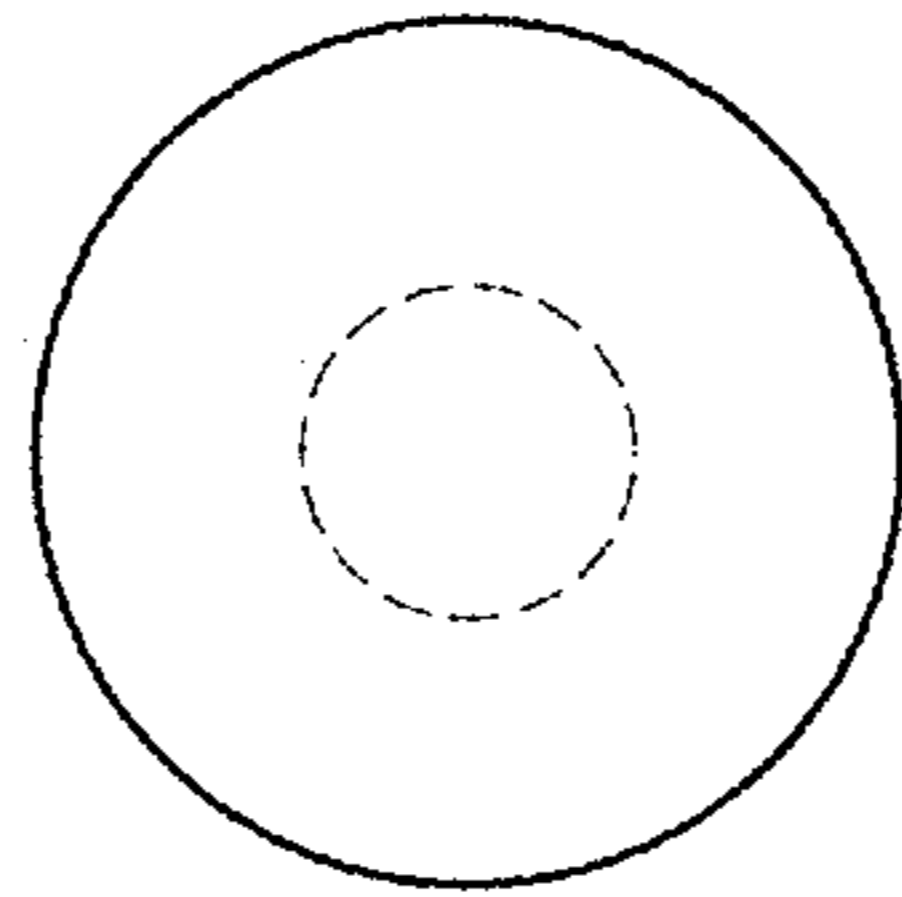


FIG.3

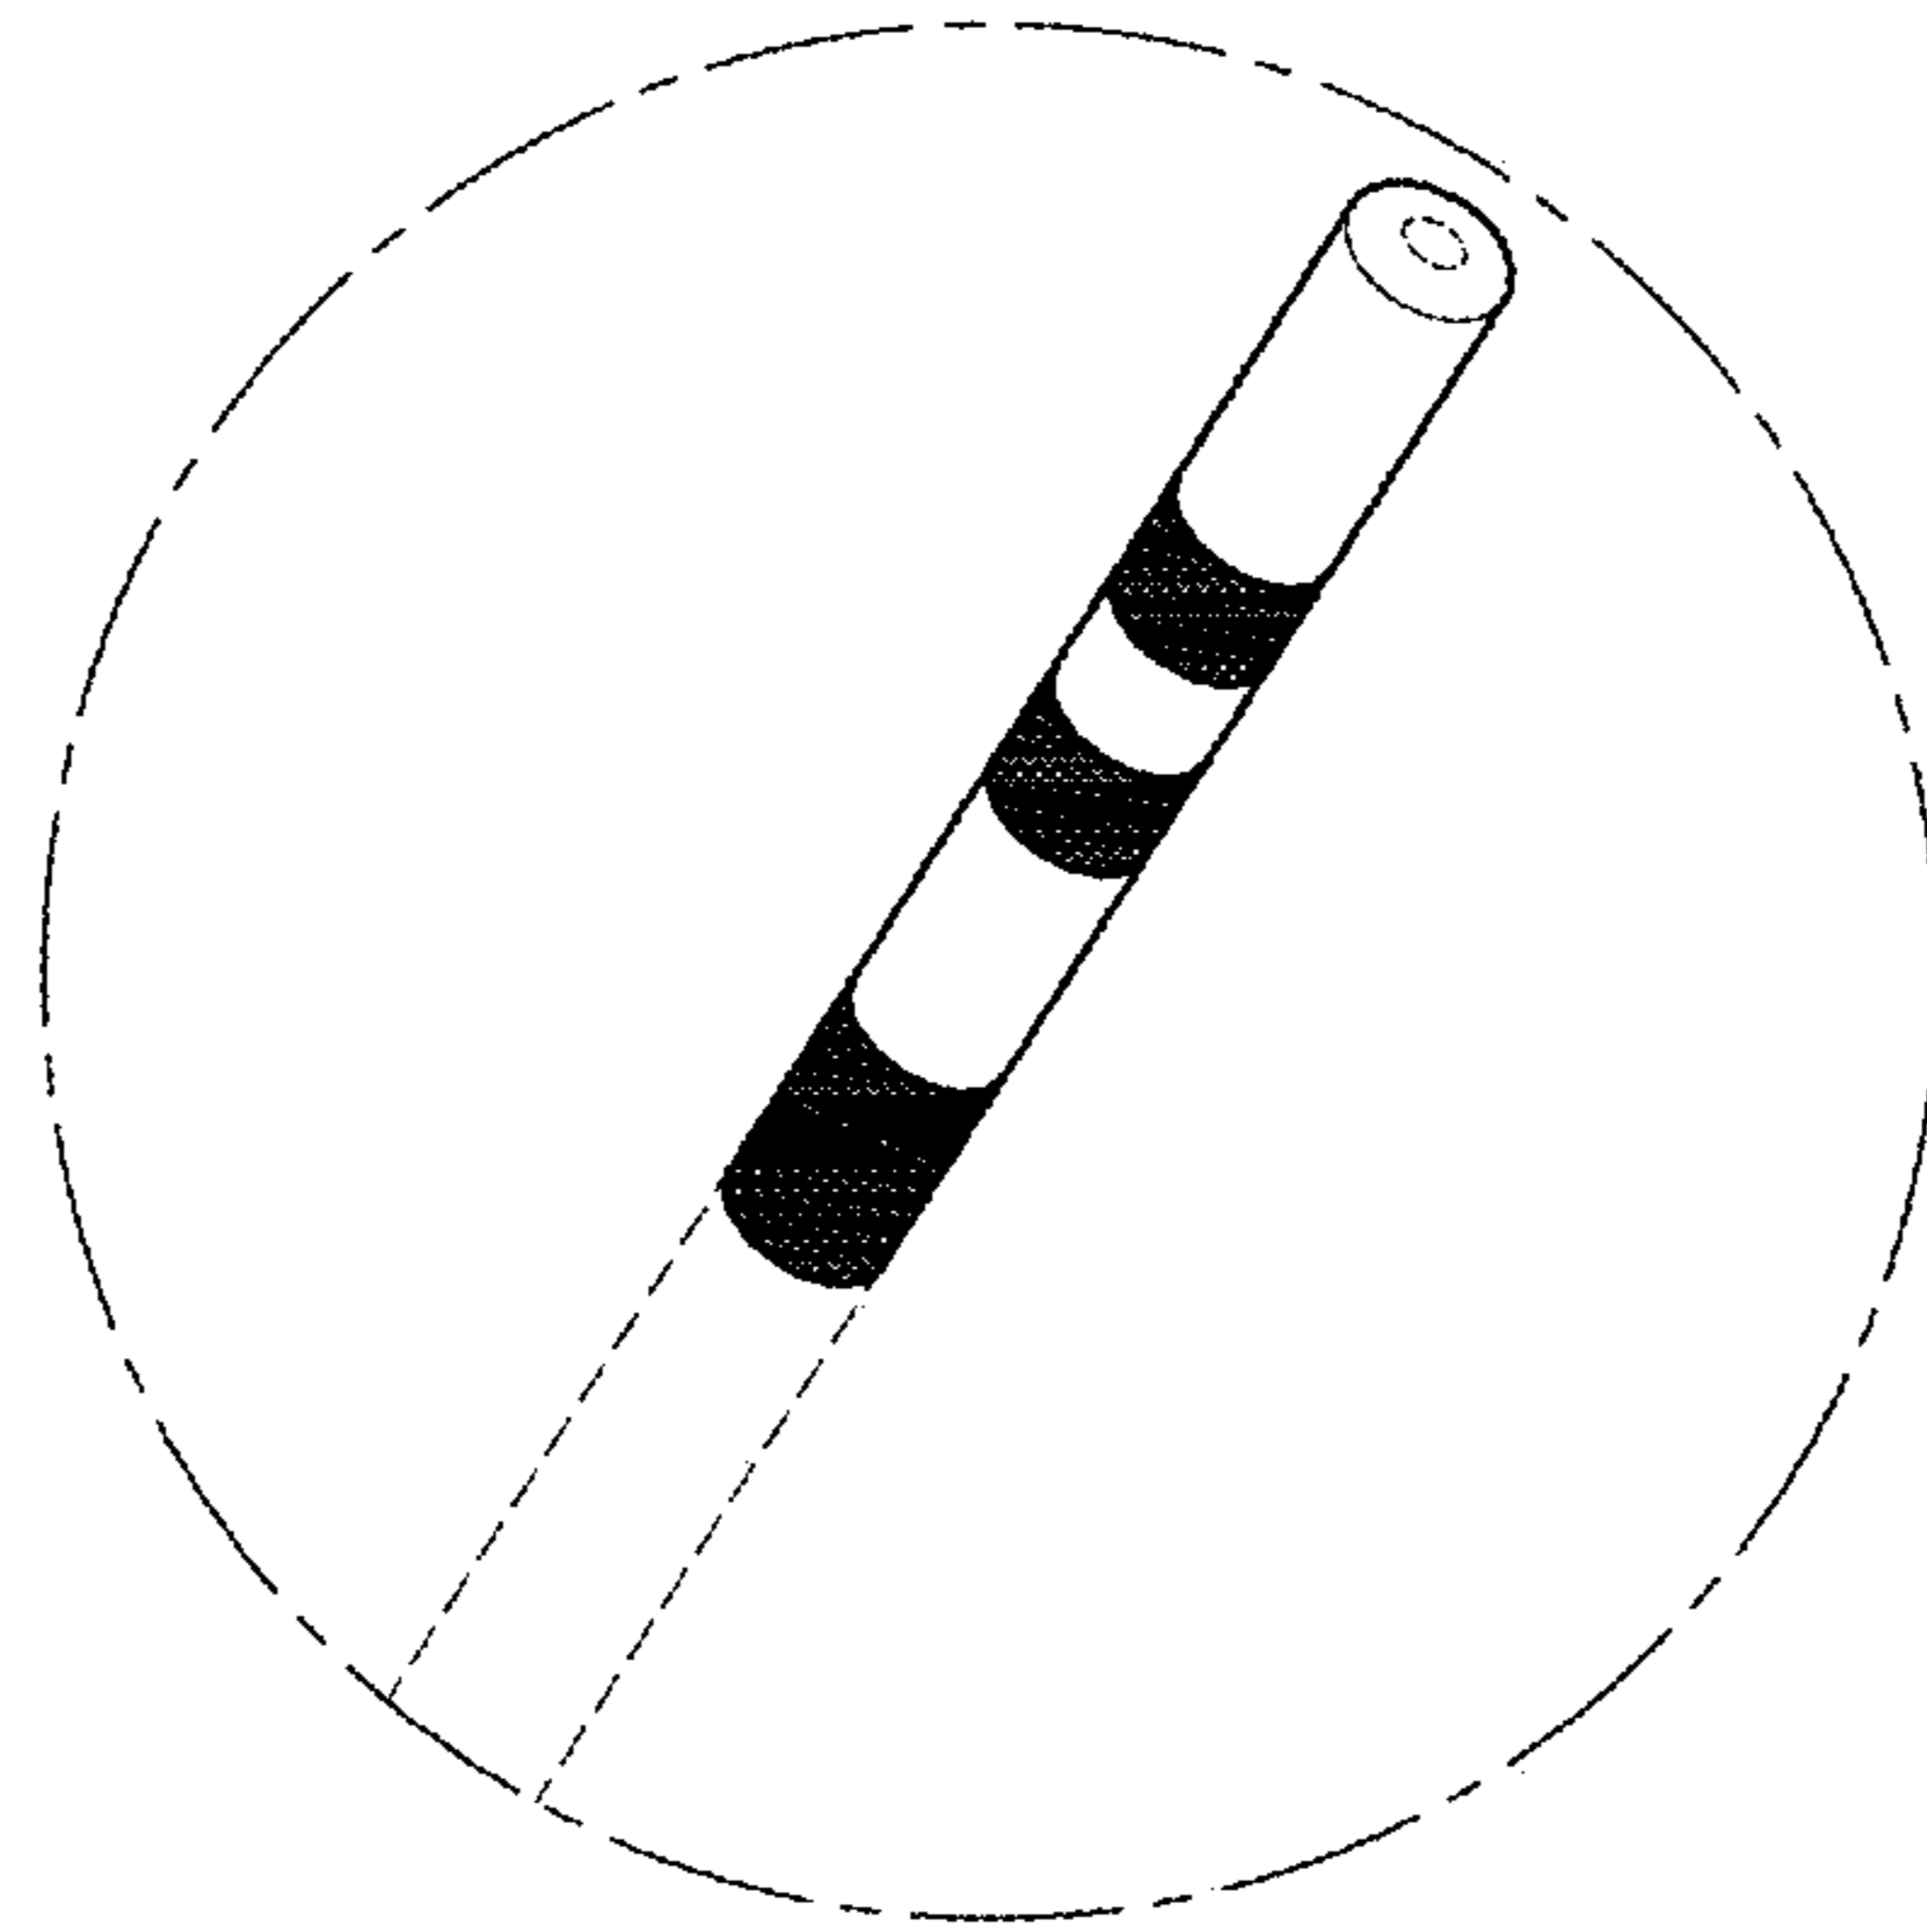


FIG. 4

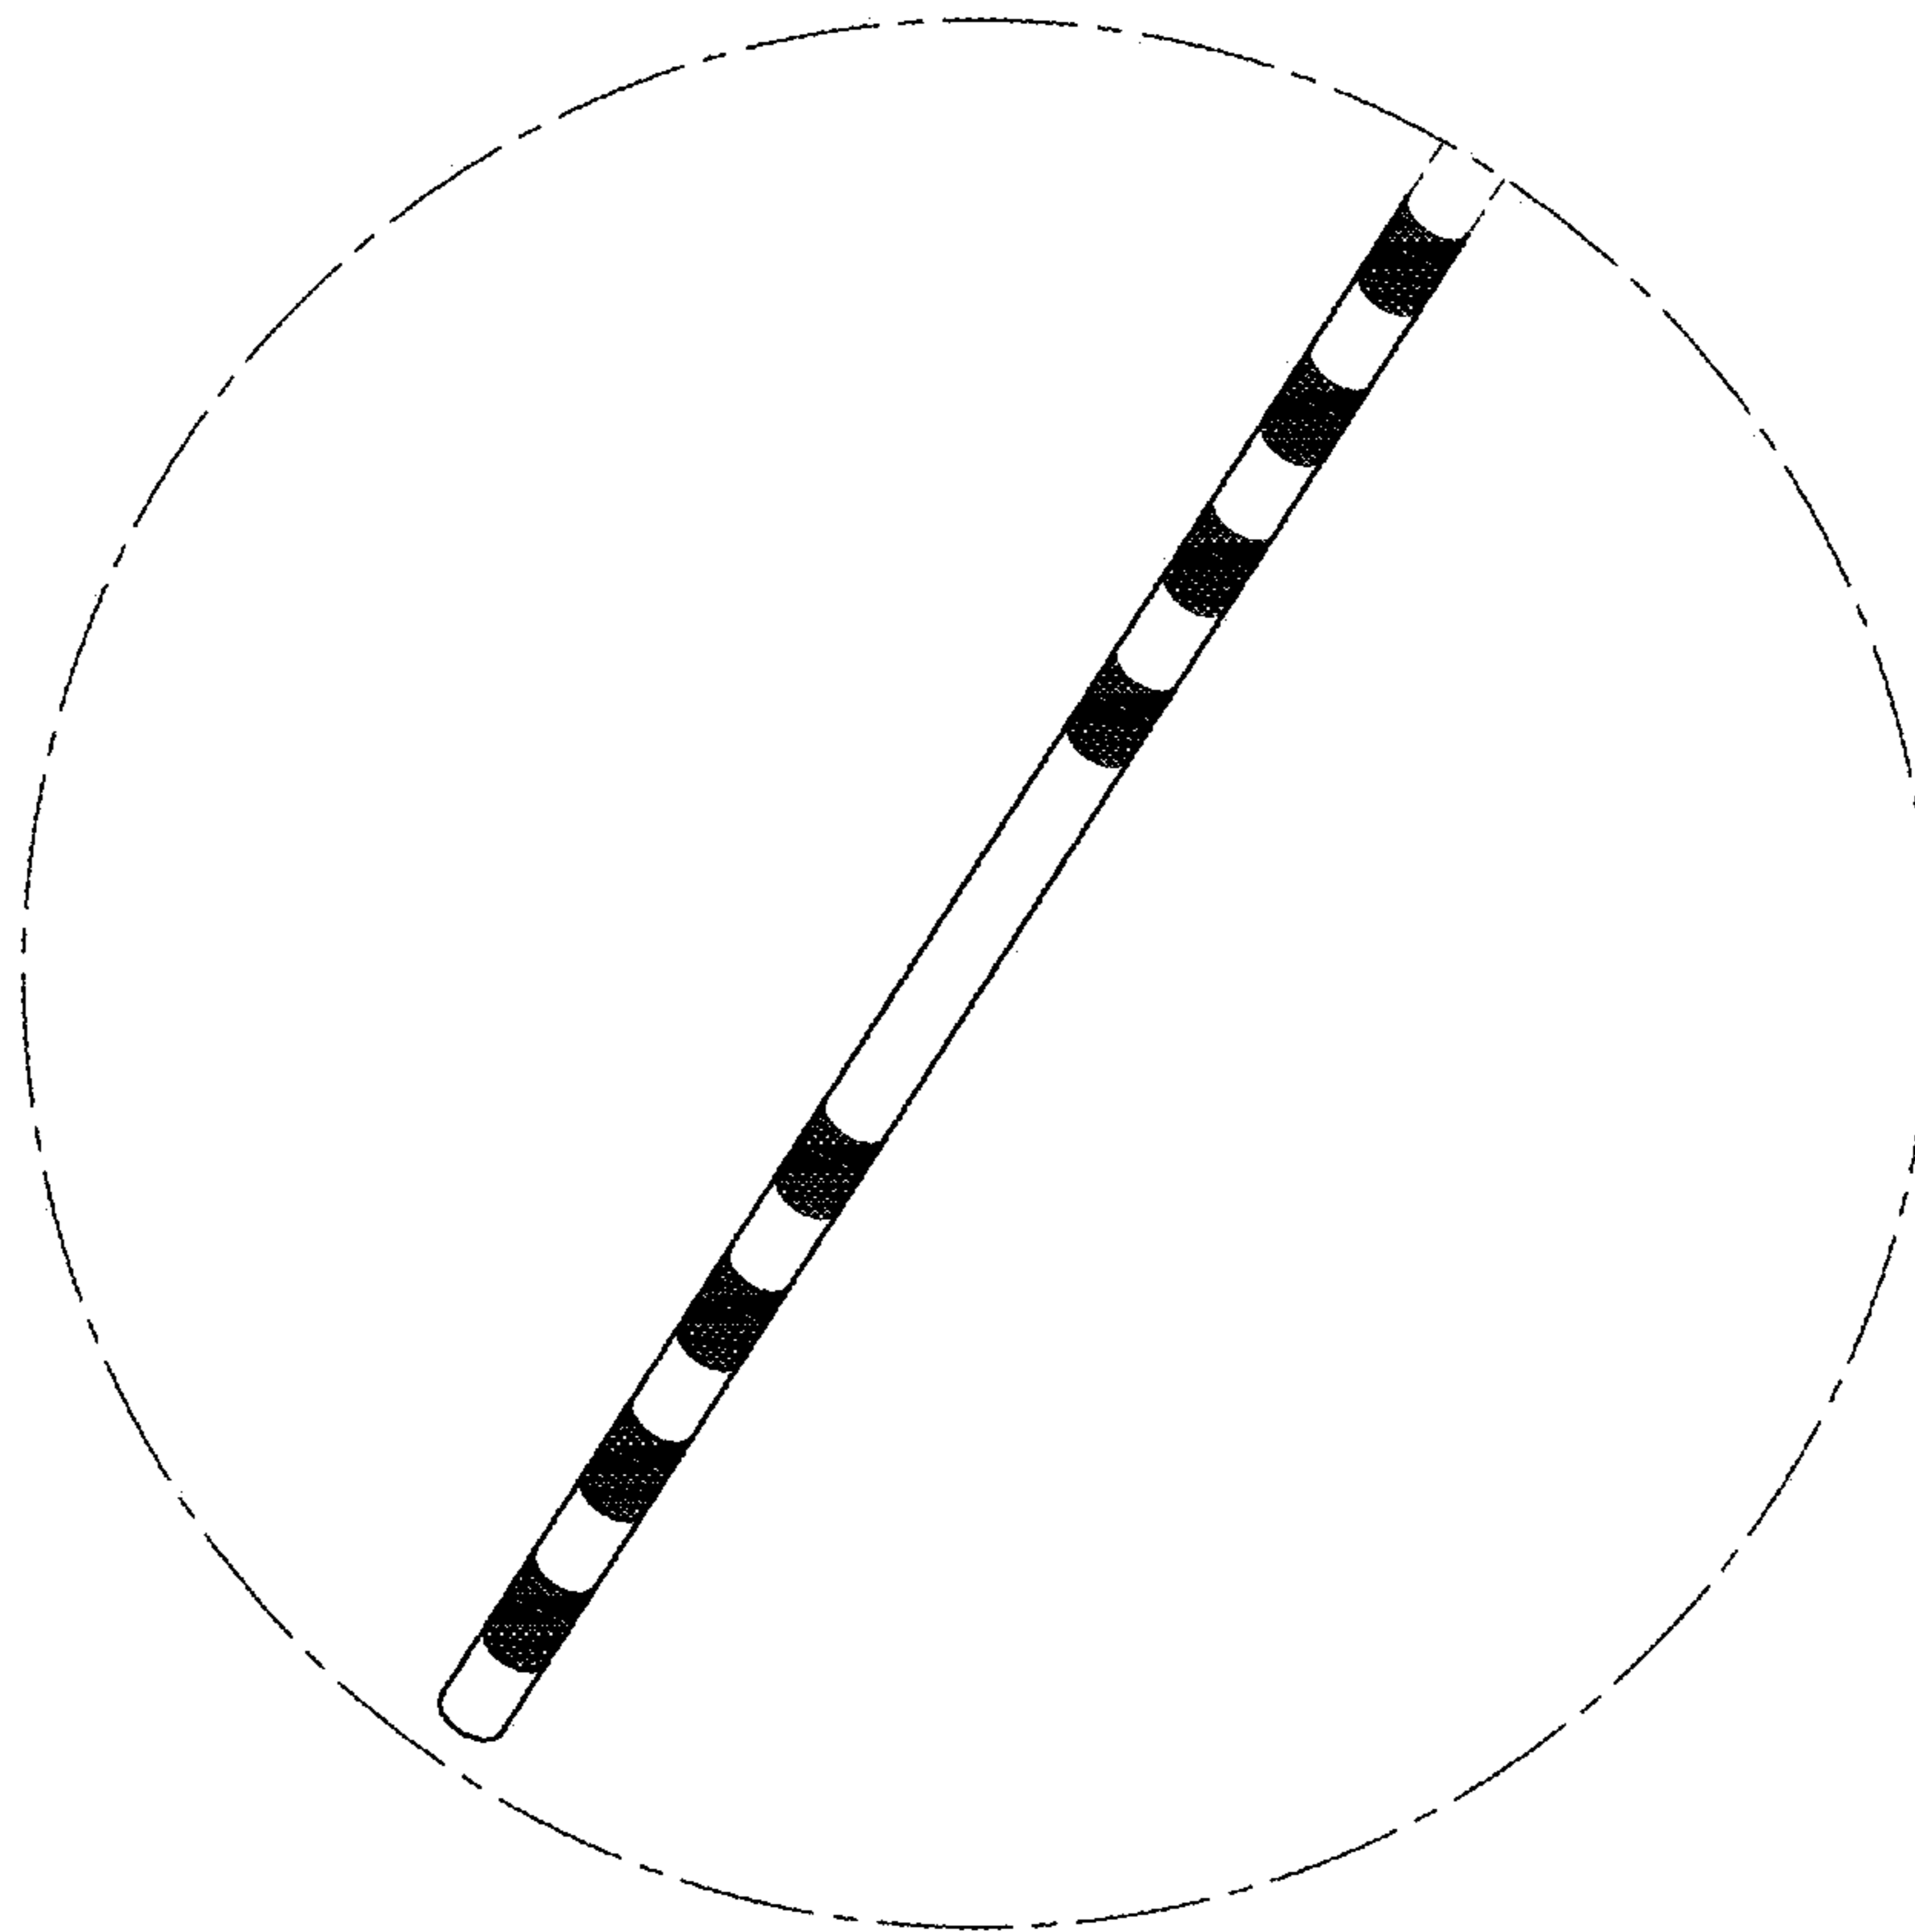


FIG. 5

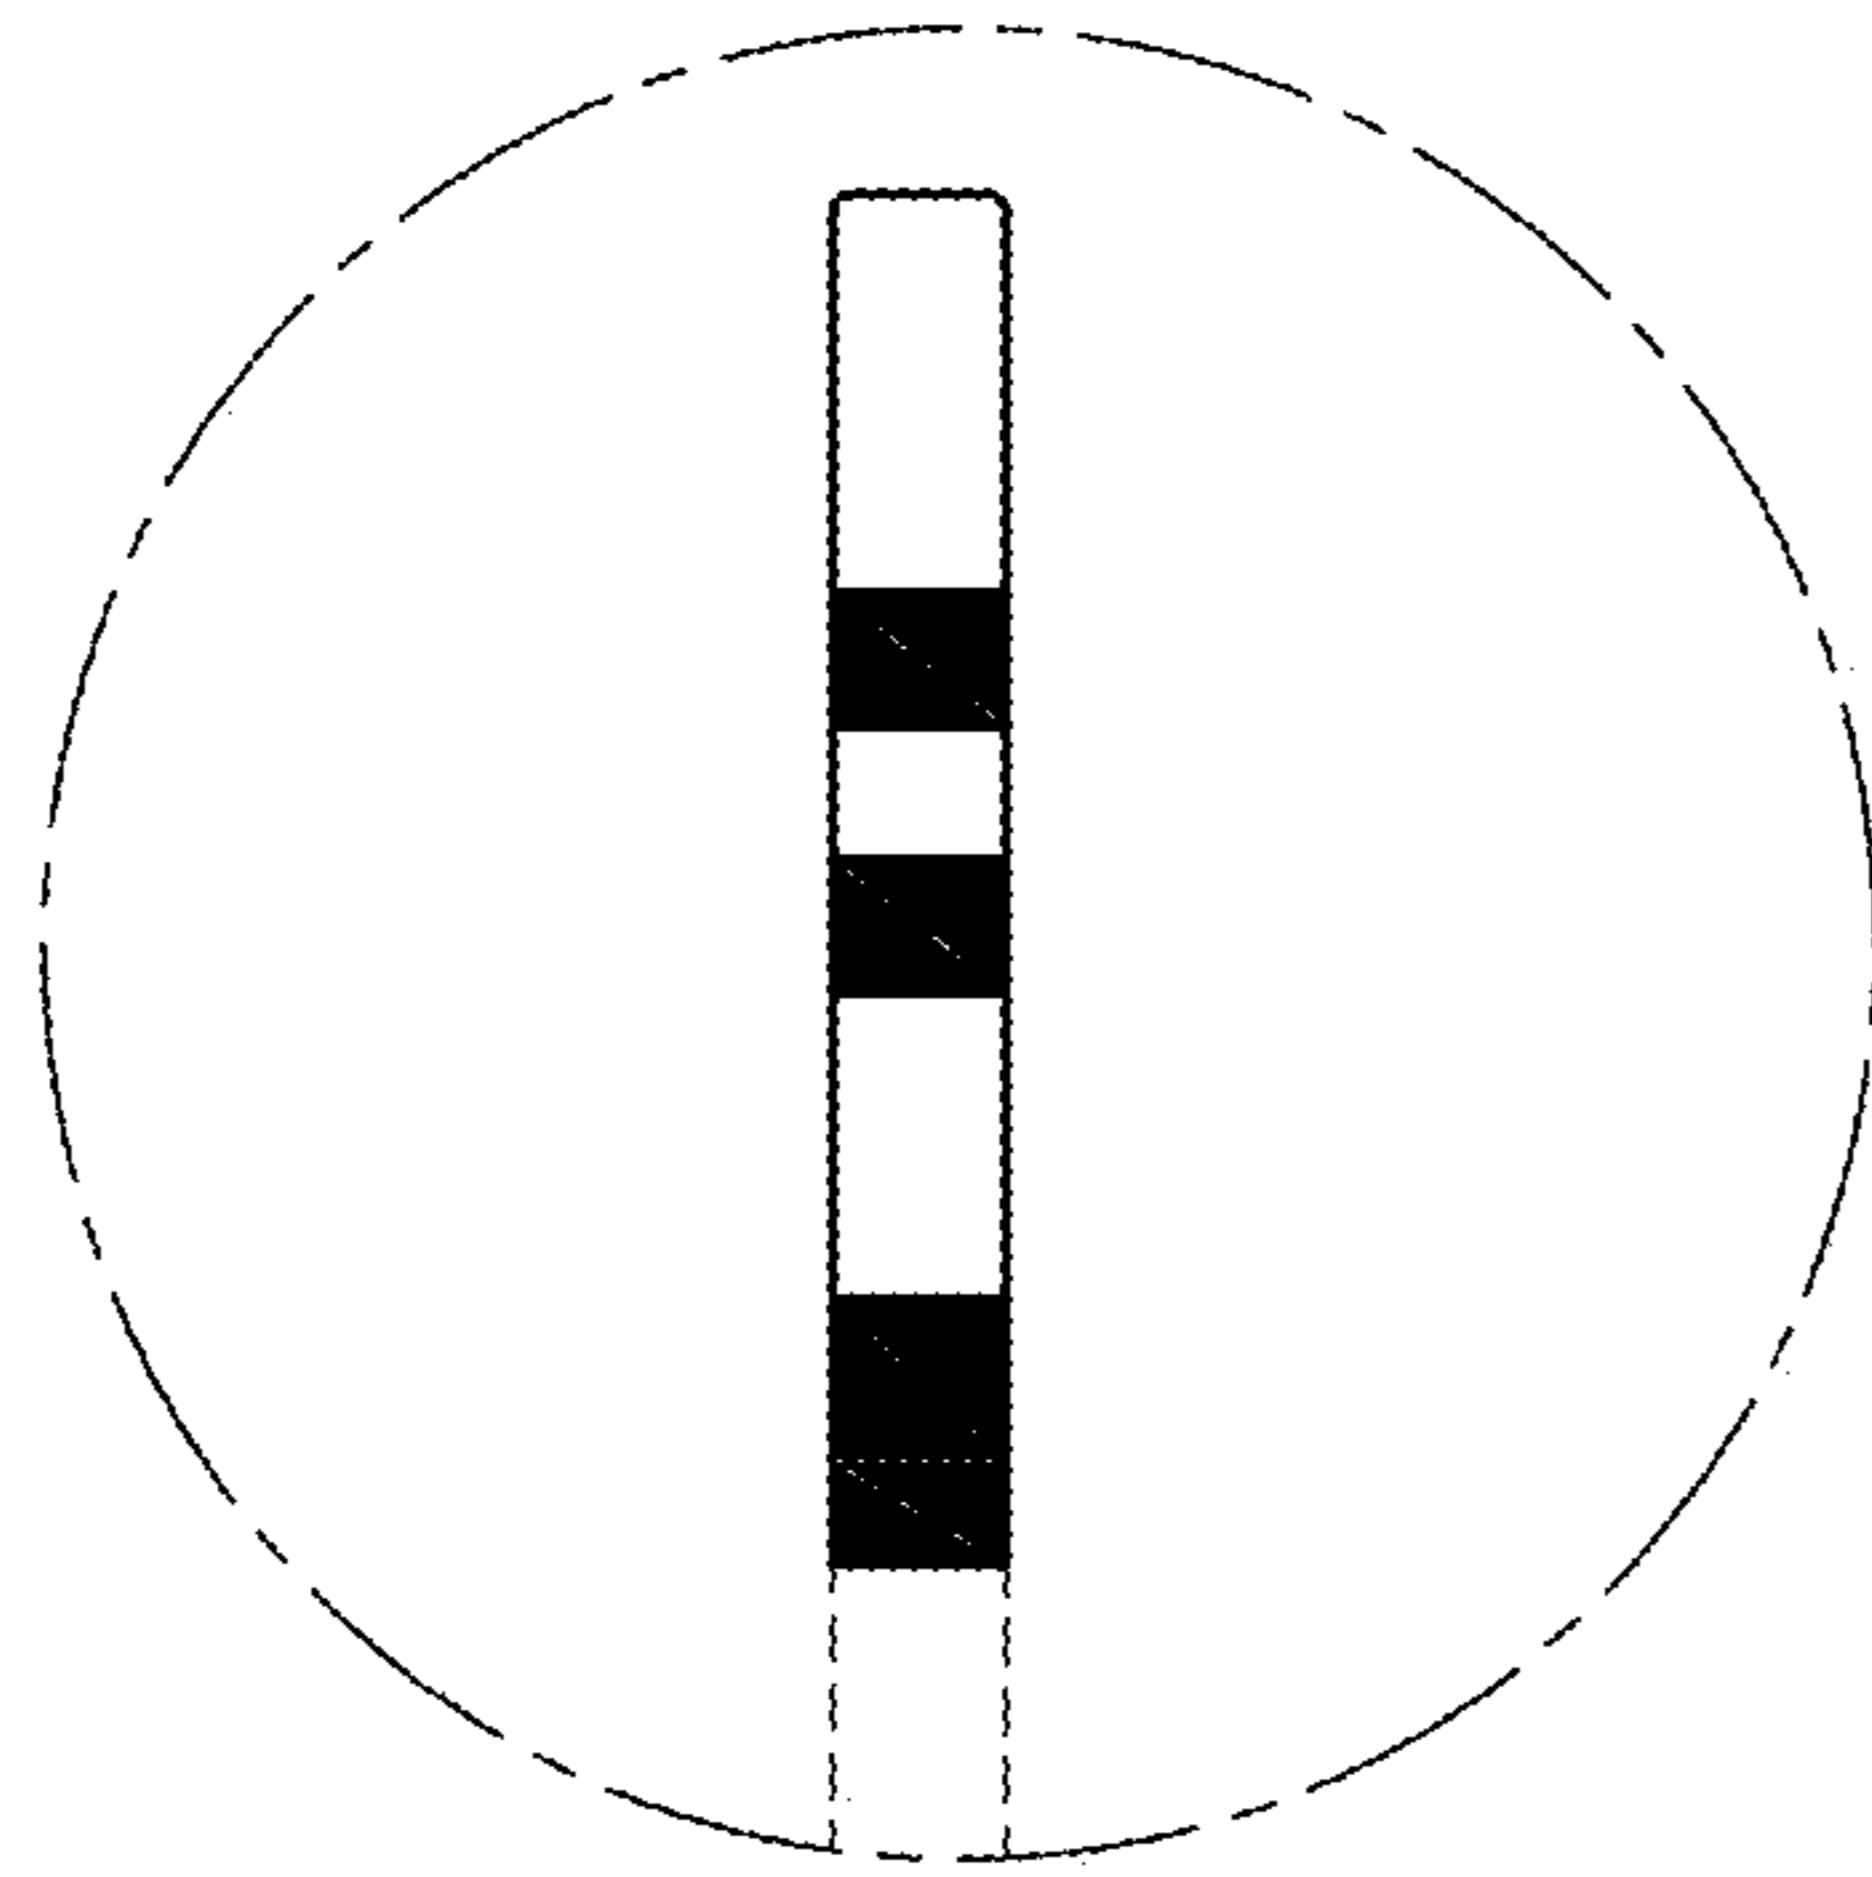


FIG. 6

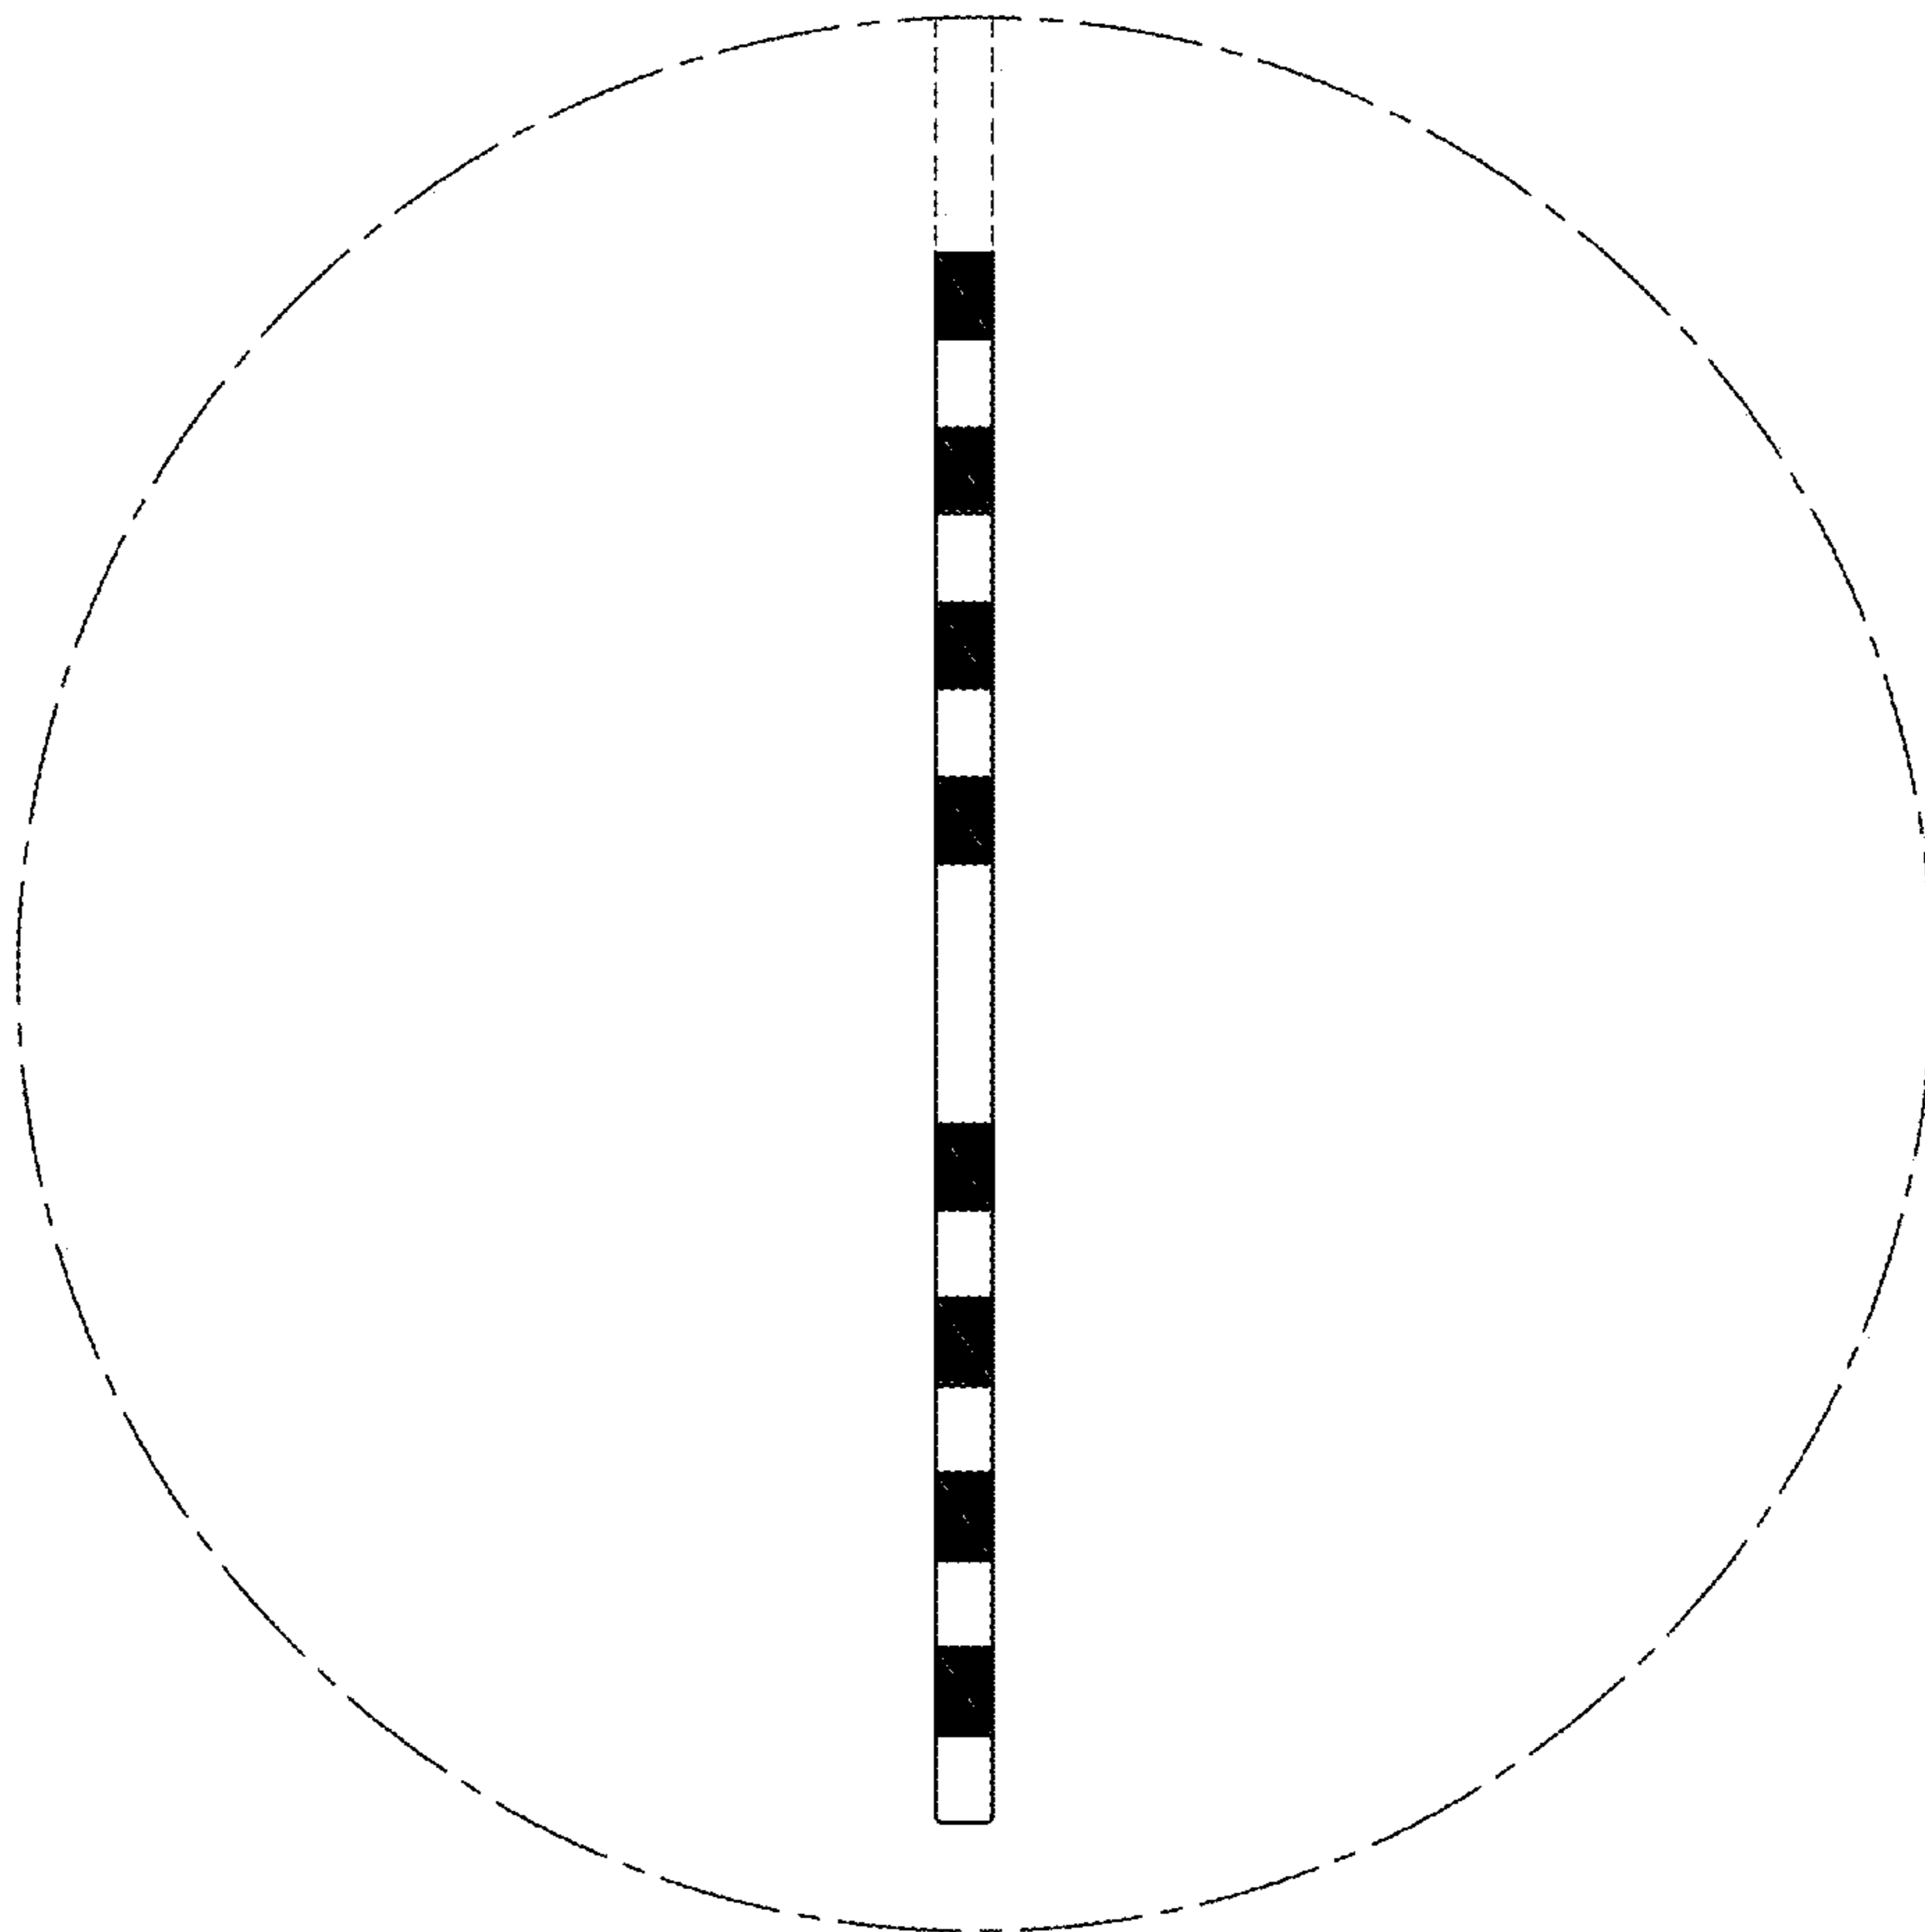


FIG. 7

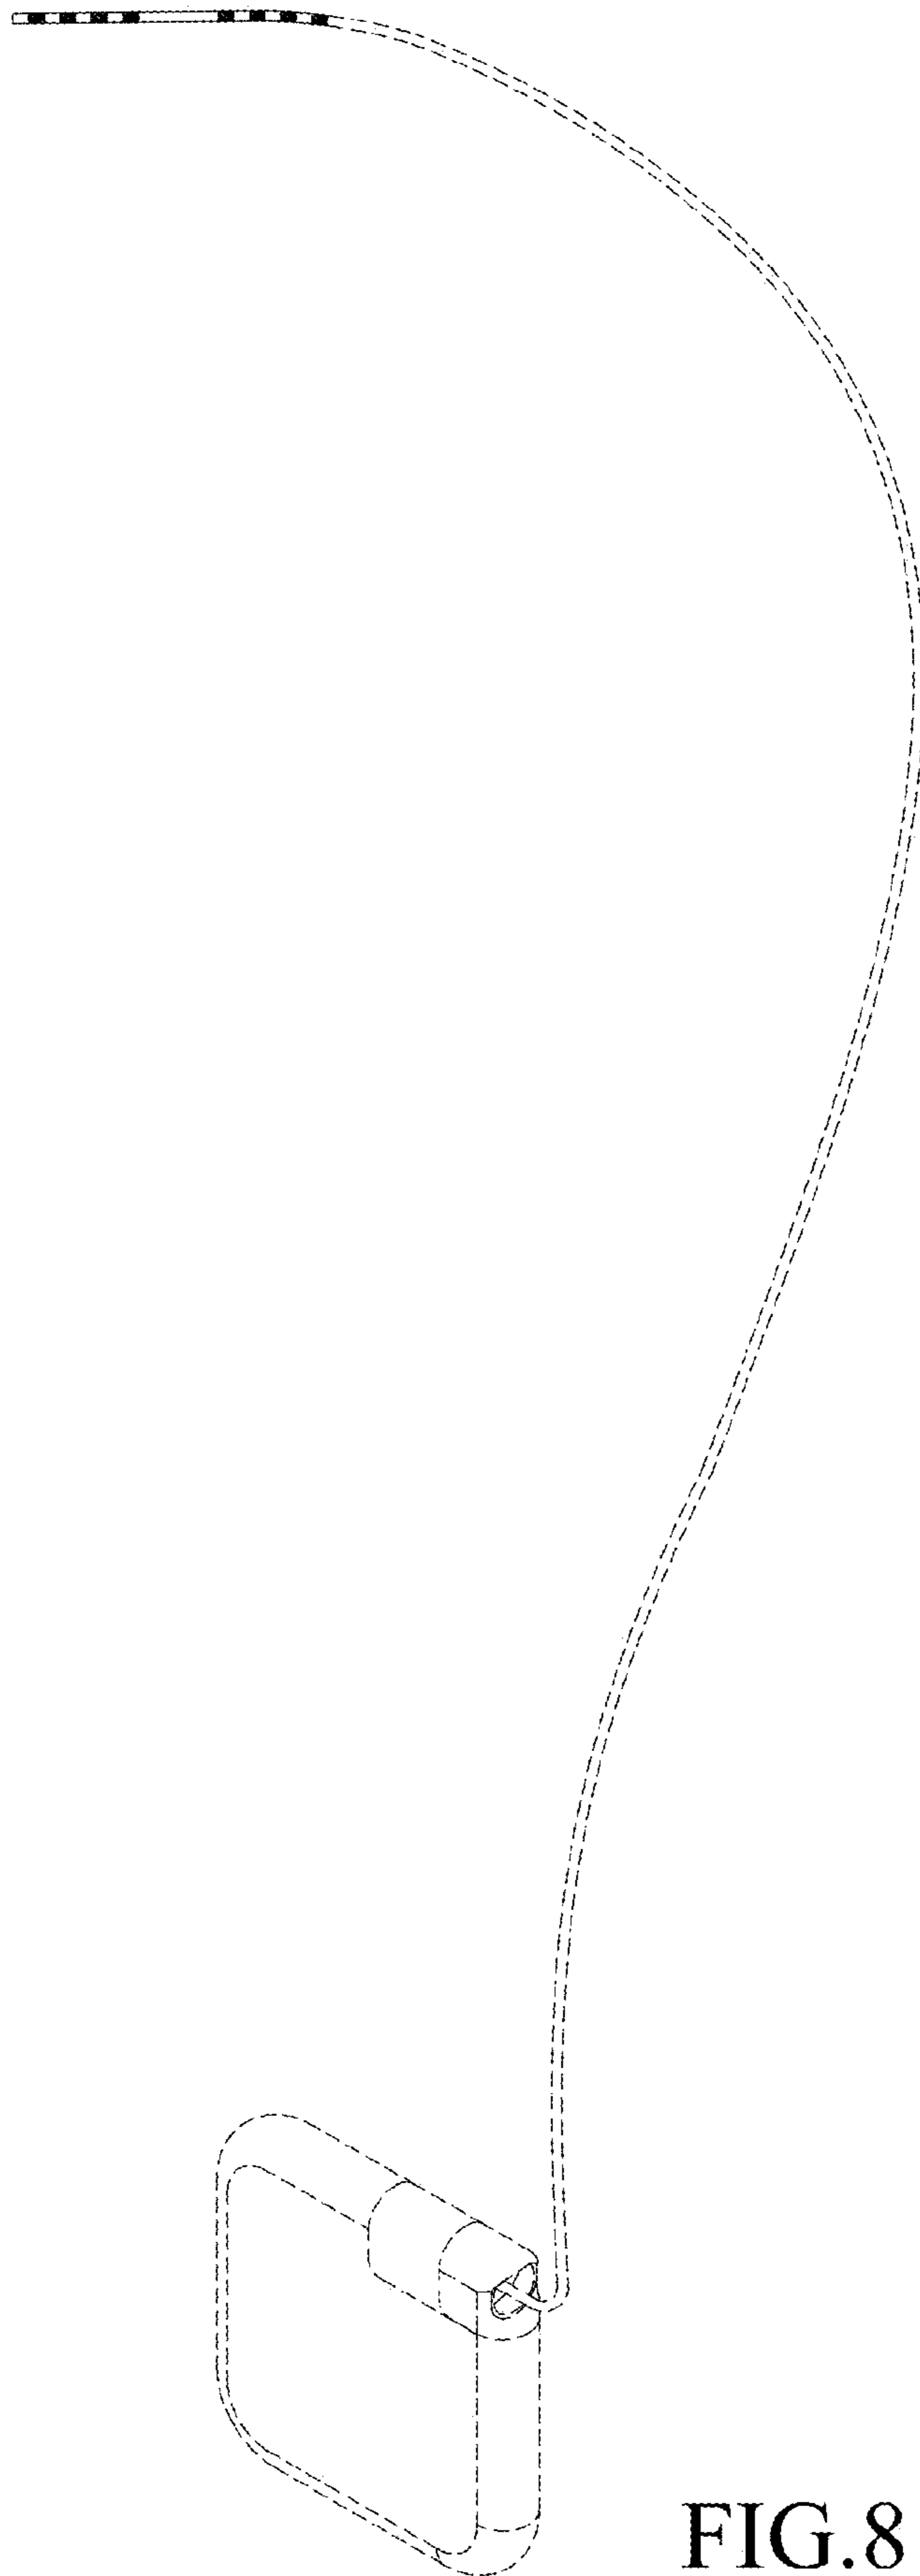


FIG.8