



US00D878603S

(12) **United States Design Patent** (10) **Patent No.:** **US D878,603 S**  
**Zhang et al.** (45) **Date of Patent:** **\*\* Mar. 17, 2020**

(54) **ULTRASOUND SCANNER**  
(71) Applicant: **Clarius Mobile Health Corp.**, Burnaby (CA)  
(72) Inventors: **Binda Zhang**, Surrey (CA); **Alex Barcenas Antonio**, Burnaby (CA); **Daniel Christian Rahardja**, Burnaby (CA)  
(73) Assignee: **Clarius Mobile Health Corp.**, Burnaby, British Columbia (CA)  
(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/668,362**  
(22) Filed: **Oct. 30, 2018**  
(51) **LOC (12) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/187**  
(58) **Field of Classification Search**  
USPC ..... D24/133, 137, 138, 141, 158, 160, 164, D24/165, 167, 170, 186, 187, 200; D10/57, 60, 78, 80  
CPC ... A61B 5/0095; A61B 8/4444; A61B 8/4455; G01S 7/5208  
See application file for complete search history.

D831,219 S \* 10/2018 Henderson ..... D24/187  
D842,482 S \* 3/2019 Harada ..... D24/187  
D844,148 S \* 3/2019 Wilson ..... D24/187  
D846,142 S \* 4/2019 Yellen ..... D24/217  
D861,884 S \* 10/2019 Moon ..... D24/187  
D862,710 S \* 10/2019 Moon ..... D24/187  
D870,296 S \* 12/2019 de Jonge ..... D24/187  
2014/0323869 A1 10/2014 Jin et al.

**FOREIGN PATENT DOCUMENTS**

JP D2018-28945 \* 12/2019

**OTHER PUBLICATIONS**

Multipurpose Ultrasound Scanner. Online, published date unknown. Retrieved on Dec. 29, 2019 from URL: <https://clarius.com/scanners/c3/>.\*

(Continued)

*Primary Examiner* — Susan Bennett Hattan  
*Assistant Examiner* — Omeed Agilee  
(74) *Attorney, Agent, or Firm* — Julian Ho

(57) **CLAIM**

The ornamental design of an ultrasound scanner, substantially as shown and described.

**DESCRIPTION**


FIG. 1 is a front perspective view of an ultrasound scanner in accordance with the present design; FIG. 2 is a rear perspective view thereof; FIG. 3 is a top view thereof; FIG. 4 is a front view thereof; FIG. 5 is a right side view thereof; FIG. 6 is a left side view thereof; FIG. 7 is a rear view thereof; and, FIG. 8 is a bottom view thereof. The broken lines in the figures represent portions of the article which form no part of the claimed design.

**1 Claim, 4 Drawing Sheets**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D392,044 S \* 3/1998 Mesaros ..... D24/186  
6,780,154 B2 8/2004 Hunt et al.  
D555,252 S \* 11/2007 Kitayama ..... D24/186  
D667,557 S \* 9/2012 Boudier ..... D24/186  
D704,341 S \* 5/2014 Ryu ..... D24/187  
D745,972 S \* 12/2015 Kitayama ..... D24/187  
D763,452 S \* 8/2016 Ryu ..... D24/187  
D811,607 S \* 2/2018 Kitayama ..... D24/187  
D816,850 S \* 5/2018 Asai ..... D24/187  
D822,837 S \* 7/2018 Naka ..... D24/187

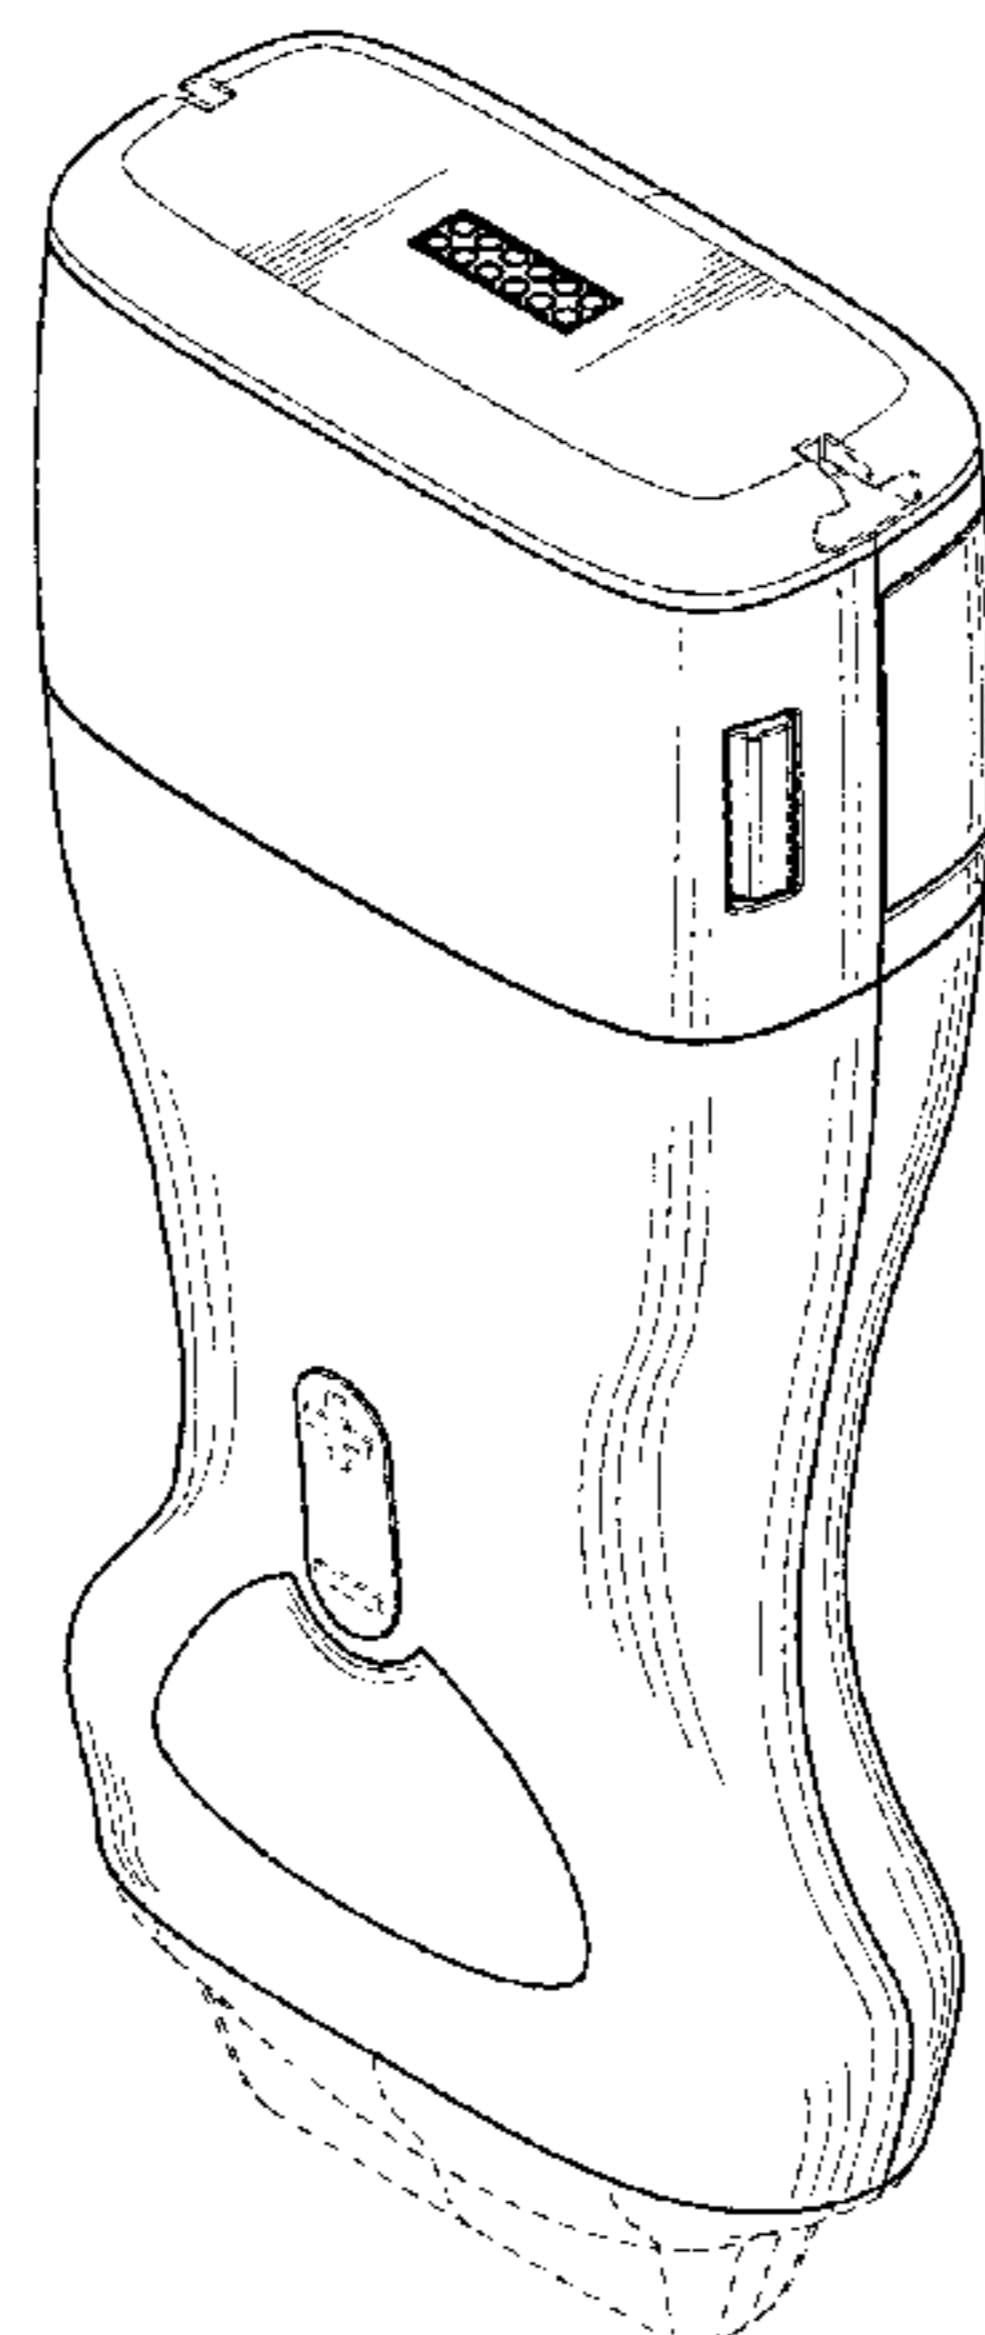

(56)

**References Cited**


OTHER PUBLICATIONS

Wireless for greater ultrasound efficiency. Online, published date unknown. Retrieved on Dec. 29, 2019 from URL: <https://mides.com/en/wireless-probe/>.\*


Sonostar, "UProbe-2/UProbe-3 Series (Convex and Linear) Array Ultrasound Probe Scanner", publication date unknown, available online: <http://sonostar.net/EnProductShow.asp?ID=310>, last accessed Nov. 13, 2018.

Healcerion, "Sonon 300L", publication date unknown, available online: <https://www.healcerion.com/products/ultrasounds/>, last accessed Nov. 13, 2018.


\* cited by examiner

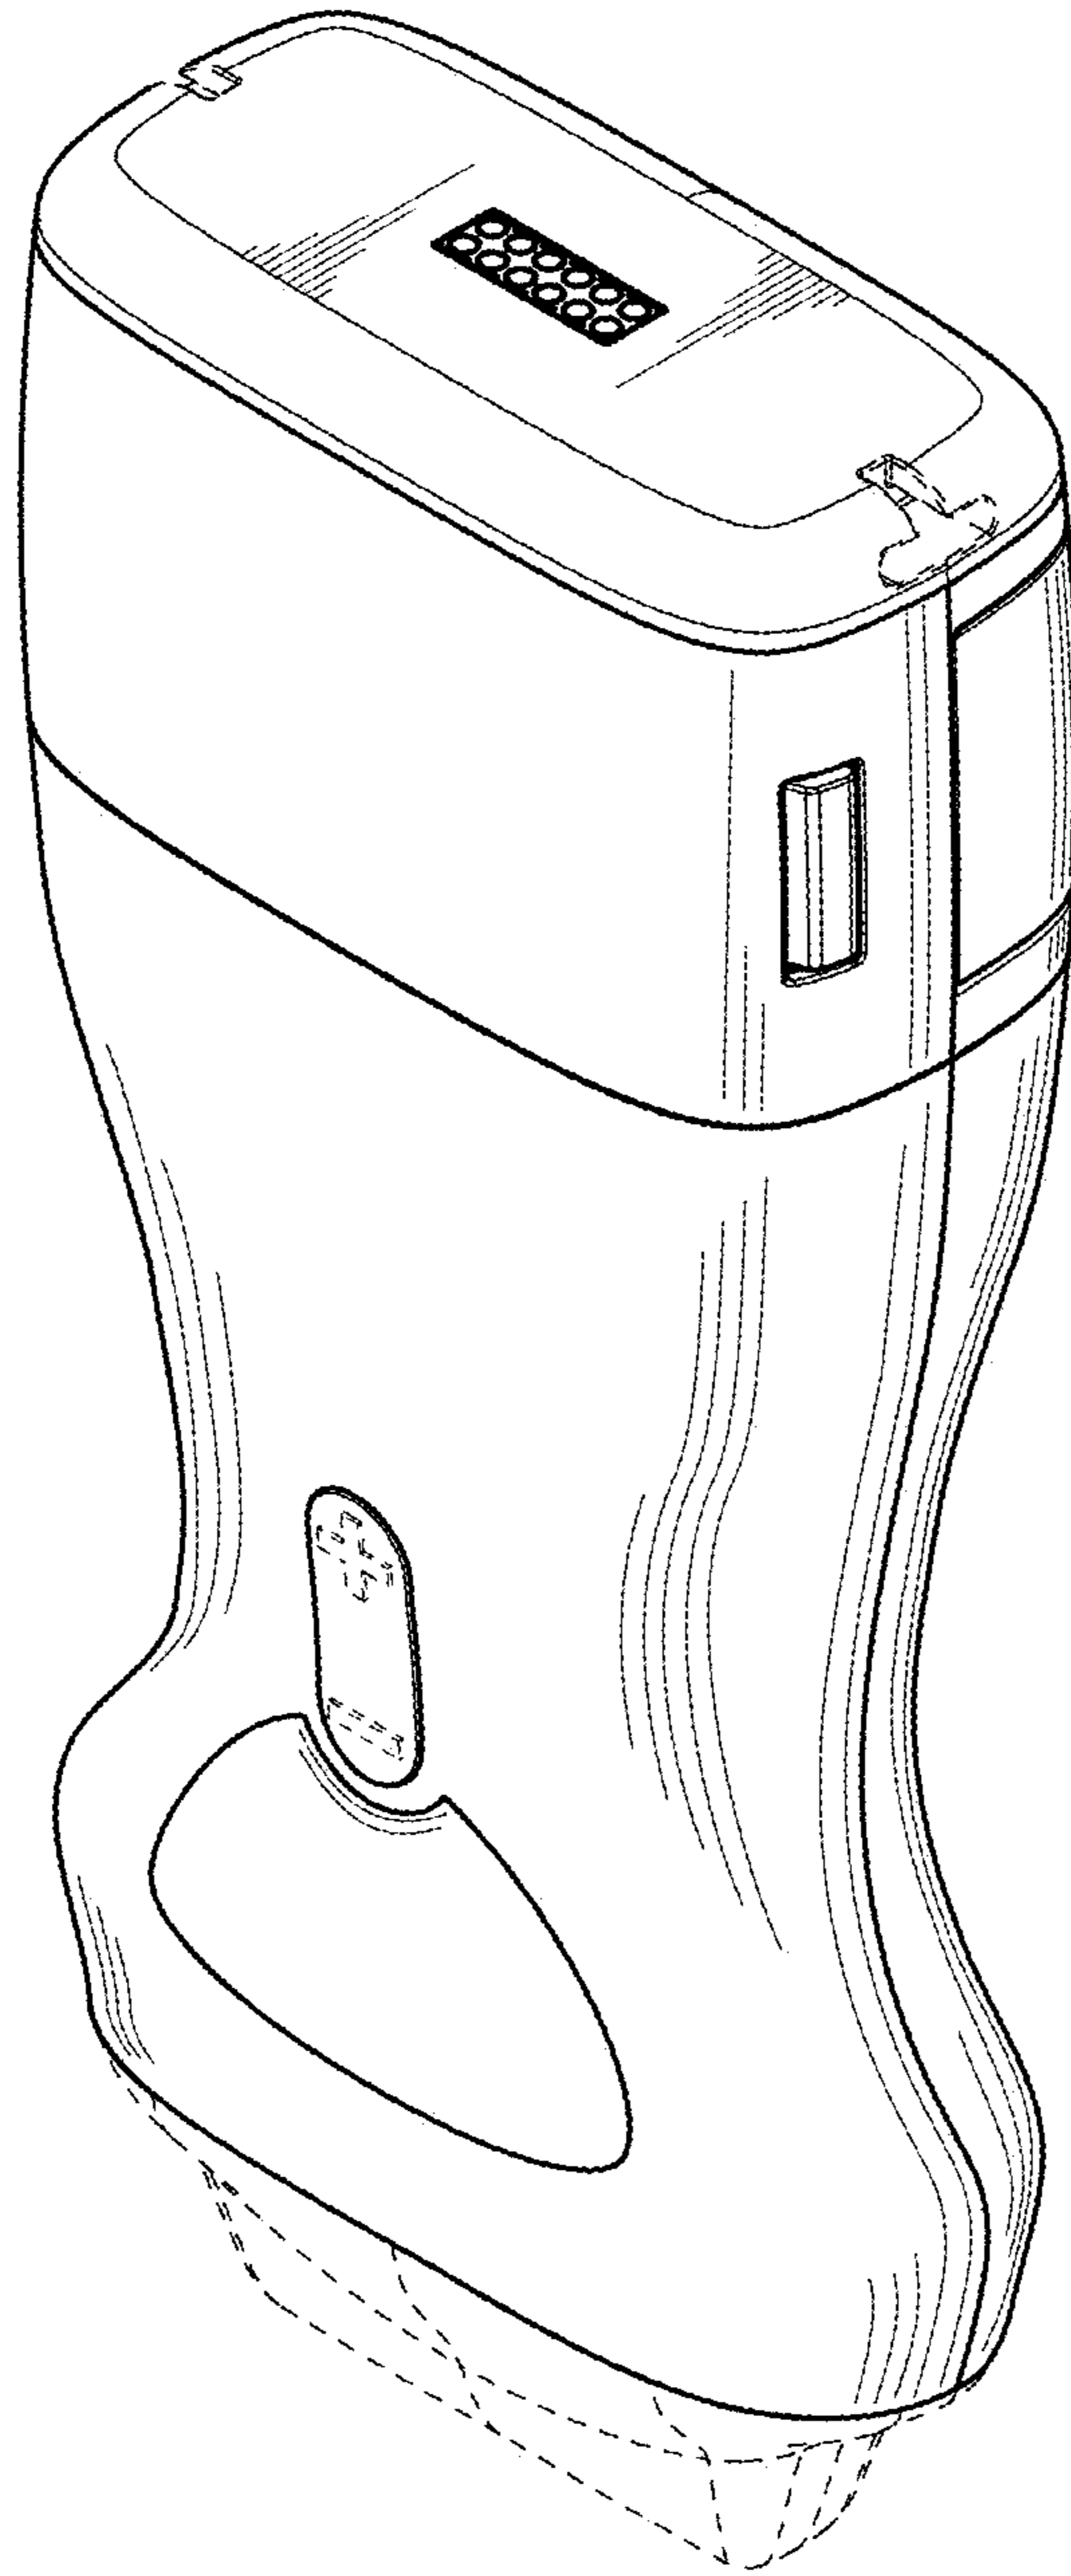


**FIG. 1**

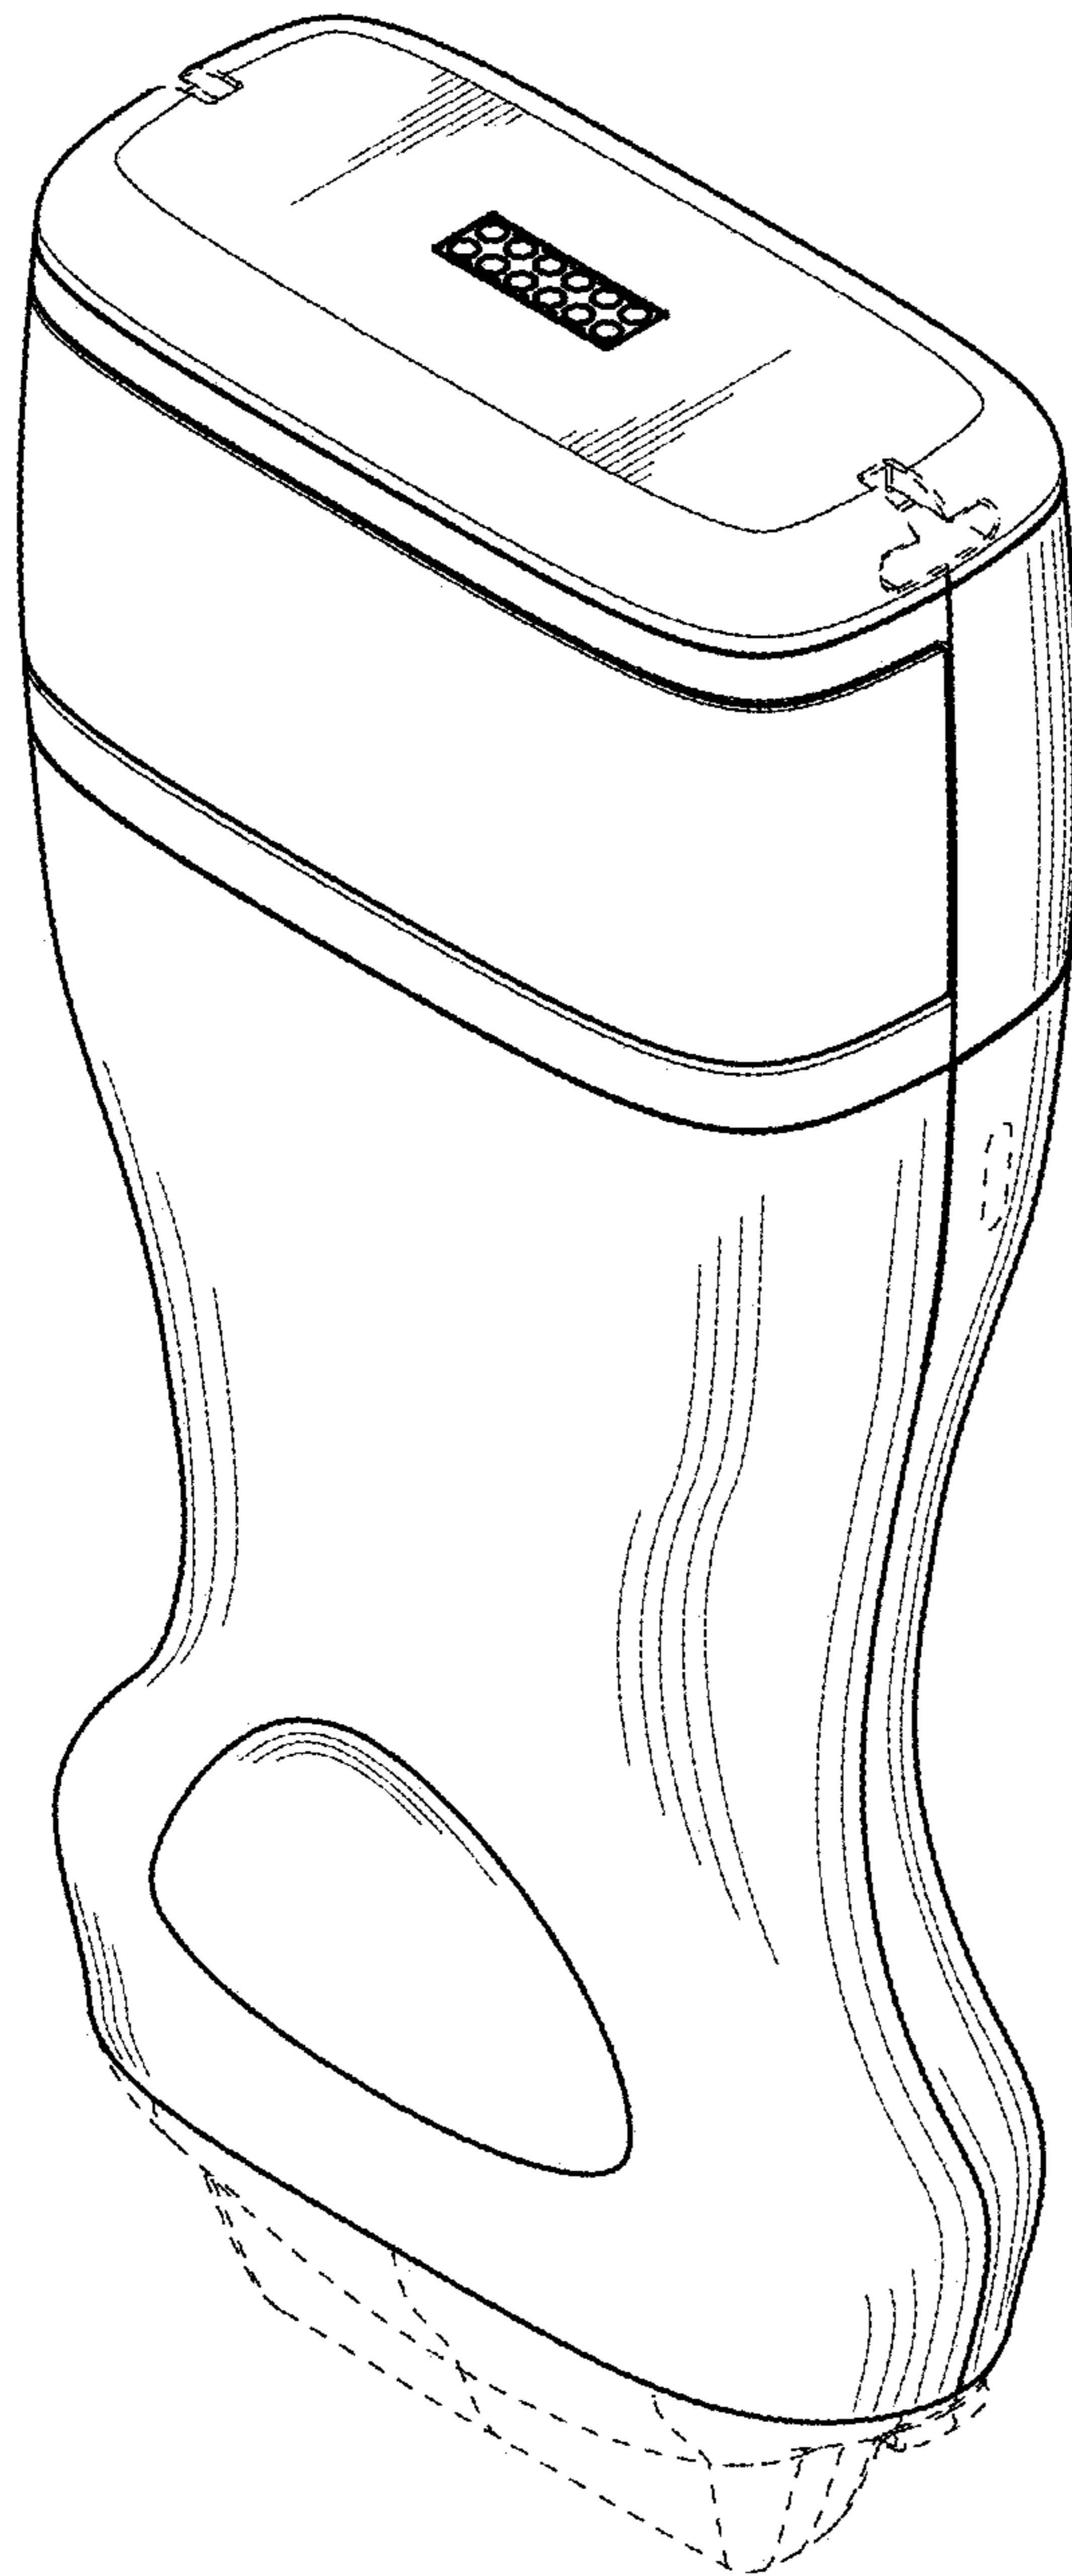


**FIG. 2**

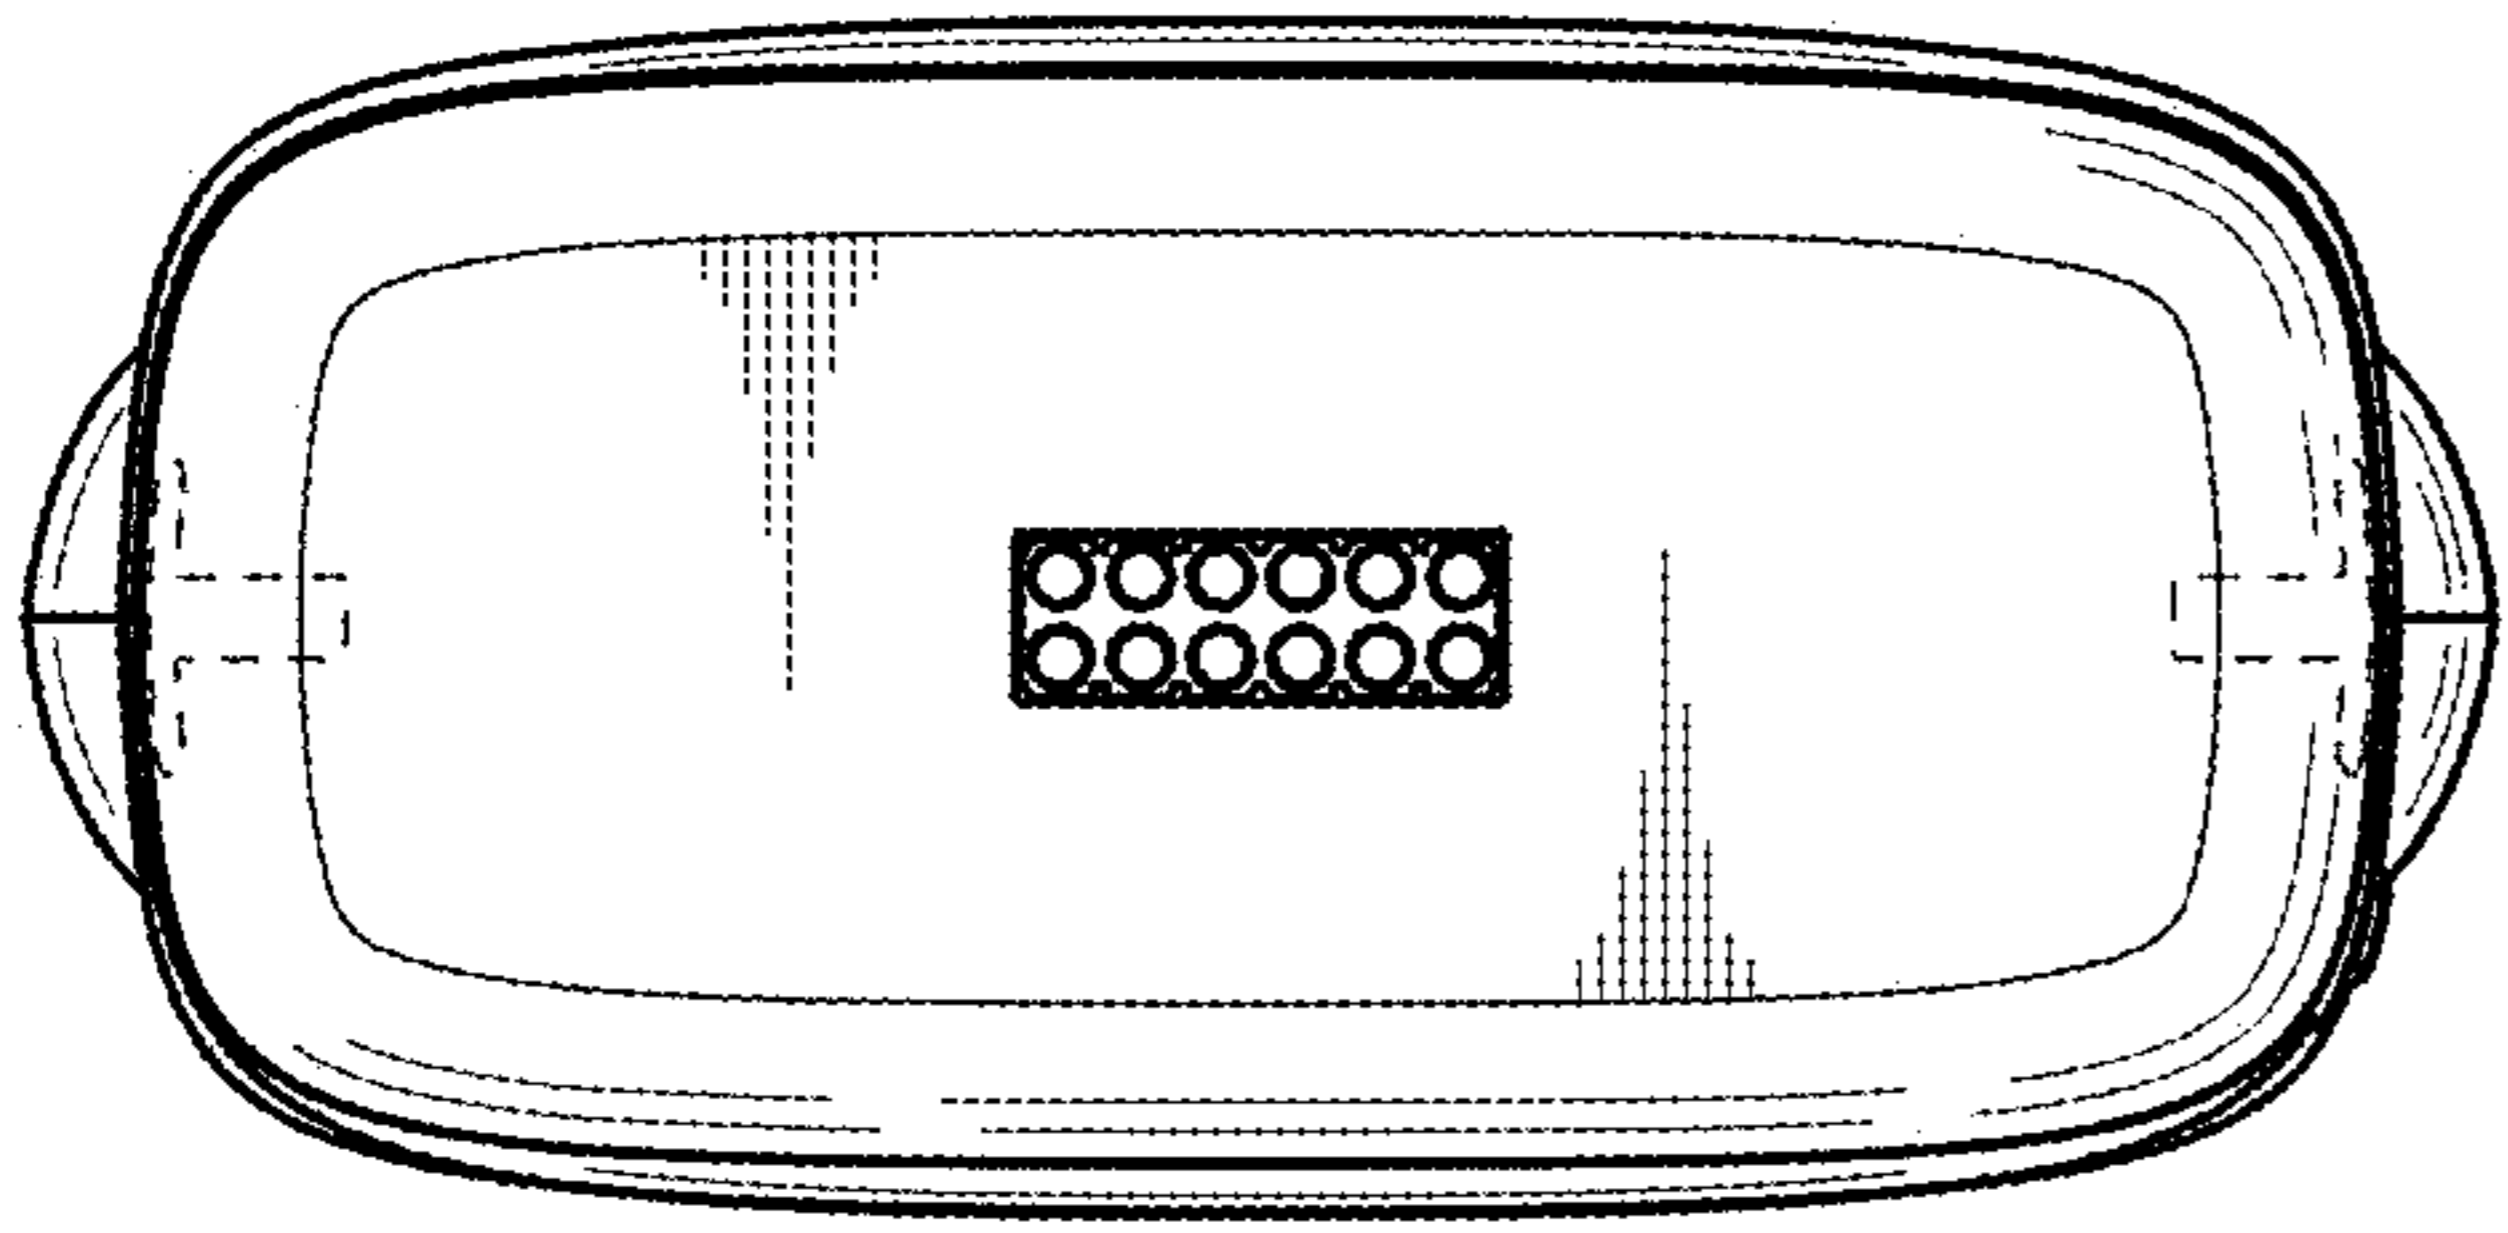

**FIG. 3**

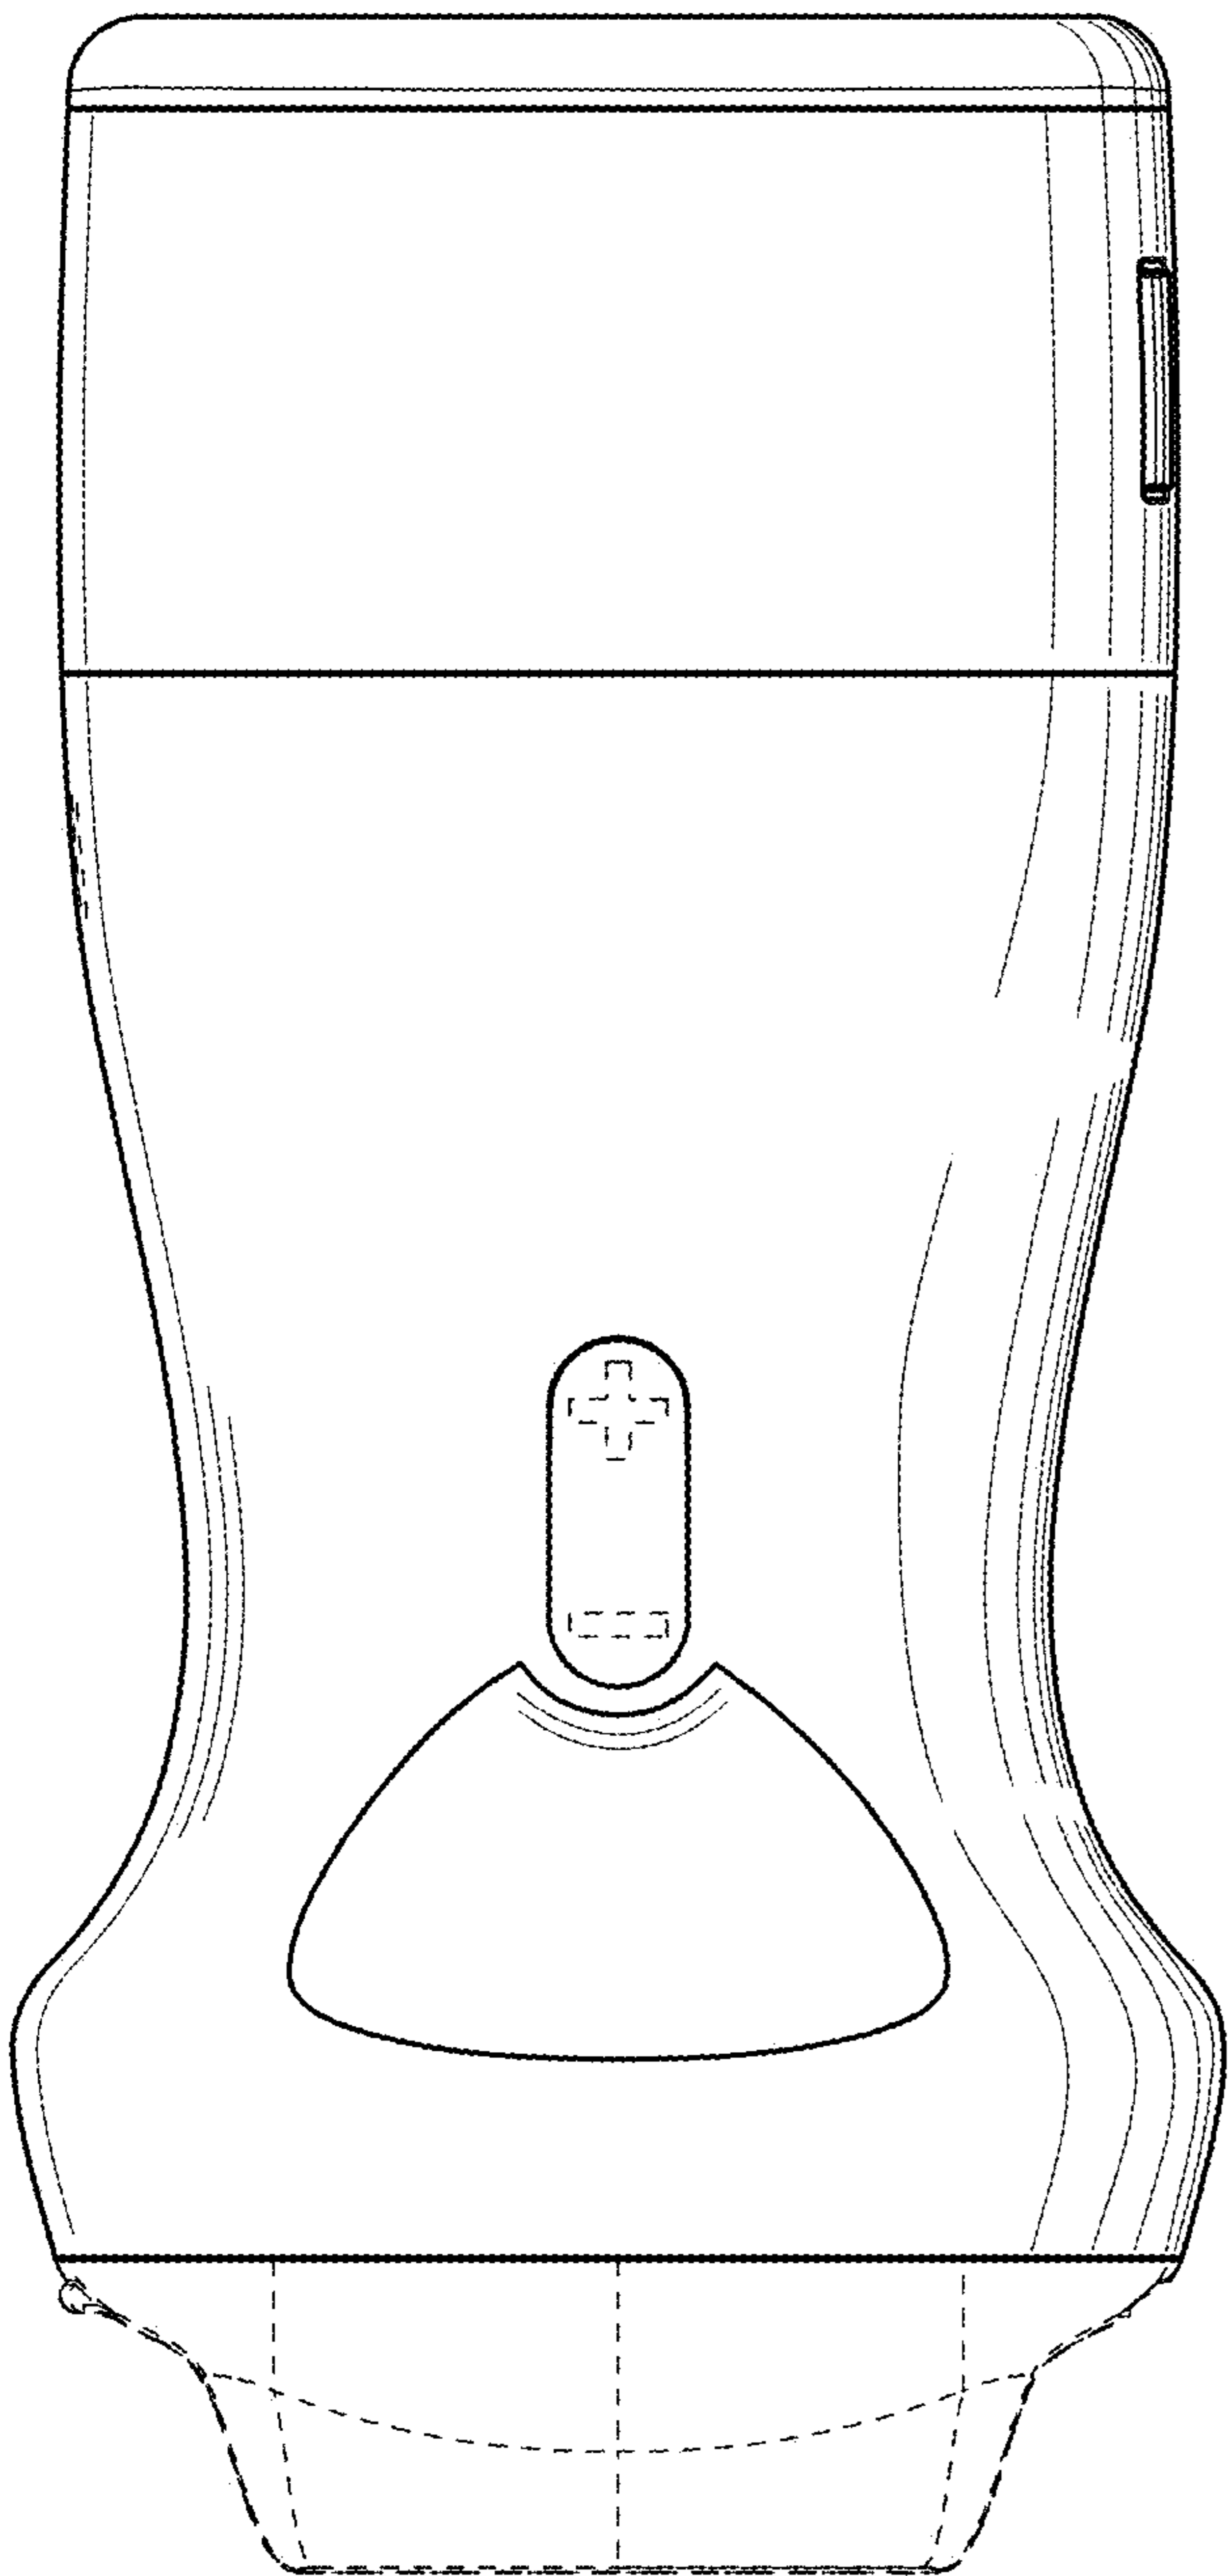

**FIG. 4**

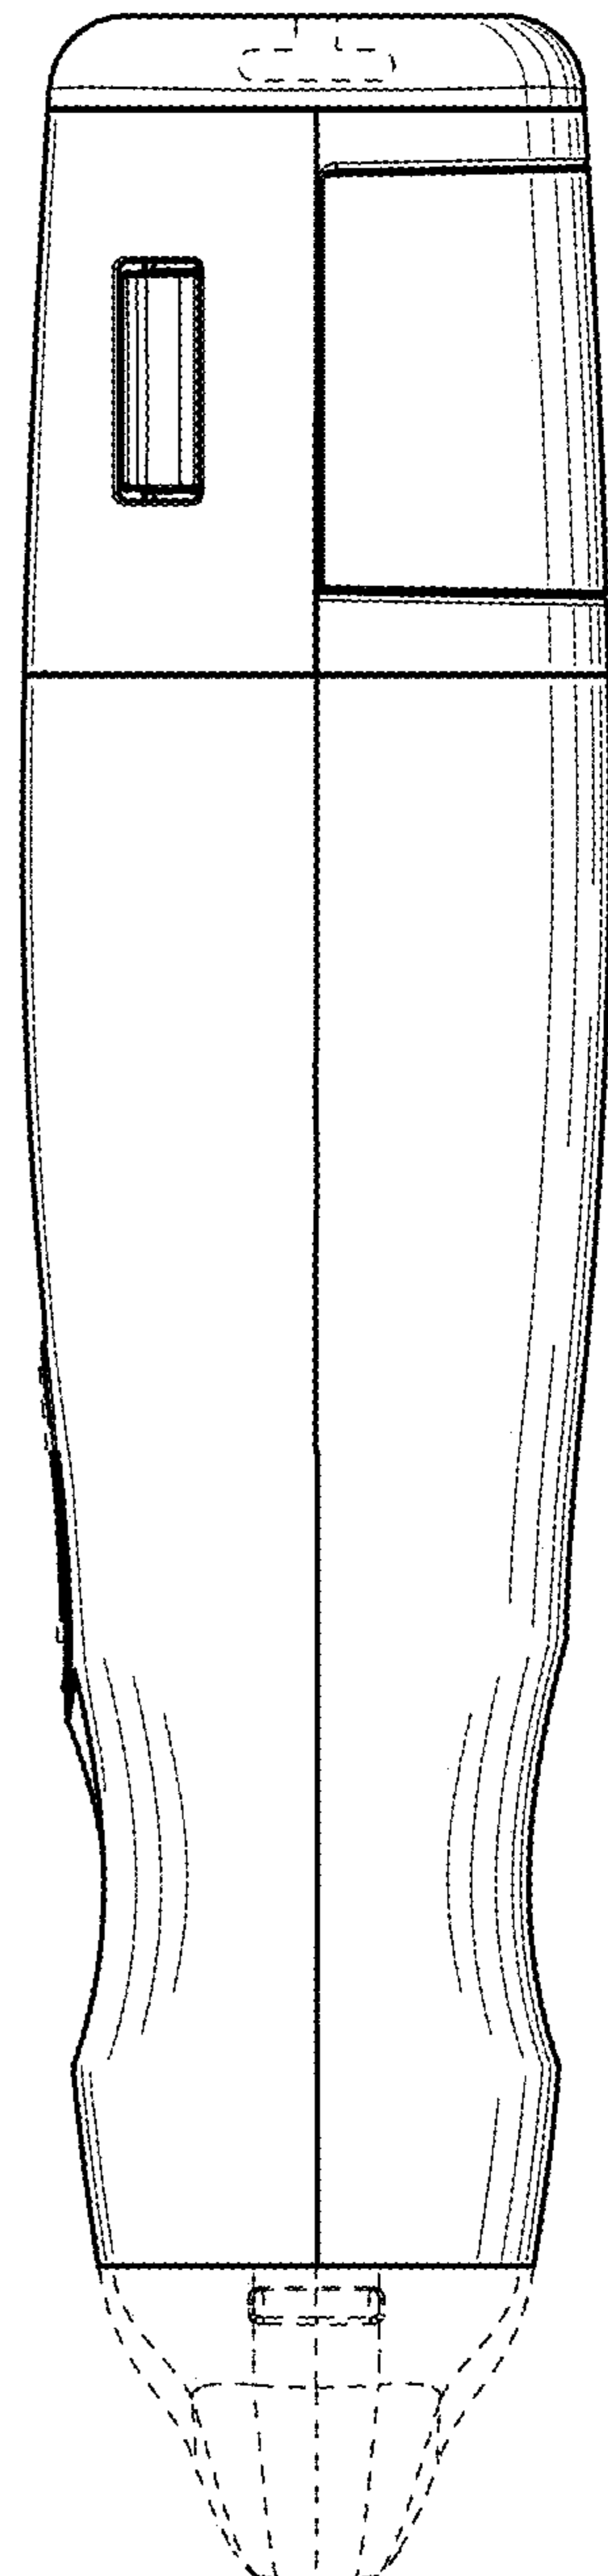

**FIG. 5**



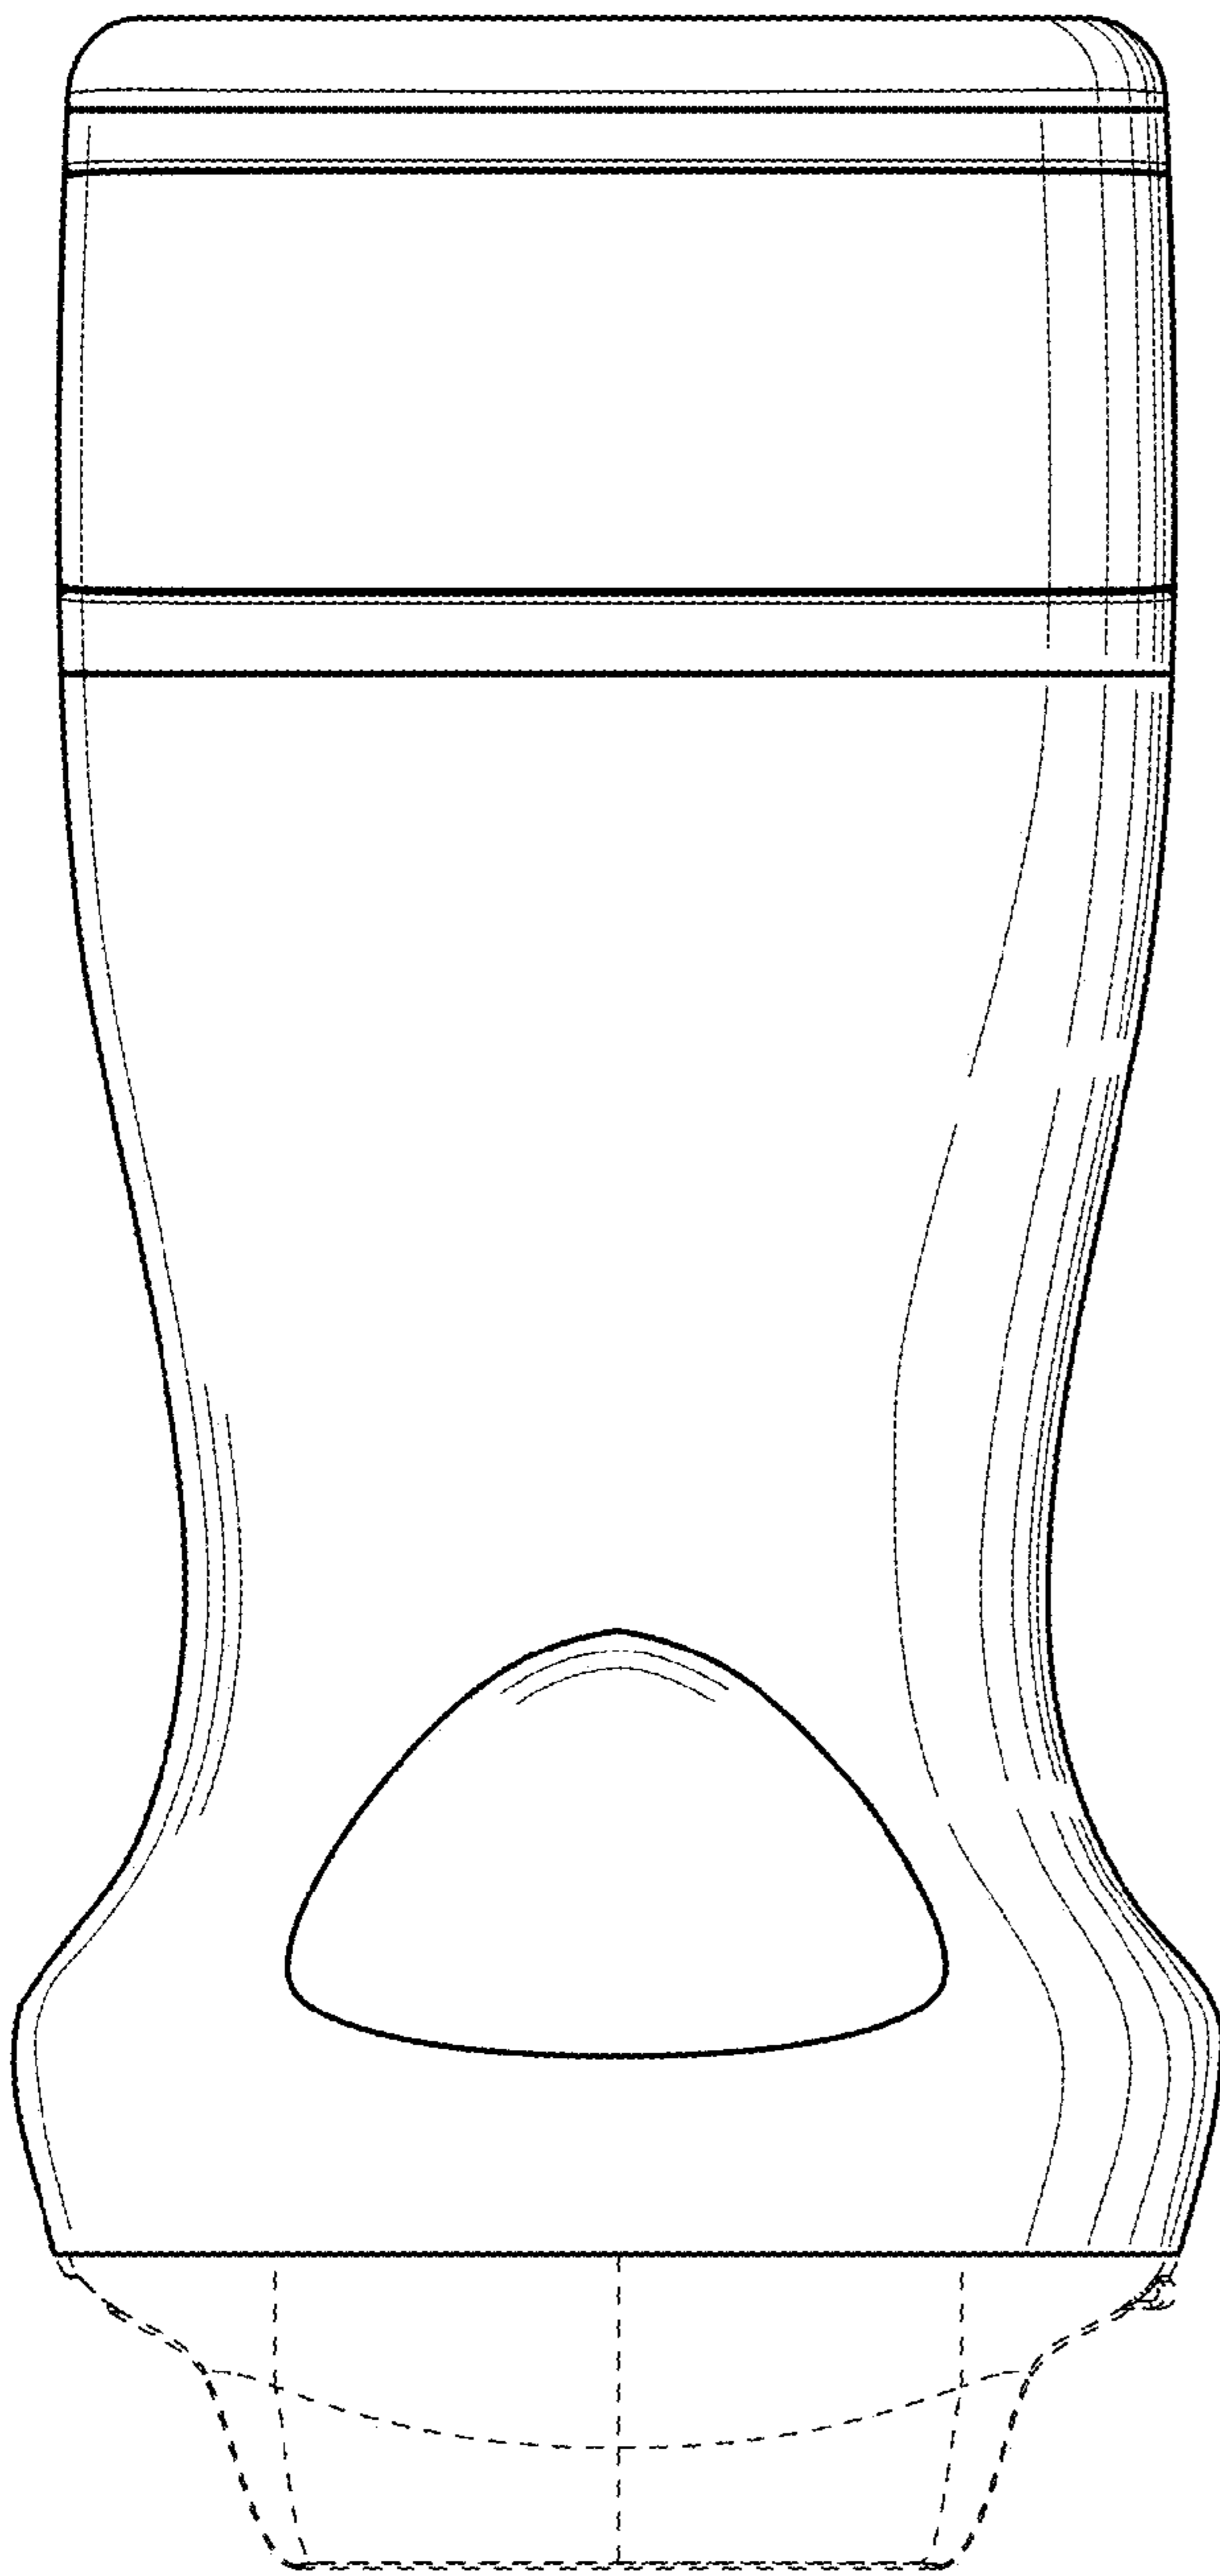


FIG. 7

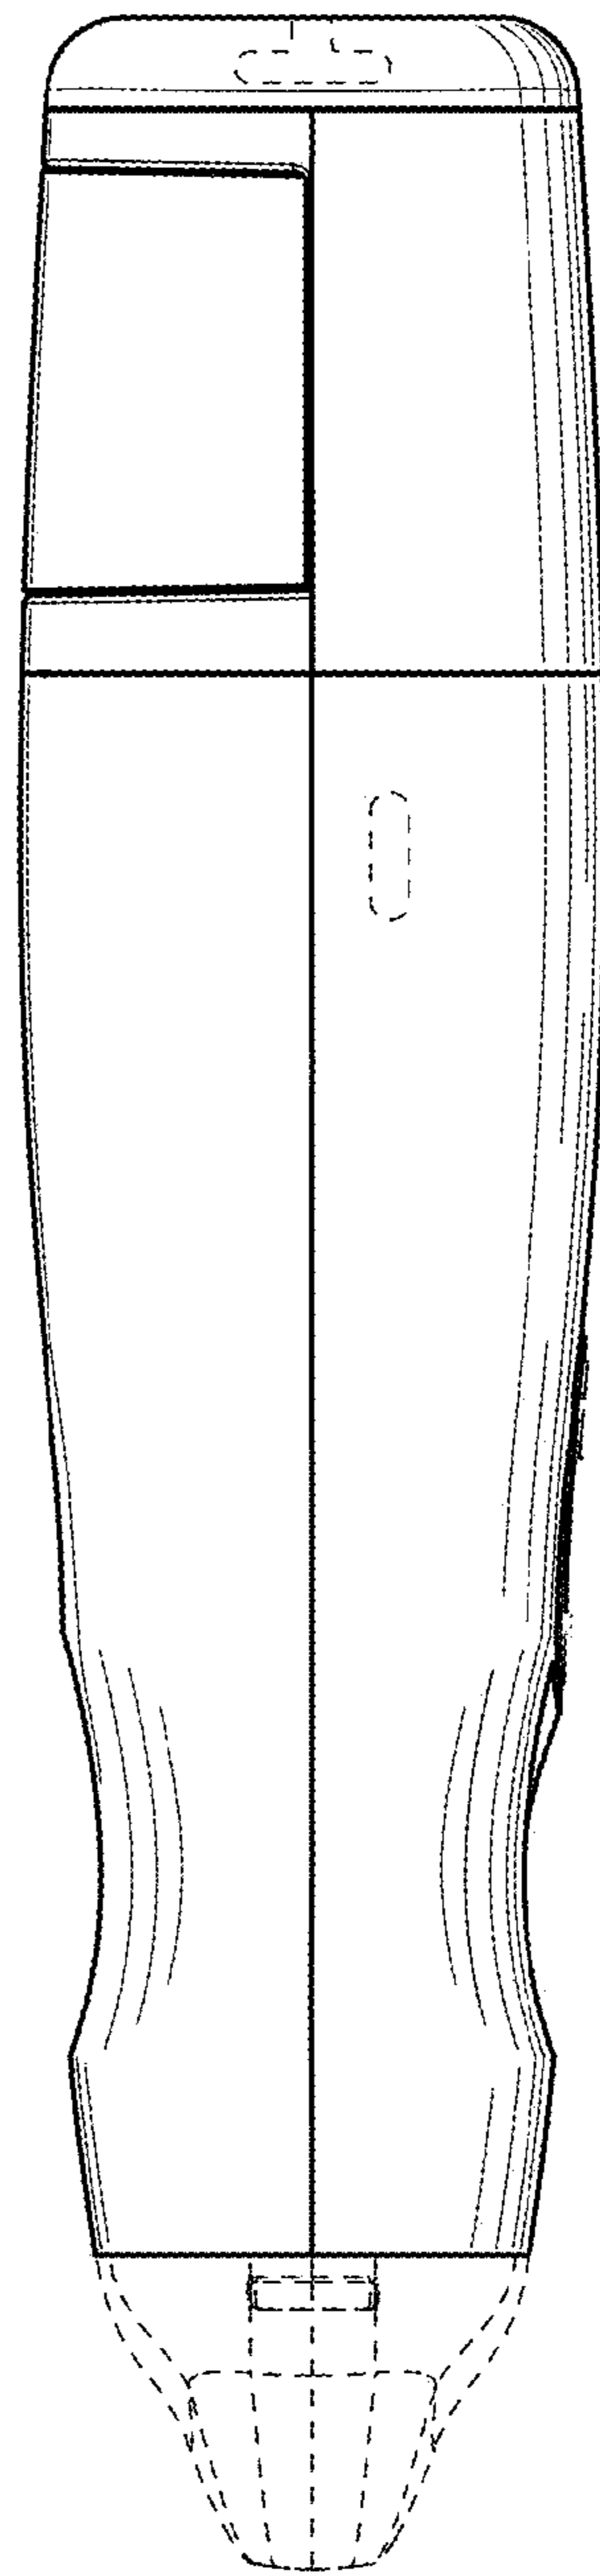


FIG. 6

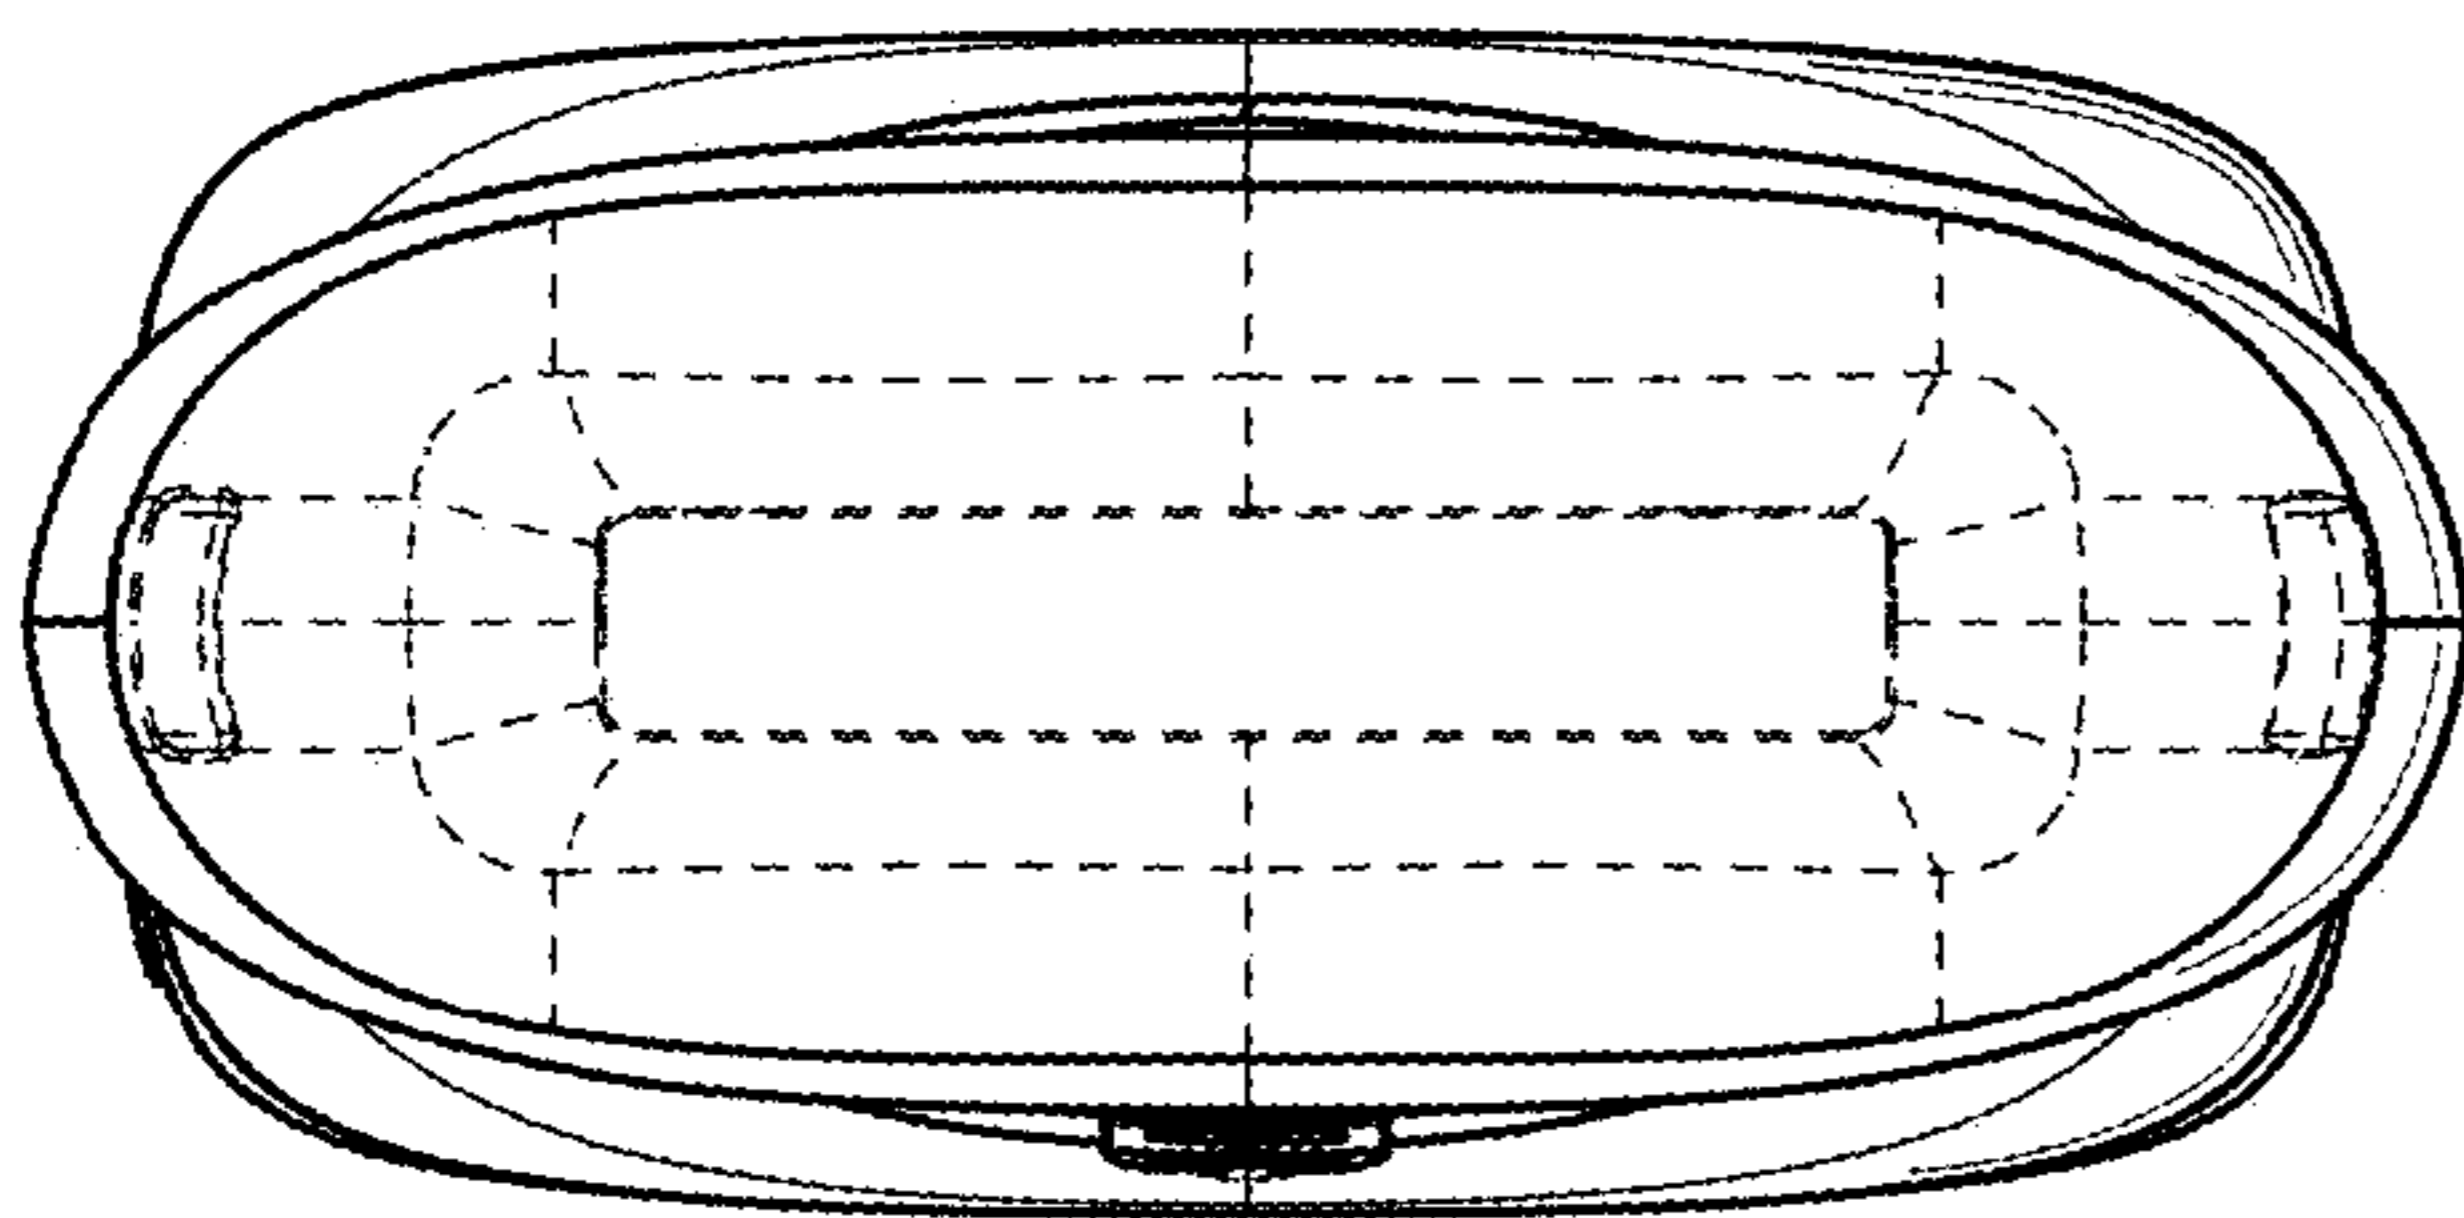


FIG. 8