



US00D878603S

(12) **United States Design Patent** (10) **Patent No.:** **US D878,603 S**
Zhang et al. (45) **Date of Patent:** **** Mar. 17, 2020**

(54) **ULTRASOUND SCANNER**
(71) Applicant: **Clarius Mobile Health Corp.**, Burnaby (CA)
(72) Inventors: **Binda Zhang**, Surrey (CA); **Alex Barcenas Antonio**, Burnaby (CA); **Daniel Christian Rahardja**, Burnaby (CA)
(73) Assignee: **Clarius Mobile Health Corp.**, Burnaby, British Columbia (CA)
(**) Term: **15 Years**
(21) Appl. No.: **29/668,362**
(22) Filed: **Oct. 30, 2018**
(51) **LOC (12) Cl.** **24-02**
(52) **U.S. Cl.**
USPC **D24/187**
(58) **Field of Classification Search**
USPC D24/133, 137, 138, 141, 158, 160, 164, D24/165, 167, 170, 186, 187, 200; D10/57, 60, 78, 80
CPC ... A61B 5/0095; A61B 8/4444; A61B 8/4455; G01S 7/5208
See application file for complete search history.

D831,219 S * 10/2018 Henderson D24/187
D842,482 S * 3/2019 Harada D24/187
D844,148 S * 3/2019 Wilson D24/187
D846,142 S * 4/2019 Yellen D24/217
D861,884 S * 10/2019 Moon D24/187
D862,710 S * 10/2019 Moon D24/187
D870,296 S * 12/2019 de Jonge D24/187
2014/0323869 A1 10/2014 Jin et al.

FOREIGN PATENT DOCUMENTS

JP D2018-28945 * 12/2019

OTHER PUBLICATIONS

Multipurpose Ultrasound Scanner. Online, published date unknown. Retrieved on Dec. 29, 2019 from URL: <https://clarius.com/scanners/c3/>.*

(Continued)

Primary Examiner — Susan Bennett Hattan
Assistant Examiner — Omeed Agilee
(74) *Attorney, Agent, or Firm* — Julian Ho

(57) **CLAIM**

The ornamental design of an ultrasound scanner, substantially as shown and described.


DESCRIPTION

FIG. 1 is a front perspective view of an ultrasound scanner in accordance with the present design; FIG. 2 is a rear perspective view thereof; FIG. 3 is a top view thereof; FIG. 4 is a front view thereof; FIG. 5 is a right side view thereof; FIG. 6 is a left side view thereof; FIG. 7 is a rear view thereof; and, FIG. 8 is a bottom view thereof. The broken lines in the figures represent portions of the article which form no part of the claimed design.

1 Claim, 4 Drawing Sheets

(56) **References Cited**
U.S. PATENT DOCUMENTS

D392,044 S * 3/1998 Mesaros D24/186
6,780,154 B2 8/2004 Hunt et al.
D555,252 S * 11/2007 Kitayama D24/186
D667,557 S * 9/2012 Boudier D24/186
D704,341 S * 5/2014 Ryu D24/187
D745,972 S * 12/2015 Kitayama D24/187
D763,452 S * 8/2016 Ryu D24/187
D811,607 S * 2/2018 Kitayama D24/187
D816,850 S * 5/2018 Asai D24/187
D822,837 S * 7/2018 Naka D24/187

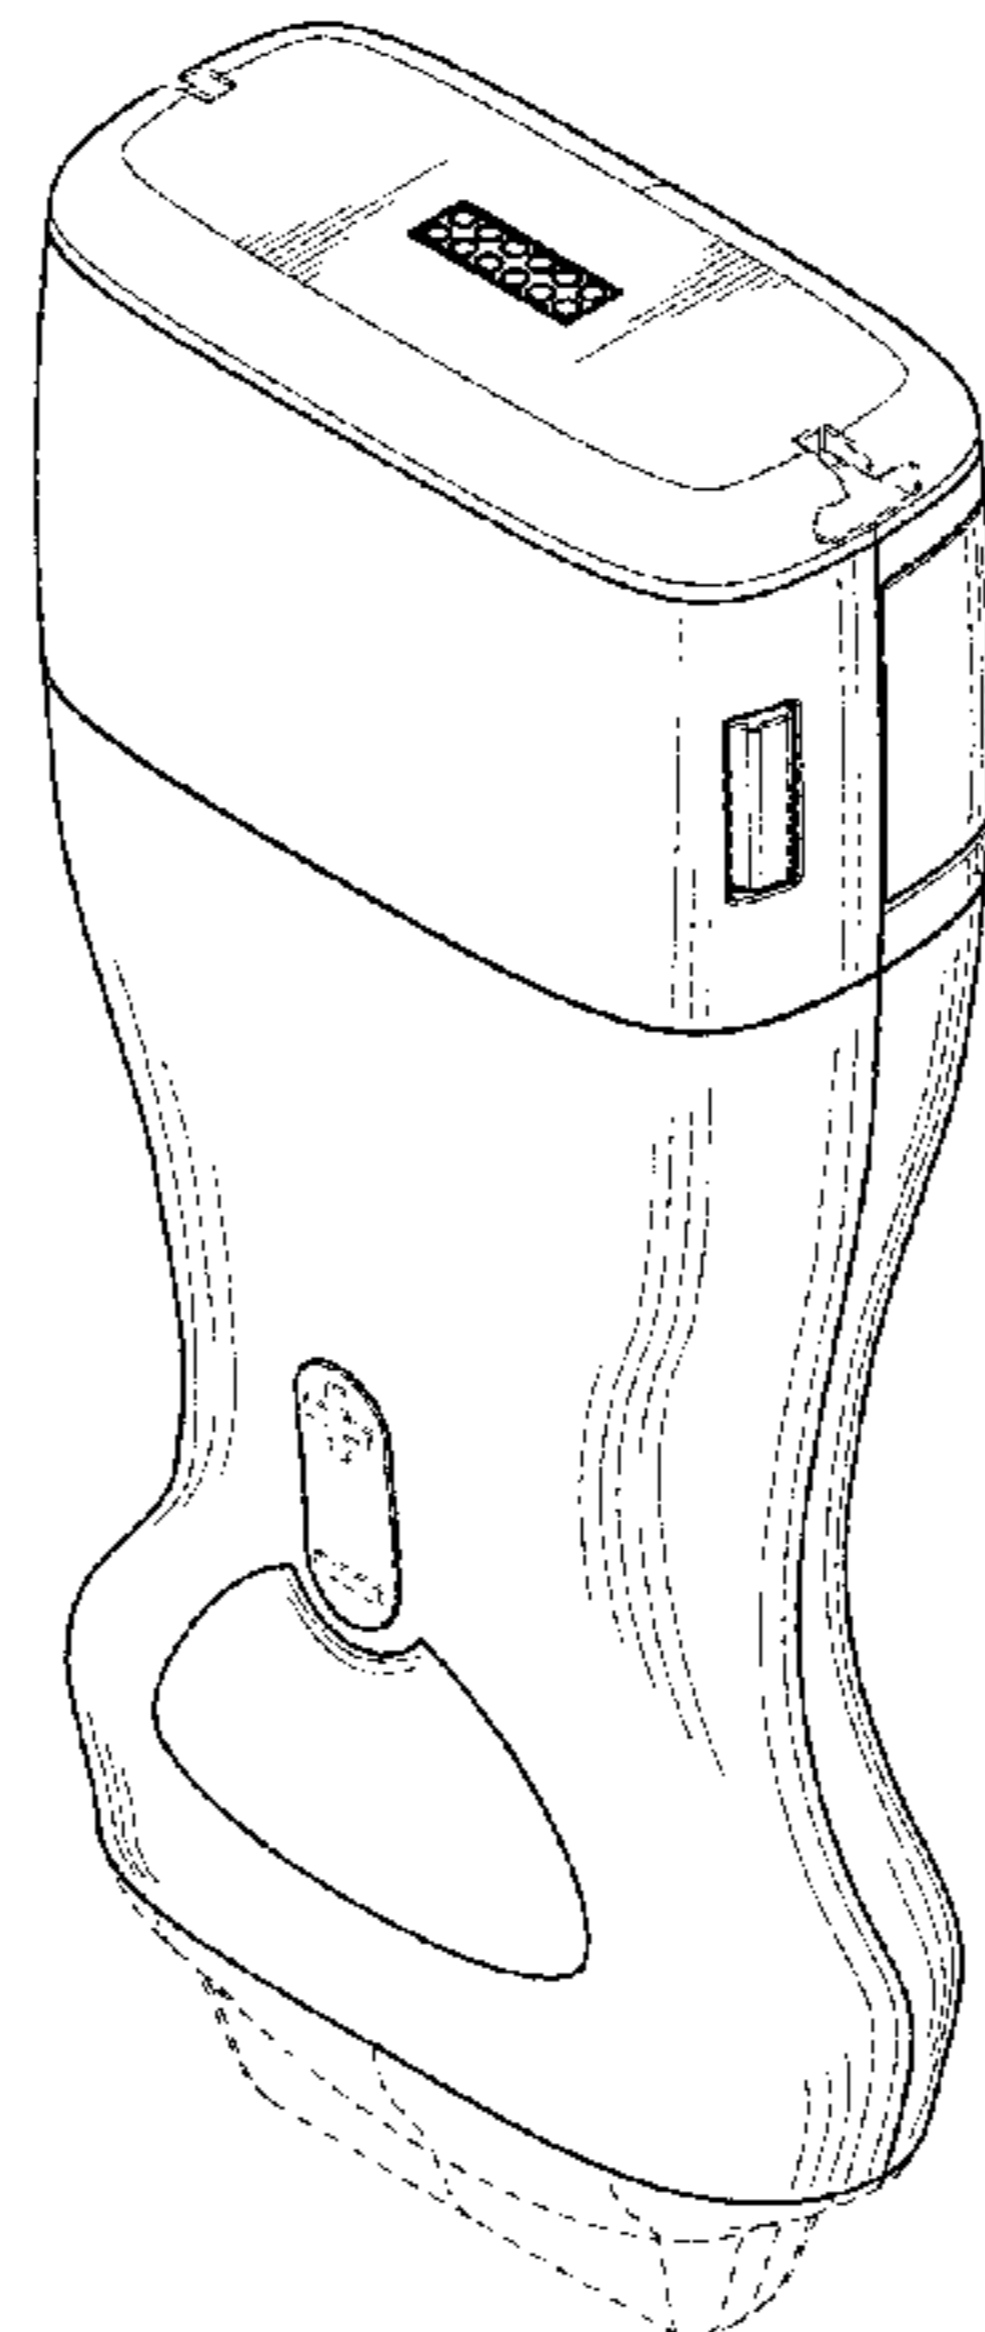

(56)

References Cited

OTHER PUBLICATIONS

Wireless for greater ultrasound efficiency. Online, published date unknown. Retrieved on Dec. 29, 2019 from URL: <https://mides.com/en/wireless-probe/>.*

Sonostar, "UProbe-2/UProbe-3 Series (Convex and Linear) Array Ultrasound Probe Scanner", publication date unknown, available online: <http://sonostar.net/EnProductShow.asp?ID=310>, last accessed Nov. 13, 2018.

Healcerion, "Sonon 300L", publication date unknown, available online: <https://www.healcerion.com/products/ultrasounds/>, last accessed Nov. 13, 2018.

* cited by examiner

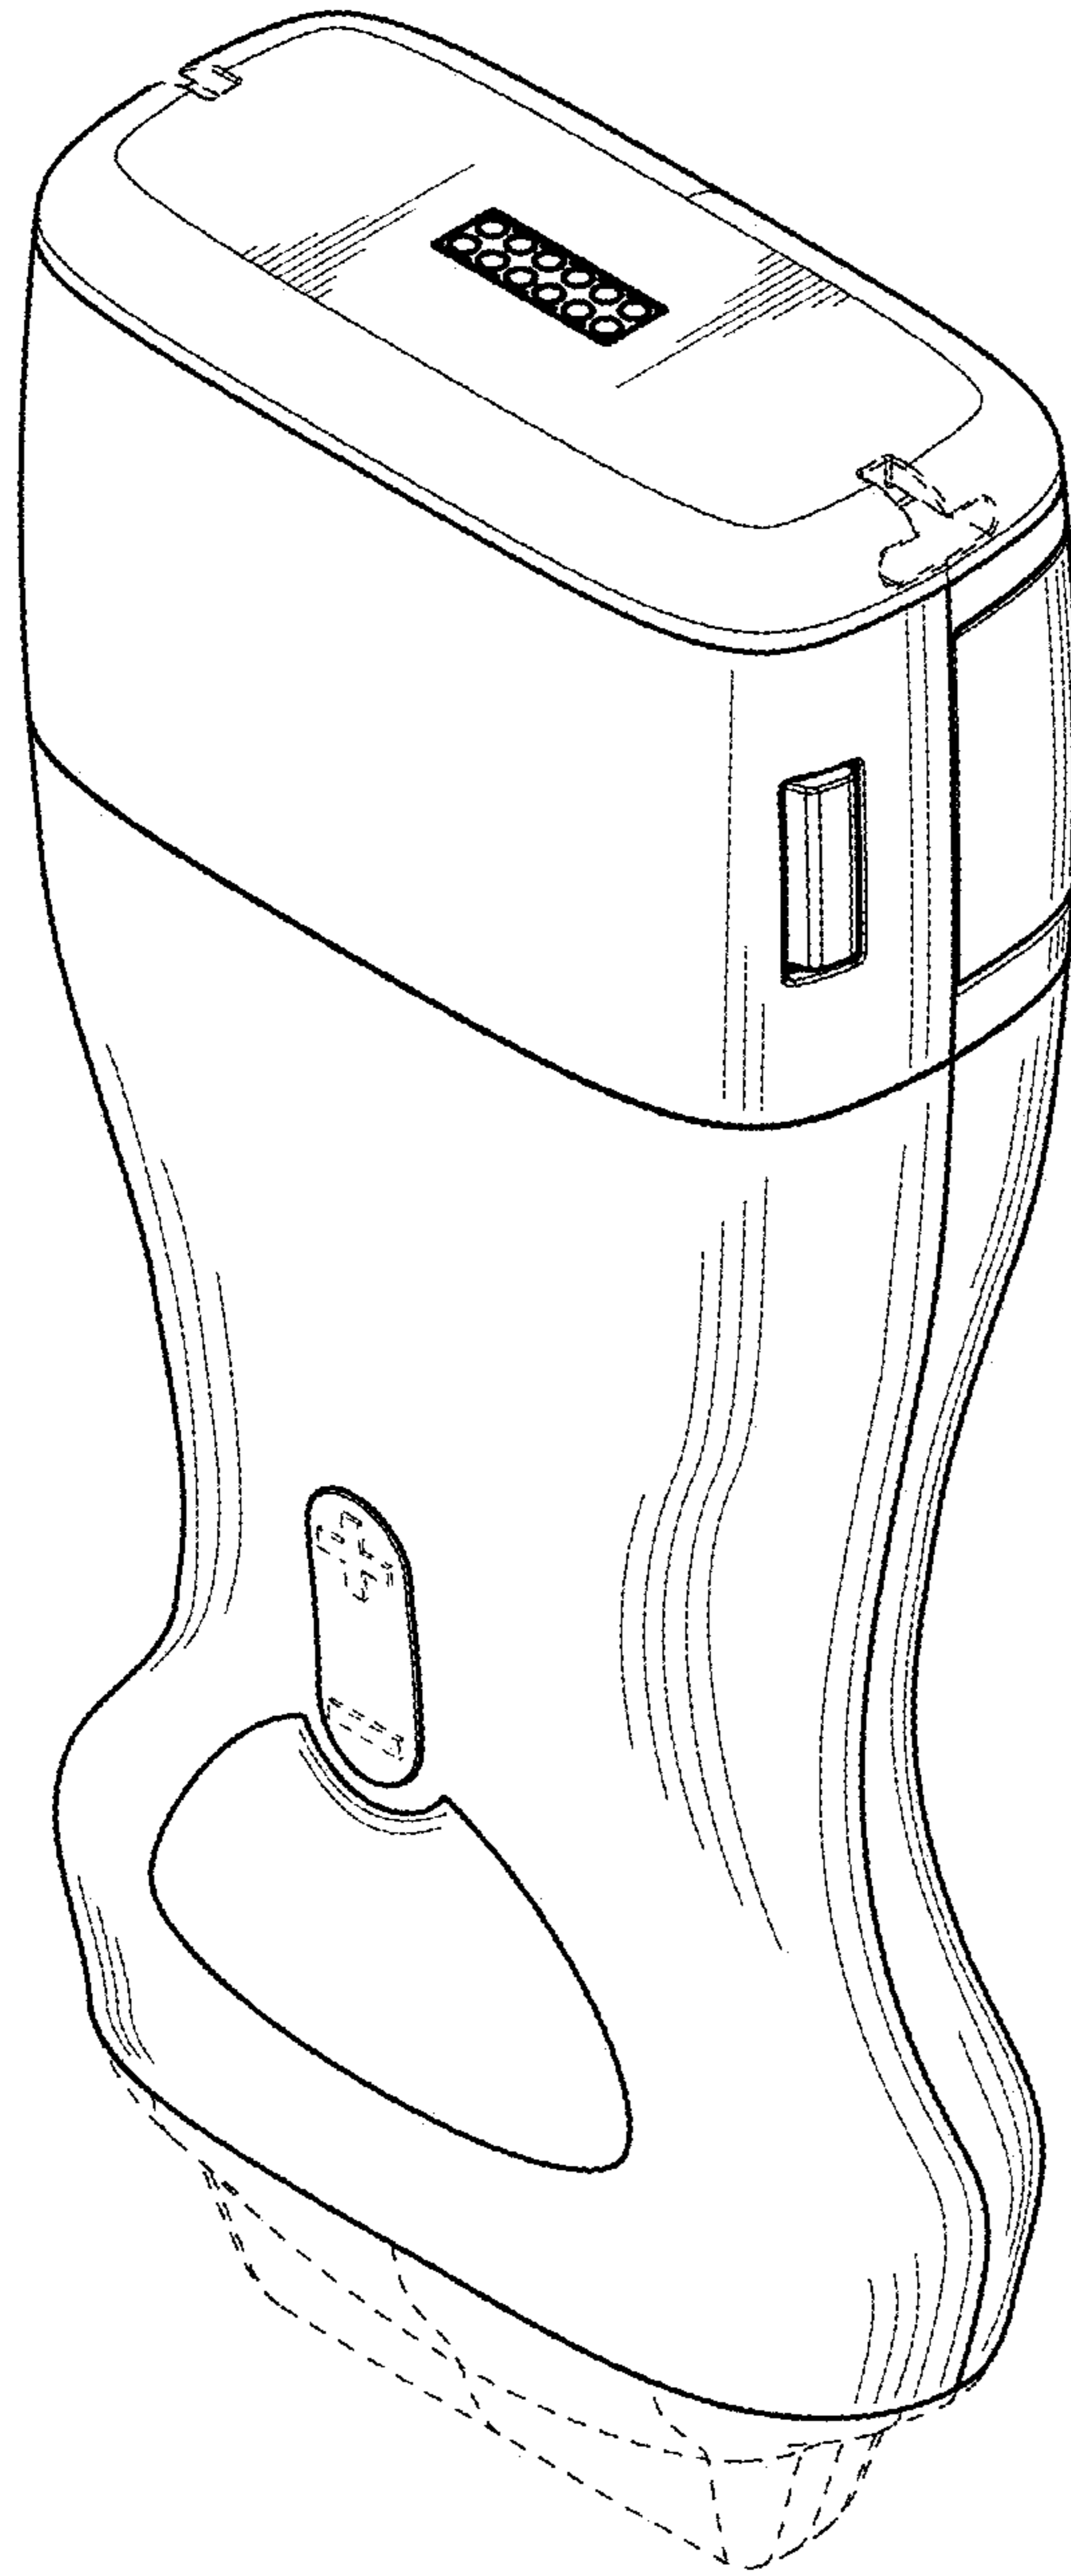


FIG. 1

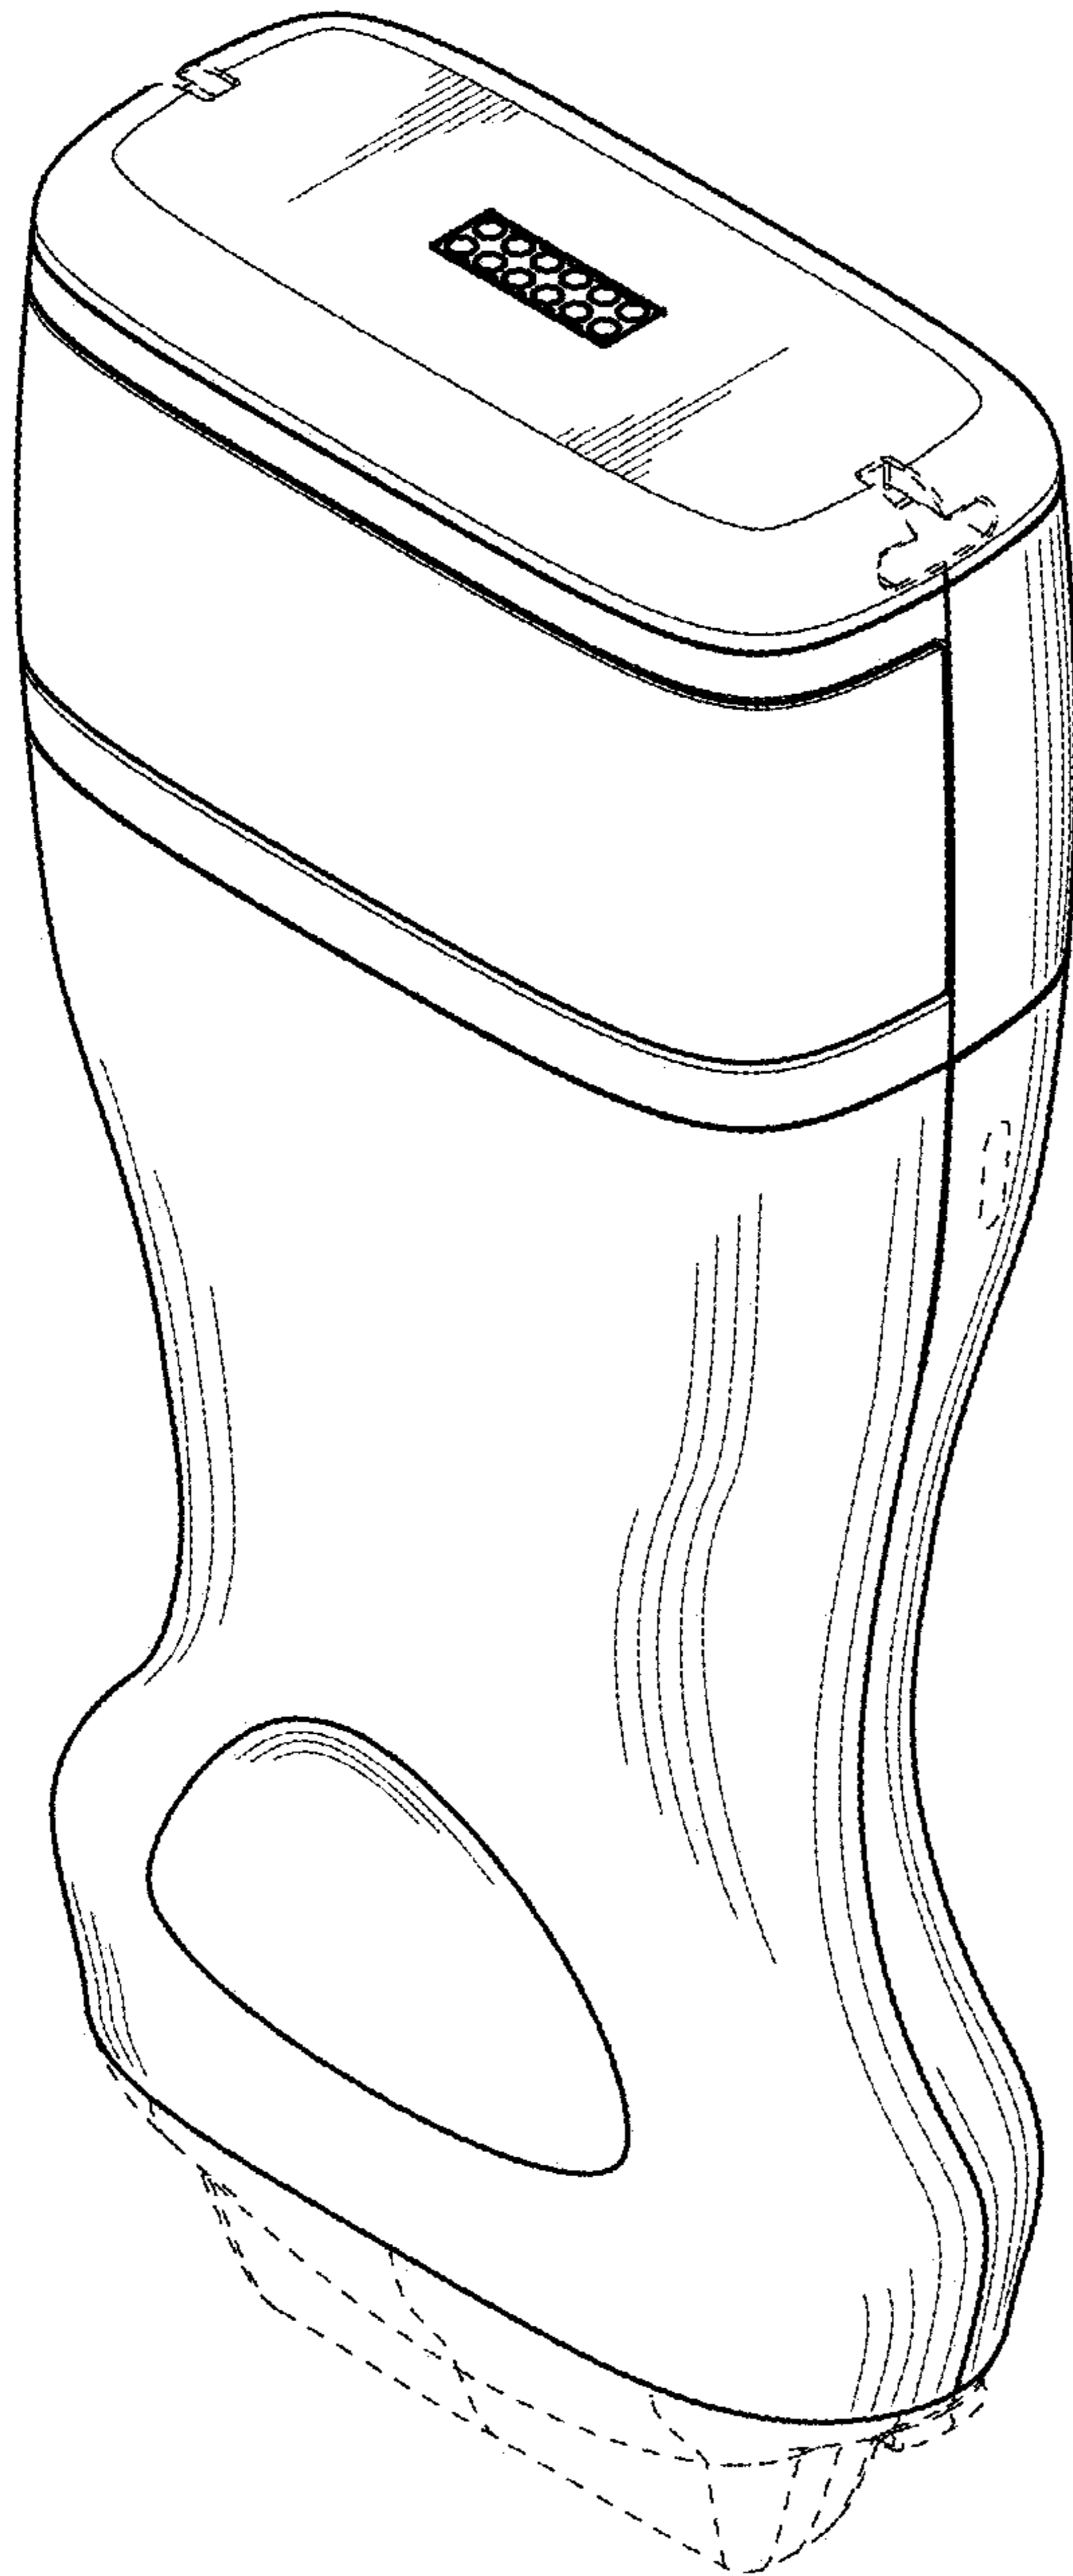


FIG. 2

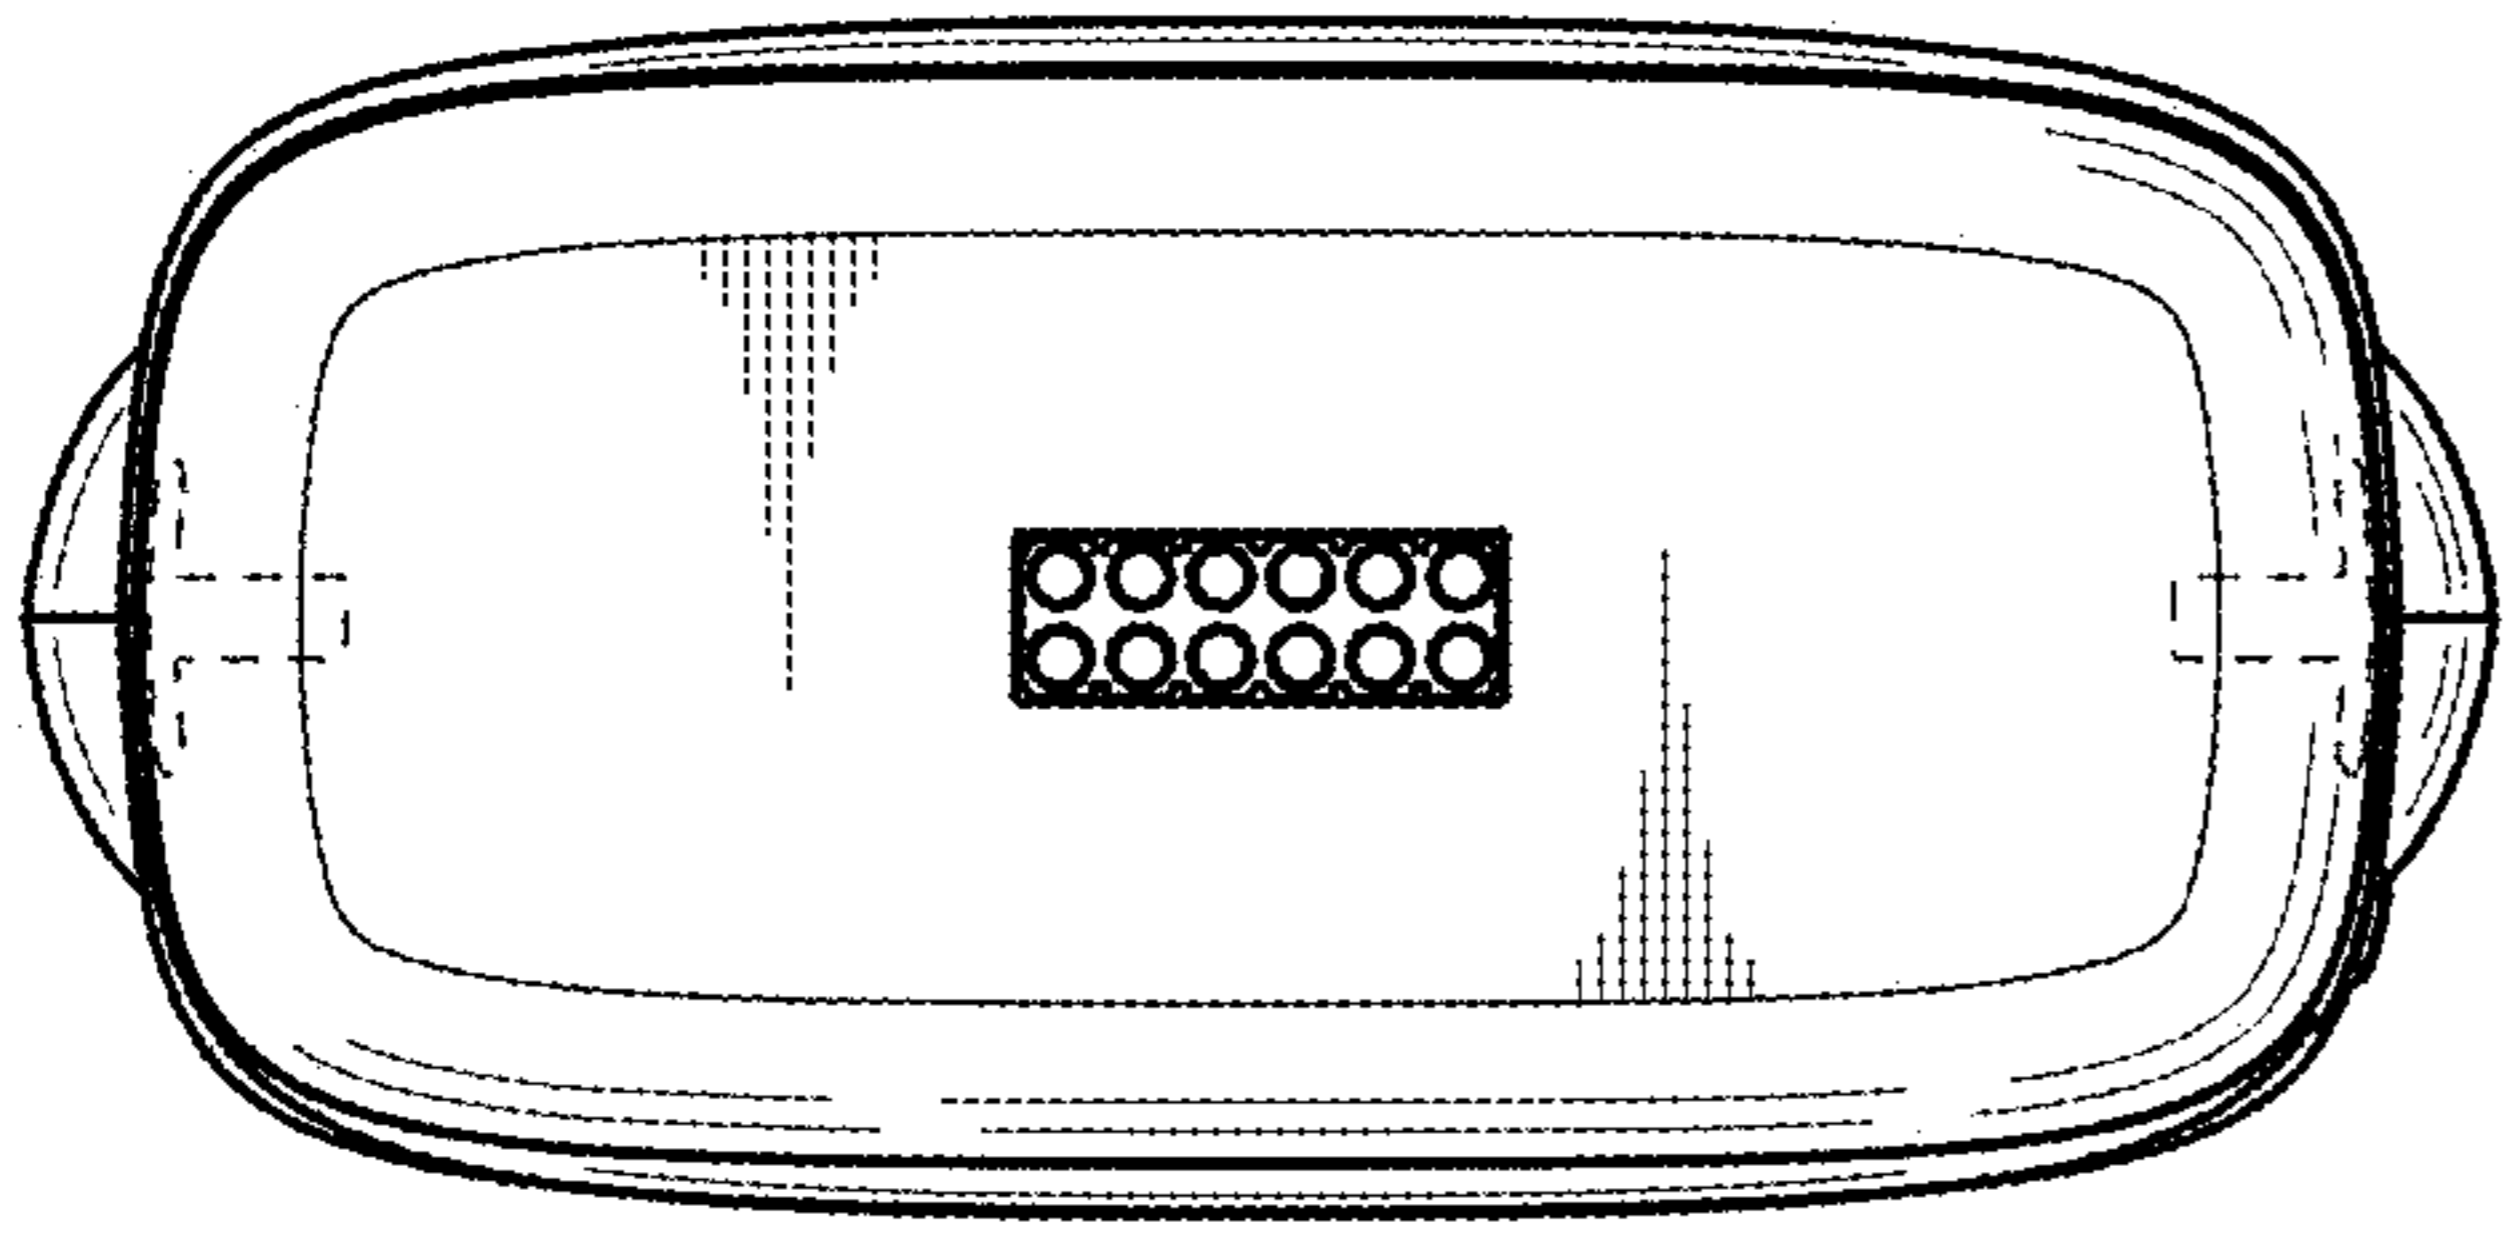


FIG. 3

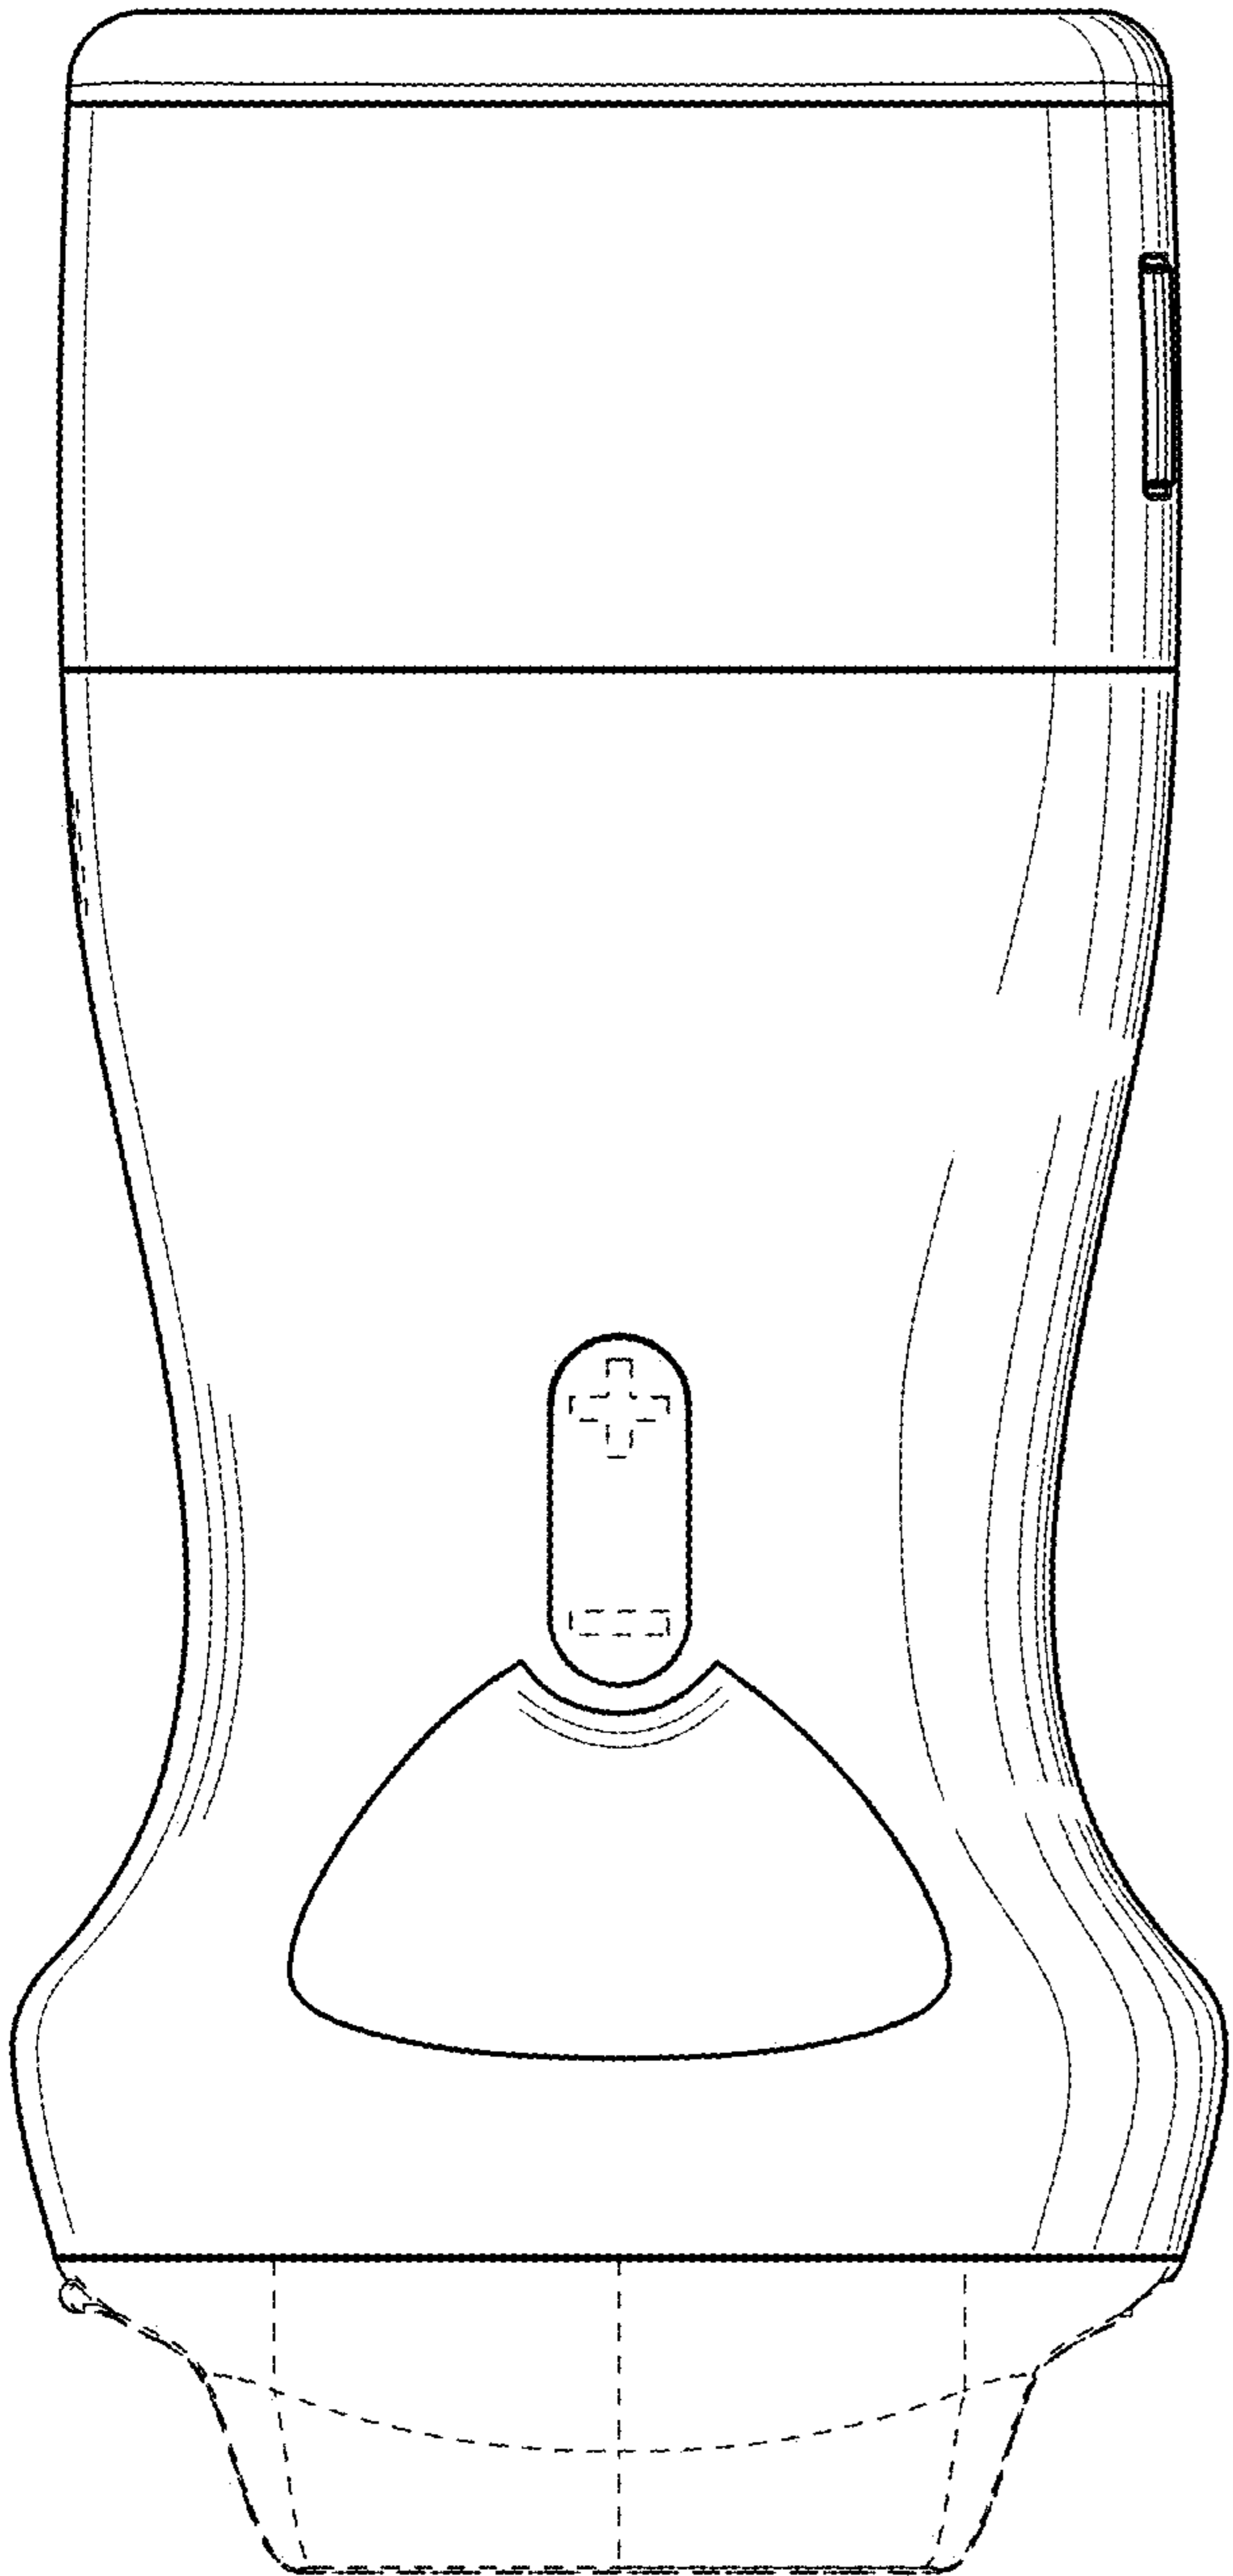


FIG. 4

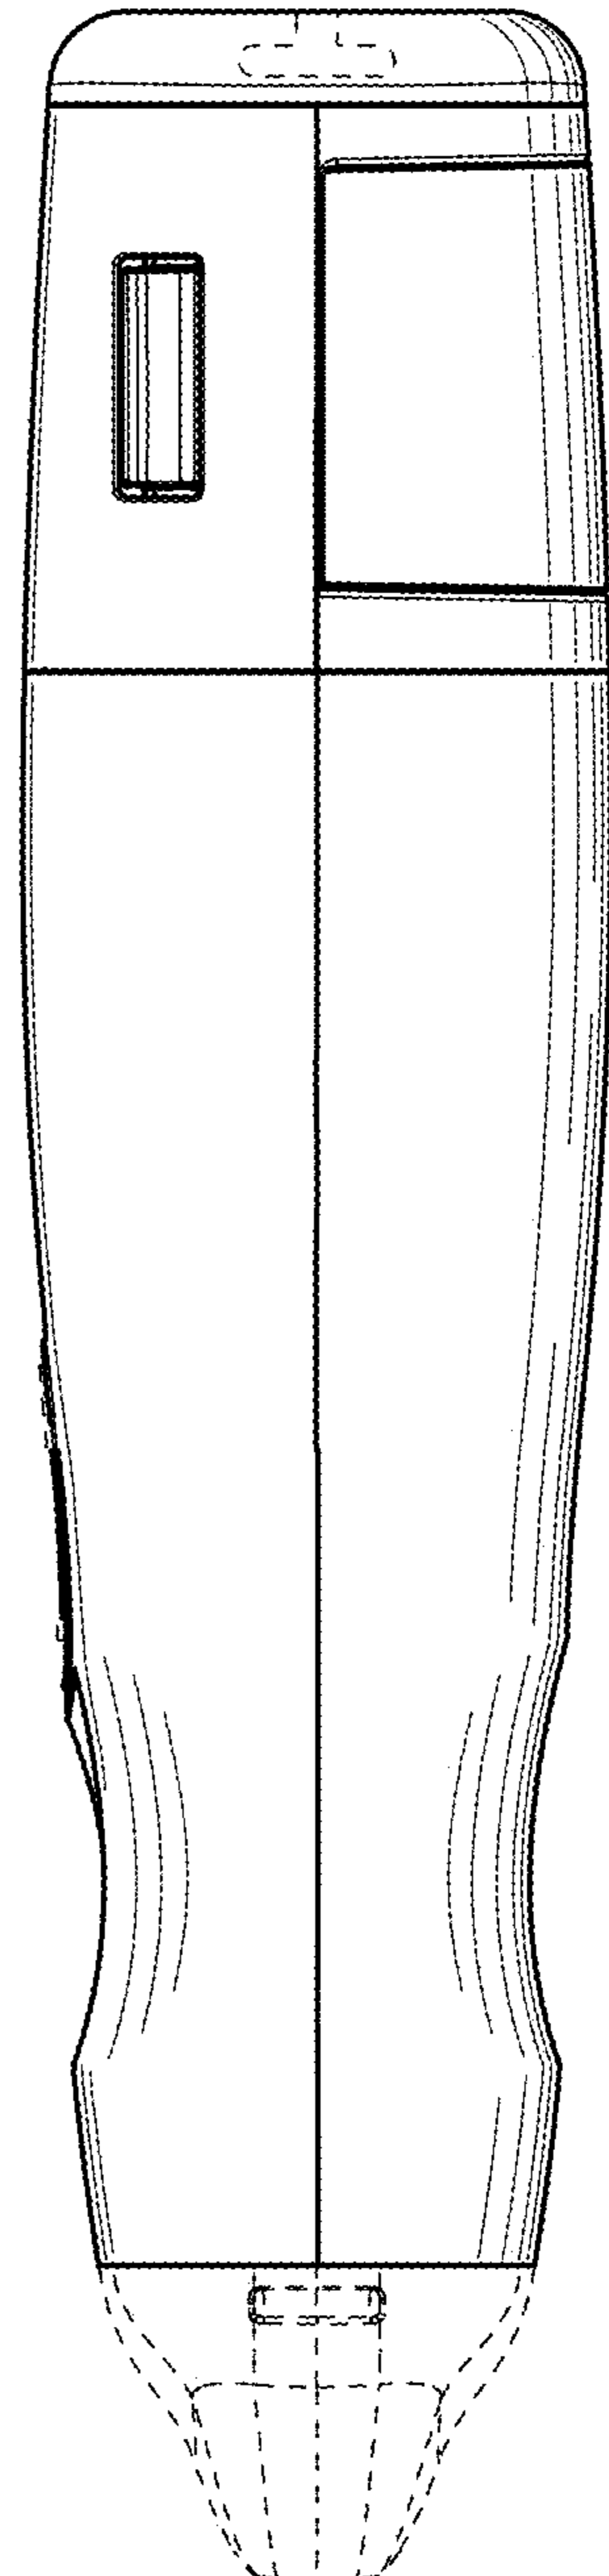


FIG. 5

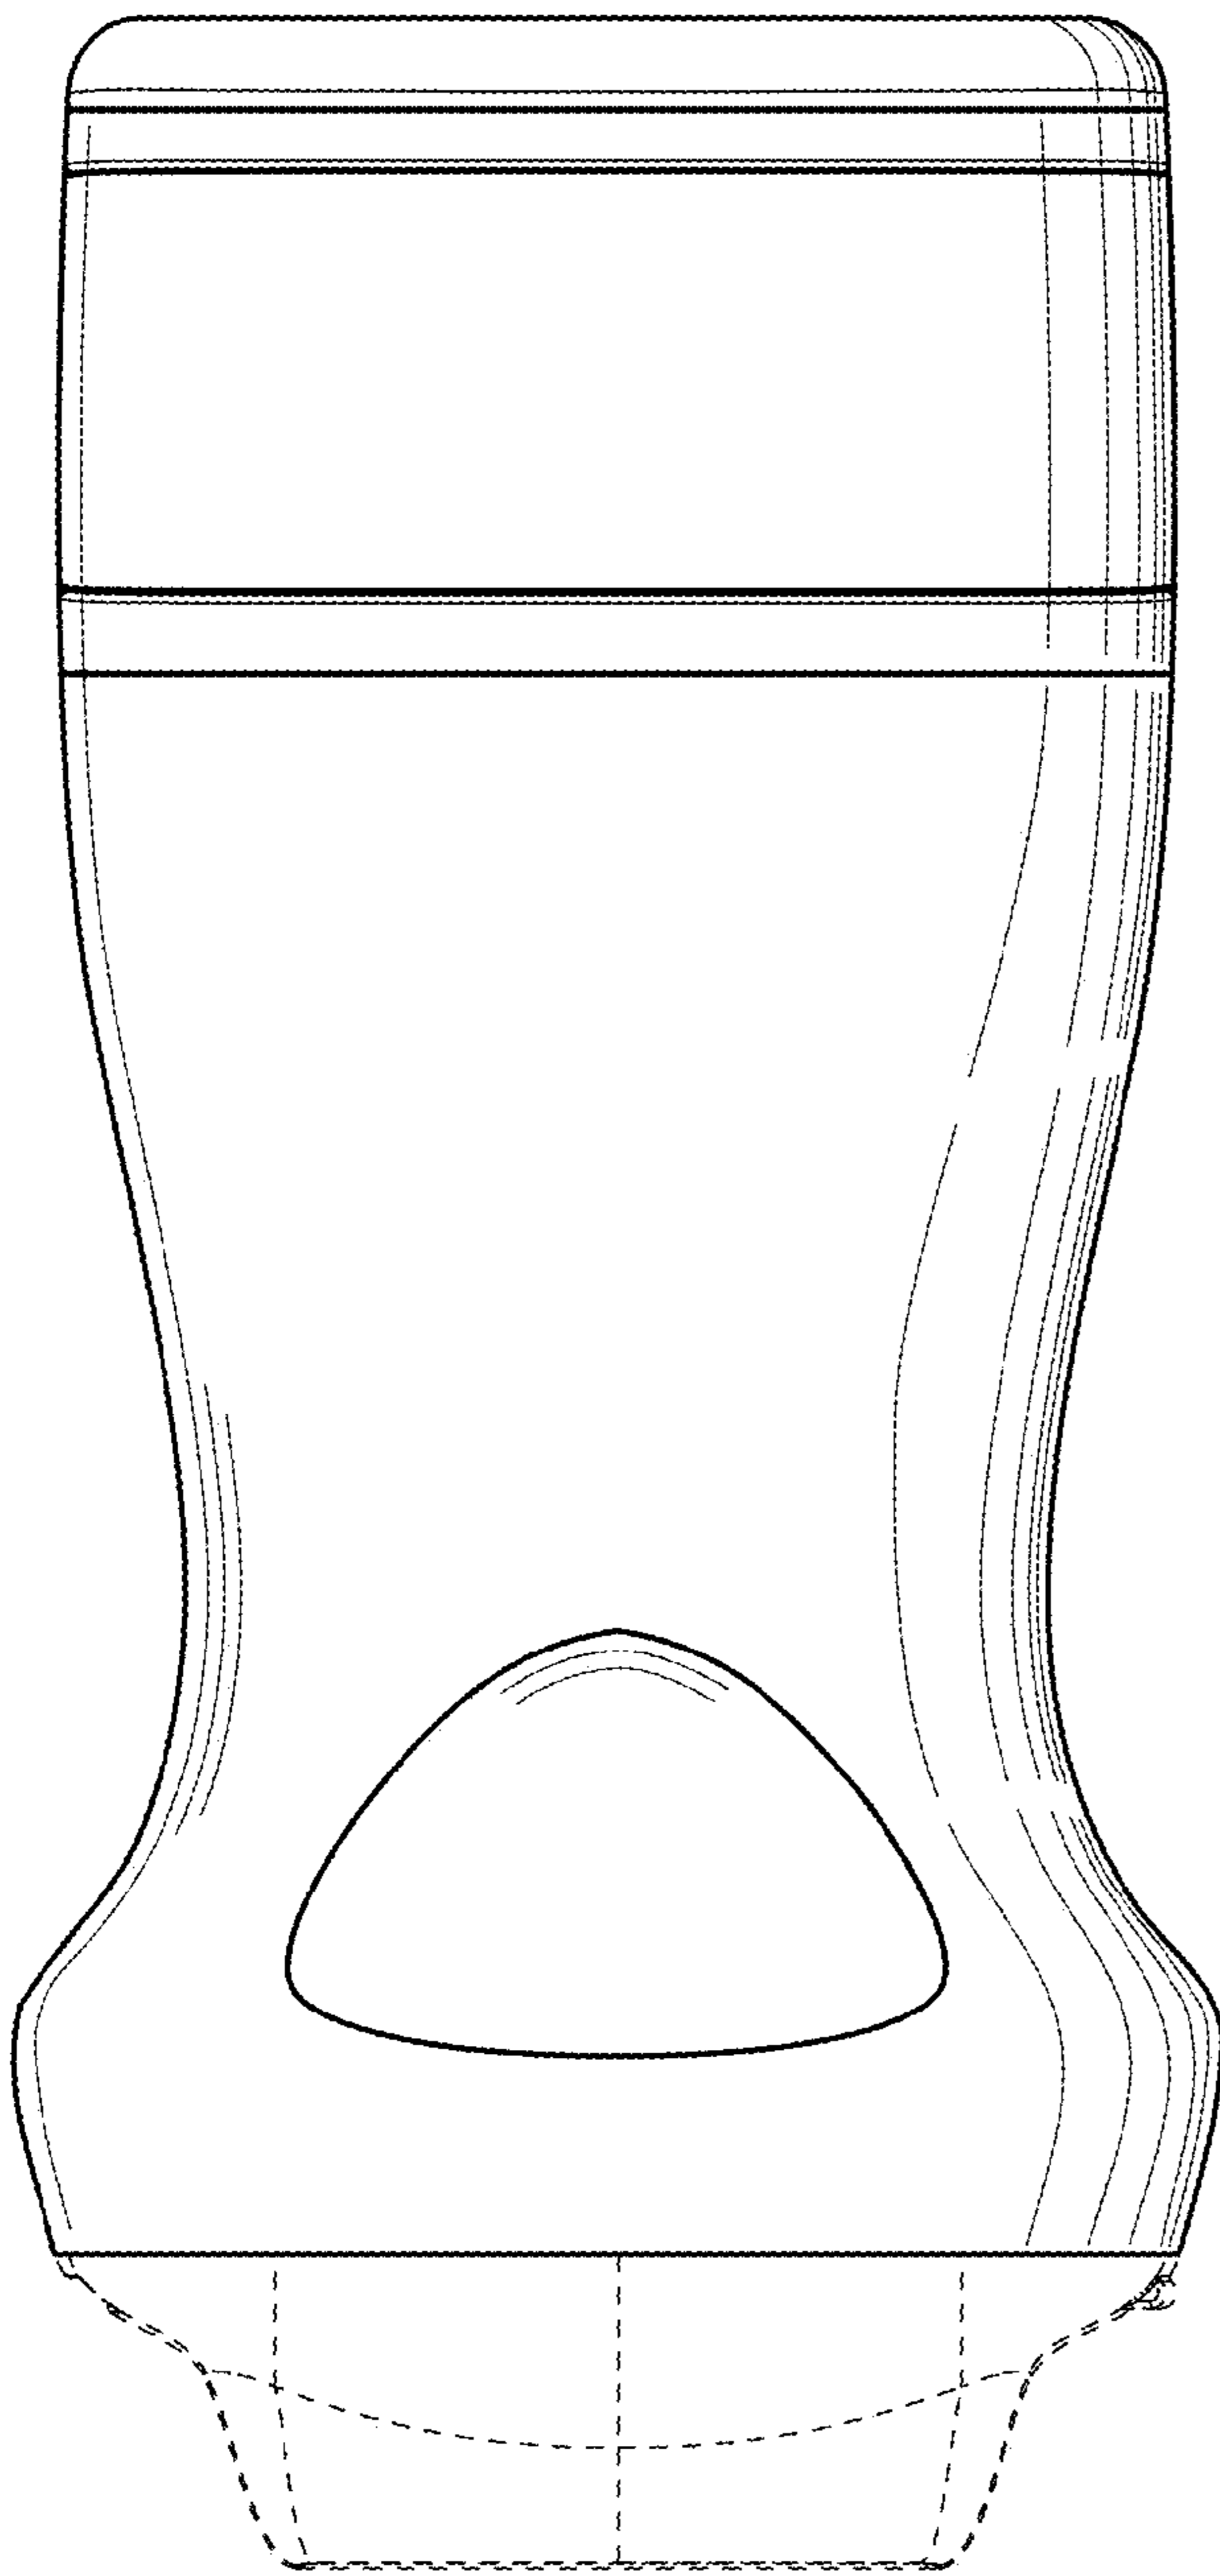


FIG. 7

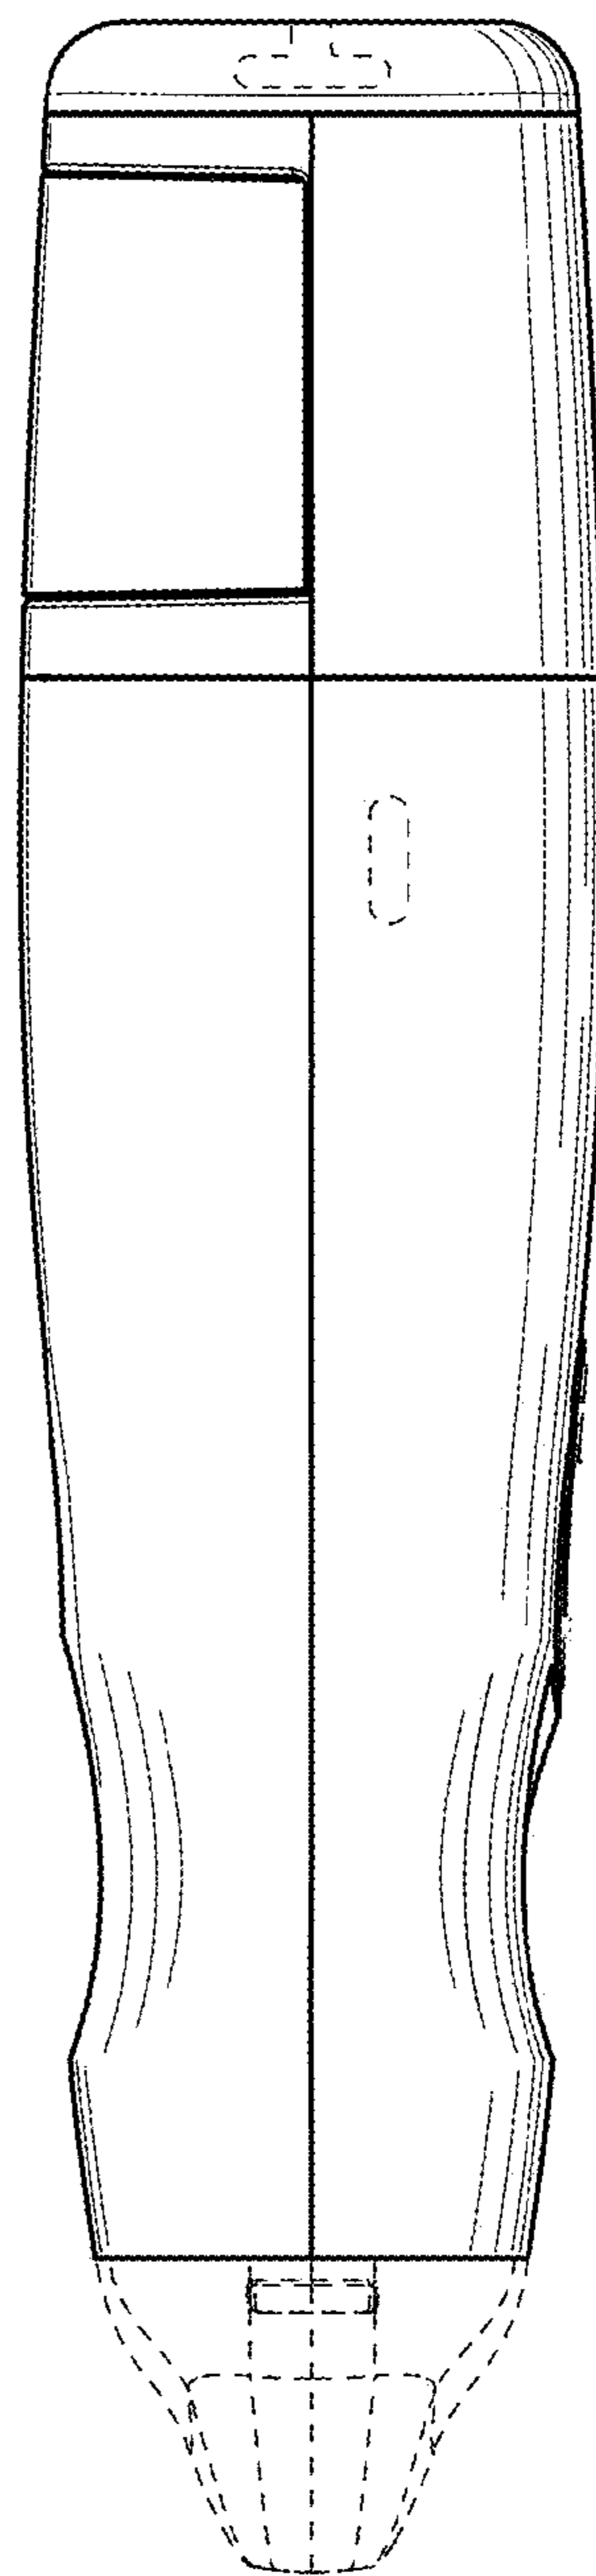


FIG. 6

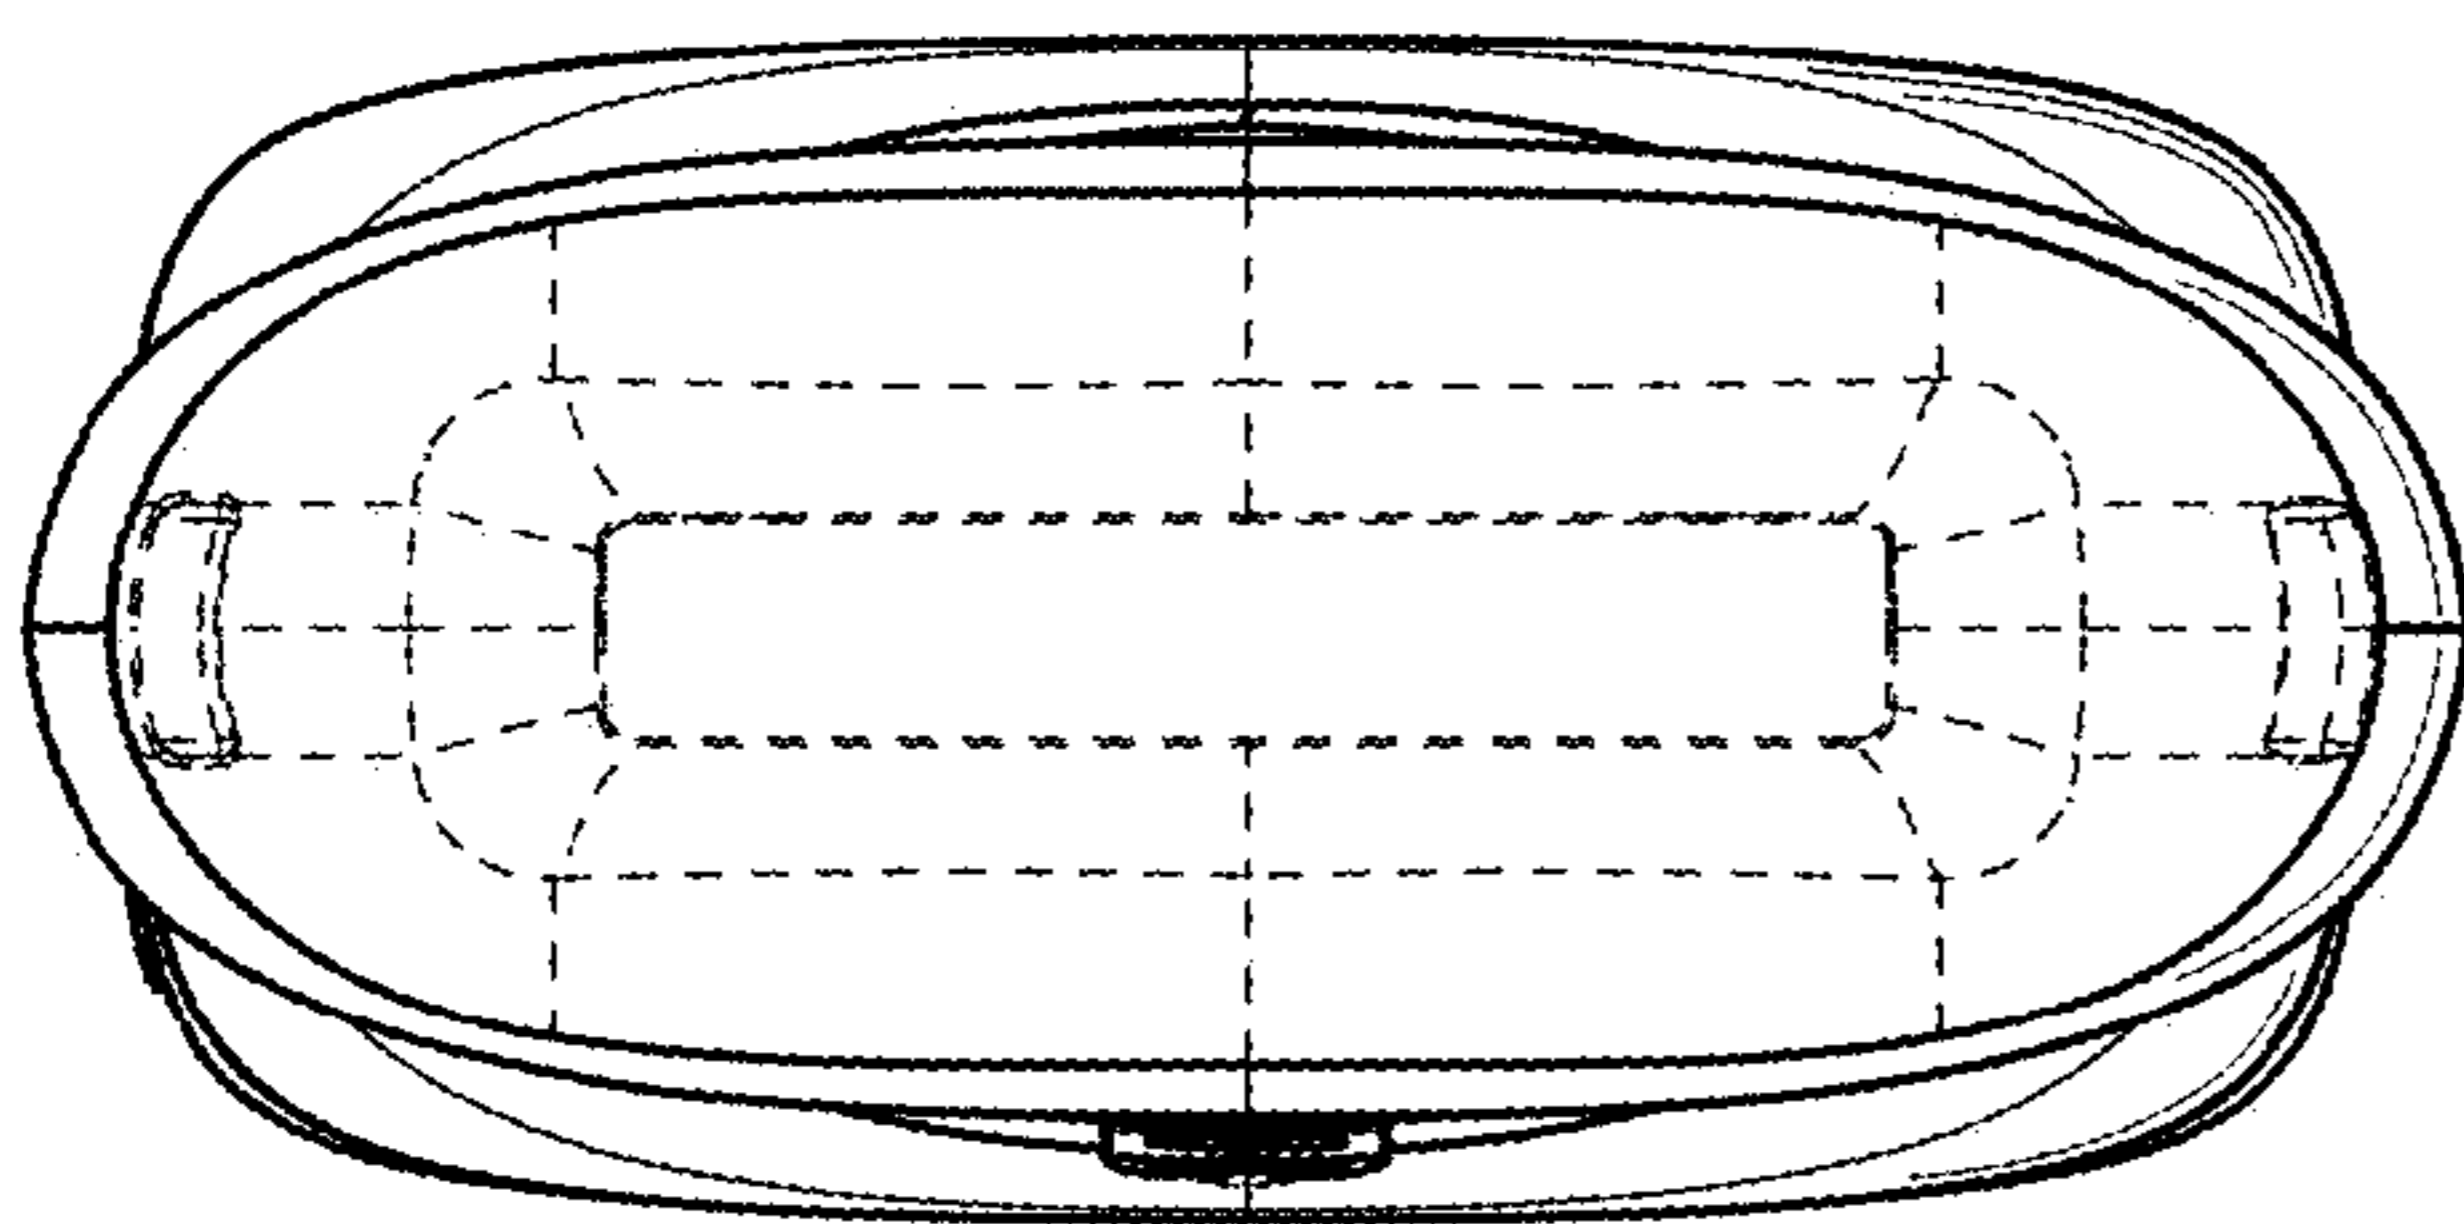


FIG. 8