



US00D879949S

(12) **United States Design Patent**
Spyridis et al.

(10) **Patent No.:** **US D879,949 S**

(45) **Date of Patent:** **** Mar. 31, 2020**

(54) **SURFACE ORNAMENTATION FOR A STEERABLE CATHETER HANDLE**

(71) Applicant: **Baylis Medical Company Inc.**,
Montreal (CA)

(72) Inventors: **Marina Stavroula Artemis Spyridis**,
Etobicoke (CA); **Lyndsay Stephenson**,
Toronto (CA); **Natalia Burachynsky**,
Toronto (CA)

(73) Assignee: **Baylis Medical Company Inc.**,
Mississauga (CA)

(**) Term: **15 Years**

(21) Appl. No.: **29/621,288**

(22) Filed: **Oct. 6, 2017**

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/112**

(58) **Field of Classification Search**
USPC D24/112–114, 108, 130, 127, 133, 186;
D14/489, 491; 606/181, 185; 604/264,
604/523–528, 272, 164.01–164.11, 187,
604/93.01; 600/101, 139, 143;
128/200.24, 207.14, 207.15
CPC A61M 25/00; A61M 39/00; A61M 27/00;
A61M 25/0043; A61M 25/0067; A61M
25/0097; A61F 2/958
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D347,473 S *	5/1994	Nitzsche	D24/112
D525,981 S *	8/2006	Hally	D14/485
D545,836 S *	7/2007	Haldimann	D14/491
D550,245 S *	9/2007	Niijima	D14/491
D559,264 S *	1/2008	Niijima	D14/490

D628,587 S *	12/2010	Vandeberghe	D14/491
D648,851 S *	11/2011	Copeland	D24/112
D683,754 S *	6/2013	Phelan	D14/489
D686,246 S *	7/2013	Gardner	D14/491
D706,824 S *	6/2014	Smith	D14/489
D715,835 S *	10/2014	Montgomery	D14/491
D729,273 S *	5/2015	Mariet	D14/491
D735,755 S *	8/2015	Bray	D14/491
D757,737 S *	5/2016	Chaudhri	G06F 3/04817 D14/485
D764,544 S *	8/2016	Ward	D14/491
D775,667 S *	1/2017	Vulk	D14/492
D778,317 S *	2/2017	Lee	D14/492
D788,163 S *	5/2017	Kim	D14/489
D792,457 S *	7/2017	Huh	D14/489
D792,459 S *	7/2017	Lee	D14/491
D793,430 S *	8/2017	Huh	D14/489

(Continued)

Primary Examiner — David G Muller

(74) *Attorney, Agent, or Firm* — Samuel Tekie; Glenn Arnold; Vincent Man


(57) **CLAIM**

The ornamental design for a surface ornamentation for a steerable catheter handle, as shown and described.

DESCRIPTION

FIG. 1 is a rear top right perspective view of a steerable catheter handle with surface ornamentation, showing our new design;
FIG. 2 is a front bottom left perspective view thereof;
FIG. 3 is a right side elevation view thereof;
FIG. 4 is a left side elevation view thereof;
FIG. 5 is a front elevation view thereof;
FIG. 6 is a rear elevation view thereof;
FIG. 7 is a top plan view thereof; and,
FIG. 8 is a bottom plan view thereof.
The broken lines in the drawing show structure illustrating the design in an environment of use. The broken lines form no part of the claimed design.

1 Claim, 5 Drawing Sheets

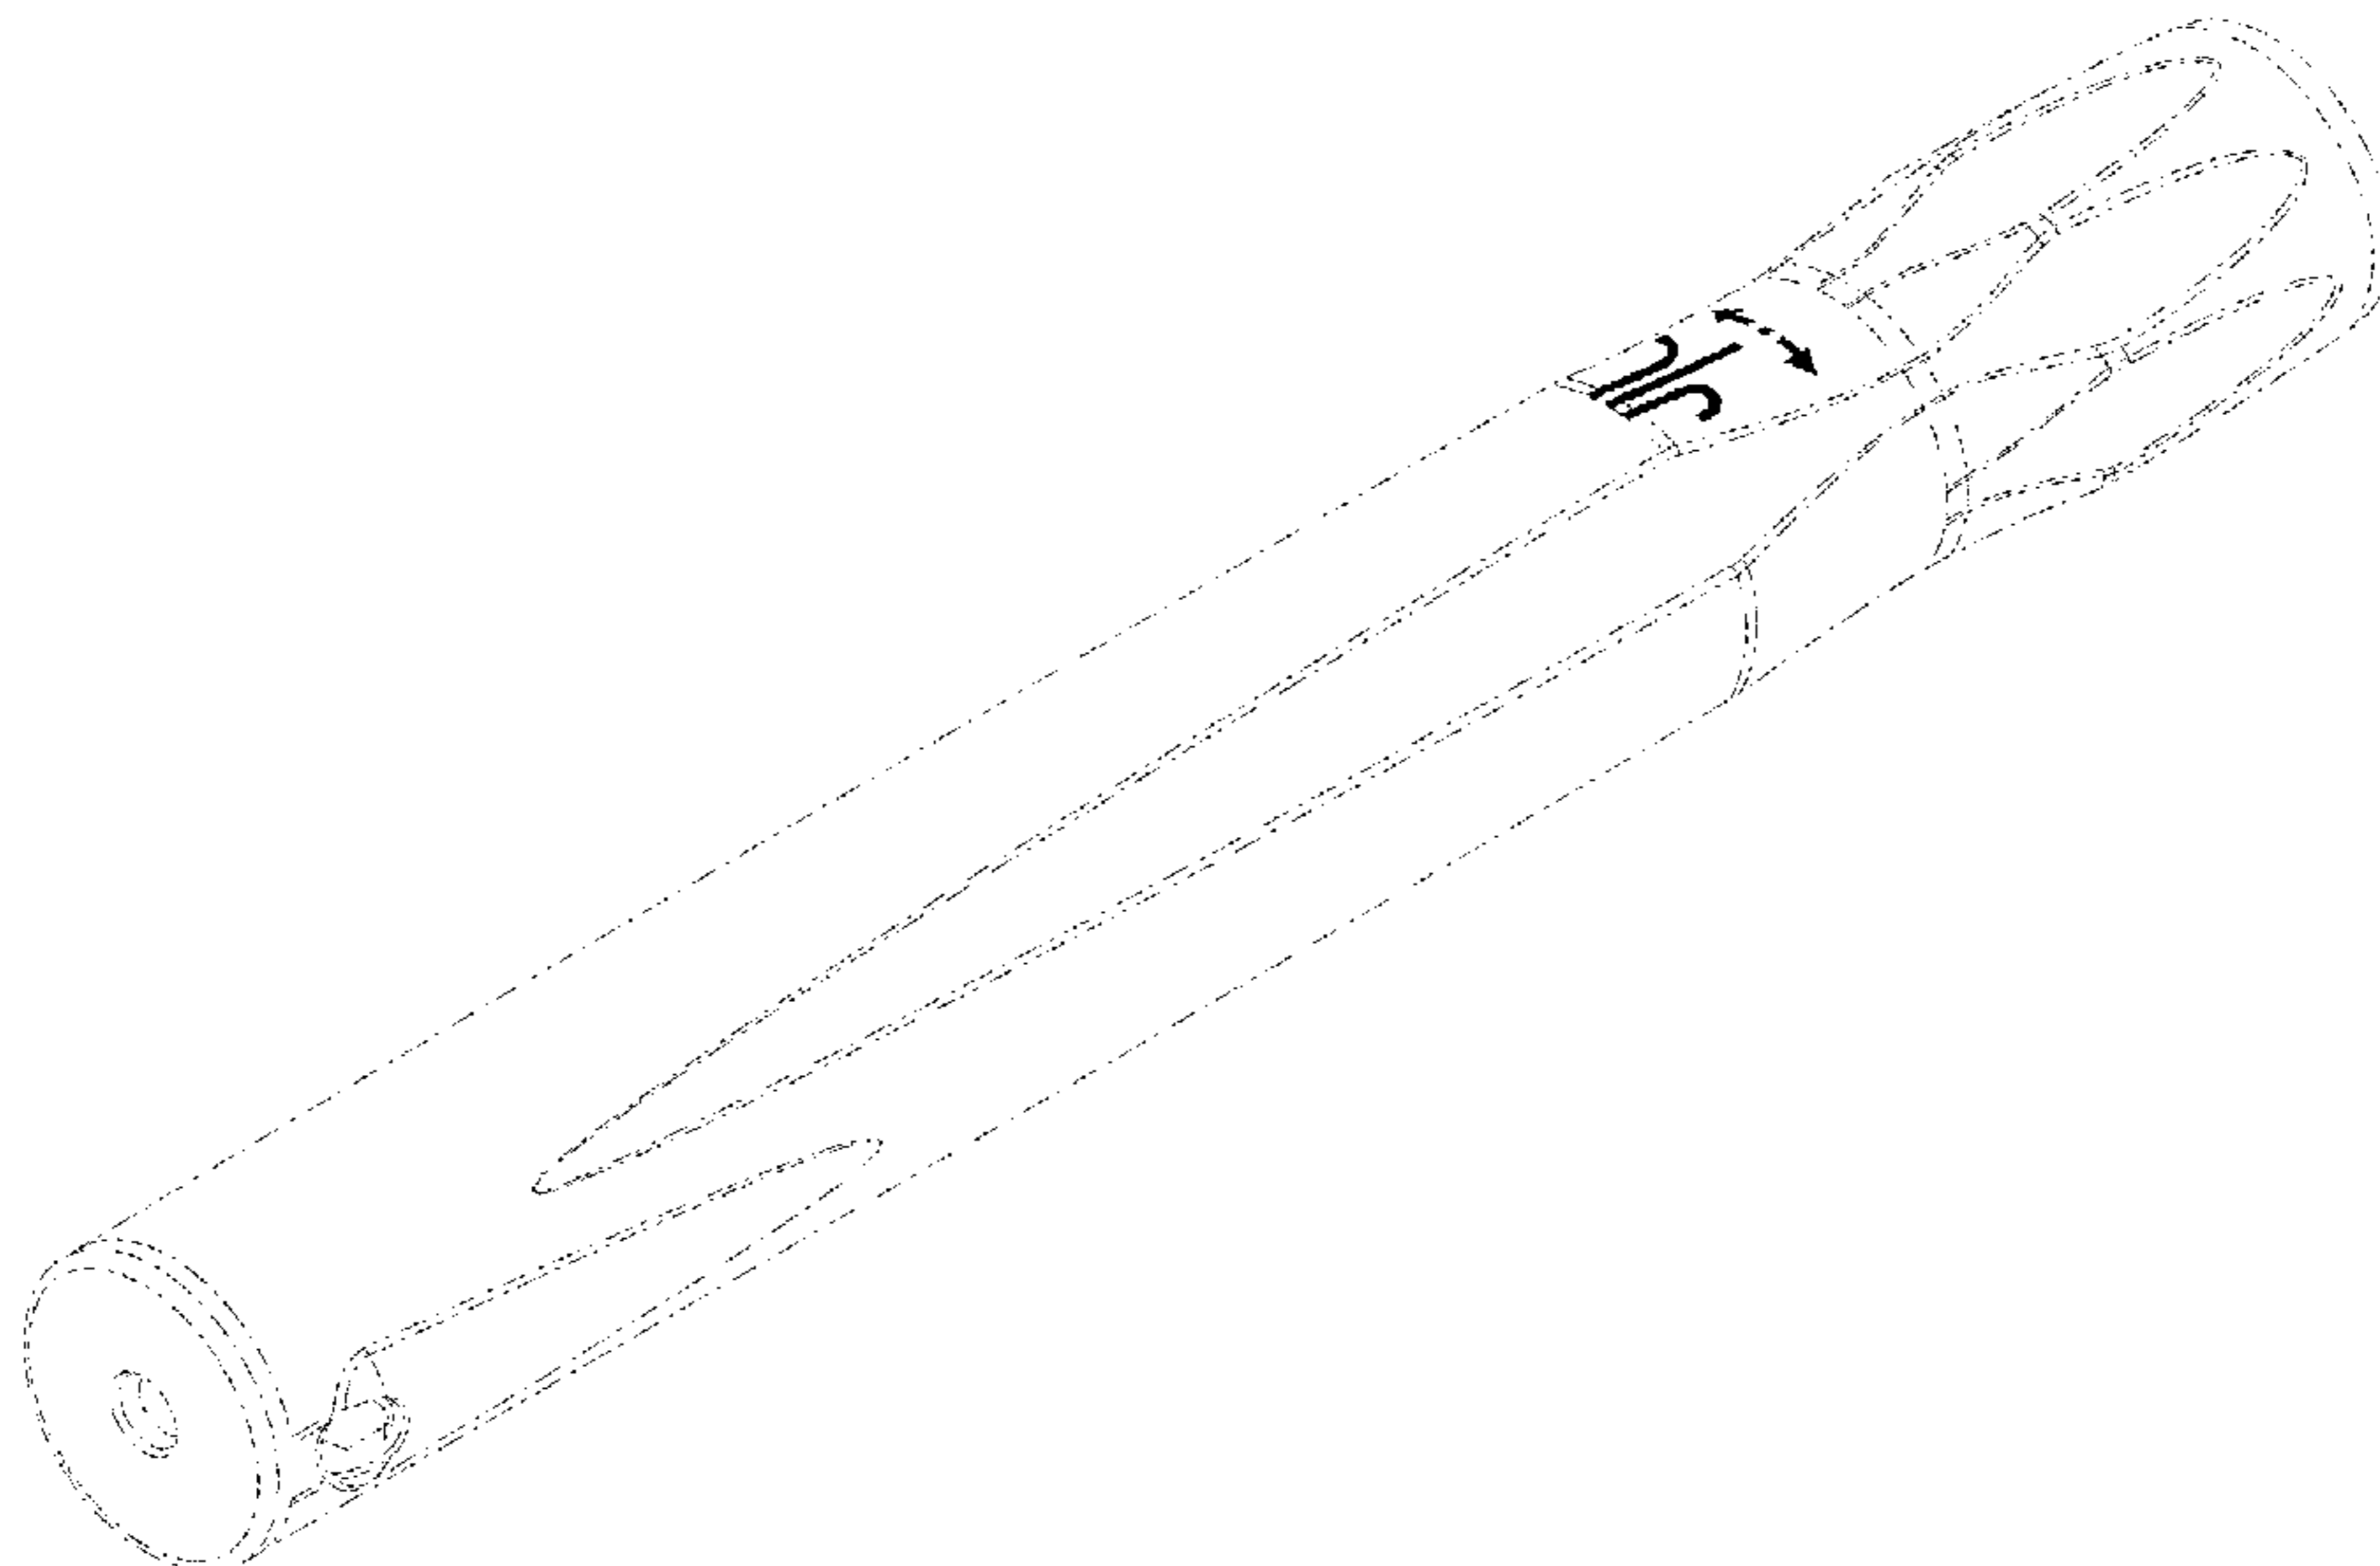

(56)

References Cited

U.S. PATENT DOCUMENTS

D803,872 S	*	11/2017	Cole	D14/488
D806,116 S	*	12/2017	Springer	D14/489
D816,713 S	*	5/2018	Kang	D14/492
D828,392 S	*	9/2018	Lee	D14/489

* cited by examiner

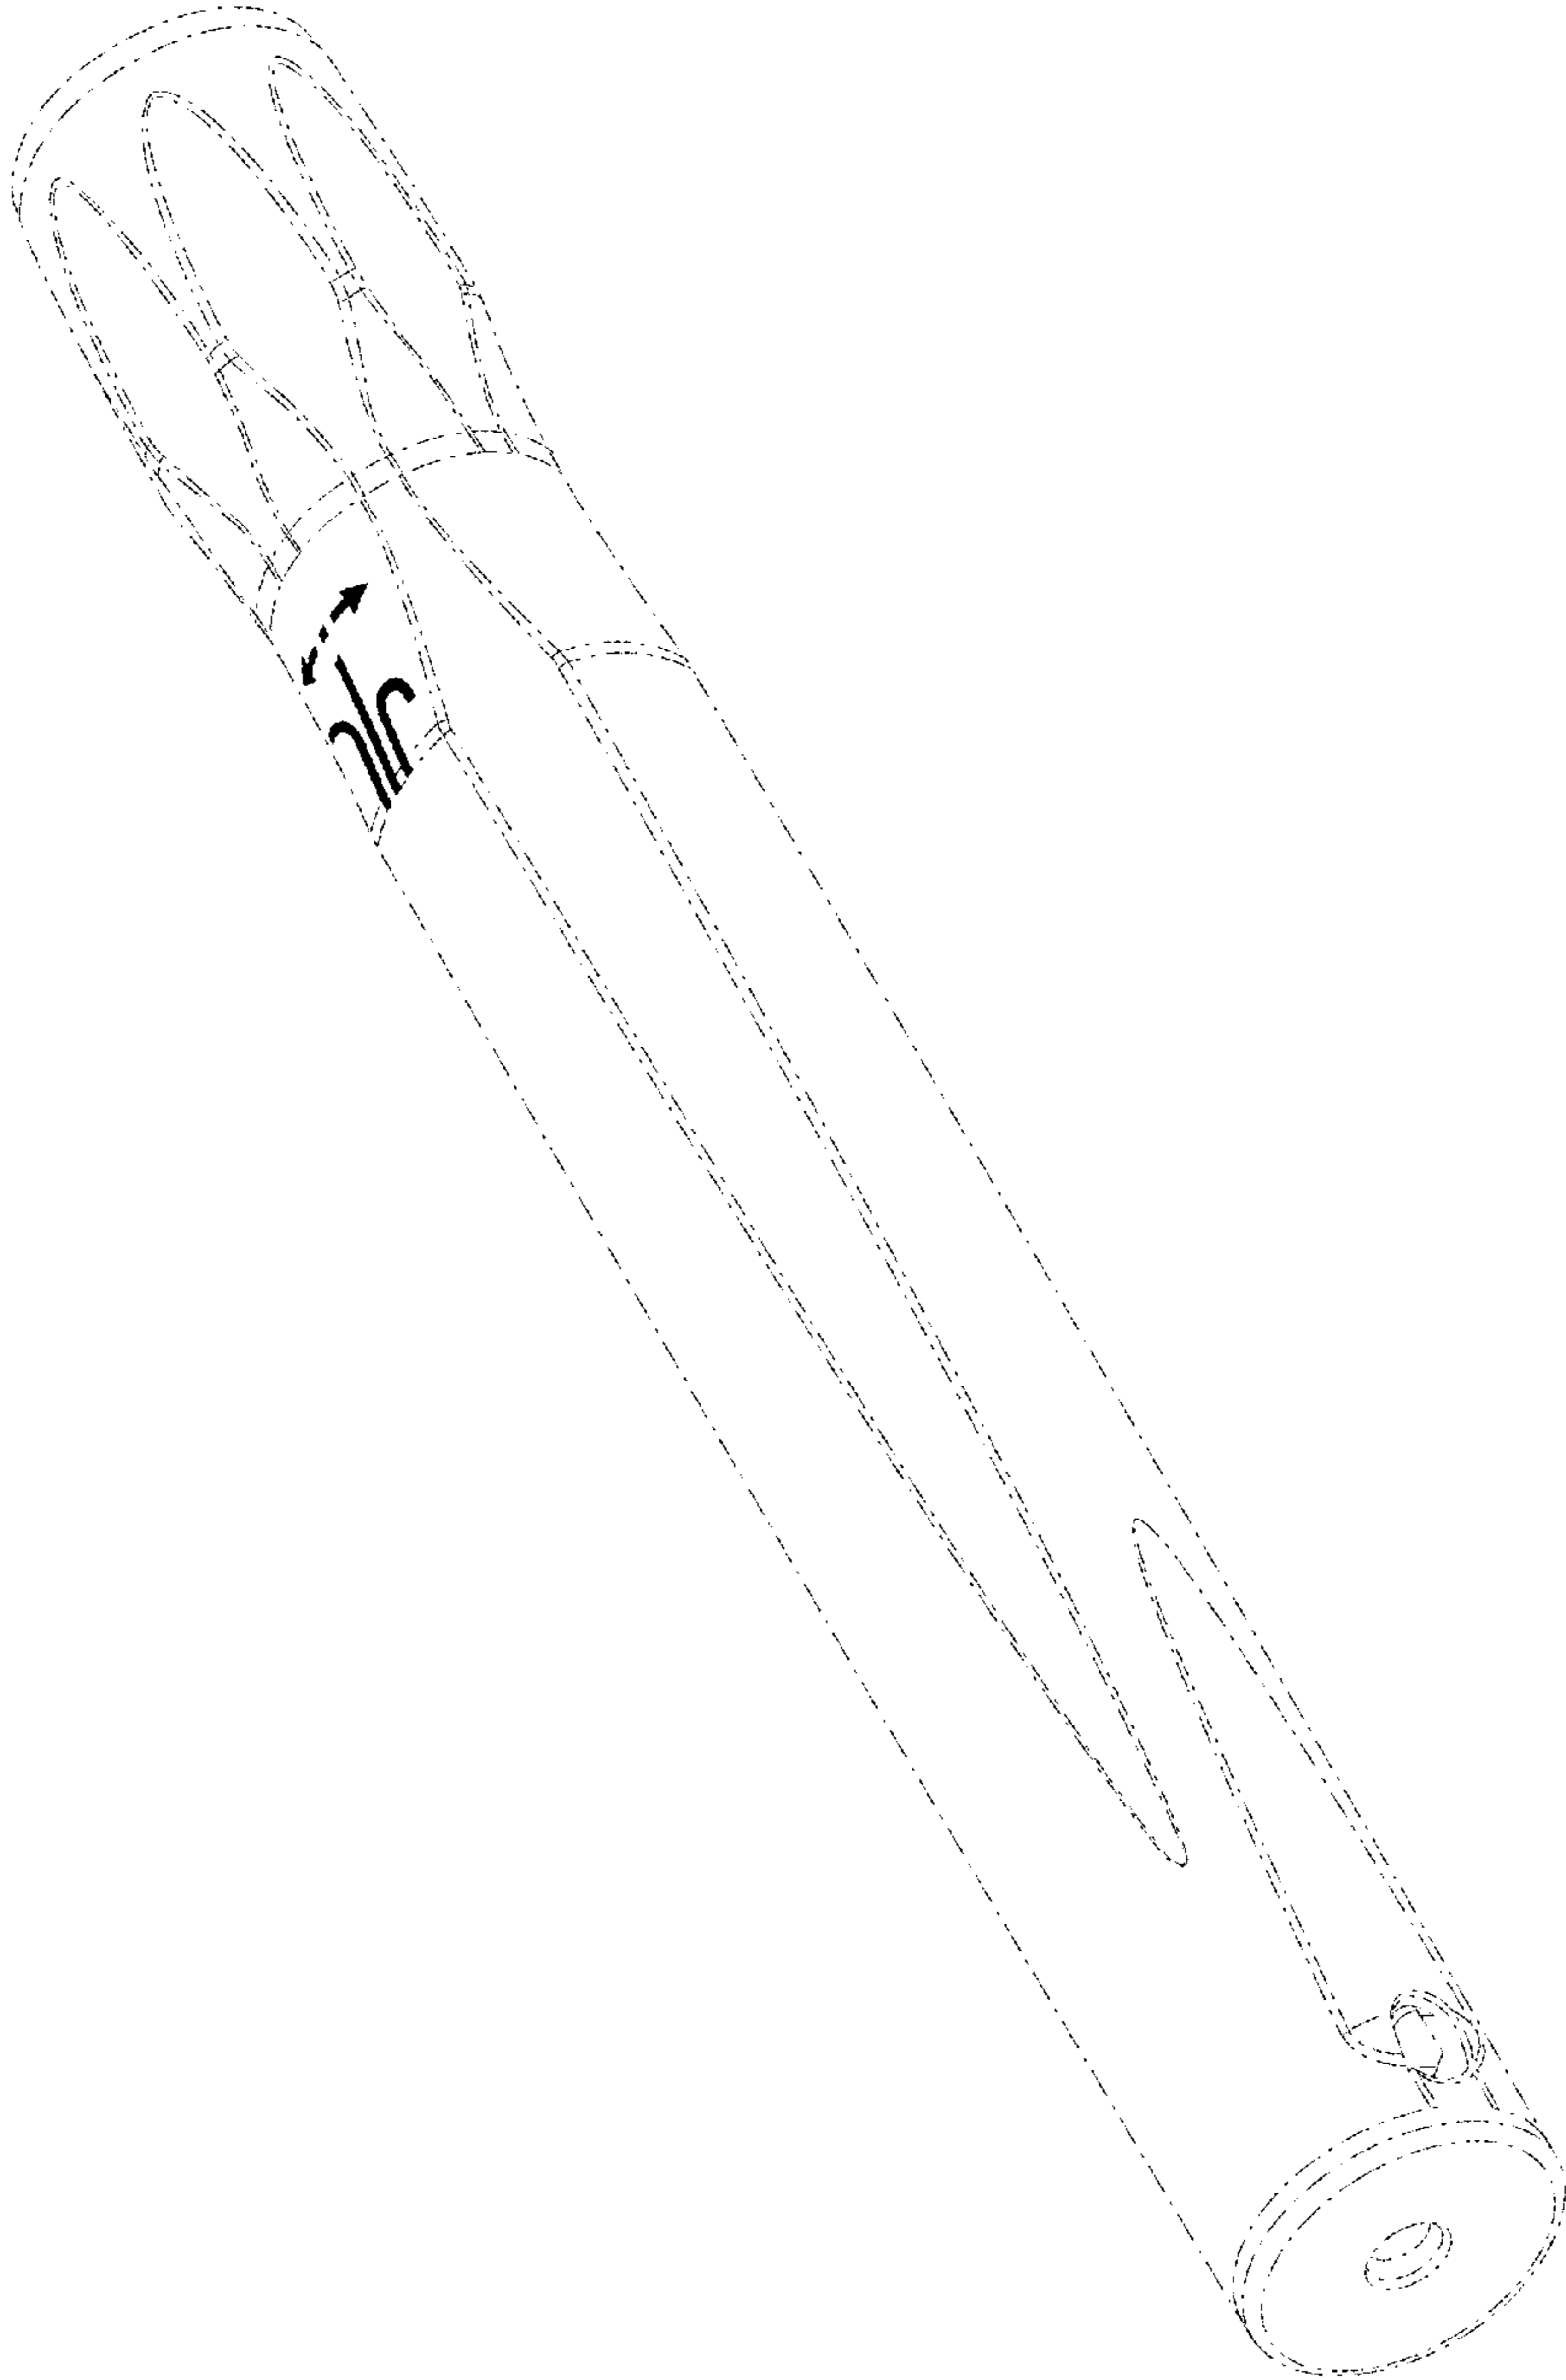


FIG. 1

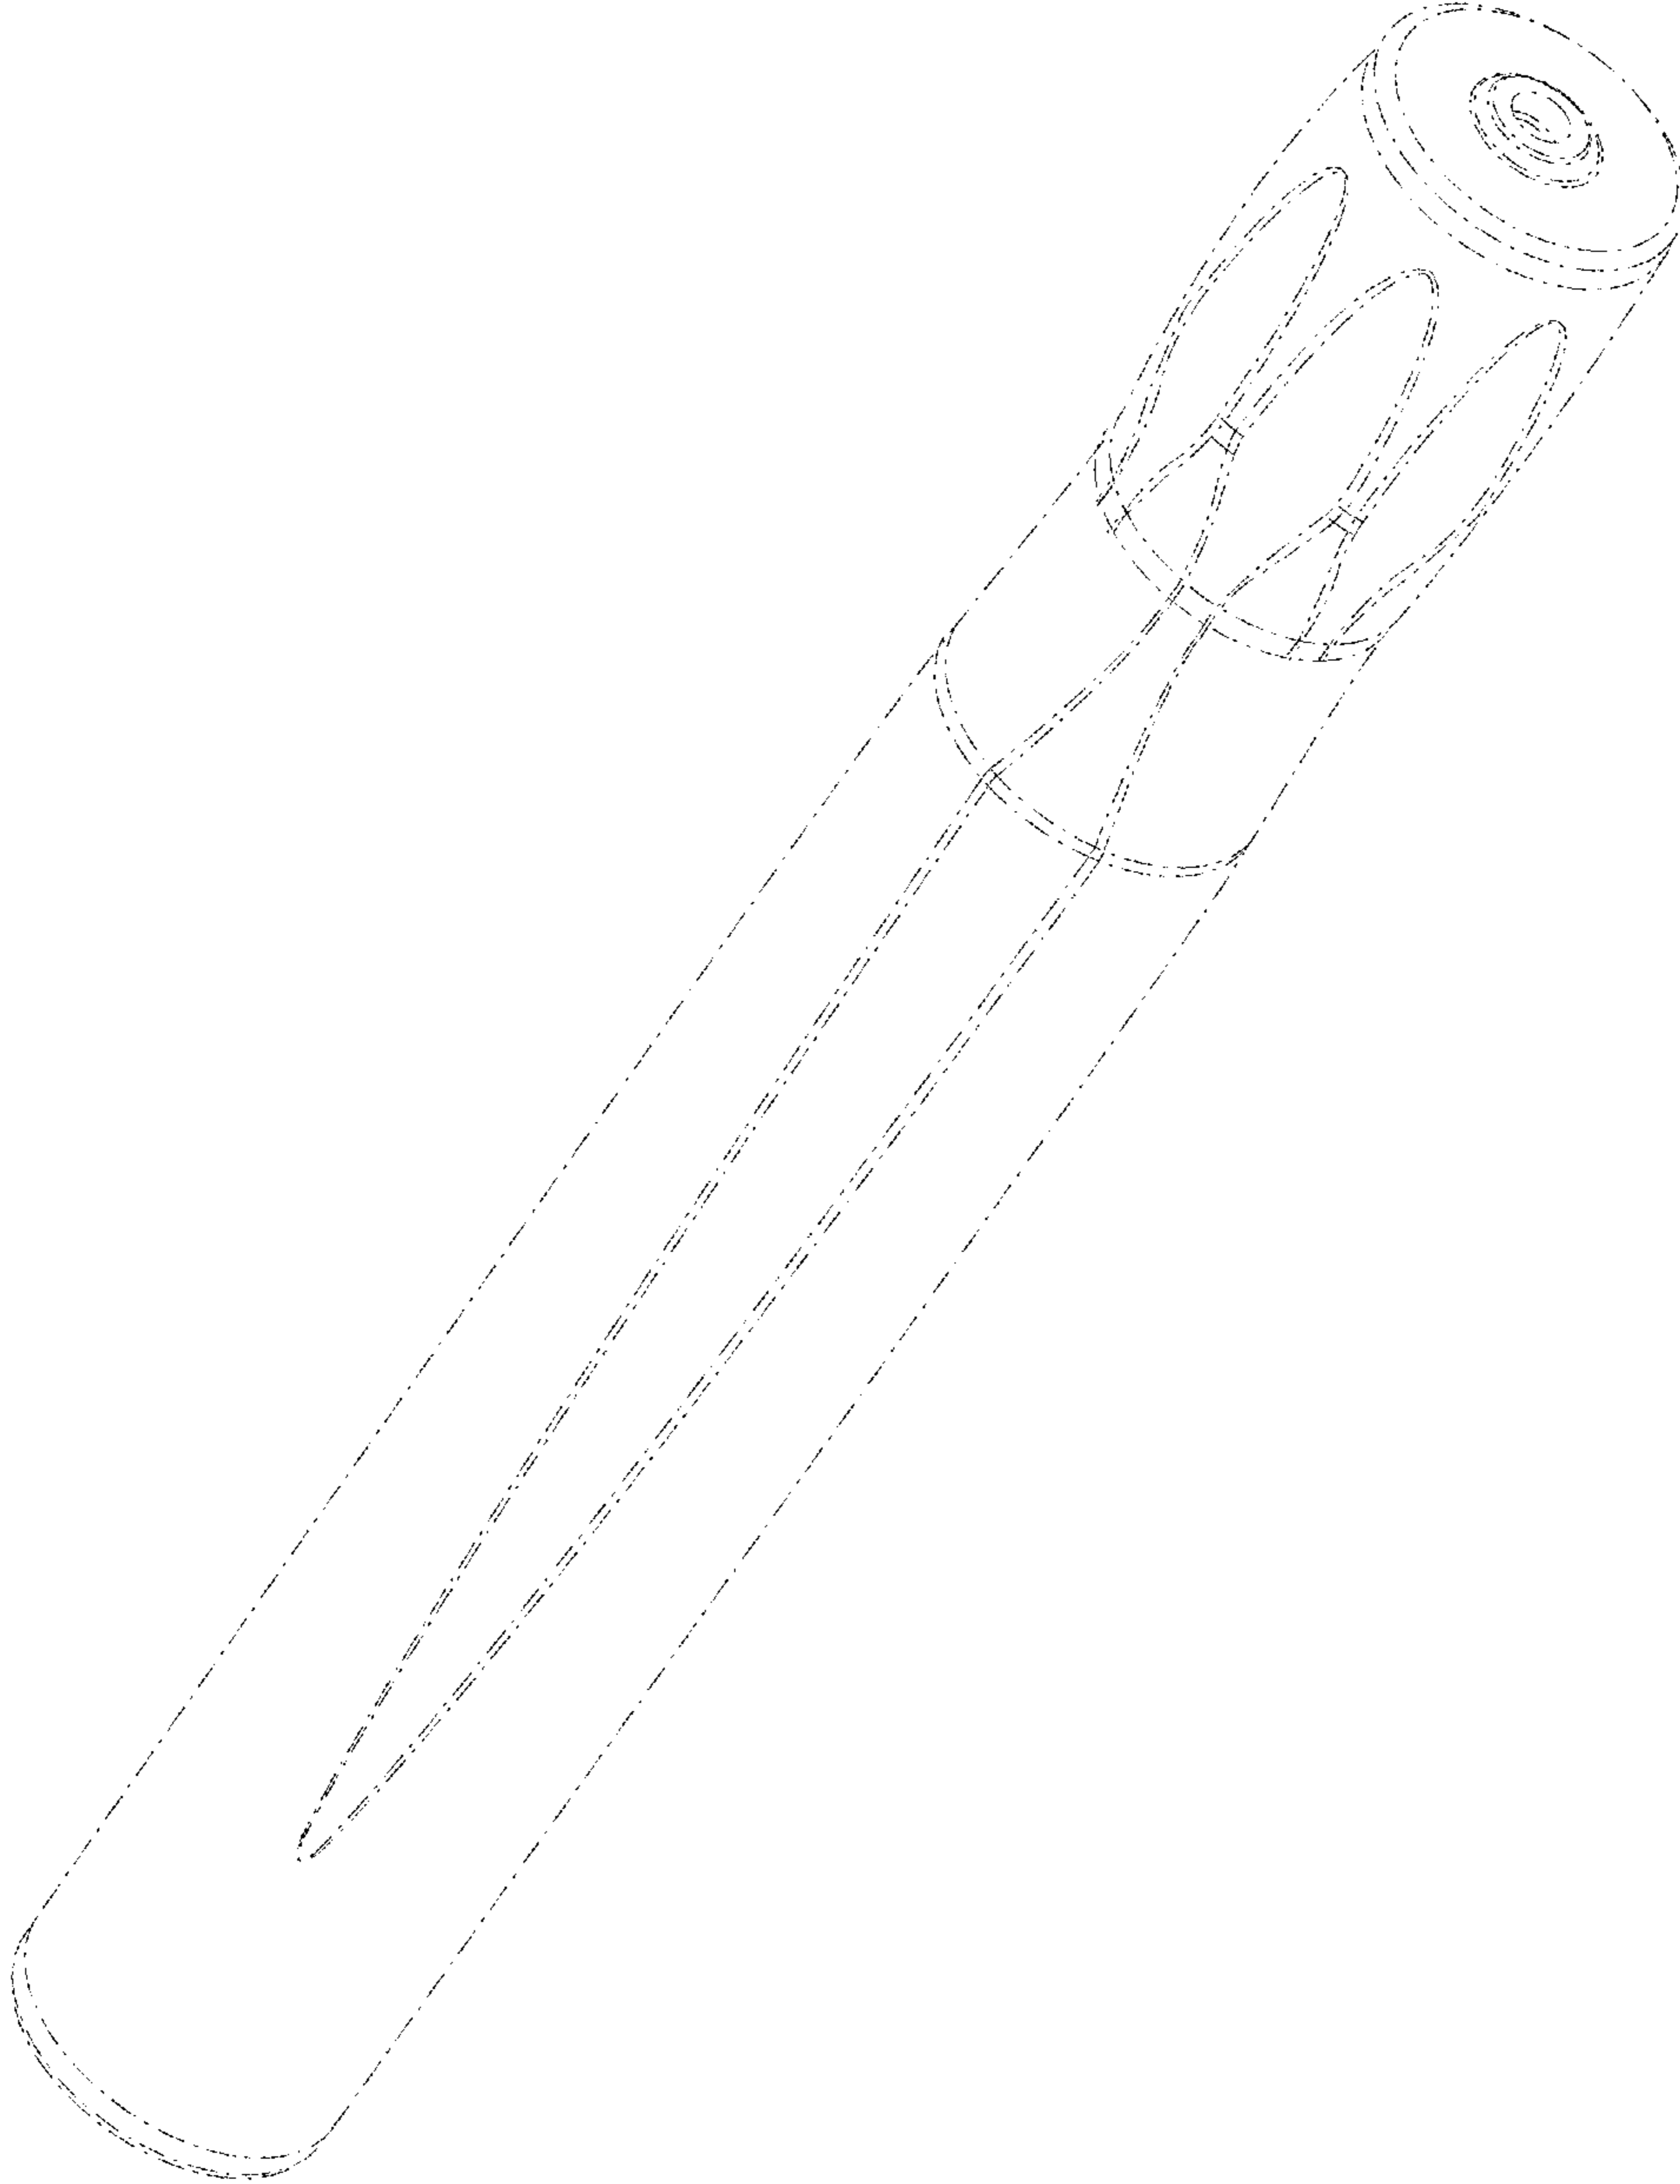


FIG. 2

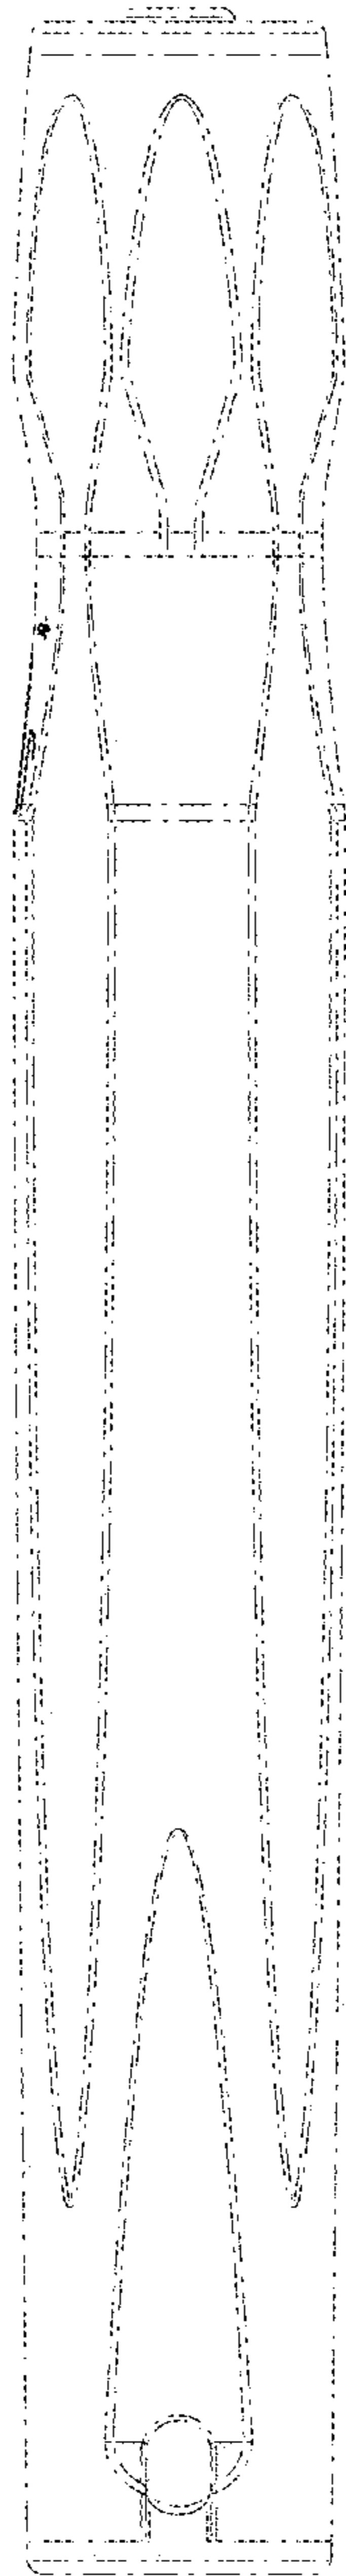


FIG. 3

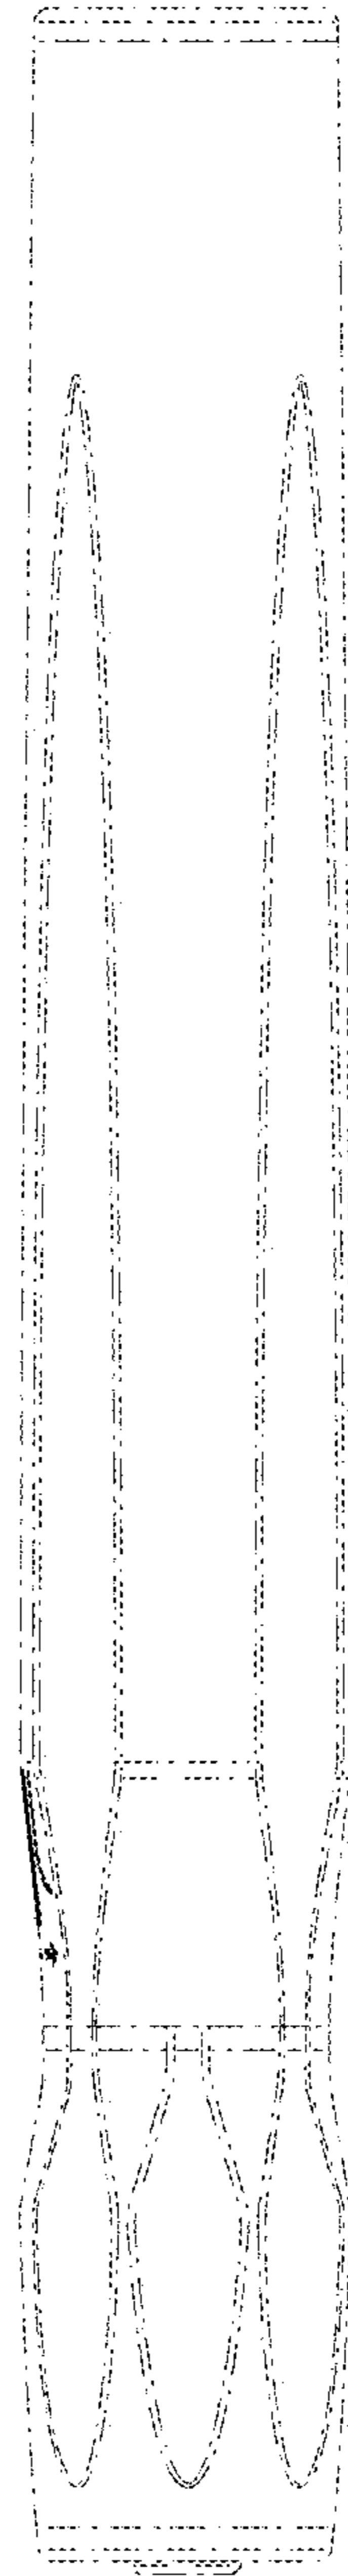


FIG. 4

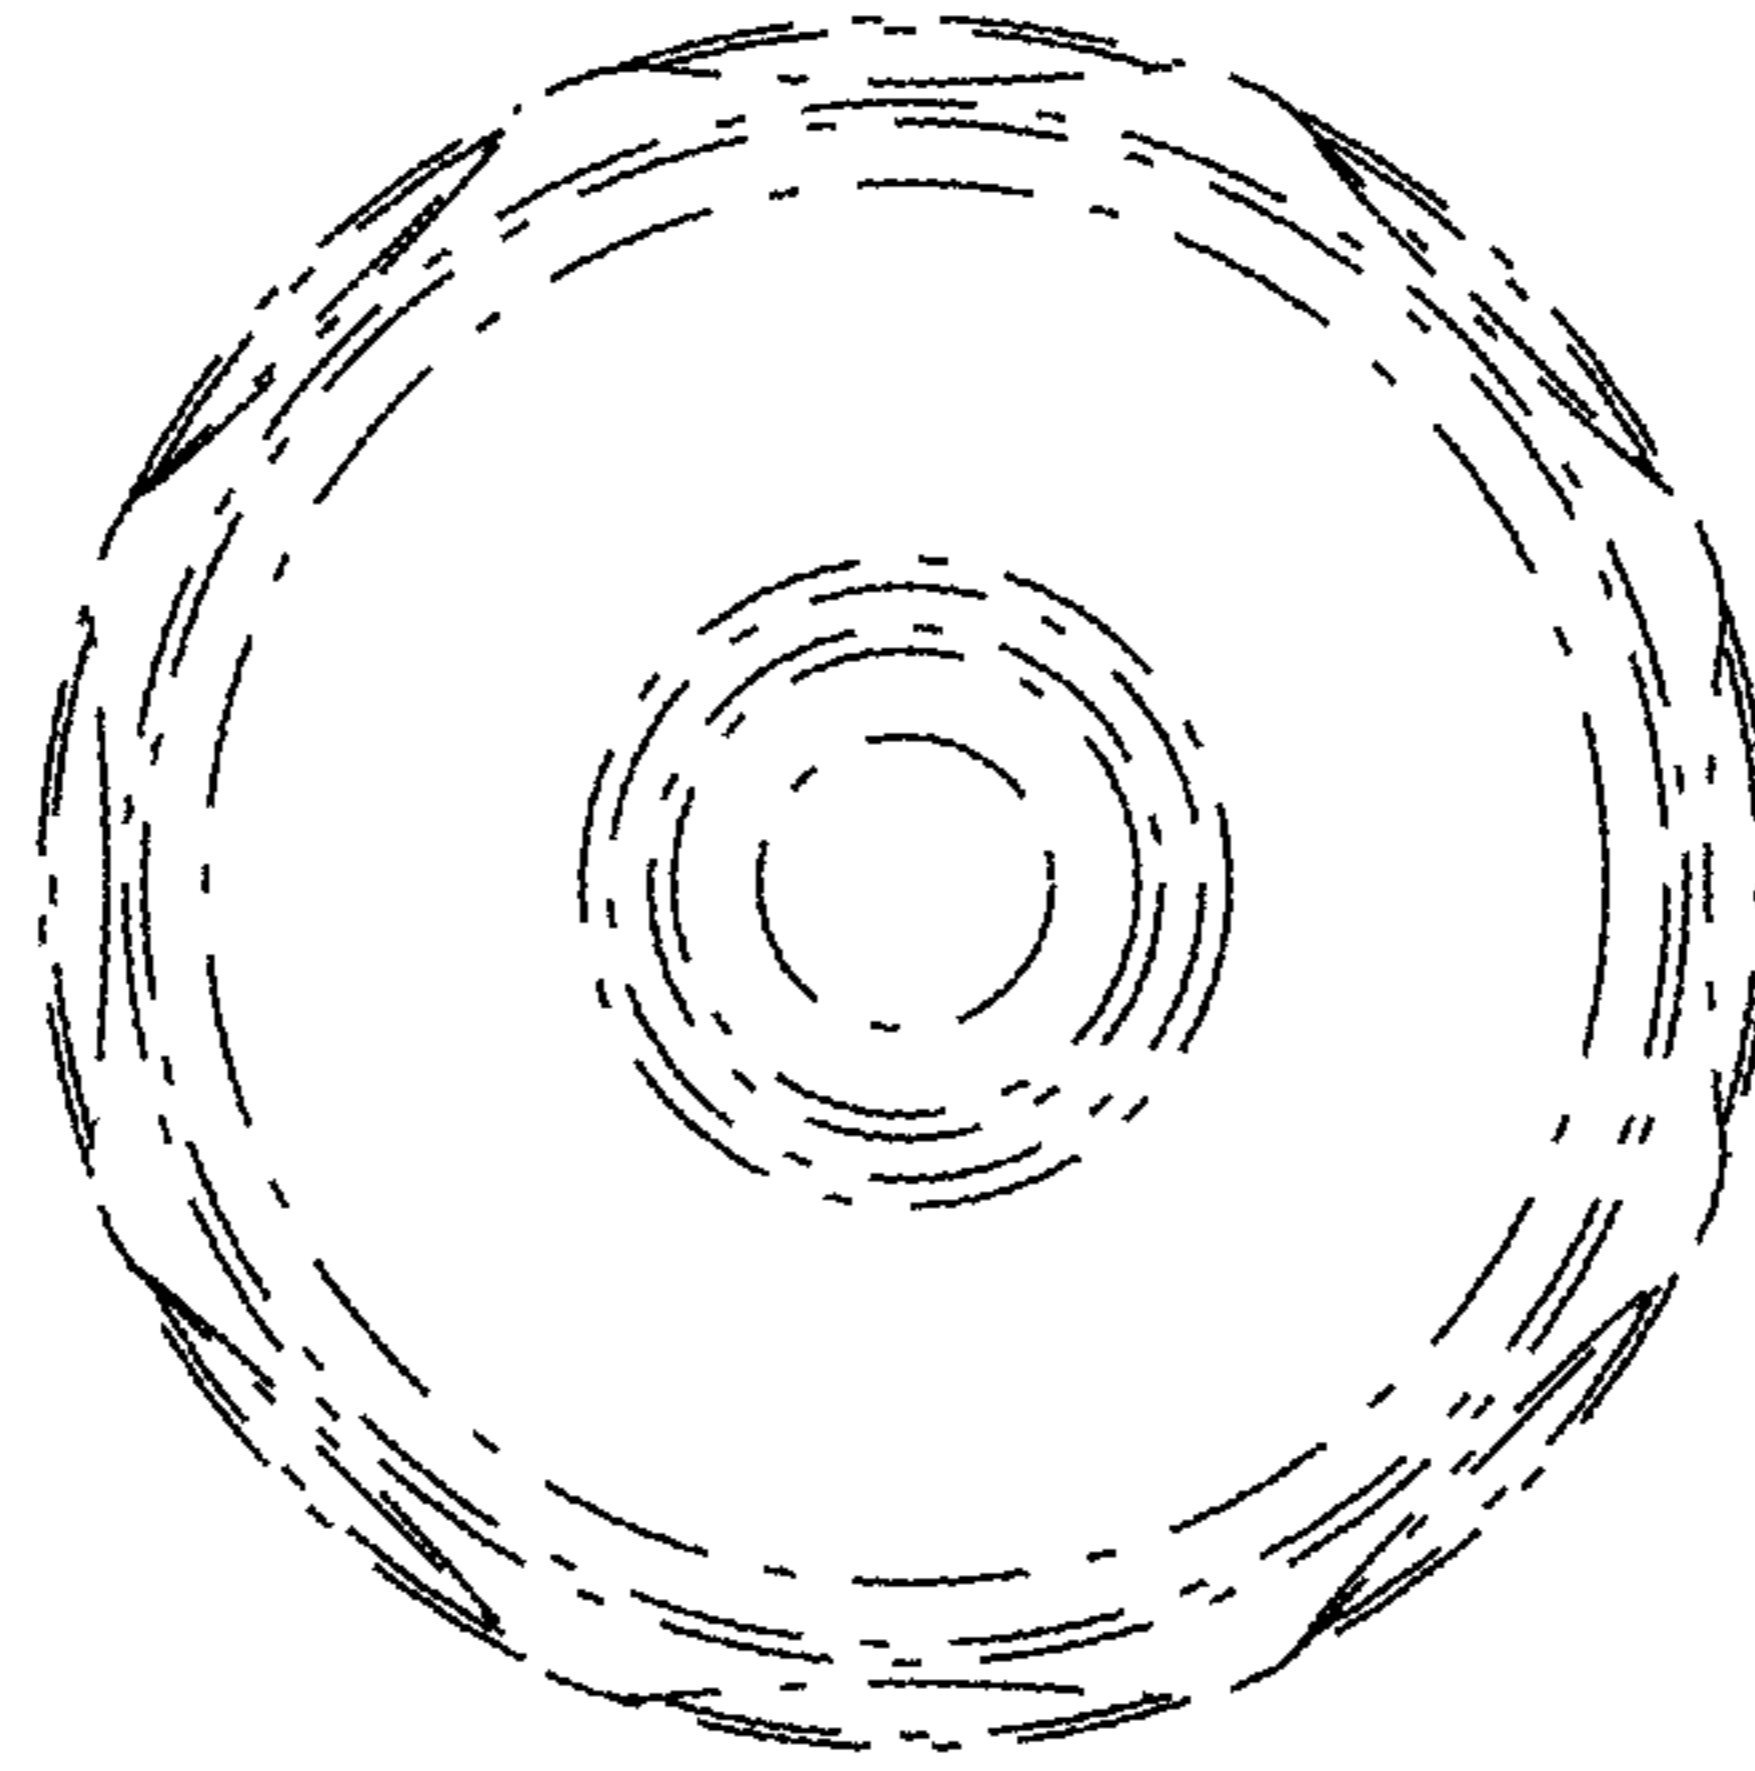


FIG. 5

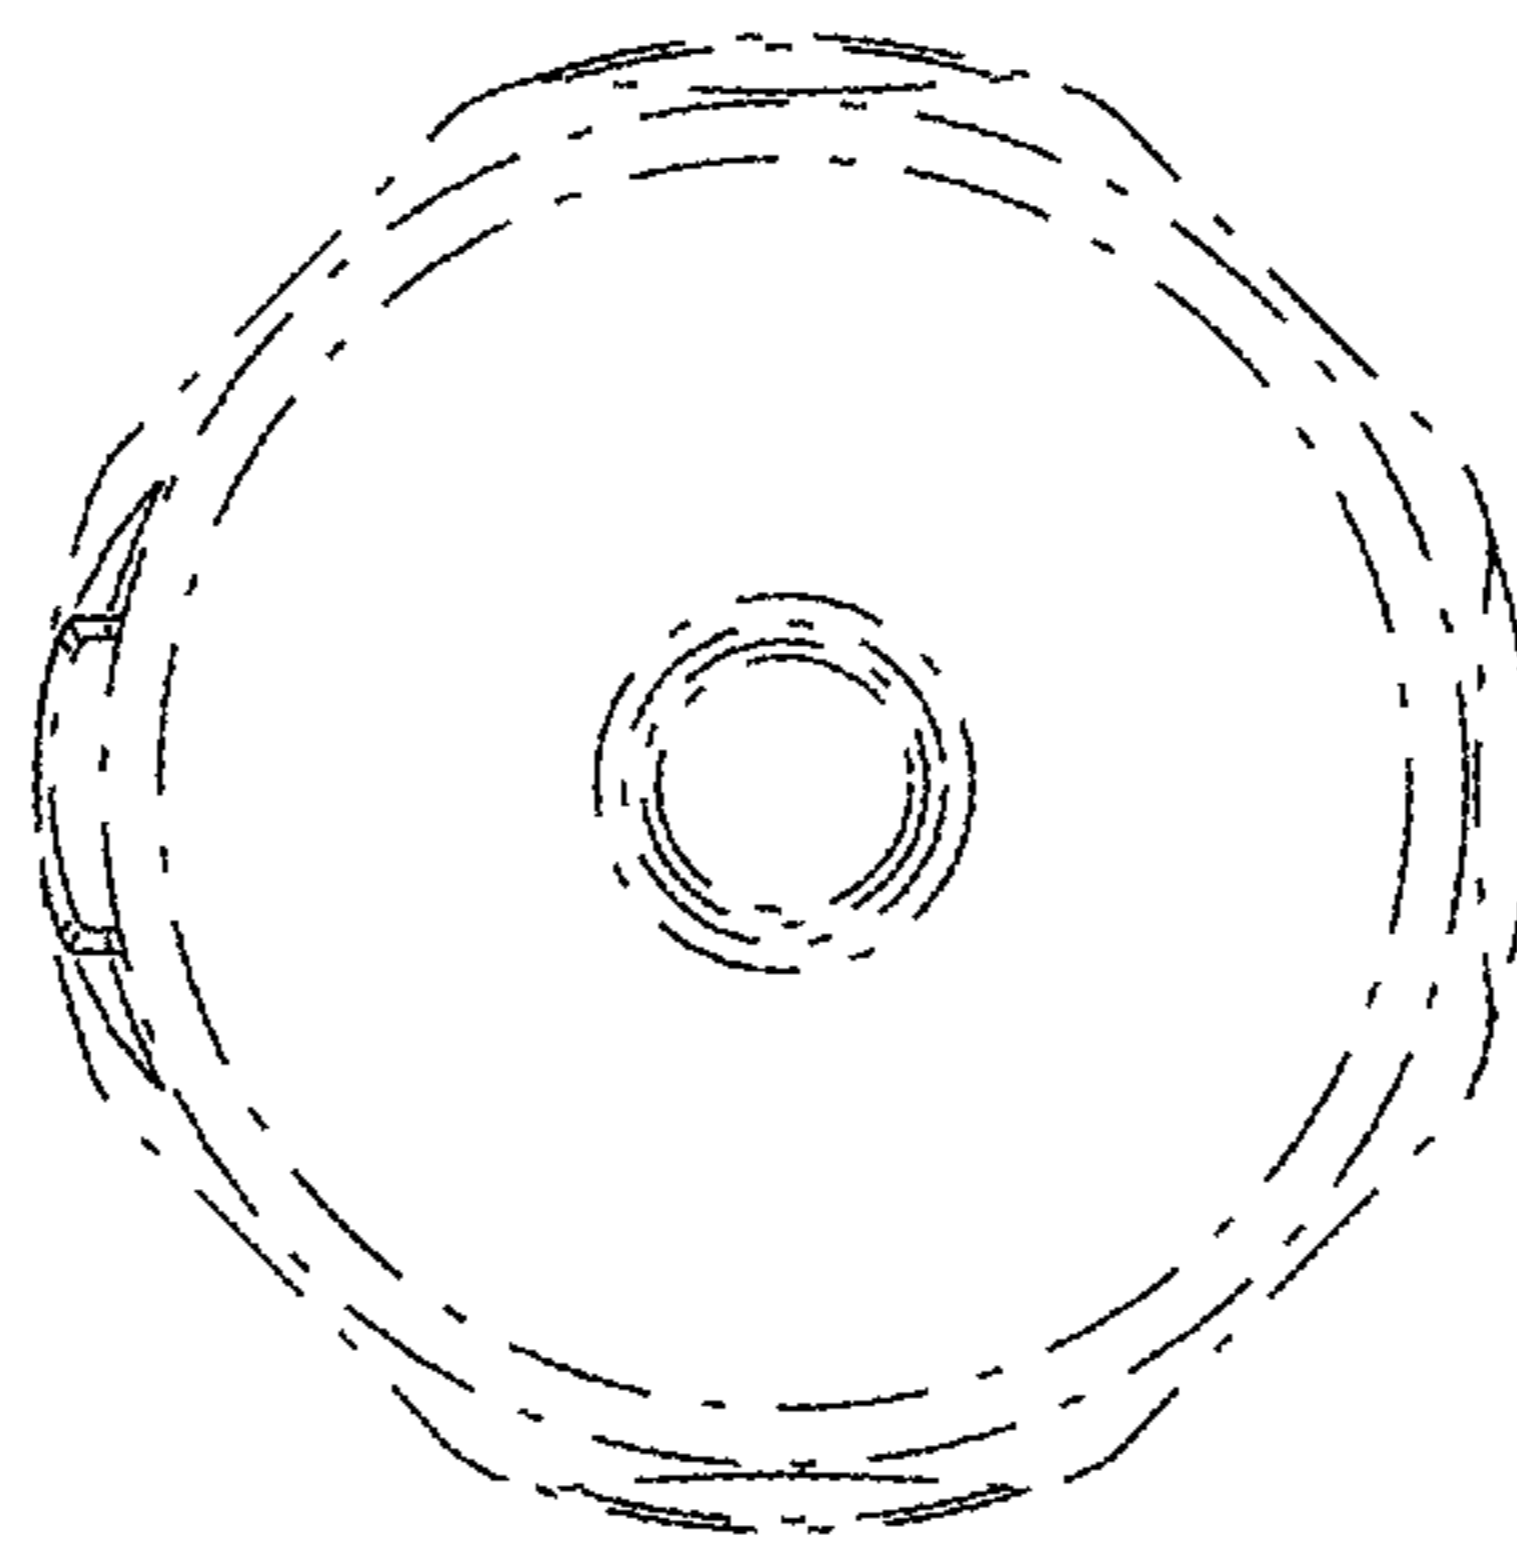


FIG. 6

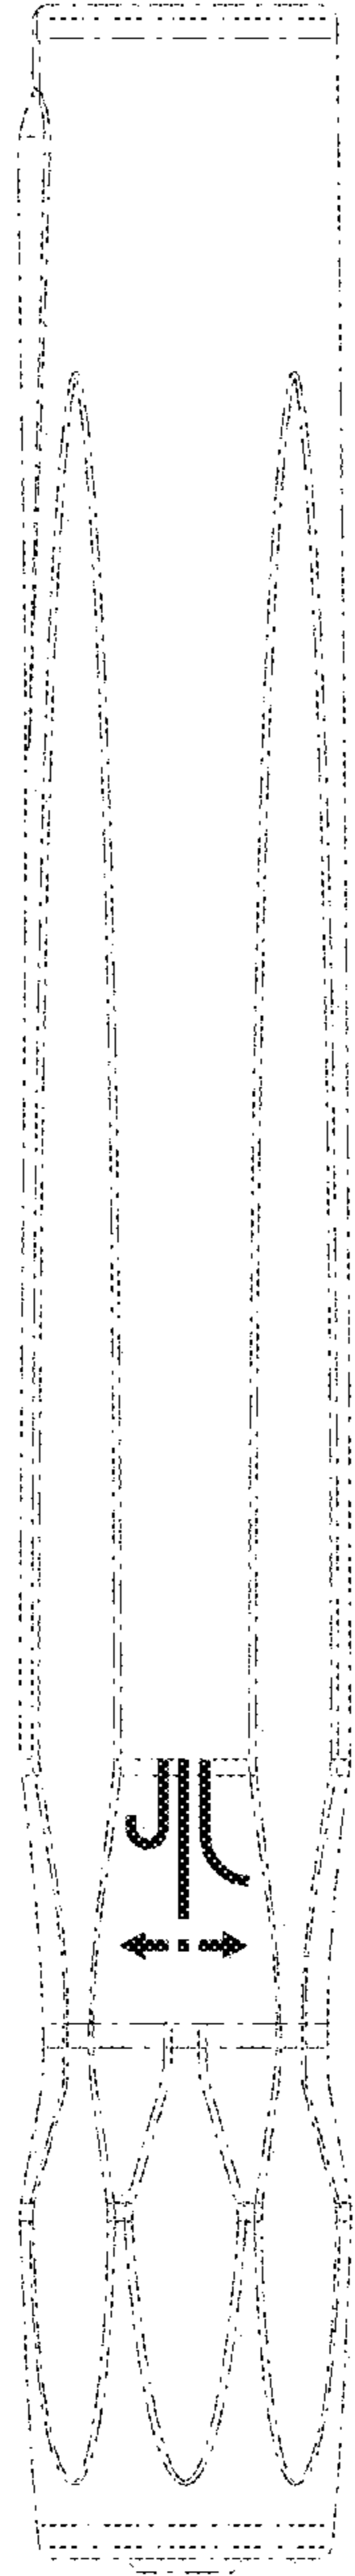


FIG. 7

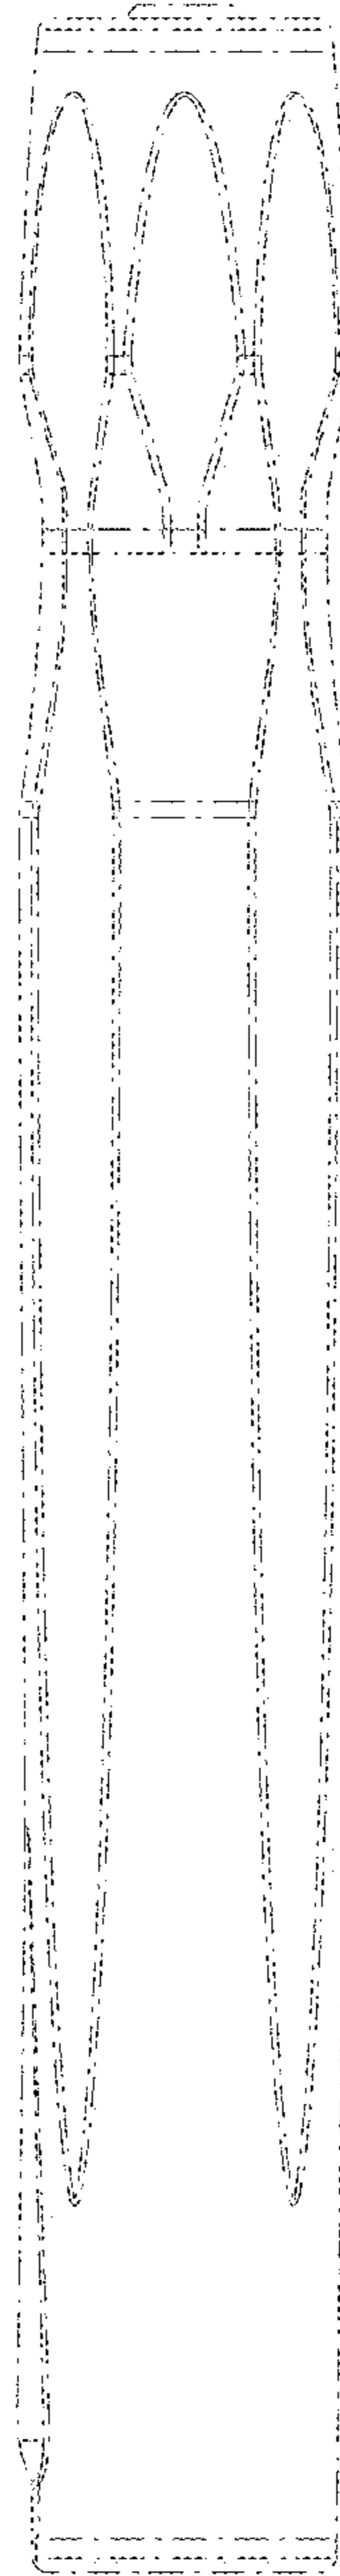


FIG. 8