



US00D882063S

(12) **United States Design Patent**  
**Sutherland et al.**

(10) **Patent No.:** **US D882,063 S**  
(45) **Date of Patent:** **\*\* Apr. 21, 2020**

(54) **COMPLIANCE MONITOR FOR A  
MEDICAMENT INHALER**  
(71) Applicant: **Adherium (NZ) Limited**, Auckland  
(NZ)  
(72) Inventors: **Garth Campbell Sutherland**, Auckland  
(NZ); **Michael James Gormack**,  
Auckland (NZ); **Benjamin Lance Catt**,  
Auckland (NZ); **Edward Scholten**,  
Auckland (NZ)

(73) Assignee: **ADHERIUM (NZ) LIMITED**,  
Auckland (NZ)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/569,112**

(22) Filed: **Jun. 23, 2016**

(30) **Foreign Application Priority Data**

Dec. 23, 2015 (NZ) ..... 421072

(51) **LOC (12) Cl.** ..... **29-02**

(52) **U.S. Cl.**  
USPC ..... **D24/110; D24/127**

(58) **Field of Classification Search**  
USPC ..... D24/107, 108, 110, 111, 127, 164, 188  
CPC ..... A61M 15/00; A61M 15/0065; A61M  
15/0091; A61M 15/0021; A61M 15/0026;  
A61M 11/00; A61M 11/02; A61M 11/04;  
A61M 15/0001; A61M 15/0068; A61M  
15/008; A61M 15/0083

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,363,842 A \* 11/1994 Mishevich ..... A61B 8/0875  
128/200.14  
6,202,642 B1 \* 3/2001 McKinnon ..... A61M 15/009  
128/200.14

D475,133 S \* 5/2003 McLuckie ..... D24/110  
D511,208 S \* 11/2005 Pardonge ..... D24/110  
8,342,172 B2 \* 1/2013 Levy ..... A61M 15/009  
128/200.14  
8,424,517 B2 \* 4/2013 Sutherland ..... A61M 15/00  
128/203.12  
9,004,062 B2 \* 4/2015 Lang ..... A61M 15/009  
128/200.14

(Continued)

**OTHER PUBLICATIONS**

SmartTouch Symbicort. Smartinhaler. YouTube.com. Date pub-  
lished: Nov. 14, 2016. <<https://www.youtube.com/watch?v=WQRJHuEmUTA>> (Year: 2016).\*

*Primary Examiner* — Lilyana Bekic

(74) *Attorney, Agent, or Firm* — Kenealy Vaidya LLP

(57) **CLAIM**

The ornamental design for a compliance monitor for a  
medicament inhaler, as shown and described.

**DESCRIPTION**

FIG. 1 is a left side view of a compliance monitor for a  
medicament inhaler showing our new design.


FIG. 2 is a front view of the compliance monitor of FIG. 1.  
FIG. 3 is a right side view of the compliance monitor of FIG.  
1.

FIG. 4 is a rear view of the compliance monitor of FIG. 1.  
FIG. 5 is a top view of the compliance monitor of FIG. 1.  
FIG. 6 is a bottom view of the compliance monitor of FIG.  
1; and,

FIG. 7 is a front perspective view of the compliance monitor  
of FIG. 1.

The broken lines in the drawings depict portions of the  
compliance monitor for a medicament inhaler that forms no  
part of the claimed design.

**1 Claim, 7 Drawing Sheets**

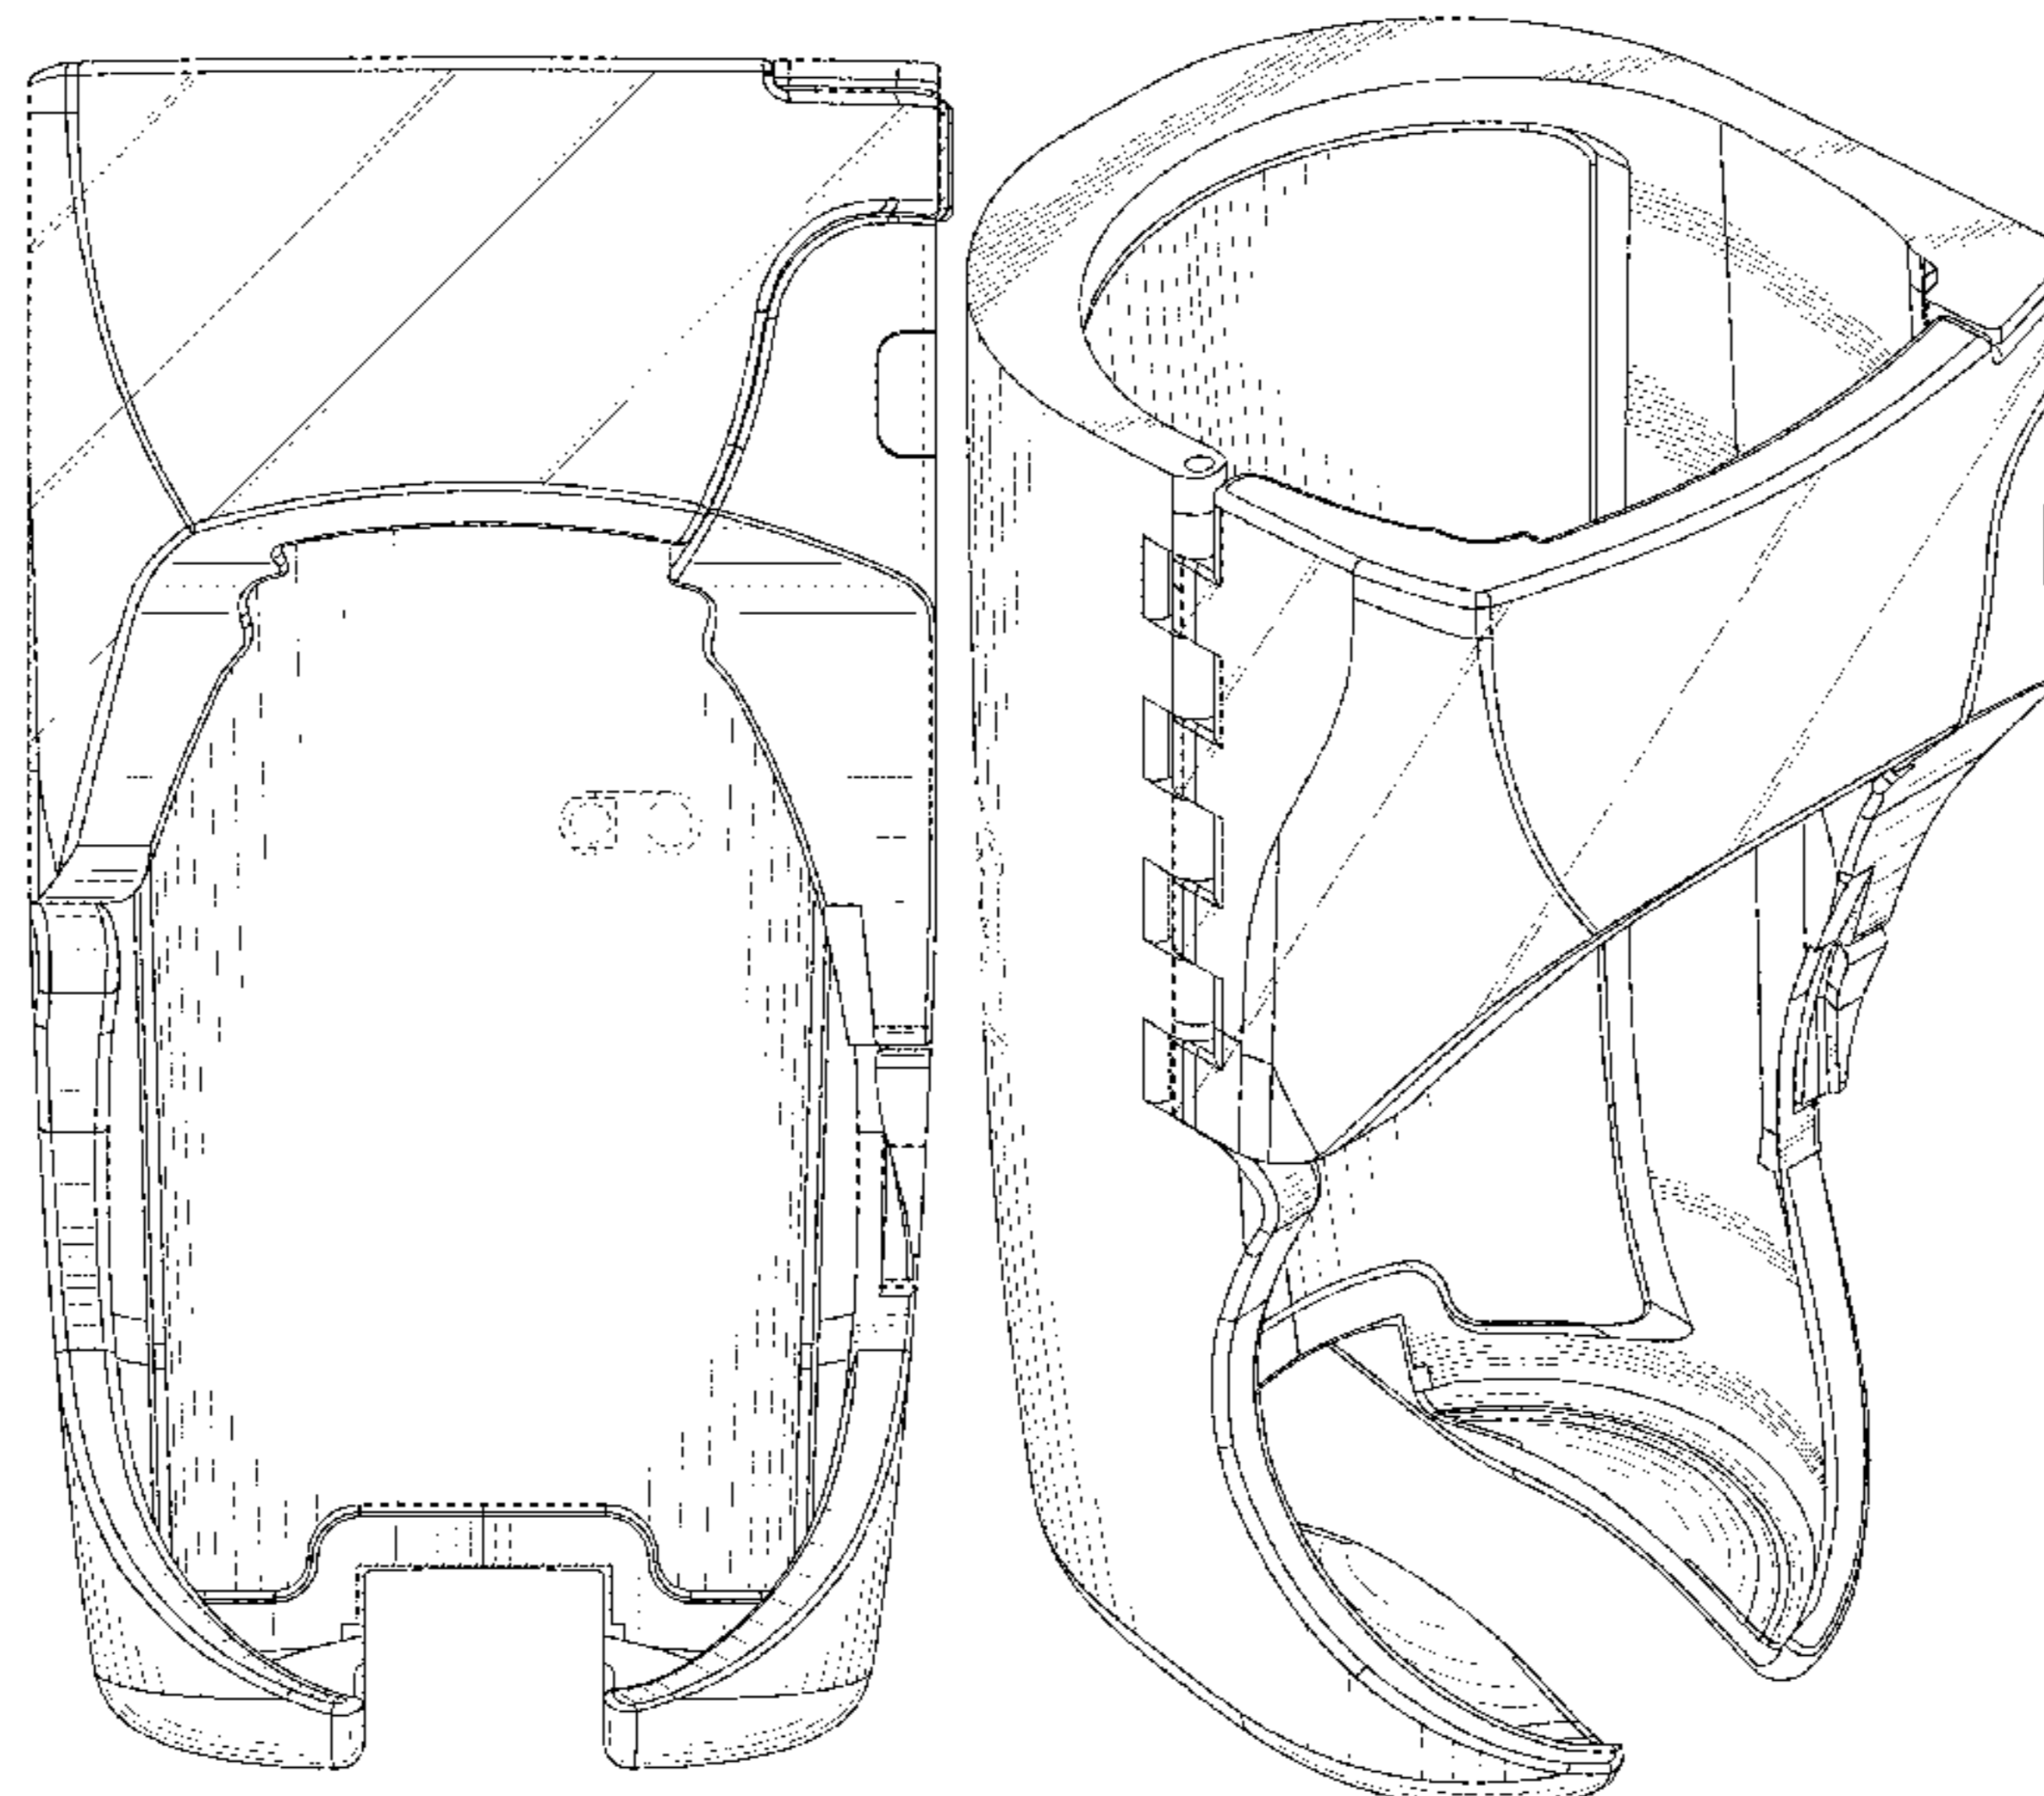

(56)

**References Cited**

## U.S. PATENT DOCUMENTS

9,072,846	B2 *	7/2015	Helmlinger	.....	A61M 15/009
D757,926	S *	5/2016	Van Sickle	.....	D24/110
D774,178	S *	12/2016	Van Sickle	.....	D24/110
D777,904	S *	1/2017	Van Sickle	.....	D24/110
D861,157	S *	9/2019	Hubanks	.....	D24/110
2010/0192948	A1 *	8/2010	Sutherland	.....	A61M 15/0065 128/203.15
2010/0250280	A1 *	9/2010	Sutherland	.....	A61M 15/0065 705/3
2010/0252036	A1 *	10/2010	Sutherland	.....	A61M 15/00 128/203.12
2011/0253139	A1 *	10/2011	Guthrie	.....	A61M 15/009 128/203.14
2014/0182584	A1 *	7/2014	Sutherland	.....	A61M 15/009 128/200.23
2016/0228657	A1 *	8/2016	Sutherland	.....	A61M 15/009
2016/0325058	A1 *	11/2016	Samson	.....	A61M 16/021
2017/0325734	A1 *	11/2017	Sutherland	.....	A61B 5/4833
2019/0105450	A1 *	4/2019	Sutherland	.....	A61M 15/0026

\* cited by examiner

FIG. 1

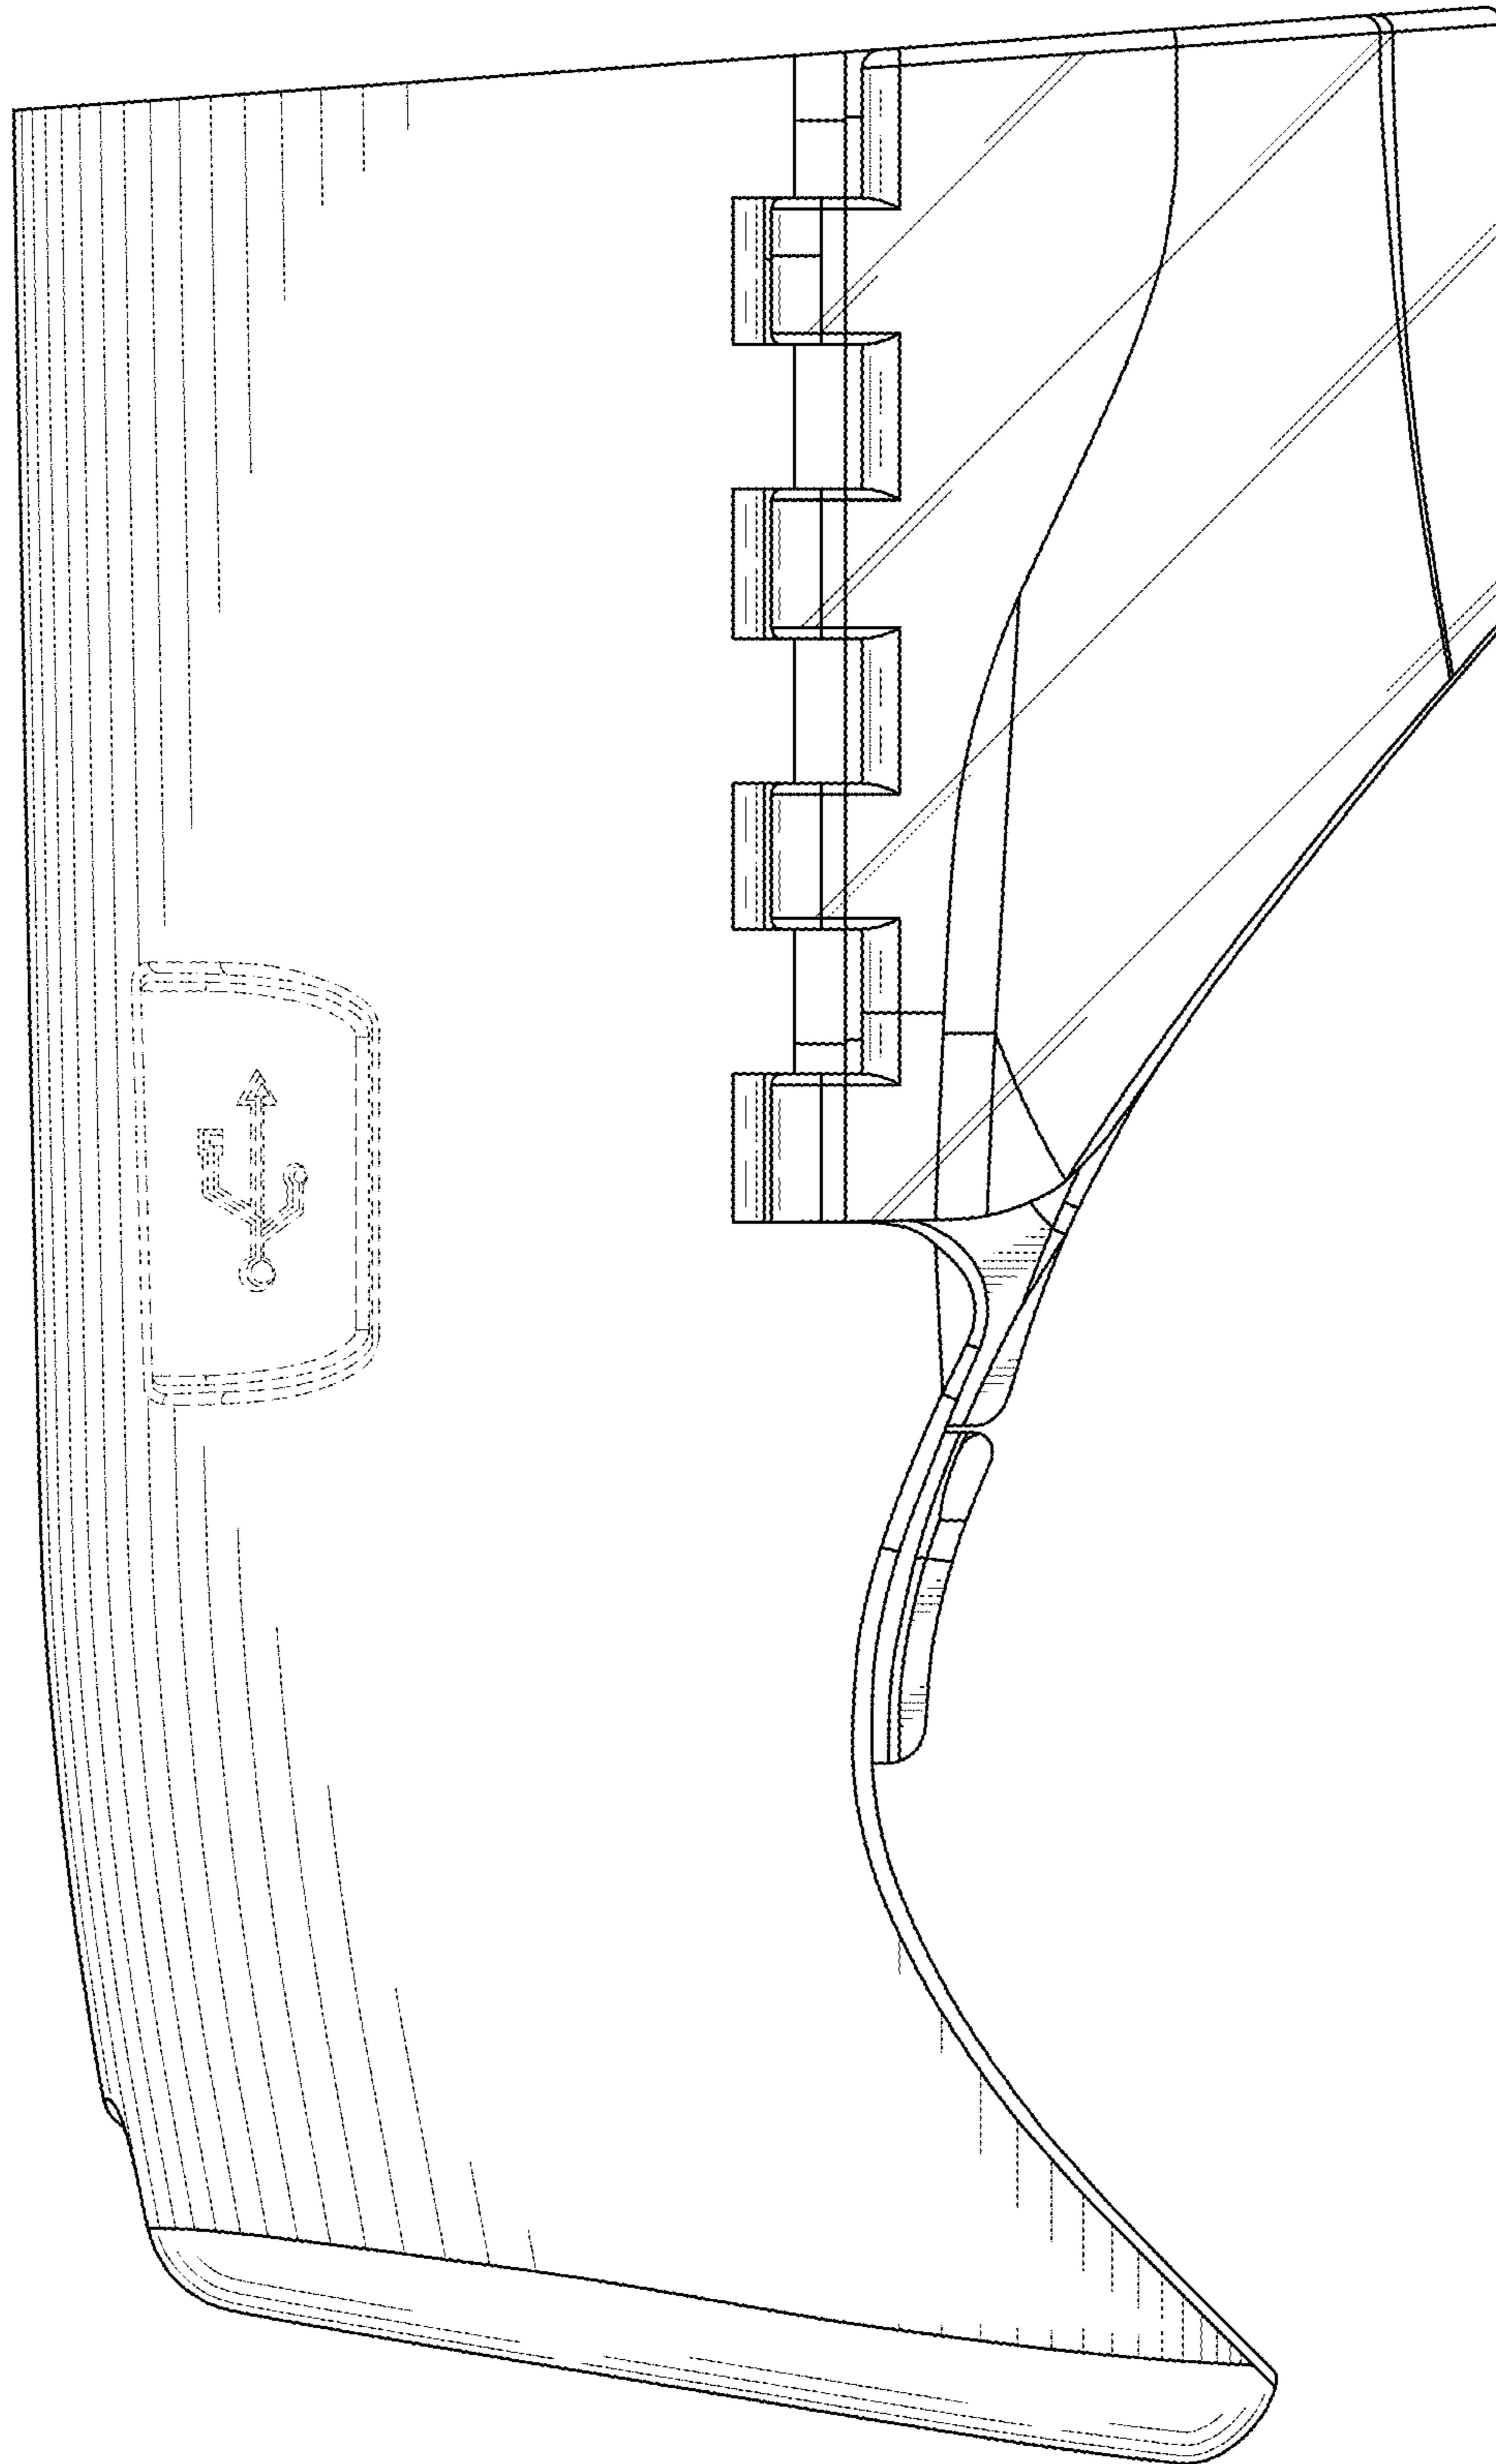




FIG. 2

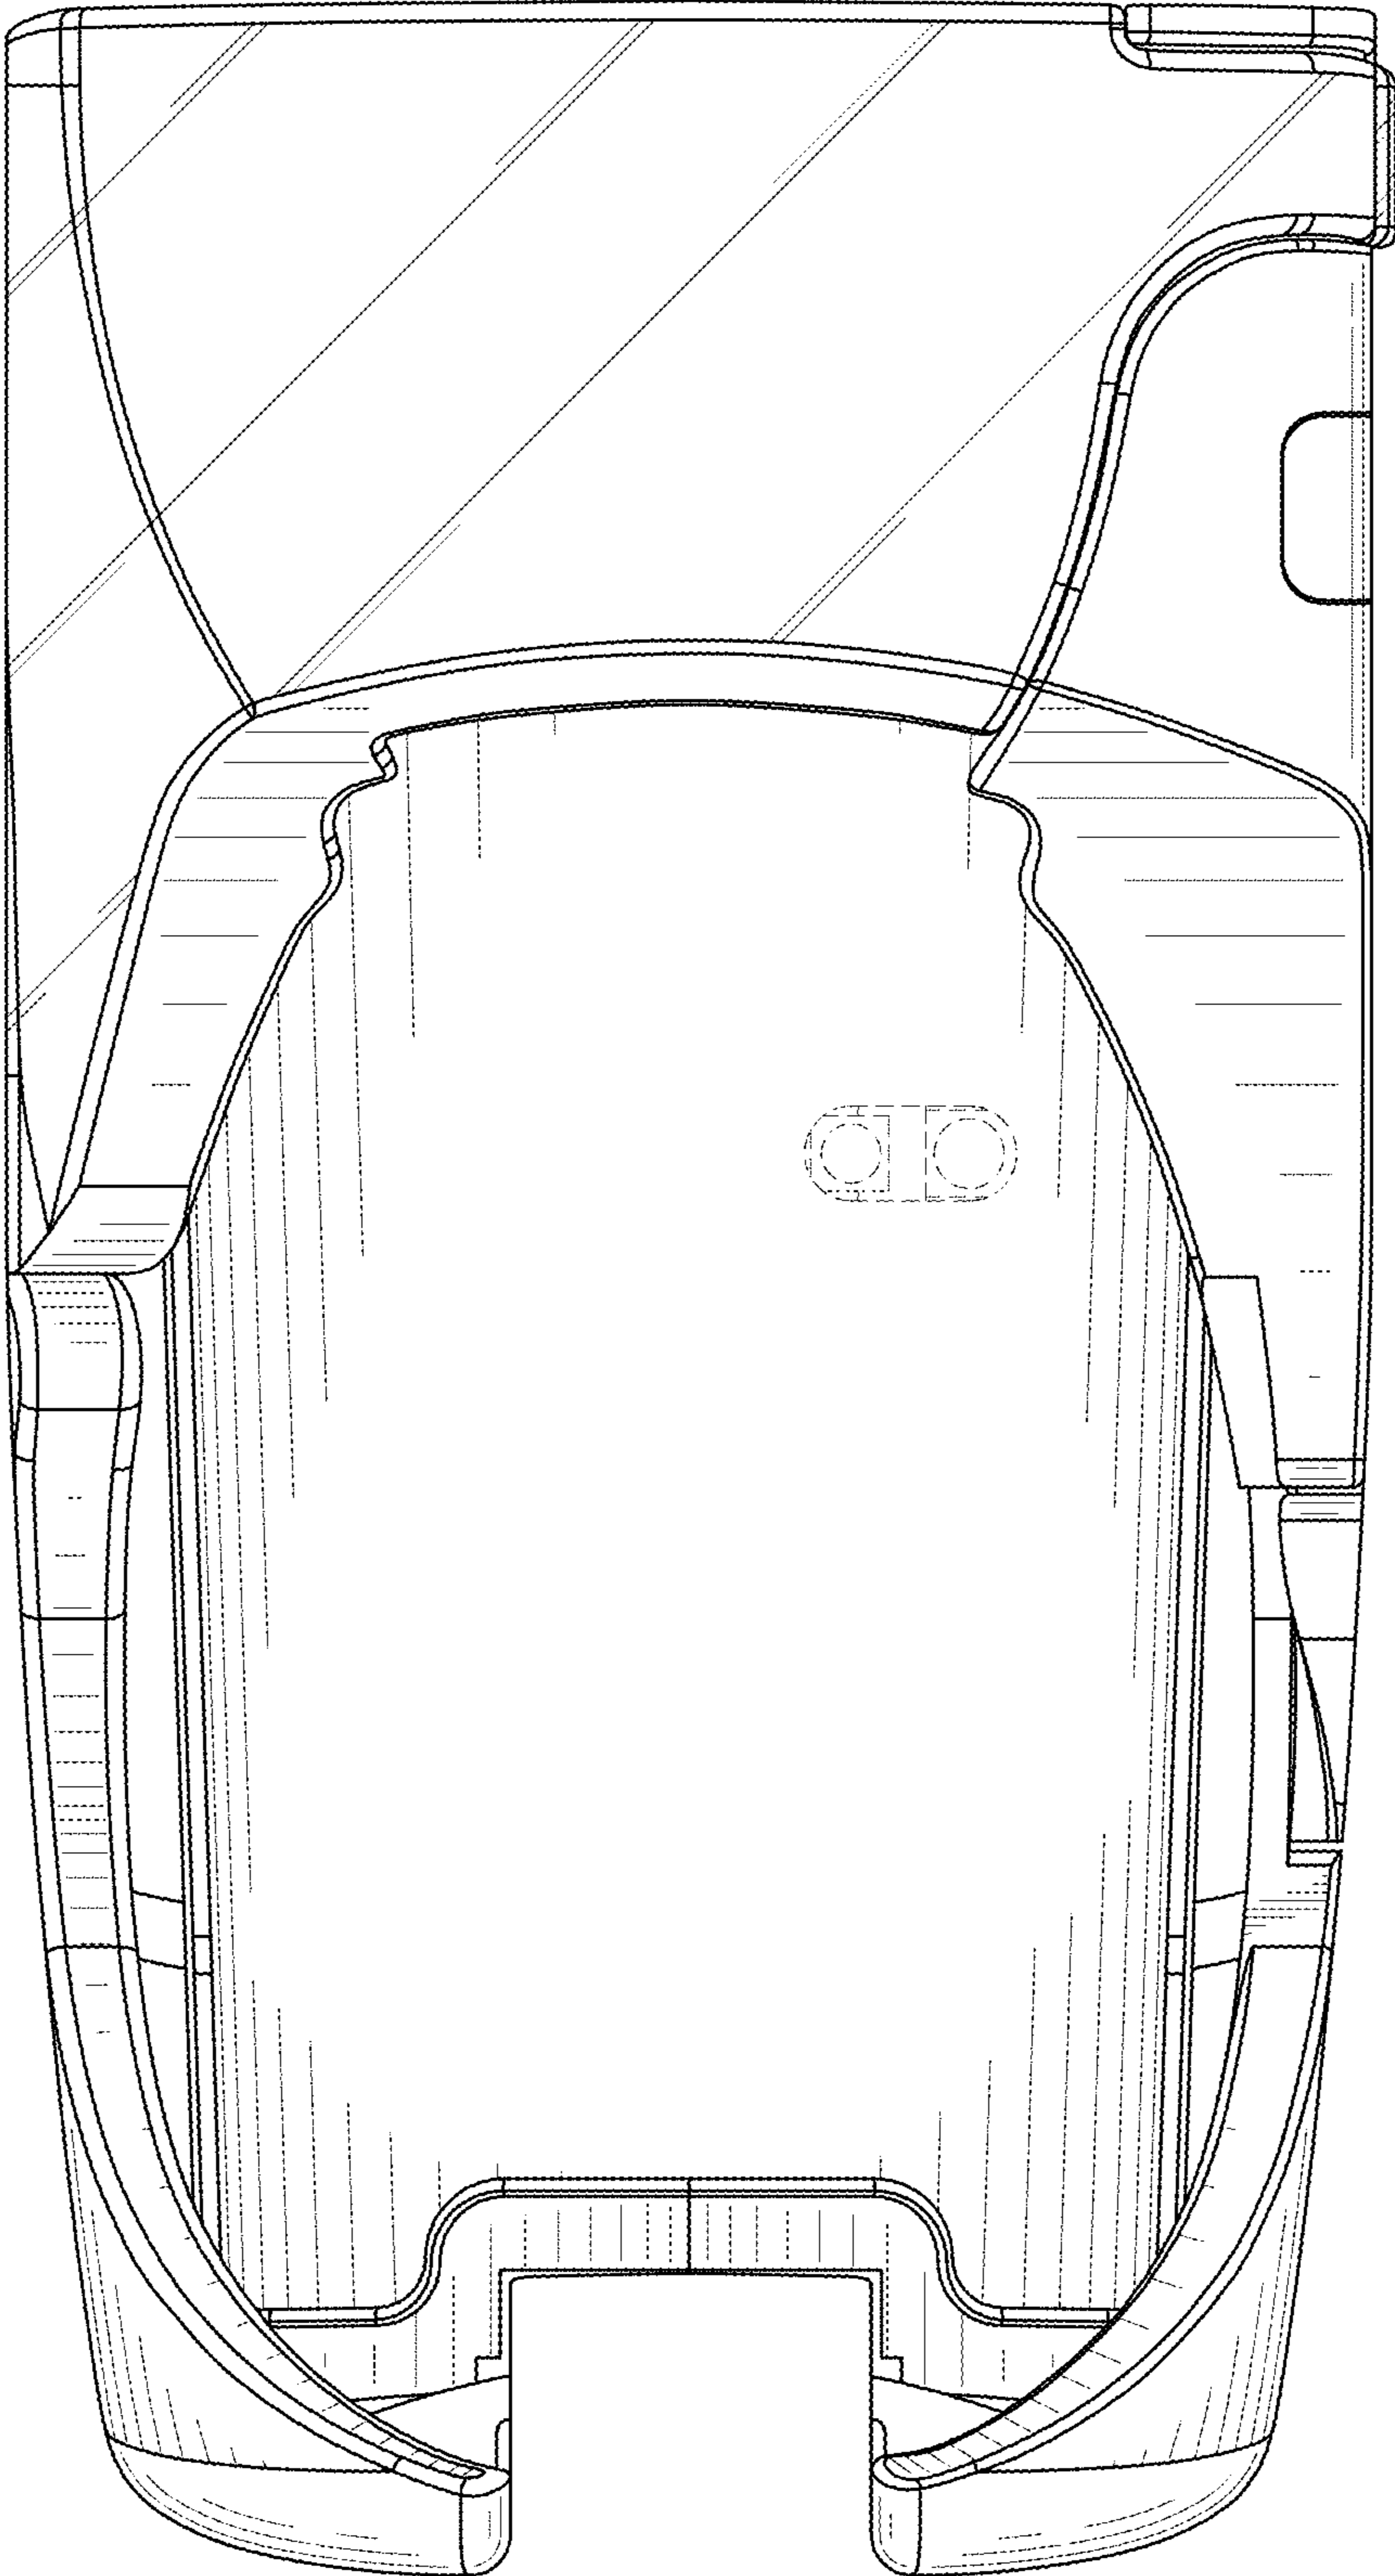


FIG. 3

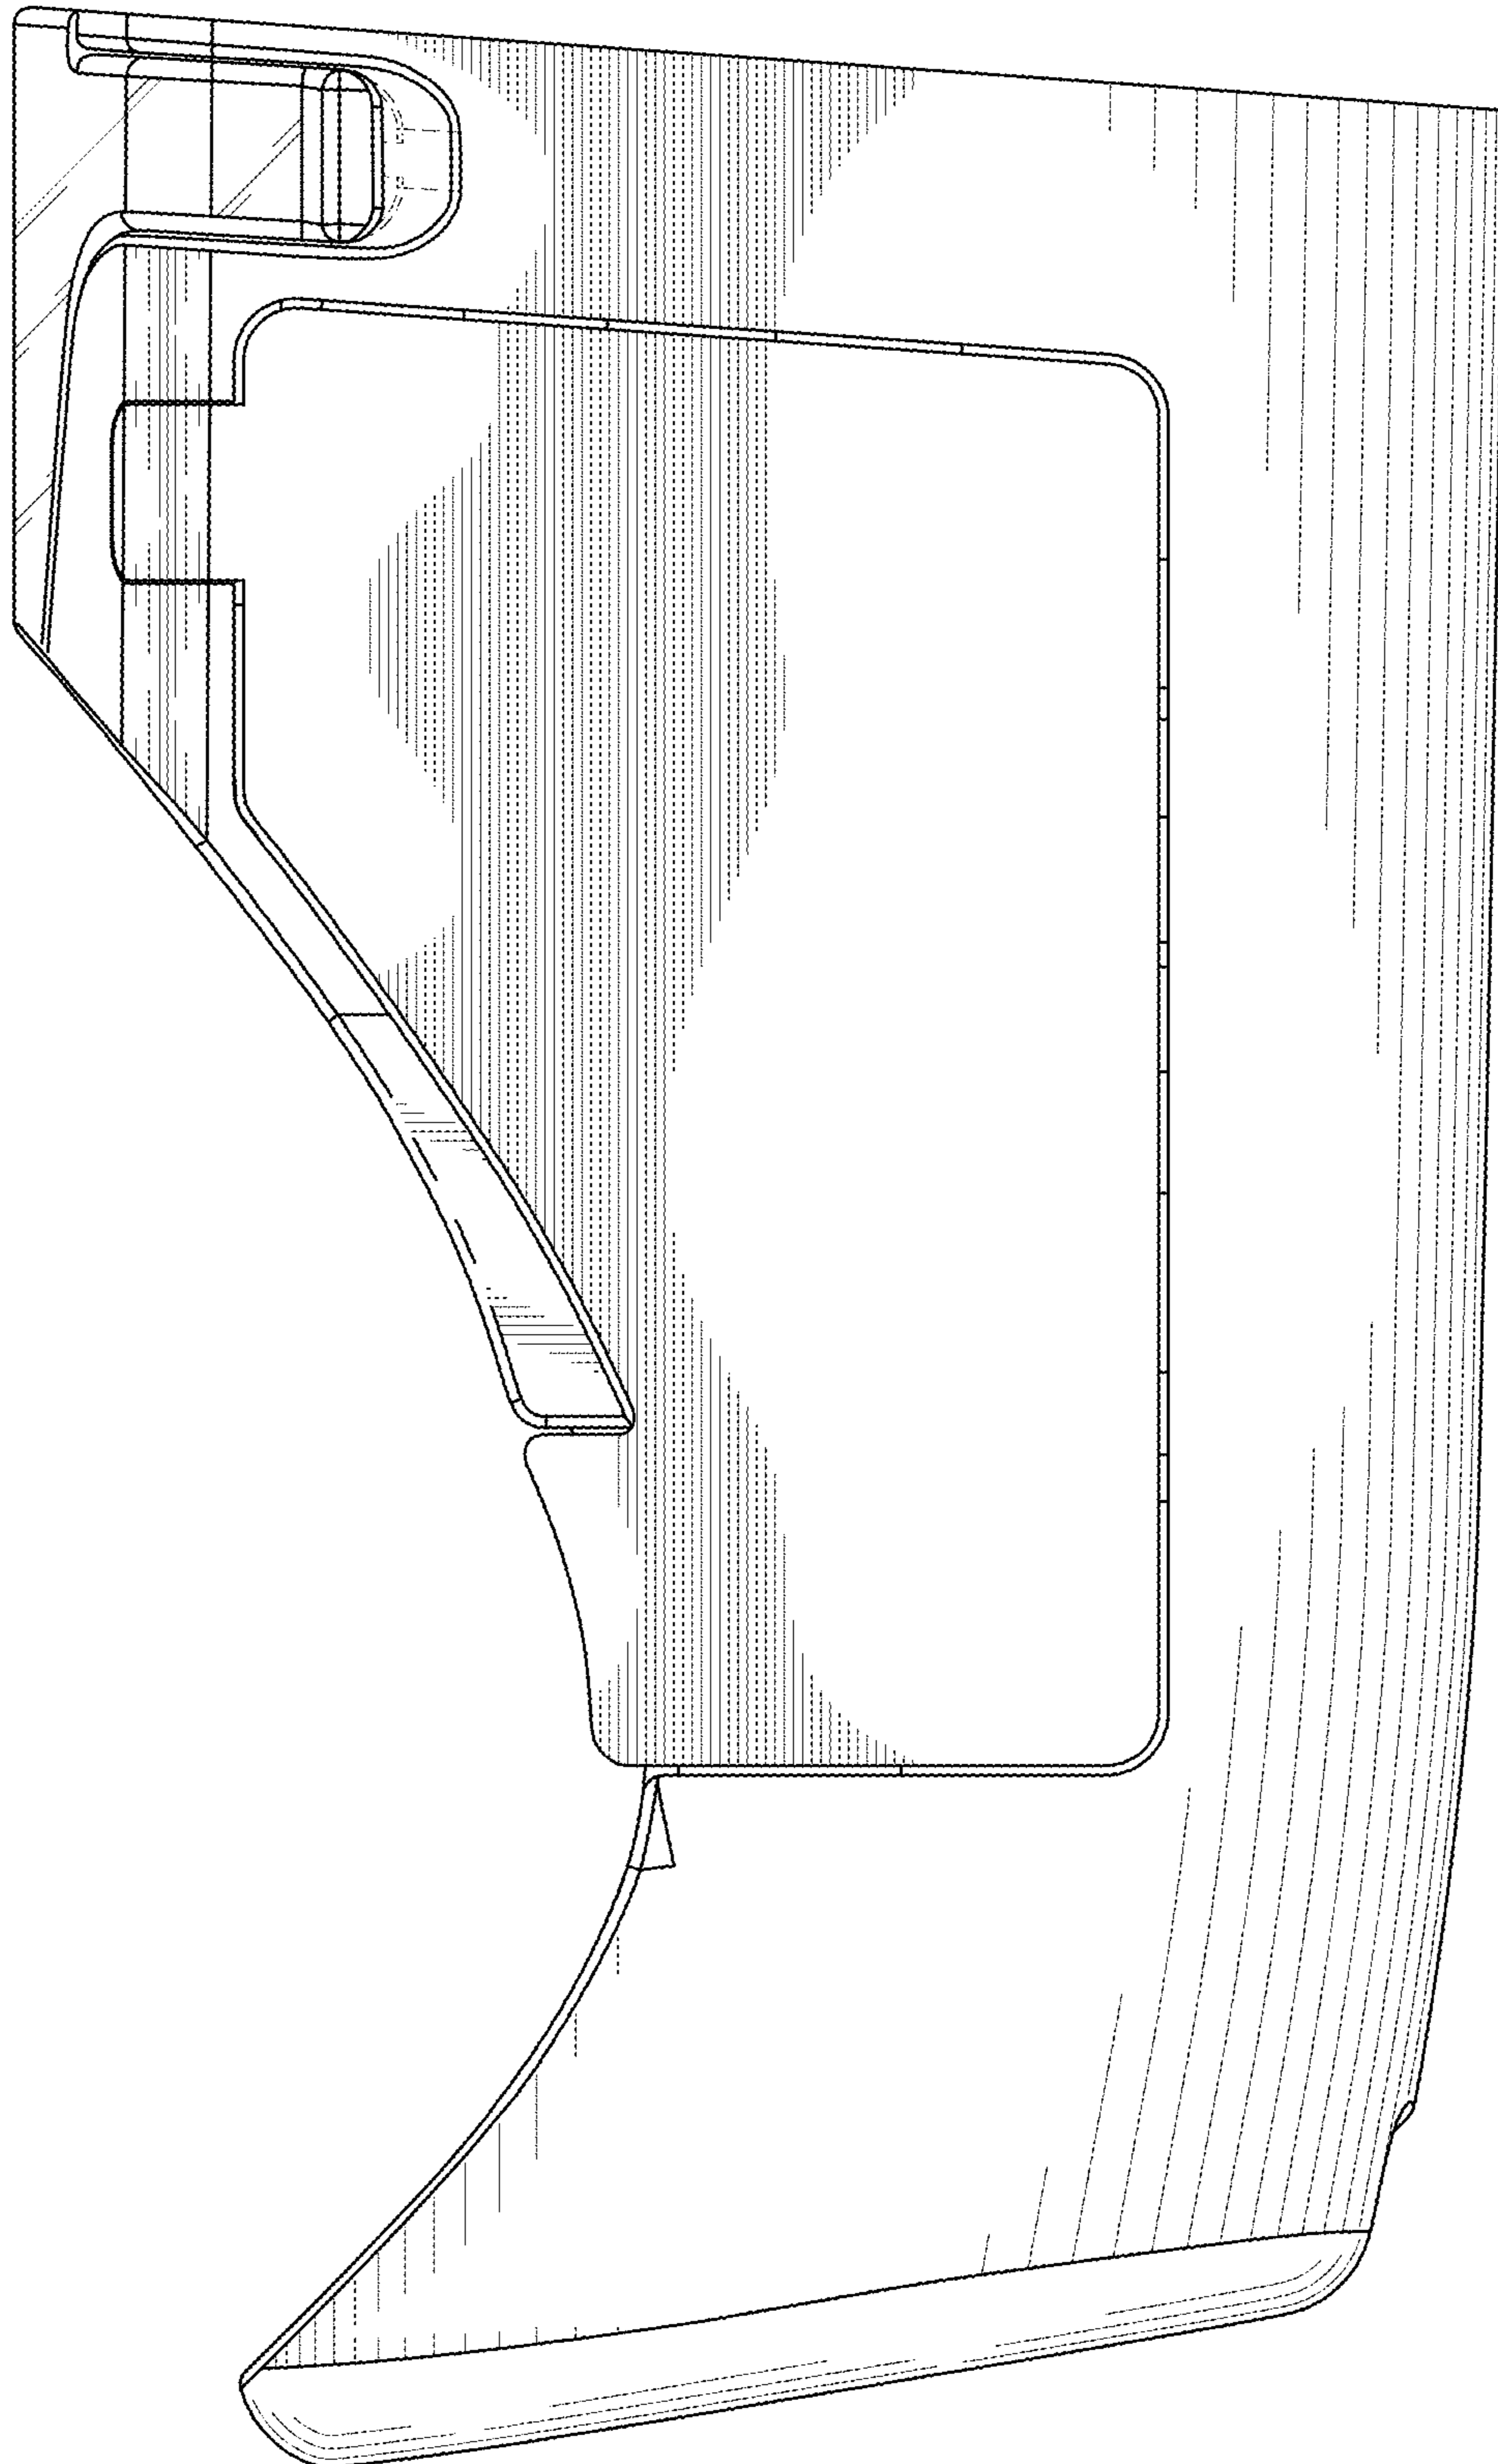


FIG. 4

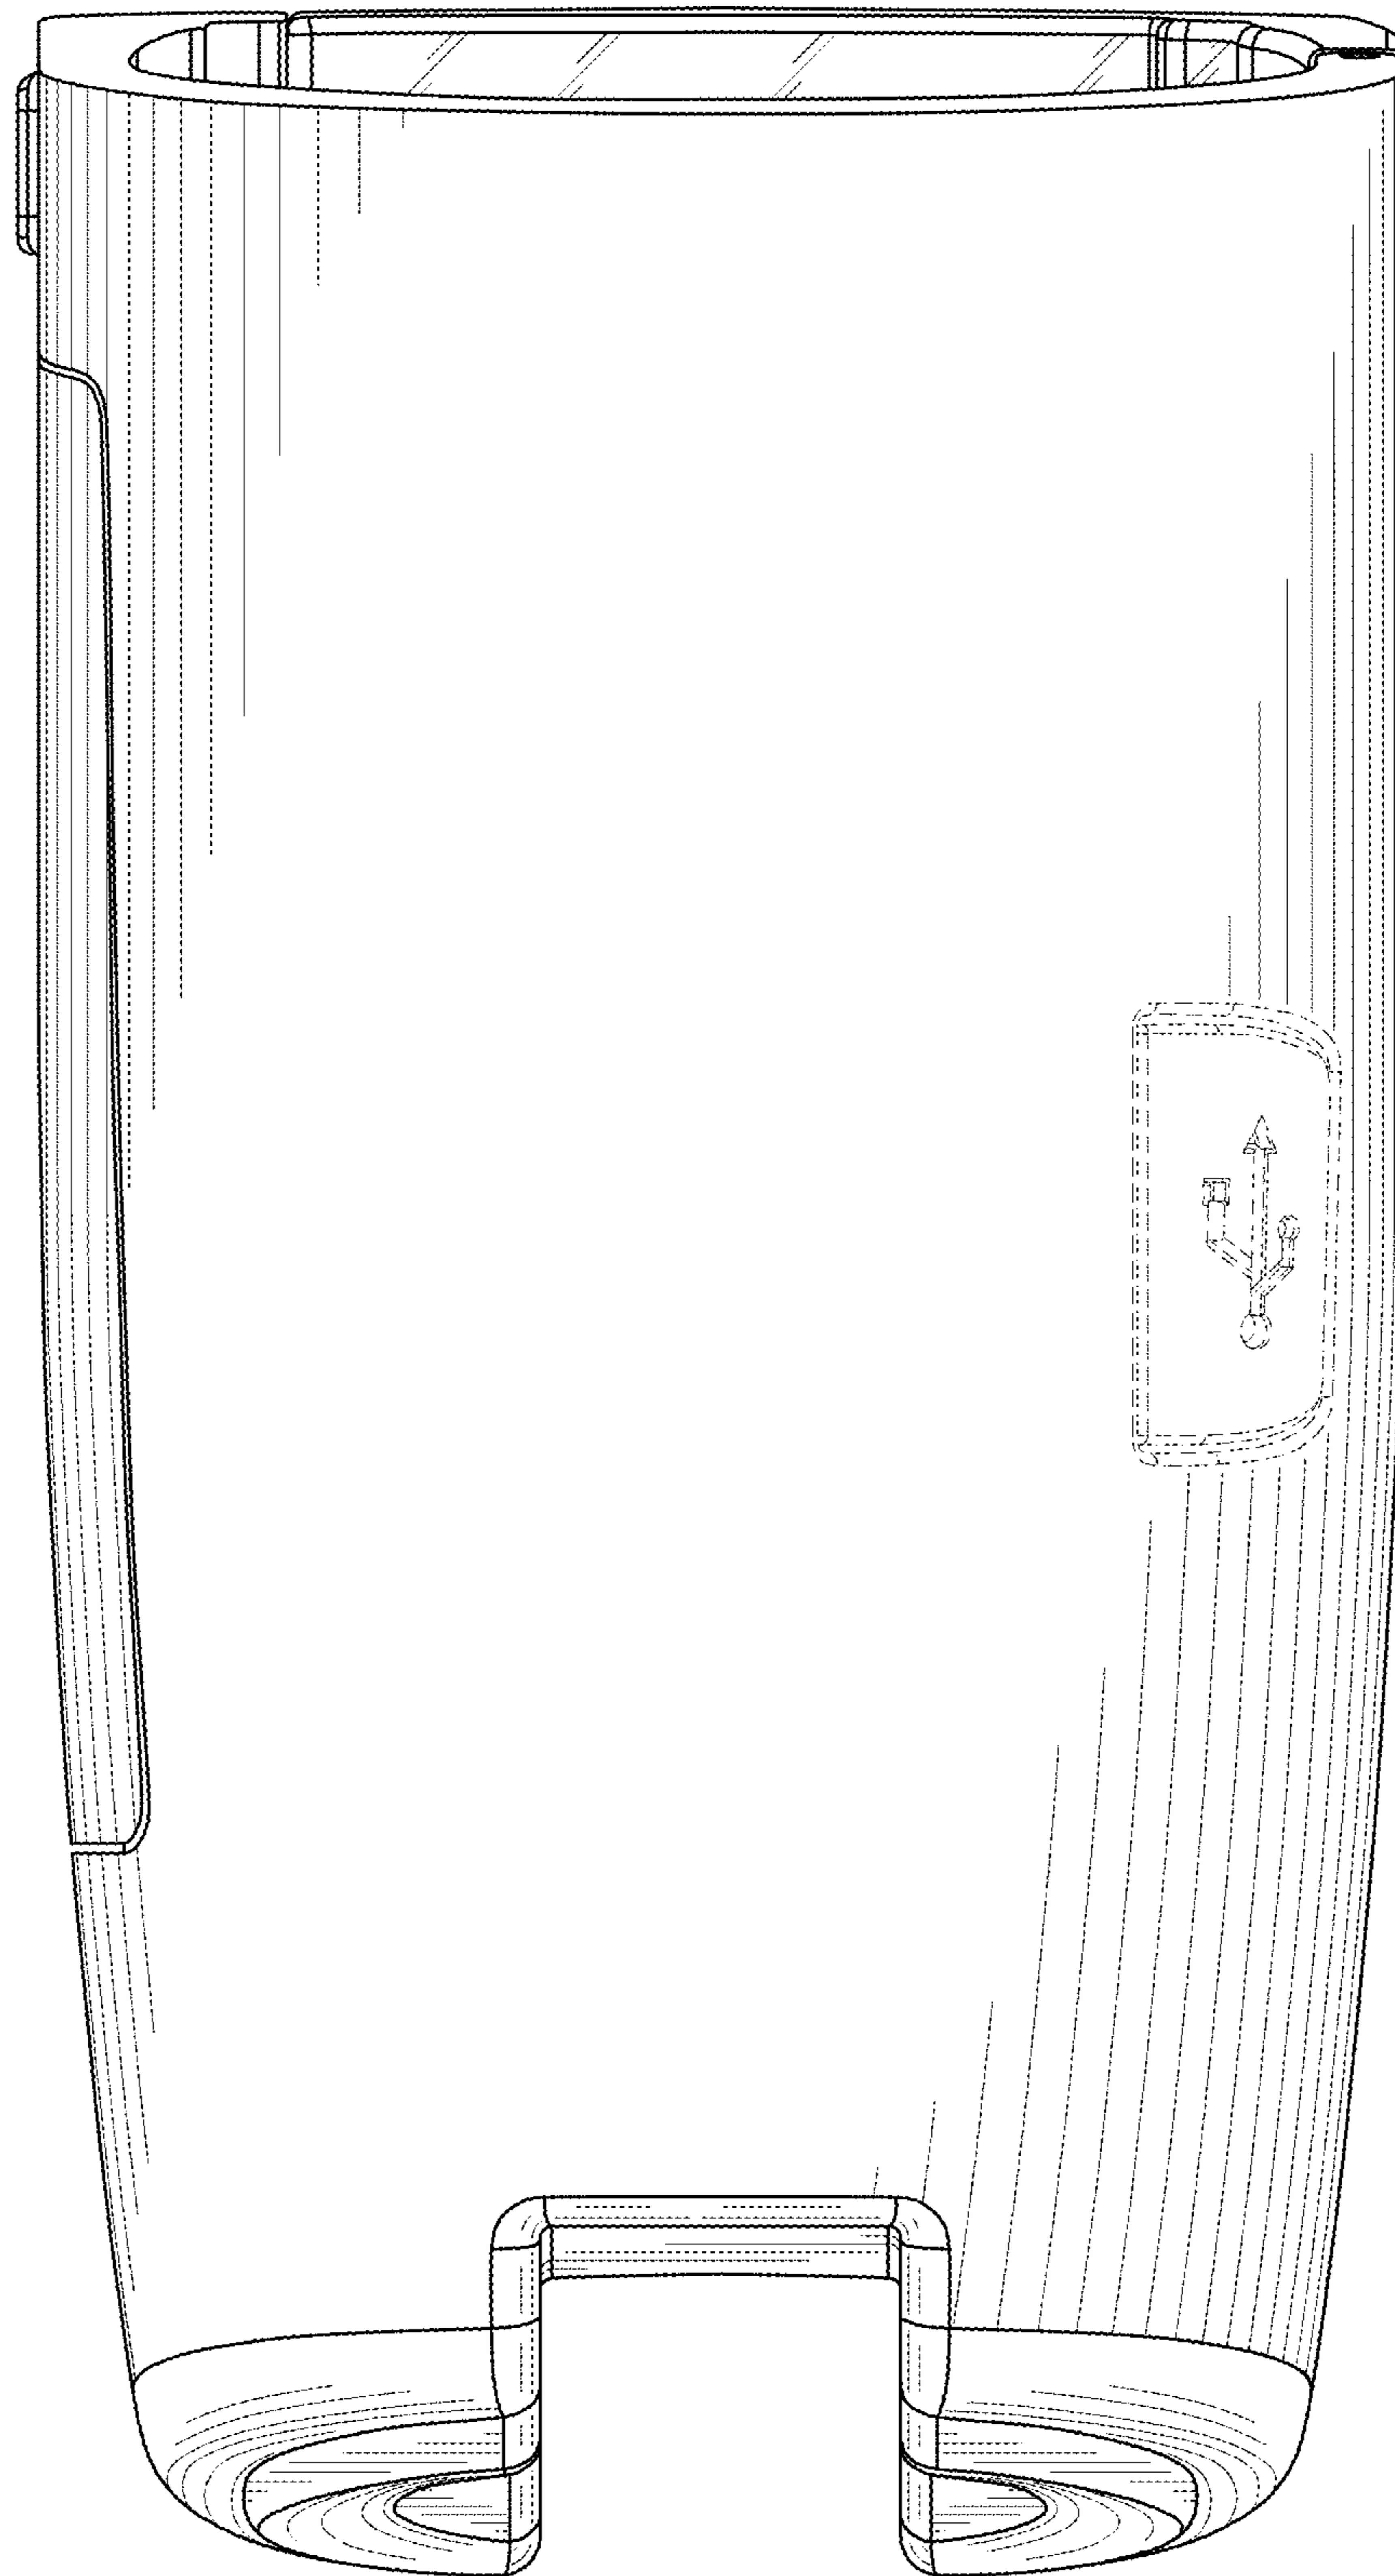


FIG. 5

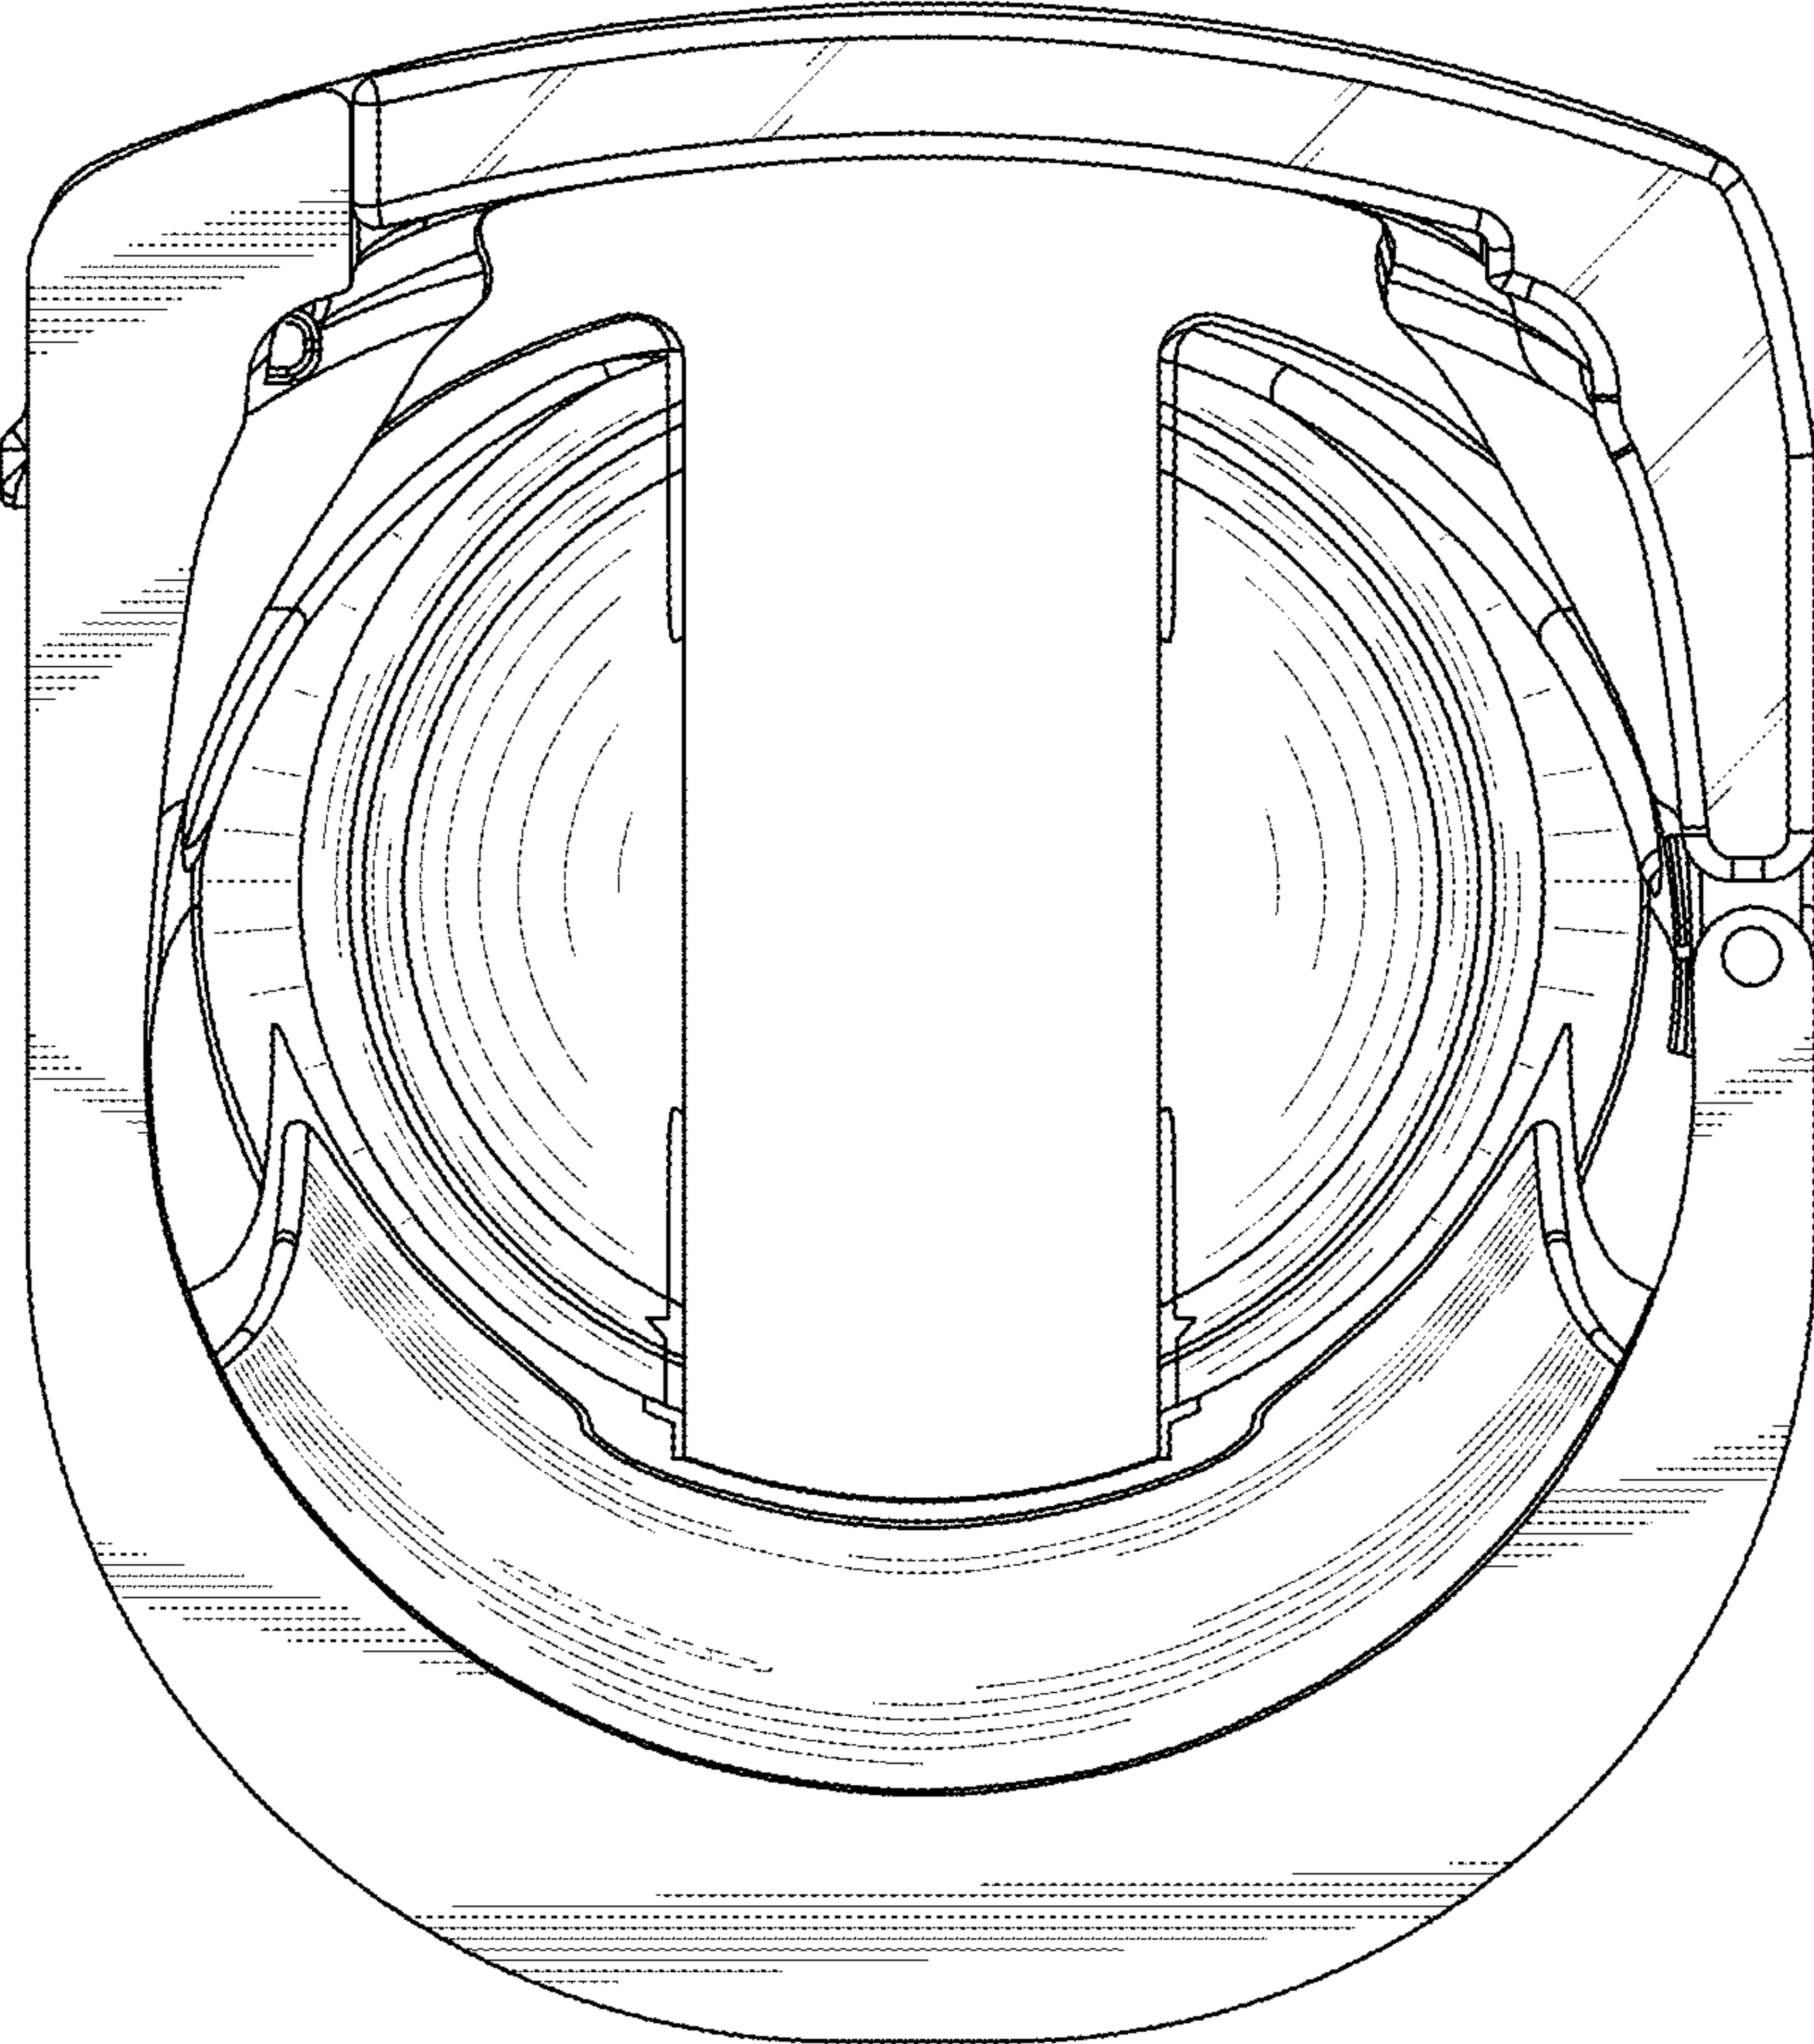




FIG. 6

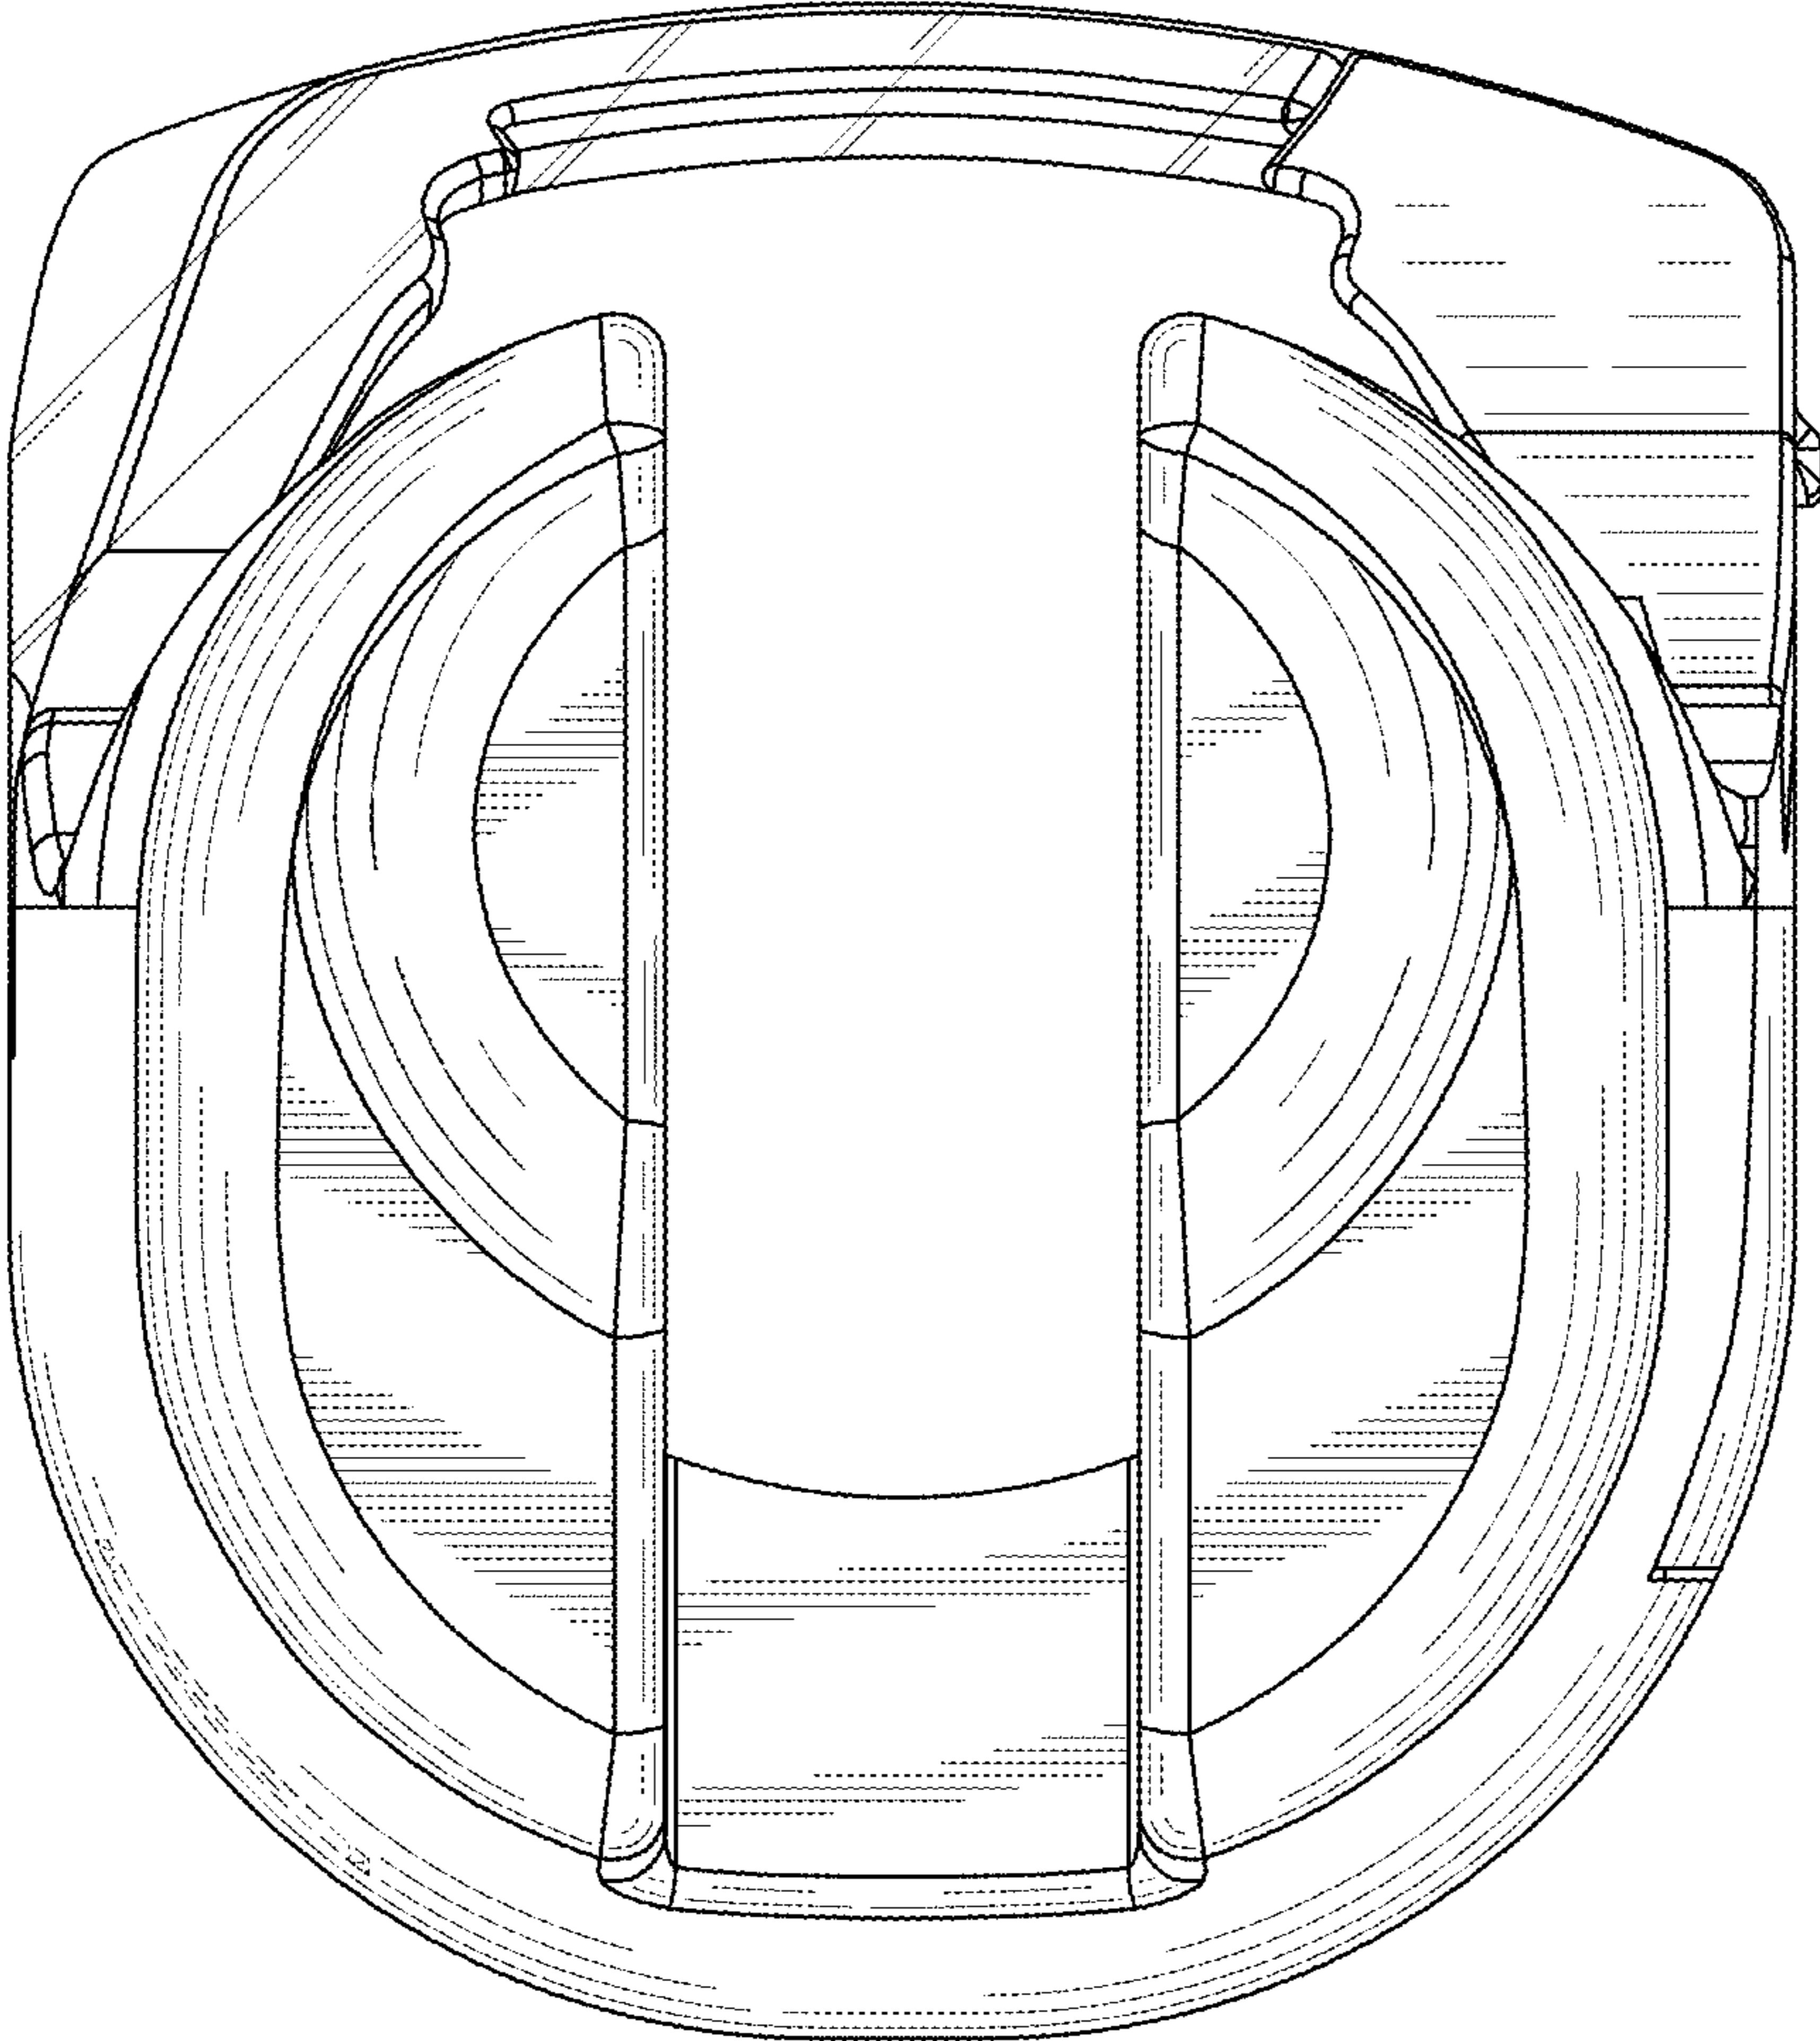




FIG. 7

