



US00D884189S

(12) **United States Design Patent** (10) **Patent No.:** **US D884,189 S**
Wassermann et al. (45) **Date of Patent:** **** May 12, 2020**

(54) **BLOOD TESTING APPARATUS**
(71) Applicant: **Roche Diagnostics Operations, Inc.**,
Indianapolis, IN (US)
(72) Inventors: **Johann Florian Wassermann**,
Rotkreuz (CH); **Roman Gebhard**,
Munich (DE); **Samuel Coendet**,
Munich (DE)

D648,029 S 11/2011 Presta et al.
D670,810 S * 11/2012 Fukuzawa D24/169
8,427,817 B2 4/2013 Lewis et al.
8,515,775 B2 8/2013 Galley et al.
D690,422 S 9/2013 Oka
D696,404 S 12/2013 Golnik et al.

(Continued)

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Dinsmore & Shohl LLP

(73) Assignee: **Roche Diagnostics Operations, Inc.**,
Indianapolis, IN (US)
(**) Term: **15 Years**

(57) **CLAIM**
The ornamental design for a blood testing apparatus, as shown and described.


(21) Appl. No.: **29/650,825**
(22) Filed: **Jun. 11, 2018**
(30) **Foreign Application Priority Data**
Dec. 15, 2017 (EP) 004548766-0001
Dec. 15, 2017 (EP) 004548766-0002
(51) **LOC (12) Cl.** **24-01**
(52) **U.S. Cl.**
USPC **D24/169**
(58) **Field of Classification Search**
USPC D24/164–169, 186, 107, 216; D10/81
CPC A61B 5/14532; A61B 5/14865; A61B
2560/0412; A61B 2560/0443; A61B
2560/0462; A61M 25/0606; A61M
25/0631
See application file for complete search history.

DESCRIPTION

FIG. 1 is a right side, front perspective view of a first embodiment of a blood testing apparatus showing of our new design;
FIG. 2 is a left side, rear perspective view thereof;
FIG. 3 is a front view thereof;
FIG. 4 is a rear view thereof;
FIG. 5 is a bottom plan view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a left side view thereof, the right side being the same;
FIG. 8 is a right side, front perspective view of a second embodiment of a blood testing apparatus showing our new design;
FIG. 9 is a left side, rear perspective view thereof;
FIG. 10 is a front view thereof;
FIG. 11 is a rear view thereof;
FIG. 12 is a bottom plan view thereof;
FIG. 13 is a top plan view thereof; and,
FIG. 14 is a left side view thereof.
In FIGS. 8-14, the difference in shading represents surfaces having the contrast in appearance shown.
The broken lines in the drawing views illustrate portions of the blood testing apparatus that form no part of the claimed design.

(56) **References Cited**
U.S. PATENT DOCUMENTS
5,281,395 A * 1/1994 Markart G01N 21/8483
235/375
D406,895 S 3/1999 Byrd et al.
D493,536 S 7/2004 Jaeck et al.
D545,436 S 6/2007 Padain
D627,068 S 11/2010 Brauer et al.

1 Claim, 14 Drawing Sheets

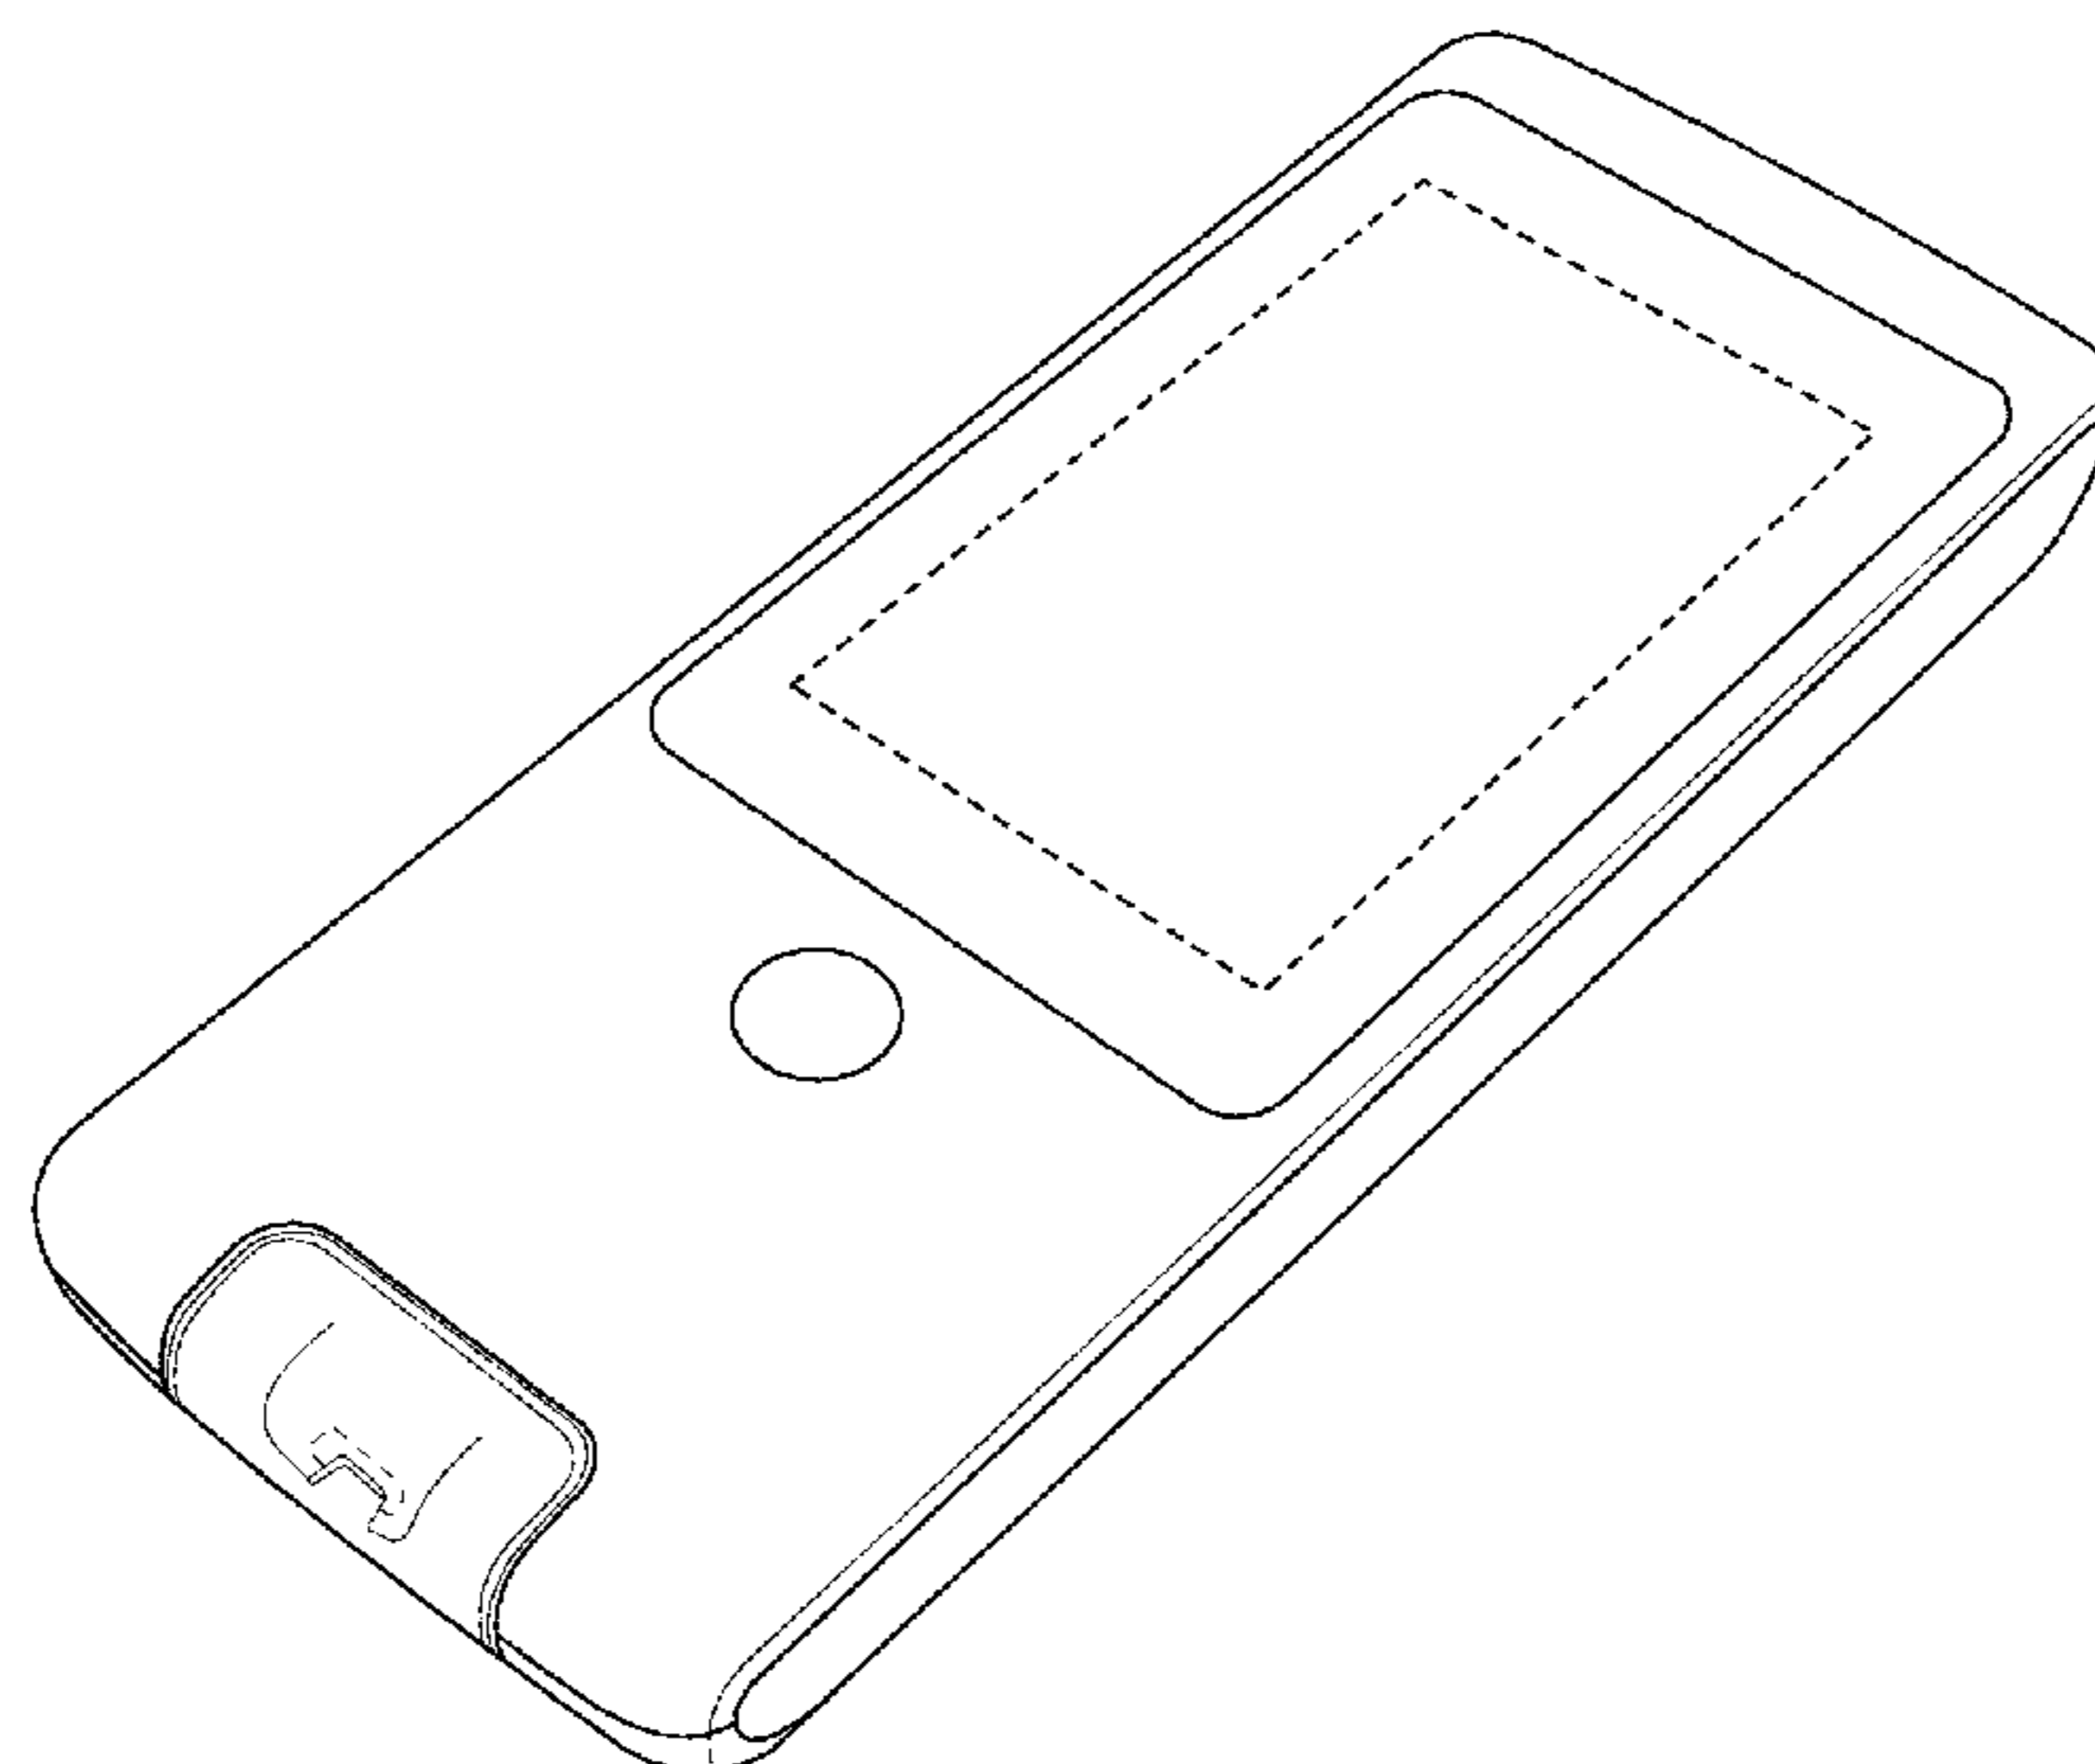

(56)

References Cited

U.S. PATENT DOCUMENTS

D721,177 S	1/2015	Ahlstrom et al.	
D721,178 S	1/2015	Harkin et al.	
D723,695 S	3/2015	Chung	
D724,223 S	3/2015	Nishiyama et al.	
9,022,931 B2	5/2015	Brauer et al.	
D734,468 S	7/2015	Murakami et al.	
D739,945 S	9/2015	Cadio et al.	
D747,490 S	1/2016	Harkin et al.	
D766,442 S	9/2016	Prais et al.	
D787,067 S	5/2017	Wightmann et al.	
D794,803 S	8/2017	Thom	
9,717,452 B2 *	8/2017	Roe	A61B 5/150022
D804,033 S	11/2017	Wightmann et al.	
D822,216 S *	7/2018	Barker	D24/186
2012/0095316 A1	4/2012	Lewis et al.	
2012/0095318 A1	4/2012	Galley et al.	
2012/0095691 A1	4/2012	Galley et al.	
2012/0165640 A1	6/2012	Galley et al.	
2012/0266251 A1	10/2012	Birtwhistle et al.	
2017/0138929 A1 *	5/2017	Lee	A61B 5/145

* cited by examiner

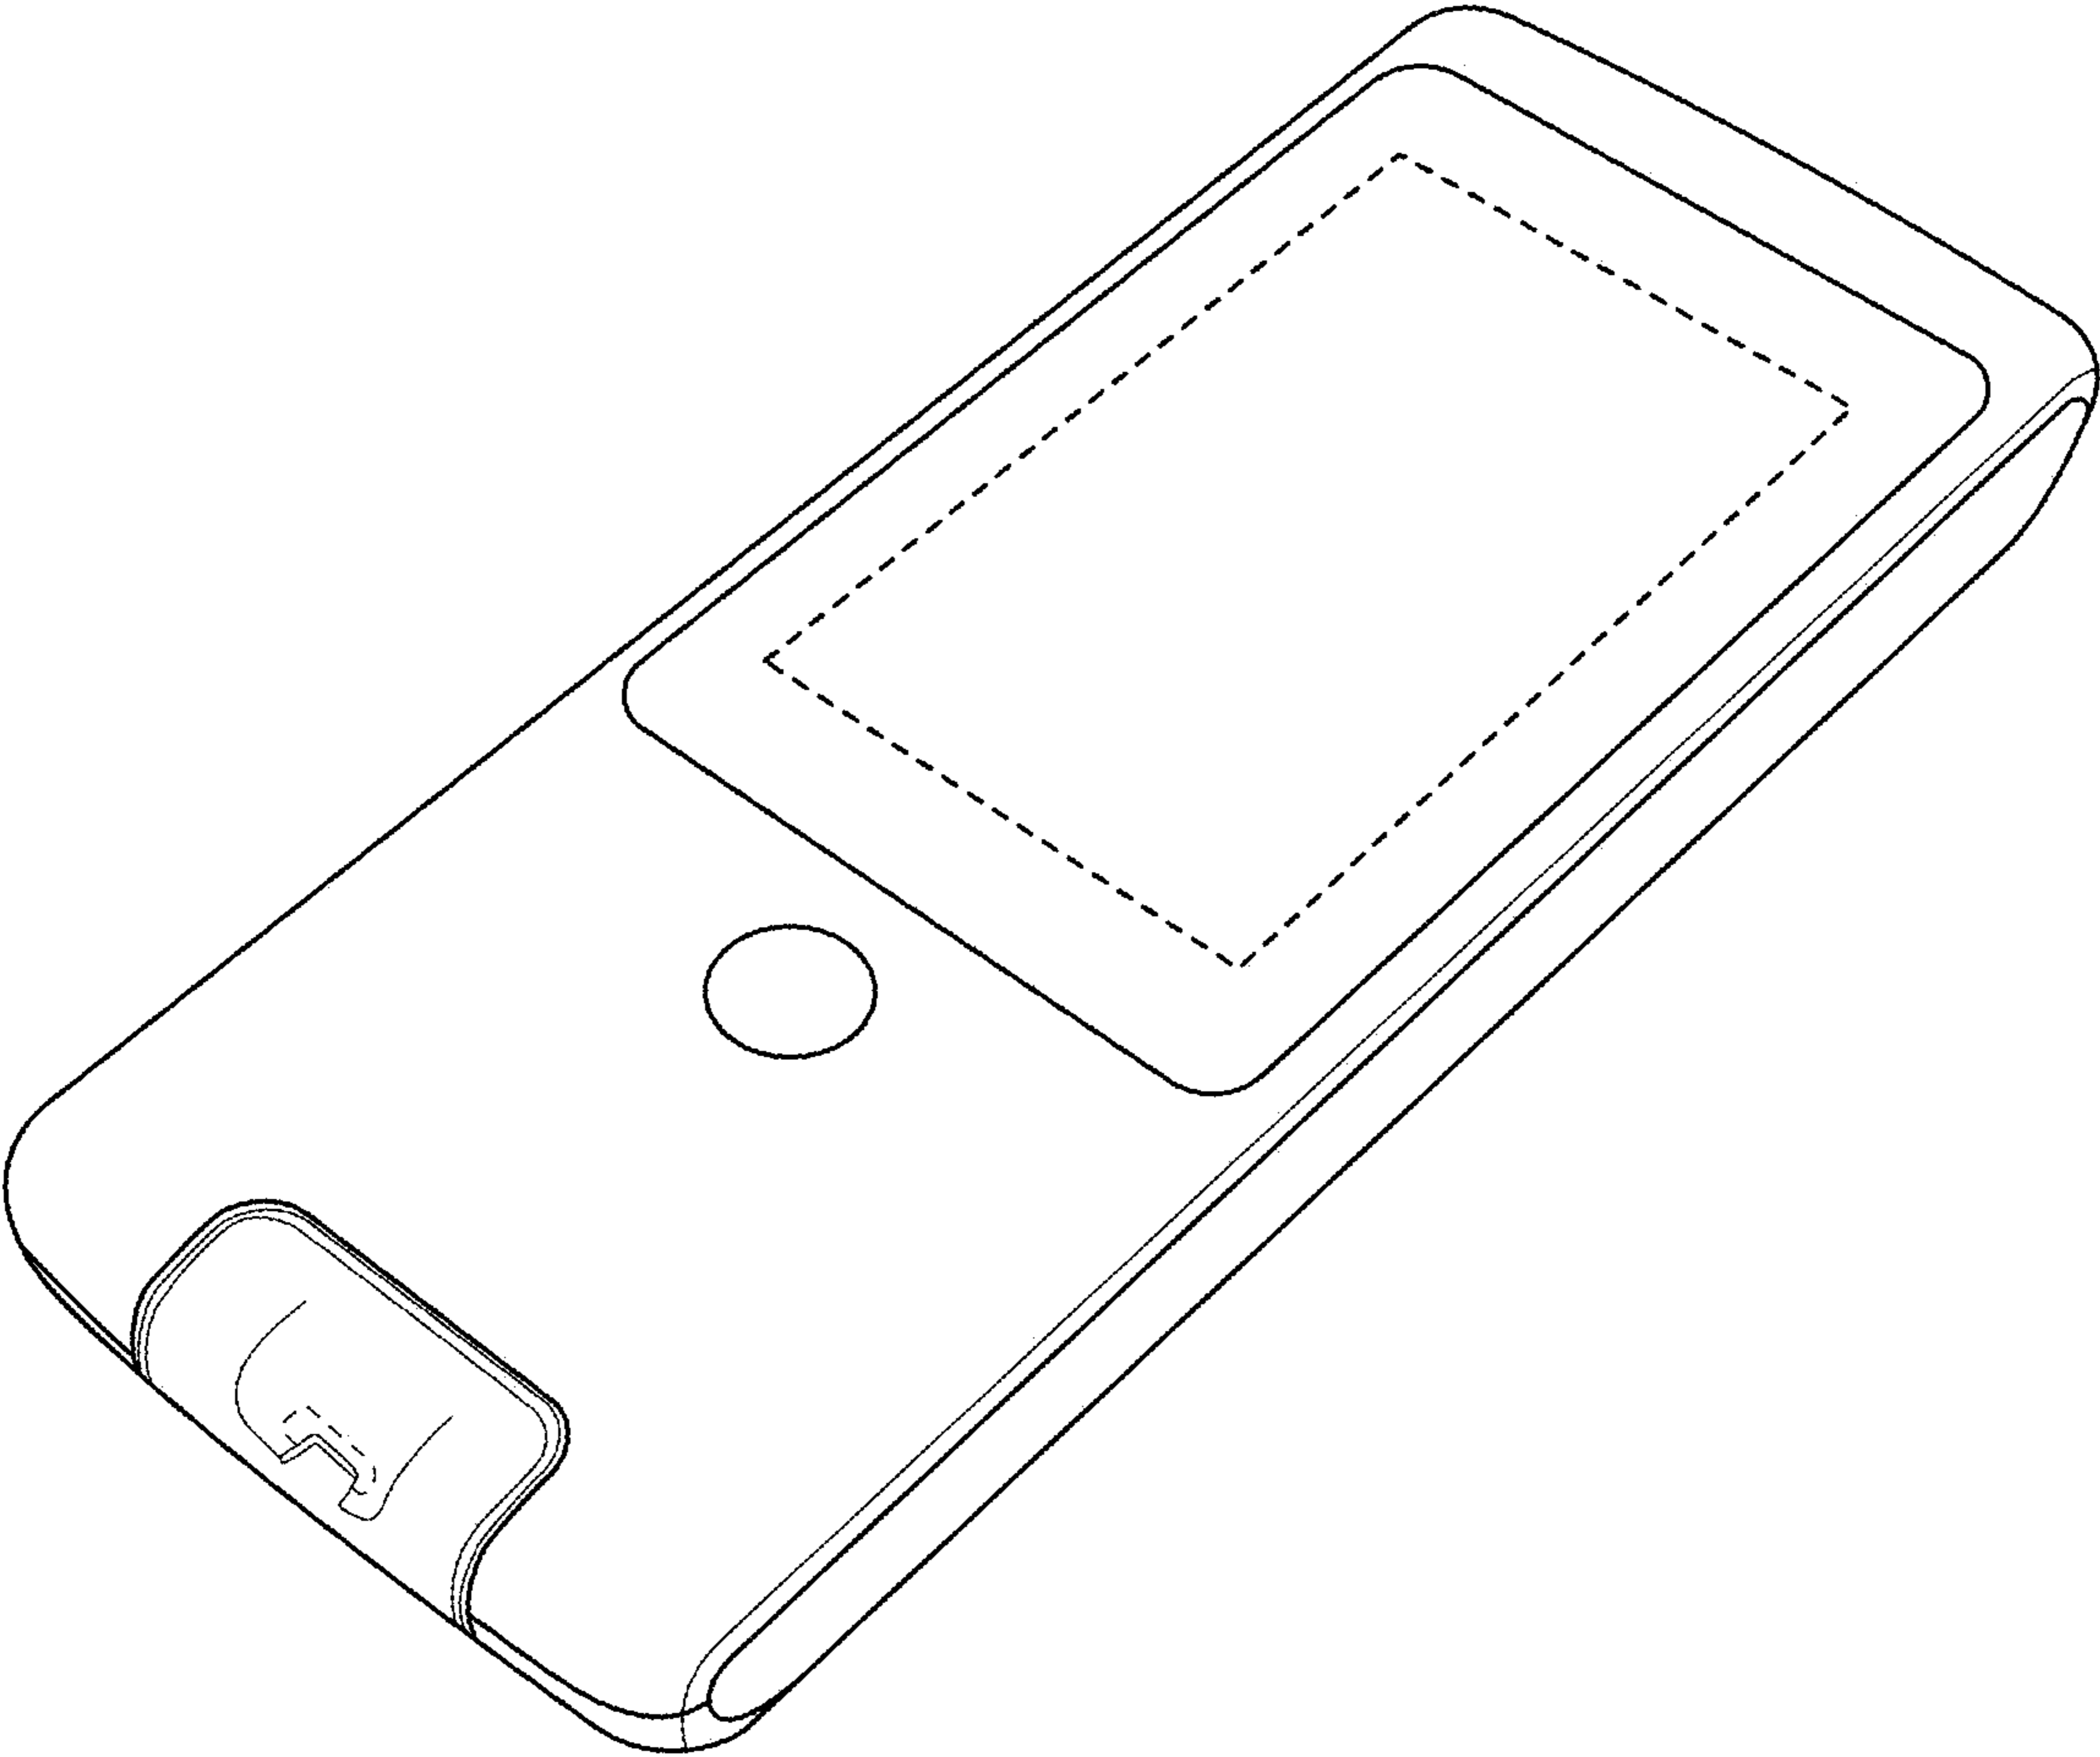


FIG. 1

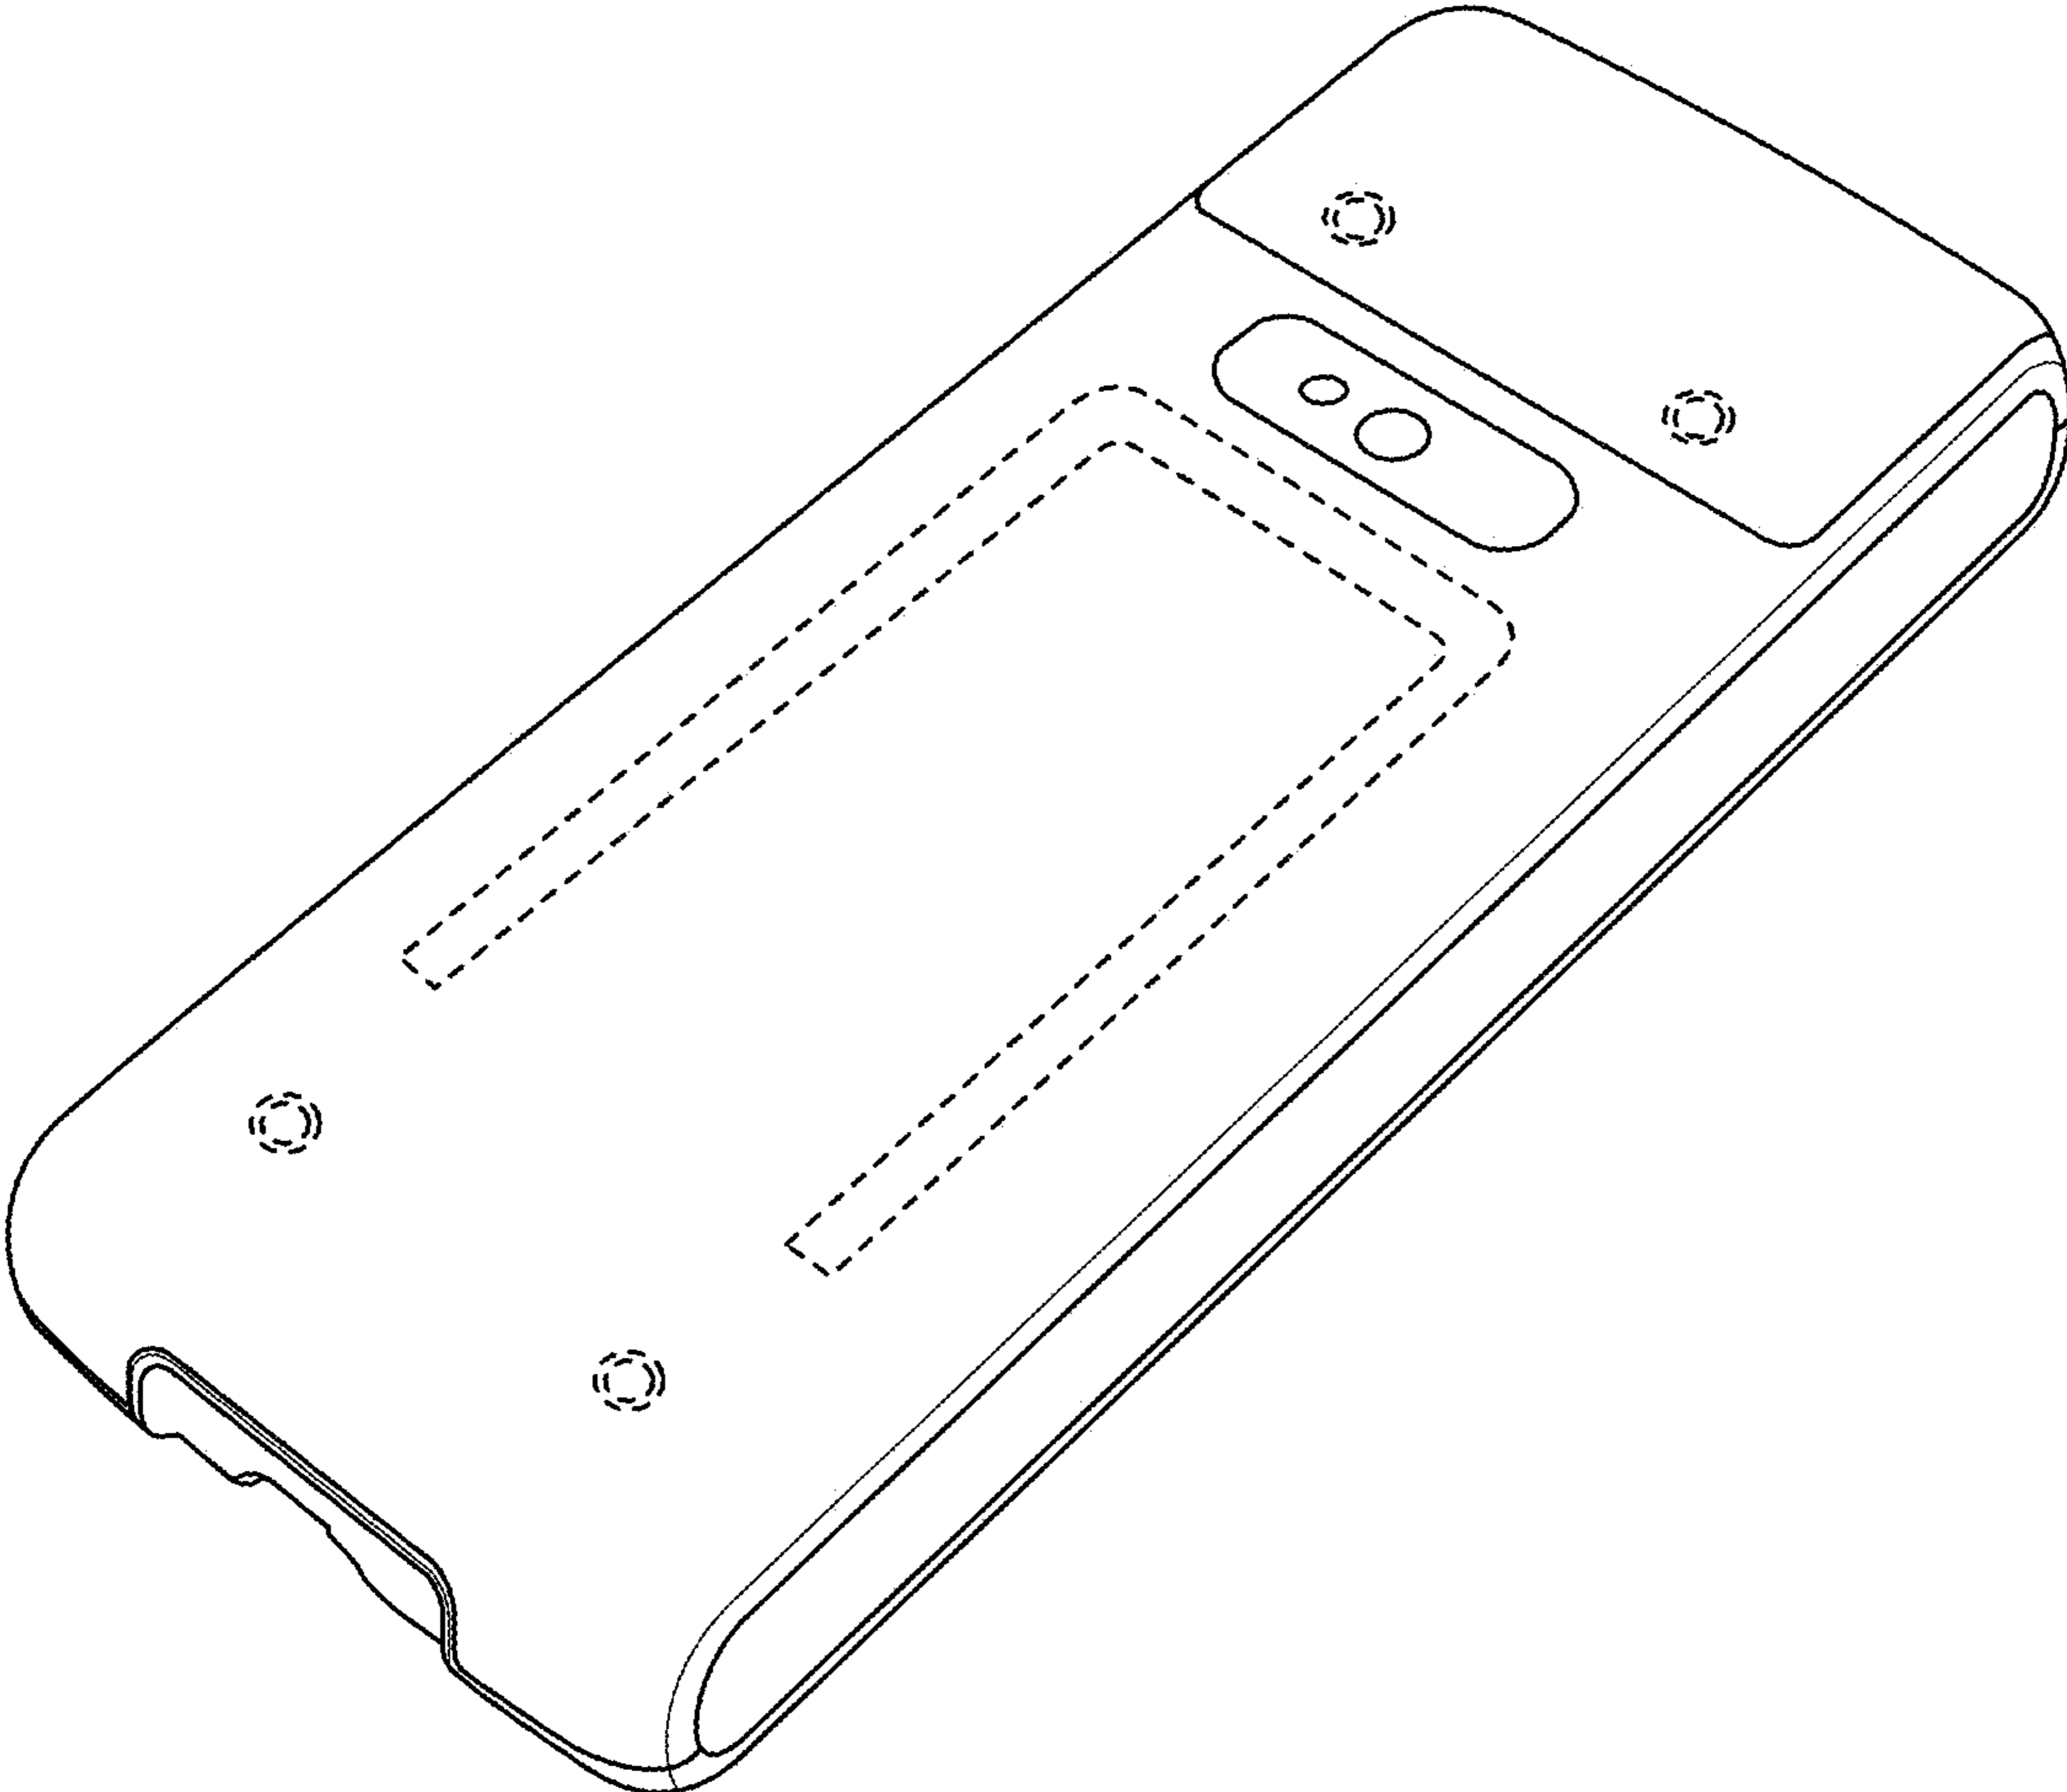


FIG. 2

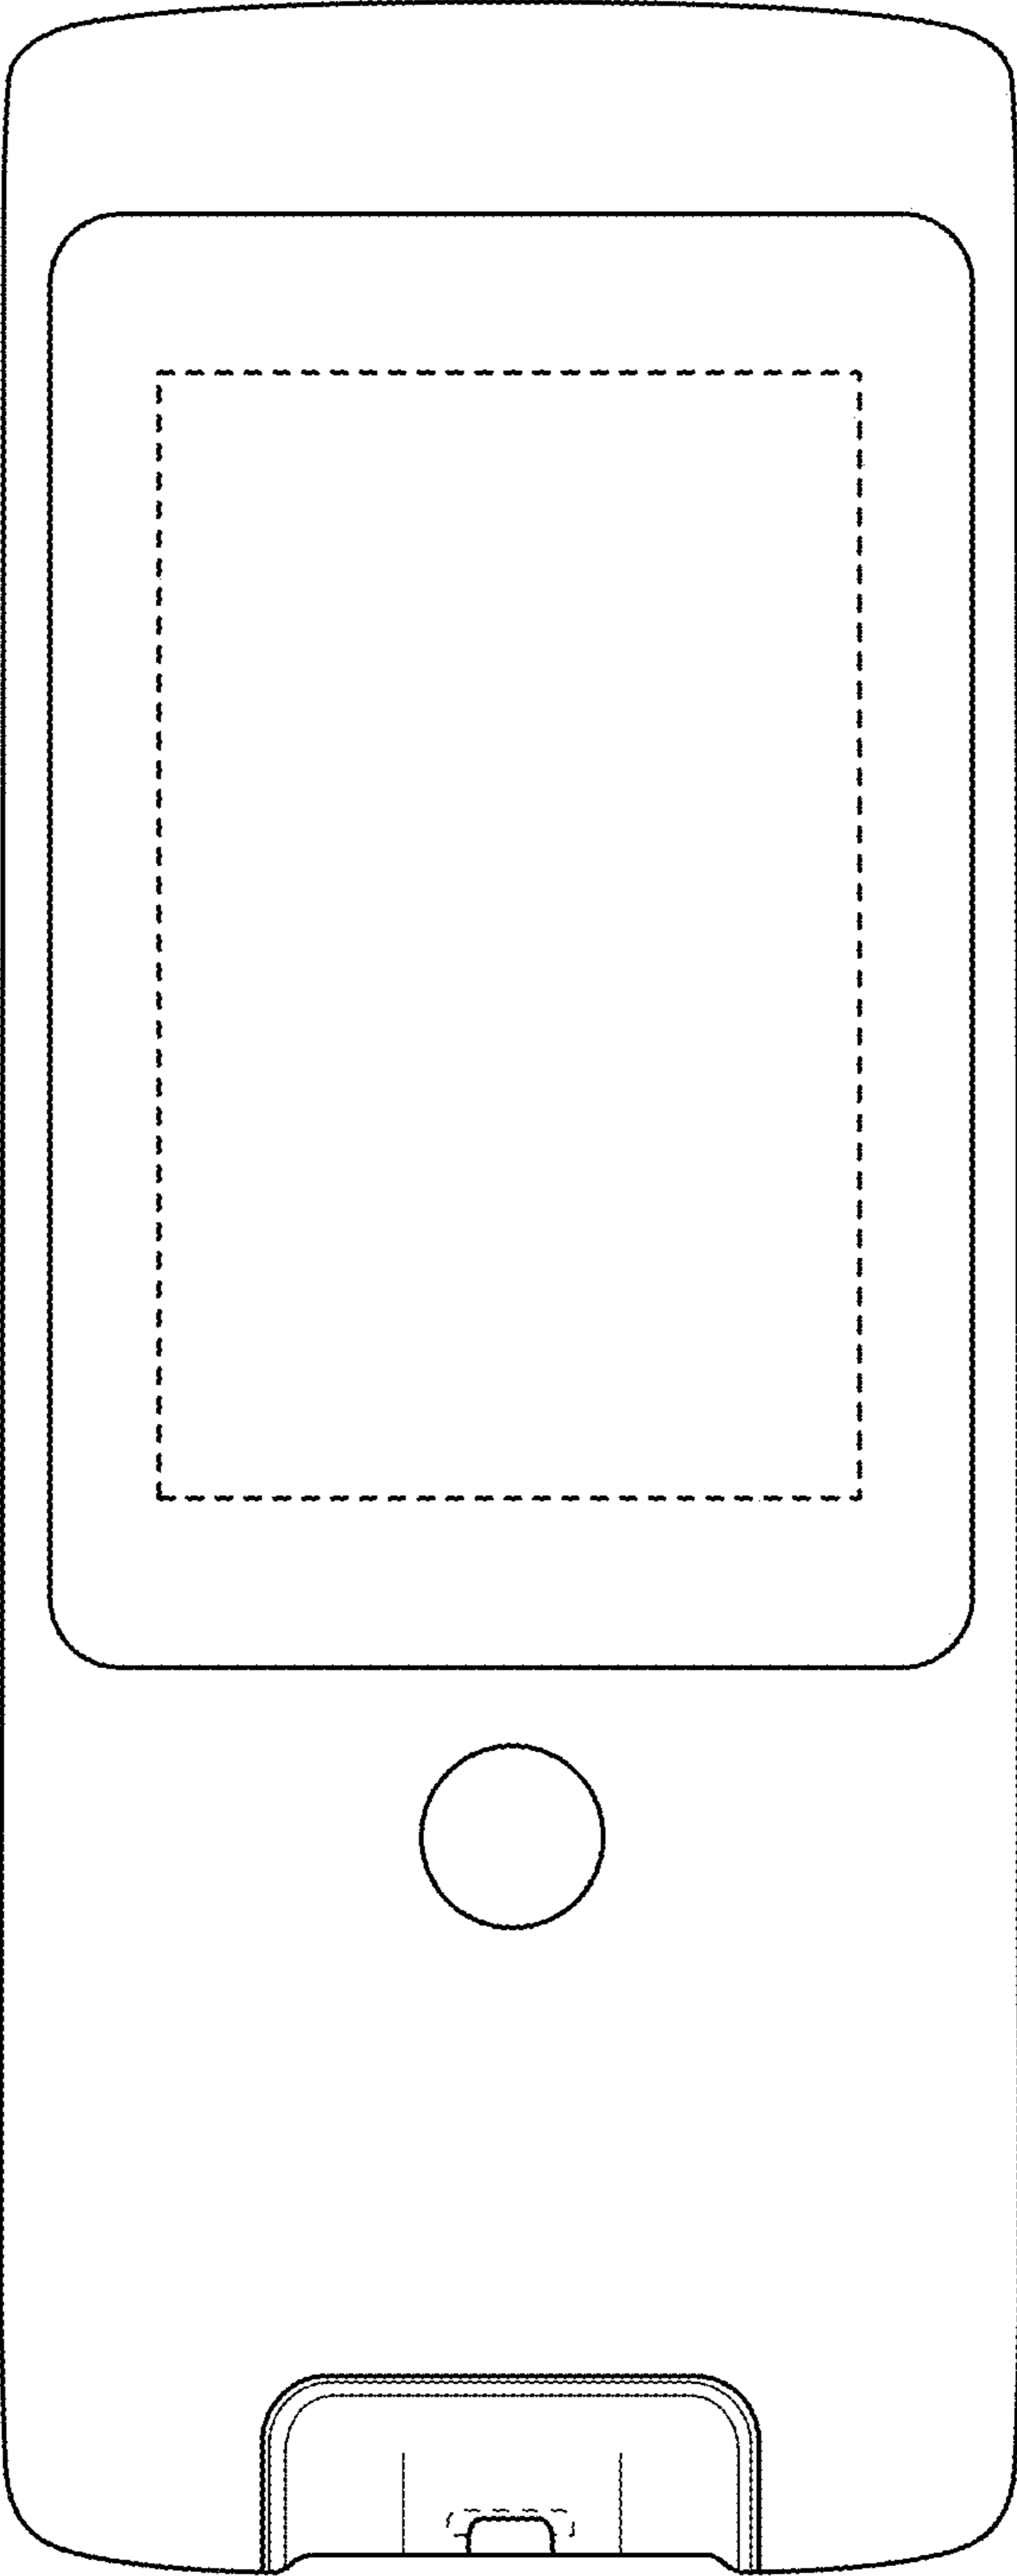


FIG. 3

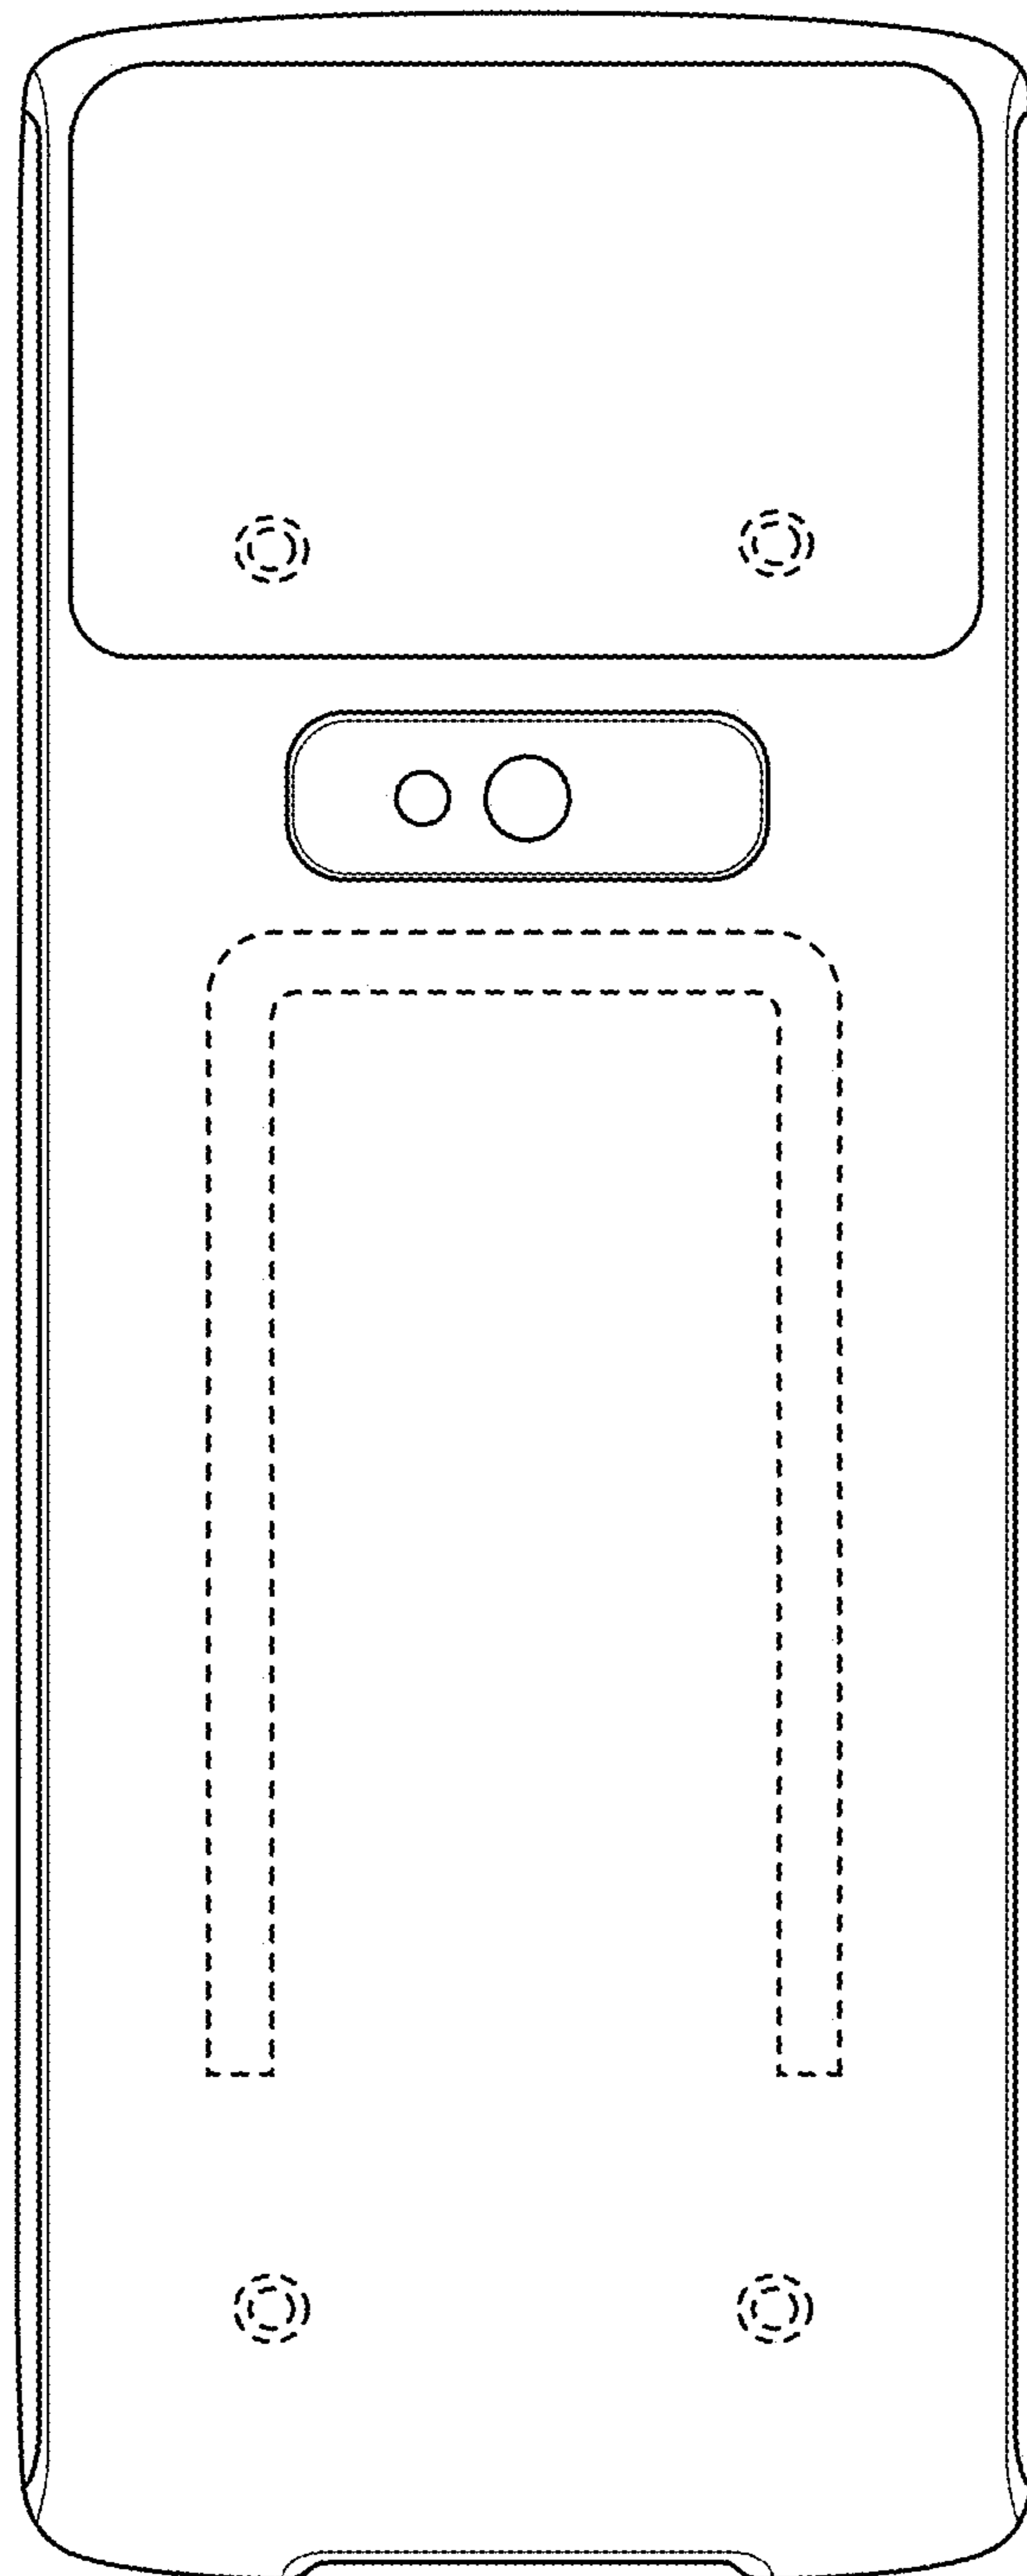


FIG. 4

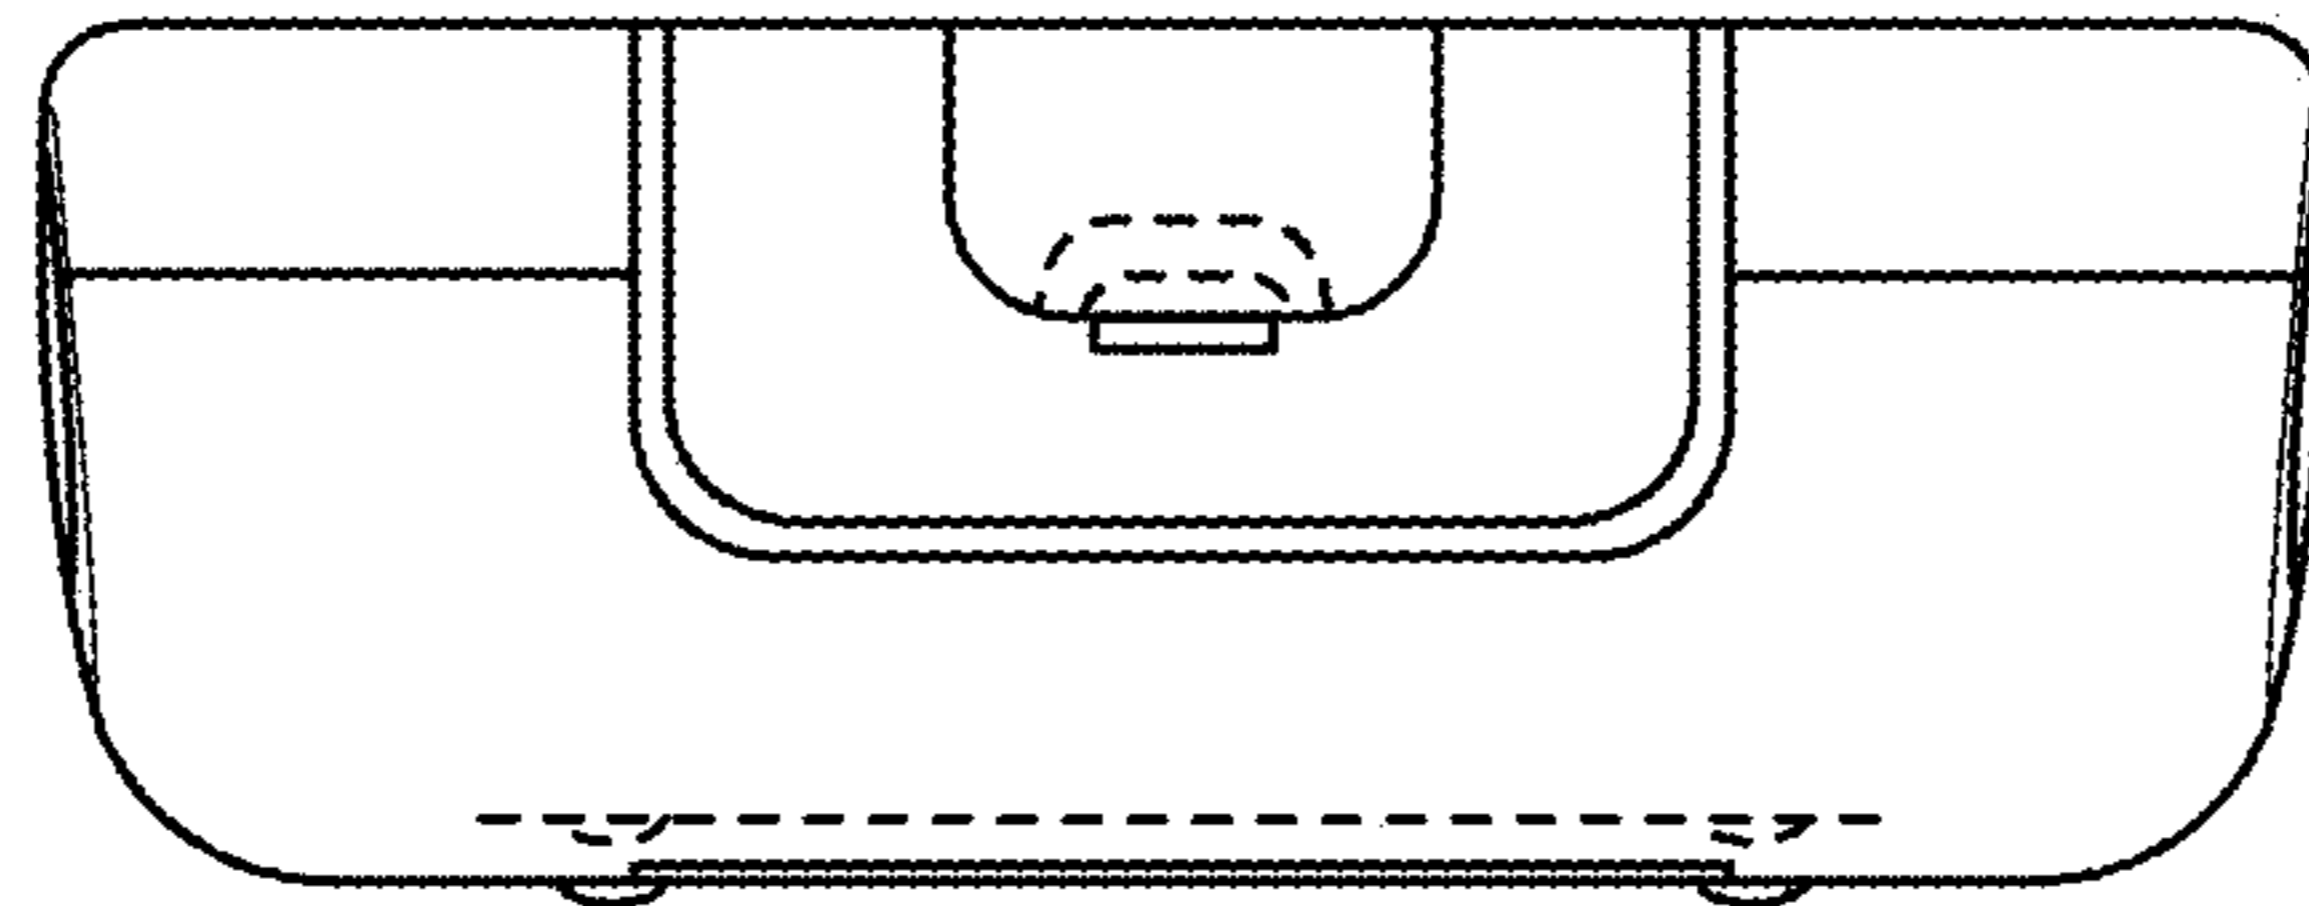


FIG. 5

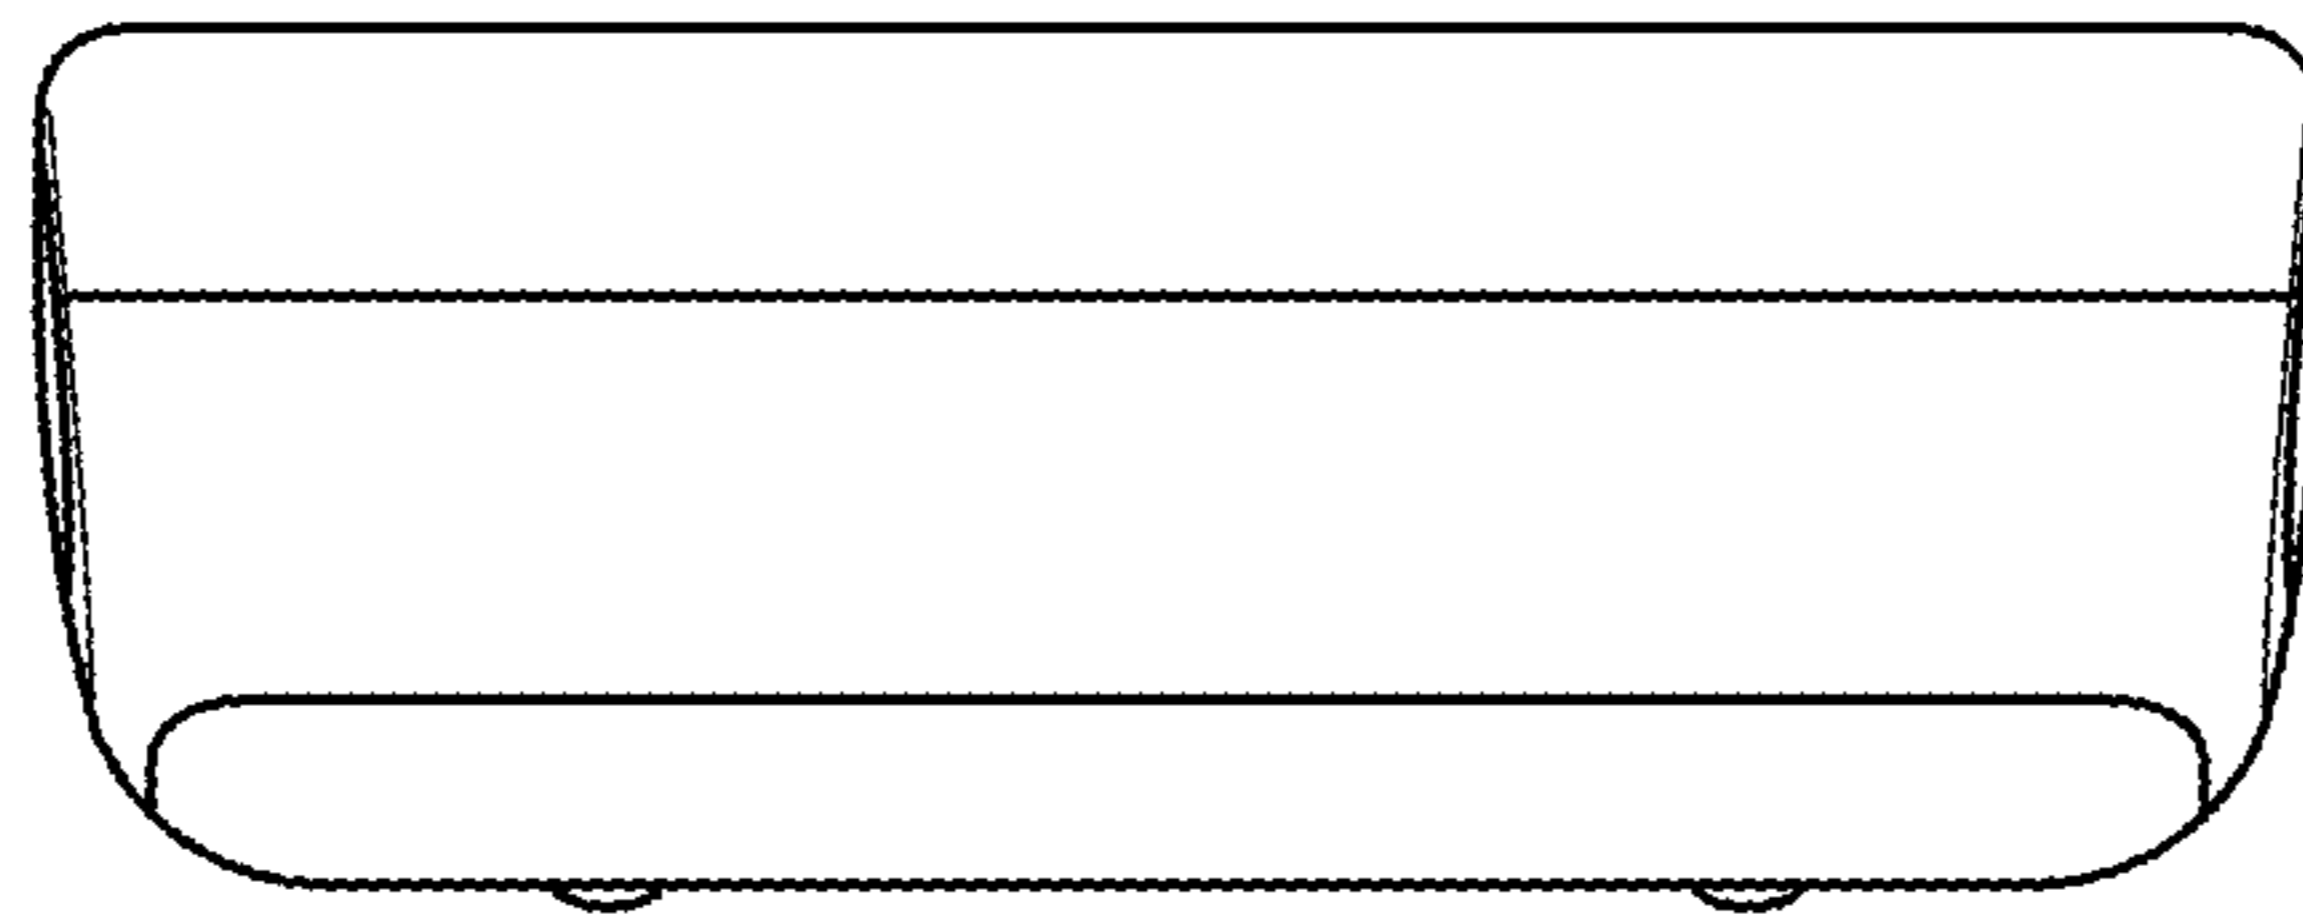


FIG. 6

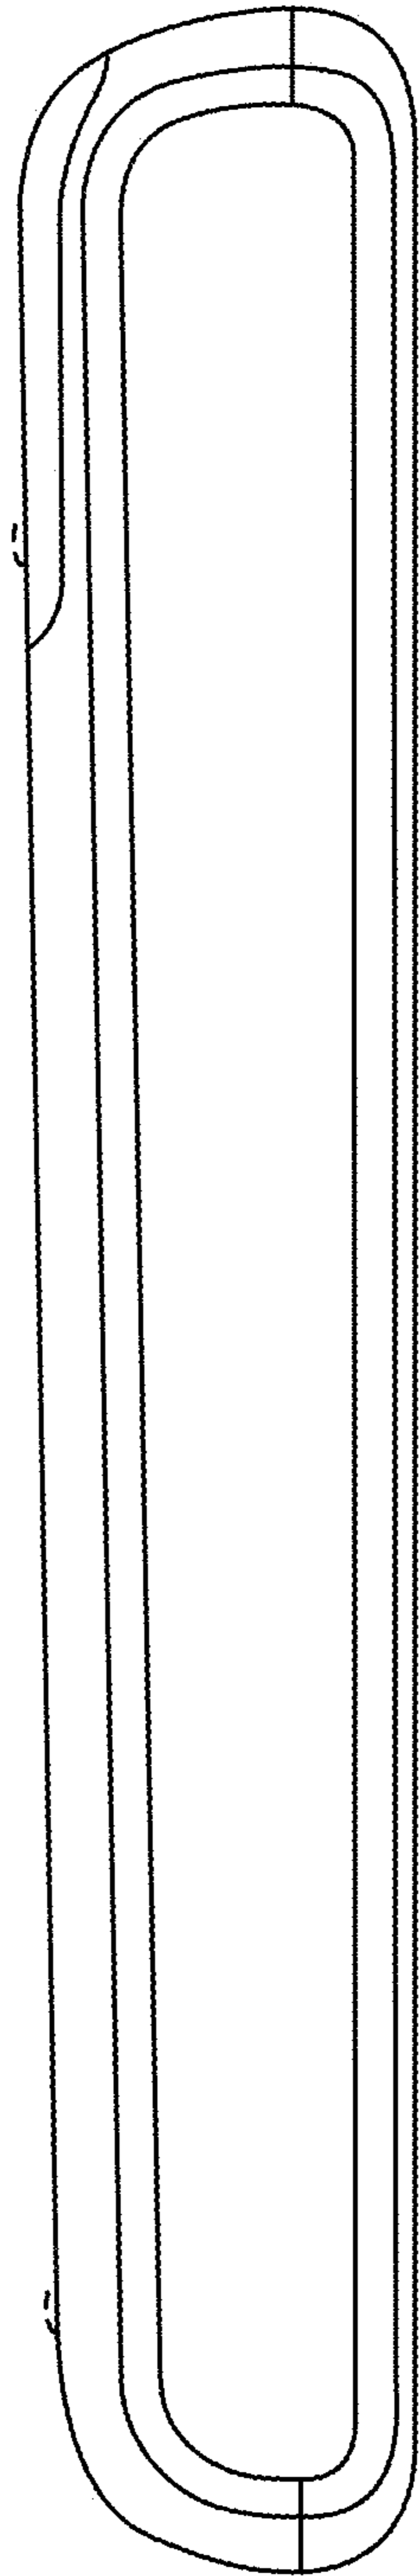


FIG. 7

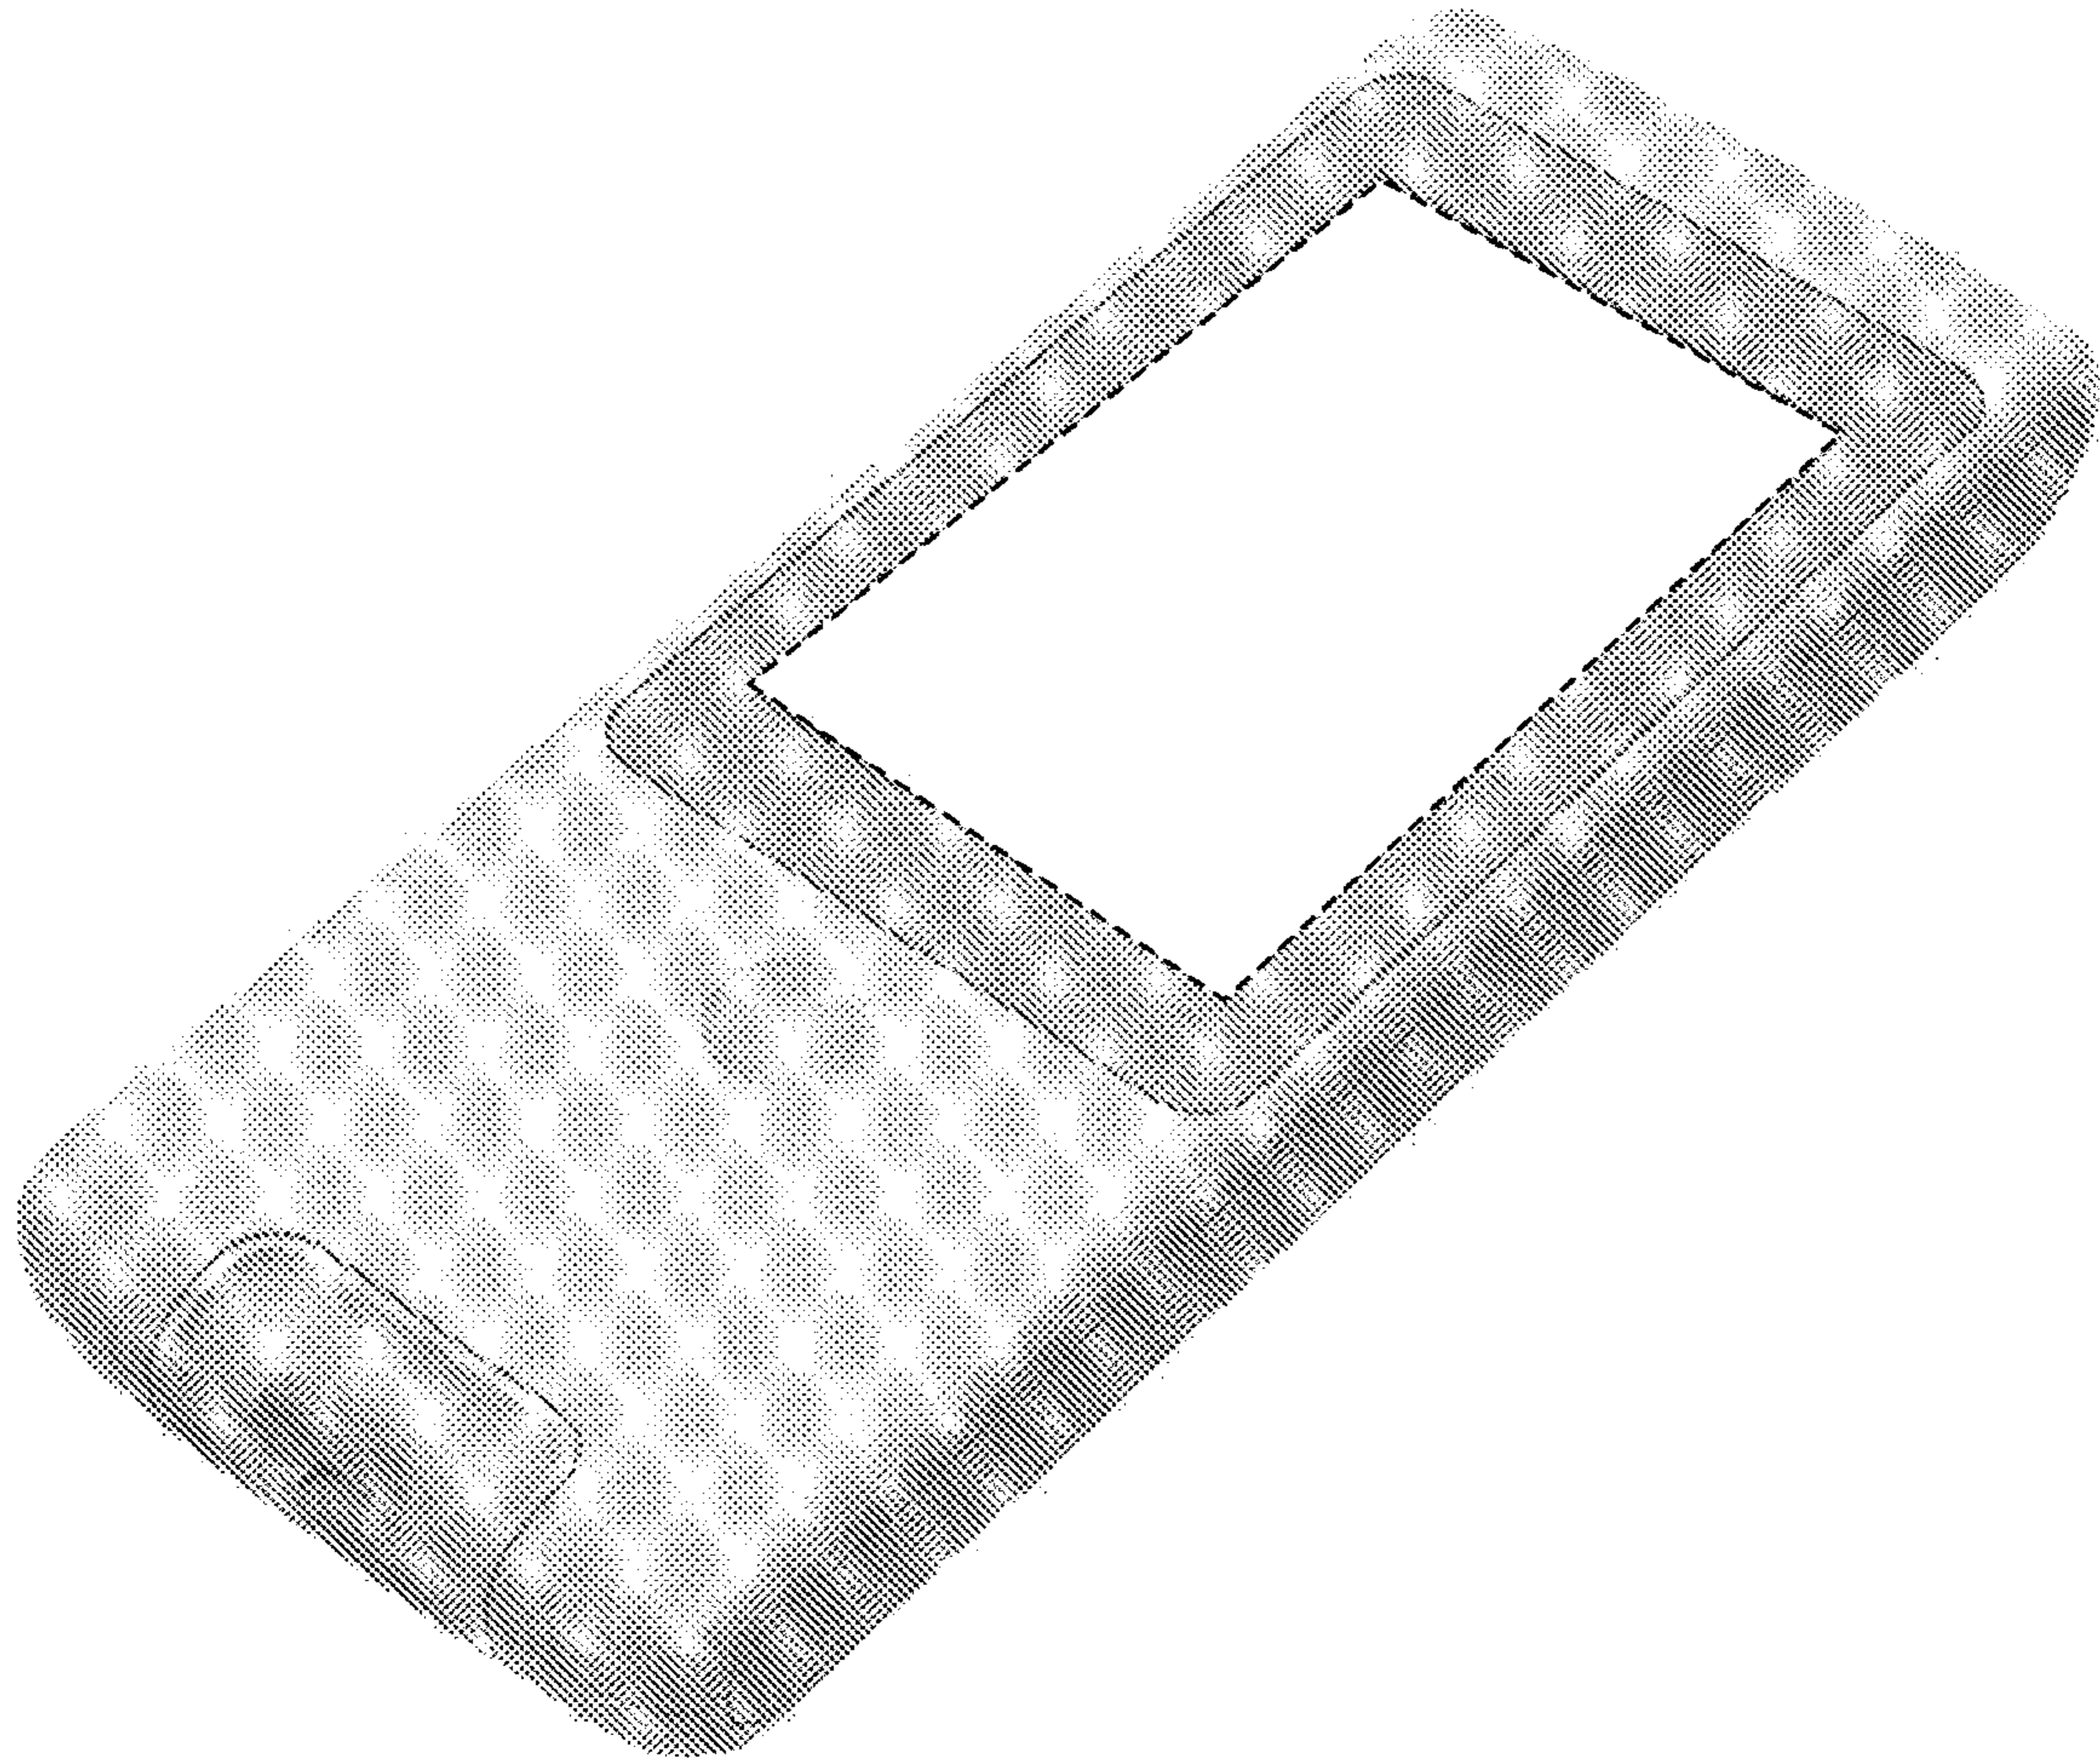


FIG. 8

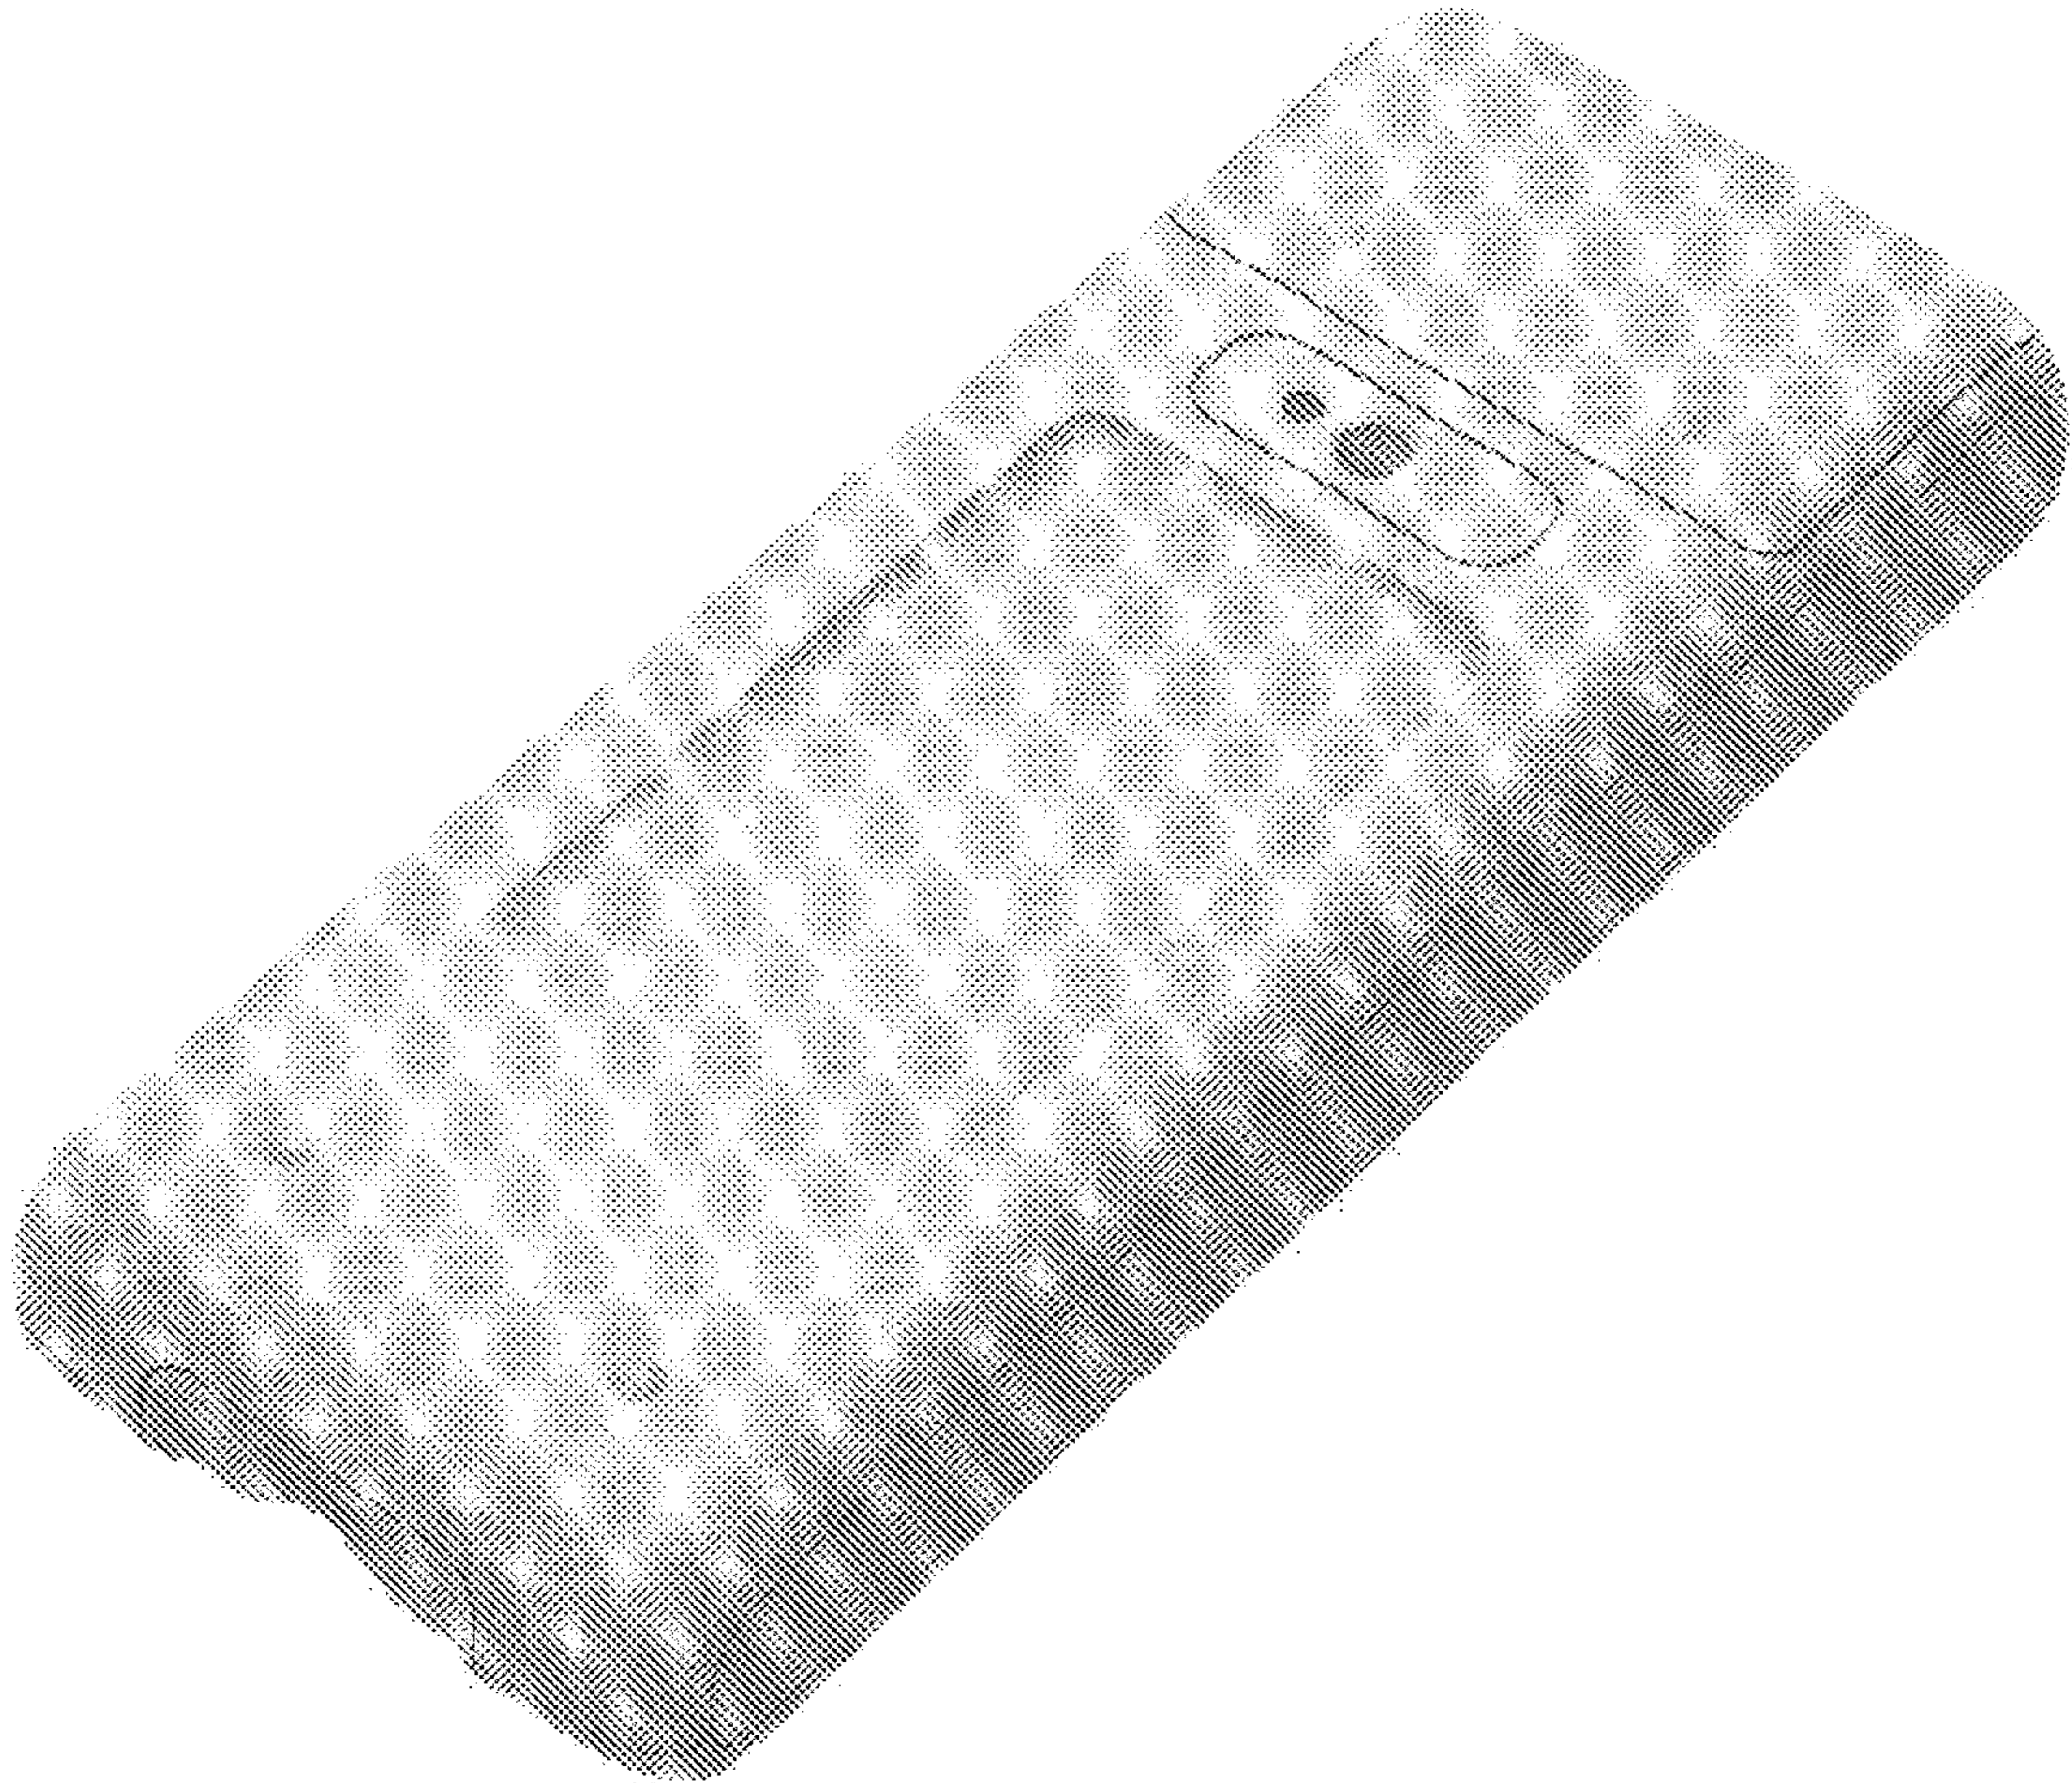


FIG. 9

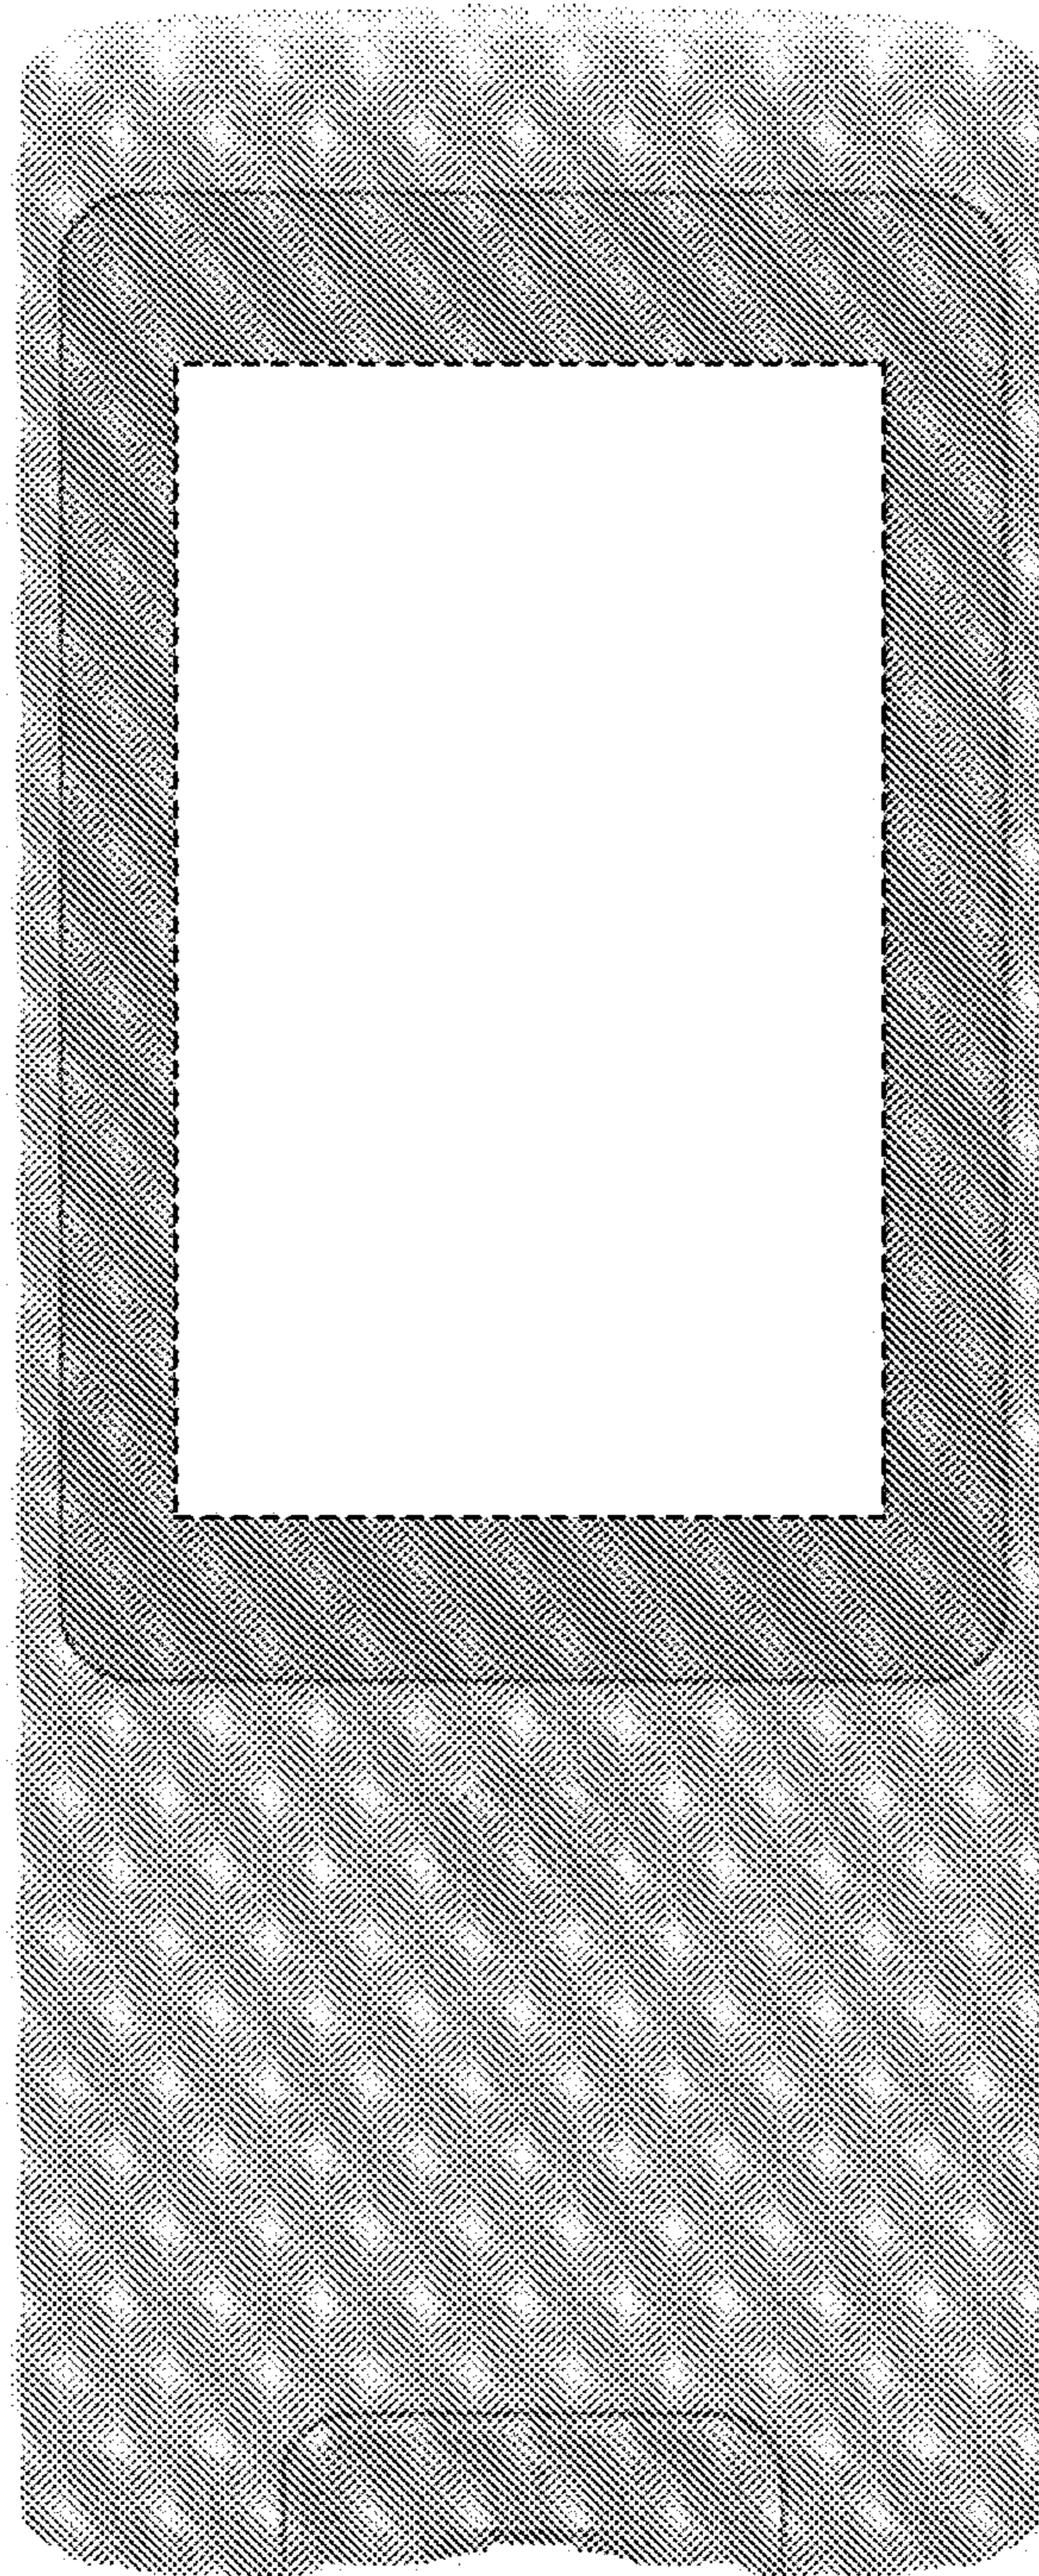


FIG. 10

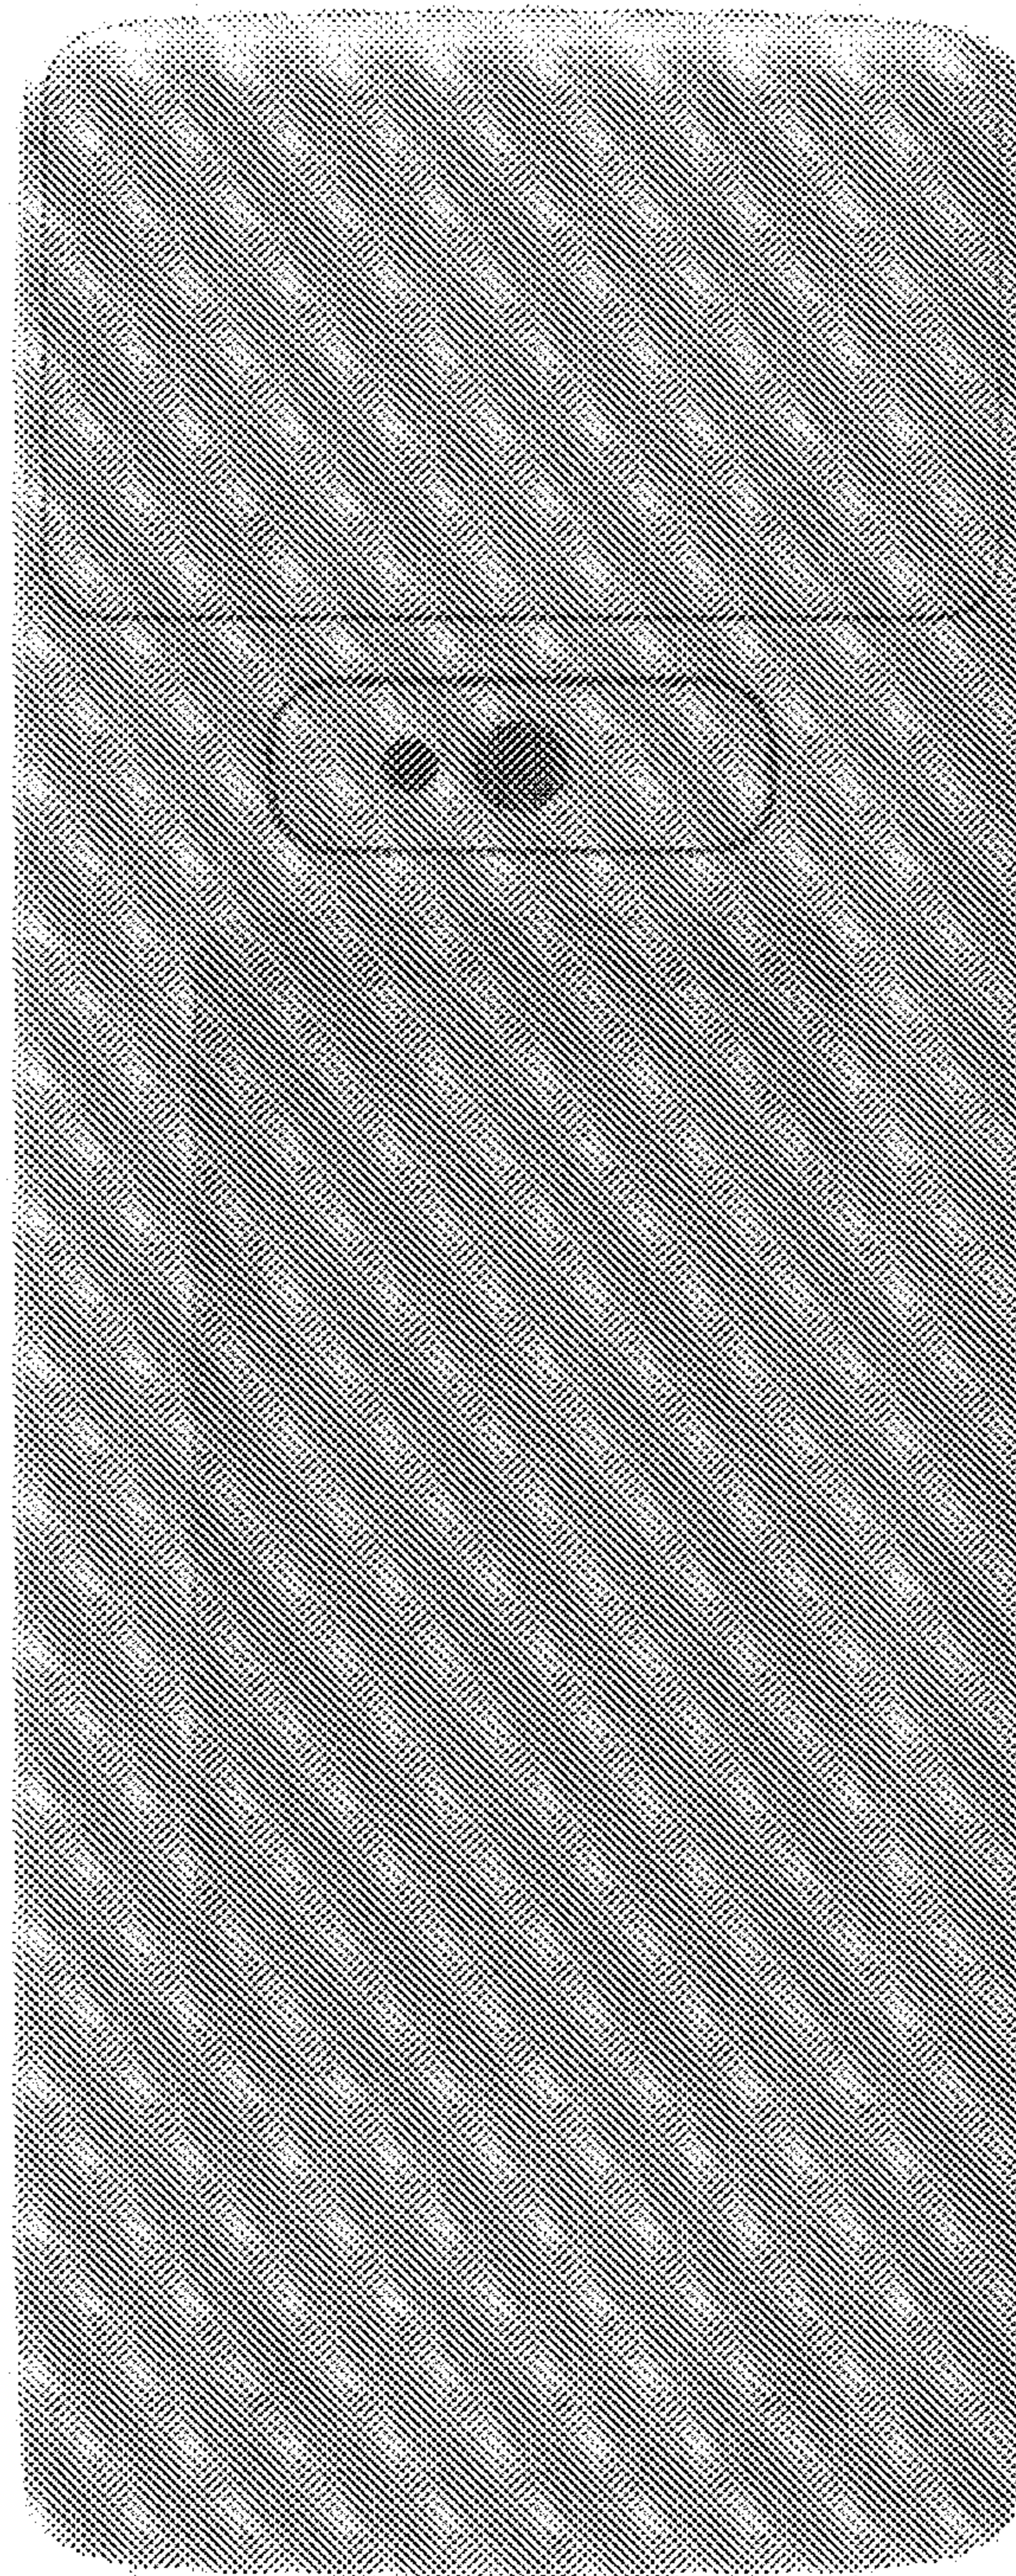


FIG. 11

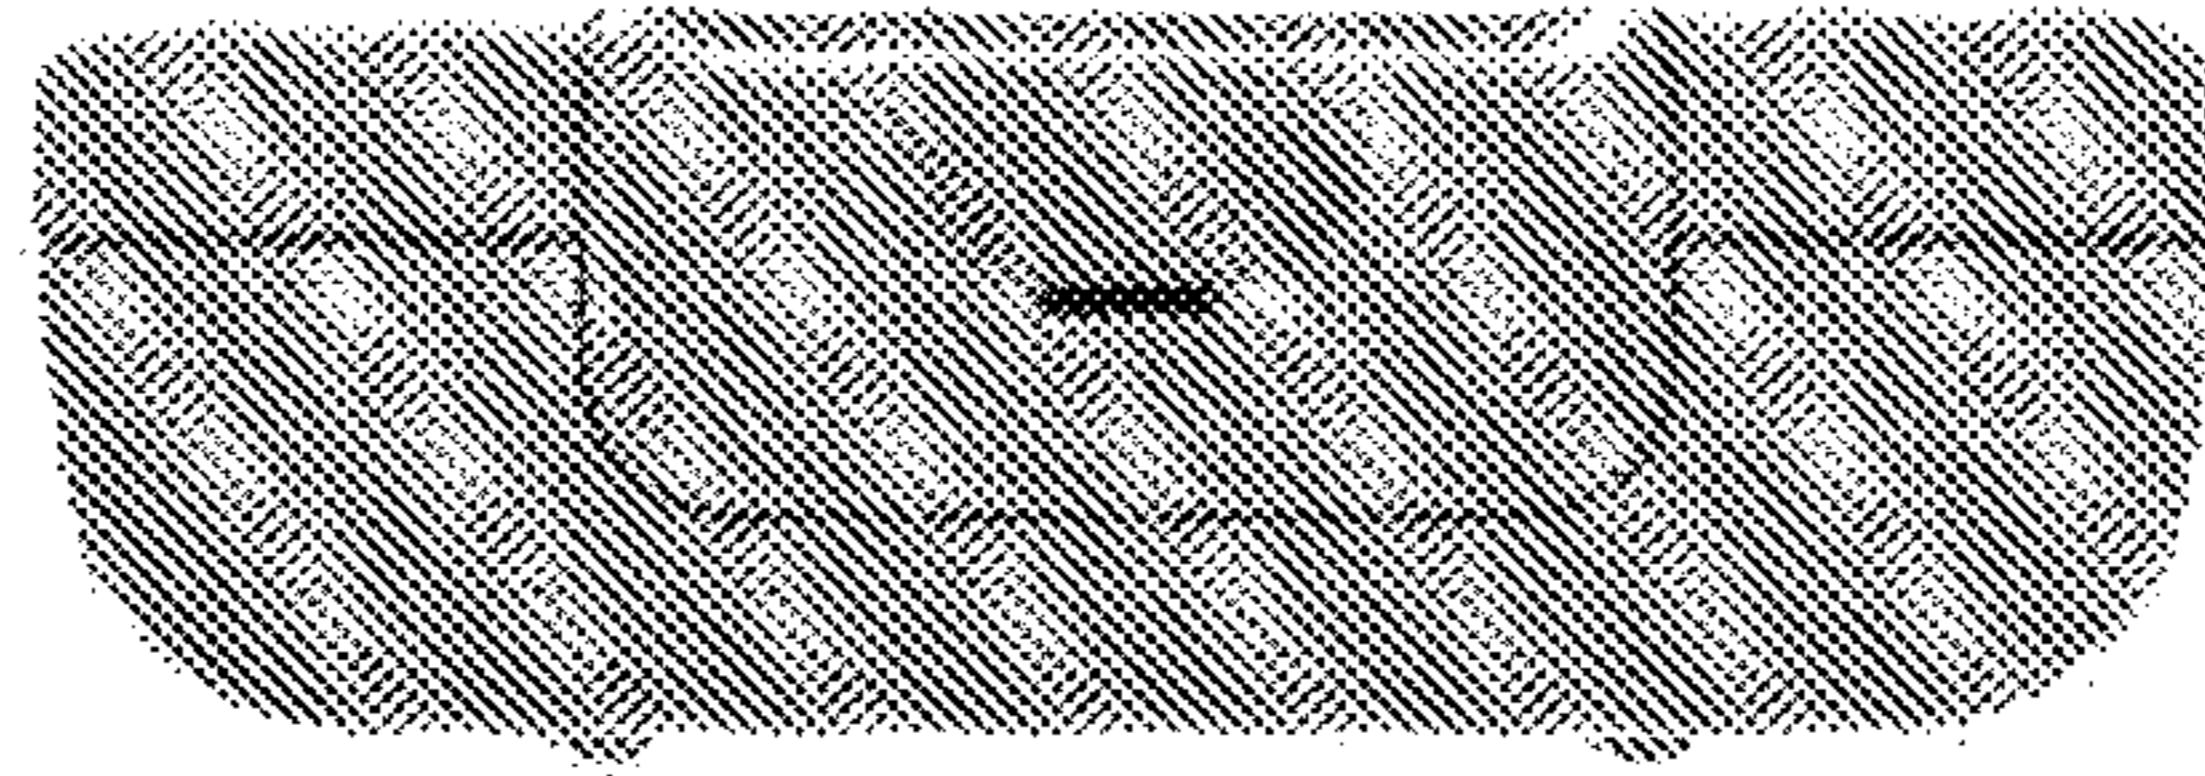


FIG. 12

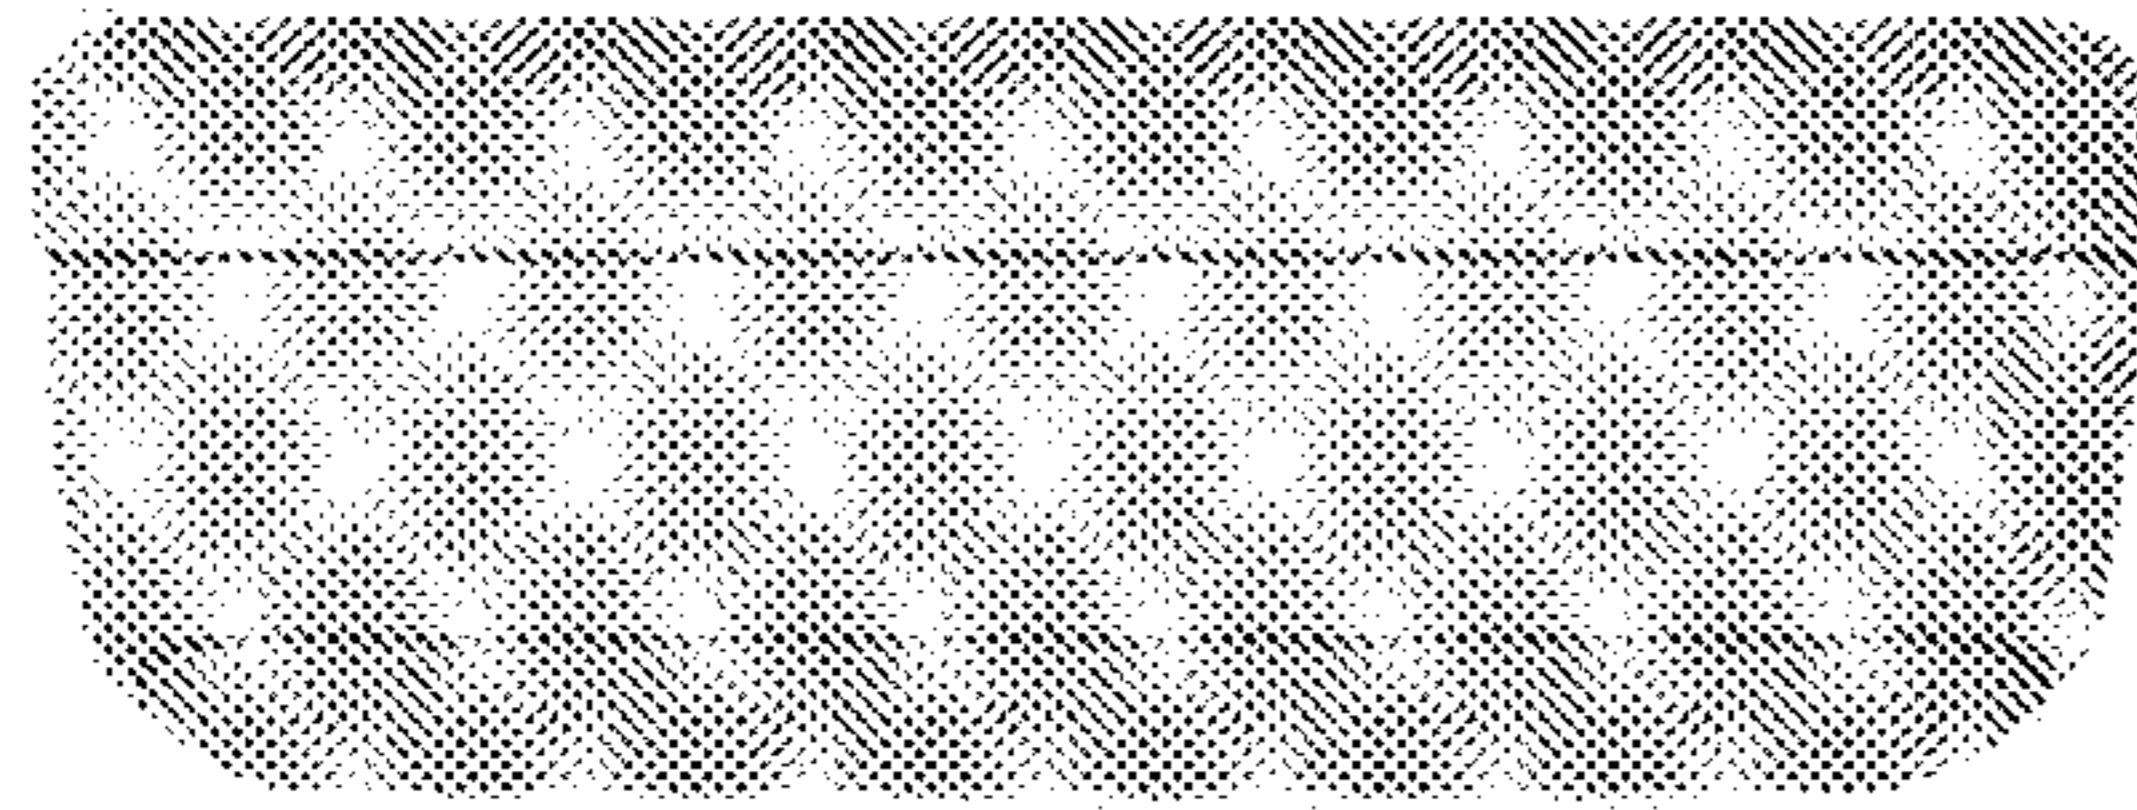


FIG. 13

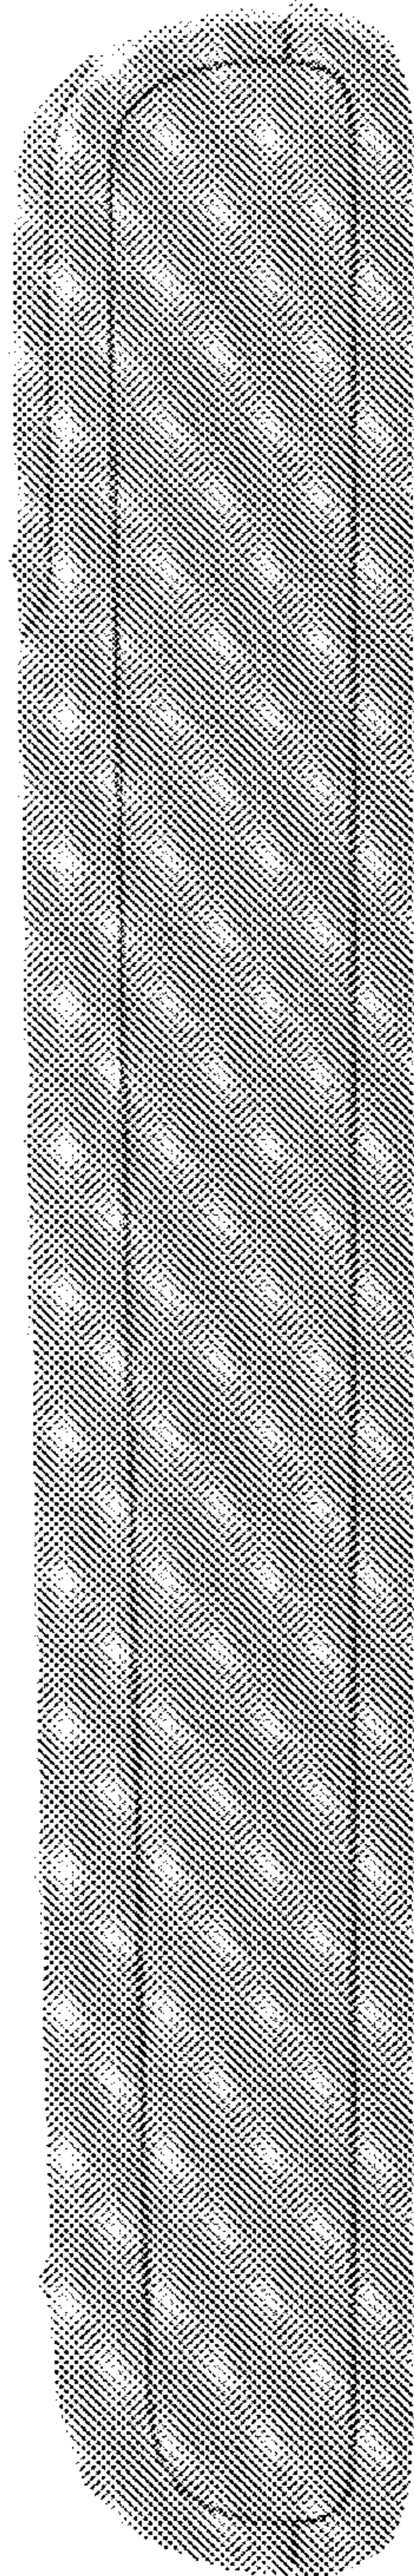


FIG. 14

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : D884,189 S
APPLICATION NO. : 29/650825
DATED : May 12, 2020
INVENTOR(S) : Johann Florian Wassermann et al.

Page 1 of 8

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the Drawings

Please replace FIGS. 8-14 with FIGS. 8-14 as shown on the attached pages.

Signed and Sealed this
Fourteenth Day of December, 2021



Drew Hirshfeld
*Performing the Functions and Duties of the
Under Secretary of Commerce for Intellectual Property and
Director of the United States Patent and Trademark Office*



FIG. 8



FIG. 9

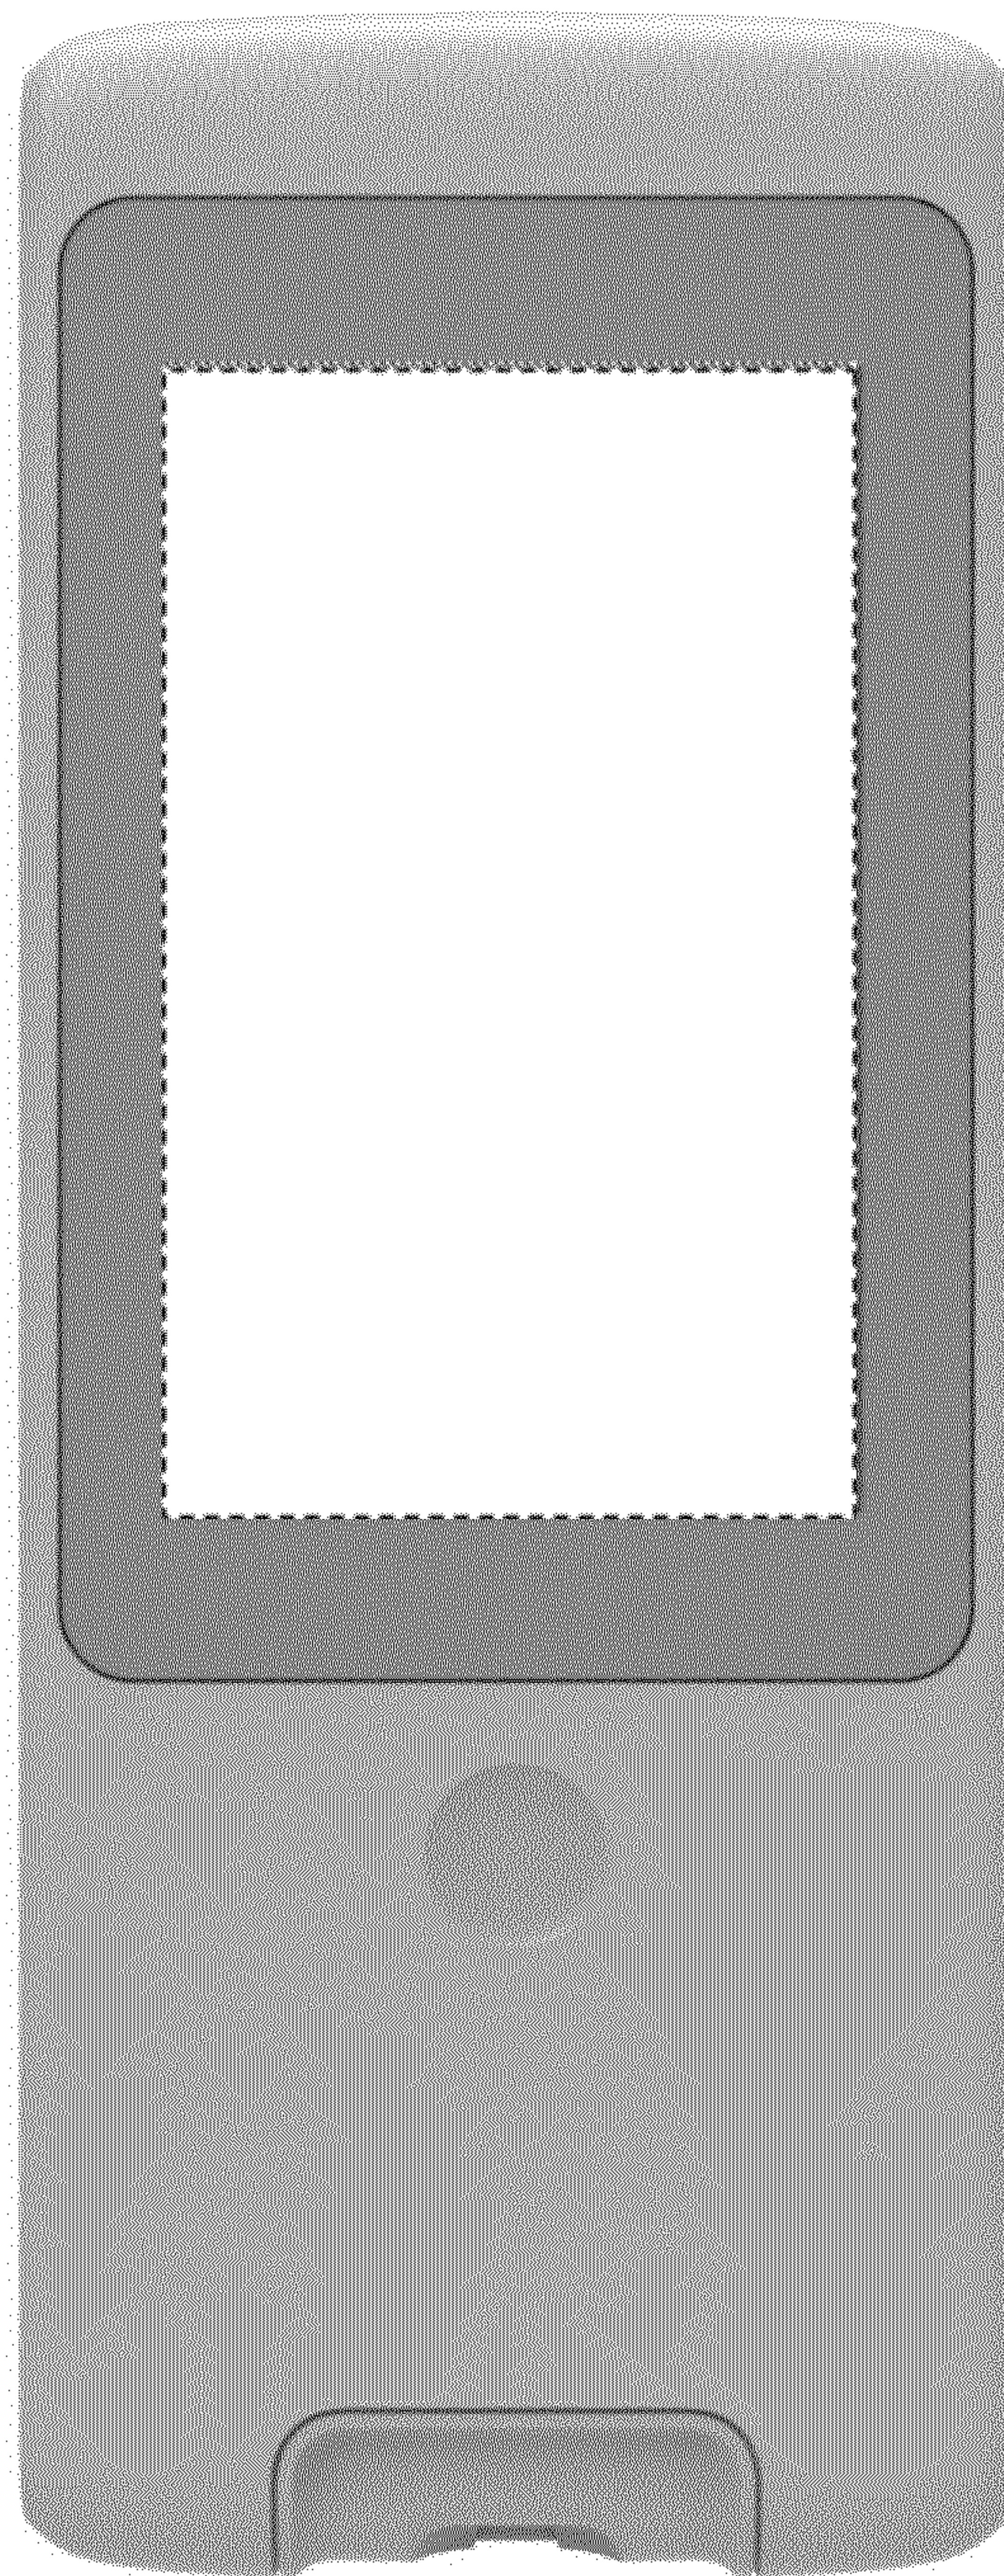


FIG. 10



FIG. 11

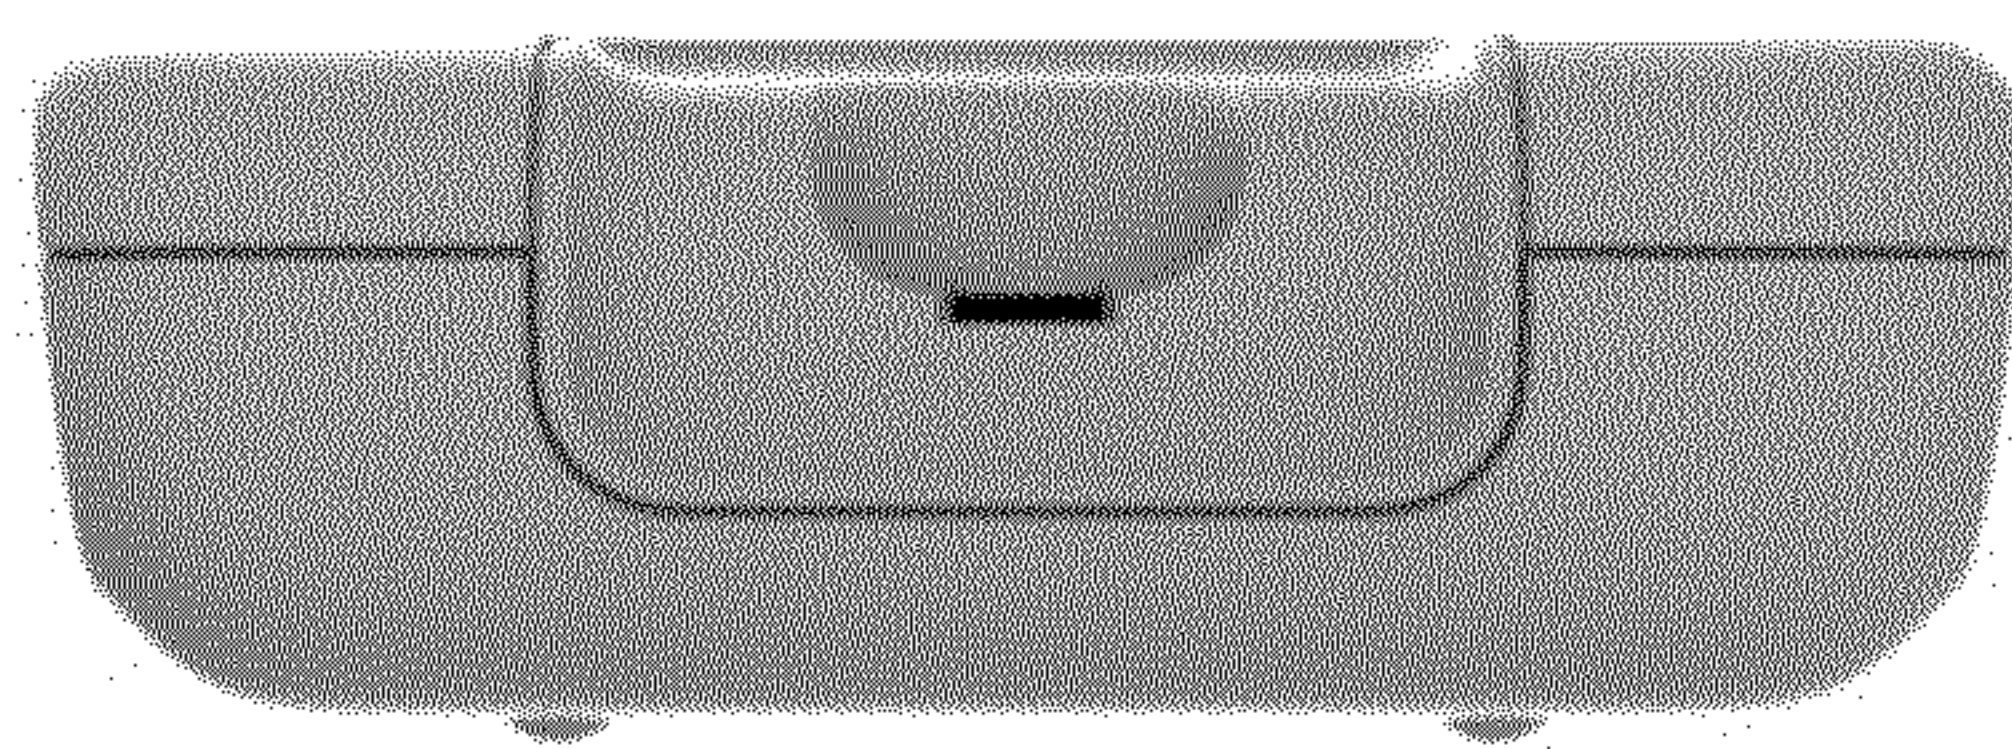


FIG. 12

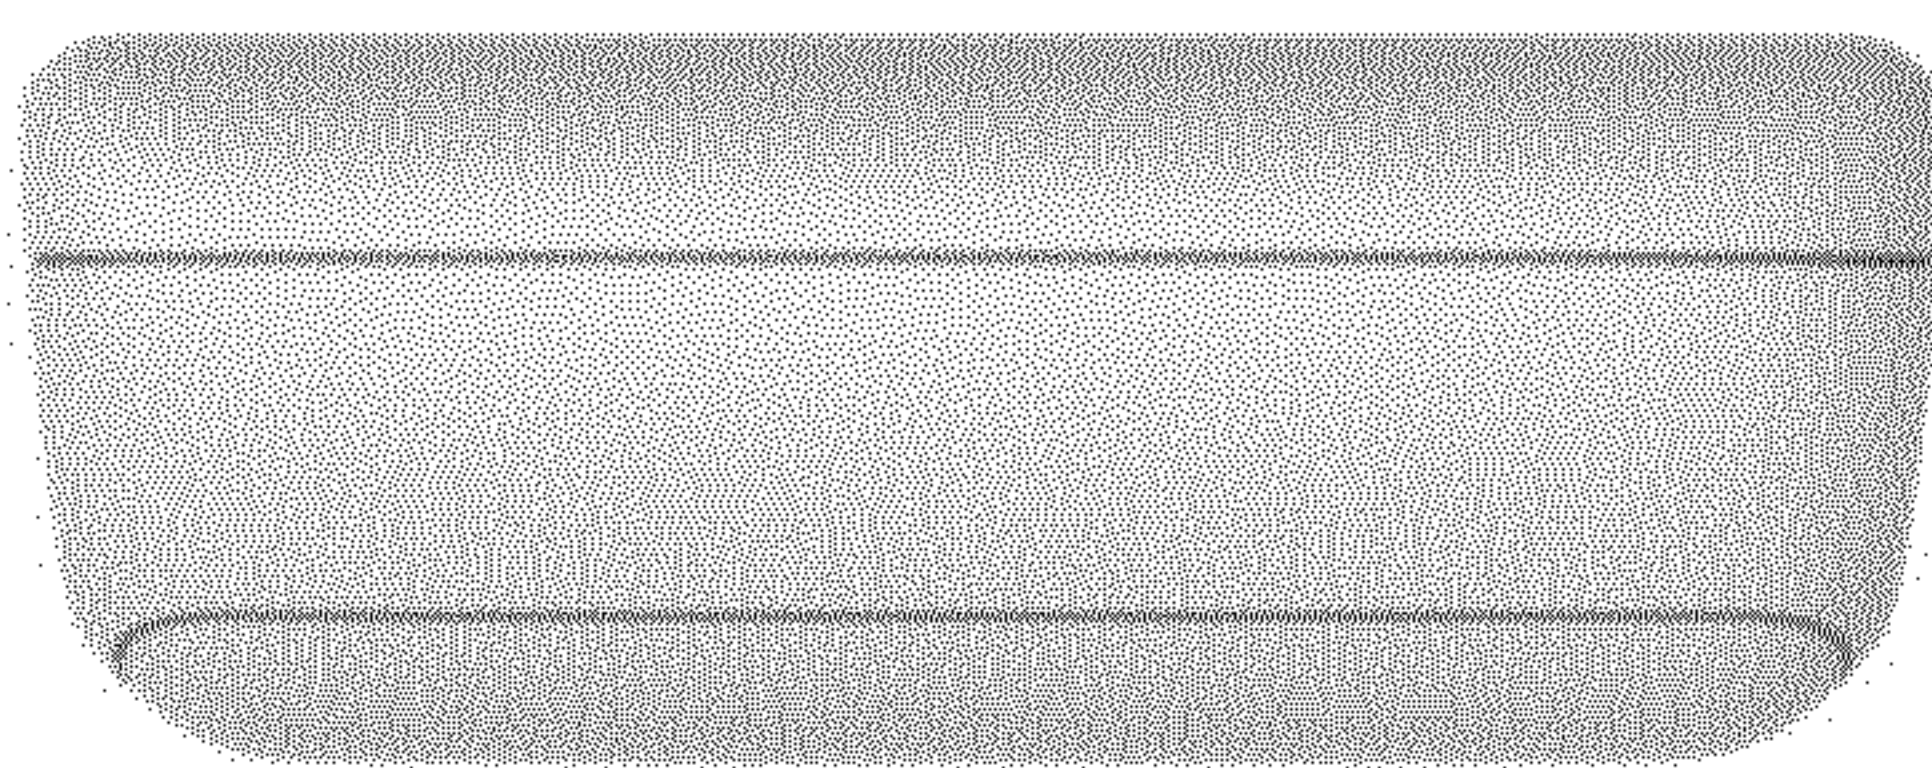


FIG. 13

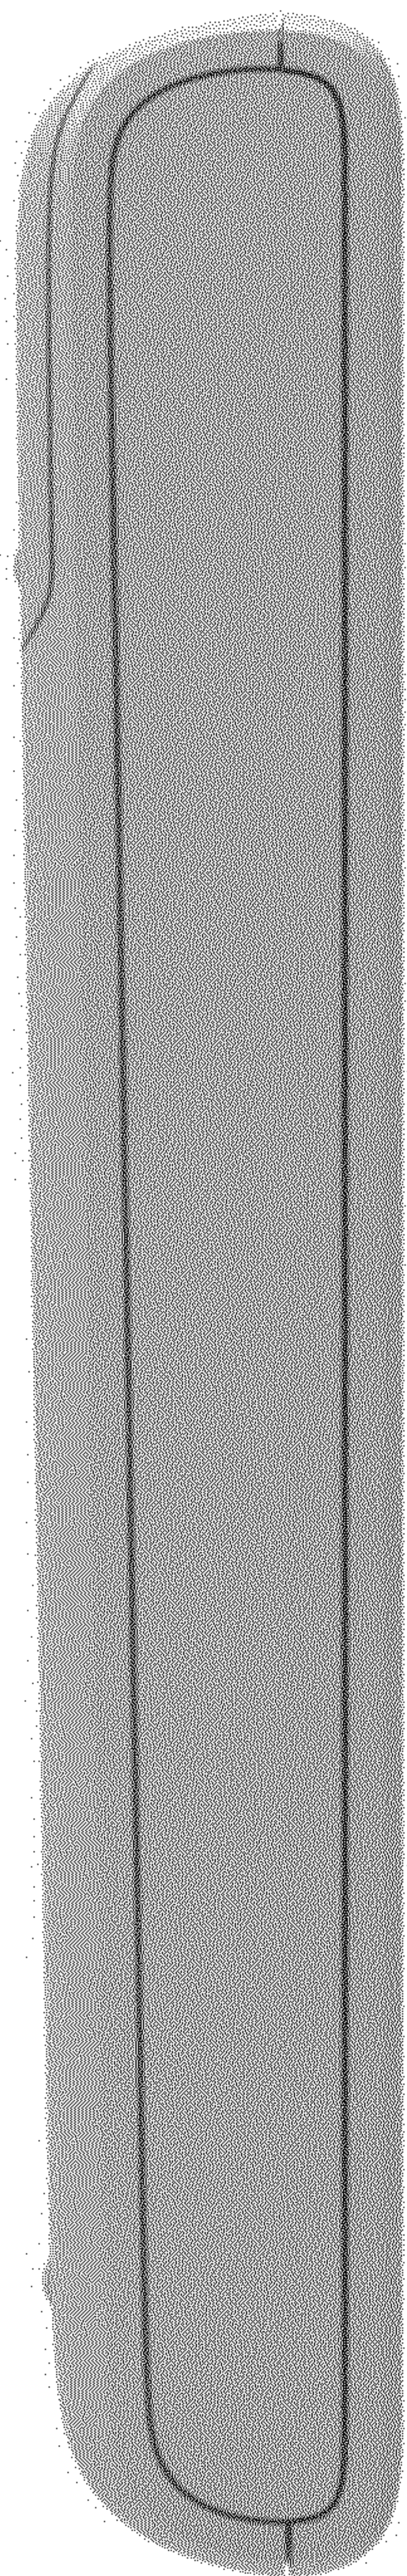


FIG. 14