



US00D884918S

(12) **United States Design Patent**
Roberts

(10) **Patent No.:** **US D884,918 S**

(45) **Date of Patent:** **** May 19, 2020**

(54) **BREATHING EQUIPMENT SANITIZING CHAMBER**

D457,314 S * 5/2002 Stephens D3/276
D560,361 S * 1/2008 Huang D3/301
D600,440 S * 9/2009 Gaikwad D3/203.1

(Continued)

(71) Applicant: **Exceleron Medical, LLC.**, St. Paul, MN (US)

(72) Inventor: **Keith Roberts**, St. Paul, MN (US)

(73) Assignee: **Exceleron Medical, LLC.**, St. Paul, MN (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/647,220**

(22) Filed: **May 10, 2018**

(51) **LOC (12) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/217**

(58) **Field of Classification Search**
USPC D24/216, 217, 218, 219, 227-232;
D32/1, 25; D3/201, 203.1, 203.2, 203.3,
D3/203.4, 294, 289, 301; D7/629;
D9/414, 418, 419, 420, 423, 430, 428,
D9/432; D14/138 R; 383/97
CPC A61L 2/26; A61L 2/24; A61L 2/17; A61L
2/18; A61L 2/025; A61L 2202/122; A61L
2202/10; A61L 2202/11; A61L 2202/14;
A61L 2202/23; A61L 2202/24; A61L
2202/182

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,556,066 A * 6/1951 Cline A45C 11/008
190/111
5,047,021 A 9/1991 Utterberg
5,713,137 A 2/1998 Fujita
D396,750 S * 8/1998 Slater D3/284
D412,267 S * 7/1999 Anderson D7/605
6,134,806 A 10/2000 Dhaemers

OTHER PUBLICATIONS

CPAP Sanitizer VirtuCLEAN, posted at mckesson.com, no posting date available, online, URL:https://mms.mckesson.com/product/1087308/HLS-2200 (Year: 2019).*

(Continued)

Primary Examiner — Anhdao Doan

Assistant Examiner — Mary Shannon Malley

(74) *Attorney, Agent, or Firm* — Moss & Barnett;
Michael A. Bondi

(57) **CLAIM**

The ornamental design for a breathing equipment sanitizing chamber, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the breathing equipment sanitizing chamber;

FIG. 2 is a top view of the breathing equipment sanitizing chamber;

FIG. 3 is a bottom view of the breathing equipment sanitizing chamber;

FIG. 4 is a first side view of the breathing equipment sanitizing chamber;


FIG. 5 is a second side view of the breathing equipment sanitizing chamber;

FIG. 6 is a first end view of the breathing equipment sanitizing chamber; and,

FIG. 7 is a second end view of the breathing equipment sanitizing chamber.

The broken lines depict portions of the breathing equipment sanitizing chamber that form no part of the claimed design.

1 Claim, 7 Drawing Sheets

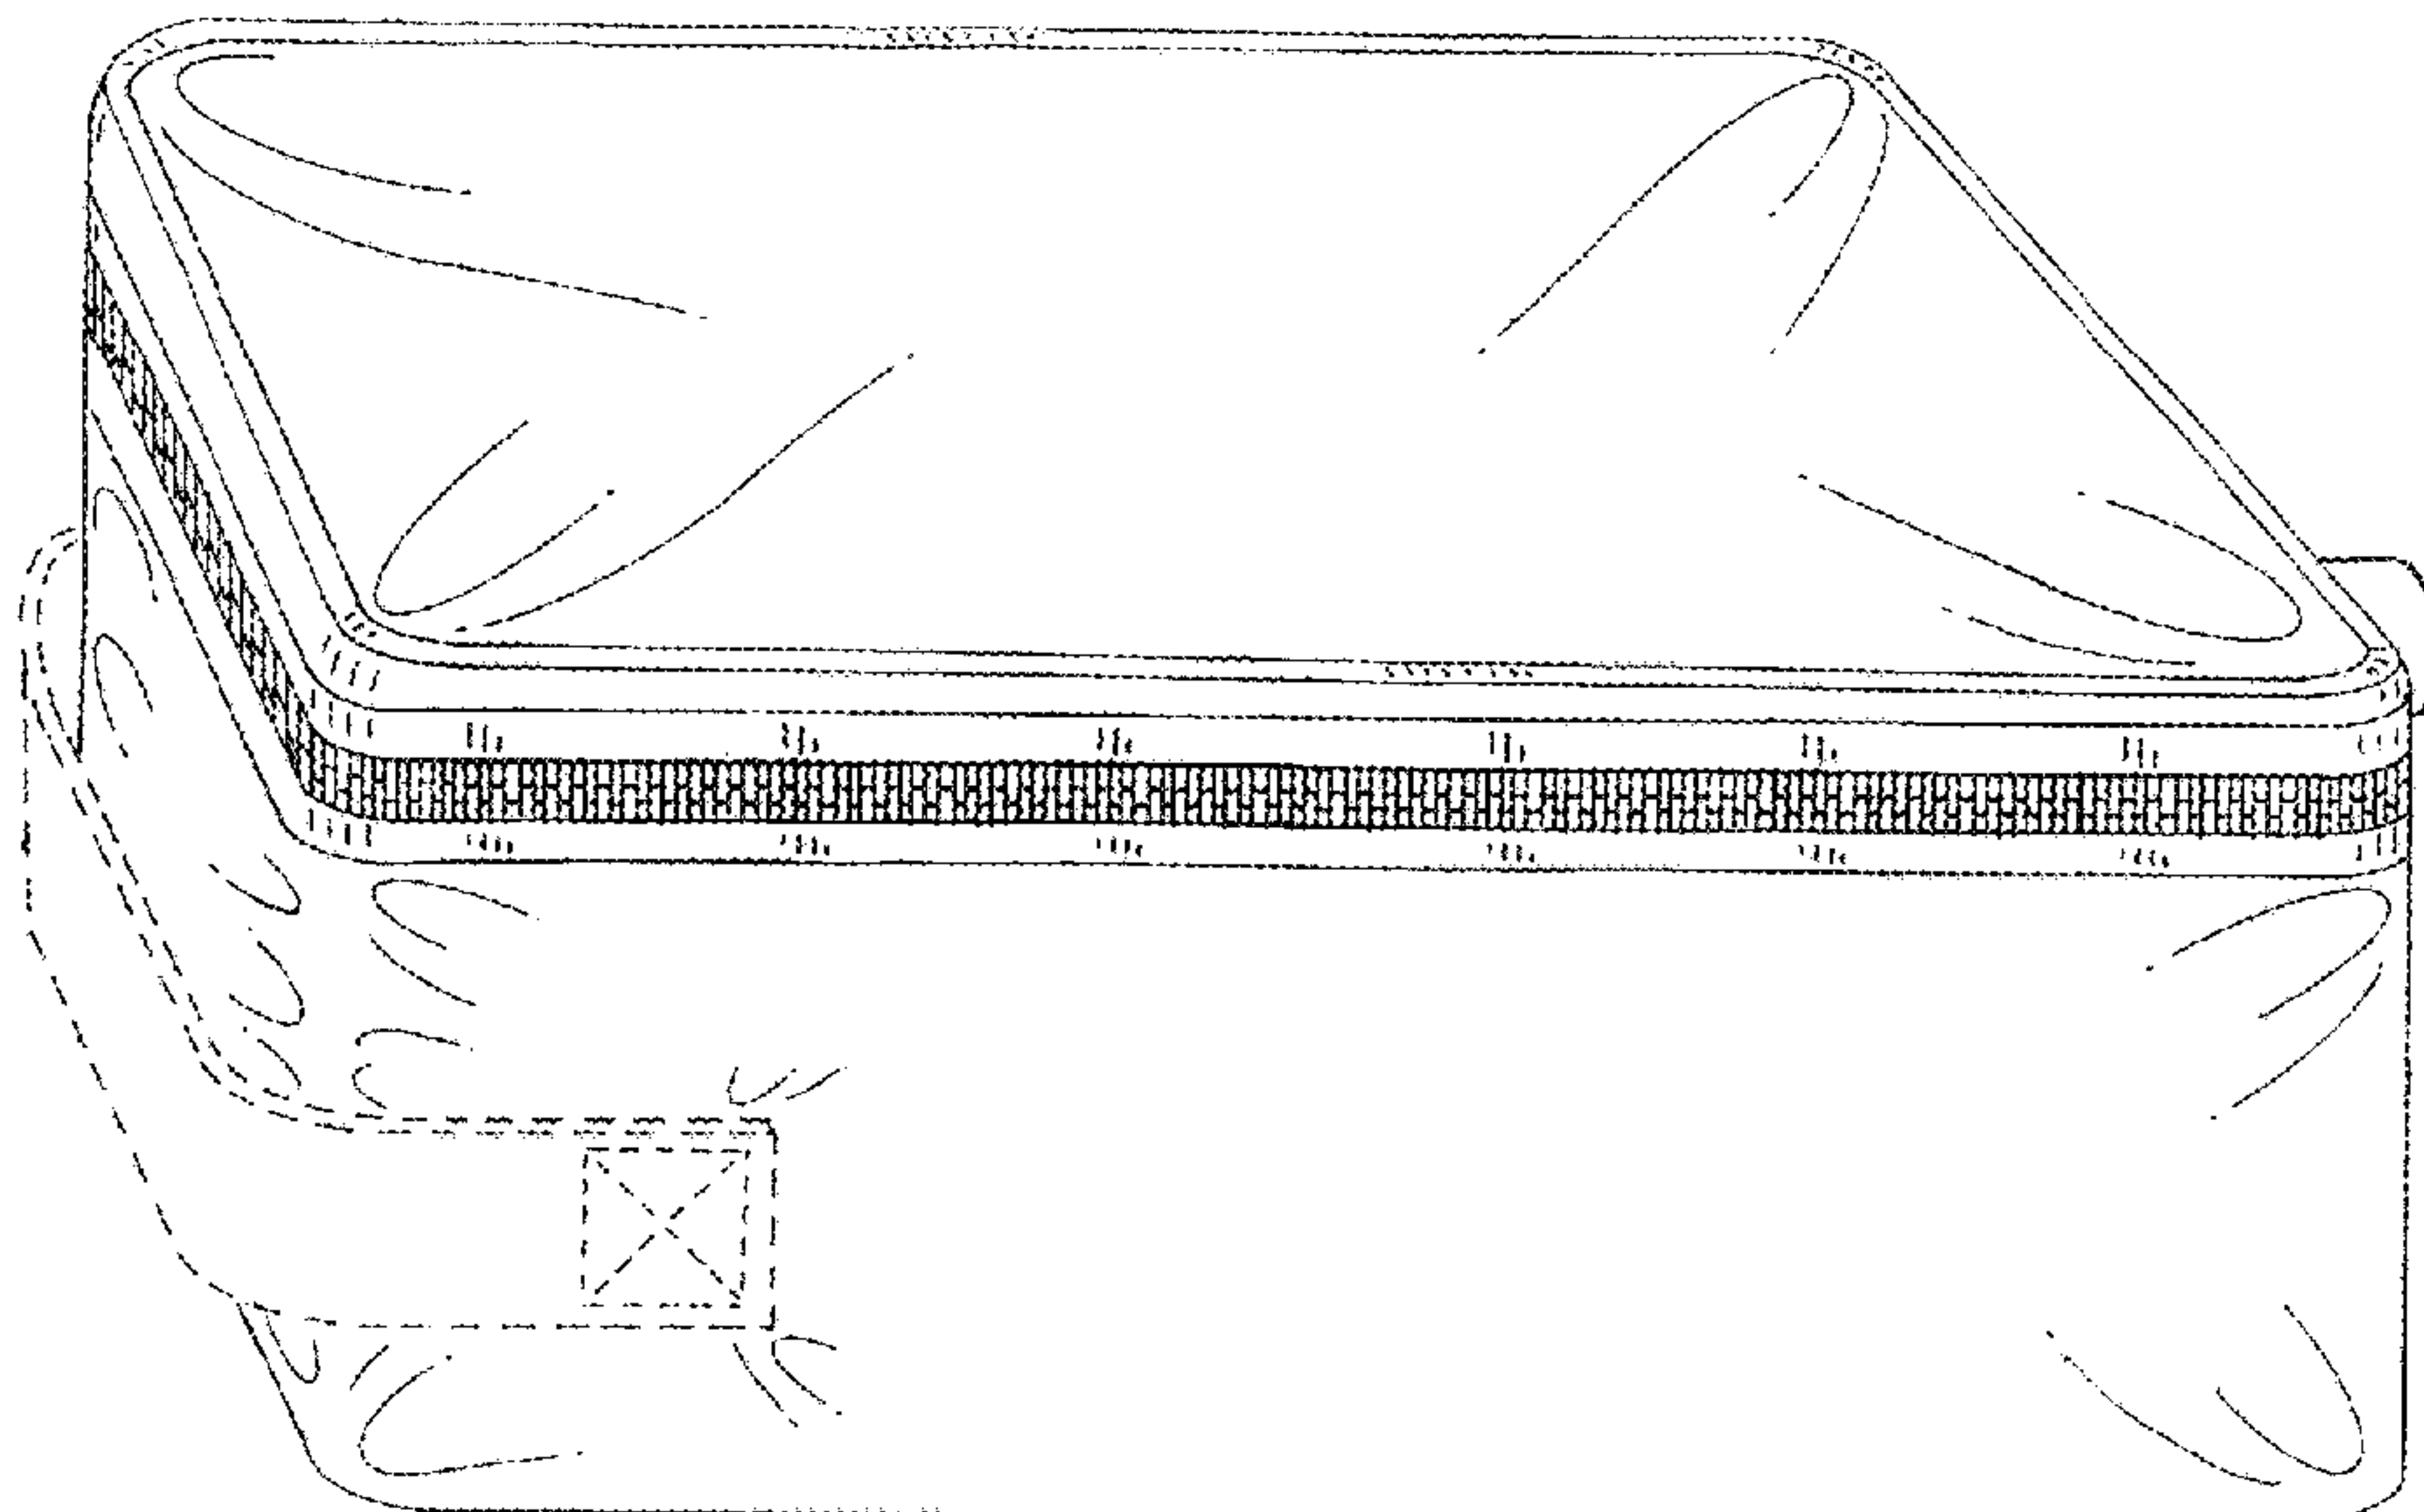

(56)

References Cited

U.S. PATENT DOCUMENTS

D639,064 S * 6/2011 Raible D3/301
 8,038,963 B1 10/2011 Chen
 D651,393 S * 1/2012 Coleman D3/203.6
 D730,648 S * 6/2015 Lentner D3/285
 D731,792 S * 6/2015 Lentner D3/285
 9,358,316 B2 6/2016 Leyva
 9,610,373 B2 4/2017 Leyva
 9,616,147 B2 4/2017 Leyva
 9,669,124 B2 6/2017 Leyva
 9,895,461 B2 2/2018 Leyva
 9,907,872 B2 3/2018 Schmidt
 D841,974 S * 3/2019 Peng D3/205
 2003/0044308 A1 3/2003 Toth
 2008/0118411 A1 5/2008 D'Arinzo
 2014/0154134 A1 6/2014 Leyva
 2016/0235875 A1 8/2016 Leyva
 2016/0235876 A1 8/2016 Leyva
 2016/0243268 A1 8/2016 Leyva
 2016/0243269 A1 8/2016 Leyva

2016/0250366 A1 9/2016 Leyva
 2017/0165443 A1 6/2017 Leyva
 2017/0202990 A1 7/2017 Leyva
 2017/0209610 A1 7/2017 Leyva
 2017/0225985 A1 8/2017 Leyva
 2018/0140730 A1 5/2018 Leyva
 2018/0161466 A1 6/2018 Schmidt

OTHER PUBLICATIONS

Philips DreamStation Travel Bag, posted at cpapoffice.com, no posting date available, online, URL: <https://www.cpapoffice.com/philips-dreamstation-travel-bag> (Year: 2019).*

CPAP Cleaner and Sanitizer Bundle, posted at amazon.com, no posting date, online, URL: https://www.amazon.com/dp/B07XGRLL94/ref=sspa_dk_detail_0?psc=1&pd_rd_ (Year: 2019).*

Wave Portable CPAP Cleaner and Sanitizer System, posted at thebestcpapcleaner.com, no posting date, online, URL: <https://thebestcpapcleaner.com/products/wave-portable-cpap-cleaner-and-sanitizer-system> (Year: 2019).*

* cited by examiner

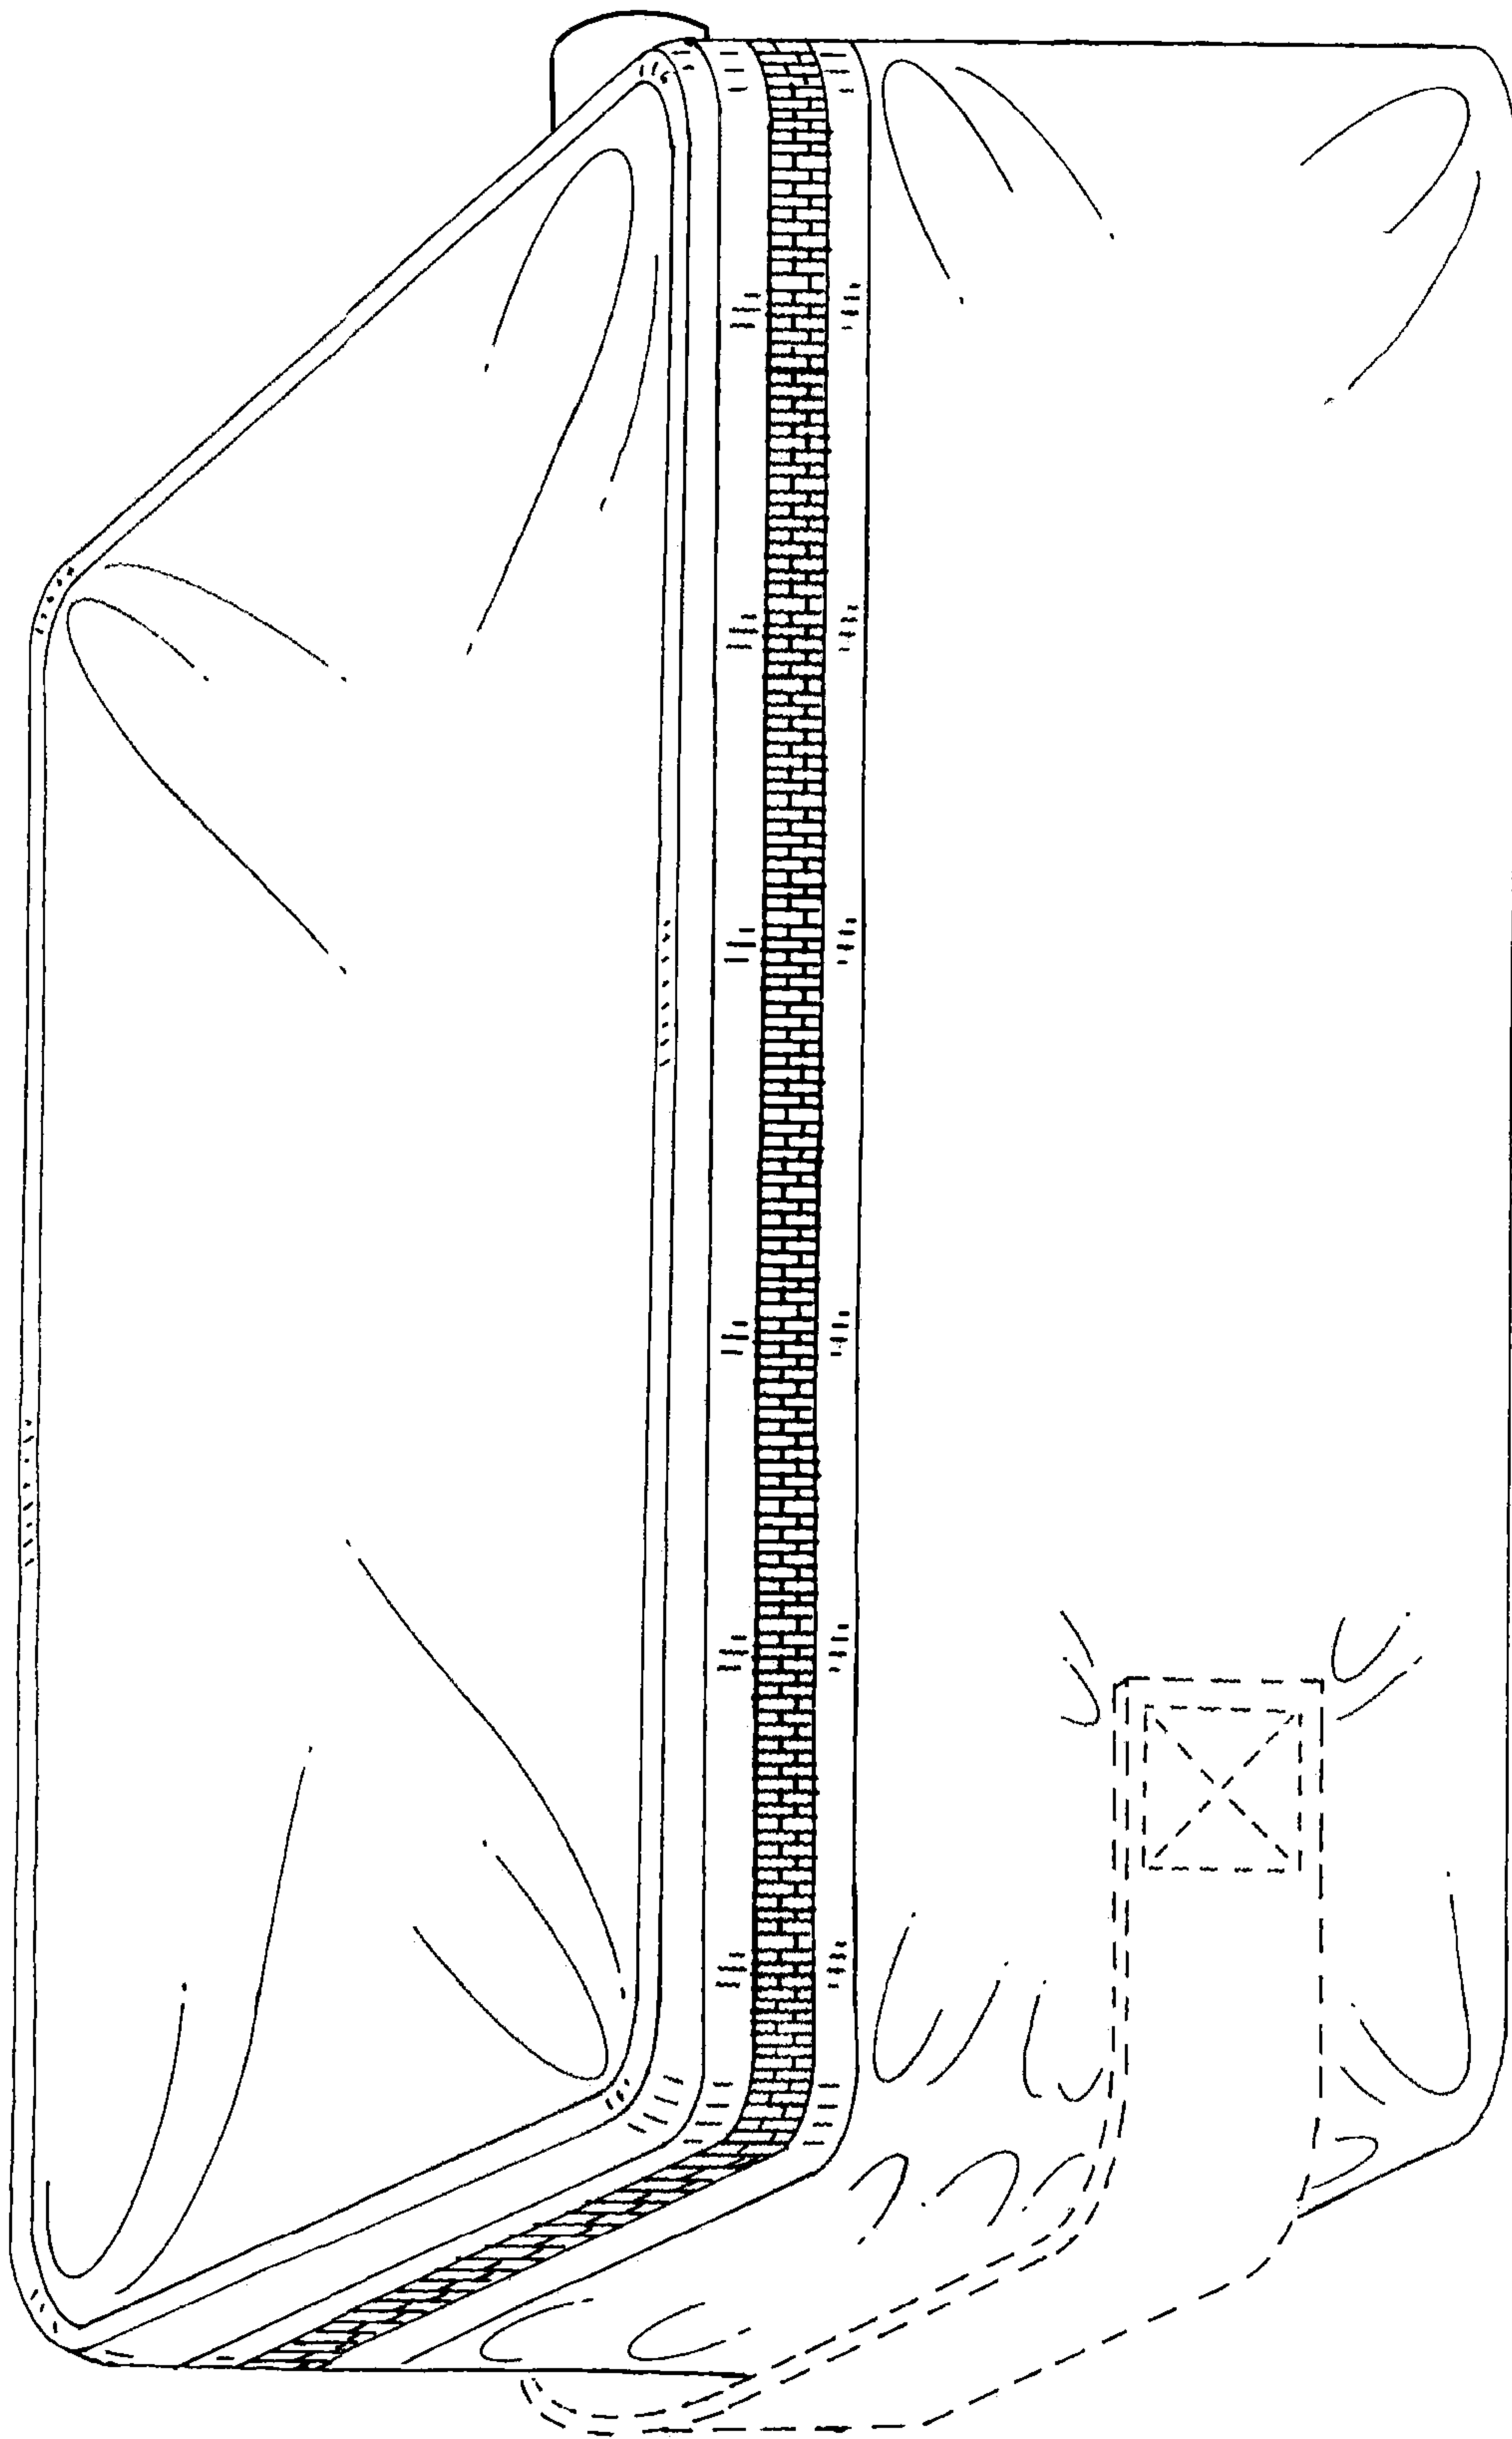


FIG. 1

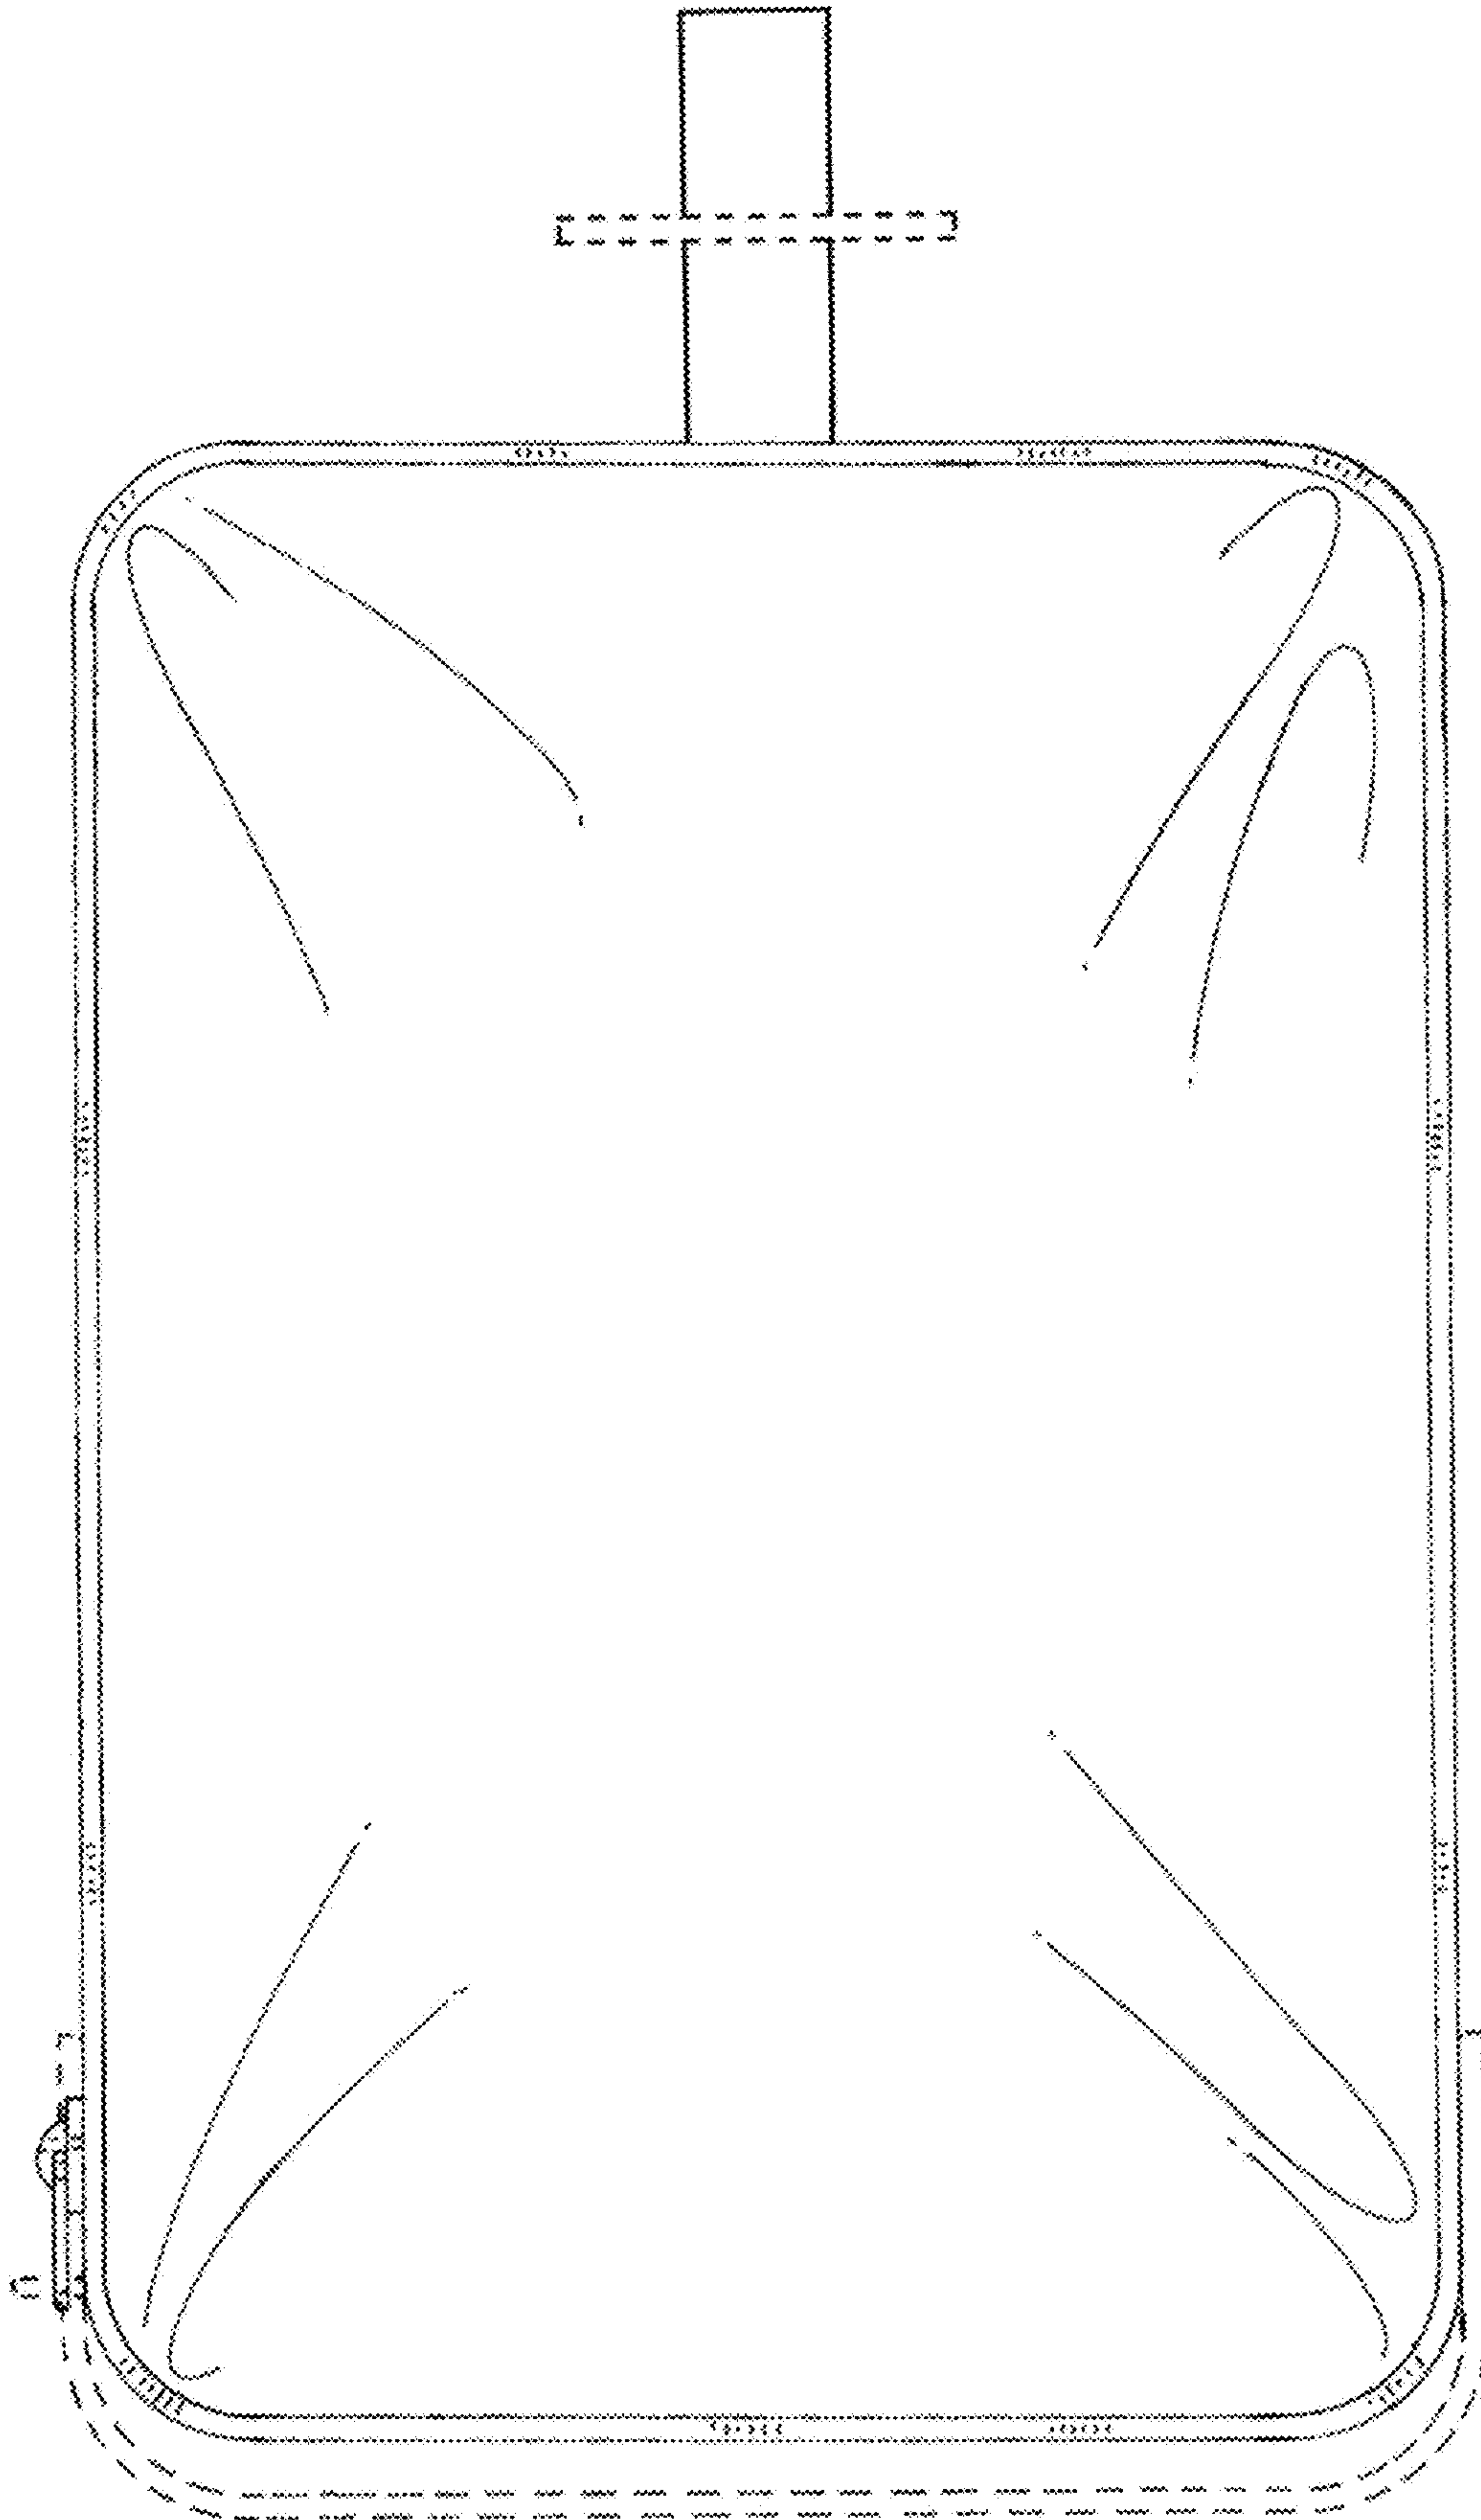


FIG. 2

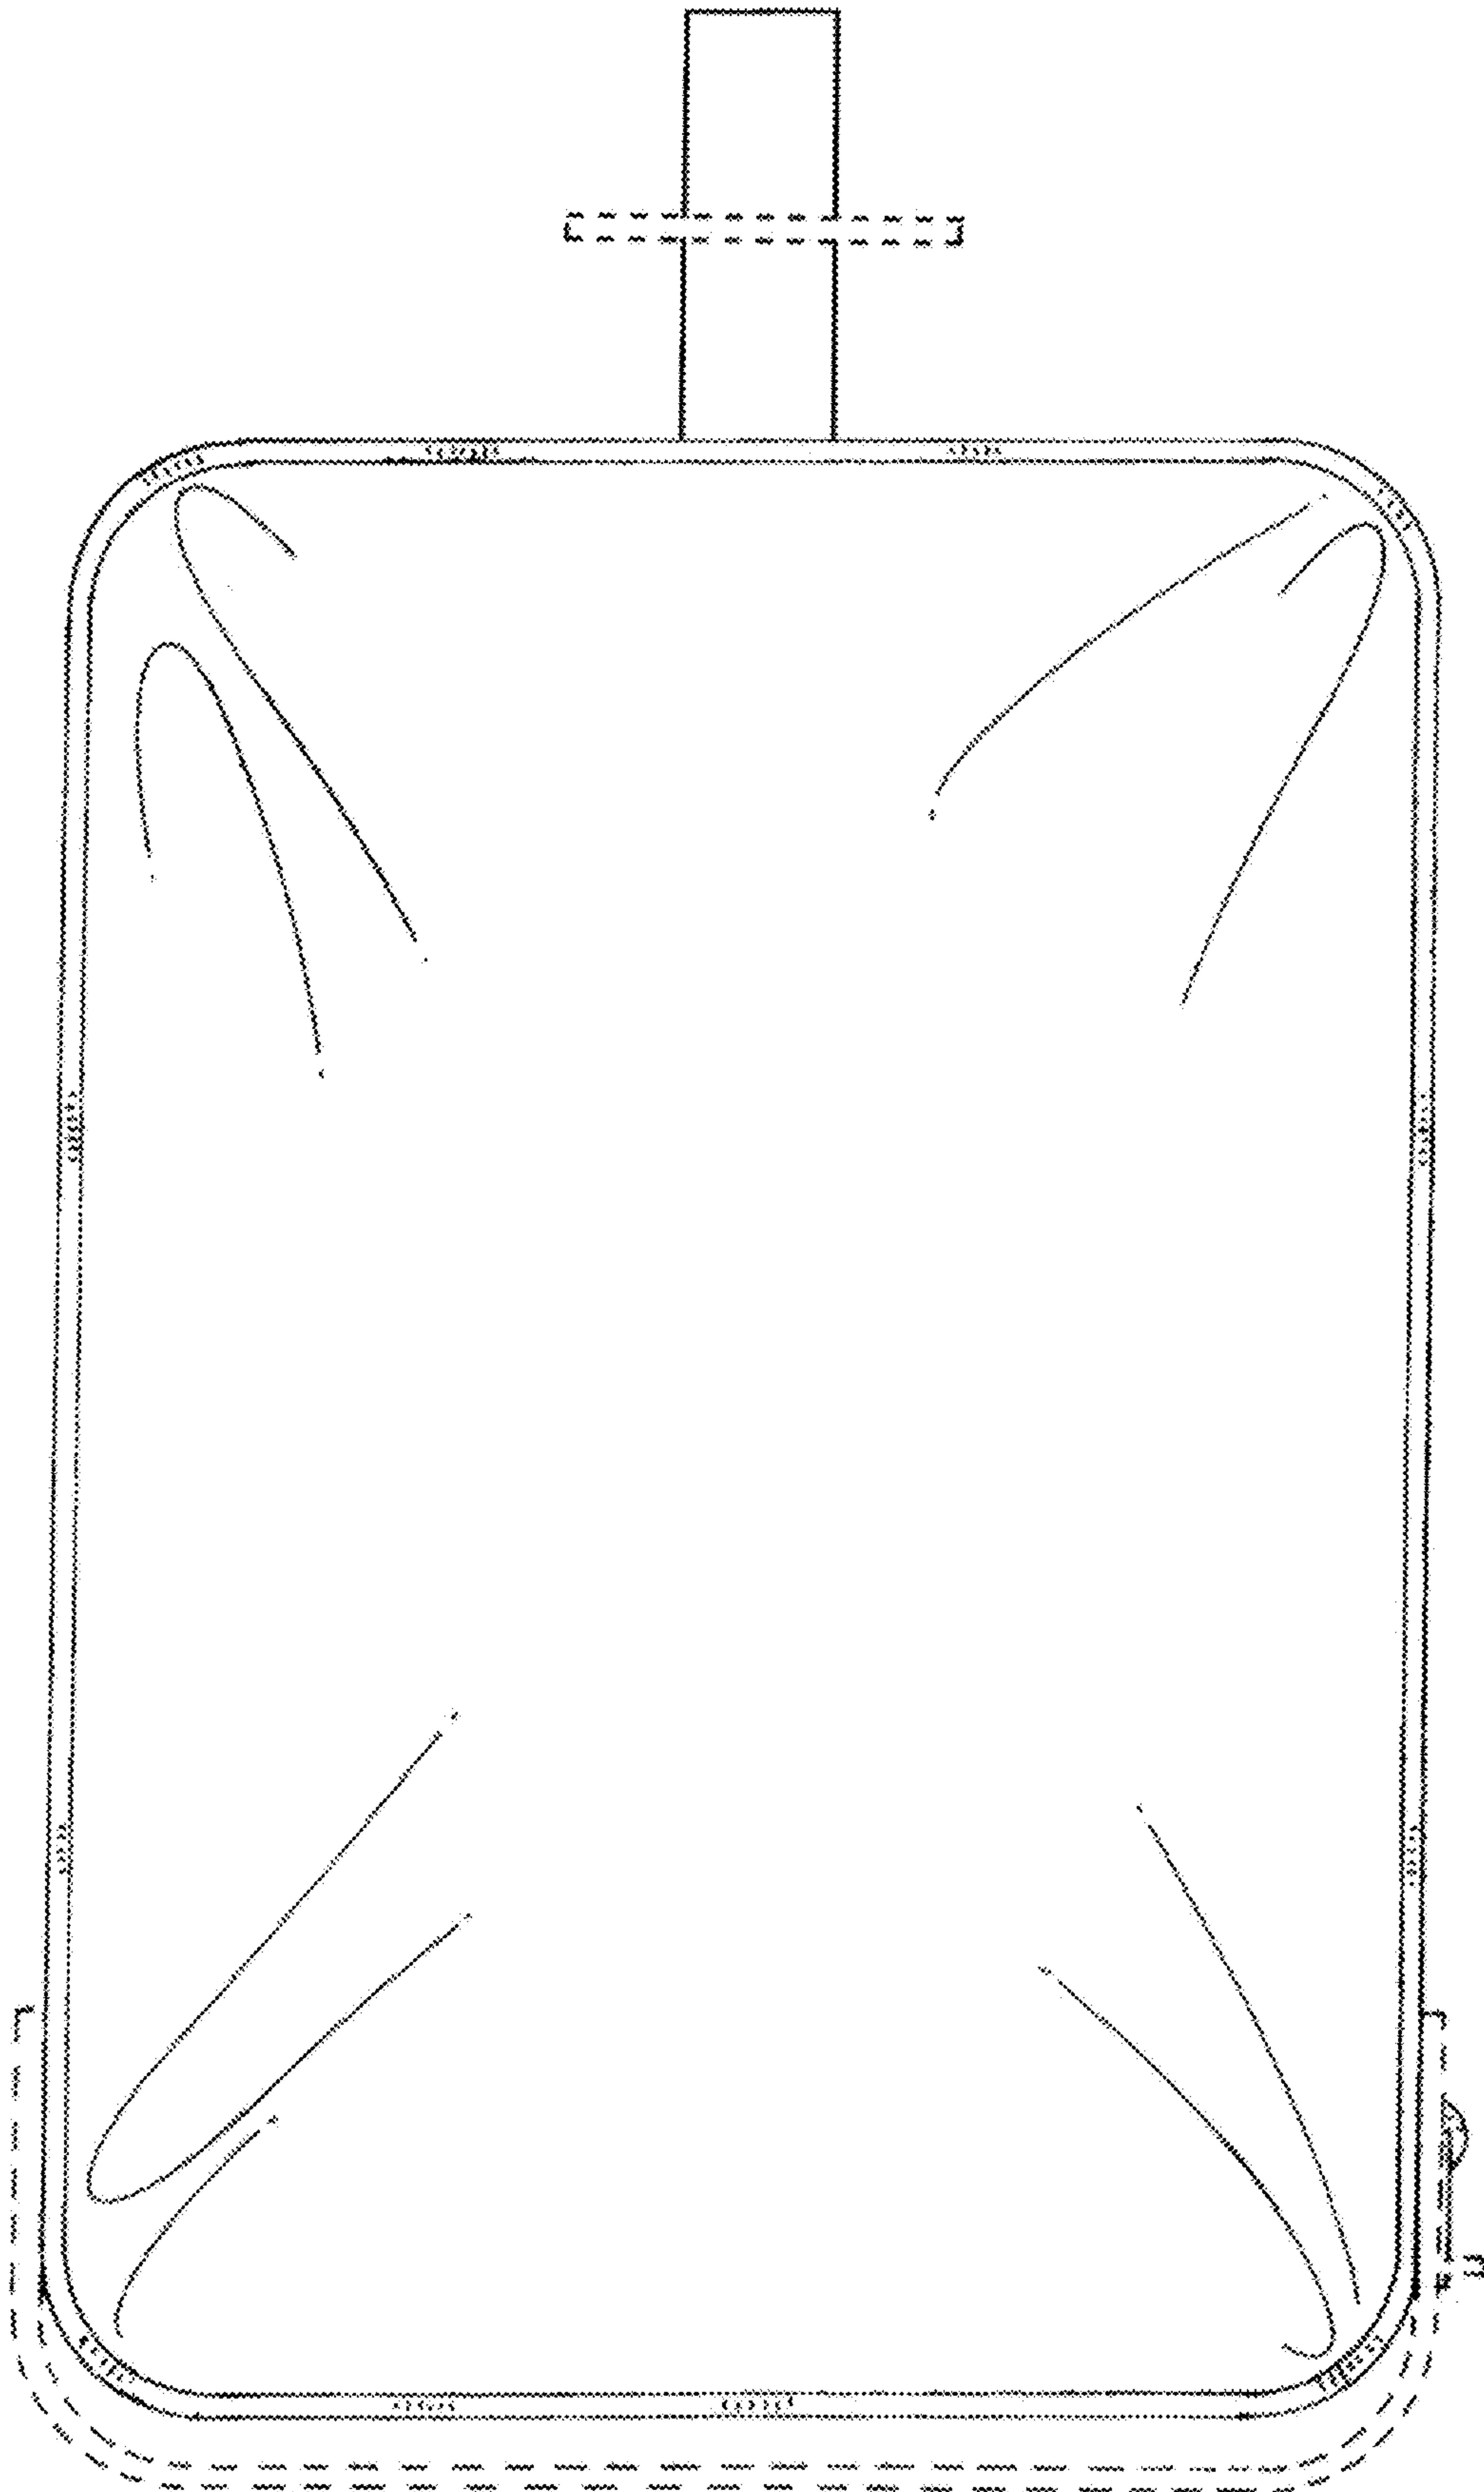


FIG. 3

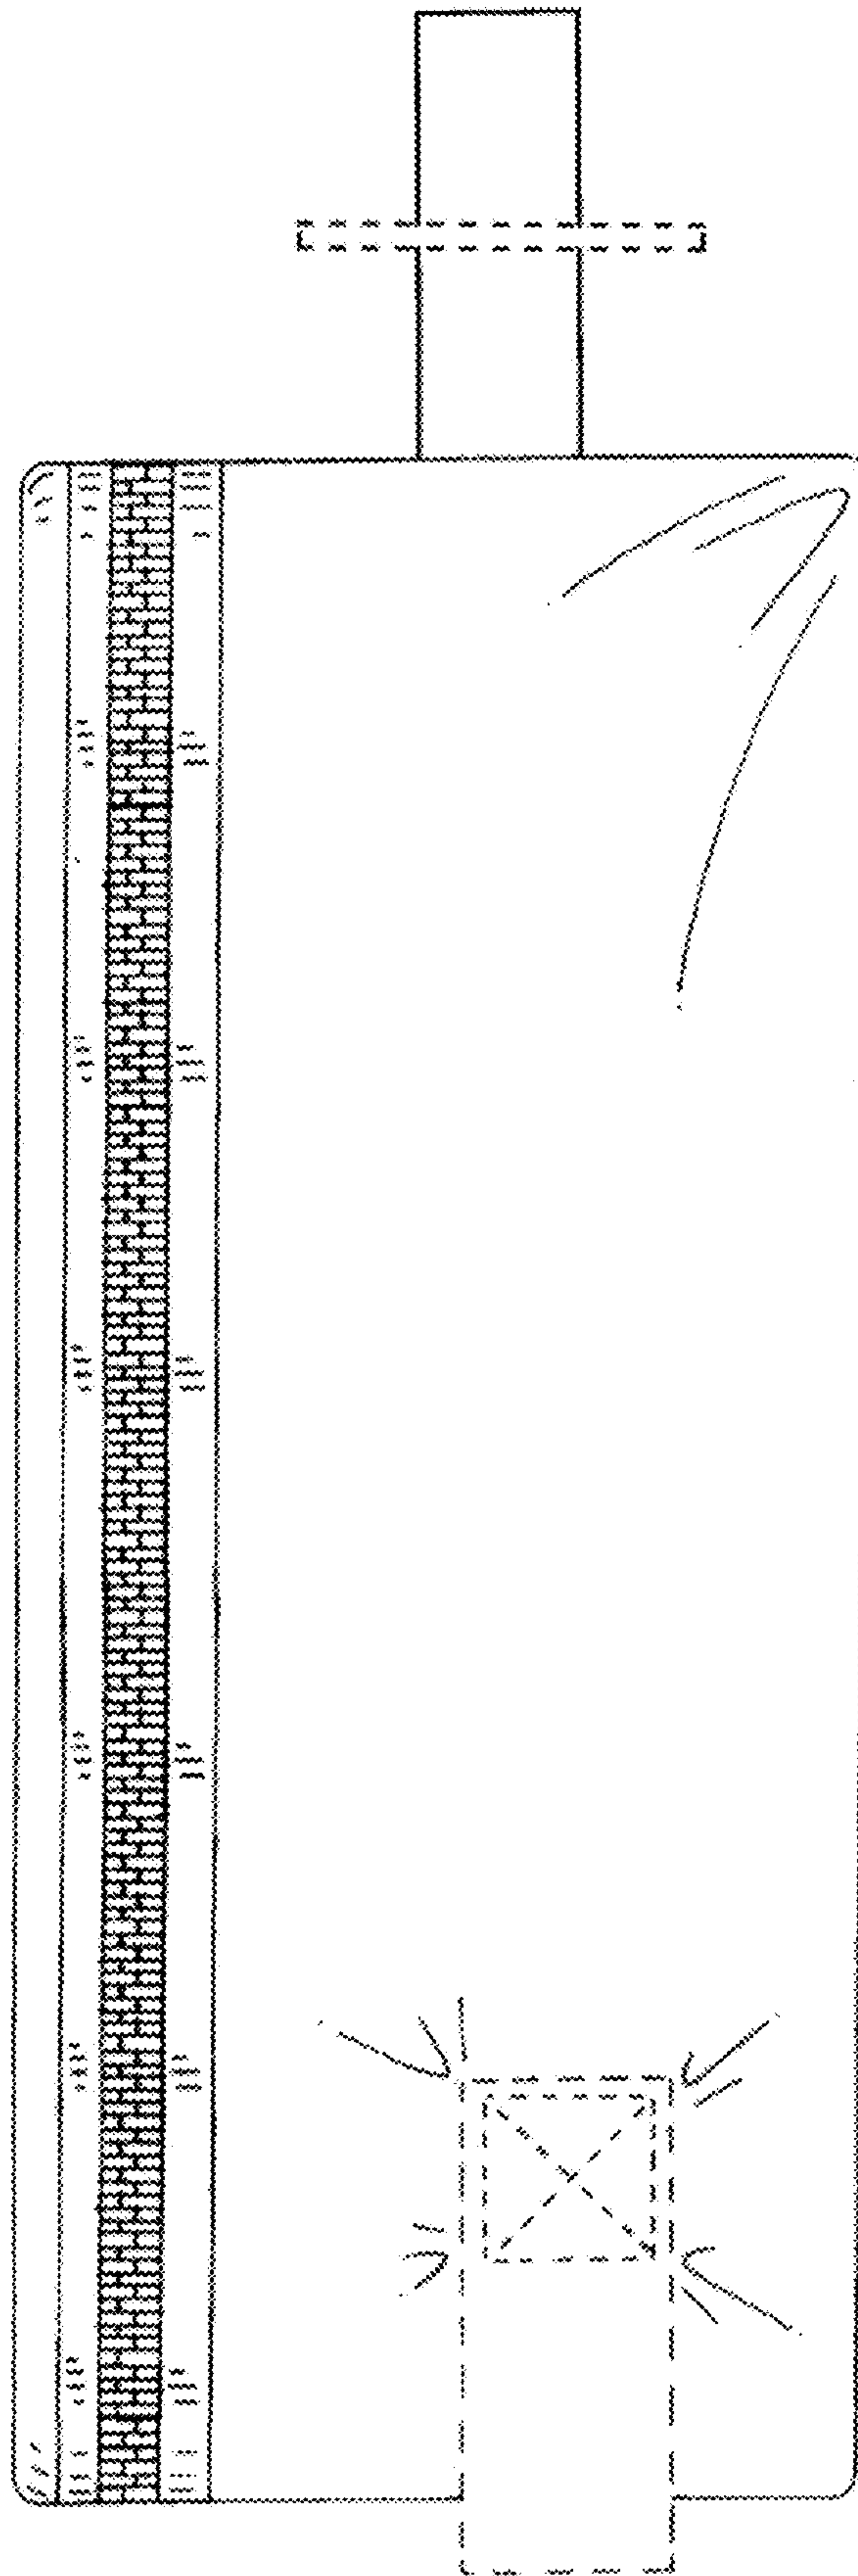


FIG. 4

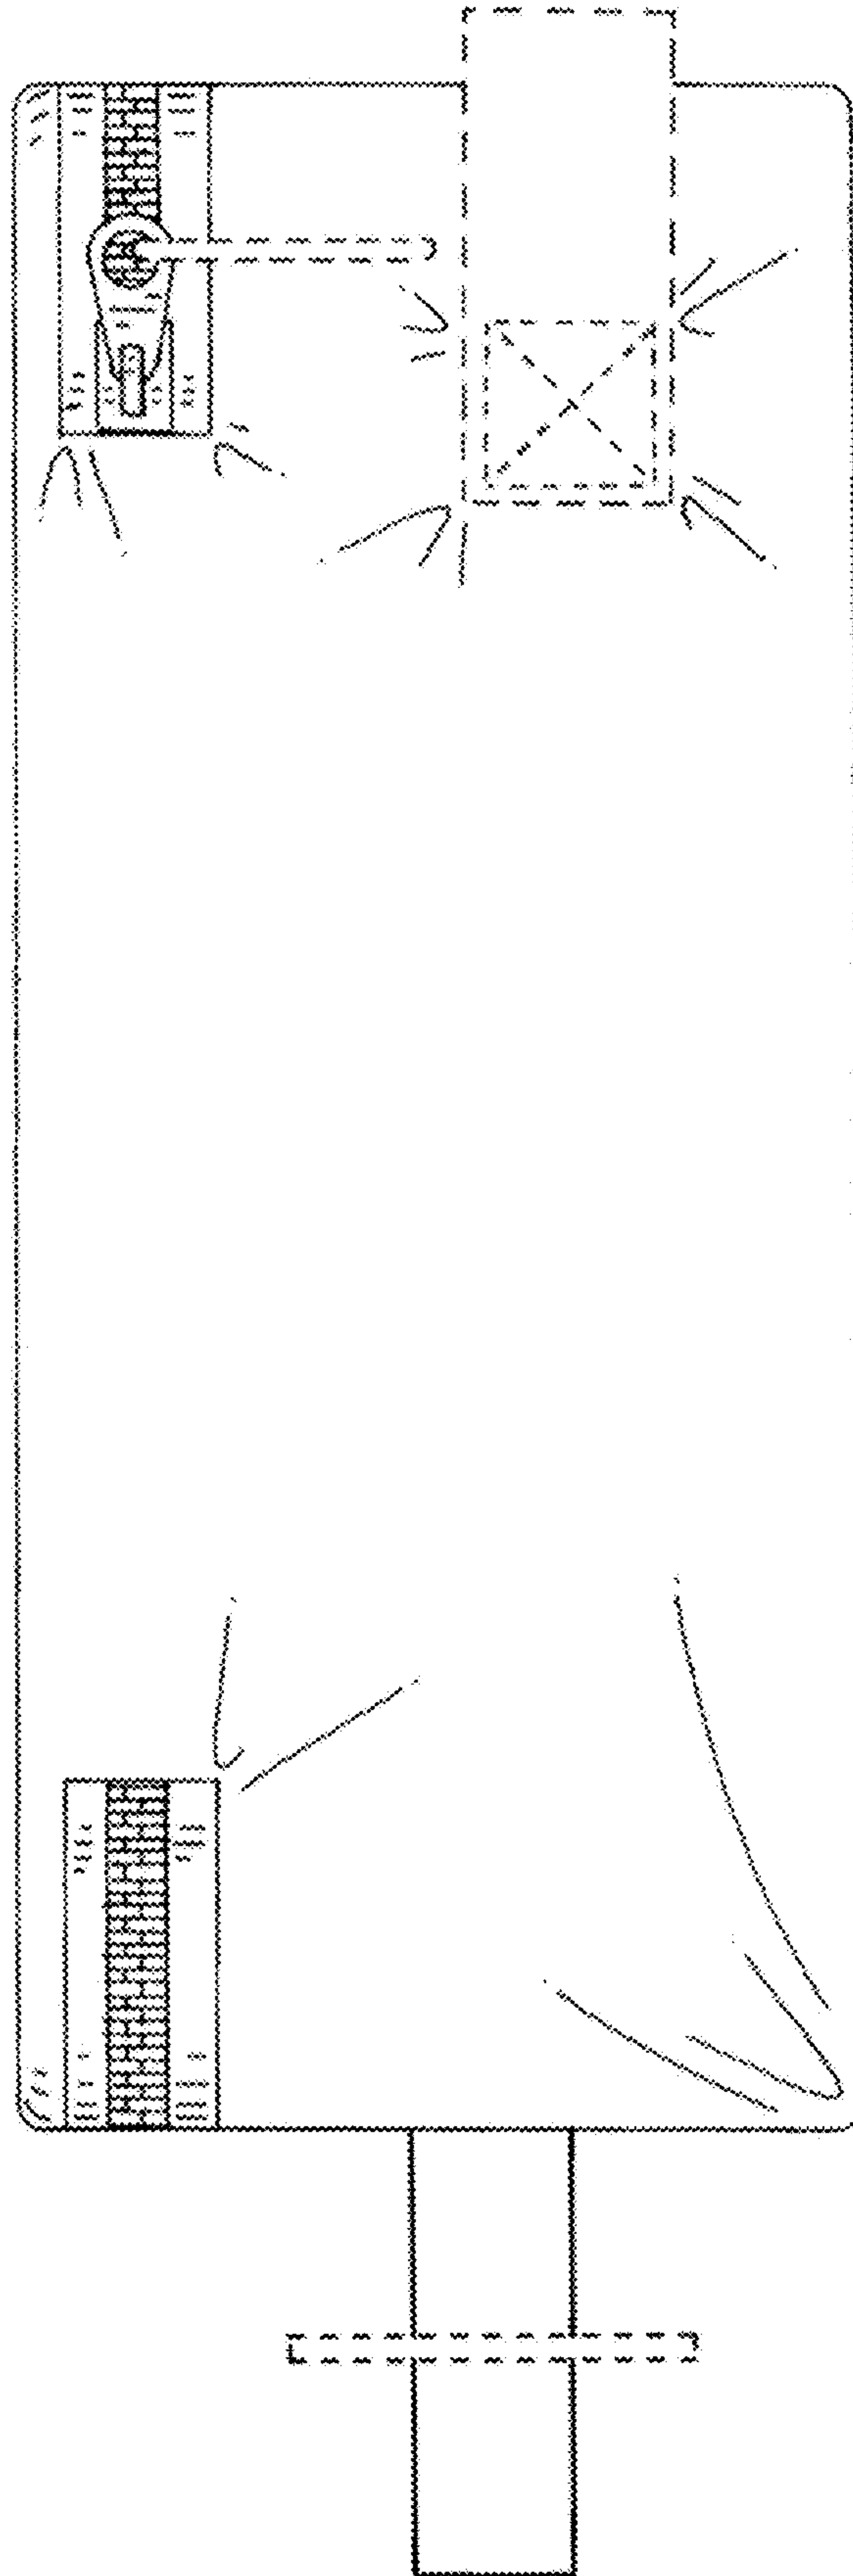


FIG. 5

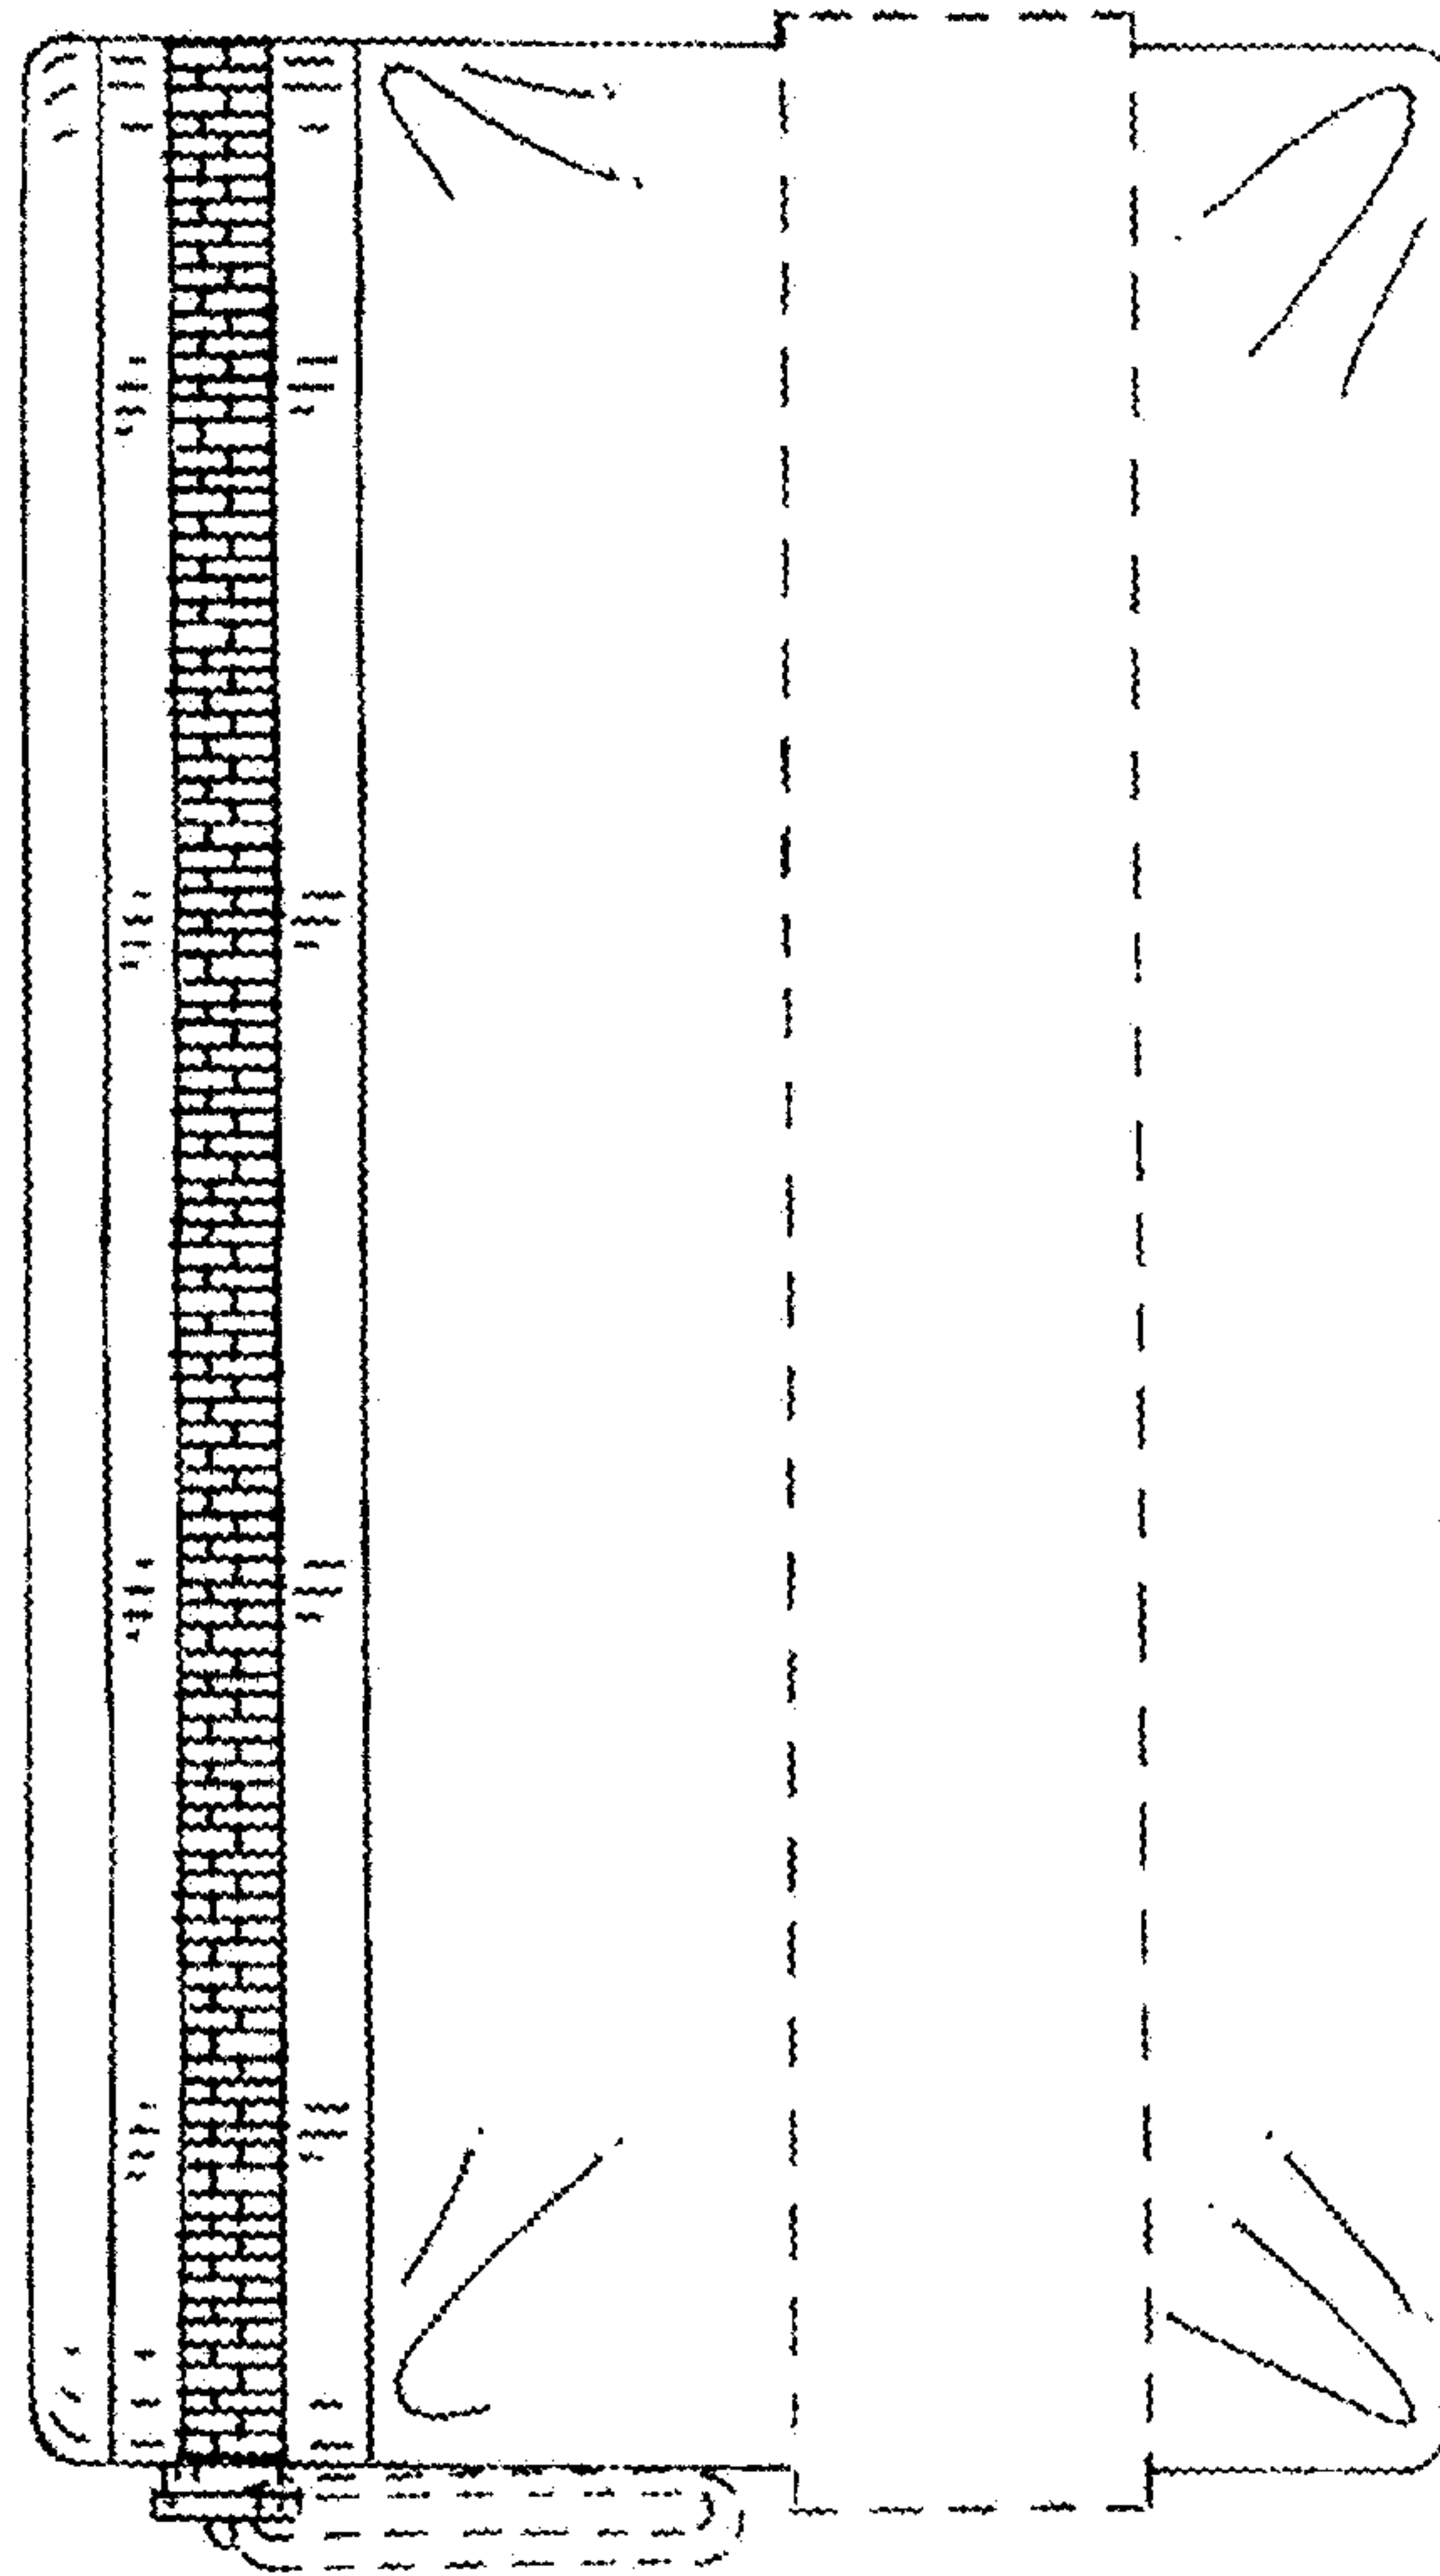


FIG. 6

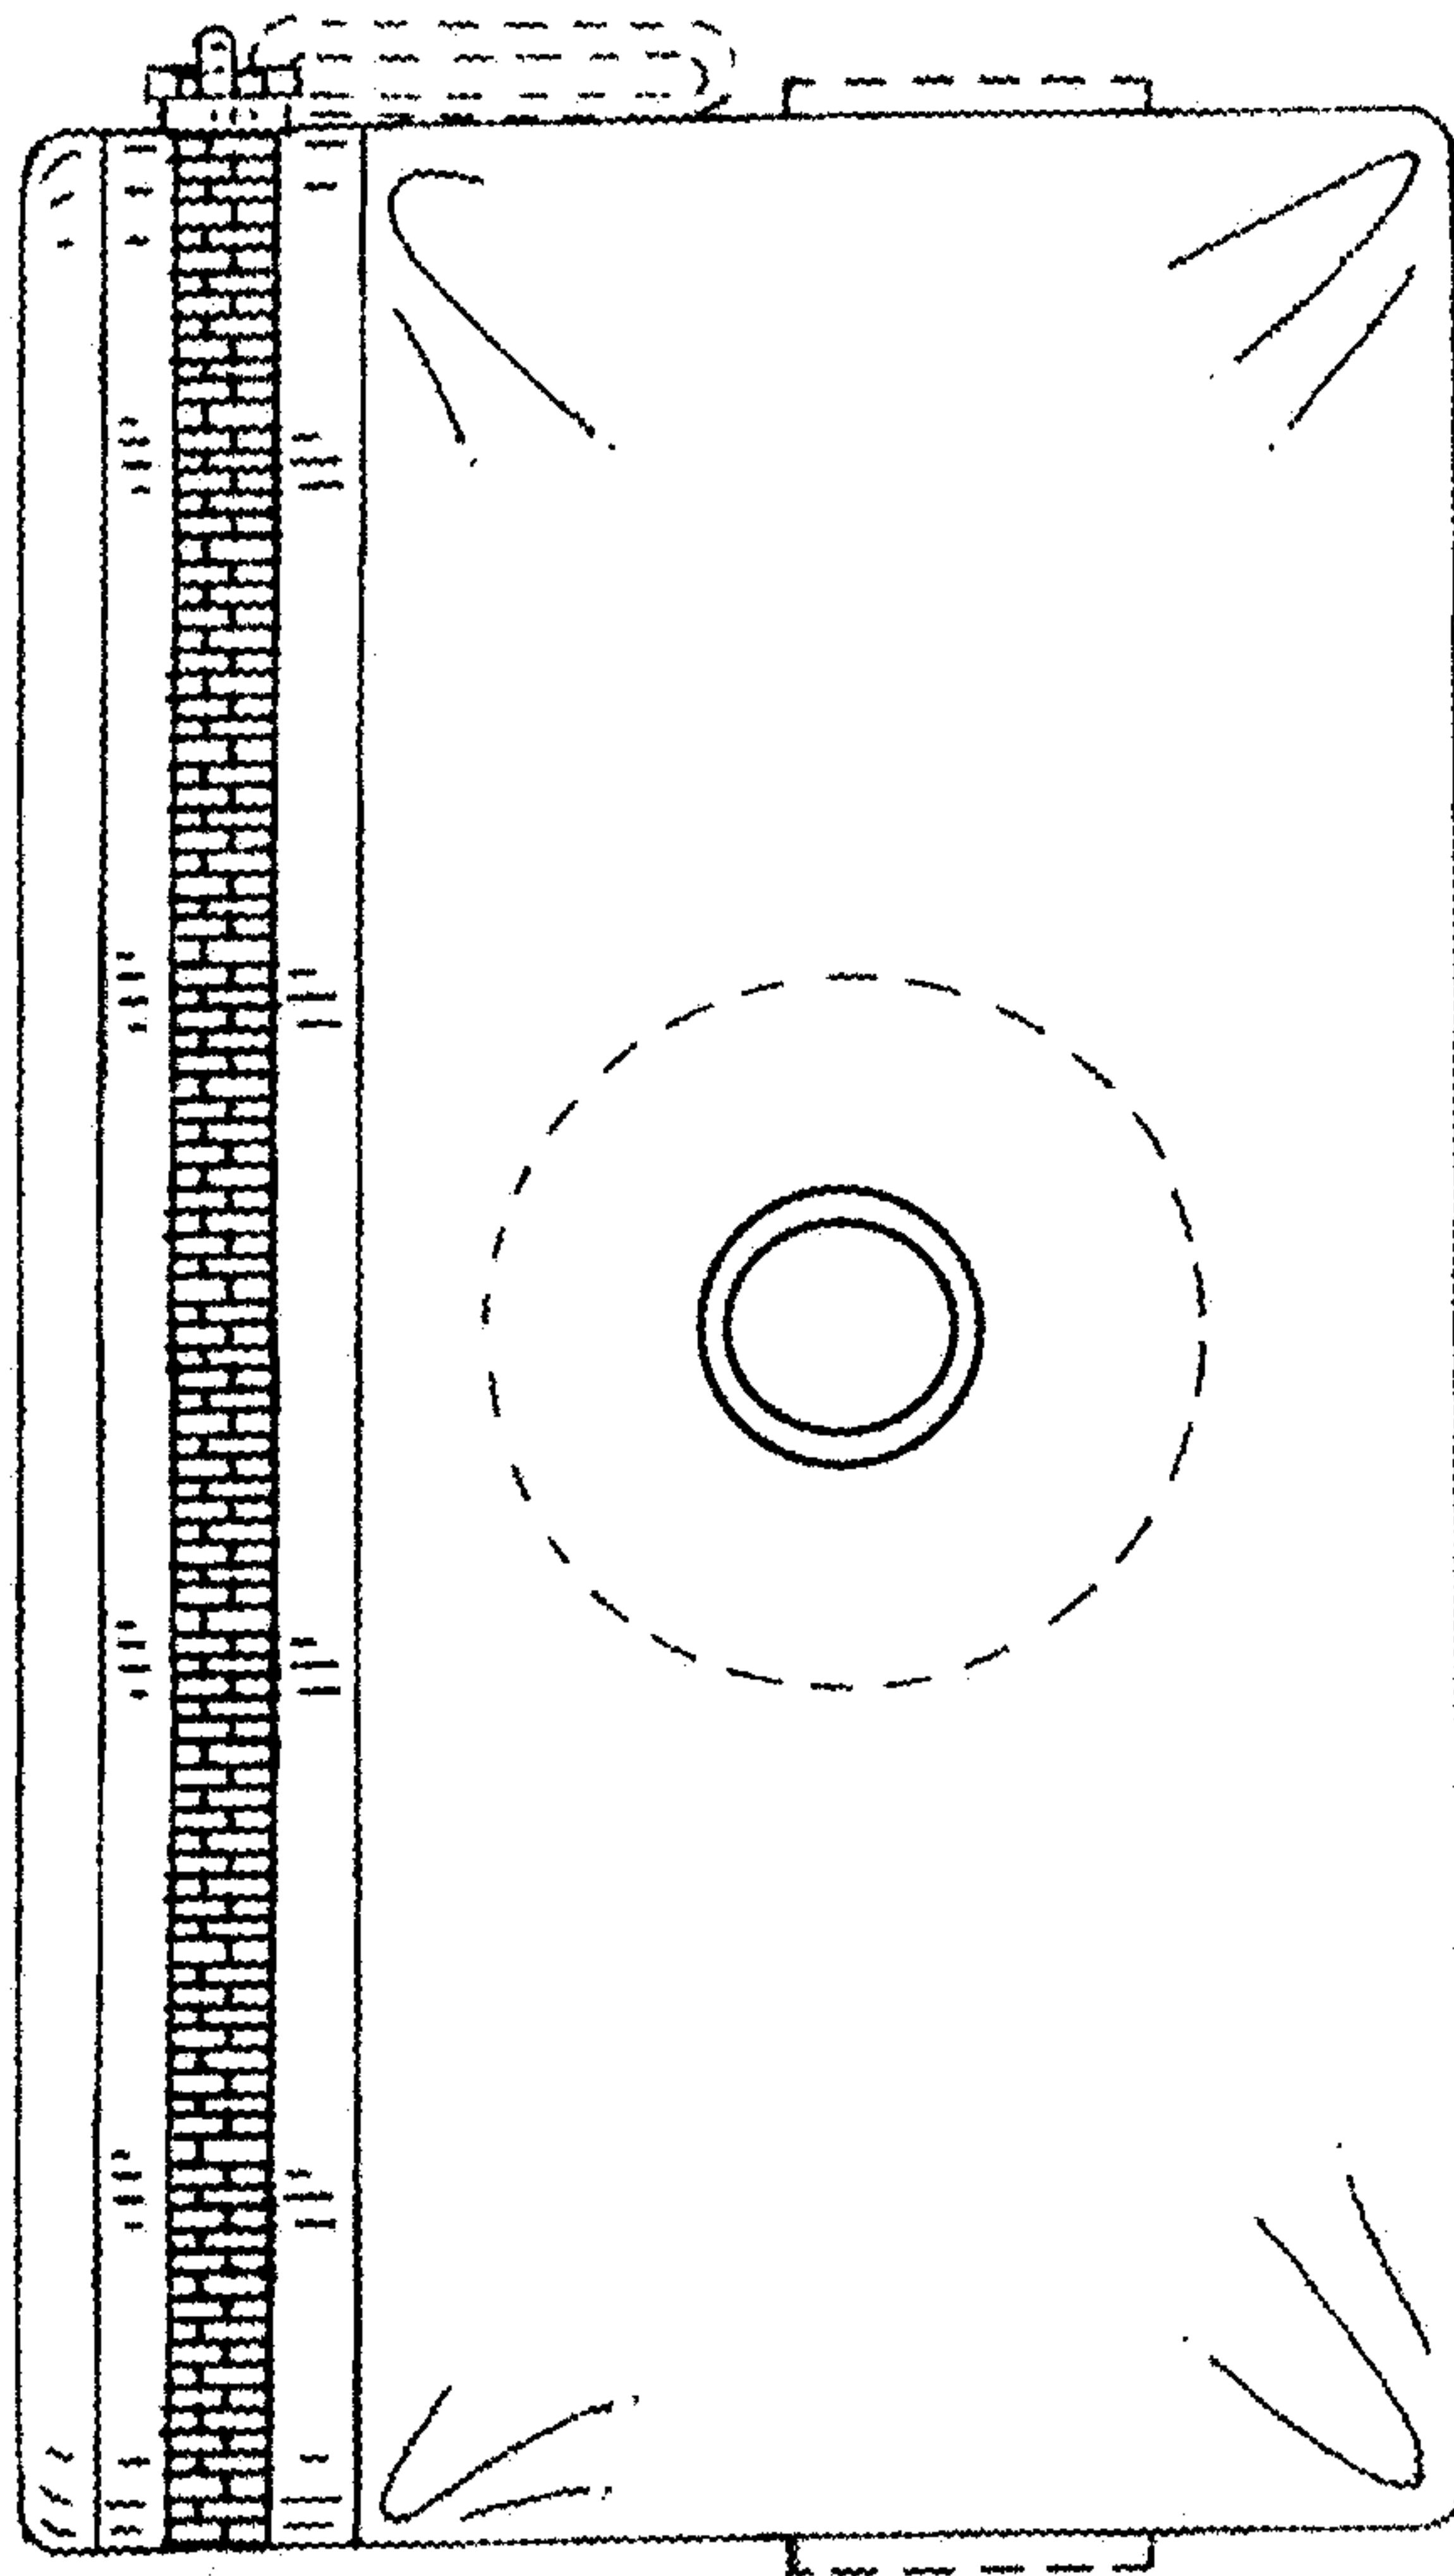


FIG. 7