



US00D886305S

(12) **United States Design Patent**  
**de Jonge et al.**

(10) **Patent No.:** **US D886,305 S**  
(45) **Date of Patent:** **\*\* Jun. 2, 2020**

(54) **ULTRASOUND PROBE**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **Butterfly Network, Inc.**, Guilford, CT (US)

JP D1457814 12/2012  
JP D151349 1/2015

(Continued)

(72) Inventors: **Matthew de Jonge**, New York, NY (US); **Christopher Thomas McNulty**, Guilford, CT (US); **David Elgena**, Brooklyn, NY (US); **Stephen Christopher**, Philadelphia, PA (US); **Paul Maxted**, Guilford, CT (US); **Jonathan C. Schultz**, Guildford, CT (US); **Benjamin Chopra**, Guilford, CT (US)

OTHER PUBLICATIONS

[No Author Listed], HDI 5000 Transducer Listing. Publicly known prior to Oct. 27, 2017. 6 pages.

(Continued)

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Wolf, Greenfield & Sacks, P.C.

(73) Assignee: **Butterfly Network, Inc.**, Guilford, CT (US)

(\*\*) Term: **15 Years**

(57) **CLAIM**

(21) Appl. No.: **29/677,073**

The ornamental design for an ultrasound probe, as shown and described.

(22) Filed: **Jan. 16, 2019**

**Related U.S. Application Data**

**DESCRIPTION**

(62) Division of application No. 29/623,977, filed on Oct. 27, 2017, now Pat. No. Des. 846,749.

(51) **LOC (12) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/187**; D24/186

(58) **Field of Classification Search**  
USPC ..... D24/152, 158, 160, 161, 186, 187, 231;  
D10/78; D14/420, 426  
CPC ..... A61B 8/445; A61B 8/4455; A61B 8/4461  
See application file for complete search history.

FIG. 1 is a bottom, front, right side perspective view of an ultrasound probe showing our new design; FIG. 2 is a front elevation view thereof; FIG. 3 is a rear elevation view thereof; FIG. 4 is a left side elevation view thereof; FIG. 5 is a right side elevation view thereof; FIG. 6 is a top plan view thereof; and, FIG. 7 is a bottom plan view thereof.

The dot-dash broken lines in the figures represent boundaries of the claimed design and form no part thereof. All other broken lines illustrate portions of the ultrasound probe that form no part of the claimed design.

The ultrasound probe is shown with a symbolic break in its length. The appearance of any portion of the article between the break lines forms no part of the claimed design.


(56) **References Cited**

U.S. PATENT DOCUMENTS

D545,433 S 6/2007 Messerly et al.  
D681,824 S 5/2013 Shinohara et al.  
D703,332 S \* 4/2014 Saeki ..... D24/187  
D703,821 S \* 4/2014 Moon ..... D24/187

(Continued)

**1 Claim, 4 Drawing Sheets**

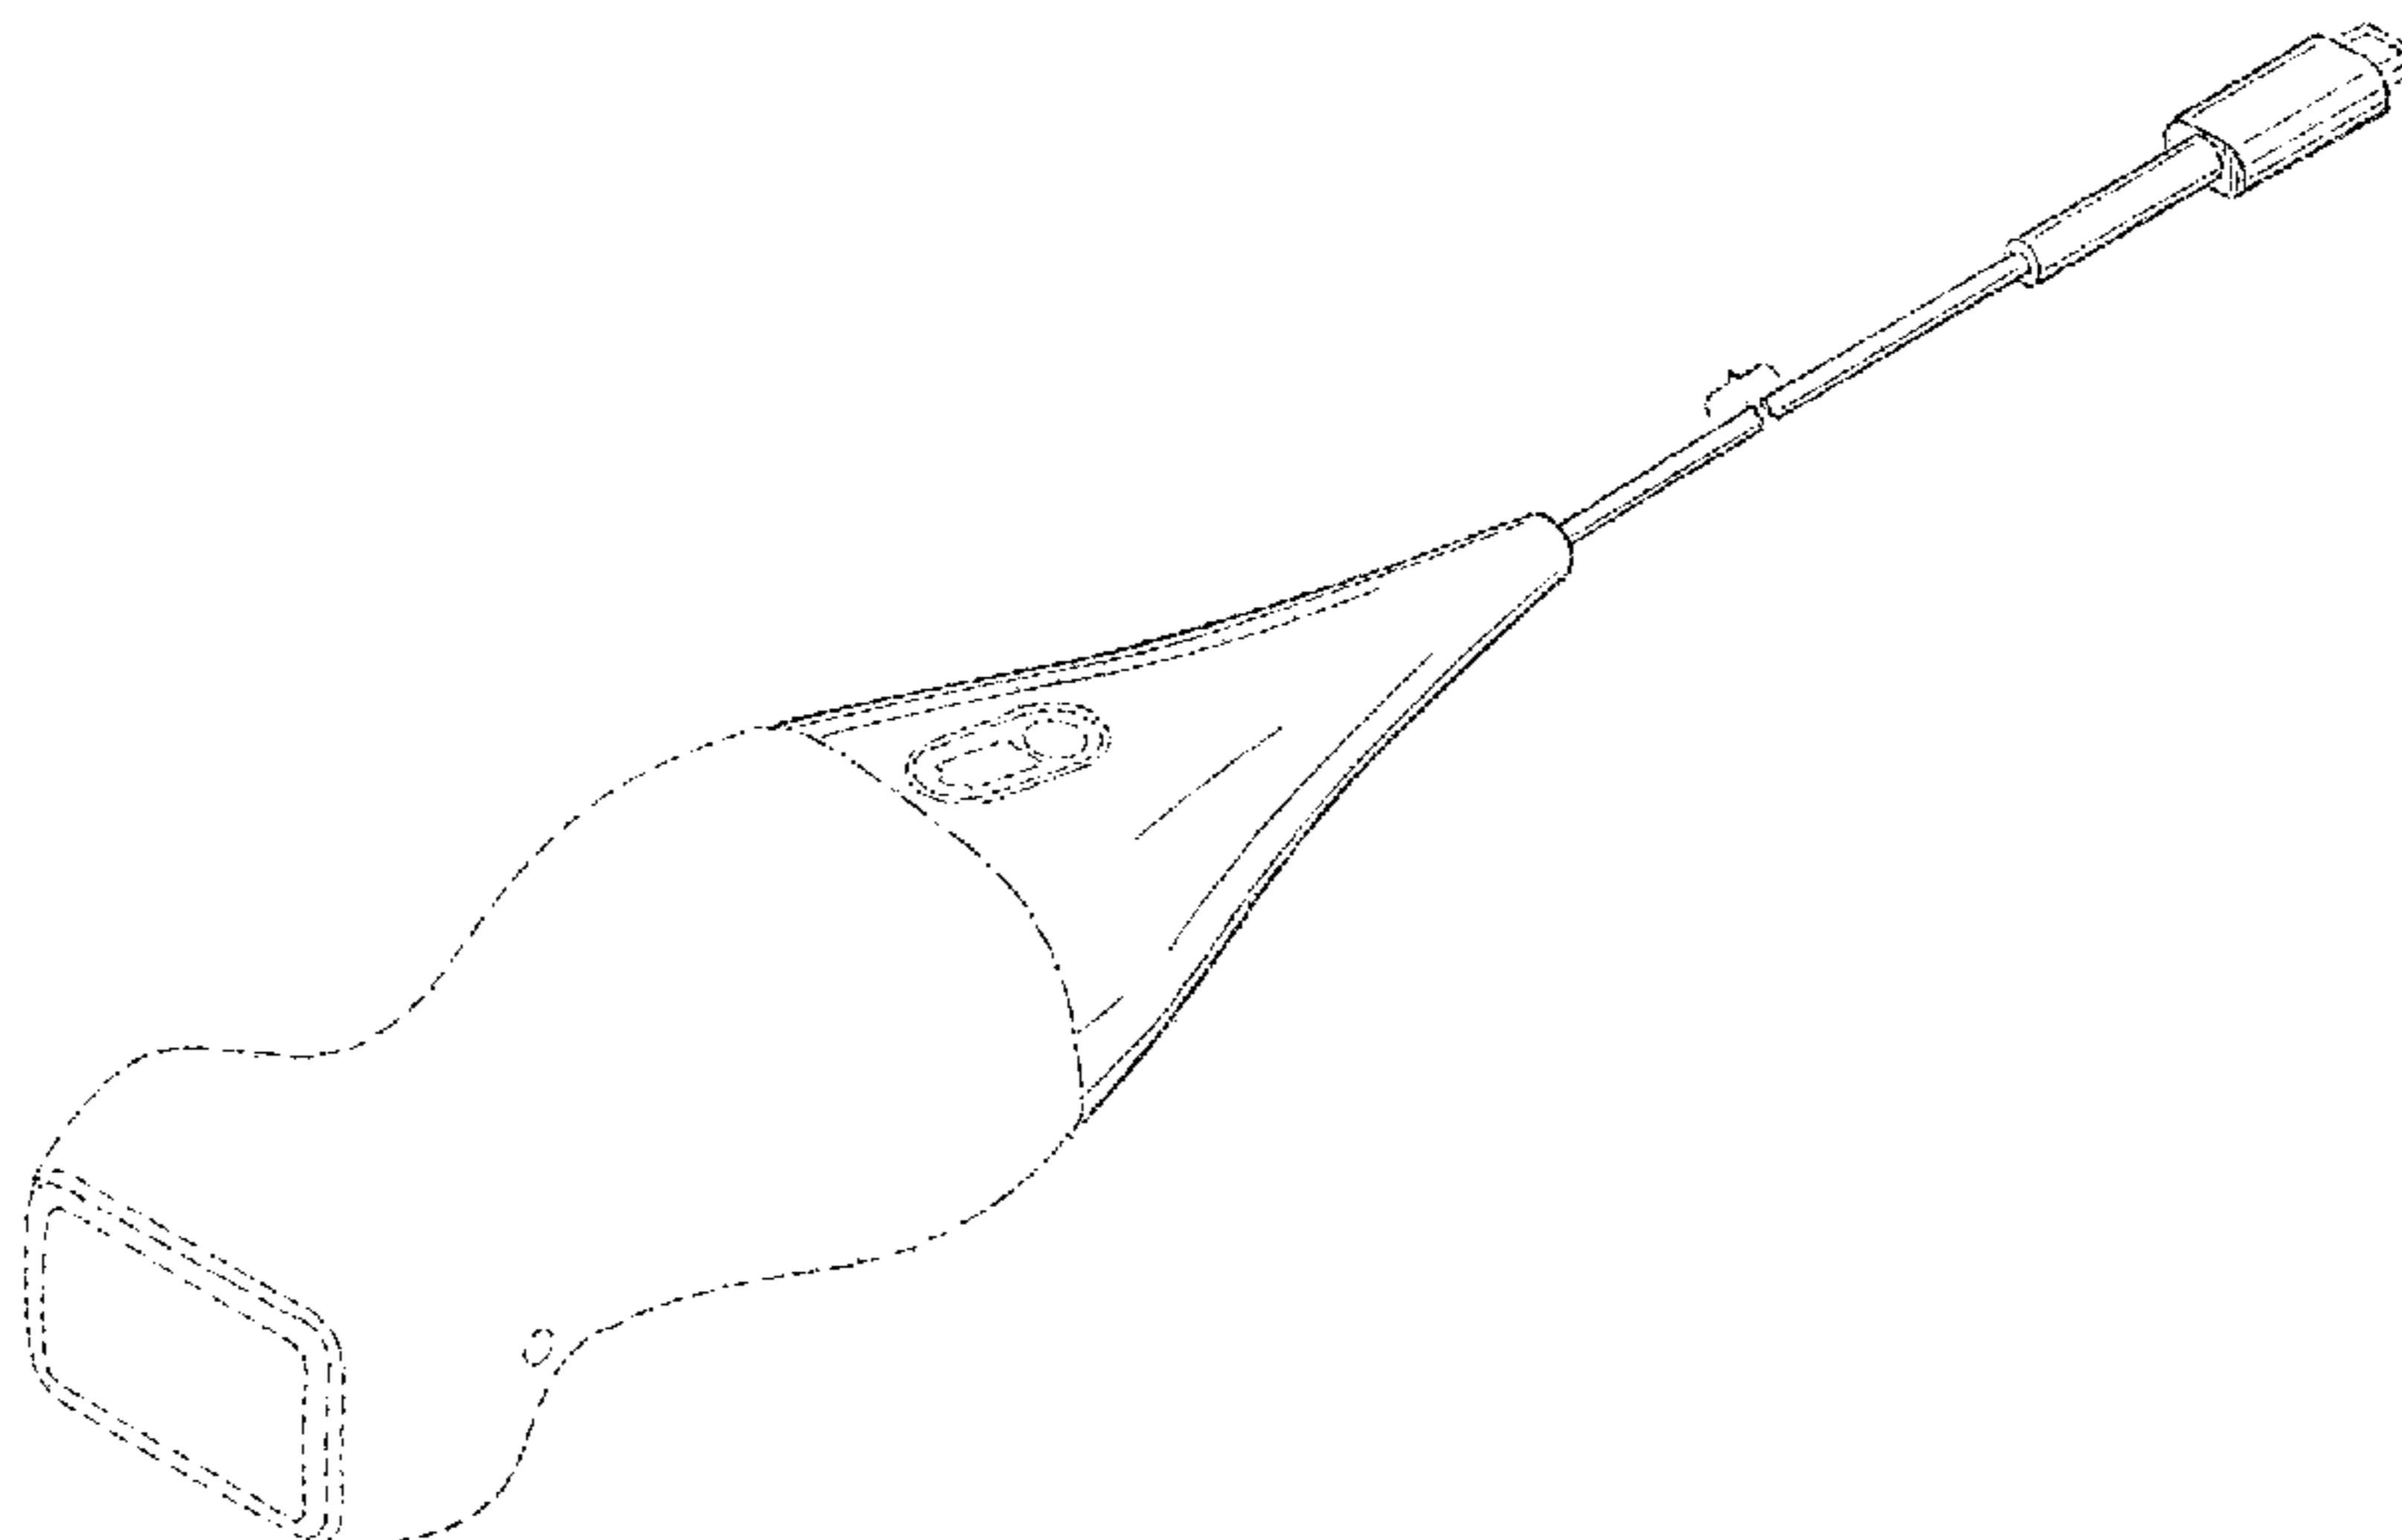

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D704,844	S	5/2014	Saeki	
9,072,487	B2	7/2015	Hebrard et al.	
D745,175	S	12/2015	Kitayama	
D749,224	S *	2/2016	Iritani .....	D24/187
D816,850	S	5/2018	Asai et al.	
D831,219	S *	10/2018	Henderson .....	D24/187
D846,128	S *	4/2019	de Jonge .....	D24/187
D846,749	S *	4/2019	de Jonge .....	D24/187
2011/0055447	A1	3/2011	Costa	
2015/0112200	A1	4/2015	Oberg et al.	
2017/0172542	A1	6/2017	Lee et al.	
2017/0360397	A1	12/2017	Rothberg et al.	
2017/0360401	A1	12/2017	Rothberg et al.	
2018/0028159	A1	2/2018	Hageman et al.	

FOREIGN PATENT DOCUMENTS


JP	D1564542	12/2016
JP	D1593697	12/2017
KR	30-0726181	1/2014
KR	30-0726182	1/2014
KR	30-0751362	7/2014
KR	30-0764107	10/2014

OTHER PUBLICATIONS


Declaration of David Elgena, signed May 11, 2018, submitted to the Japanese Patent Office in co-pending application No. JP 2018-009209.

Enriquez et al., An Introduction to Ultrasound Equipment and Knobology. Crit Care Clin. Jan. 2014; 30(1):25-45.


\* cited by examiner

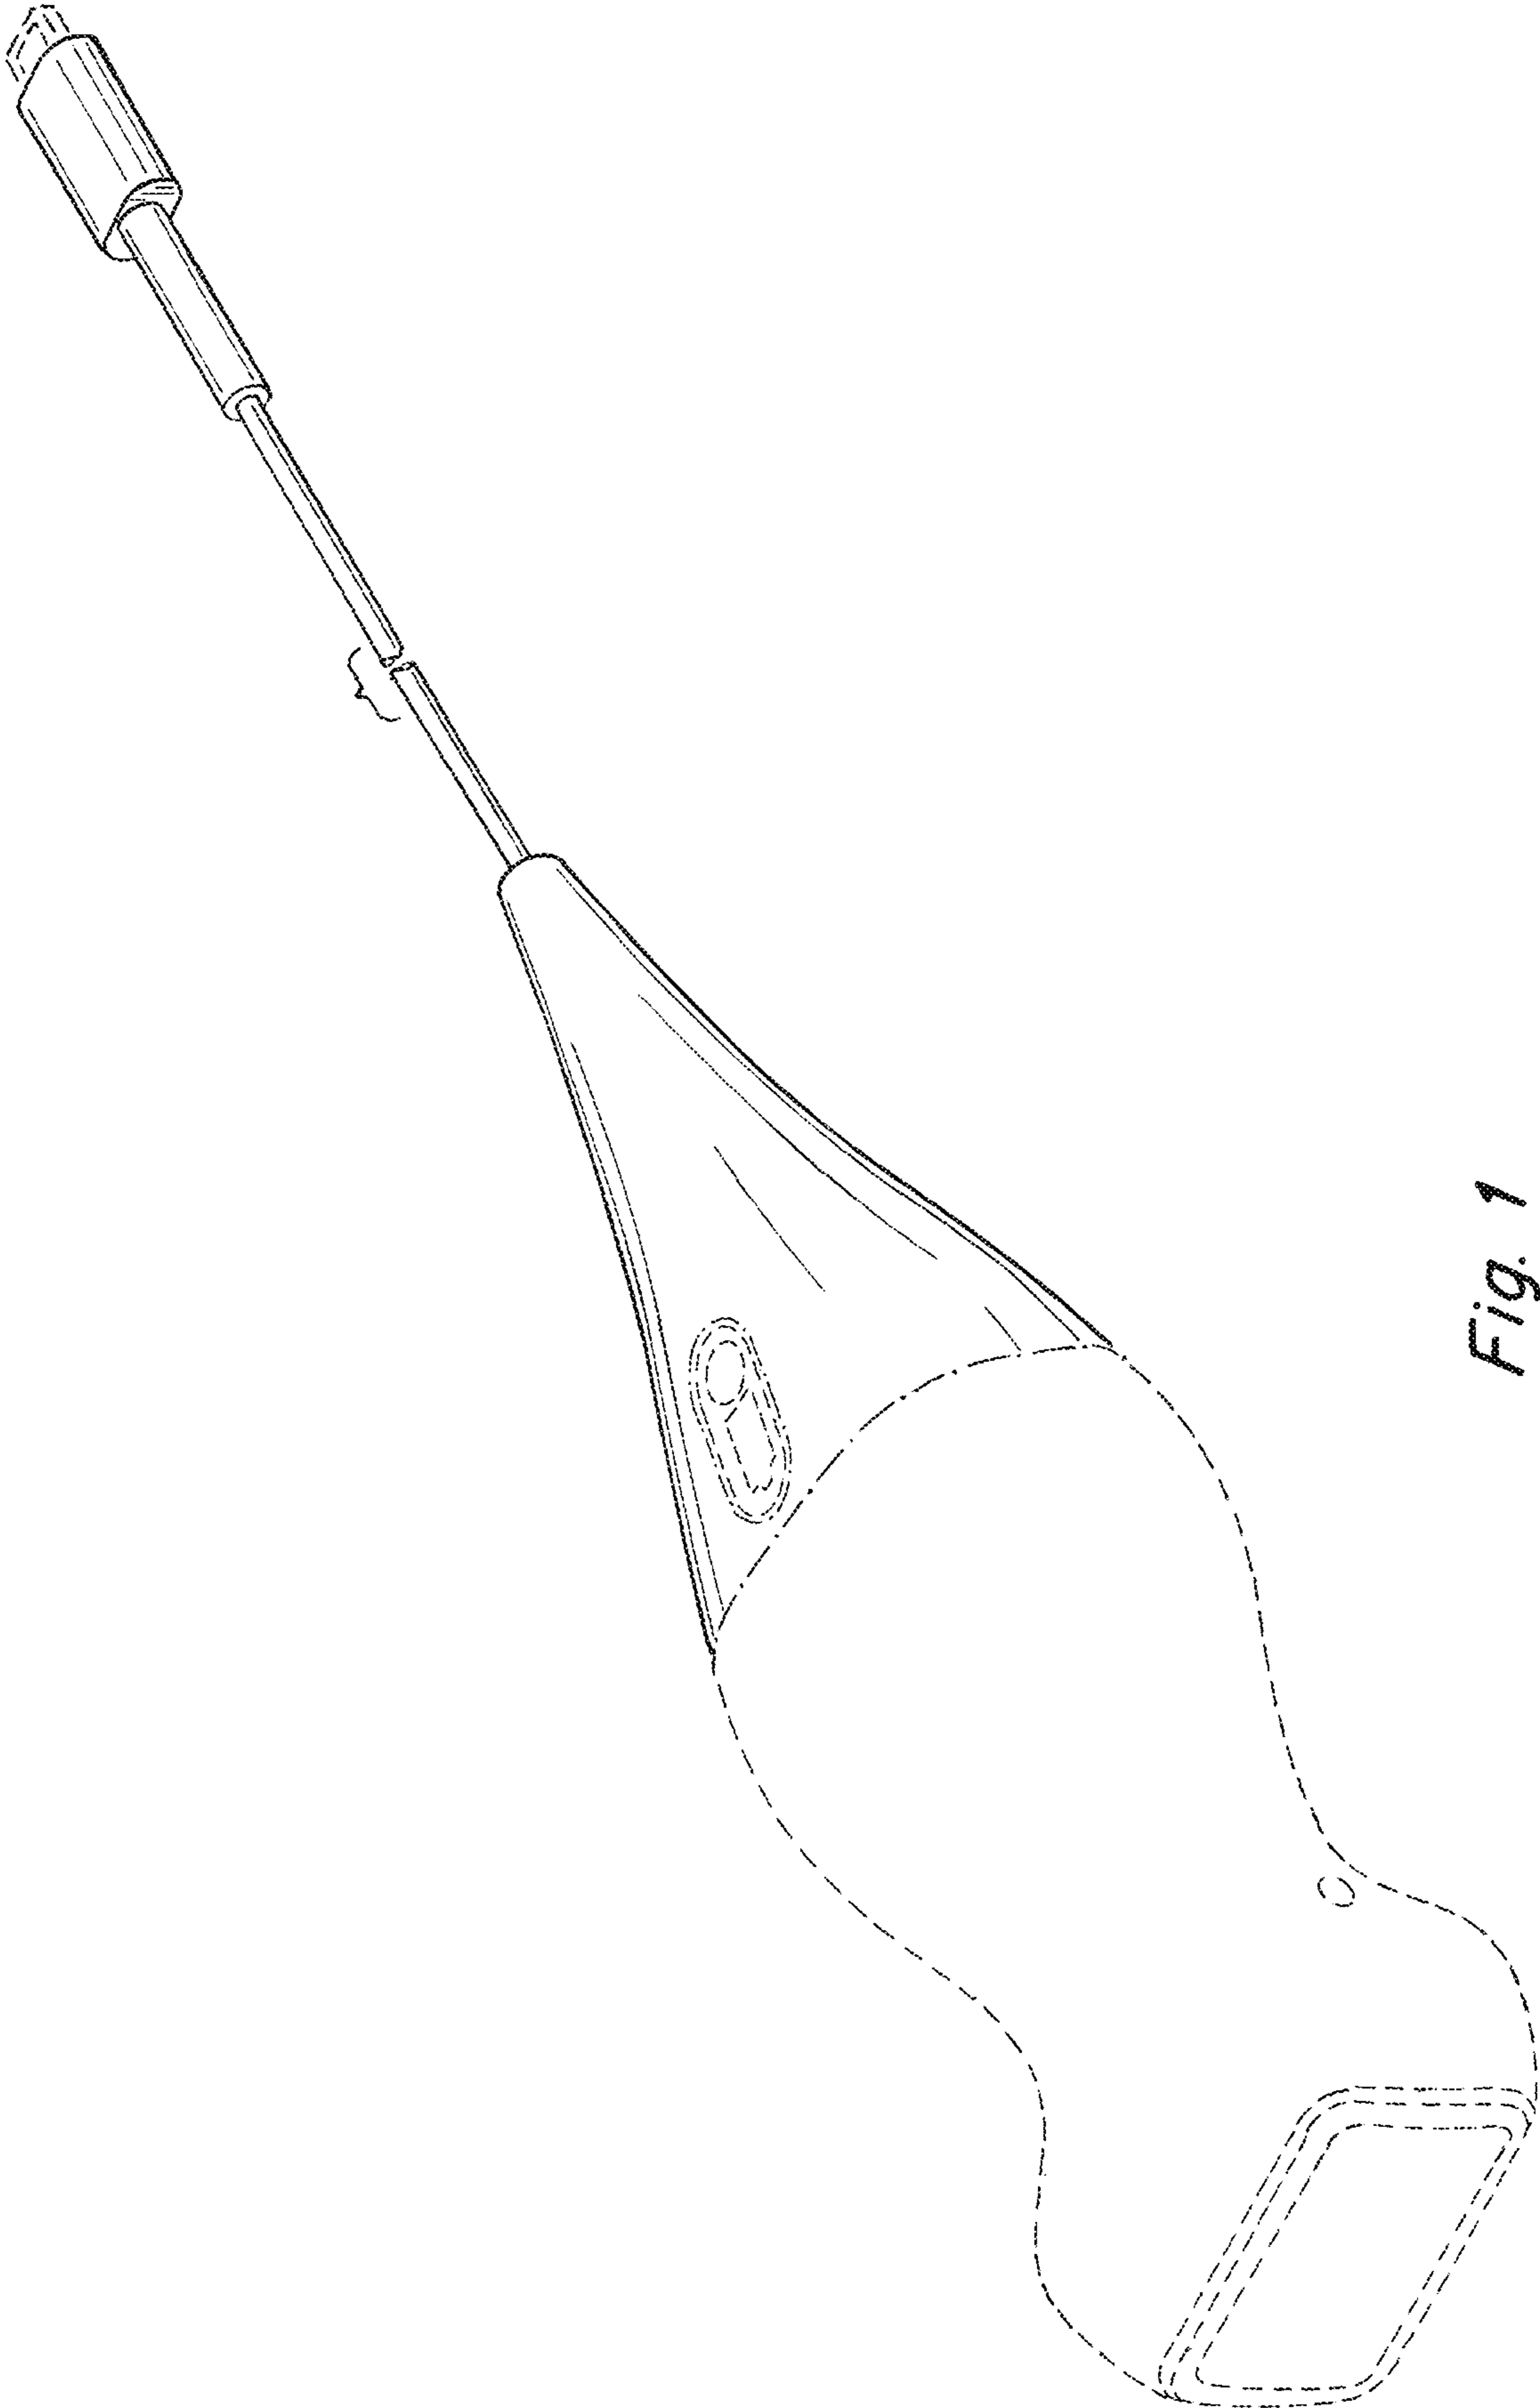


*Fig. 1*

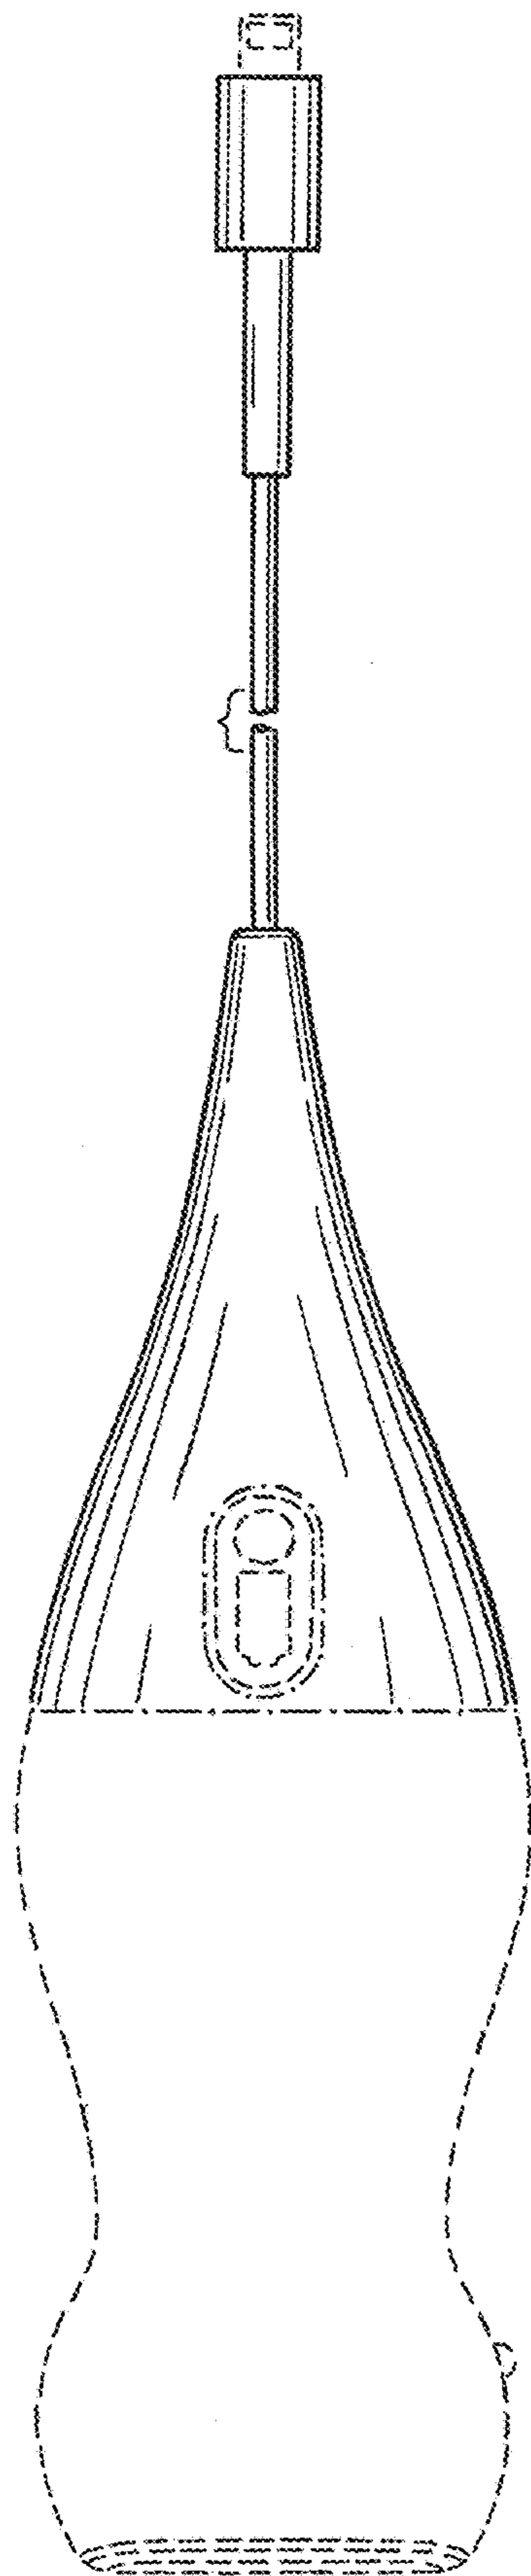


*Fig. 2*

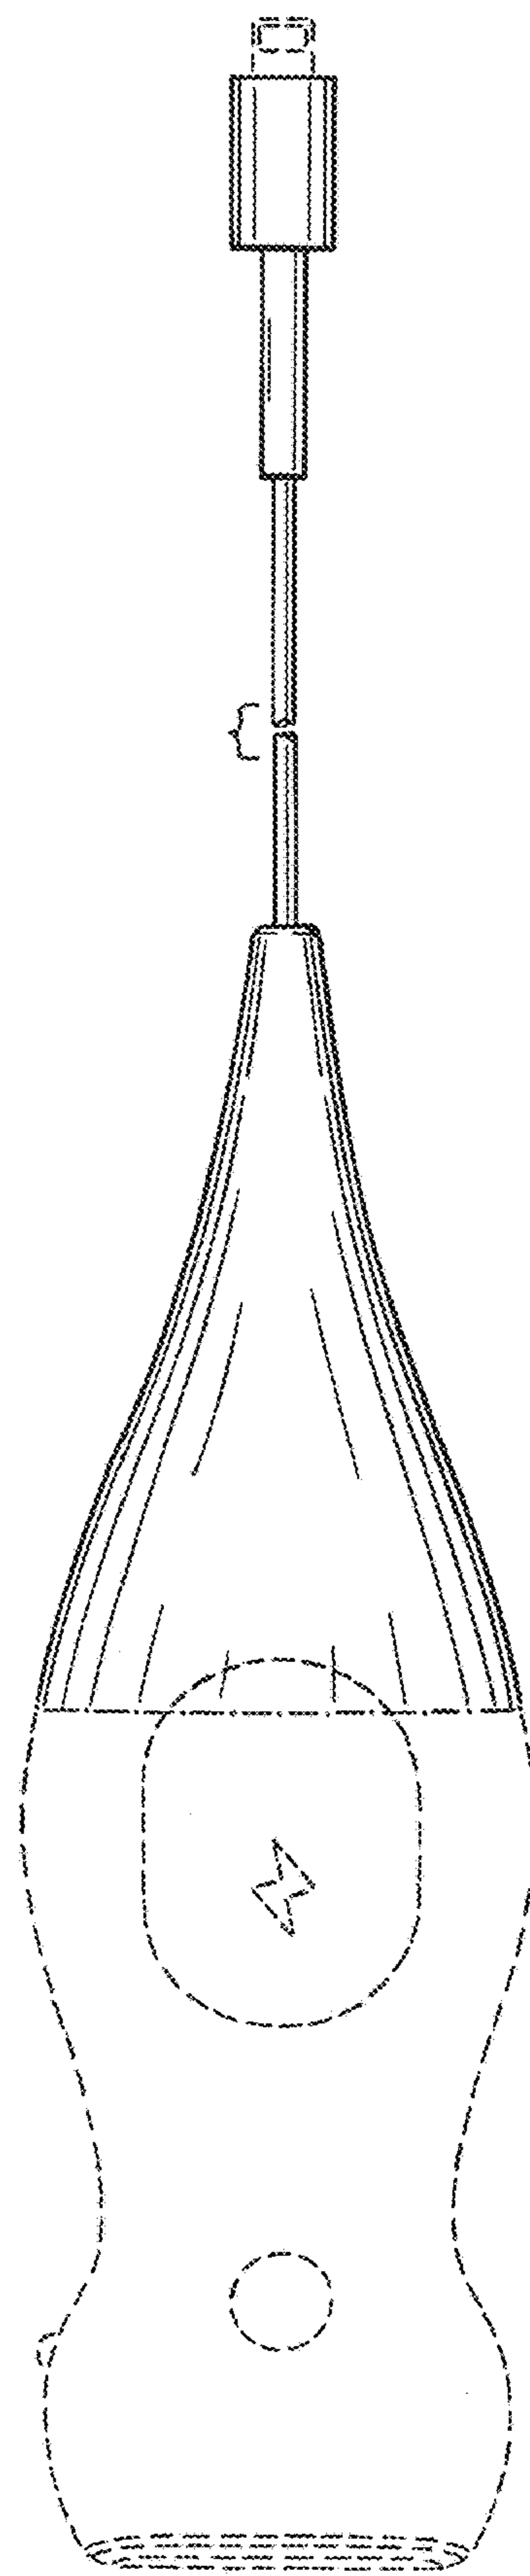


*Fig. 3*

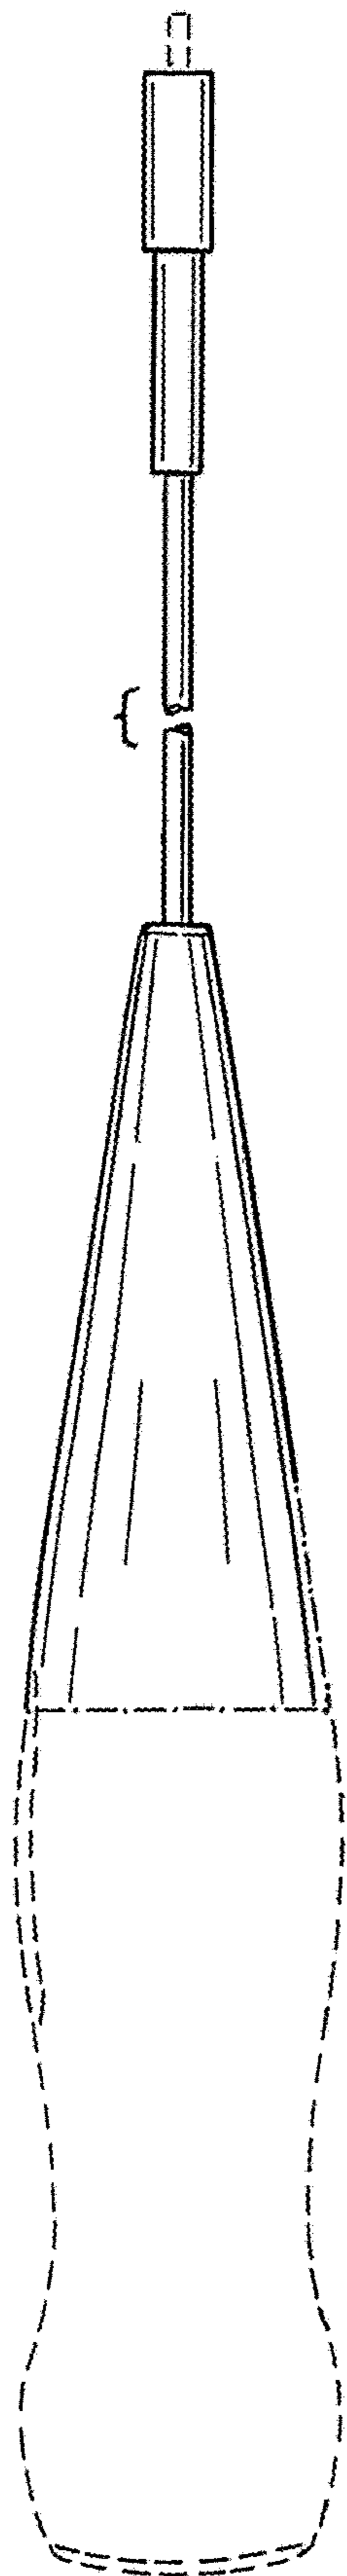


*Fig. 4*

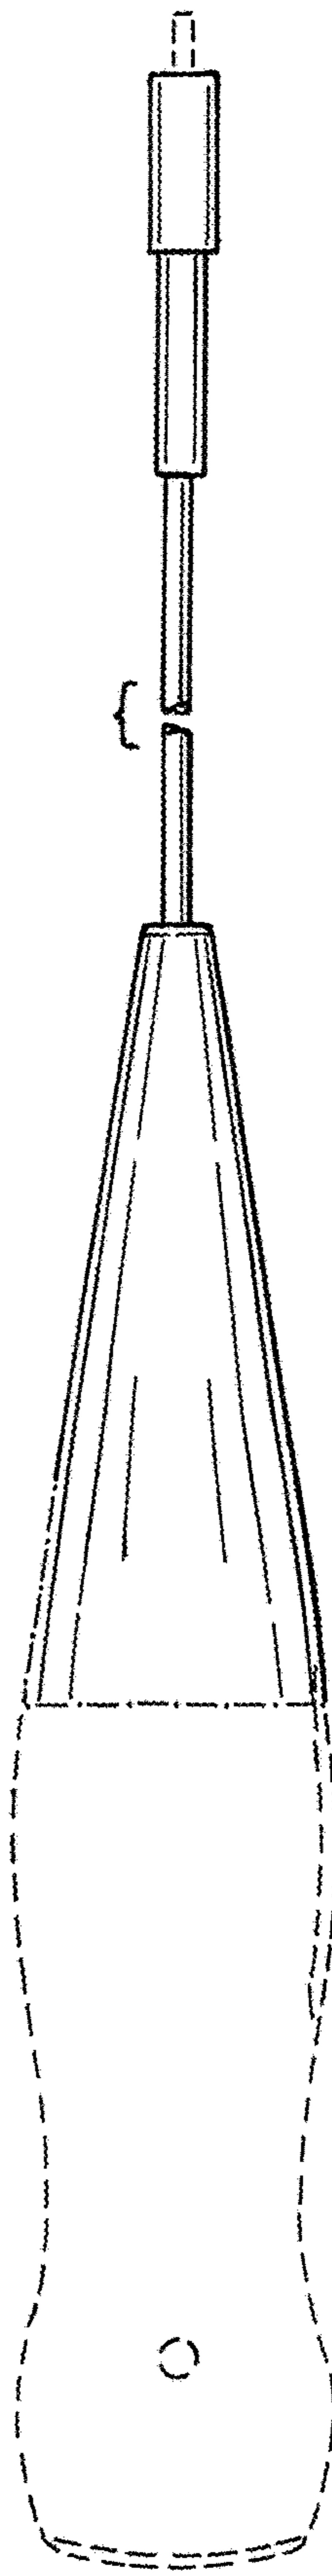

*Fig. 5*

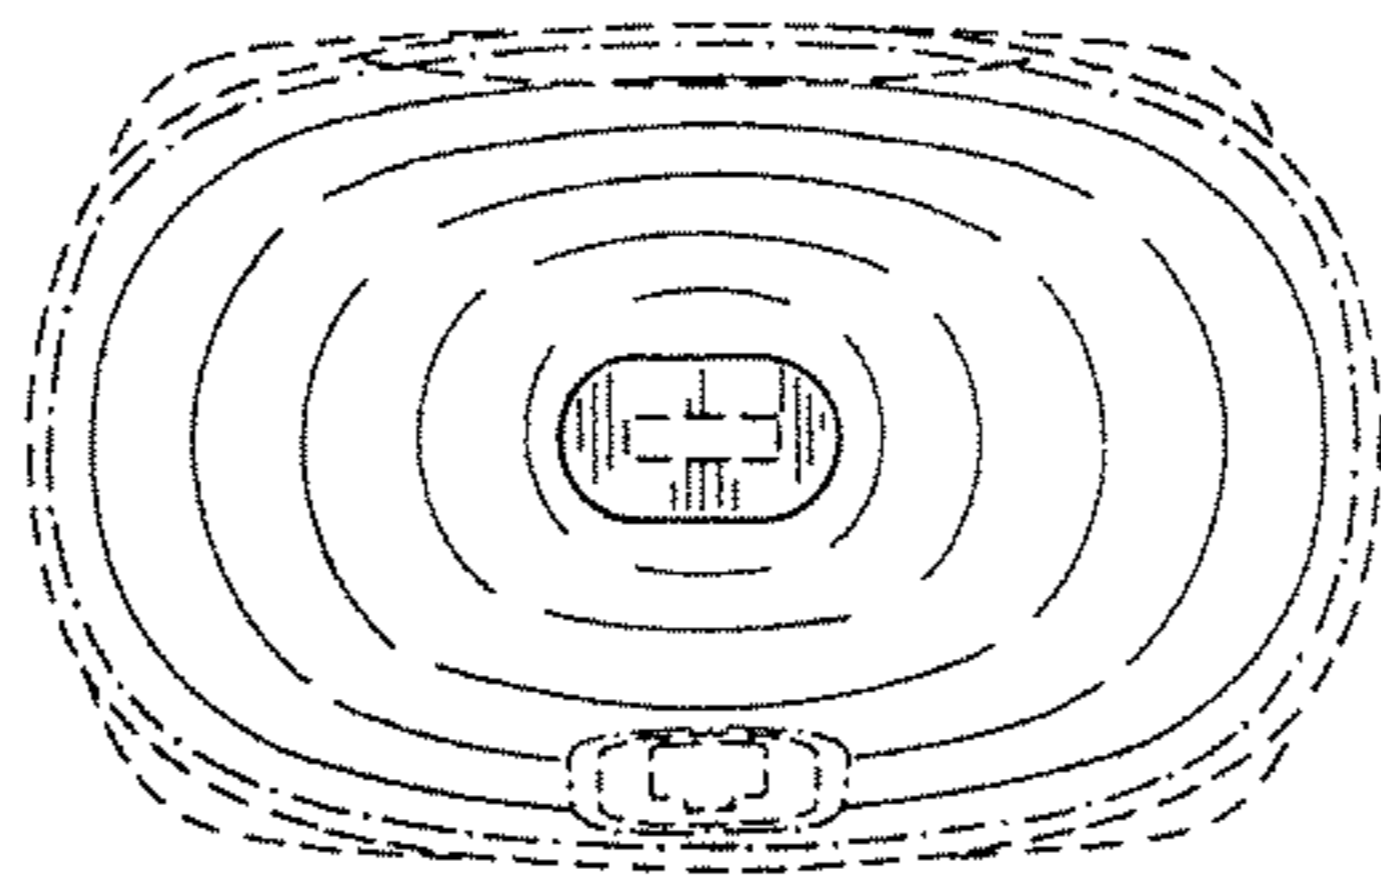

**FIG. 6**

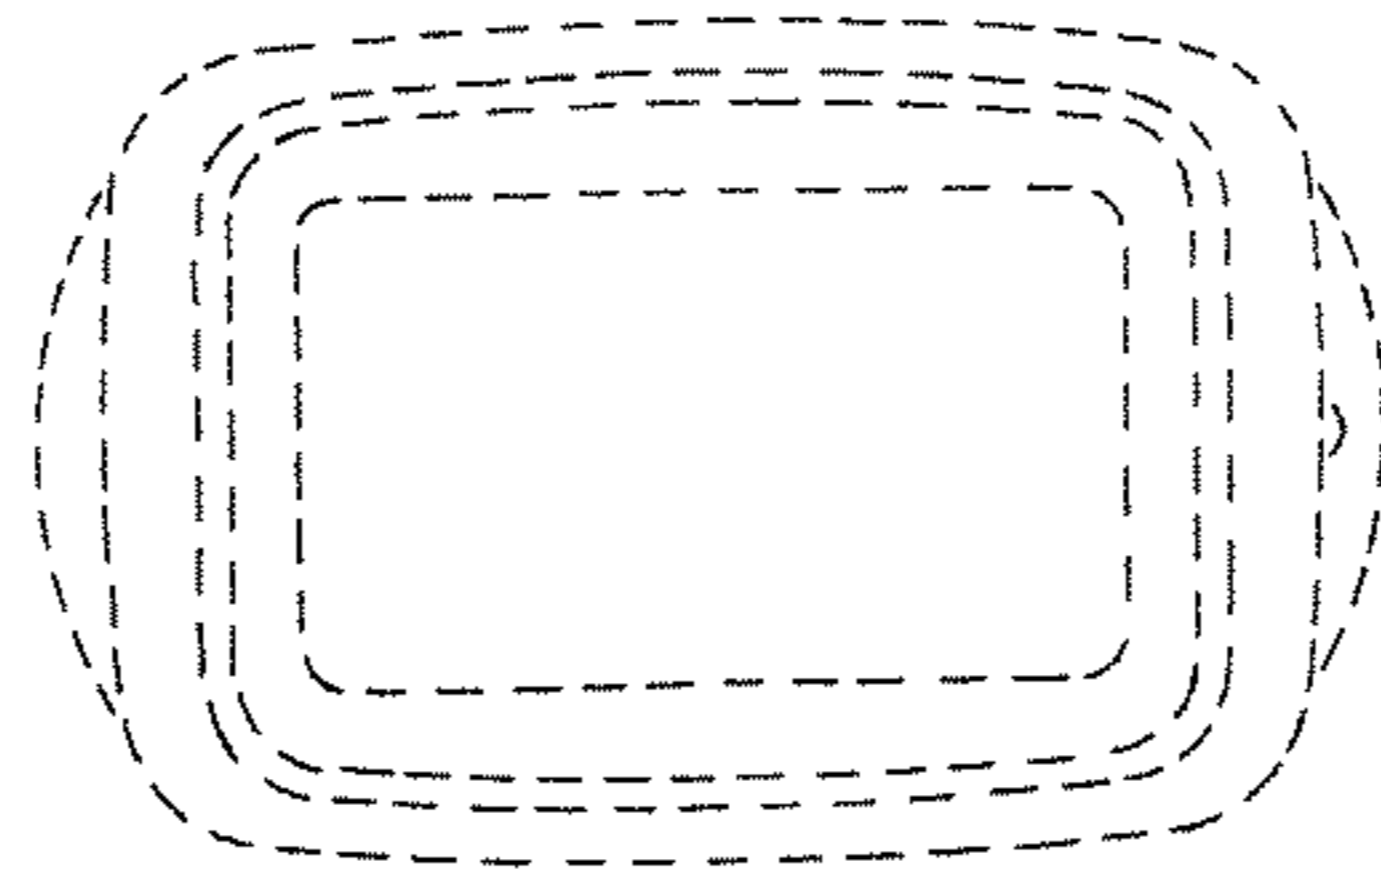

**FIG. 7**