



US00D886997S

(12) **United States Design Patent** (10) **Patent No.:** **US D886,997 S**  
**Kalina, Jr. et al.** (45) **Date of Patent:** **\*\* Jun. 9, 2020**

(54) **GONIOSCOPE**  
(71) Applicant: **GLAUKOS CORPORATION**, San Clemente, CA (US)  
(72) Inventors: **Charles Raymond Kalina, Jr.**, Irvine, CA (US); **Huong Khac Huynh**, Mission Viejo, CA (US)  
(73) Assignee: **GLAUKOS CORPORATION**, San Clemente, CA (US)

3,112,570 A 12/1963 Vasconcellos  
D205,094 S \* 6/1966 Pulos ..... D24/137  
D207,371 S \* 4/1967 Pulos ..... D24/137  
(Continued)

**FOREIGN PATENT DOCUMENTS**

WO WO 94/010900 5/1994  
WO WO 2009/158517 12/2009  
(Continued)

**OTHER PUBLICATIONS**

U.S. Clinical Wick Trials, Oct. 11, 1999, website <http://www.cornea.org/us.htm>. Allingham, R. R., et al., "Morphometric Analysis of Schlemm's Canal in Normal and Glaucomatous Human Eyes", Glaucoma Paper Presentation, (abstract only—not dated).  
(Continued)

(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/664,456**  
(22) Filed: **Sep. 25, 2018**

**Related U.S. Application Data**

(62) Division of application No. 29/595,348, filed on Feb. 27, 2017, now Pat. No. Des. 833,008.  
(51) **LOC (12) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/137; D16/135**  
(58) **Field of Classification Search**  
USPC ..... D16/130, 131, 134, 135, 136, 137;  
D24/107, 133, 137, 232; D10/65  
CPC ..... A61B 3/117; A61B 3/125; A61B 3/132;  
A61B 3/0033; A61B 3/0083; A61B  
17/0231; A61B 2090/067; A61F 9/013;  
A61F 9/0017  
See application file for complete search history.

*Primary Examiner* — Leanne Was-Englehart

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear LLP

(57) **CLAIM**

The ornamental design for a gonioscope, as shown and described.

**DESCRIPTION**


FIG. 1 is a top, front, and right side perspective view of the gonioscope.  
FIG. 2 is a front elevation view thereof.  
FIG. 3 is a rear elevation view thereof.  
FIG. 4 is a right side elevation view thereof.  
FIG. 5 is a left side elevation view thereof.  
FIG. 6 is a top plan view thereof.  
FIG. 7 is a bottom plan view thereof; and,  
FIG. 8 is a bottom, rear, and left side perspective view thereof.  
The broken lines in the drawings depict portions of the gonioscope that form no part of the claimed design.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

2,430,851 A 11/1947 Allen  
D166,597 S 4/1952 Filsinger  
D166,842 S \* 5/1952 Armbruster ..... D24/137  
D175,322 S \* 8/1955 Stegeman ..... D24/137  
D196,610 S \* 10/1963 Kolbeck ..... D24/150

**1 Claim, 7 Drawing Sheets**

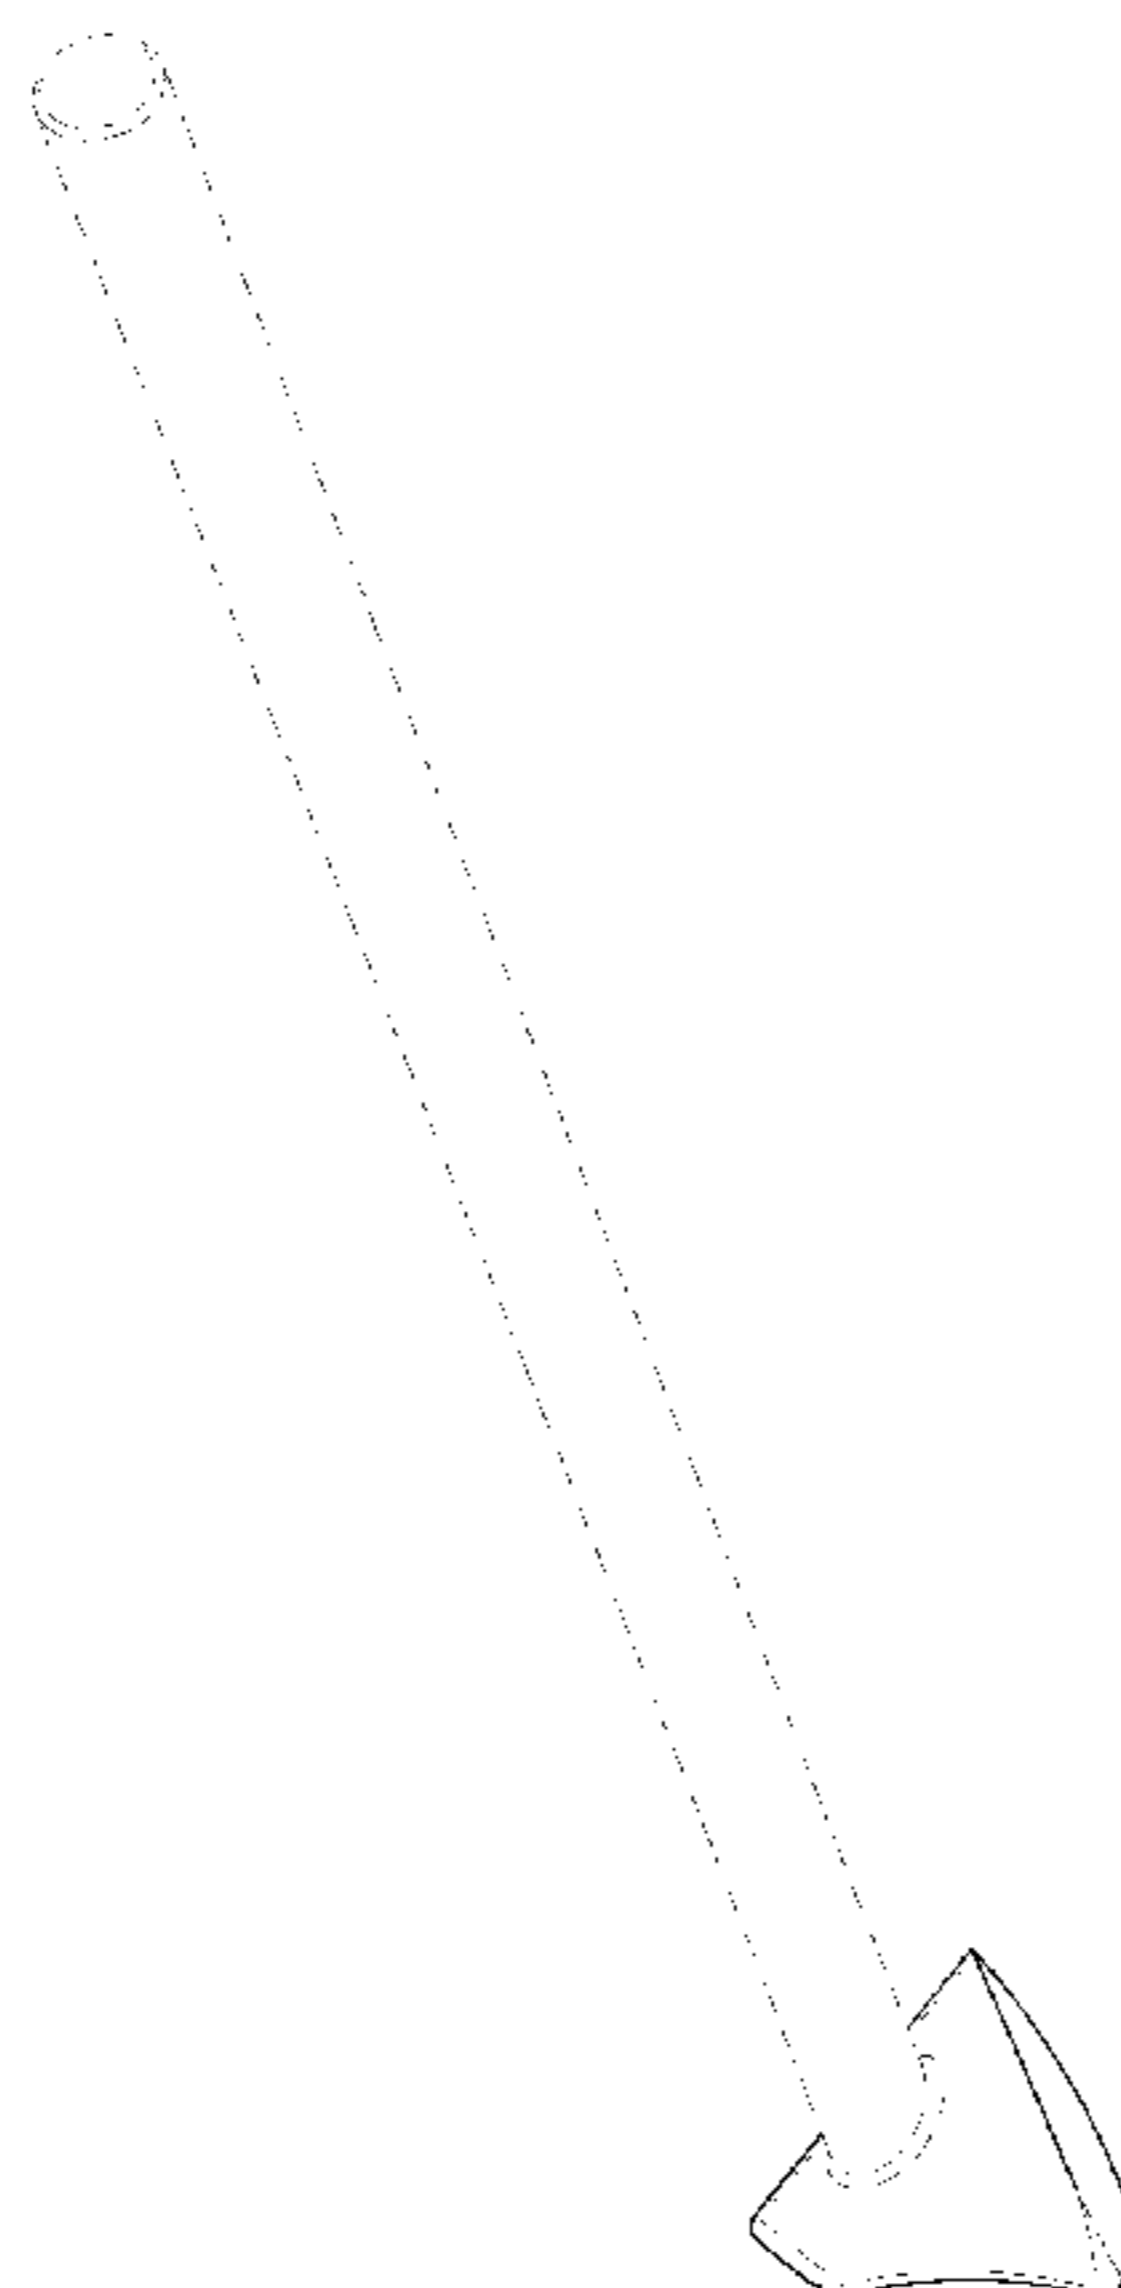



(56)

**References Cited**

U.S. PATENT DOCUMENTS

2010/0265461 A1\* 10/2010 Gille ..... A61B 3/117  
351/219  
2011/0026789 A1 2/2011 Hsu et al.  
2011/0103658 A1 5/2011 Davis et al.  
2011/0213342 A1 9/2011 Tripathi et al.  
2012/0099077 A1 4/2012 Abt  
2012/0257167 A1\* 10/2012 Gille ..... A61B 3/117  
351/219  
2013/0103145 A1 4/2013 John et al.  
2013/0182223 A1\* 7/2013 Wardle ..... A61B 3/117  
351/219  
2014/0307229 A1 10/2014 Hassan et al.  
2017/0181622 A1\* 6/2017 Graham ..... A61B 3/125  
2018/0070817 A1\* 3/2018 Kalina, Jr. .... A61B 3/117  
2018/0310821 A1\* 11/2018 Kalina, Jr. .... A61B 17/0231

FOREIGN PATENT DOCUMENTS


WO WO 10/077987 7/2010  
WO WO 2013/109771 7/2013

OTHER PUBLICATIONS


Bahler, Cindy K., BS, Gregroy T. Smedley, PhD, Jianbo Zhou, PhD, Douglas H. Johnson, MD., Trabecular Bypass Stents Decrease Intraocular Pressure in Cultured Human Anterior Segments, American Journal of Ophthalmology, Dec. 2004, vol. 138, pp. 988-994. "Beam Steering by Wedge Prisms," last updated Jun. 15, 2006, available at: <http://micro.magnet.fsu.edu/primer/java/prismsandbeamsplitters/wedgeprisms/index.html>.  
Beck, Allen D., et al., "360° Trabeculotomy for Primary Glaucoma," Arch. Ophthalmol, 113 (Sep. 1995), pp. 1200-1202.

Buskirk, E. Michael et al., "Lens Depression and Aqueous Outflow in Enuclated Primate Eyes", American Journal of Ophthalmology, vol. 76, No. 5, Nov. 1973, pp. 632-640.  
Guttman, Cheryl, Continuous IOP Monitoring Possible with Microsensor: Implantable Device Aims to Overcome Deficiencies of Current Monitoring Techniques. (Improvement in Patient Management) (Intraocular Pressure), Ophthalmology Times, Oct. 15, 2003, as cited in HighBeam Research, <http://www.highbeam.com/DocPrint.aspx?DocId=1G1:109595800>.  
<http://glaucomatoday.com/2016/10/gonioscopy-is-essential-for-migs/> Posted Oct. 2016.  
<https://entokey.com/gonioscopy-2/> Uploaded Oct. 2016.  
<https://web.archive.org/web/20170106073123/http://ocularinc.com/> Available Jan. 6, 2017.  
Haag-Streit Contact Glasses Brochure, retrieved Mar. 20, 2007.  
Newell, Frank W., Ophthalmology Principles and Concepts, 1996, Anne S. patterson/Mosby, Eighth edition, pp. 10-21 and 32.  
Nickells, Robert W., Apoptosis of Retinal Ganglion Cells in Glaucoma: An Update of the Molecular Pathways Involved in Cell Death, Survey of Ophthalmology, vol. 43, Supplement 1, Jun. 1999, pp. S-151 through S-161.  
Ocular Hill Surgical Gonioprism from at least as early as Jun. 29, 2007 in 3 pages, downloaded from <http://www.ocularinc.com>.  
Ocular Khaw Surgical Gonioprism from at least as early as Jun. 29, 2007 in 3 pages, downloaded from <http://ocularinc.com>.  
Ocular Swan Autoclavable Gonioprism from at least as early as Jun. 29, 2007 in 3 pages, downloaded from <http://ocularinc.com>.  
VanDenburgh, A.M., et al.; A Novel Ocular Hypotensive Lipid: Initial Safety and Efficacy of AGN 192024; Glaucoma Clinical Pharmacology II, Abstract B58, IVOS 1998 vol. 39, (cover page and p. S258).  
Volk, "Aspheric Ophthalmic Lenses", Refraction, International Ophthalmology Clinics, vol. 5, No. 2, Jun. 1965.


\* cited by examiner

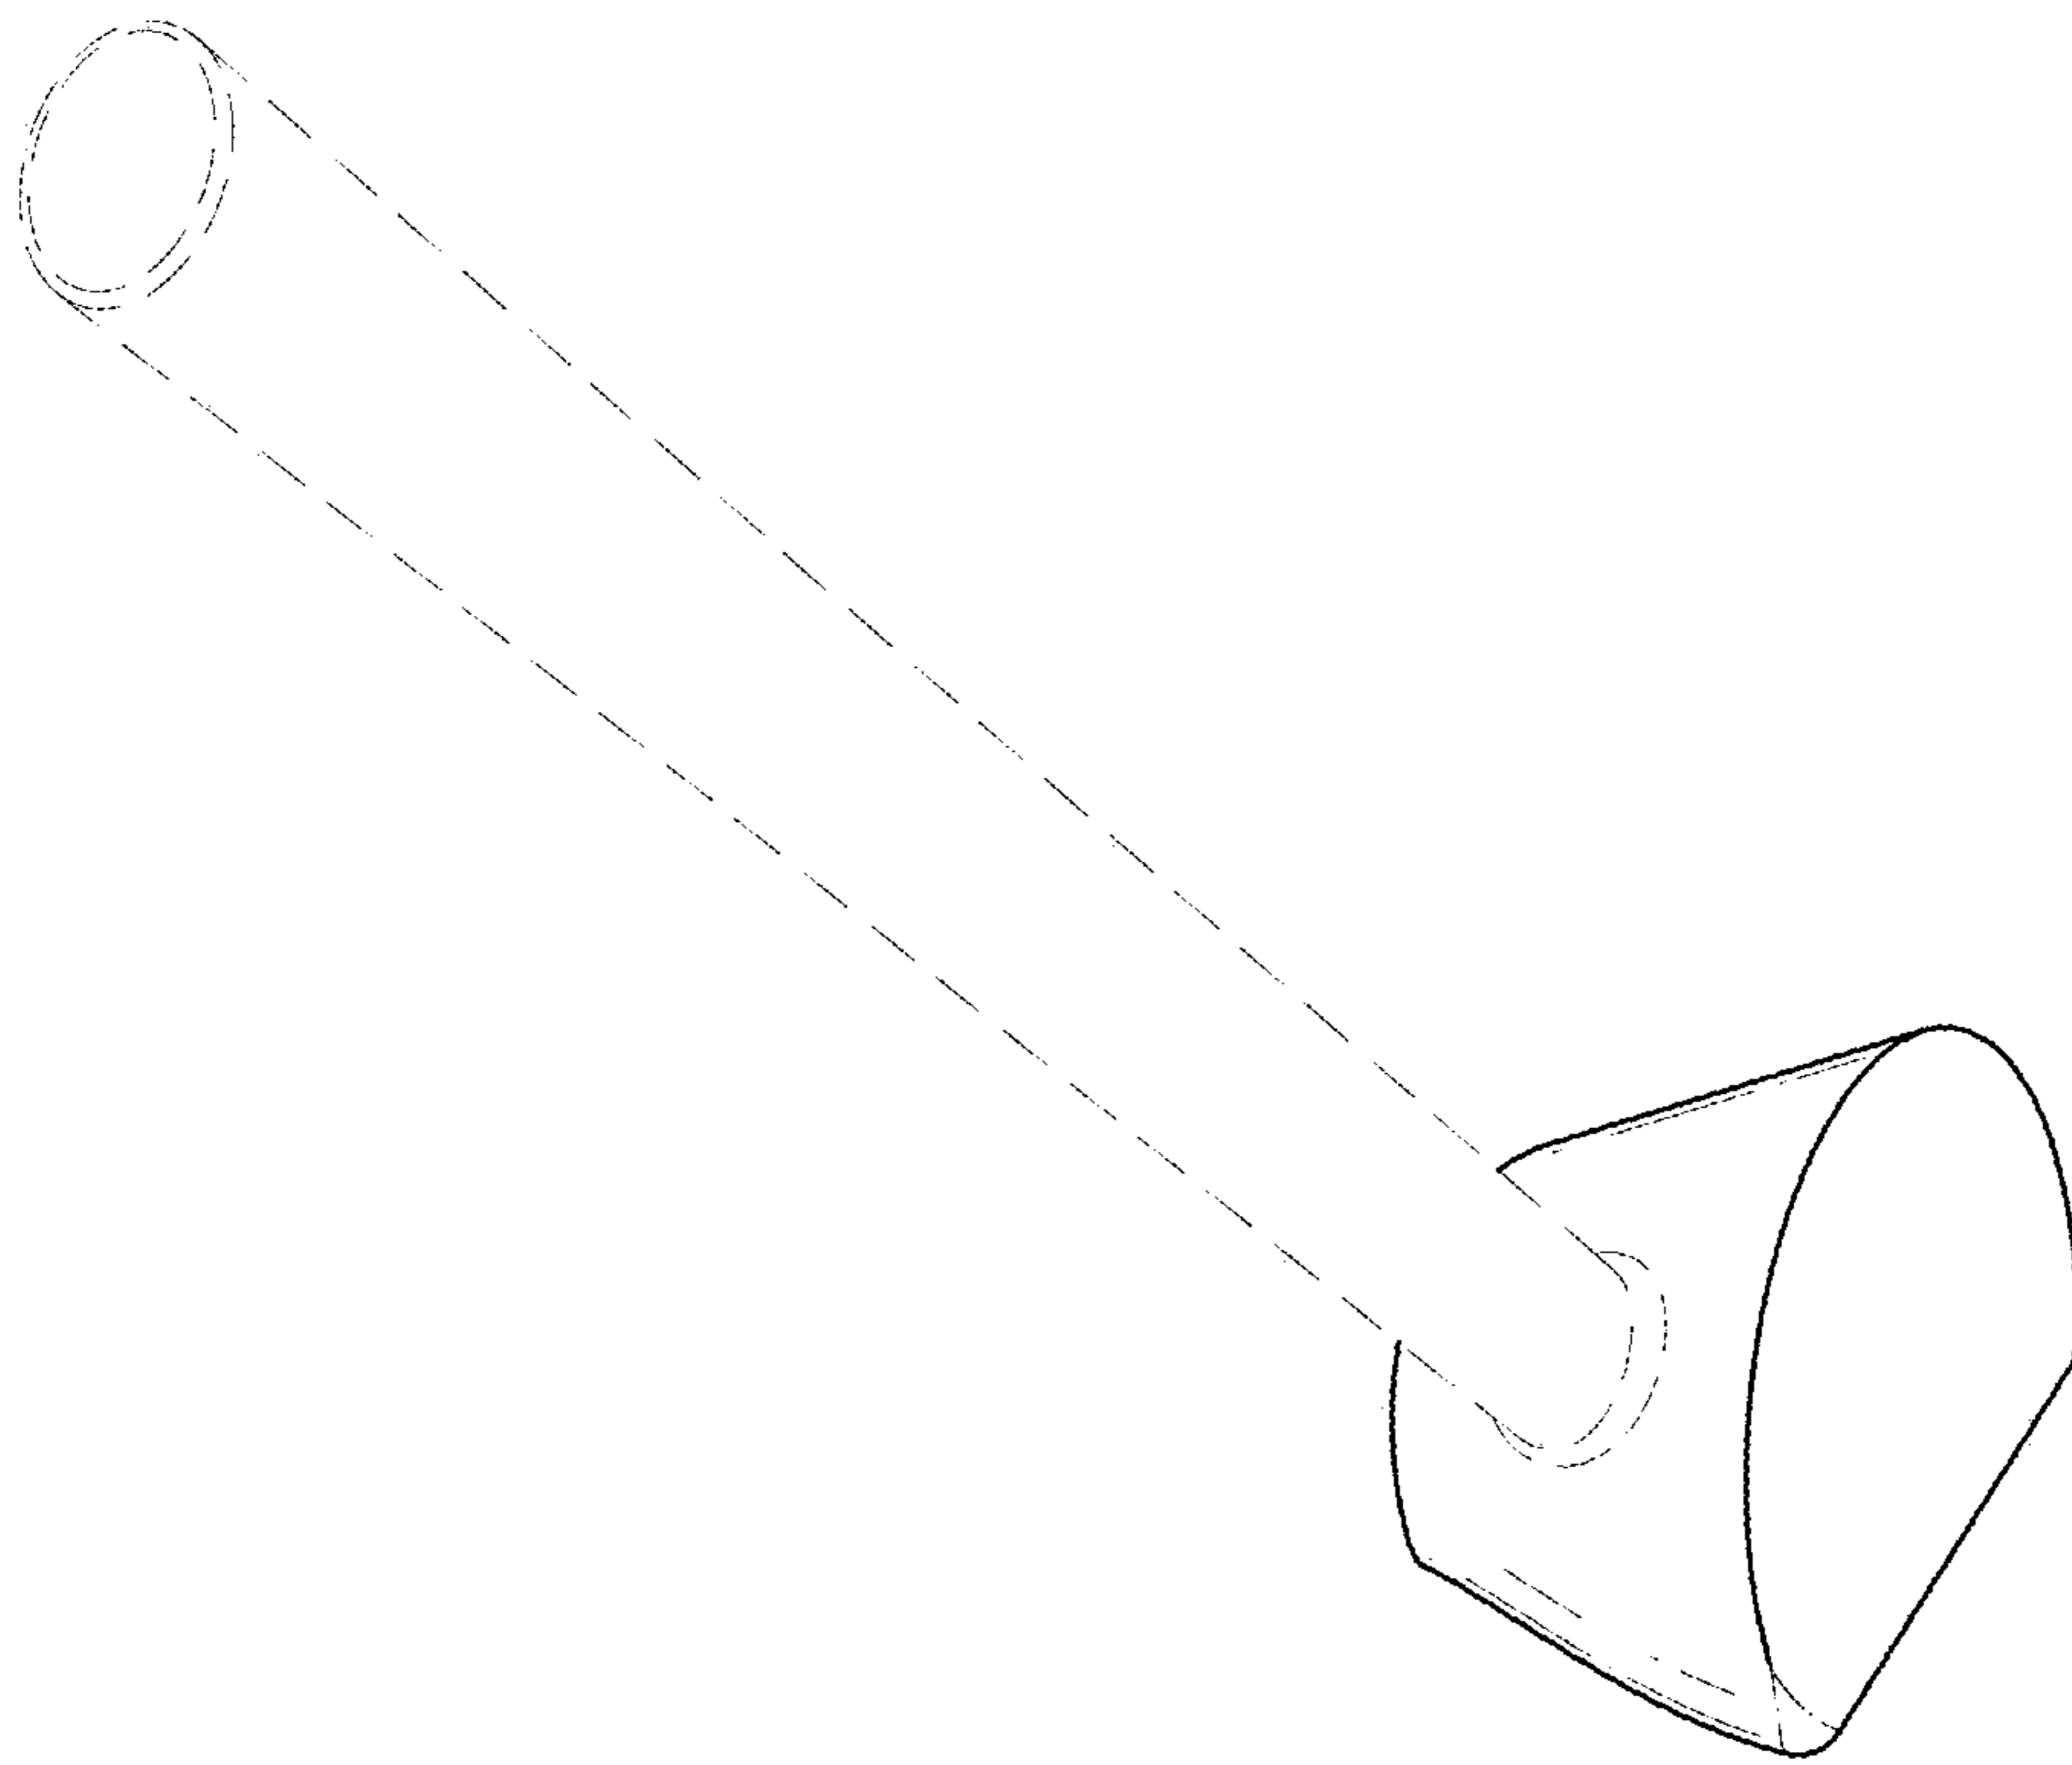


*FIG. 1*

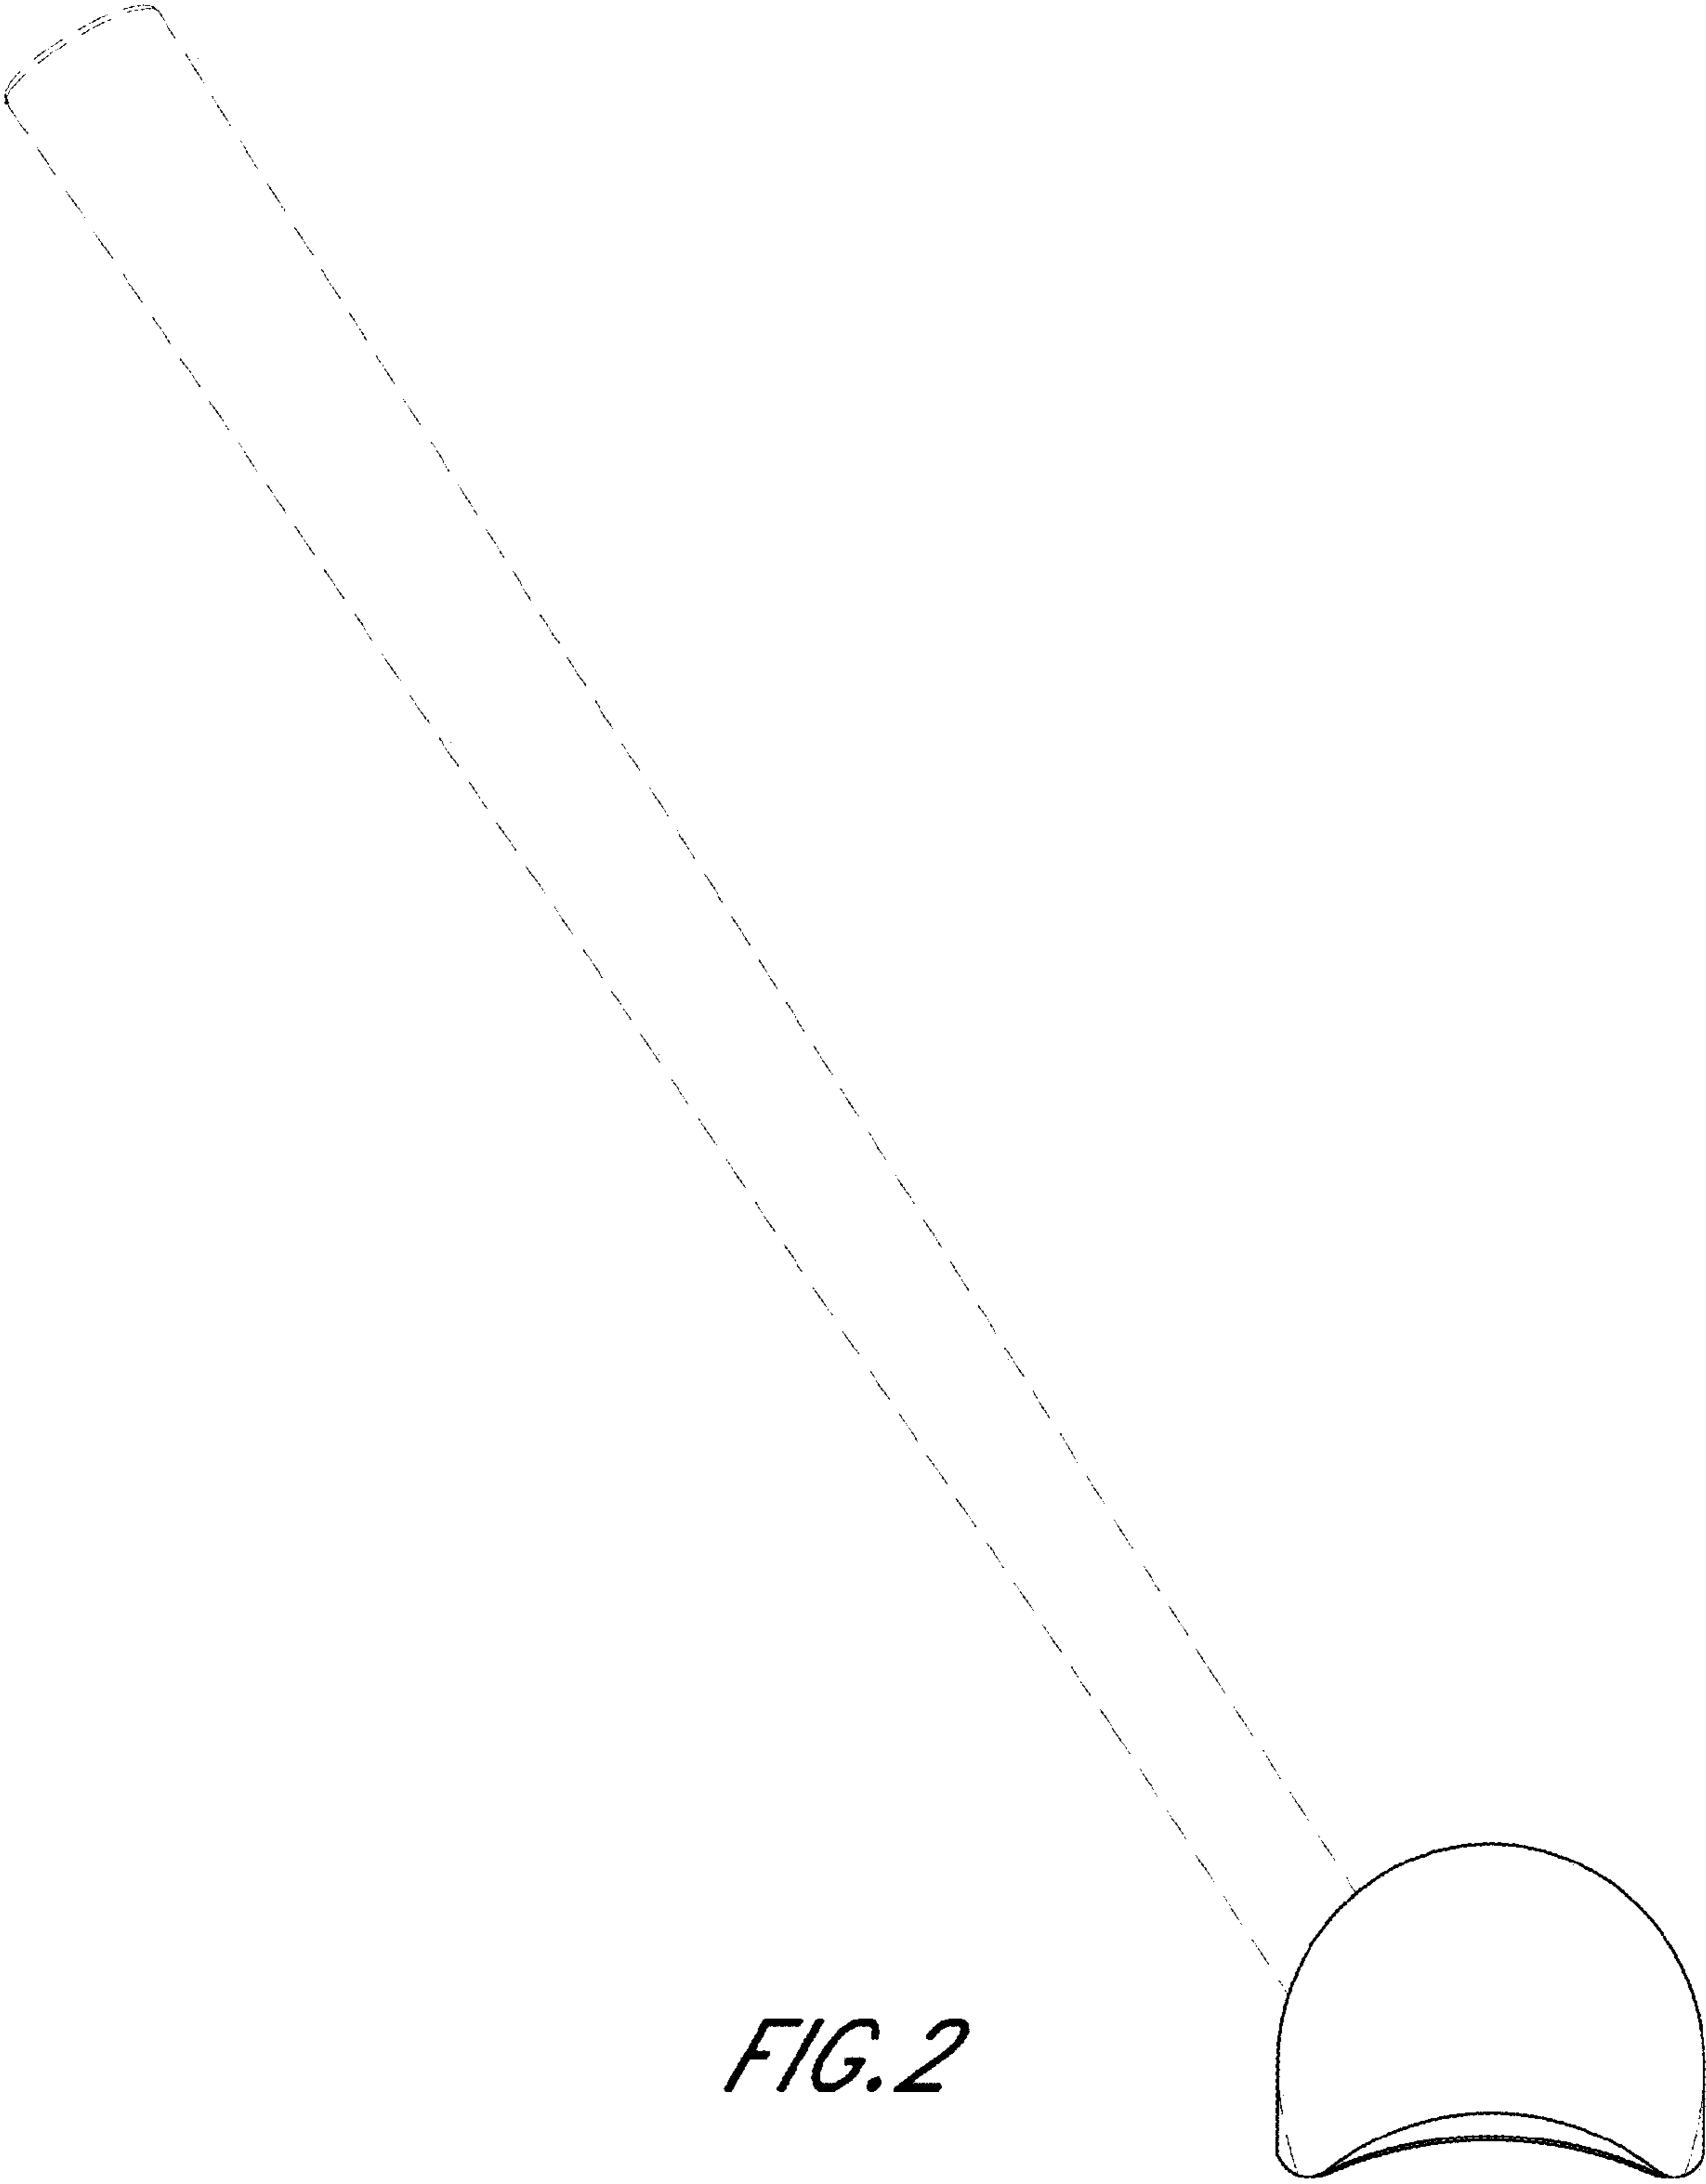


*FIG. 2*

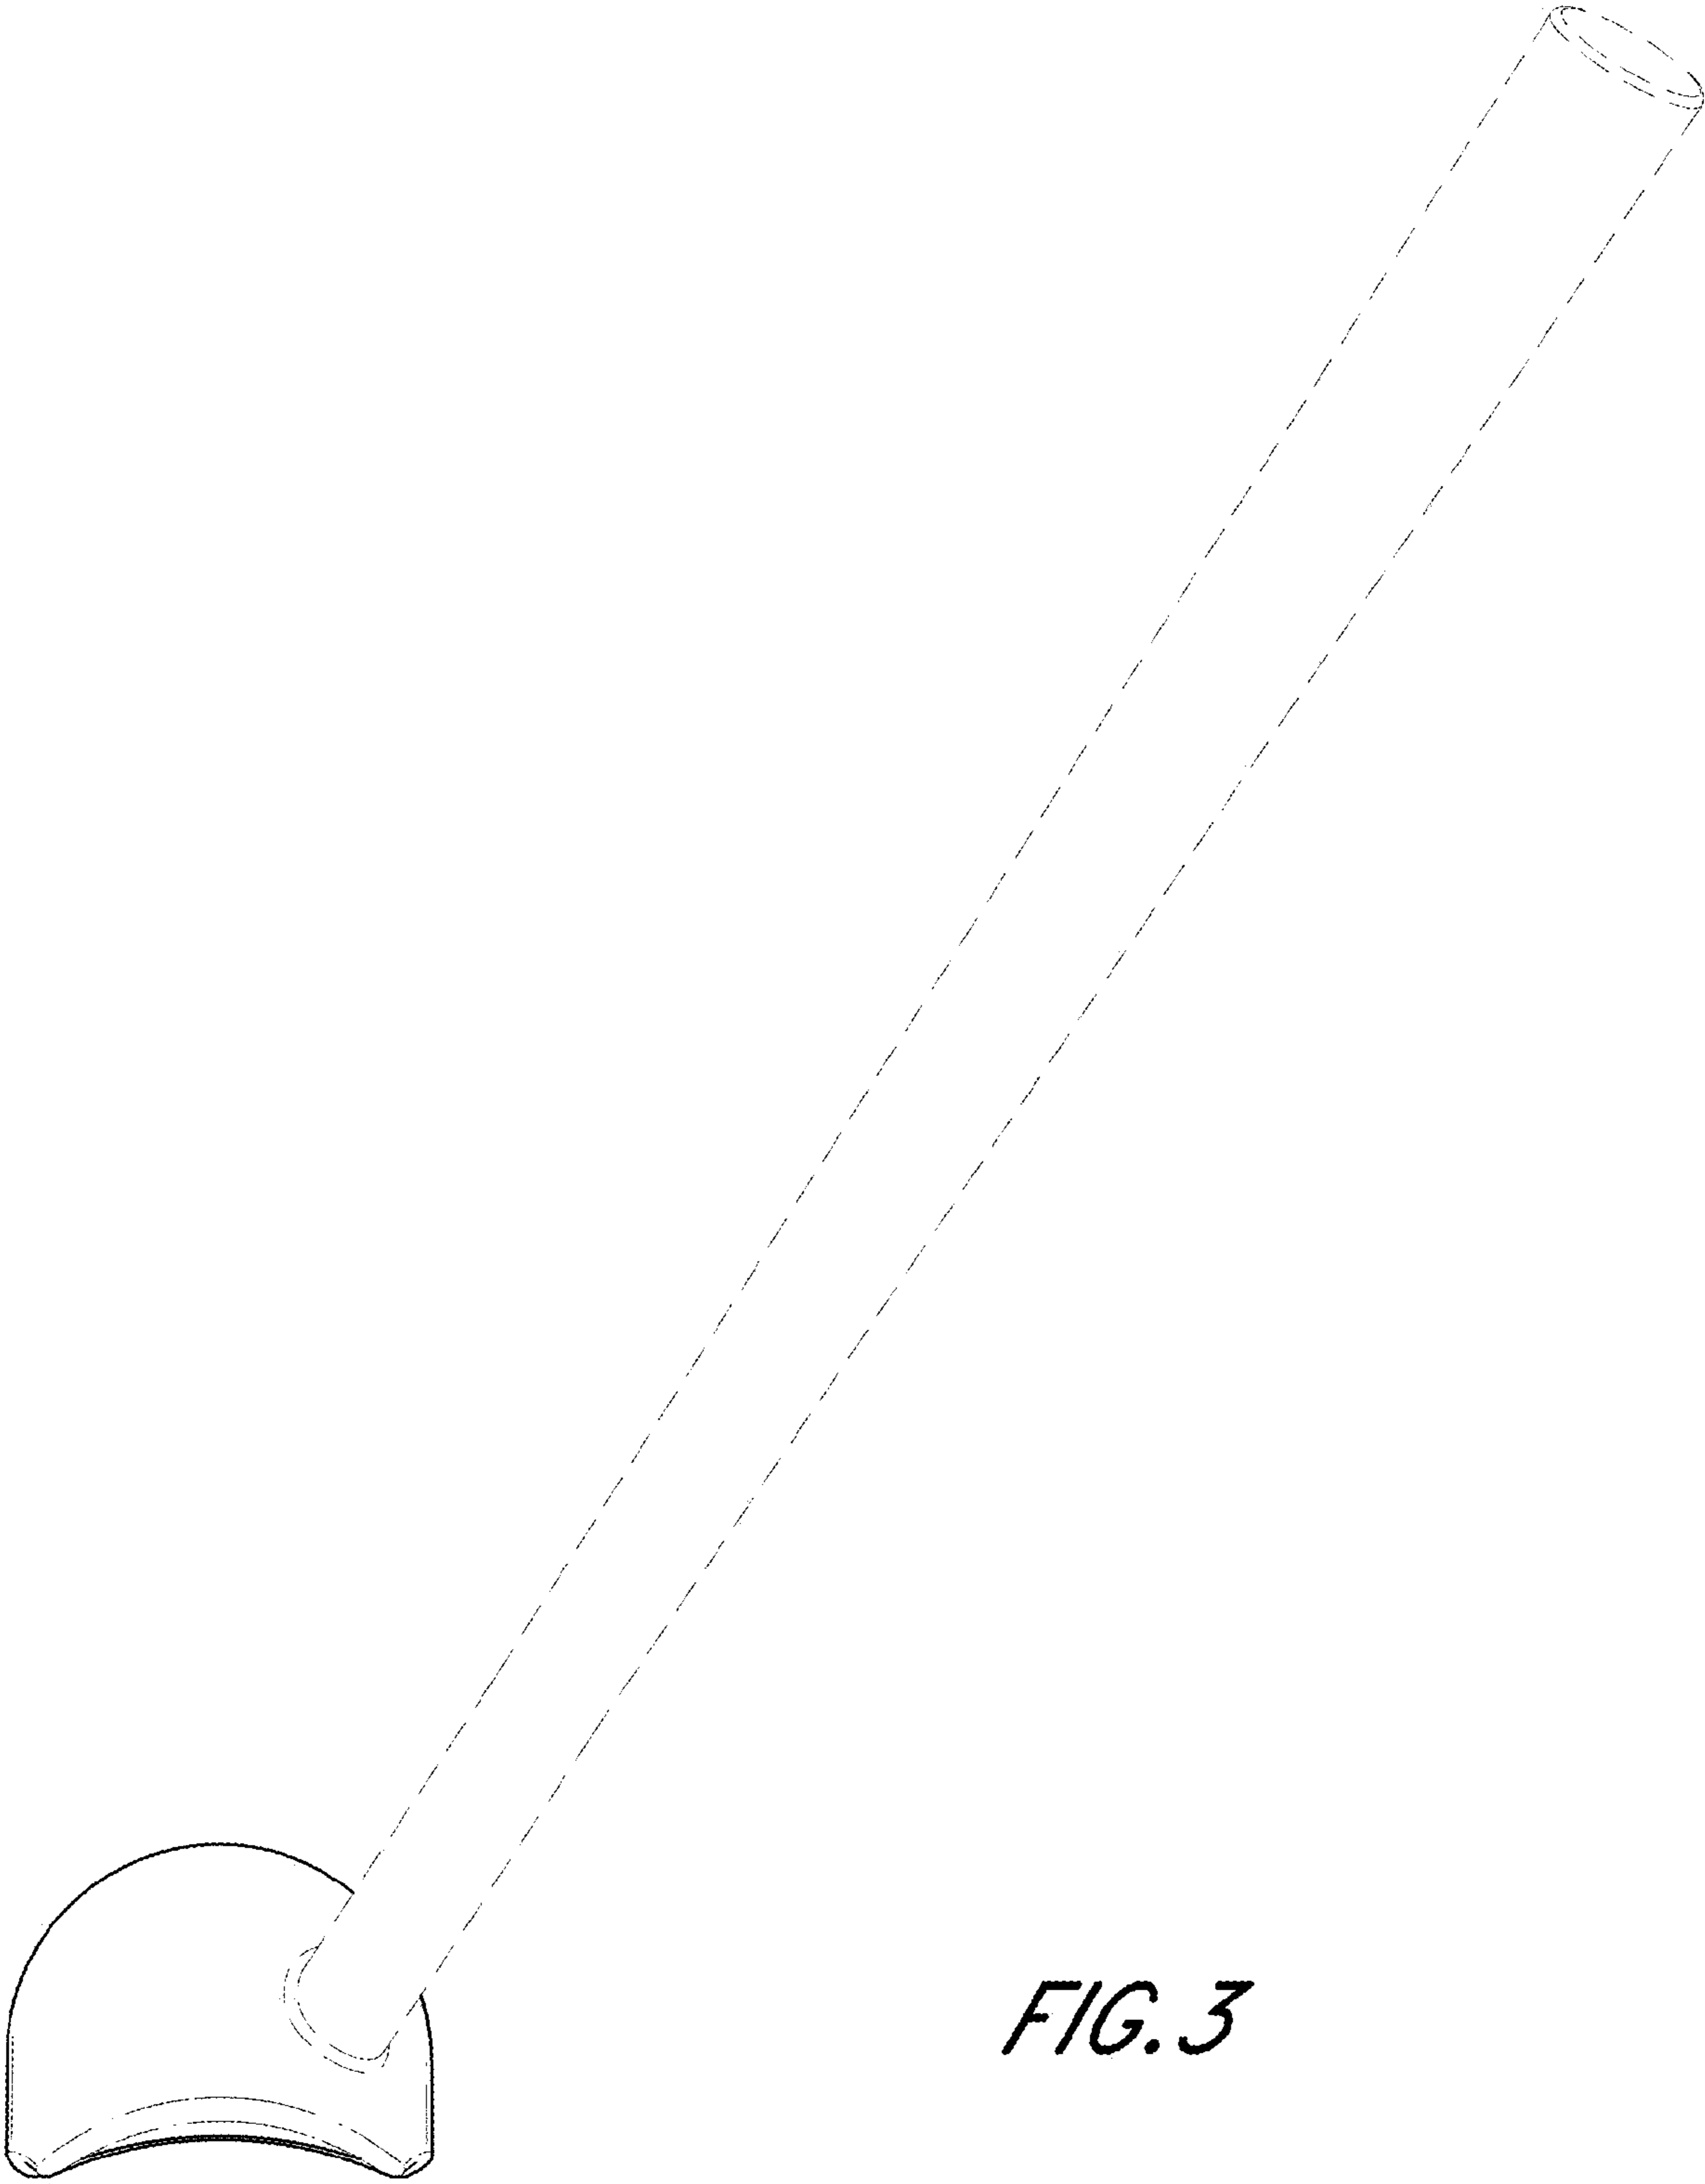

*FIG. 3*

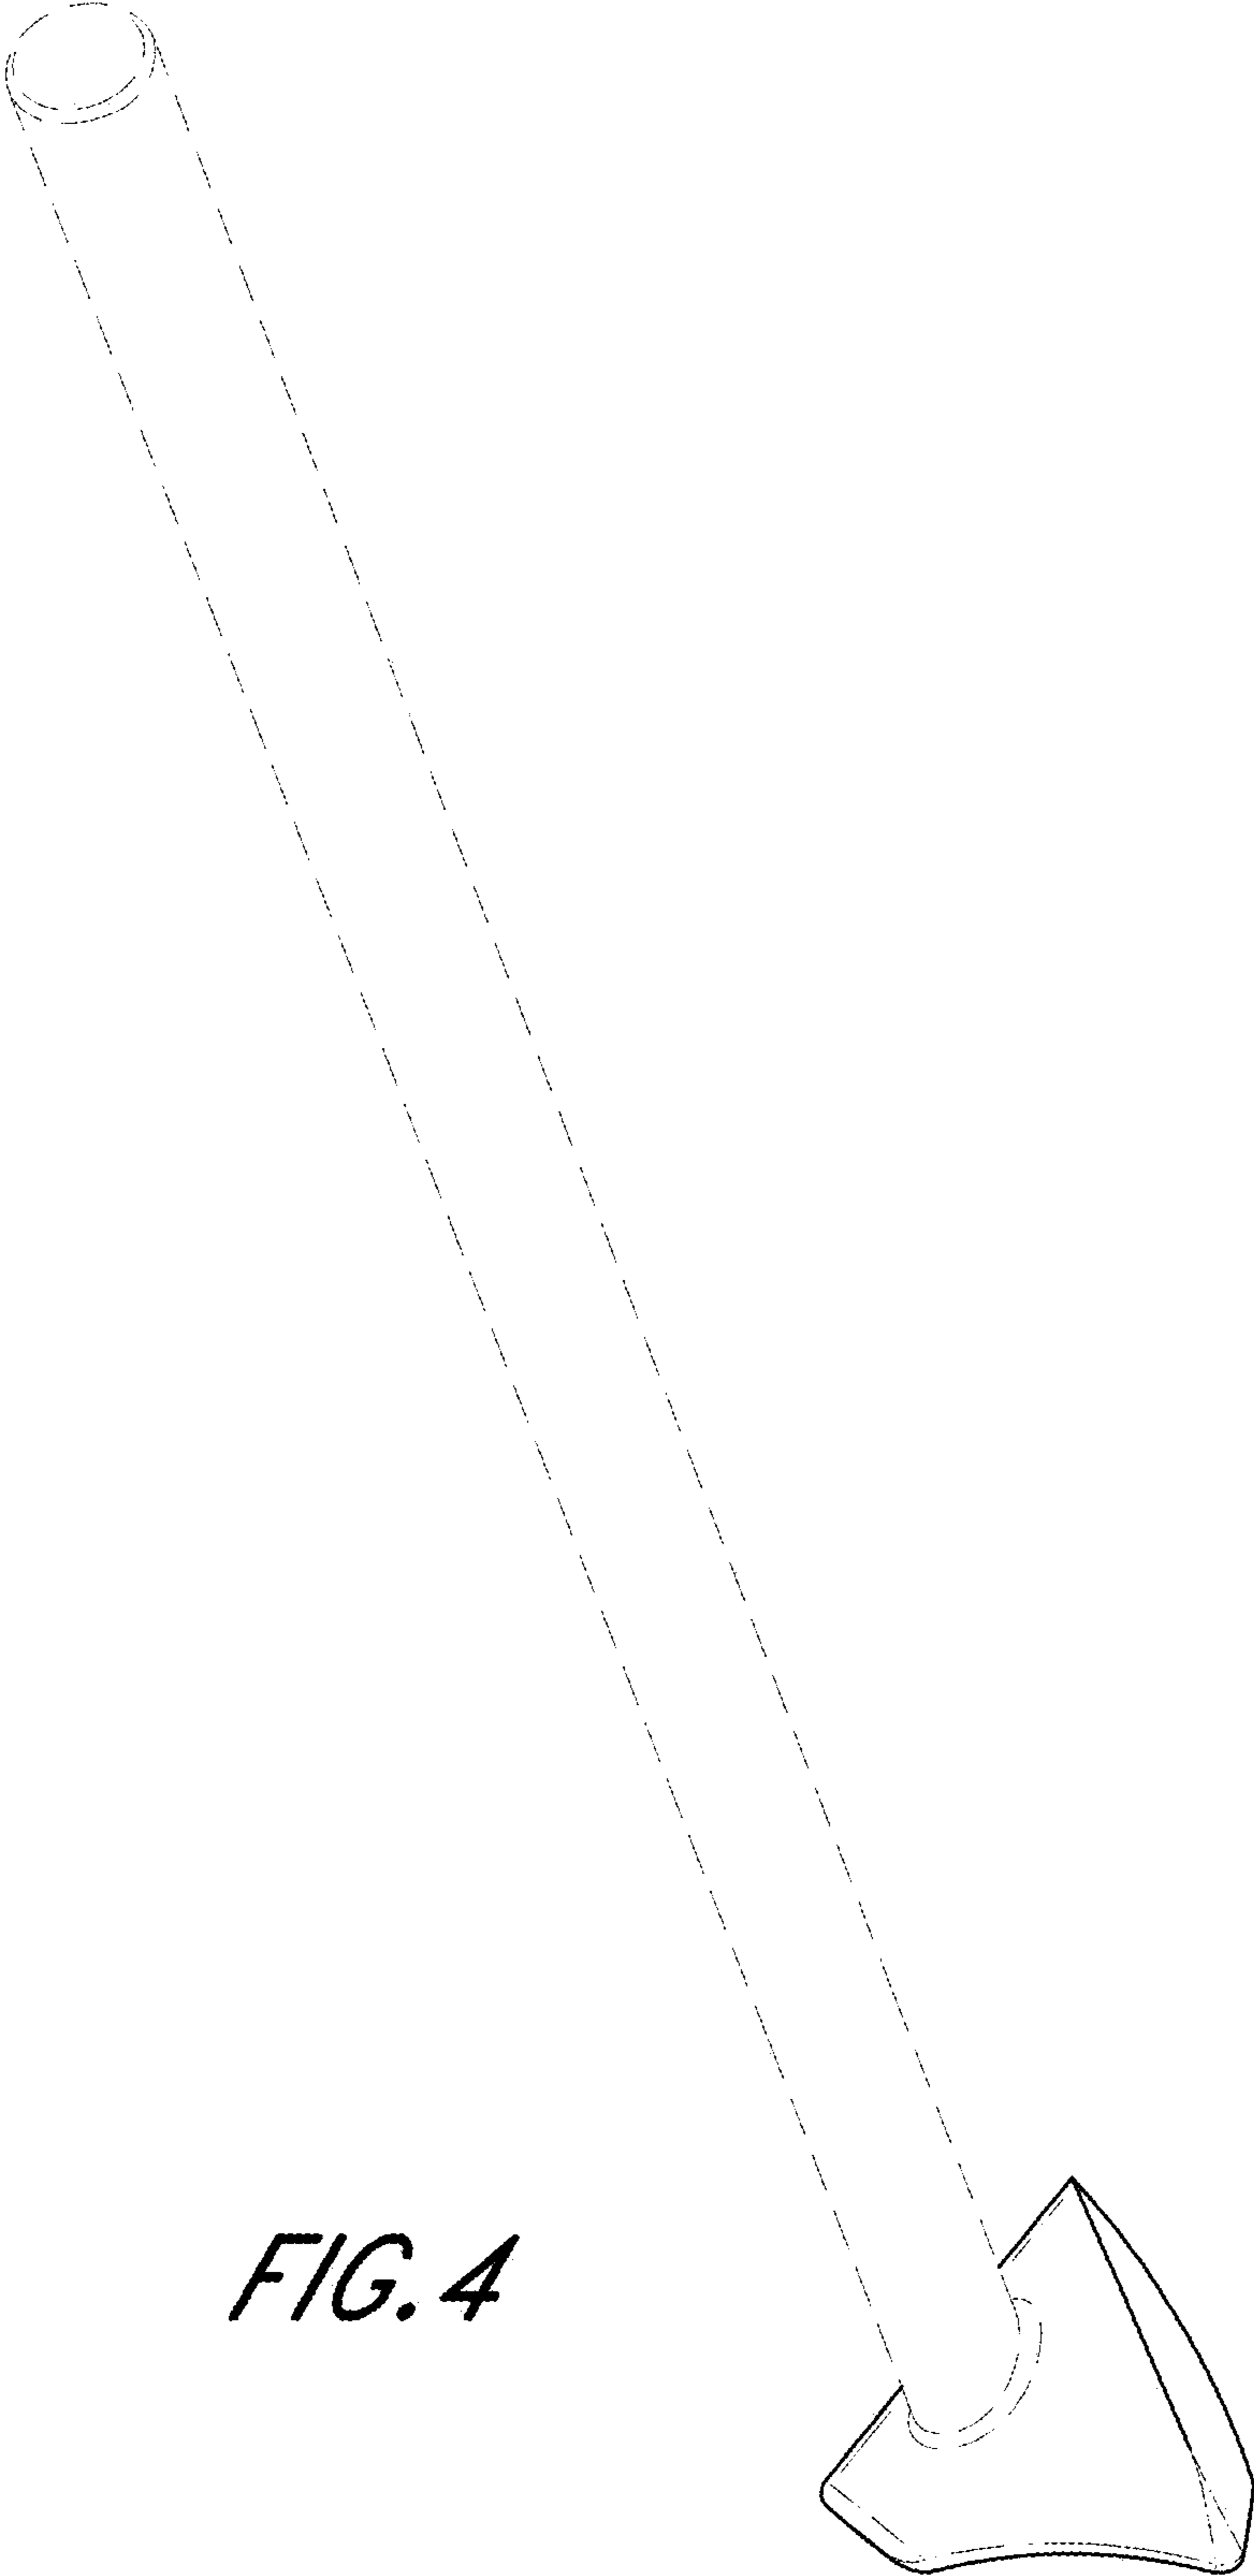


*FIG. 4*

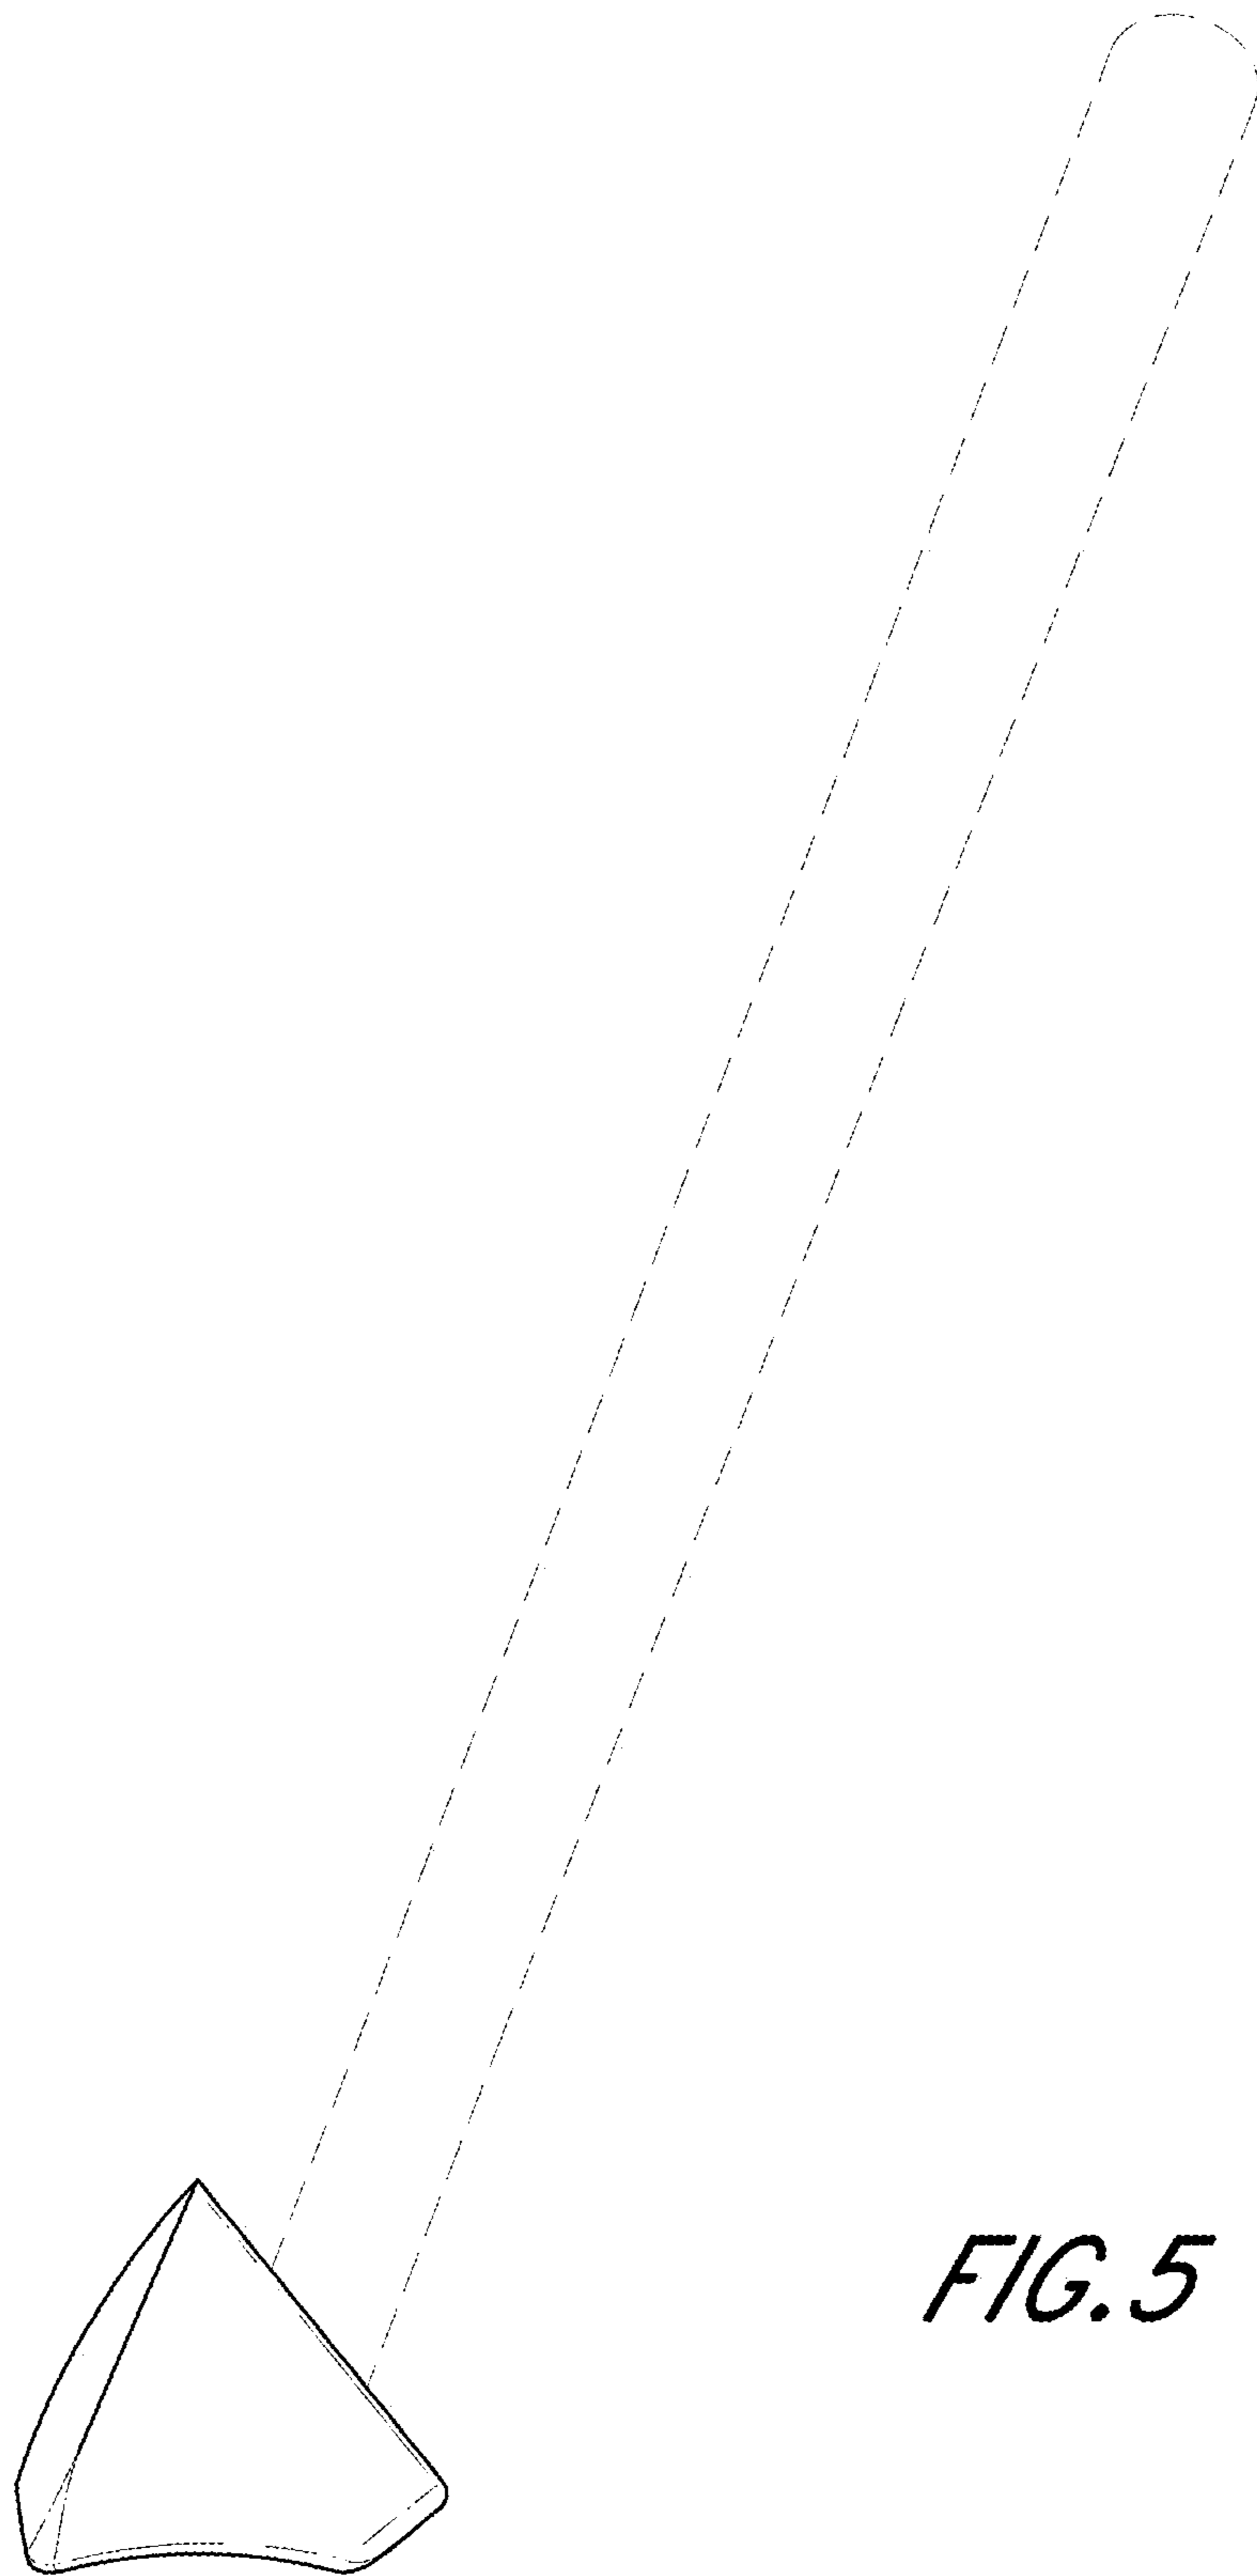


*FIG. 5*




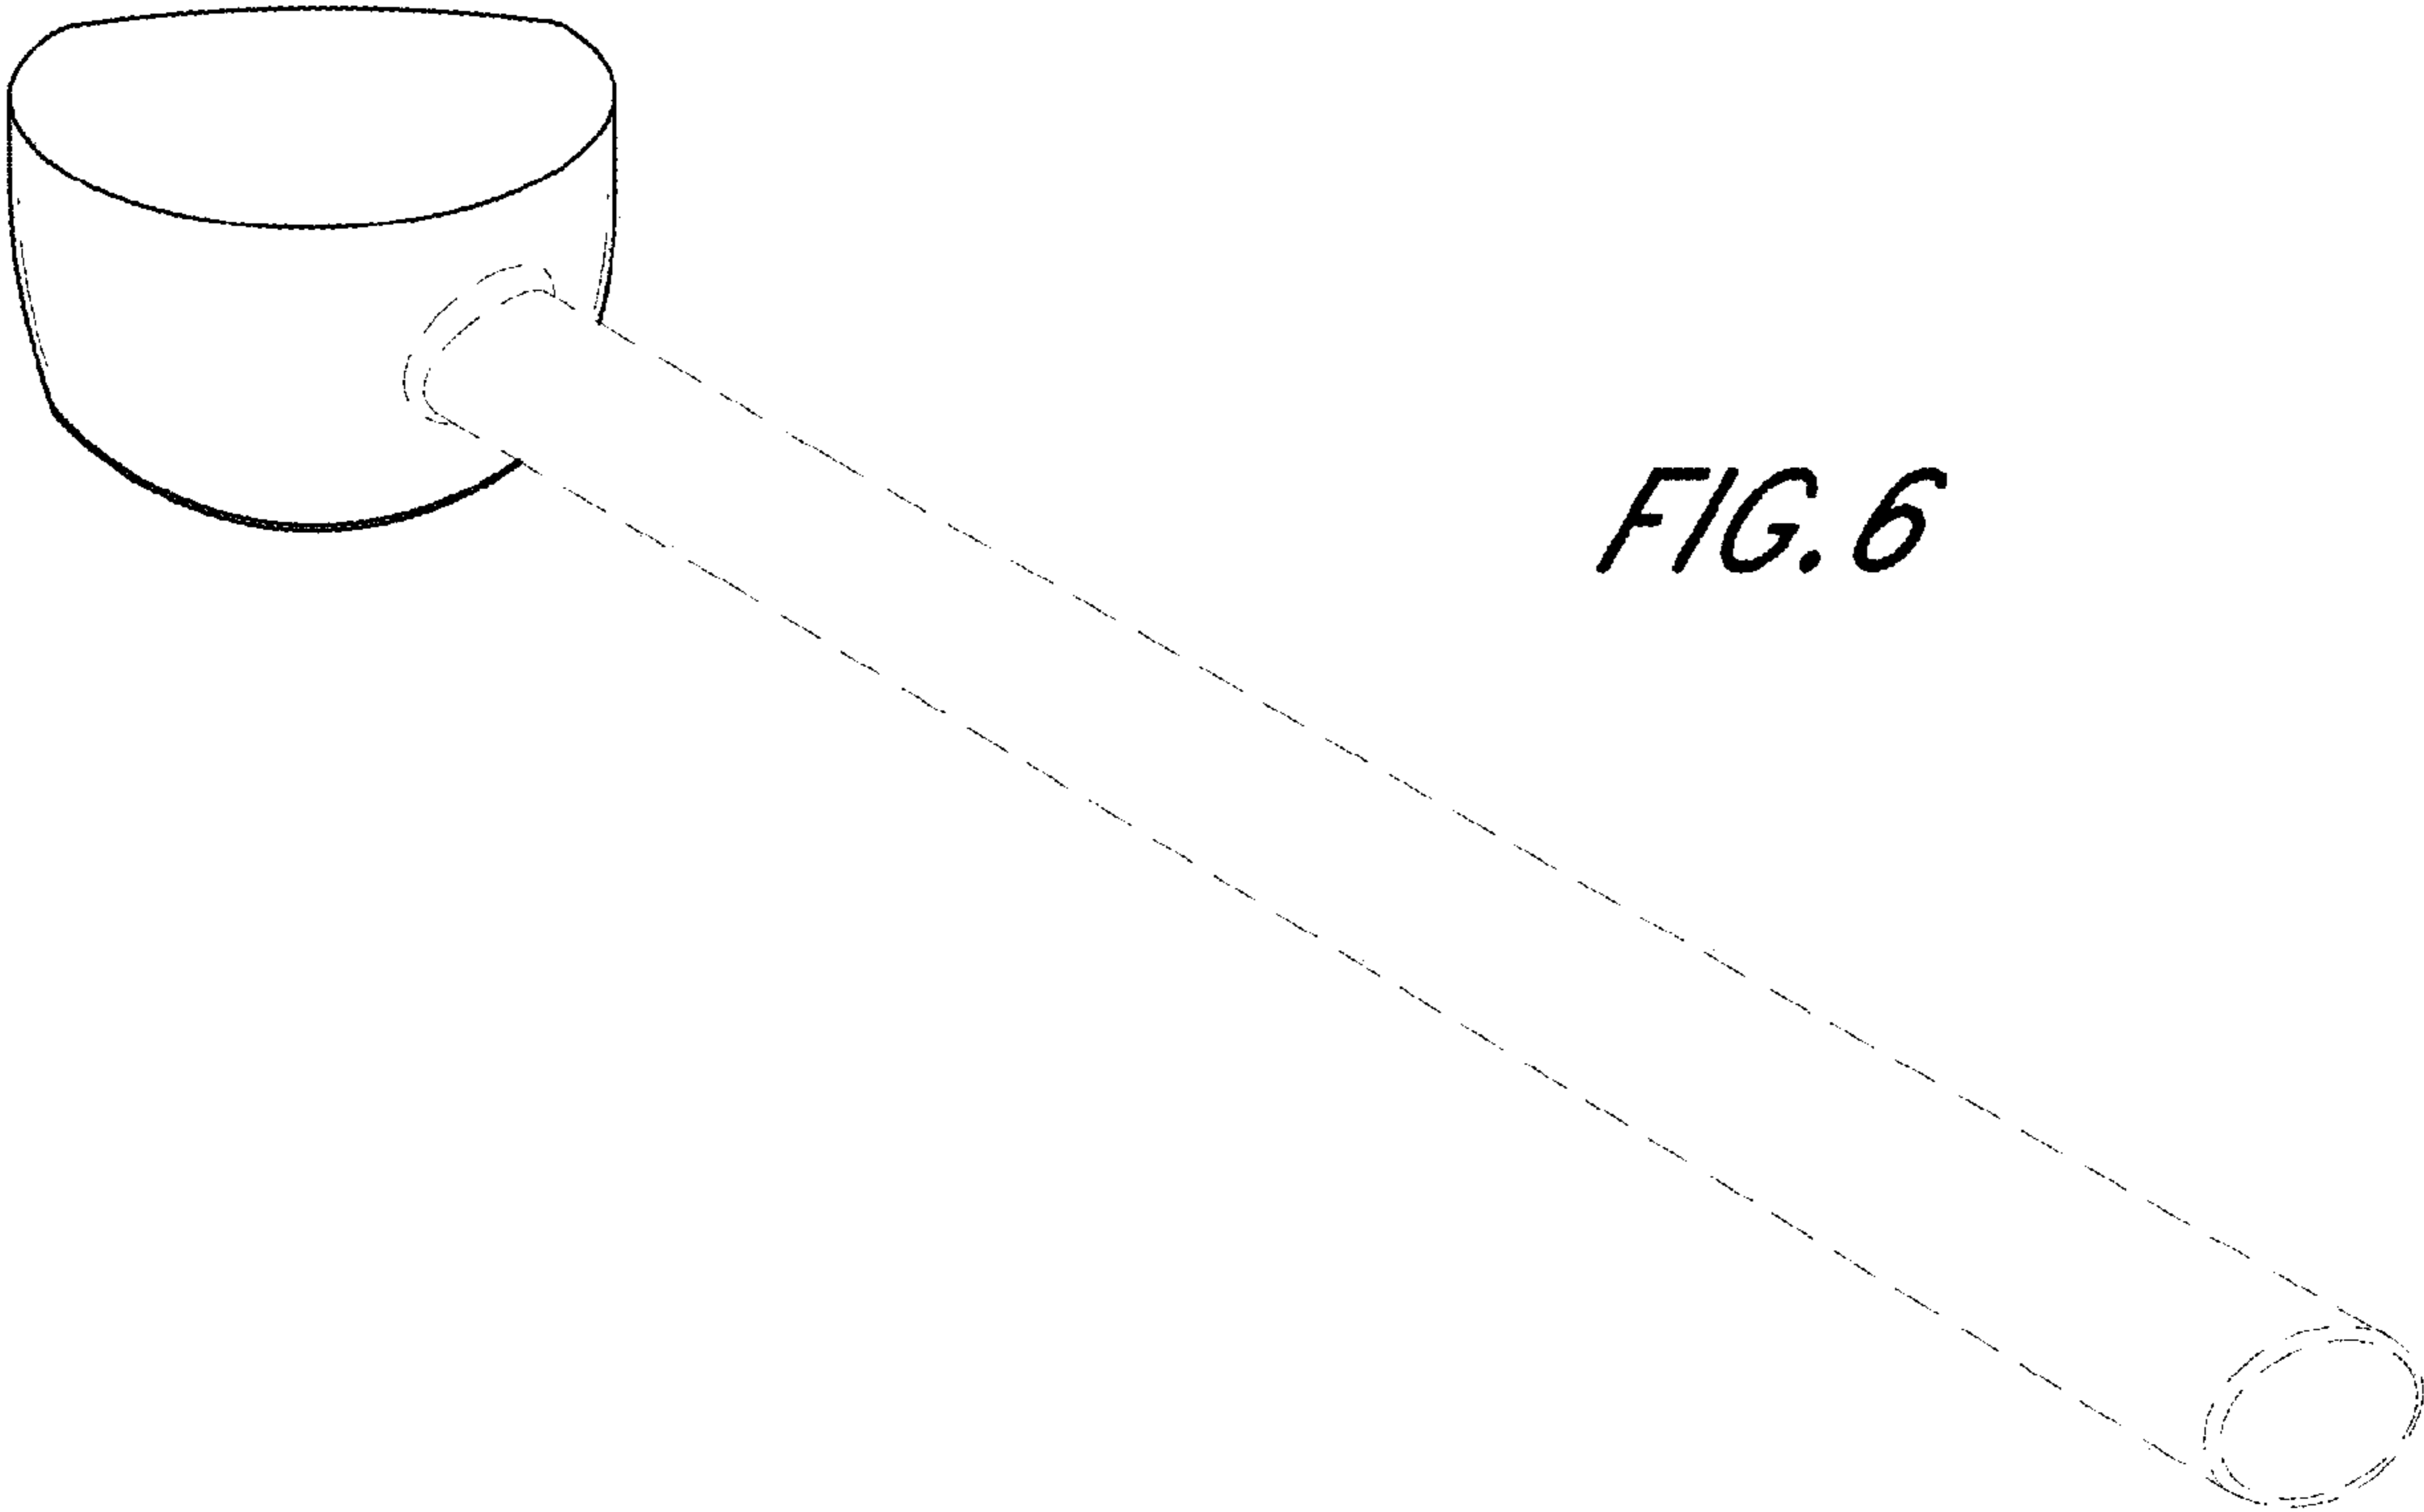

*FIG. 6*

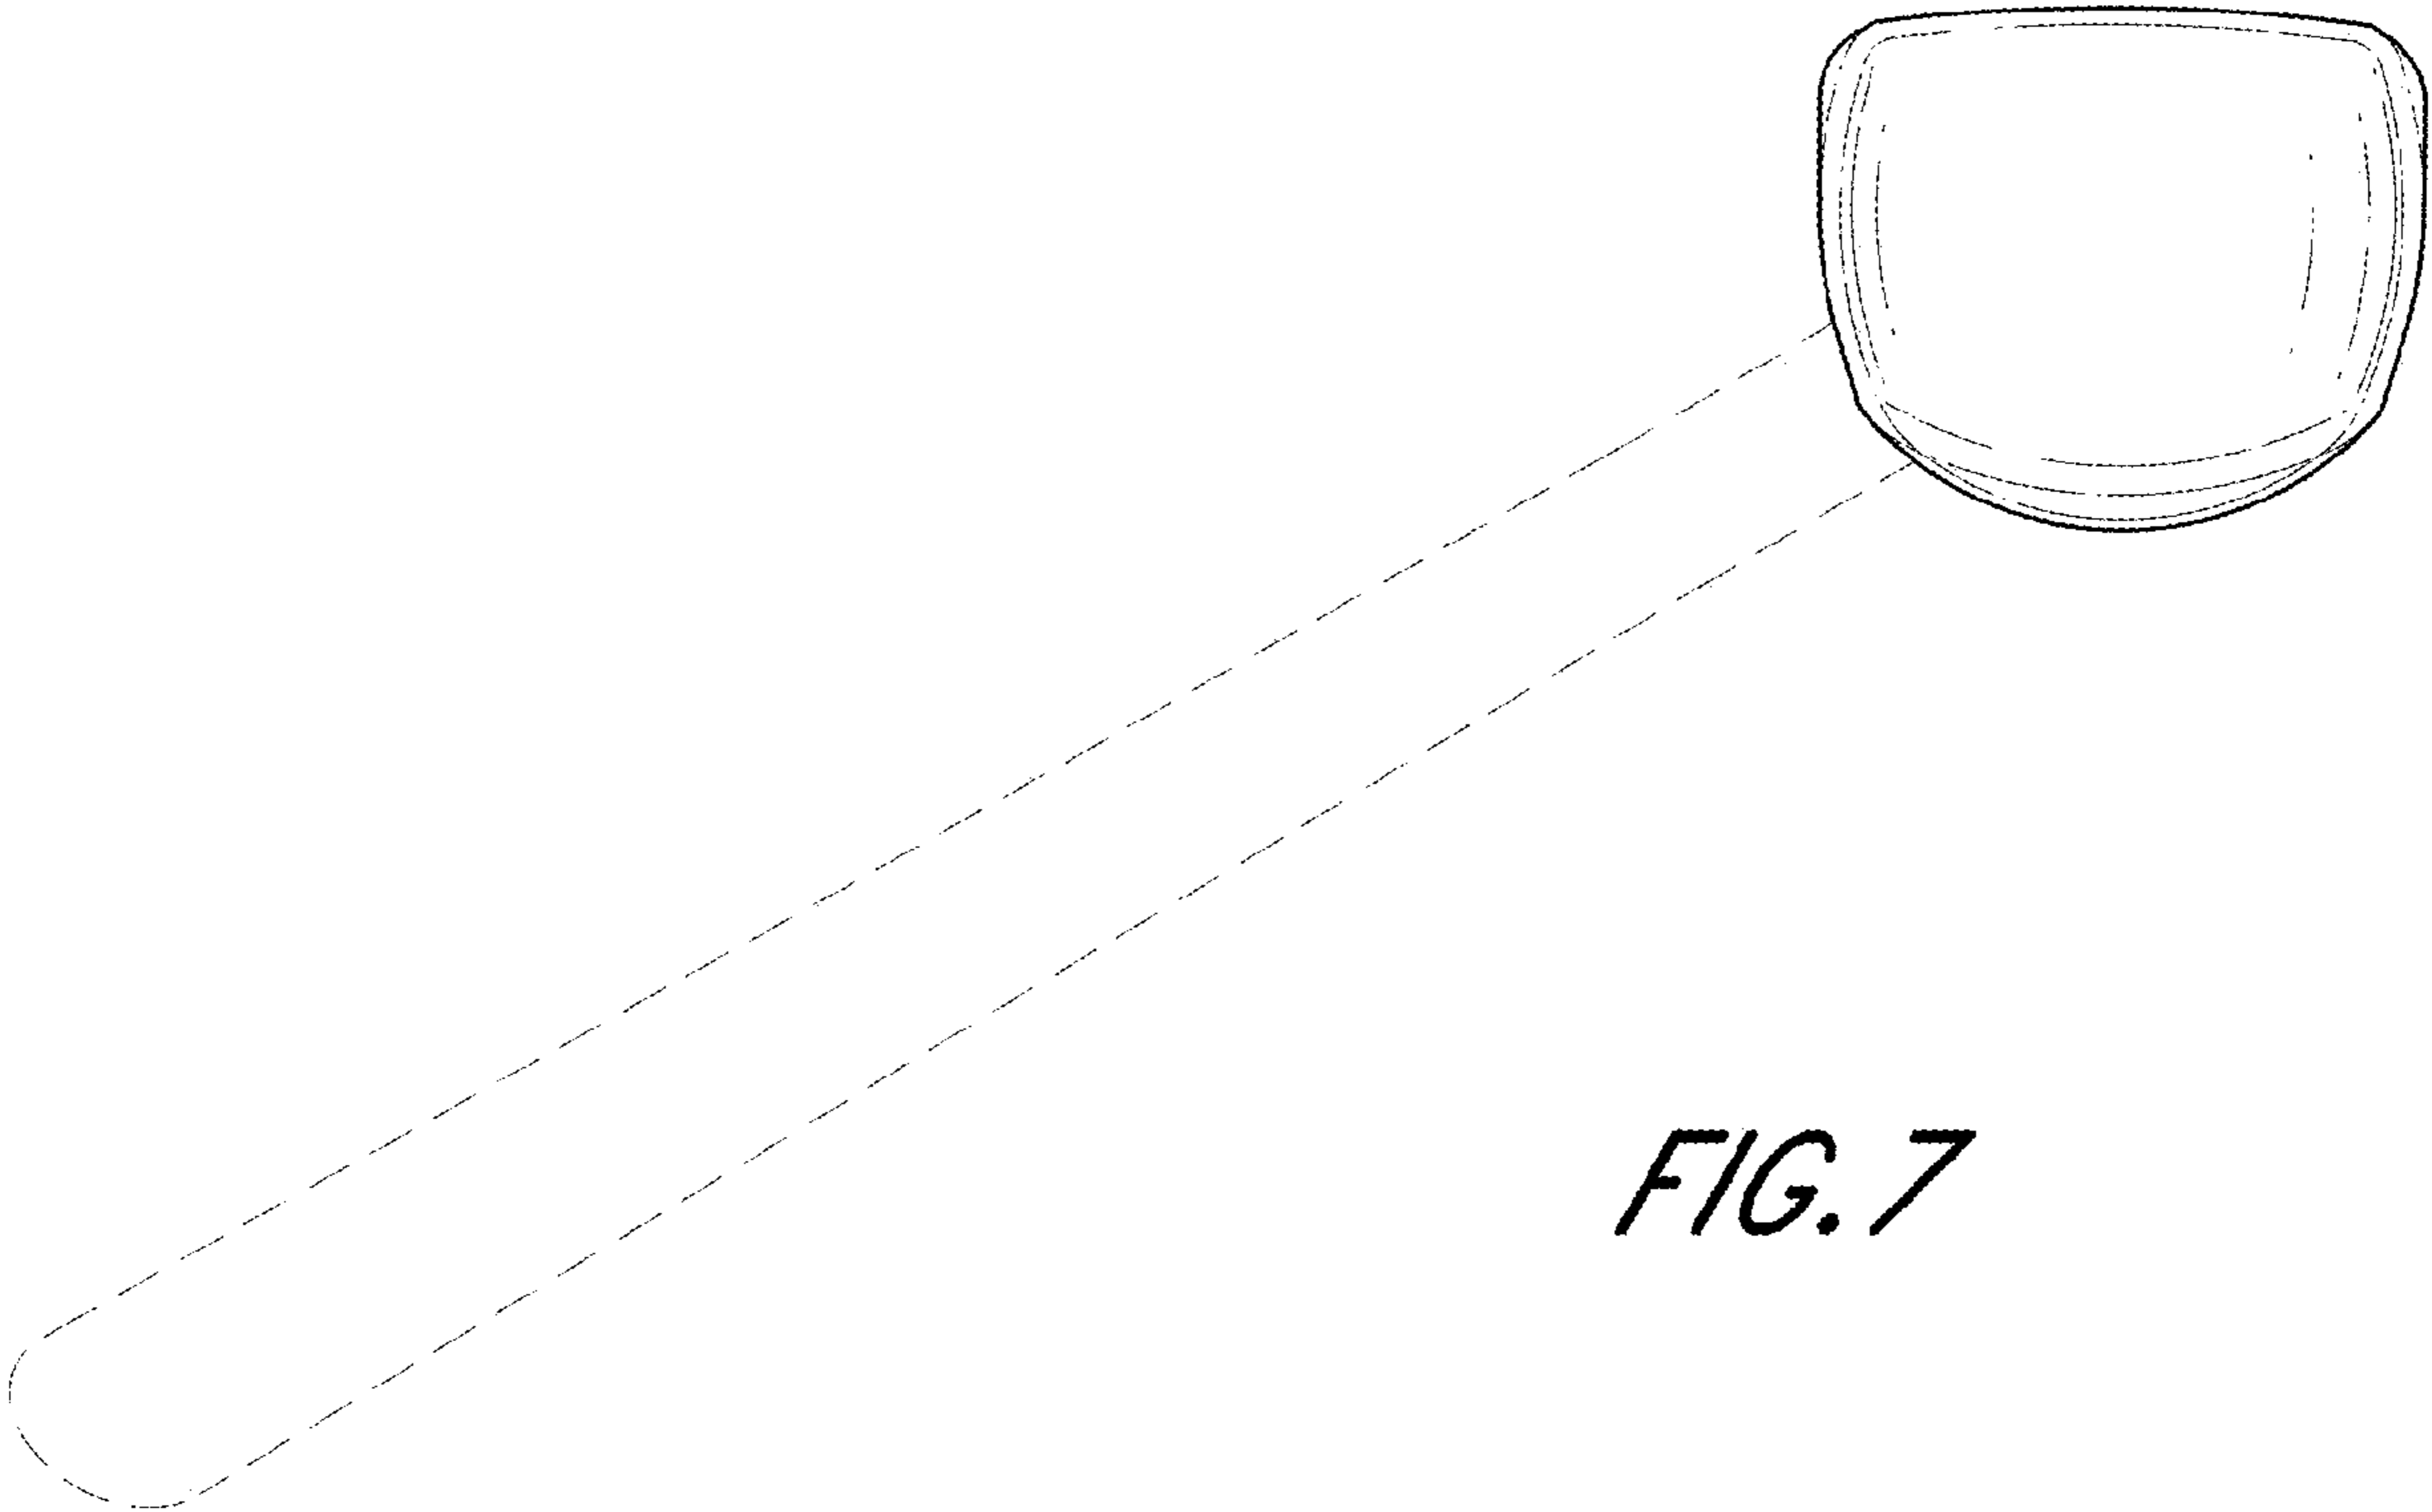

*FIG. 7*

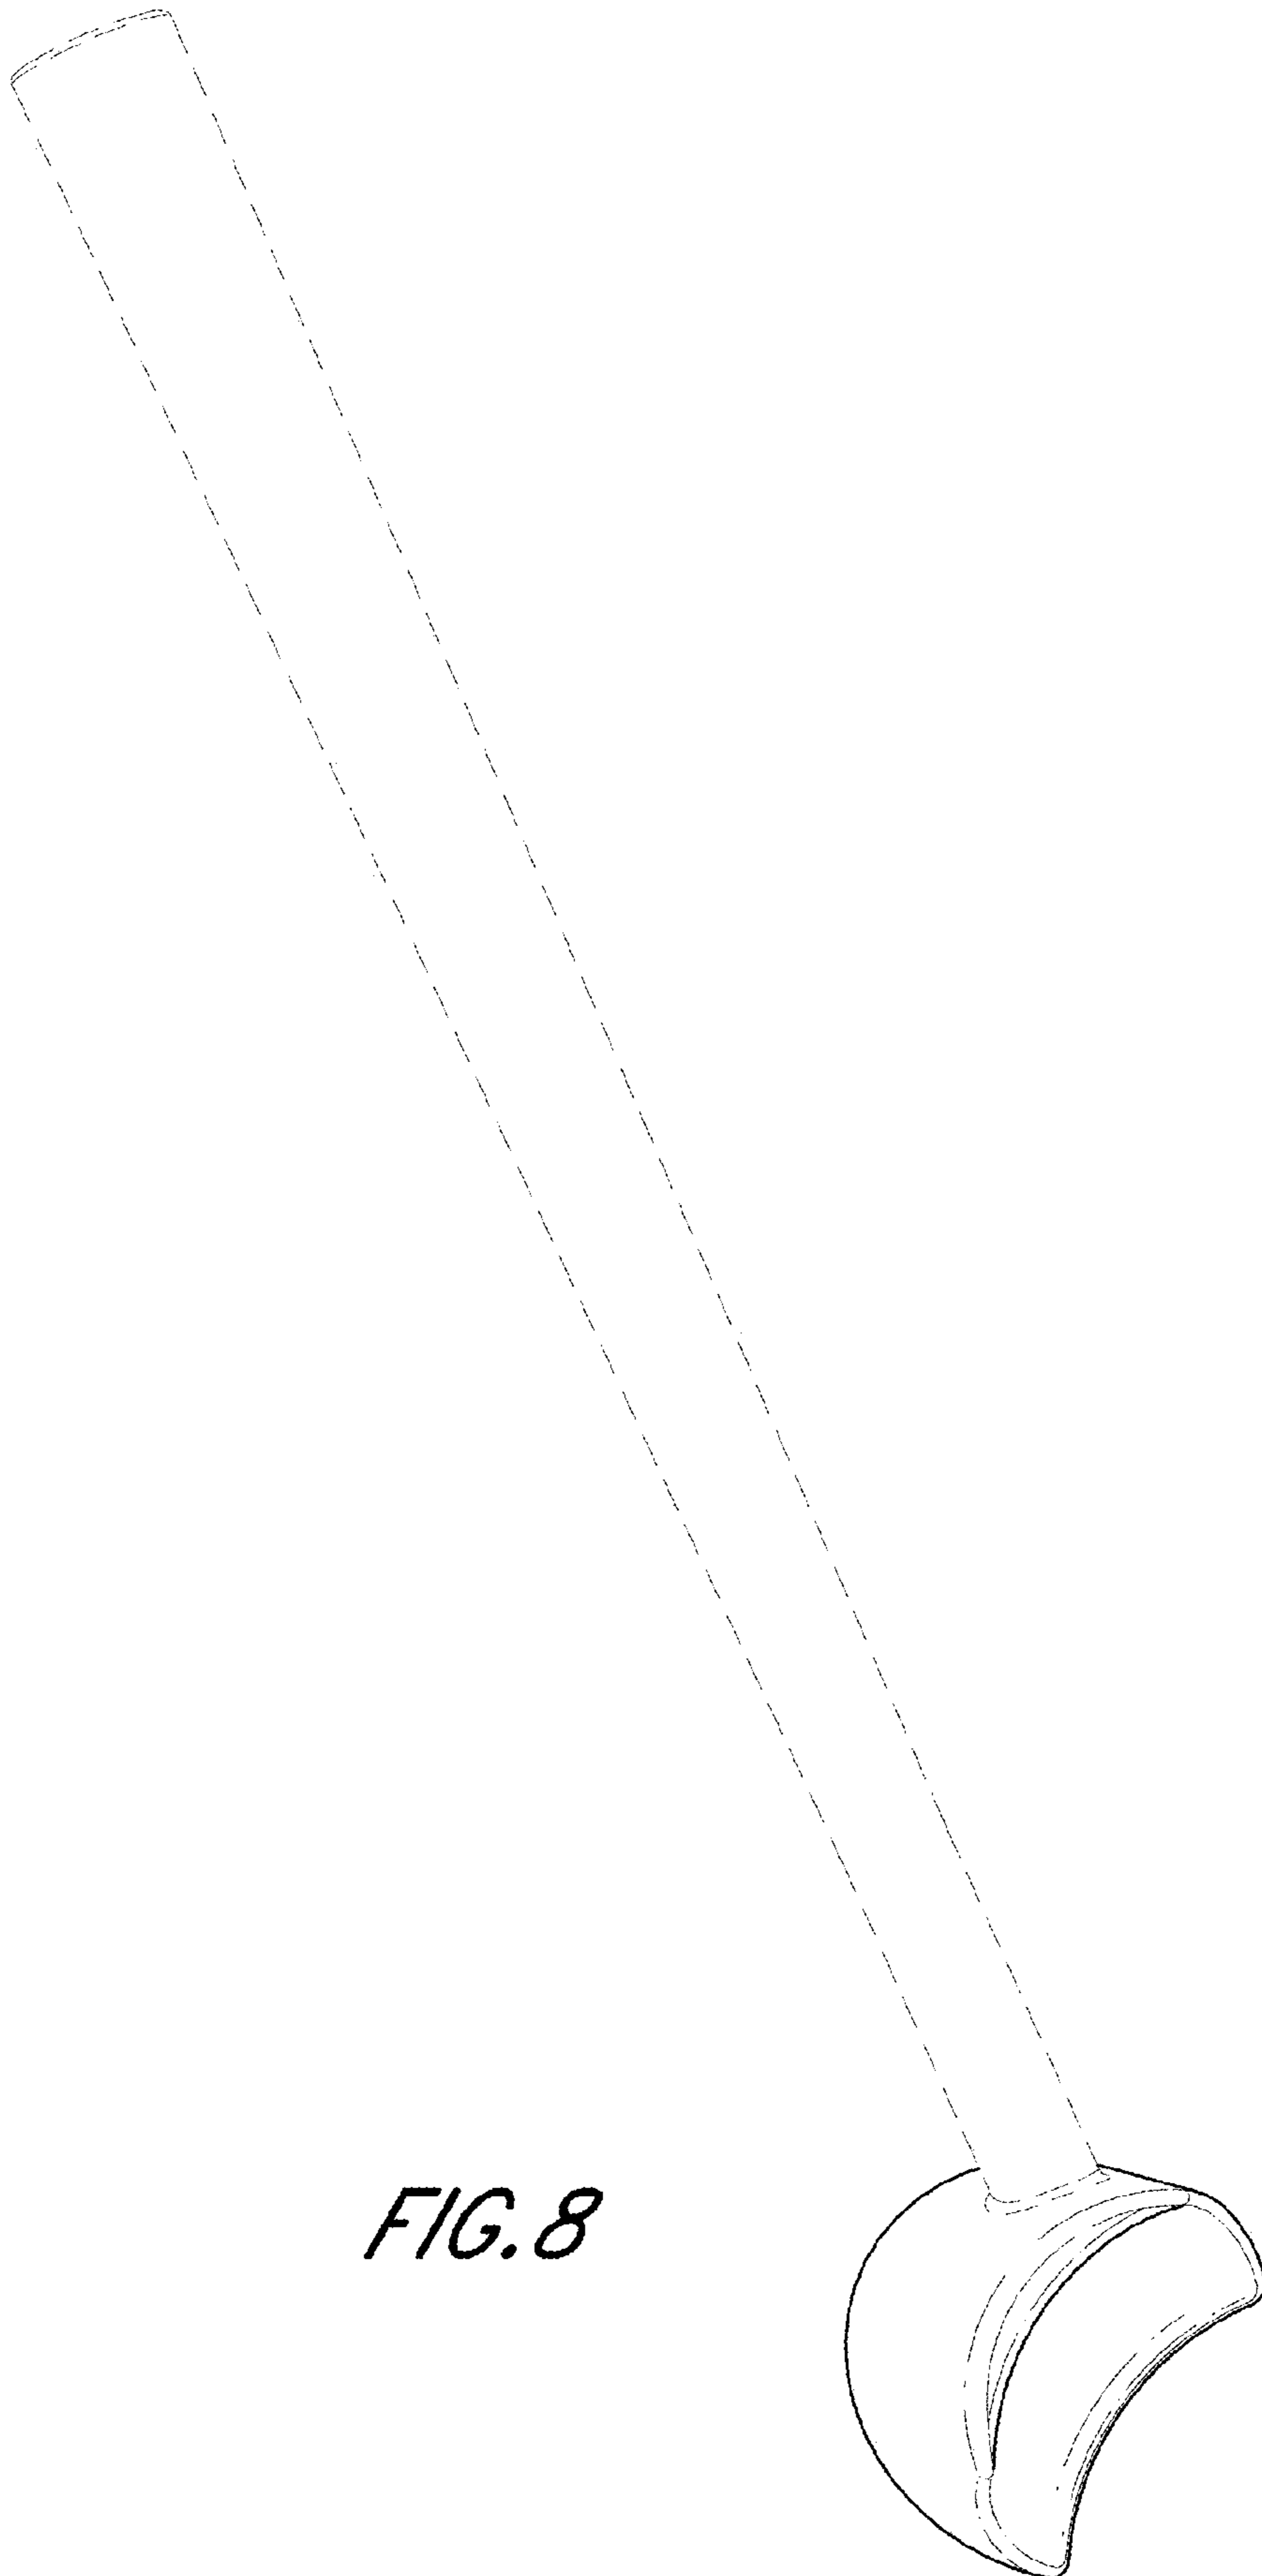

*FIG. 8*