



US00D887002S

(12) **United States Design Patent**  
**Geng**

(10) **Patent No.:** **US D887,002 S**

(45) **Date of Patent:** **\*\* Jun. 9, 2020**

(54) **MEDICAL PUNCTURE DEVICE**  
(71) Applicant: **TianJin Uwell Medical Device Manufacturing Co., Ltd, Tianjin (CN)**  
(72) Inventor: **Baogong Geng, Tianjin (CN)**  
(73) Assignee: **TIANJIN UWELL MEDICAL DEVICE MANUFACTURING CO., LTD, Tianjin (CN)**

2009/0093835 A1\* 4/2009 Heinrich ..... A61B 17/3209  
606/190  
2010/0016878 A1\* 1/2010 Smith ..... A61B 17/3417  
606/185  
2011/0046449 A1\* 2/2011 Minelli ..... A61B 1/00128  
600/205

(\*\*) Term: **15 Years**  
(21) Appl. No.: **29/656,509**

(22) Filed: **Jul. 13, 2018**  
(51) **LOC (12) Cl.** ..... **24-02**  
(52) **U.S. Cl.**  
USPC ..... **D24/146**  
(58) **Field of Classification Search**  
USPC ..... D24/127, 130, 133, 146, 147, 148;  
128/848; 606/106, 108; D7/649; D8/93,  
D8/97, 300, 310, 311, 313  
CPC ..... A61B 1/018; A61B 2017/2939; A61F  
2210/0038; A61F 5/566  
See application file for complete search history.

**OTHER PUBLICATIONS**

The Bladeless Trocar For Single Use [http://www.uwellmed.com/PRODUCT-DETAILS.html?product\\_id=12](http://www.uwellmed.com/PRODUCT-DETAILS.html?product_id=12) Accessed Sep. 29, 2019.\*  
The Bladeless Trocar for Single Use [http://www.uwellmed.com/PRODUCT-DETAILS.html?product\\_id=14&product\\_category=9](http://www.uwellmed.com/PRODUCT-DETAILS.html?product_id=14&product_category=9) Date Unknown.\*

\* cited by examiner

*Primary Examiner* — Samantha Q Lawrence  
(74) *Attorney, Agent, or Firm* — Gokalp Bayramoglu

(57) **CLAIM**

The ornamental design for a medical puncture device, as shown and described.

**DESCRIPTION**


(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D606,193 S \* 12/2009 Oberlaender ..... D24/146  
D713,033 S \* 9/2014 Sauer ..... D24/146  
D797,288 S \* 9/2017 Zhou ..... D24/146  
D813,389 S \* 3/2018 Zhou ..... D24/146  
D814,032 S \* 3/2018 Zhou ..... D24/146  
2004/0230161 A1\* 11/2004 Zeiner ..... A61B 17/34  
604/167.06  
2007/0066988 A1\* 3/2007 Datta ..... A61B 17/3417  
606/185  
2007/0185453 A1\* 8/2007 Michael ..... A61B 17/3462  
604/164.01

FIG. 1 is a front view of a medical puncture device showing the new design;  
FIG. 2 is a rear view thereof;  
FIG. 3 is a right side view thereof;  
FIG. 4 is a left side view thereof;  
FIG. 5 is a top view thereof;  
FIG. 6 is a bottom view thereof; and,  
FIG. 7 is a perspective view thereof.  
The broken lines shown in FIGS. 1-7 illustrate portions of the medical puncture device that form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

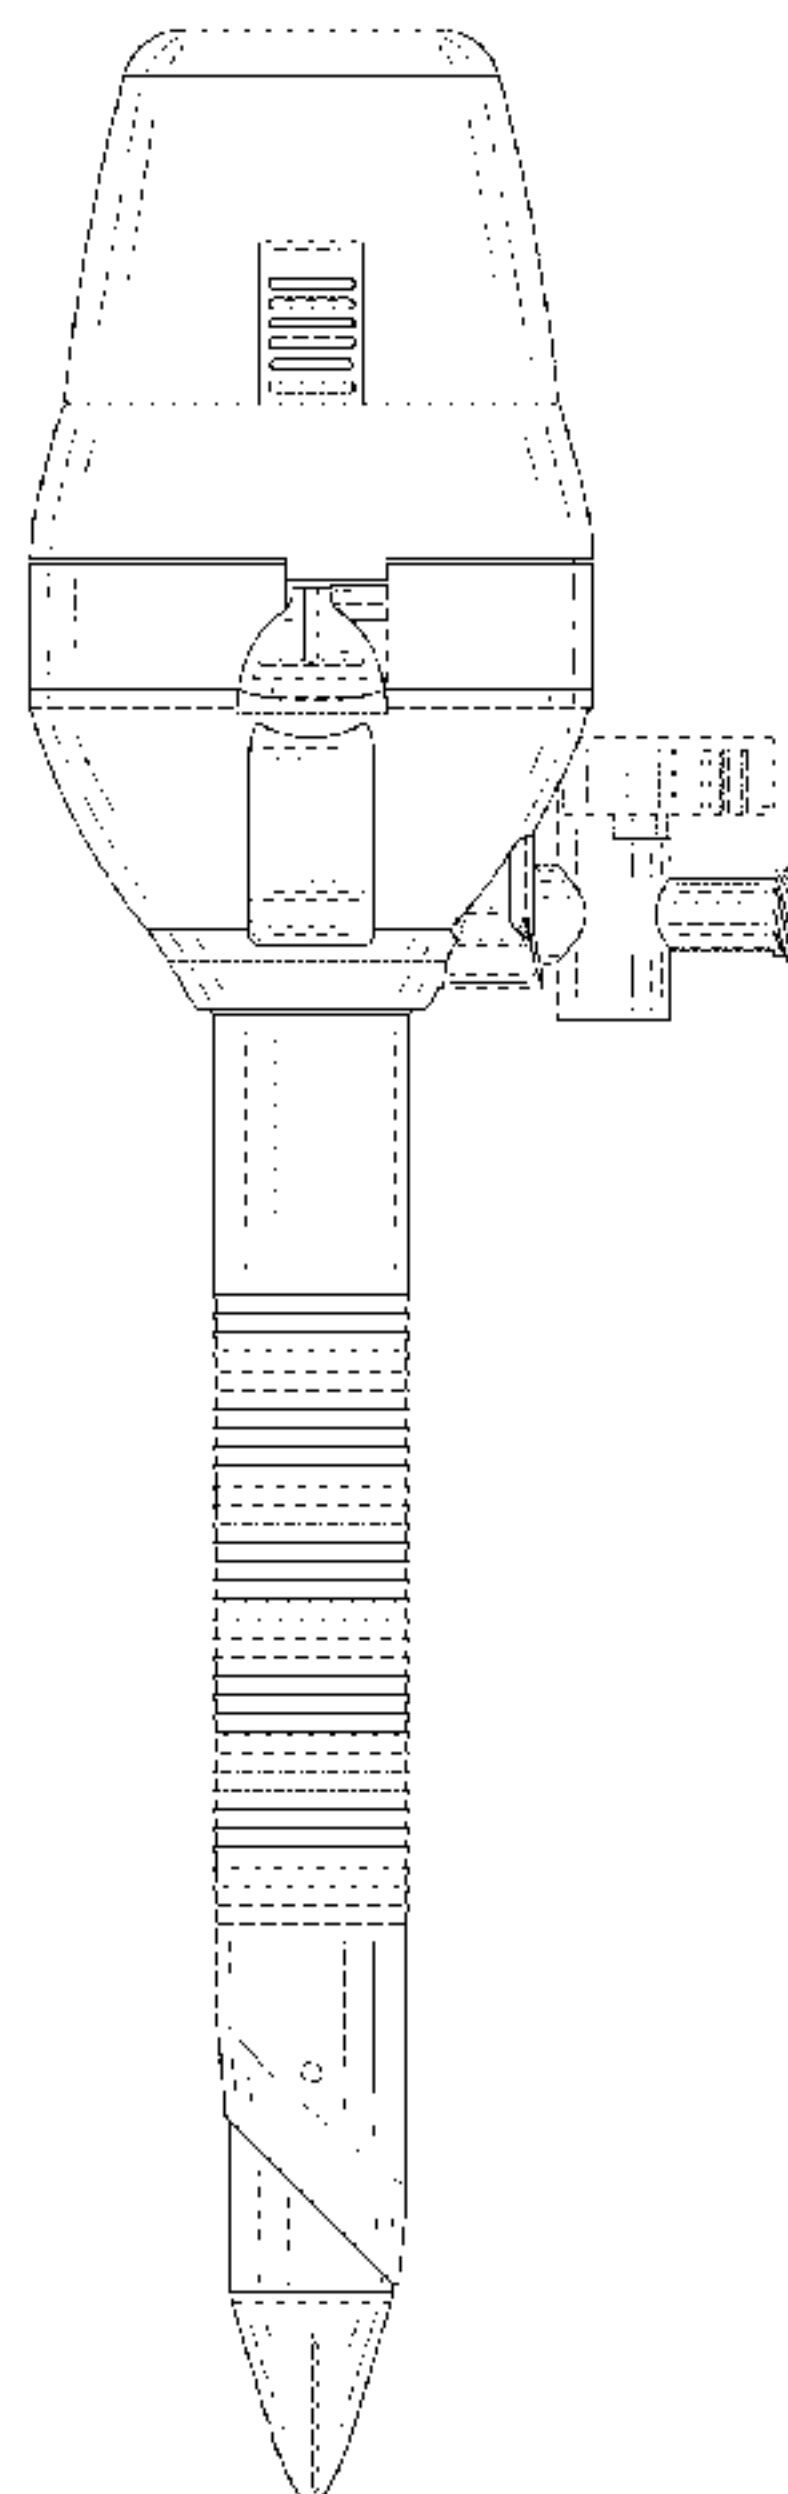

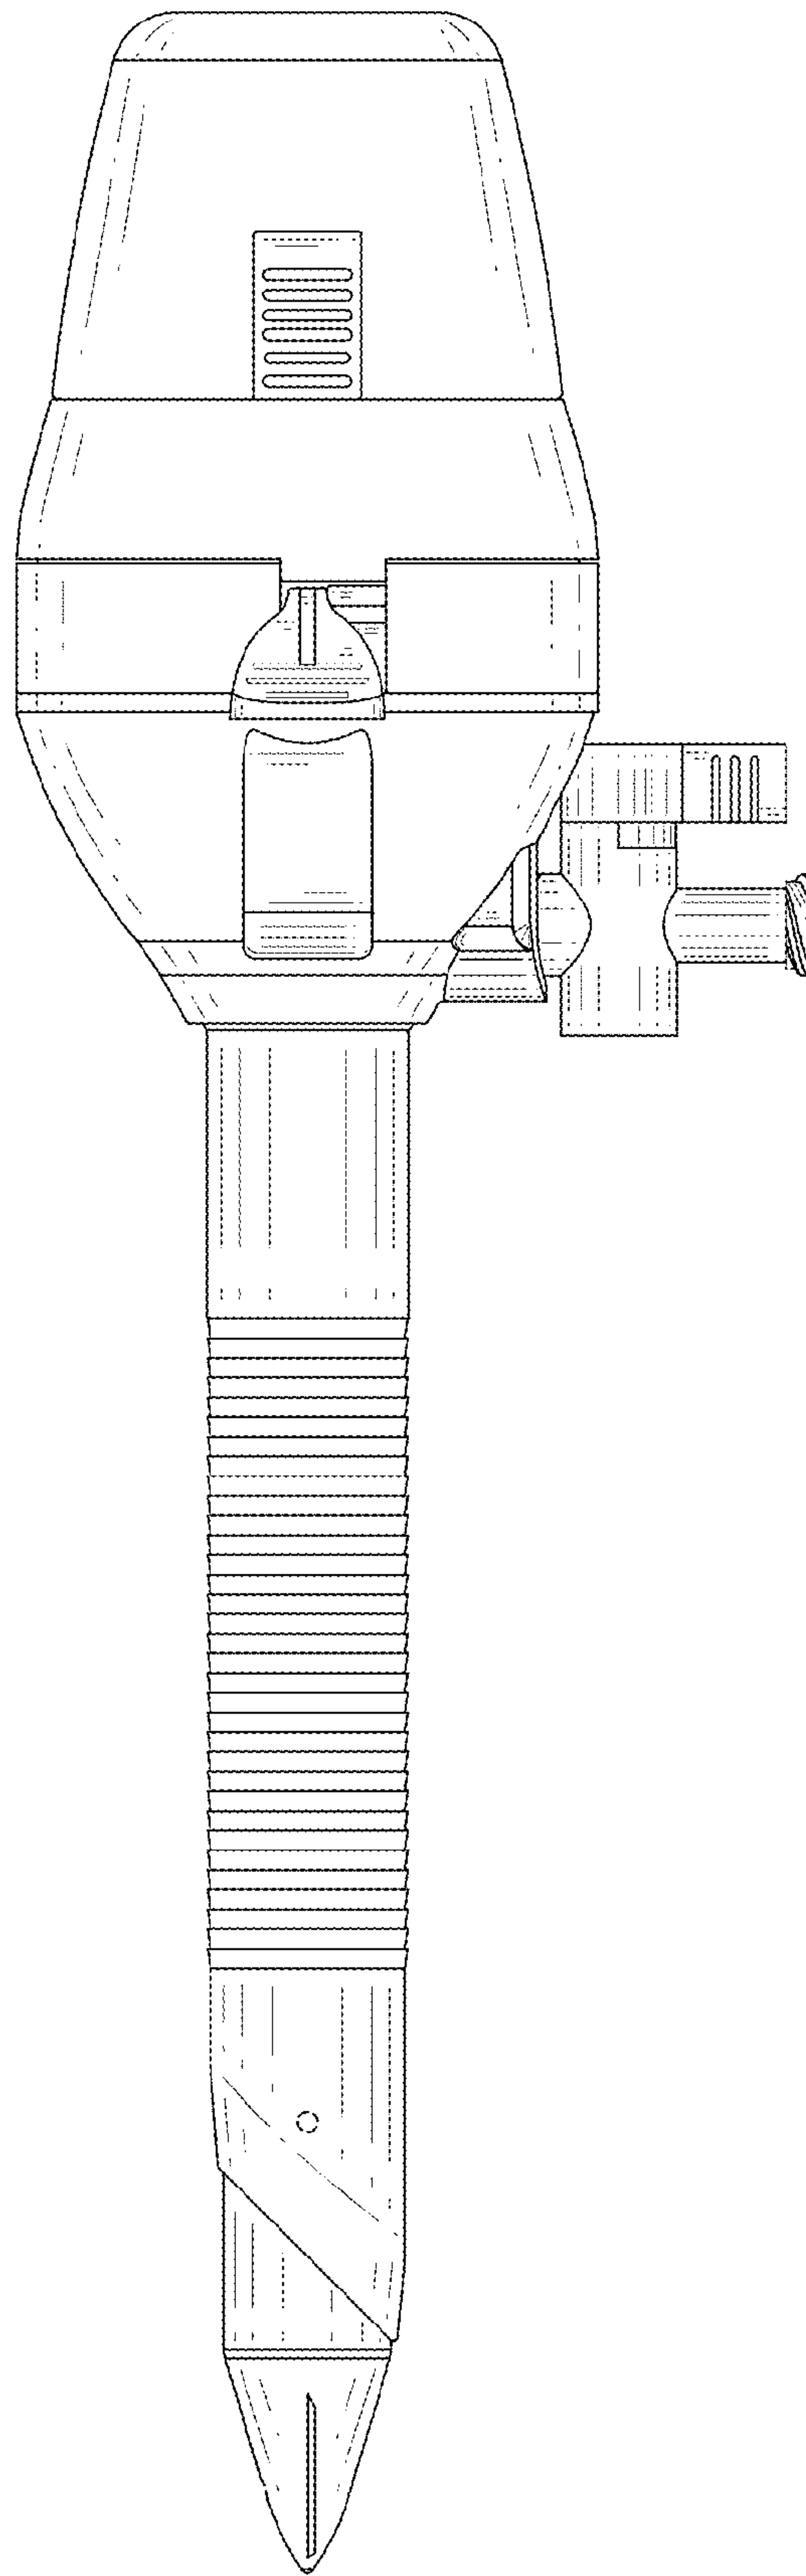


Fig. 1

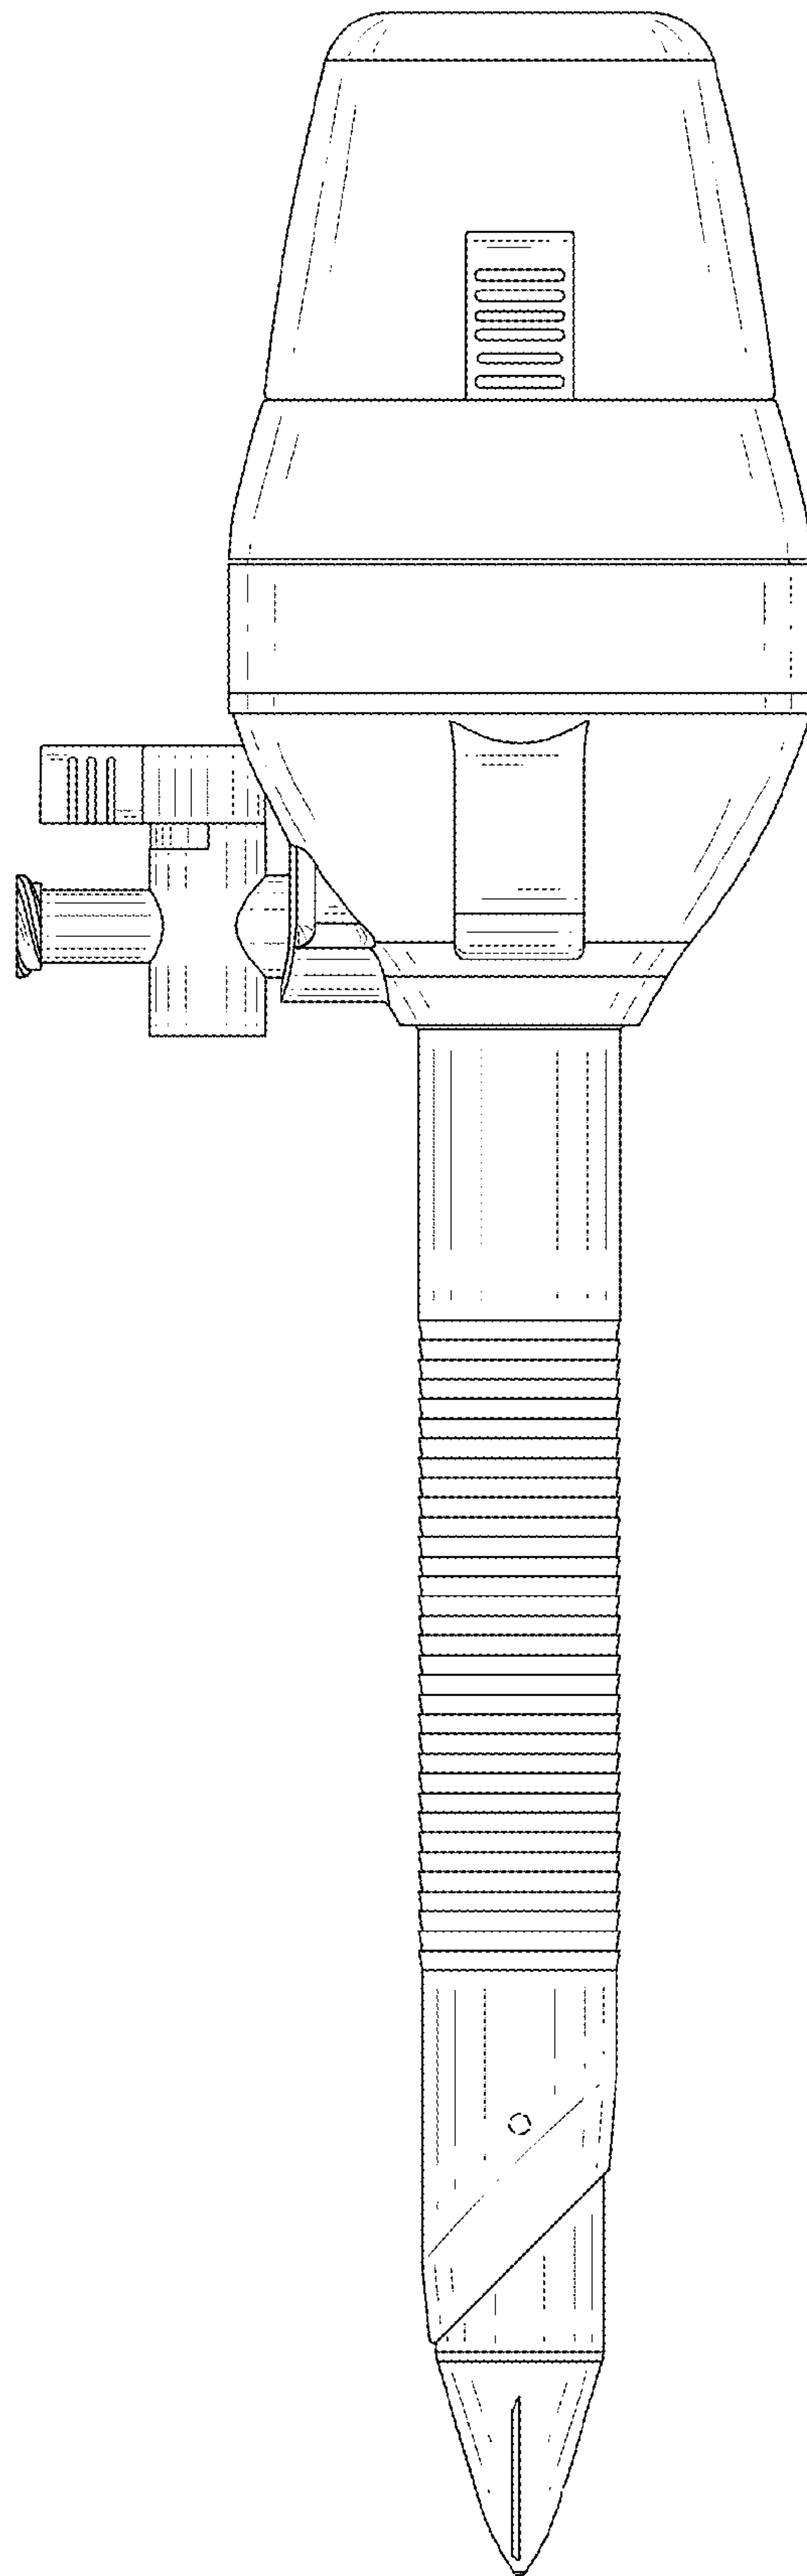


Fig. 2

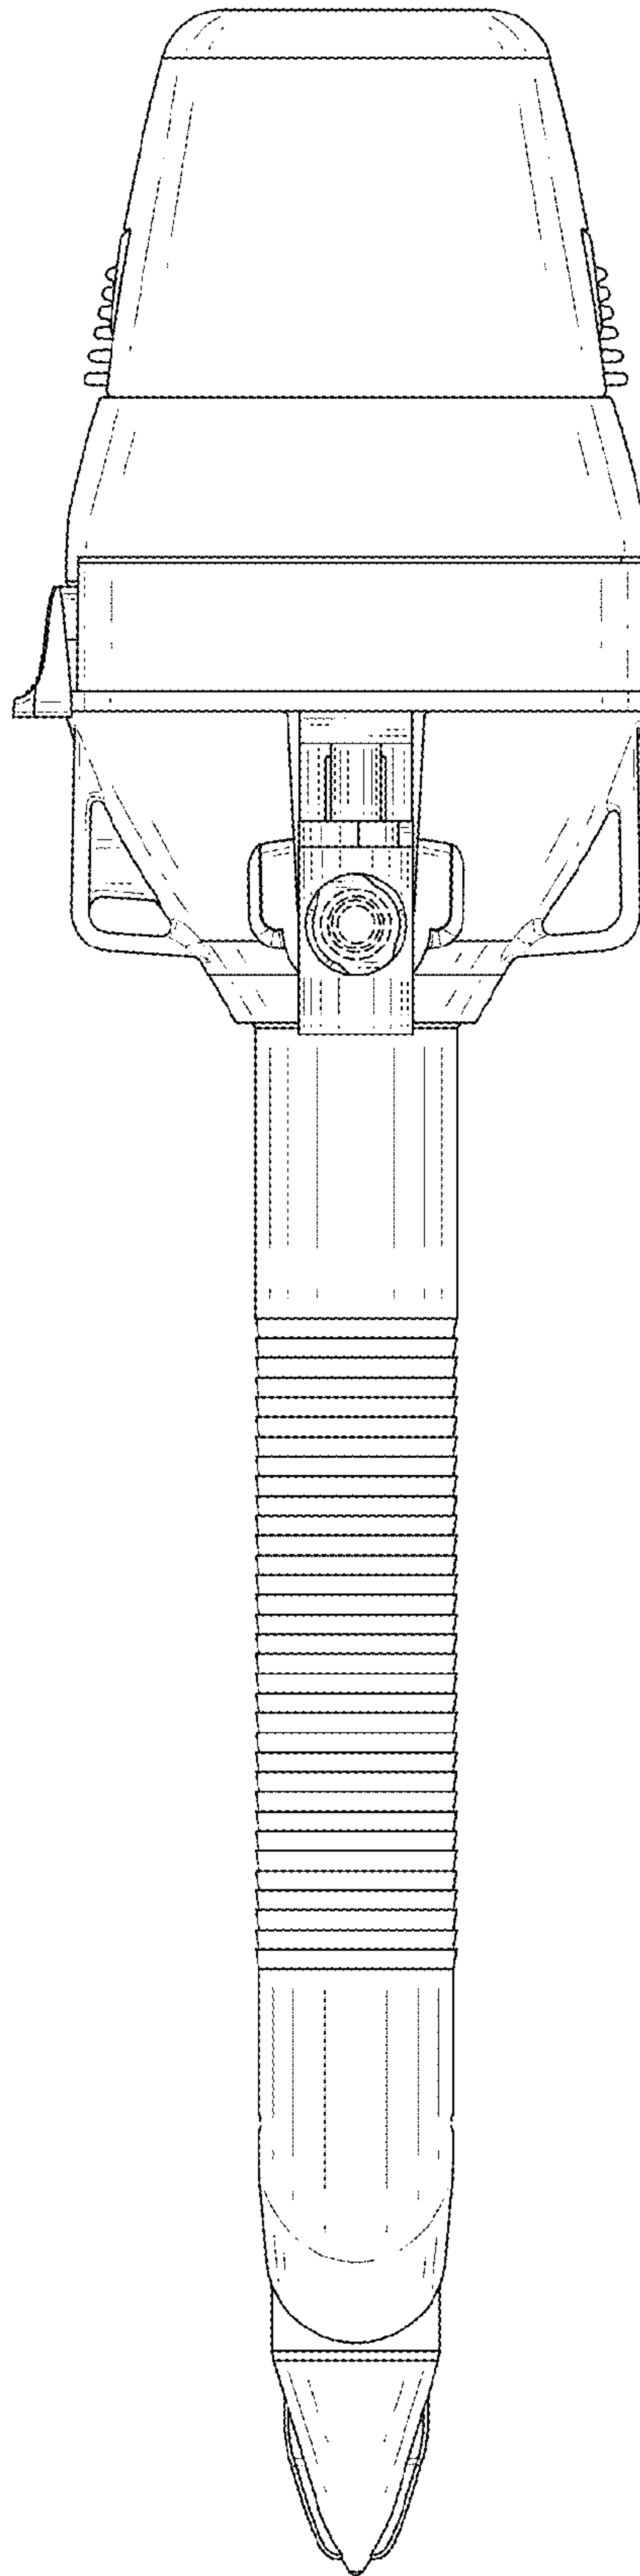


Fig. 3

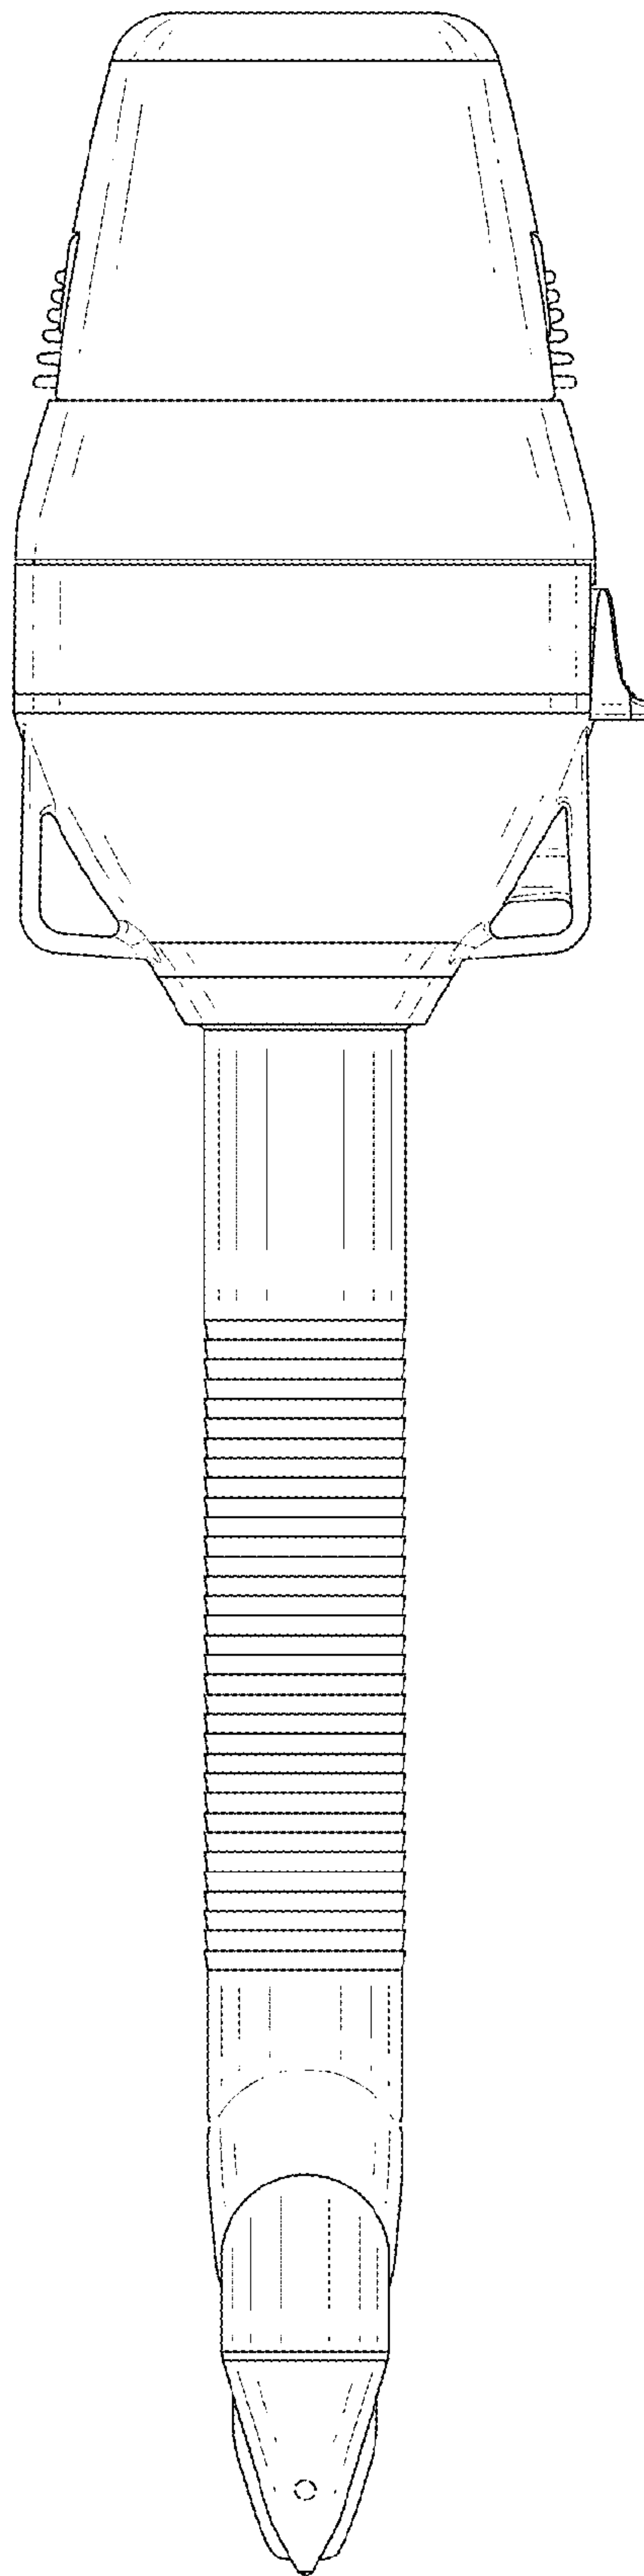


Fig. 4

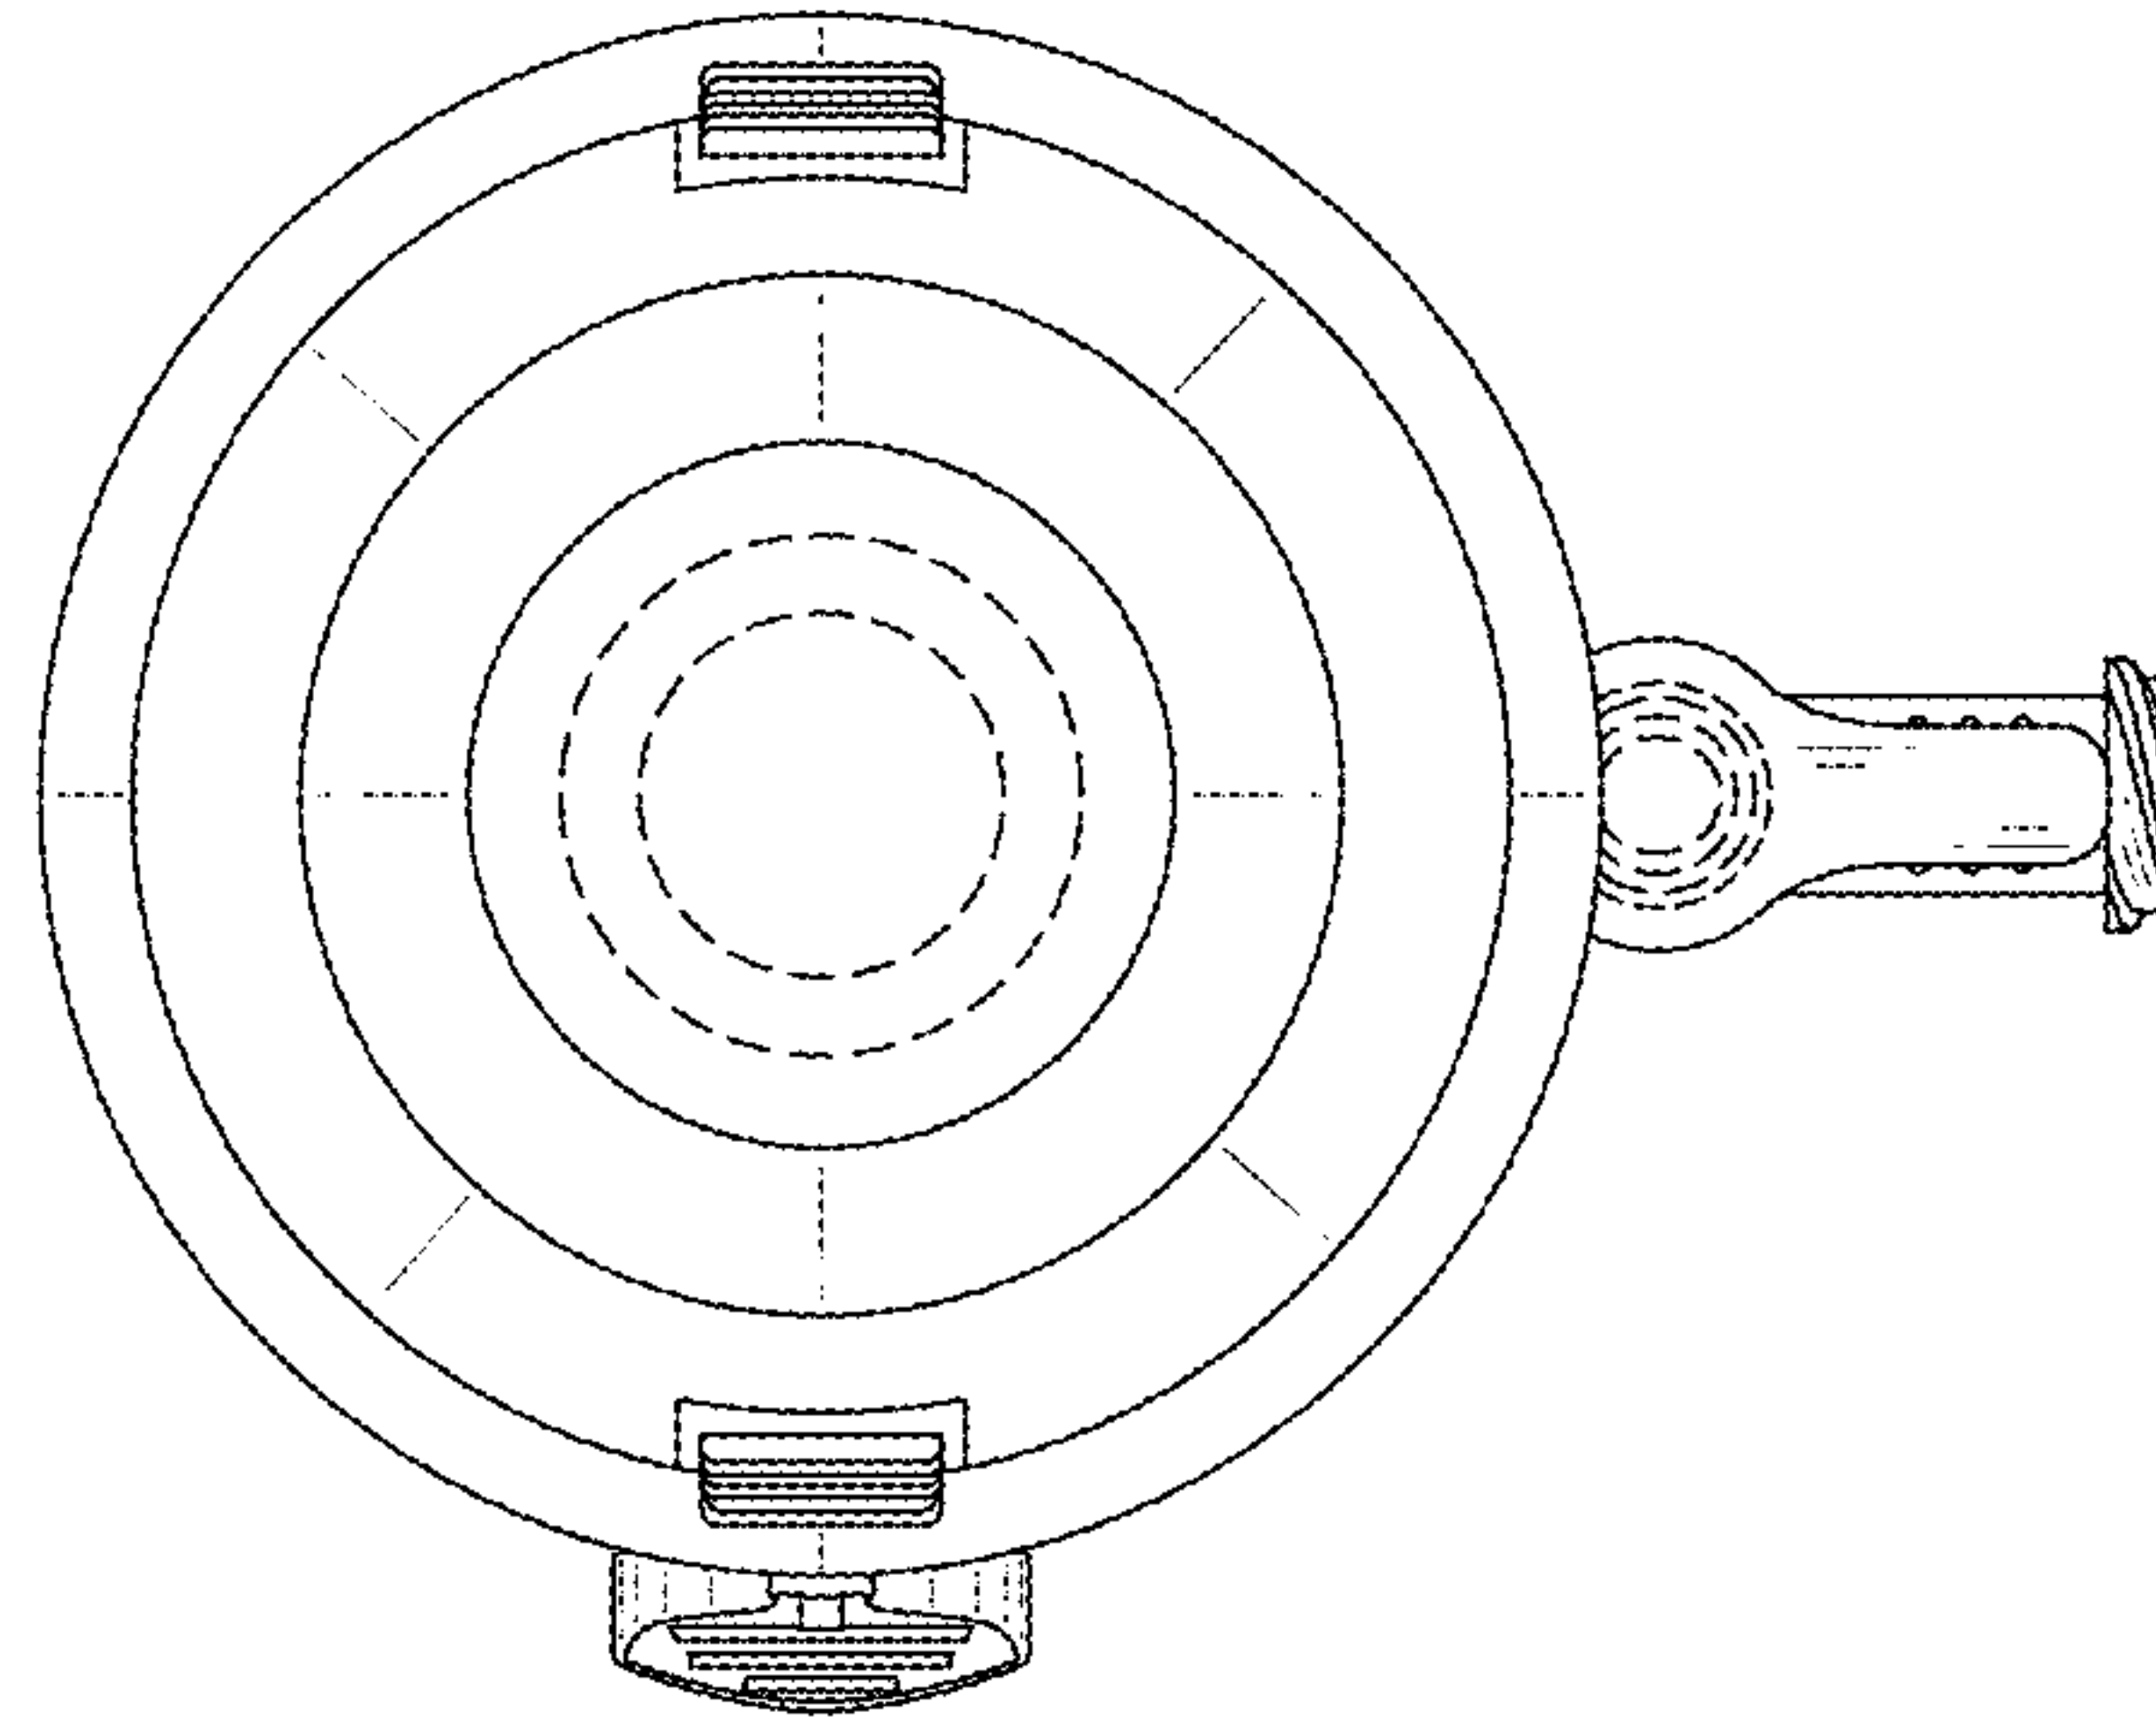


Fig. 5

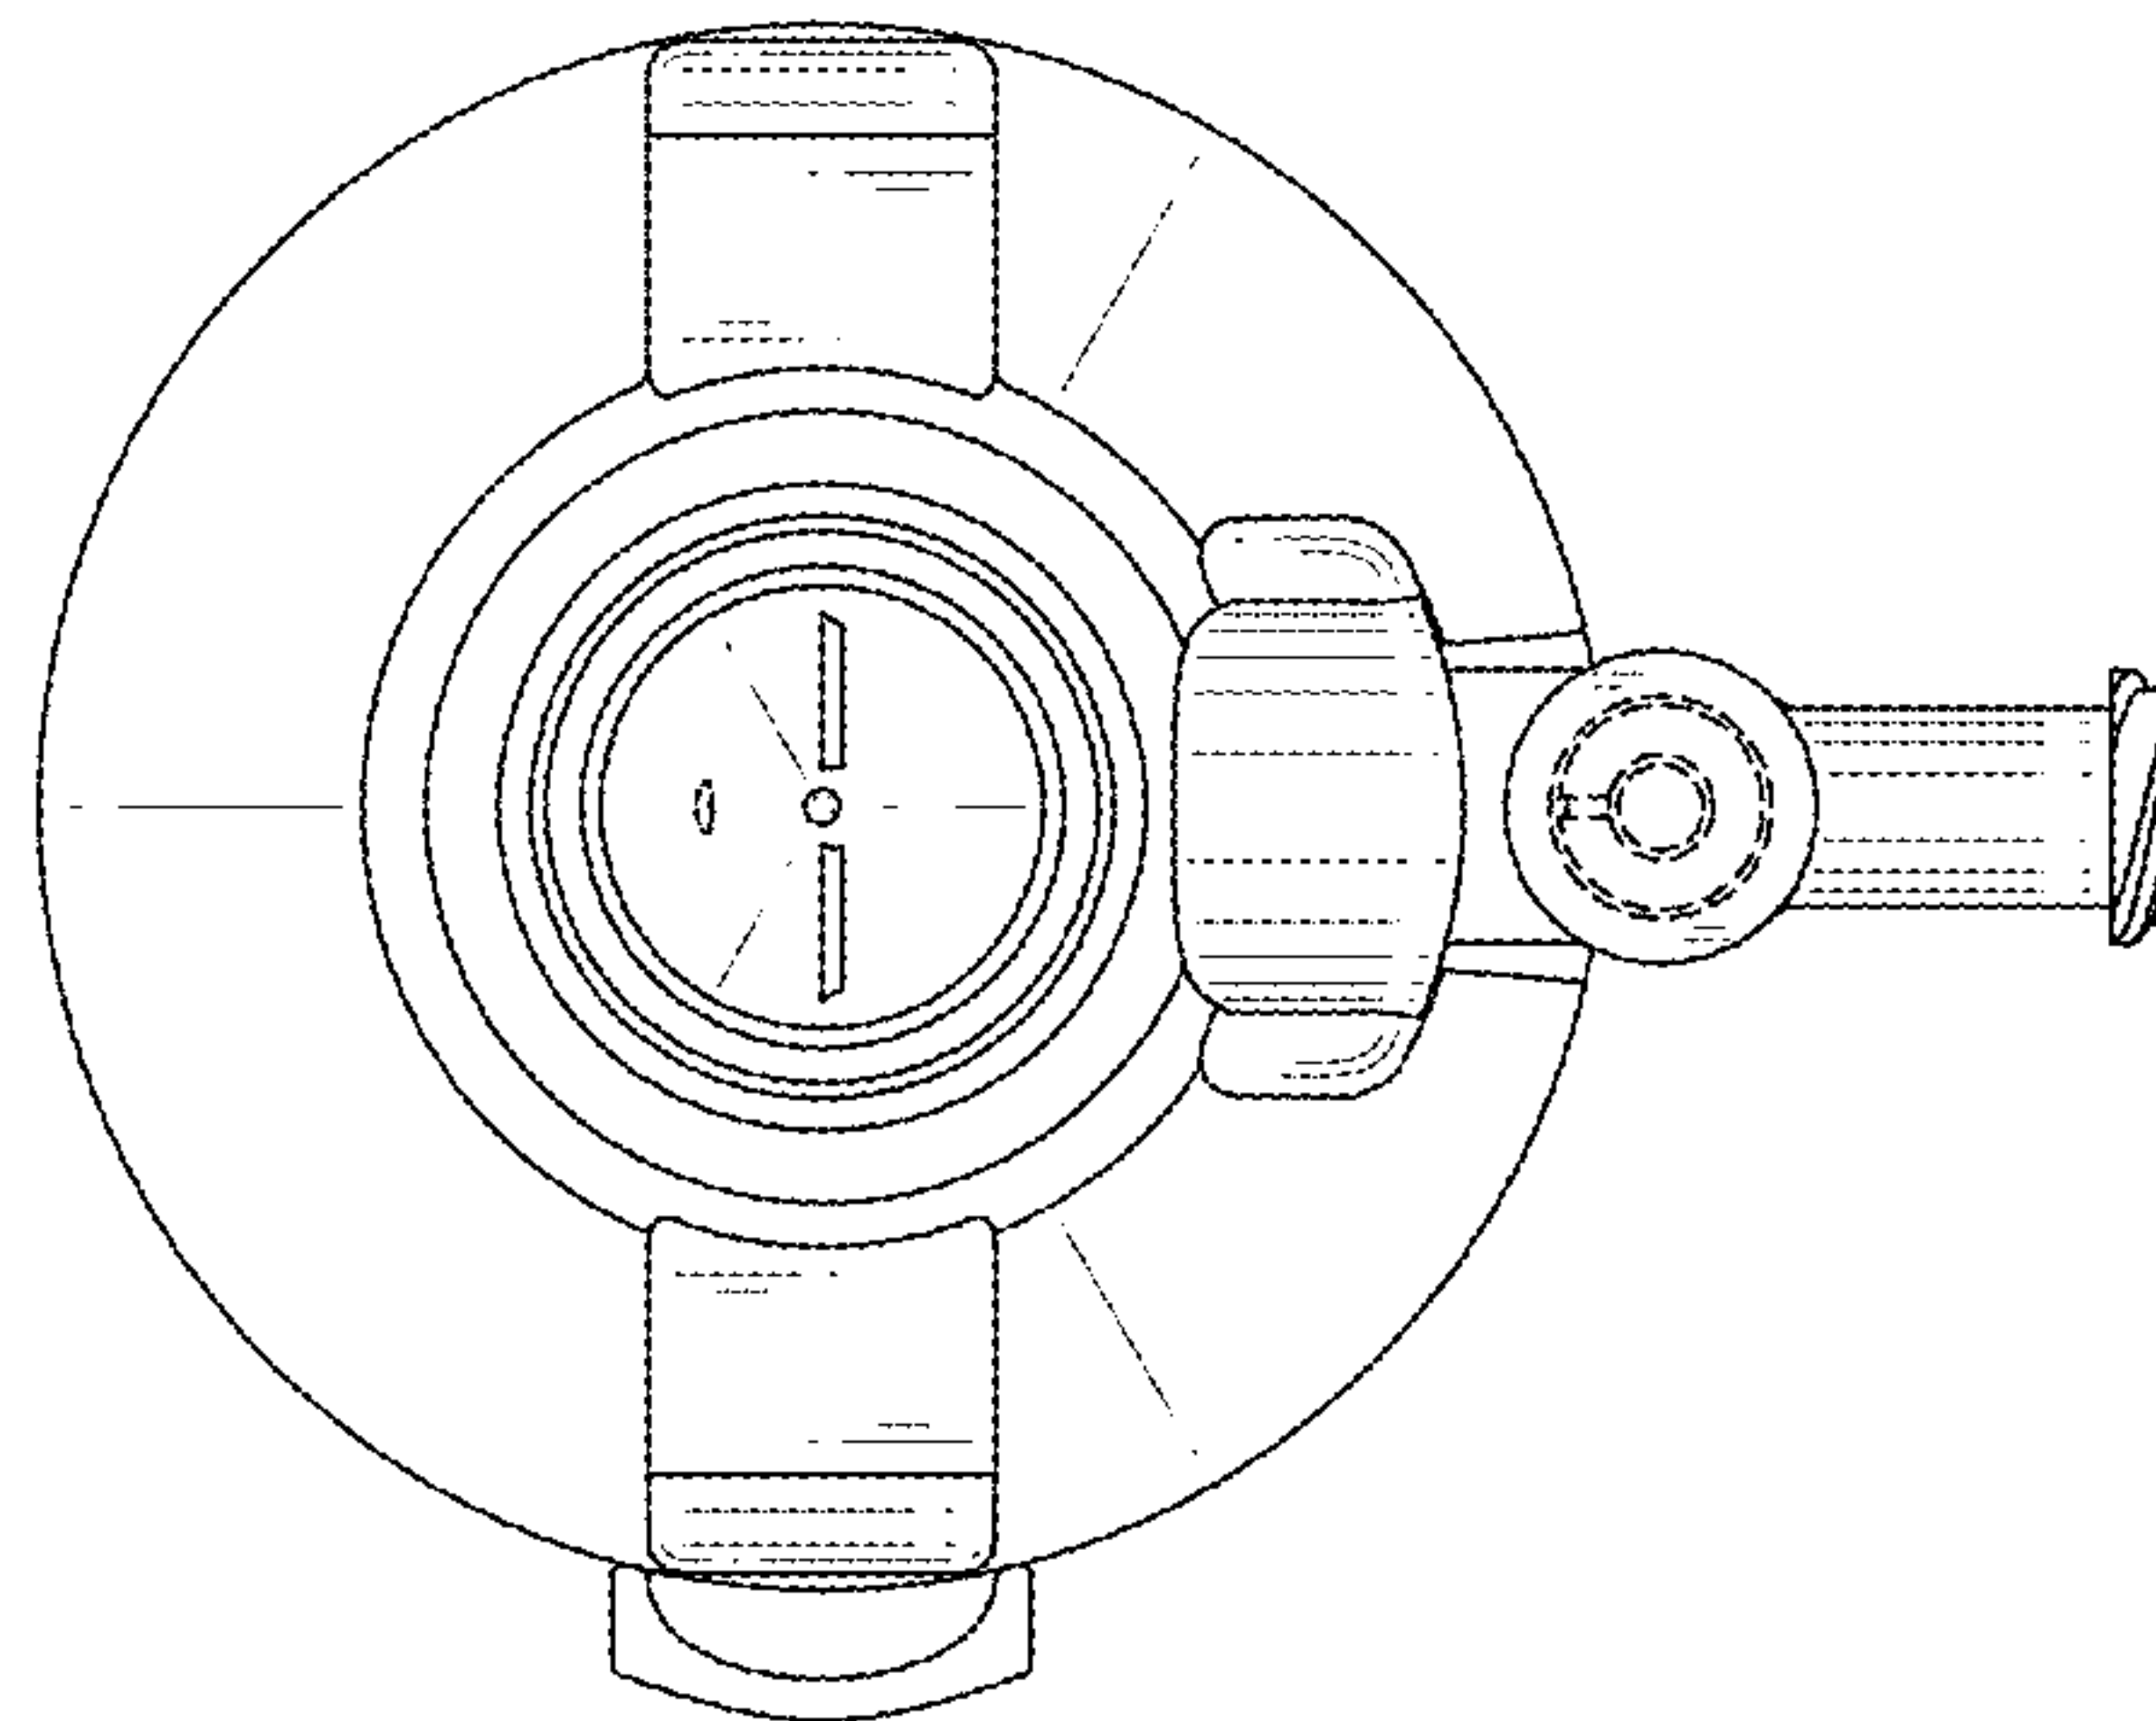


Fig. 6



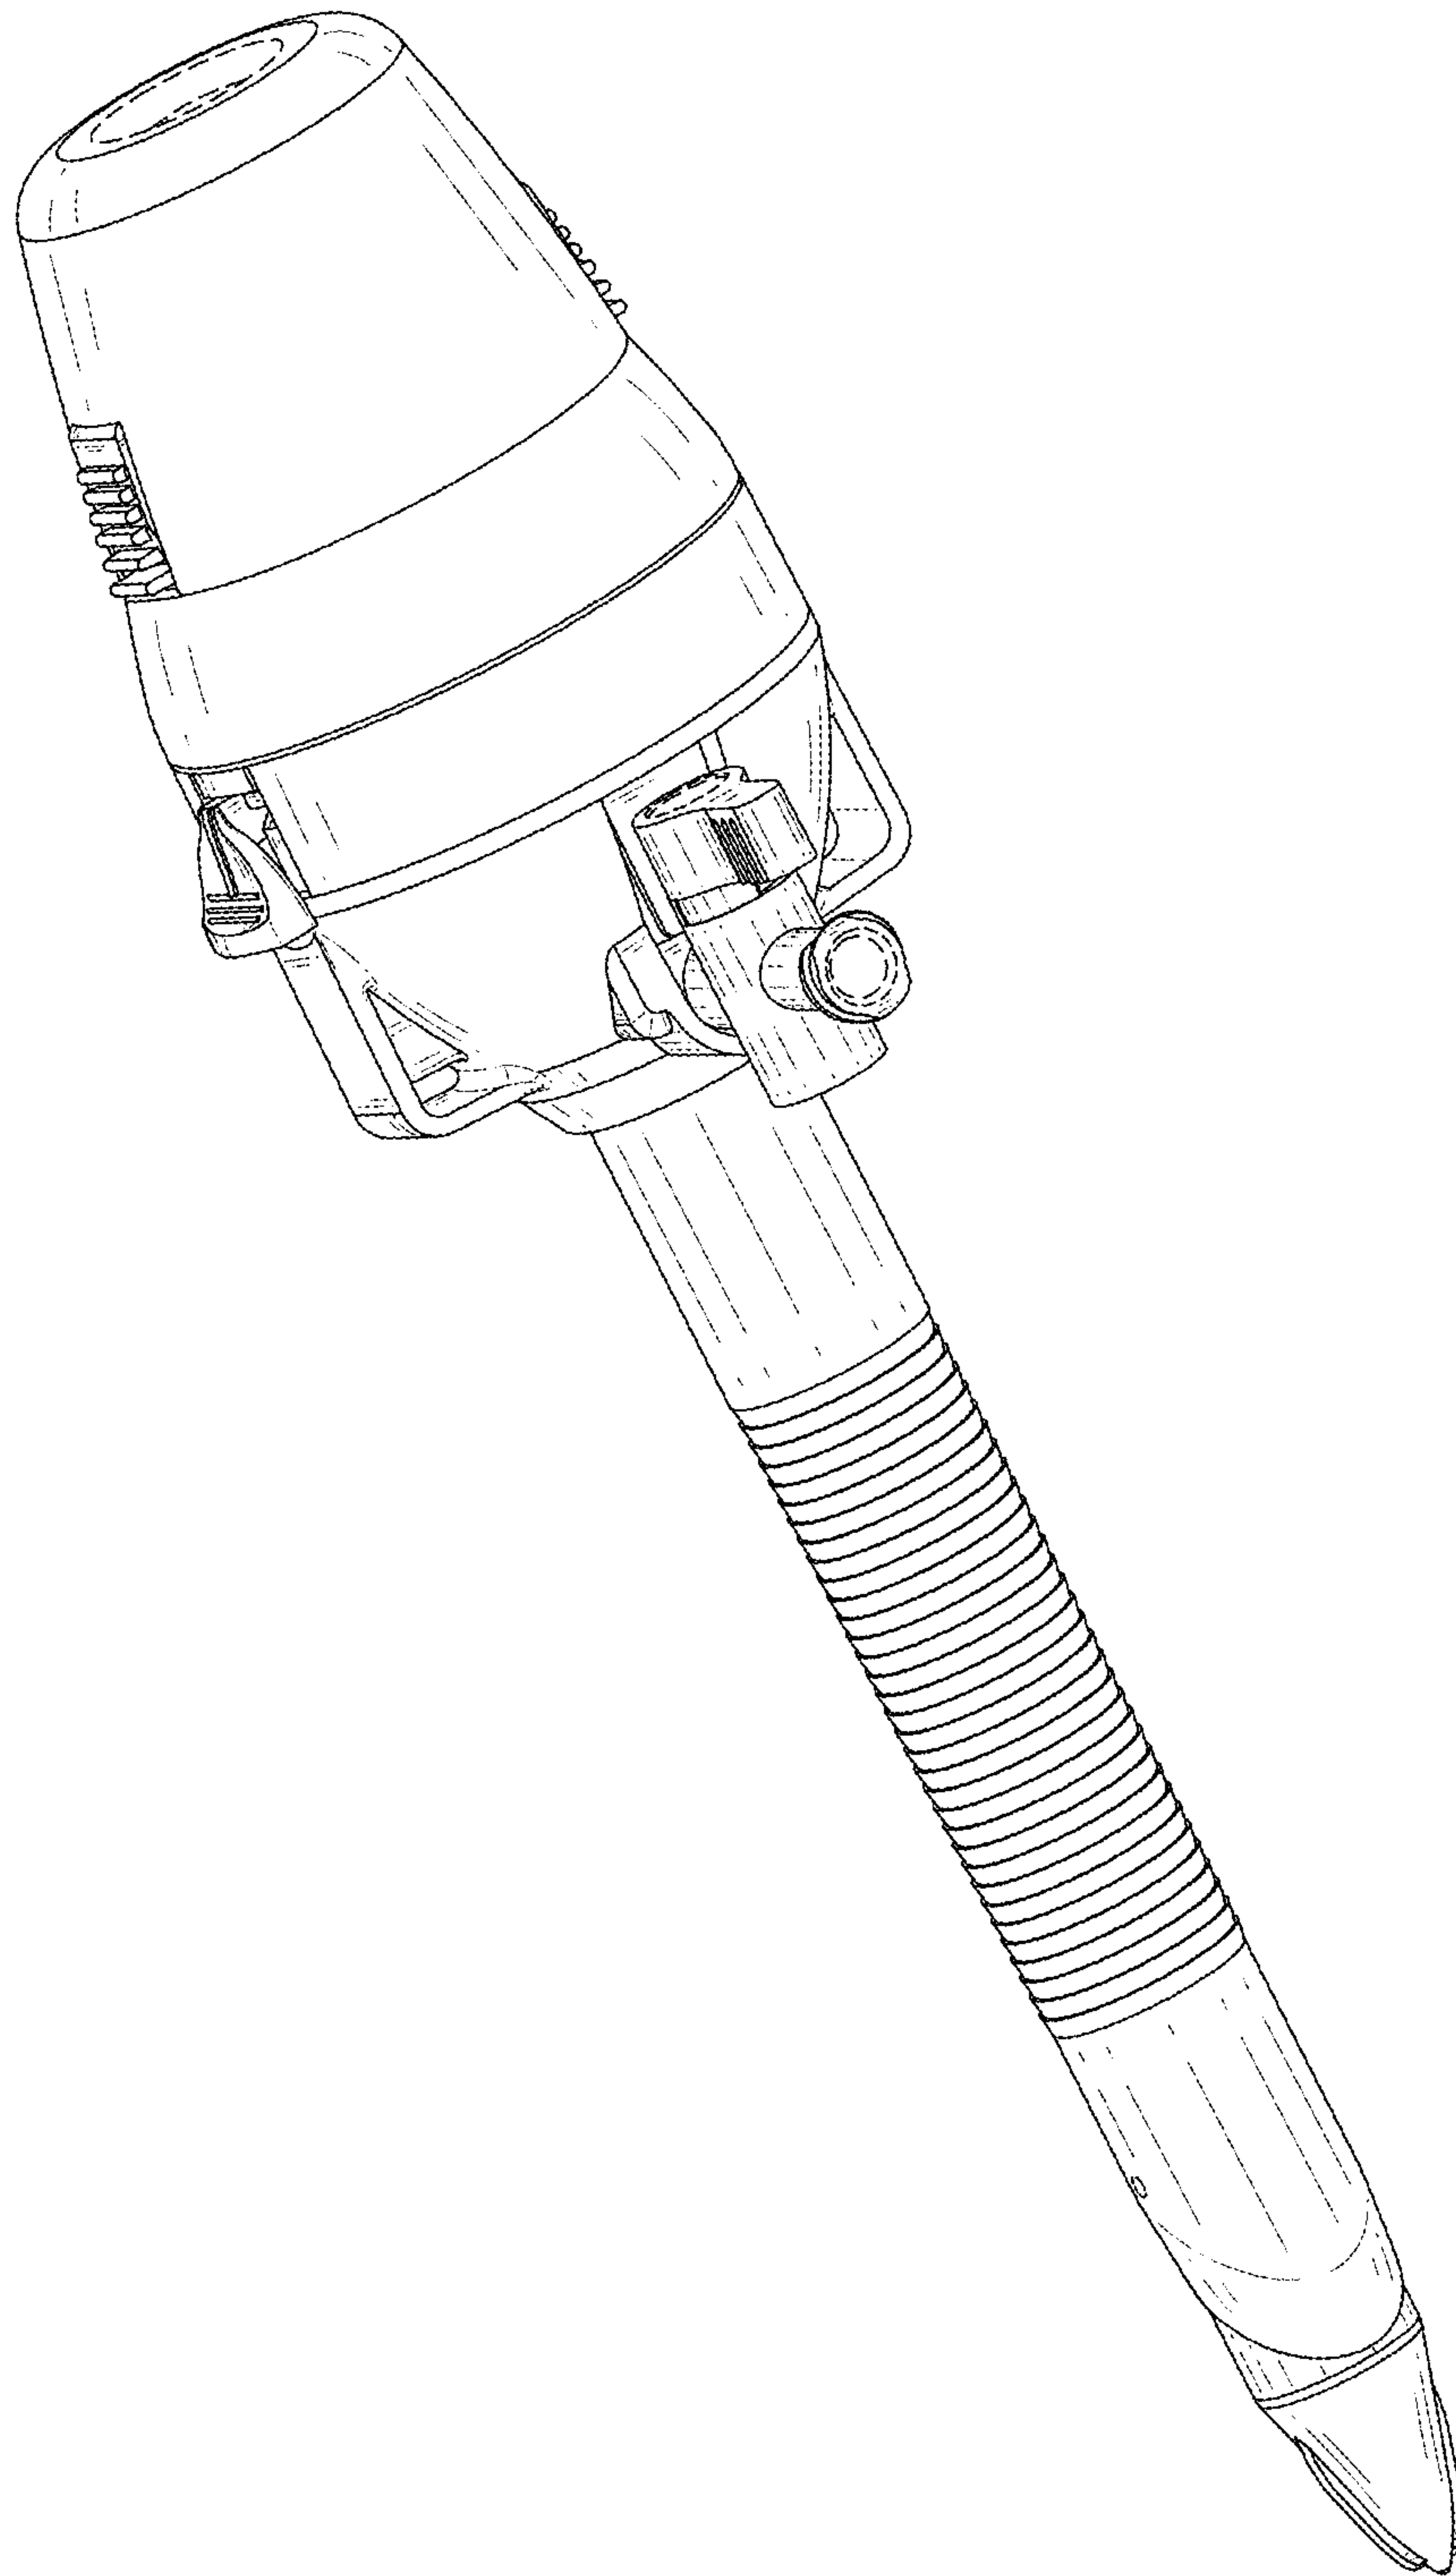


Fig. 7