



US00D887556S

(12) **United States Design Patent**  
**Lockenwitz**

(10) **Patent No.:** **US D887,556 S**

(45) **Date of Patent:** **\*\* Jun. 16, 2020**

(54) **AUXILIARY DEVICE**

(71) Applicant: **Oticon A/S**, Smørum (DK)

(72) Inventor: **Christian Lockenwitz**, København (DK)

(73) Assignee: **OTICON A/S**, Smørum (DK)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/638,539**

(22) Filed: **Feb. 27, 2018**

(30) **Foreign Application Priority Data**

Aug. 28, 2017 (EM) ..... 004168797-0001

Aug. 28, 2017 (EM) ..... 004168797-0002

(51) **LOC (12) Cl.** ..... **24-99**

(52) **U.S. Cl.**  
USPC ..... **D24/173**; D14/225

(58) **Field of Classification Search**  
USPC ..... D24/106, 151, 173-175, 186, 200, 231;  
D14/205, 206, 223, 224, 225, 226, 249,  
D14/216, 228

CPC .. H04R 2225/025; H04R 25/60; H04R 25/63;  
H04R 25/67; H04R 25/602; H04R  
25/604; H04R 25/608; H04R 25/65;  
H04R 25/652; H04R 1/105; H04R 1/75  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D300,852 S \* 4/1989 Sunderland ..... D24/174  
D380,048 S \* 6/1997 Hampf ..... D24/174  
D567,379 S \* 4/2008 Svensson ..... D24/174  
D627,069 S \* 11/2010 Mehlsen ..... D24/174

D656,924 S \* 4/2012 Mehlsen ..... D14/226  
D681,213 S \* 4/2013 Solby ..... D24/174  
D712,885 S \* 9/2014 James ..... D14/225  
D720,461 S \* 12/2014 Svensson ..... D24/174  
D753,091 S \* 4/2016 Miyake ..... D14/205  
D762,858 S \* 8/2016 Iwabuchi ..... D24/174  
D839,242 S \* 1/2019 Pang ..... D14/223  
D848,876 S \* 5/2019 Lee ..... D24/186

**OTHER PUBLICATIONS**

Hearingaidsi—New Oticon ConnectClip Streamer & Remote Micro-  
phone for Hearing aid—Date not available.\*

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Birch, Stewart, Kolasch  
& Birch, LLP

(57) **CLAIM**


The ornamental design for an auxiliary device, as shown and  
described.


**DESCRIPTION**

FIG. 1 is a perspective view of the auxiliary device;  
FIG. 2 is another perspective view of the auxiliary device;  
FIG. 3 is a front view of the auxiliary device;  
FIG. 4 is a rear view of the auxiliary device;  
FIG. 5 is a bottom view of the auxiliary device;  
FIG. 6 is a top view of the auxiliary device;  
FIG. 7 is a left side view of the auxiliary device; and,  
FIG. 8 is a right side view of the auxiliary device.


The broken lines showing in the views are for the purpose  
of illustrating portions of the auxiliary device that form no  
part of the claimed design; the broken lines form no part of  
the claimed design.

**1 Claim, 8 Drawing Sheets**

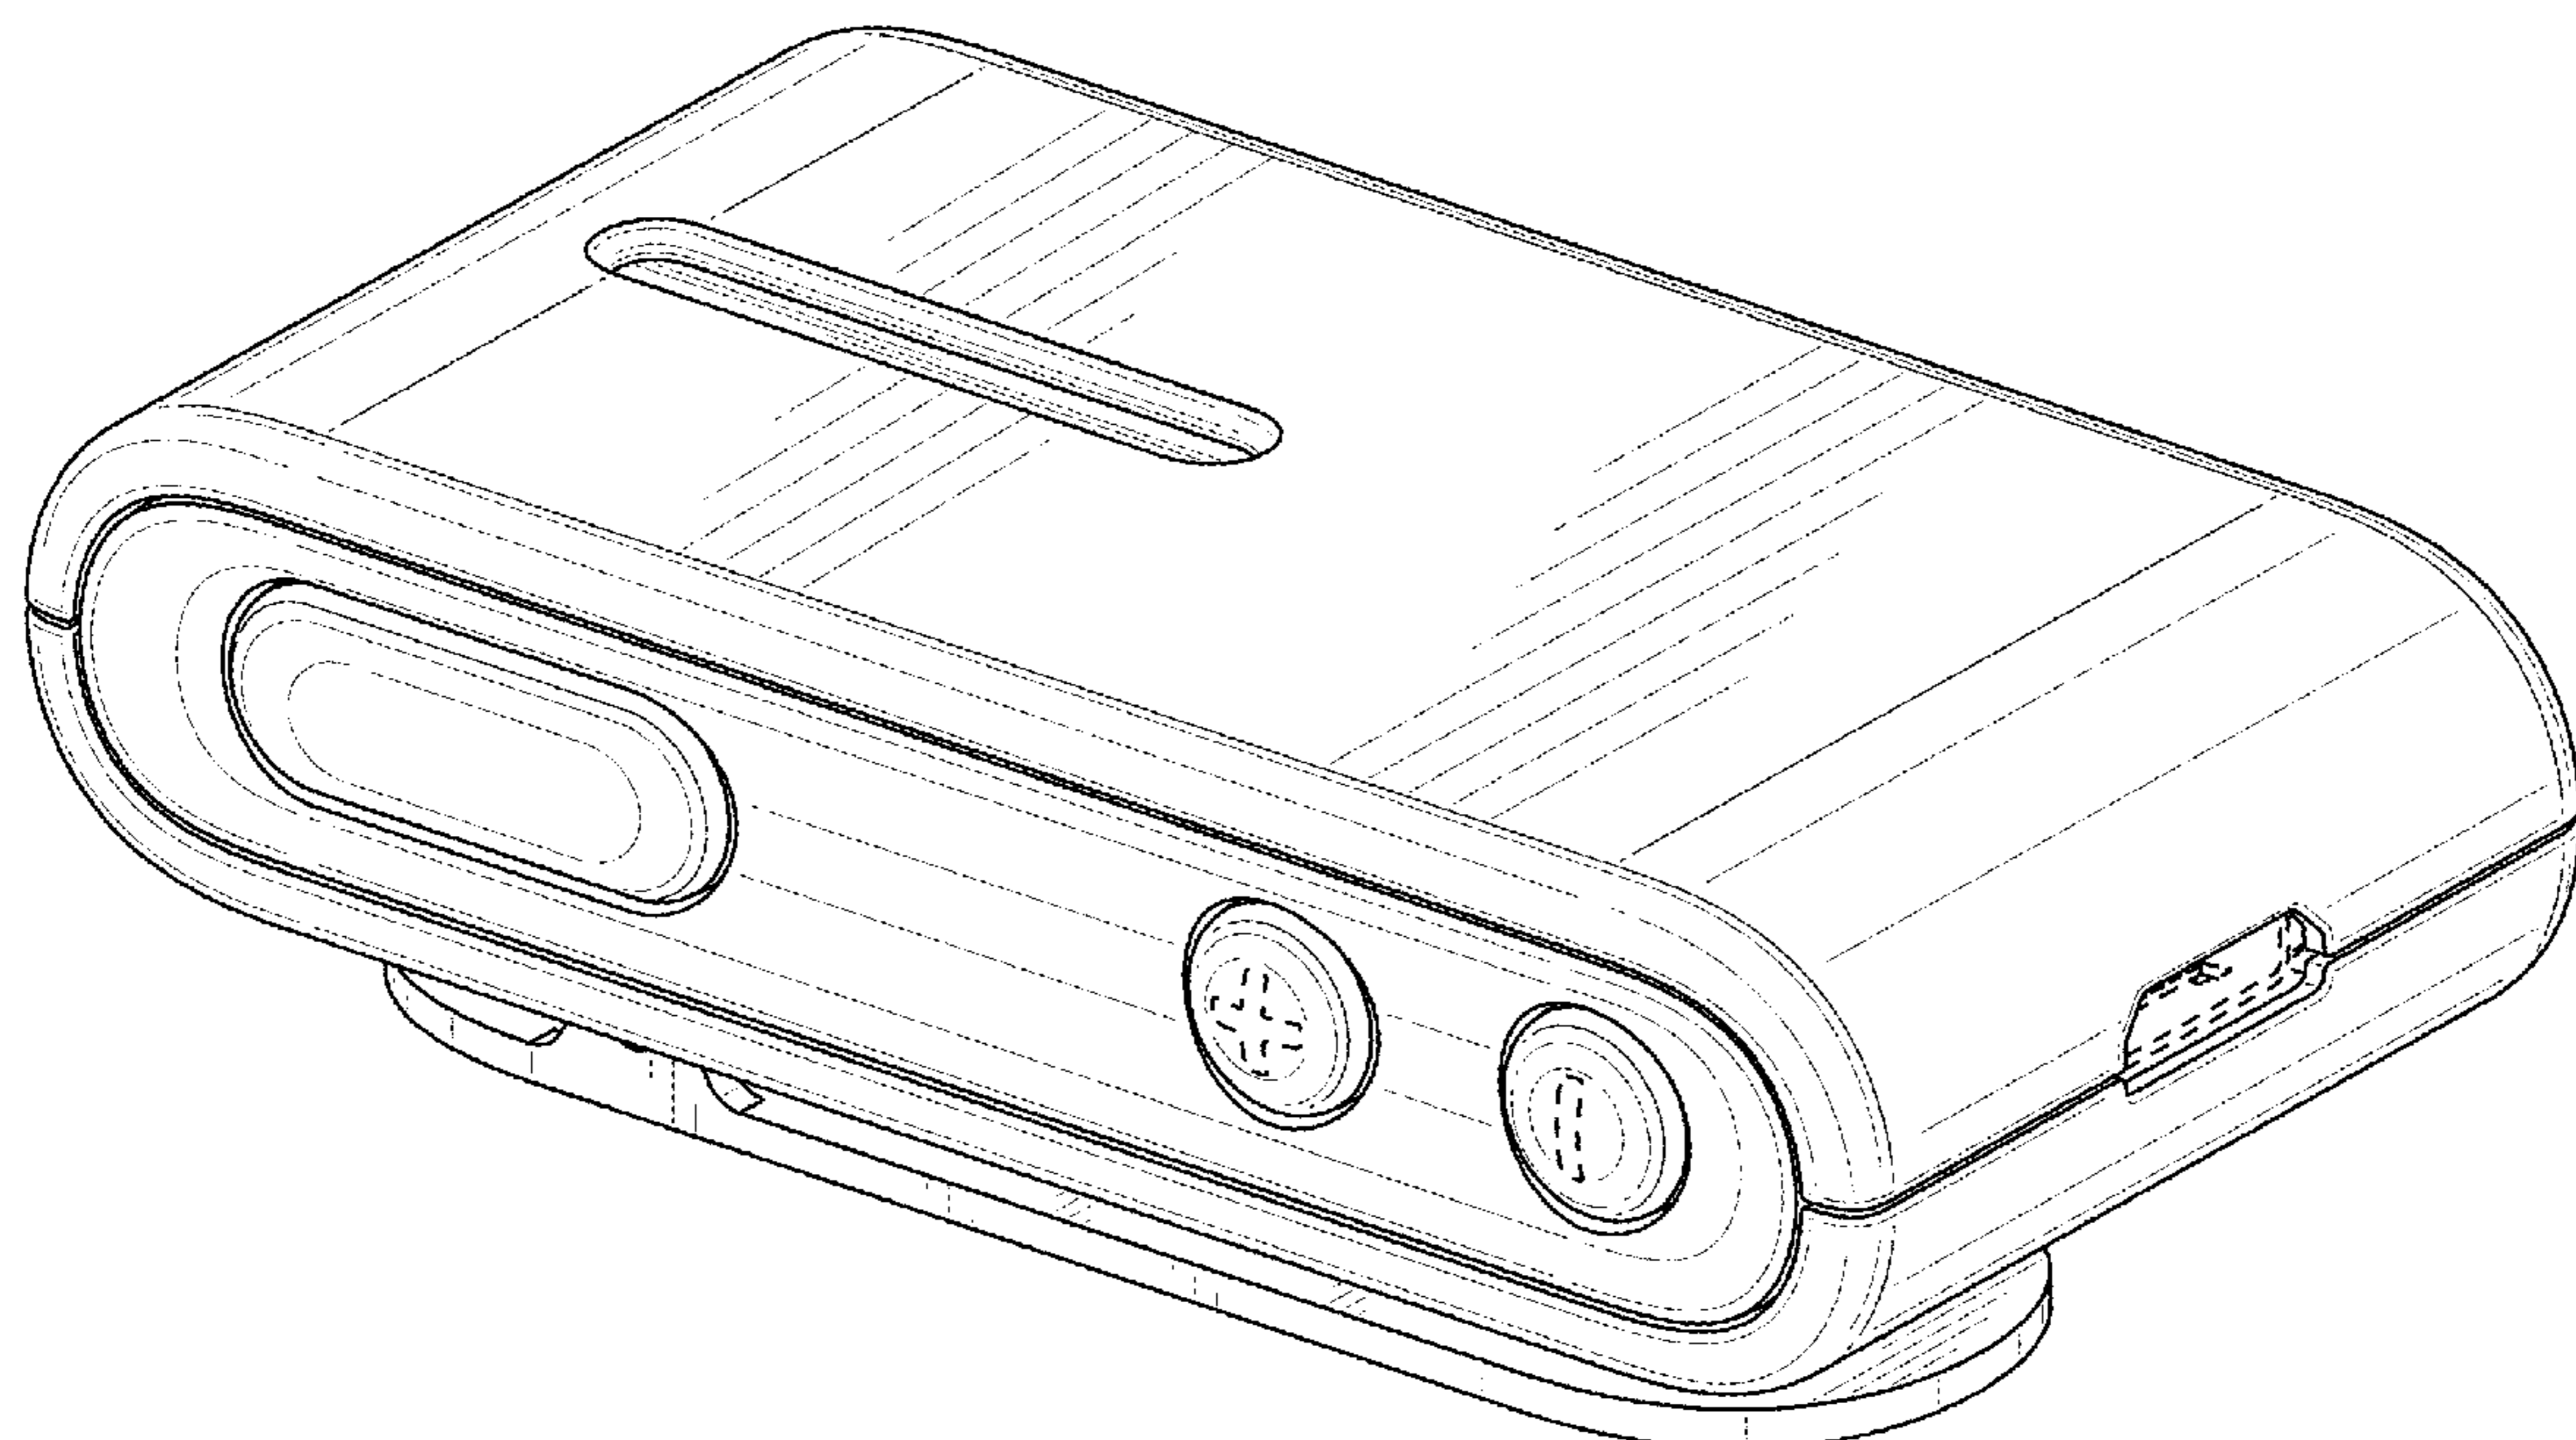


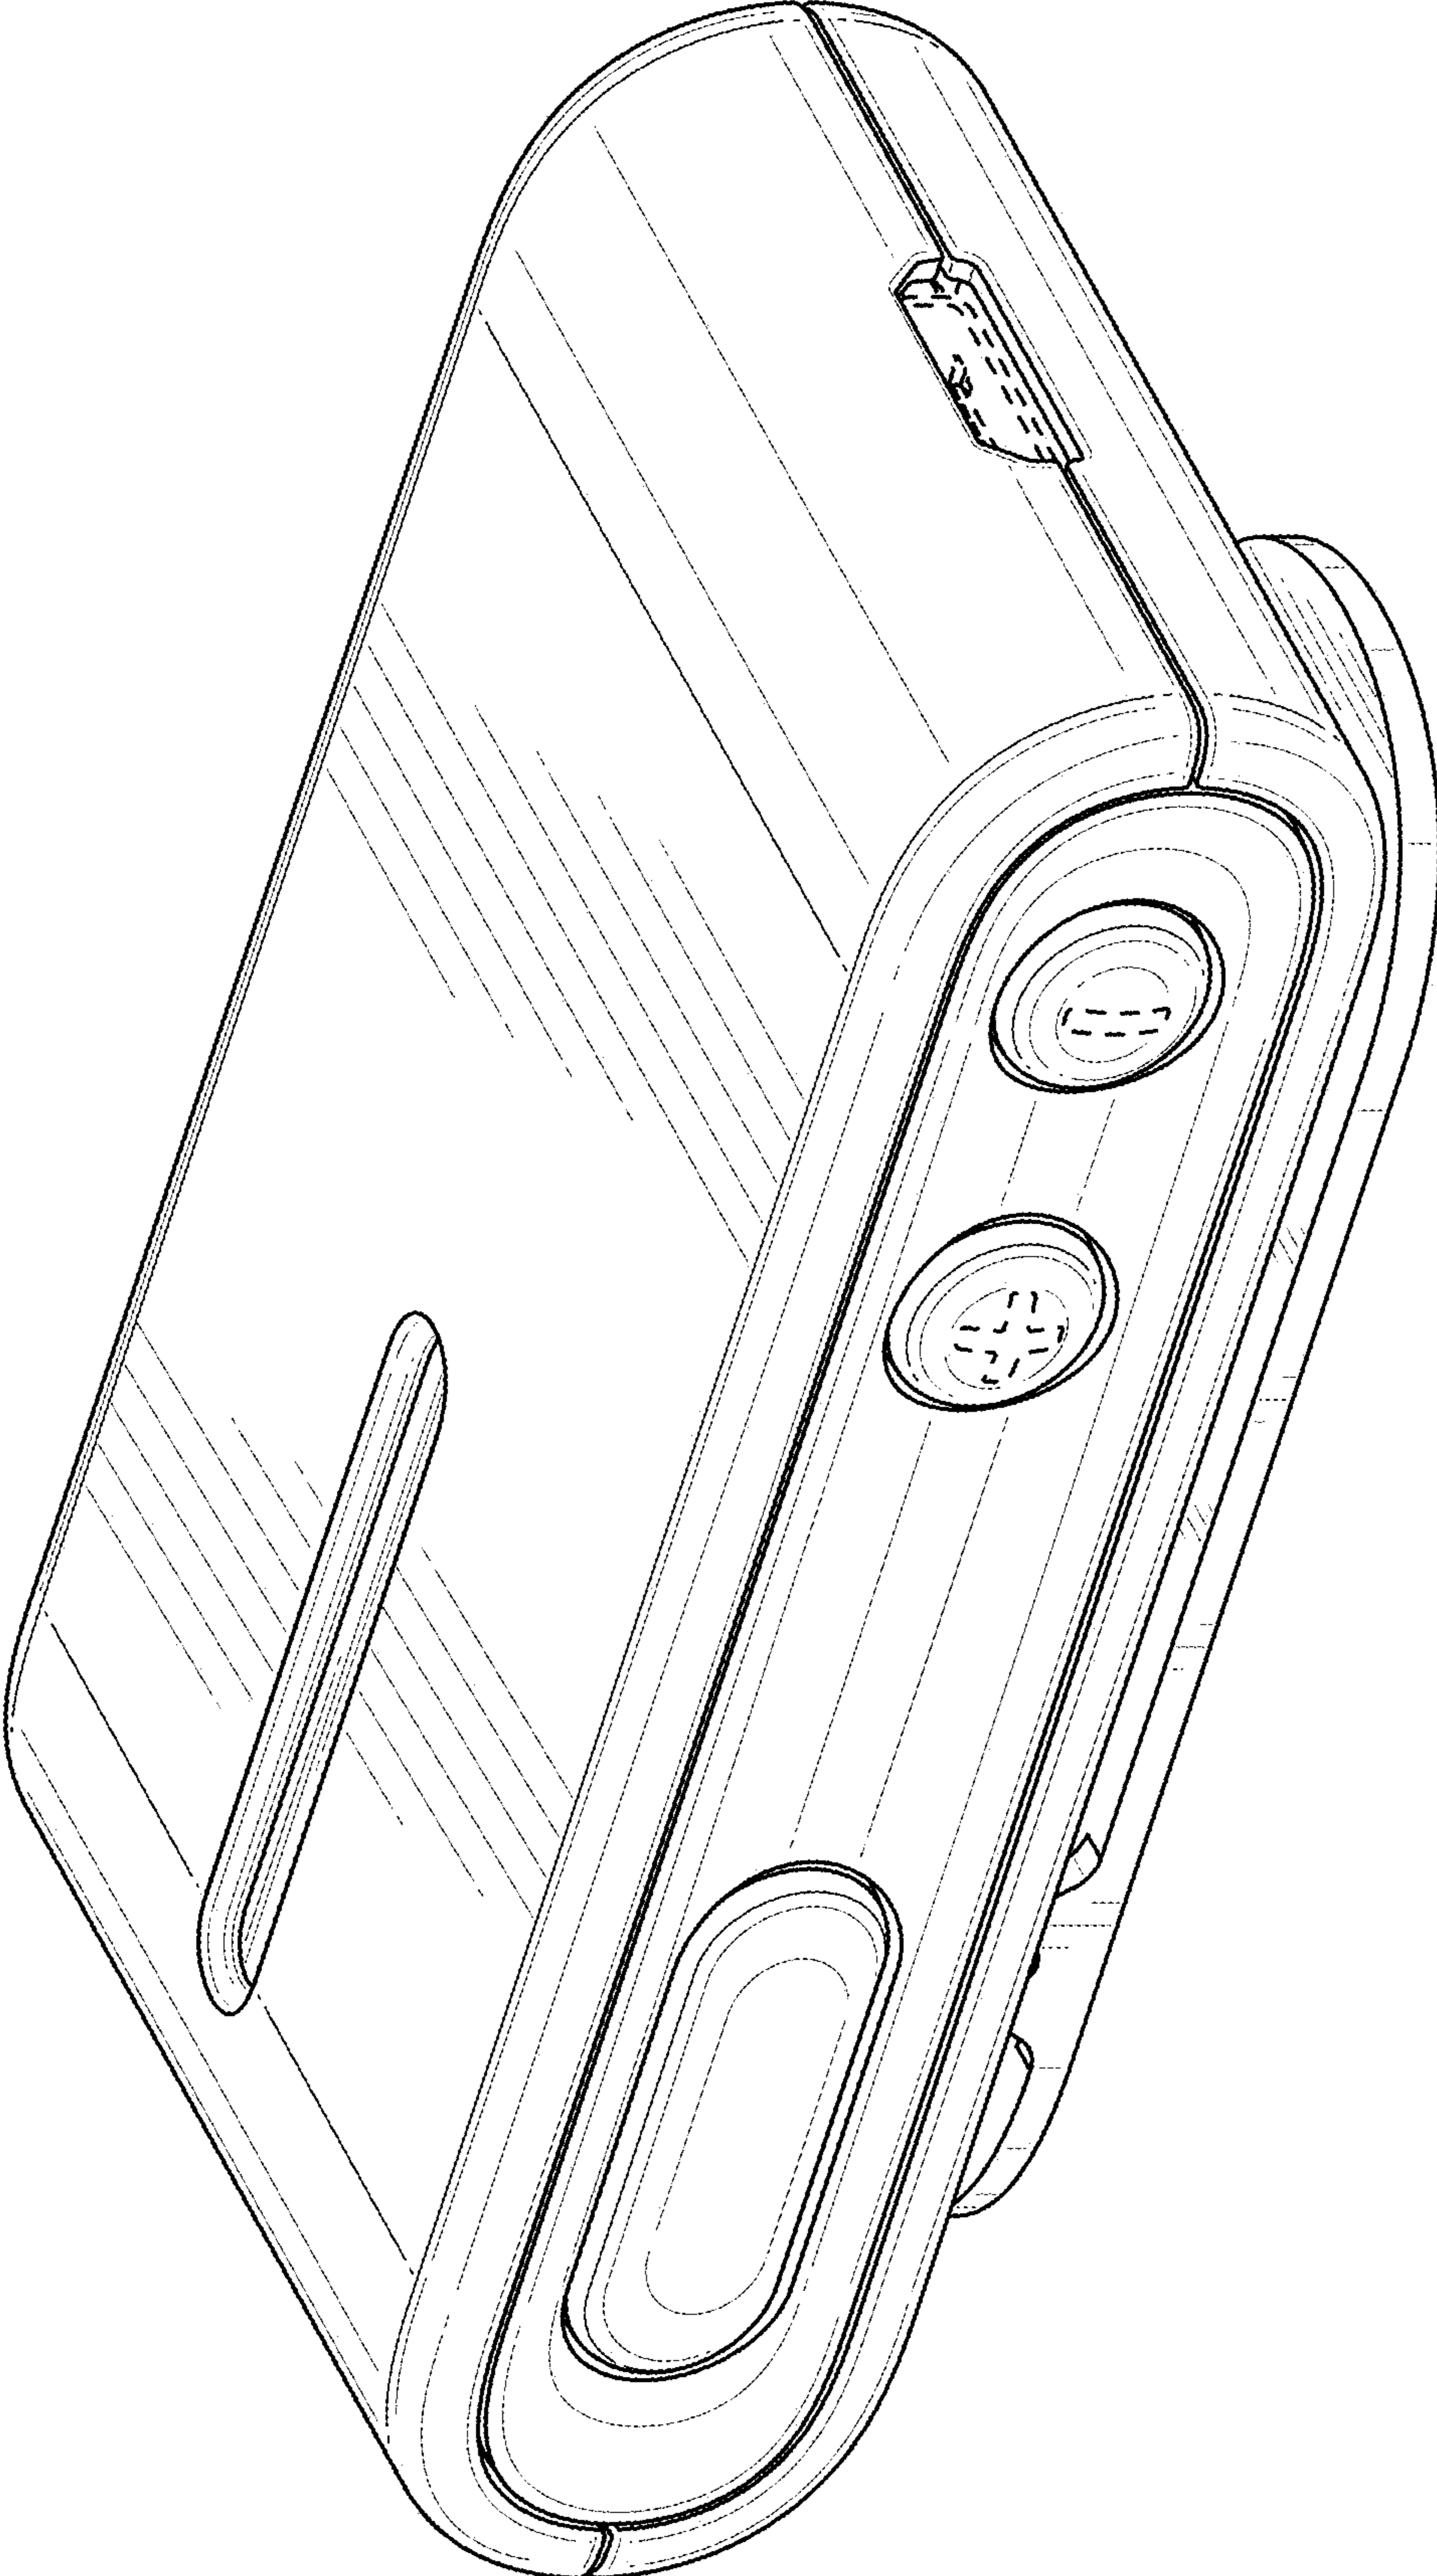


**FIG. 1**

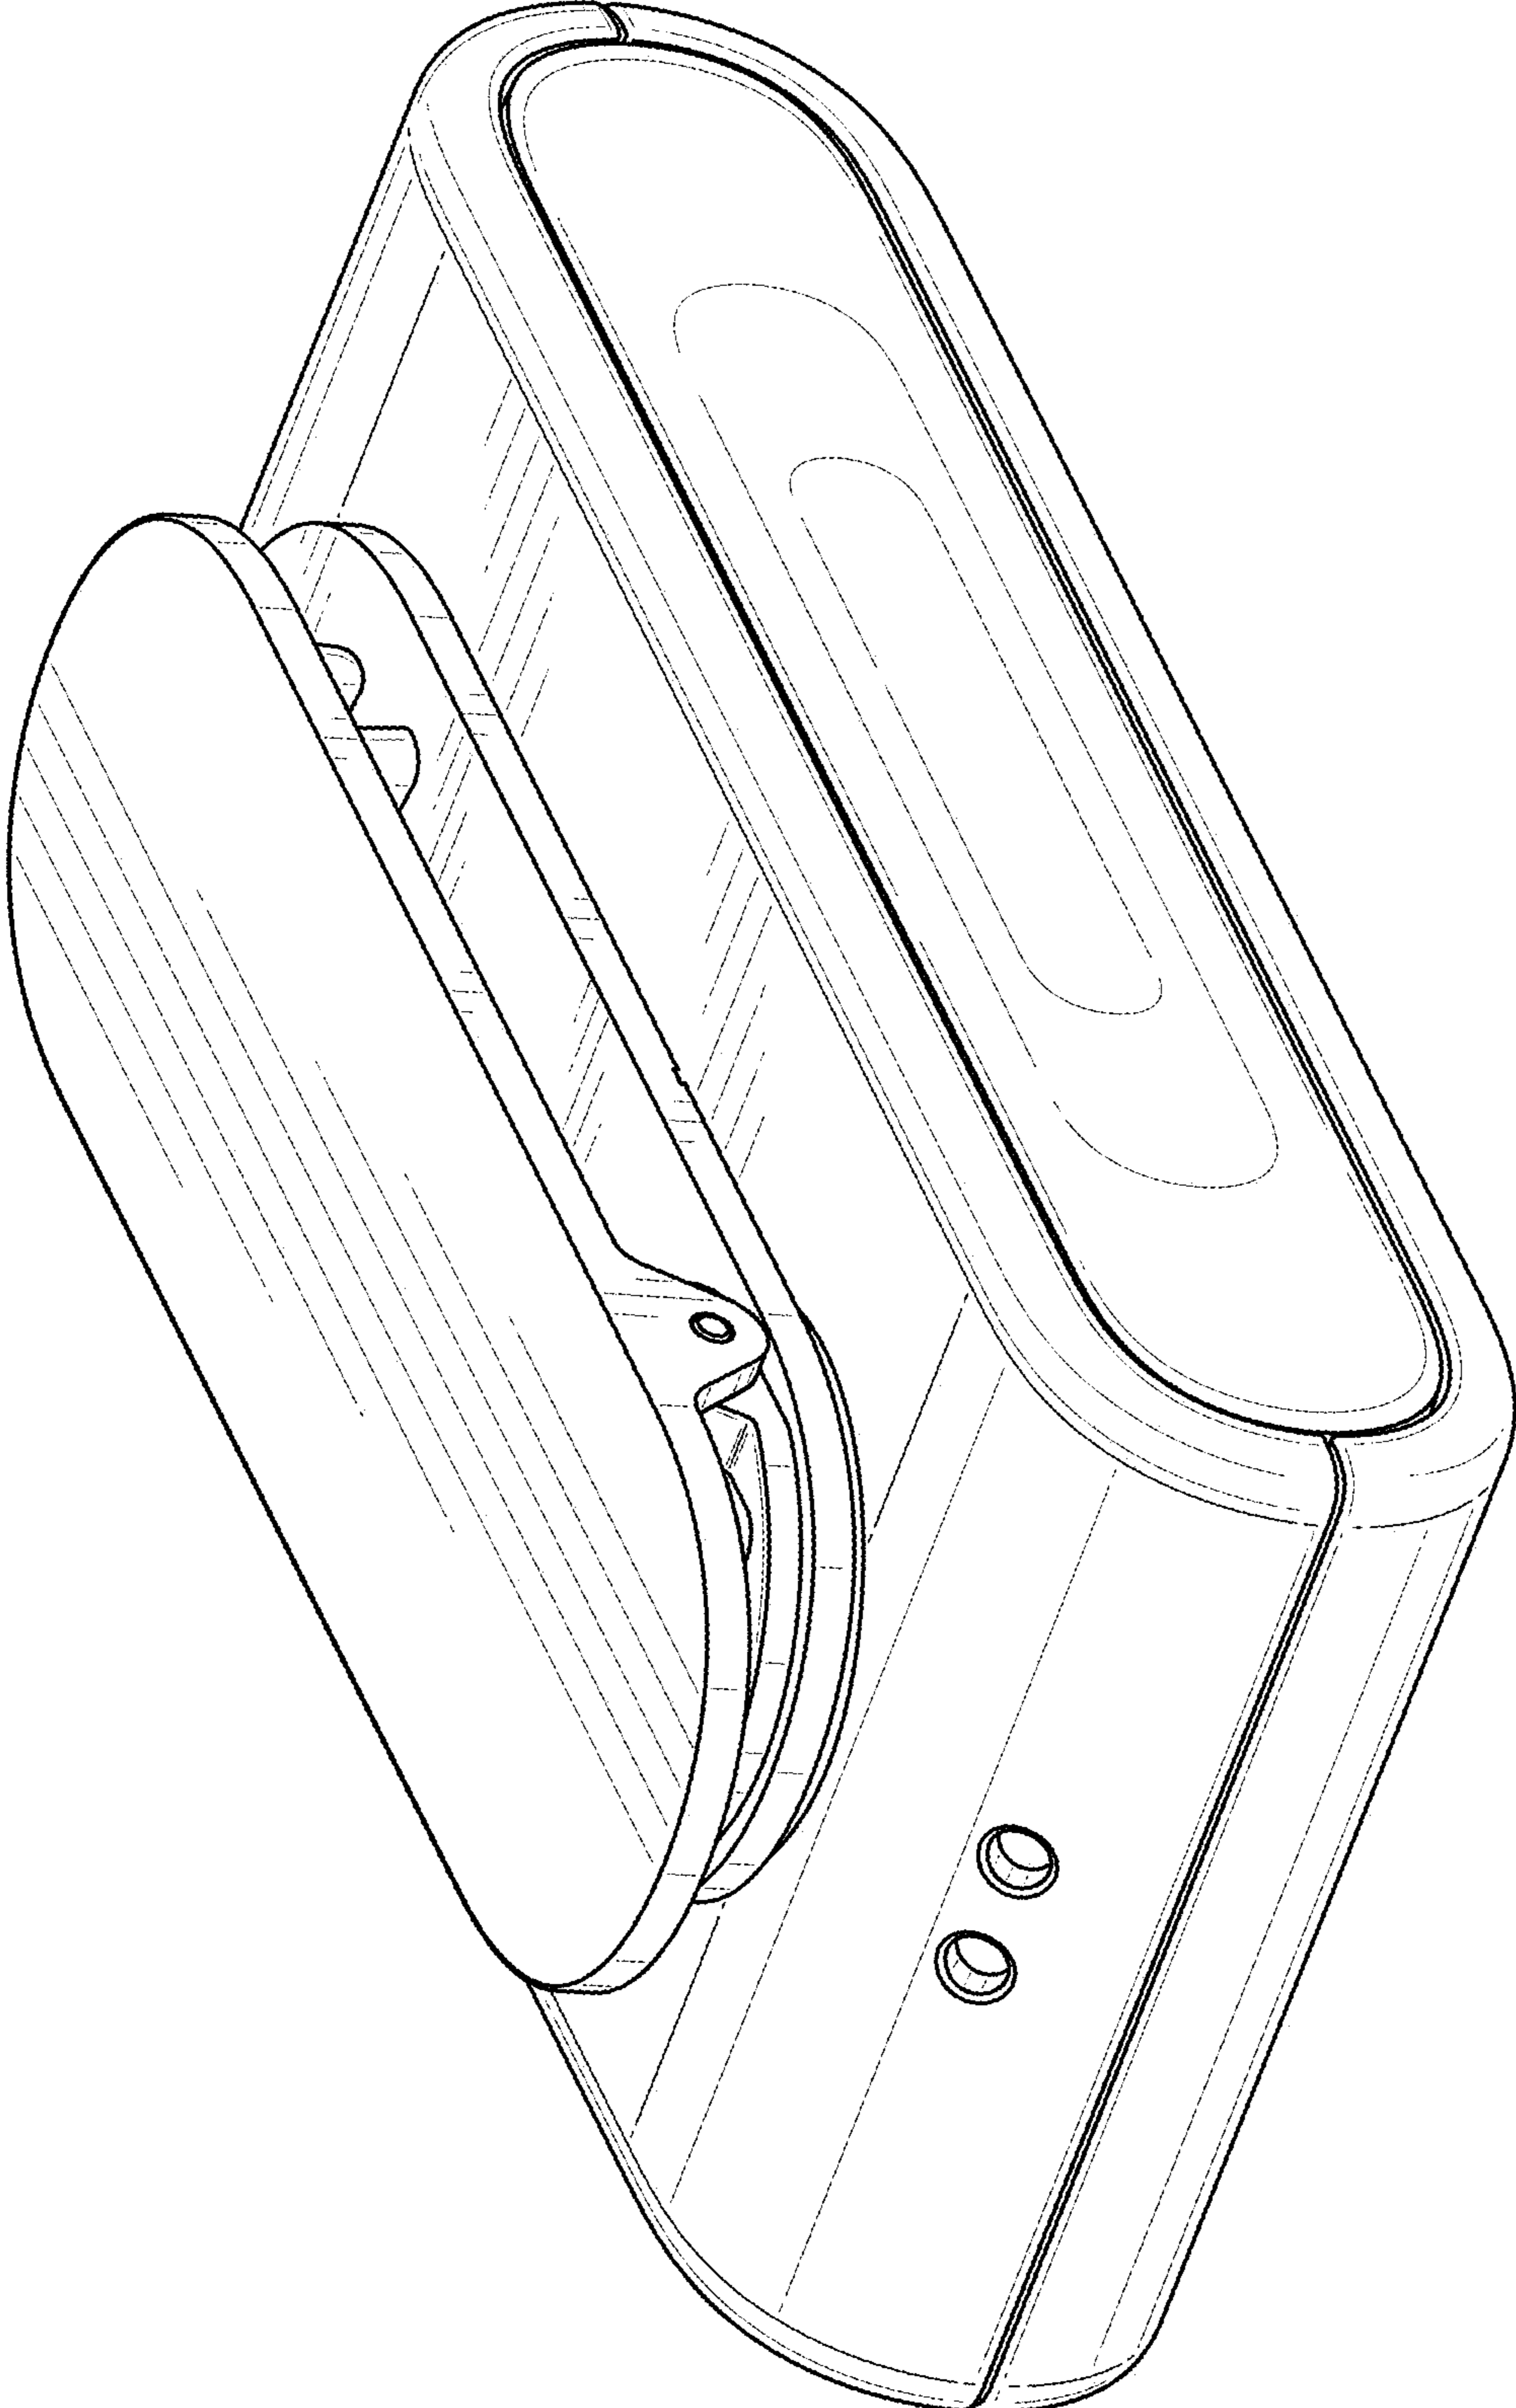


**FIG. 2**

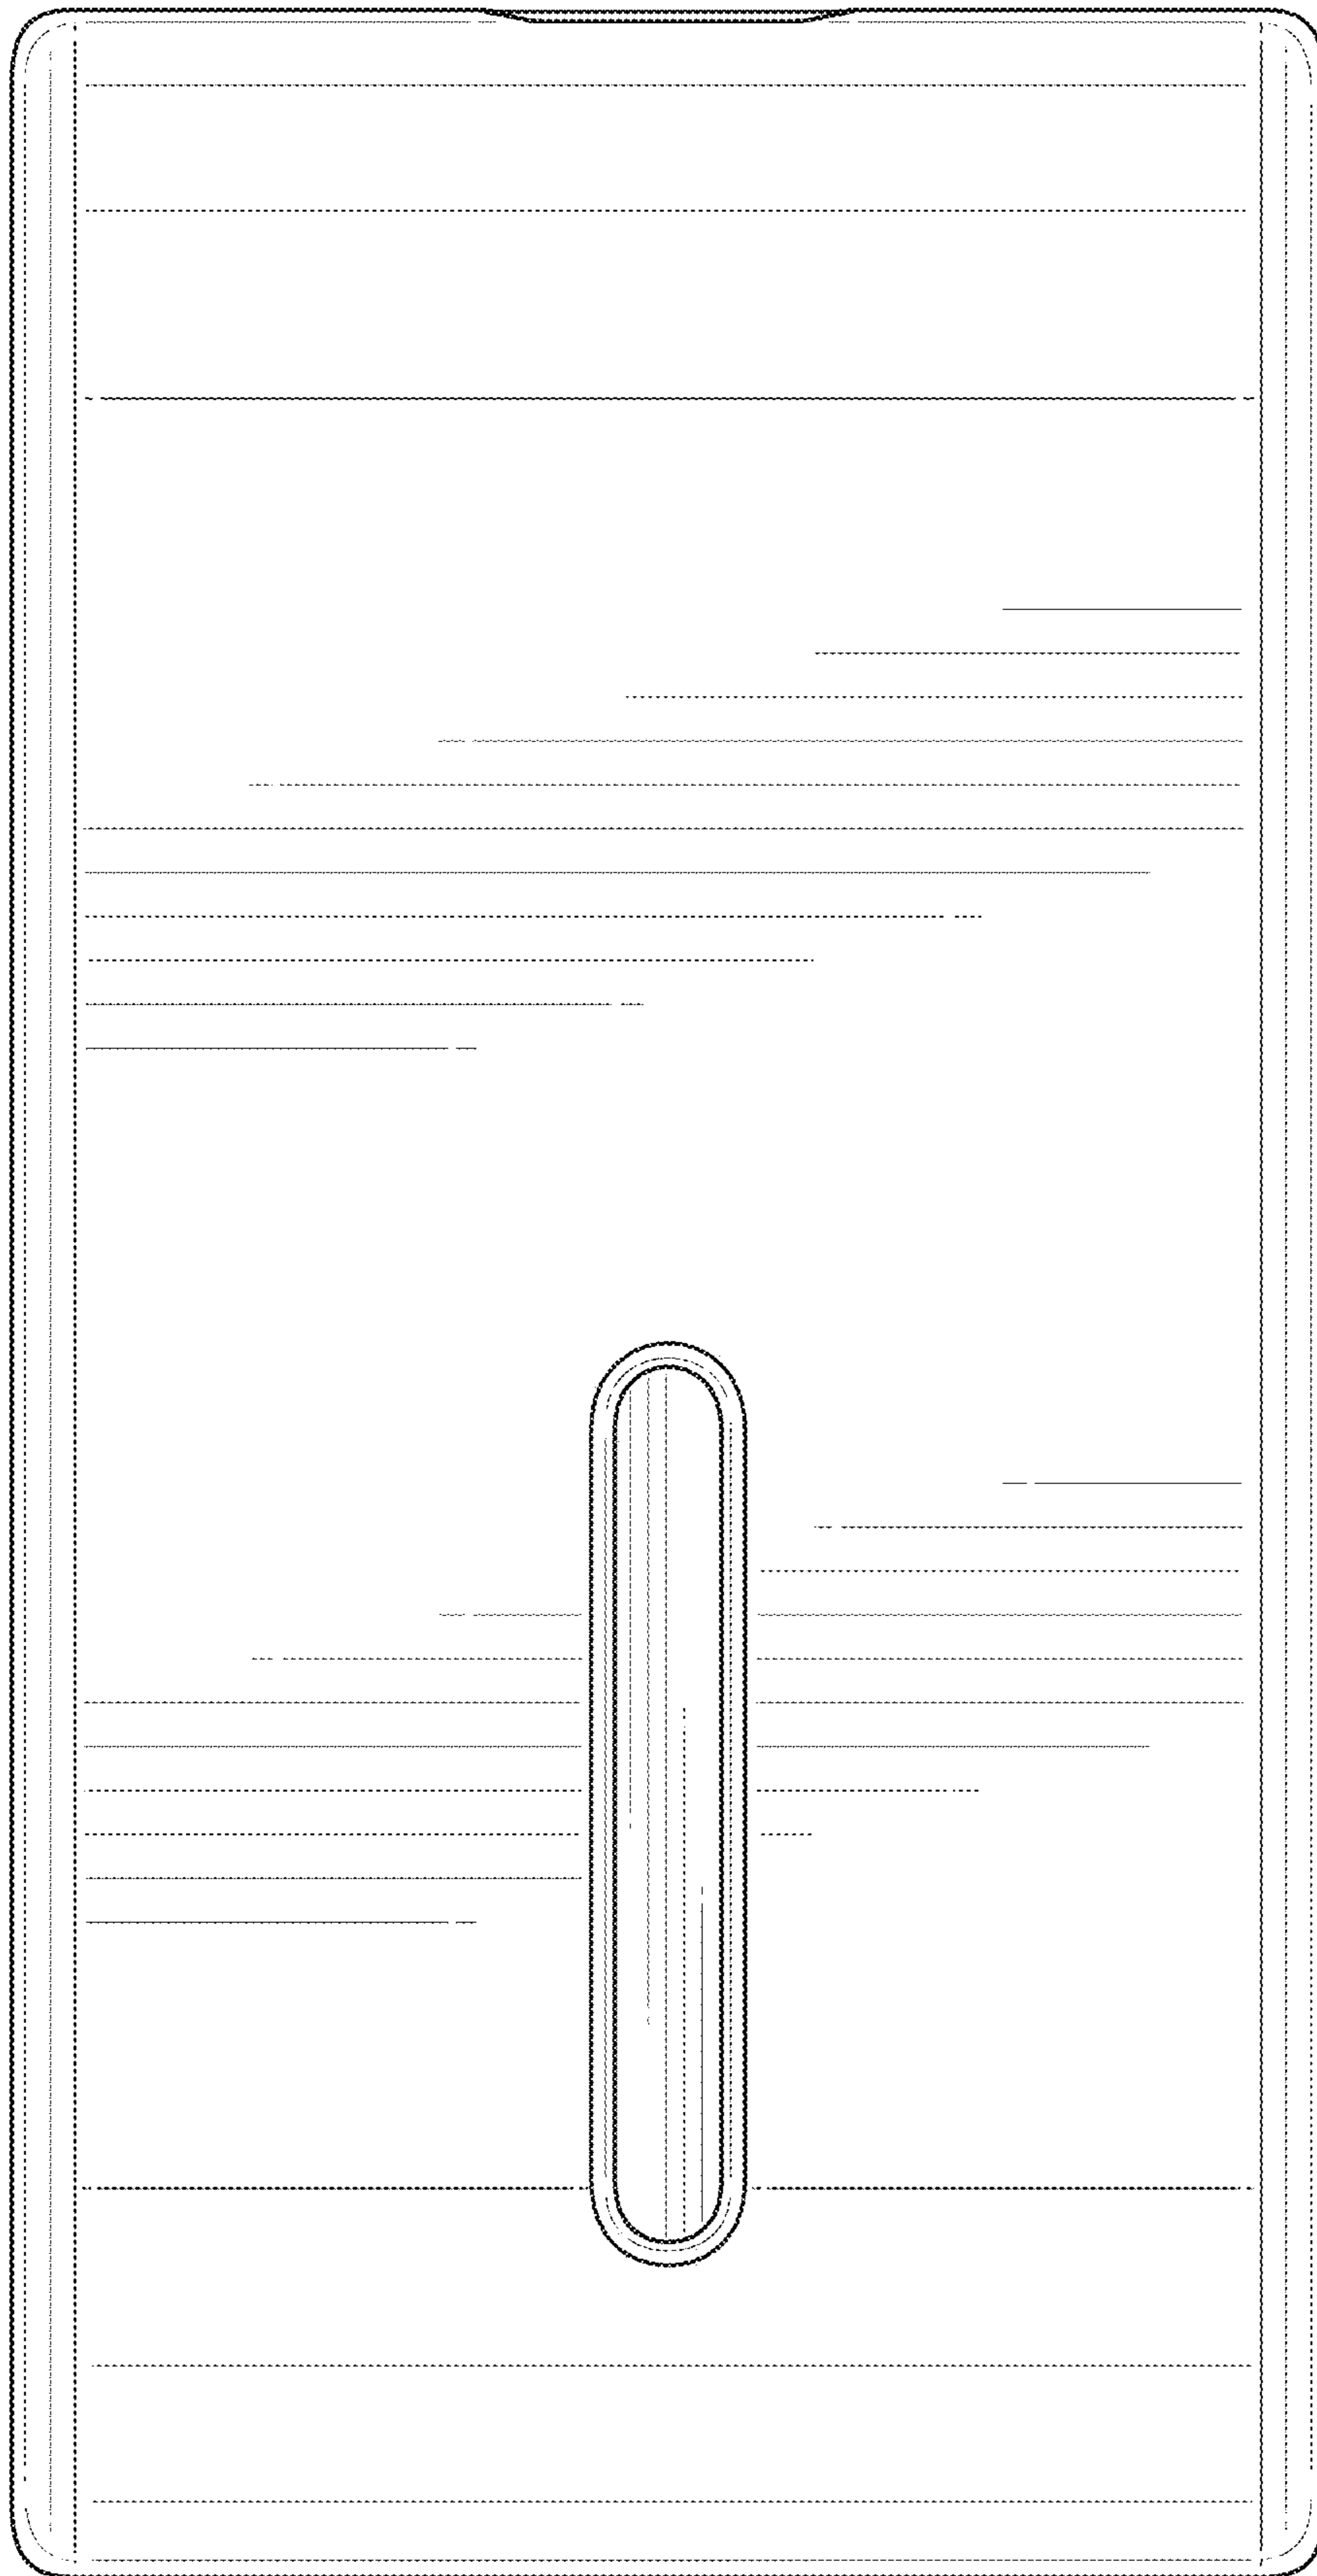


**FIG. 3**

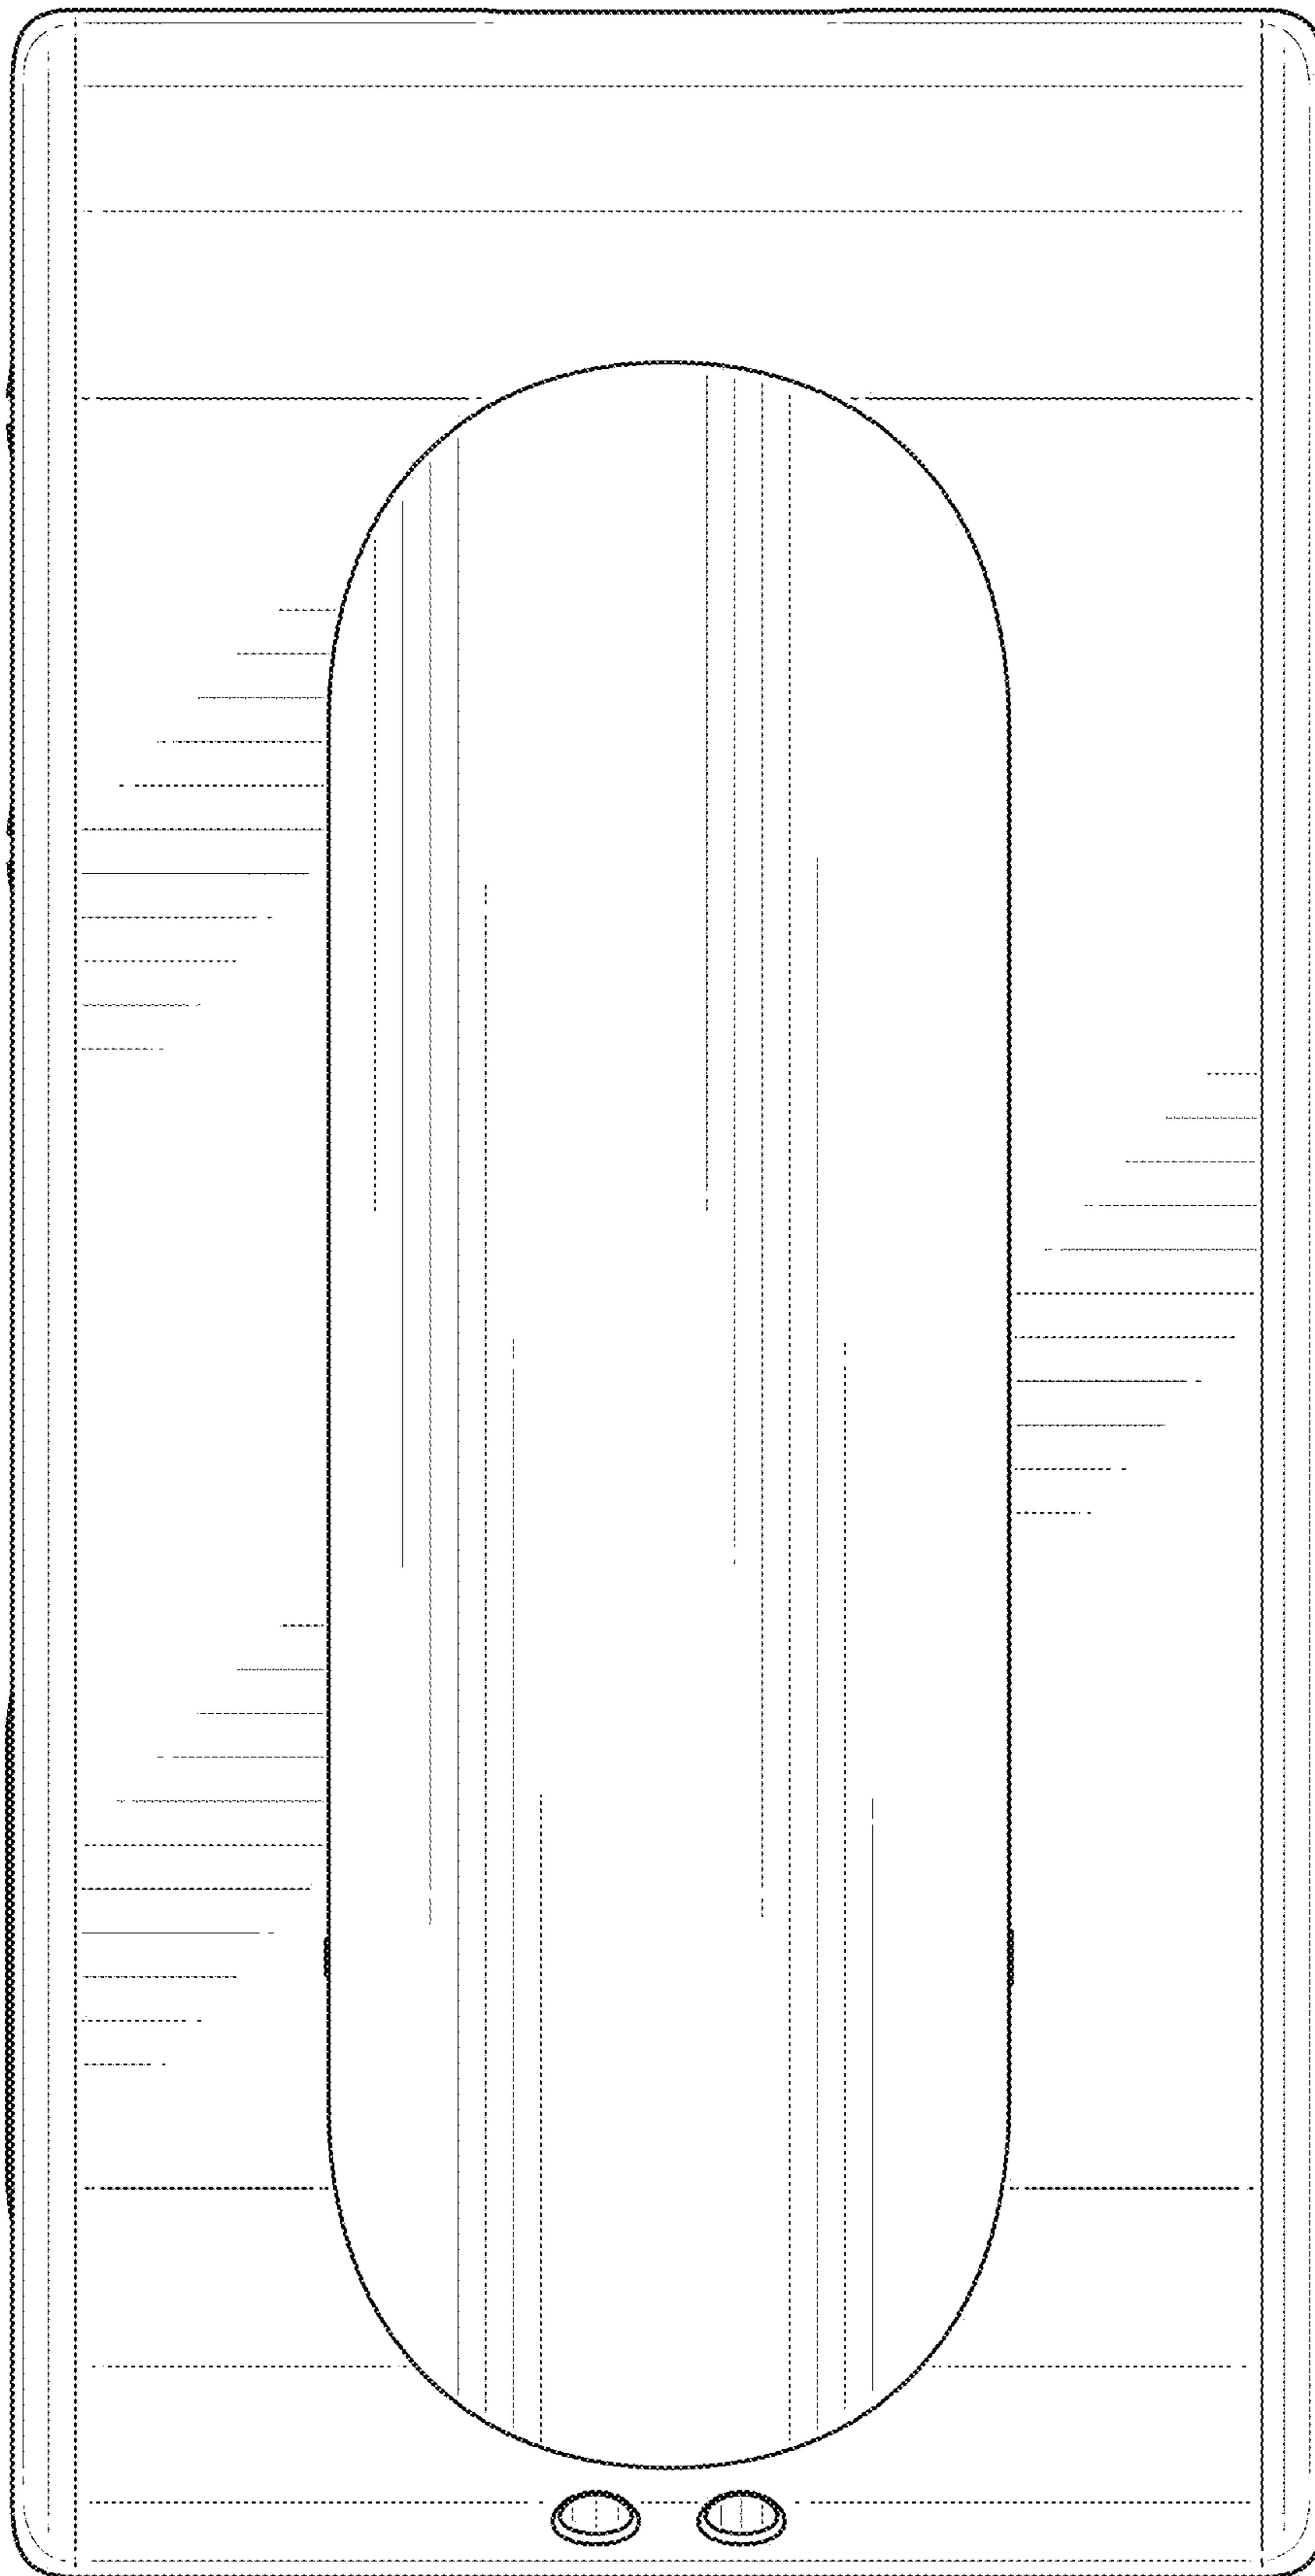

**FIG. 4**

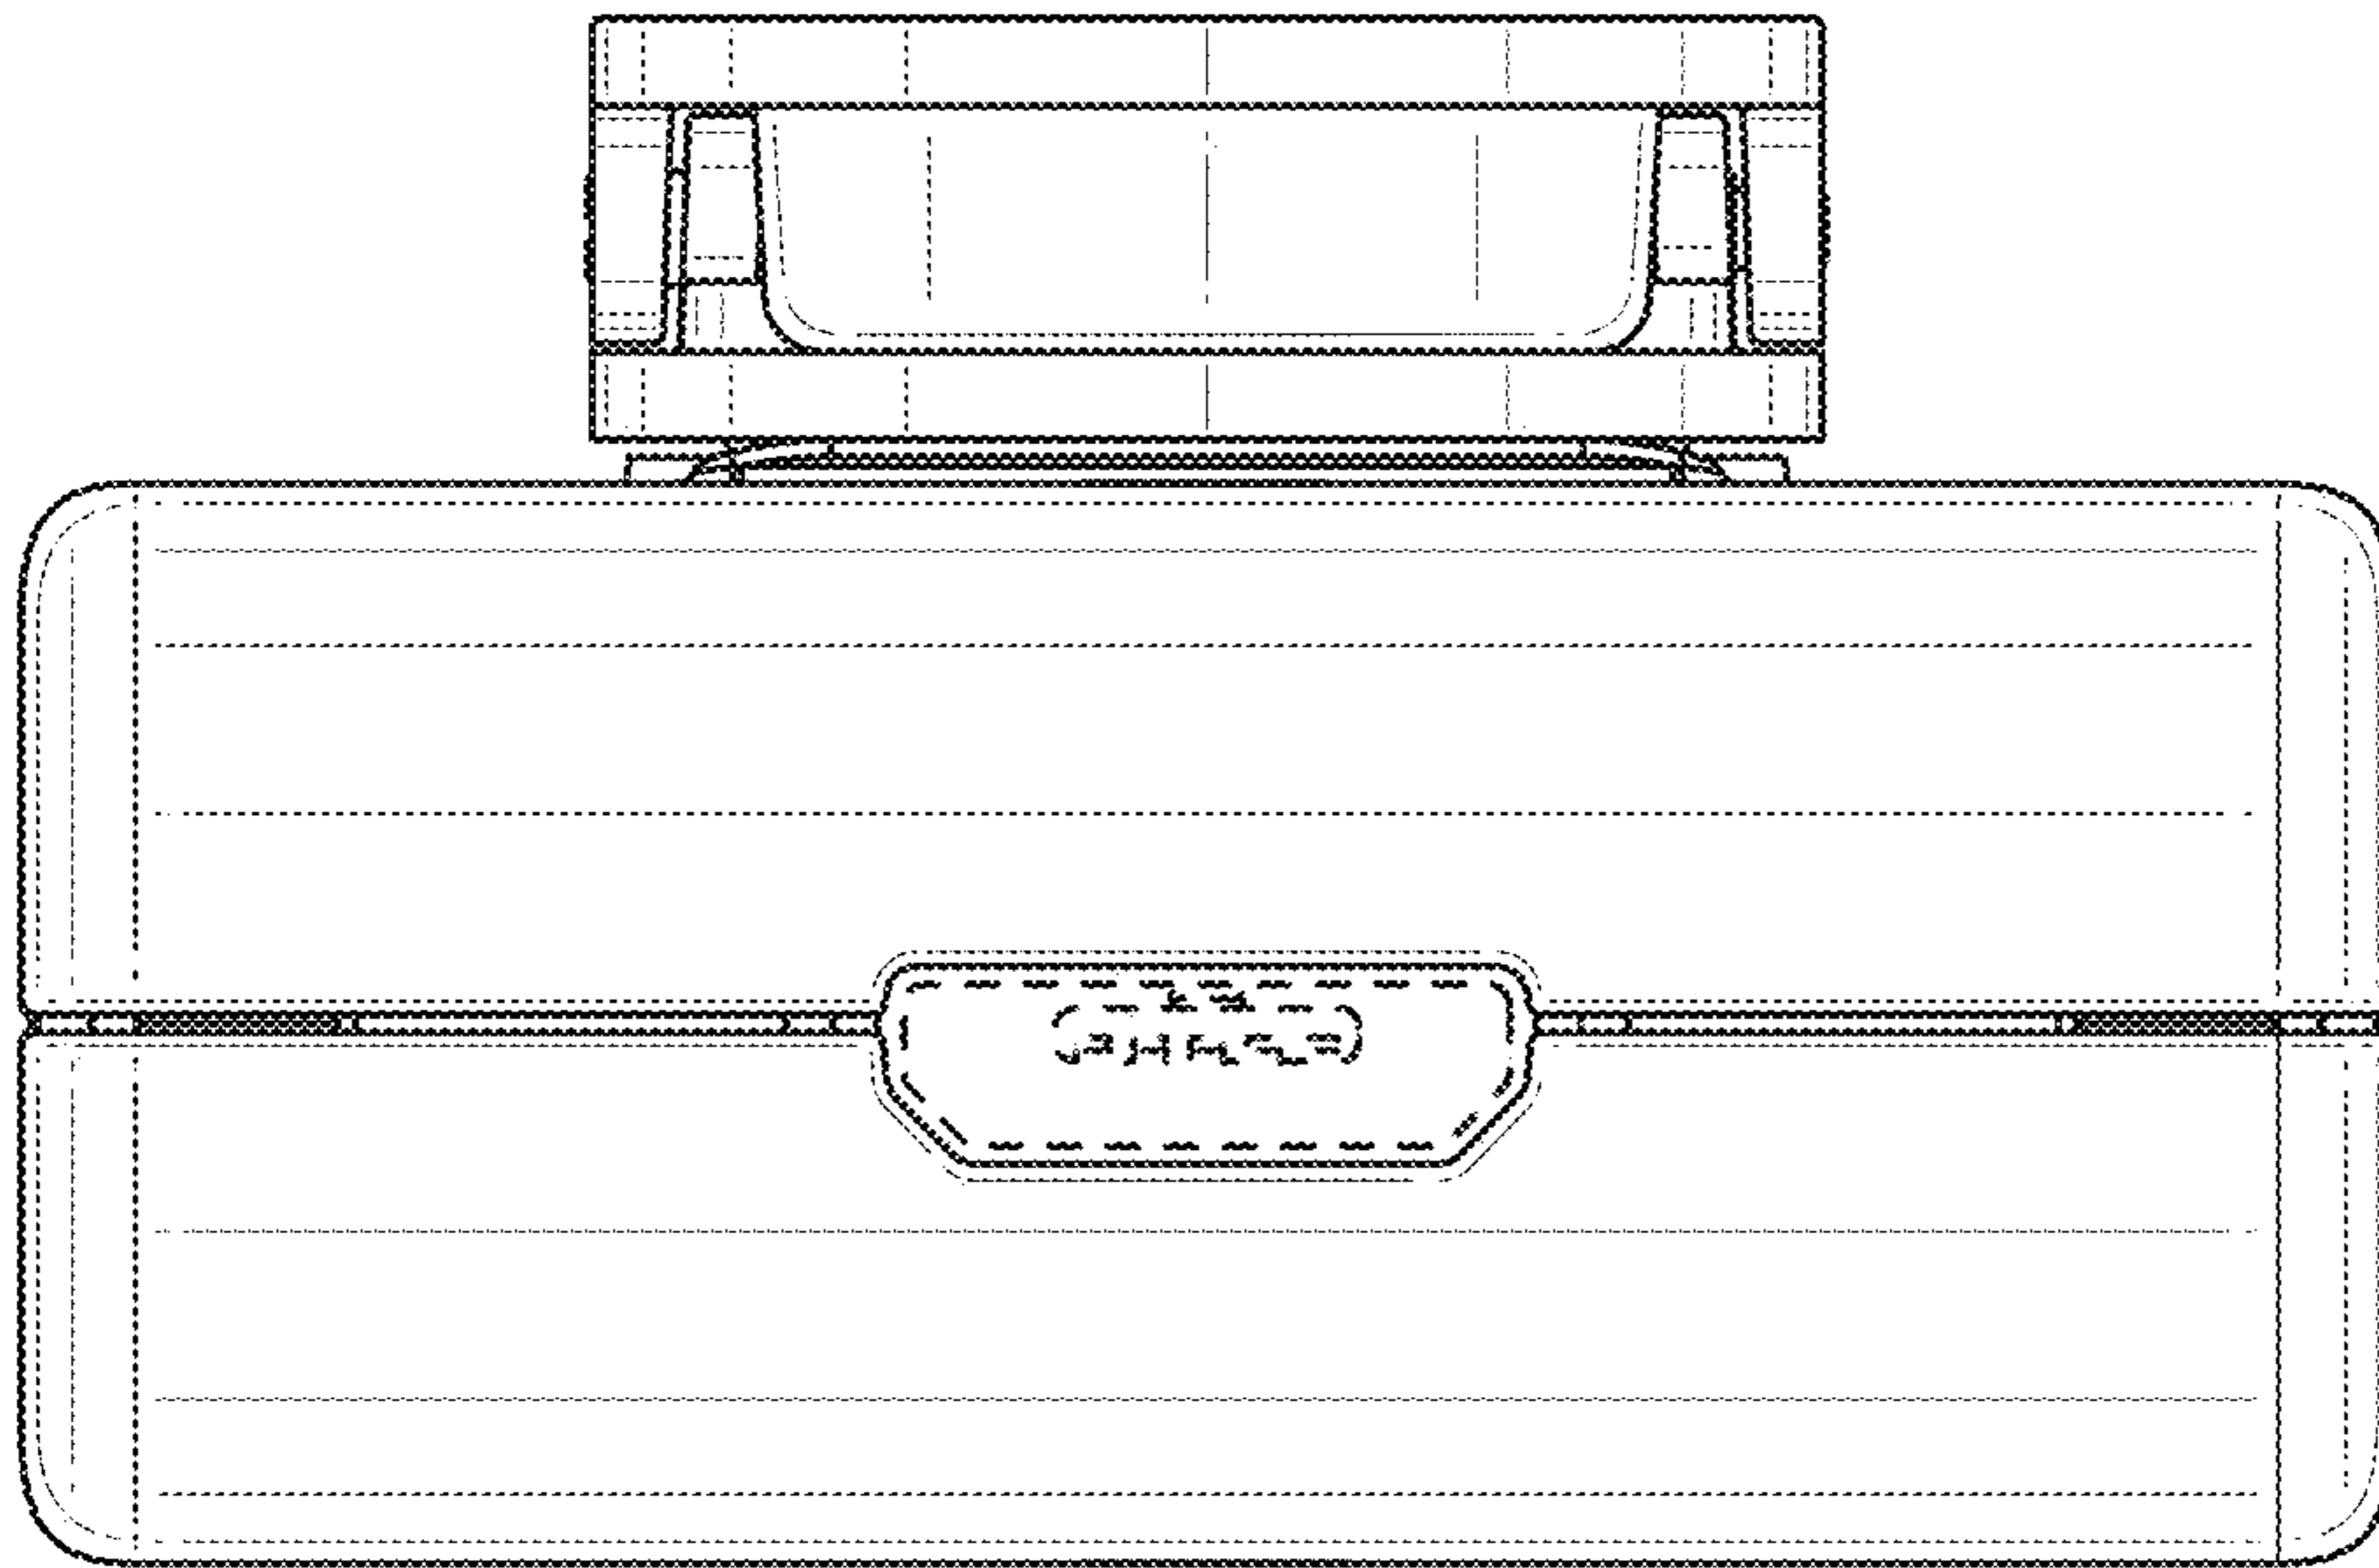

**FIG. 5**

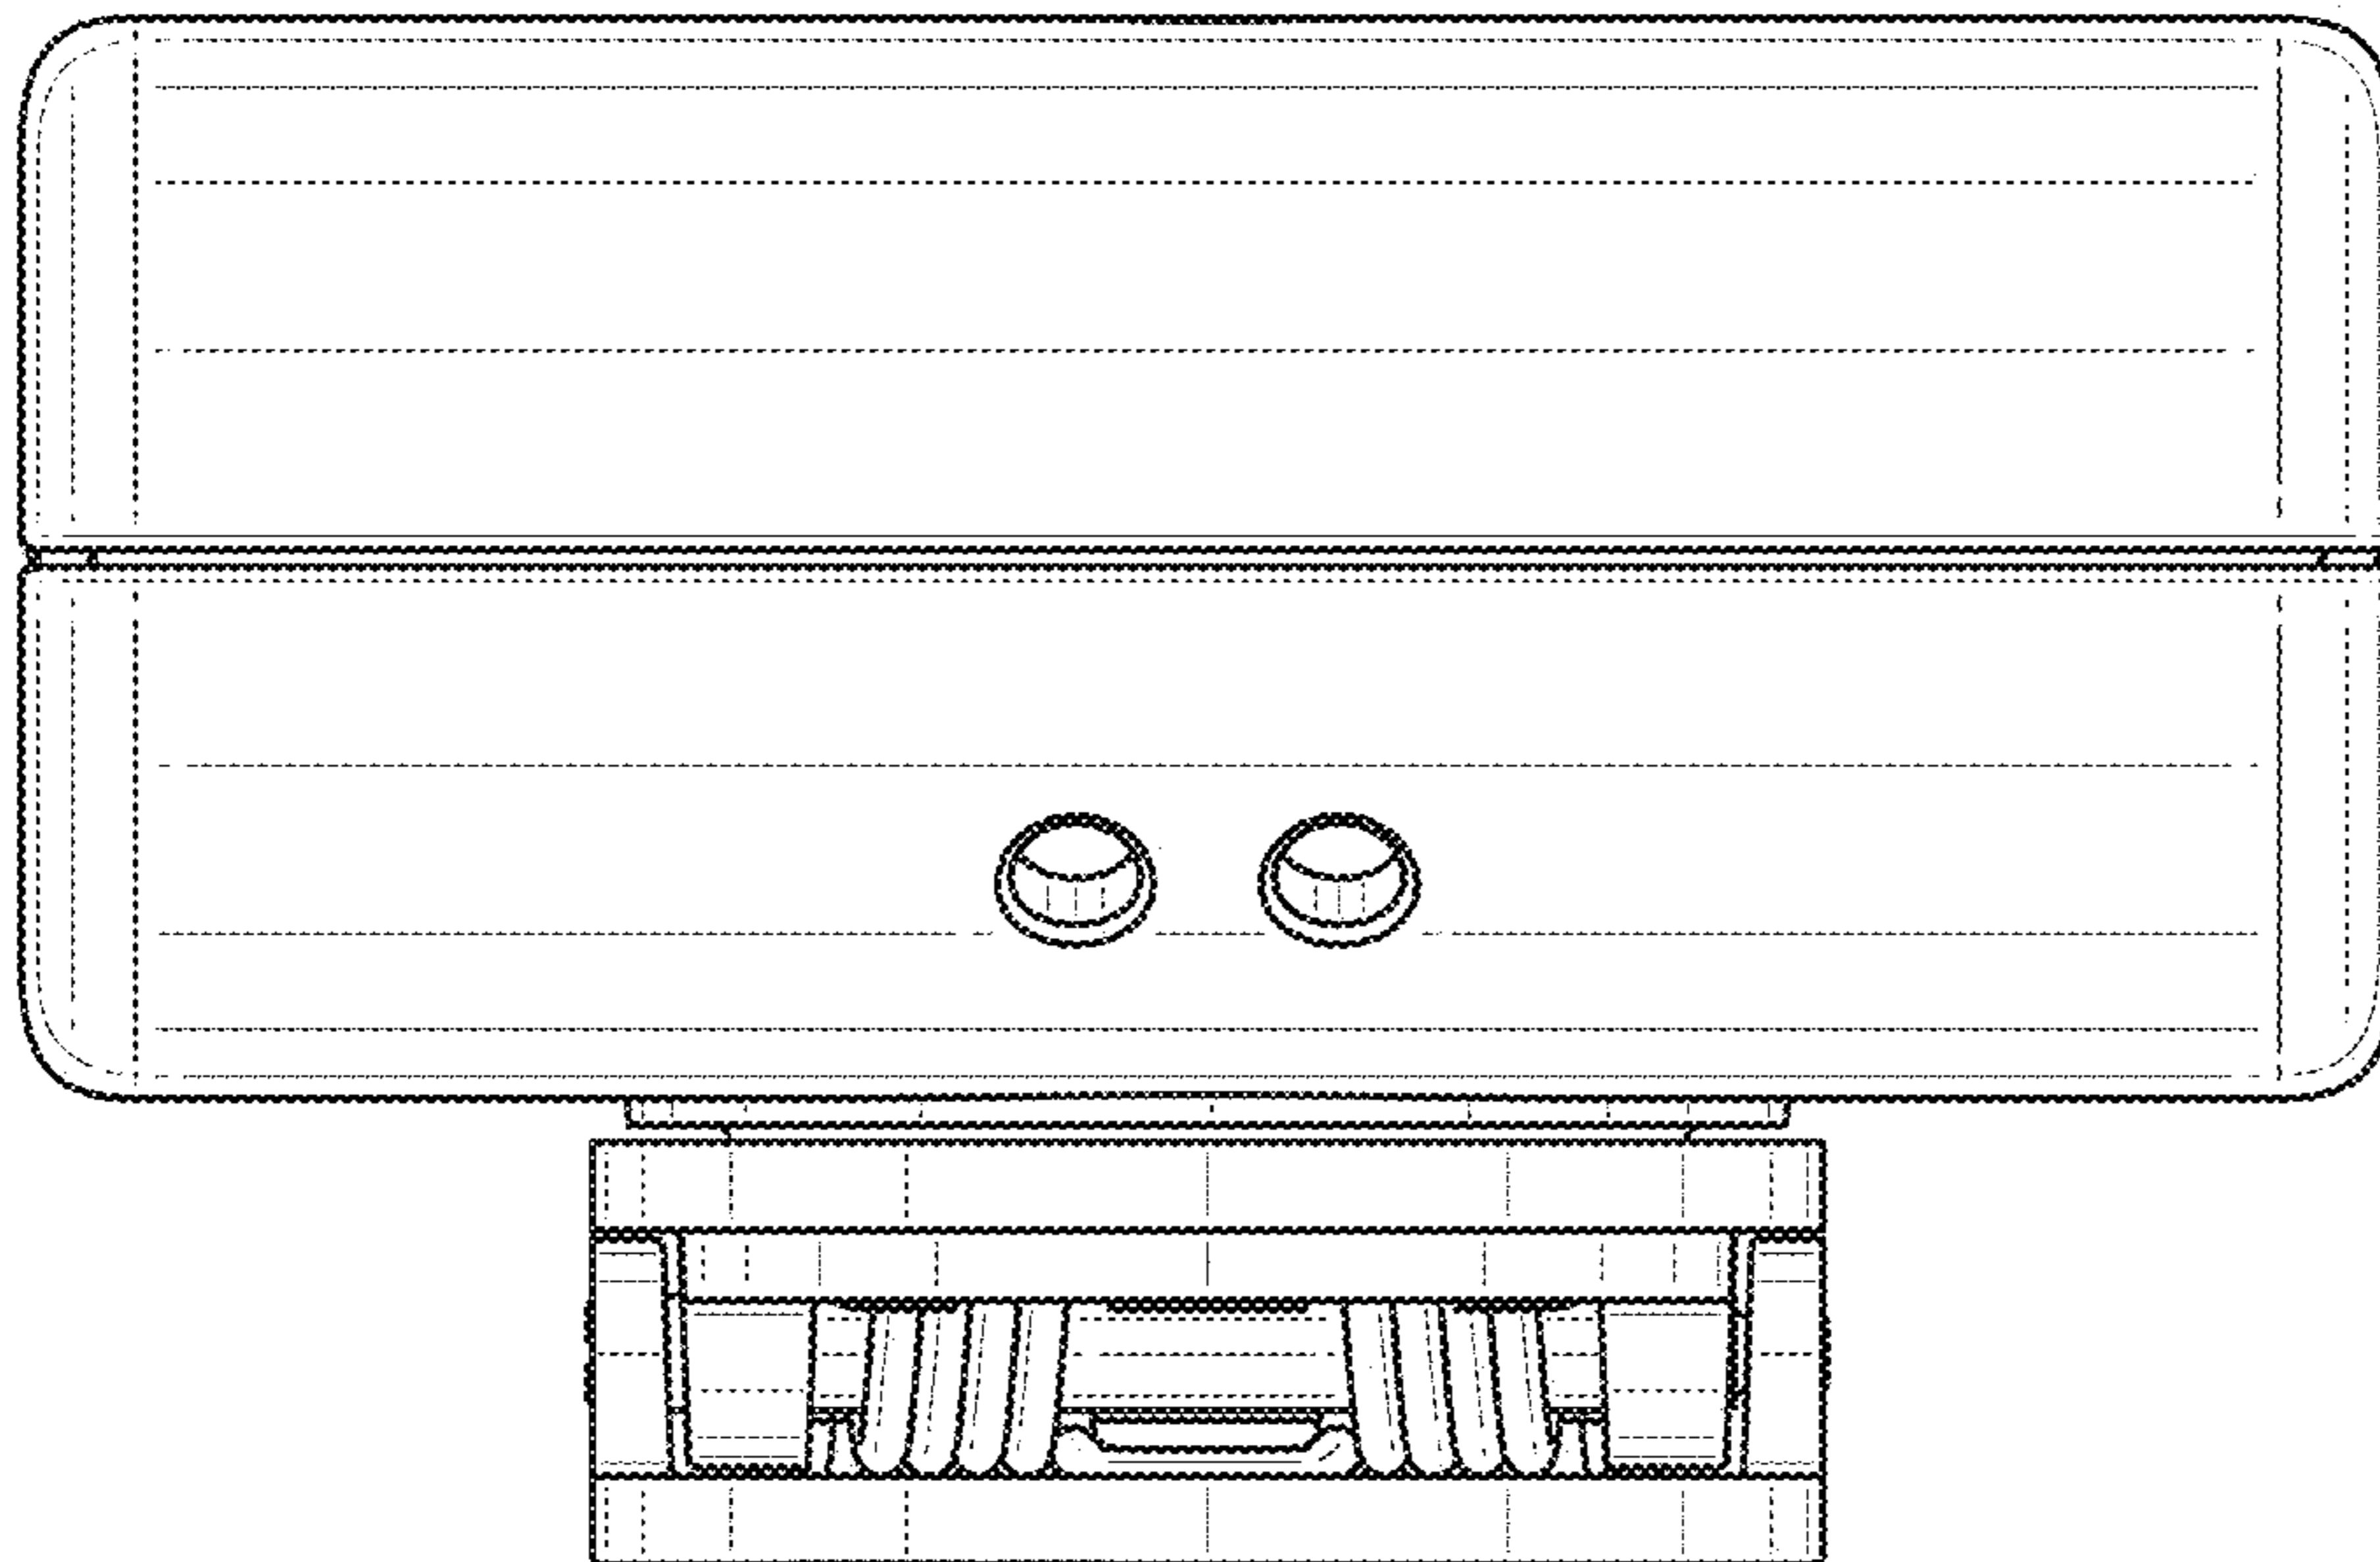

**FIG. 6**


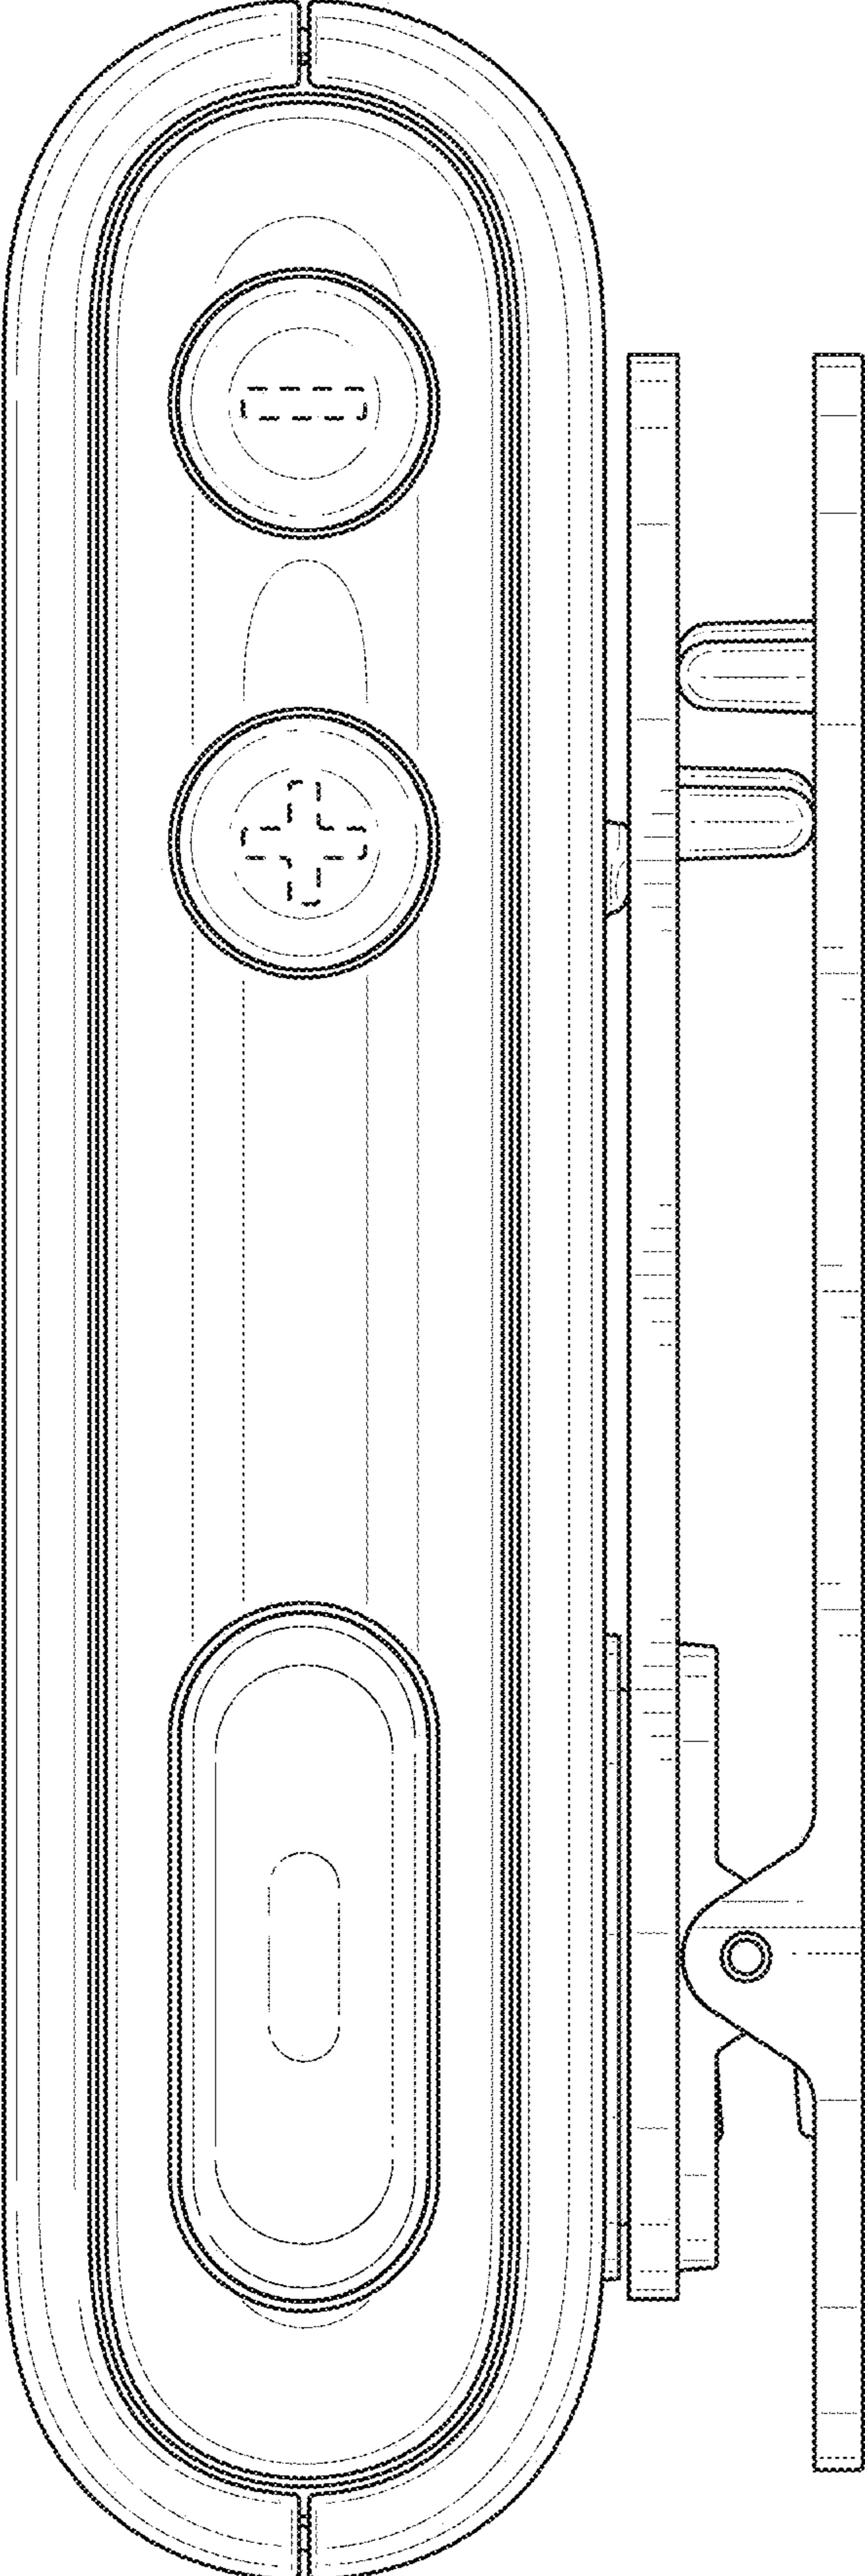


FIG. 7



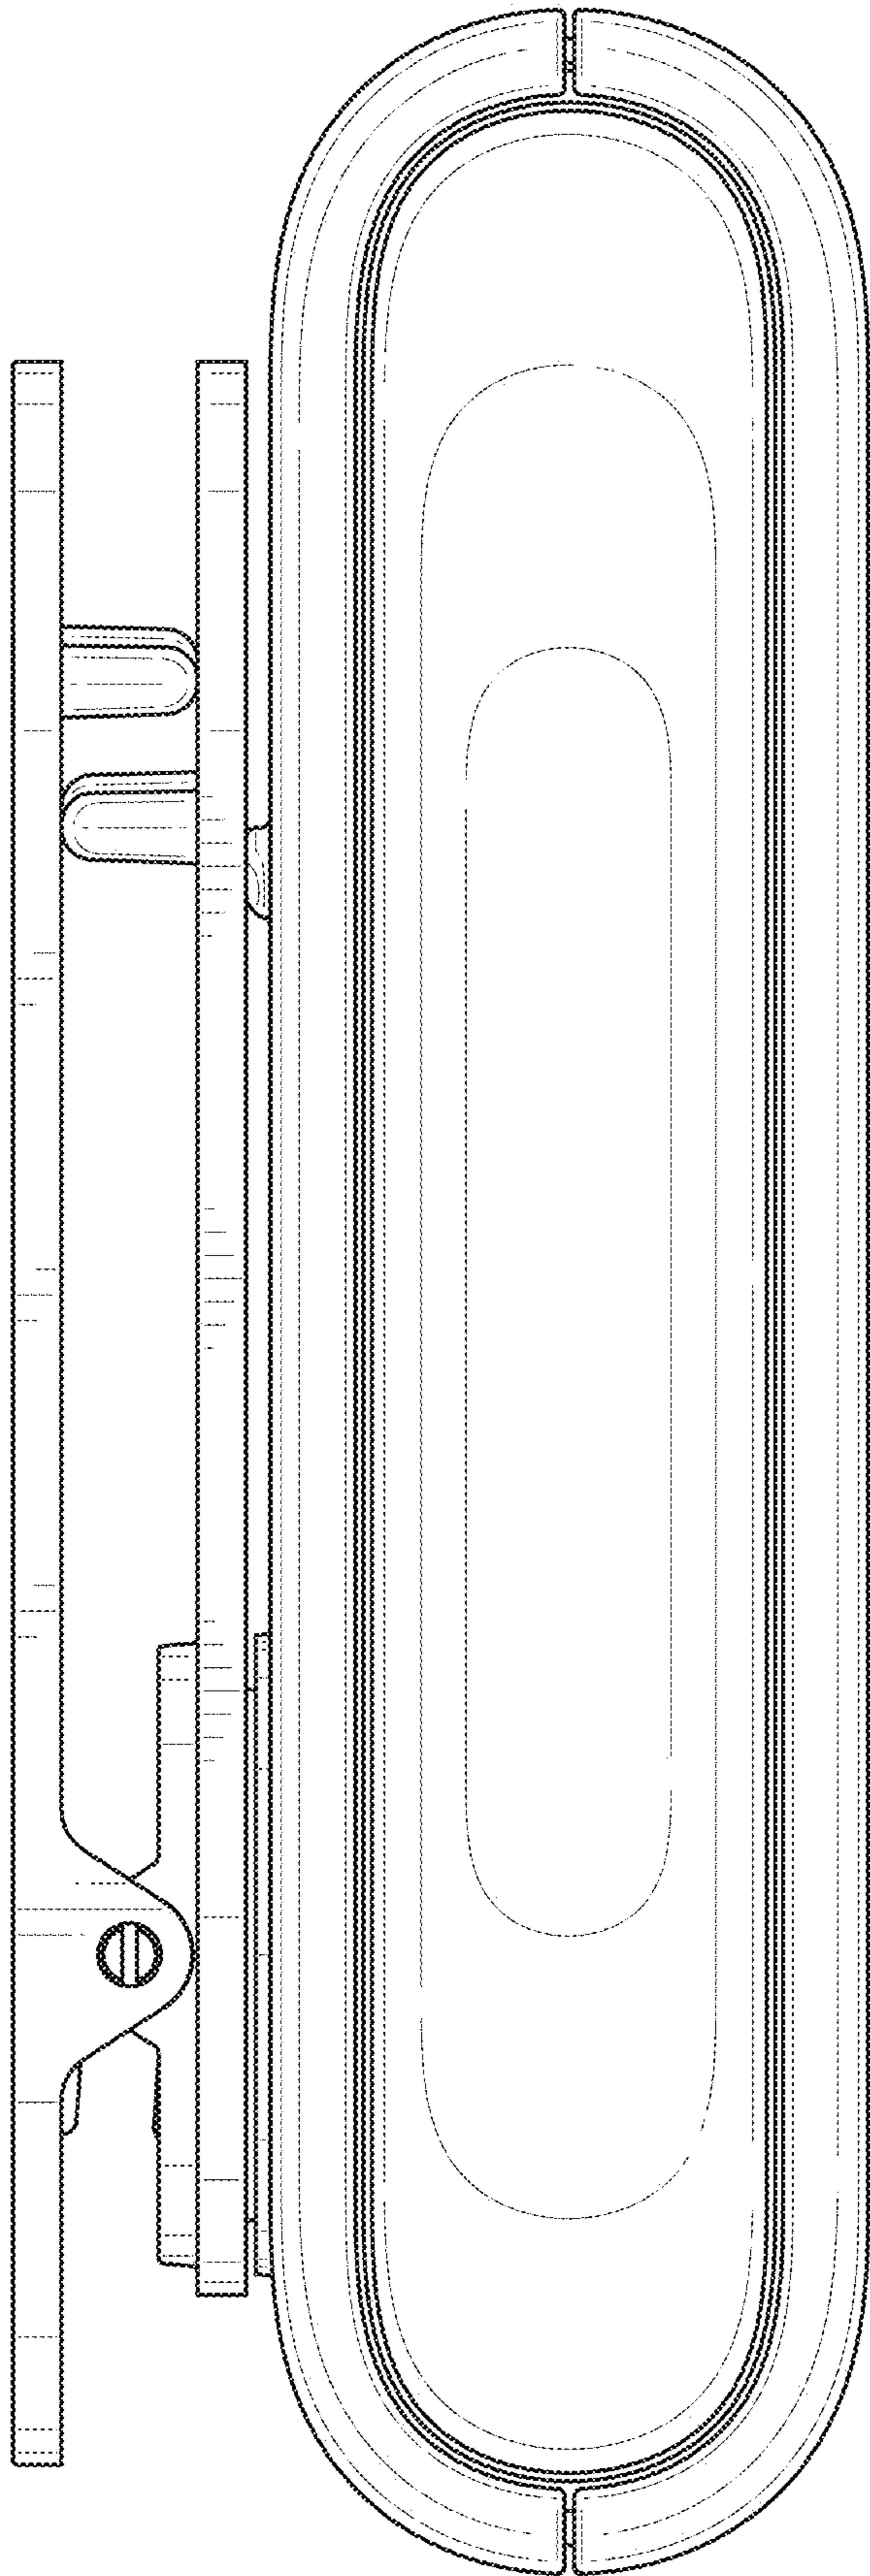

**FIG. 8**