



US00D887562S

(12) **United States Design Patent**
de Jonge et al.

(10) **Patent No.:** **US D887,562 S**
(45) **Date of Patent:** **** Jun. 16, 2020**

(54) **ULTRASOUND PROBE**
(71) Applicant: **Butterfly Network, Inc.**, Guilford, CT (US)
(72) Inventors: **Matthew de Jonge**, New York, NY (US); **Christopher Thomas McNulty**, Guilford, CT (US); **David Elgena**, Brooklyn, NY (US); **Stephen Christopher**, Philadelphia, PA (US); **Paul Maxted**, Guilford, CT (US); **Jonathan C. Schultz**, Guilford, CT (US); **Benjamin Chopra**, Guilford, CT (US)

D703,821 S * 4/2014 Moon D24/187
D704,844 S 5/2014 Saeki
9,072,487 B2 7/2015 Hebrard et al.
D745,175 S 12/2015 Kitayama
D749,224 S * 2/2016 Iritani D24/187
(Continued)

FOREIGN PATENT DOCUMENTS

JP D1457814 12/2012
JP D1515349 1/2015
(Continued)

OTHER PUBLICATIONS

[No Author Listed], HDI 5000 Transducer Listing, Publically known prior to Oct. 27, 2017. 6 pages.
(Continued)

(73) Assignee: **Butterfly Network, Inc.**, Guilford, CT (US)
(**) Term: **15 Years**
(21) Appl. No.: **29/677,065**
(22) Filed: **Jan. 16, 2019**

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Wolf, Greenfield & Sacks, P.C.

Related U.S. Application Data

(62) Division of application No. 29/623,977, filed on Oct. 27, 2017, now Pat. No. Des. 846,749.
(51) **LOC (12) Cl.** **24-01**
(52) **U.S. Cl.**
USPC **D24/187**; D24/186
(58) **Field of Classification Search**
USPC D24/152, 158, 160, 161, 186, 187, 231;
D10/78; D14/420, 426
CPC A61B 8/445; A61B 8/4455; A61B 8/4461
See application file for complete search history.

(57) **CLAIM**

The ornamental design for an ultrasound probe, as shown and described.

DESCRIPTION


FIG. 1 is a bottom, front, right side perspective view of an ultrasound probe showing our new design;
FIG. 2 is a front elevation view thereof;
FIG. 3 is a rear elevation view thereof;
FIG. 4 is a left side elevation view thereof;
FIG. 5 is a right side elevation view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The dot-dash broken lines in the figures represent boundaries of the claimed design and form no part thereof. All other broken lines illustrate portions of the ultrasound probe that form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D545,433 S 6/2007 Messerly et al.
D681,824 S 5/2013 Shinohara et al.
D703,332 S * 4/2014 Saeki D24/187

1 Claim, 4 Drawing Sheets

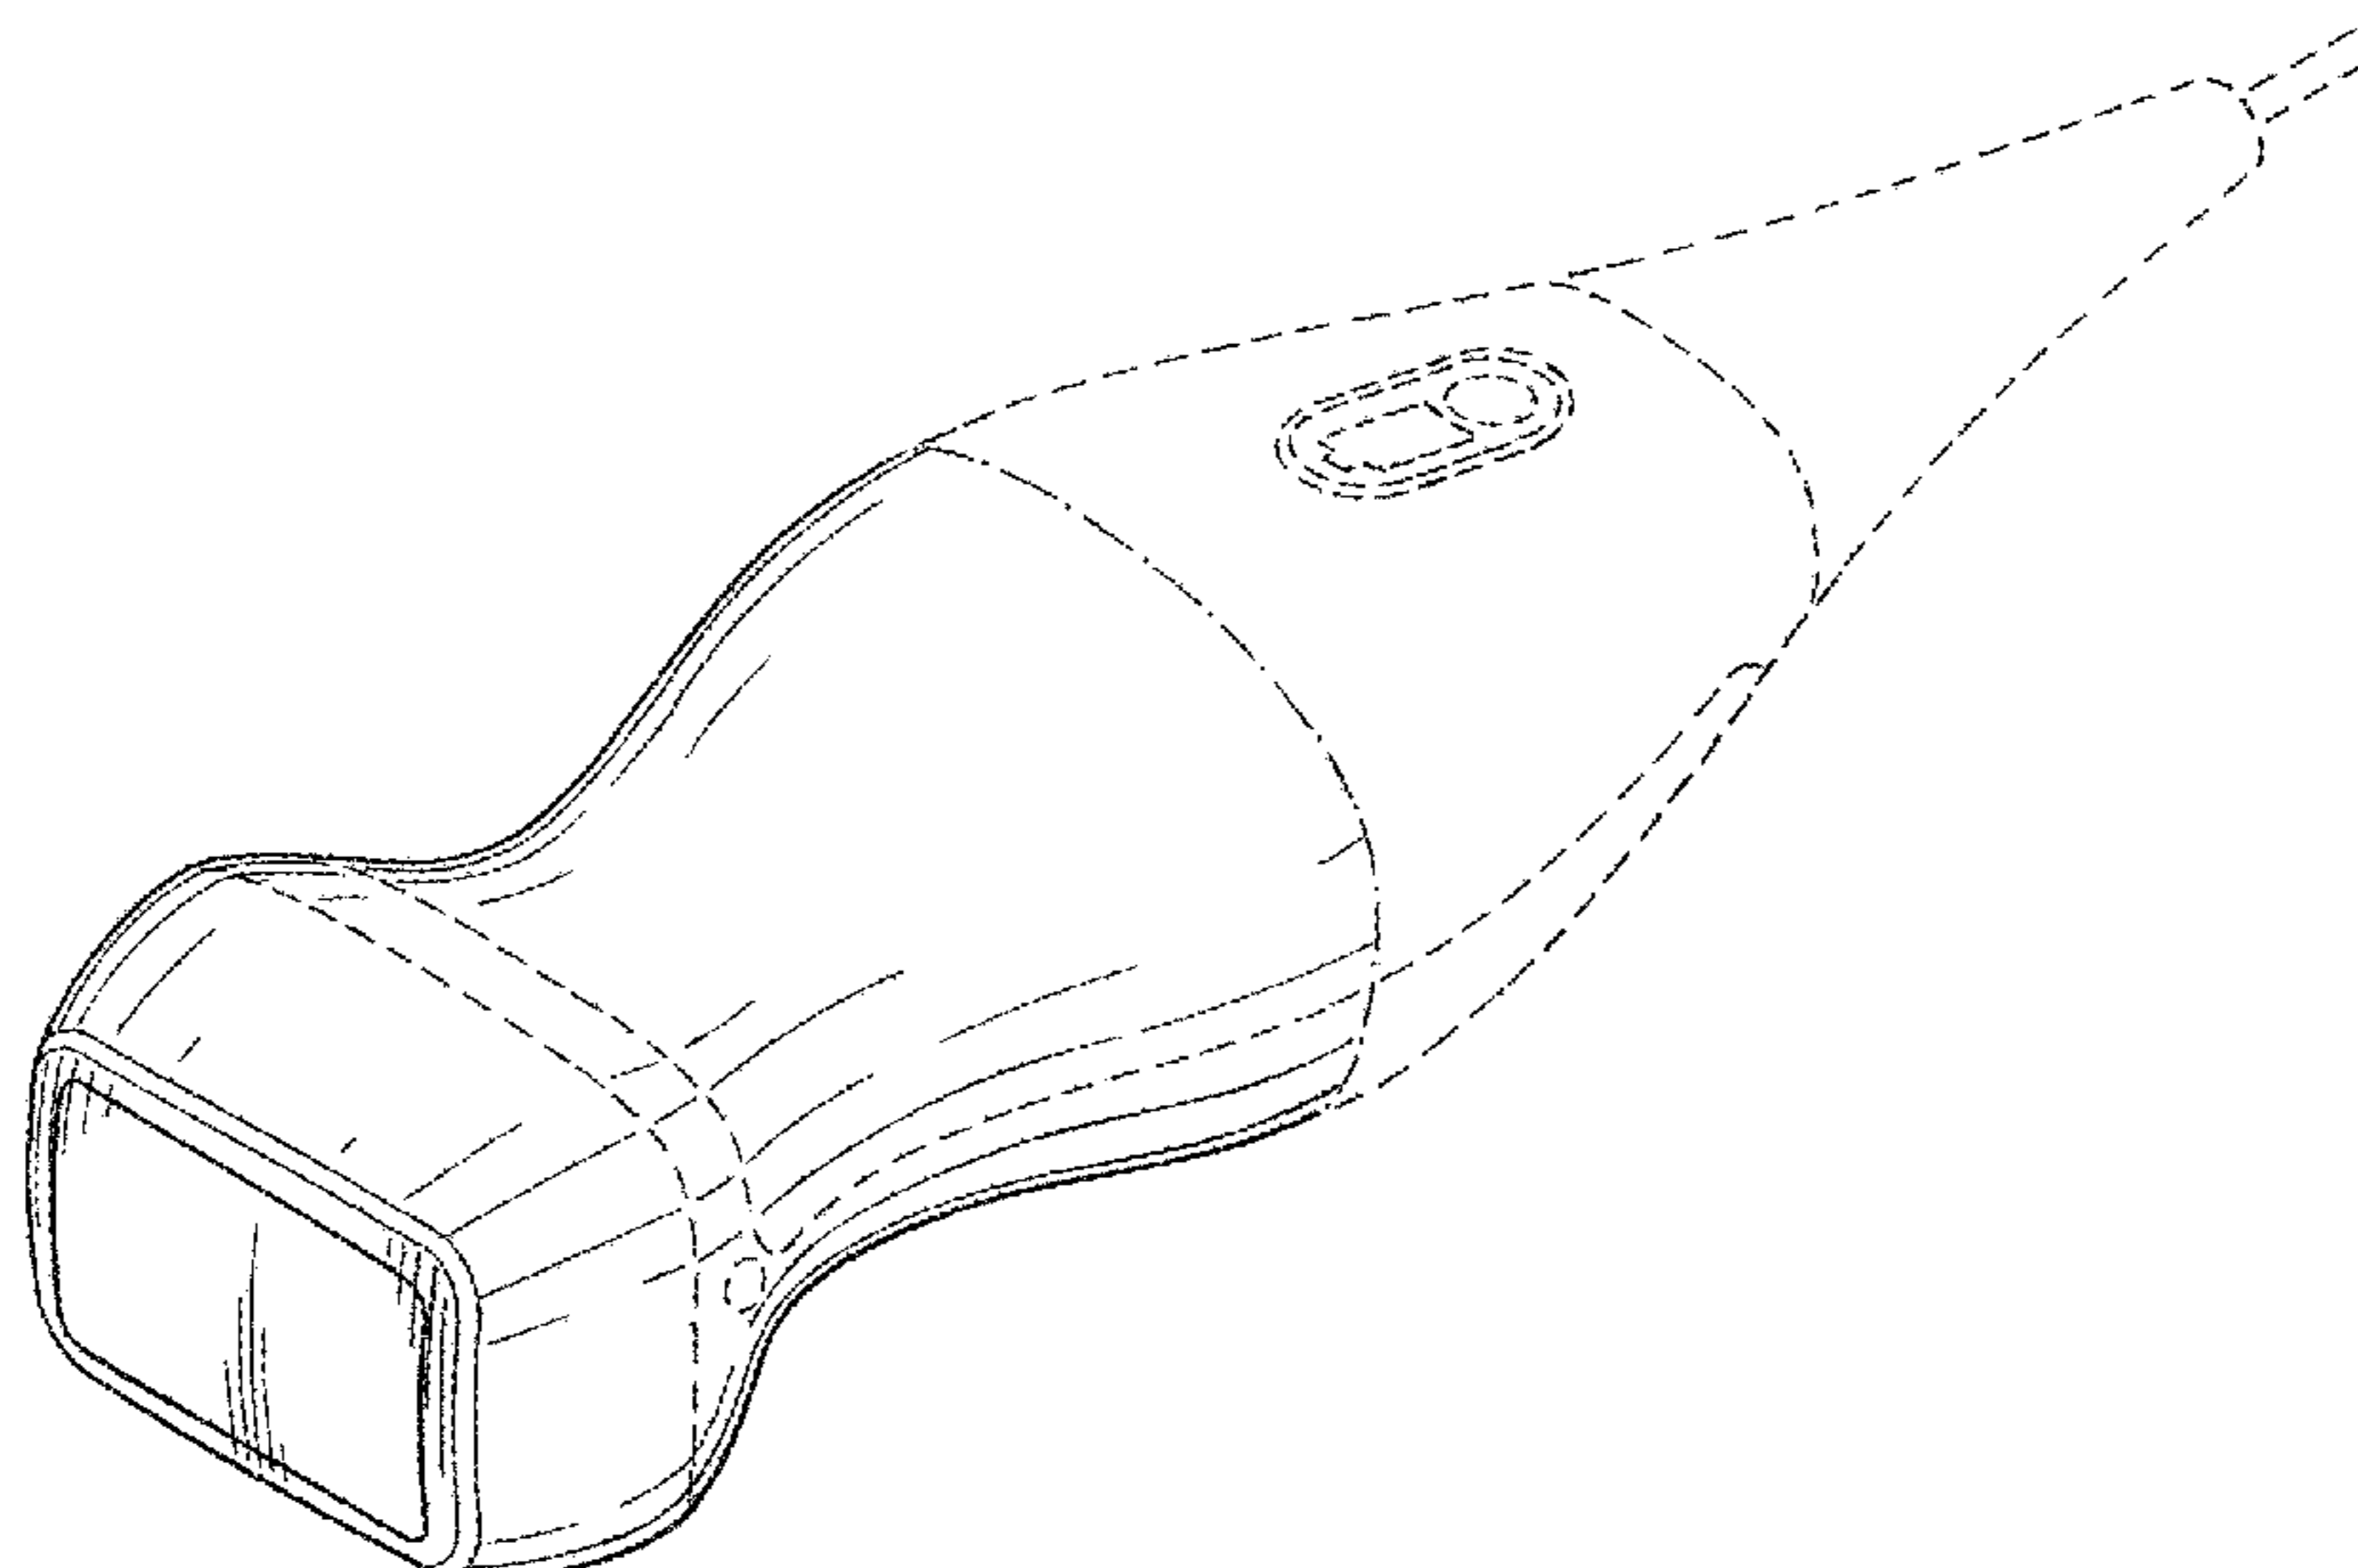

(56)

References Cited

U.S. PATENT DOCUMENTS

D816,850	S	5/2018	Asai et al.	
D831,219	S	* 10/2018	Henderson	D24/187
D846,128	S	* 4/2019	de Jonge	D24/187
D846,749	S	* 4/2019	de Jonge	D24/187
2011/0055447	A1	3/2011	Costa	
2015/0112200	A1	4/2015	Oberg et al.	
2017/0172542	A1	6/2017	Lee et al.	
2017/0360397	A1	12/2017	Rothberg et al.	
2017/0360401	A1	12/2017	Rothberg et al.	
2018/0028159	A1	2/2018	Hageman et al.	

FOREIGN PATENT DOCUMENTS

JP	D1564542	12/2016
KR	30-0726181	1/2014
KR	30-0726182	1/2014
KR	30-0751362	7/2014
KR	30-0764107	10/2014

OTHER PUBLICATIONS

Declaration of David Elegna, signed May 11, 2018, submitted to the Japanese Patent Office in co-pending application No. JP 2018-009209.

Enriquez et al., An Introduction to Ultrasound Equipment and Knobology. Crit Care Clin. Jan. 2014; 30(1):25-45.

* cited by examiner

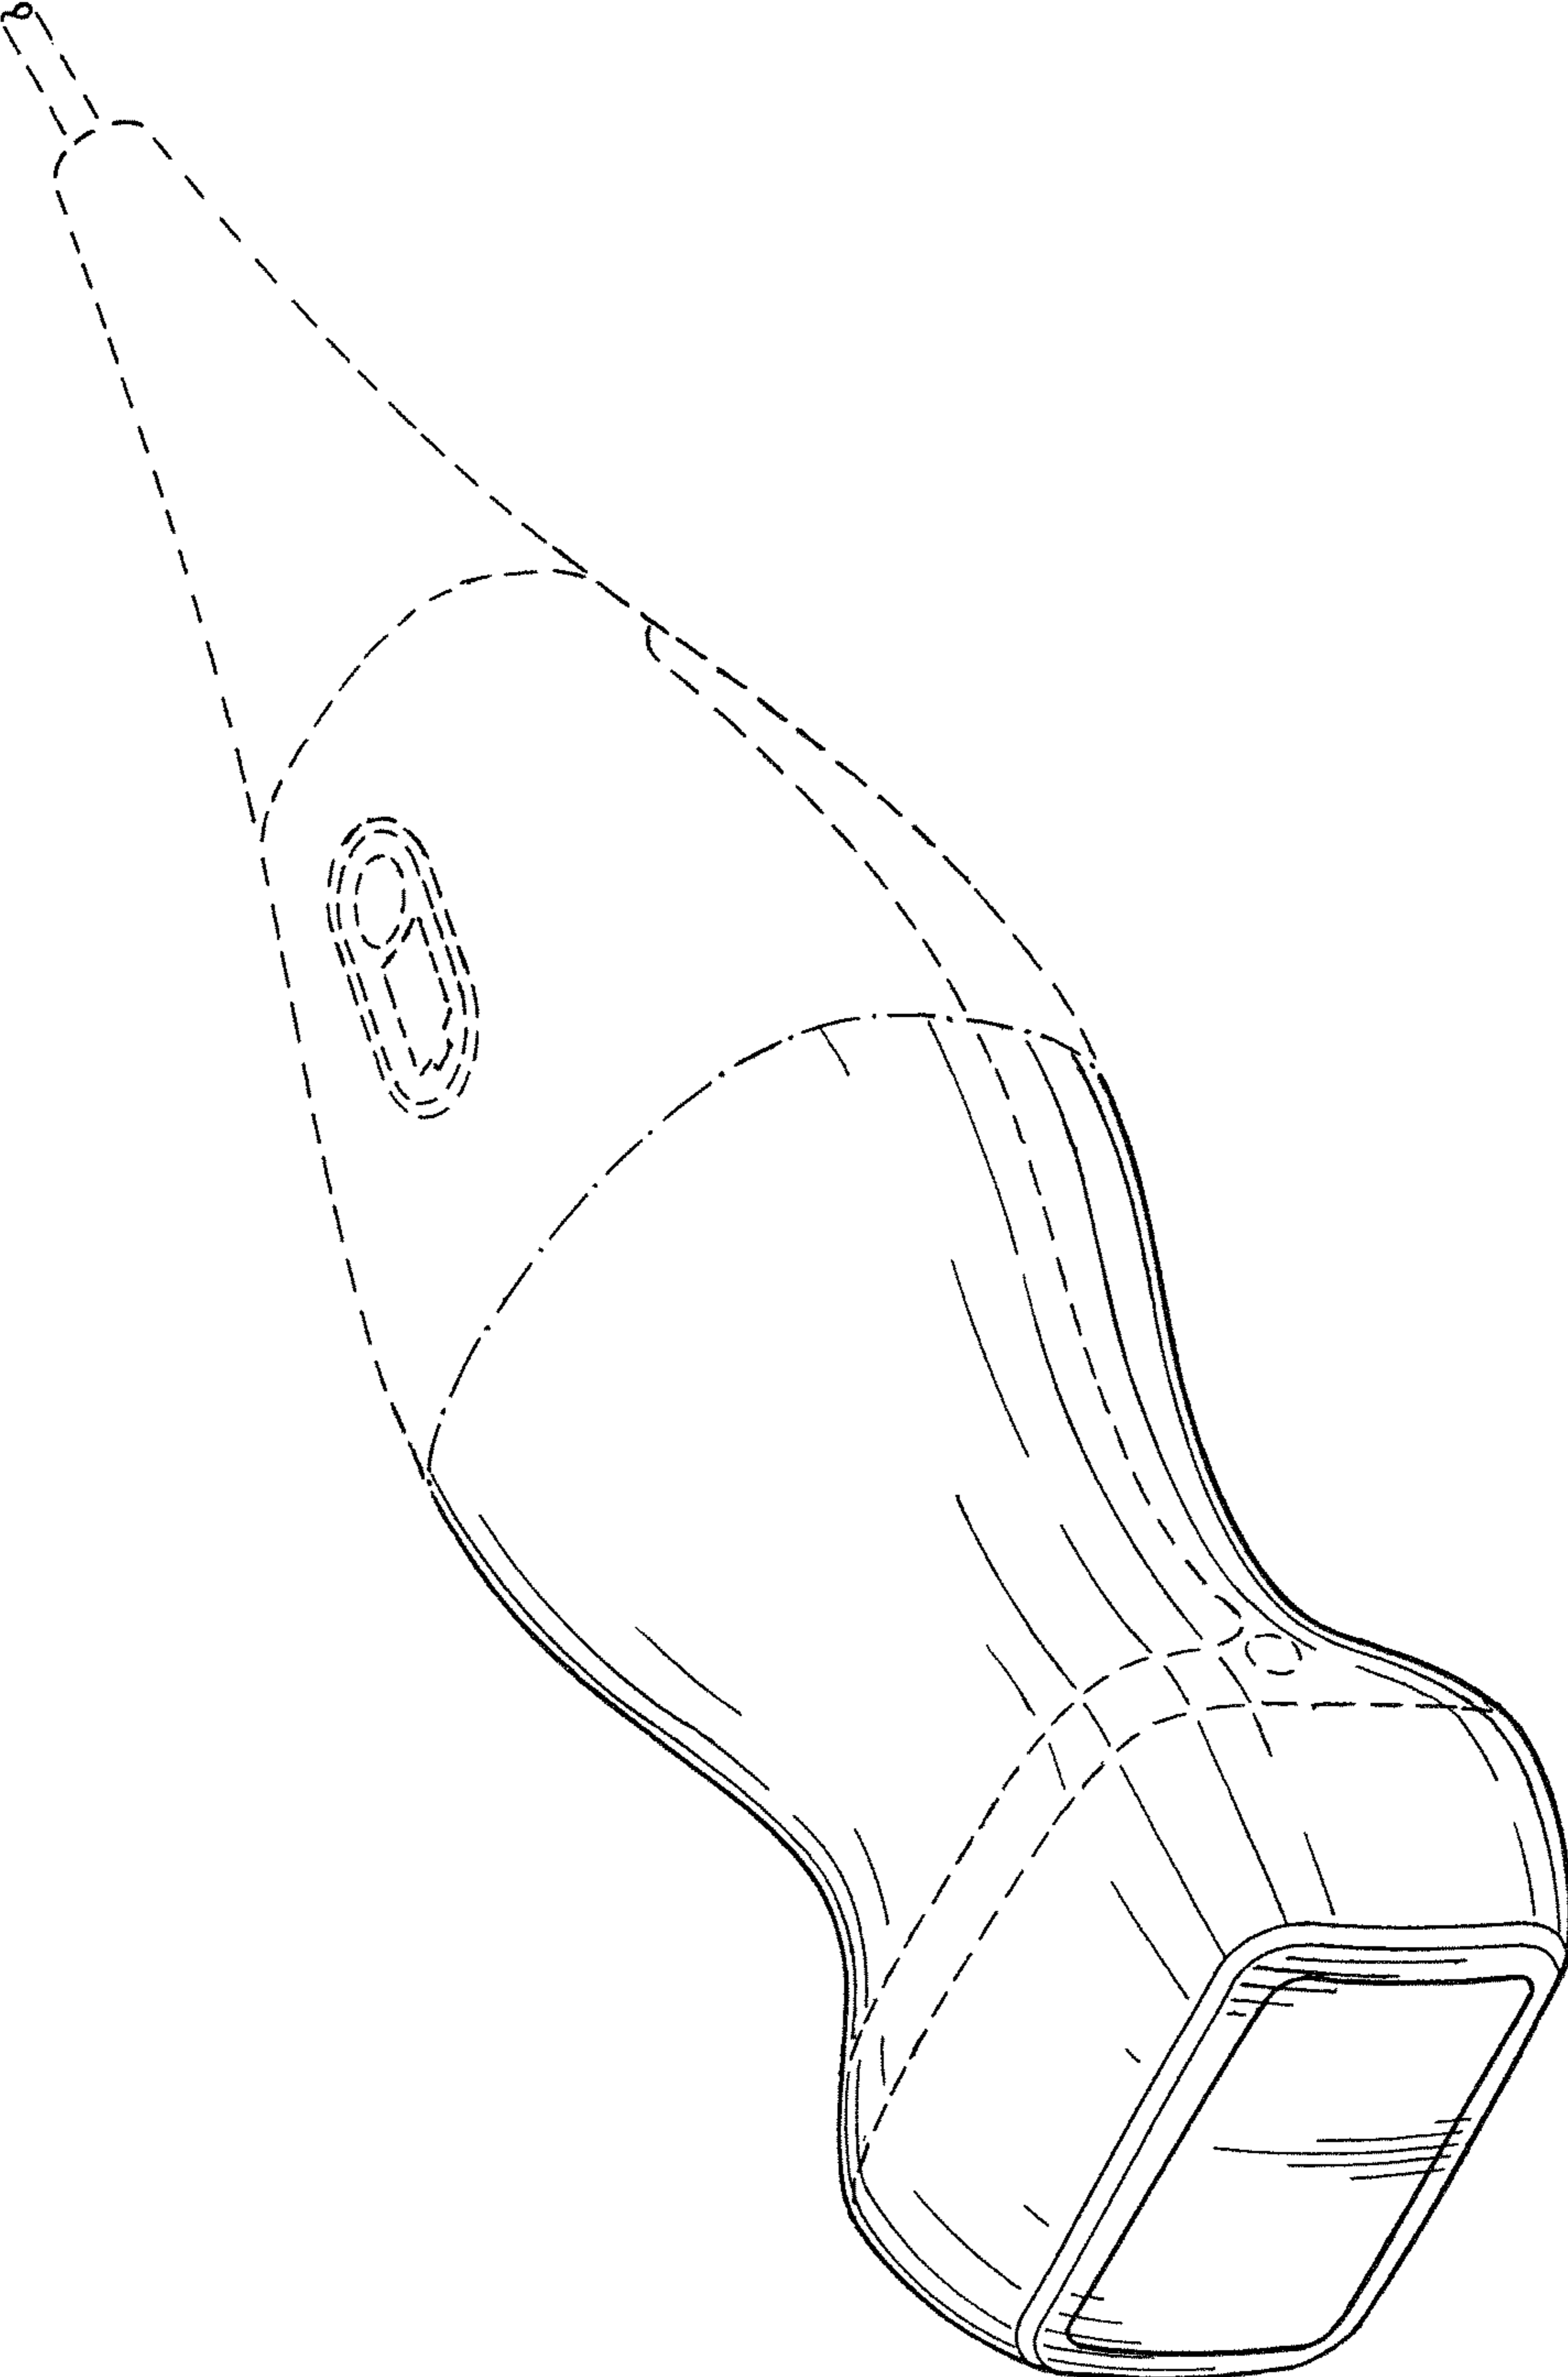


Fig. 1

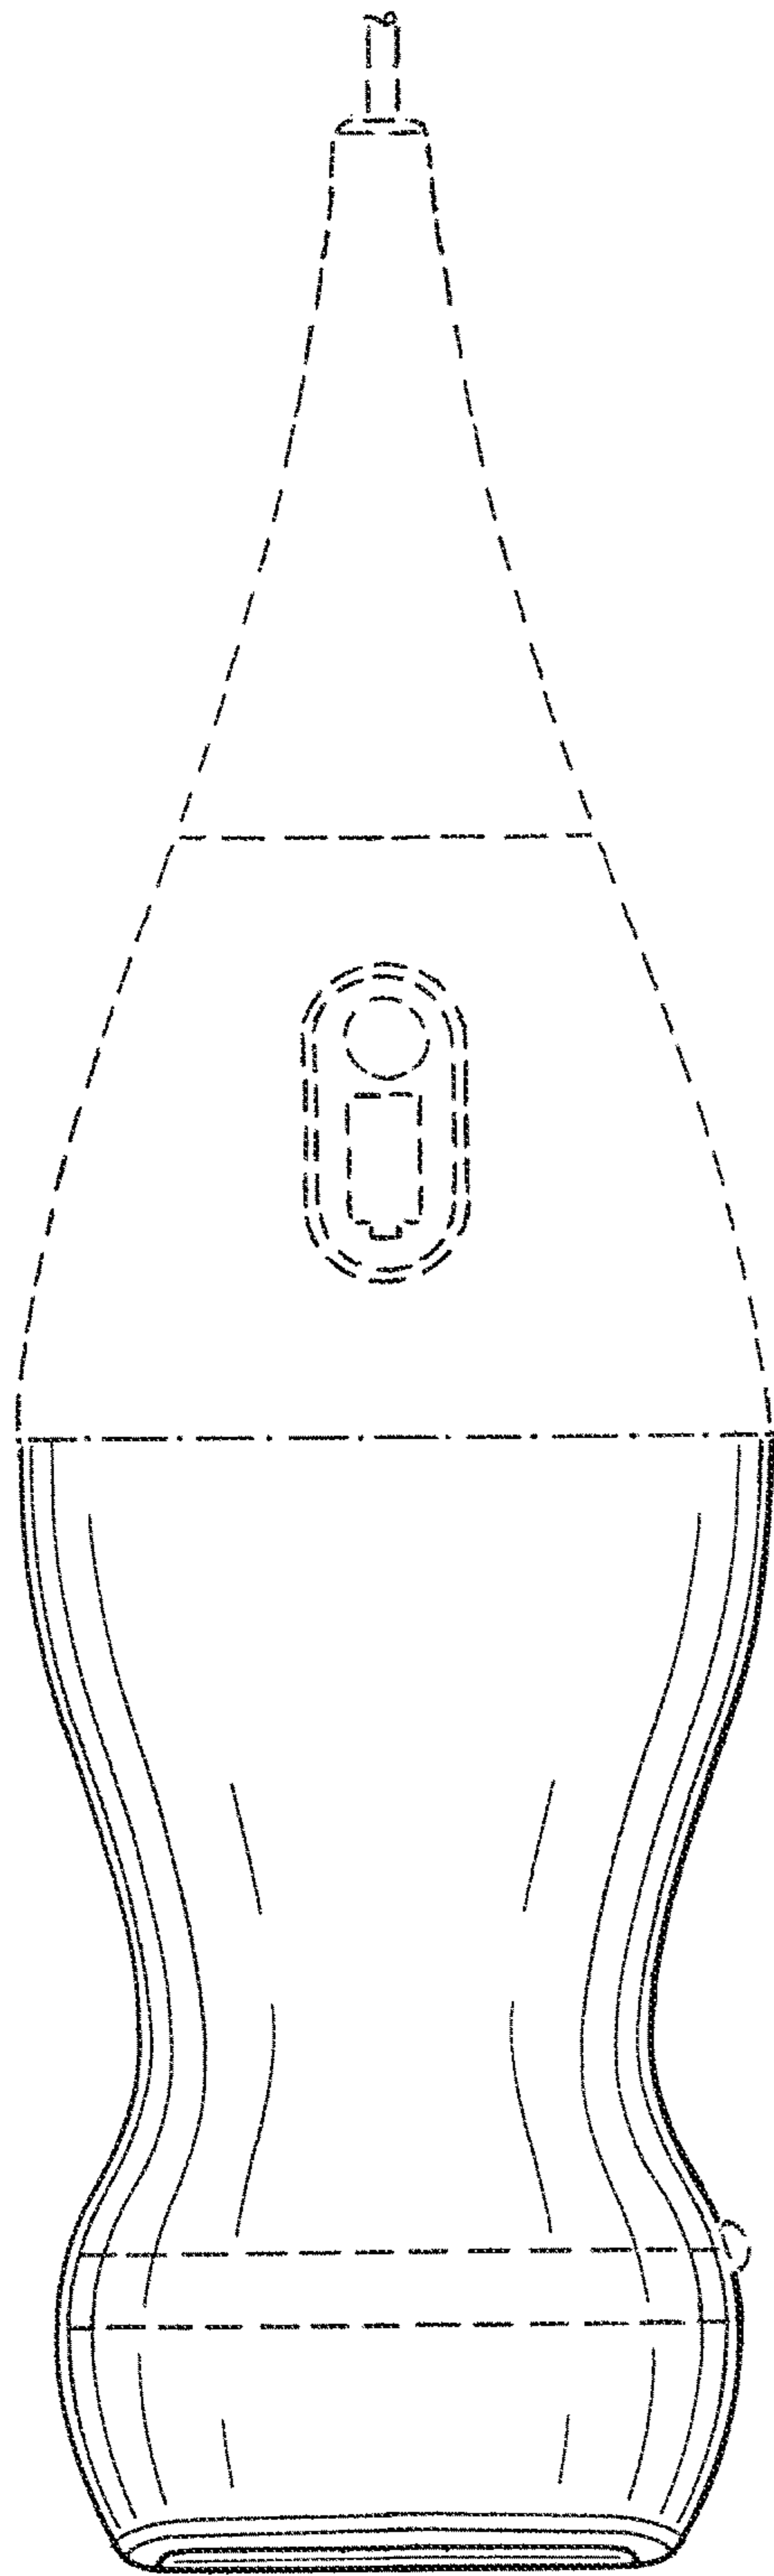


Fig. 2

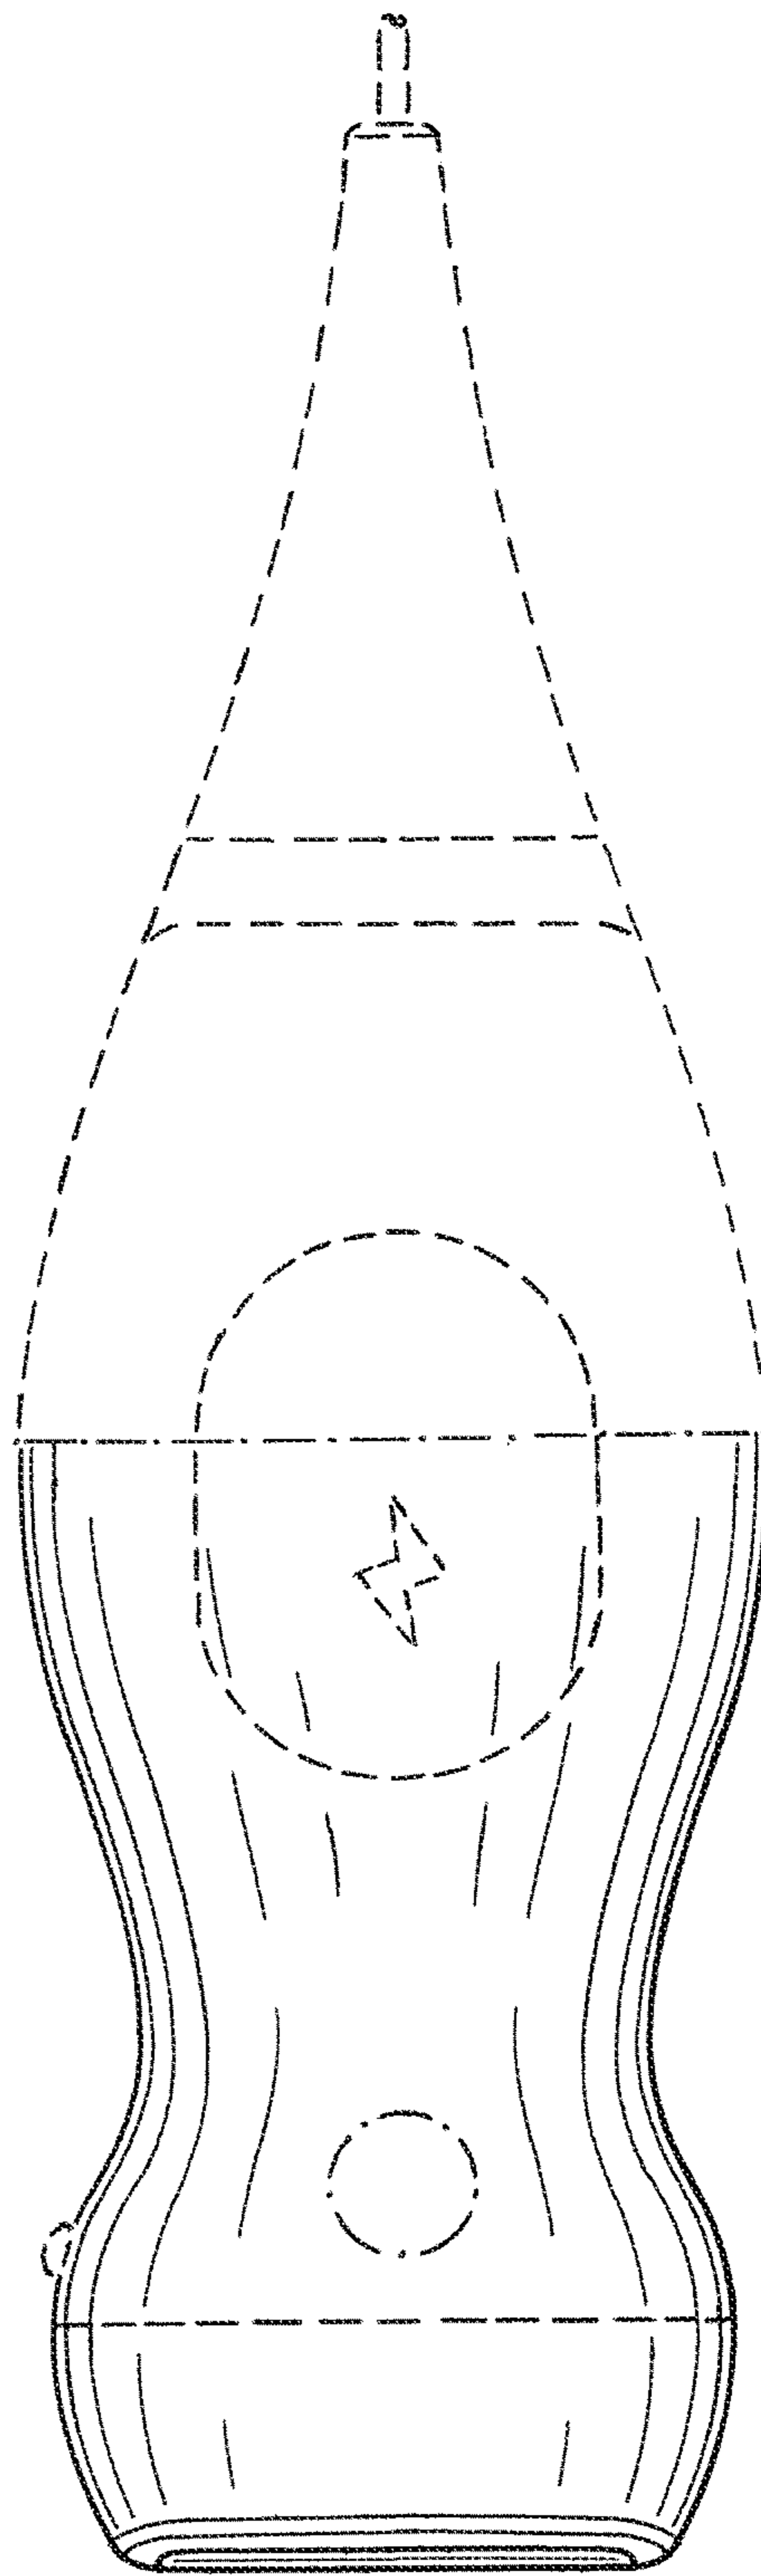


Fig. 3

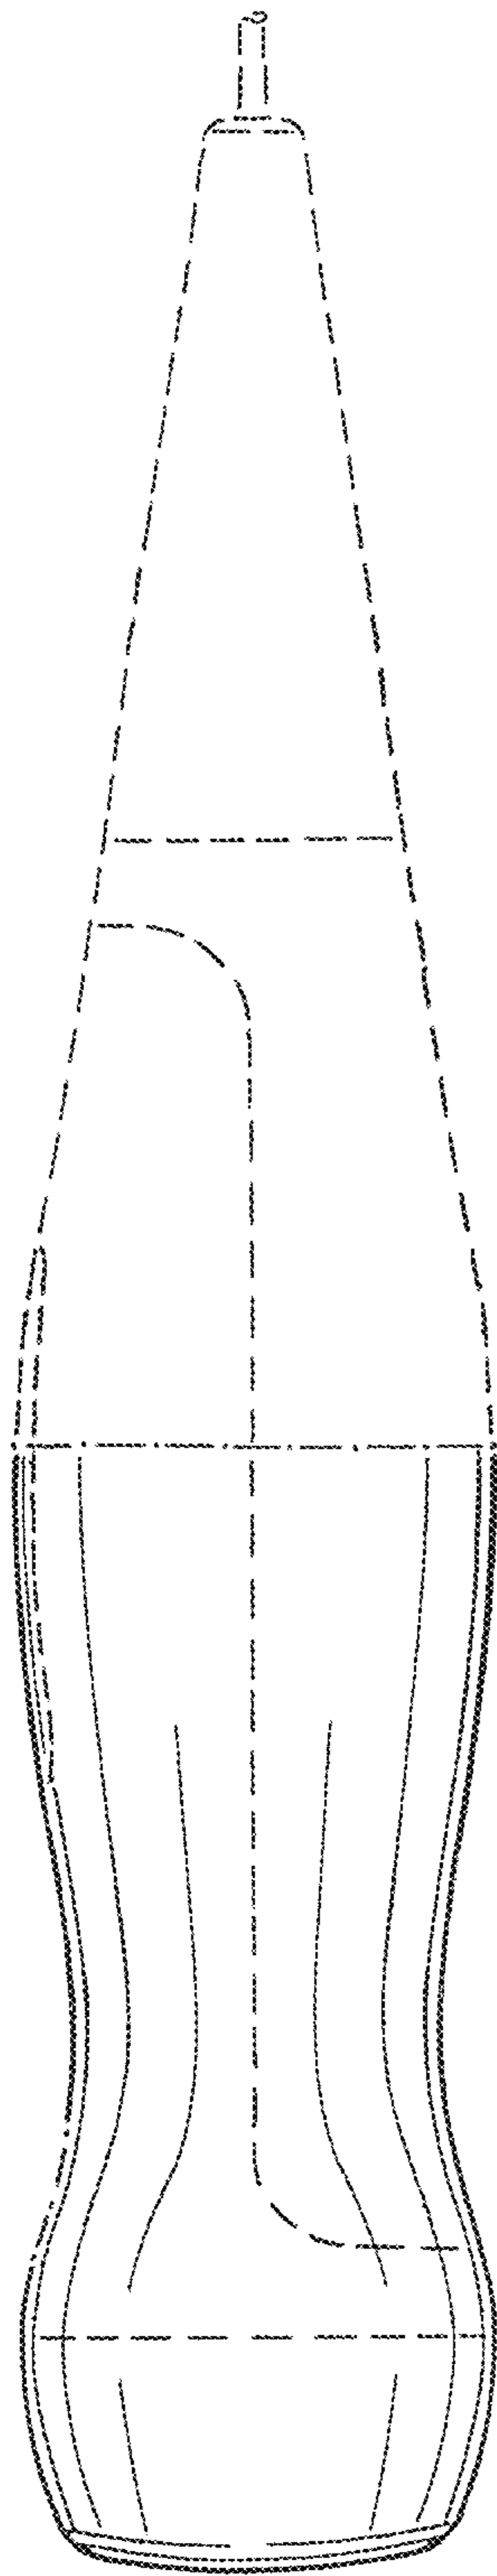


Fig. 4

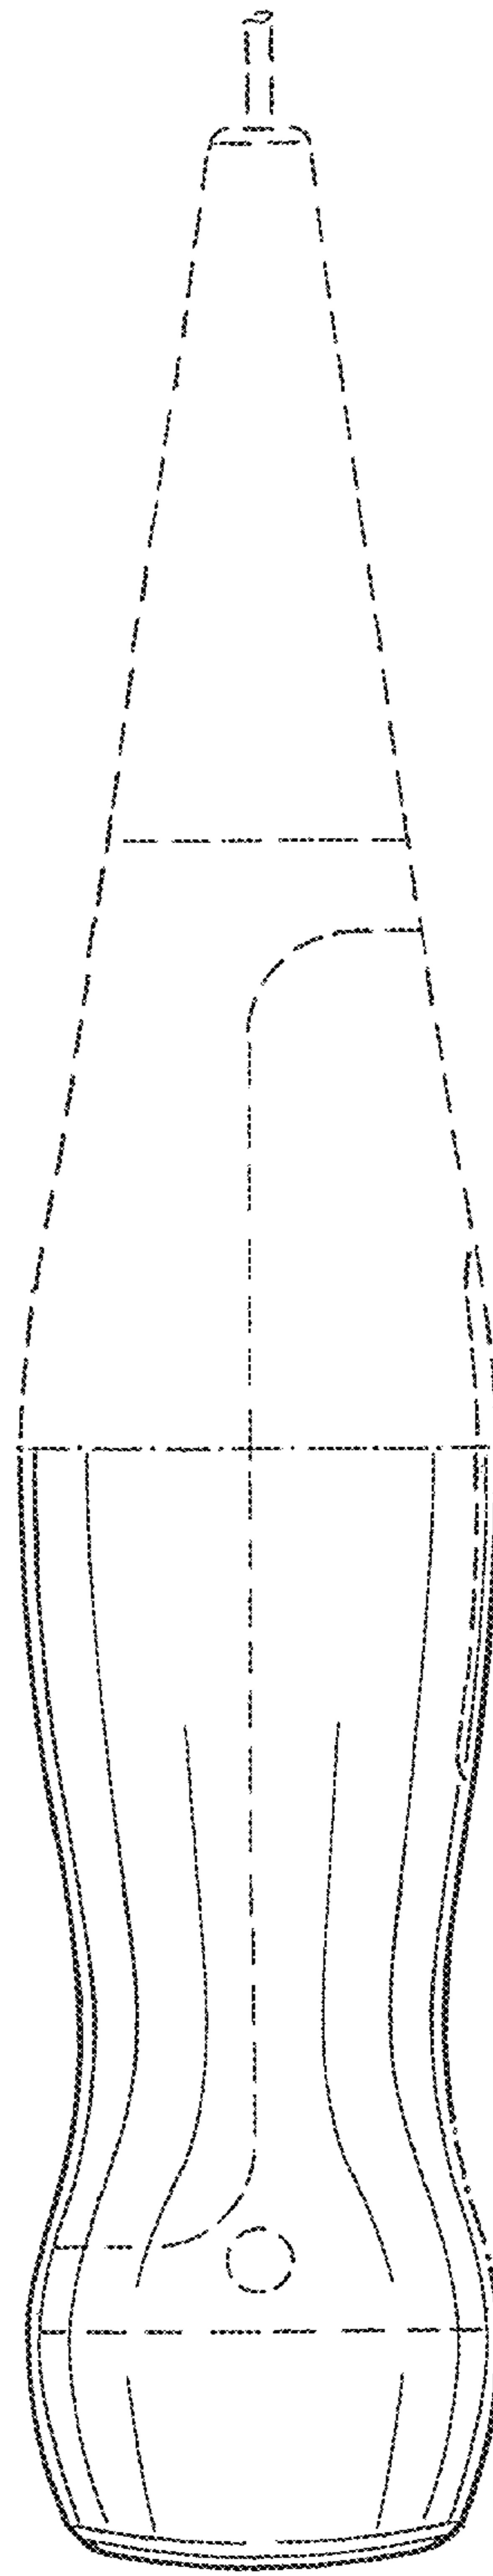


Fig. 5

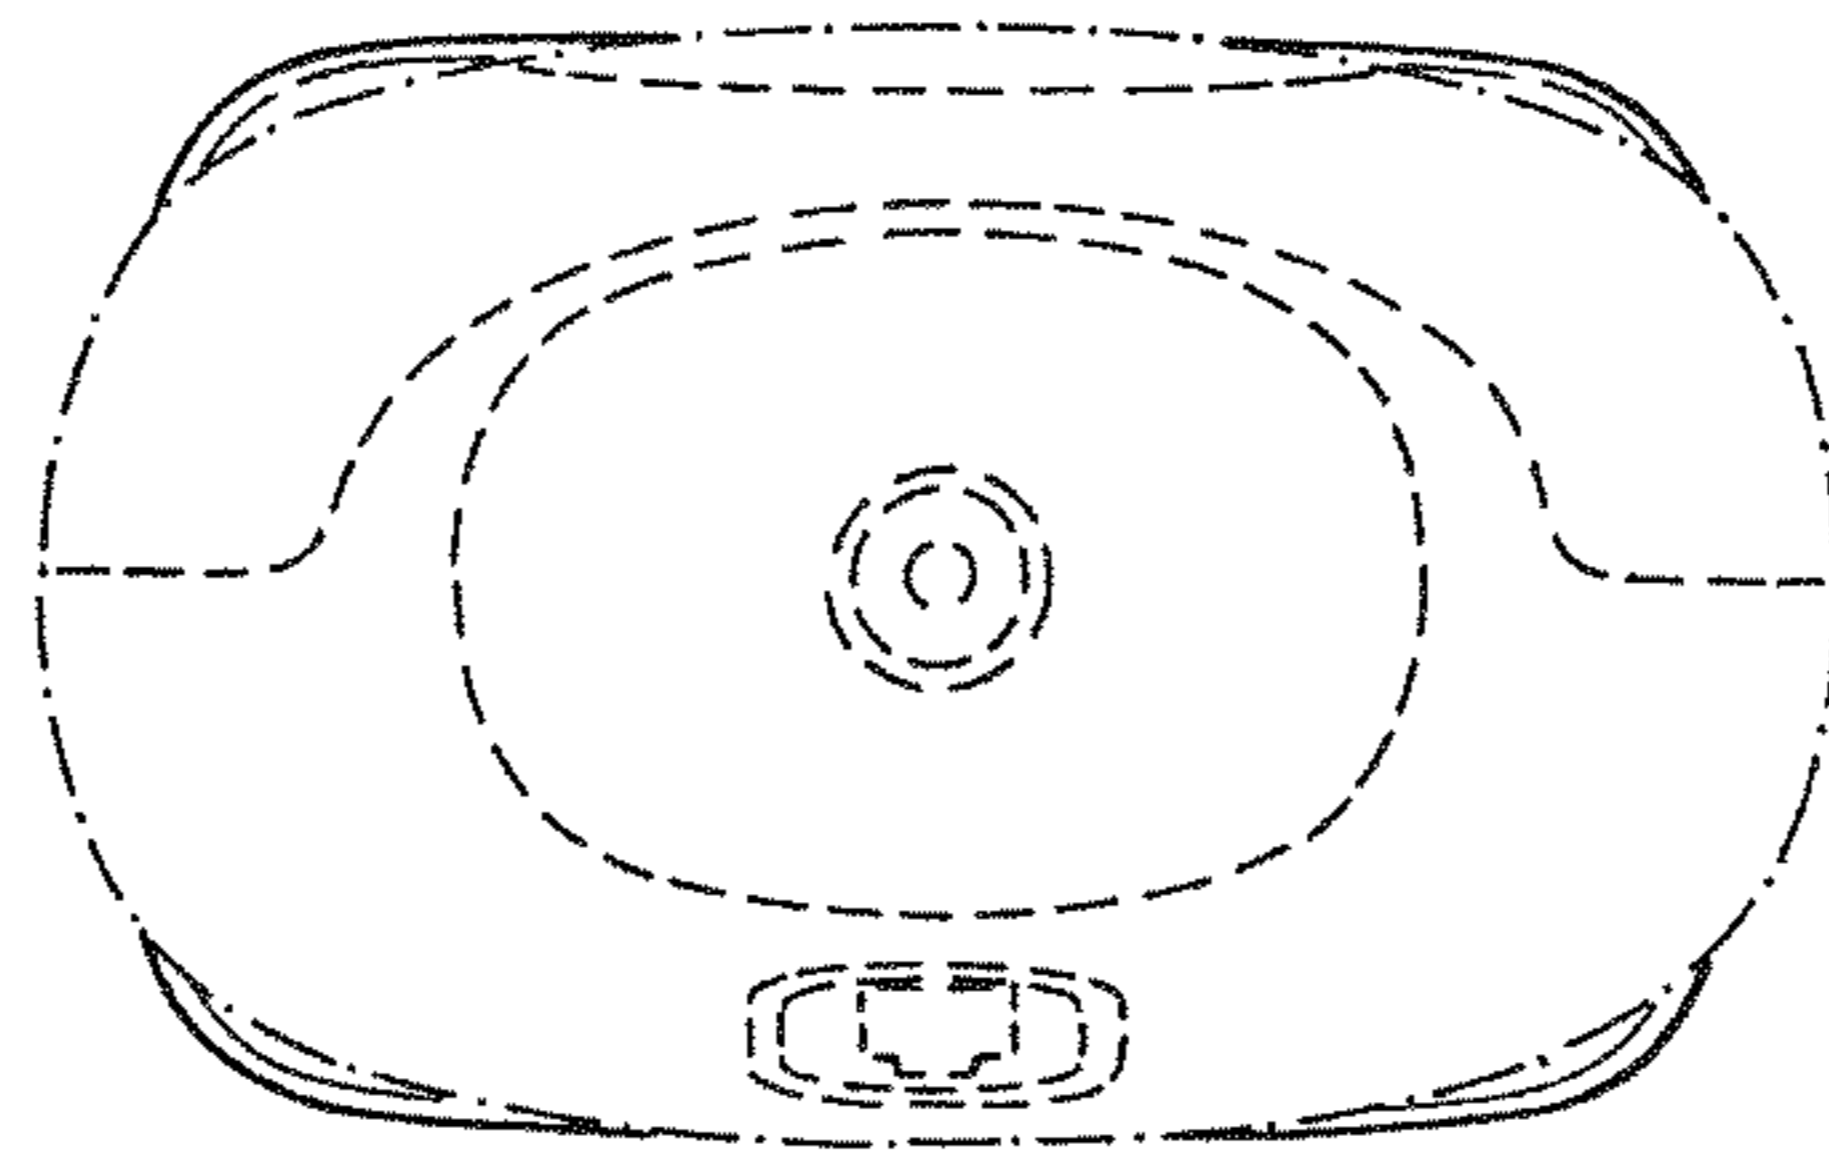


Fig. 6

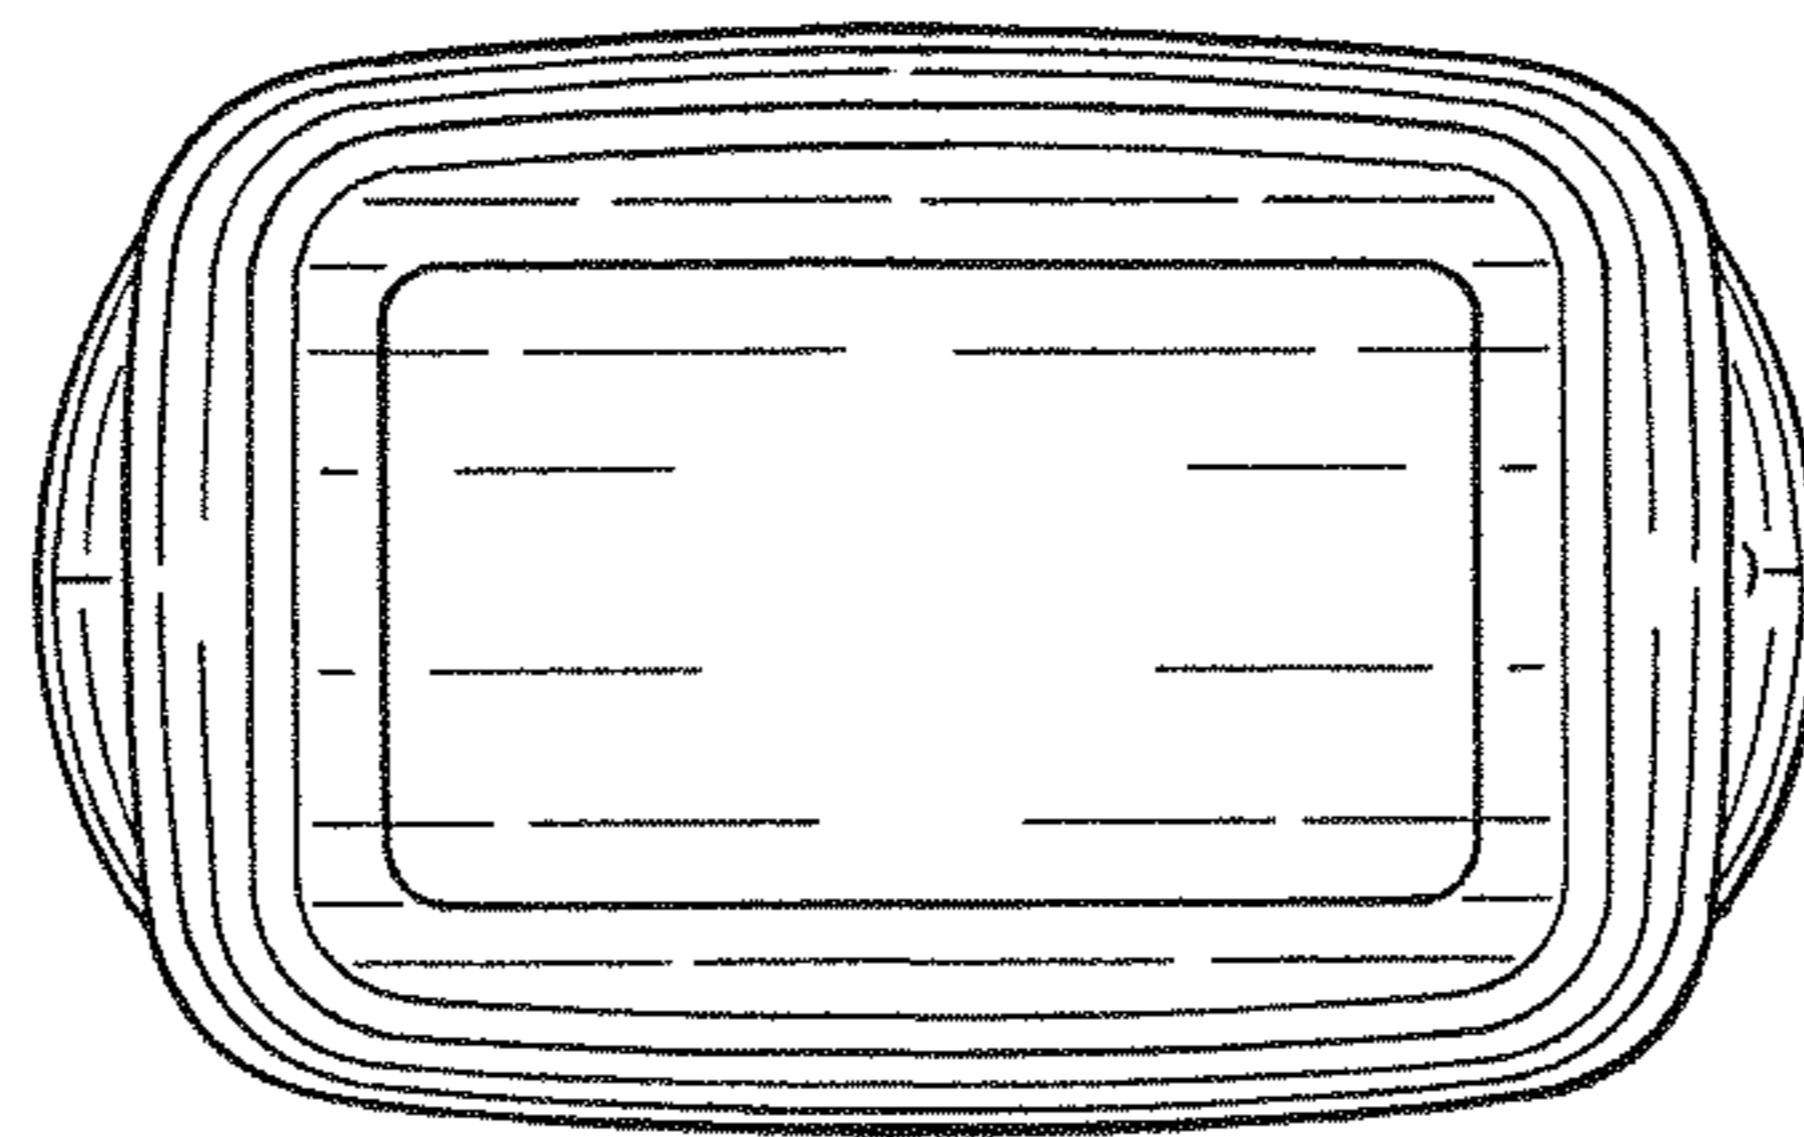


Fig. 7