



US00D888267S

(12) **United States Design Patent**  
**Salomon et al.**

(10) **Patent No.:** **US D888,267 S**  
(45) **Date of Patent:** **\*\* Jun. 23, 2020**

(54) **DIAGNOSTIC INSTRUMENT**

D649,658 S 11/2011 Belfance et al.  
D669,169 S 10/2012 Washington et al.  
D682,441 S \* 5/2013 Kim ..... D24/216  
(Continued)

(71) Applicant: **MeMed Diagnostics Ltd.**, Tirat  
HaCarmel (IL)

(72) Inventors: **Noga Salomon**, Carmiel (IL); **Kfir Oved**, Hof HaCarmel (IL); **Roy Navon**, Tel-Aviv (IL); **Assaf Cohen-Dotan**, Natania (IL); **Eran Eden**, Haifa (IL); **Salit Tzaban**, Nofit (IL); **Yana Khalfin**, Haifa (IL); **Ofer Halbreich**, Tel-Aviv (IL); **Matthew Fenwick**, Mount Waverley (AU); **Adrian Charles Ian Scott-Murphy**, Surrey Hills (AU); **Matthew Hou-Pou Yeung**, Nunawading (AU); **James William Luther**, Milan (IT); **Barbara Tornaghi**, Monza (IT); **Andrea Besana**, Seveso (IT)

FOREIGN PATENT DOCUMENTS

WO WO 2019/087176 5/2019

OTHER PUBLICATIONS

The platform: MeMed Key™, posted at www.me-med.com, no posting date, online, URL:https://www.me-med.com/ (Year: 2019).\*  
(Continued)

*Primary Examiner* — Lilyana Bekic  
*Assistant Examiner* — Mary Shannon Malley

(73) Assignee: **MeMed Diagnostics Ltd.**, Tirat  
HaCarmel (IL)

(57) **CLAIM**

The ornamental design for a diagnostic instrument, as shown and described.

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/645,126**

**DESCRIPTION**

(22) Filed: **Apr. 24, 2018**

(51) **LOC (12) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/216**

(58) **Field of Classification Search**  
USPC ..... D24/216, 219, 223, 224, 227, 229, 230, D24/231, 232, 233, 234, 107, 186, 217, D24/220, 225, 226; D10/81, 97  
CPC ..... G01N 2035/00306; G01N 2035/00326; G01N 2035/00336; G01N 33/53; G01N 33/5302; G01N 33/569; B01L 7/52  
See application file for complete search history.

This invention was made with government support under contract number HDTRA1-17-C-0011 awarded by the Defense Threat Reduction Agency and grant number W81XWH-17-1-0694 awarded by the U.S. Army Medical Research Acquisition Activity. The government has certain rights in the invention.

FIG. 1 is a front perspective view of a diagnostic instrument showing our new design;  
FIG. 2 is a front view thereof;  
FIG. 3 is a right side view thereof;  
FIG. 4 is a left side thereof;  
FIG. 5 is a top view thereof;  
FIG. 6 is a back view thereof; and,  
FIG. 7 is a bottom view thereof.


The broken lines depict portions of the diagnostic instrument that do not form part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,576,185 A 3/1986 Proud et al.  
D631,554 S 1/2011 Jackson et al.

**1 Claim, 7 Drawing Sheets**

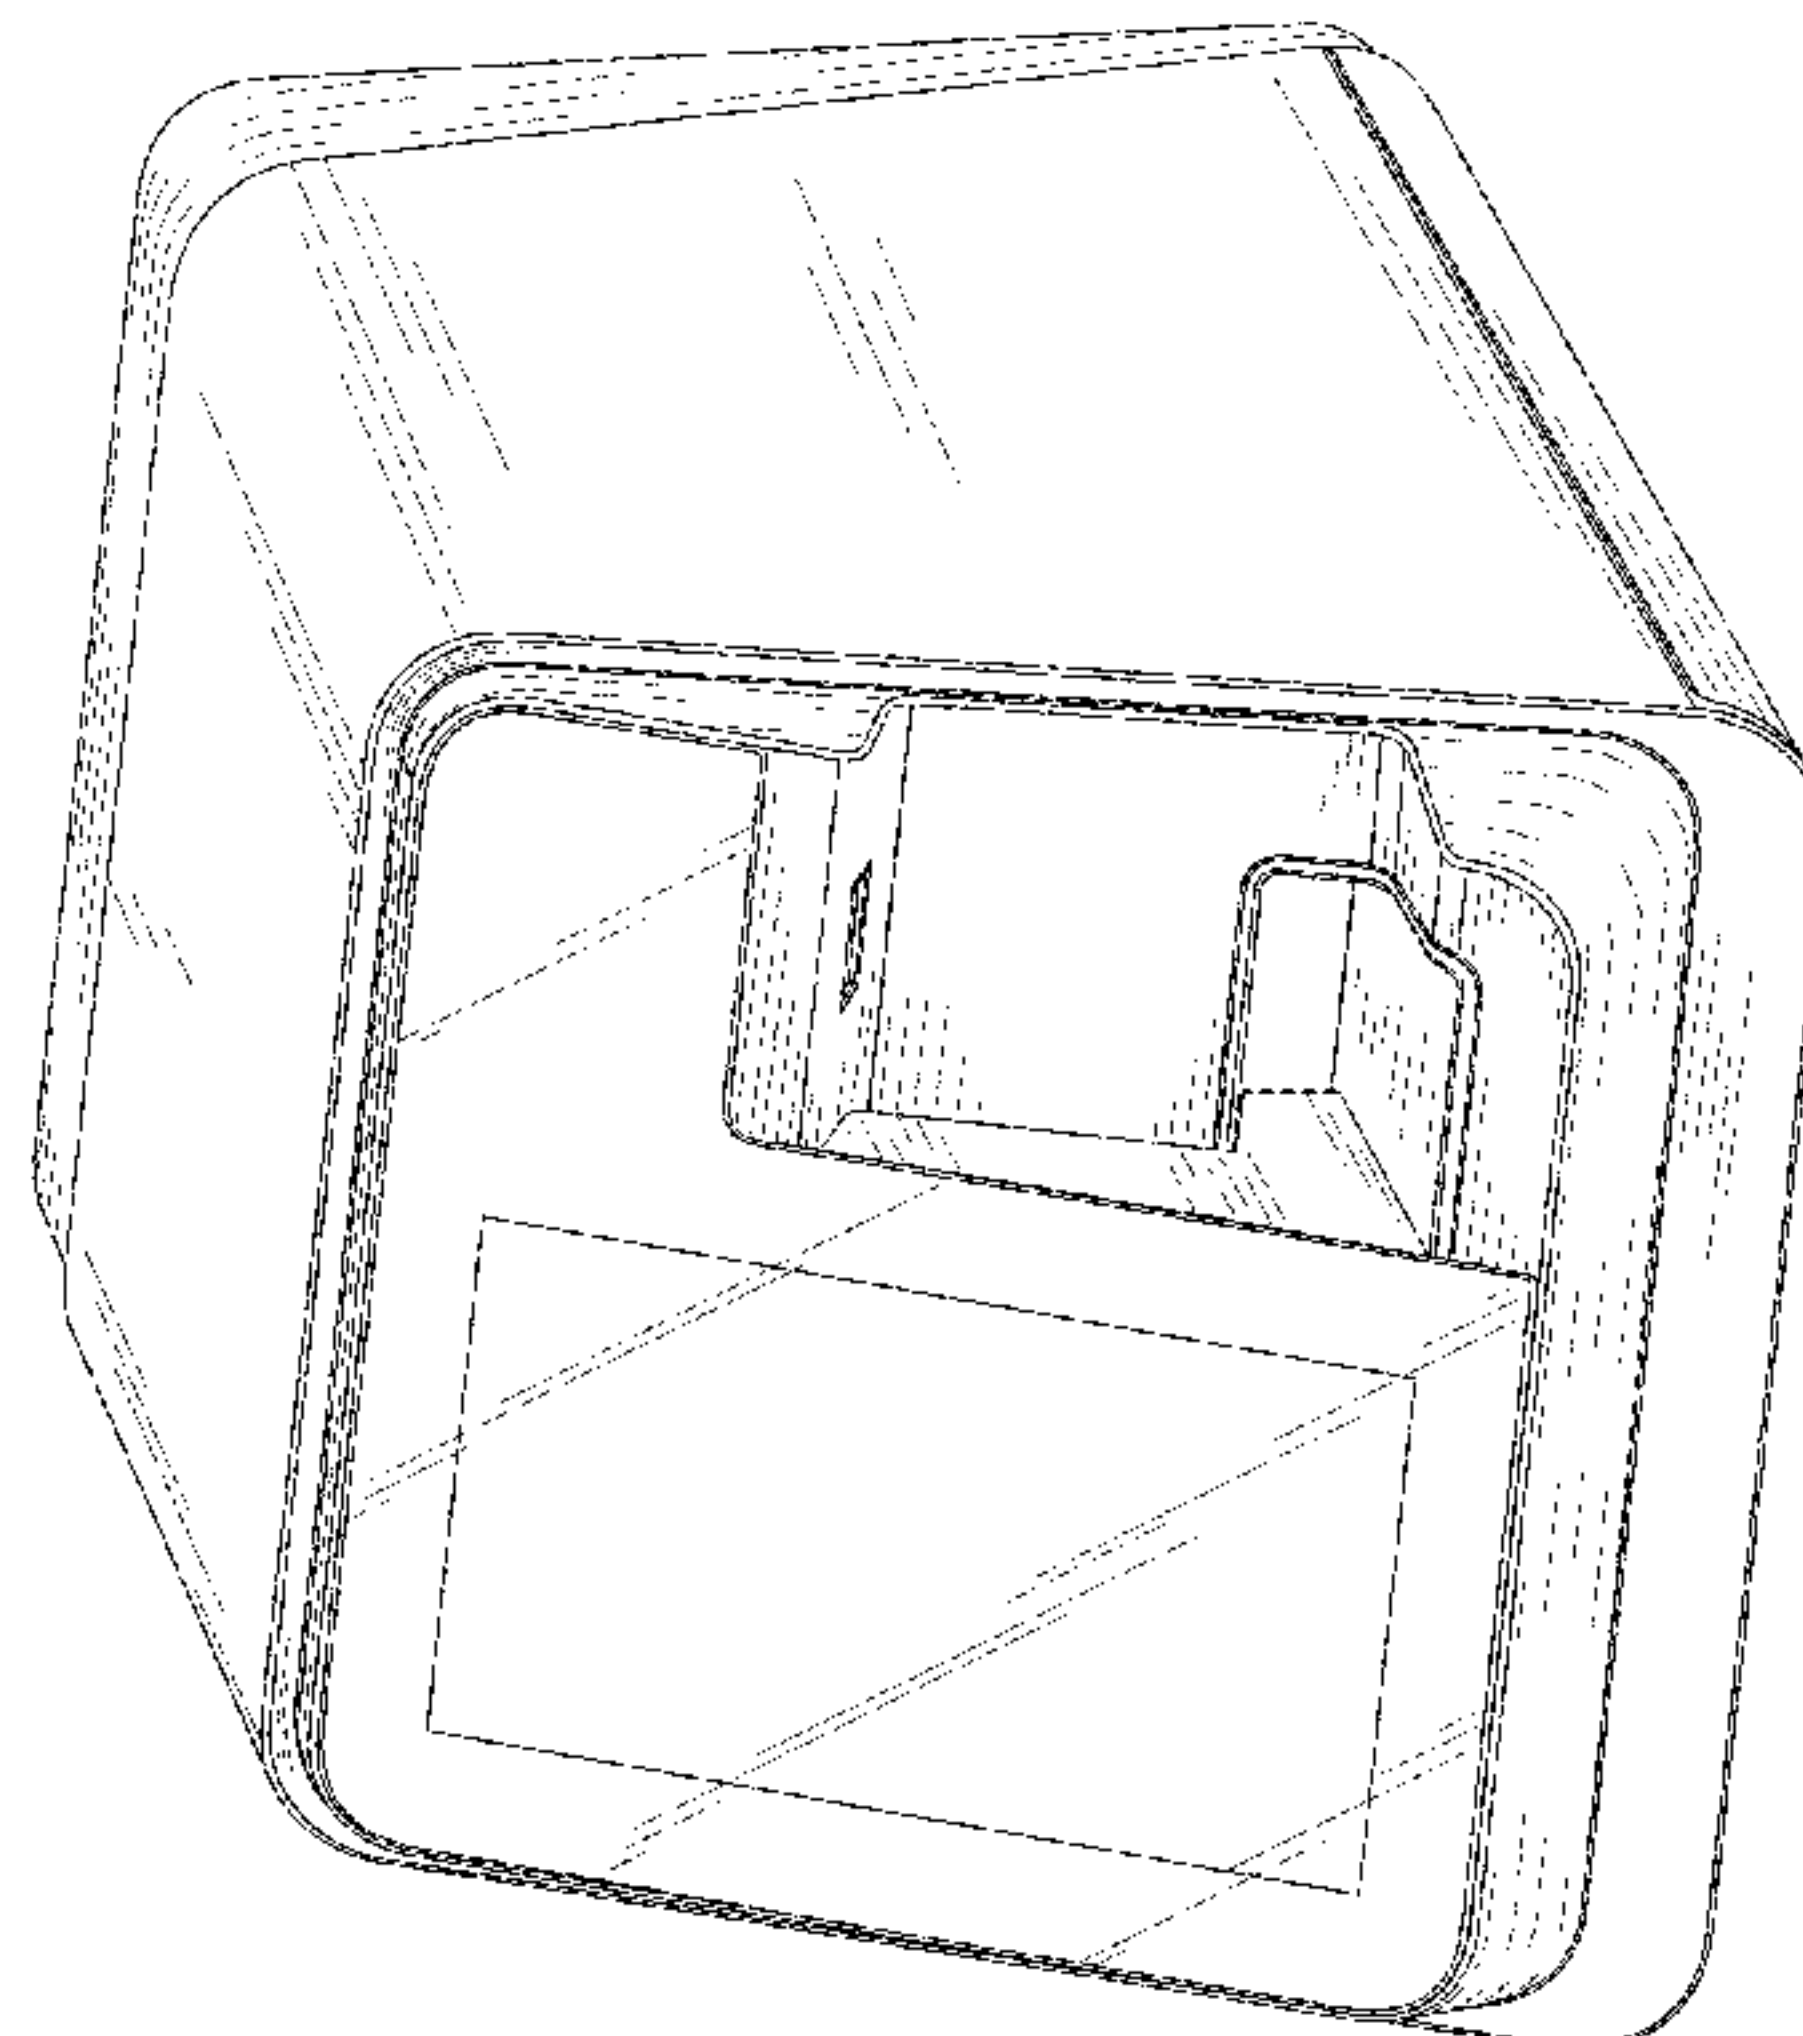

(56)

**References Cited**

U.S. PATENT DOCUMENTS

D704,348 S \* 5/2014 Shibata ..... D24/216  
D707,825 S 6/2014 Murai  
D718,462 S \* 11/2014 Cook ..... D24/216  
9,446,406 B2 9/2016 Gordon et al.  
D774,205 S \* 12/2016 Grace ..... D24/169  
D818,146 S \* 5/2018 Tanaka ..... D24/216  
D821,601 S \* 6/2018 Henderson ..... D24/216  
D827,859 S \* 9/2018 Mathers ..... D24/232  
D830,548 S 10/2018 Kemp  
D833,639 S 11/2018 Peltosaari et al.  
D853,873 S \* 7/2019 Schueren ..... D10/81  
D854,703 S \* 7/2019 Juhlin ..... D24/216  
2012/0227471 A1 \* 9/2012 Smith ..... G01N 35/1011  
73/61.59  
2015/0250456 A1 9/2015 Olgun  
2016/0051415 A1 2/2016 Kuan et al.  
2017/0065971 A1 3/2017 Kreifels et al.

OTHER PUBLICATIONS

Official Action Dated Nov. 26, 2019 From the US Patent and  
Trademark Office Re. U.S. Appl. No. 29/662,120. (13 pages).

\* cited by examiner

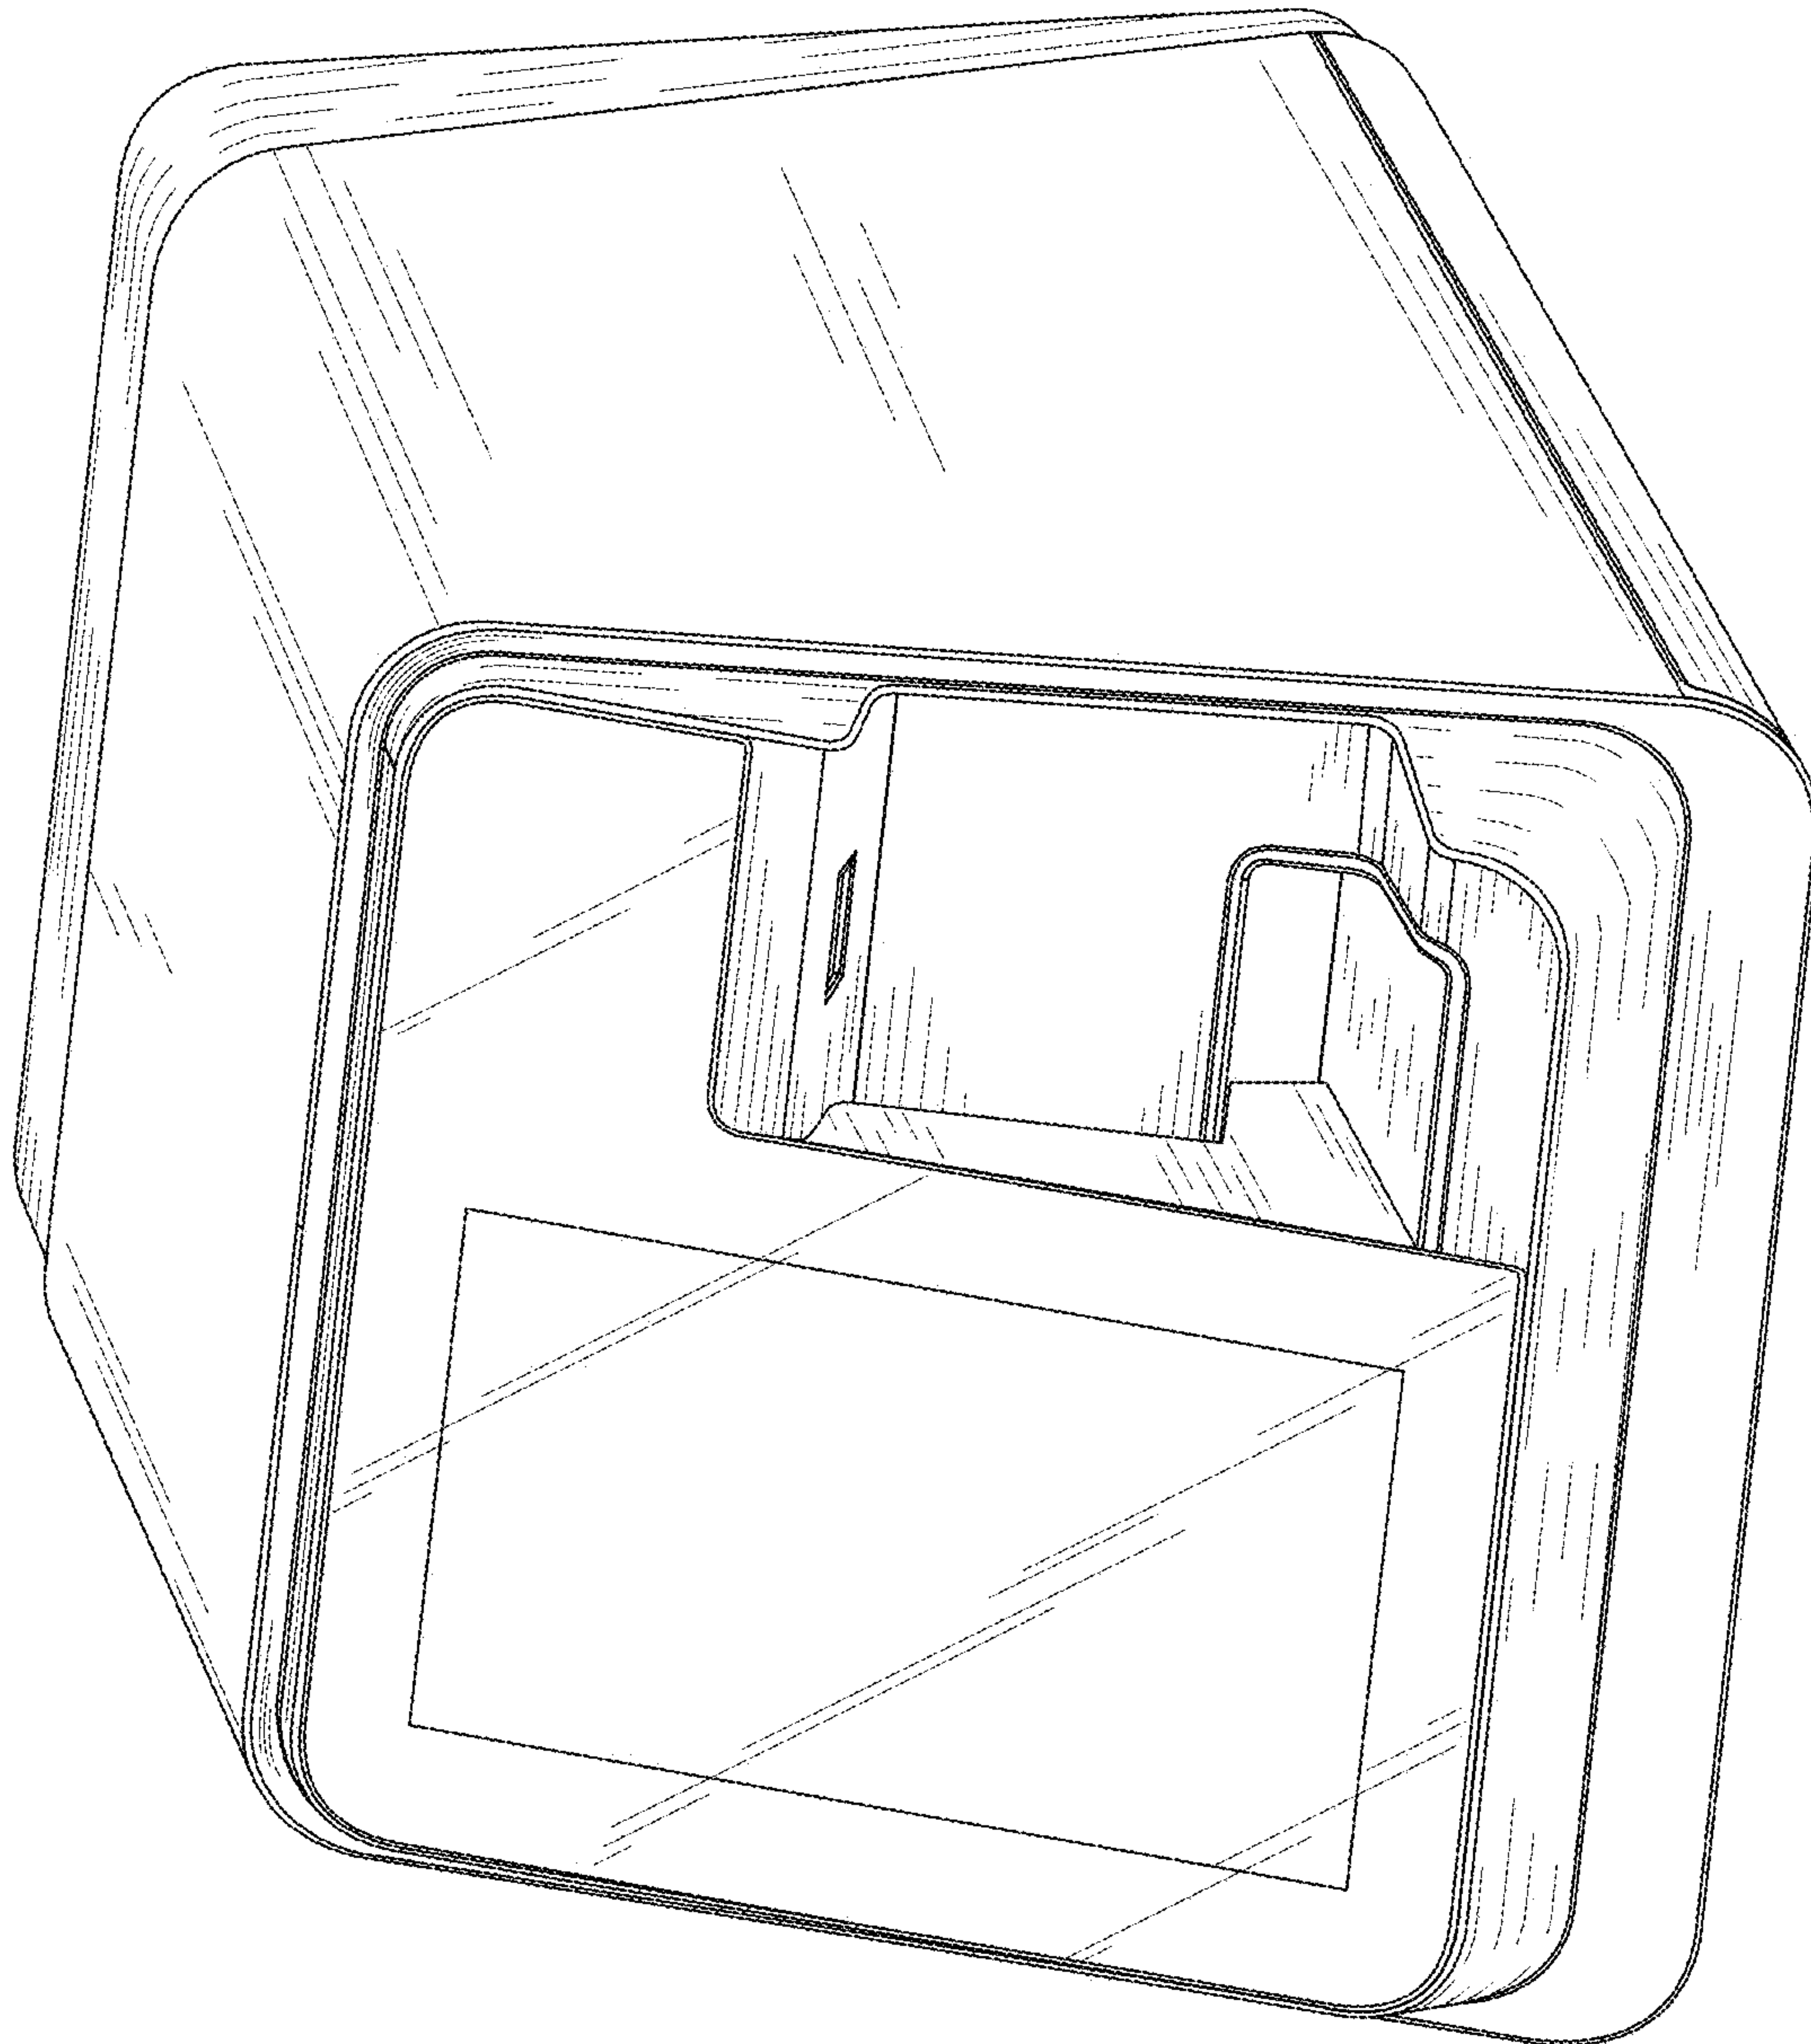


FIG. 1



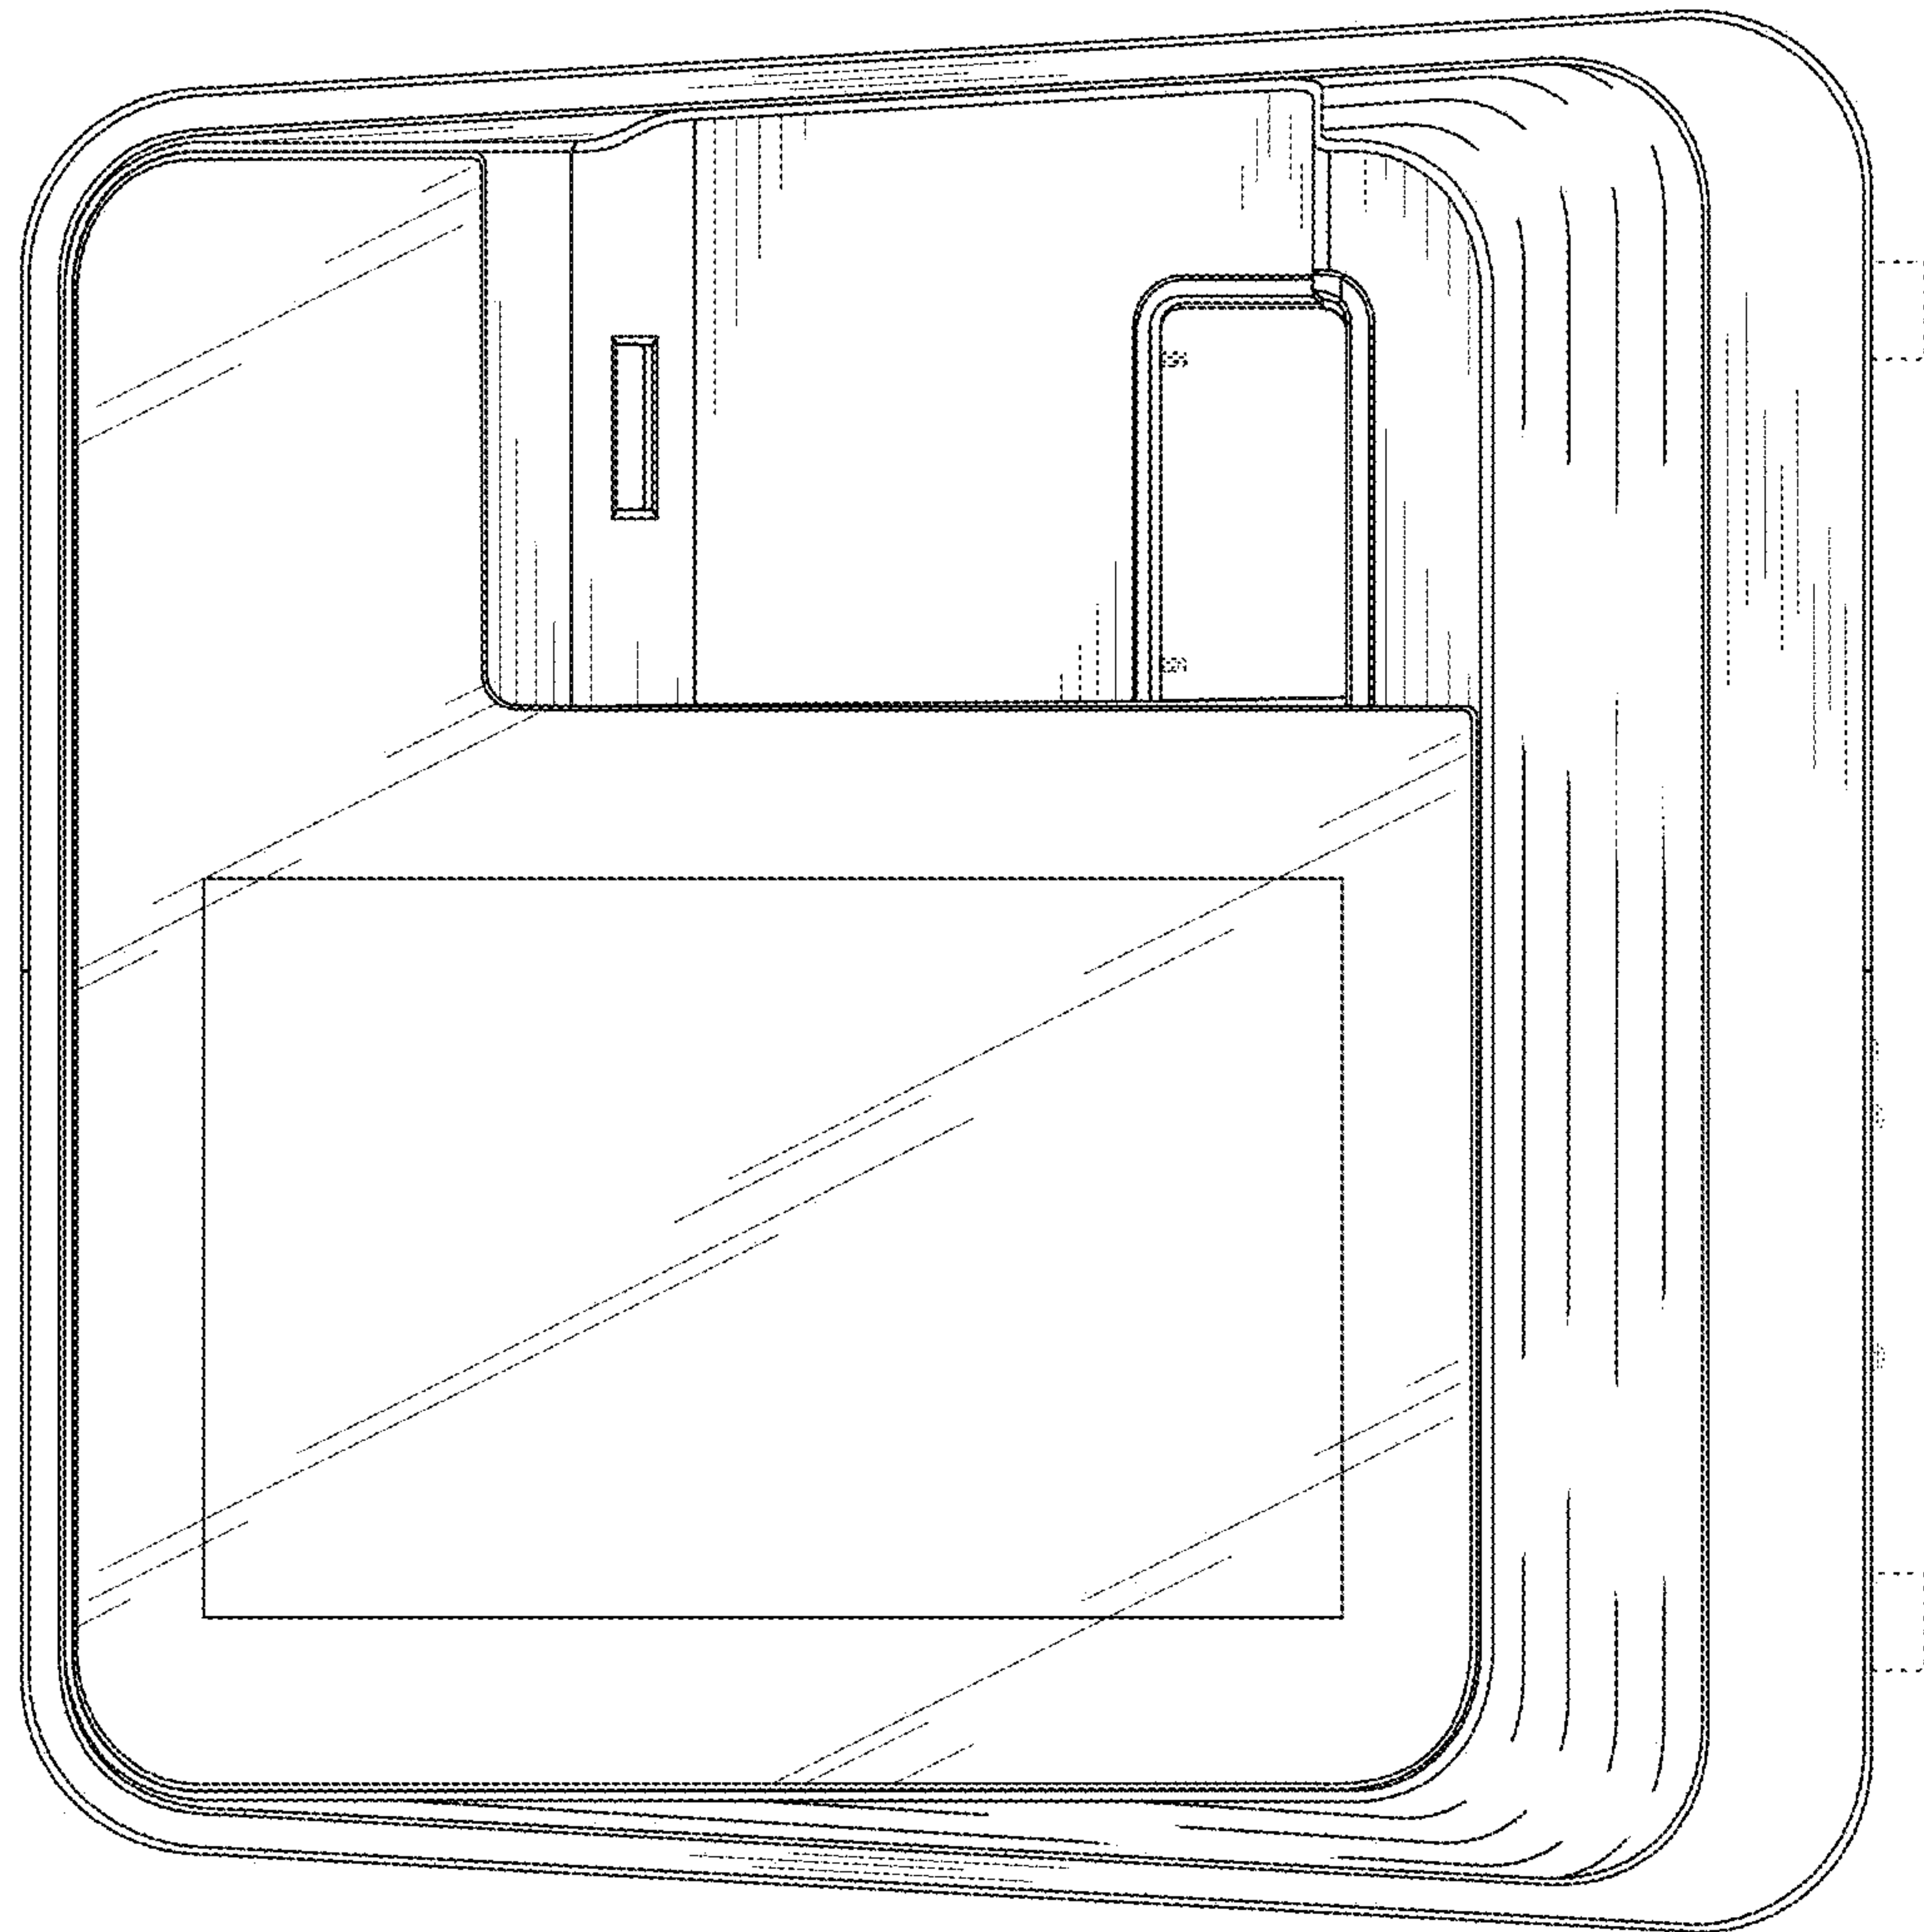


FIG. 2

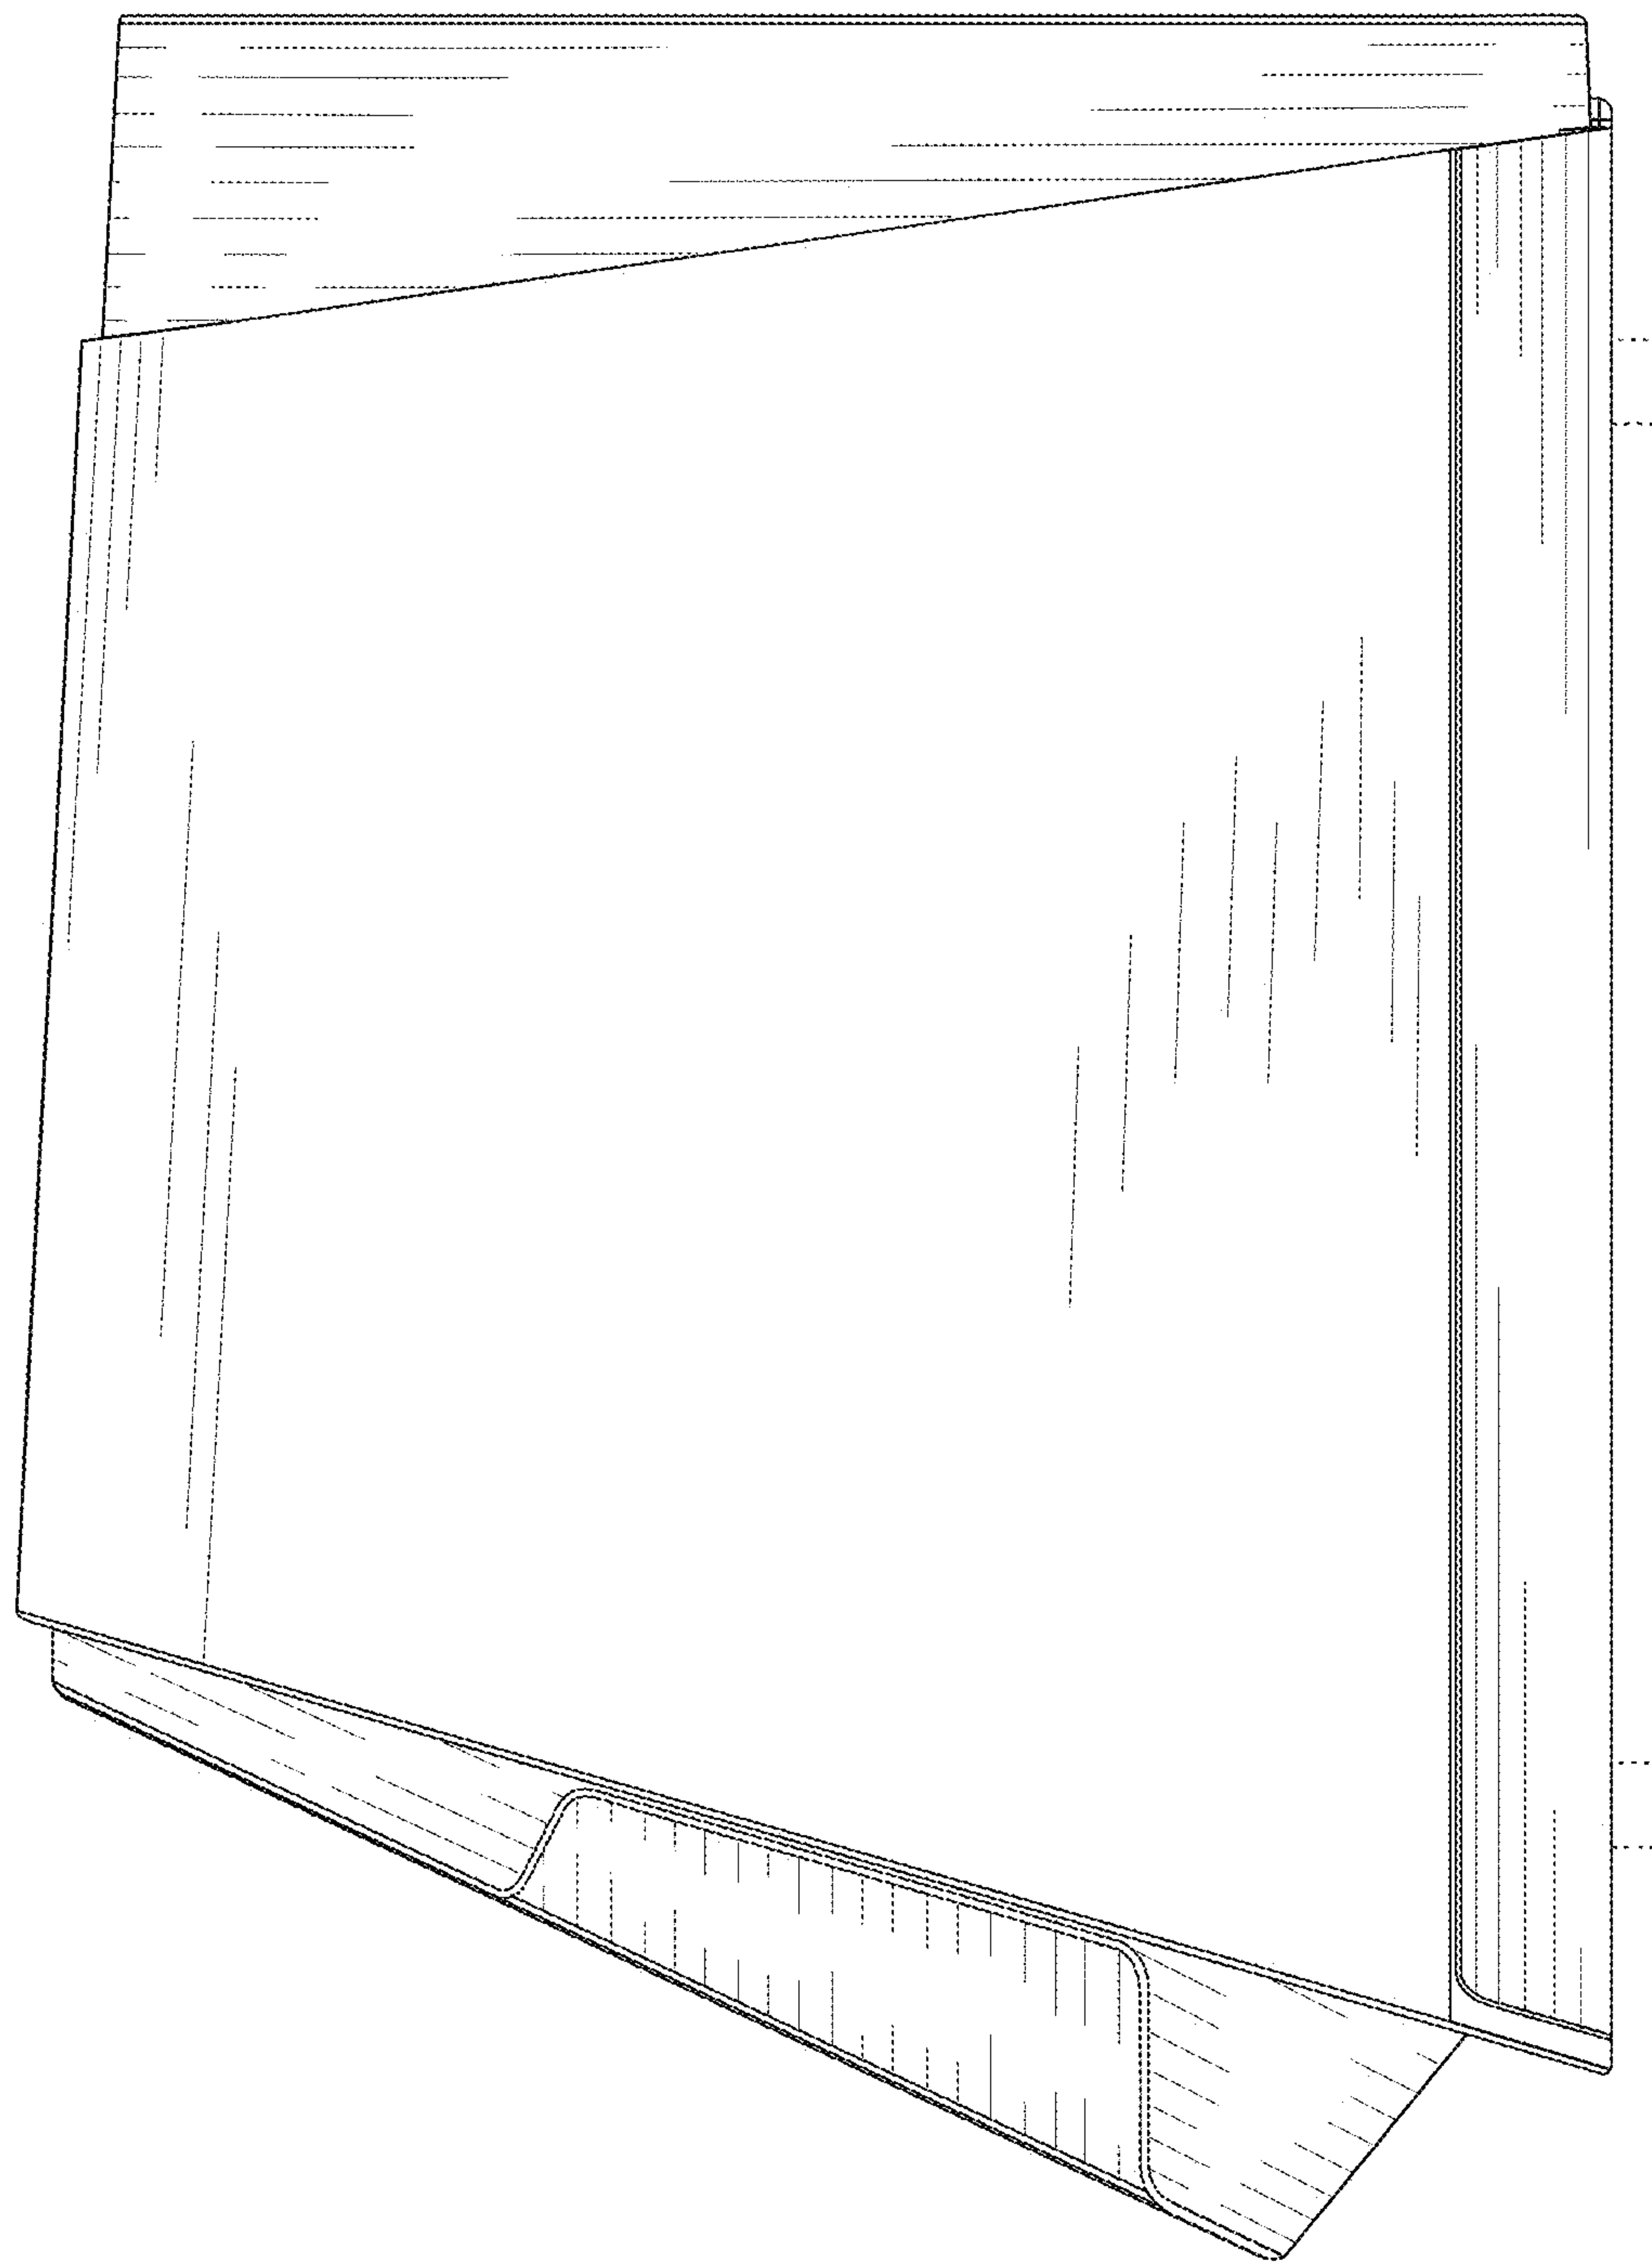


FIG. 3

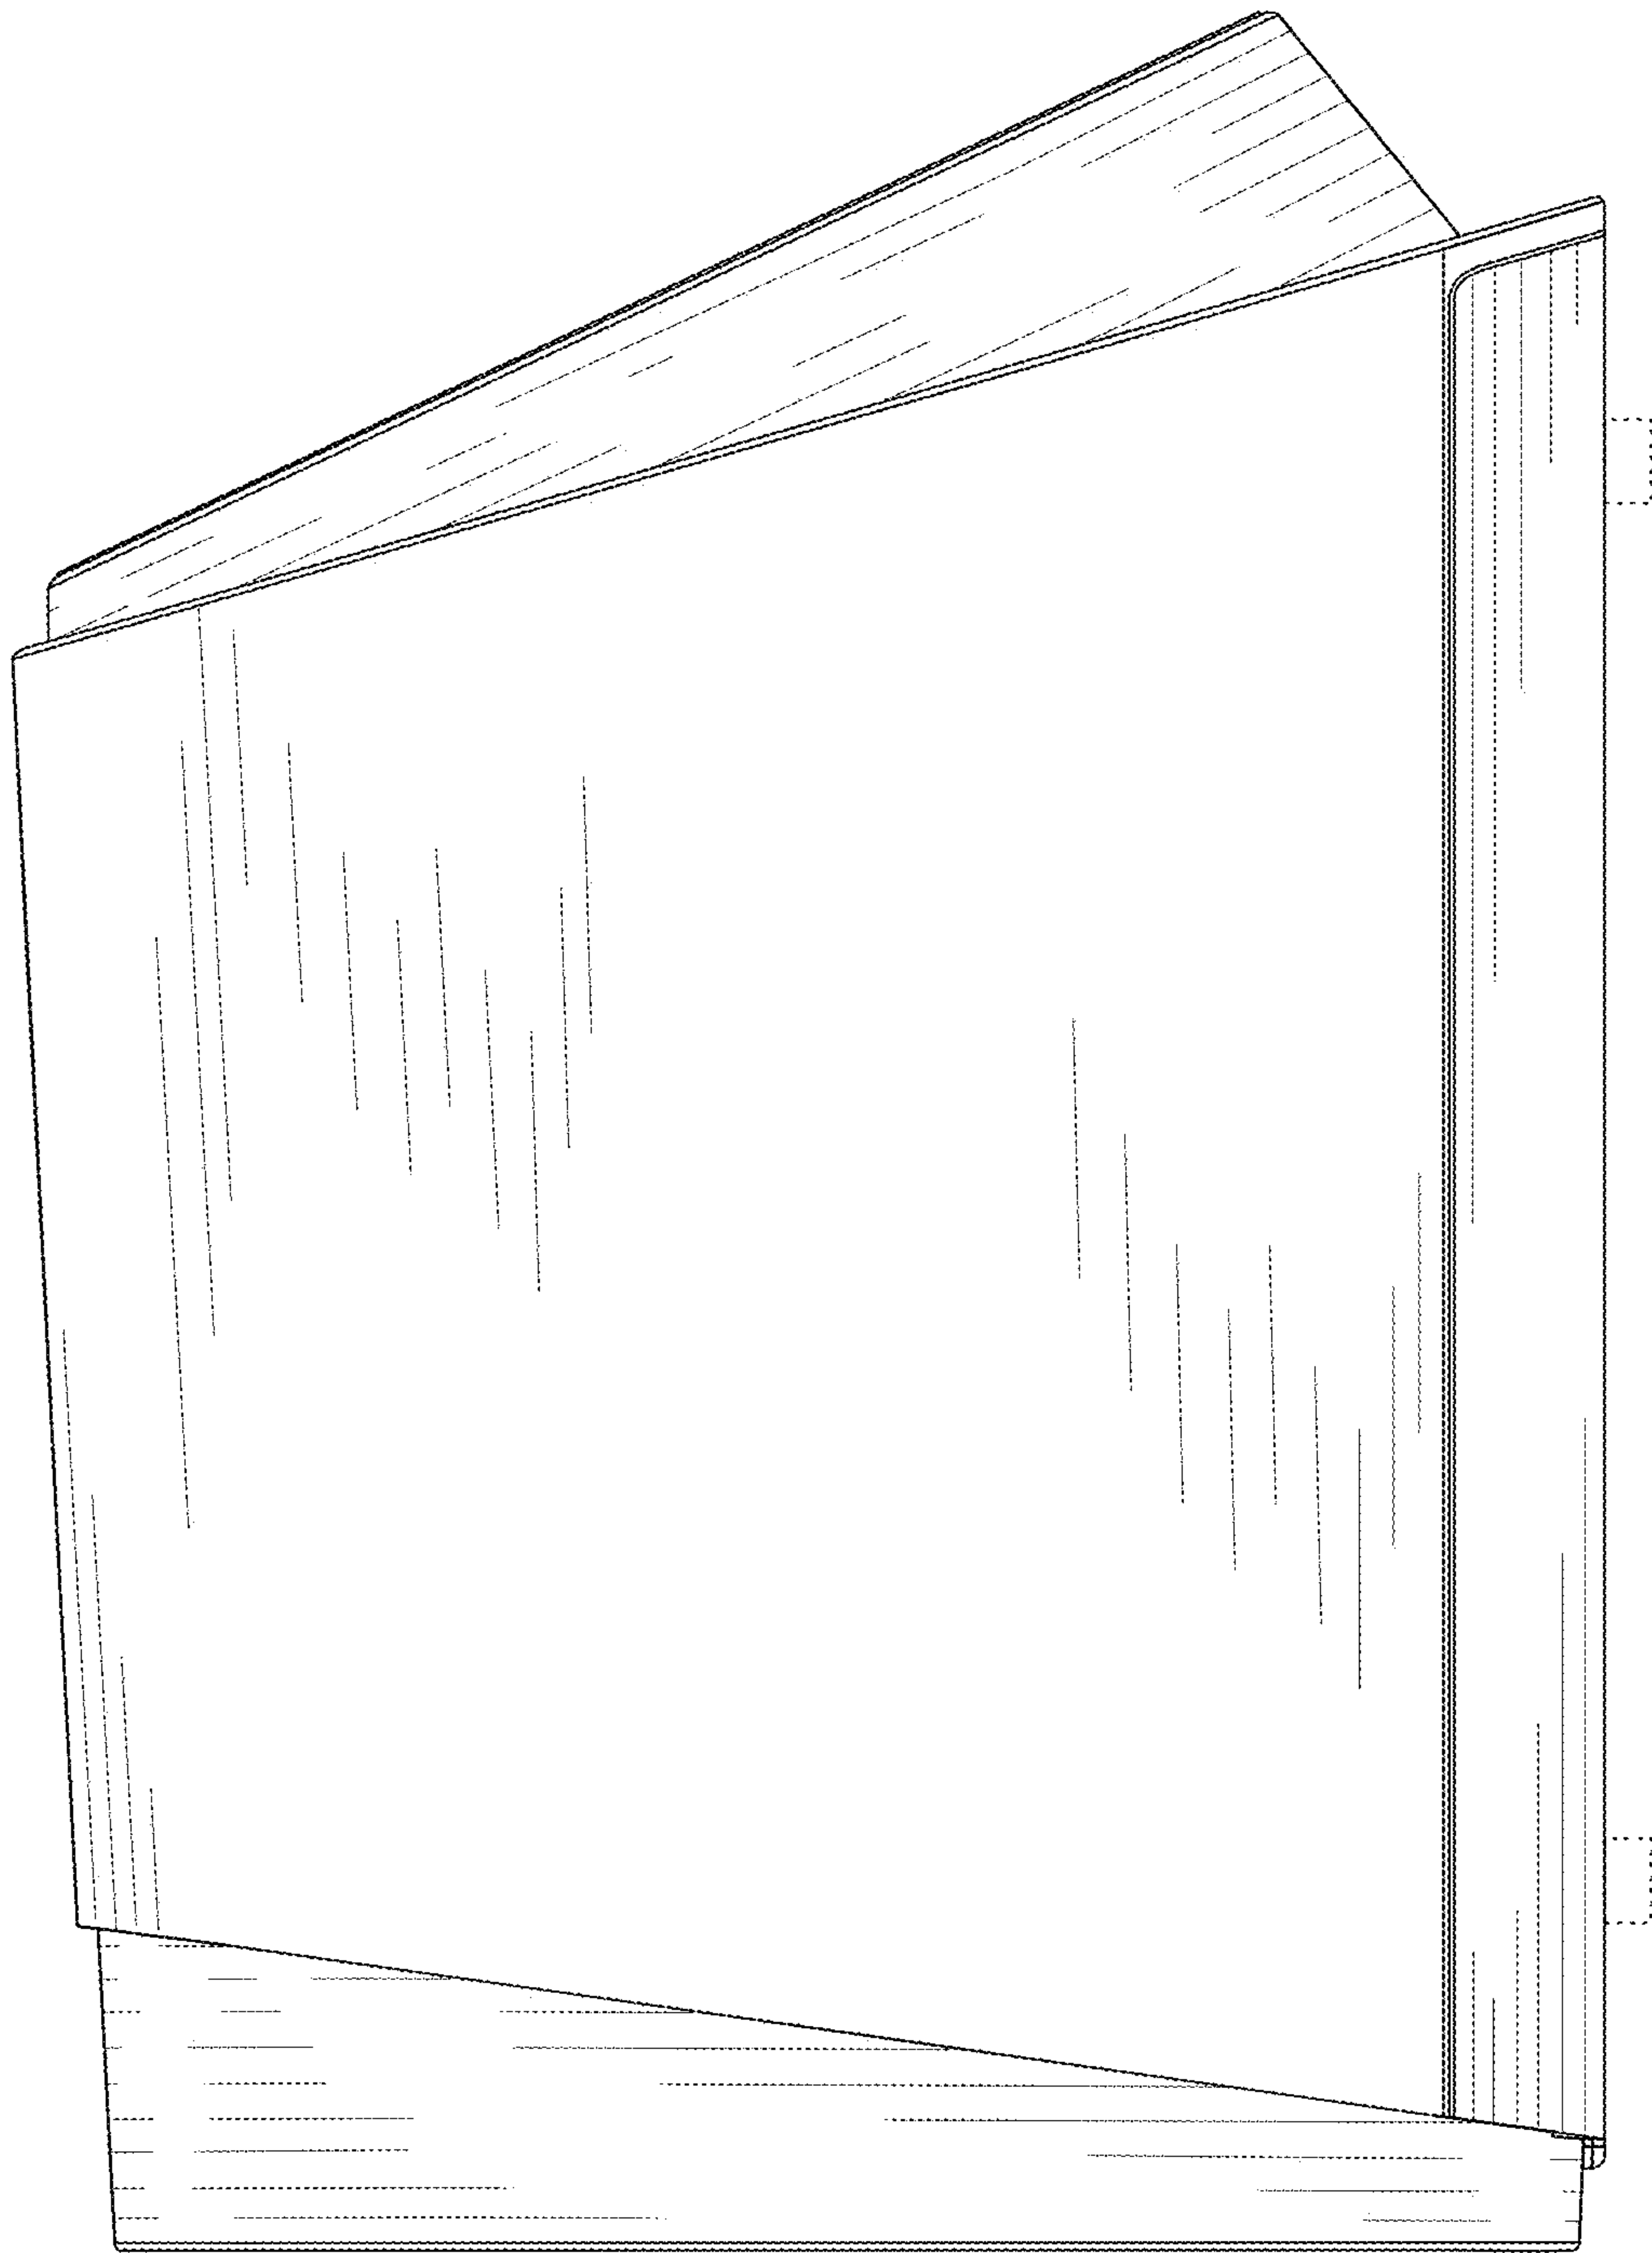


FIG. 4

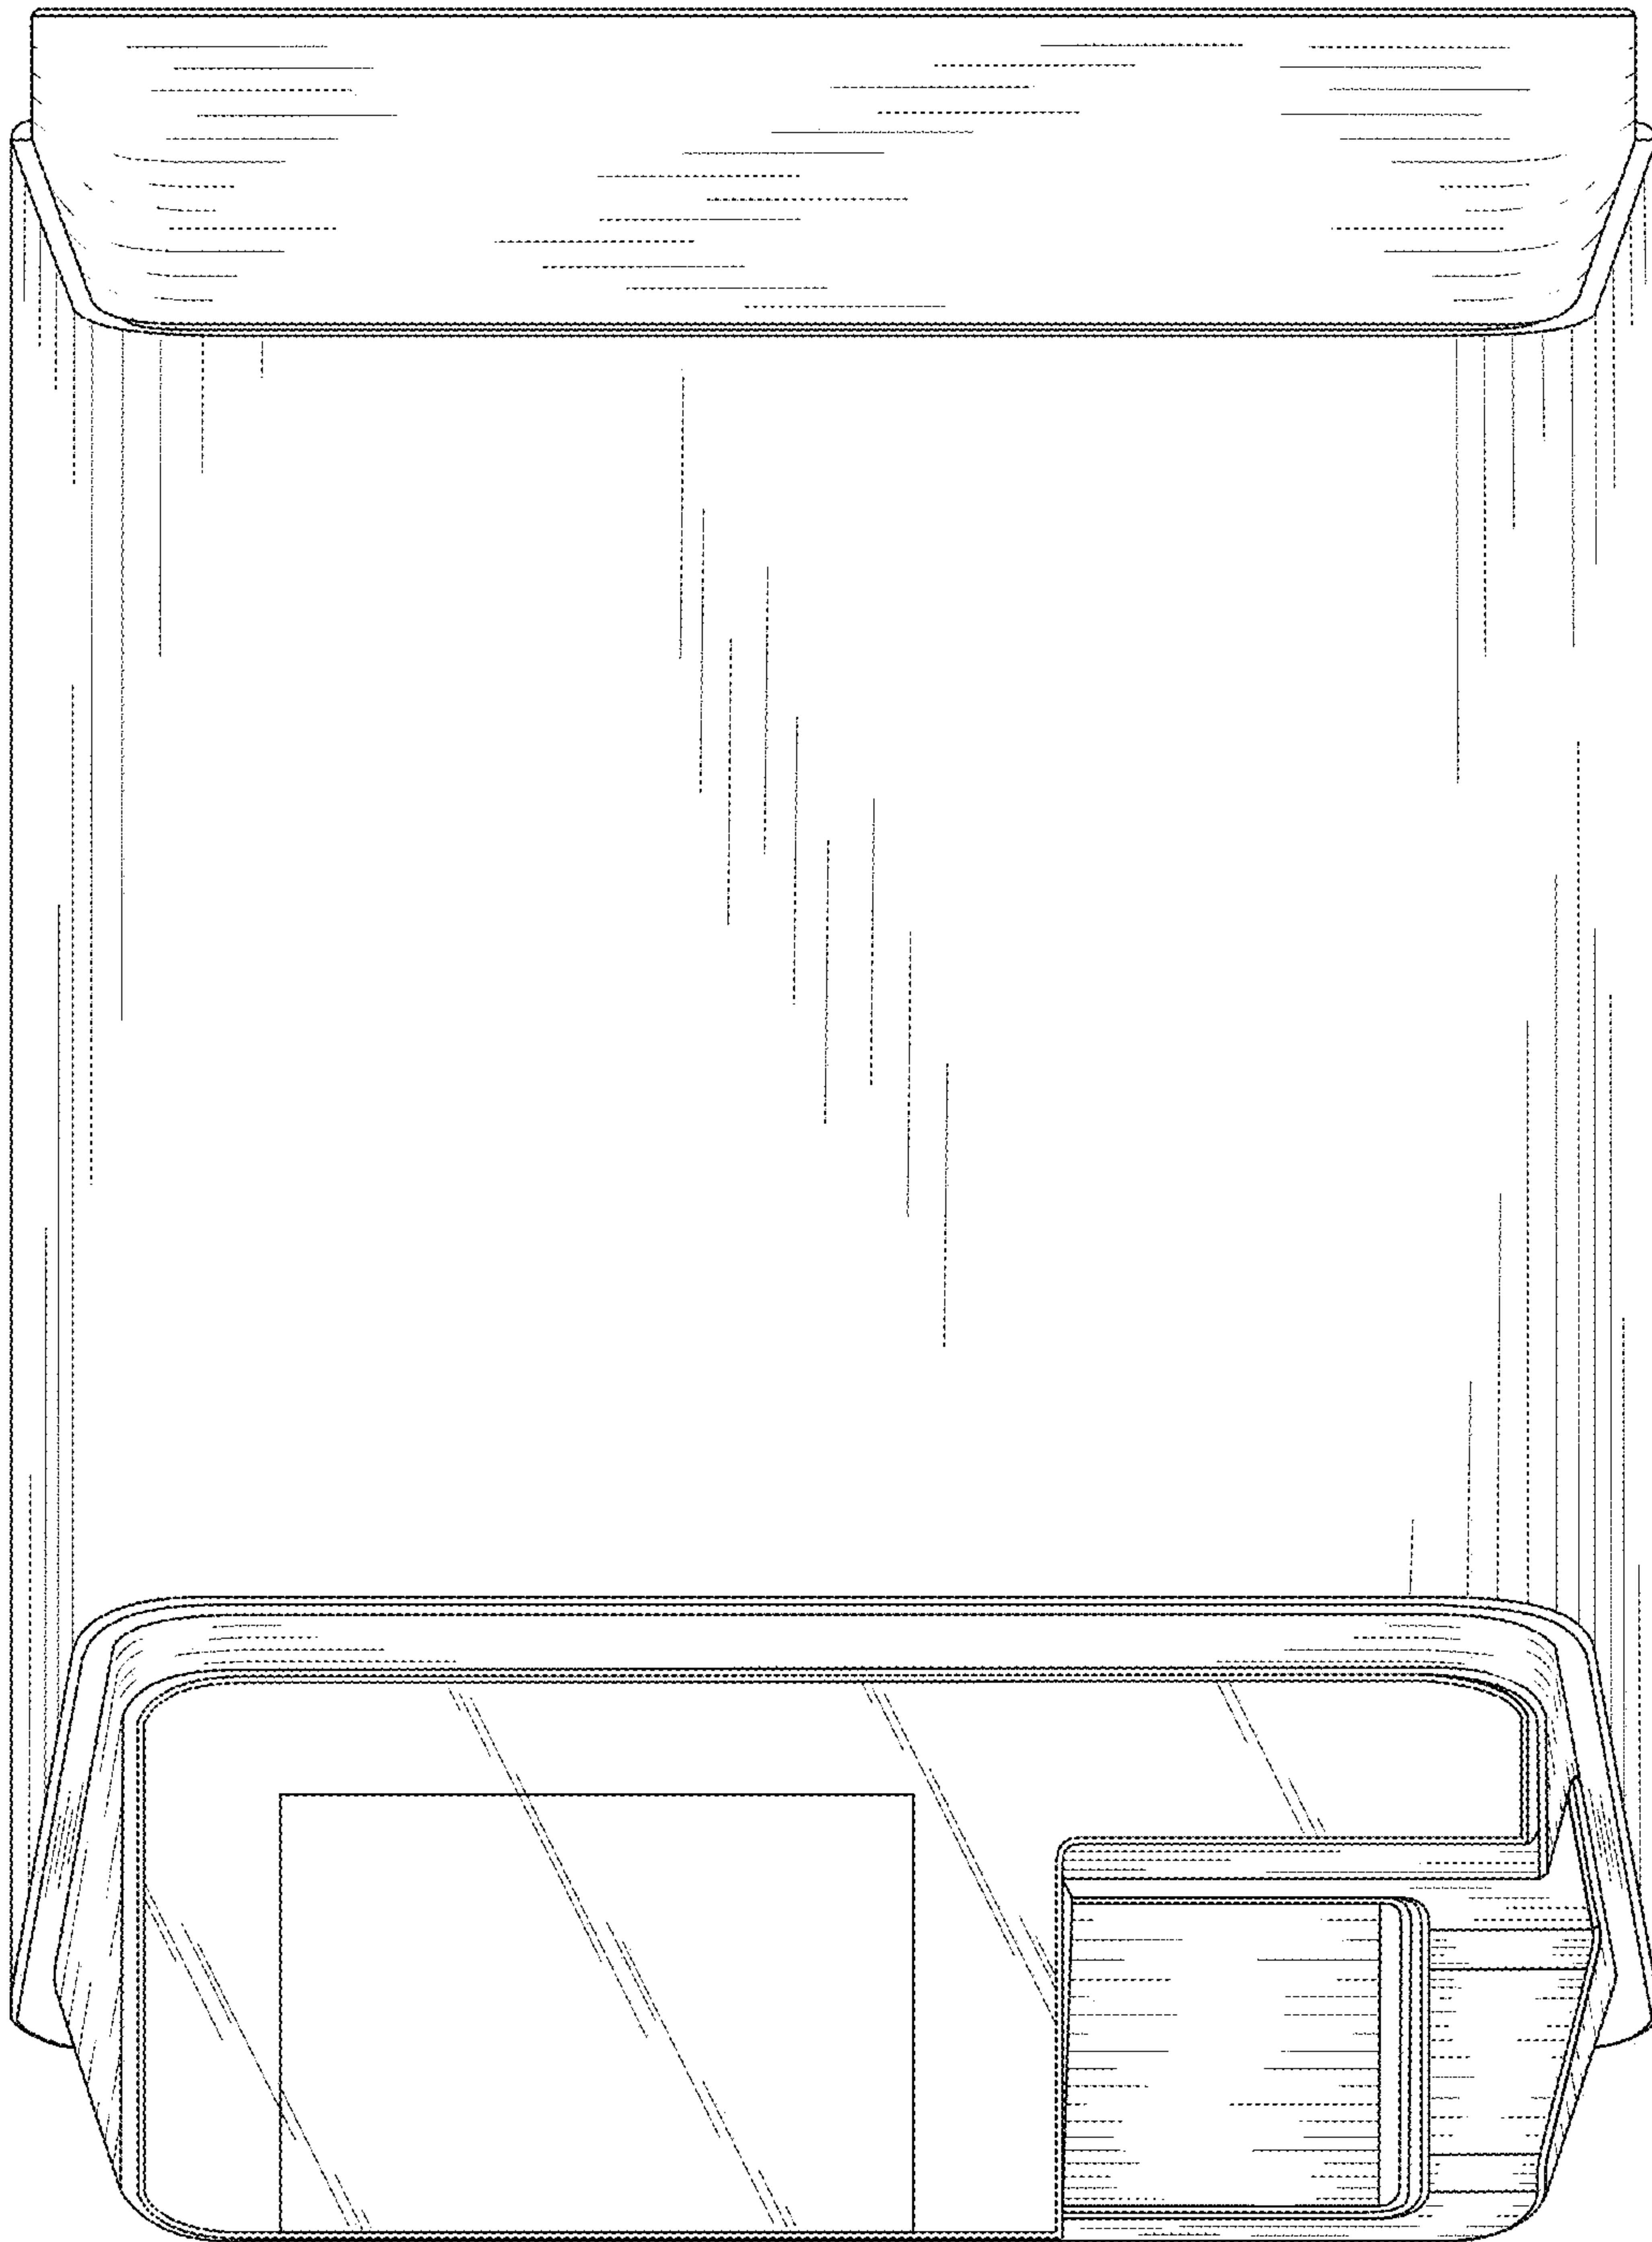


FIG. 5



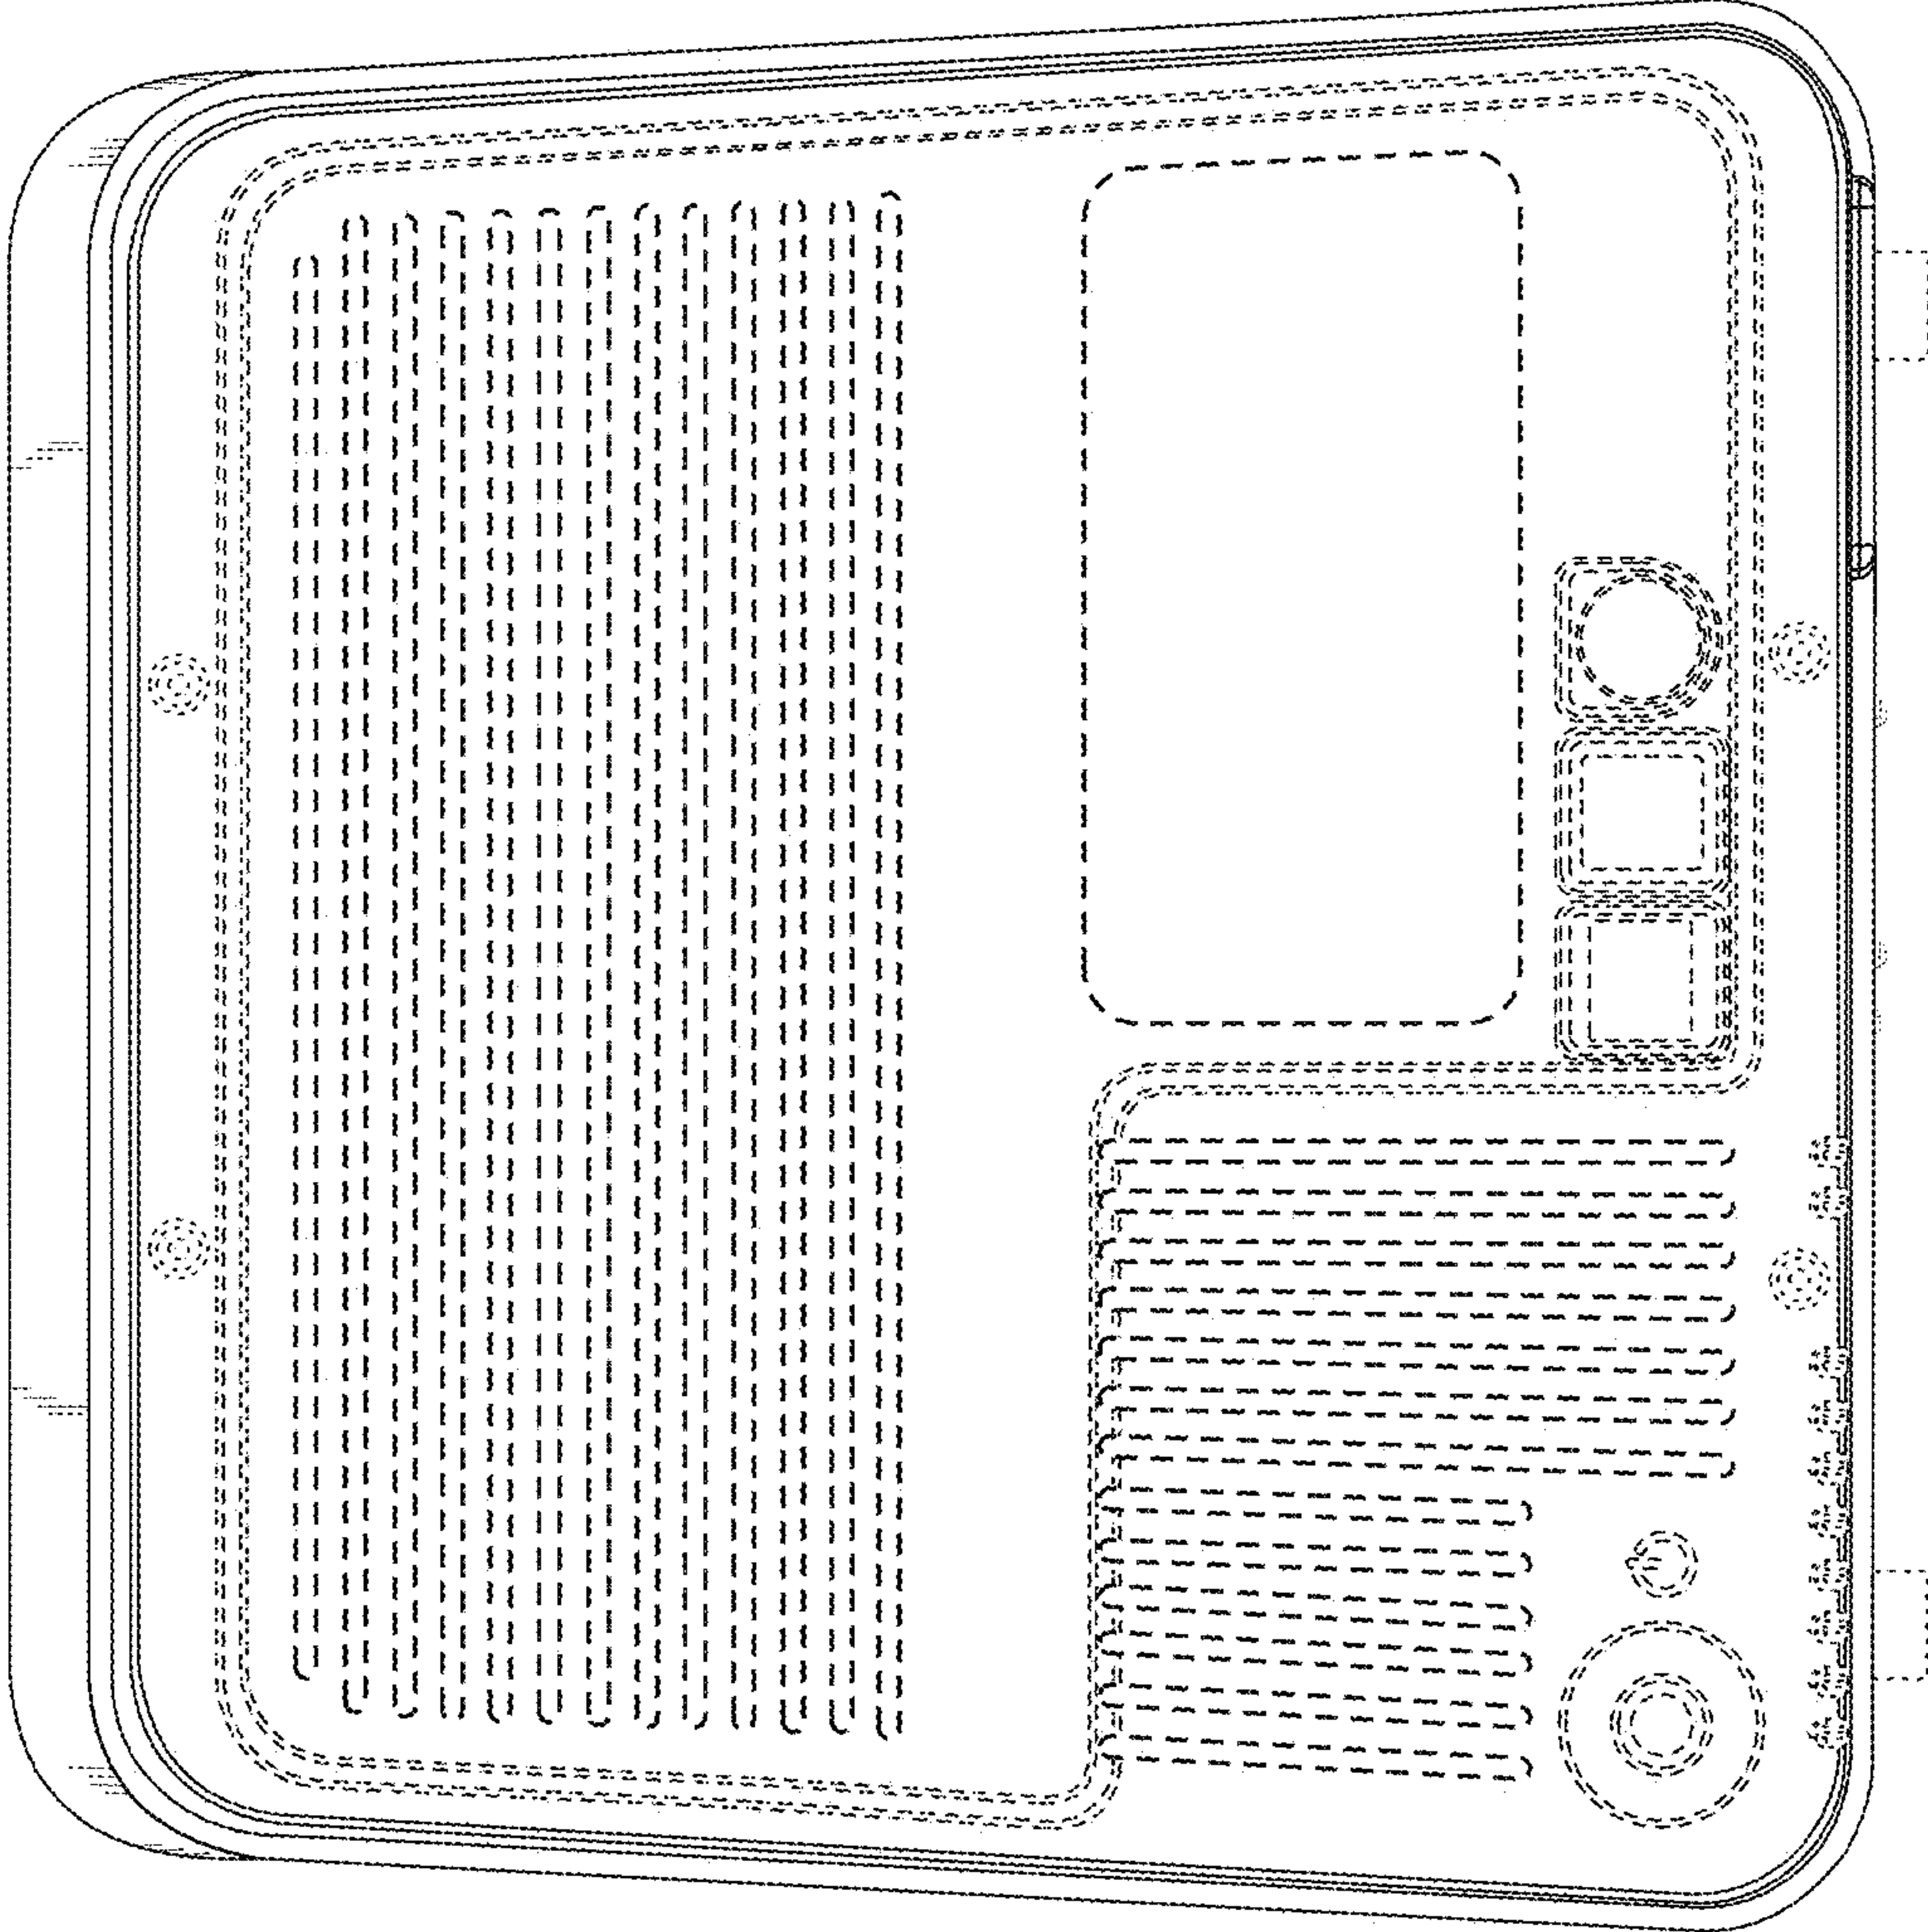


FIG. 6



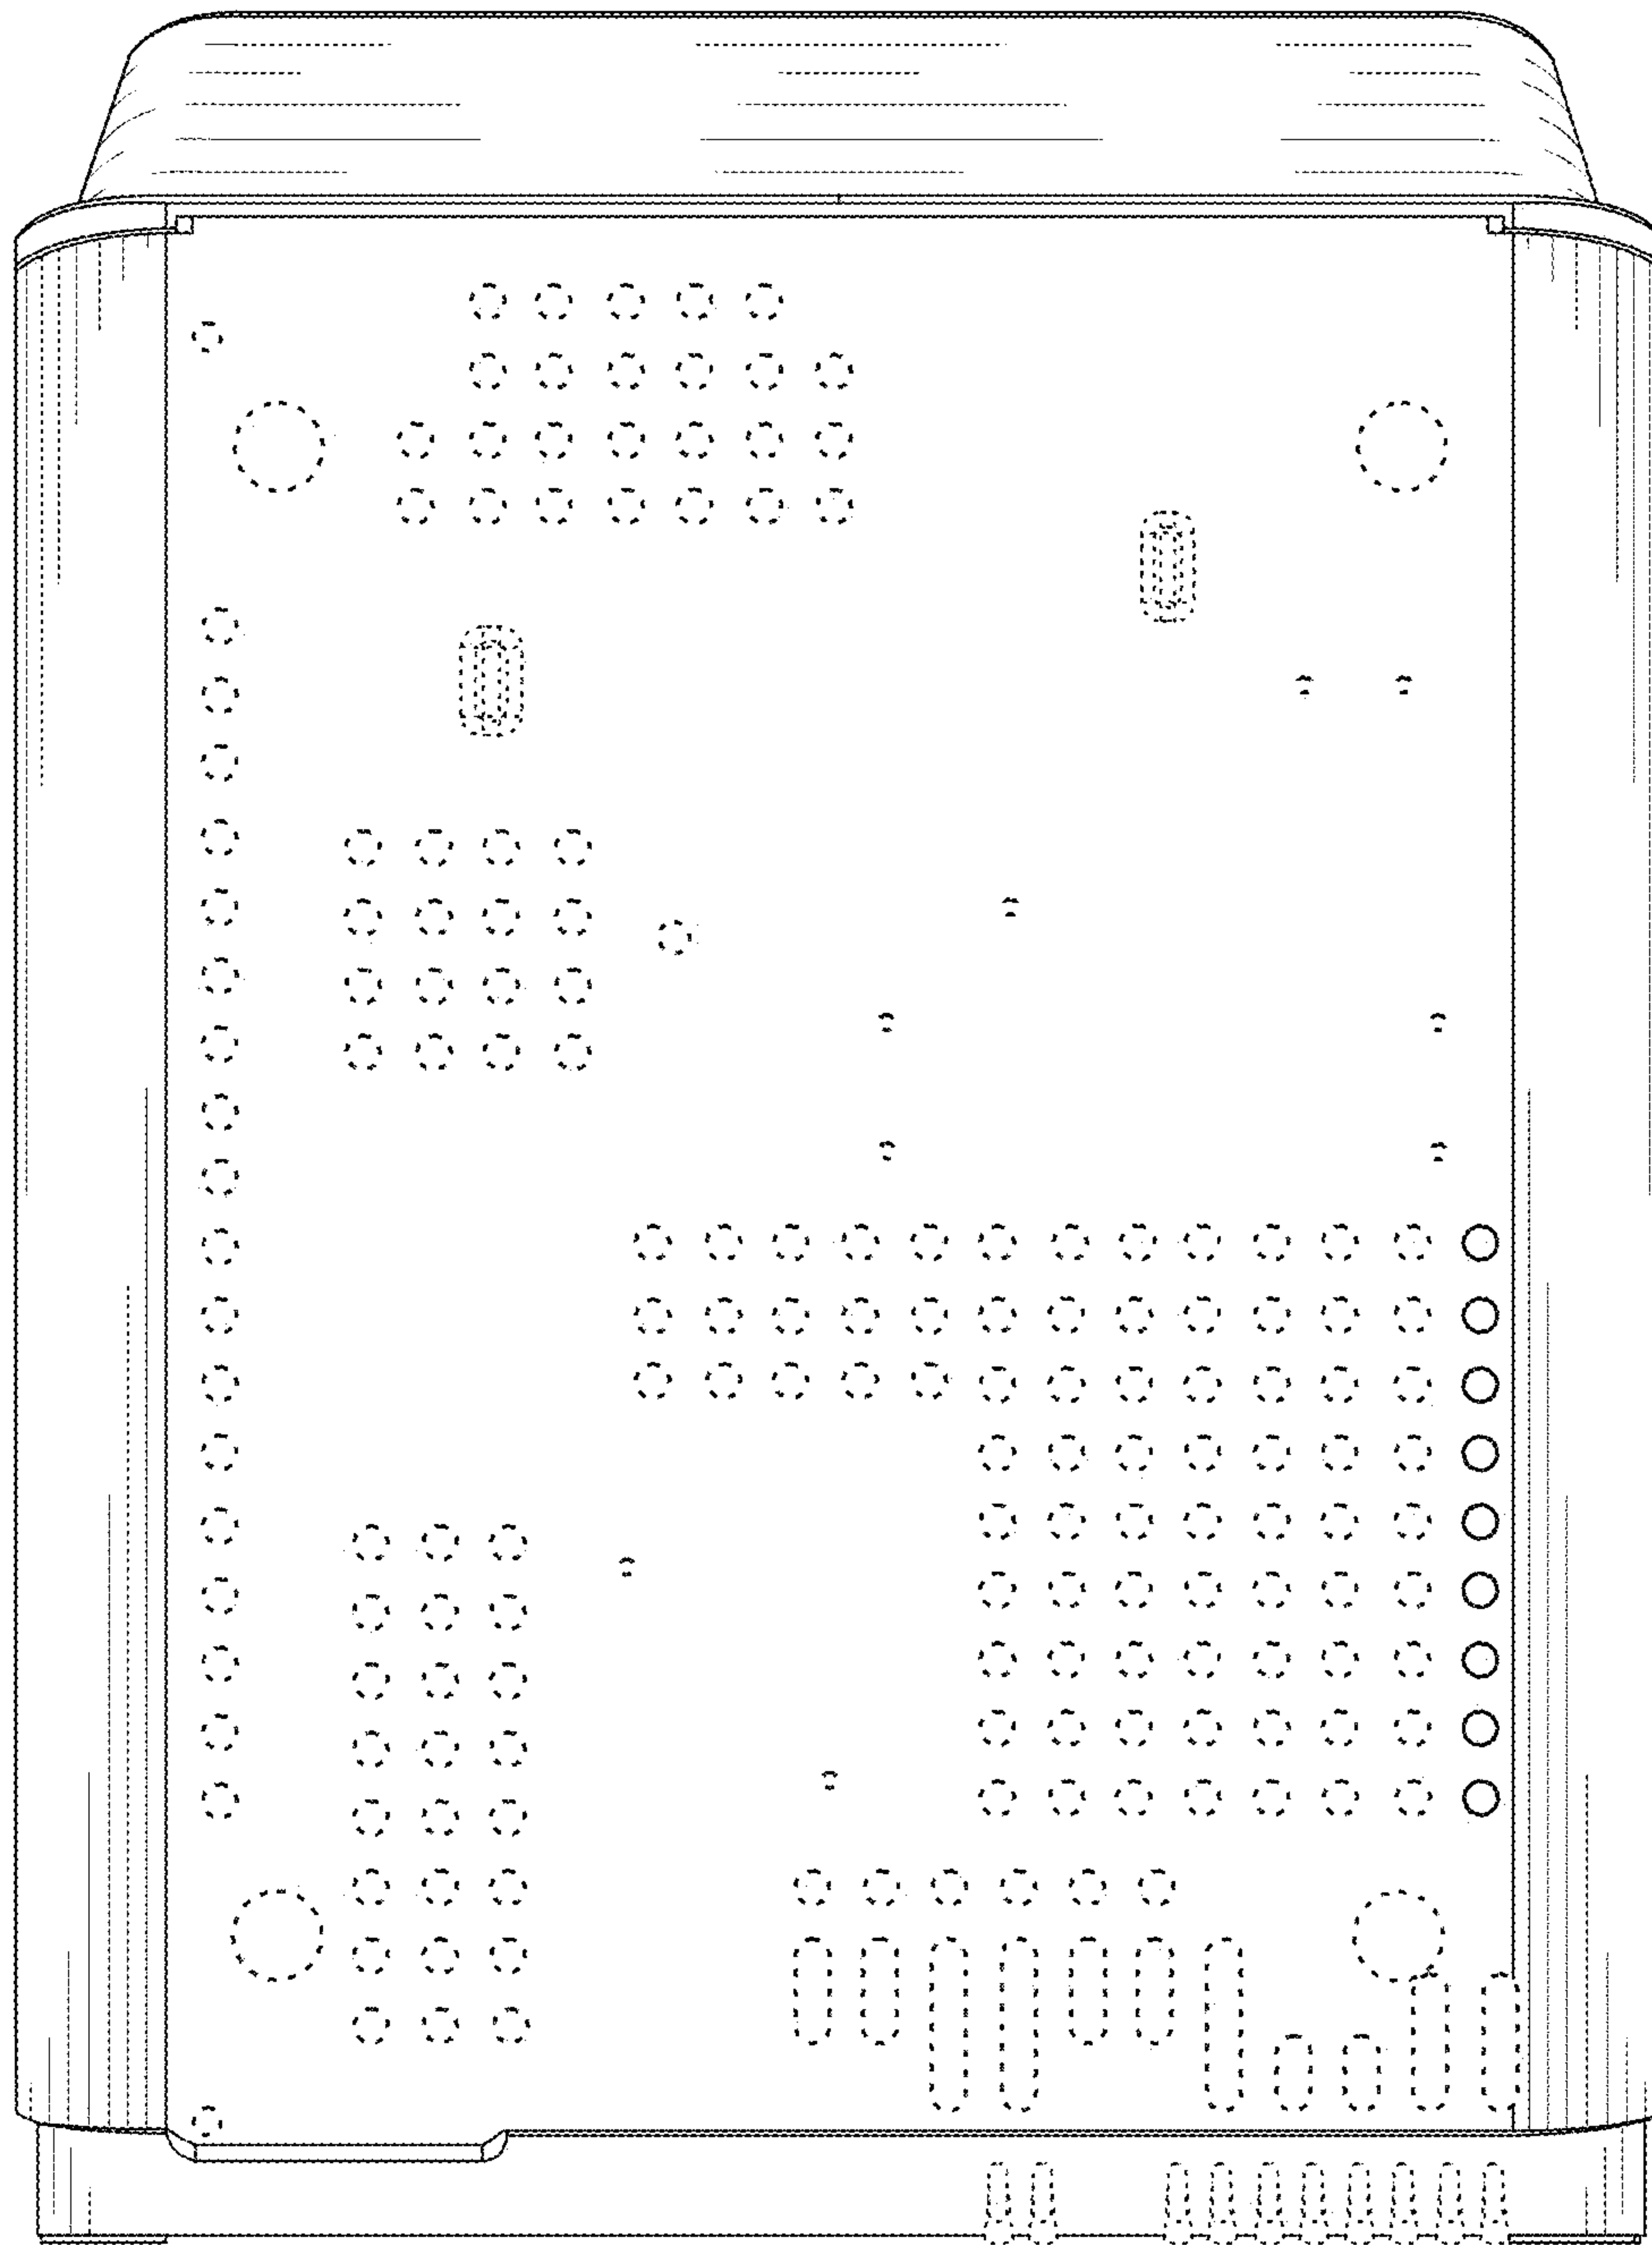


FIG. 7