



US00D889634S

(12) **United States Design Patent** (10) **Patent No.:** **US D889,634 S**
Tuononen et al. (45) **Date of Patent:** **** Jul. 7, 2020**

(54) **PRESSURE CONTROL UNIT** 5,029,579 A 7/1991 Trammell
5,425,742 A 6/1995 Joy
(71) Applicant: **OTIVIO AS**, Oslo (NO) 5,458,562 A 10/1995 Cooper
(Continued)

(72) Inventors: **Sanna Tuononen**, Oslo (NO); **Petri Rantanen**, Oslo (NO)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **OTIVIO AS**, Oslo (NO)

EM 0026509370001 3/2015
EM 0026509370002 3/2015

(**) Term: **15 Years**

(Continued)

(21) Appl. No.: **29/659,685**

OTHER PUBLICATIONS

(22) Filed: **Aug. 10, 2018**

FlowOx First Time Assembly Instructional Video. Posted by Otivio AS on YouTube.com. Date published: Apr. 3, 2019. Retrieved from Internet: https://www.youtube.com/watch?v=2VVStprMr28&feature=emb_logo (Year: 2019).*

(51) **LOC (12) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/107; D24/188**

(Continued)

(58) **Field of Classification Search**
USPC D24/107, 108, 111, 169, 185, 186, 188, D24/200, 213
CPC A61M 2205/3344; A61H 2209/00; A61H 1/00; A61H 9/00

Primary Examiner — Lilyana Bekic
(74) *Attorney, Agent, or Firm* — Workman Nydegger

See application file for complete search history.

(57) **CLAIM**

(56) **References Cited**

The ornamental design for a pressure control unit, as shown and described.


U.S. PATENT DOCUMENTS

| | | |
|-------------|---------|-----------------|
| 1,110,494 A | 9/1914 | Kellogg |
| 1,399,095 A | 12/1921 | Webb |
| 2,113,253 A | 4/1938 | Gray |
| 2,168,611 A | 8/1939 | Thompson |
| 3,094,983 A | 6/1963 | MacLeod |
| 3,292,613 A | 12/1966 | MacLeod |
| 3,403,673 A | 10/1968 | MacLeod |
| 3,465,748 A | 9/1969 | Kravchenko |
| 3,654,919 A | 4/1972 | Birtwell |
| 3,757,806 A | 9/1973 | Bhaskar et al. |
| 3,859,989 A | 1/1975 | Spielberg |
| 3,878,839 A | 4/1975 | Norton et al. |
| 3,896,794 A | 7/1975 | McGrath |
| 3,977,396 A | 8/1976 | Cartier |
| 4,054,129 A | 10/1977 | Byars et al. |
| 4,149,529 A | 4/1979 | Copeland et al. |
| 5,000,164 A | 3/1991 | Cooper |

DESCRIPTION

FIG. 1 is a front perspective view of a pressure control unit showing our new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear elevational view thereof;
FIG. 4 is a right side elevational view thereof;
FIG. 5 is a left side elevational view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The broken lines in the drawings depict portions of the pressure control unit that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

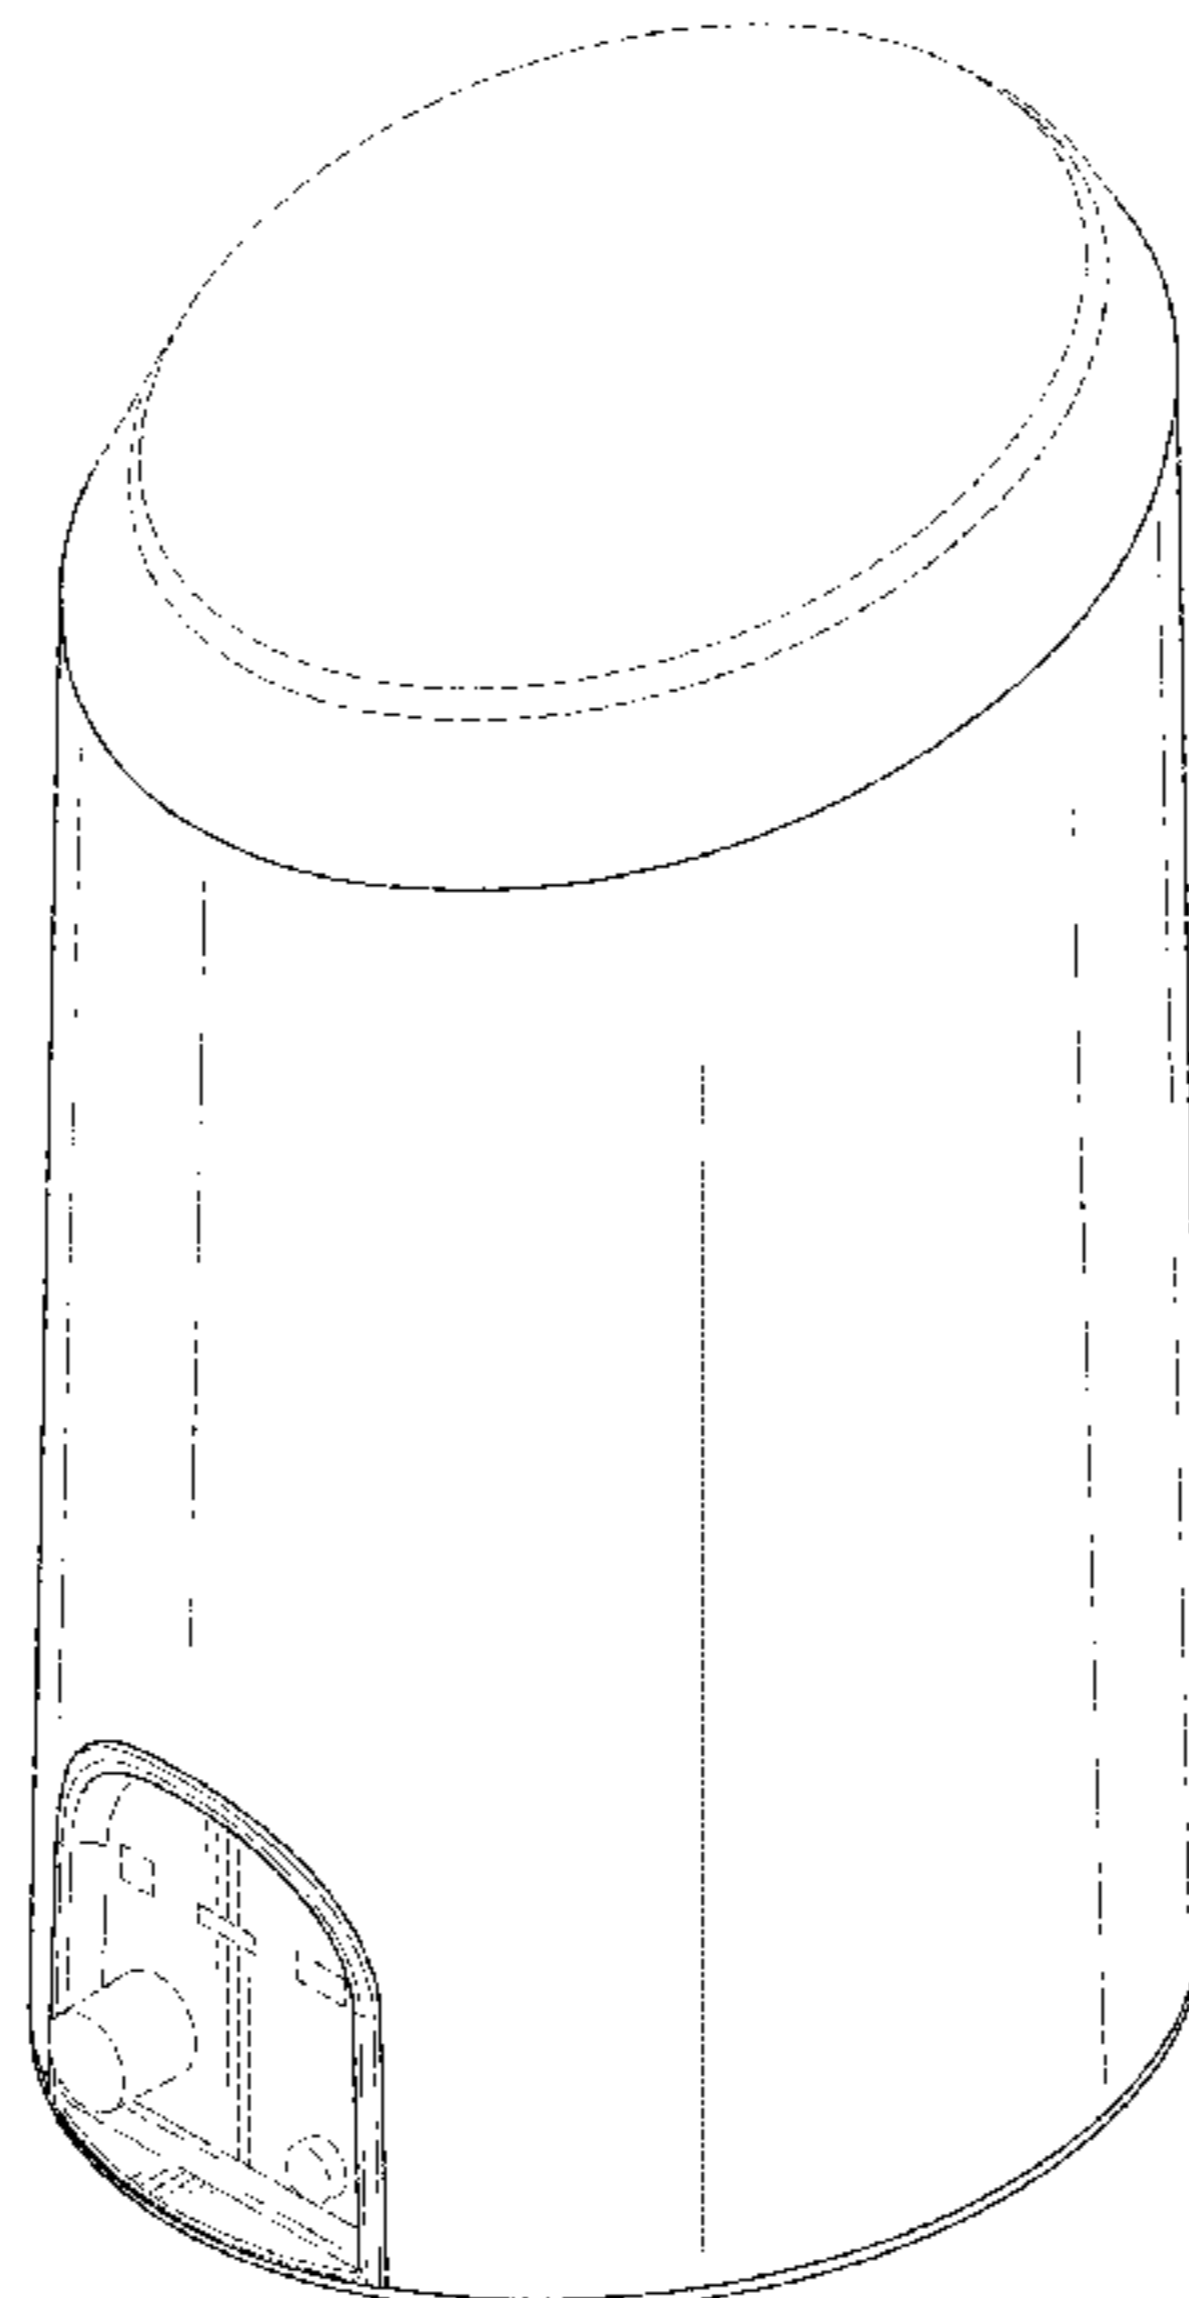

(56)

References Cited

OTHER PUBLICATIONS

U.S. PATENT DOCUMENTS

5,697,920 A 12/1997 Gibbons
 6,027,464 A 2/2000 Dahlquist
 6,149,674 A 11/2000 Borders
 6,277,052 B1 8/2001 Howard
 D452,570 S * 12/2001 Since D24/200
 6,423,017 B2 7/2002 Brotz
 6,565,593 B2 5/2003 Diana
 7,354,410 B2 * 4/2008 Perry A61H 9/0078
 601/151
 7,833,179 B2 11/2010 Filtvedt et al.
 7,833,180 B2 11/2010 Filtvedt et al.
 7,896,825 B2 3/2011 Atkinson et al.
 D644,250 S * 8/2011 Barber D15/7
 8,021,314 B2 9/2011 Filtvedt et al.
 8,100,887 B2 1/2012 Weston et al.
 8,361,001 B2 1/2013 Filtvedt et al.
 8,657,864 B2 2/2014 Rein et al.
 8,821,422 B2 9/2014 Filtvedt et al.
 D790,070 S * 6/2017 Acosta D24/188
 D791,955 S * 7/2017 Gilbert D24/109
 D816,854 S * 5/2018 Acosta D24/189
 D857,215 S * 8/2019 Lin D24/200
 2003/0097163 A1 5/2003 Kane et al.
 2003/0125649 A1 7/2003 McIntosh et al.
 2005/0027218 A1 2/2005 Filtvedt et al.
 2005/0137446 A1 6/2005 Rastegar et al.
 2009/0143719 A1 6/2009 Loori et al.
 2009/0312675 A1 12/2009 Sampson et al.
 2010/0152633 A1 6/2010 Rein et al.
 2011/0000484 A1 1/2011 Melsheimer
 2011/0130712 A1 6/2011 Topaz
 2011/0288458 A1 11/2011 Jones et al.
 2012/0209153 A1 * 8/2012 Farrow A61H 9/0092
 601/18
 2012/0238924 A1 9/2012 Avni
 2013/0331747 A1 * 12/2013 Helgeson A61H 9/0078
 601/48
 2014/0128781 A1 5/2014 Rein et al.
 2014/0276288 A1 9/2014 Randolph et al.
 2015/0065931 A1 3/2015 Alnabulsi et al.
 2015/0374571 A1 * 12/2015 Denson A61H 1/008
 601/150

FOREIGN PATENT DOCUMENTS

EM 0026509370003 3/2015
 EM 0026509370004 3/2015
 EM 0026509370005 3/2015
 FR 1562252 A 4/1969
 WO 9840039 A1 9/1998
 WO 0180790 A1 11/2001
 WO 03045289 A1 6/2003
 WO 2004058131 A2 7/2004

Allen et al., "Intermittent Pressure and Suction in the Treatment of Chronic Occlusive Arterial Disease," The Journal of the American Medical Association, vol. 105, No. 25, Dec. 21, 1935, pp. 2029-2034.
 De Takats, "Obliterative Vascular Disease: Preliminary Report on Treatment by Alternating Negative and Positive Pressure," Journal of the American Medical Association, vol. 103, No. 25, Dec. 22, 1934, pp. 1920-1924.
 Herrmann et al., "The Conservative Treatment of Arteriosclerotic Peripheral Vascular Diseases: Passive Vascular Exercises (Pavaex Therapy)," Annals of Surgery, vol. 100, No. 4, Oct. 1934, pp. 750-760.
 Herrmann et al., "Passive Vascular Exercises: Treatment of Peripheral Obliterative Arterial Diseases by Rhythmic Alternation of Environmental Pressure," Archives of Surgery, vol. 29, No. 5, Nov. 1934, pp. 697-704.
 Landis et al., "The Effects of Alternate Suction and Pressure on Blood Flow to the Lower Extremities," The Journal of Clinical Investigation, vol. 12, No. 5, Sep. 1933, pp. 925-961.
 Landis et al., "Treatment of Peripheral Vascular Disease by Means of Suction and Pressure," Annals of Internal Medicine, vol. 9, No. 3, Sep. 1, 1935, pp. 264-273.
 Meyer et al., "Bier's Hyperemic Treatment," California State Journal of Medicine, vol. 8, No. 4, Apr. 1910, pp. 142-143.
 Reid, "Diagnosis and Treatment of Peripheral Vascular Diseases," The American Journal of Surgery, vol. 24, No. 1, Apr. 1934, pp. 11-35.
 Theis et al., "Peripheral Circulatory Diseases Effect of Alternating Positive and Negative Pressure Treatments on Venous Blood and the Skin Temperatures: Preliminary Report," The Journal of the American Medical Association, vol. 107, No. 14, Oct. 3, 1936, pp. 1097-1104.
 Goodney et al., "National Trends in Lower Extremity Bypass Surgery, Endovascular Interventions, and Major Amputations", Journal of Vascular Surgery vol. 50 No. 1, Jul. 2009, pp. 54-60.
 Hiramori et al., "Impact of Runoff Grade After Endovascular Therapy for Femoropopliteal Lesions", Journal of Vascular Surgery, vol. 59, No. 3, Mar. 2014, pp. 720-727.
 Norgren et al., "Inter-Society Consensus for the Management of Peripheral Arterial Disease (TASC II)", Journal of Vascular Surgery, vol. 45, No. 1, Supplement S, Jan. 2007, p. S5A-S67A.
 Rowe et al., "Patterns of Treatment for Peripheral Arterial Disease in the United States: 1996-2005", Journal of Vascular Surgery vol. 49, No. 4, Apr. 2009, pp. 910-917.
 Siracuse et al., "Results for Primary Bypass Versus Primary Angioplasty/Stent for Intermittent Claudication Due to Superficial Femoral Artery Occlusive Disease", Journal of Vascular Surgery, vol. 55, No. 4, Apr. 2012, pp. 1001-1007.
 "Nanova Therapy System," Acelity, retrieved from <https://www.acelity.com/products/nanova-therapy-system-uk> on Aug. 27, 2018, 11 Pages.

* cited by examiner

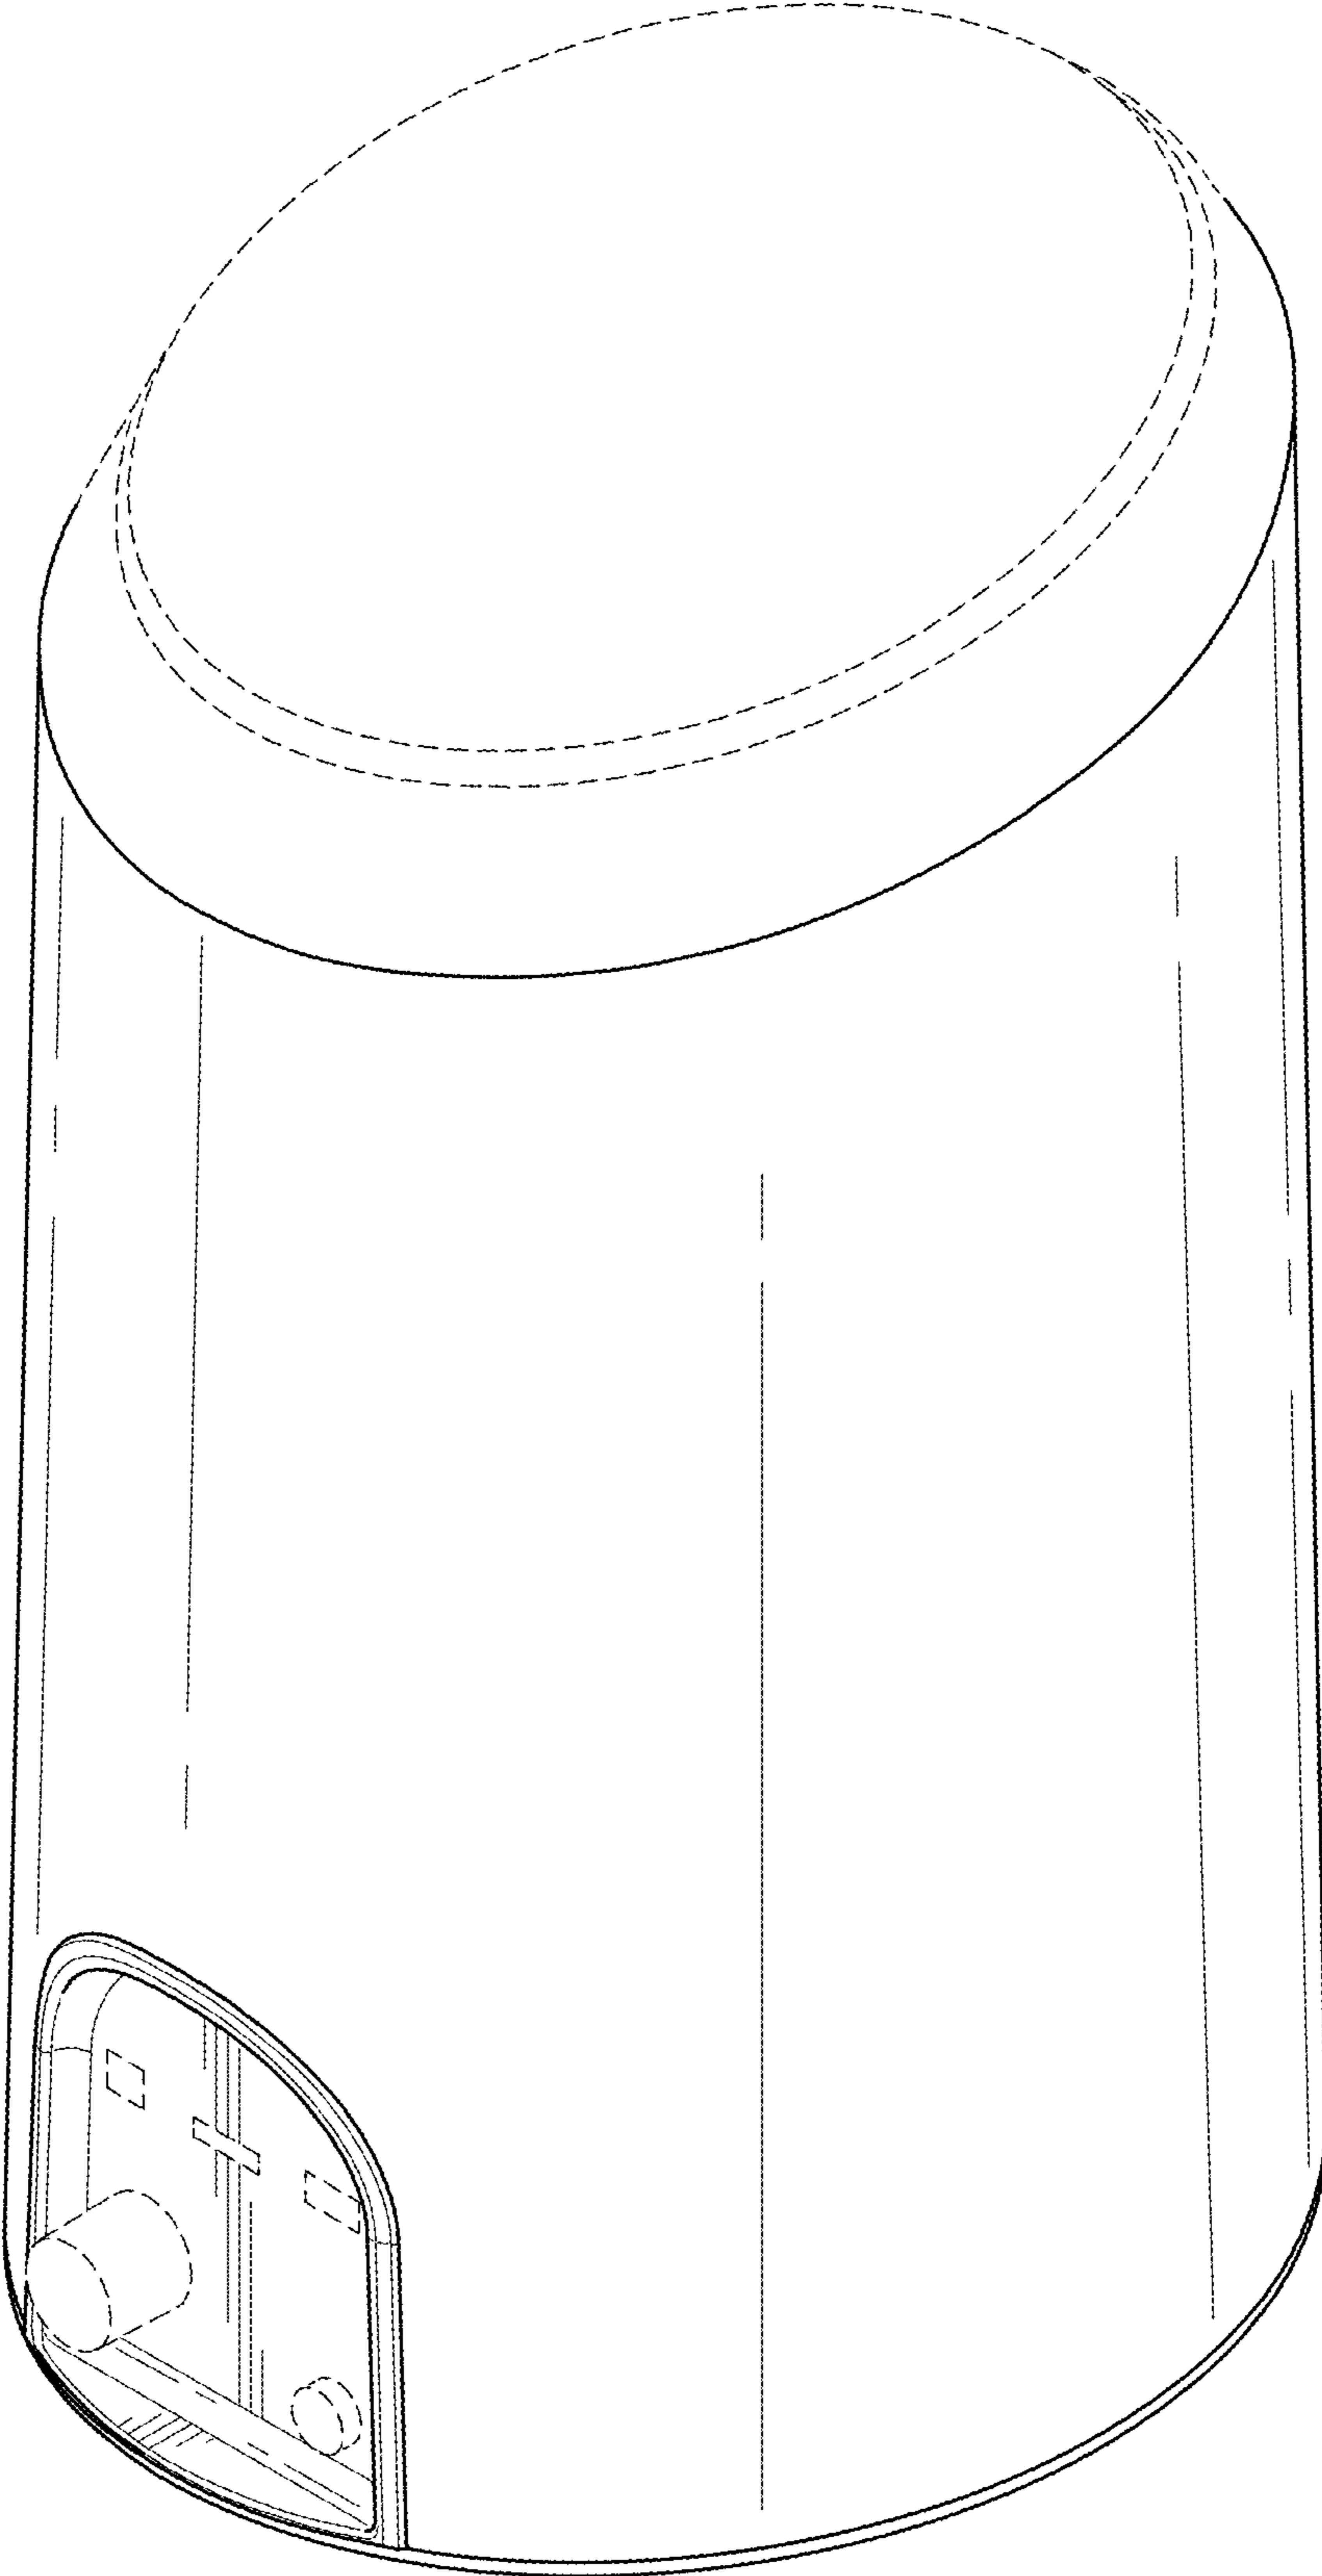


FIG. 1

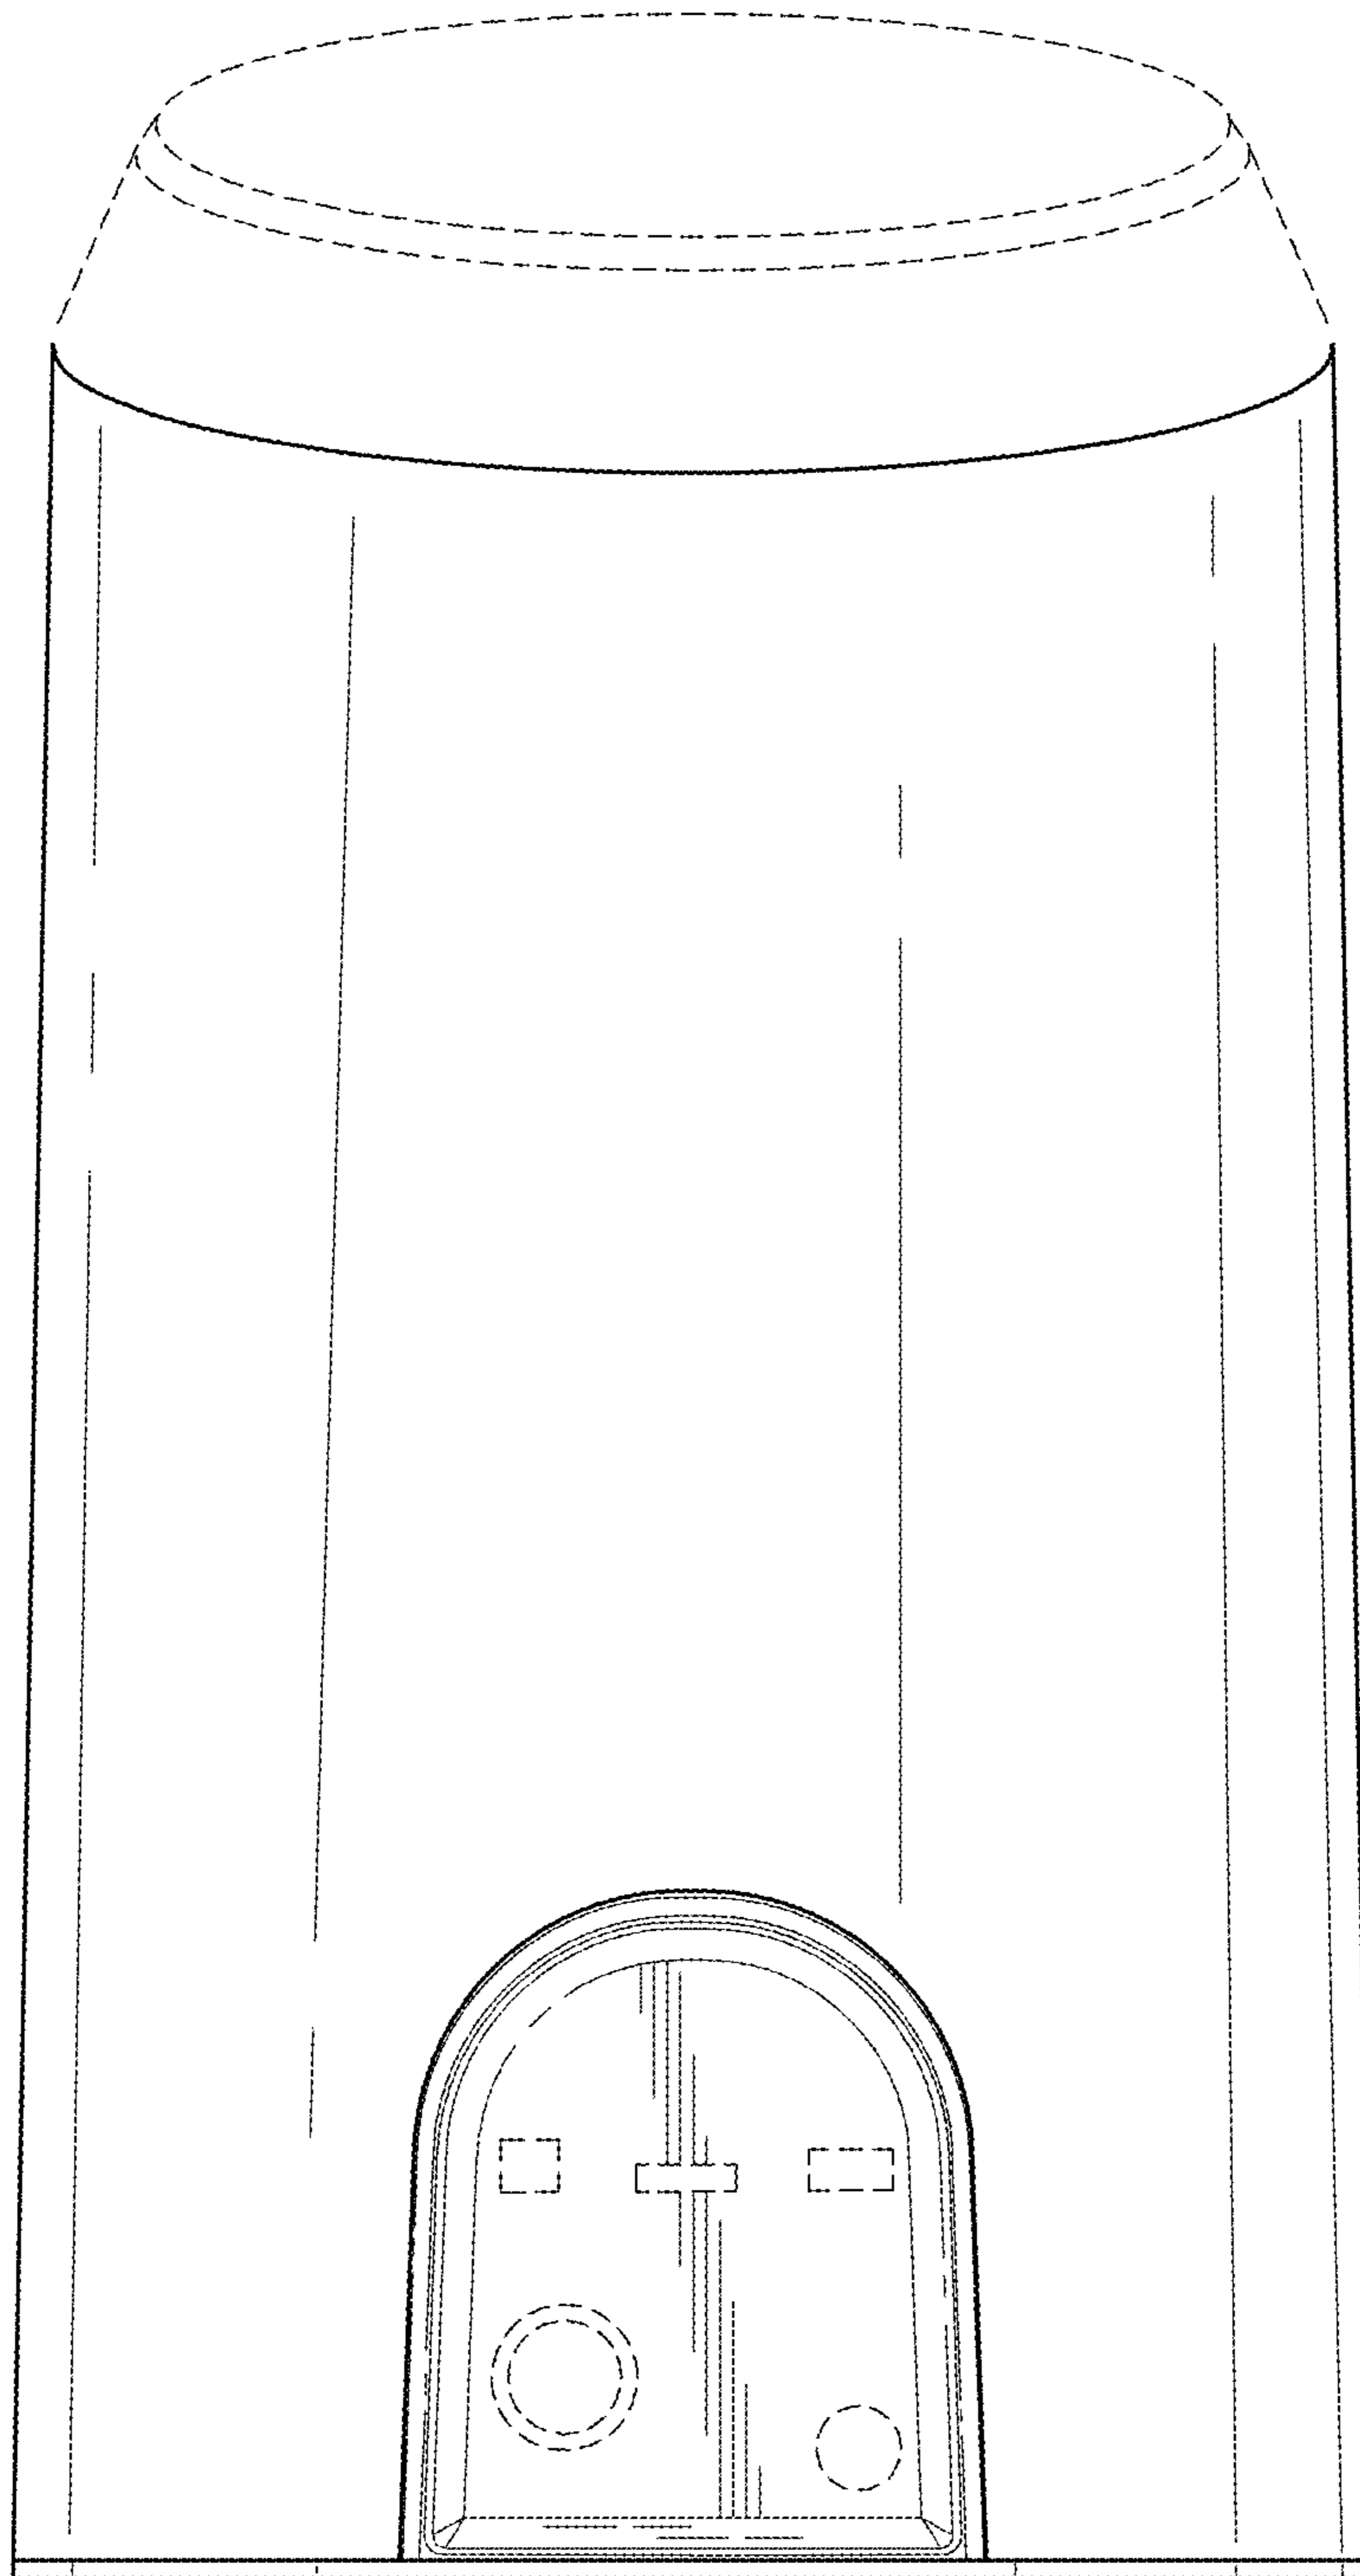


FIG. 2

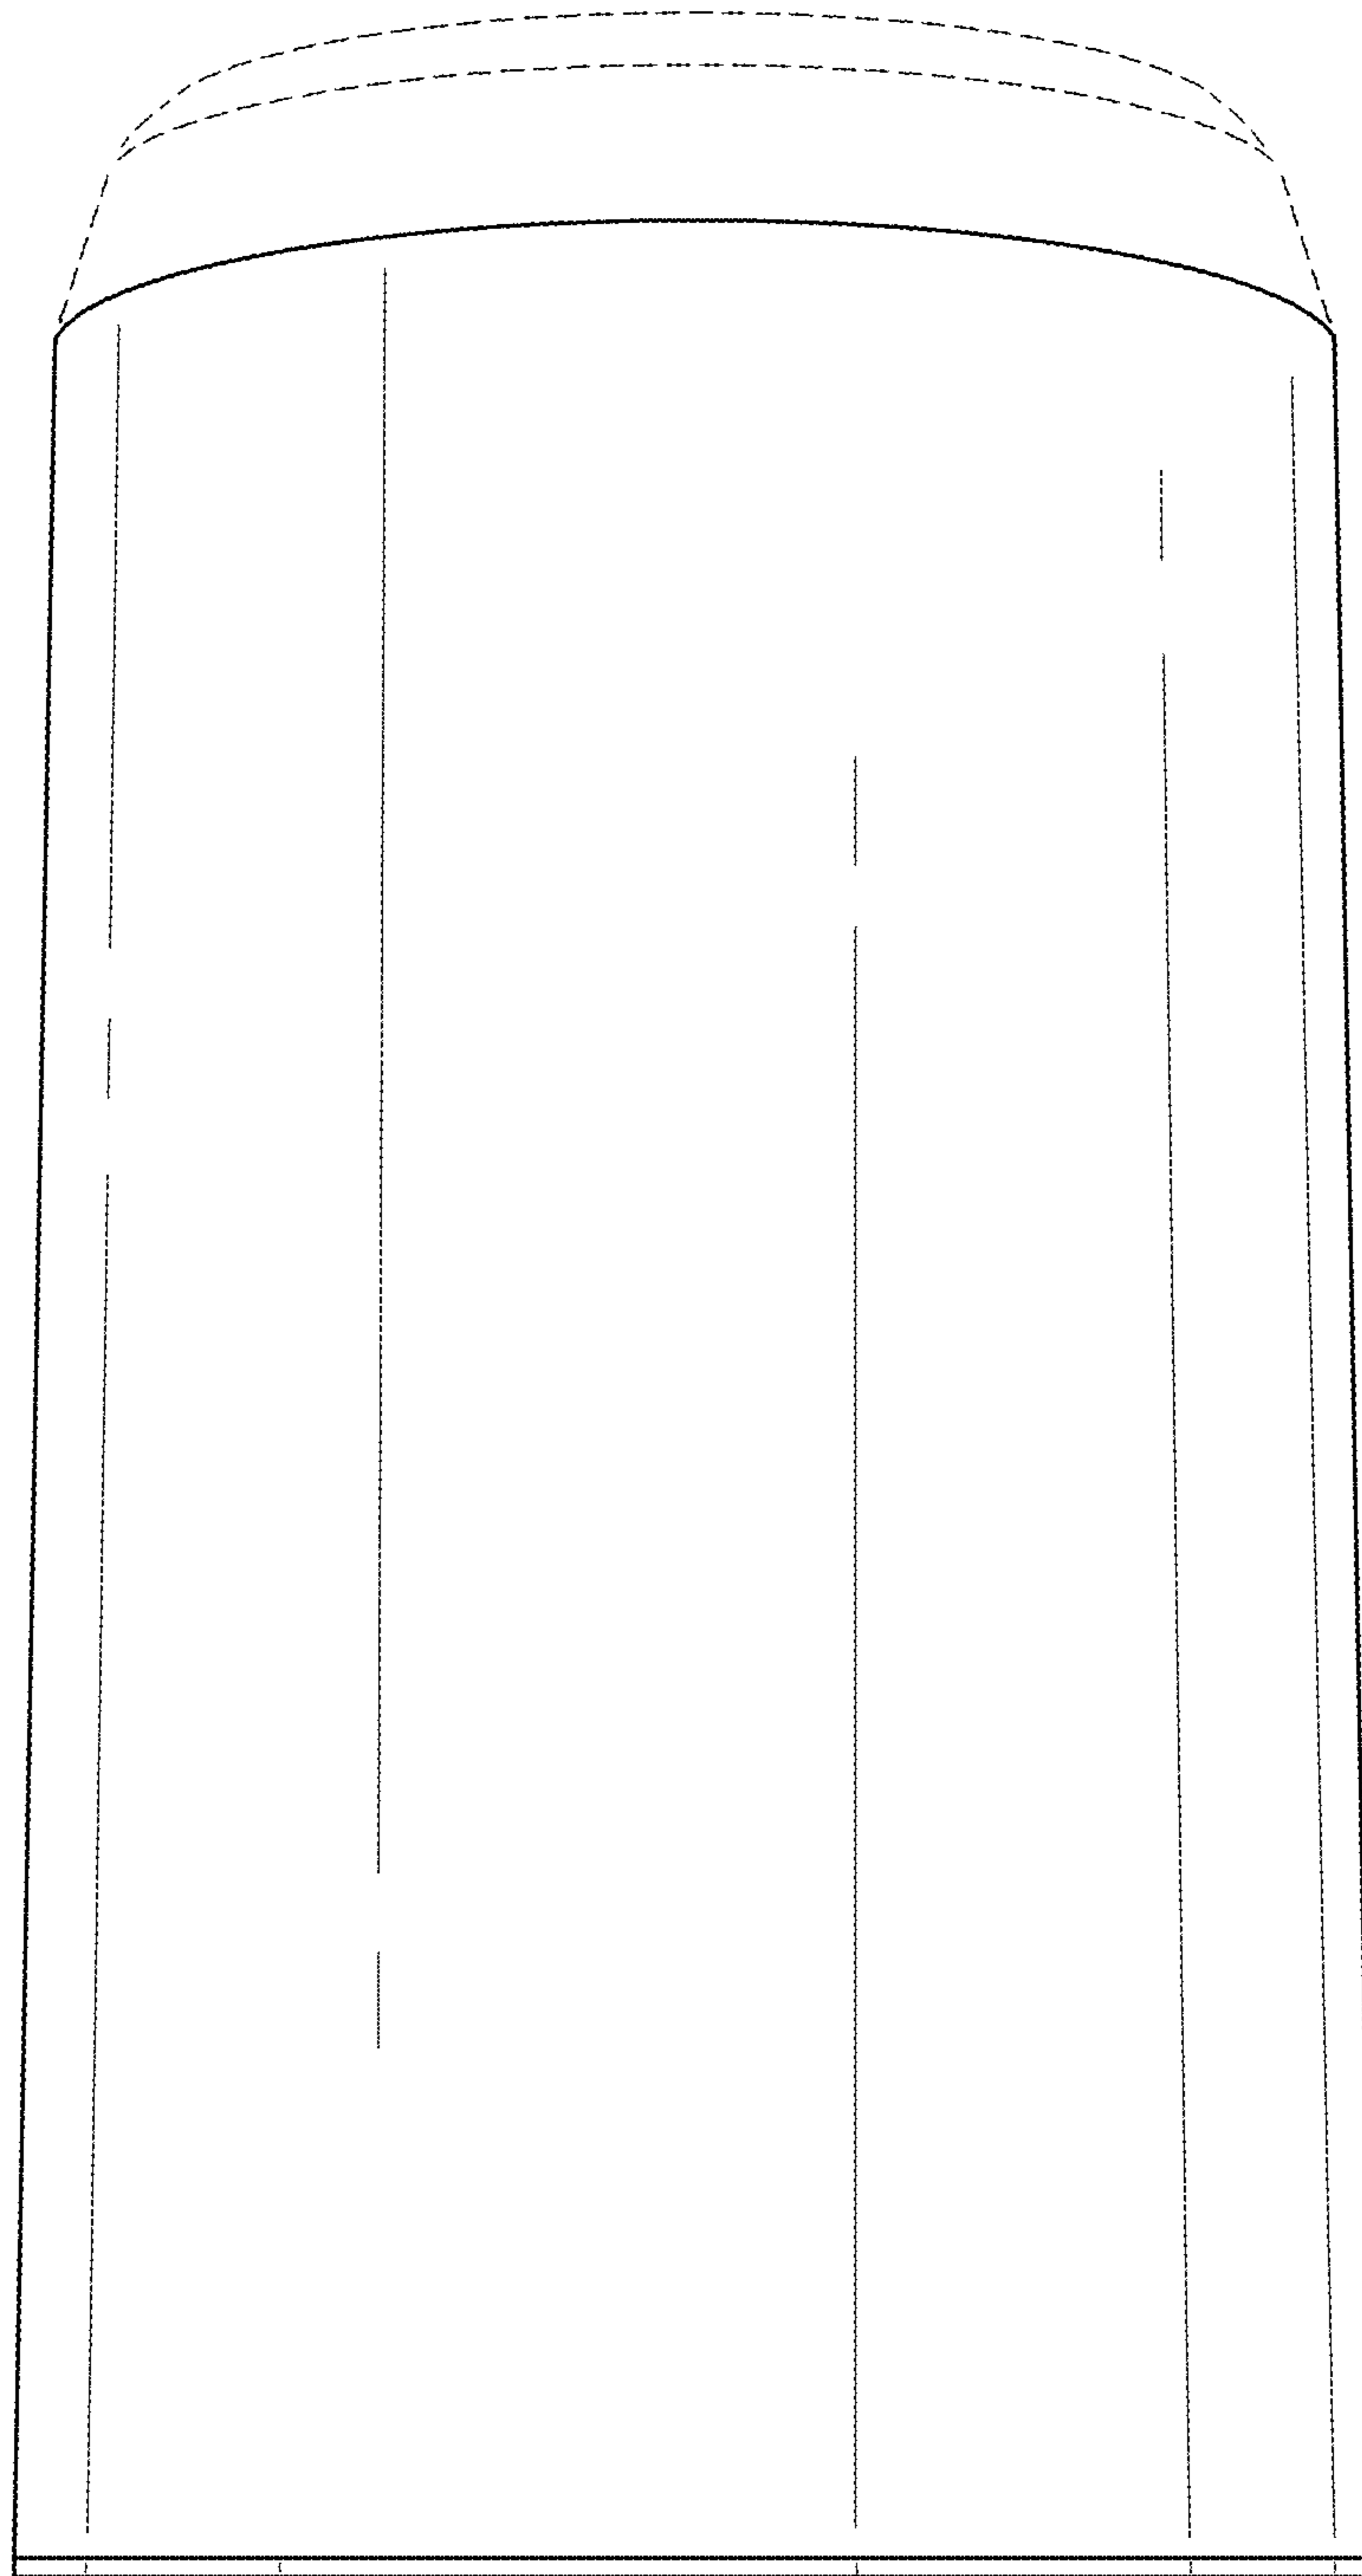


FIG. 3

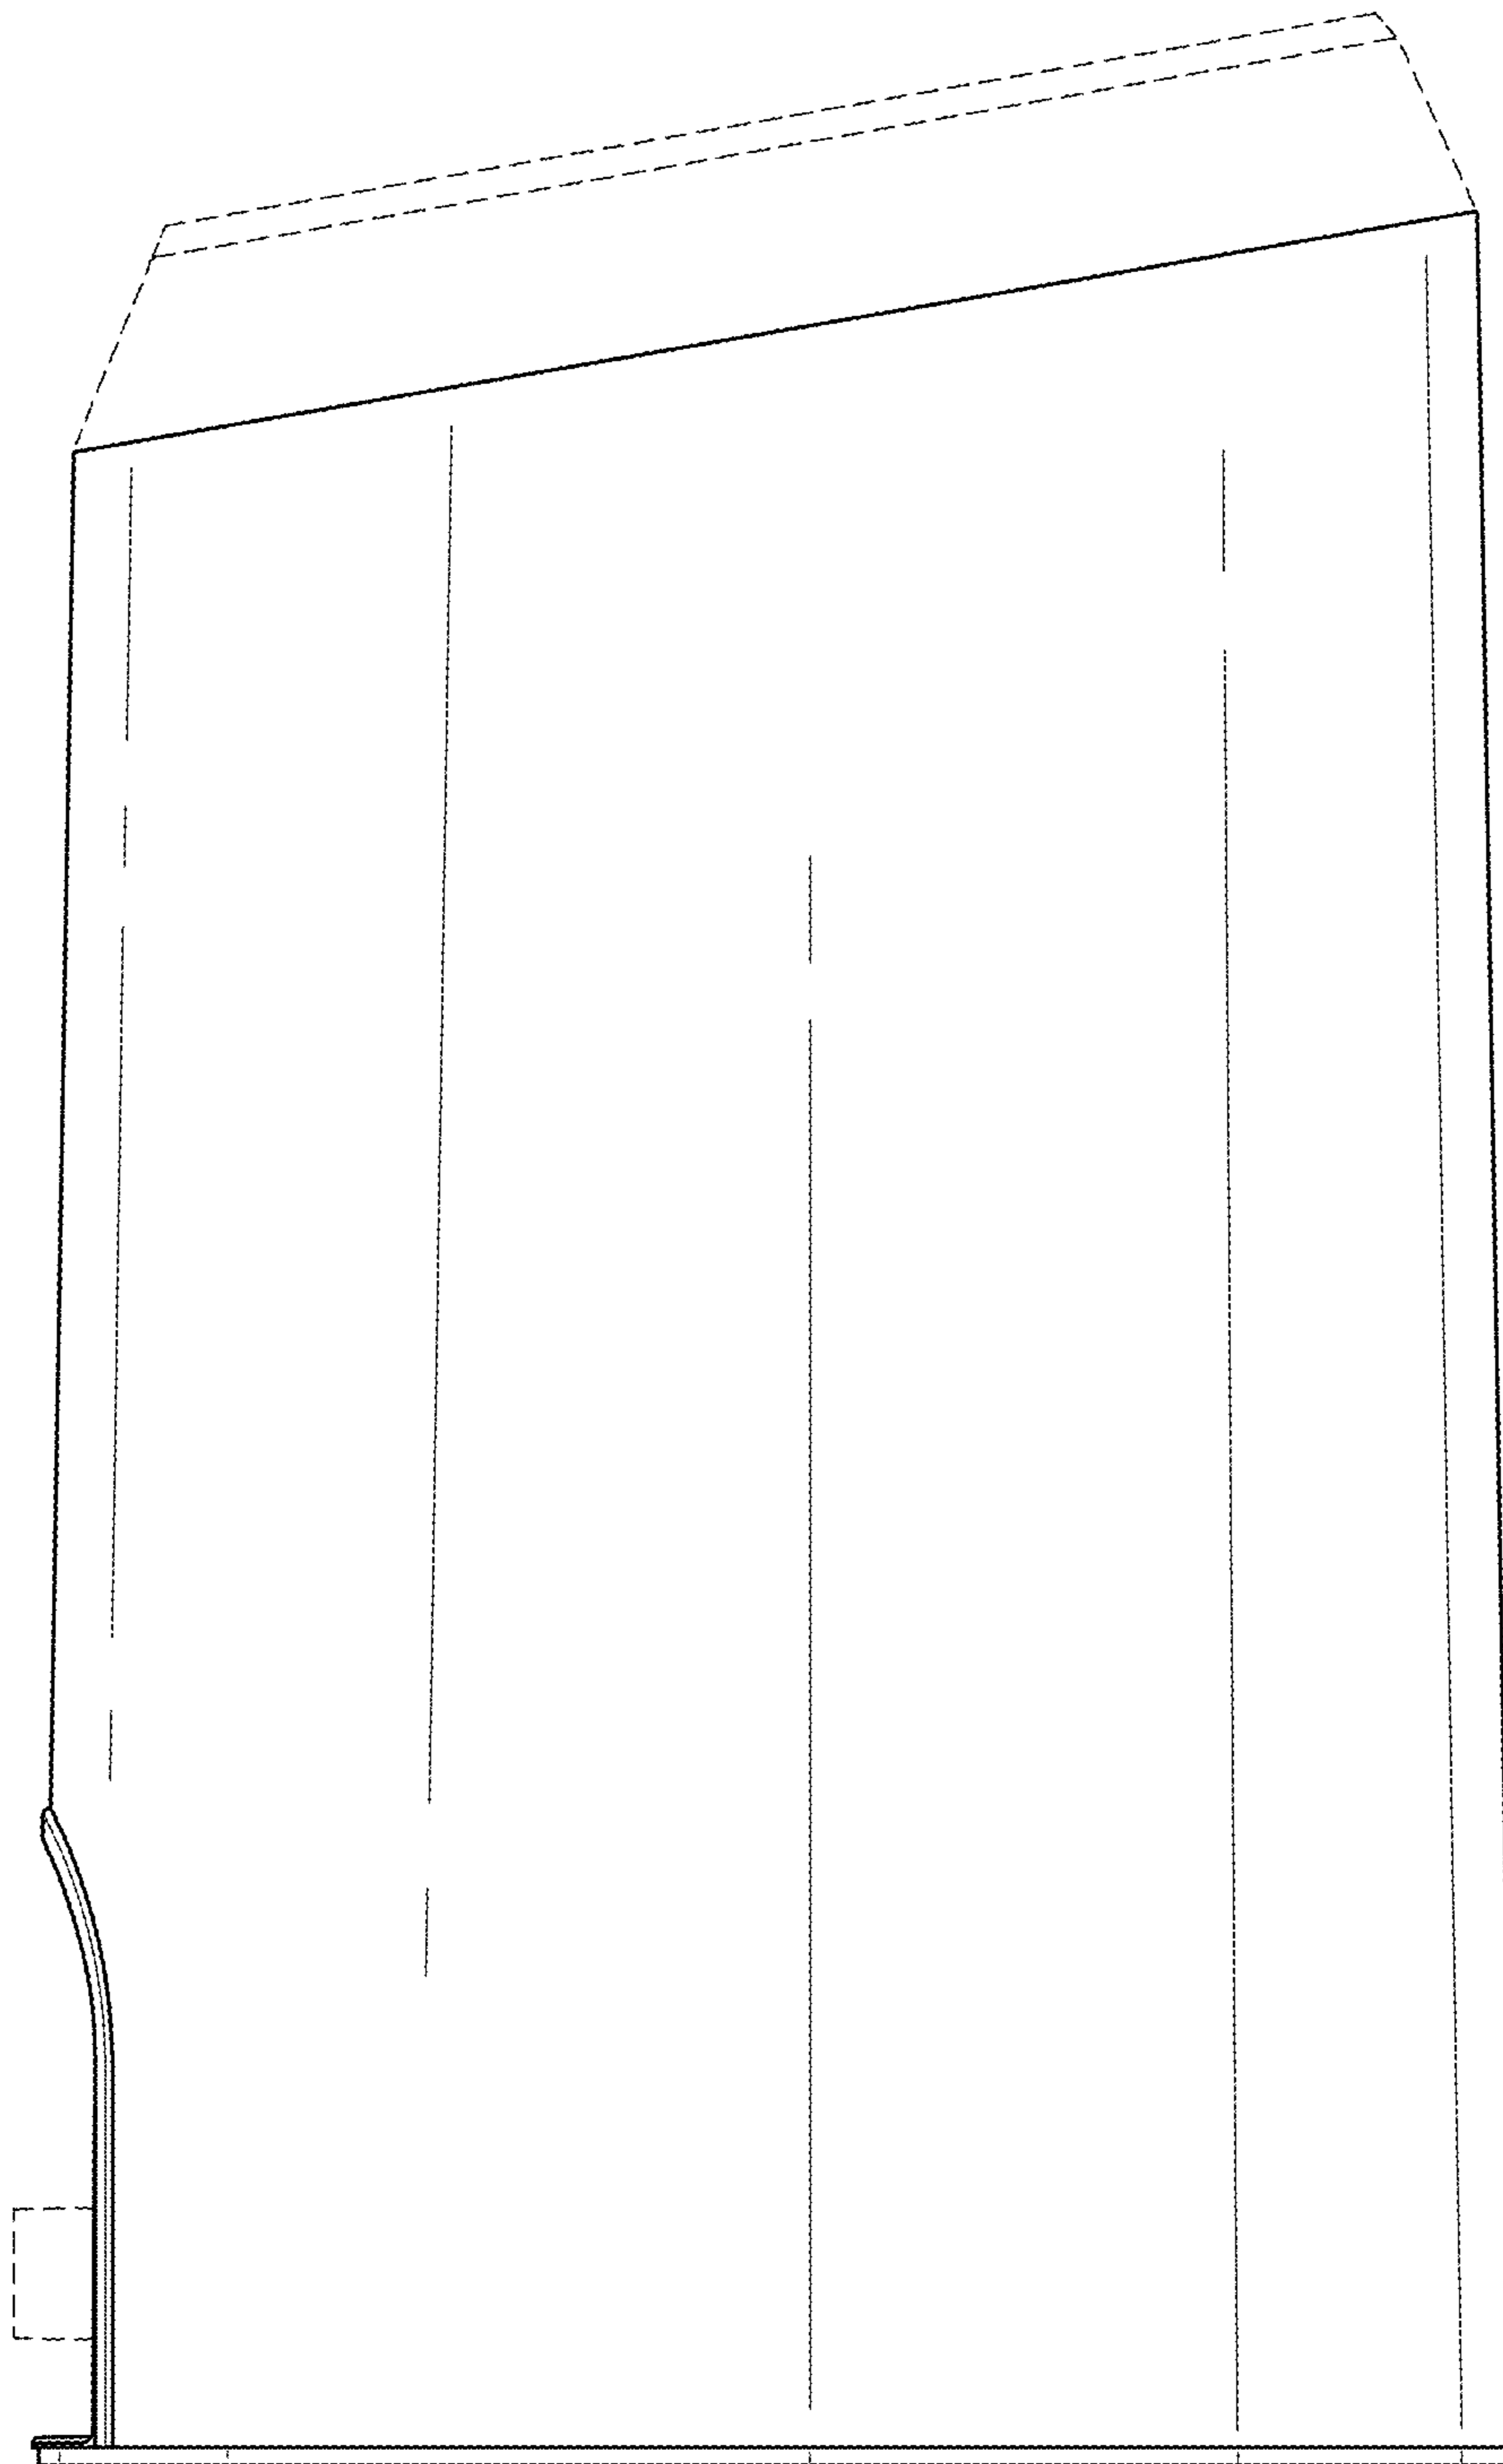


FIG. 4

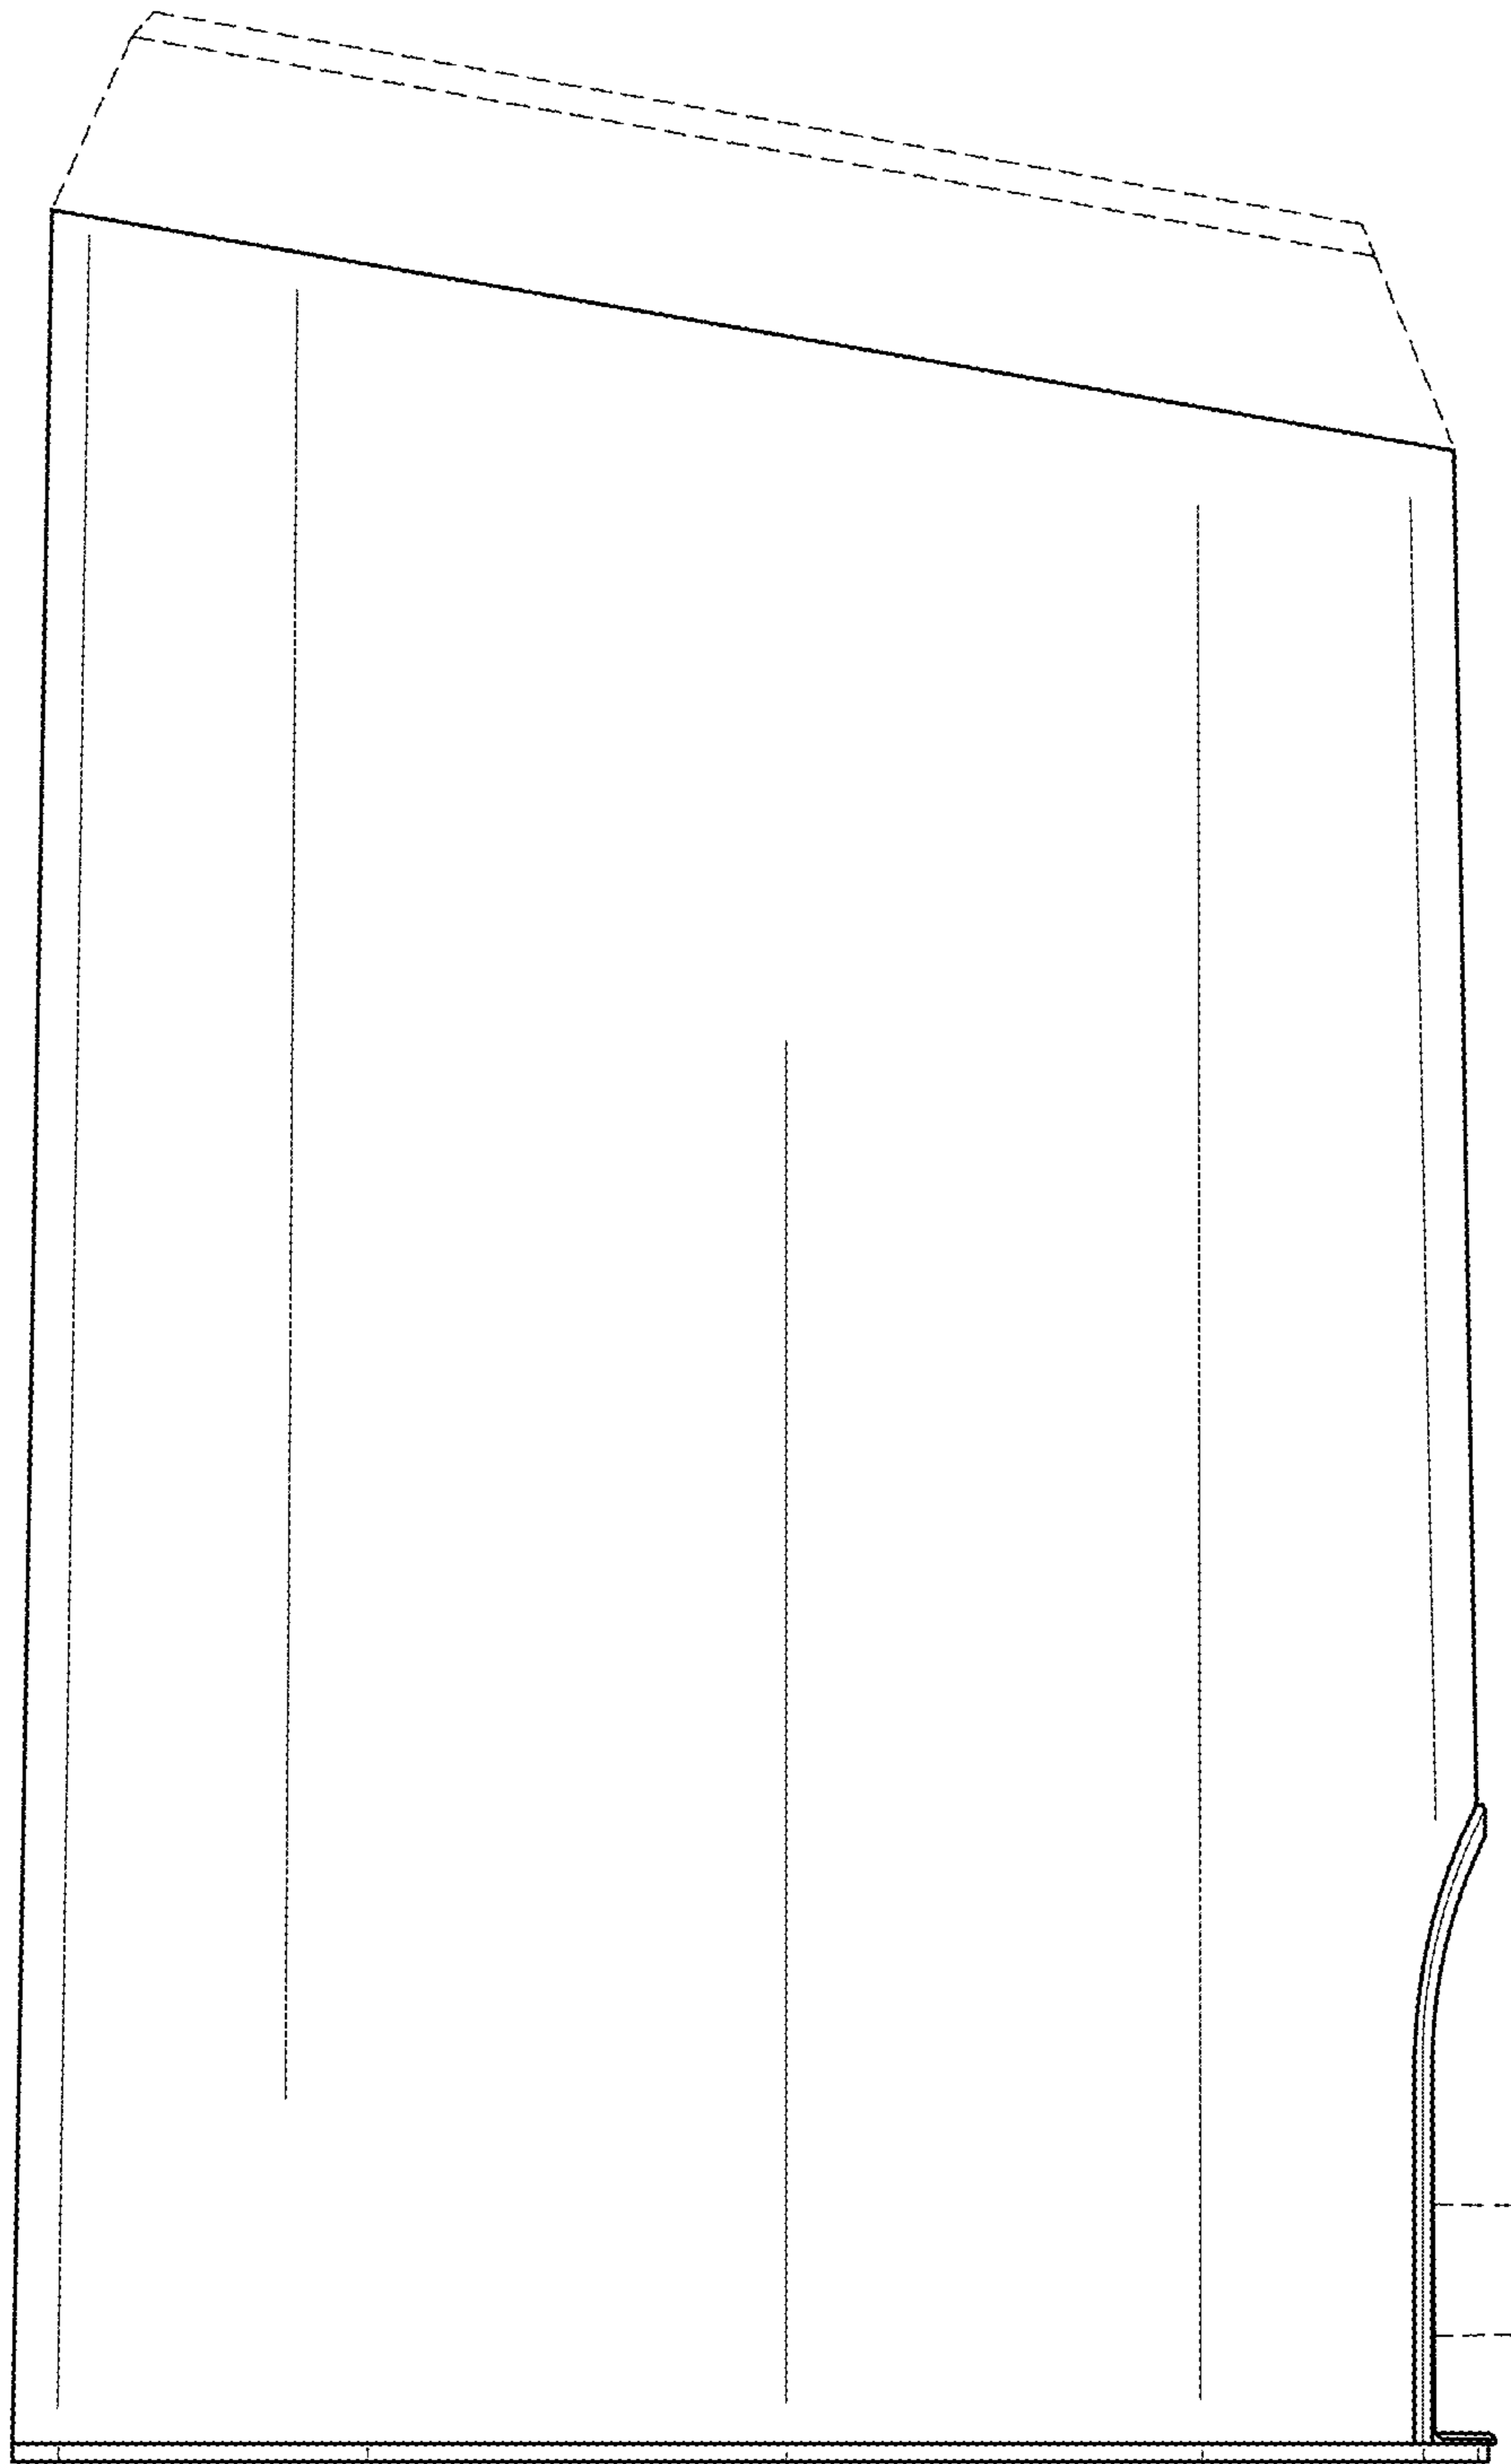


FIG. 5

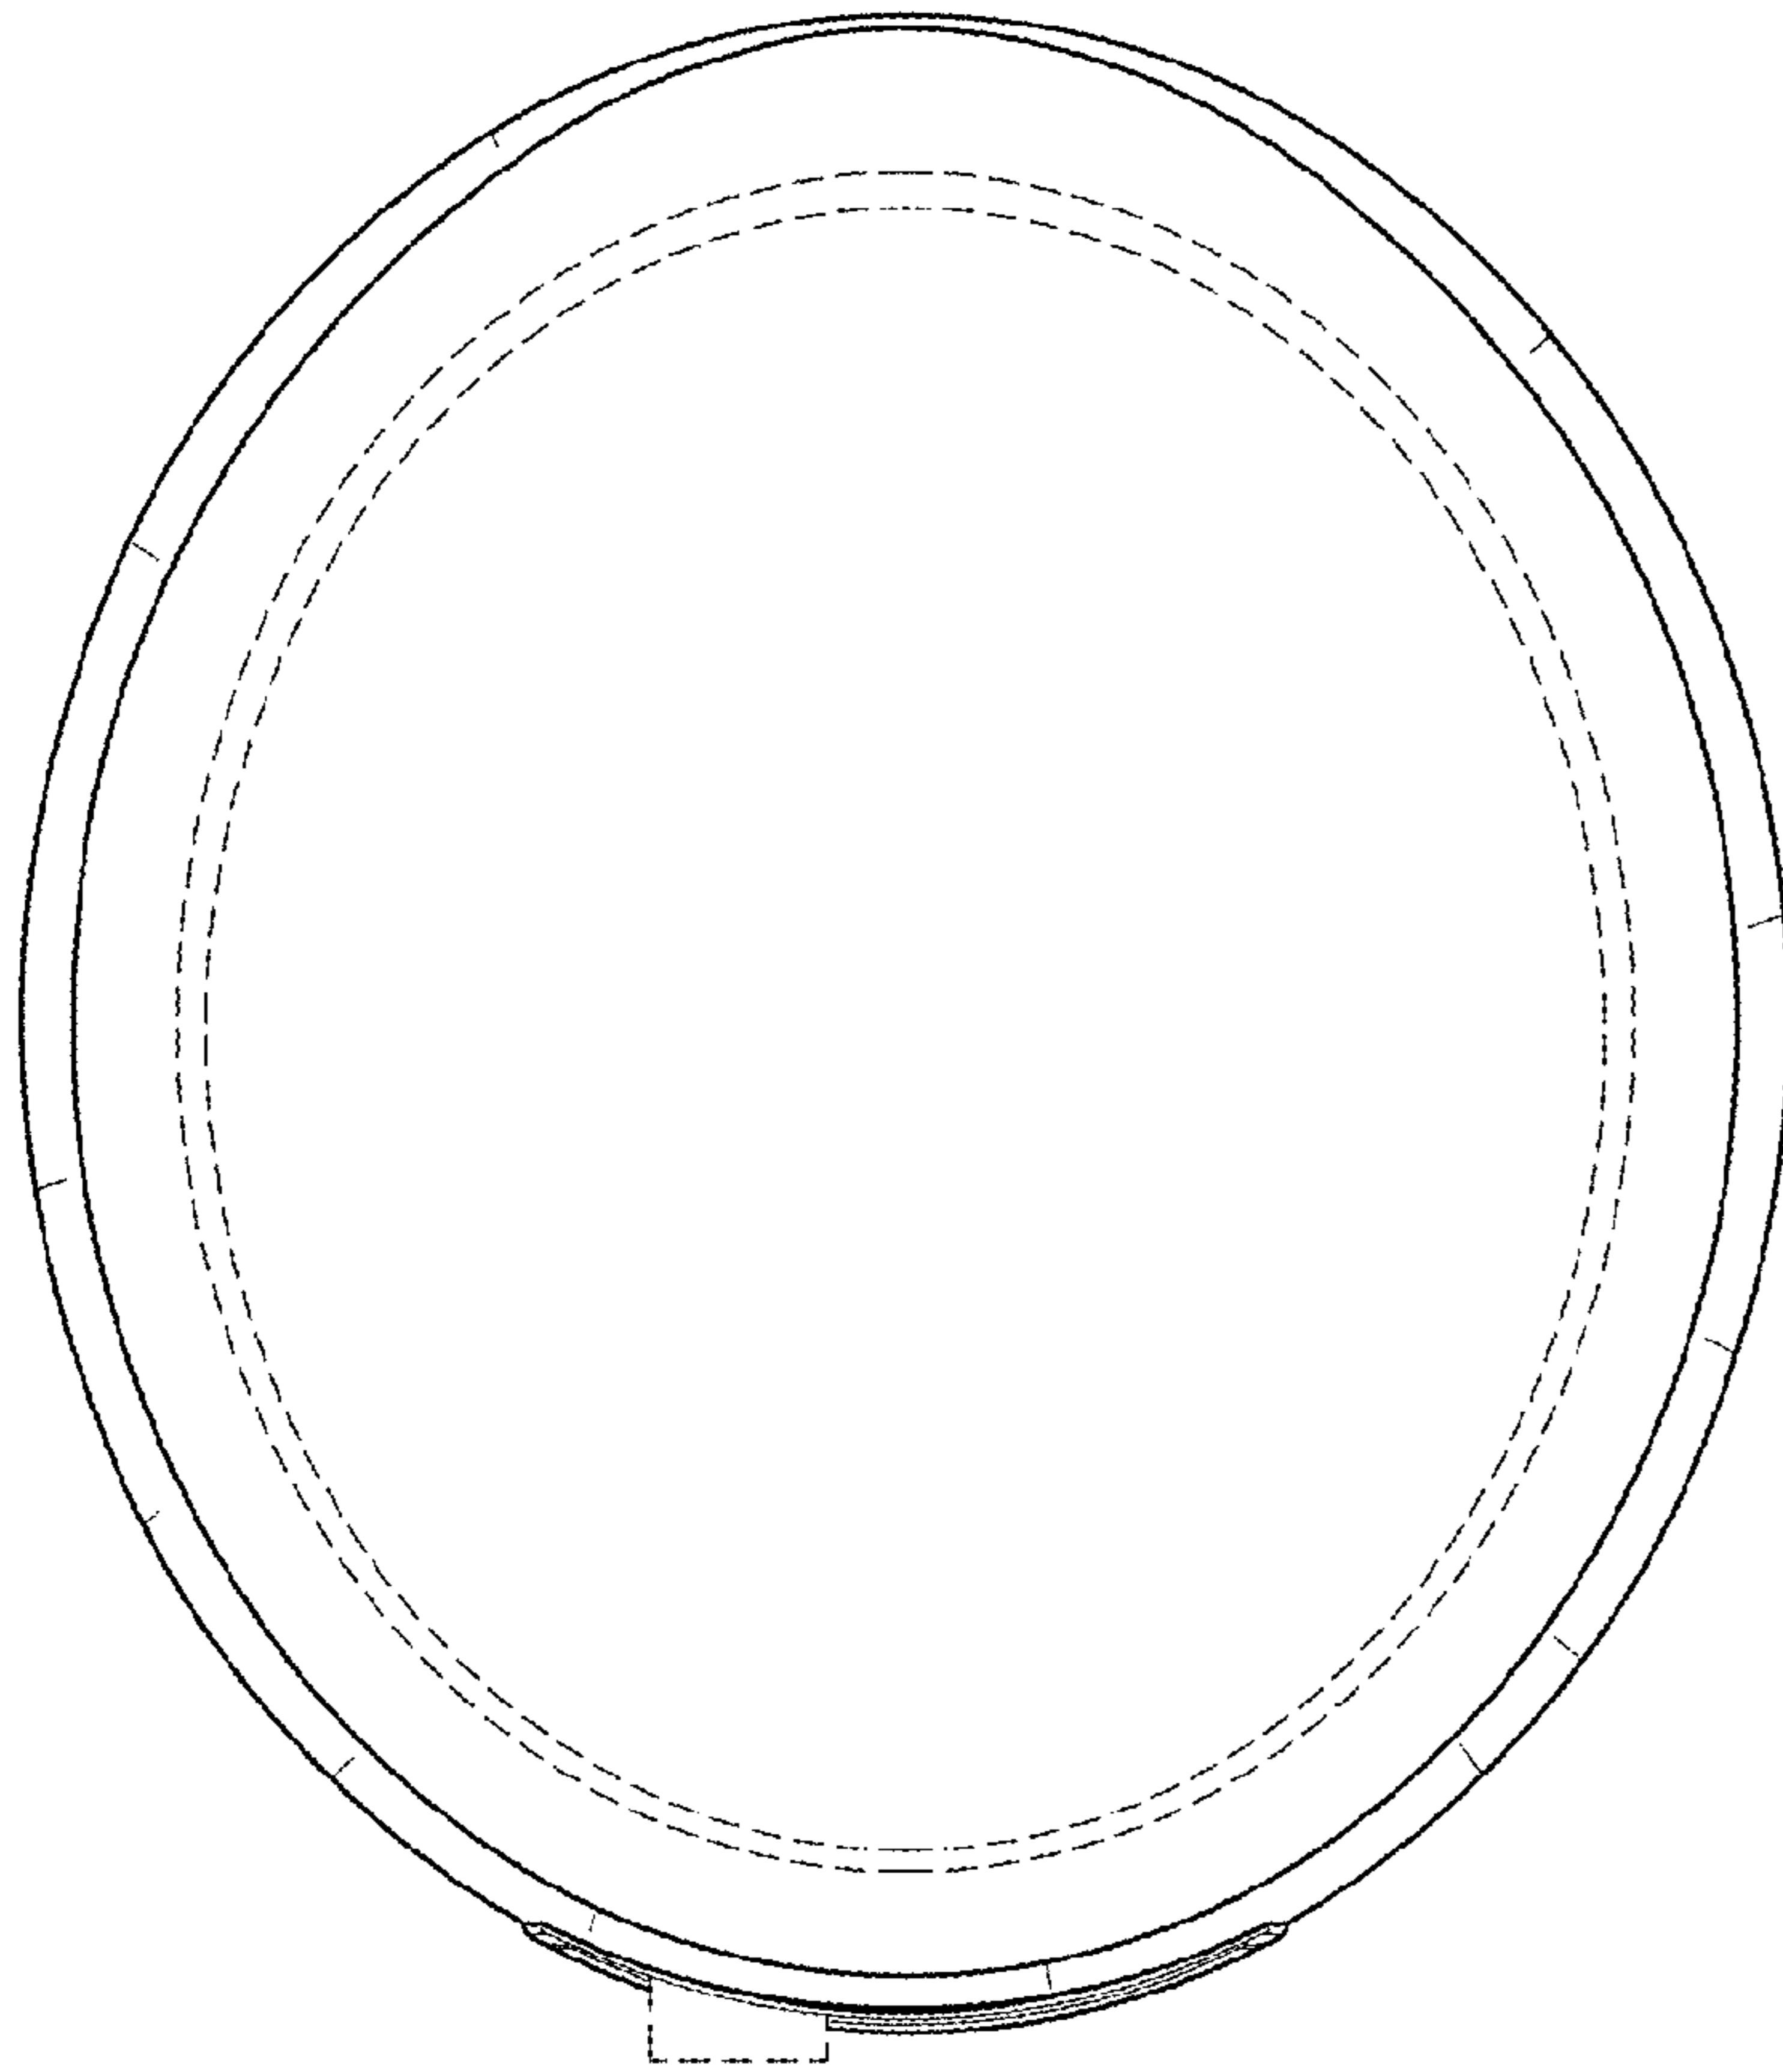


FIG. 6

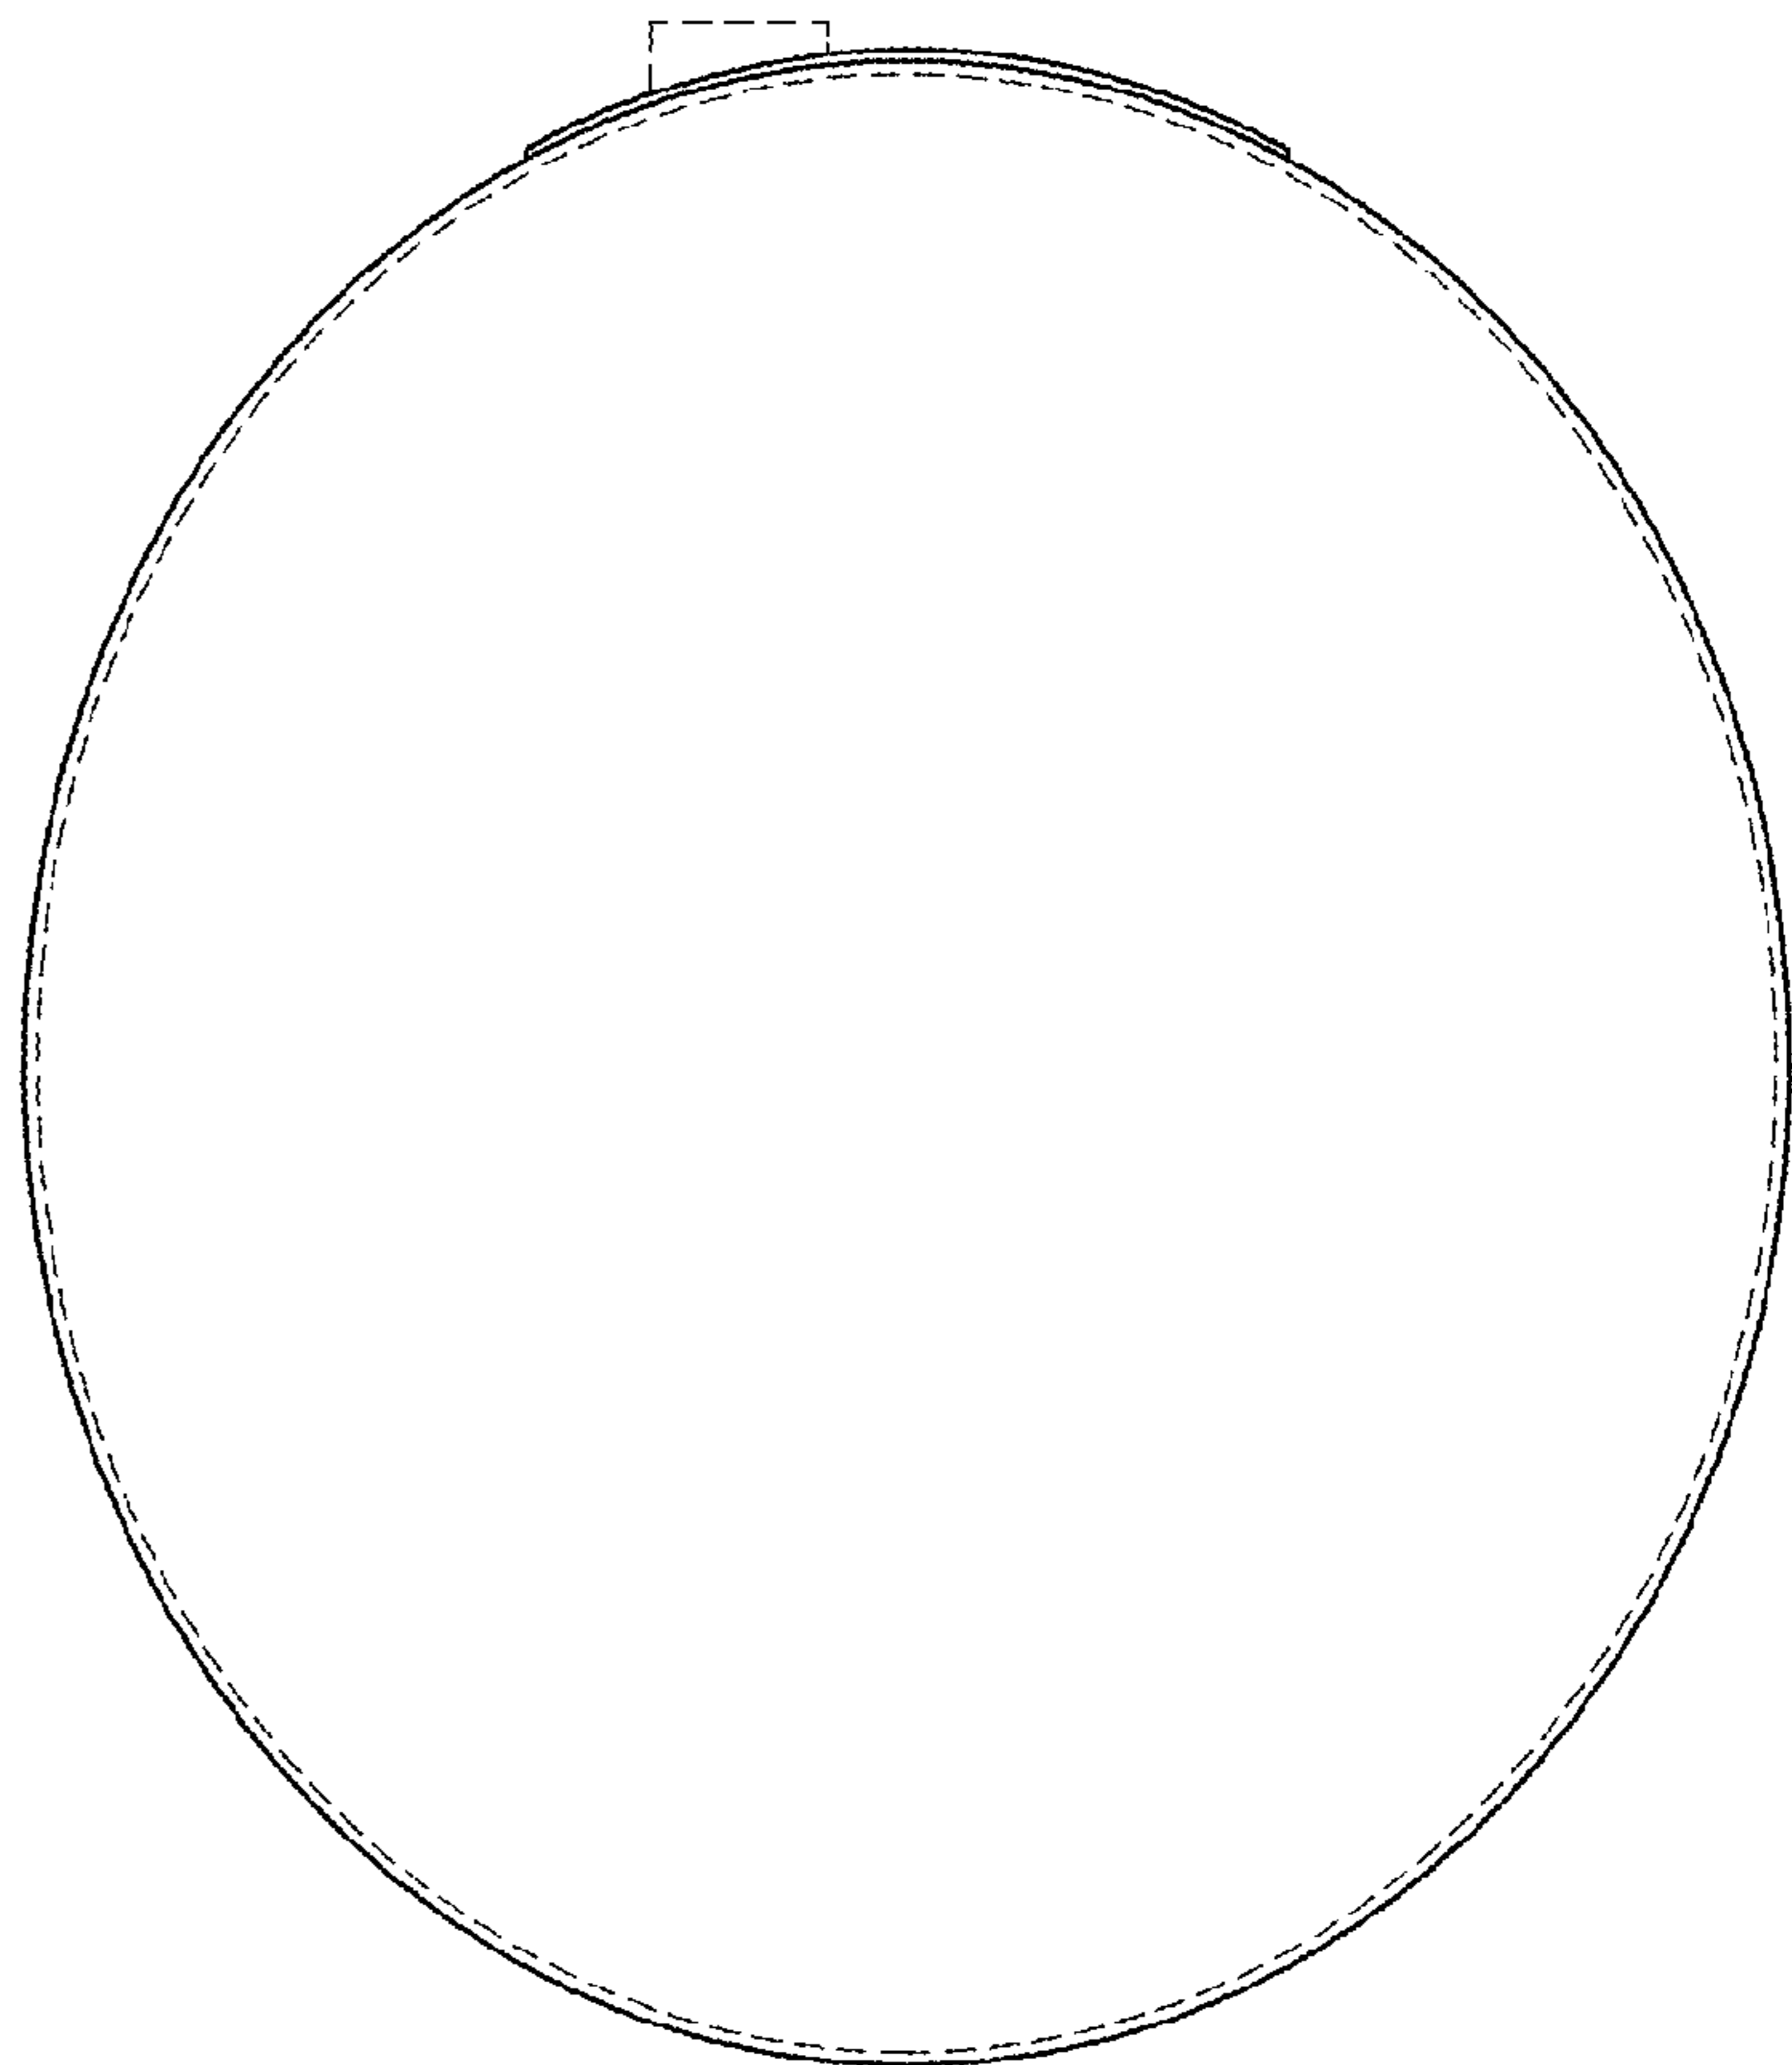


FIG. 7