



US00D889655S

(12) **United States Design Patent** (10) **Patent No.:** **US D889,655 S**  
**Limem et al.** (45) **Date of Patent:** **\*\* Jul. 7, 2020**

(54) **THREE DIMENSIONAL MASTOPEXY IMPLANT**

5,755,611 A 5/1998 Noble et al.  
5,759,204 A 6/1998 Seare  
5,990,378 A 11/1999 Ellis

(Continued)

(71) Applicant: **Tepha, Inc.**, Lexington, MA (US)

FOREIGN PATENT DOCUMENTS

(72) Inventors: **Skander Limem**, Melrose, MA (US);  
**Said Rizk**, Windham, NH (US); **Simon F. Williams**, Lexington, MA (US)

WO 2004/096098 A1 11/2004  
WO 2006/117622 A1 11/2006

(Continued)

(73) Assignee: **Tepha, Inc.**, Lexington, MA (US)

OTHER PUBLICATIONS

(\*\*) Term: **15 Years**

“GalaFLEX Mesh . . . Supporting Your Quest for Timeless Beauty,”  
Tepha, Inc. 400109 Rev.B, Oct. 2012.

(Continued)

(21) Appl. No.: **29/636,699**

(22) Filed: **Feb. 9, 2018**

*Primary Examiner* — Charles D Hanson

(51) **LOC (12) Cl.** ..... **24-03**

(74) *Attorney, Agent, or Firm* — Richard Batt

(52) **U.S. Cl.**

USPC ..... **D24/155**

(57) **CLAIM**

(58) **Field of Classification Search**

USPC ..... D24/155

CPC ..... A61F 2/12

See application file for complete search history.

The ornamental design for a three dimensional mastopexy implant, as shown and described.

**DESCRIPTION**


(56) **References Cited**

U.S. PATENT DOCUMENTS

2,701,879 A 2/1955 Bennett  
3,280,818 A 10/1966 Pankey et al.  
3,934,593 A 1/1976 Mellinger  
4,372,293 A 2/1983 Vijil-Rosales  
4,936,858 A 6/1990 O’Keeffe  
5,217,494 A 6/1993 Coggins et al.  
5,356,429 A 10/1994 Seare  
5,383,929 A 1/1995 Ledergerber  
5,500,019 A 3/1996 Johnson et al.  
5,545,221 A 8/1996 Hang-Fu  
5,584,884 A 12/1996 Pignataro  
5,658,328 A 8/1997 Johnson  
5,676,161 A 10/1997 Breiner  
5,716,404 A 2/1998 Vacanti et al.

FIG. 1 is a front view of a three dimensional mastopexy implant showing our new design;  
FIG. 2 is a left side view of the three dimensional mastopexy implant shown in FIG. 1;  
FIG. 3 is a right side view of the three dimensional mastopexy implant shown in FIG. 1;  
FIG. 4 is a bottom view of the three dimensional mastopexy implant shown in FIG. 1;  
FIG. 5 is a top view of the three dimensional mastopexy implant shown in FIG. 1;  
FIG. 6 is a rear view of the three dimensional mastopexy implant shown in FIG. 1;  
FIG. 7 is a top, front, side perspective view of the three dimensional mastopexy implant shown in FIG. 1; and,  
FIG. 8 is an enlarged view of the mesh taken from FIG. 1.

**1 Claim, 8 Drawing Sheets**

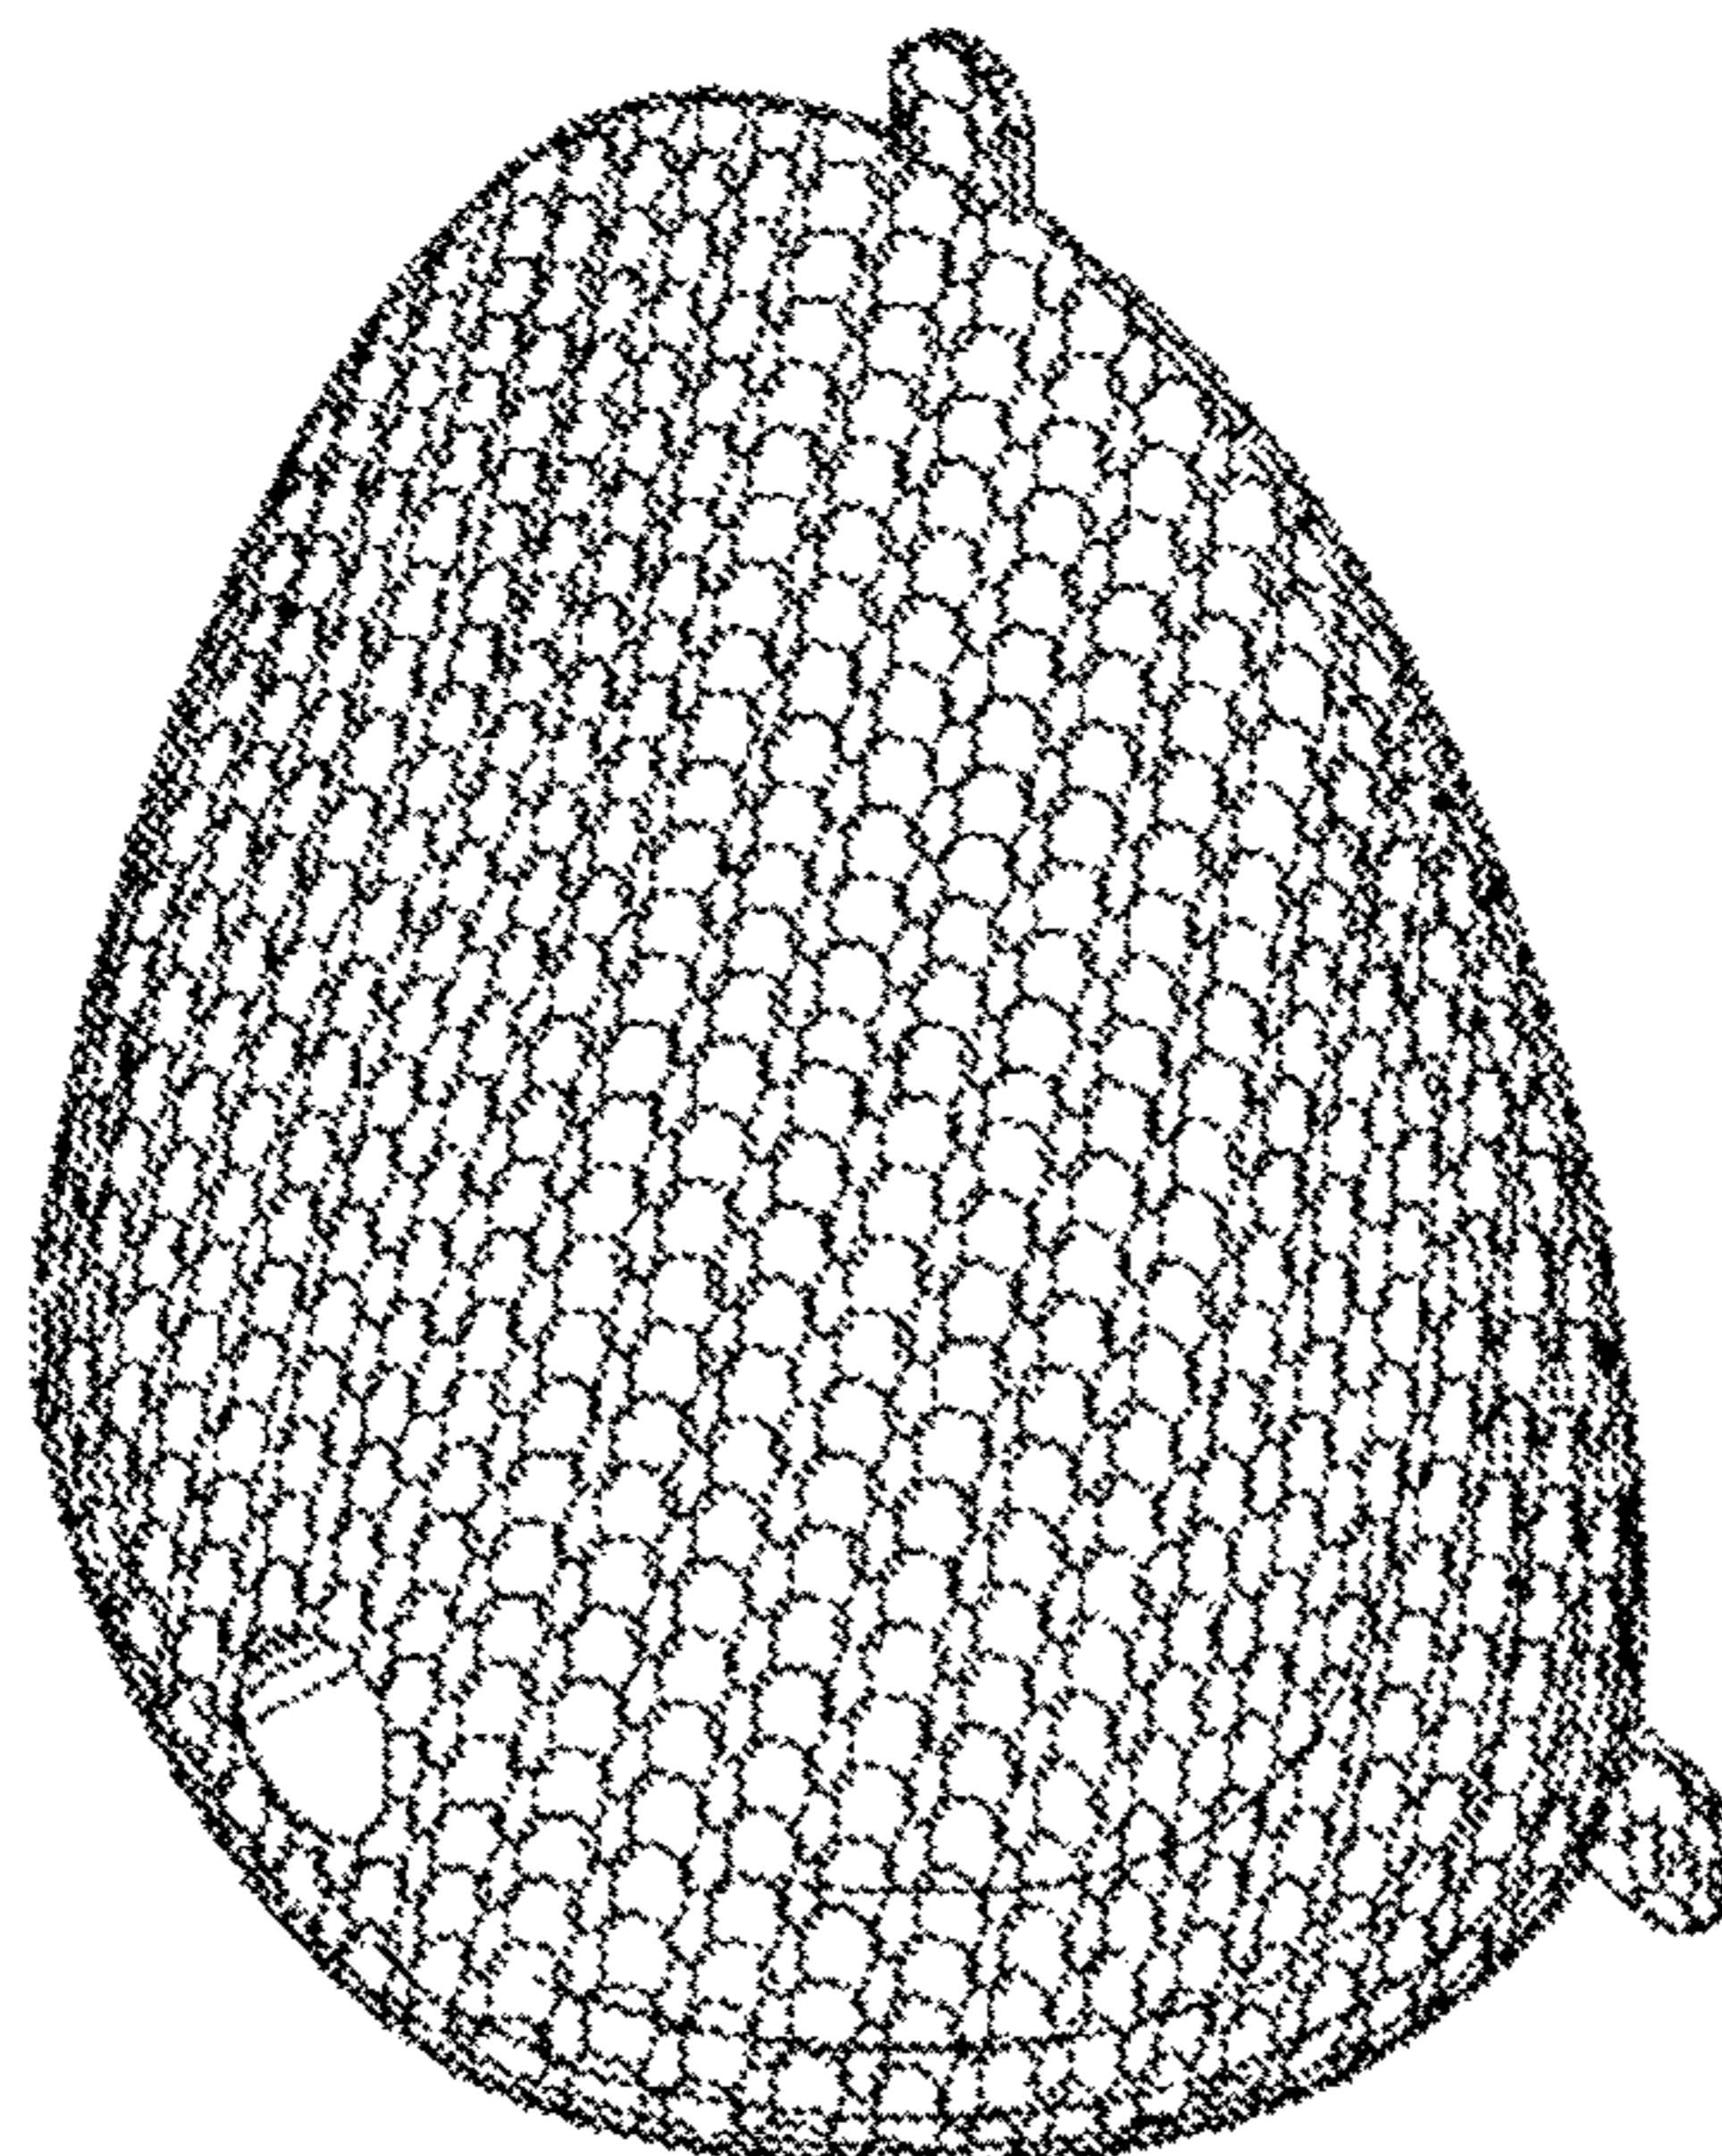



(56)

References Cited

U.S. PATENT DOCUMENTS

6,210,439 B1 4/2001 Firmin et al.  
 6,328,765 B1 12/2001 Hardwick et al.  
 6,368,541 B1 4/2002 Pajotin et al.  
 6,371,831 B1 4/2002 Dodge  
 6,599,323 B2 7/2003 Melican et al.  
 6,723,133 B1 4/2004 Pajotin  
 6,740,122 B1 5/2004 Pajotin  
 6,913,626 B2 7/2005 Mcghan  
 7,081,135 B2 7/2006 Smith et al.  
 D539,506 S 4/2007 Valentin  
 7,476,249 B2 1/2009 Frank  
 7,520,896 B2 4/2009 Benslimane  
 7,670,372 B2 3/2010 Shfaram et al.  
 7,875,074 B2 1/2011 Chen et al.  
 8,007,531 B2 8/2011 Frank  
 8,034,270 B2 10/2011 Martin et al.  
 8,858,629 B2 10/2014 Moses et al.  
 8,911,765 B2 12/2014 Moses et al.  
 8,936,504 B2 1/2015 Deal et al.  
 8,986,377 B2 3/2015 Richter et al.  
 9,532,867 B2 1/2017 Felix et al.  
 9,603,698 B2 3/2017 Kerr et al.  
 9,655,715 B2 5/2017 Limem et al.  
 9,707,073 B2 7/2017 Al-Jasim  
 9,713,350 B1 7/2017 Colburn  
 9,713,524 B2\* 7/2017 Glicksman ..... A61B 90/02  
 D799,152 S 10/2017 Brownell et al.  
 D803,401 S \* 11/2017 Limem ..... D24/155  
 D816,220 S \* 4/2018 Limem ..... D24/155  
 D816,221 S \* 4/2018 Limem ..... D24/155  
 D836,778 S \* 12/2018 Limem ..... D24/155  
 10,363,127 B2 7/2019 Mlodinow et al.  
 D856,517 S \* 8/2019 Spiegel ..... D24/155  
 D857,895 S \* 8/2019 Limem ..... D24/155  
 D870,289 S \* 12/2019 Limem ..... D24/155  
 10,595,986 B2 3/2020 Rehnke  
 2002/0165596 A1 11/2002 Wilson  
 2003/0207649 A1 11/2003 Reeder  
 2006/0167338 A1 7/2006 Shfaram  
 2006/0211334 A1 9/2006 Smith  
 2007/0198085 A1 8/2007 Benslimane  
 2008/0027273 A1\* 1/2008 Gutterman ..... A61B 17/84  
 600/37  
 2008/0082113 A1 4/2008 Bishop et al.  
 2008/0097601 A1 4/2008 Codori-Hurff et al.  
 2009/0082864 A1 3/2009 Chen et al.  
 2009/0240342 A1 9/2009 Lindh, Sr. et al.  
 2009/0248071 A1 10/2009 Saint et al.  
 2010/0042211 A1 2/2010 Epps et al.  
 2010/0137679 A1 6/2010 Lashinski et al.  
 2010/0191330 A1 7/2010 Laurysen et al.  
 2010/0204791 A1 8/2010 Shfaram et al.  
 2010/0217388 A1\* 8/2010 Cohen ..... A61F 2/0059  
 623/8  
 2010/0249924 A1 9/2010 Powell et al.  
 2010/0331612 A1 12/2010 Lashinski et al.  
 2011/0009960 A1 1/2011 Altman et al.  
 2011/0022171 A1 1/2011 Richter et al.  
 2011/0257665 A1 10/2011 Mortarino  
 2011/0264213 A1 10/2011 DeMiranda  
 2012/0004723 A1 1/2012 Mortarino et al.  
 2012/0021738 A1 1/2012 Koo et al.  
 2012/0022646 A1 1/2012 Mortarino et al.  
 2012/0158134 A1 6/2012 Codori-Hurff et al.  
 2012/0185041 A1 7/2012 Mortarino et al.  
 2012/0221105 A1 8/2012 Altman et al.  
 2012/0232653 A1 9/2012 Saint et al.  
 2012/0266348 A1 10/2012 Meginnis  
 2012/0283826 A1 11/2012 Moses et al.  
 2013/0066423 A1 3/2013 Bishop et al.  
 2013/0103149 A1 4/2013 Altman et al.  
 2013/0178699 A1 7/2013 Saint et al.  
 2013/0178875 A1 7/2013 Horton et al.  
 2013/0253645 A1 9/2013 Kerr et al.  
 2013/0304098 A1 11/2013 Mortarino

2014/0081398 A1 3/2014 Mejia et al.  
 2014/0200396 A1 7/2014 Lashinski et al.  
 2014/0222146 A1 8/2014 Moses et al.  
 2014/0222161 A1 8/2014 Mathisen  
 2014/0276997 A1 9/2014 Harrah et al.  
 2015/0012089 A1 1/2015 Shetty et al.  
 2015/0018946 A1 1/2015 Guterma  
 2015/0056131 A1 2/2015 Bernasconi et al.  
 2015/0223928 A1 8/2015 Limem et al.  
 2015/0351899 A1 12/2015 Mortarino  
 2015/0351900 A1\* 12/2015 Glicksman ..... A61B 90/94  
 623/8  
 2016/0038269 A1 2/2016 Altman et al.  
 2016/0151138 A1 6/2016 Guterma et al.  
 2016/0310262 A1 10/2016 Doucet et al.  
 2019/0247180 A1 8/2019 Limem et al.

FOREIGN PATENT DOCUMENTS

WO 2007004214 A3 5/2007  
 WO 2009/001293 A1 12/2008  
 WO 2011/119742 A2 9/2011  
 WO 2012122215 A2 9/2012  
 WO 2019094861 A1 5/2019  
 WO 2019119060 A1 6/2019

OTHER PUBLICATIONS

“GalaFLEX Mesh,” Tepha Inc., www.galateasurgical.com, P/N 400124, Rev.A, Oct. 2013.  
 Auclair, et al, “Repair of mammary ptosis by insertion of an internal absorbable support and periareolar scar,” Ann Chir Plast Esthet, 1993, 38, No. 1, pp. 107-113.  
 DeBruijn, et al, “Mastopexy with Mesh Reinforcement: The Mechanical Characteristics of Polyester Mesh in the Female Breast,” Plast. Reconstr. Surg. 124: 364, 2009.  
 European Search and Opinion dated Jul. 3, 2017, for 12754773.5-1666.  
 Goes, “Periareolar mammoplasty: double skin technique with application of polyglactine or mixed mesh,” Plast. Reconstr. Surg., 97-859-68 (1996).  
 Goes, “Periareolar mammoplasty: double-skin technique with application of mesh support,” Clin Plastic Surg 29 (2002) 349-364.  
 Goes, “Periareolar Mastopexy with FortaPerm,” Aesth. Plast. Surg., 34-350-8, 2010.  
 Hans P. deBrujin, Siegmund Johannes, “Mastopexy with 3D Preshaped Mesh for Long Term Results: Development of the Internal Bra System,” Aesth Plast Surg., 32:757-765, DOI 10.1007/s00266-008-9186-y, 2008.  
 Johnson, “Central core reduction mammoplasties and Marlex suspension of breast tissue”.  
 Malluci, Concepts in aesthetic breast dimensions: Analysis of the ideal breast, Journal of Plastic, Reconstructive & Aesthetic Surgery (2012) 65, pp. 8-16.  
 Malluci, Population Analysis of the Perfect Breast: A Morphometric Analysis, (2014), www.PRSJournal.com, vol. 134, No. 3 • the Perfect Breast, pp. 436-447.  
 P. van Deventer, Improving the Longevity and Results of Mastopexy and Breast Reduction Procedures: Reconstructing an Internal Breast Support System with Biocompatible Mesh to Replace the Supporting Function of the Ligamentous Suspension, Aesth Plast Surg (2012) 36:578-589DOI 10.1007/s00266-011-9845-2.  
 Supplementary European Search Report of the EPO dated Jul. 30, 2014, EP 12754773.5 from PCT/US2012/027075.  
 Williams, “Poly-4-hydroxybutyrate (P4HB): a new generation of resorbable medical devices for tissue repair and regeneration,” DOI 10.1515/bmt-2013-0009 Biomed Tech 2013; 58(5): 439-452.  
 Written Opinion of IPEA dated Jun. 15, 2015 for PCT/US2014/046420.  
 Written Opinion of ISR dated Nov. 5, 2012 for PCT/US2012/027975.  
 U.S. Appl. No. 16/589,903, filed Sep. 30, 2019, Skander Limem.  
 U.S. Appl. No. 62/939,786, filed Nov. 25, 2019, Skander Limem.

(56)

**References Cited**

OTHER PUBLICATIONS

Goes, Periareolar Mammoplasty: Double Skin Technique with Application of Polyglactine or Mixed Mesh, *Plastic Reconstructive Surg.*, vol .97, No. 5, Apr. 1996, 960-968.

International Search Report for PCT/US2019/015849, Dated Apr. 23, 2019.

Malluci, Design for Natural Breast Augmentation: The ICE Principle, *Plastic and Reconstructive Surgery*, Jun. 2016, vol. 137. No. 6, 1728-1737.

\* cited by examiner



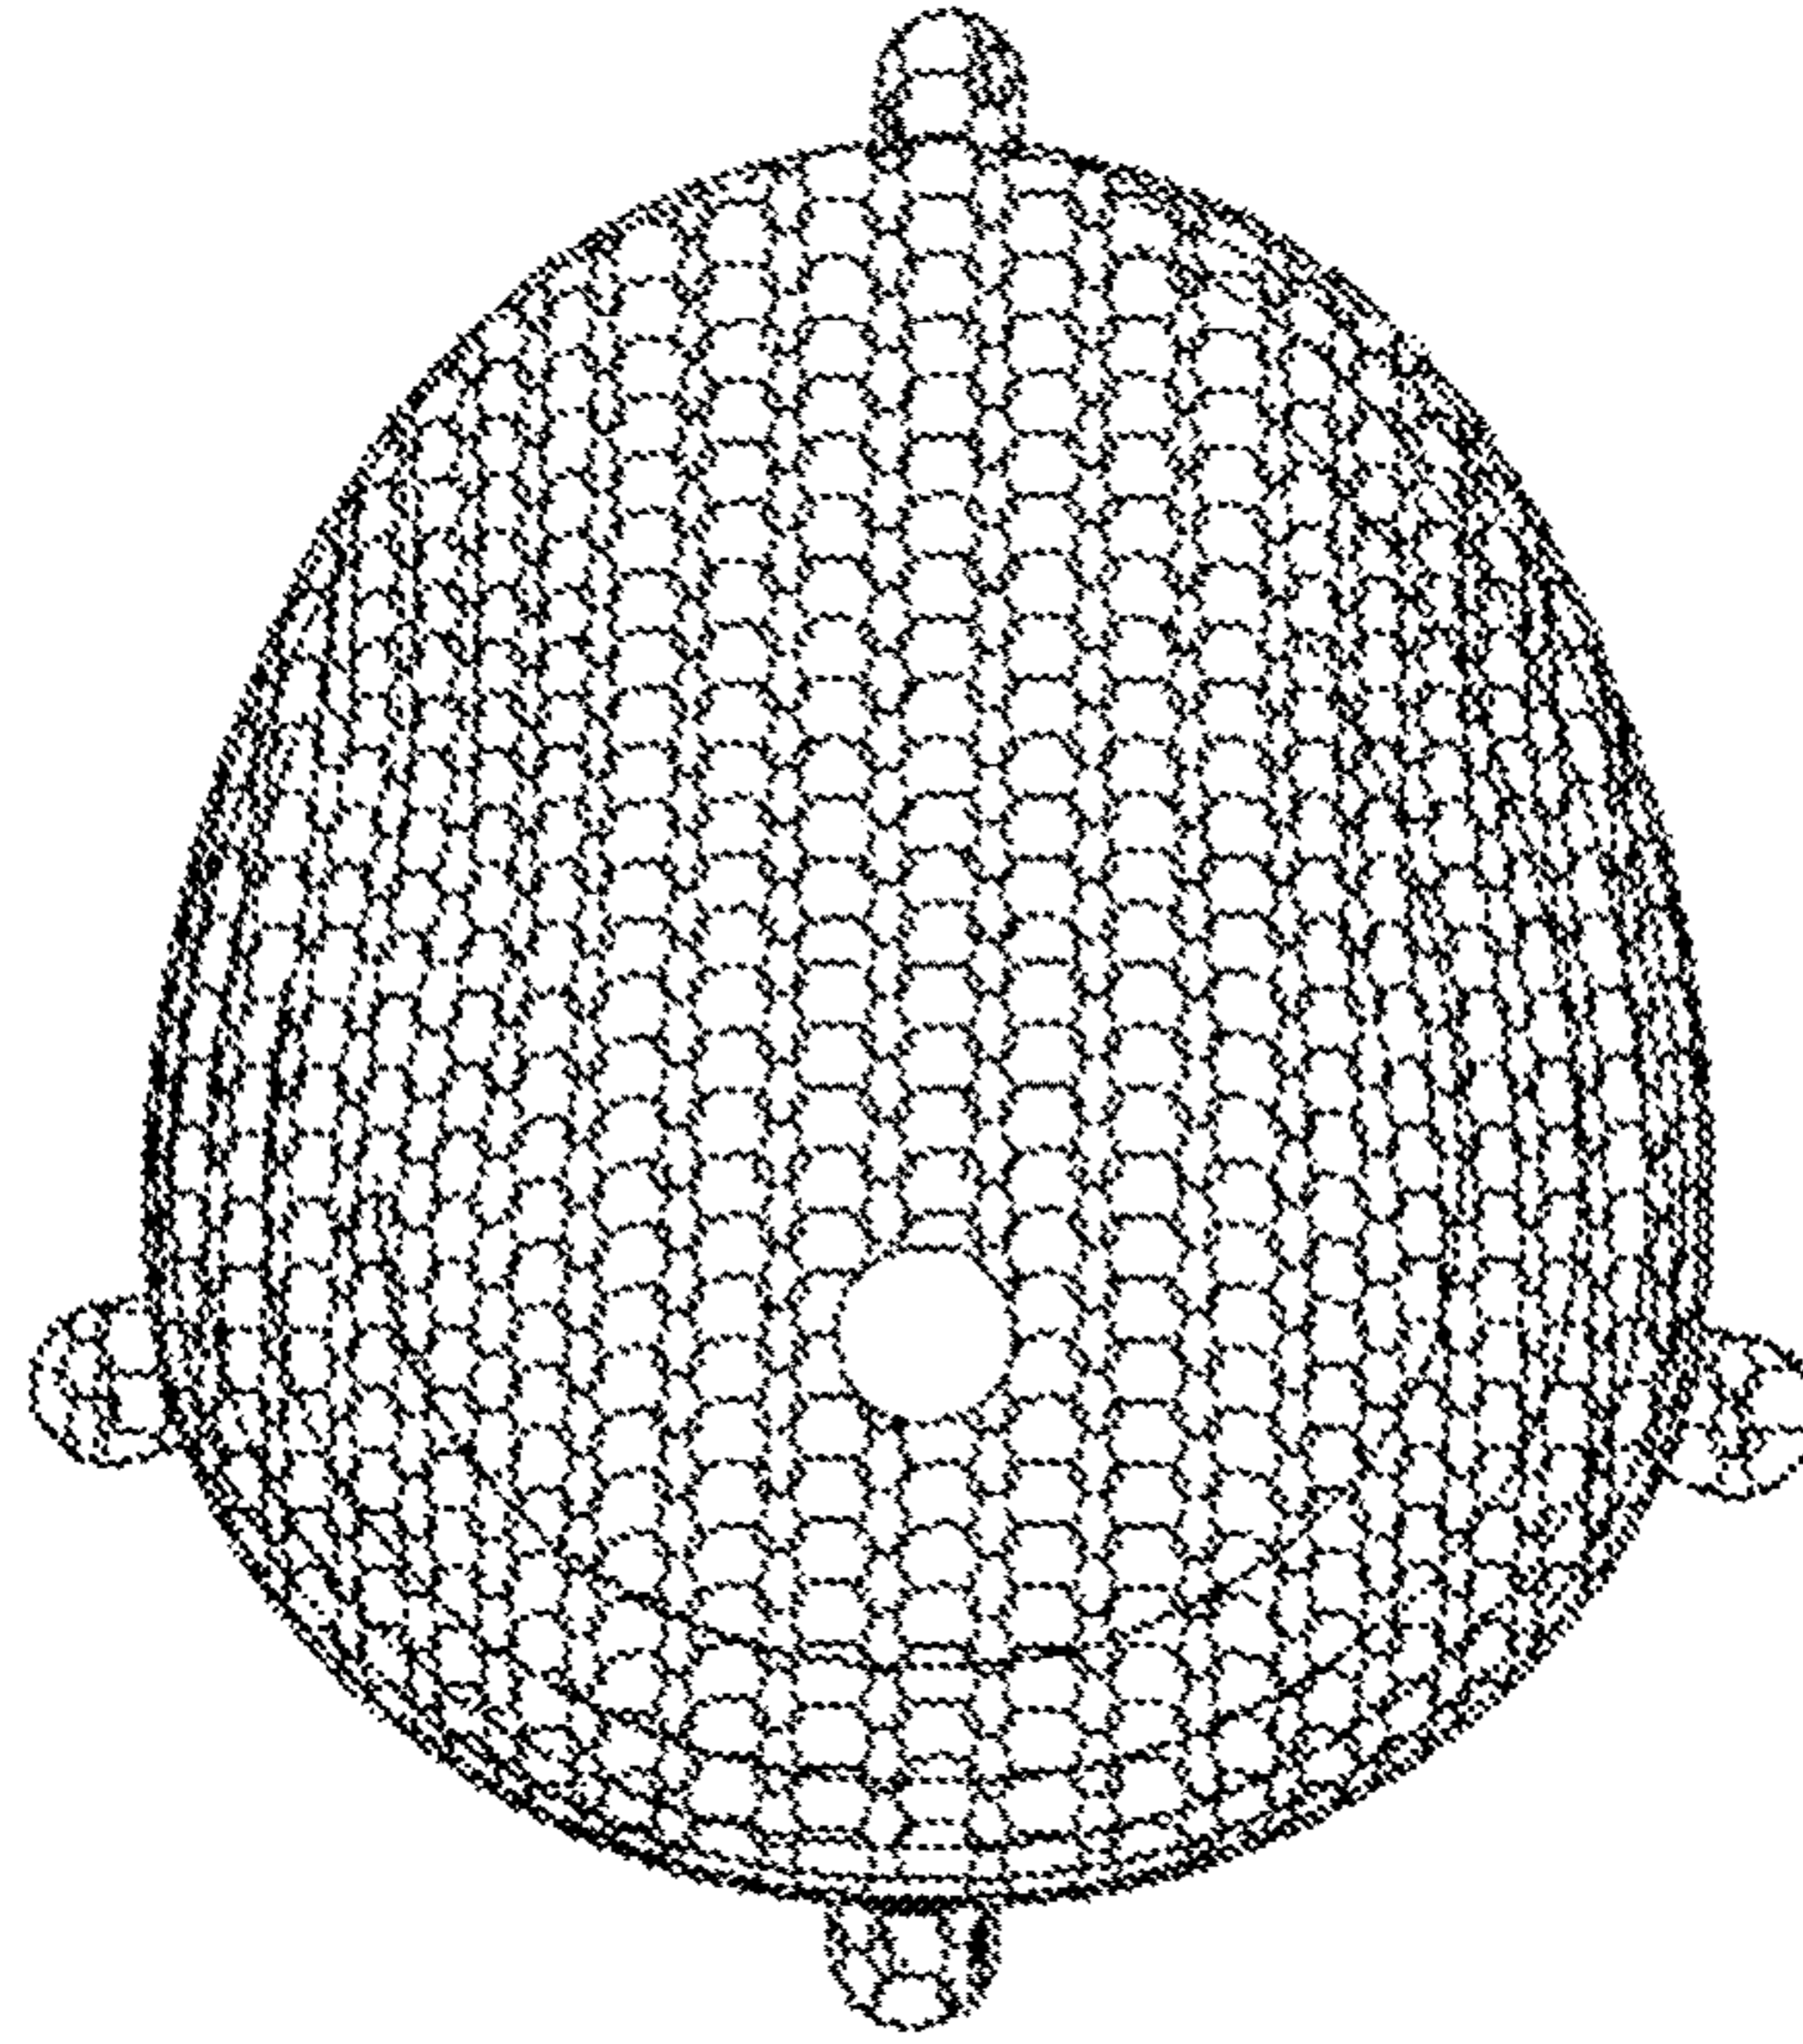


Figure 1

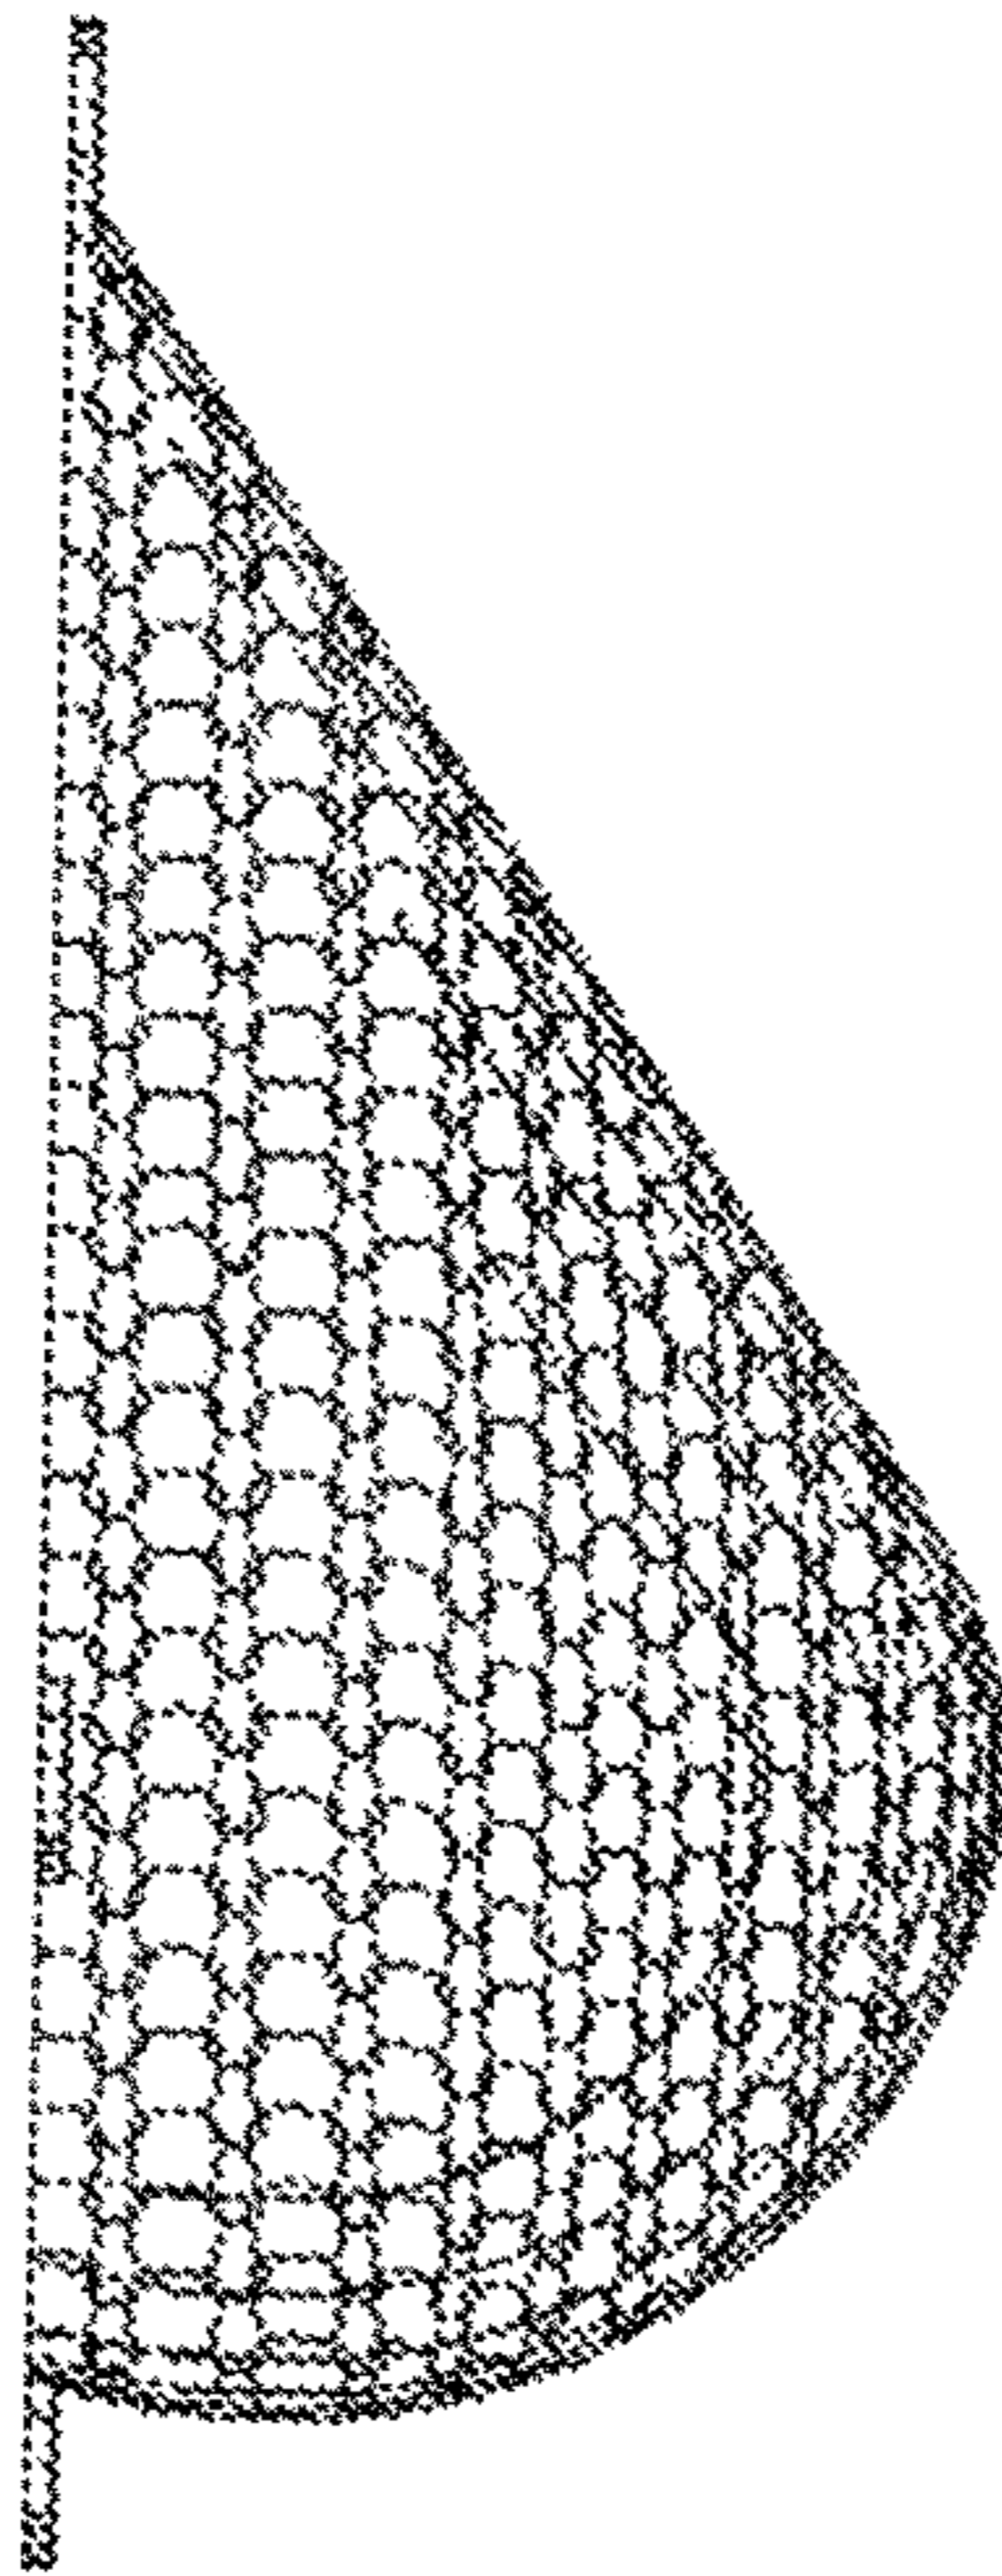


Figure 2

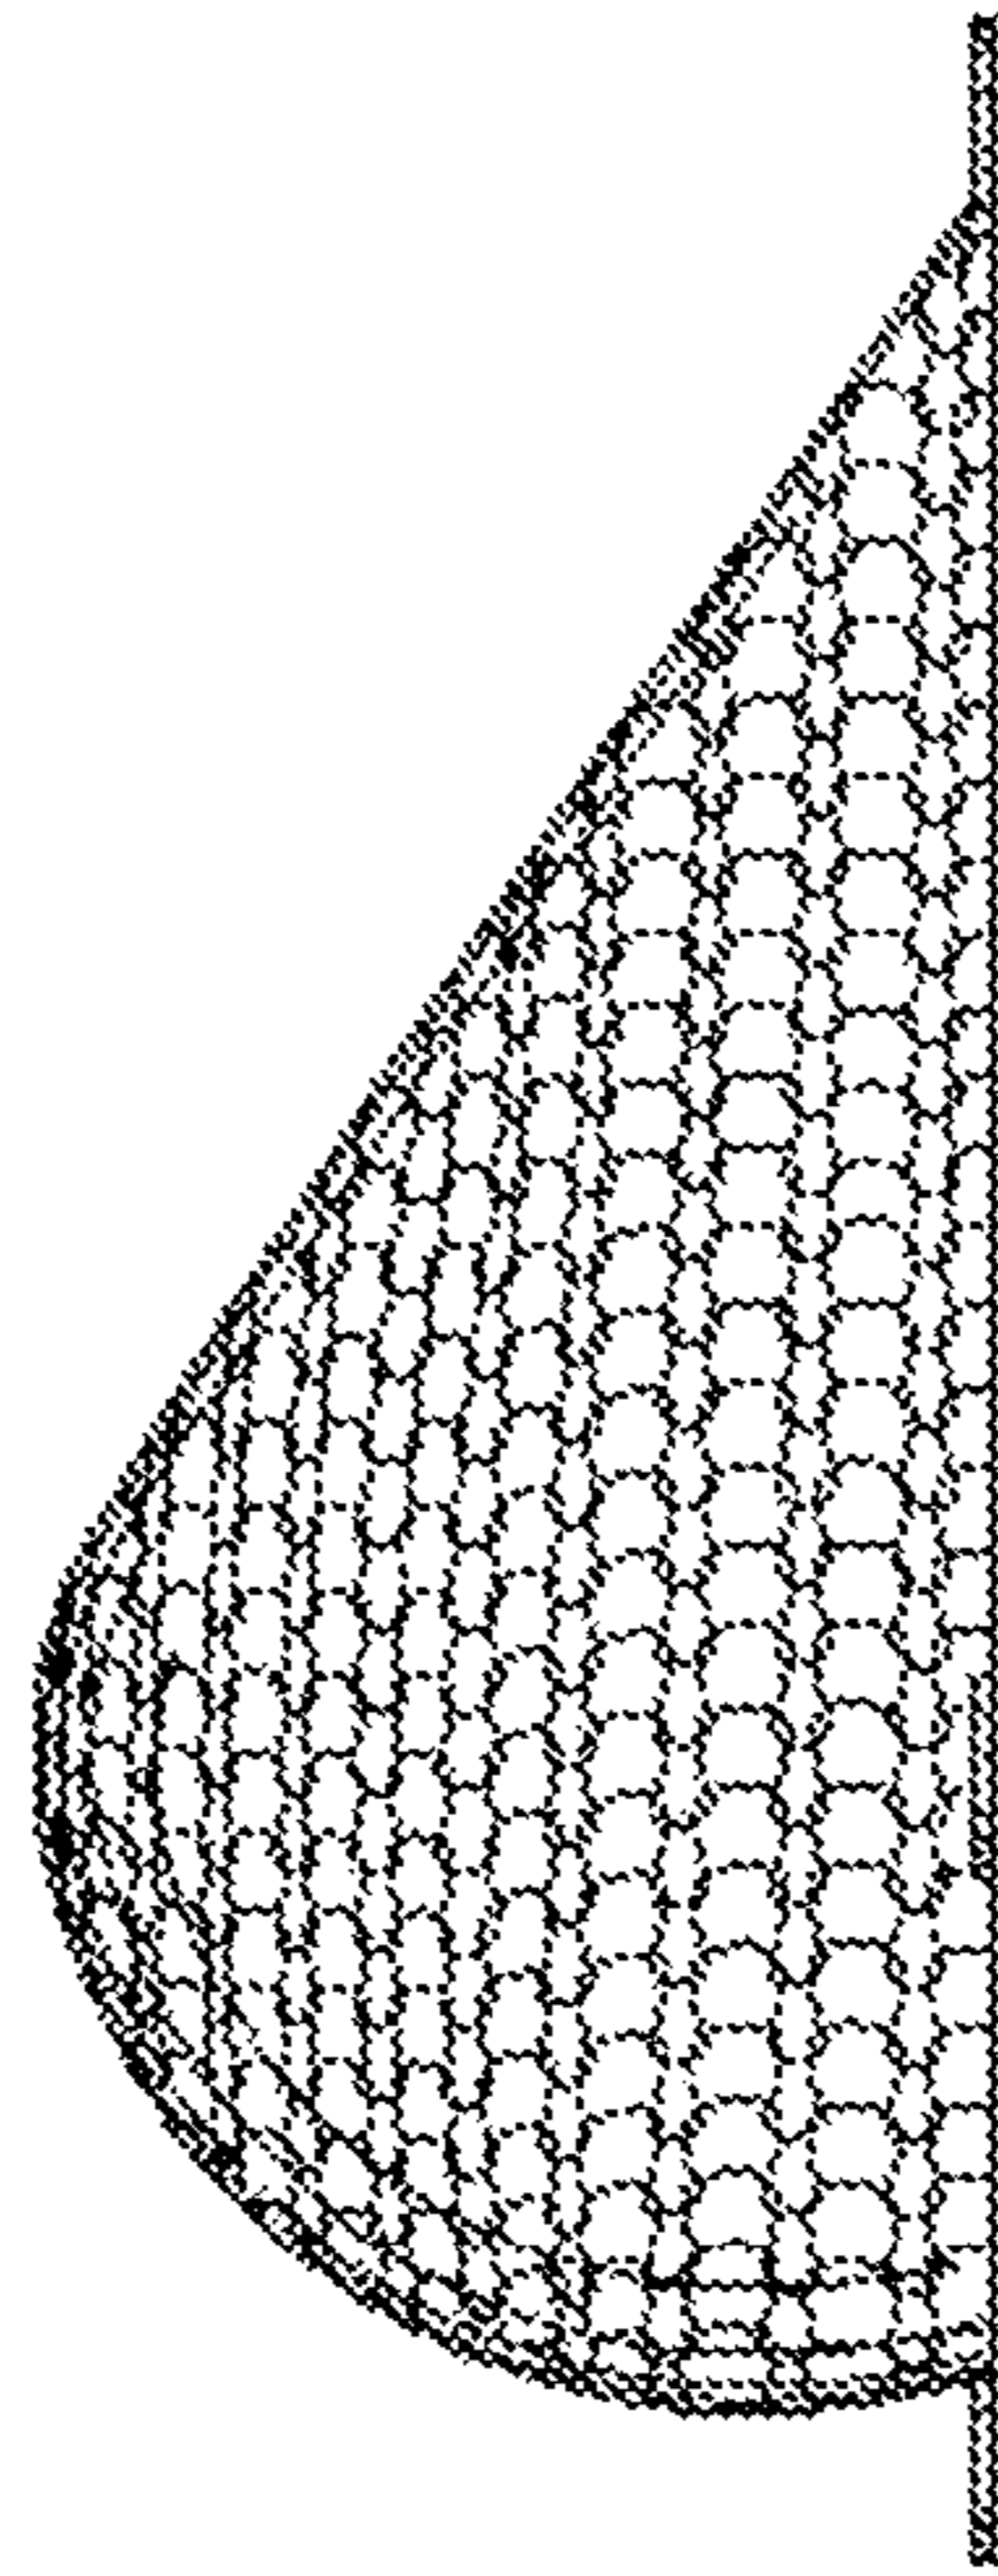


Figure 3

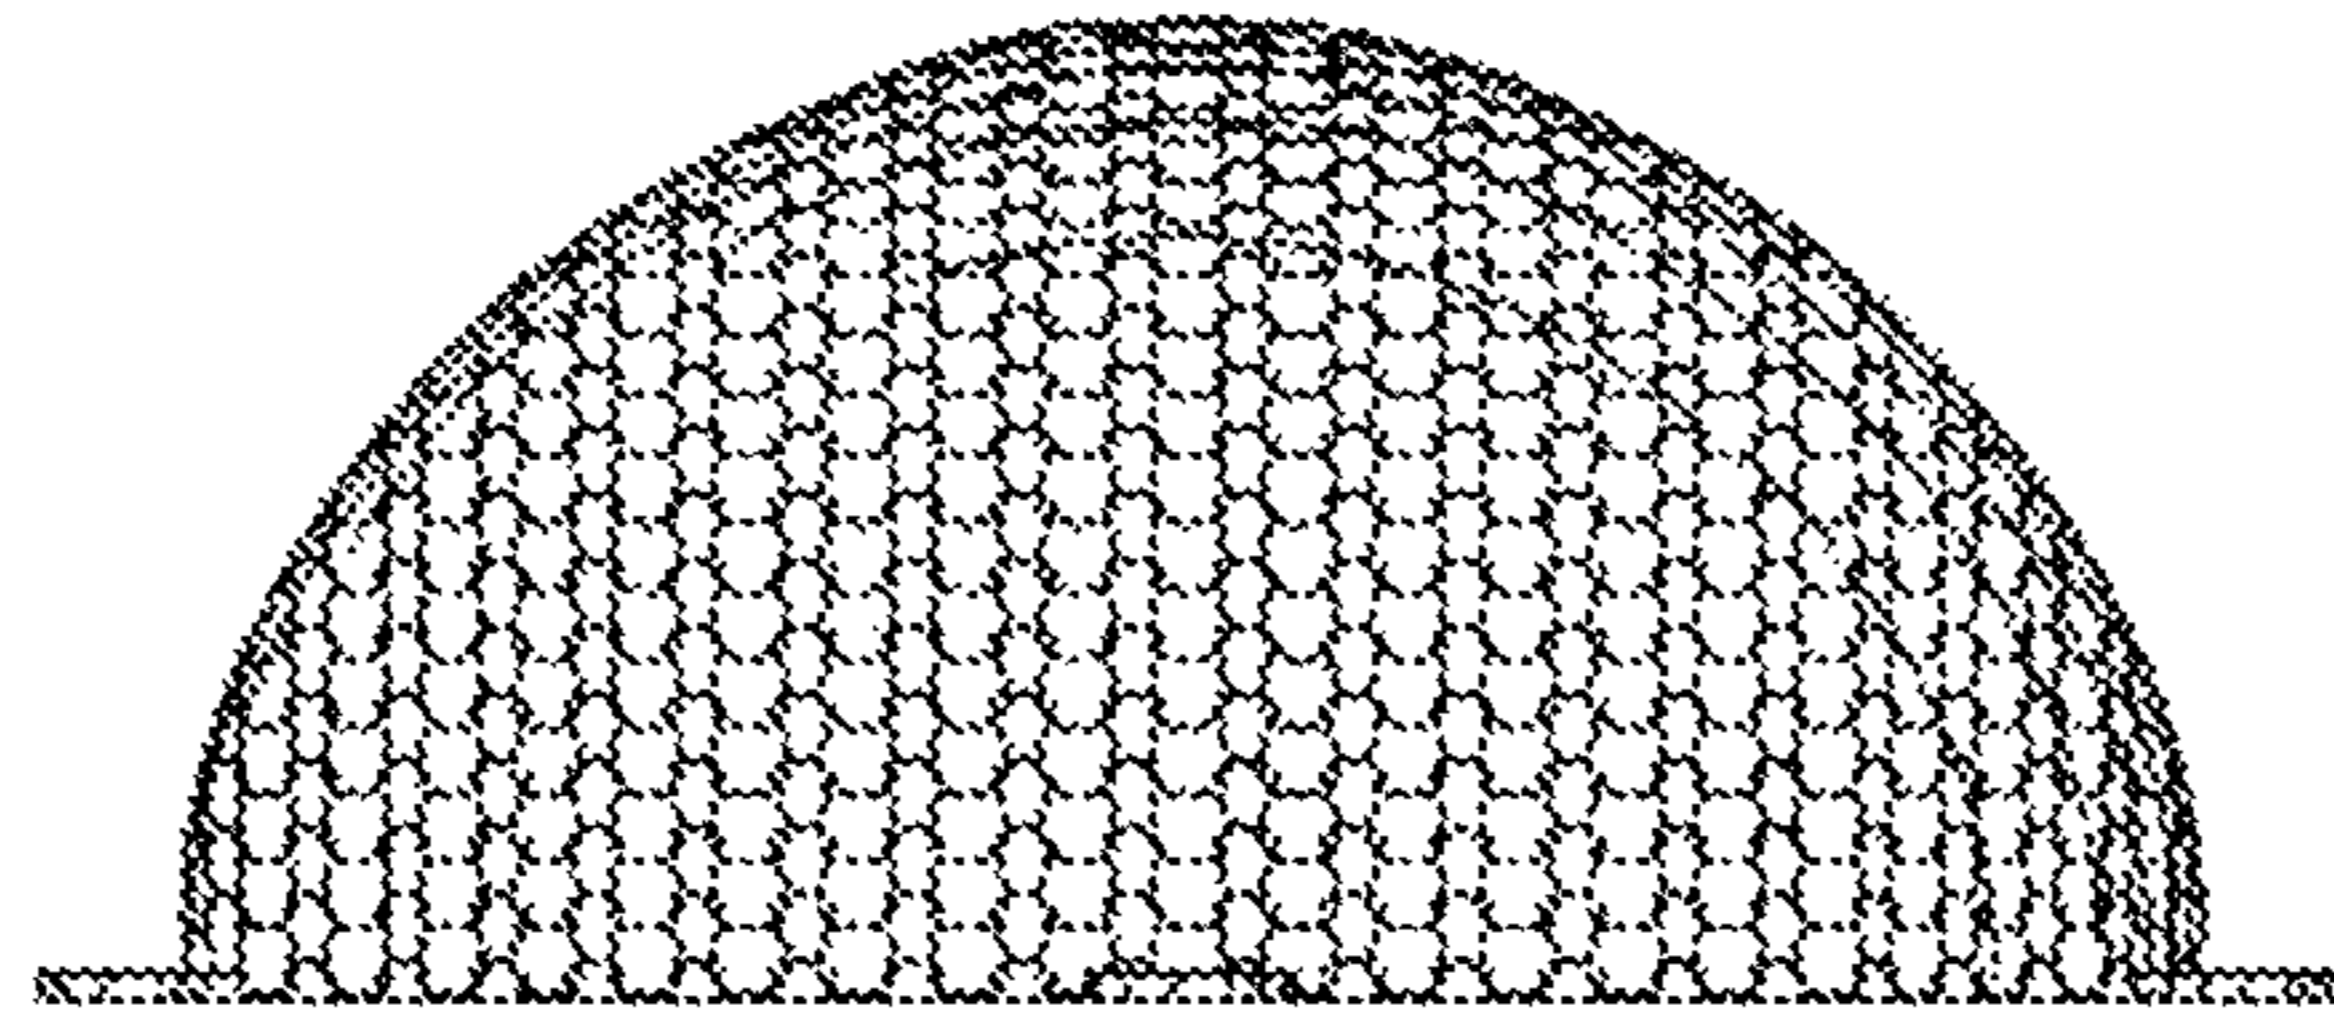


Figure 4

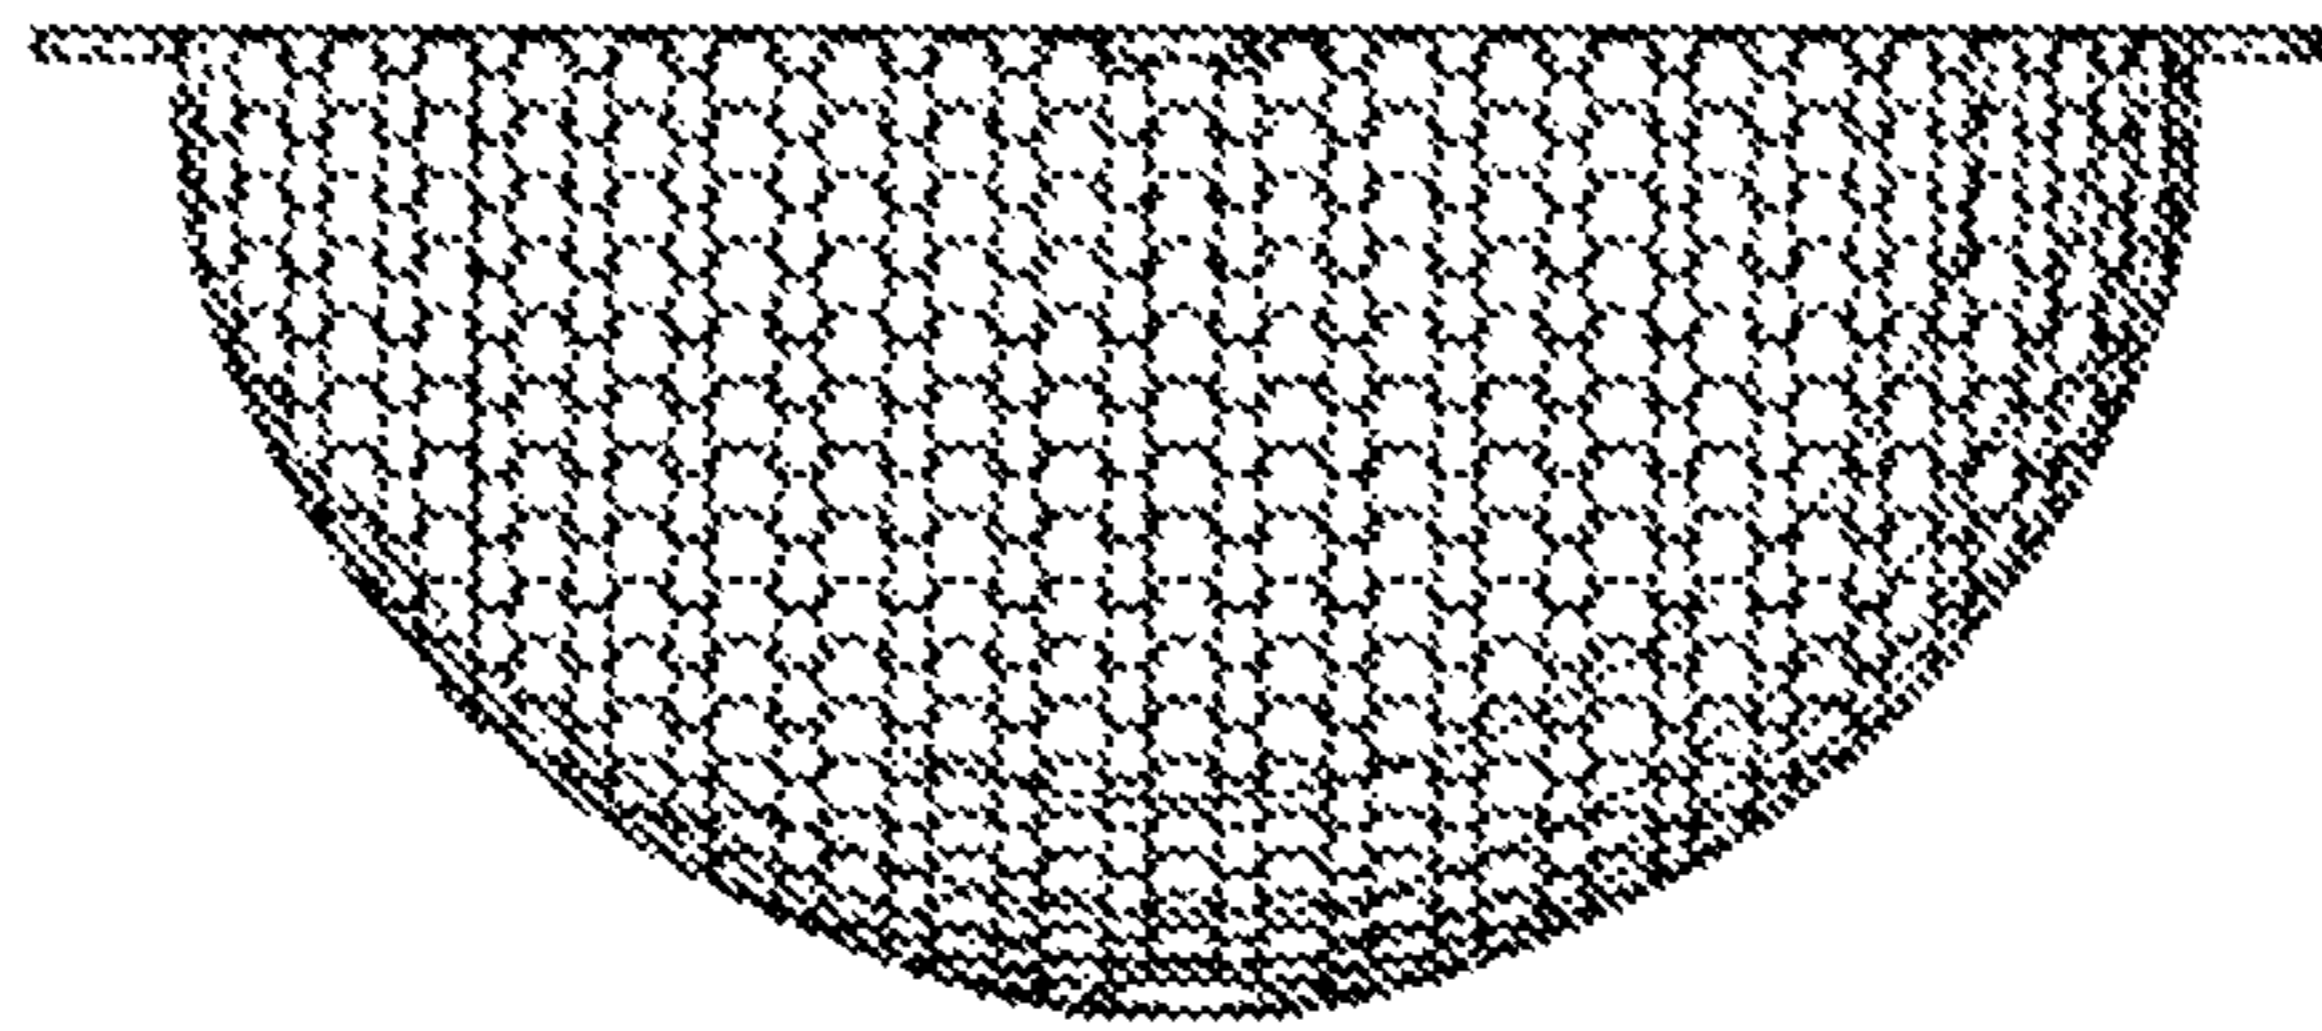


Figure 5



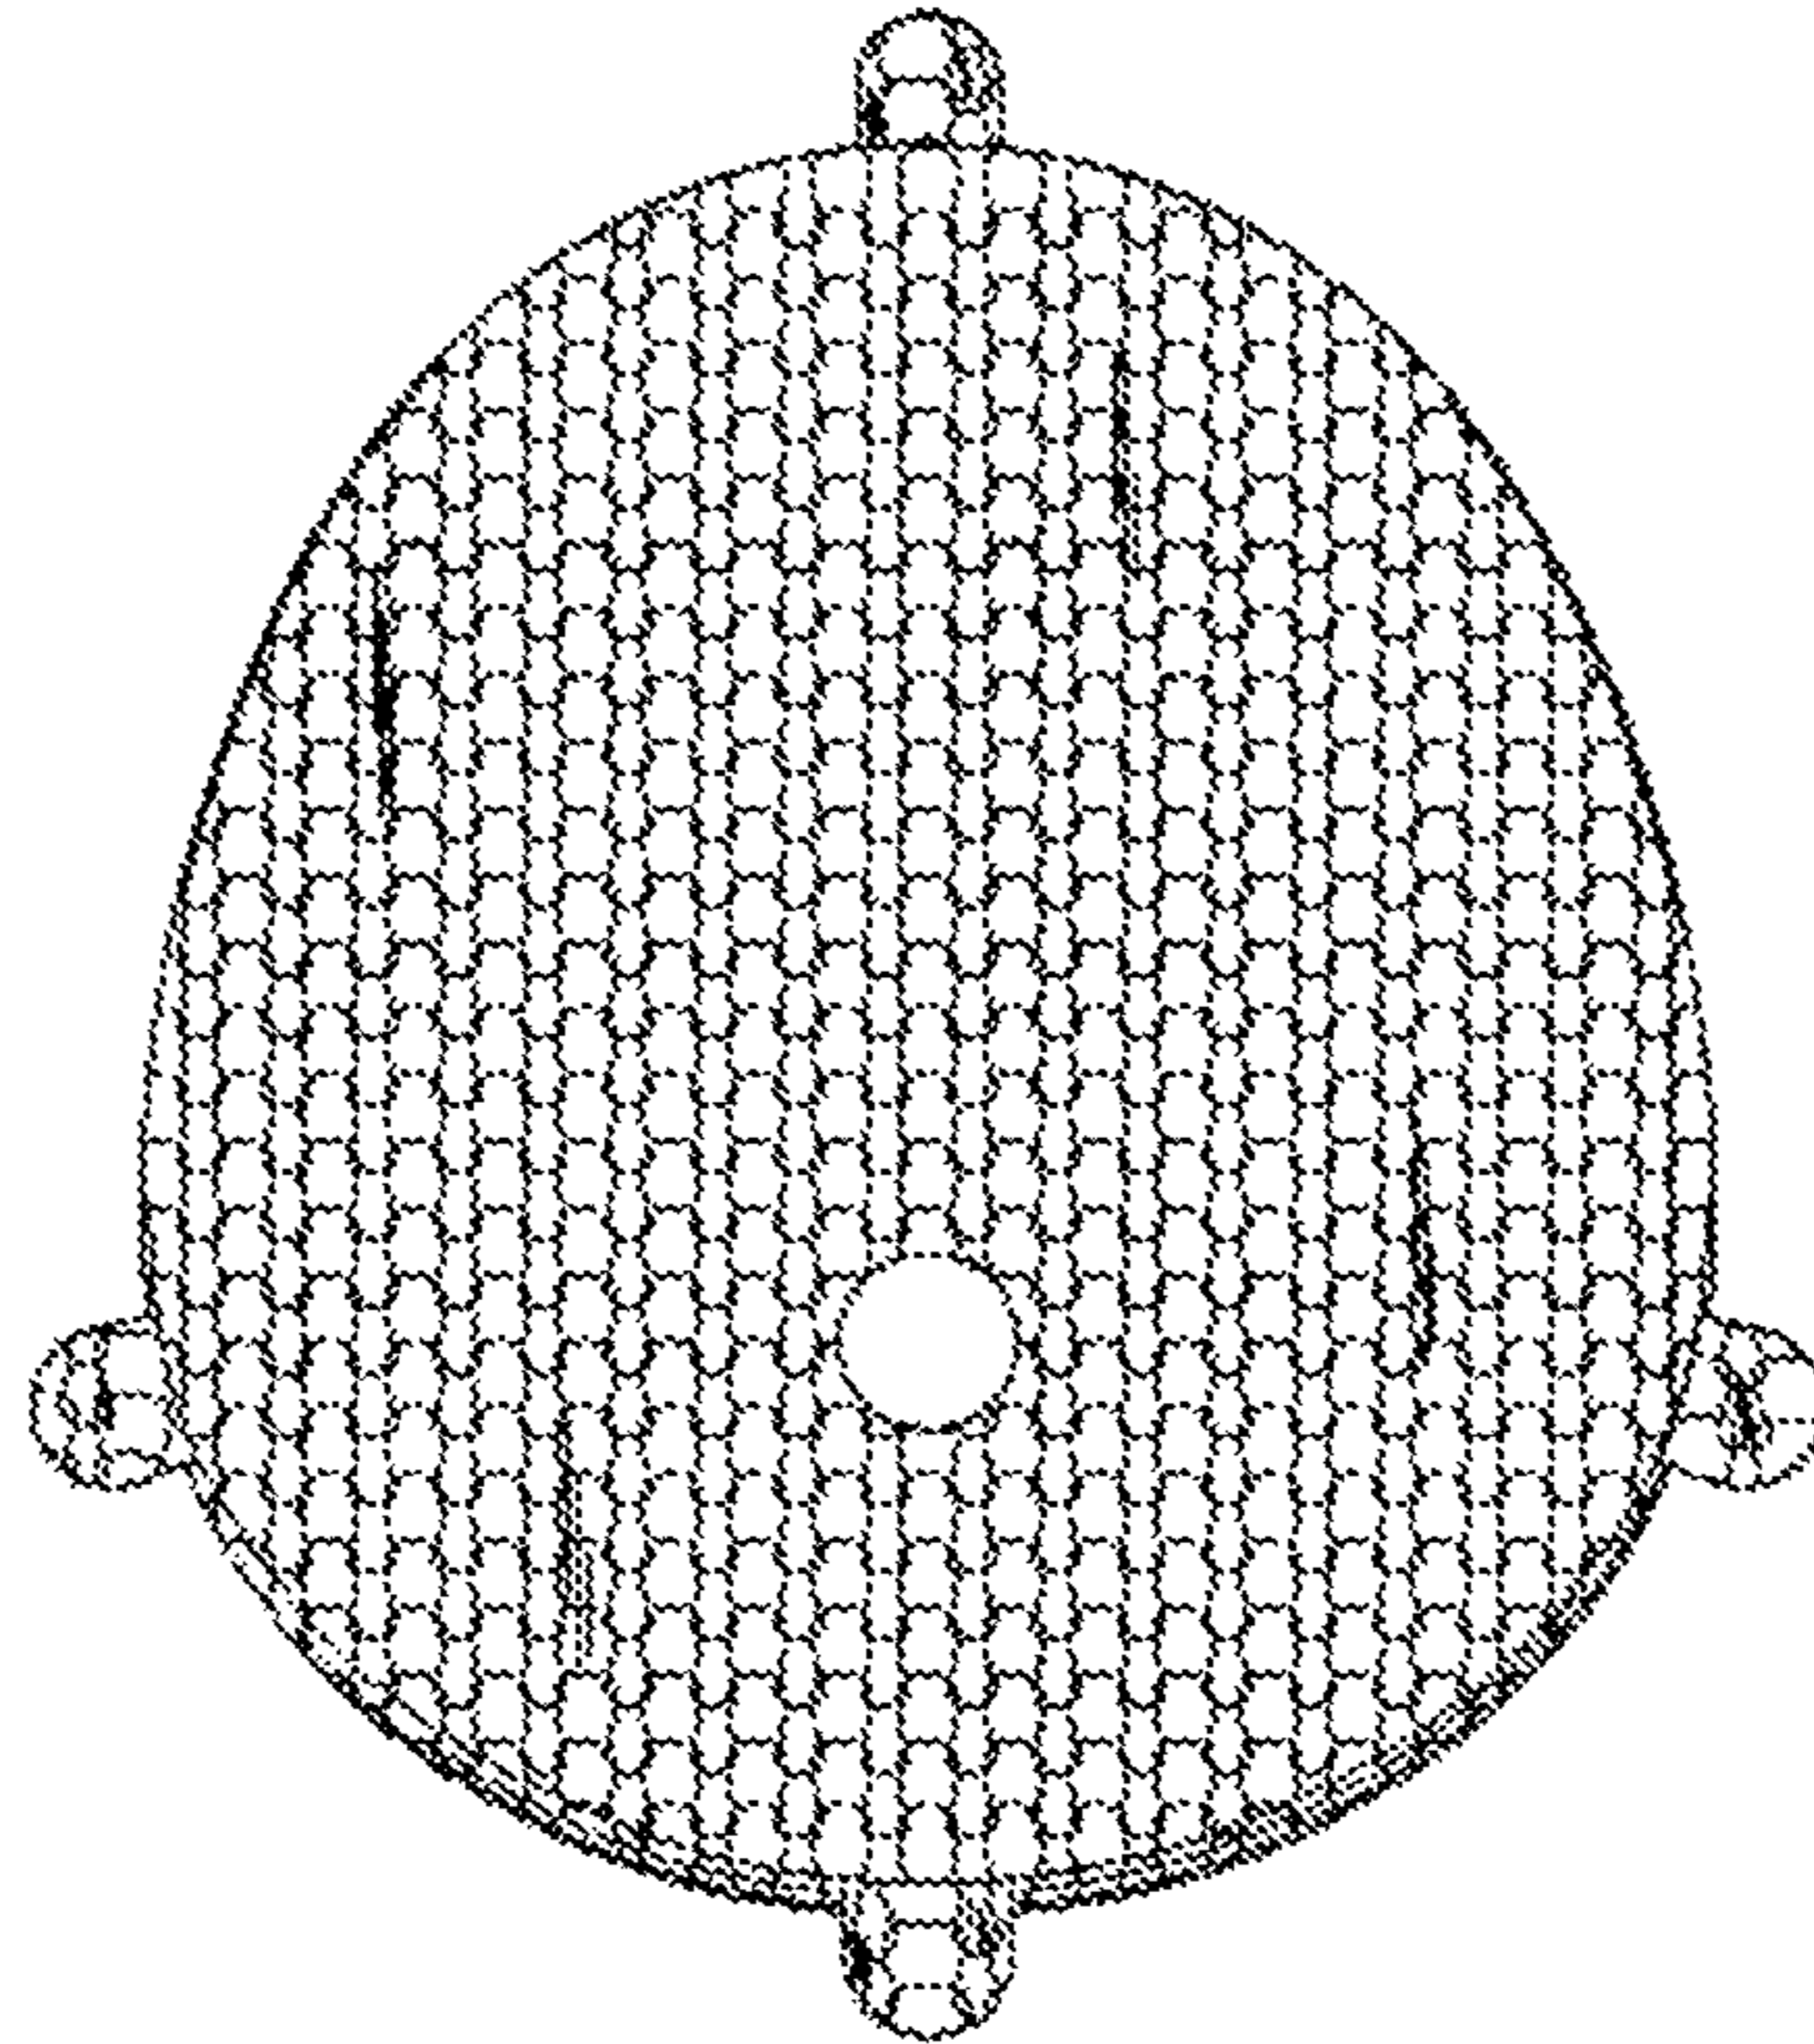


Figure 6

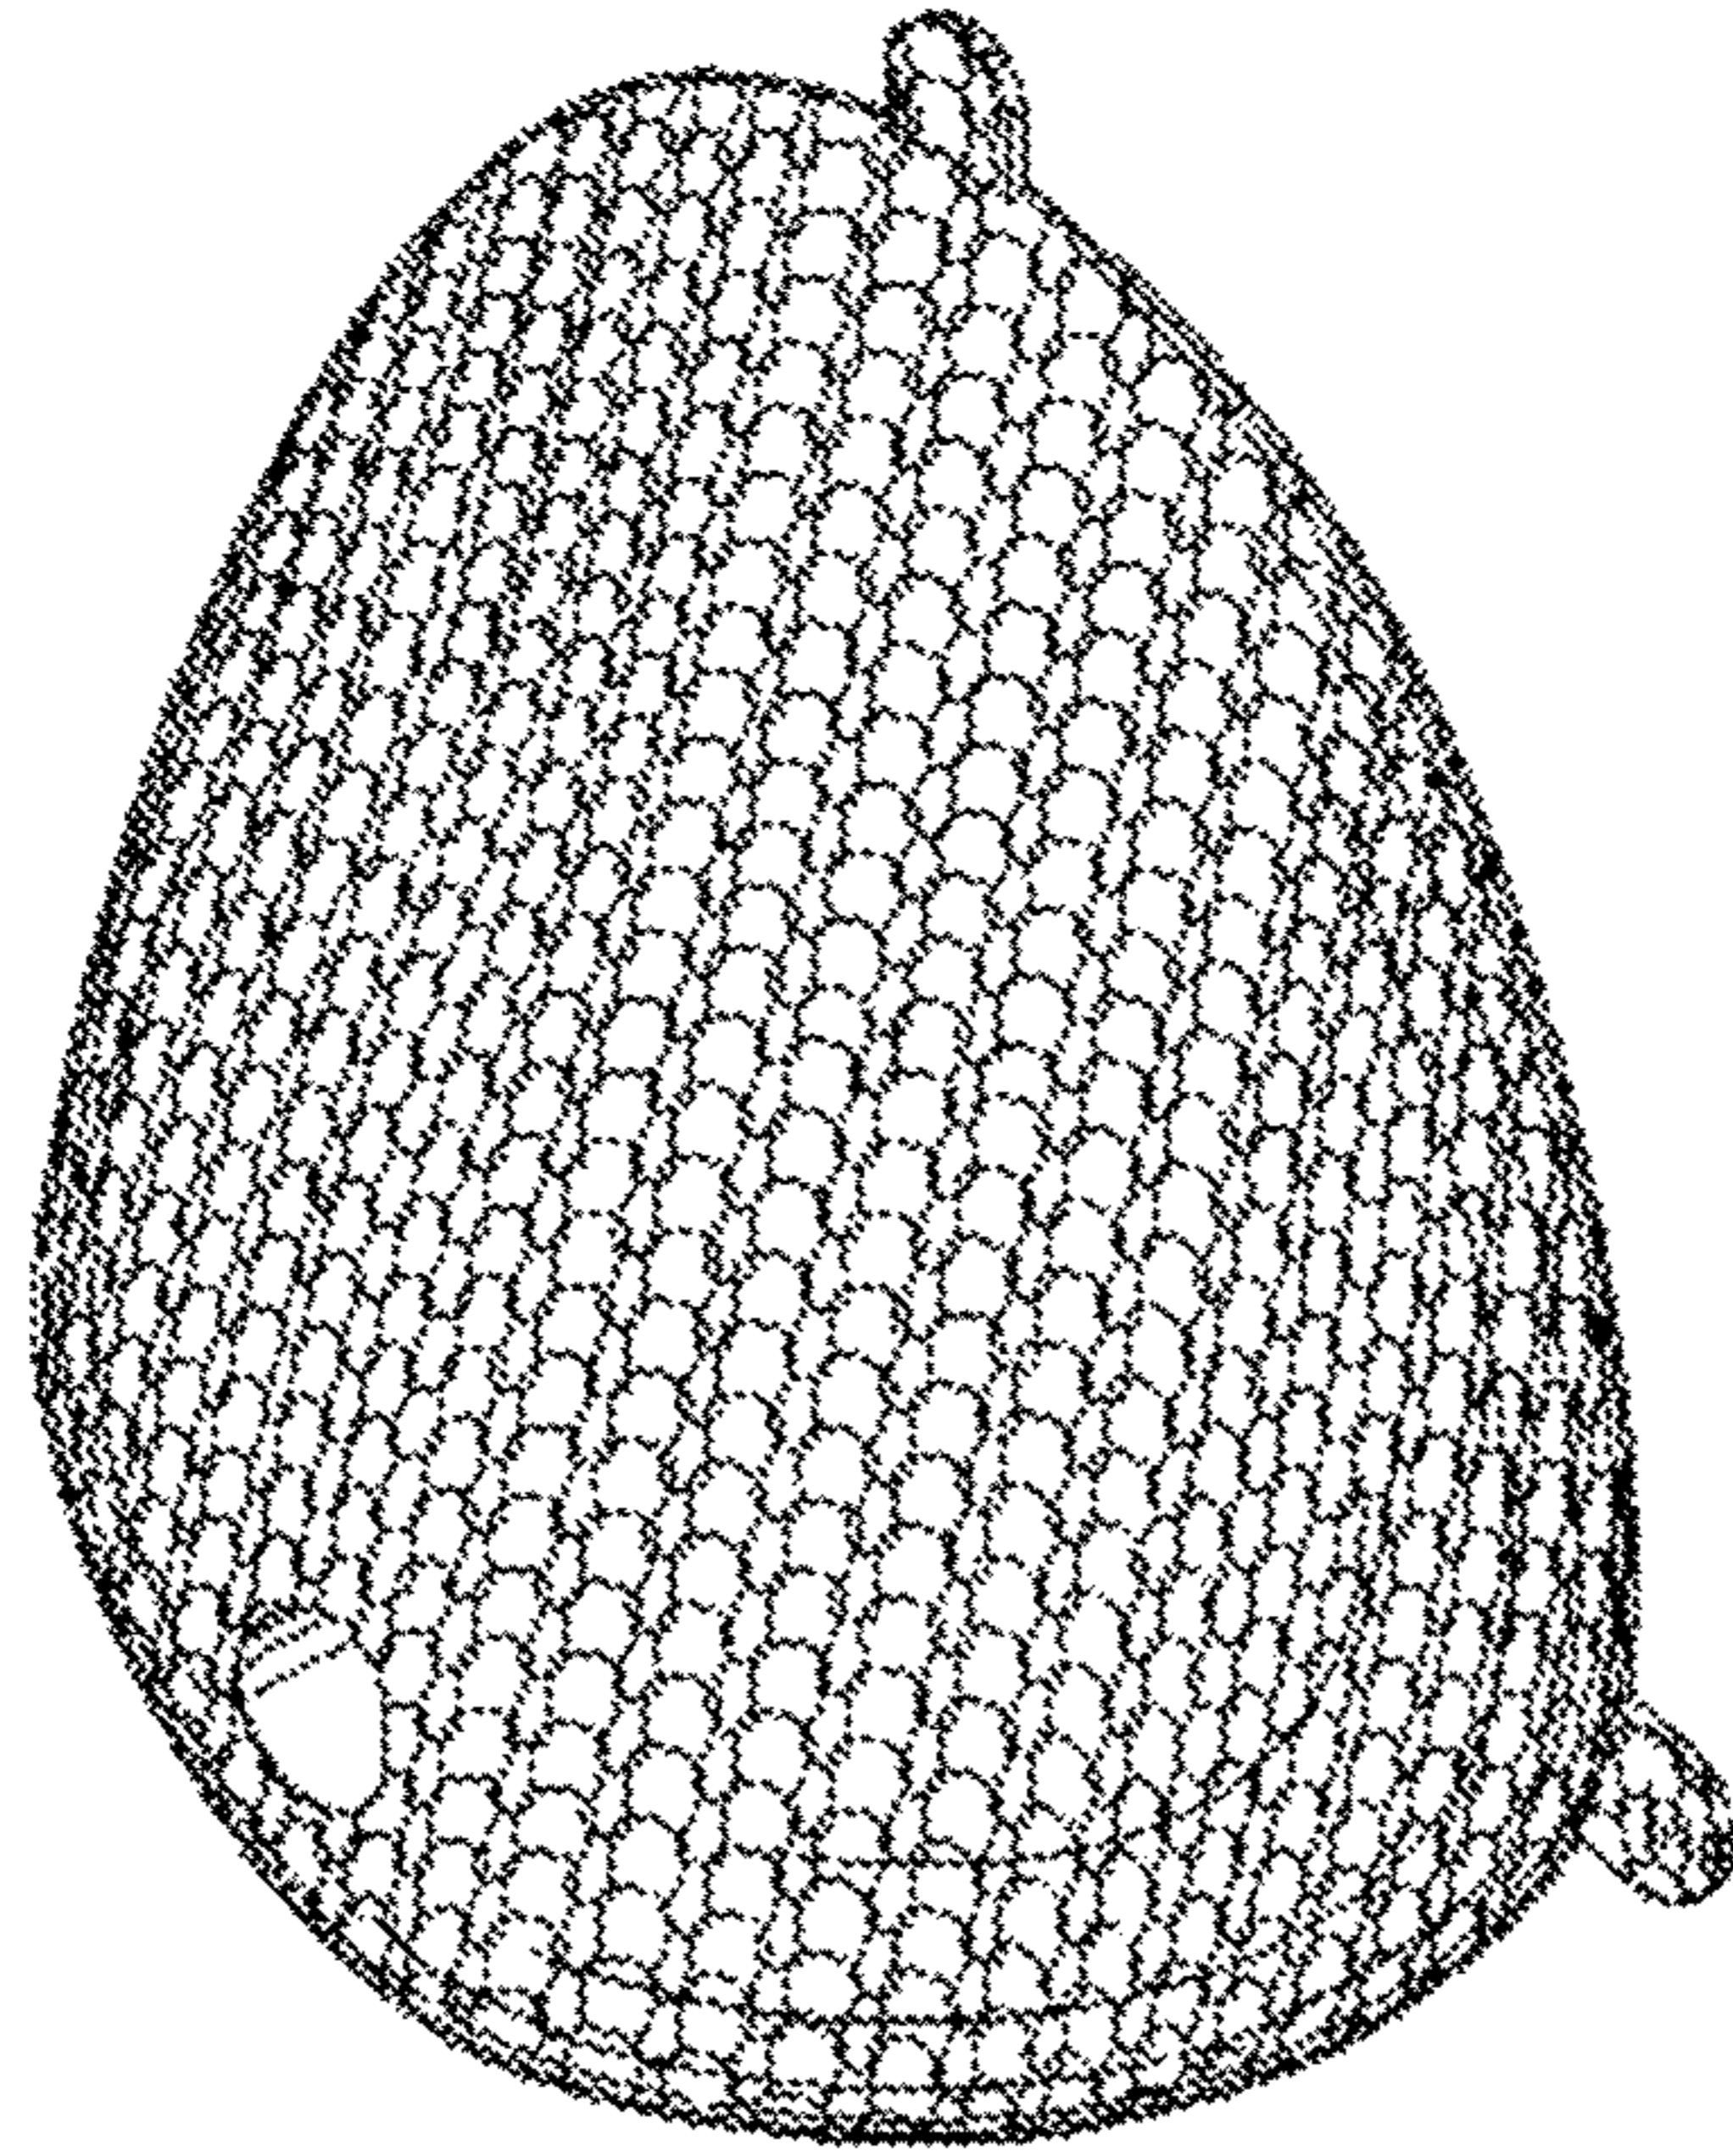


Figure 7

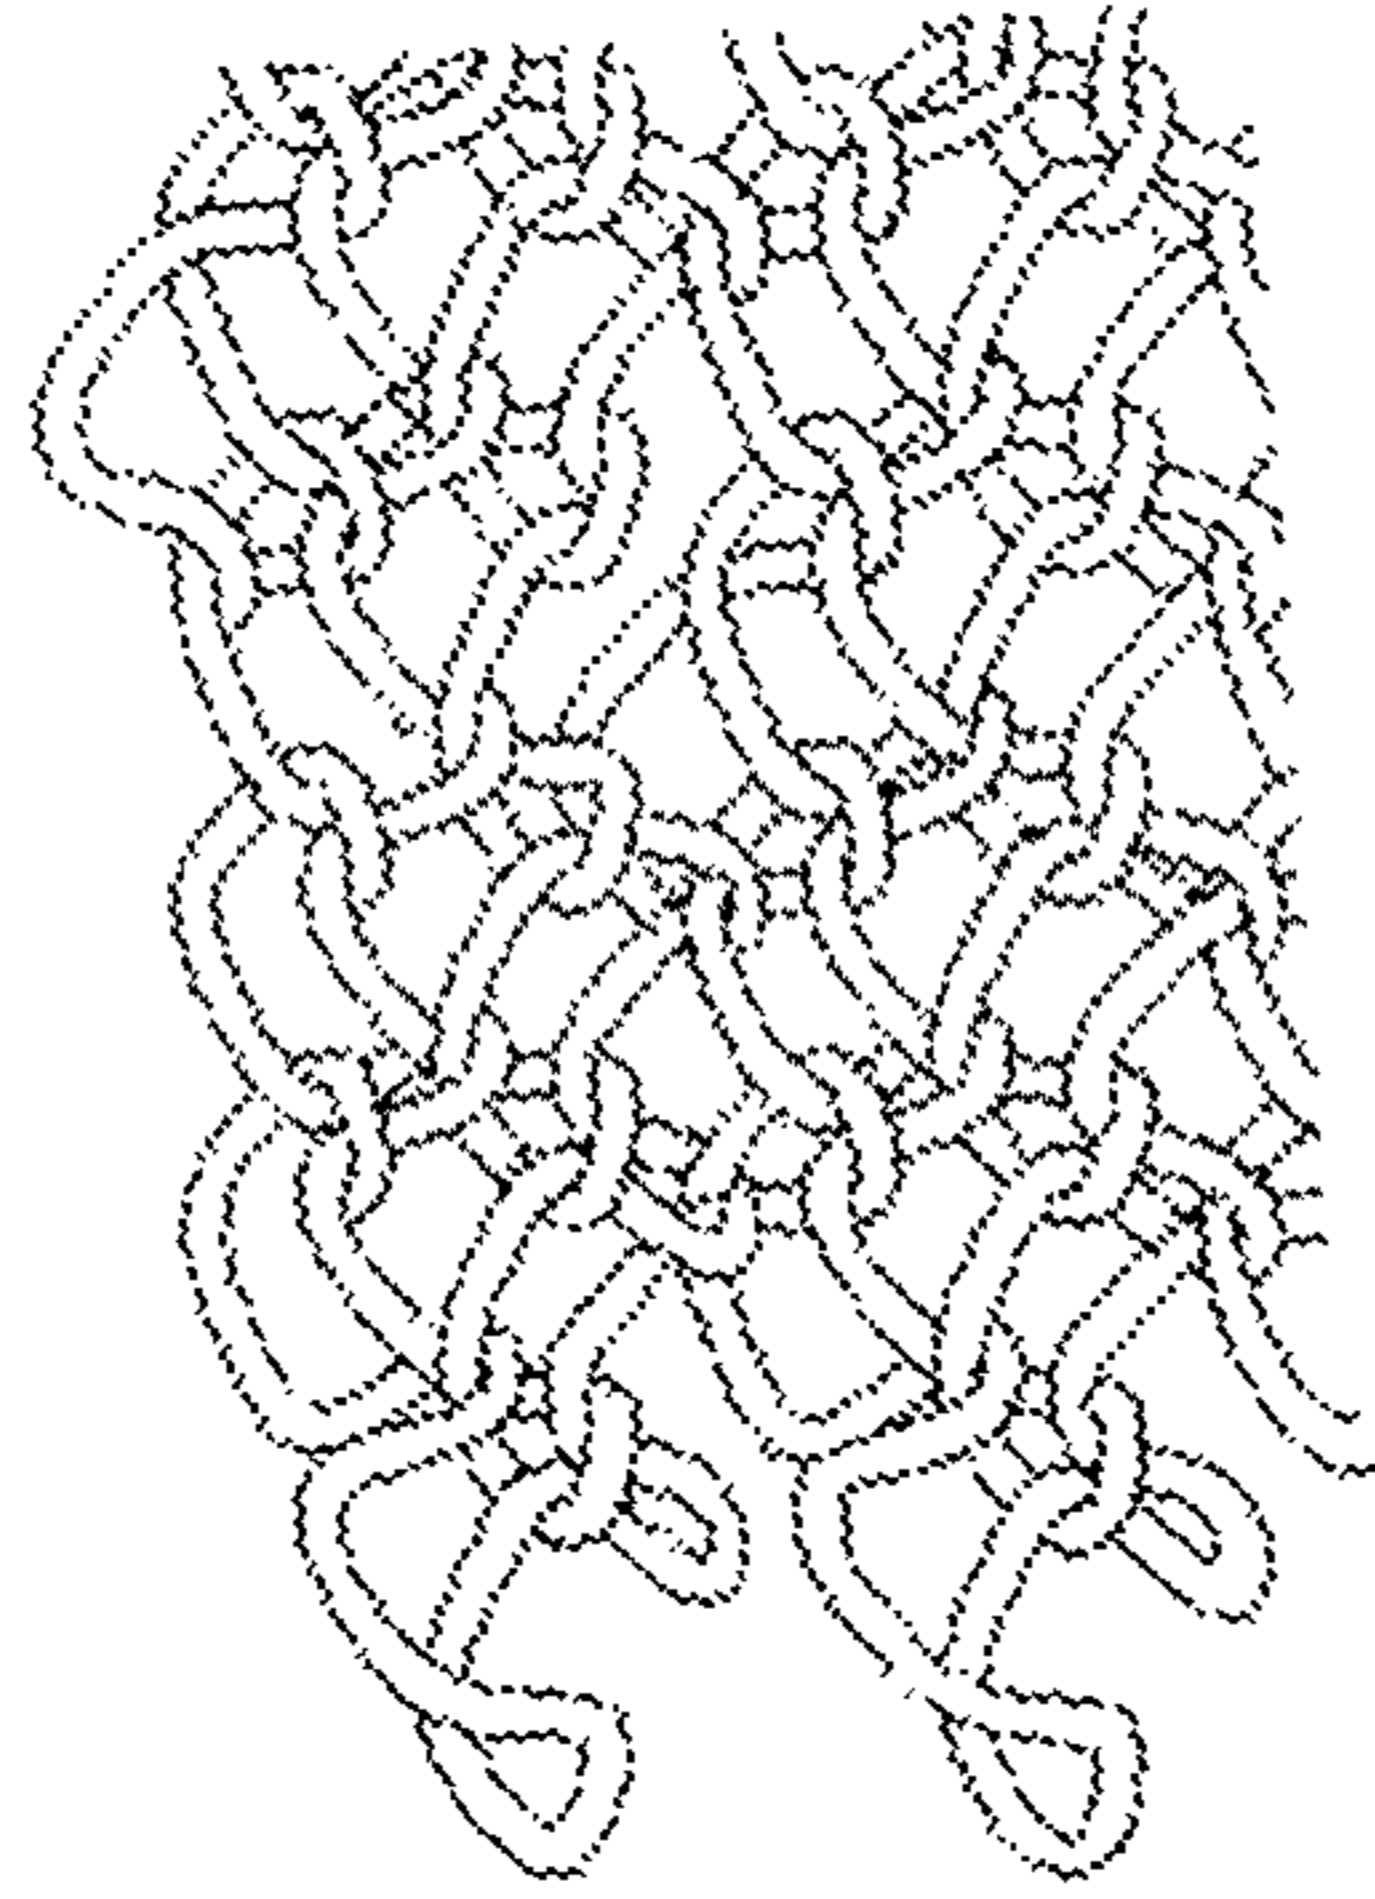


Figure 8