



US00D890999S

(12) **United States Design Patent**
Hull et al.

(10) **Patent No.:** **US D890,999 S**
(45) **Date of Patent:** **** Jul. 21, 2020**

- (54) **GLOVE WITH REDUCED FINGERTIP REGIONS AND A TEAR INDICATOR ROLLED CUFF**
- (71) Applicant: **Summit Glove Inc.**, Minerva, OH (US)
- (72) Inventors: **James L. Hull**, Malvern, OH (US);
Christopher J. Pearen, Brampton (CA); **Ronald J. Thatcher**, Bond Head (CA)
- (73) Assignee: **Summit Glove Inc.**, Minerva, OH (US)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/672,281**
- (22) Filed: **Dec. 4, 2018**

Related U.S. Application Data

- (63) Continuation-in-part of application No. 15/136,191, filed on Apr. 22, 2016, now Pat. No. 10,390,575.
- (51) **LOC (12) Cl.** **02-06**
- (52) **U.S. Cl.**
USPC **D29/117.1; D2/617**
- (58) **Field of Classification Search**
USPC D29/113, 117.1, 117.3
CPC A41D 19/015; A41D 2600/20; A41D 19/01558
See application file for complete search history.

References Cited

U.S. PATENT DOCUMENTS

1,559,114 A	10/1925	Maranville	
2,058,221 A	10/1936	Ferguson	
2,075,550 A *	3/1937	Sterling A41D 19/0062 2/168
2,266,716 A *	12/1941	Robertson A41D 19/0058 2/168
2,335,871 A *	12/1943	Milligan A41D 19/0058 2/168

2,348,773 A *	5/1944	Wyman A61B 42/20 2/21
3,283,338 A	11/1966	Landau	
4,149,601 A *	4/1979	Taylor A41D 19/01594 172/370
4,507,807 A	4/1985	Karkanen	

(Continued)

OTHER PUBLICATIONS

CURAD Germ Shield Nitrile Exam Gloves, posted at amazon.com, posting date Aug. 20, 2018, [online], [site visited Apr. 4, 2020]. Available from Internet, URL: <https://www.amazon.ca/Nitrile-Disposable-Resistant-Cleaning-Improvement/dp/B07GP3MB3D> (Year: 2018).*

(Continued)

Primary Examiner — George D. Kirschbaum
Assistant Examiner — Maria J Edwards
(74) *Attorney, Agent, or Firm* — Sand, Sebolt & Wernow Co., LPA


(57) **CLAIM**

The ornamental design for a glove with reduced fingertip regions and a tear indicator rolled cuff, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of an ambidextrous glove with reduced fingertip regions and a tear indicator rolled cuff in accordance with our design;
FIG. 2 is a rear elevation view thereof;
FIG. 3 is a left side elevation view thereof;
FIG. 4 is a right side elevation view thereof;
FIG. 5 is a top plan view thereof;
FIG. 6 is a bottom plan view thereof; and,
FIG. 7 is a longitudinal cross-section of a middle finger region taken along line 7-7 of FIG. 2.
The broken lines illustrate environment and form no part of the claimed design.

1 Claim, 4 Drawing Sheets

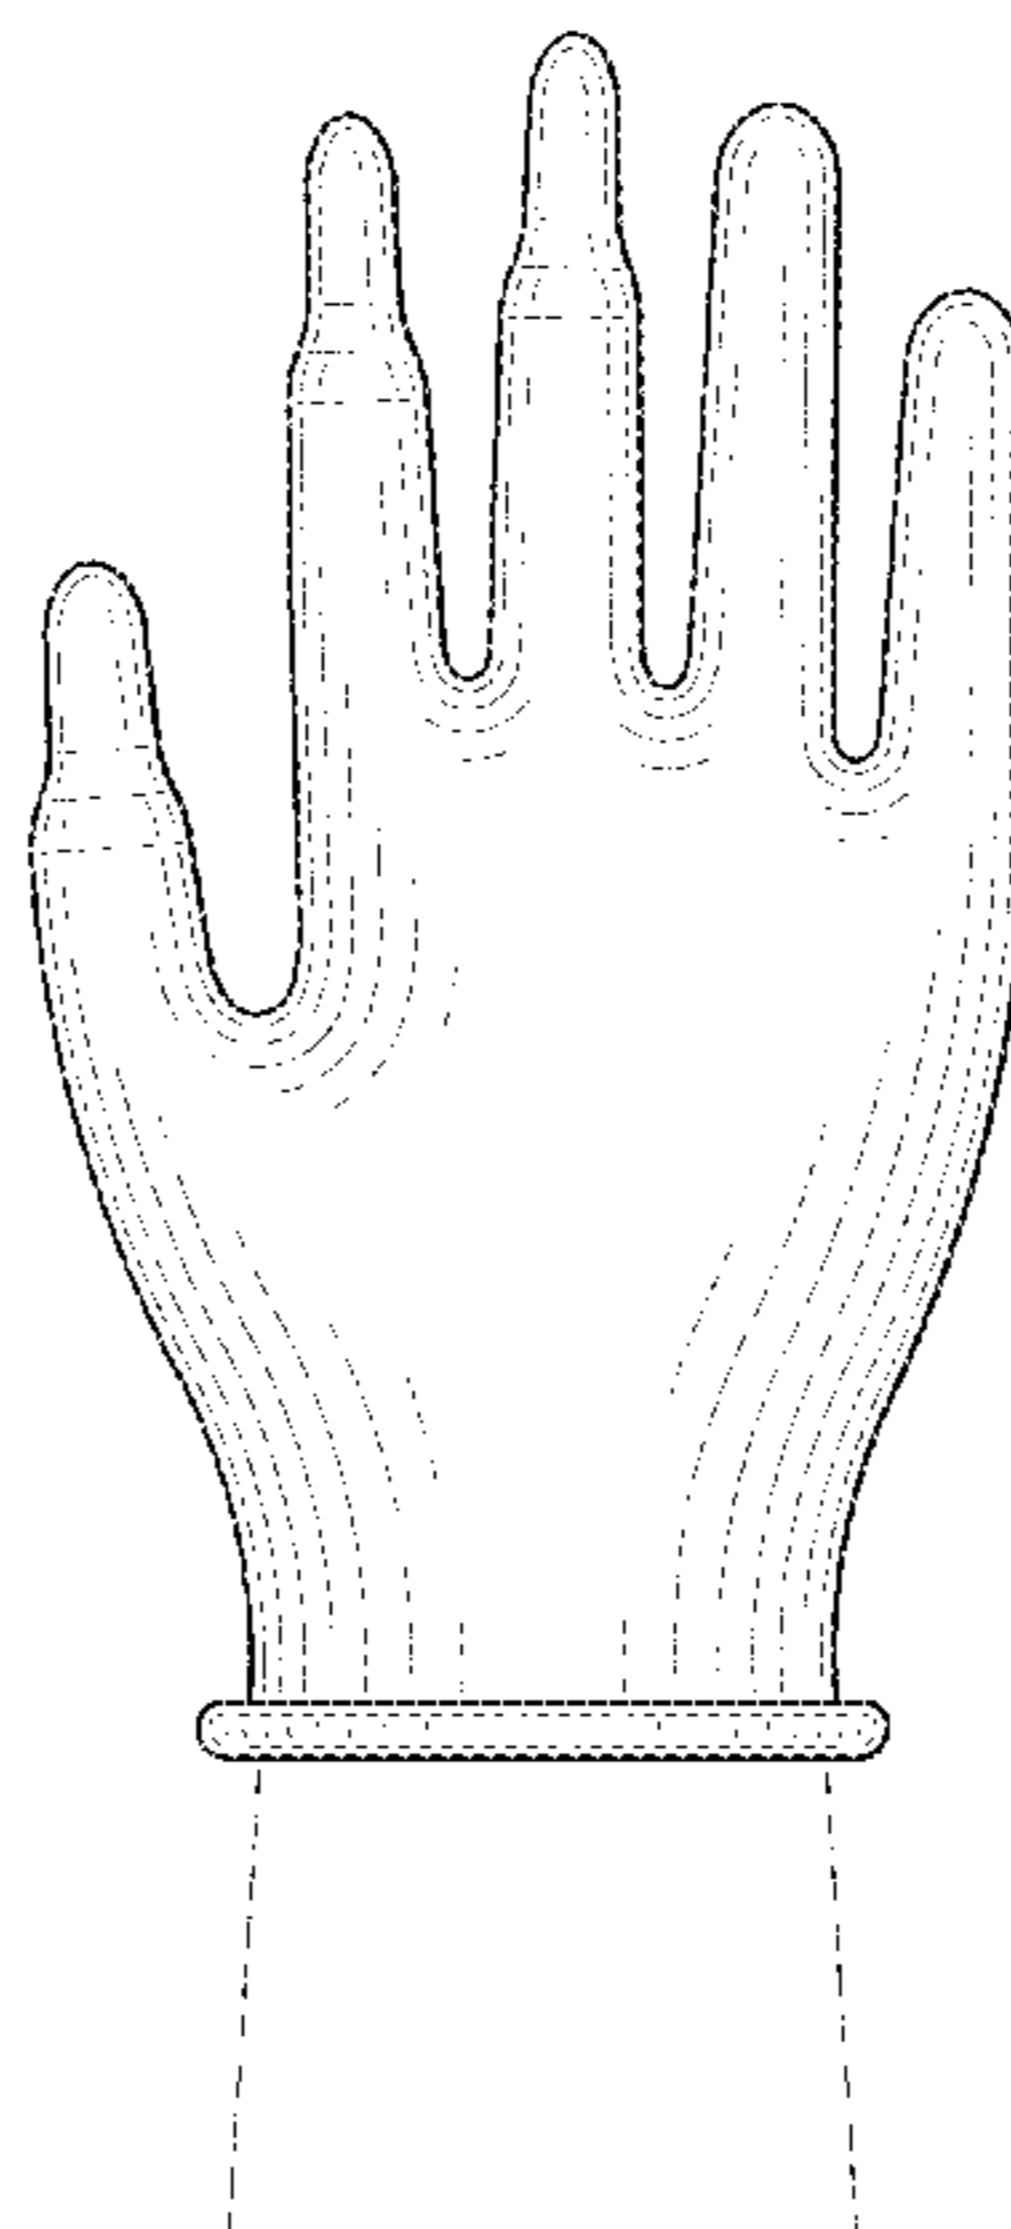

(56)

References Cited

U.S. PATENT DOCUMENTS

5,323,490 A 6/1994 Yarbrough
 5,687,424 A * 11/1997 Masley A41D 19/01547
 2/163
 5,924,137 A 7/1999 Gold
 6,031,042 A 2/2000 Lipinski
 6,032,290 A 3/2000 Lucas et al.
 6,092,238 A 7/2000 Fierabend, Jr.
 6,451,893 B1 9/2002 Tao
 D513,827 S * 1/2006 Ward D2/619
 9,179,718 B2 11/2015 Anstey
 10,238,159 B2 3/2019 Hull
 10,390,575 B2 8/2019 Hull
 10,602,787 B2 * 3/2020 Hull B32B 25/14
 10,602,788 B2 * 3/2020 Hull B32B 25/14
 2012/0036612 A1 2/2012 Hull
 2013/0239291 A1 9/2013 Harris
 2013/0291282 A1 11/2013 Anstey
 2015/0164160 A1 6/2015 Furlong
 2017/0231705 A1 8/2017 Madison
 2017/0295868 A1 10/2017 Yahnite
 2017/0318879 A1 11/2017 Gleser
 2019/0104783 A1 * 4/2019 Hull A41D 19/0055

OTHER PUBLICATIONS

Milker's Helpers Gloves, posted at rjmatthews.com, posting date not given, [online], [site visited Apr. 4, 2020]. Available from Internet, URL: <https://www.rjmatthews.com/details/Milkers-Helpers-Gloves/19-71820.html> (Year: 2020).*

Nick Gardner, Accelerator Free Fact or Fiction, Shield Scientific B.V., Health & Safety International, pp. 77-82, Oct. 2008.

SemperSure™ Nitrile, www.sempermedusa.com/products/semperasure, Sempermed USA, Inc., 2 pages, document is undated but was publically available as of Aug. 18, 2014.

Nitrite Accelerator-Free Micro-Touch®, www.ansell.be/medical/pdf/gloves/EN/Micro-Touch%20Nitrile%20Accelerator-Free.pdf, Ansell, 2 pages, document is undated but was publically available as of Aug. 18, 2014.

Accelerator-Free Nitrile Exam Gloves—a Better Alternative, <http://hourglass-intl.com/2011/04/18/accelerator-free-nitrile-exam-gloves-a-better-alternative/>, Hourglass International, 4 pages, Apr. 18, 2011.

New Glove Materials Make Nitrile Gloves Better, <http://hourglass-intl.com/2011/01/24/new-glove-materials-make-nitrile-gloves-better/>, Hourglass International, 2 pages, Jan. 24, 2011.

* cited by examiner

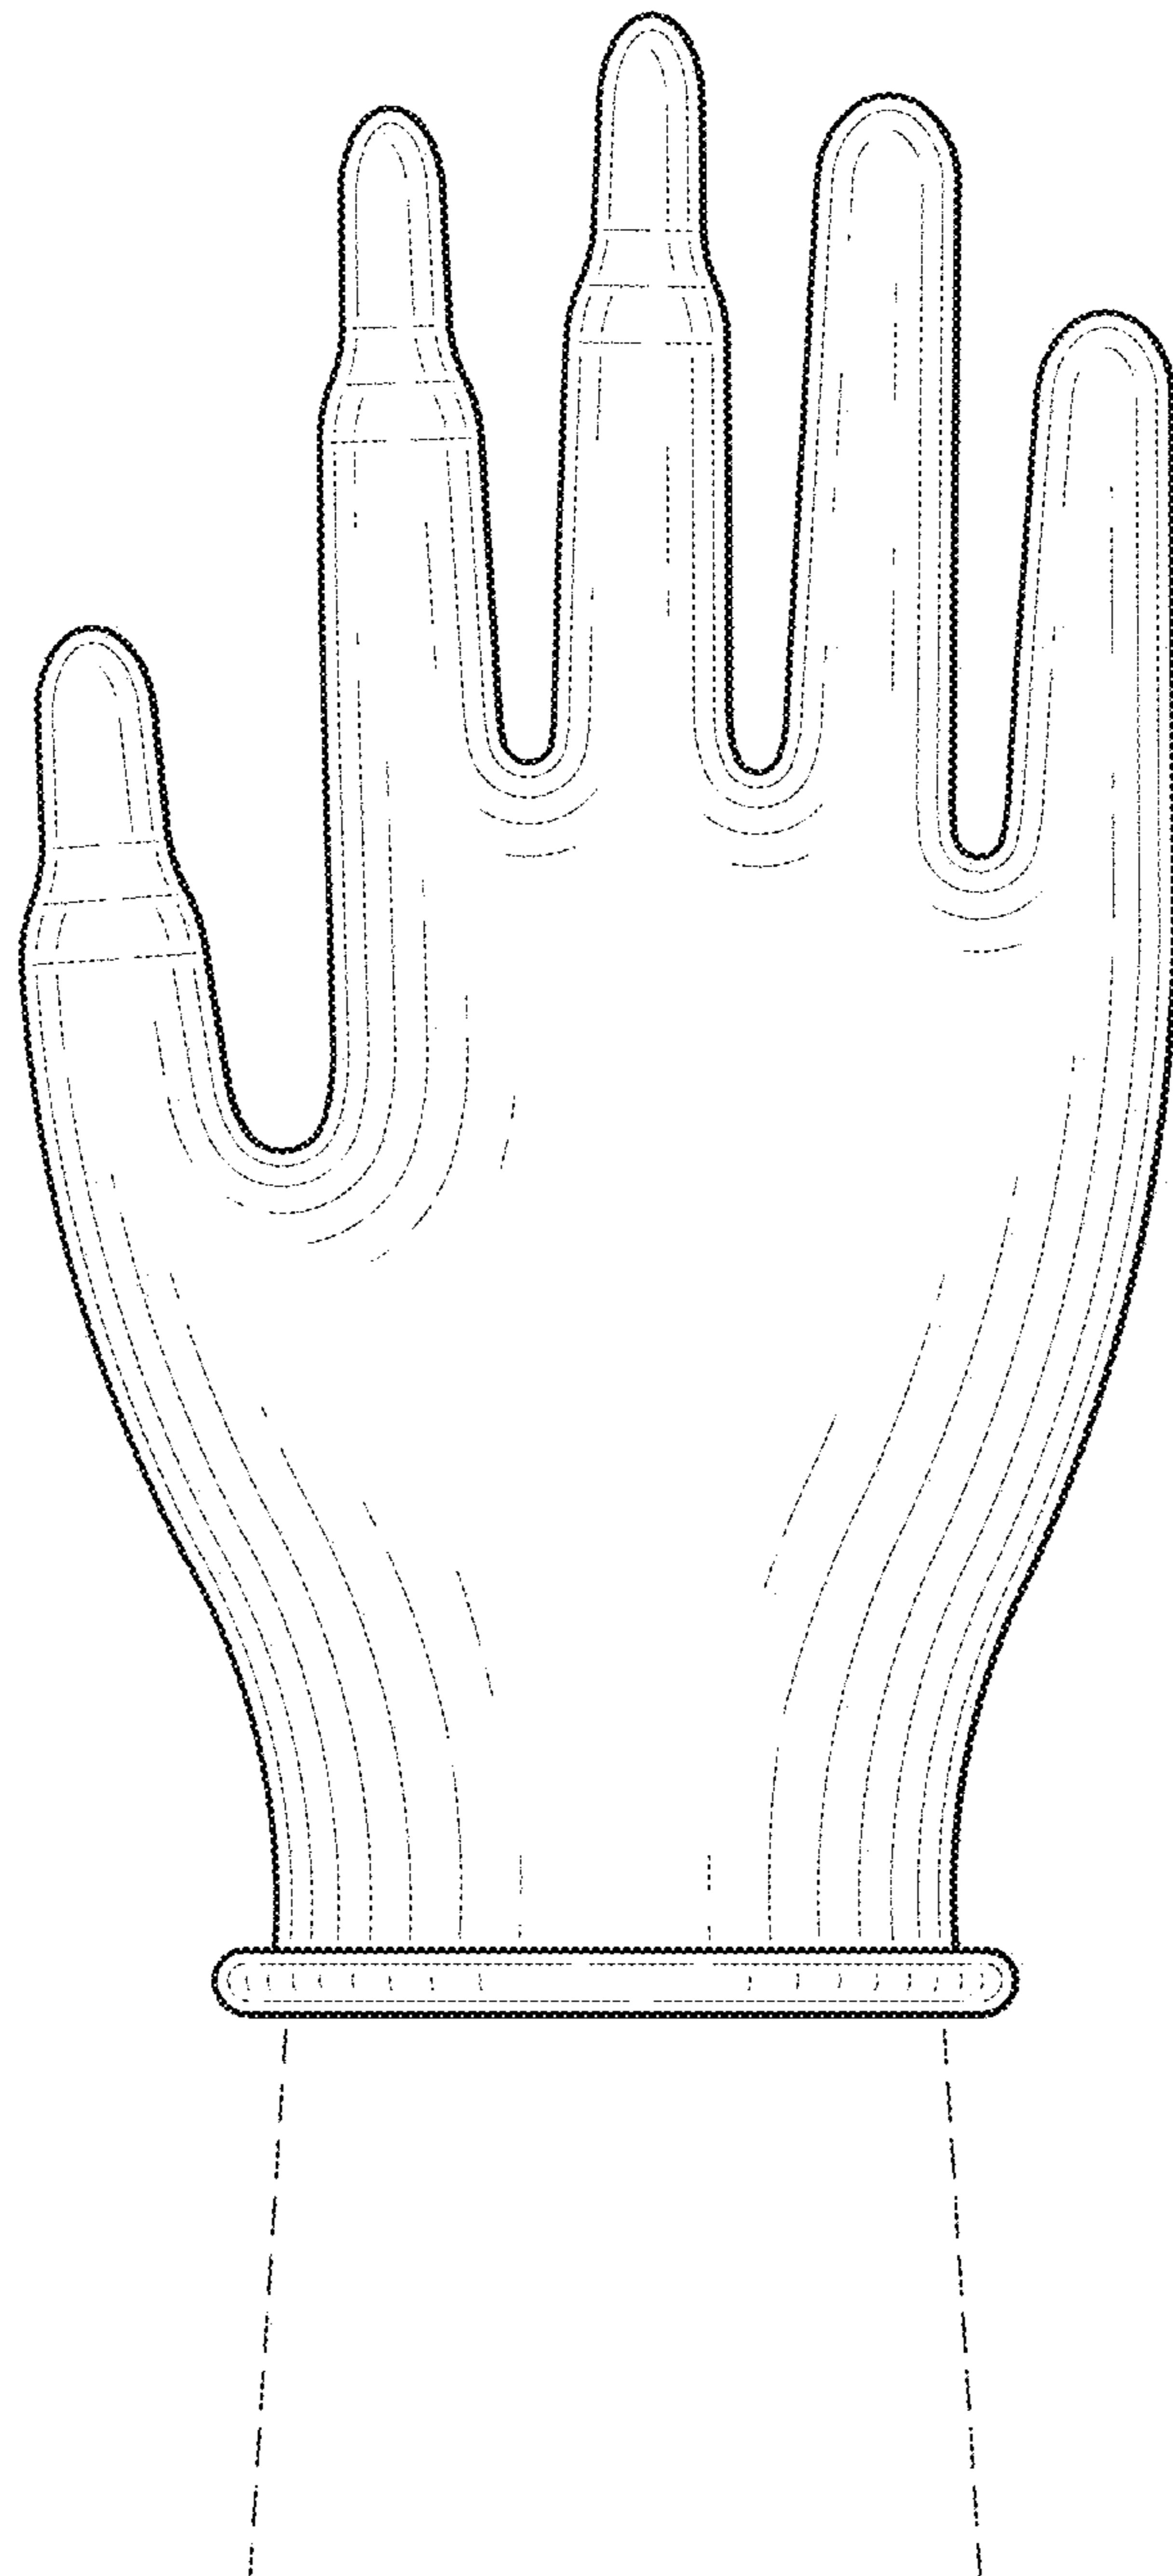


FIG. 1

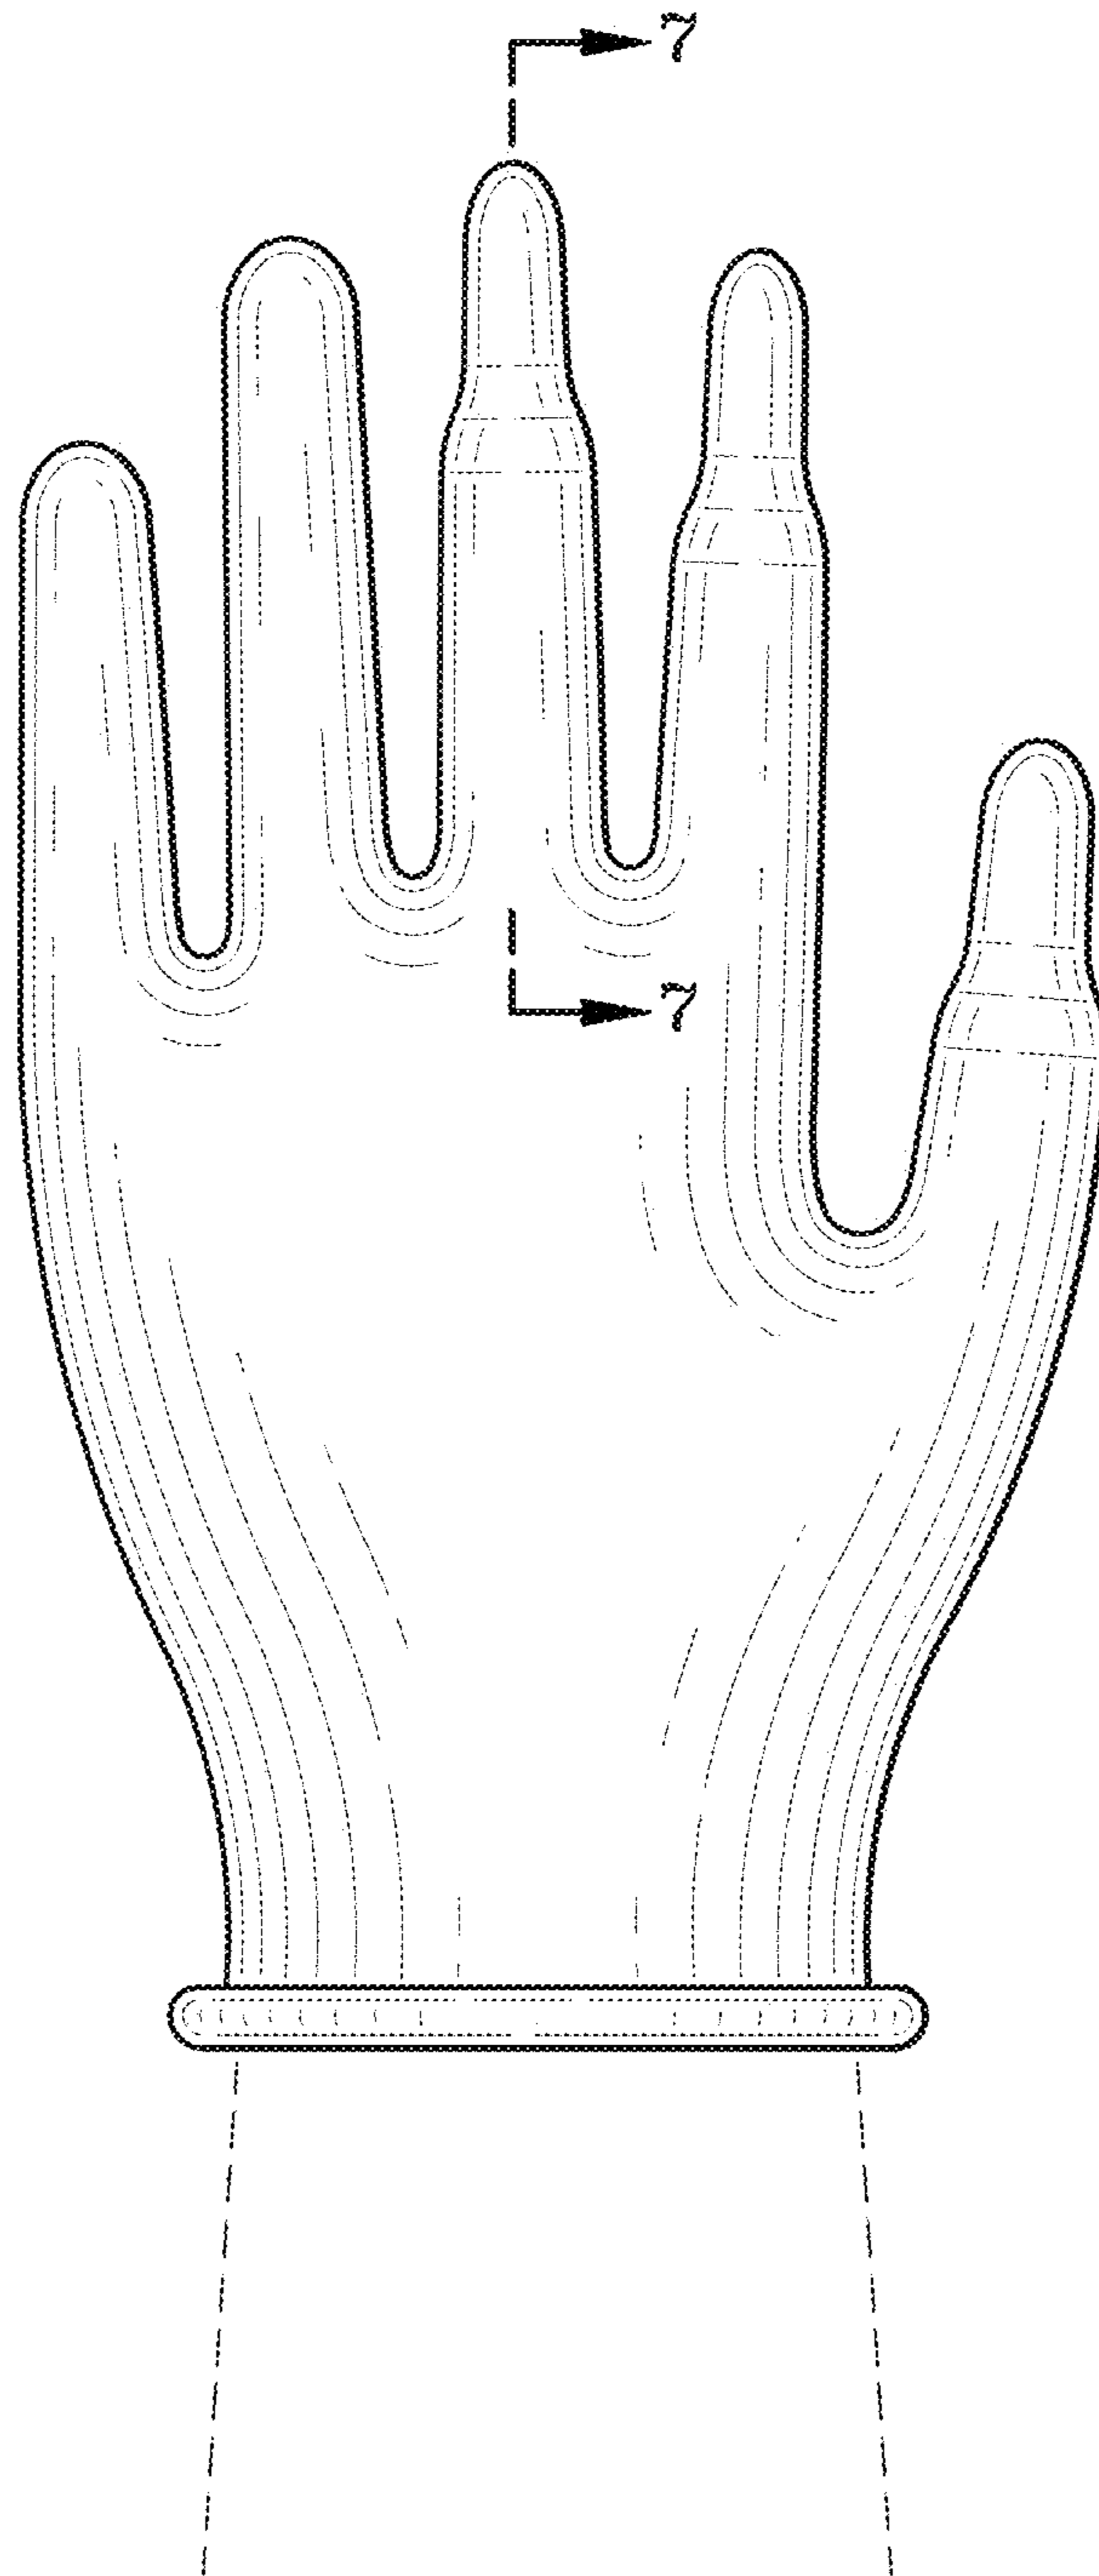


FIG.2

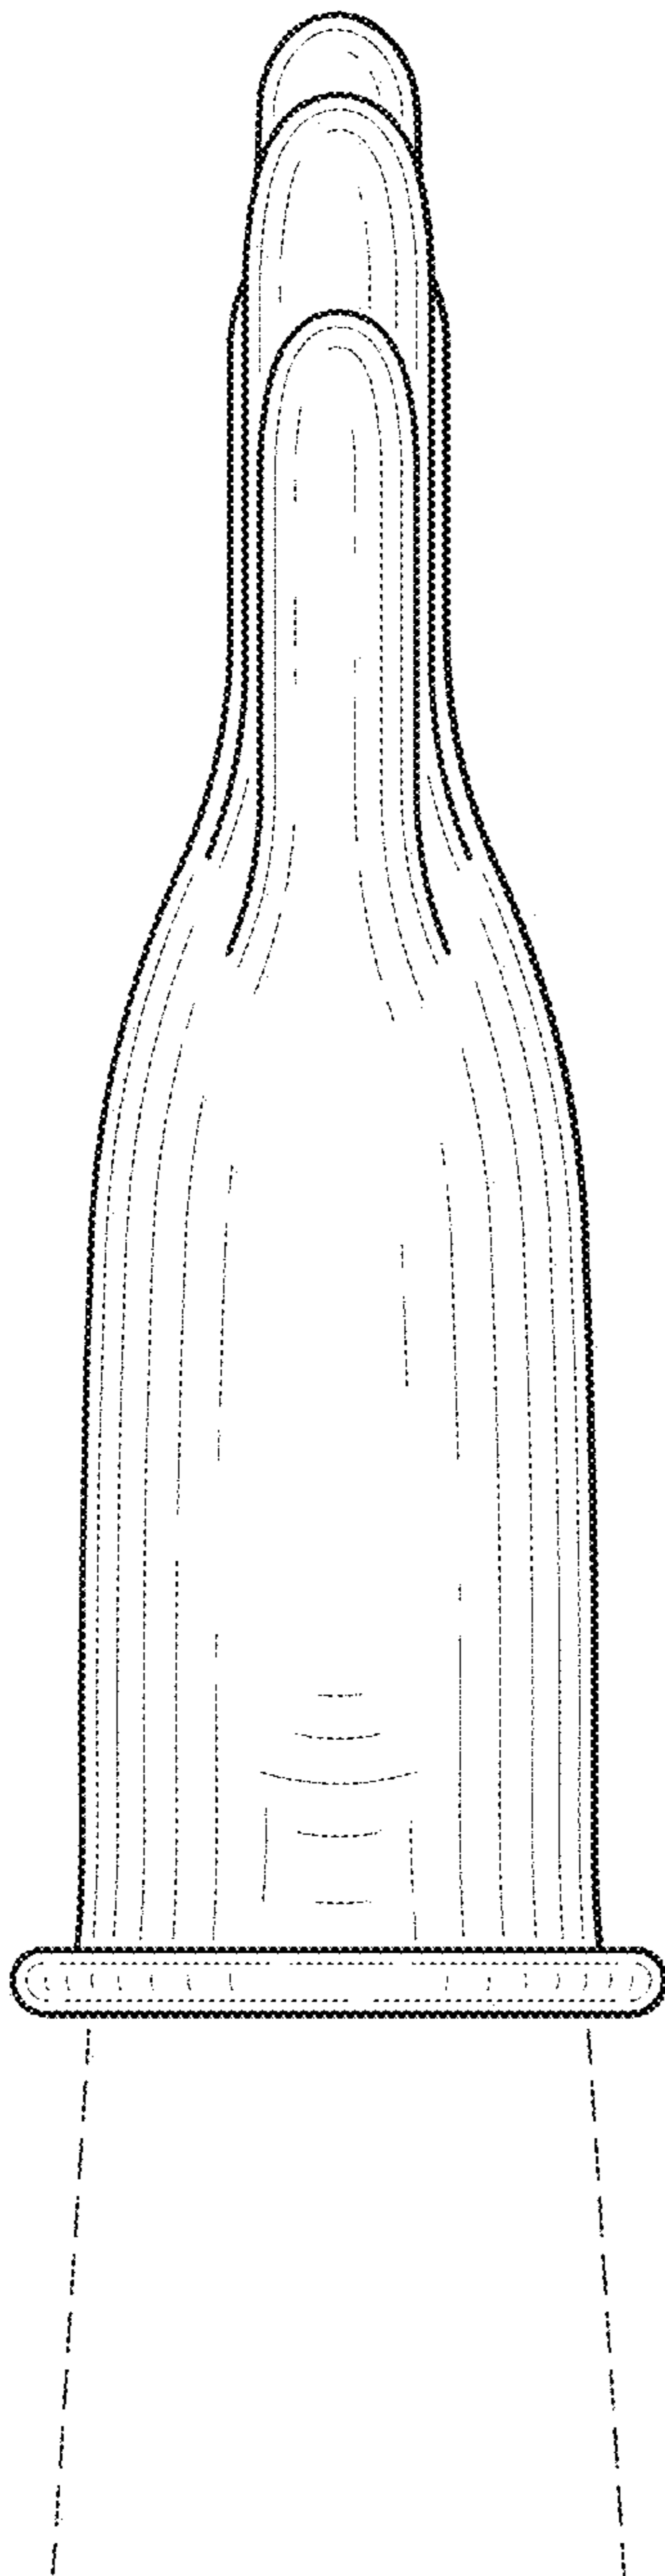


FIG. 3

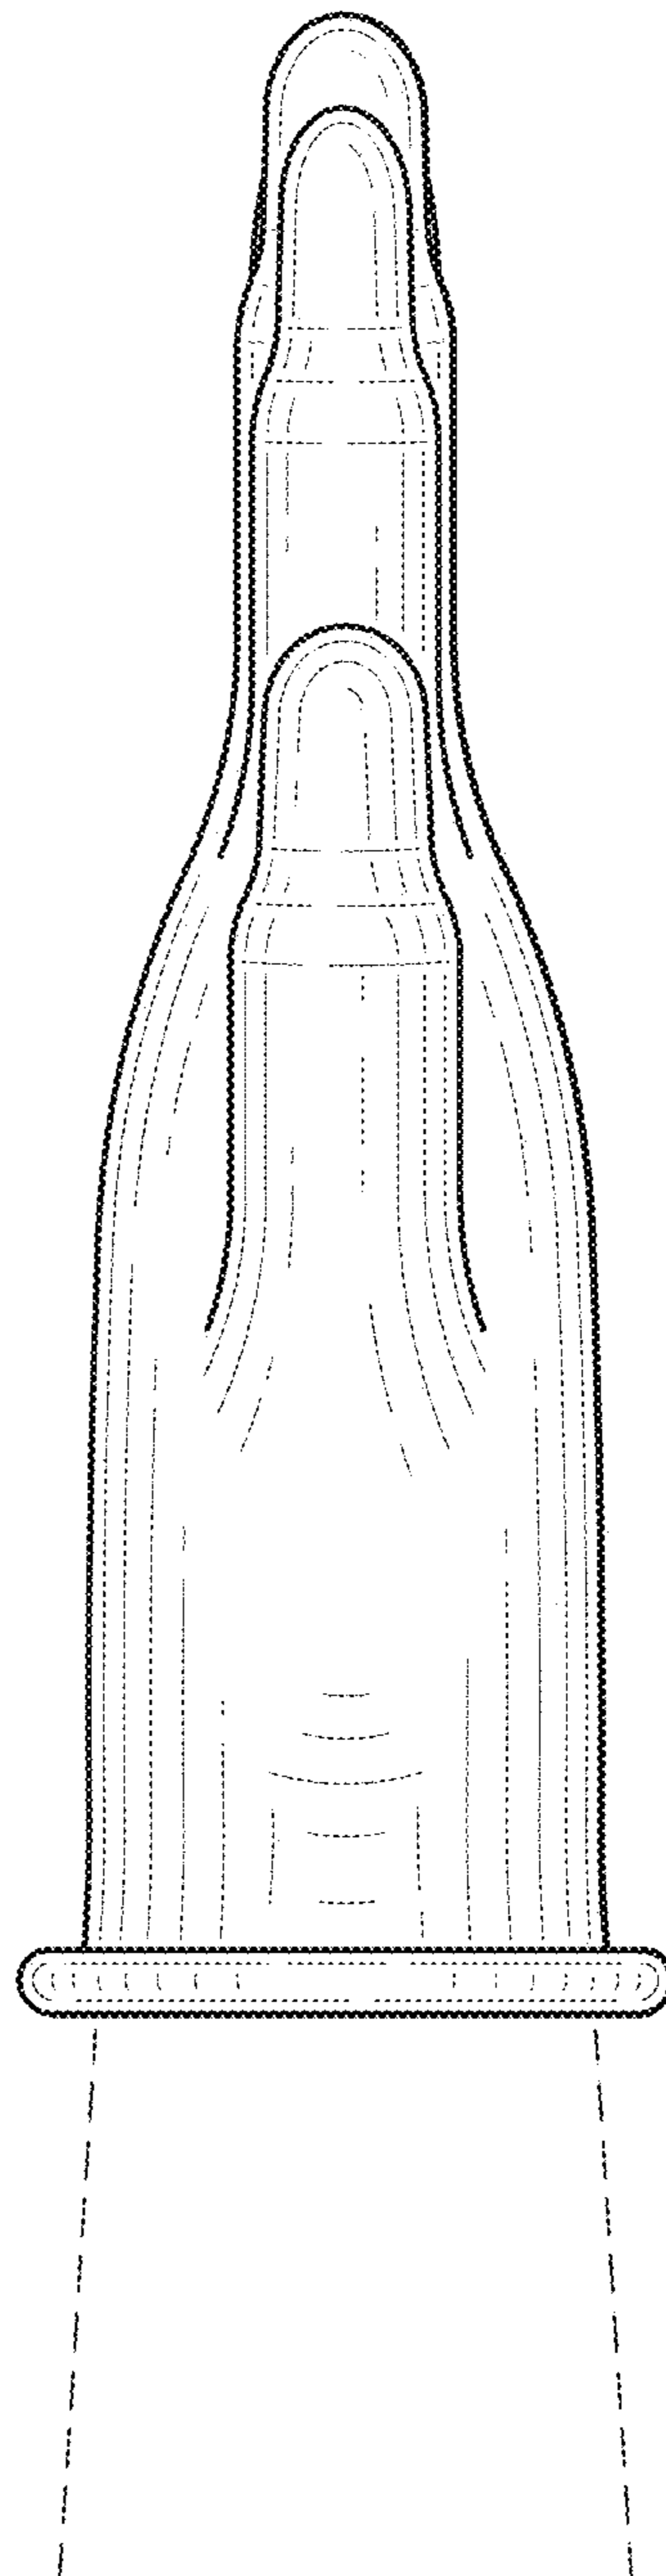


FIG. 4

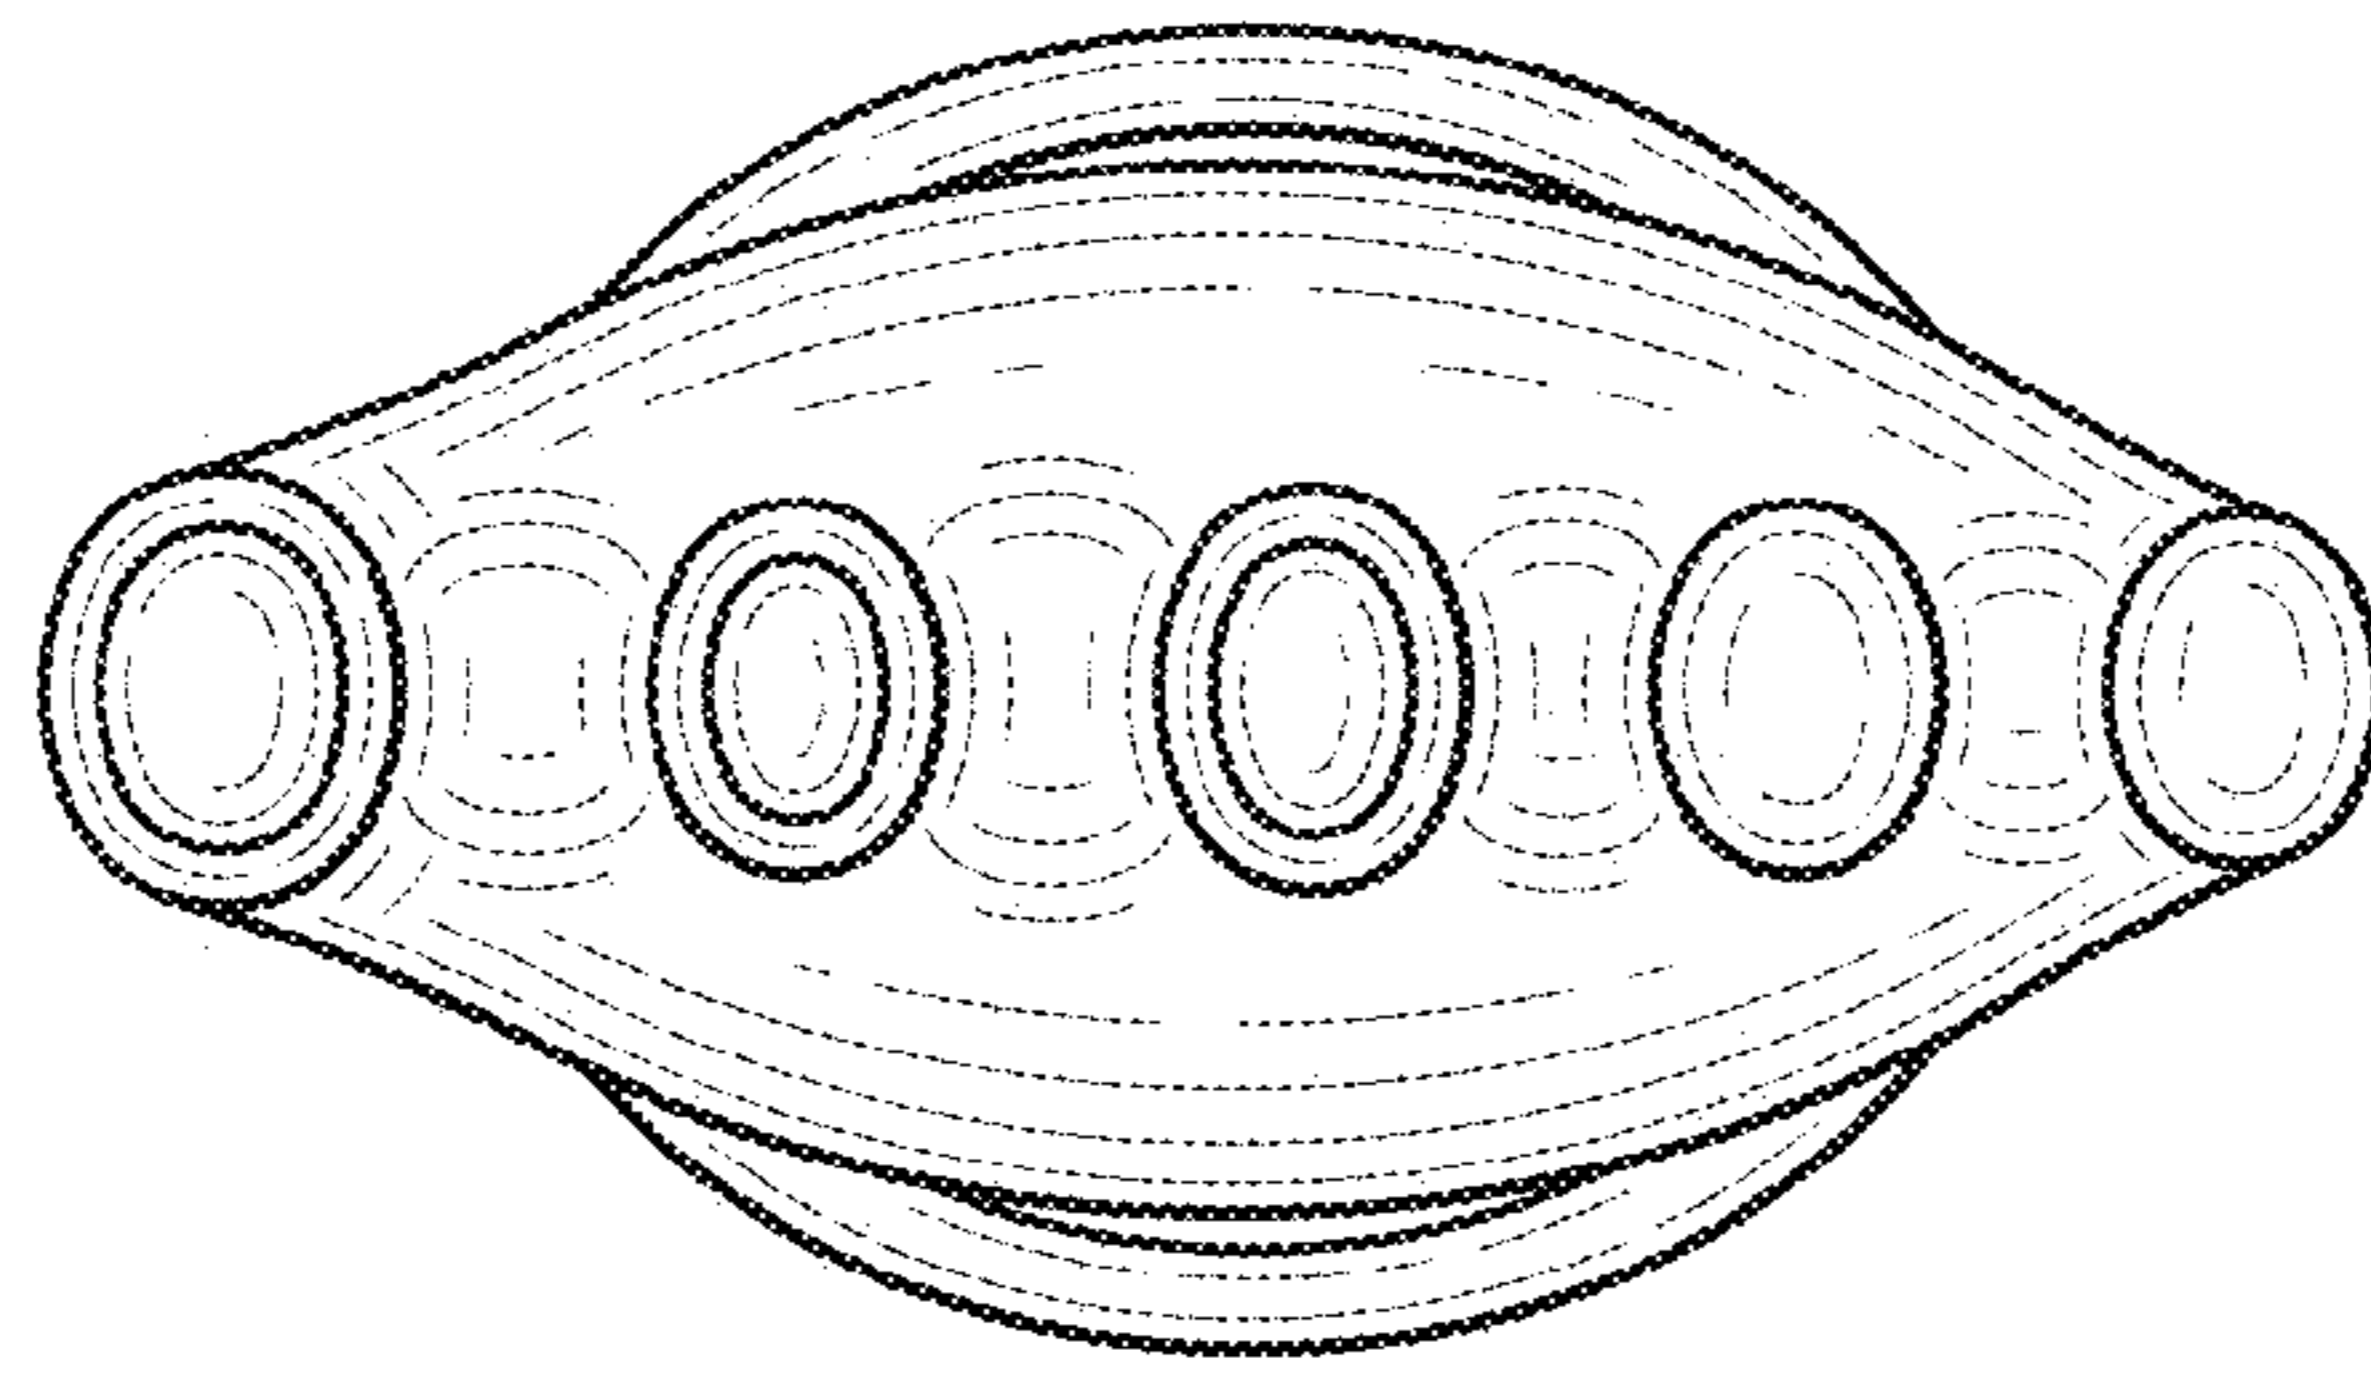


FIG. 5

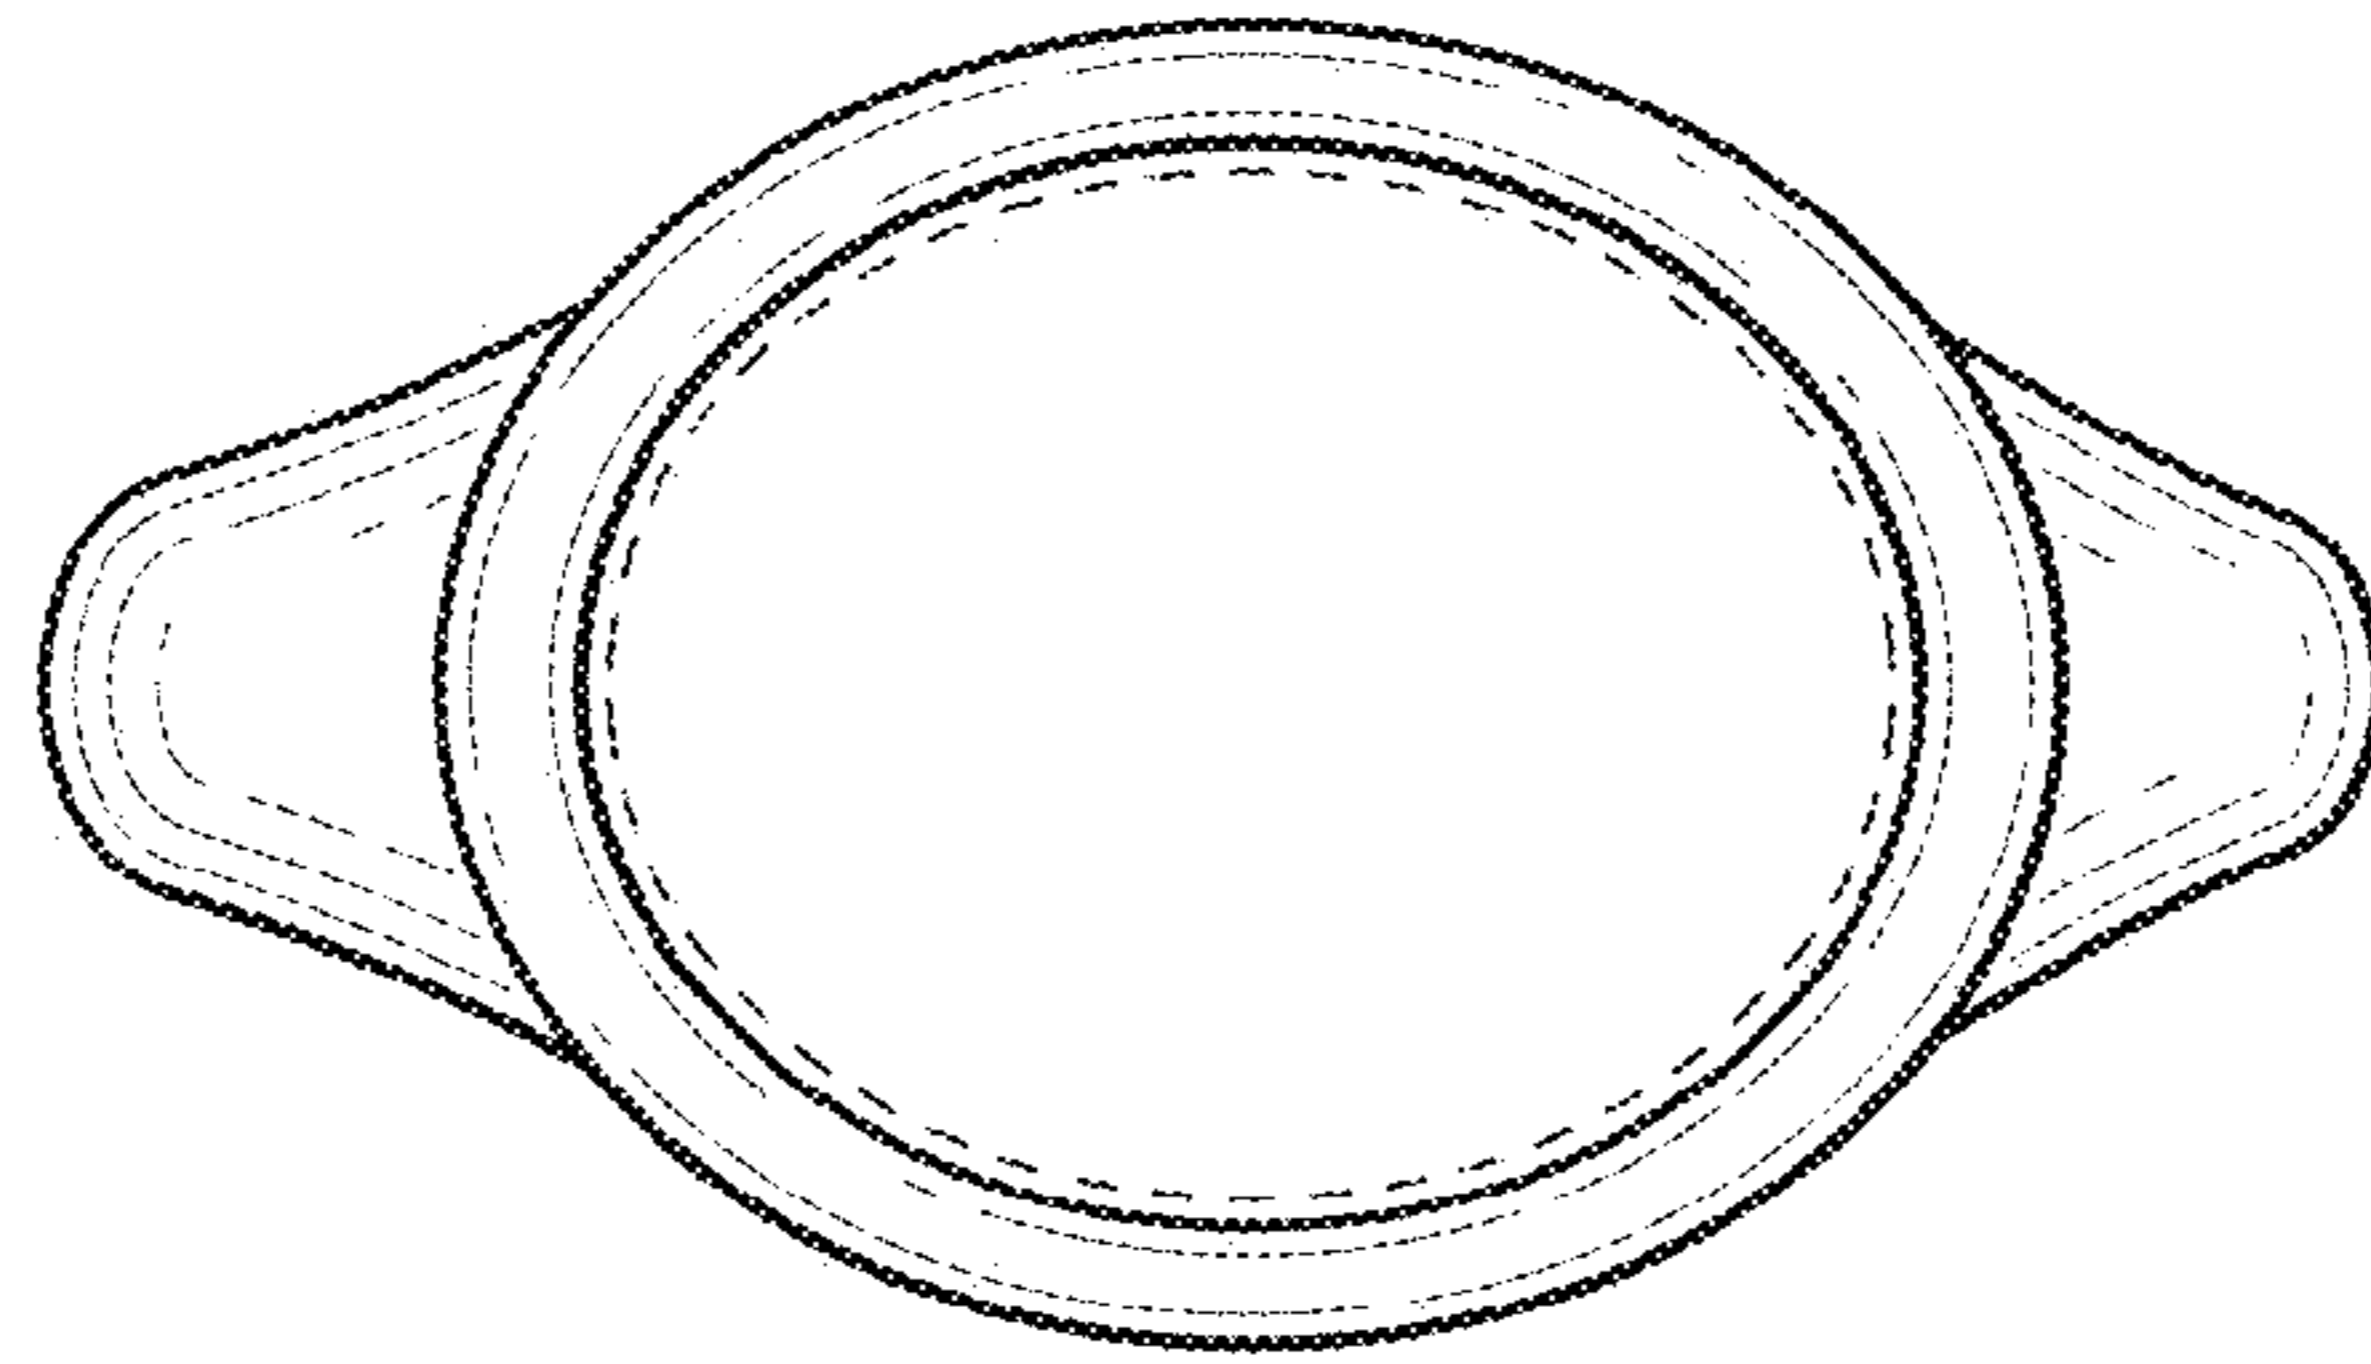


FIG. 6

FIG. 7

