

US00D891637S

(12) **United States Design Patent**  
**Newberg et al.**

(10) **Patent No.:** **US D891,637 S**  
(45) **Date of Patent:** **\*\* Jul. 28, 2020**

(54) **DIGITAL PATHOLOGY SLIDE RACK CAROUSEL**

(71) Applicant: **Leica Biosystems Imaging, Inc.**, Vista, CA (US)

(72) Inventors: **Nicholas Newberg**, San Marcos, CA (US); **Prentash Djelosevic**, Oceanside, CA (US); **Peyman Najmabadi**, San Diego, CA (US)

(73) Assignee: **LEICA BIOSYSTEMS IMAGING, INC.**, Vista, CA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/631,499**

(22) Filed: **Dec. 29, 2017**

(51) **LOC (12) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/227**

(58) **Field of Classification Search**  
USPC ..... D24/107, 122, 125, 127, 128, 133, 161, D24/224, 225, 227, 230, 232; D16/235, D16/236  
CPC ..... H05K 7/20718  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D206,032 S *	10/1966	Baring	.....	D16/236
D214,001 S *	4/1969	Steinbach	.....	D16/236
D217,642 S *	5/1970	Blecher	.....	D16/236
D244,023 S *	4/1977	Wilsch	.....	D16/236
D287,633 S *	1/1987	Hollar	.....	D24/230

D287,634 S *	1/1987	Carr	.....	D24/230
D289,199 S *	4/1987	Tag	.....	D24/230
D320,046 S *	9/1991	Clinehens	.....	D19/75
D321,057 S *	10/1991	Holen	.....	D24/224
D343,184 S *	1/1994	Kahn	.....	D16/236
D455,577 S *	4/2002	Wilson, Jr.	.....	D6/677.1
7,222,739 B2 *	5/2007	DeNatale, Jr.	.....	A47B 49/00 211/40
D584,358 S *	1/2009	Schag	.....	D19/90
D825,077 S *	8/2018	Bohm	.....	D24/227

\* cited by examiner

*Primary Examiner* — Susan Bennett Hattan

*Assistant Examiner* — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Procopio; Patric J. Rawlins; Jonathan D. Cheng

(57) **CLAIM**


The ornamental design for a digital pathology slide rack carousel, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a digital pathology slide rack carousel according to the present invention; FIG. 2 is a back perspective view thereof; FIG. 3 is a front side view thereof; FIG. 4 is a back side view thereof; FIG. 5 is a left side view thereof; FIG. 6 is a right side view thereof; FIG. 7 is a top side view thereof; and, FIG. 8 is a bottom side view thereof.

The broken lines are included for the purpose of illustrating portions of the digital pathology slide rack carousel and form no part of the claimed design. The digital pathology slide rack carousel is intended for use with a digital pathology apparatus.

**1 Claim, 8 Drawing Sheets**

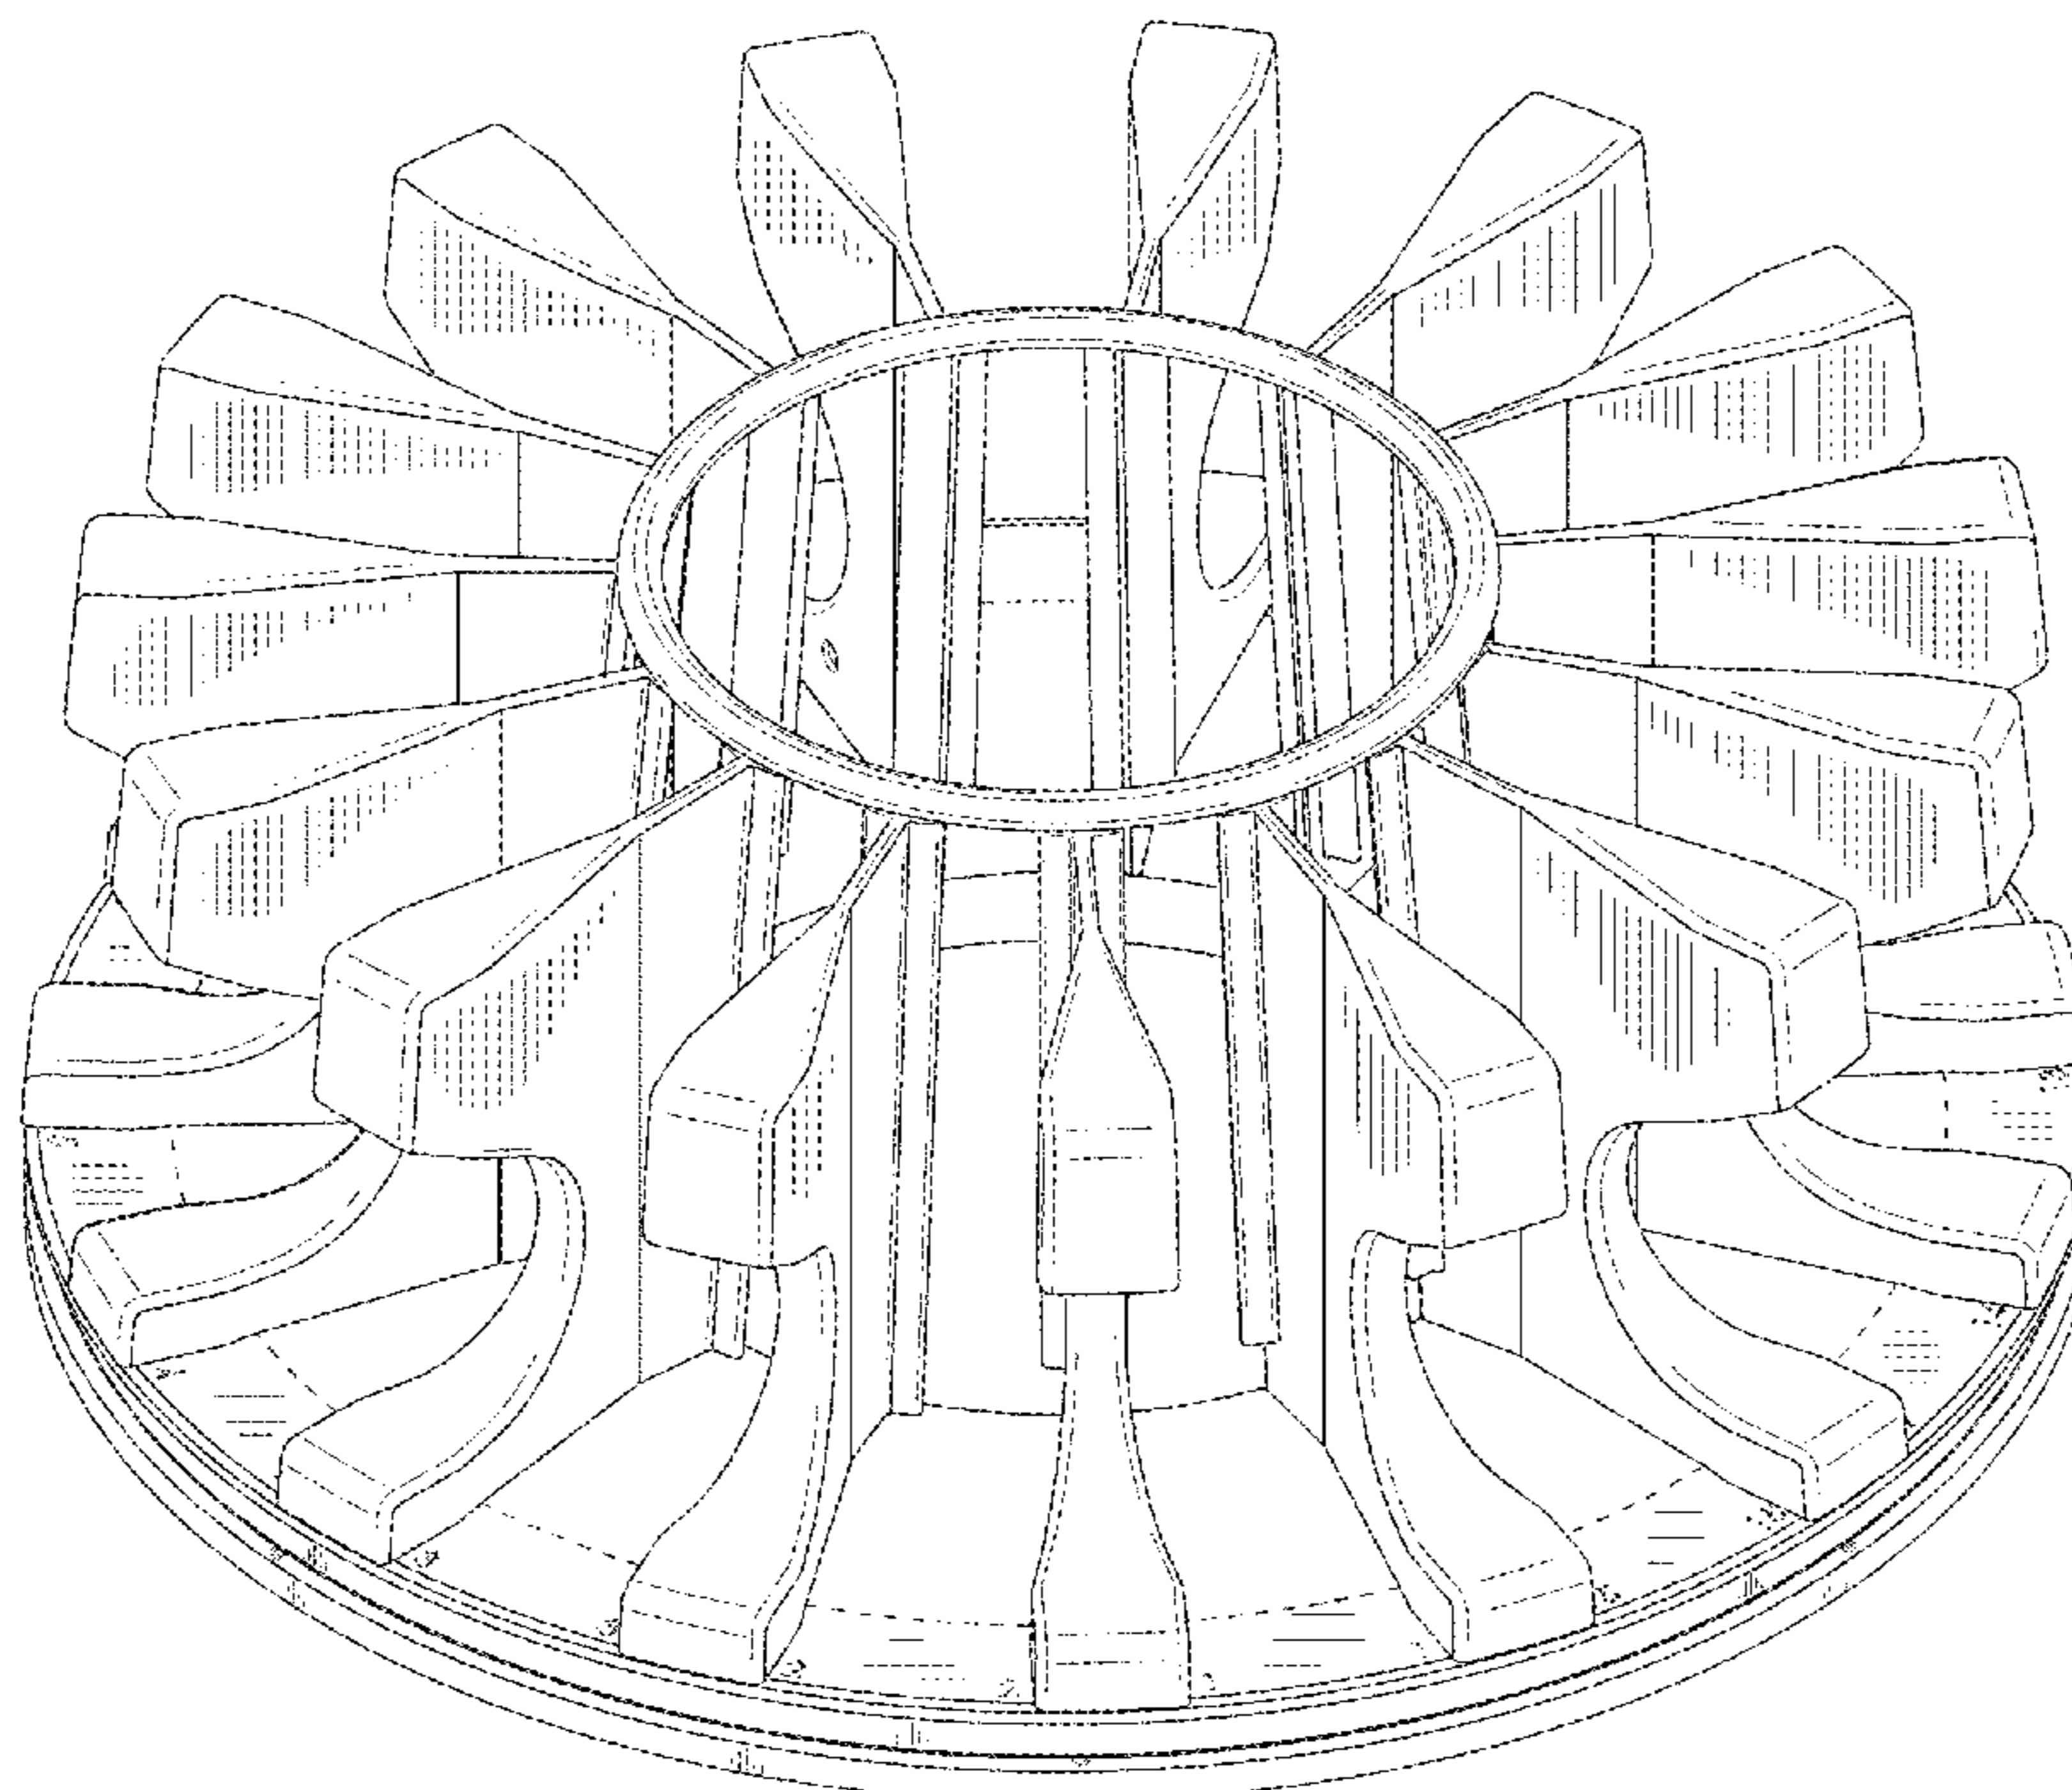

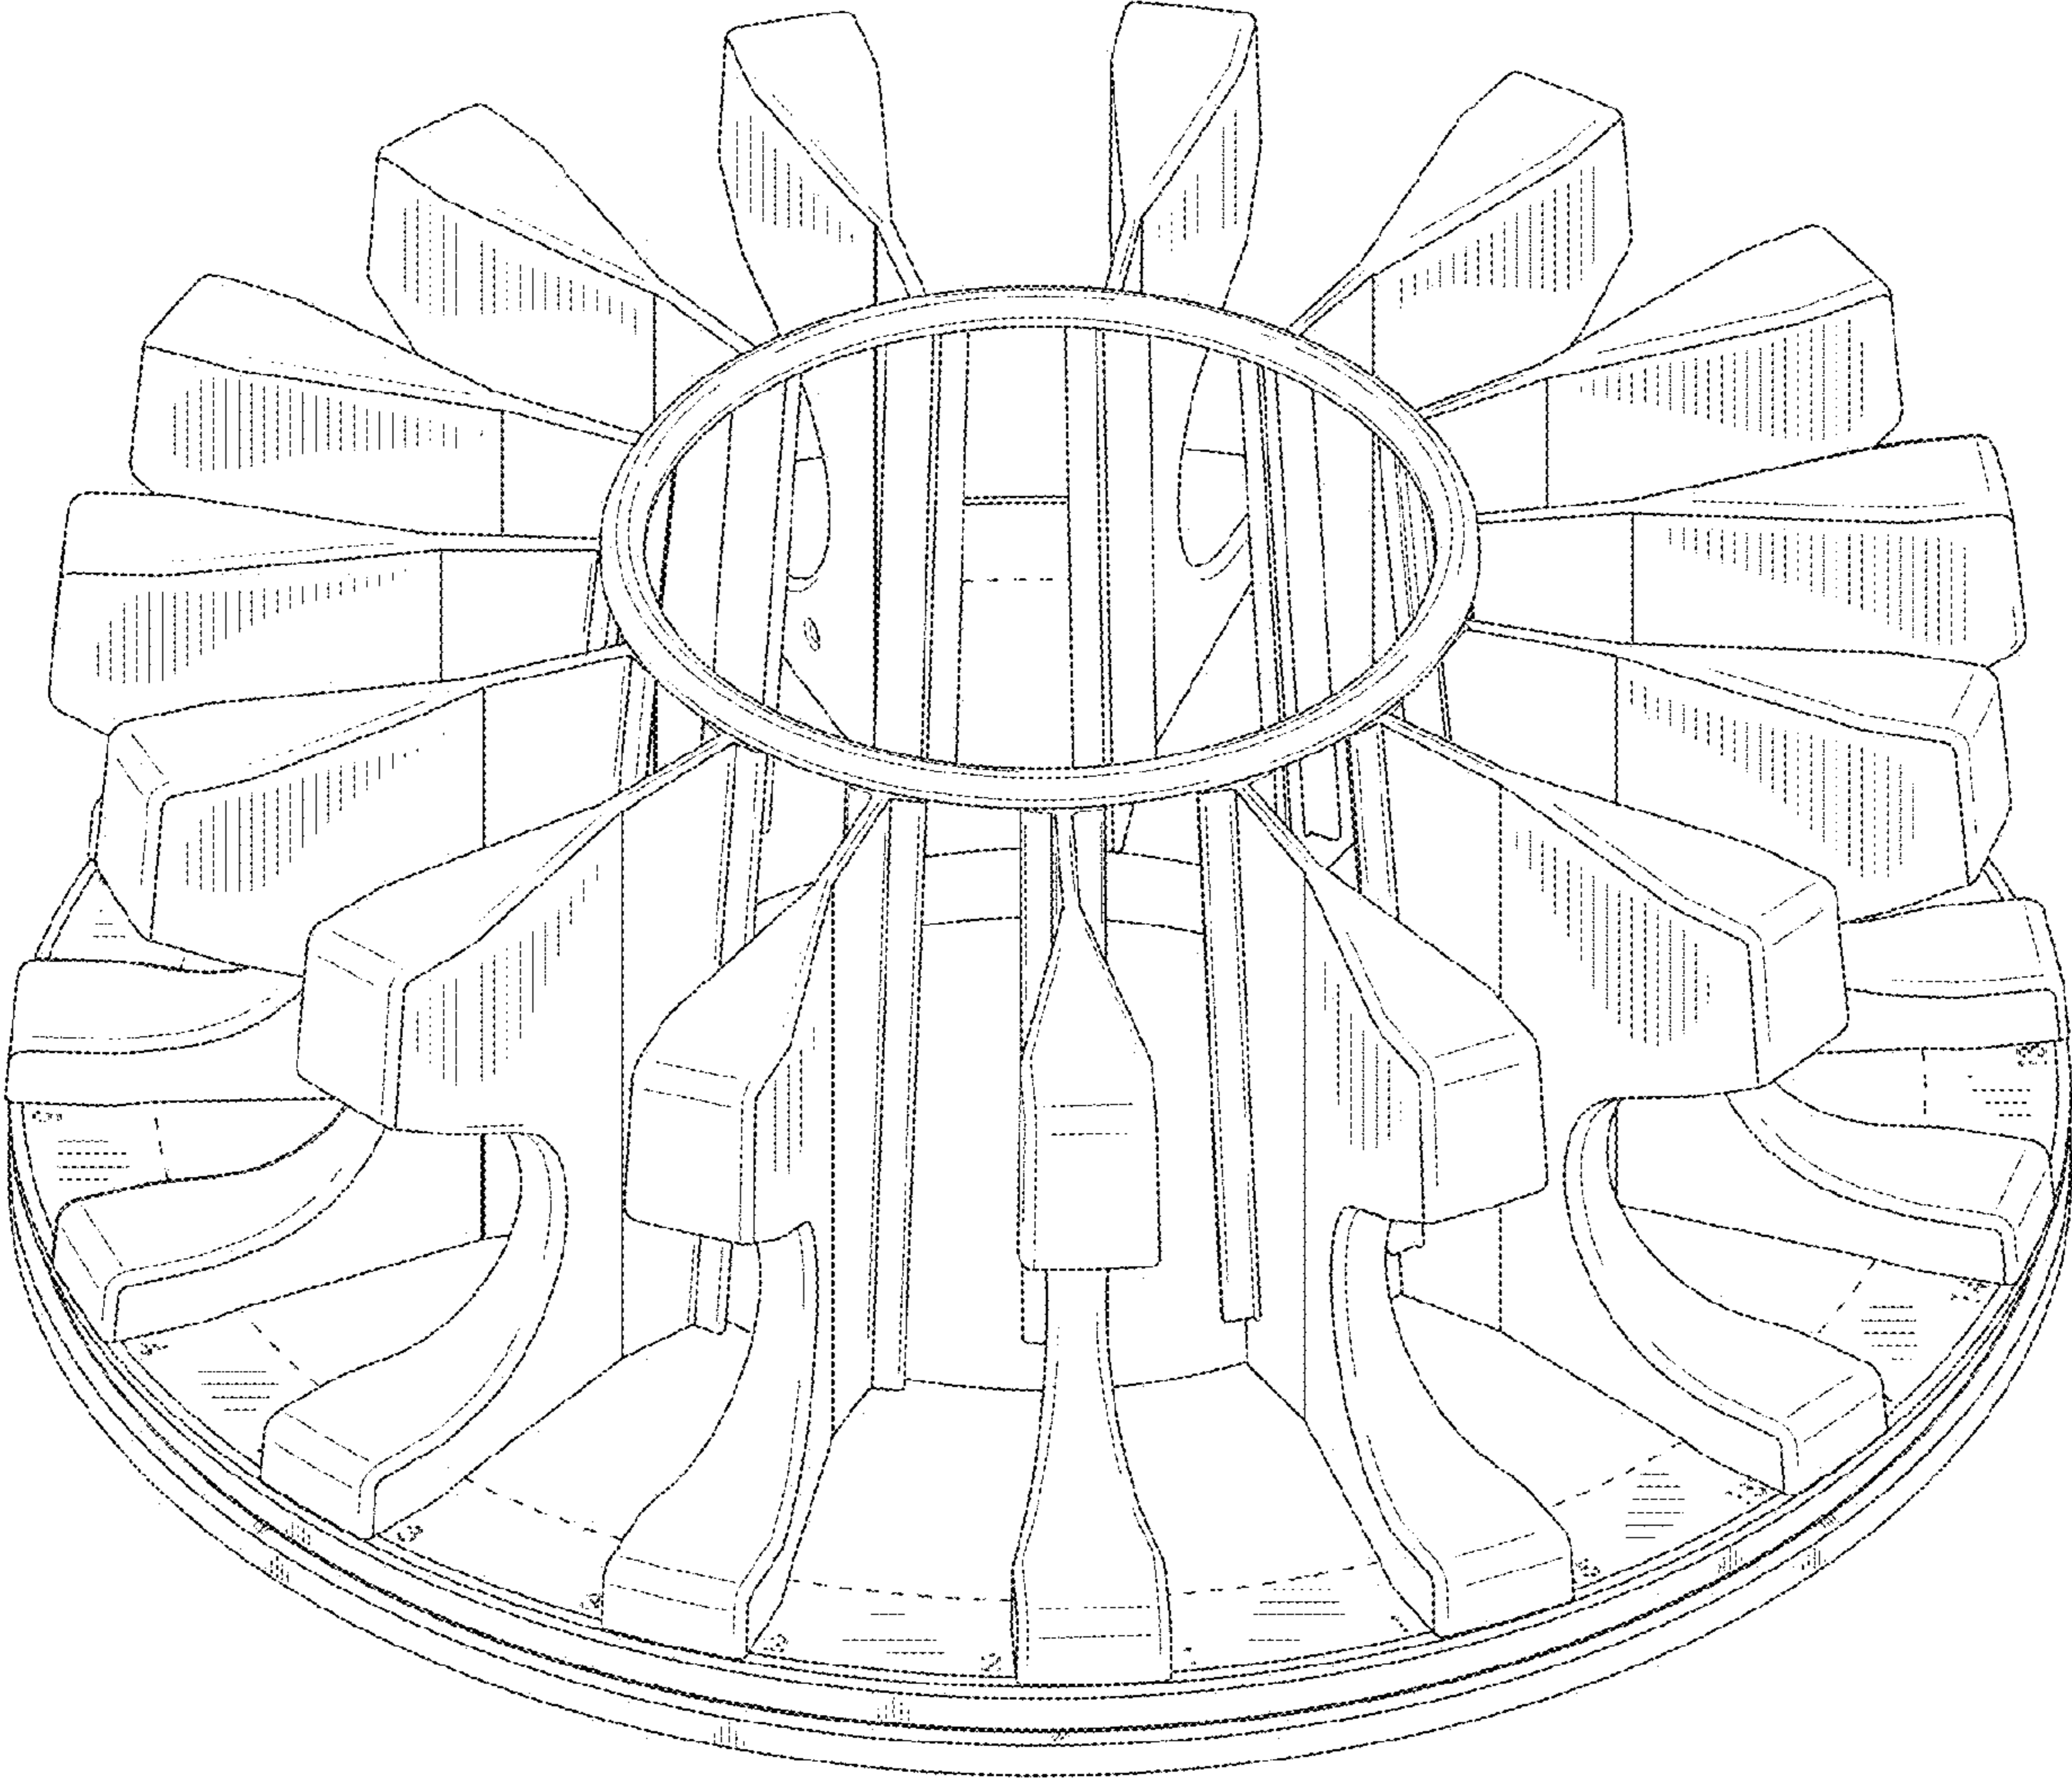


FIG. 1

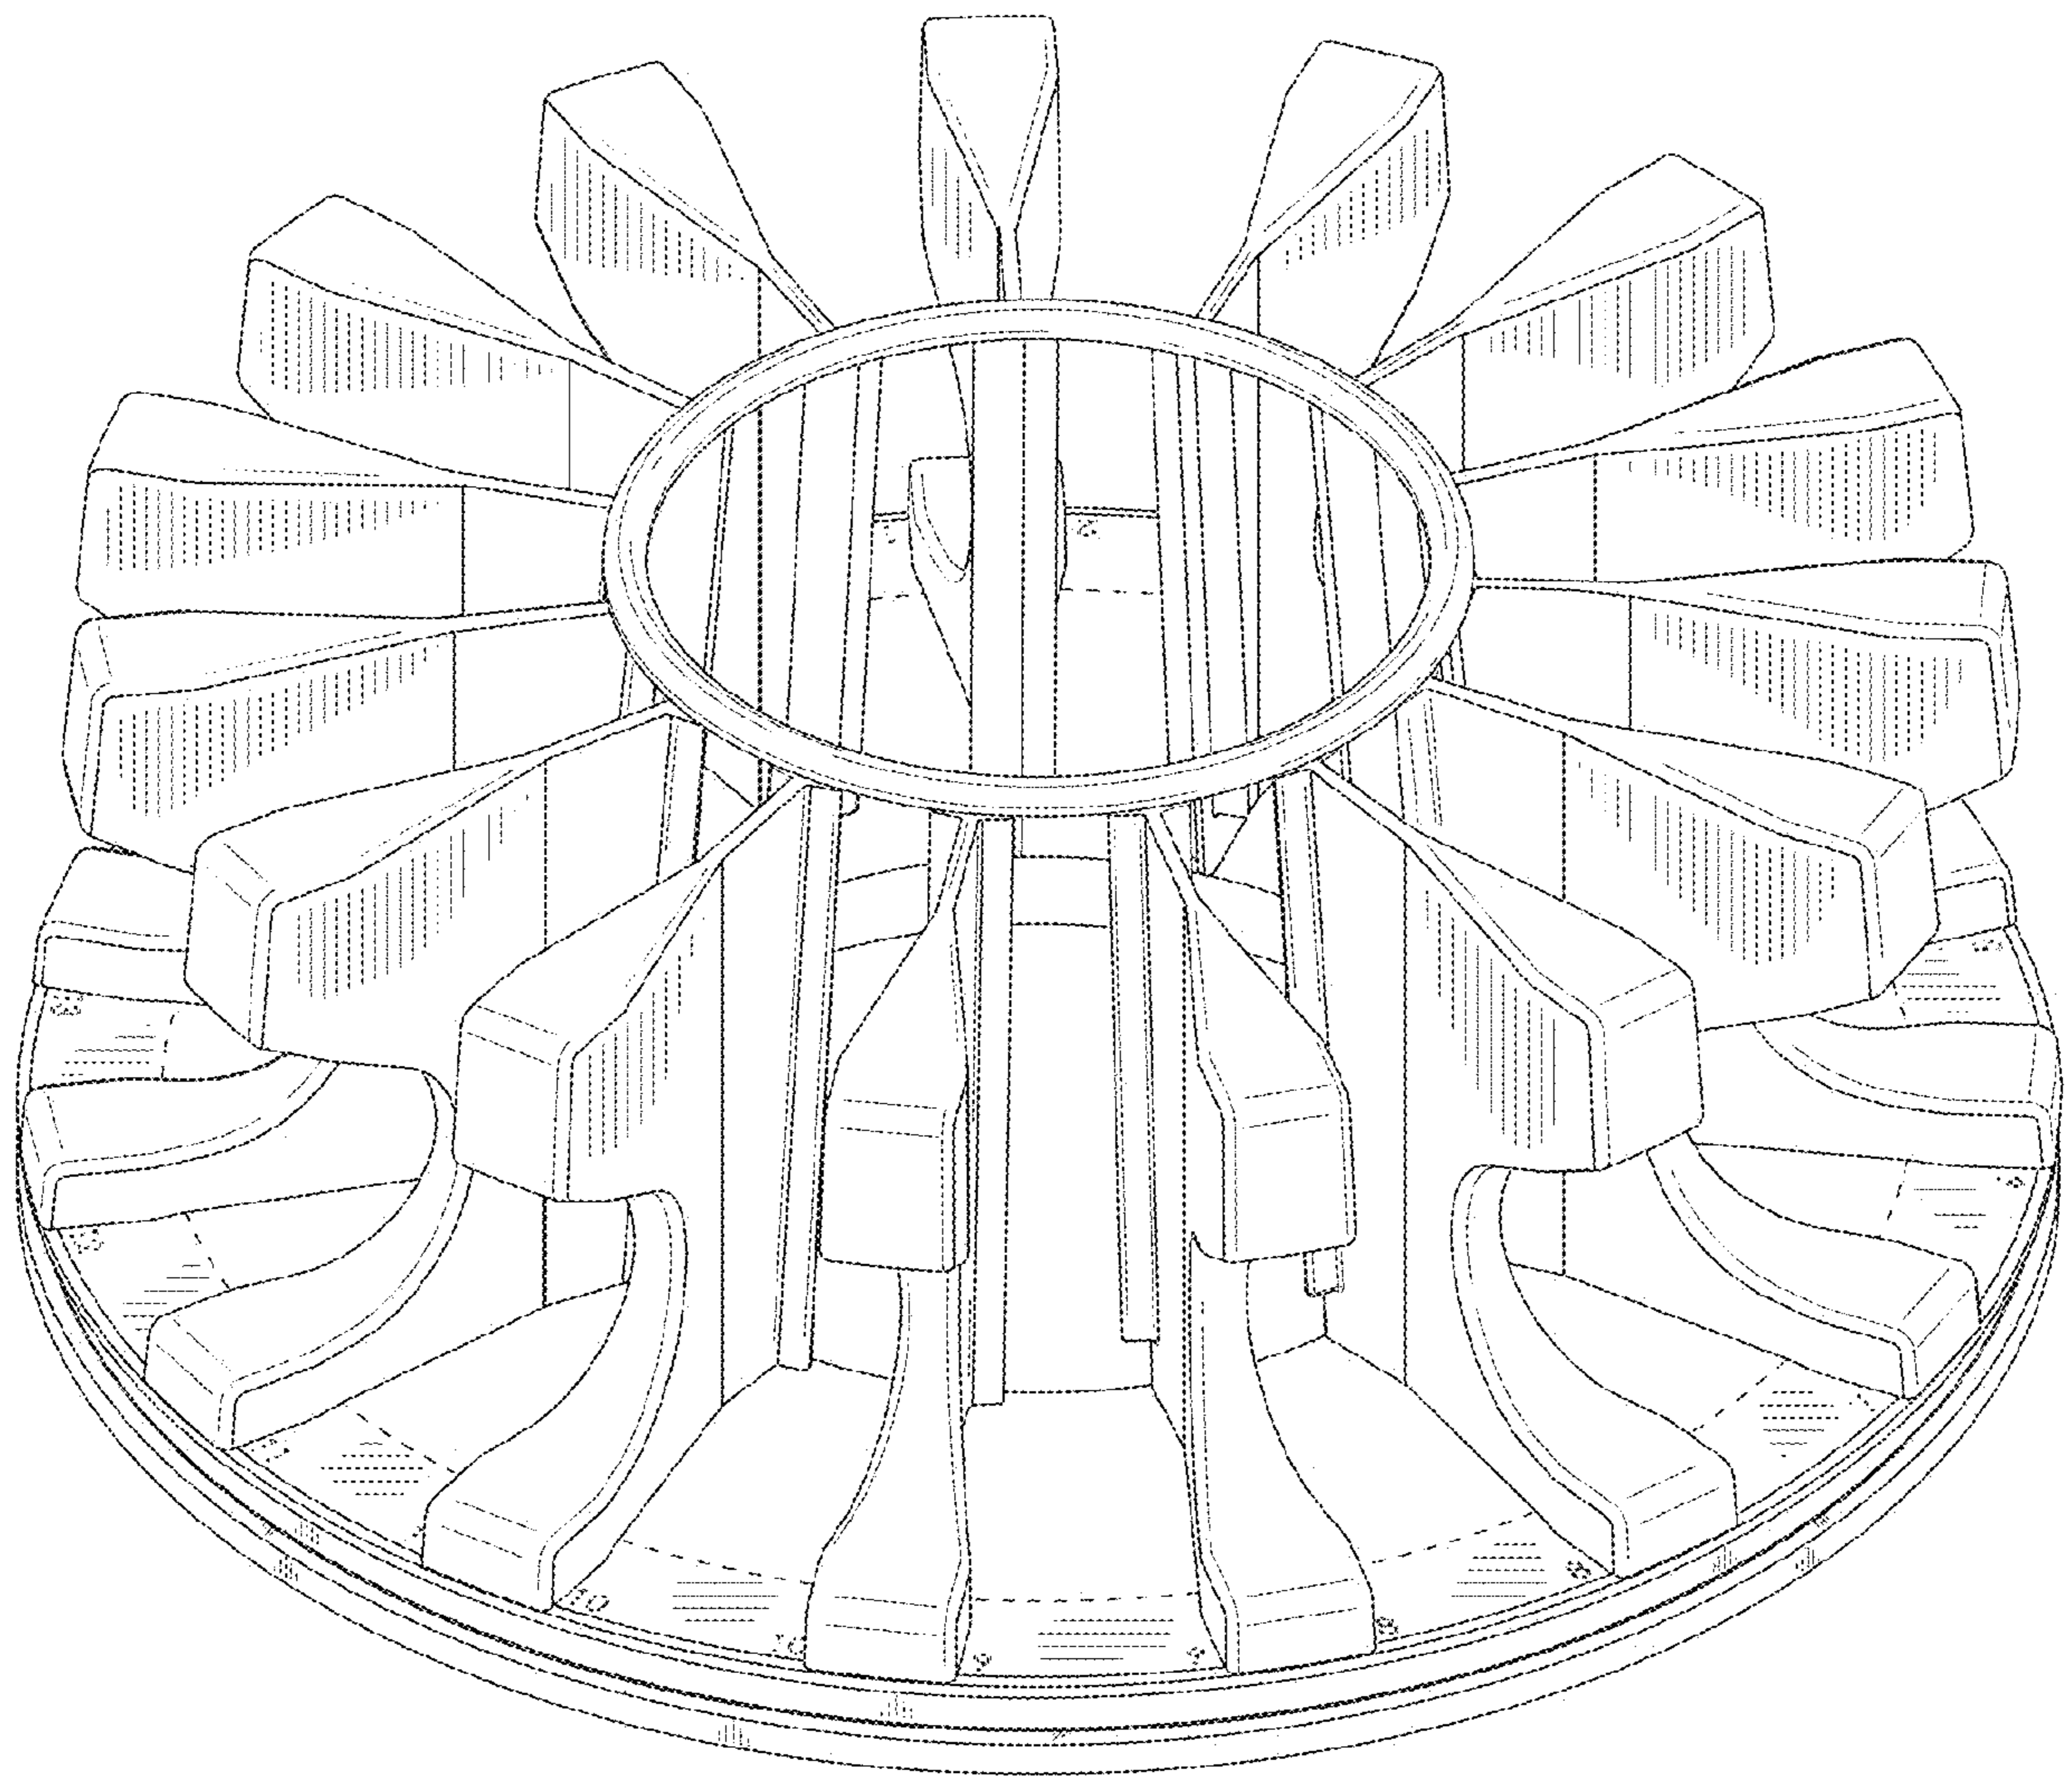


FIG. 2

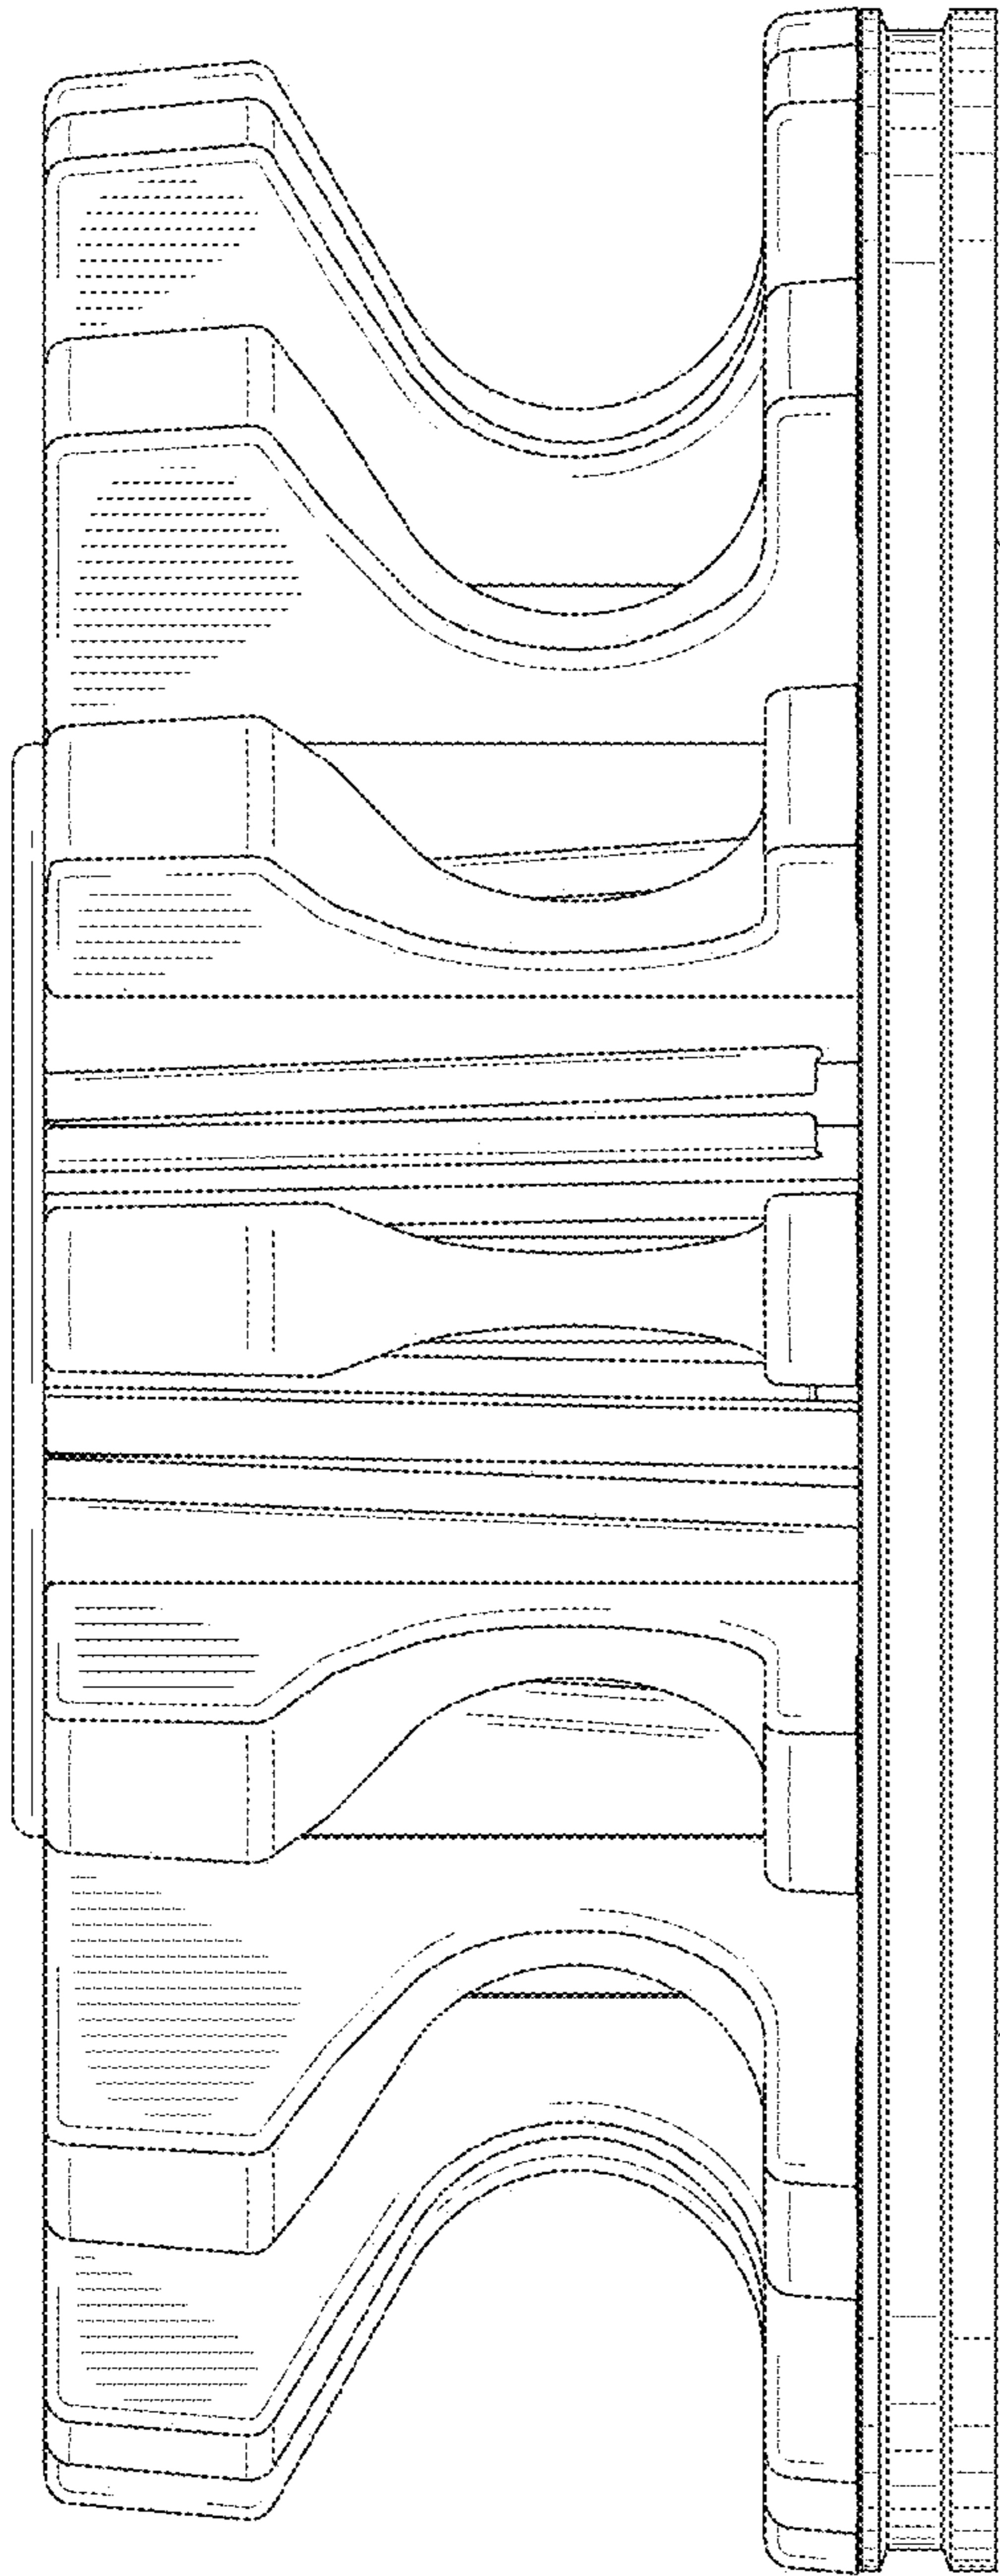


FIG. 3

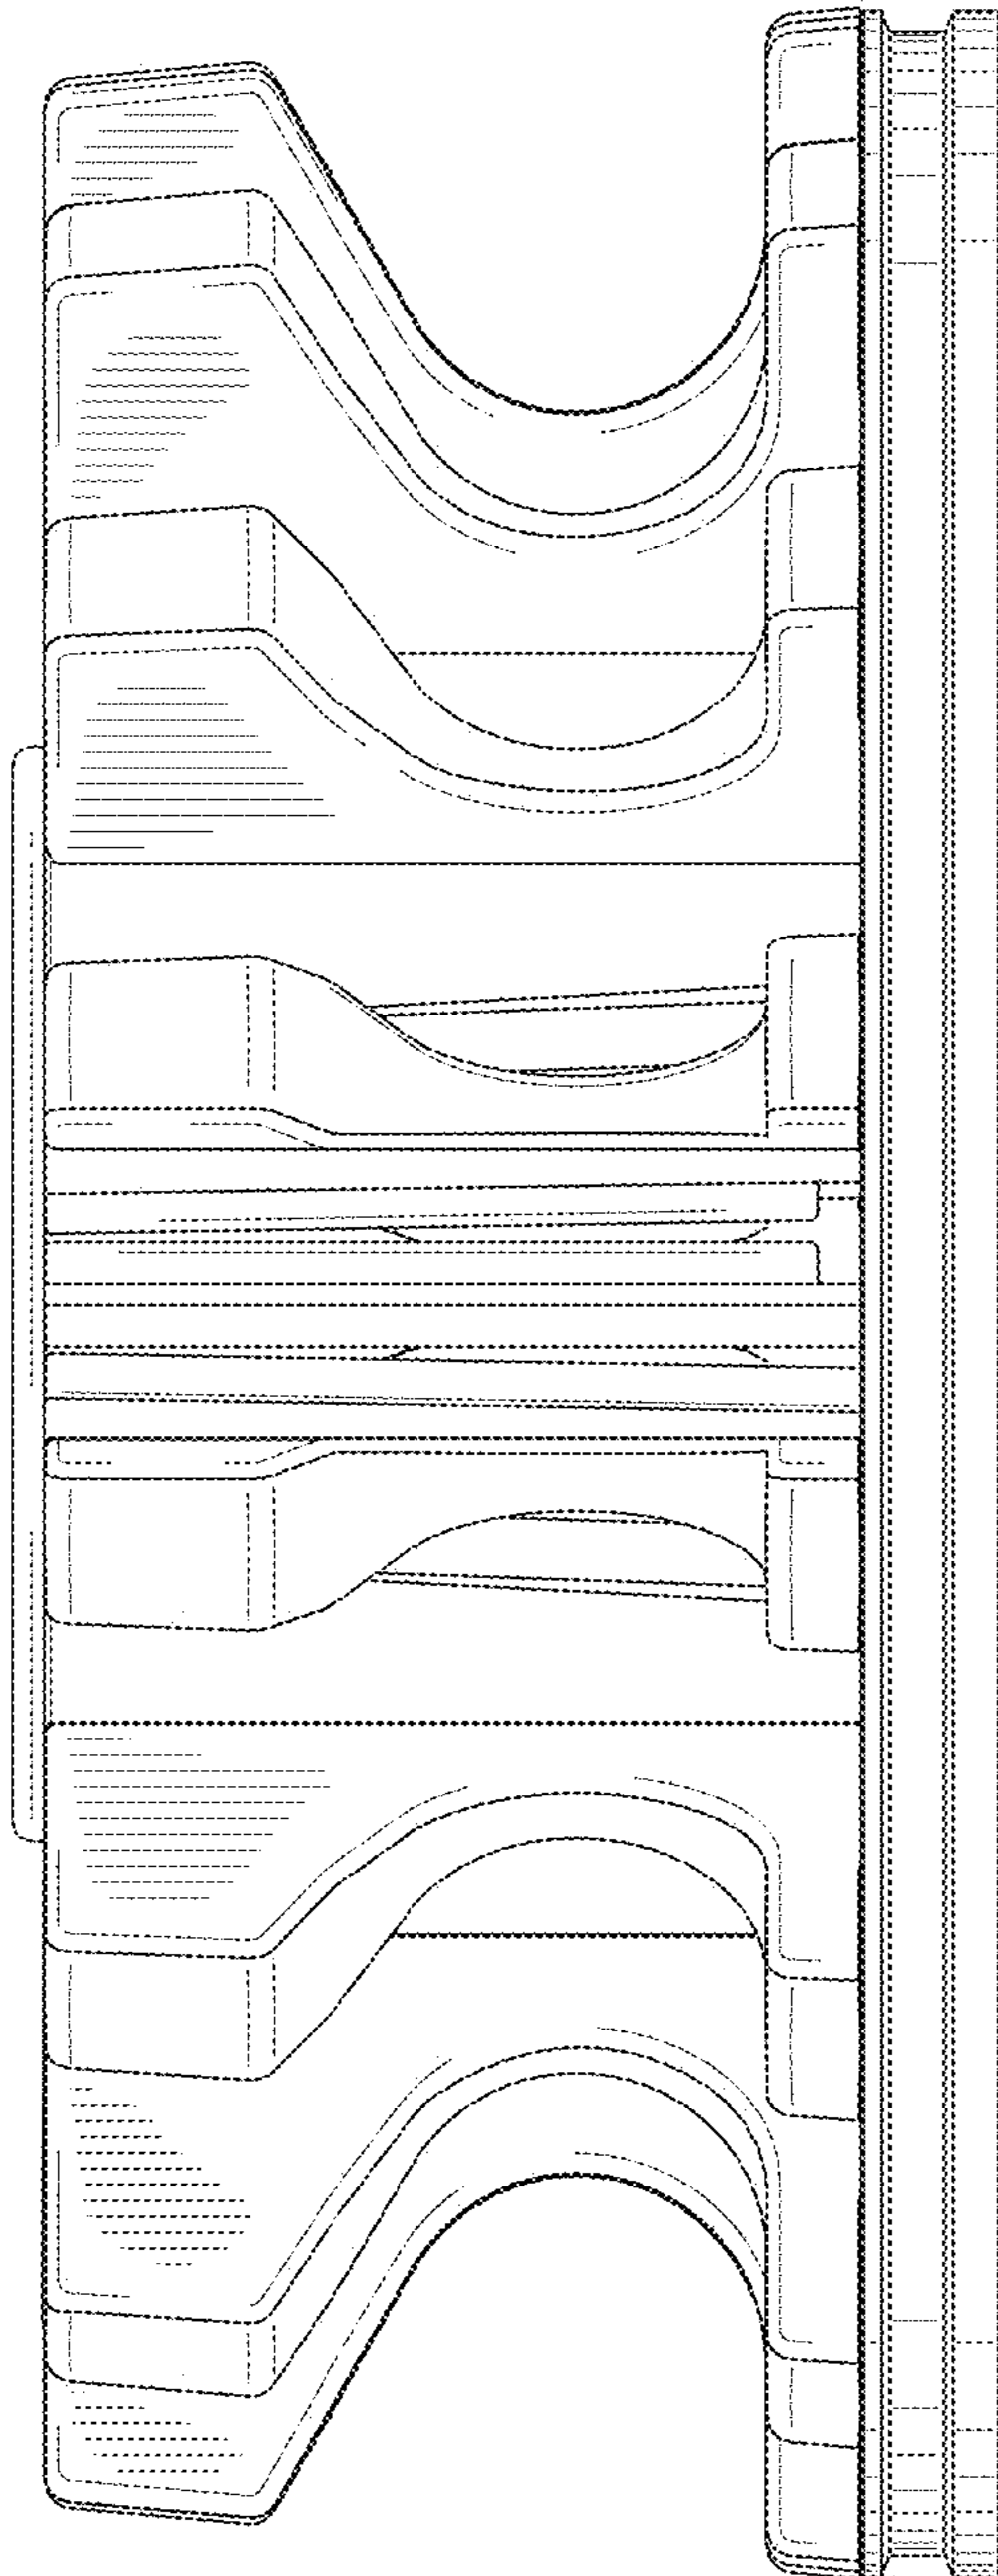


FIG. 4

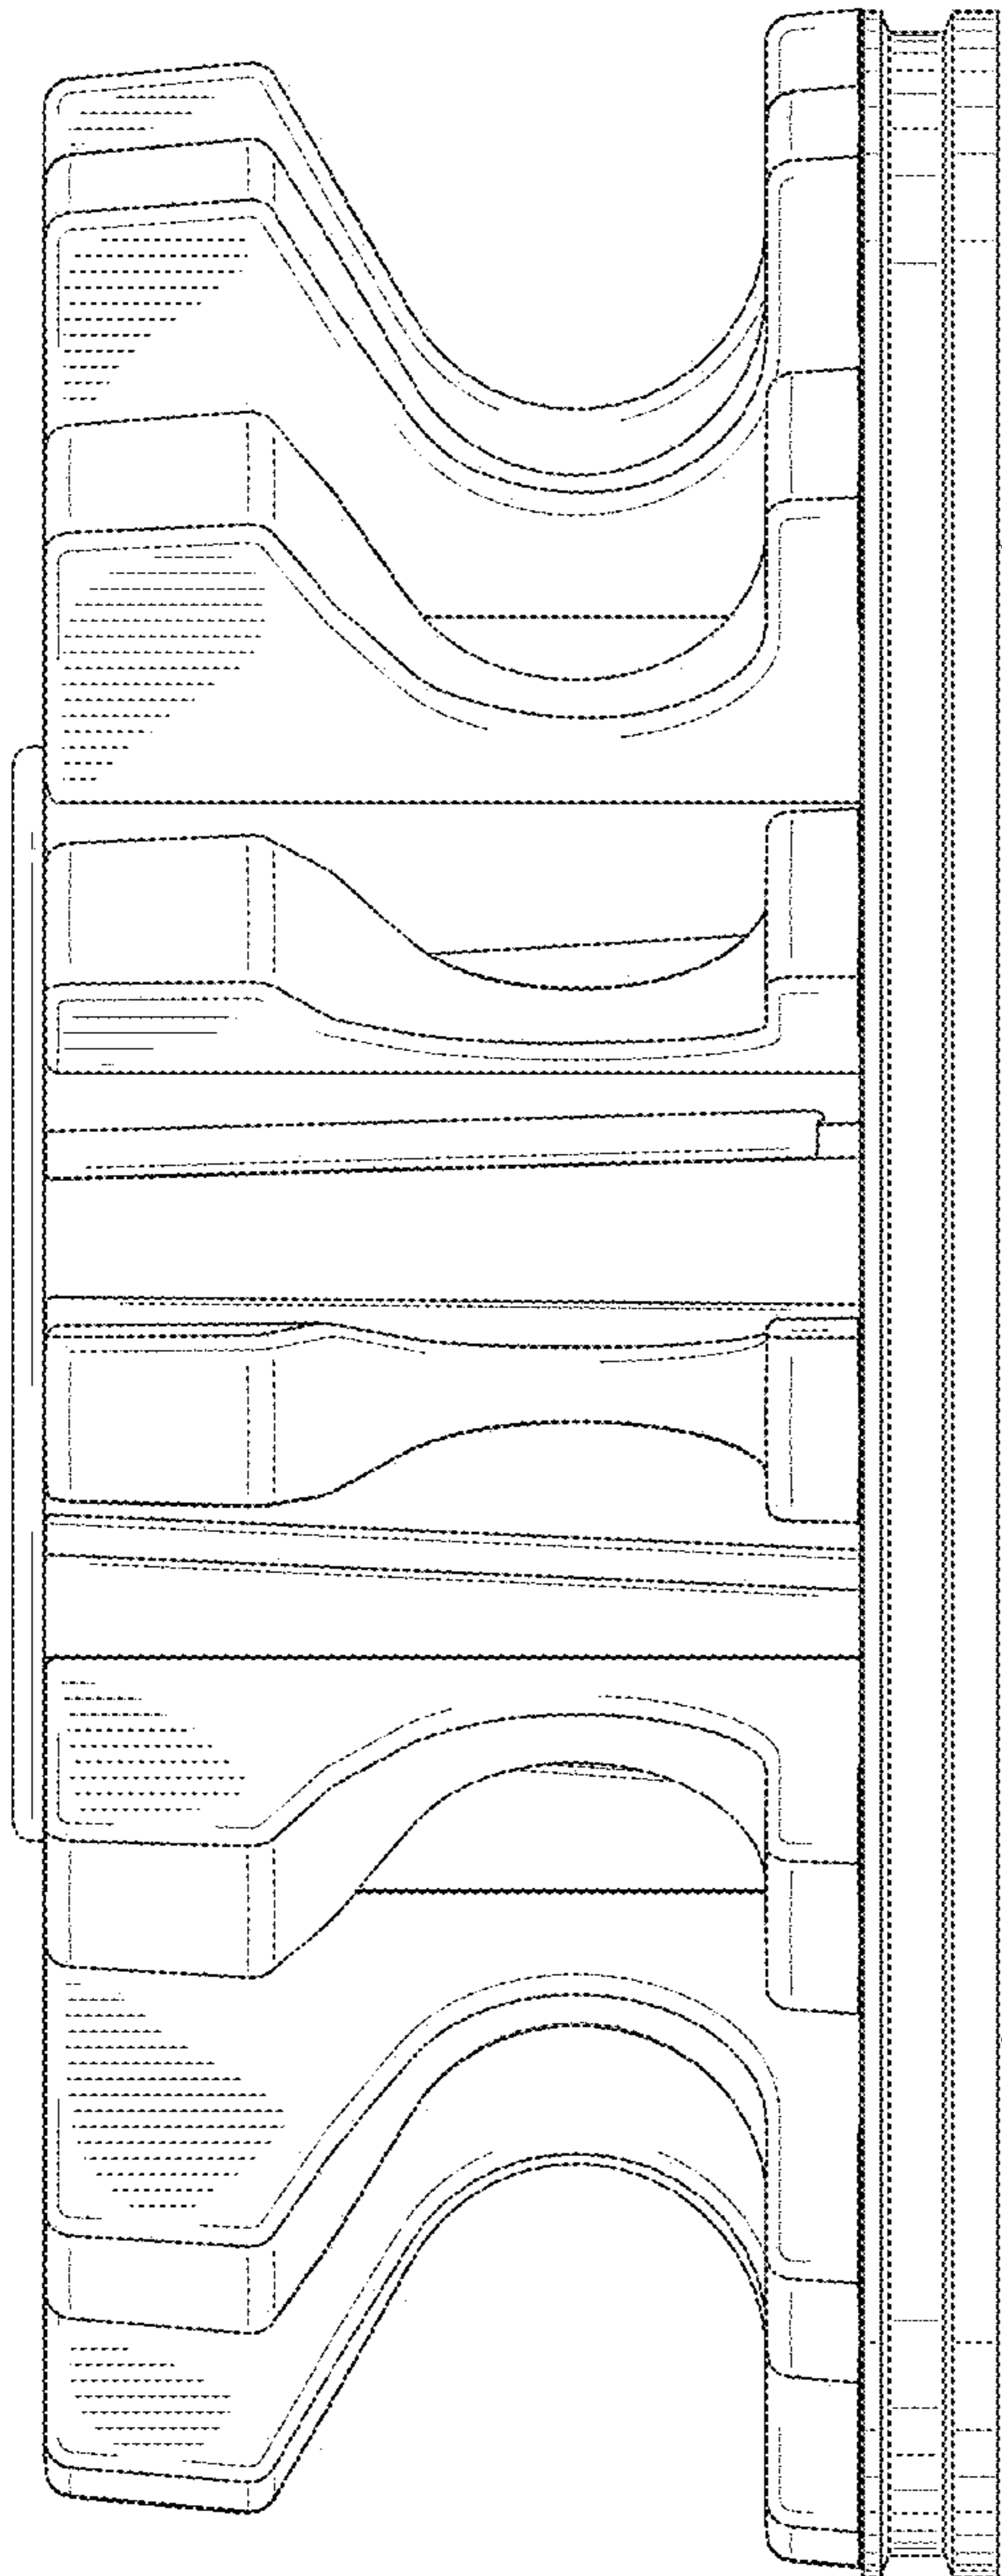


FIG. 5

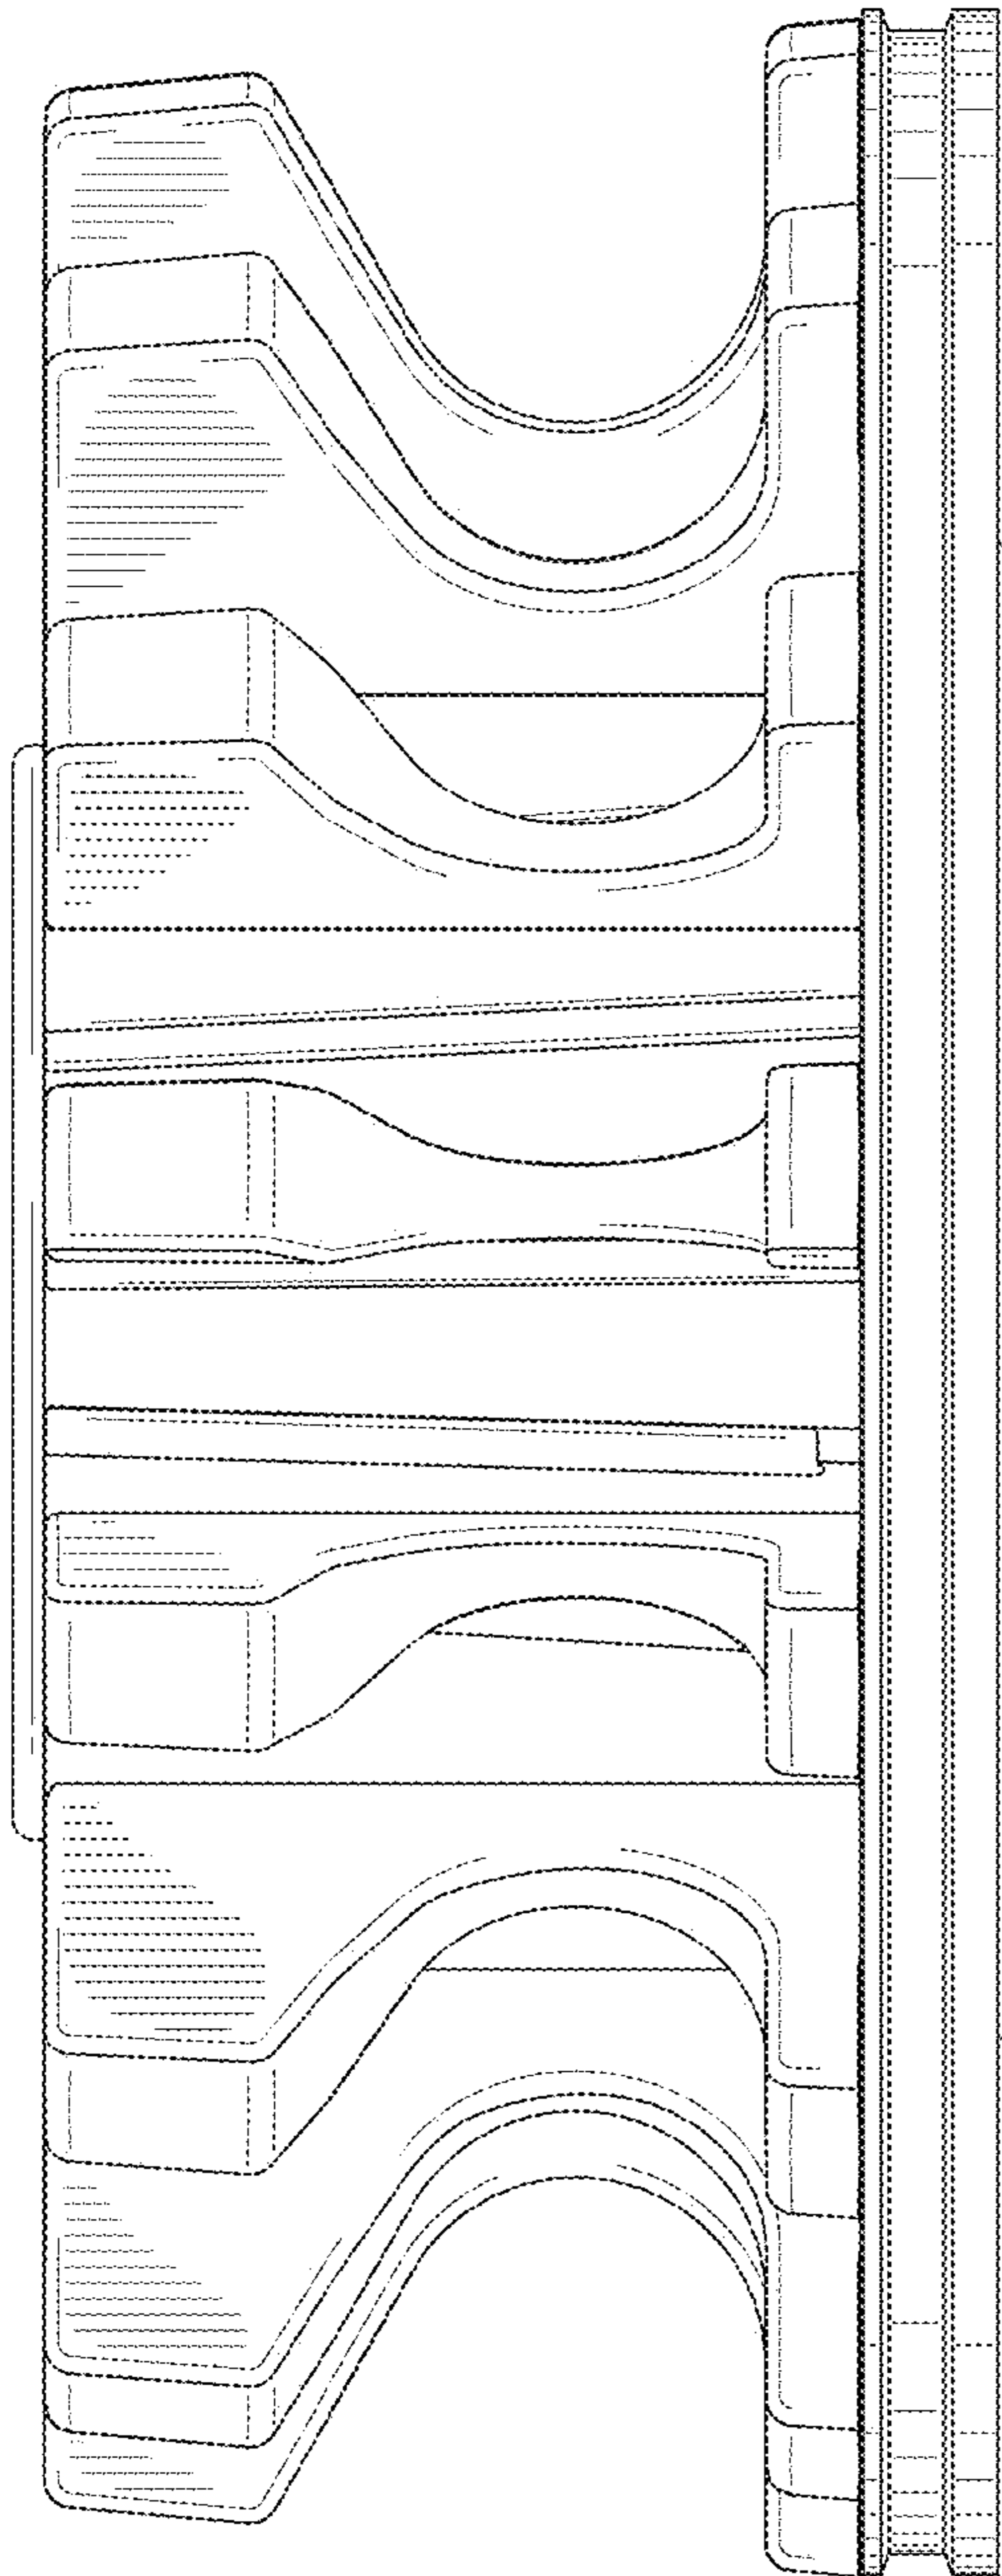


FIG. 6

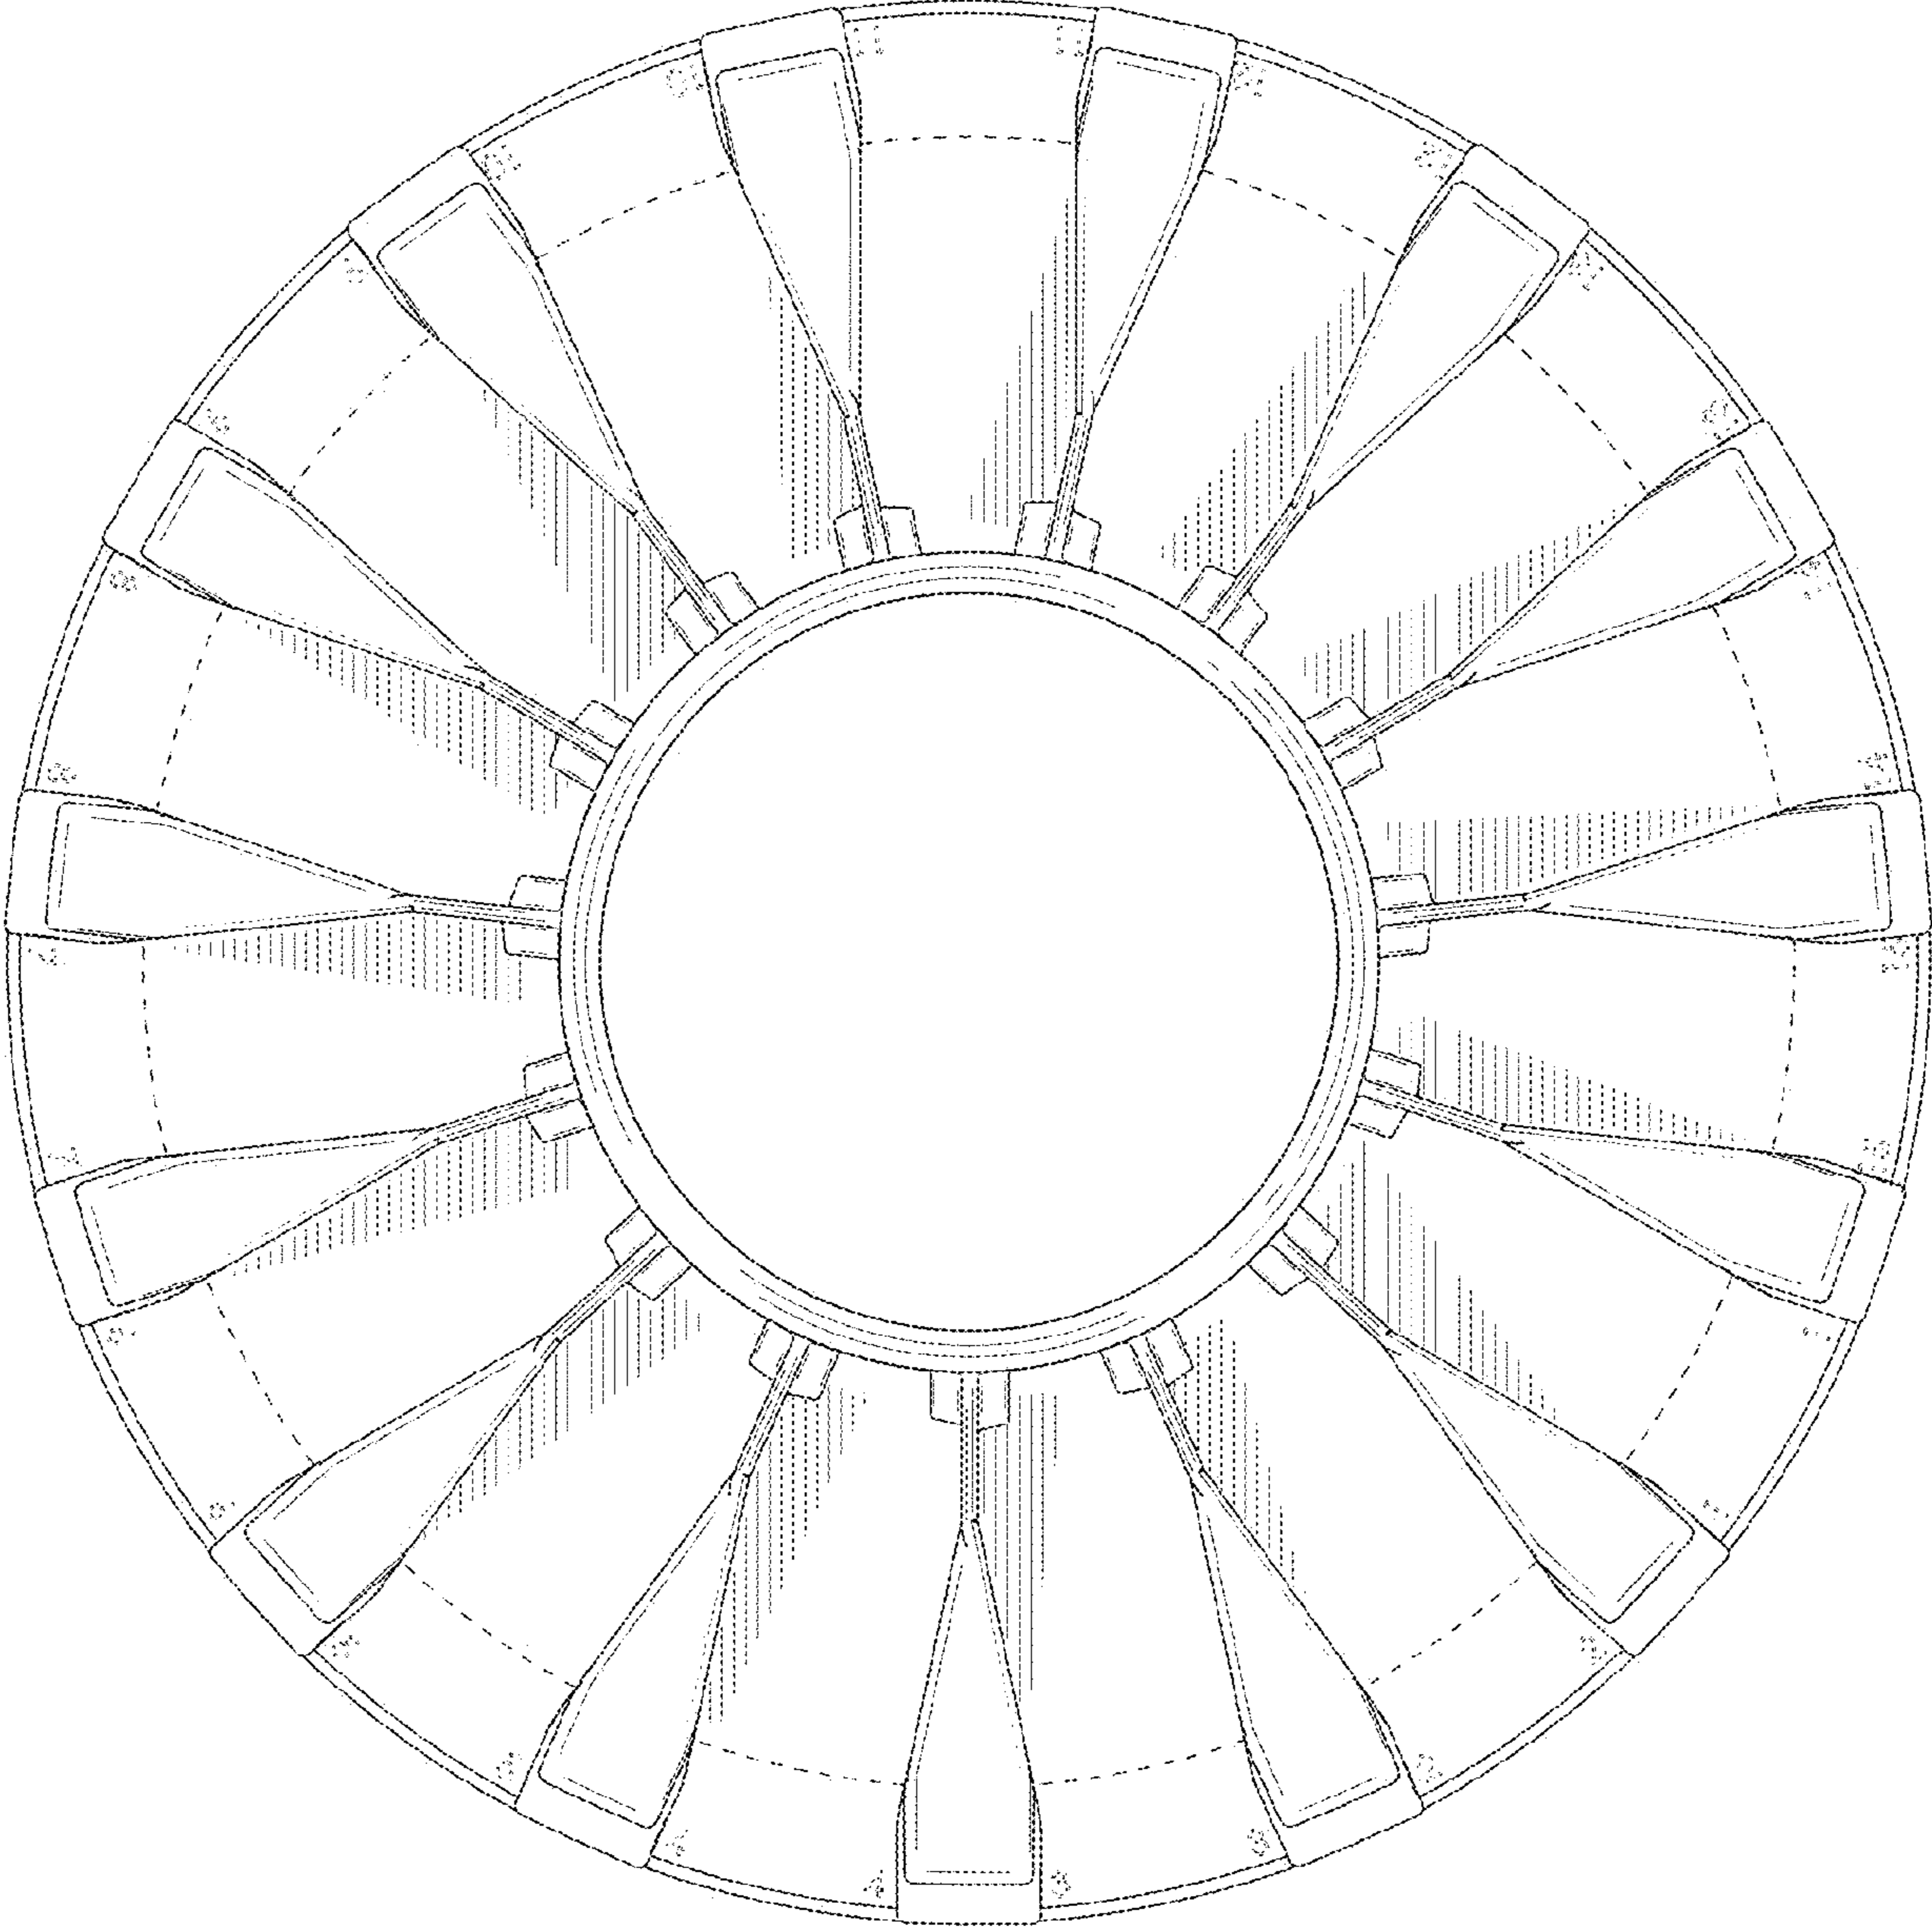


FIG. 7



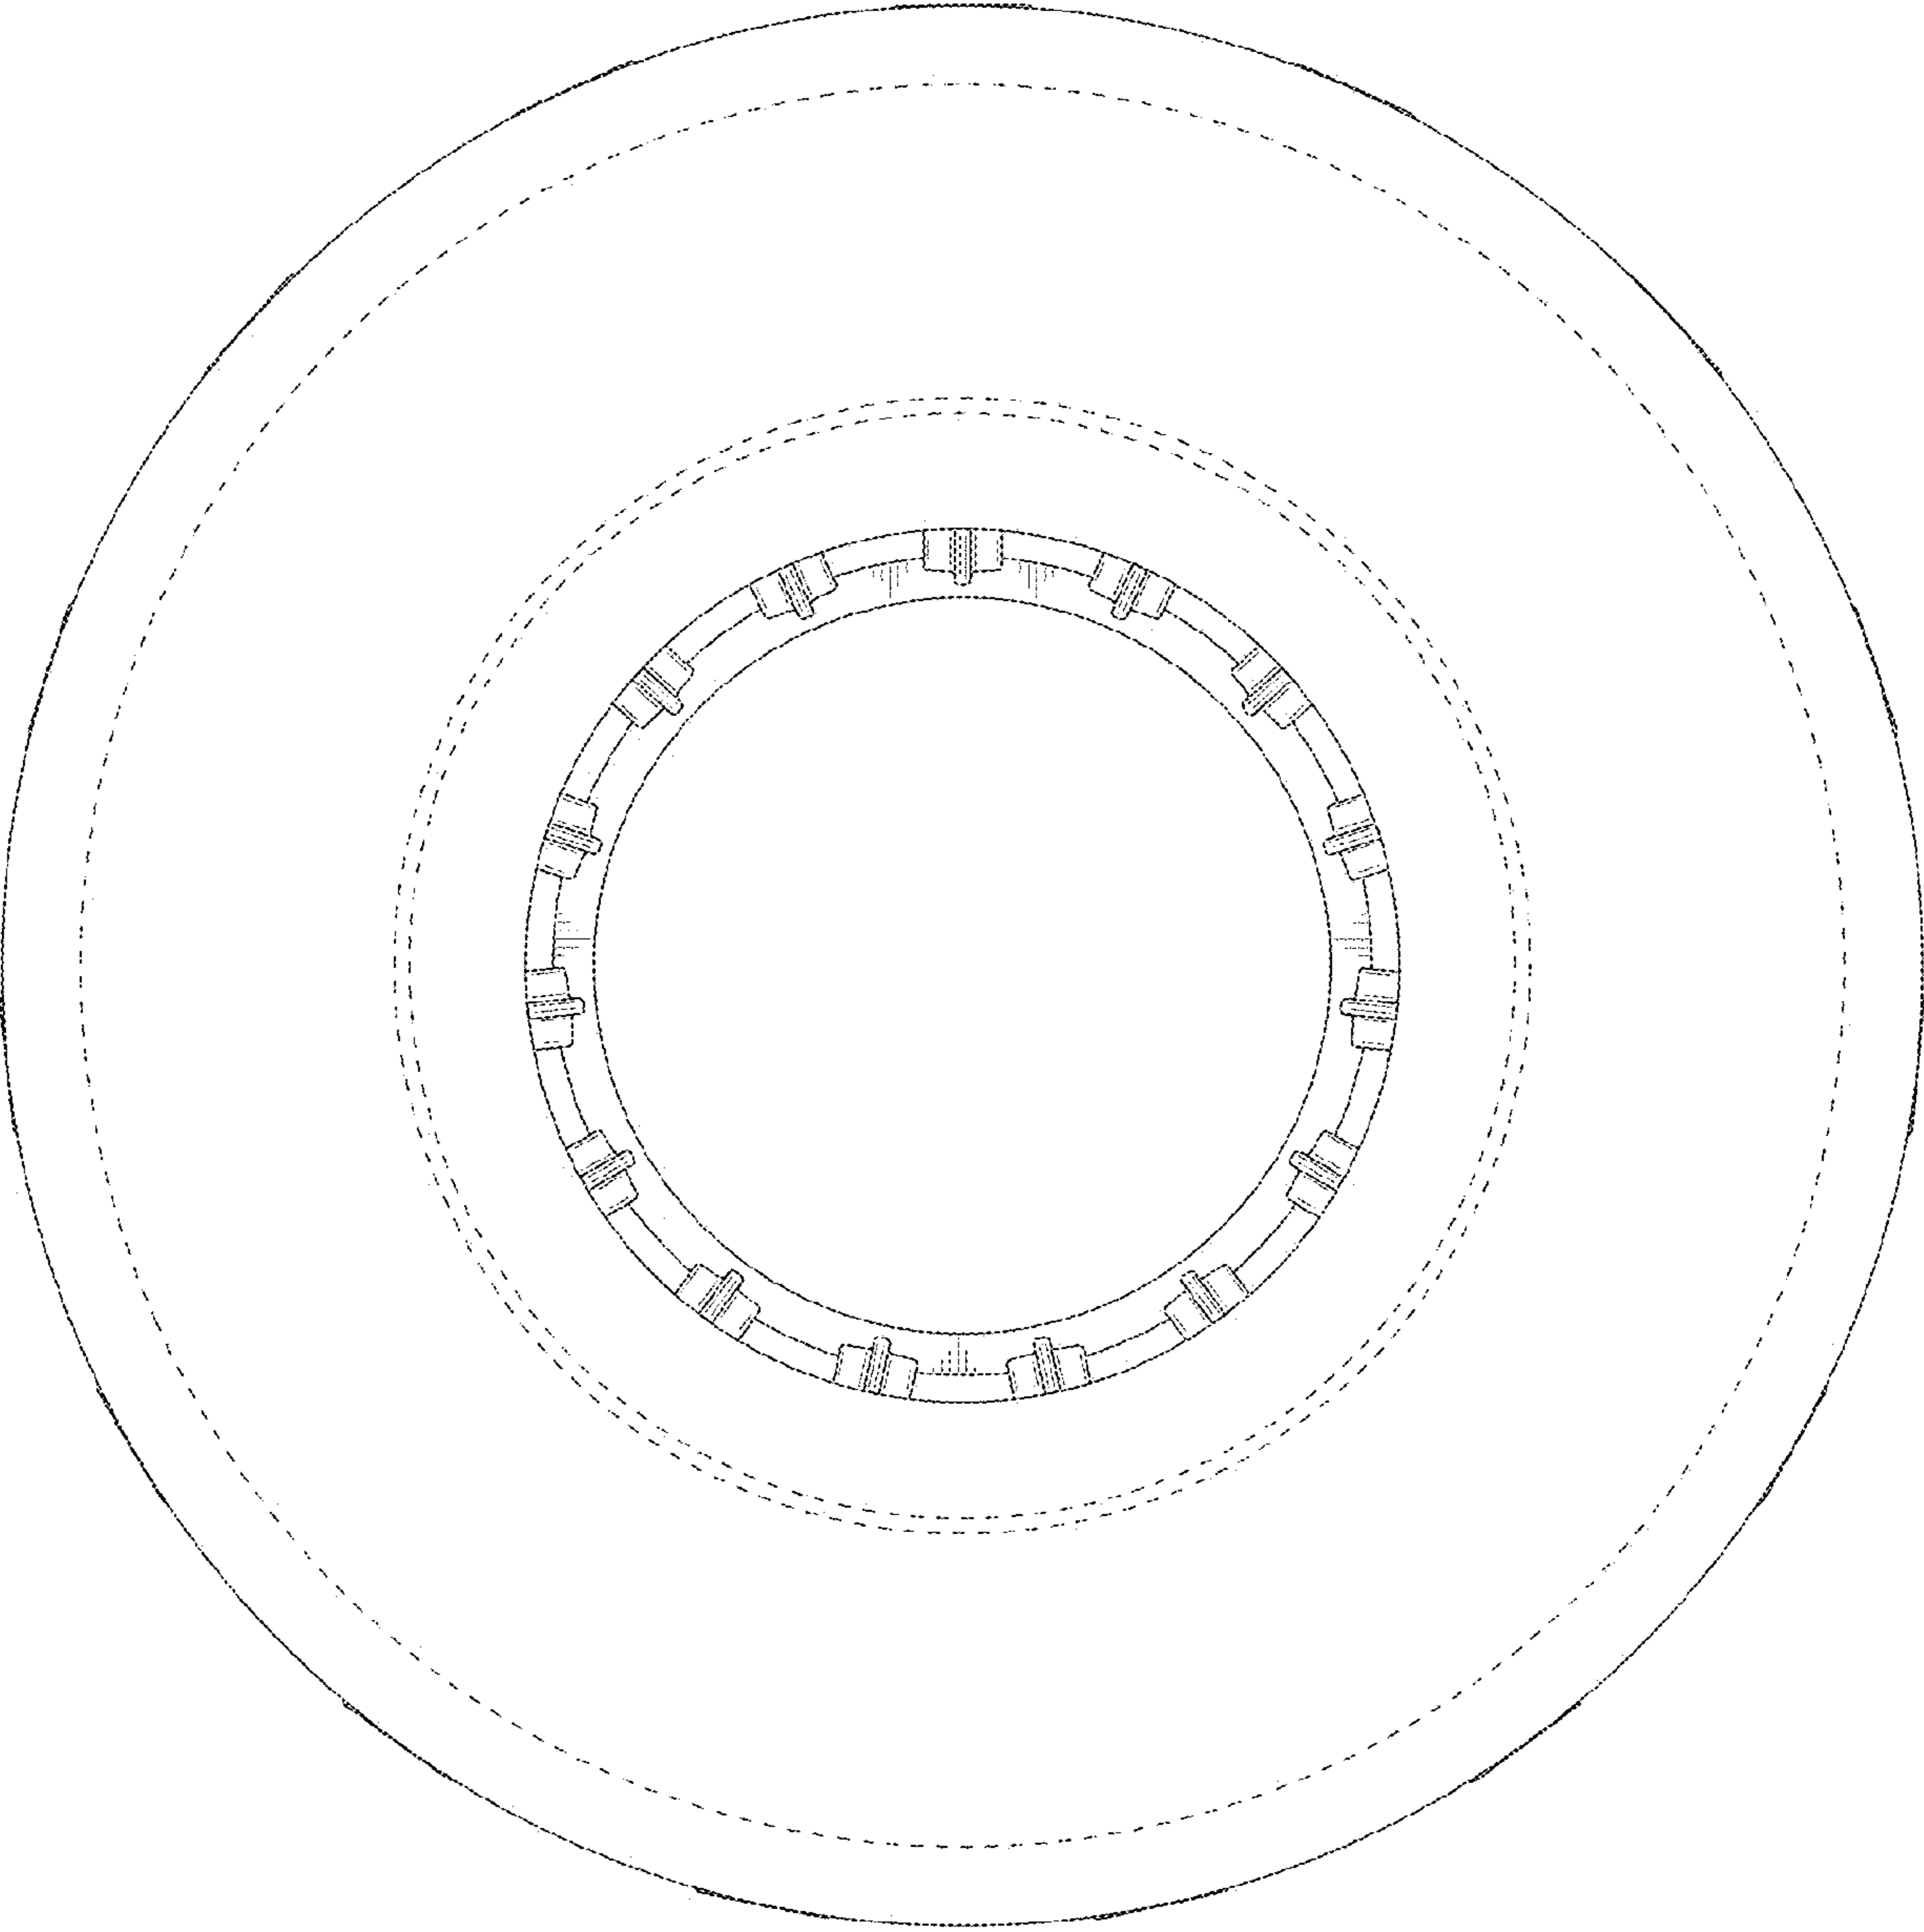


FIG. 8