



US00D893727S

(12) **United States Design Patent**  
**Zhao et al.**

(10) **Patent No.:** **US D893,727 S**

(45) **Date of Patent:** **\*\* Aug. 18, 2020**

(54) **PULSE OXIMETER**

(71) Applicant: **Xuzhou YongKang Electronic Science Technology Co., Ltd.**, Xuzhou, Jiangsu (CN)

(72) Inventors: **Xuecheng Zhao**, Xuzhou (CN);  
**Zhaohao Qiu**, Xuzhou (CN);  
**Qingyuan Li**, Xuzhou (CN)

(73) Assignee: **Xuzhou Yongkang Electronic Science Technology Co., Ltd.**, Xuzhou, Jiangsu (CN)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/682,609**

(22) Filed: **Mar. 6, 2019**

(51) **LOC (12) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/165**; D24/169

(58) **Field of Classification Search**  
USPC ..... D24/107, 164, 165–169, 186, 187;  
D10/75, 70, 98  
CPC ..... G01N 33/66; G01N 33/49; G01N 33/493;  
A61B 5/0205; A61B 5/02427; A61B  
5/02438; A61B 5/14552; A61B 5/6626;  
A61B 5/6638

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,792,052 A \* 8/1998 Isaacson ..... A61B 5/02427  
600/323  
D646,391 S \* 10/2011 Ibuki ..... D24/165

D691,726 S \* 10/2013 Jin ..... D24/167  
D718,455 S \* 11/2014 Maser ..... D24/169  
D830,557 S \* 10/2018 Sebban ..... D24/167  
D877,339 S \* 3/2020 Xian ..... D24/165  
2010/0317944 A1\* 12/2010 Wang ..... A61B 5/14552  
600/323  
2019/0090795 A1\* 3/2019 Boller ..... A61B 5/14552

**OTHER PUBLICATIONS**

U.S. Appl. No. 29/682,612, filed Mar. 6, 2019, Zhao et al.

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Leydig, Voit & Mayer, Ltd.

(57) **CLAIM**


The ornamental design for a pulse oximeter, as shown and described.


**DESCRIPTION**

FIG. 1 is a top, right, front perspective view of a pulse oximeter showing the new design;  
FIG. 2 is a bottom, back, left perspective view thereof;  
FIG. 3 is a front view thereof;  
FIG. 4 is a back view thereof;  
FIG. 5 is a side view thereof;  
FIG. 6 is another side view thereof;  
FIG. 7 is a top view thereof; and,  
FIG. 8 is a bottom view thereof.

The broken lines illustrate portions of the pulse oximeter that form no part of the claimed design. The broken lines form no part of the claimed design.

**1 Claim, 8 Drawing Sheets**

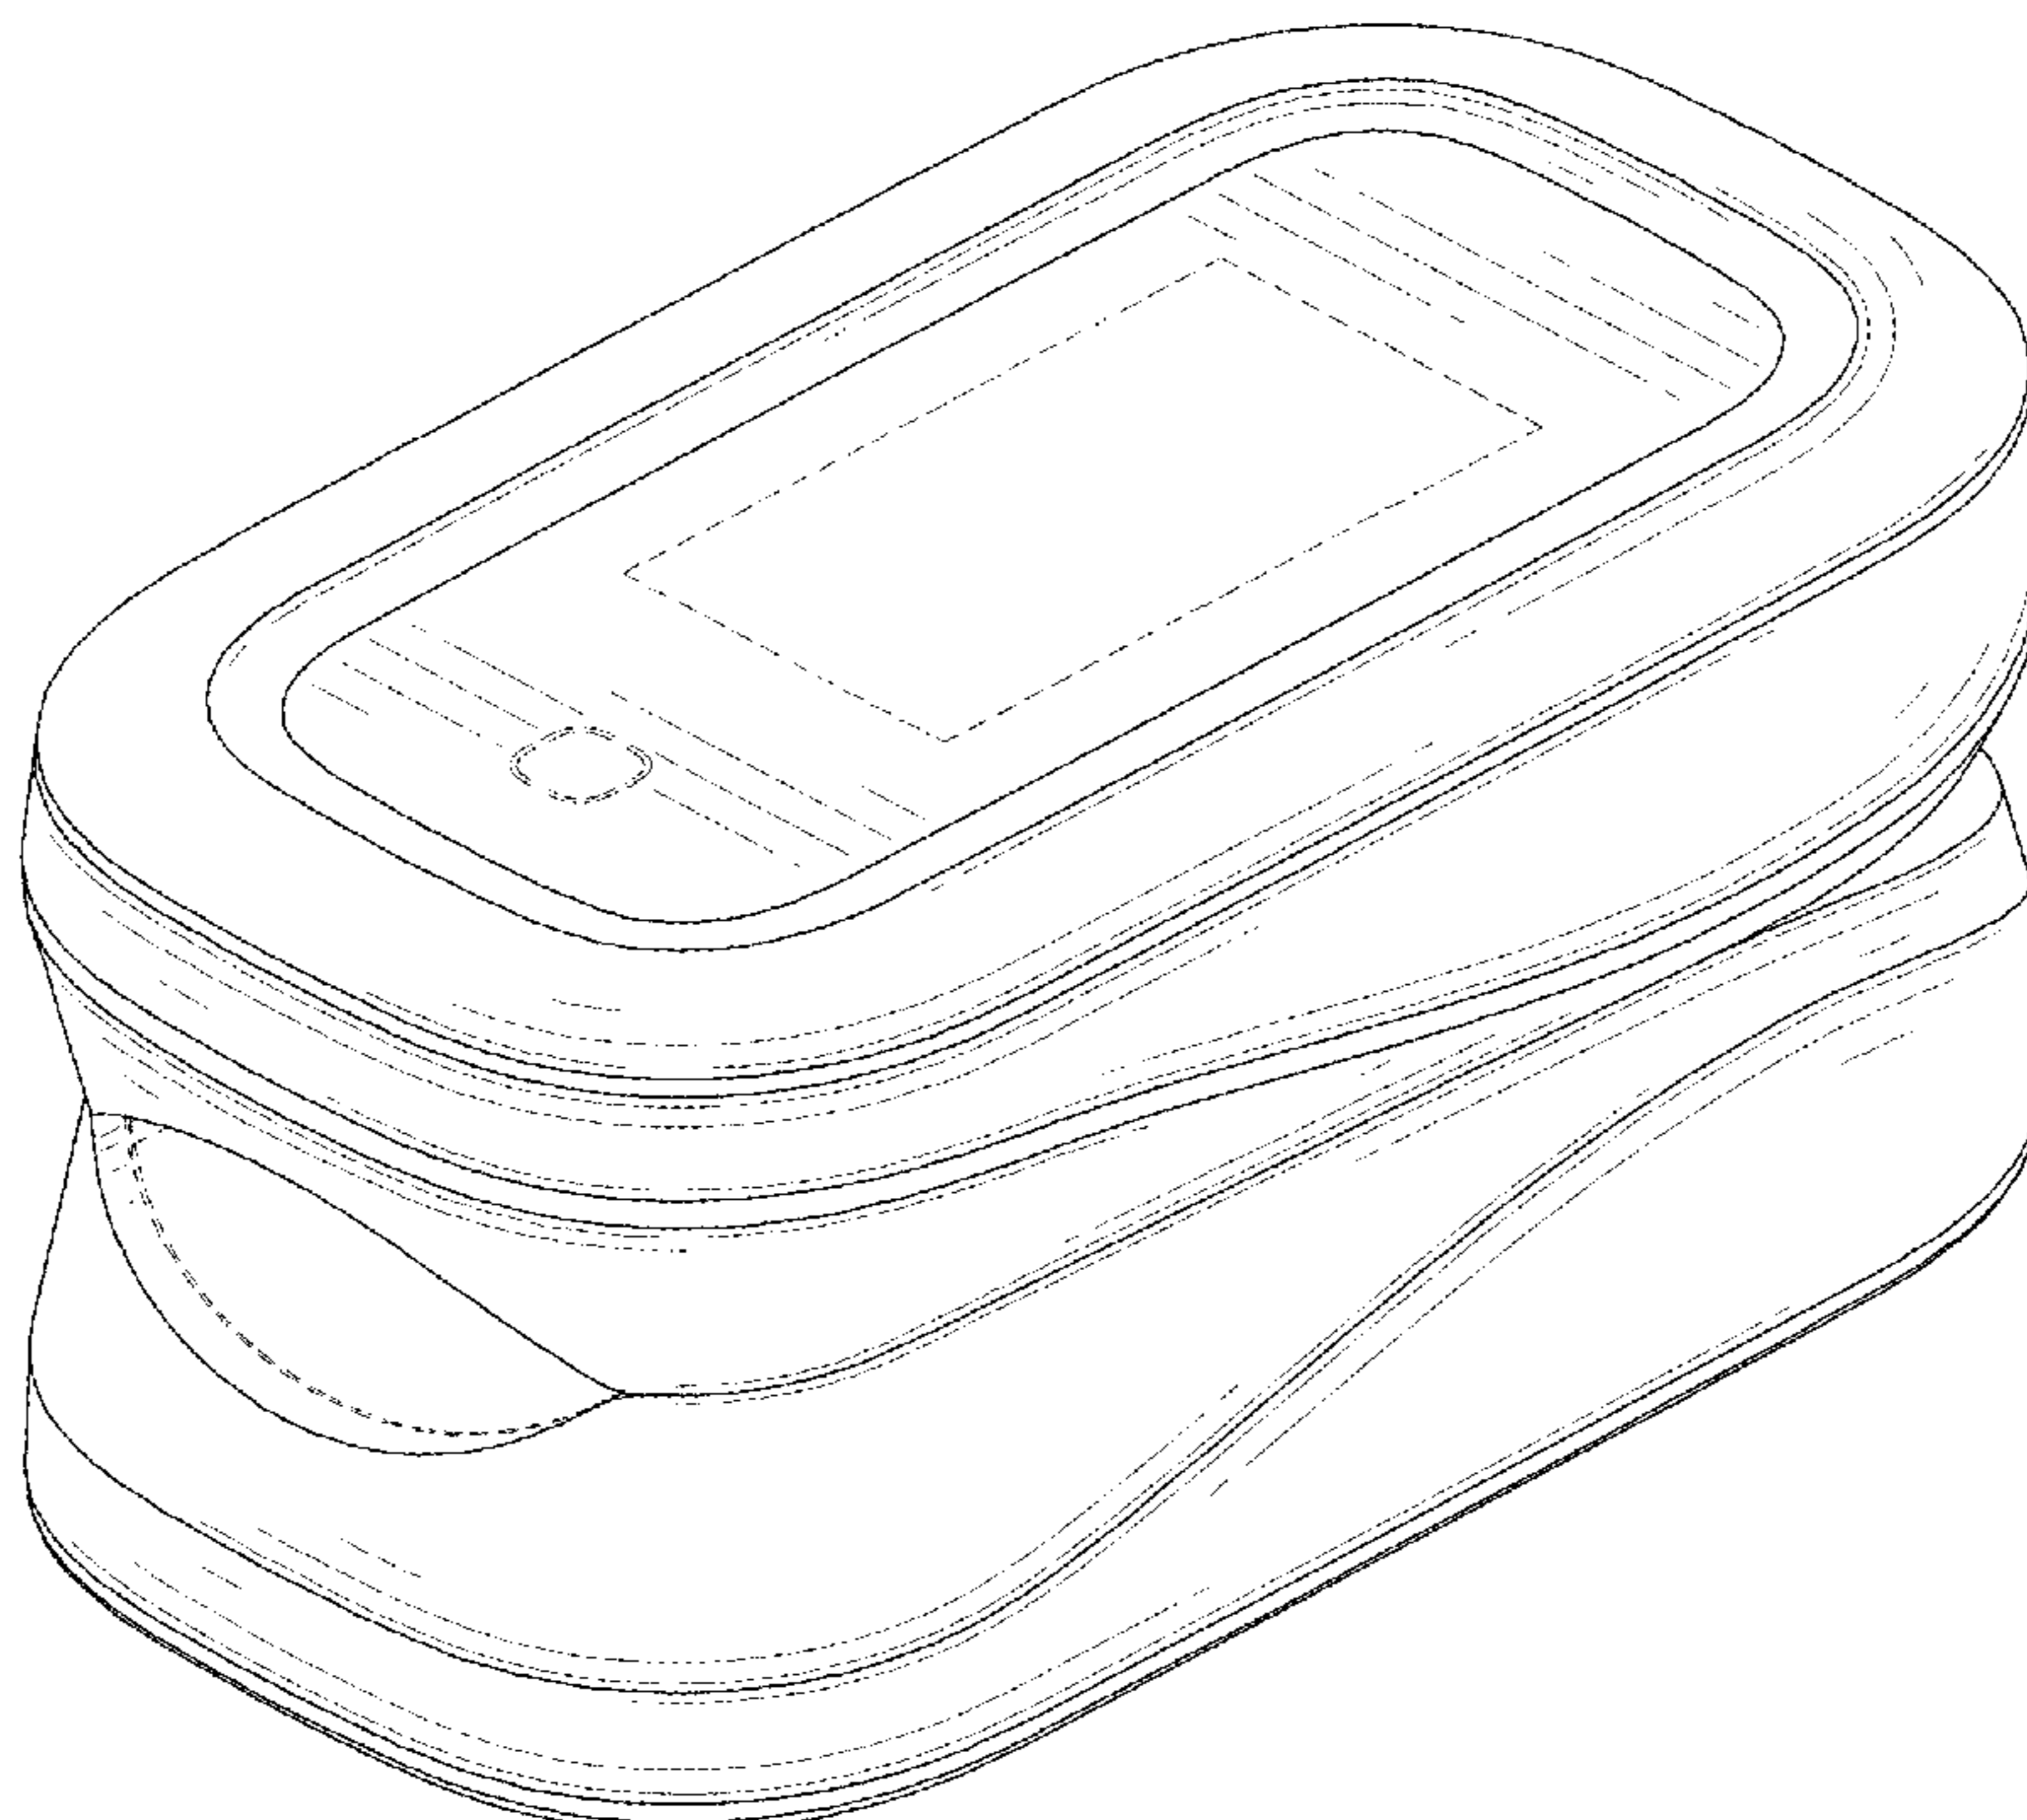

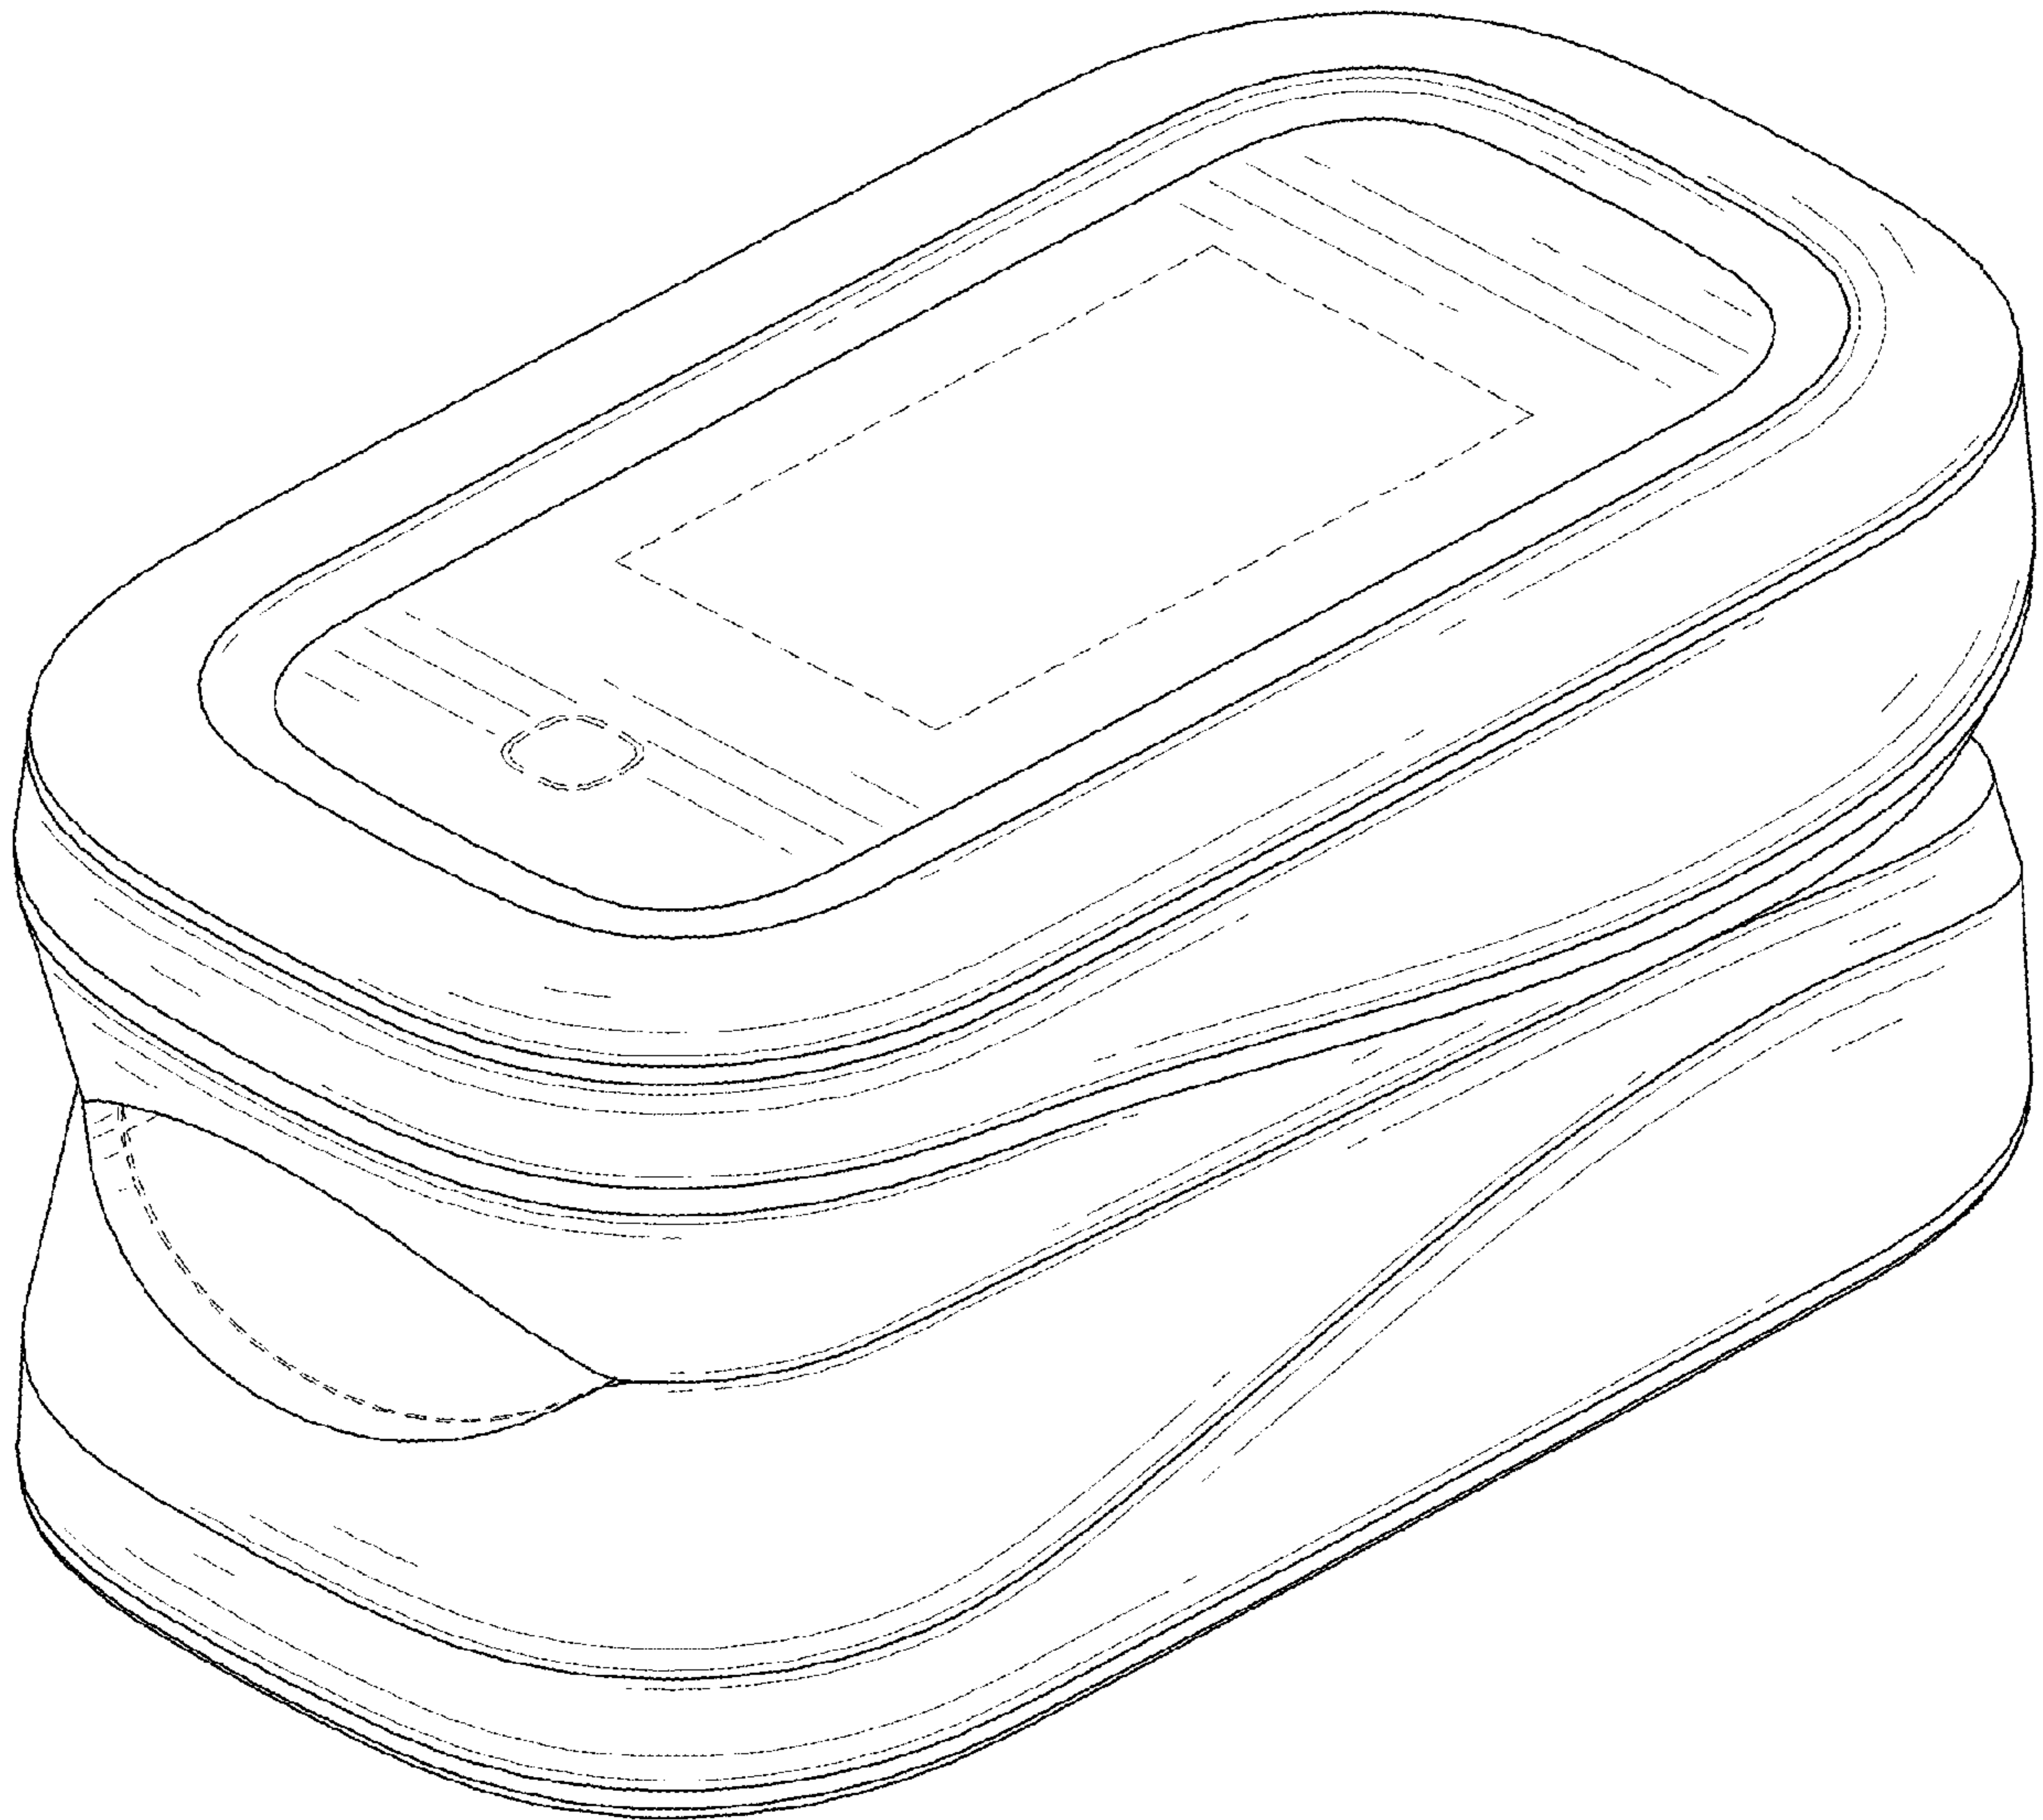

**Fig. 1**

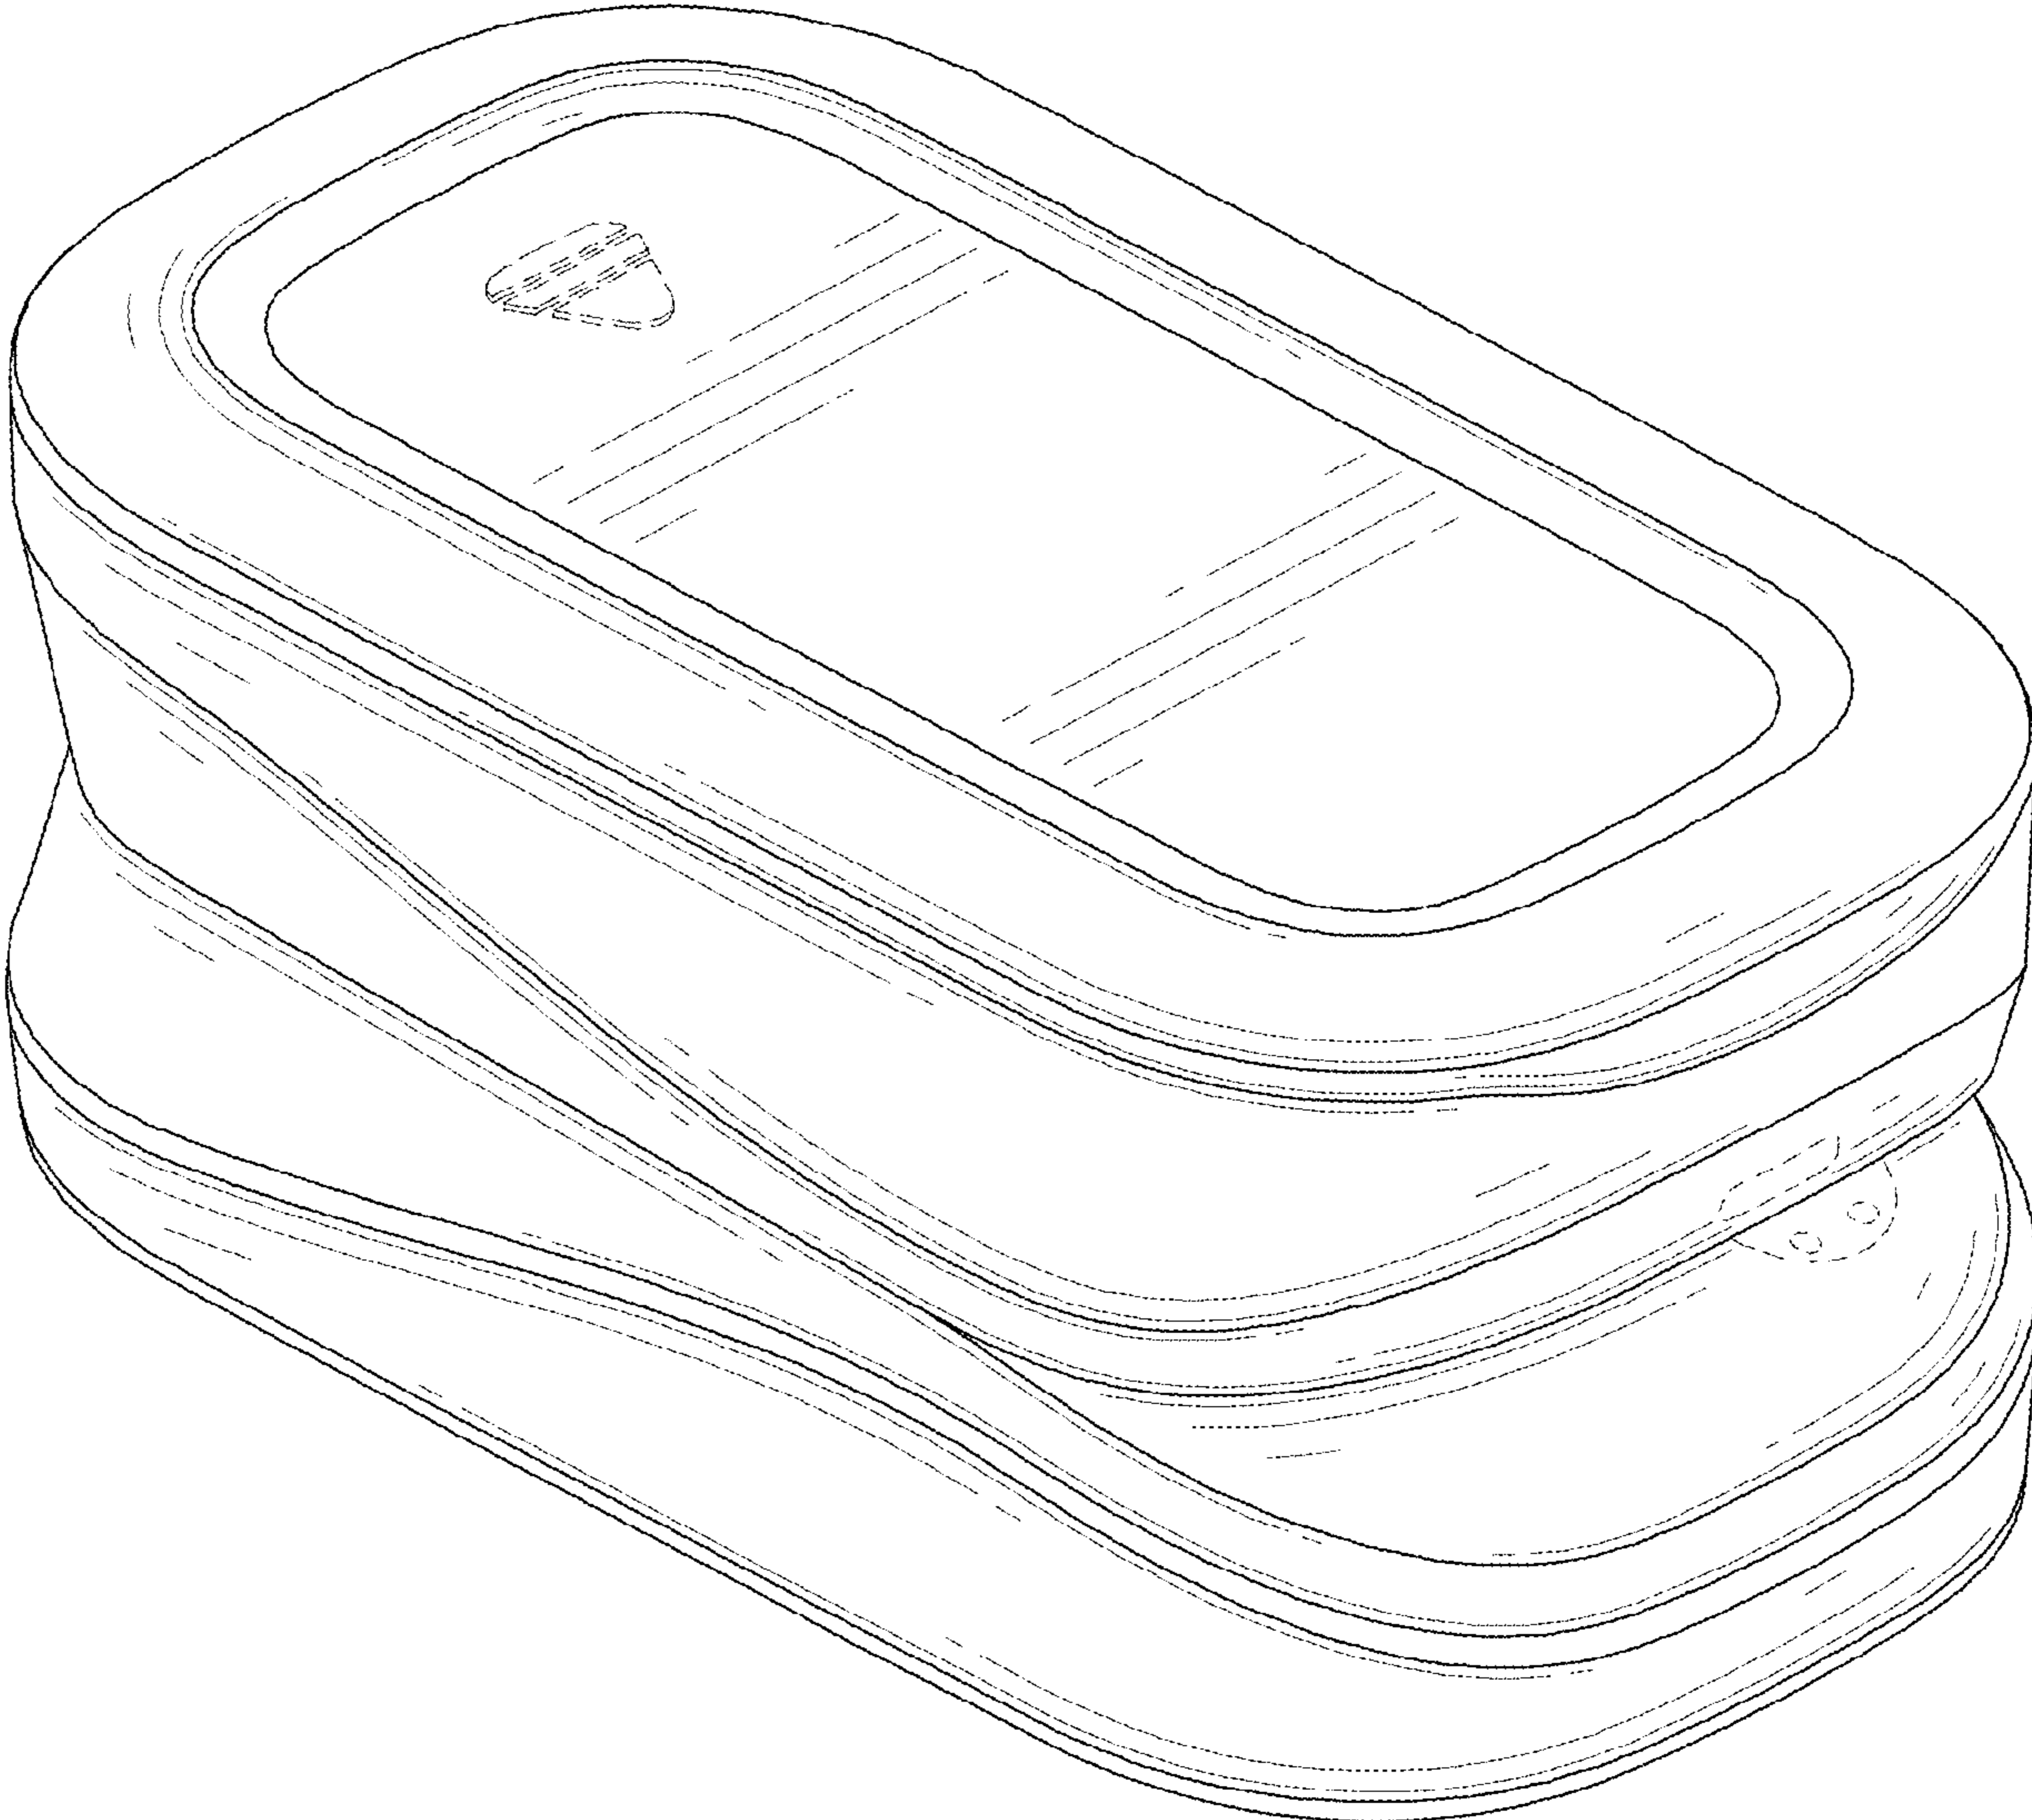


Fig. 2

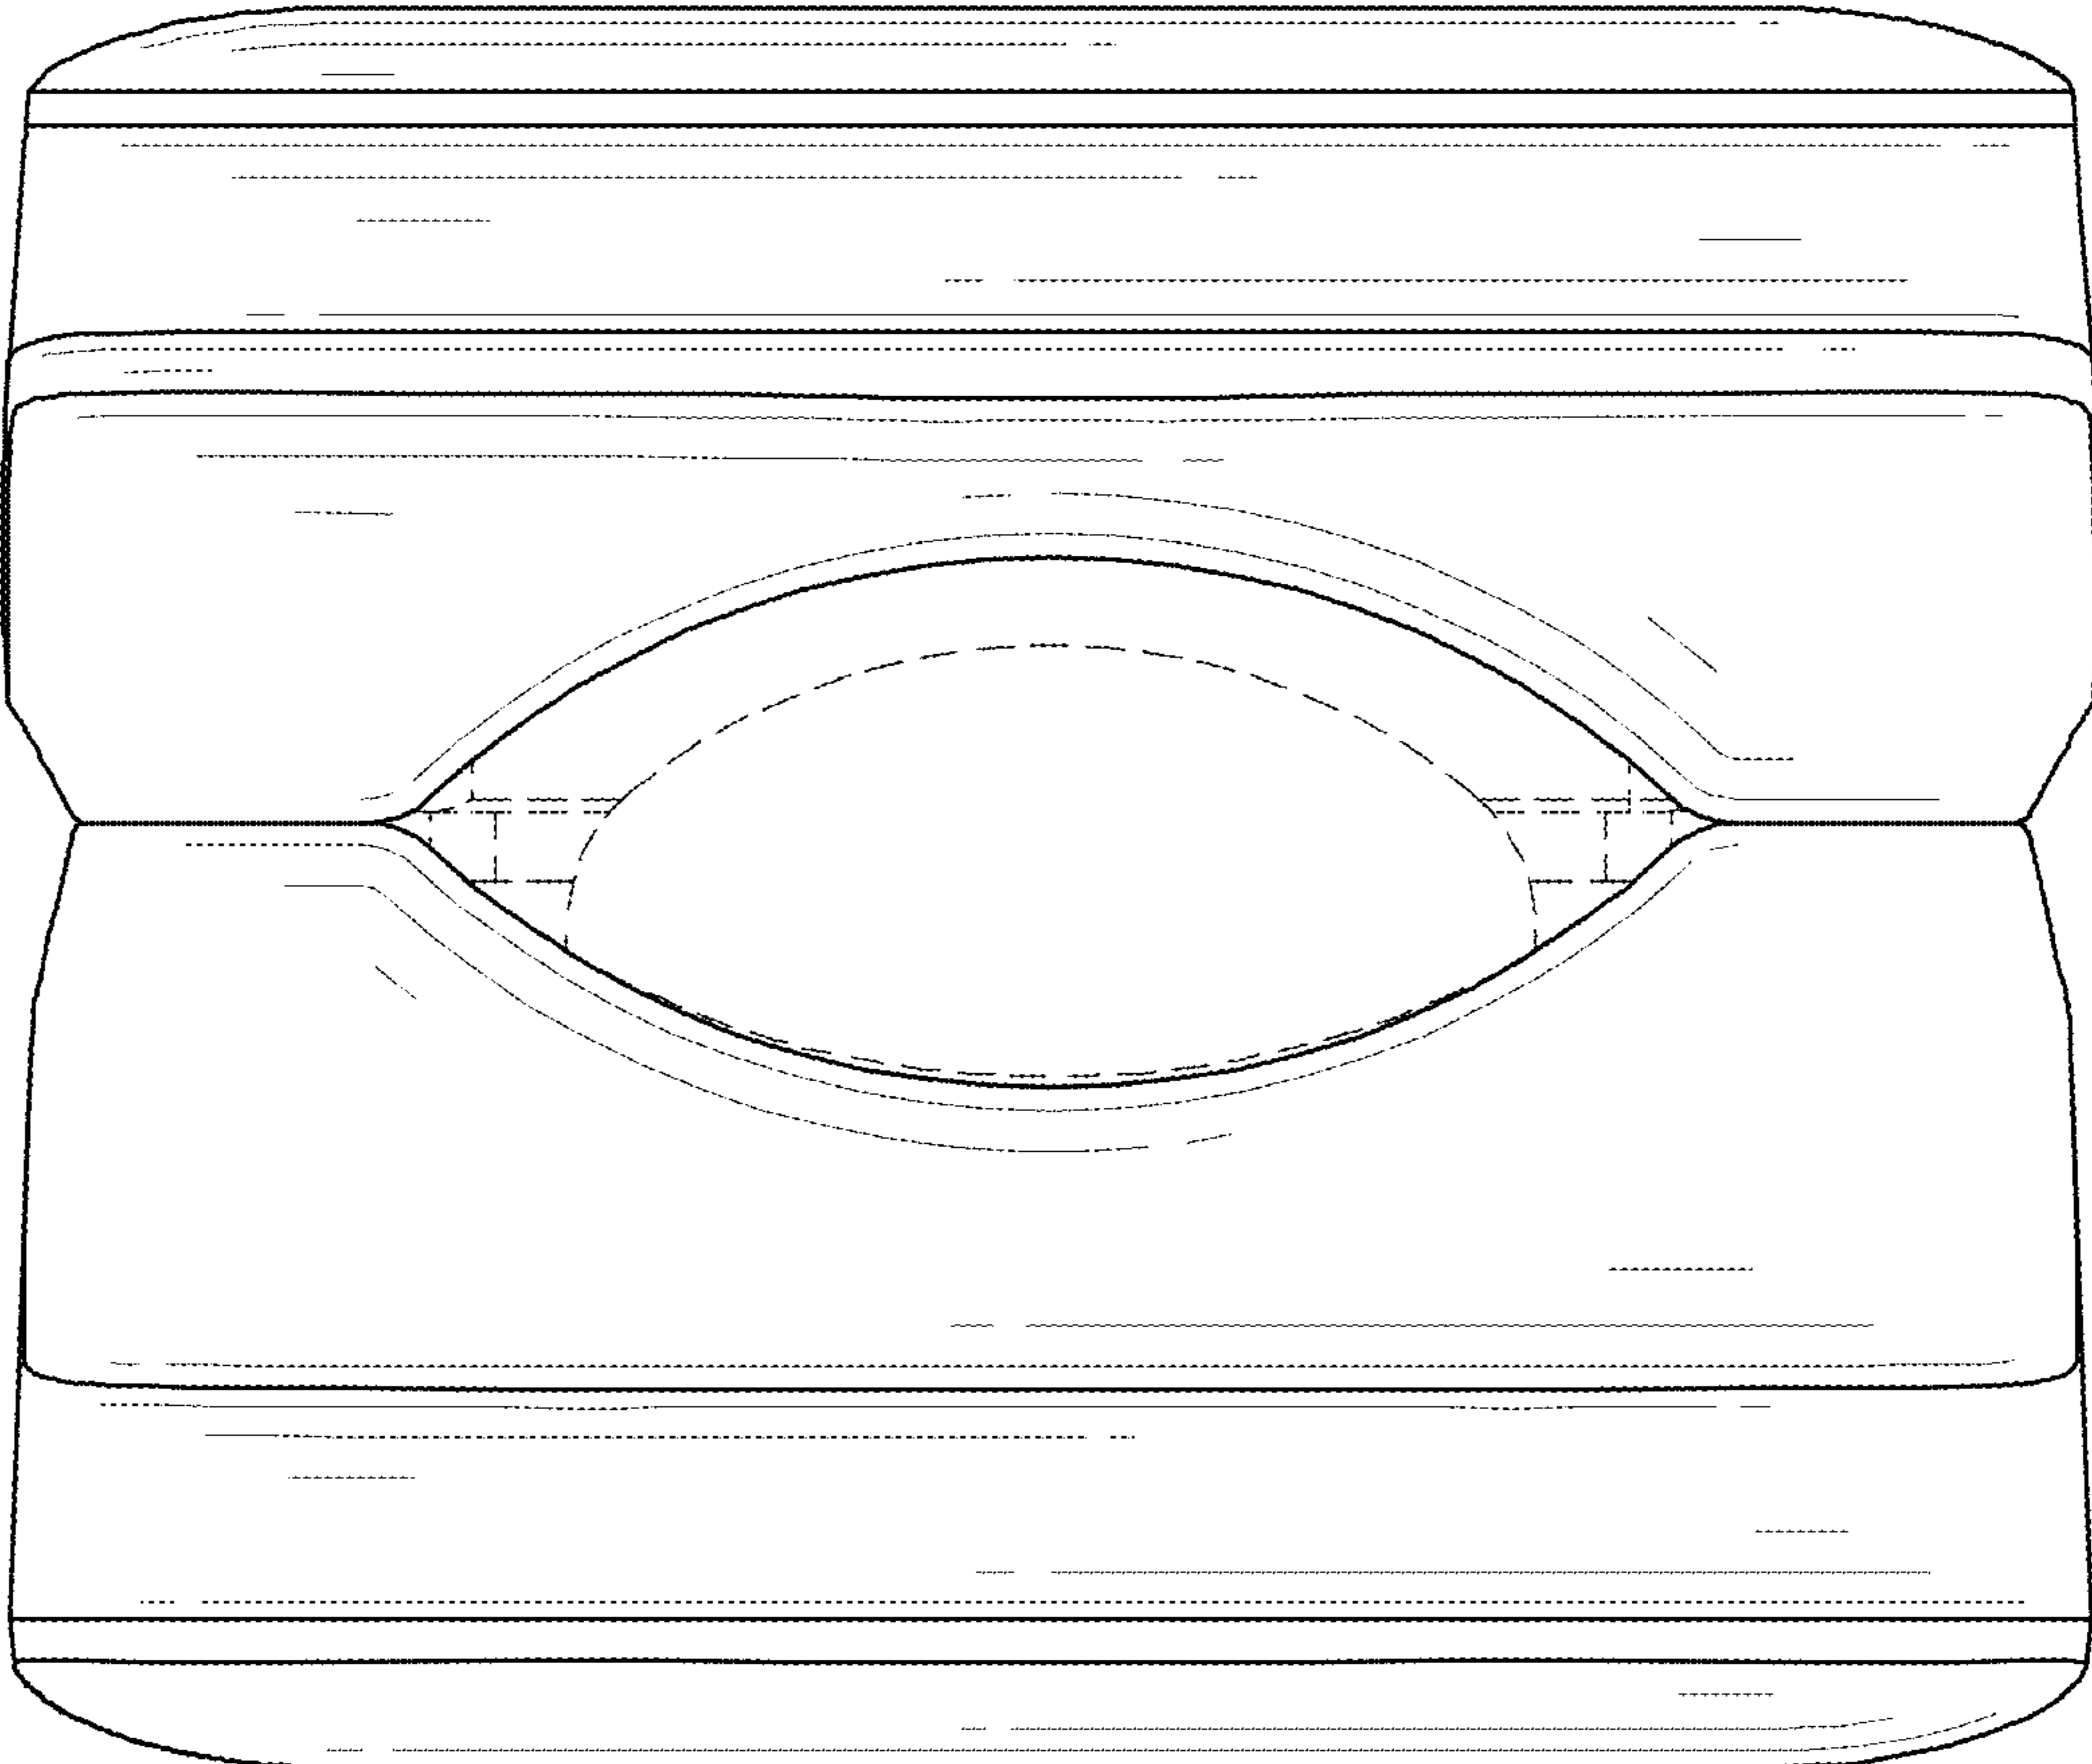


Fig. 3



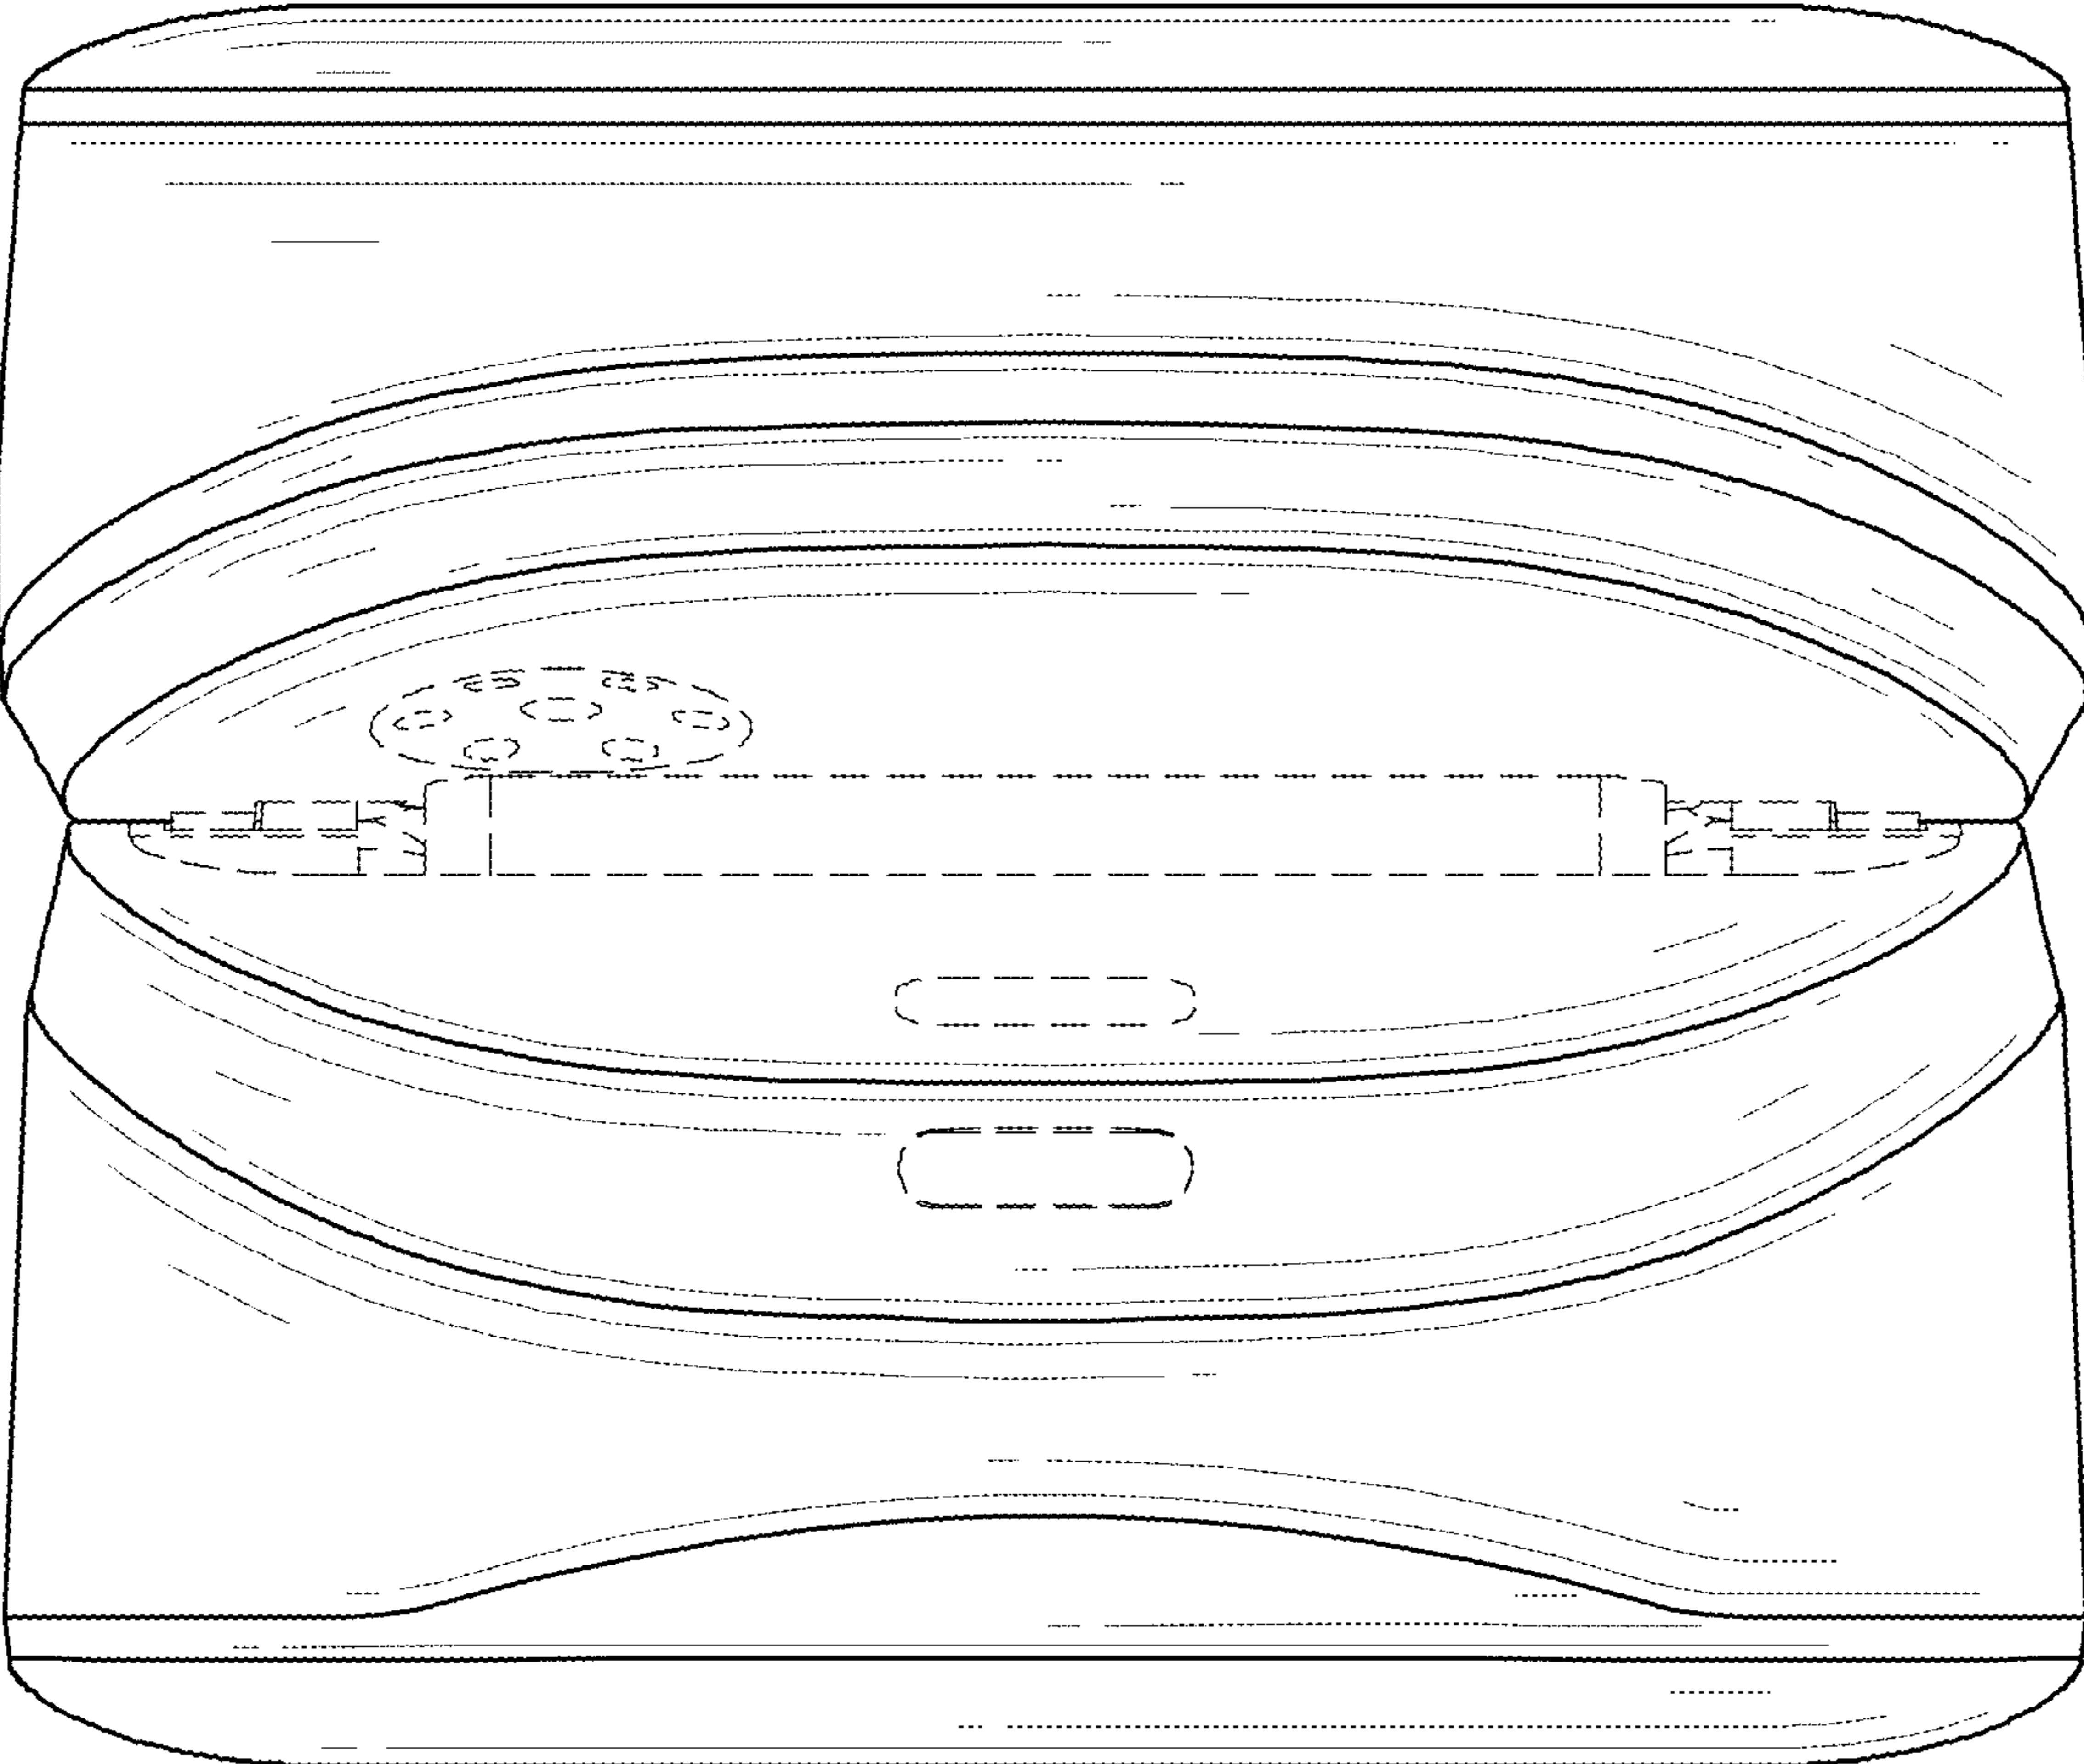


Fig. 4

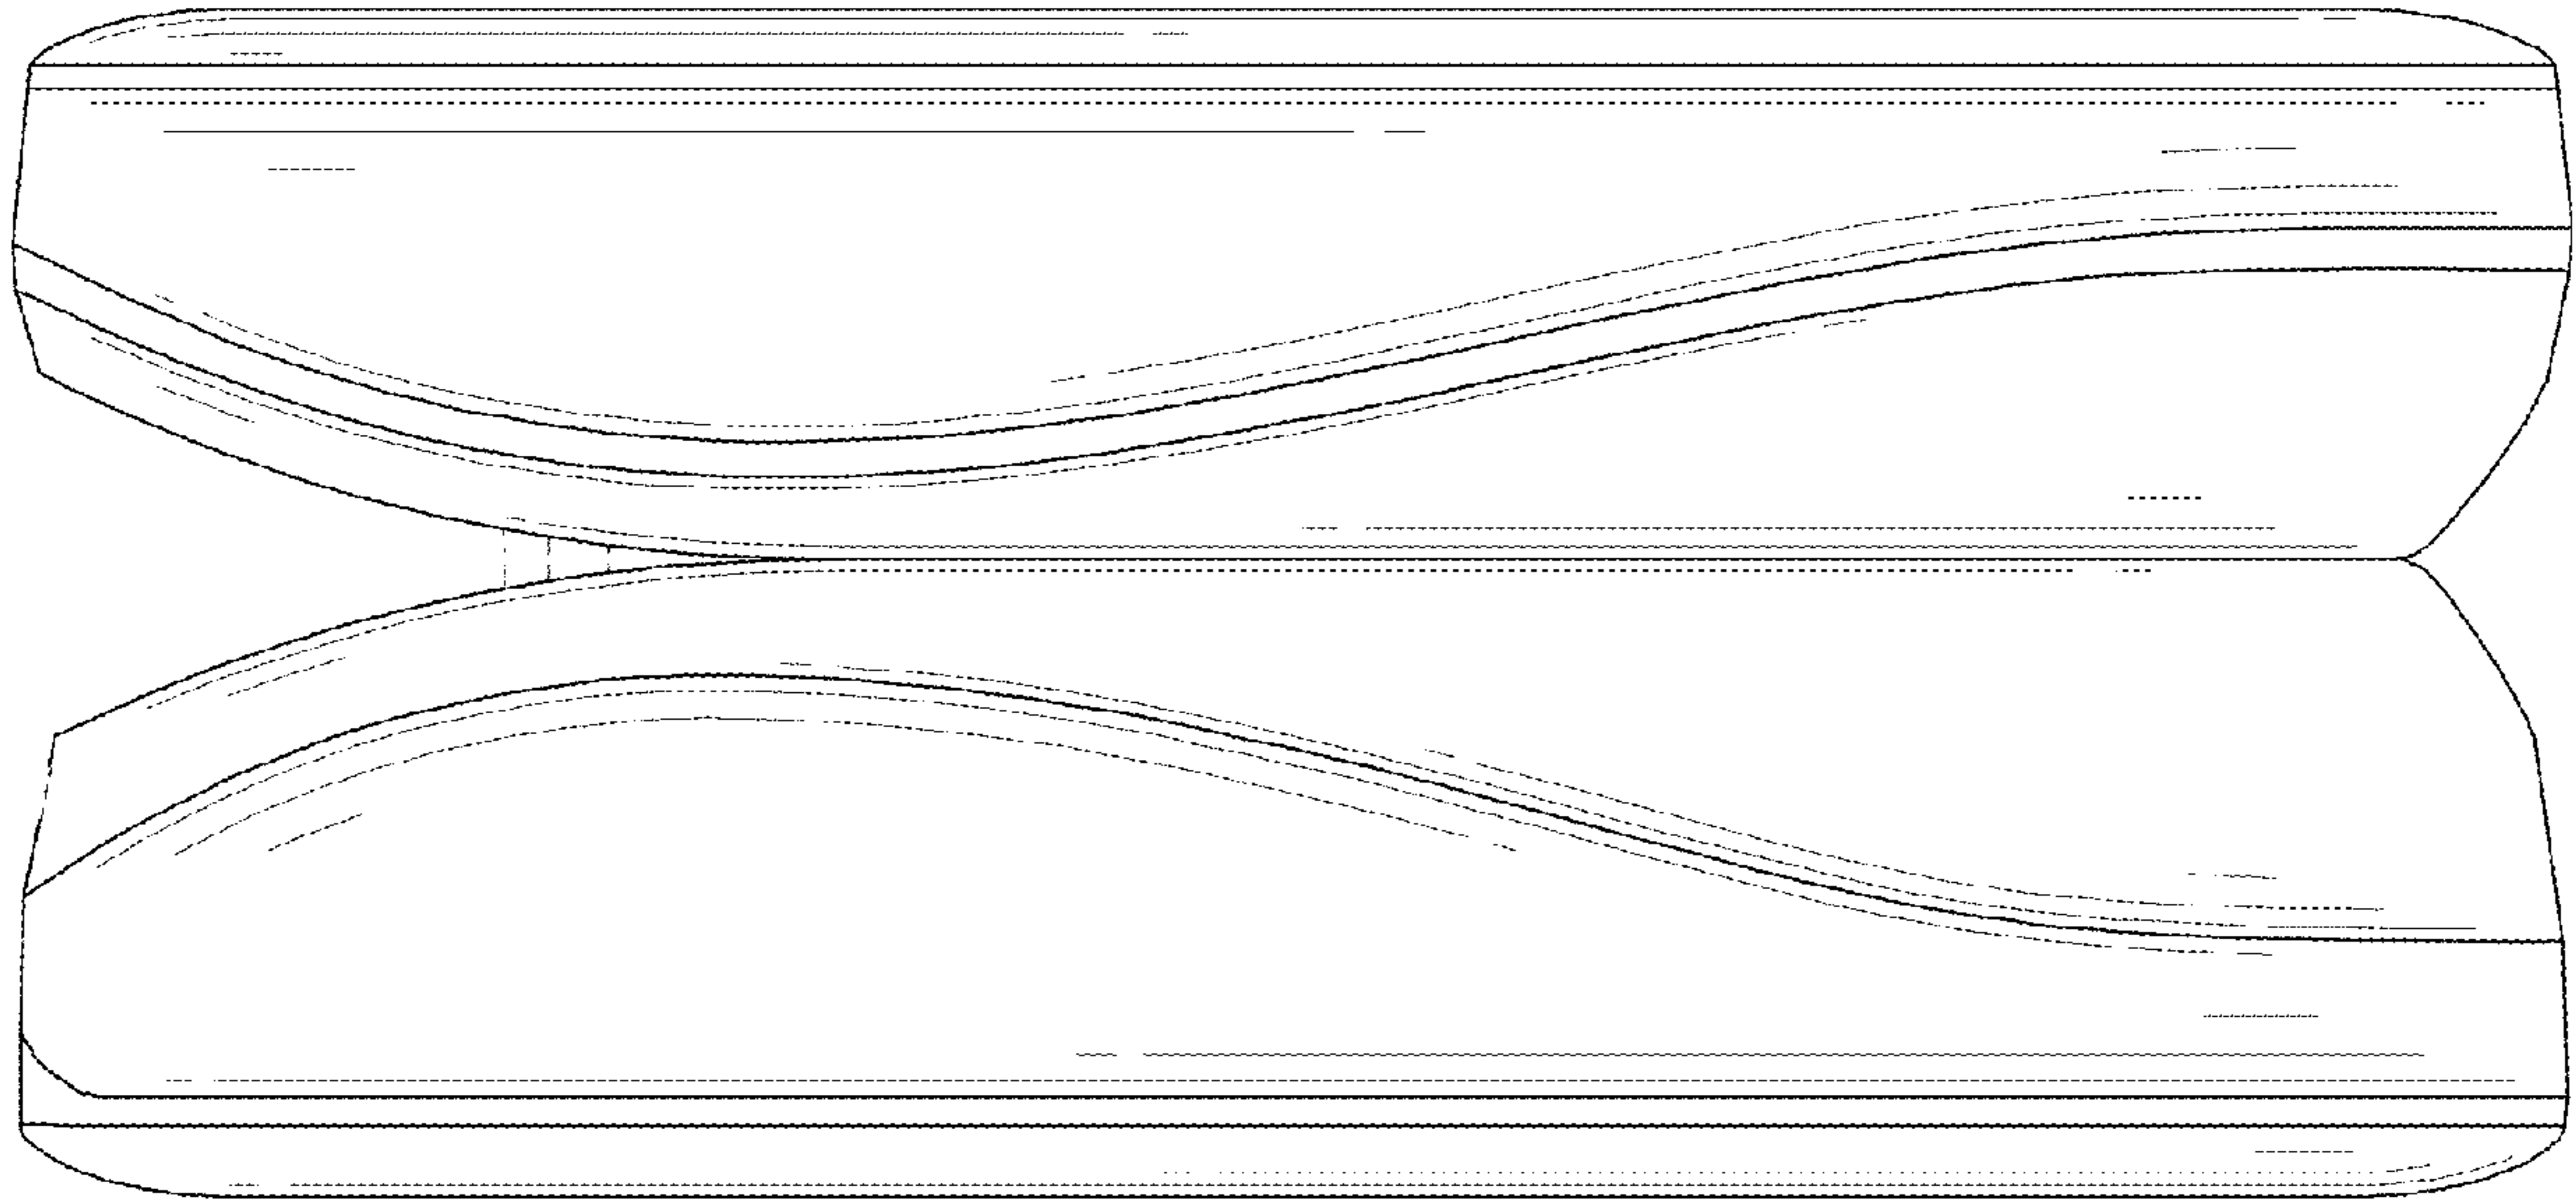

**Fig. 5**

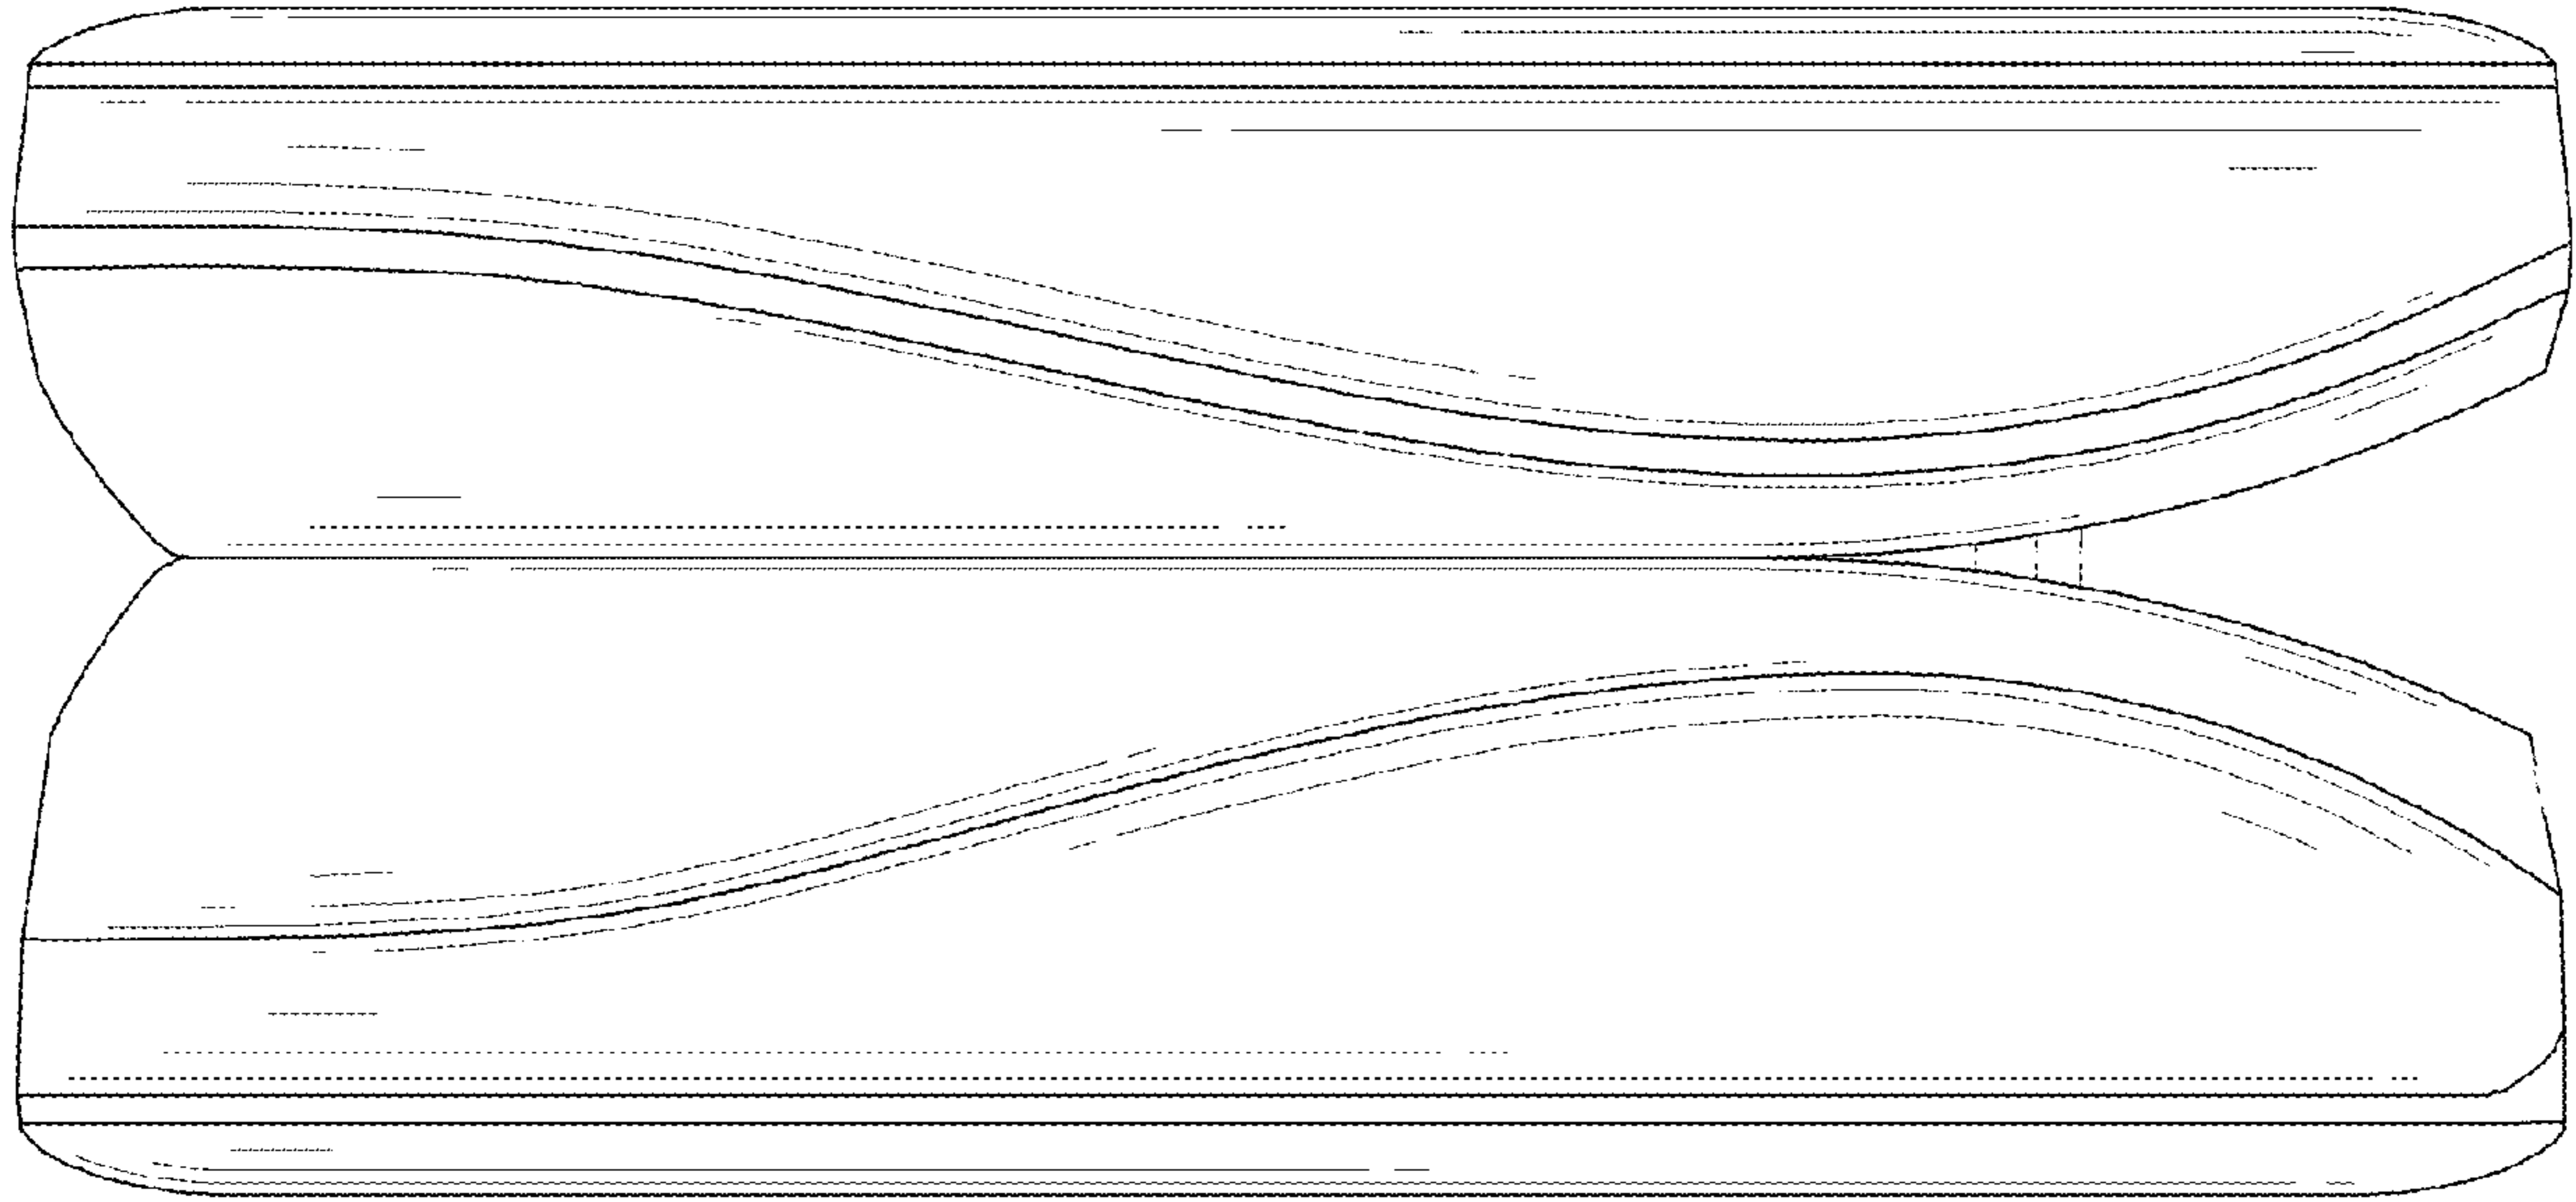

**Fig. 6**

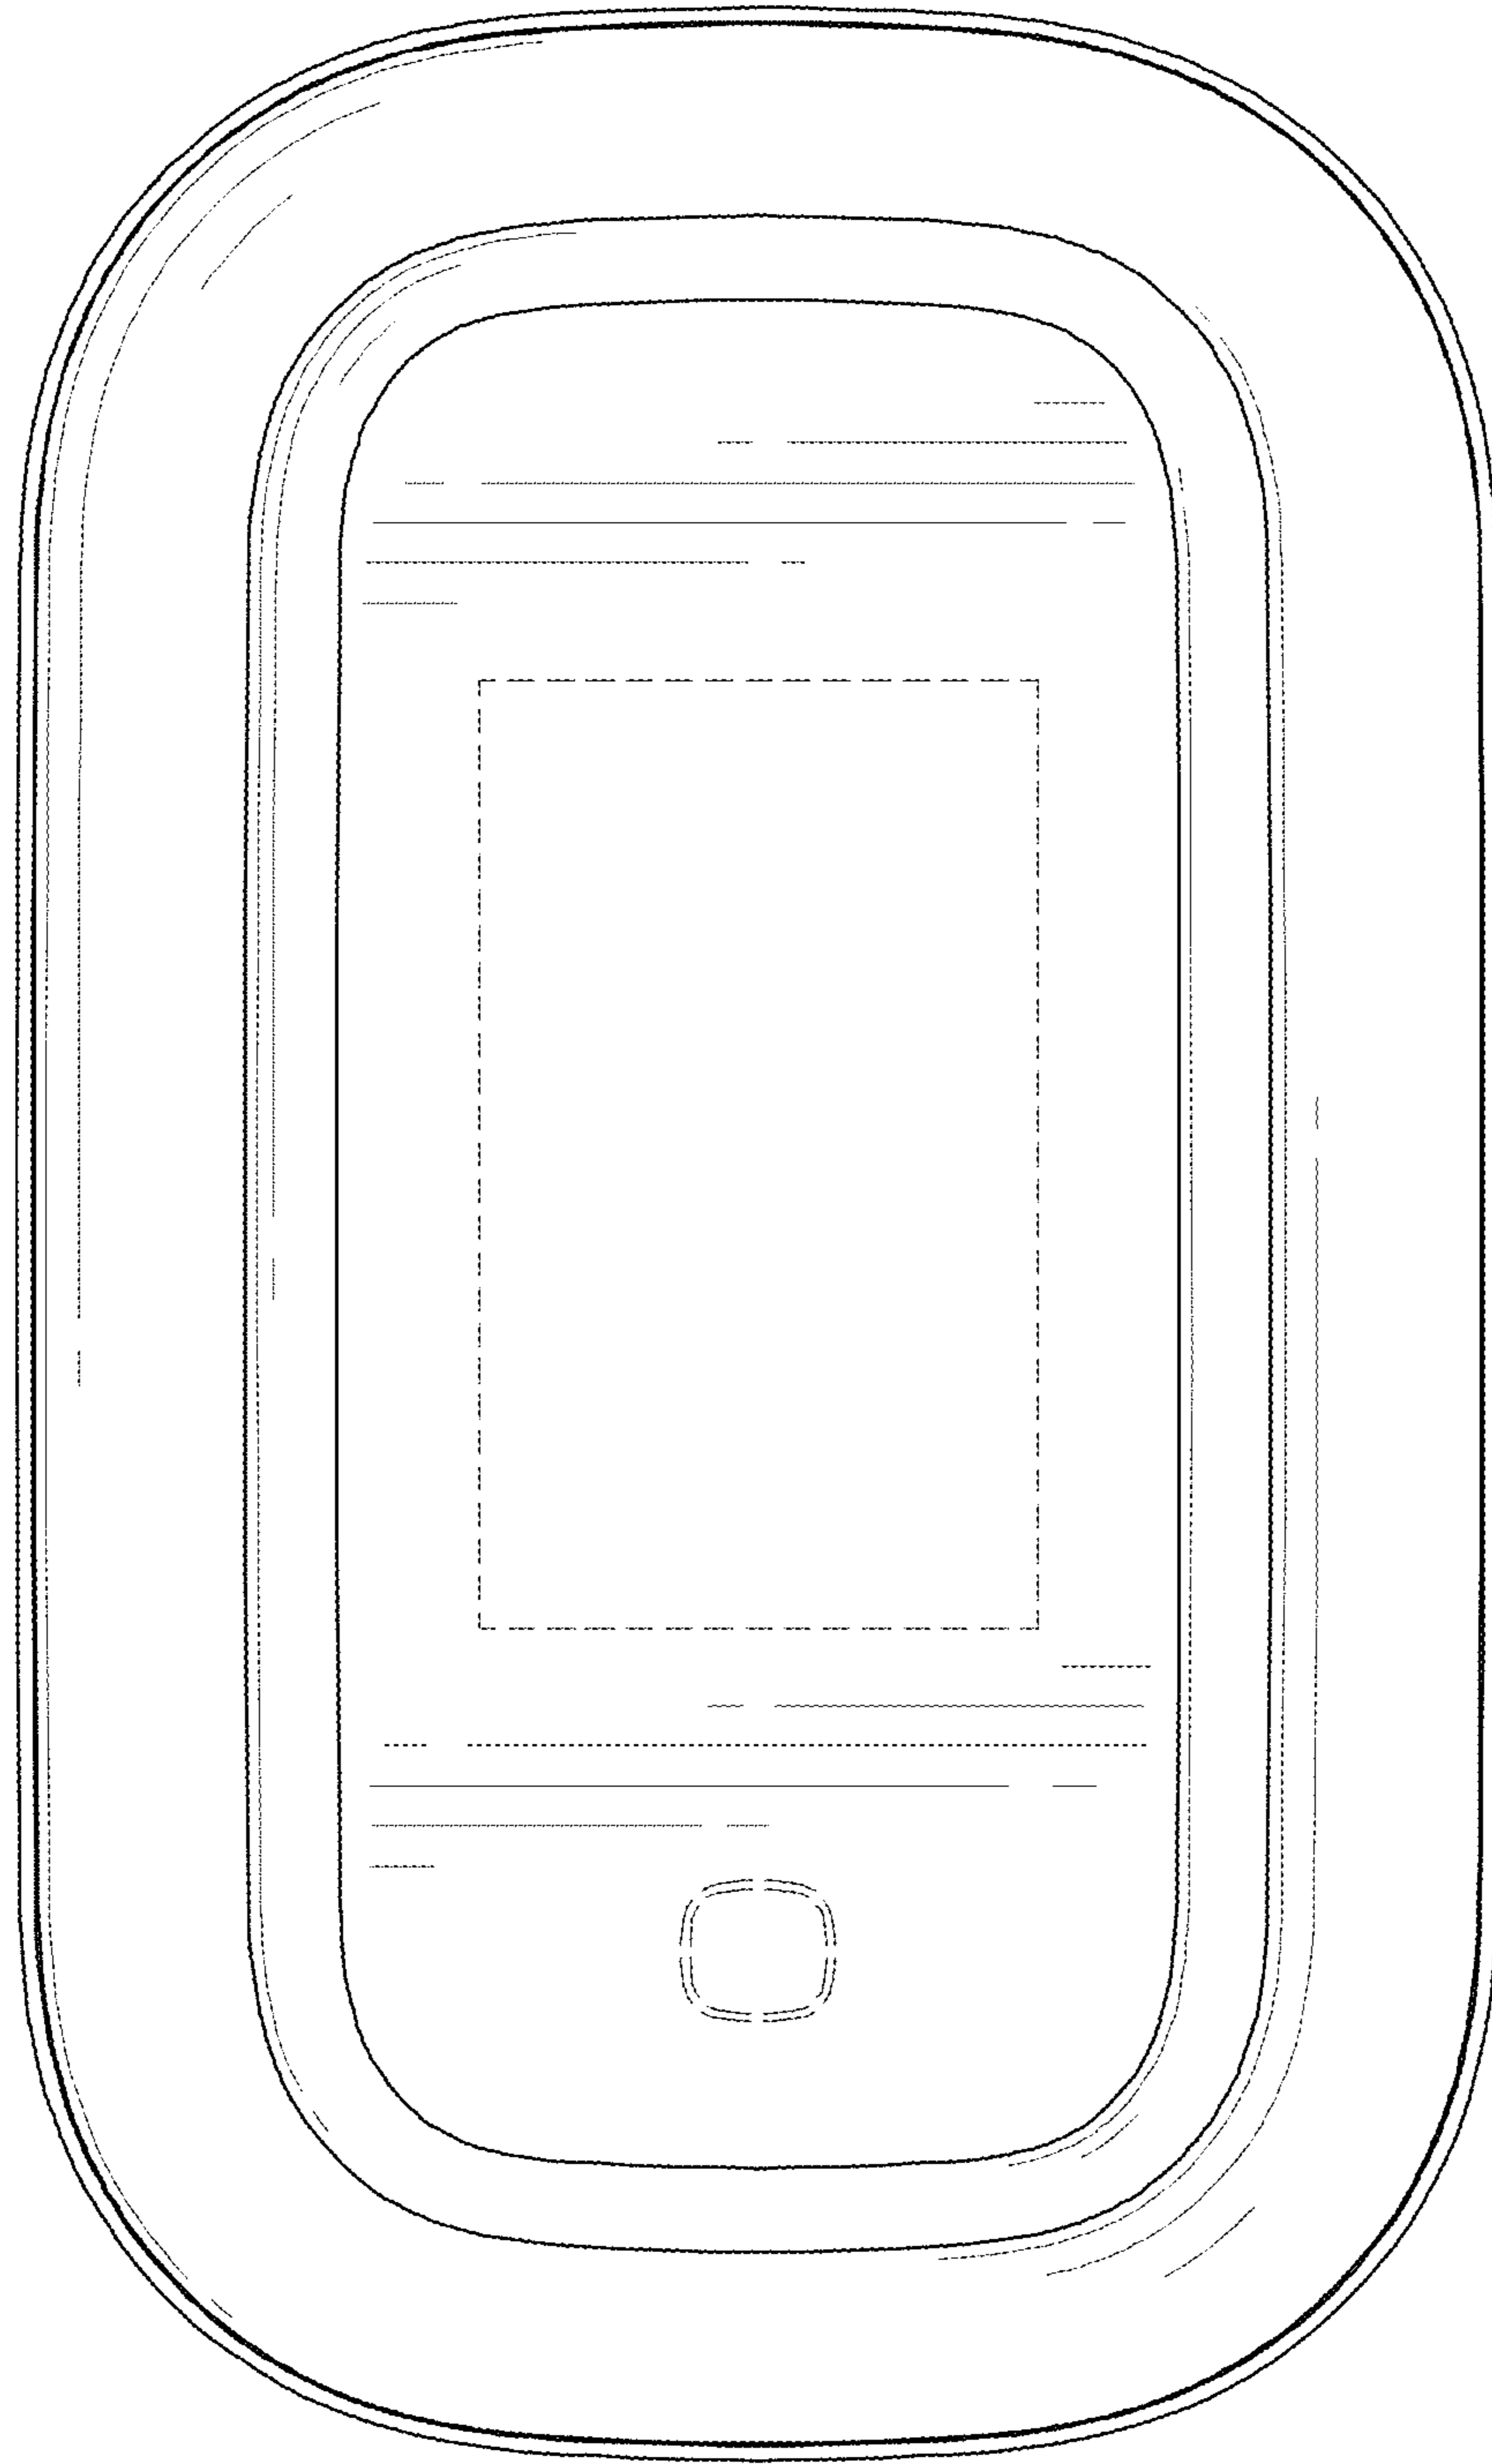


Fig. 7



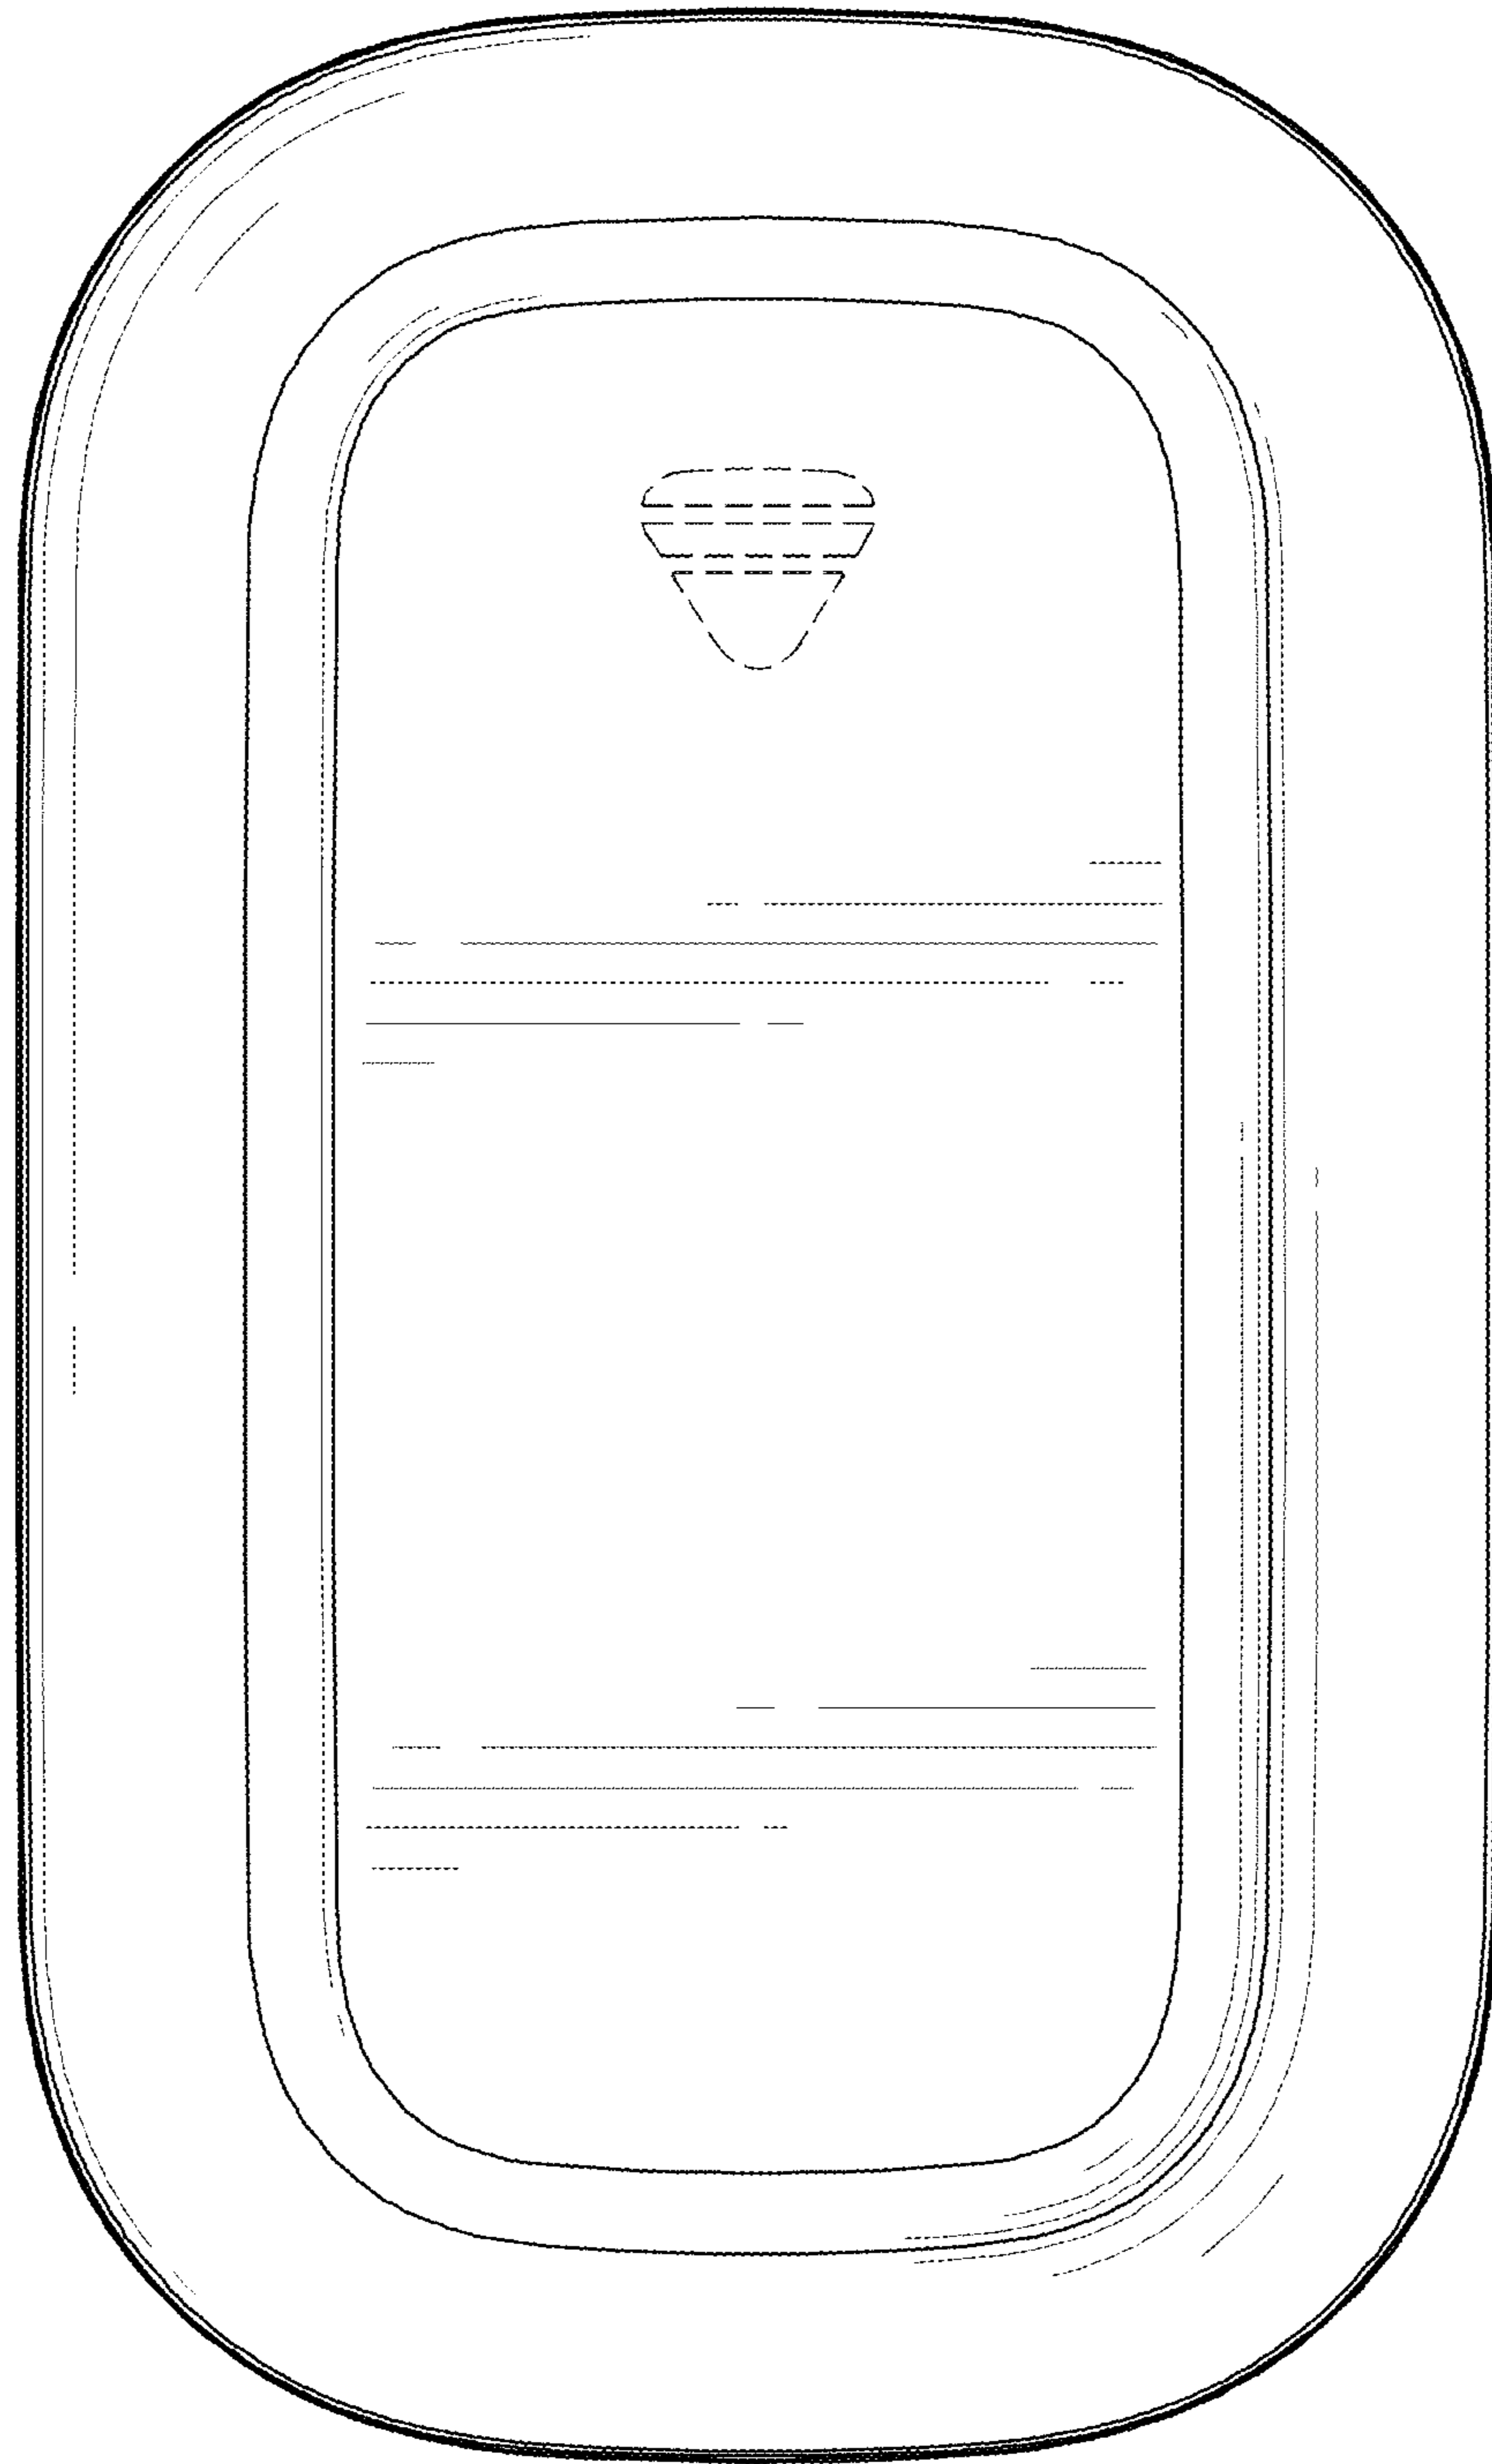


Fig. 8