



US00D893728S

(12) **United States Design Patent**
Zhao et al.

(10) **Patent No.:** **US D893,728 S**

(45) **Date of Patent:** **** Aug. 18, 2020**

(54) **PULSE OXIMETER**

(71) Applicant: **Xuzhou YongKang Electronic Science Technology Co., Ltd.**, Xuzhou, Jiangsu (CN)

(72) Inventors: **Xuecheng Zhao**, Xuzhou (CN);
Zhaohao Qiu, Xuzhou (CN);
Qingyuan Li, Xuzhou (CN)

(73) Assignee: **Xuzhou Yongkang Electronic Science Technology Co., Ltd.**, Xuzhou, Jiangsu (CN)

(**) Term: **15 Years**

(21) Appl. No.: **29/682,612**

(22) Filed: **Mar. 6, 2019**

(30) **Foreign Application Priority Data**

Dec. 11, 2018 (CN) 2018 3 0717867

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/165**; D24/169

(58) **Field of Classification Search**
USPC D24/107, 164, 165–169, 186, 187;
D10/75, 70, 98
CPC G01N 33/66; G01N 33/49; G01N 33/493;
A61B 5/0205; A61B 5/02427; A61B
5/02438; A61B 5/14552; A61B 5/6626;
A61B 5/6638
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,792,052 A * 8/1998 Isaacson A61B 5/02427
600/323
D646,391 S * 10/2011 Ibuki D24/165

D691,726 S * 10/2013 Jin D24/167
D718,455 S * 11/2014 Maser D24/169
D830,557 S * 10/2018 Sebban D24/167
D877,339 S * 3/2020 Xian D24/165
2010/0317944 A1* 12/2010 Wang A61B 5/14552
600/323
2019/0090795 A1* 3/2019 Boller A61B 5/14552

OTHER PUBLICATIONS

U.S. Appl. No. 29/682,609, Zhao et al., filed Mar. 6, 2019.

* cited by examiner

Primary Examiner — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Leydig, Voit & Mayer, Ltd.

(57) **CLAIM**

The ornamental design for a pulse oximeter, as shown and described.

DESCRIPTION

FIG. 1 is a top, right, front perspective view of a pulse oximeter showing the new design;
FIG. 2 is a bottom, back, left perspective view thereof;
FIG. 3 is a front view thereof;
FIG. 4 is a back view thereof;
FIG. 5 is a side view thereof;
FIG. 6 is another side view thereof;
FIG. 7 is a top view thereof; and,
FIG. 8 is a bottom view thereof.

The broken lines illustrate portions of the pulse oximeter that form no part of the claimed design. The broken lines form no part of the claimed design.

1 Claim, 8 Drawing Sheets



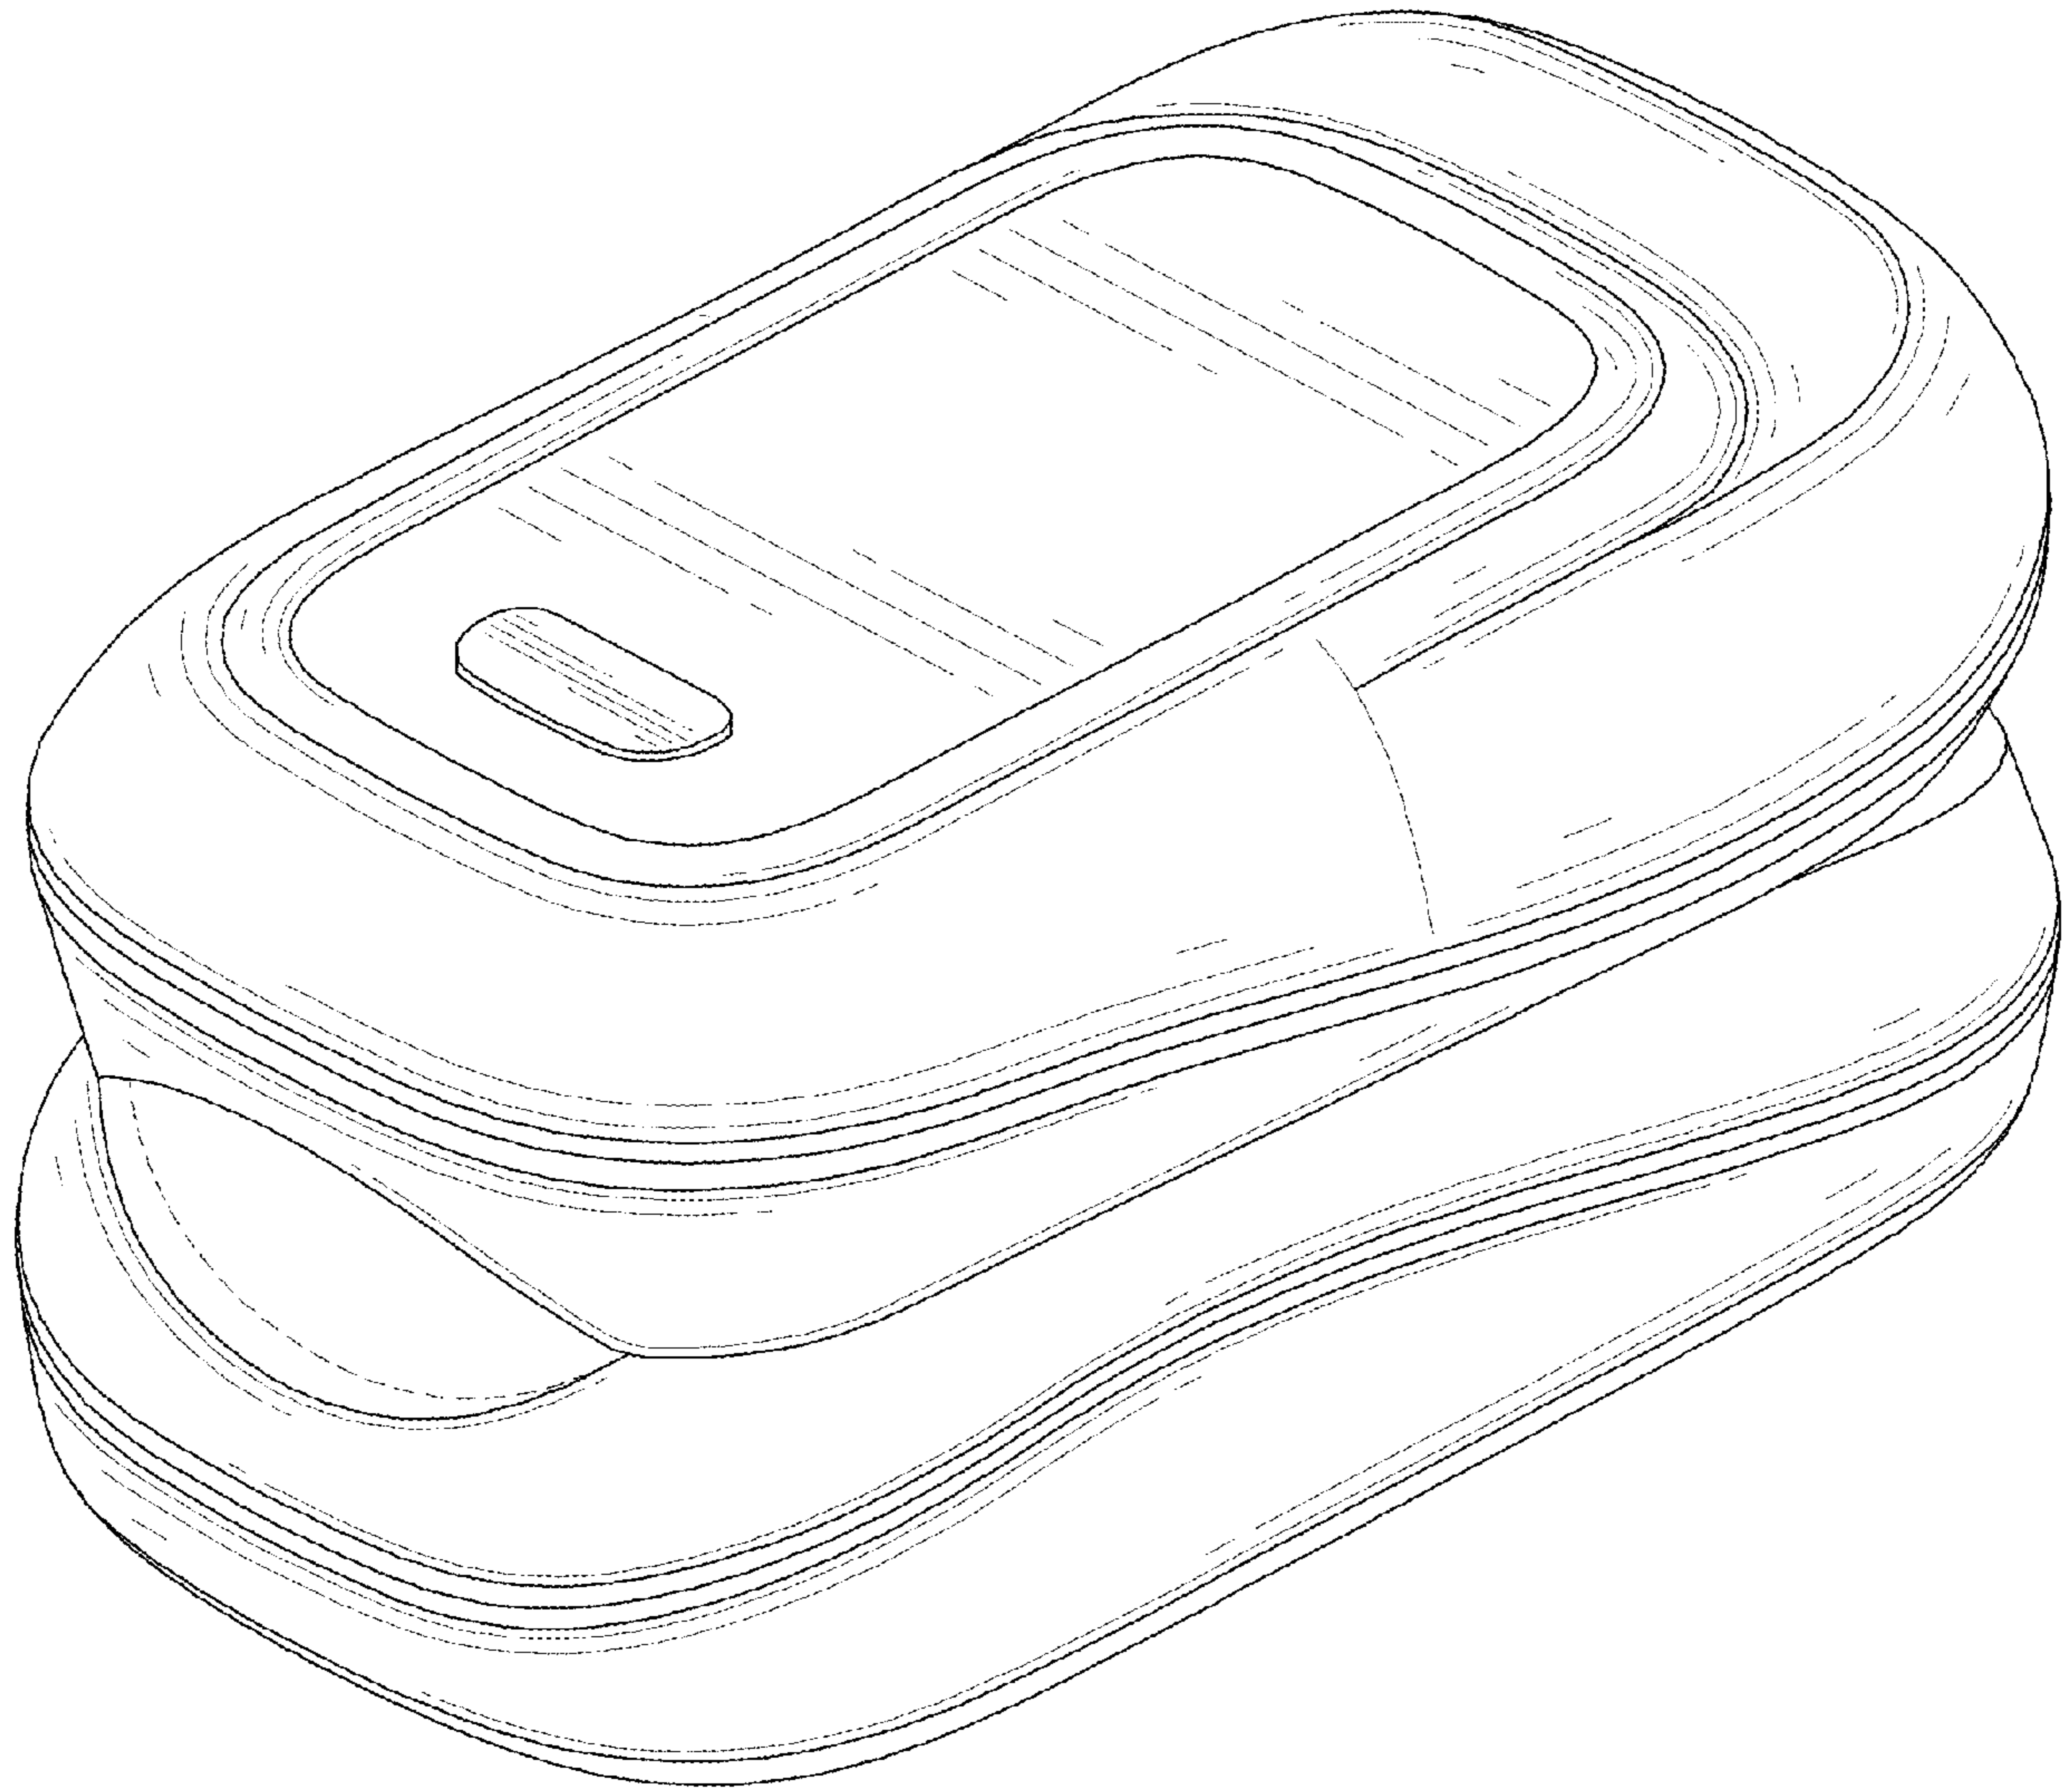


Fig. 1



Fig. 2

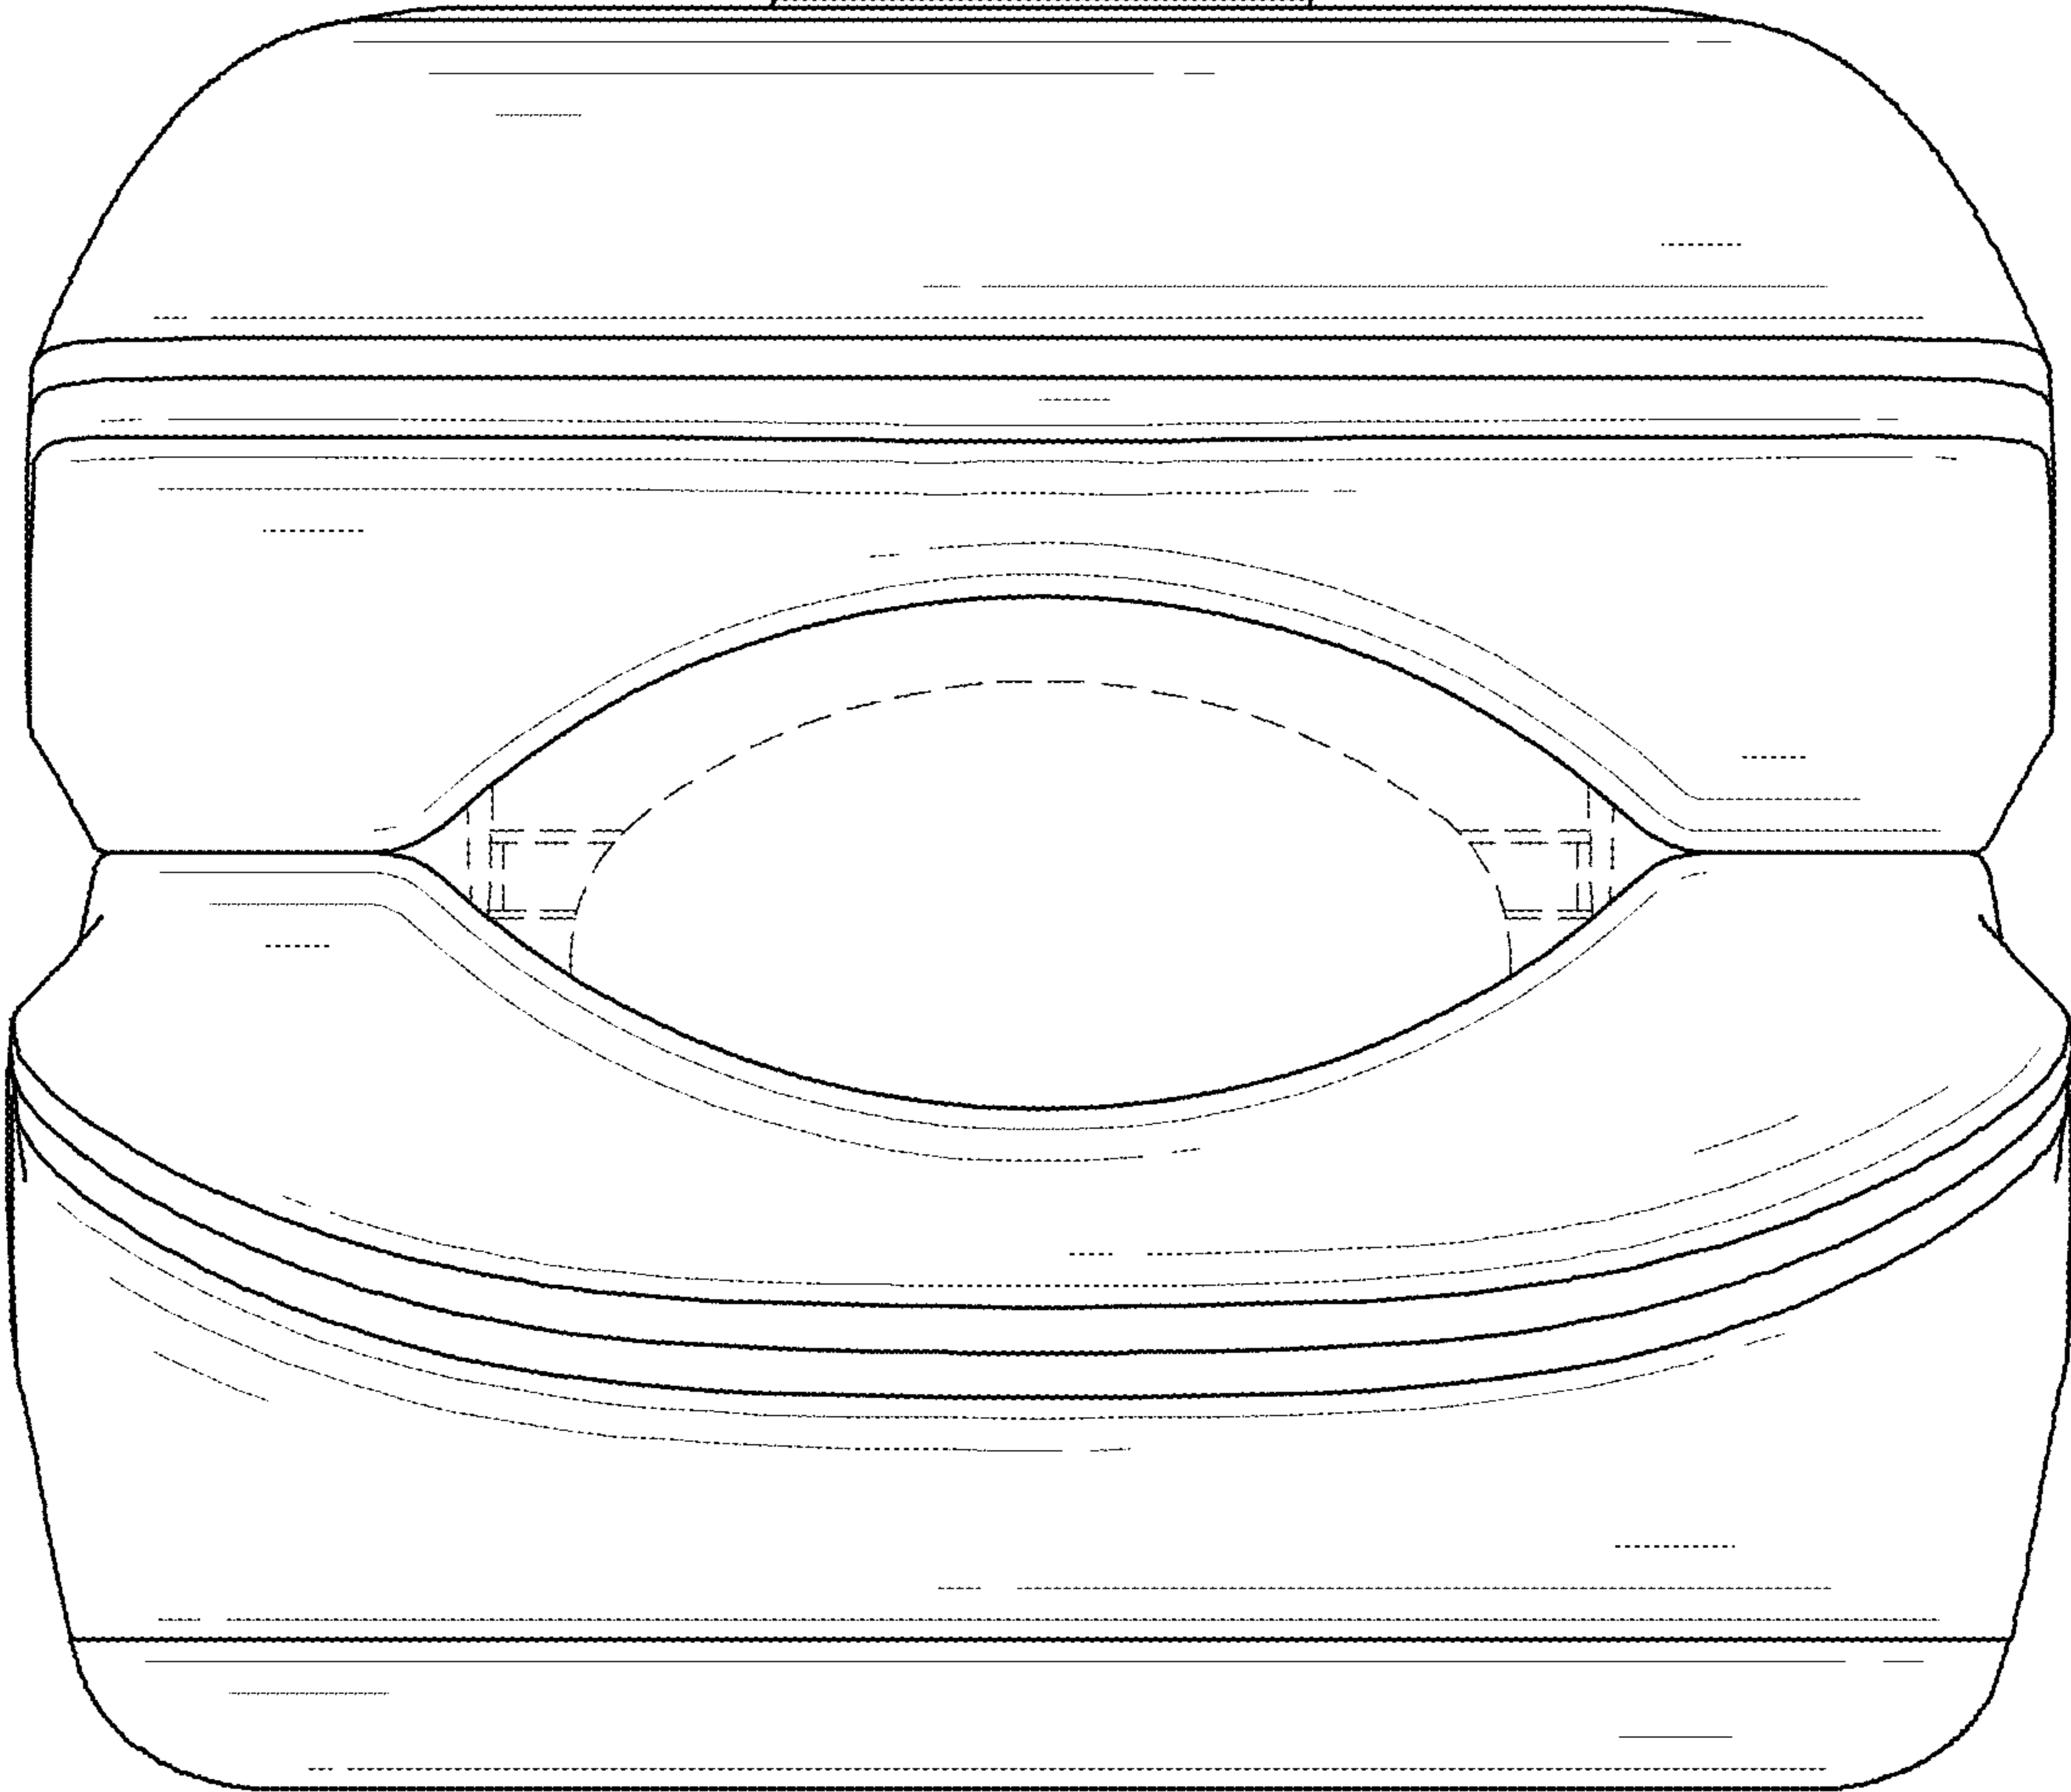


Fig. 3

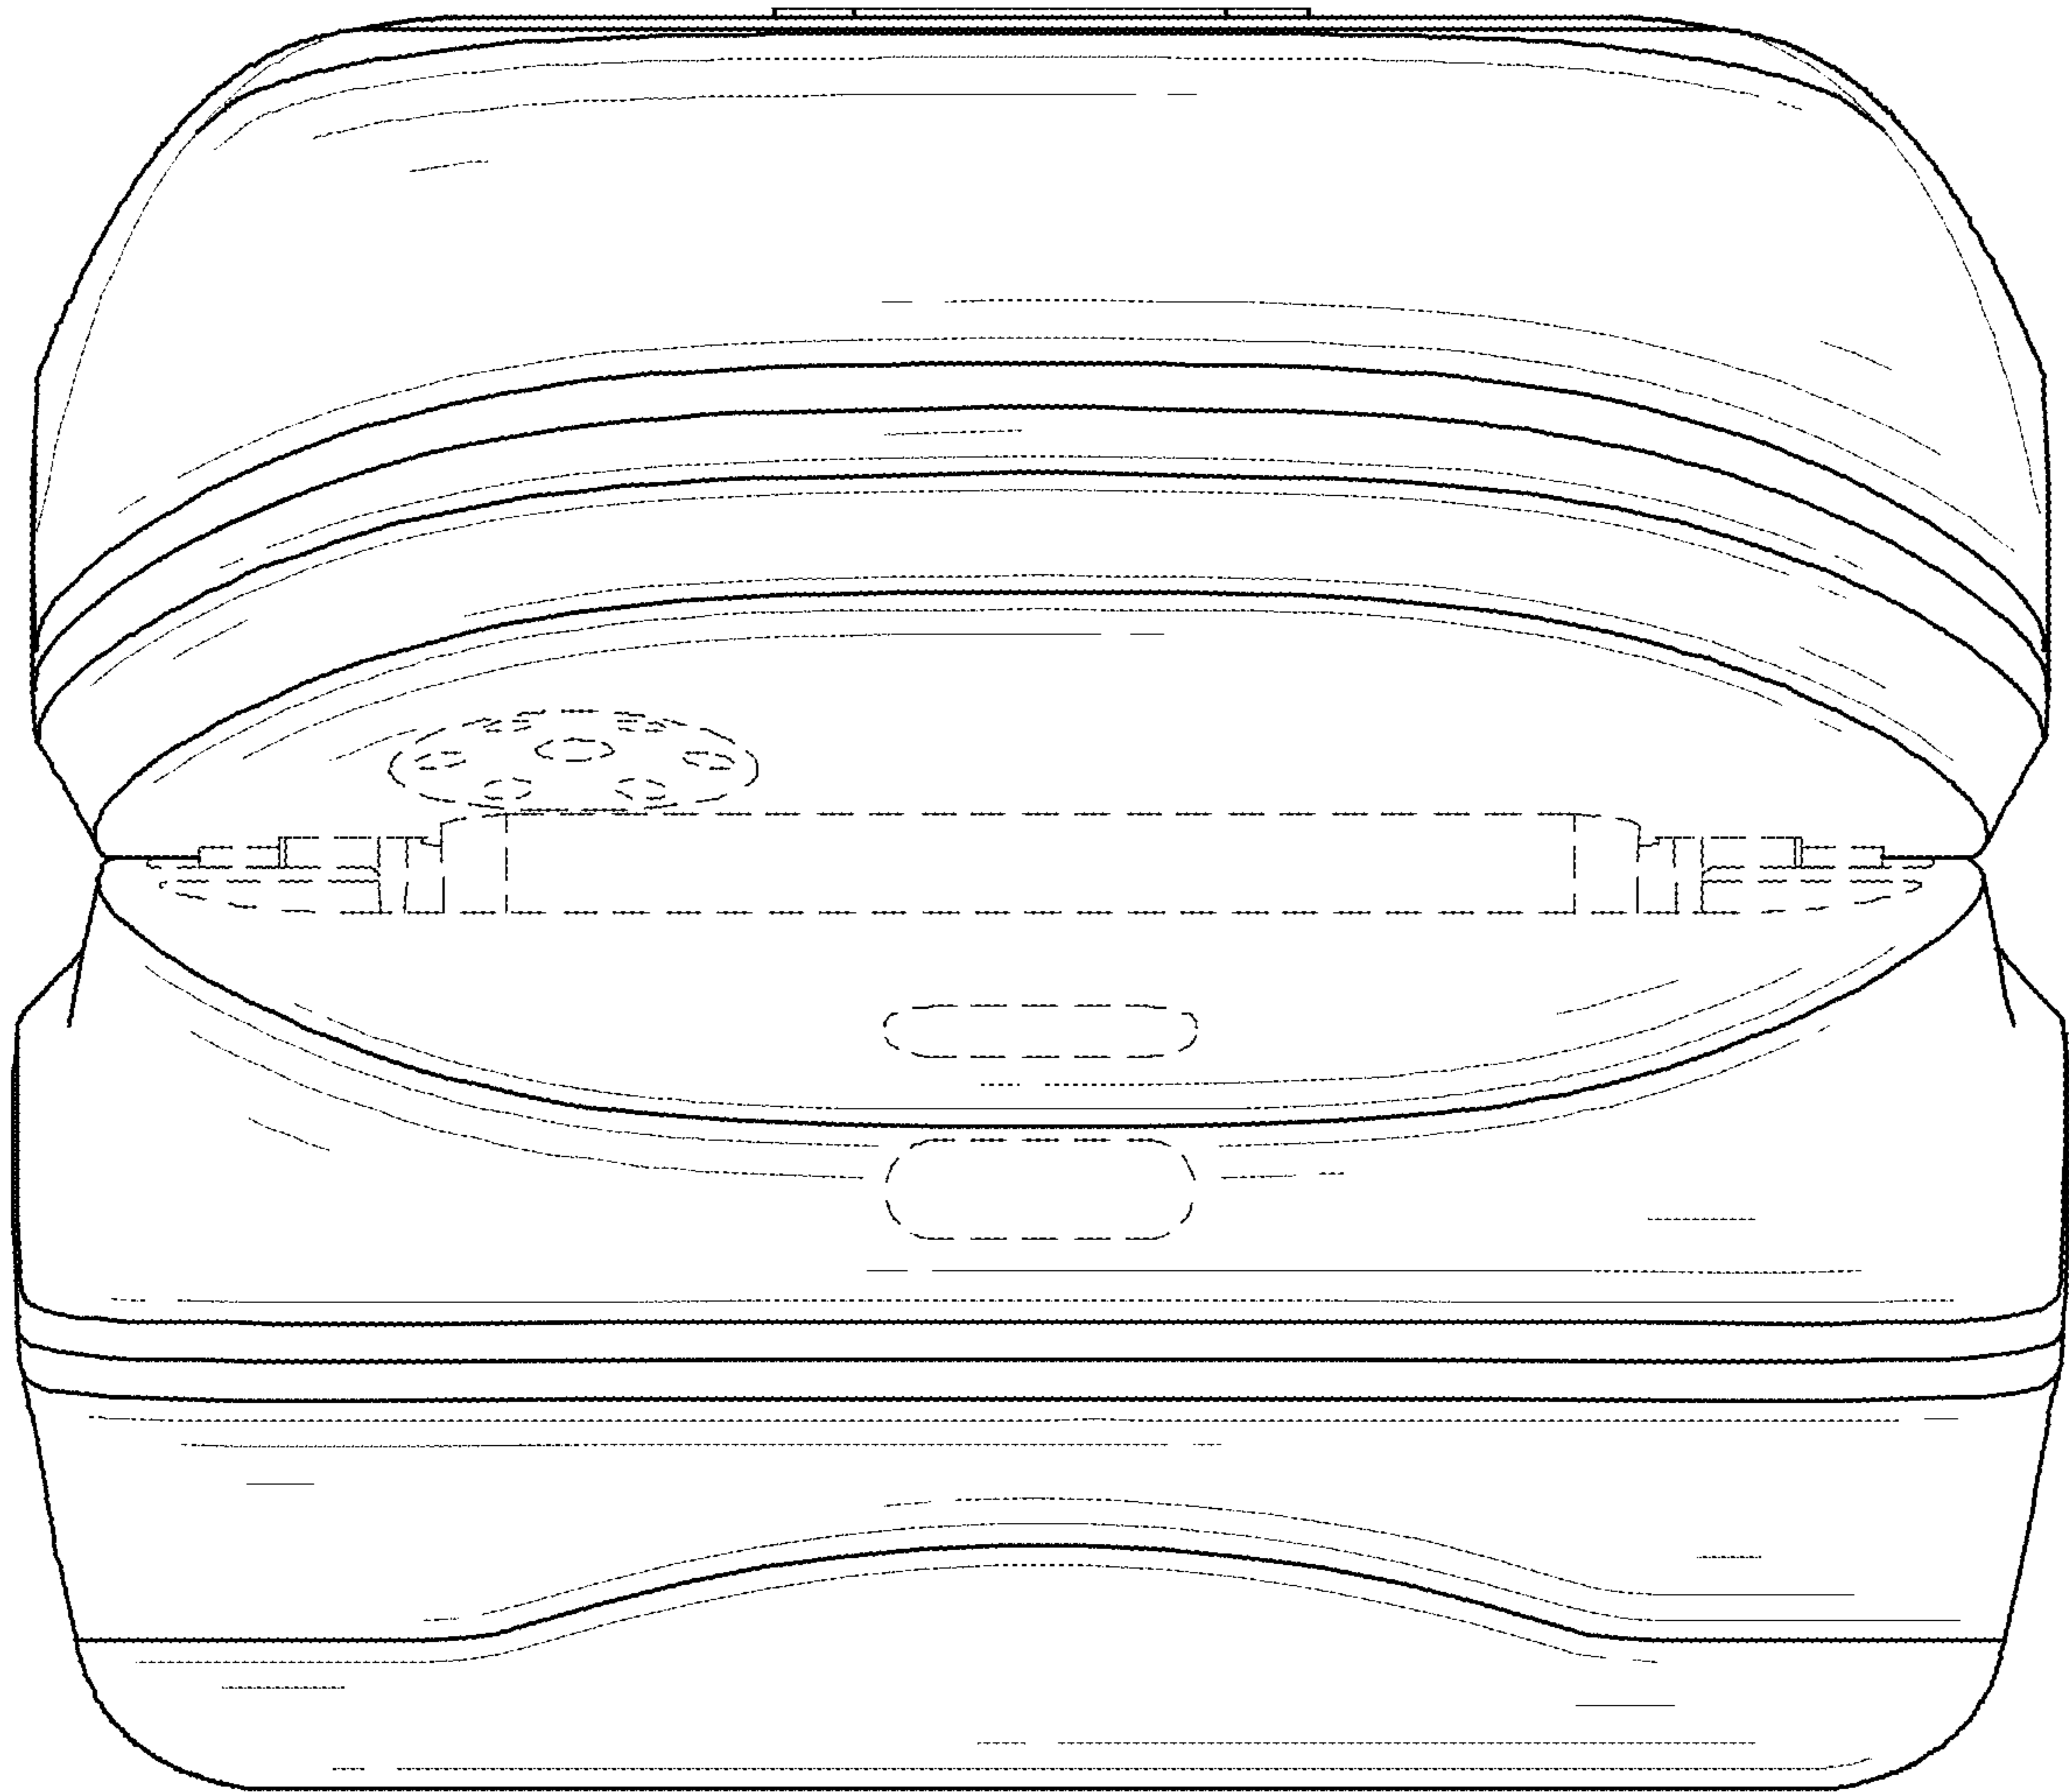


Fig. 4

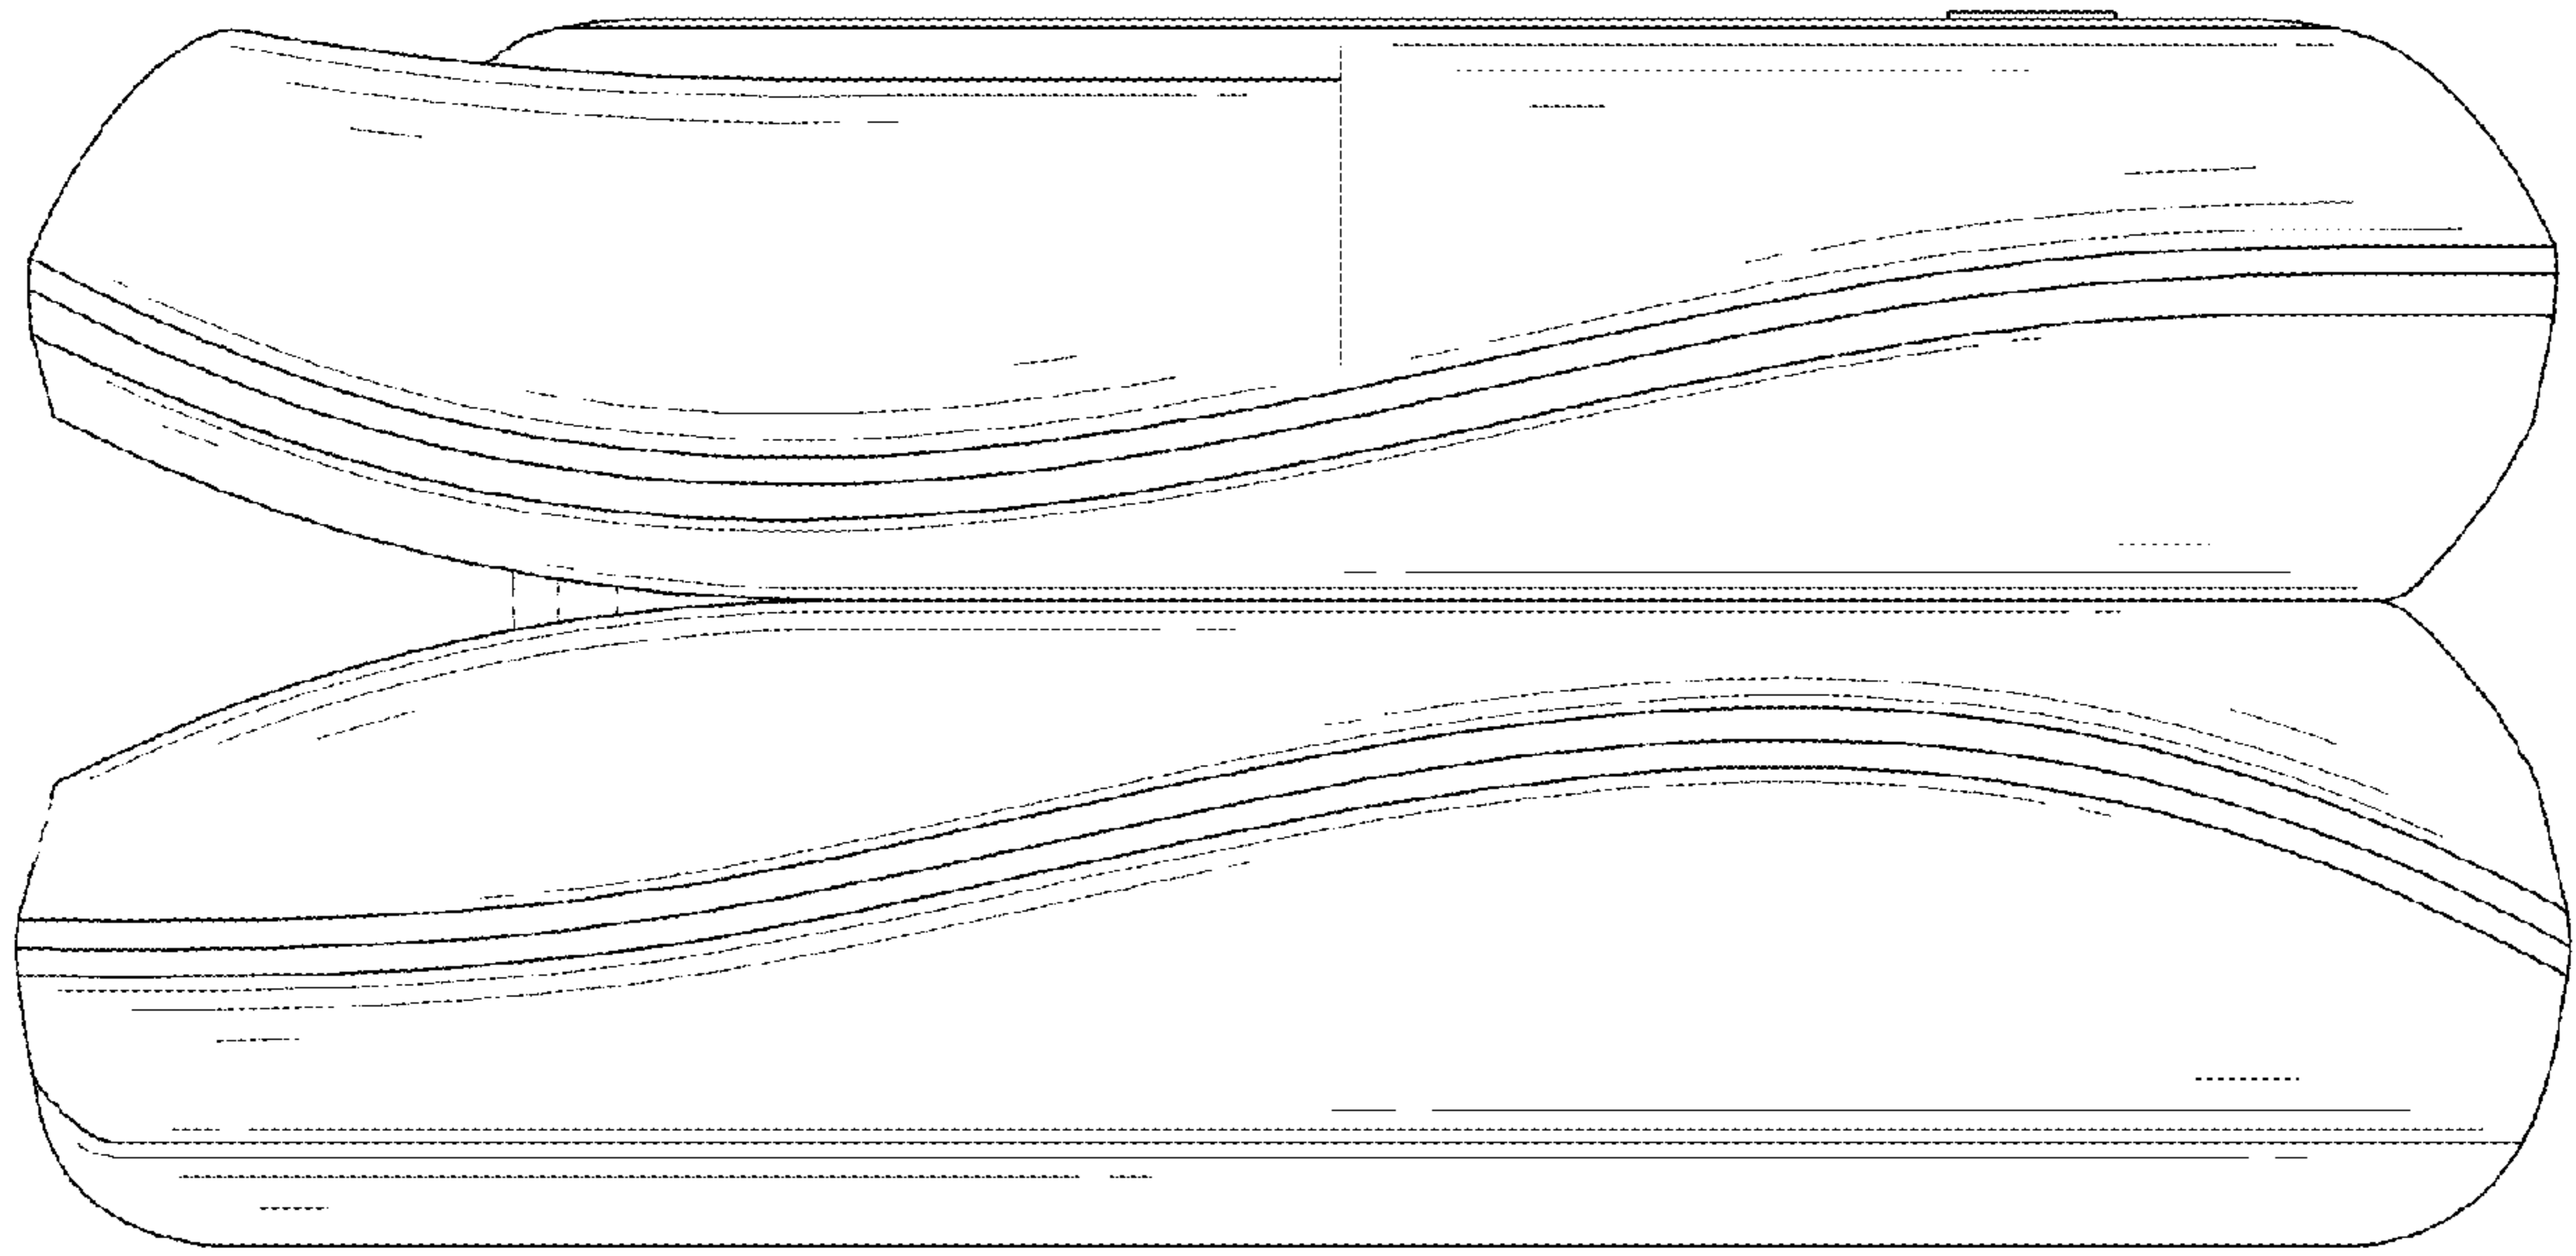


Fig. 5

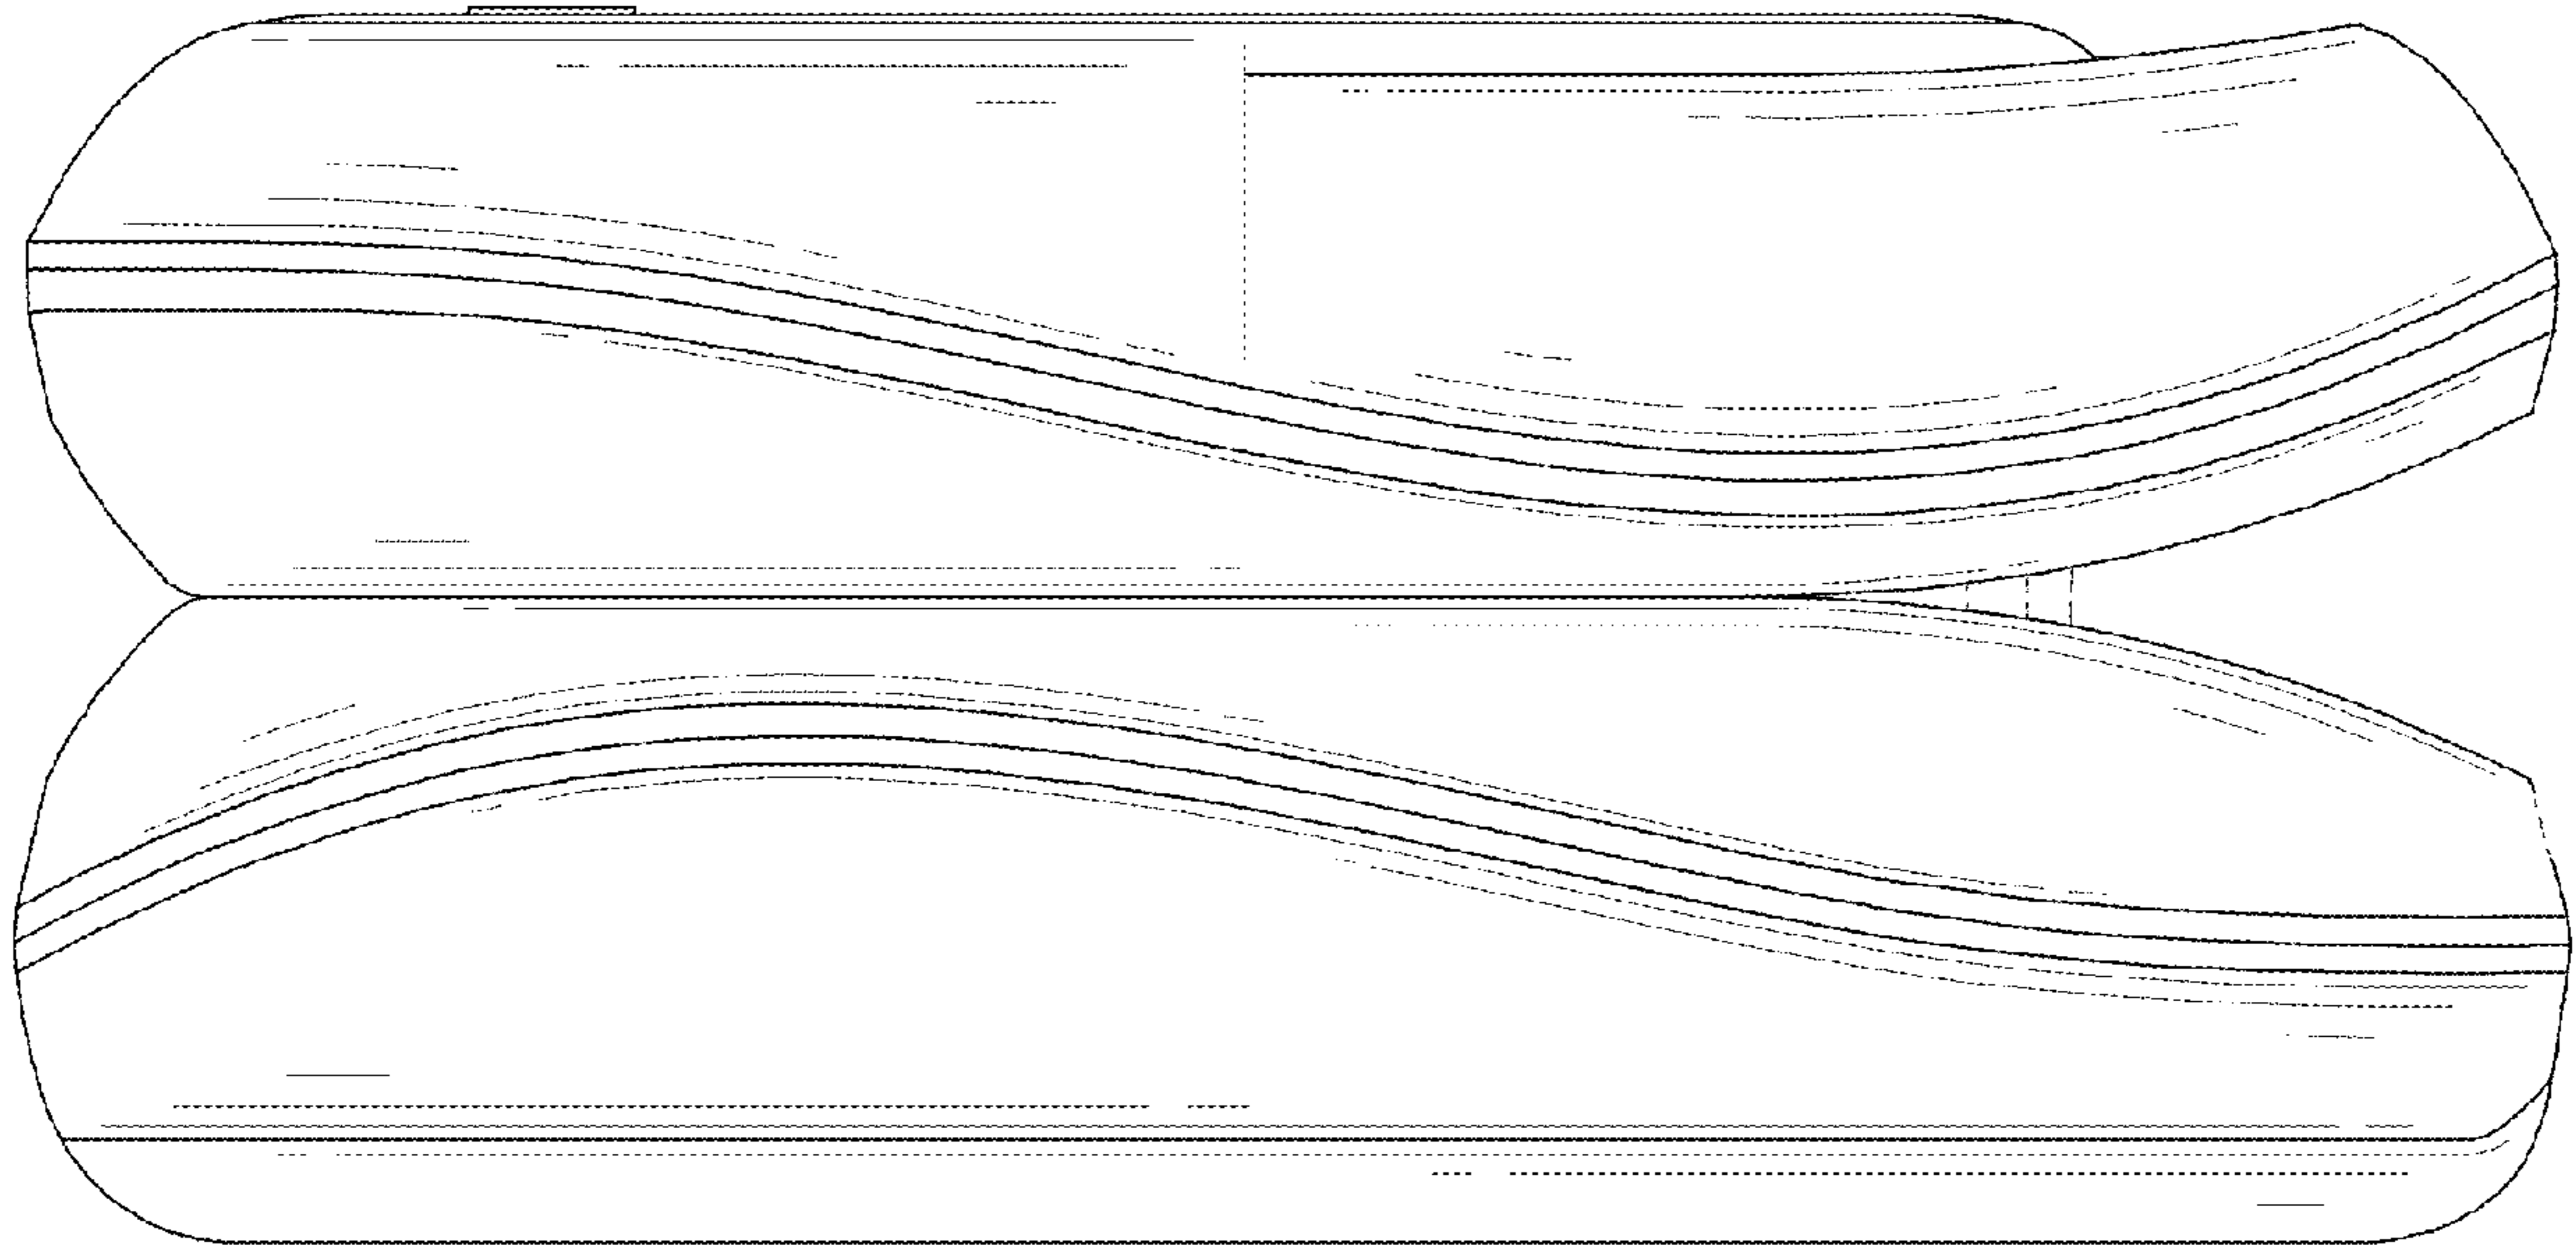


Fig. 6

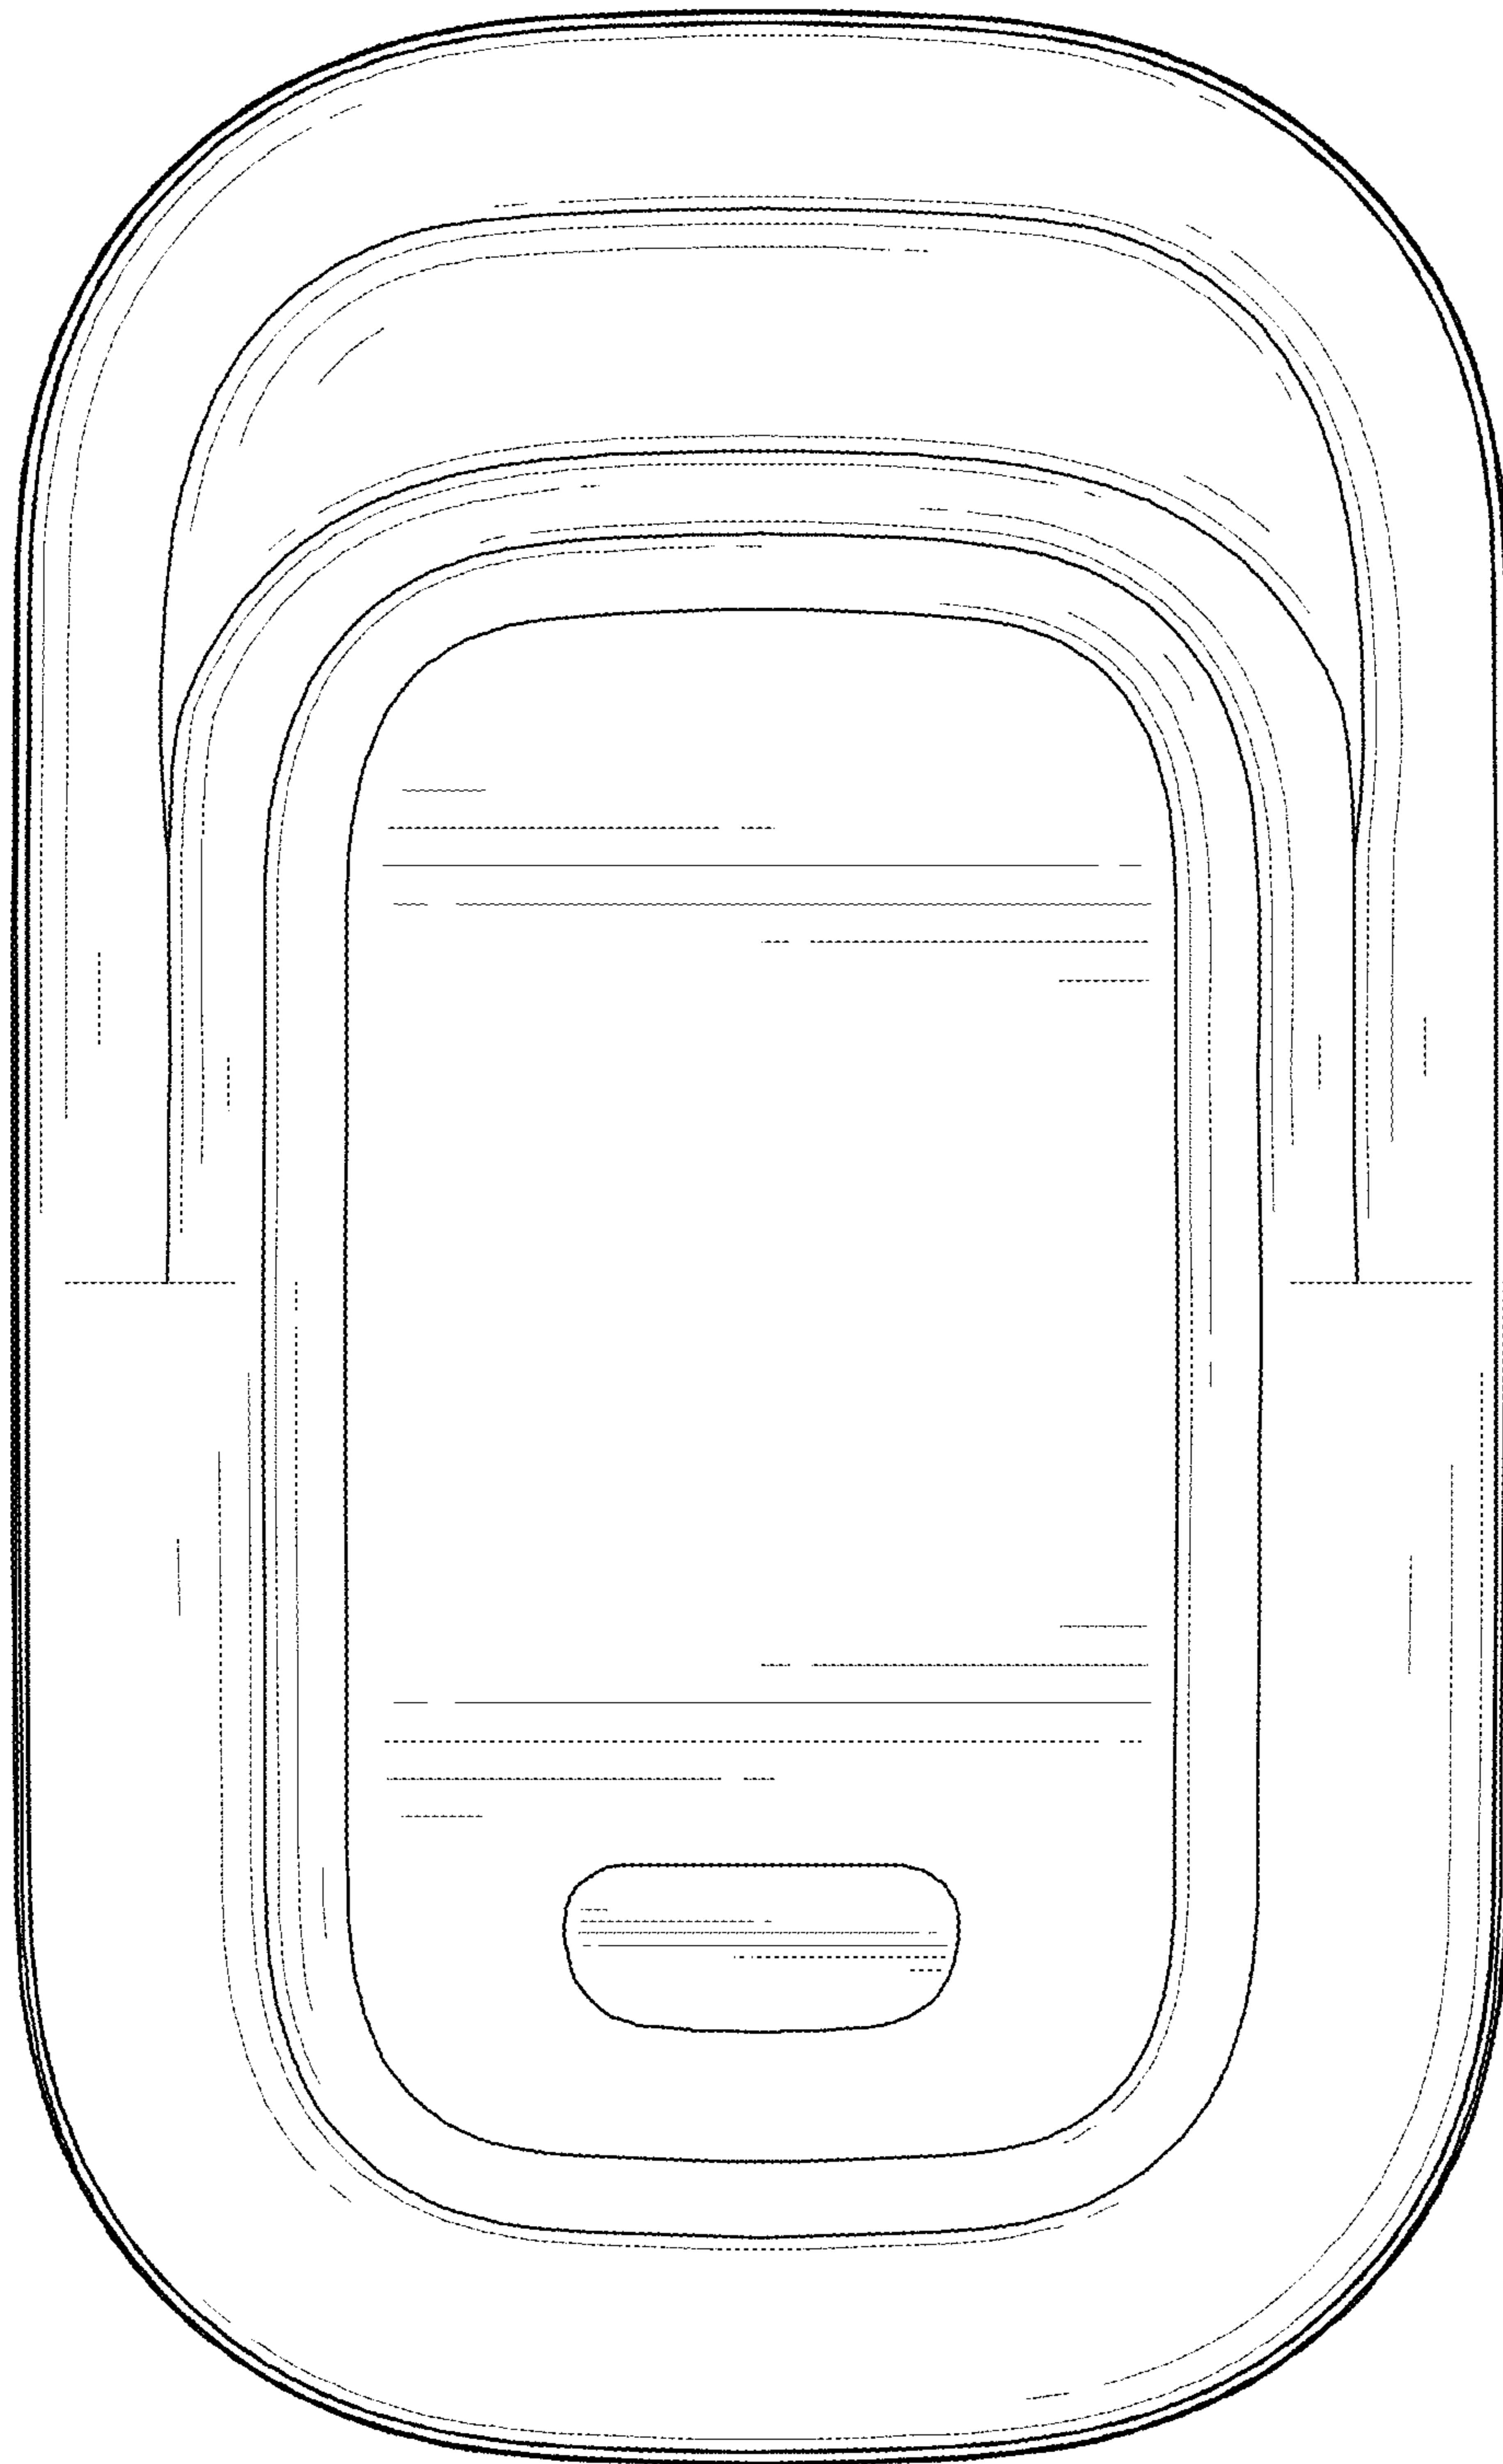


Fig. 7

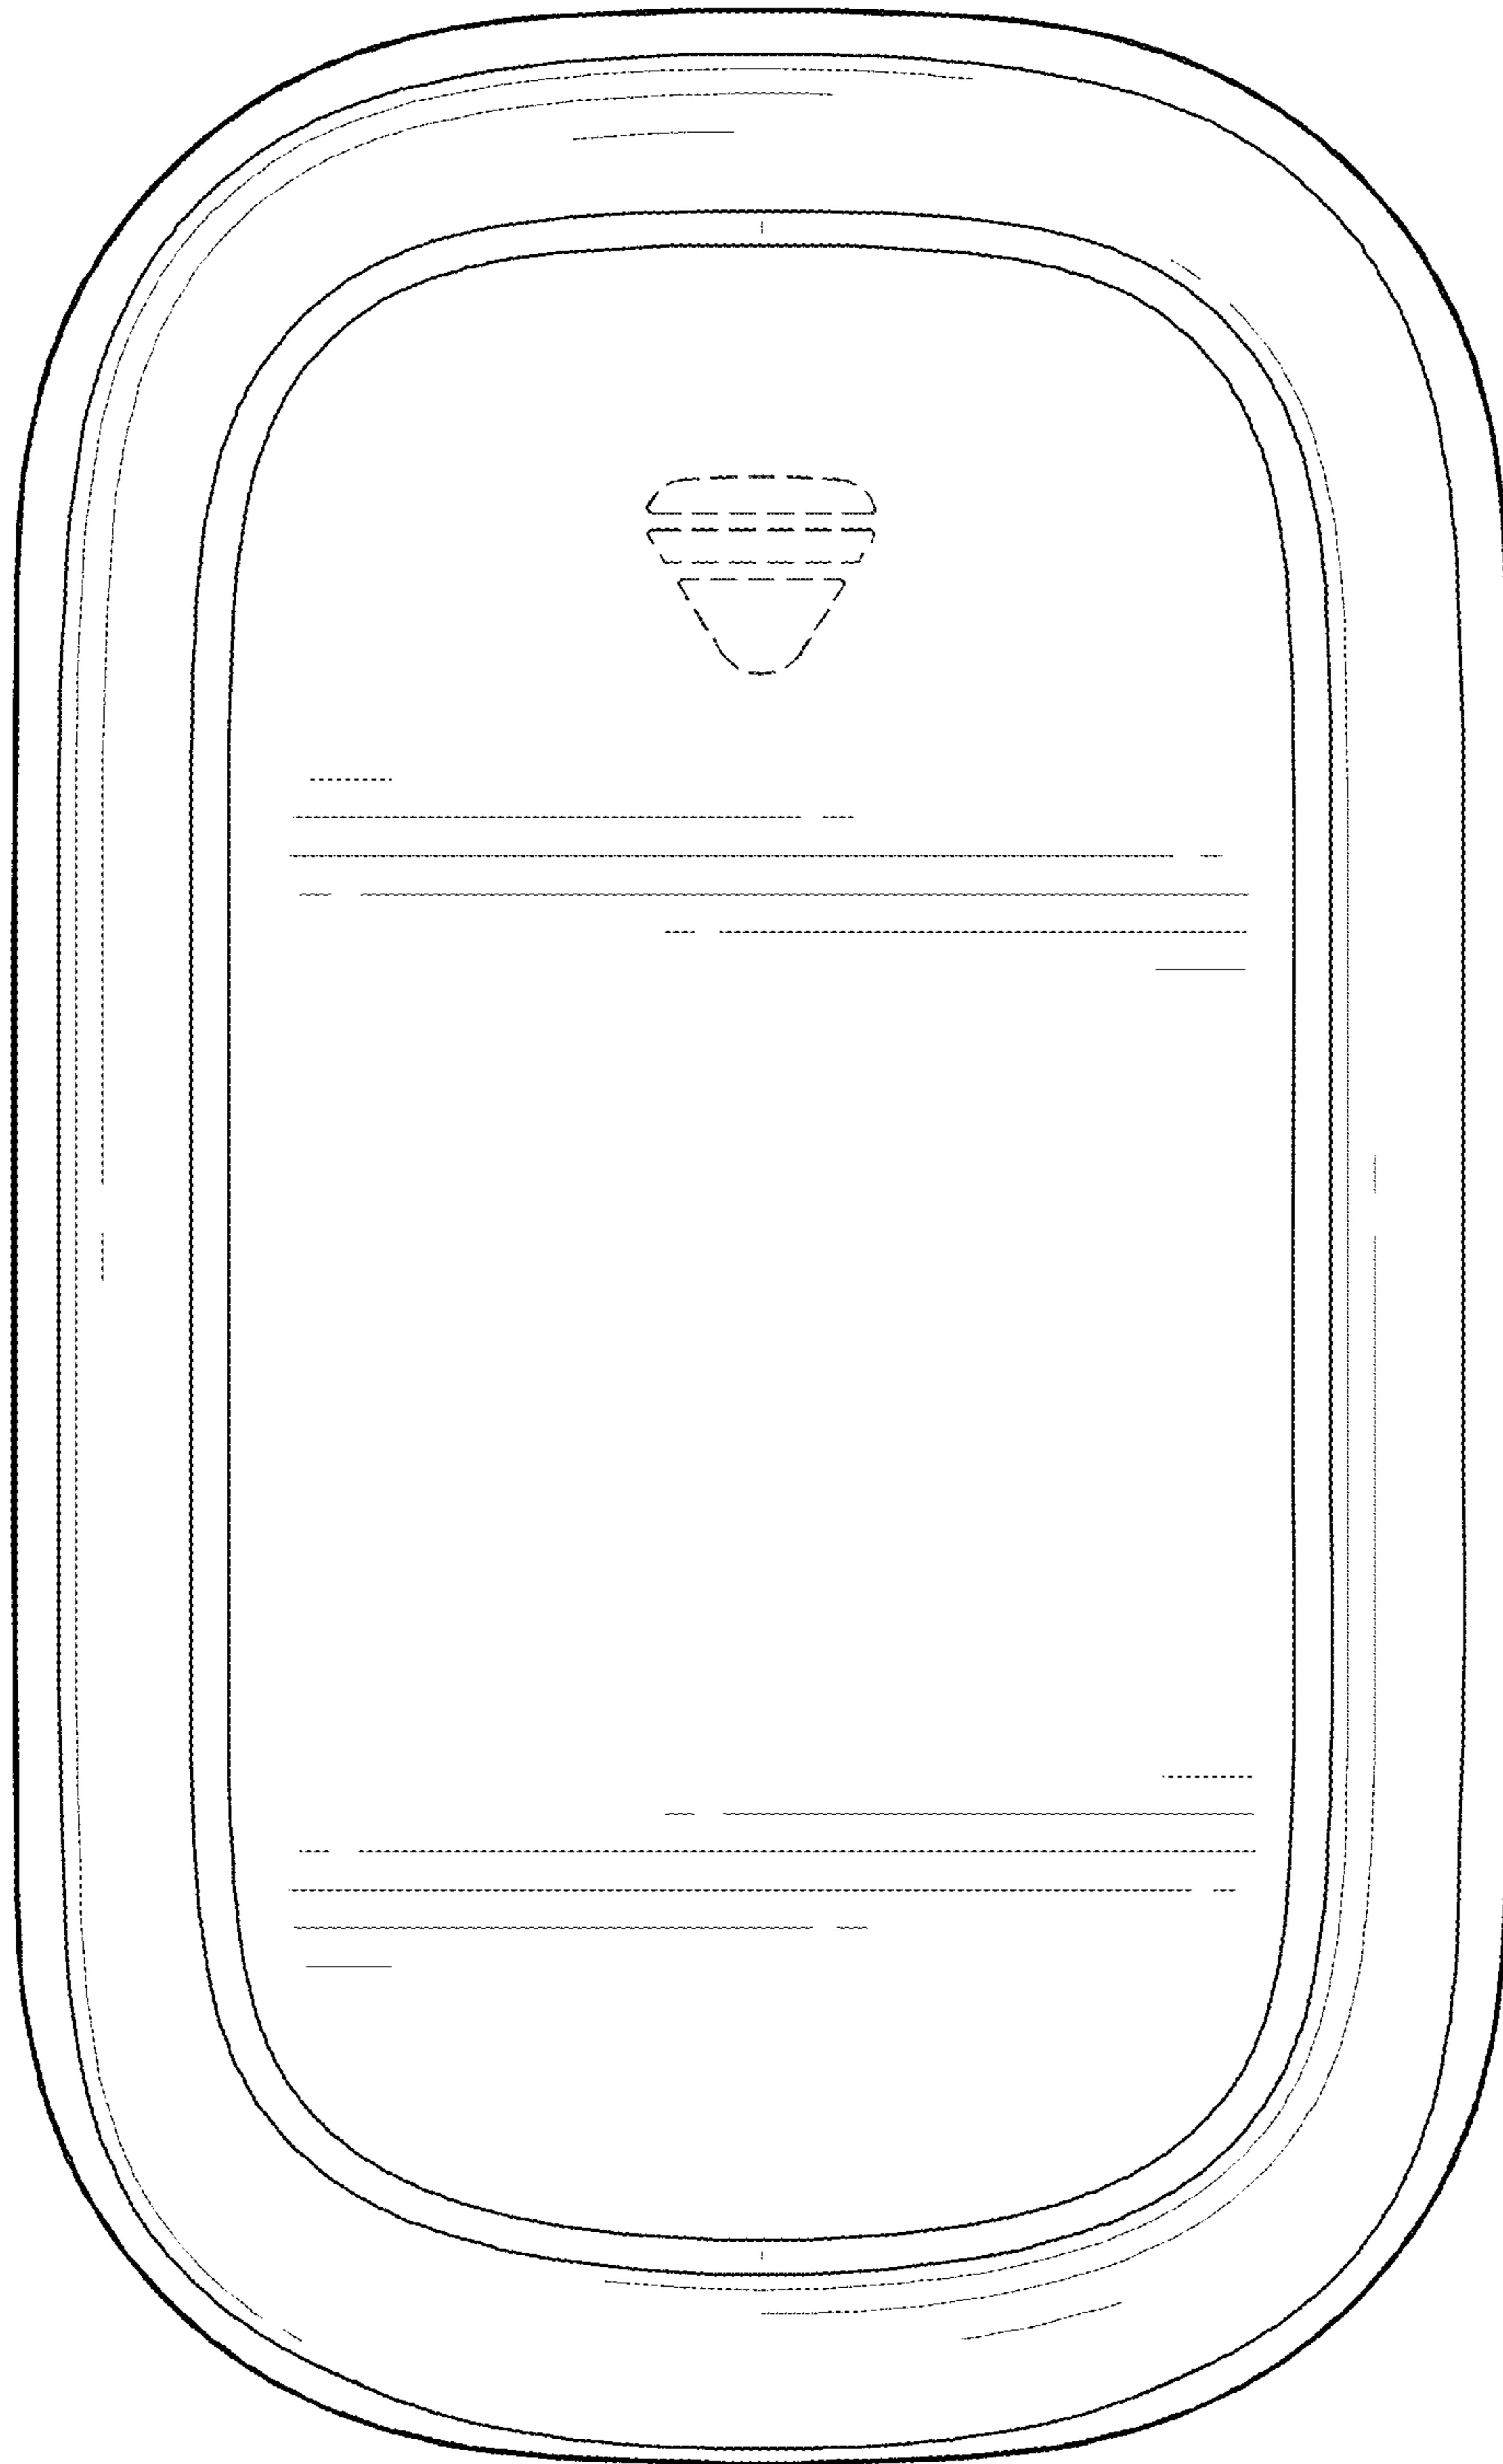


Fig. 8