



US00D896077S

(12) **United States Design Patent**
Matusek et al.

(10) **Patent No.:** **US D896,077 S**
(45) **Date of Patent:** **** Sep. 15, 2020**

(54) **COMBINED MEASURING AND DISPENSING DEVICE**

(71) Applicants: **Andrew Michael Matusek**, Medina, OH (US); **Jack Warren Gee, II**, Willoughby, OH (US)

(72) Inventors: **Andrew Michael Matusek**, Medina, OH (US); **Jack Warren Gee, II**, Willoughby, OH (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/678,479**

(22) Filed: **Jan. 29, 2019**

(51) **LOC (12) Cl.** **09-07**

(52) **U.S. Cl.**
USPC **D9/440**; D9/436; D9/449

(58) **Field of Classification Search**
USPC D3/201, 202; D7/300, 300.1, 317, 321, D7/391, 392, 392.1, 396.2, 601, 602,
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,518,520 A 8/1950 Broun
D217,759 S * 6/1970 Schweickart D9/449
(Continued)

OTHER PUBLICATIONS

Youtube. Smart Mouthwash Bottle Fills its Own 10 Millilitre Cup! by zeekzilch. Jul. 16, 2011. <https://www.youtube.com/watch?v=UrHIGHN3304> (Year: 2011).*

Primary Examiner — Darcey E Gottschalk
(74) *Attorney, Agent, or Firm* — Ralph E. Jocke; Walker & Jocke

(57) **CLAIM**

The ornamental design for a combined measuring and dispensing device, as shown and described.

DESCRIPTION

FIG. 1 is a front top left perspective view showing our new design for a combined measuring and dispensing device having a rotatable spout that is shown in a closed position. FIG. 2 is a front top left perspective view of the combined measuring and dispensing device showing the device enlarged relative to FIG. 1.

FIG. 3 is a rear top left perspective view of the combined measuring and dispensing device with the spout shown in the closed position.

FIG. 4 is a rear view of the combined measuring and dispensing device with the spout shown in the closed position.

FIG. 5 is a front view of the combined measuring and dispensing device with the spout shown in the closed position.

FIG. 6 is a left side view of the combined measuring and dispensing device with the spout shown in the closed position.

FIG. 7 is a right side view of the combined measuring and dispensing device with the spout shown in the closed position.

FIG. 8 is a top view of the combined measuring and dispensing device with the spout shown in the closed position.

FIG. 9 is a bottom view of the combined measuring and dispensing device with the spout shown in the closed position.


FIG. 10 is a bottom right perspective view of the combined measuring and dispensing device with the spout shown in the closed position.

FIG. 11 is a rear top left perspective view of the combined measuring and dispensing device with the spout shown in an open position; and,

FIG. 12 is a front top left perspective view of the combined measuring and dispensing device with the spout shown in the open position.

Features shown in broken lines form no part of the claimed design.

1 Claim, 10 Drawing Sheets

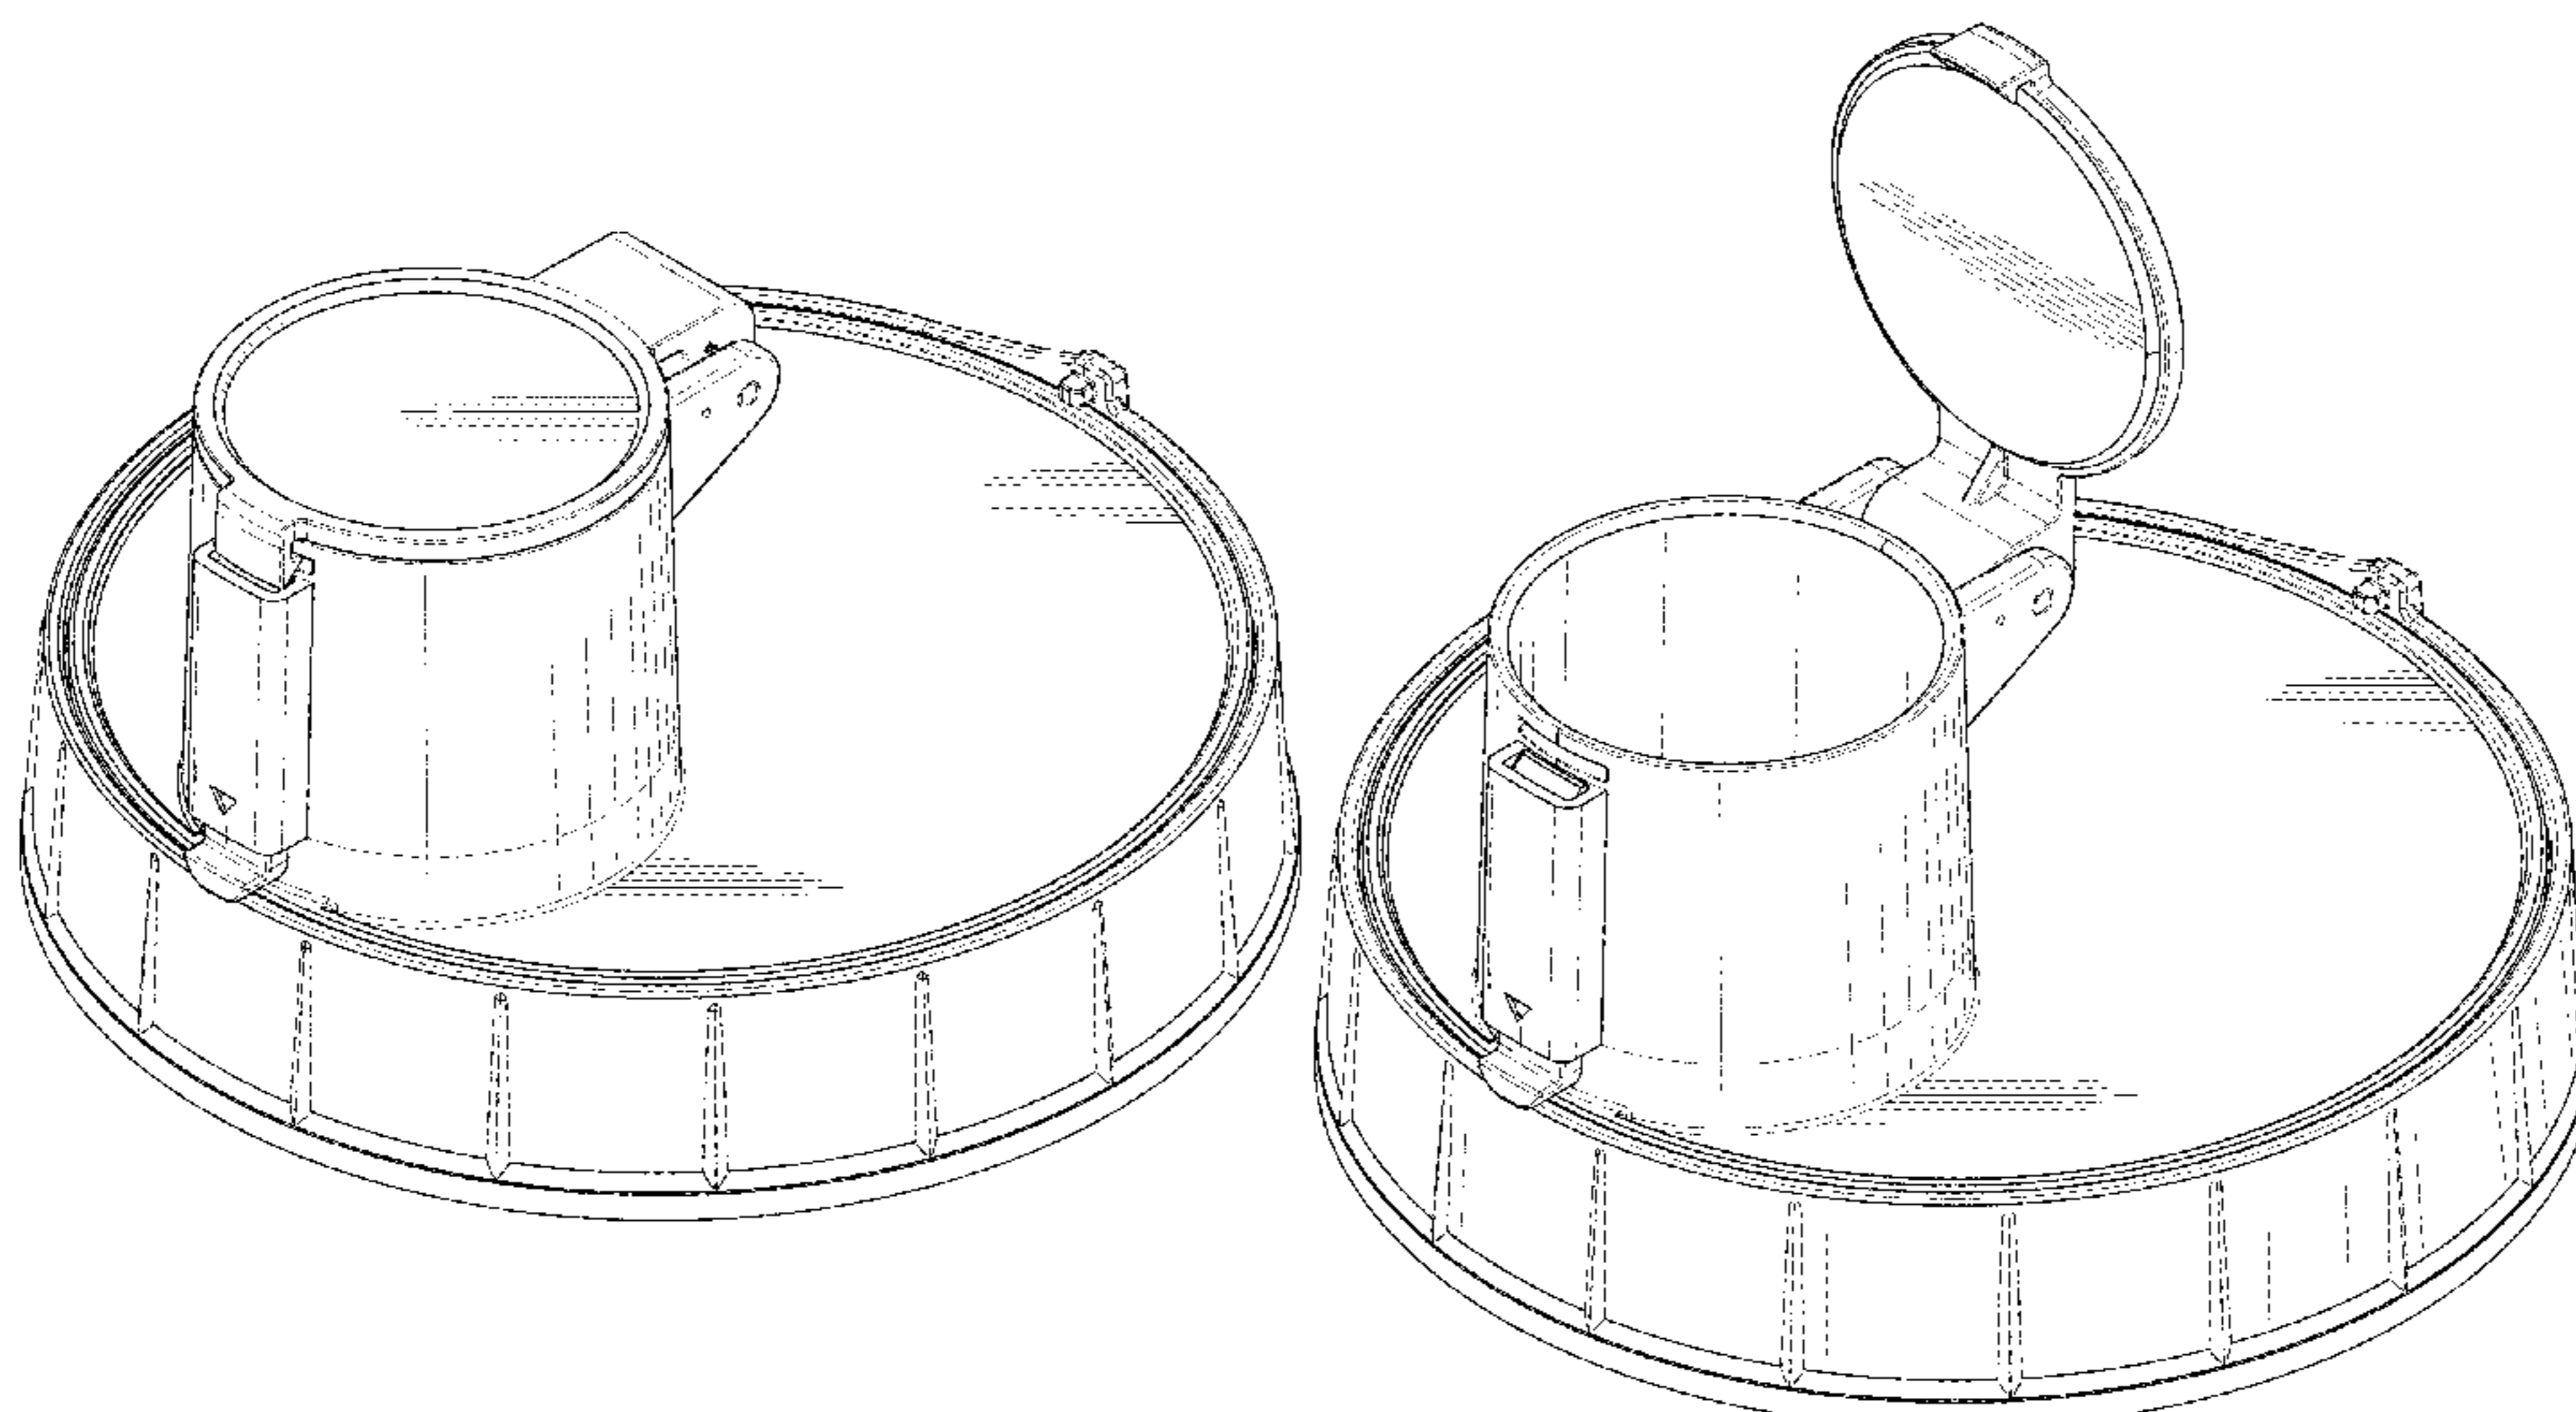

(58) **Field of Classification Search**
 USPC D7/619.1, 629; D9/434–436, 439, 440,
 D9/443, 445–447, 449, 452–454, 499
 CPC B65D 47/0885; G01F 11/261
 See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,032,050 A 6/1977 Funk
 5,495,964 A 3/1996 Santagiuliana
 5,509,582 A 4/1996 Robbins, III
 5,873,493 A 2/1999 Robinson
 6,422,426 B1 7/2002 Ribbins, III et al.
 7,090,098 B2 8/2006 Livingston et al.
 8,181,830 B2 5/2012 Flores
 D714,584 S * 10/2014 Boroski D7/392
 8,925,768 B1 1/2015 Ismail
 D741,176 S * 10/2015 Bell D9/446

D752,916 S * 4/2016 Goodwin D7/392.1
 D763,076 S * 8/2016 Lane D9/446
 D769,671 S * 10/2016 Bielawski D7/392.1
 D772,652 S * 11/2016 Yao D7/510
 D801,111 S * 10/2017 Eyal D7/392.1
 9,828,230 B2 * 11/2017 Ismail B67D 3/0041
 D813,668 S * 3/2018 Miller D9/446
 D817,084 S * 5/2018 Hammer D7/392.1
 D817,085 S * 5/2018 Davis D7/392.1
 D824,721 S * 8/2018 Hu D7/392.1
 D825,332 S * 8/2018 Miksovsky D9/446
 D831,414 S * 10/2018 Diener D7/392
 D843,778 S * 3/2019 Yao D7/392.1
 D844,376 S * 4/2019 Rosette D7/392
 D847,563 S * 5/2019 Jacobsen D7/396.2
 D856,067 S * 8/2019 Barber D7/392.1
 D858,181 S * 9/2019 Lown D7/392.1
 D862,977 S * 10/2019 Bohman D7/392
 D870,509 S * 12/2019 Bo D7/392.1

* cited by examiner

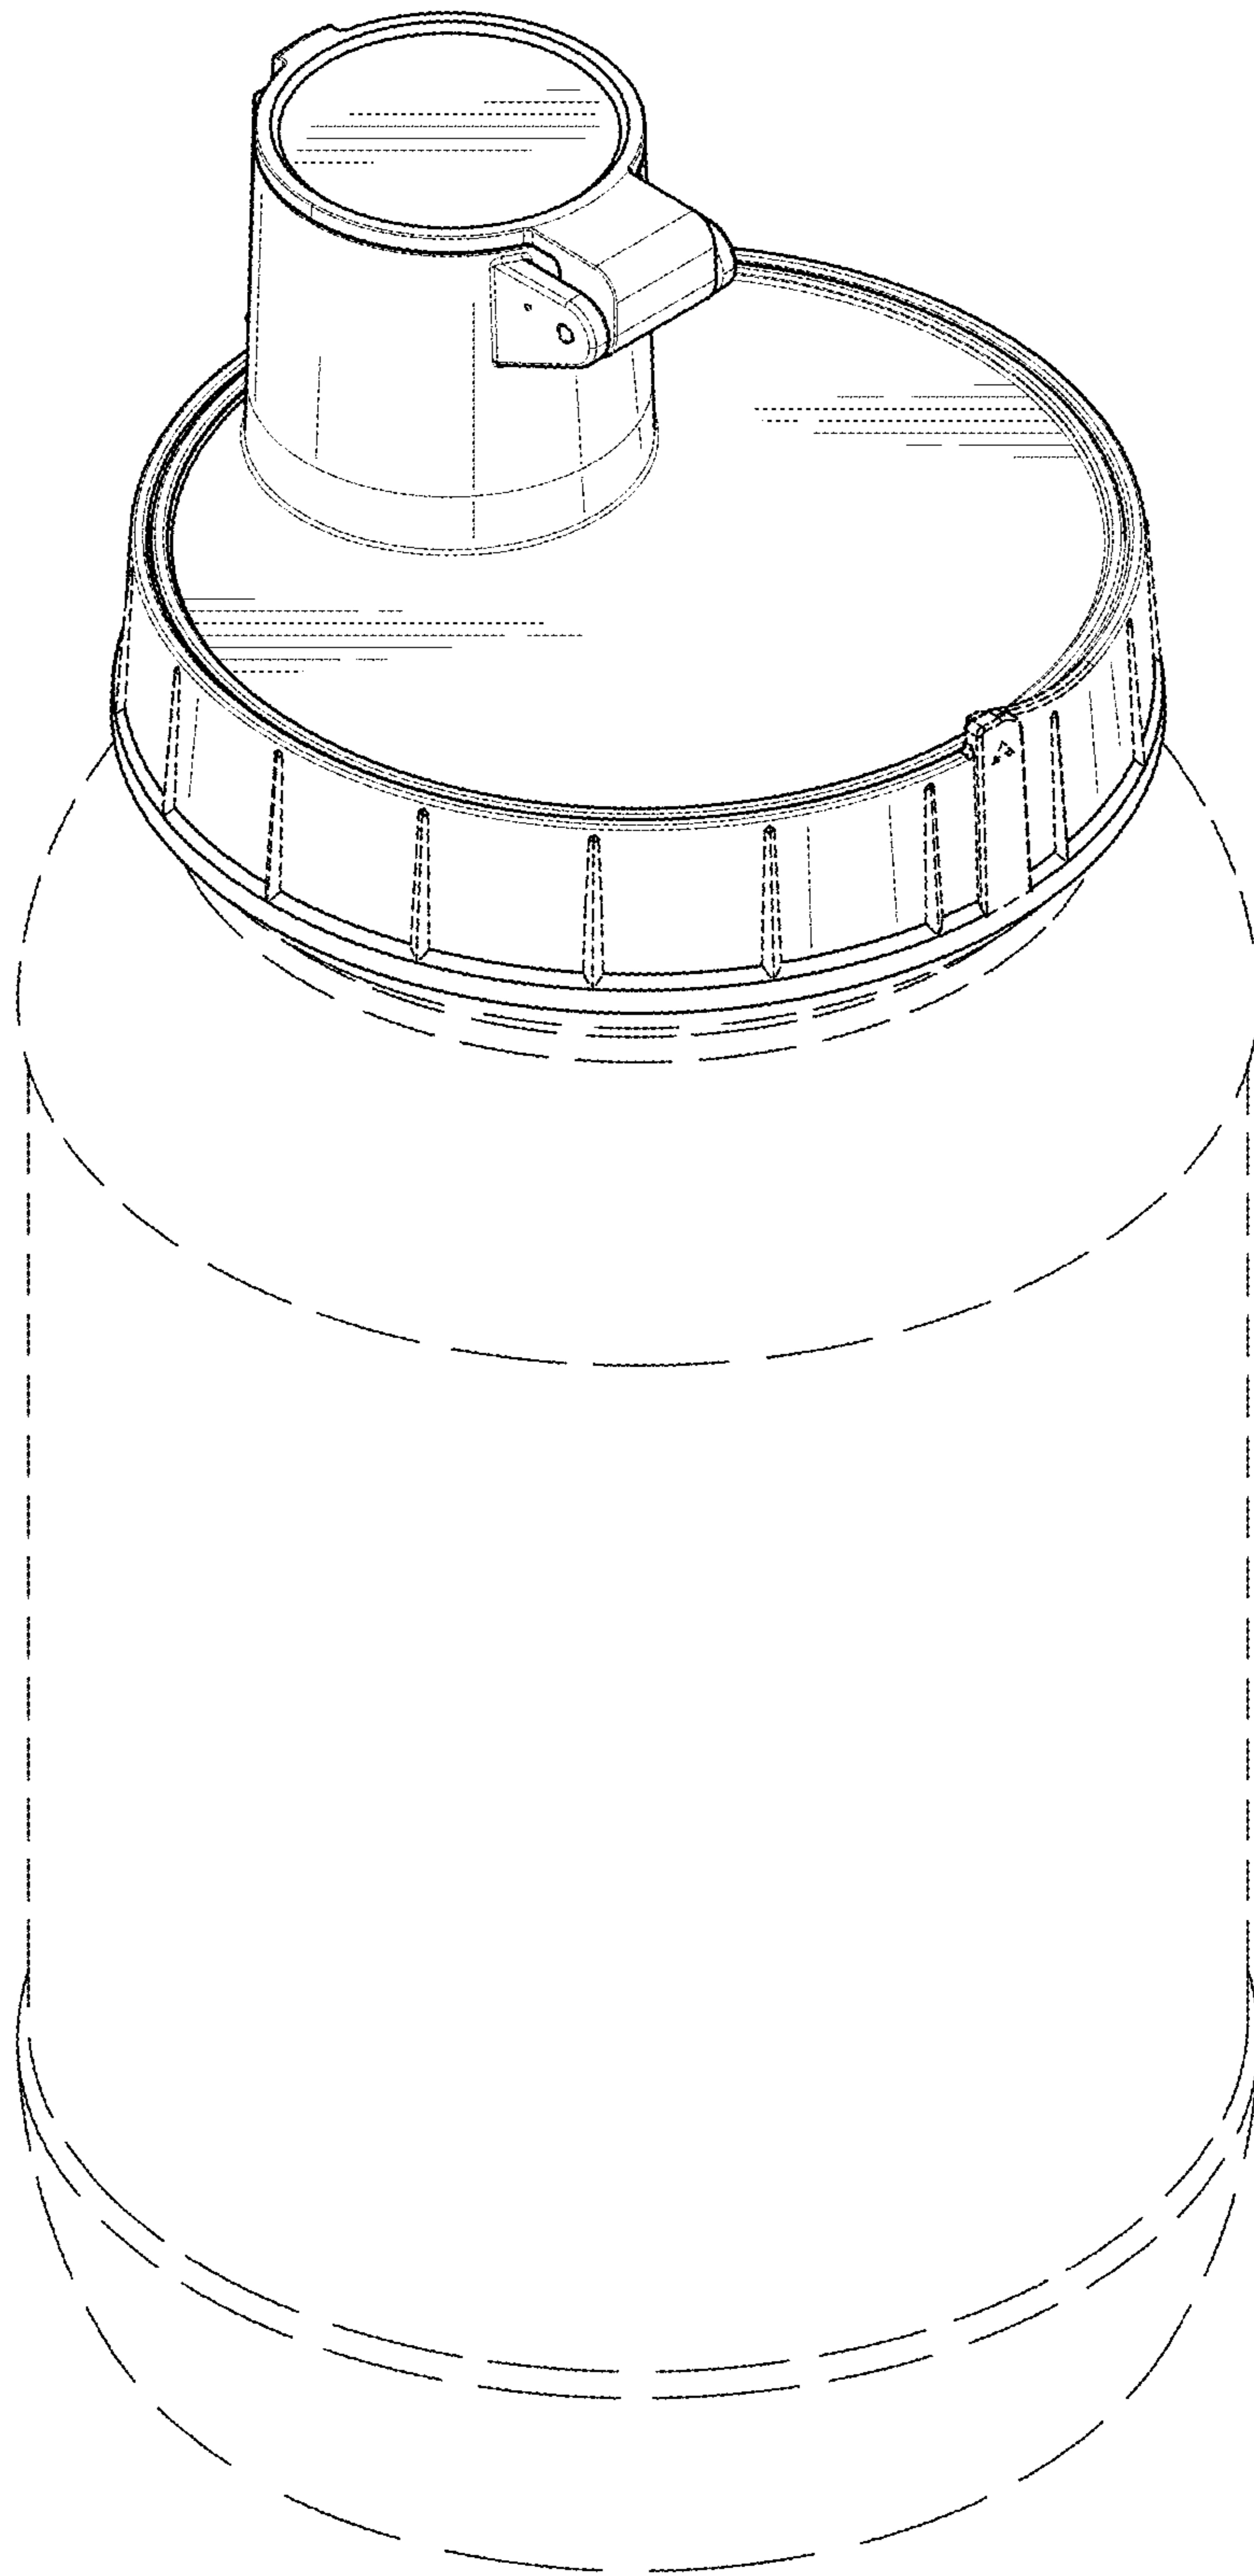


FIG. 1

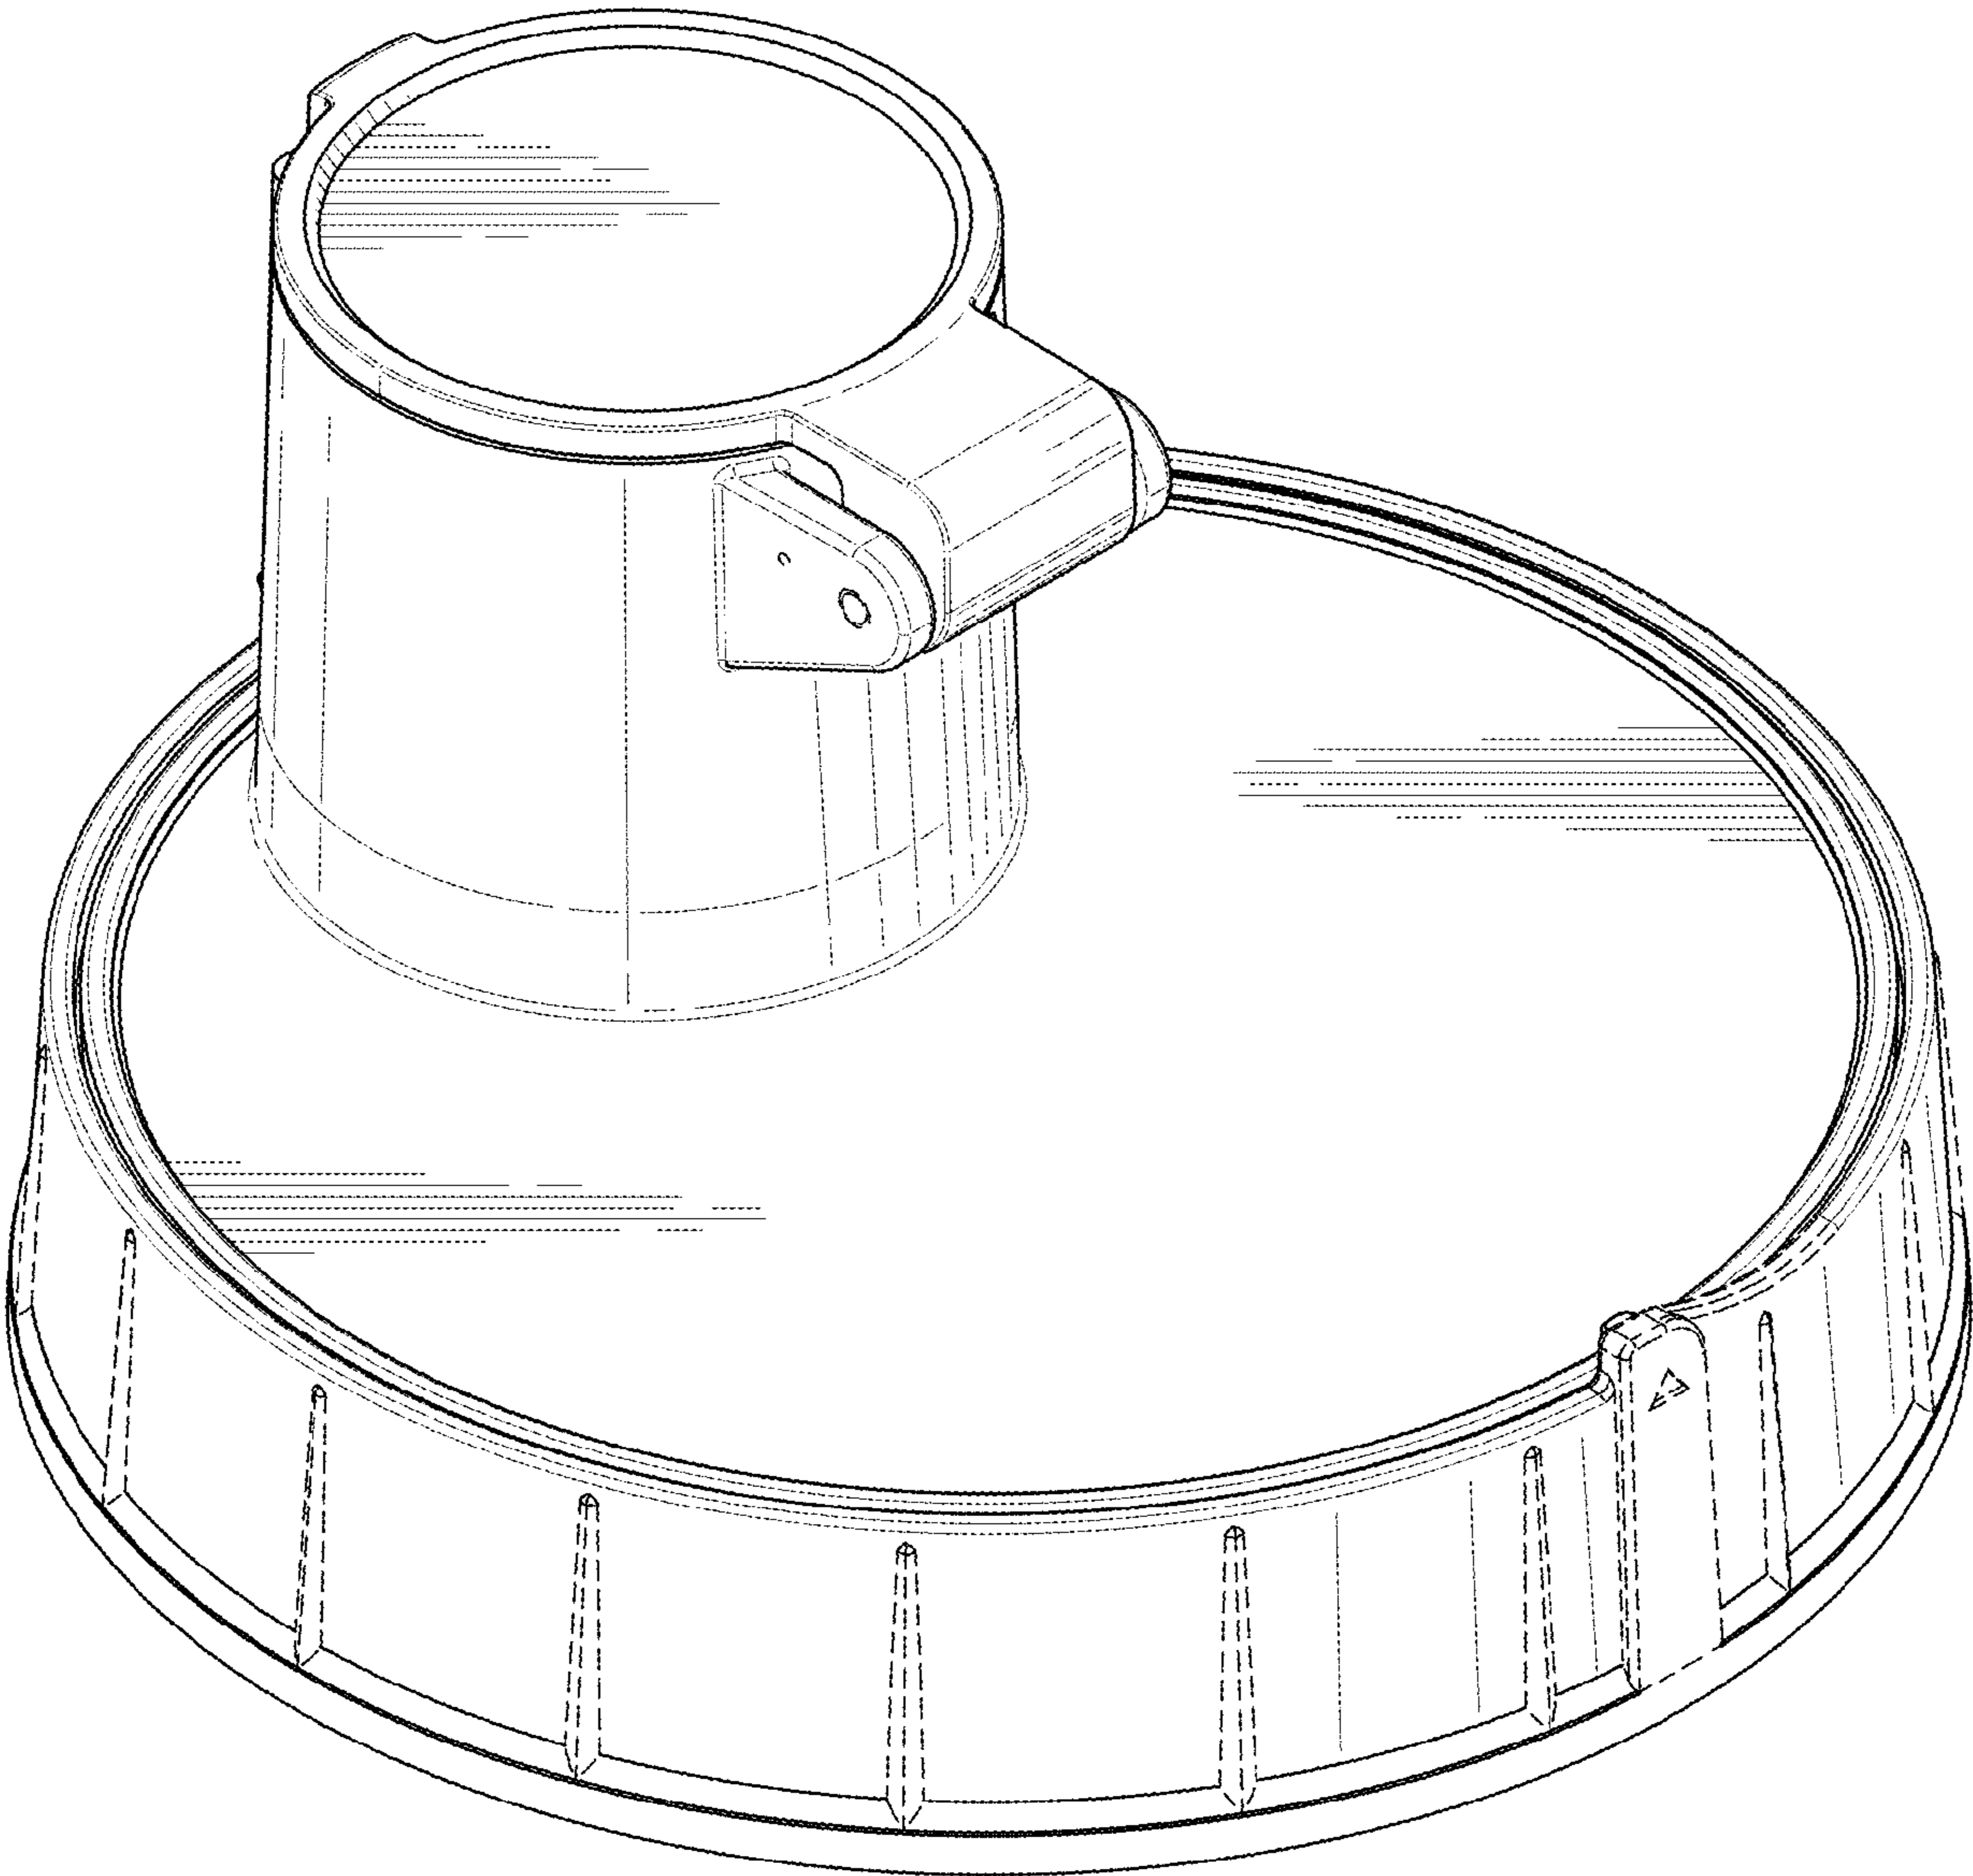


FIG. 2

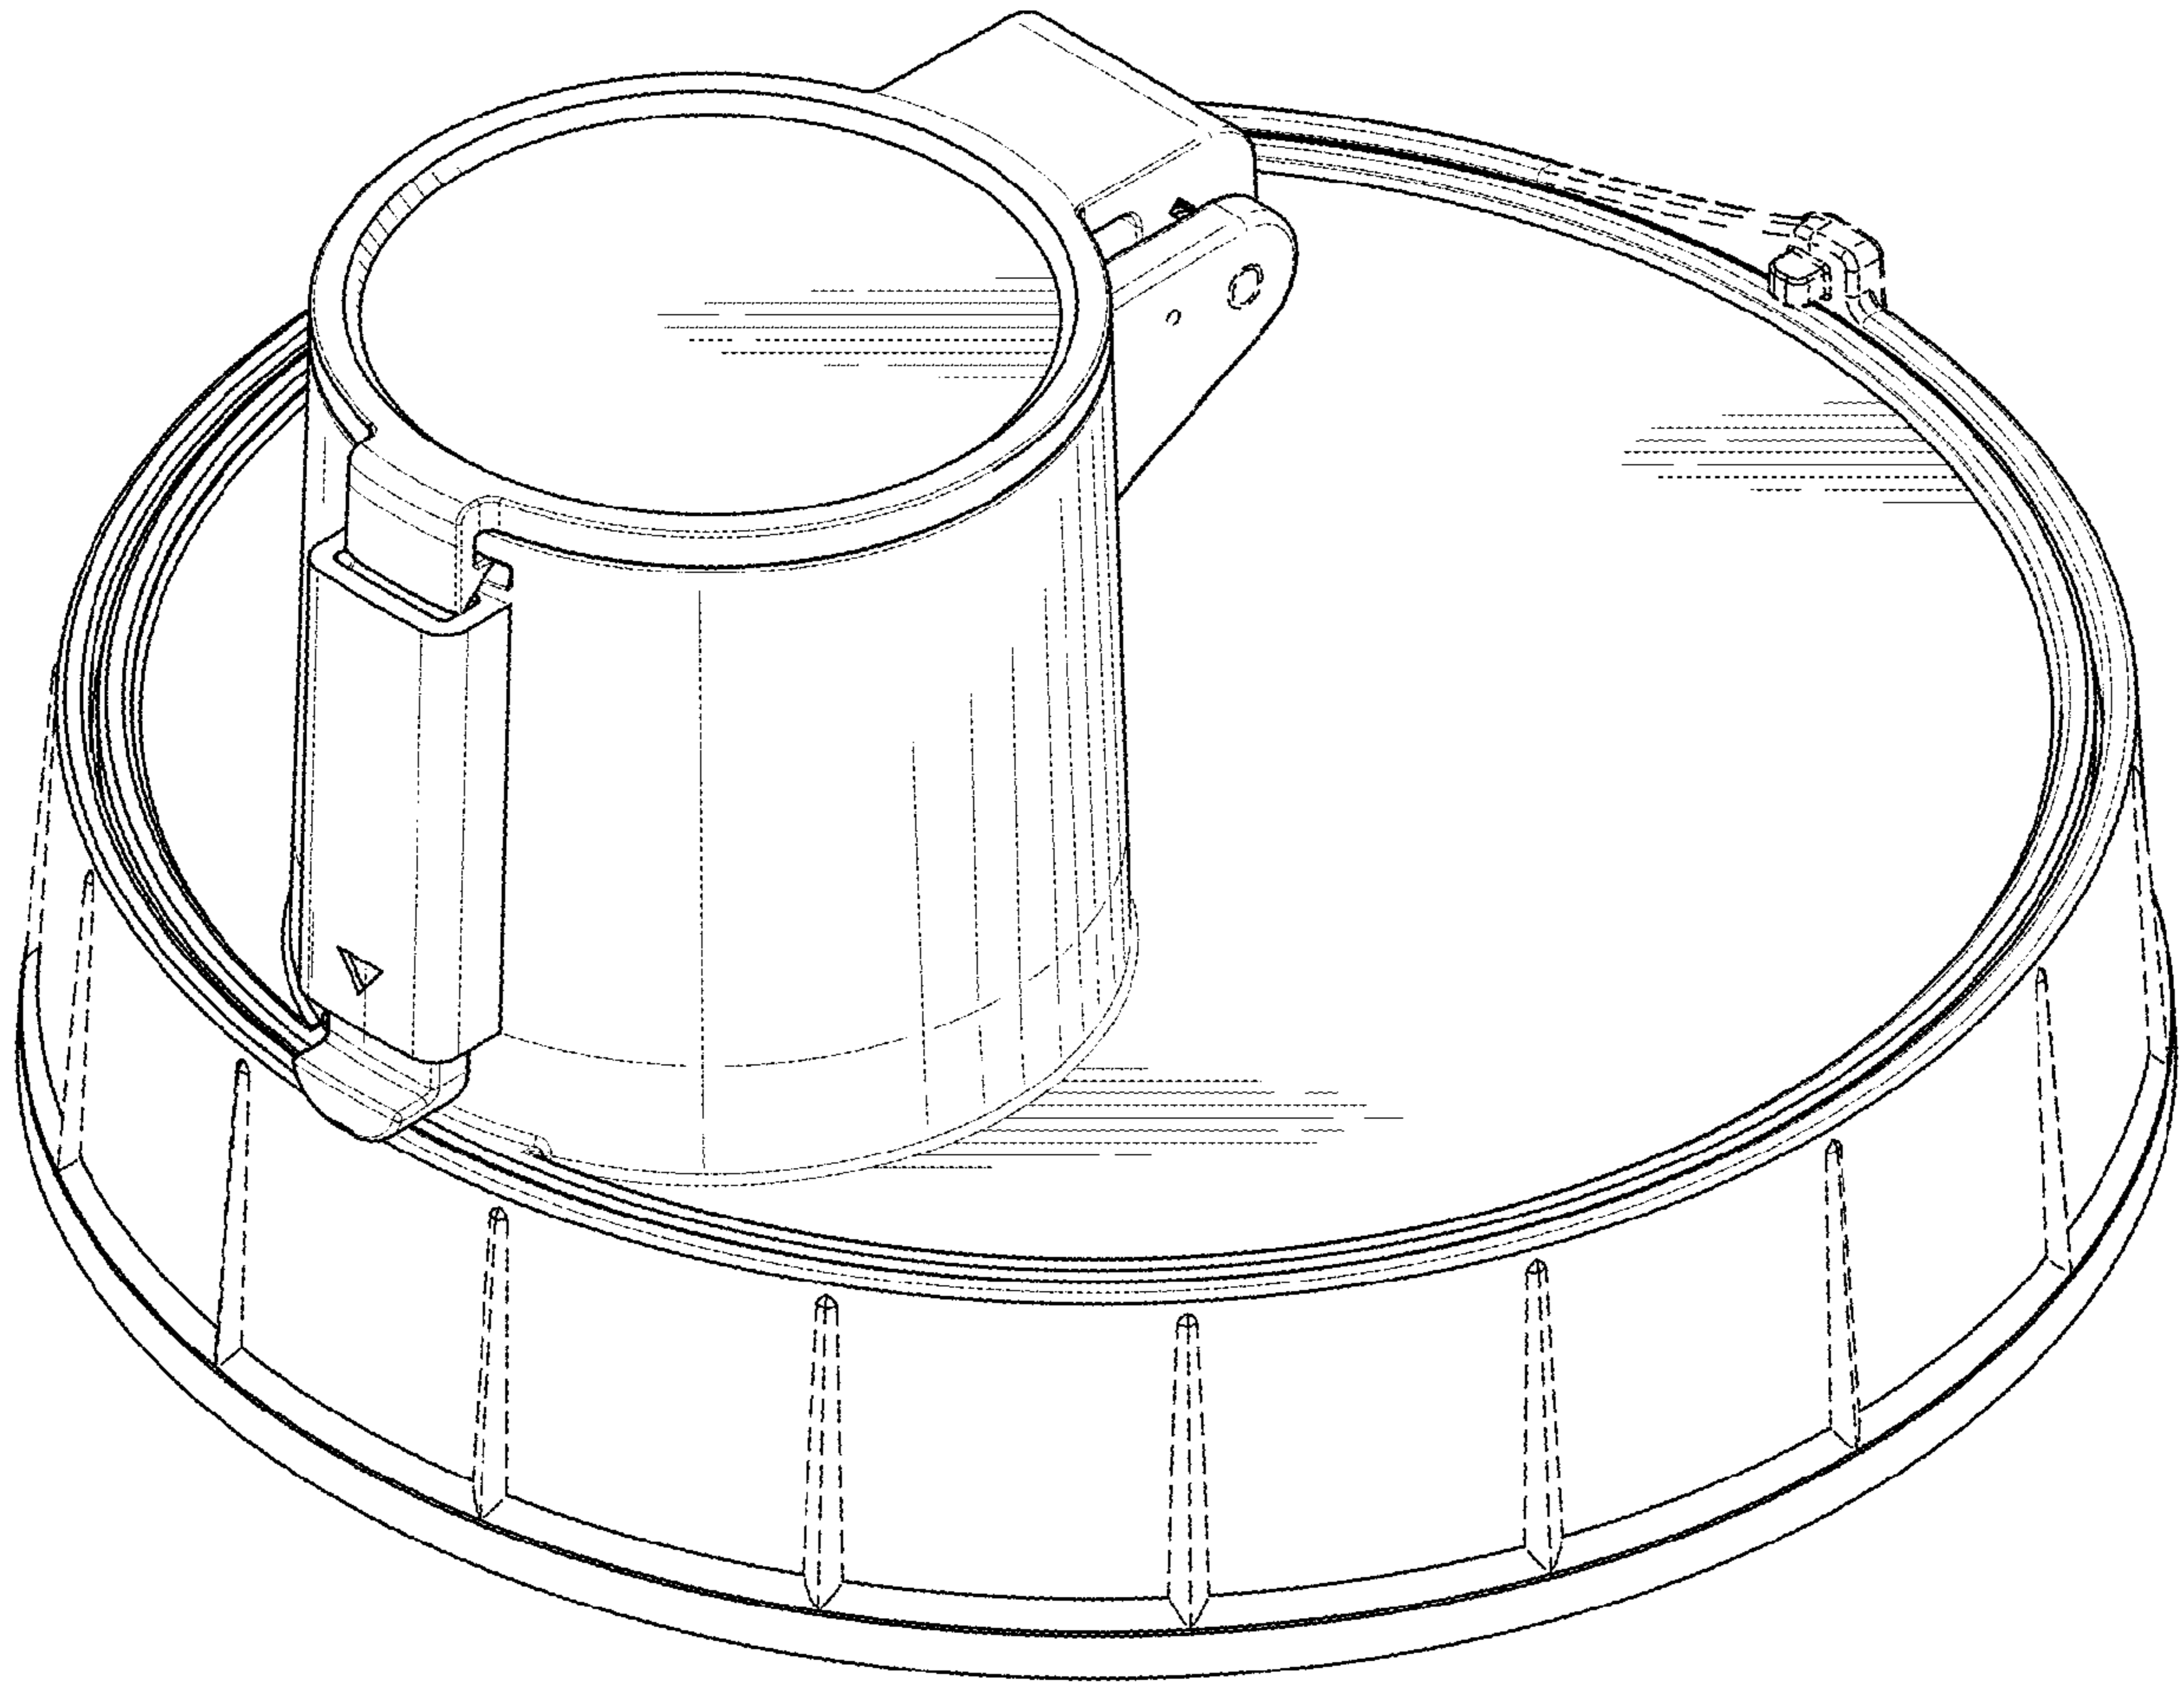


FIG. 3

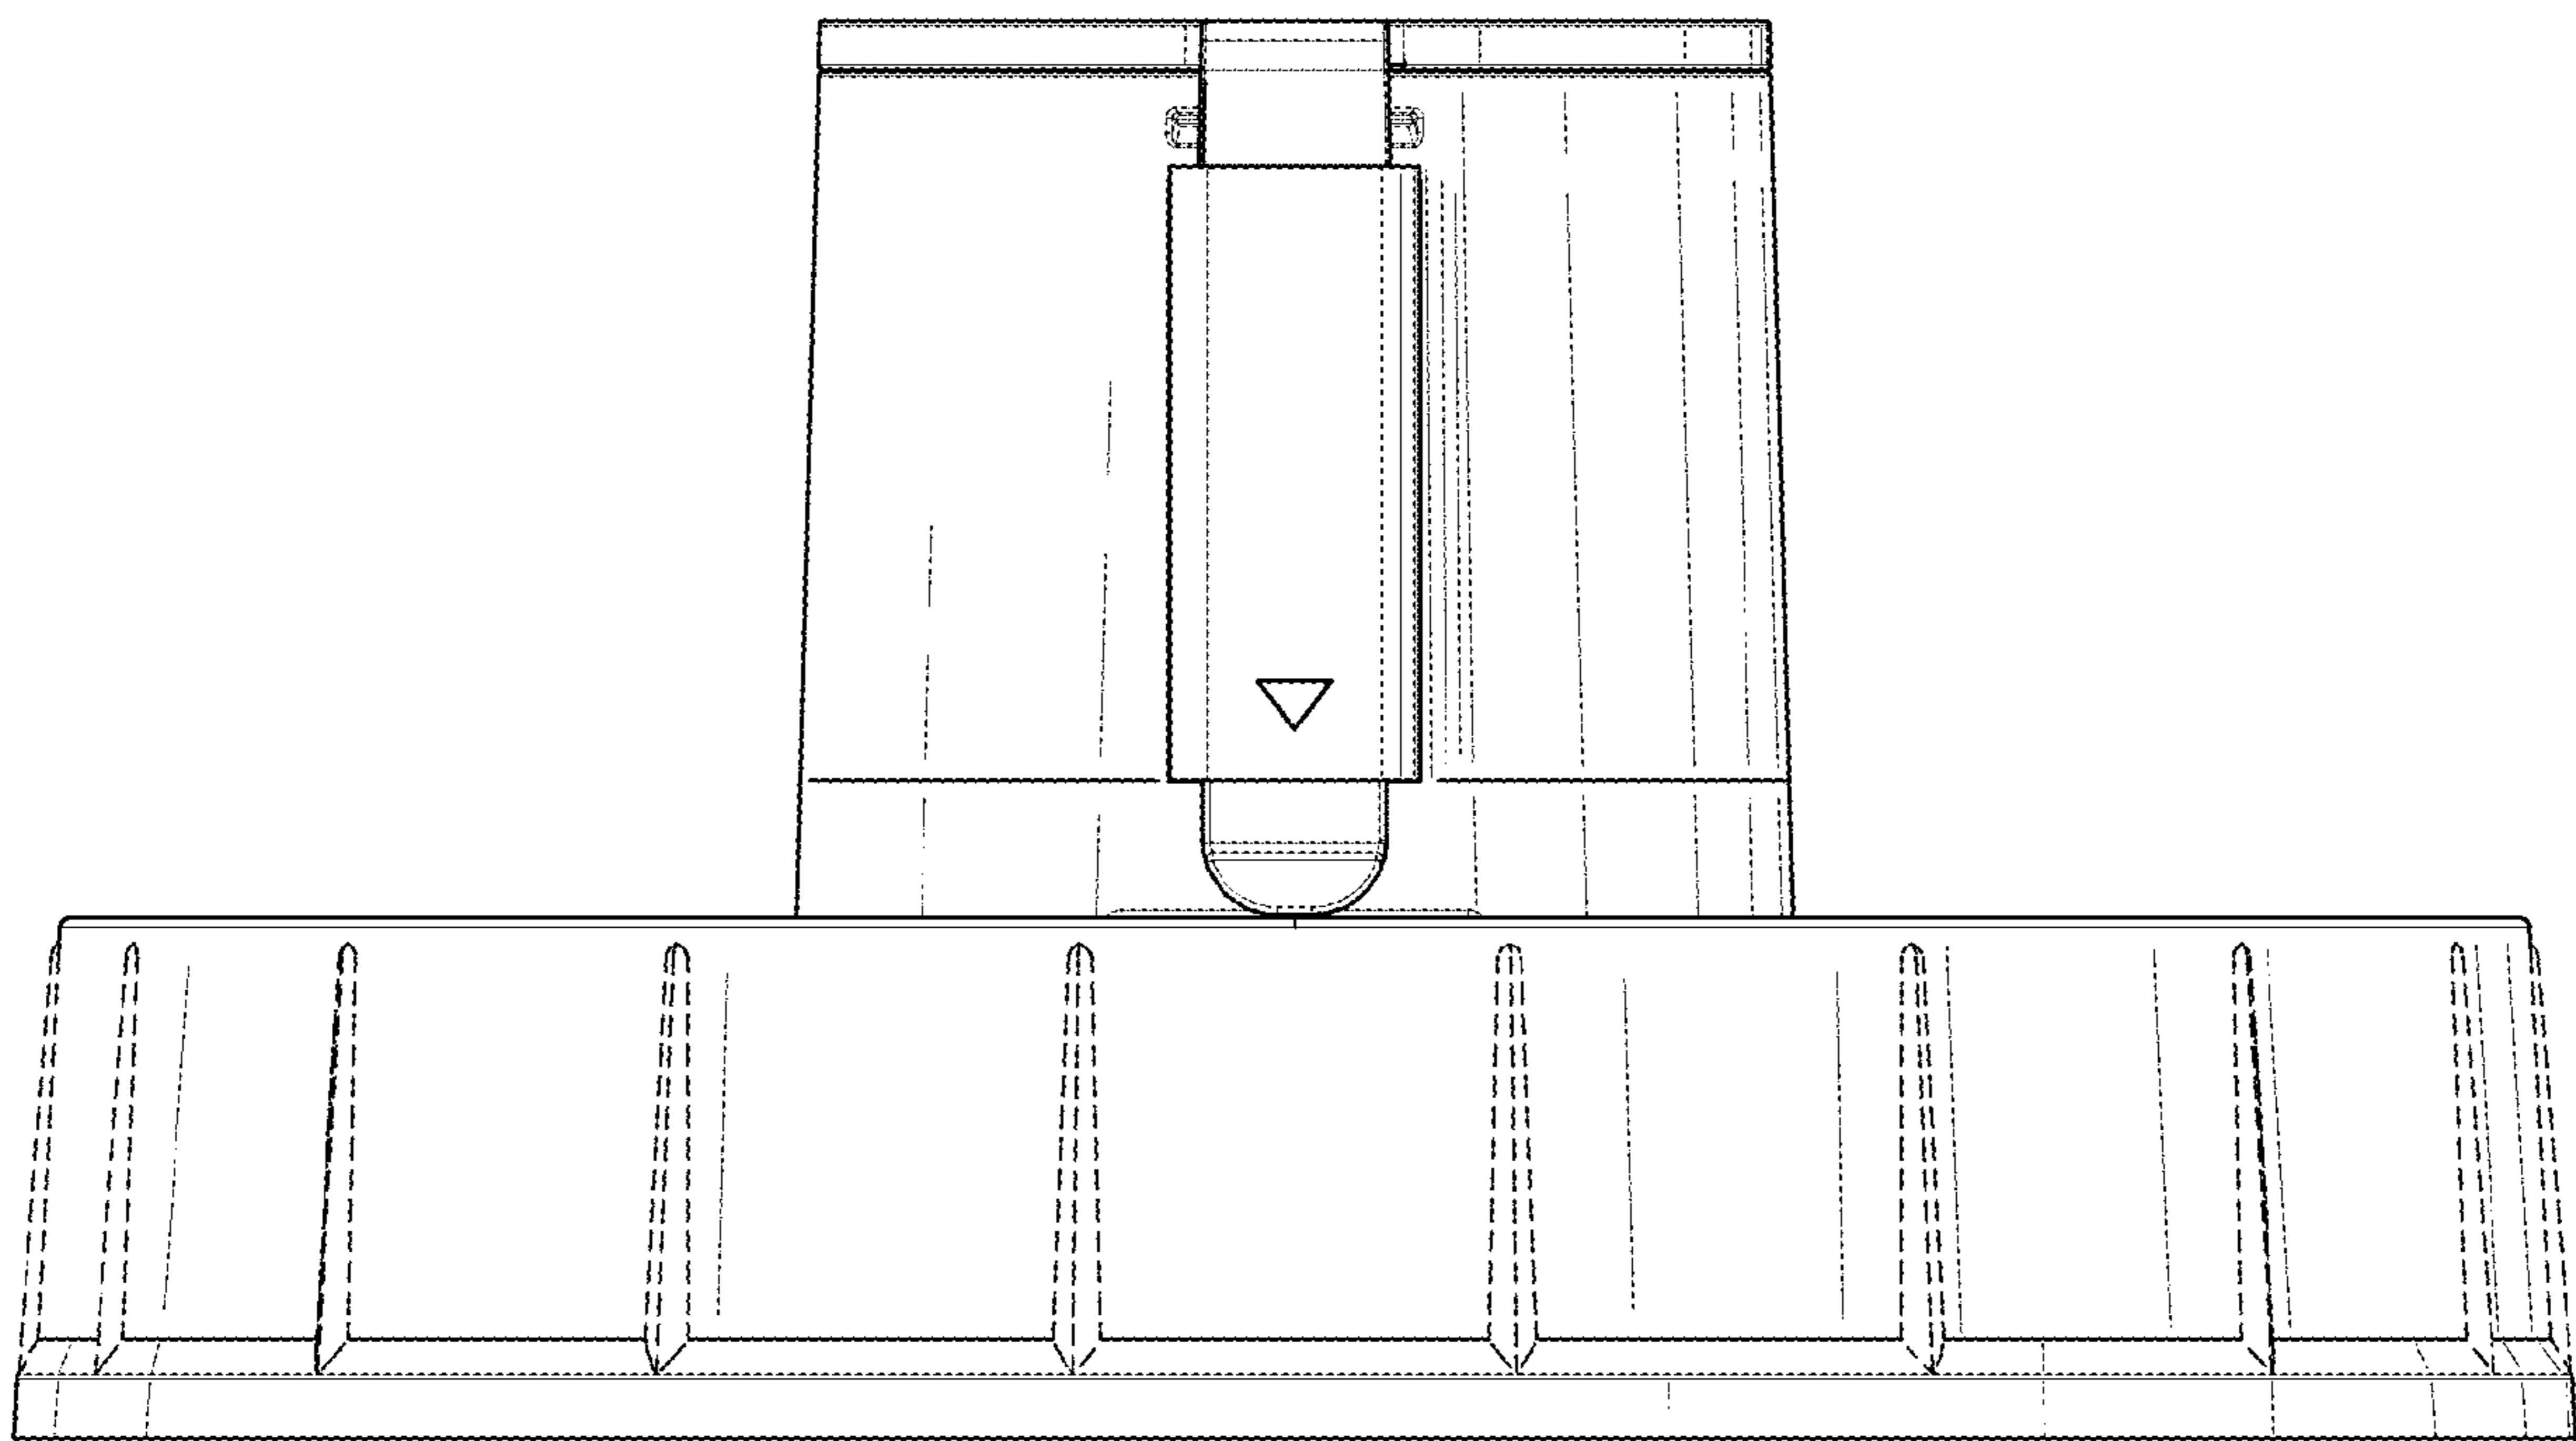


FIG. 4

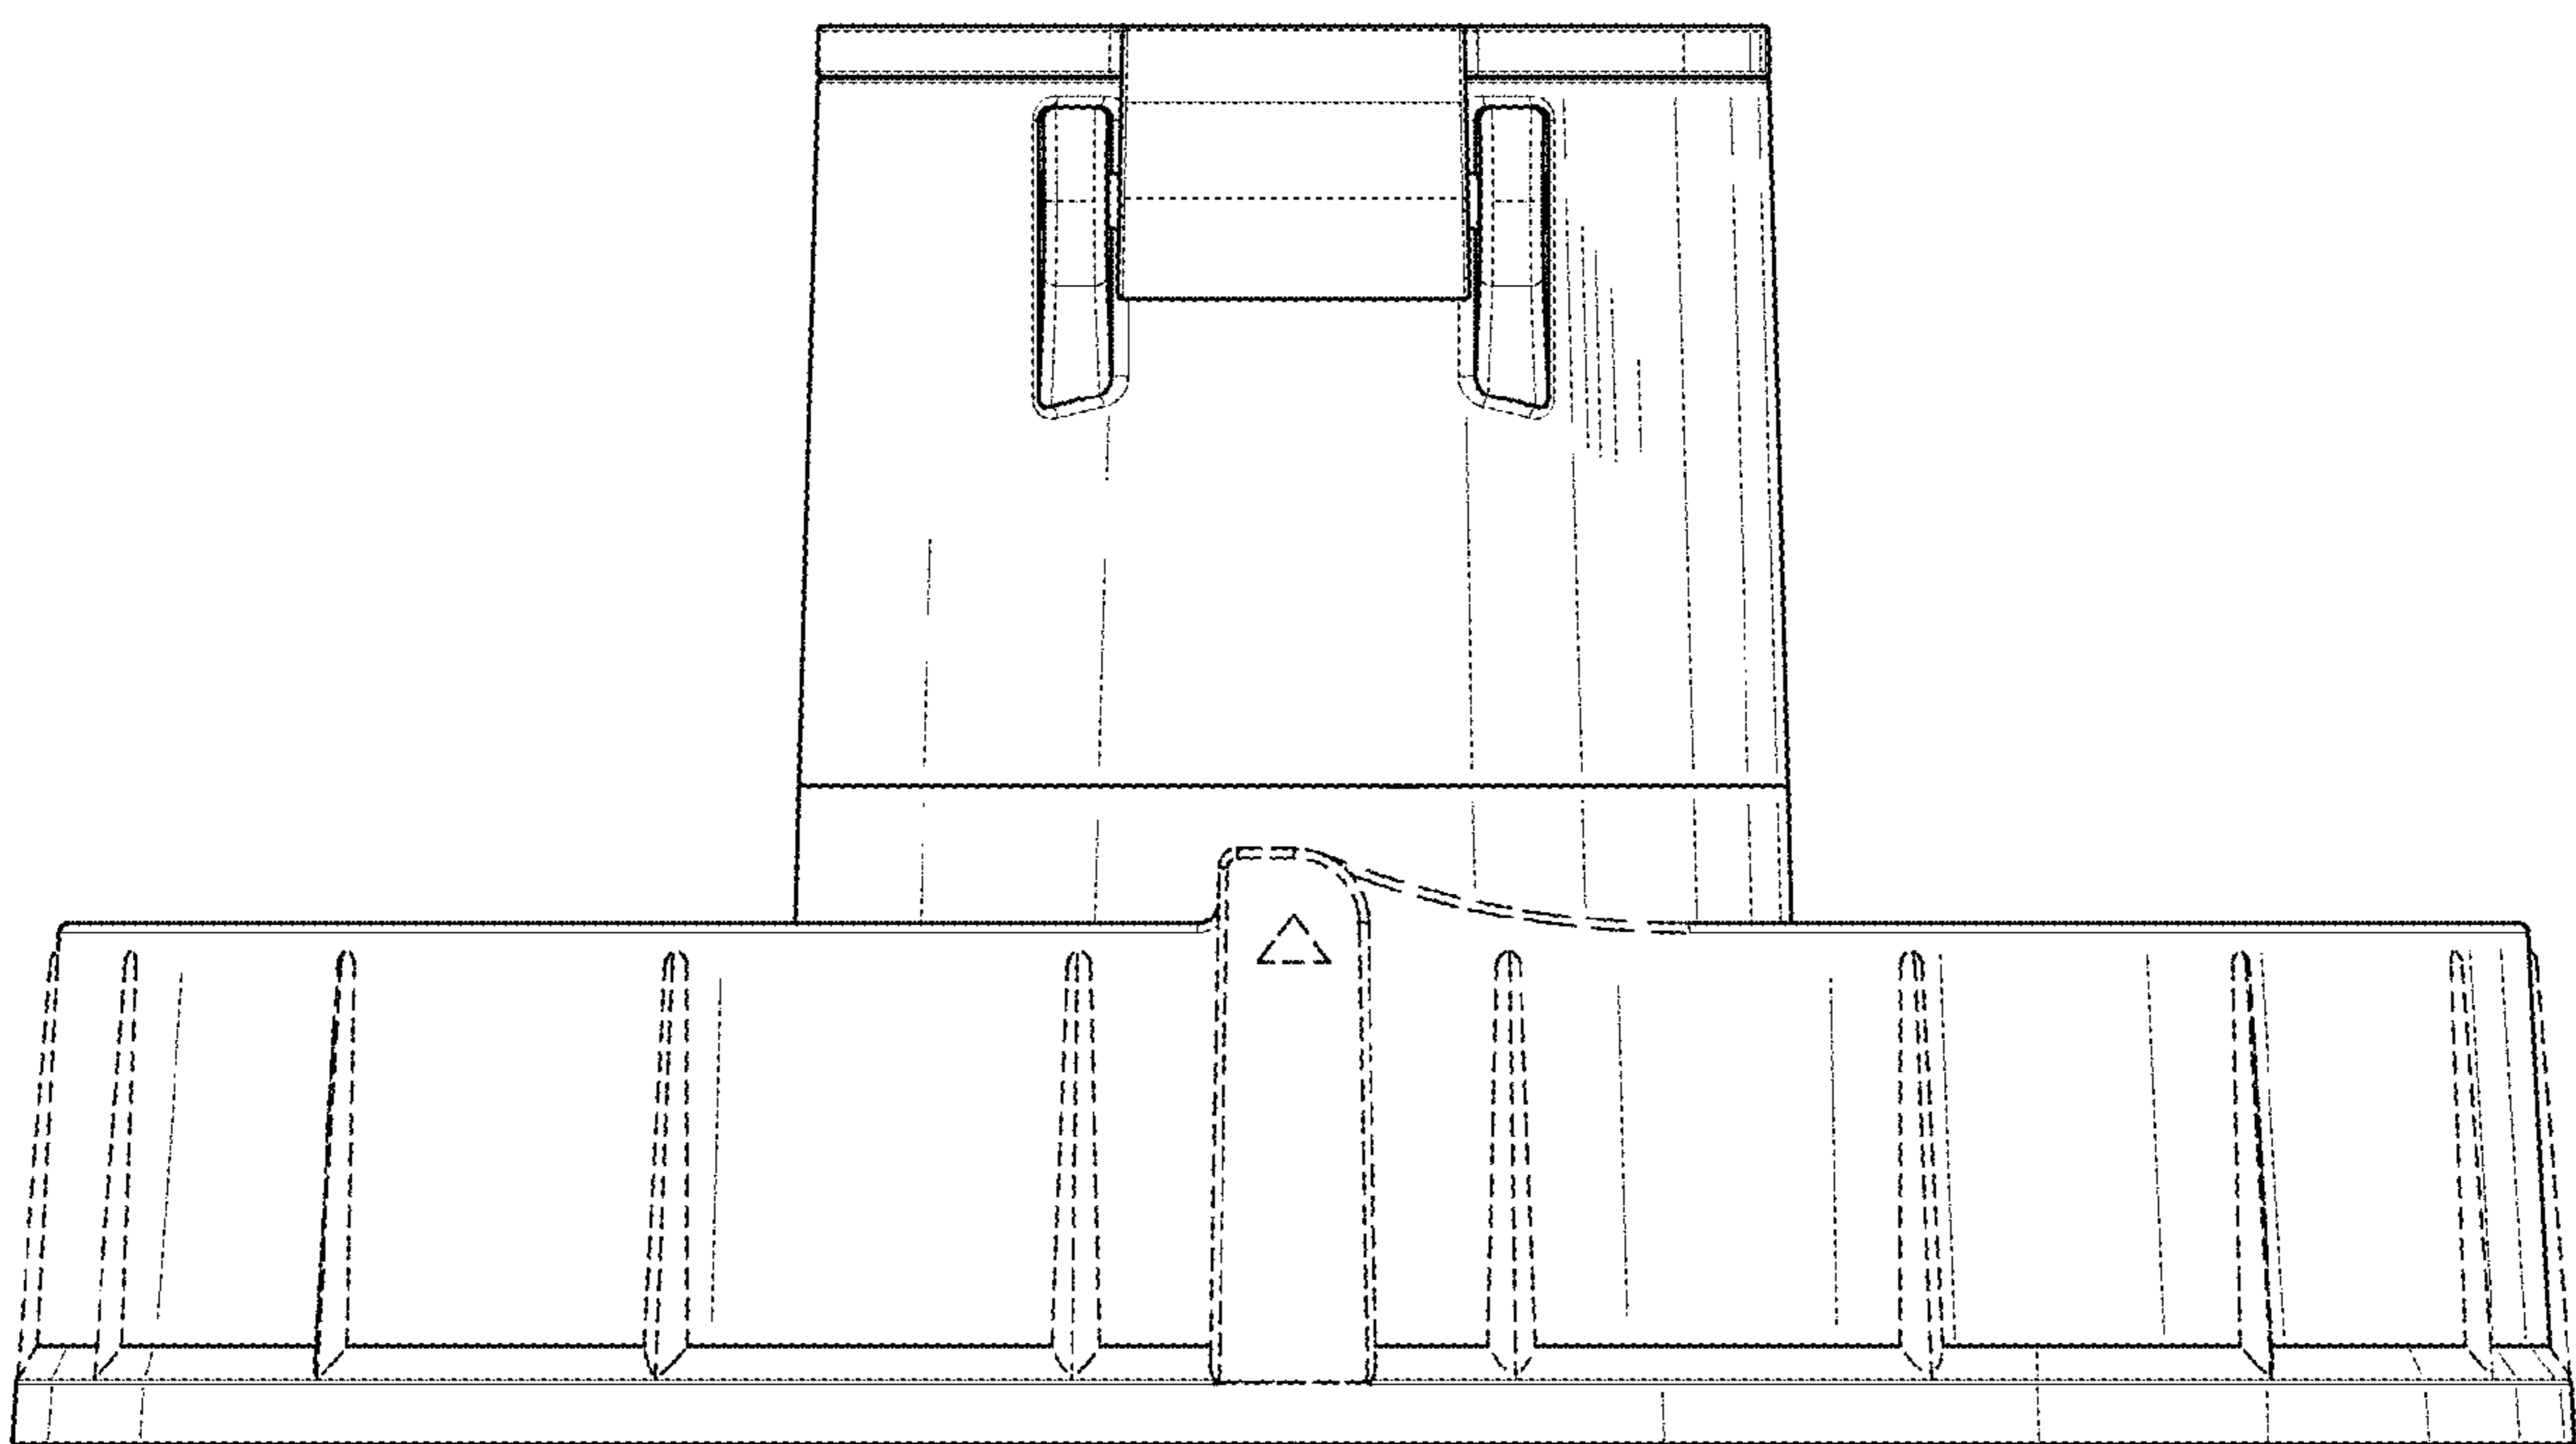


FIG. 5

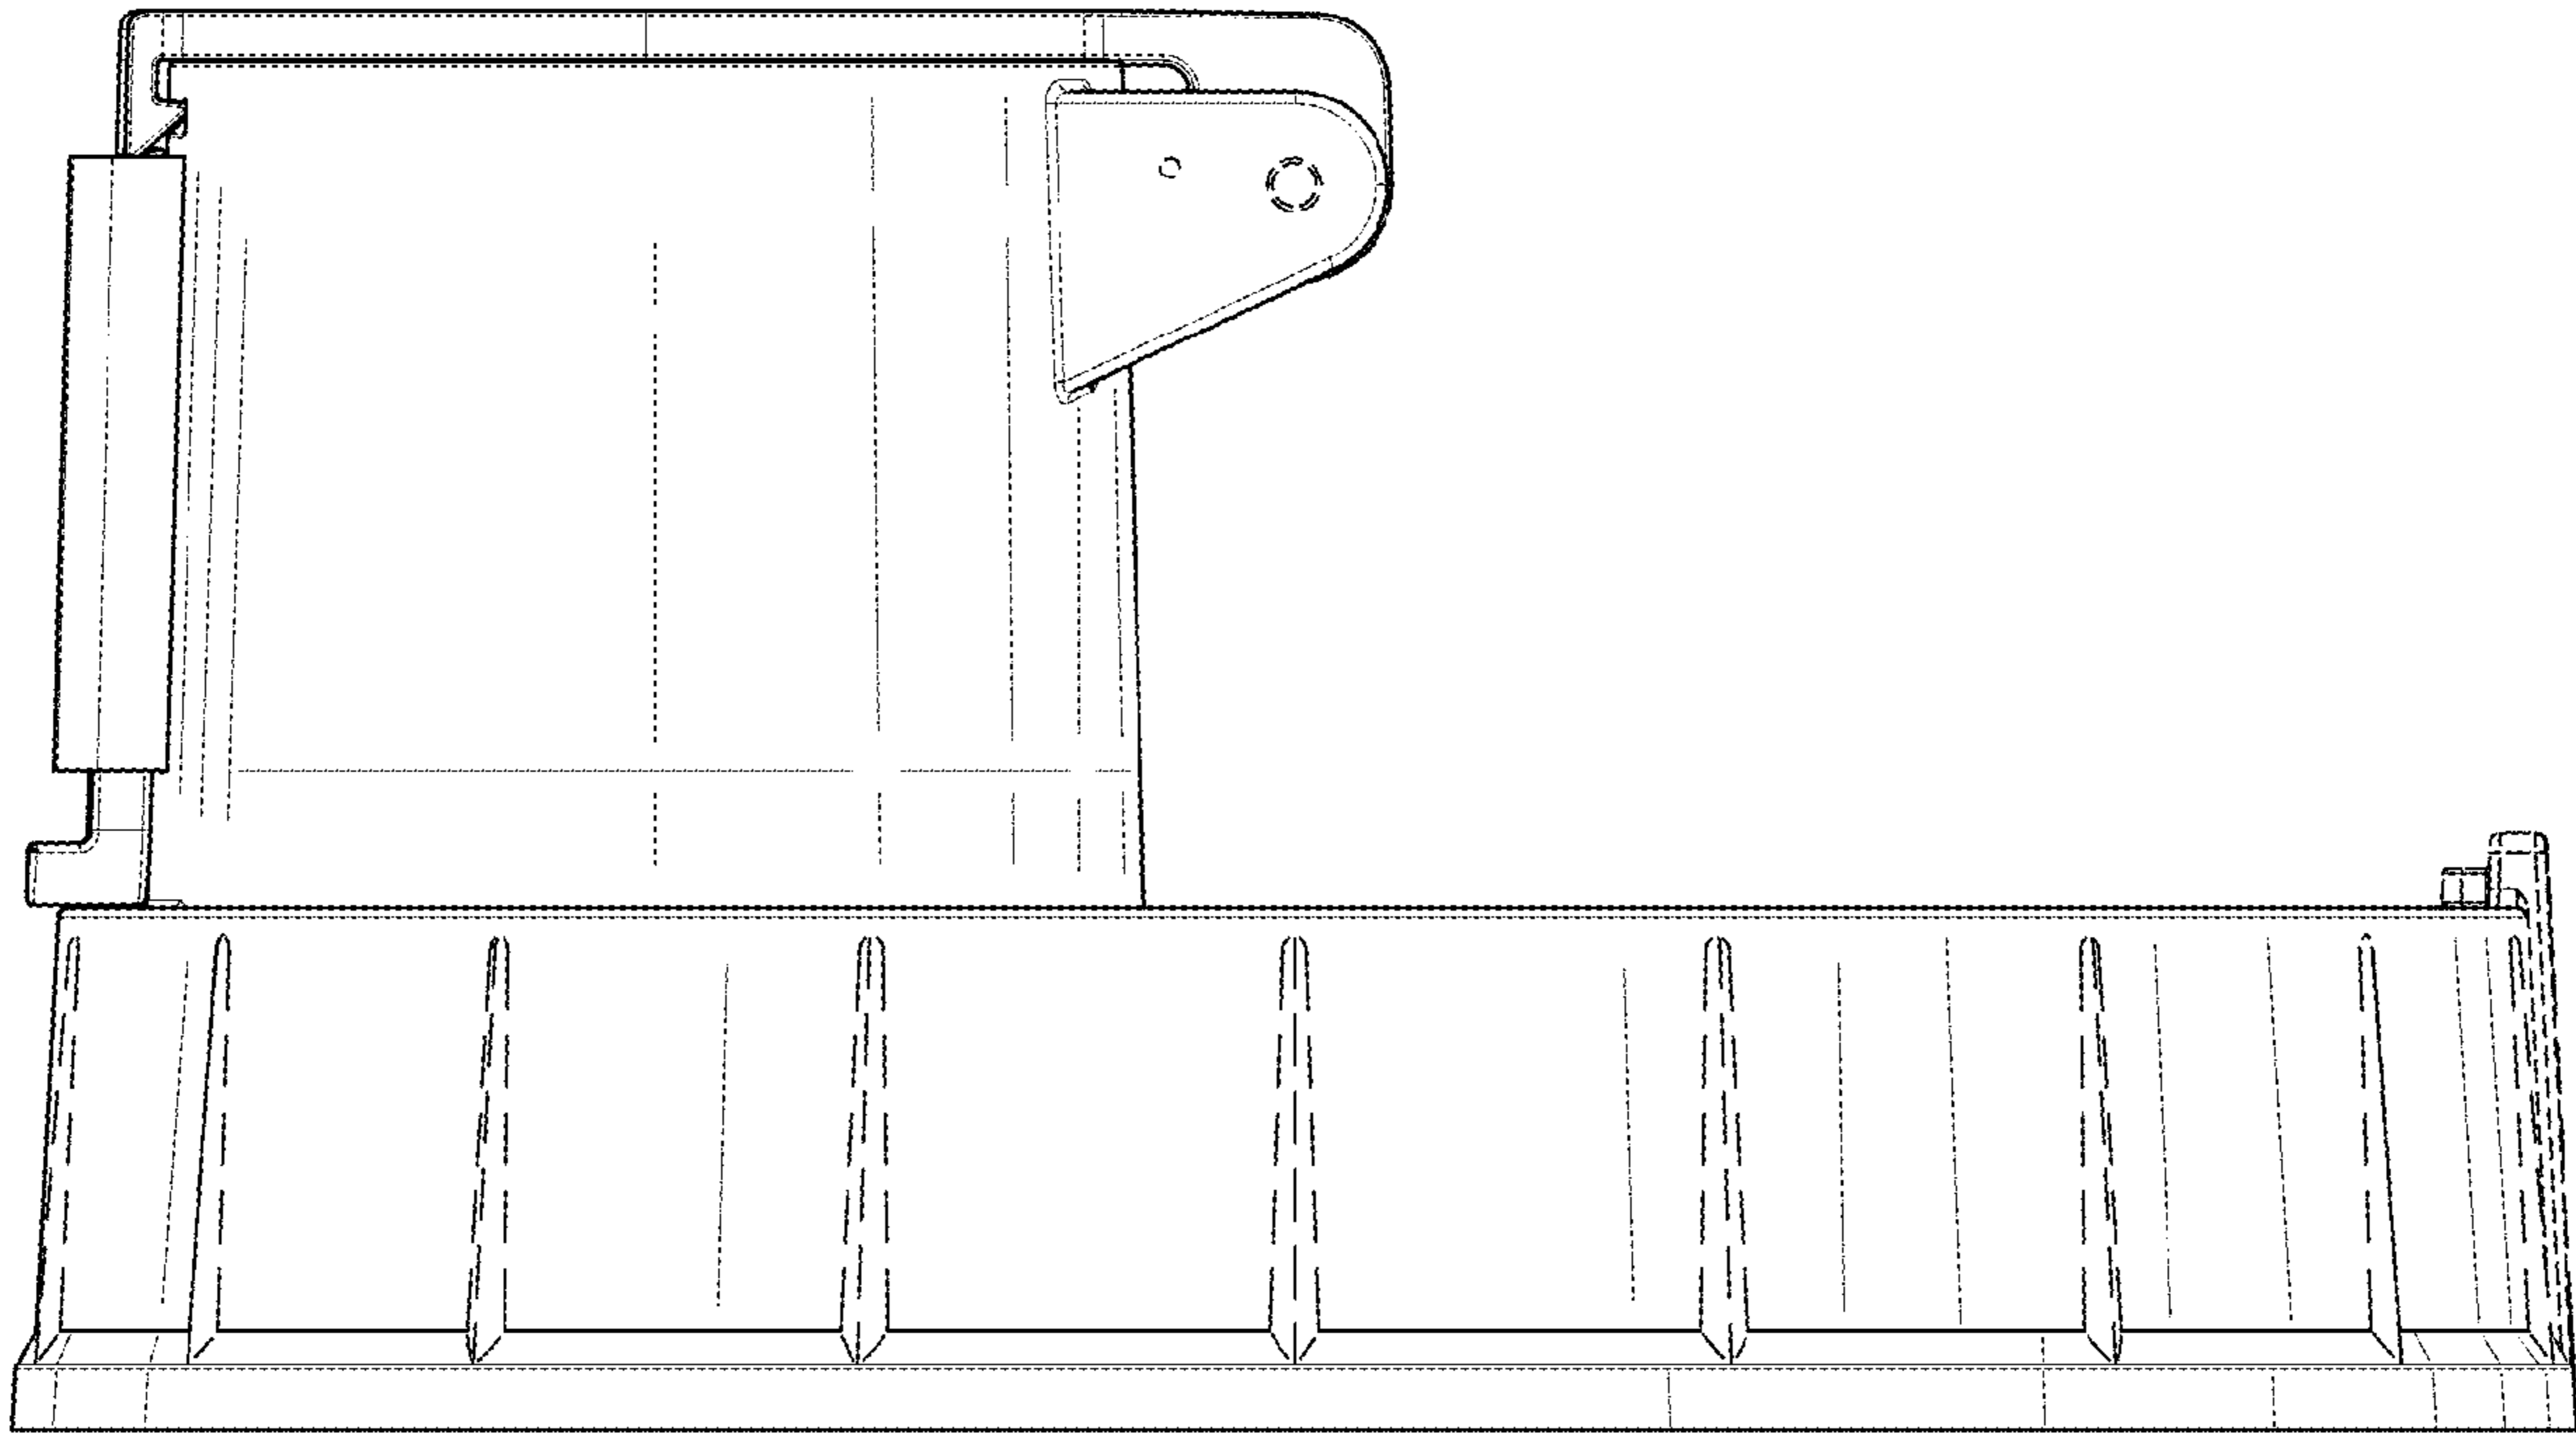


FIG. 6

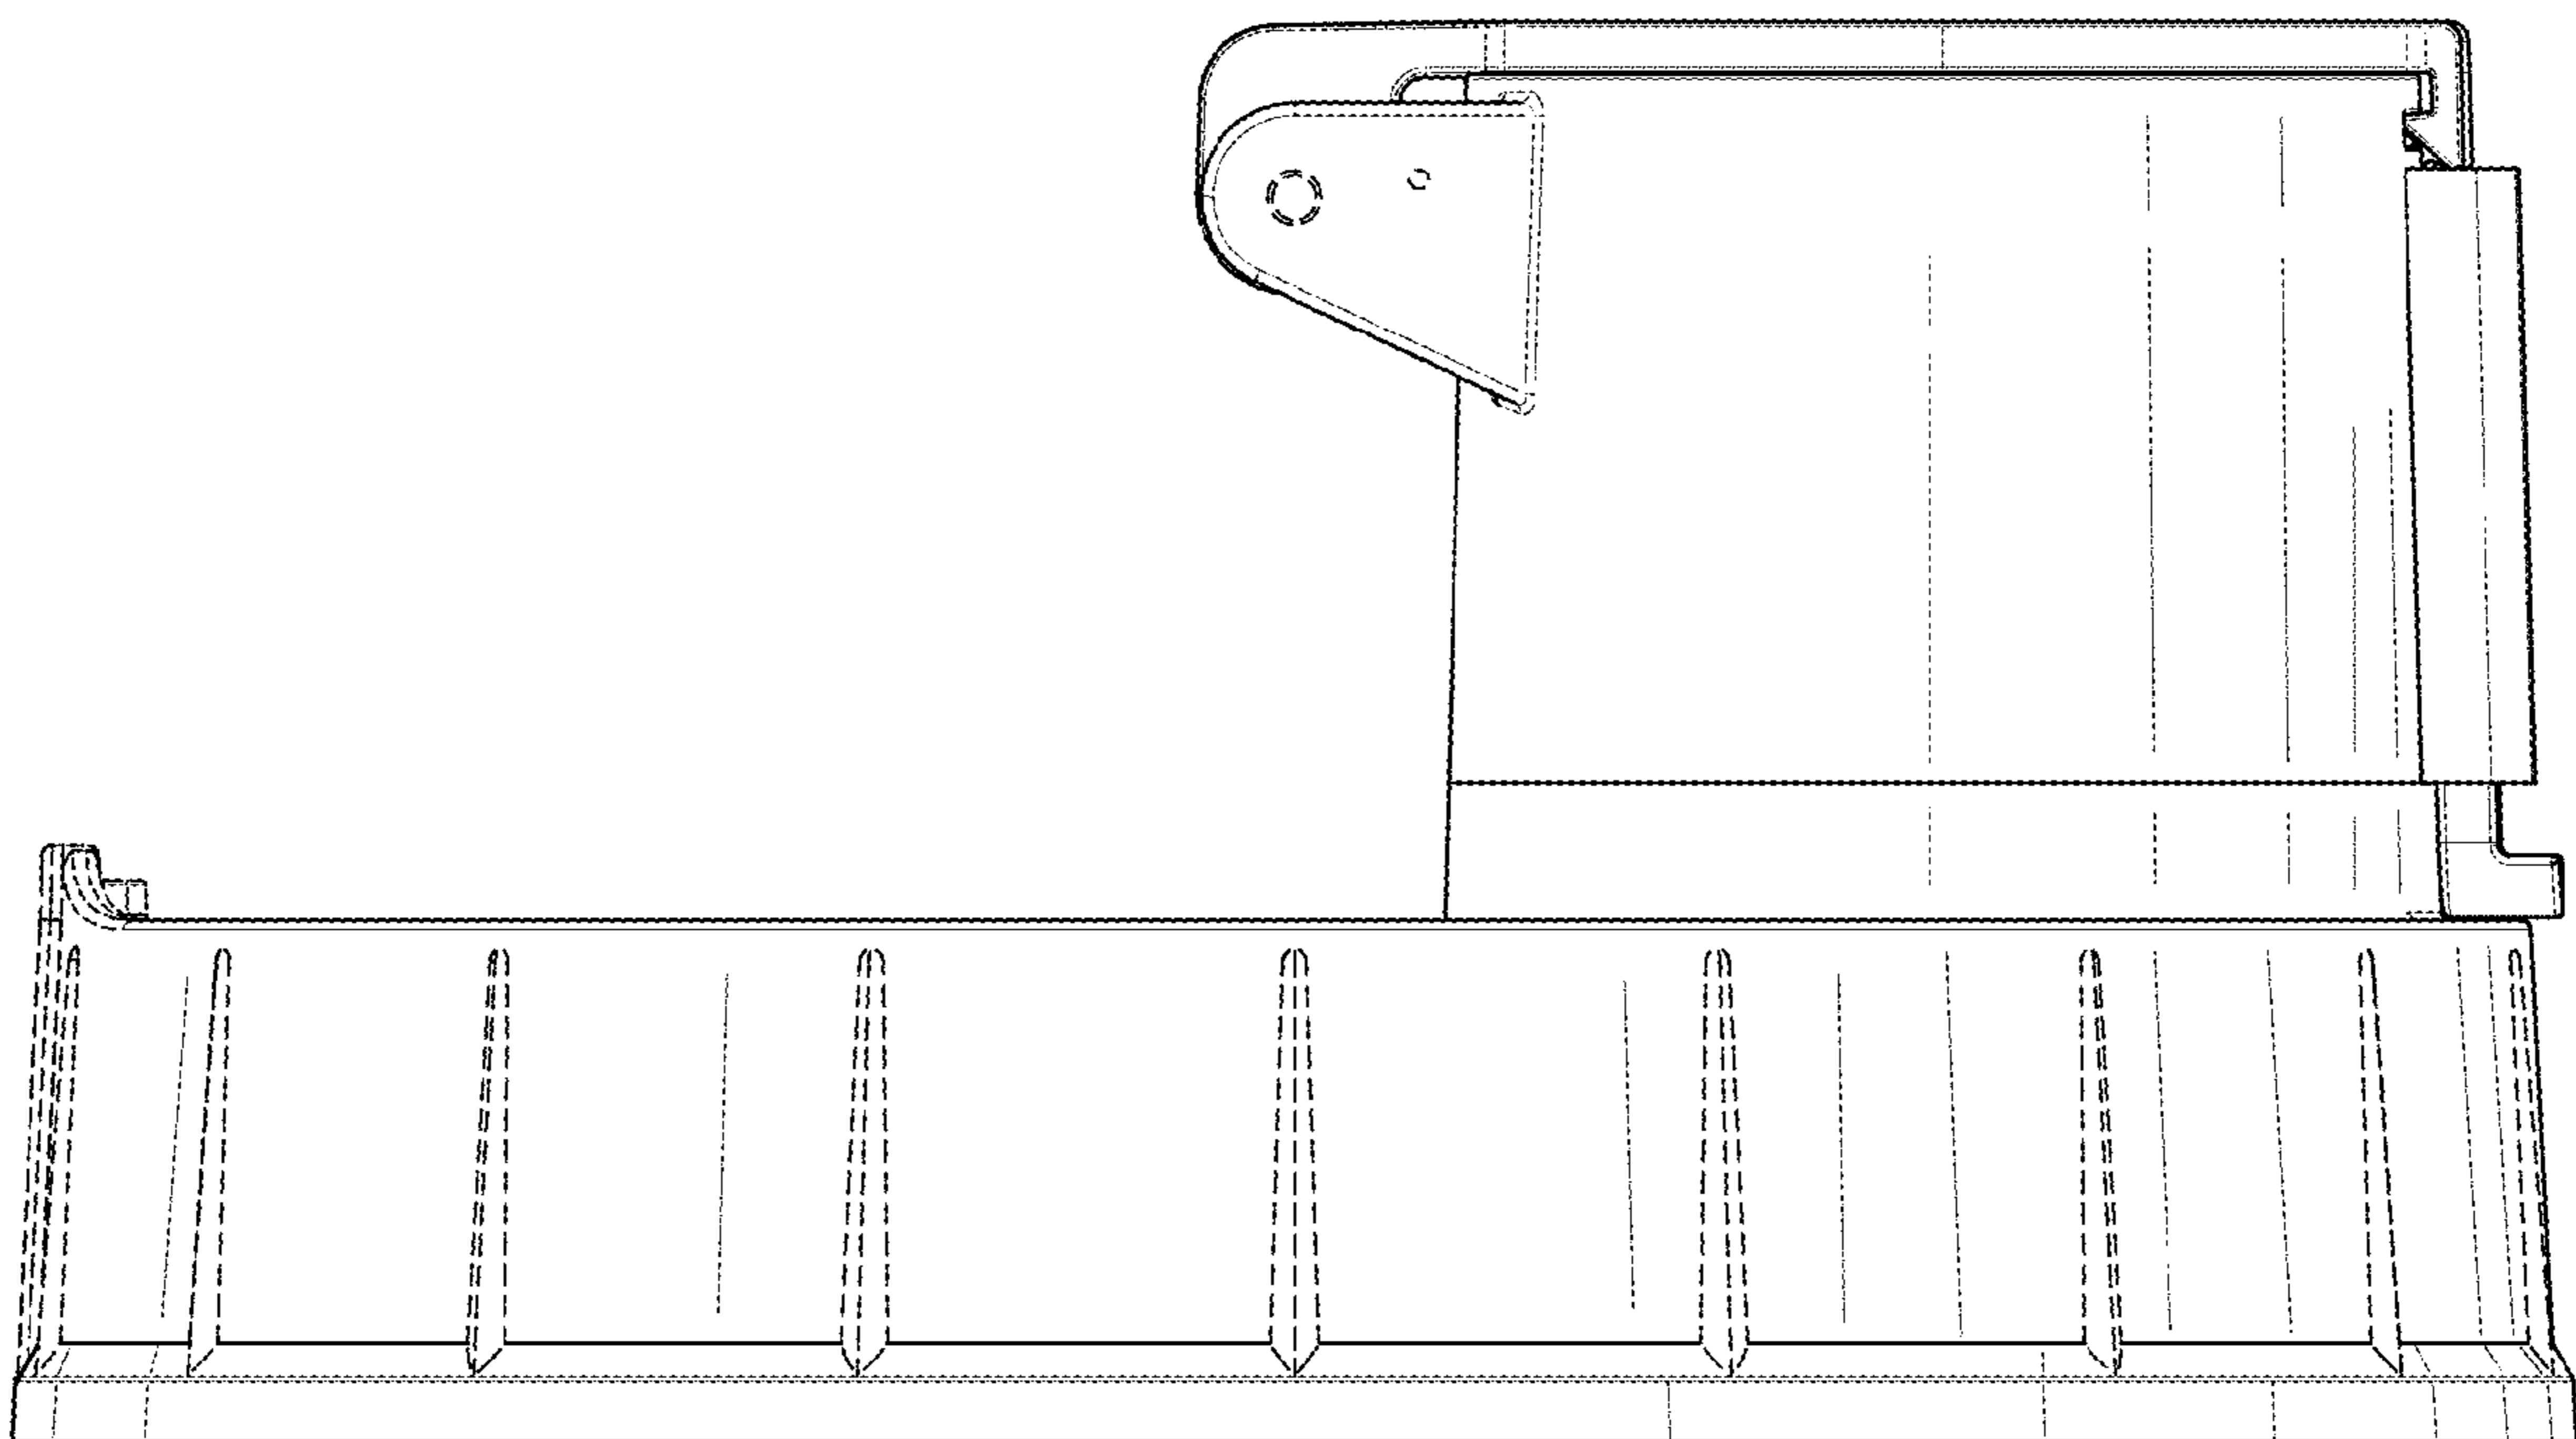


FIG. 7

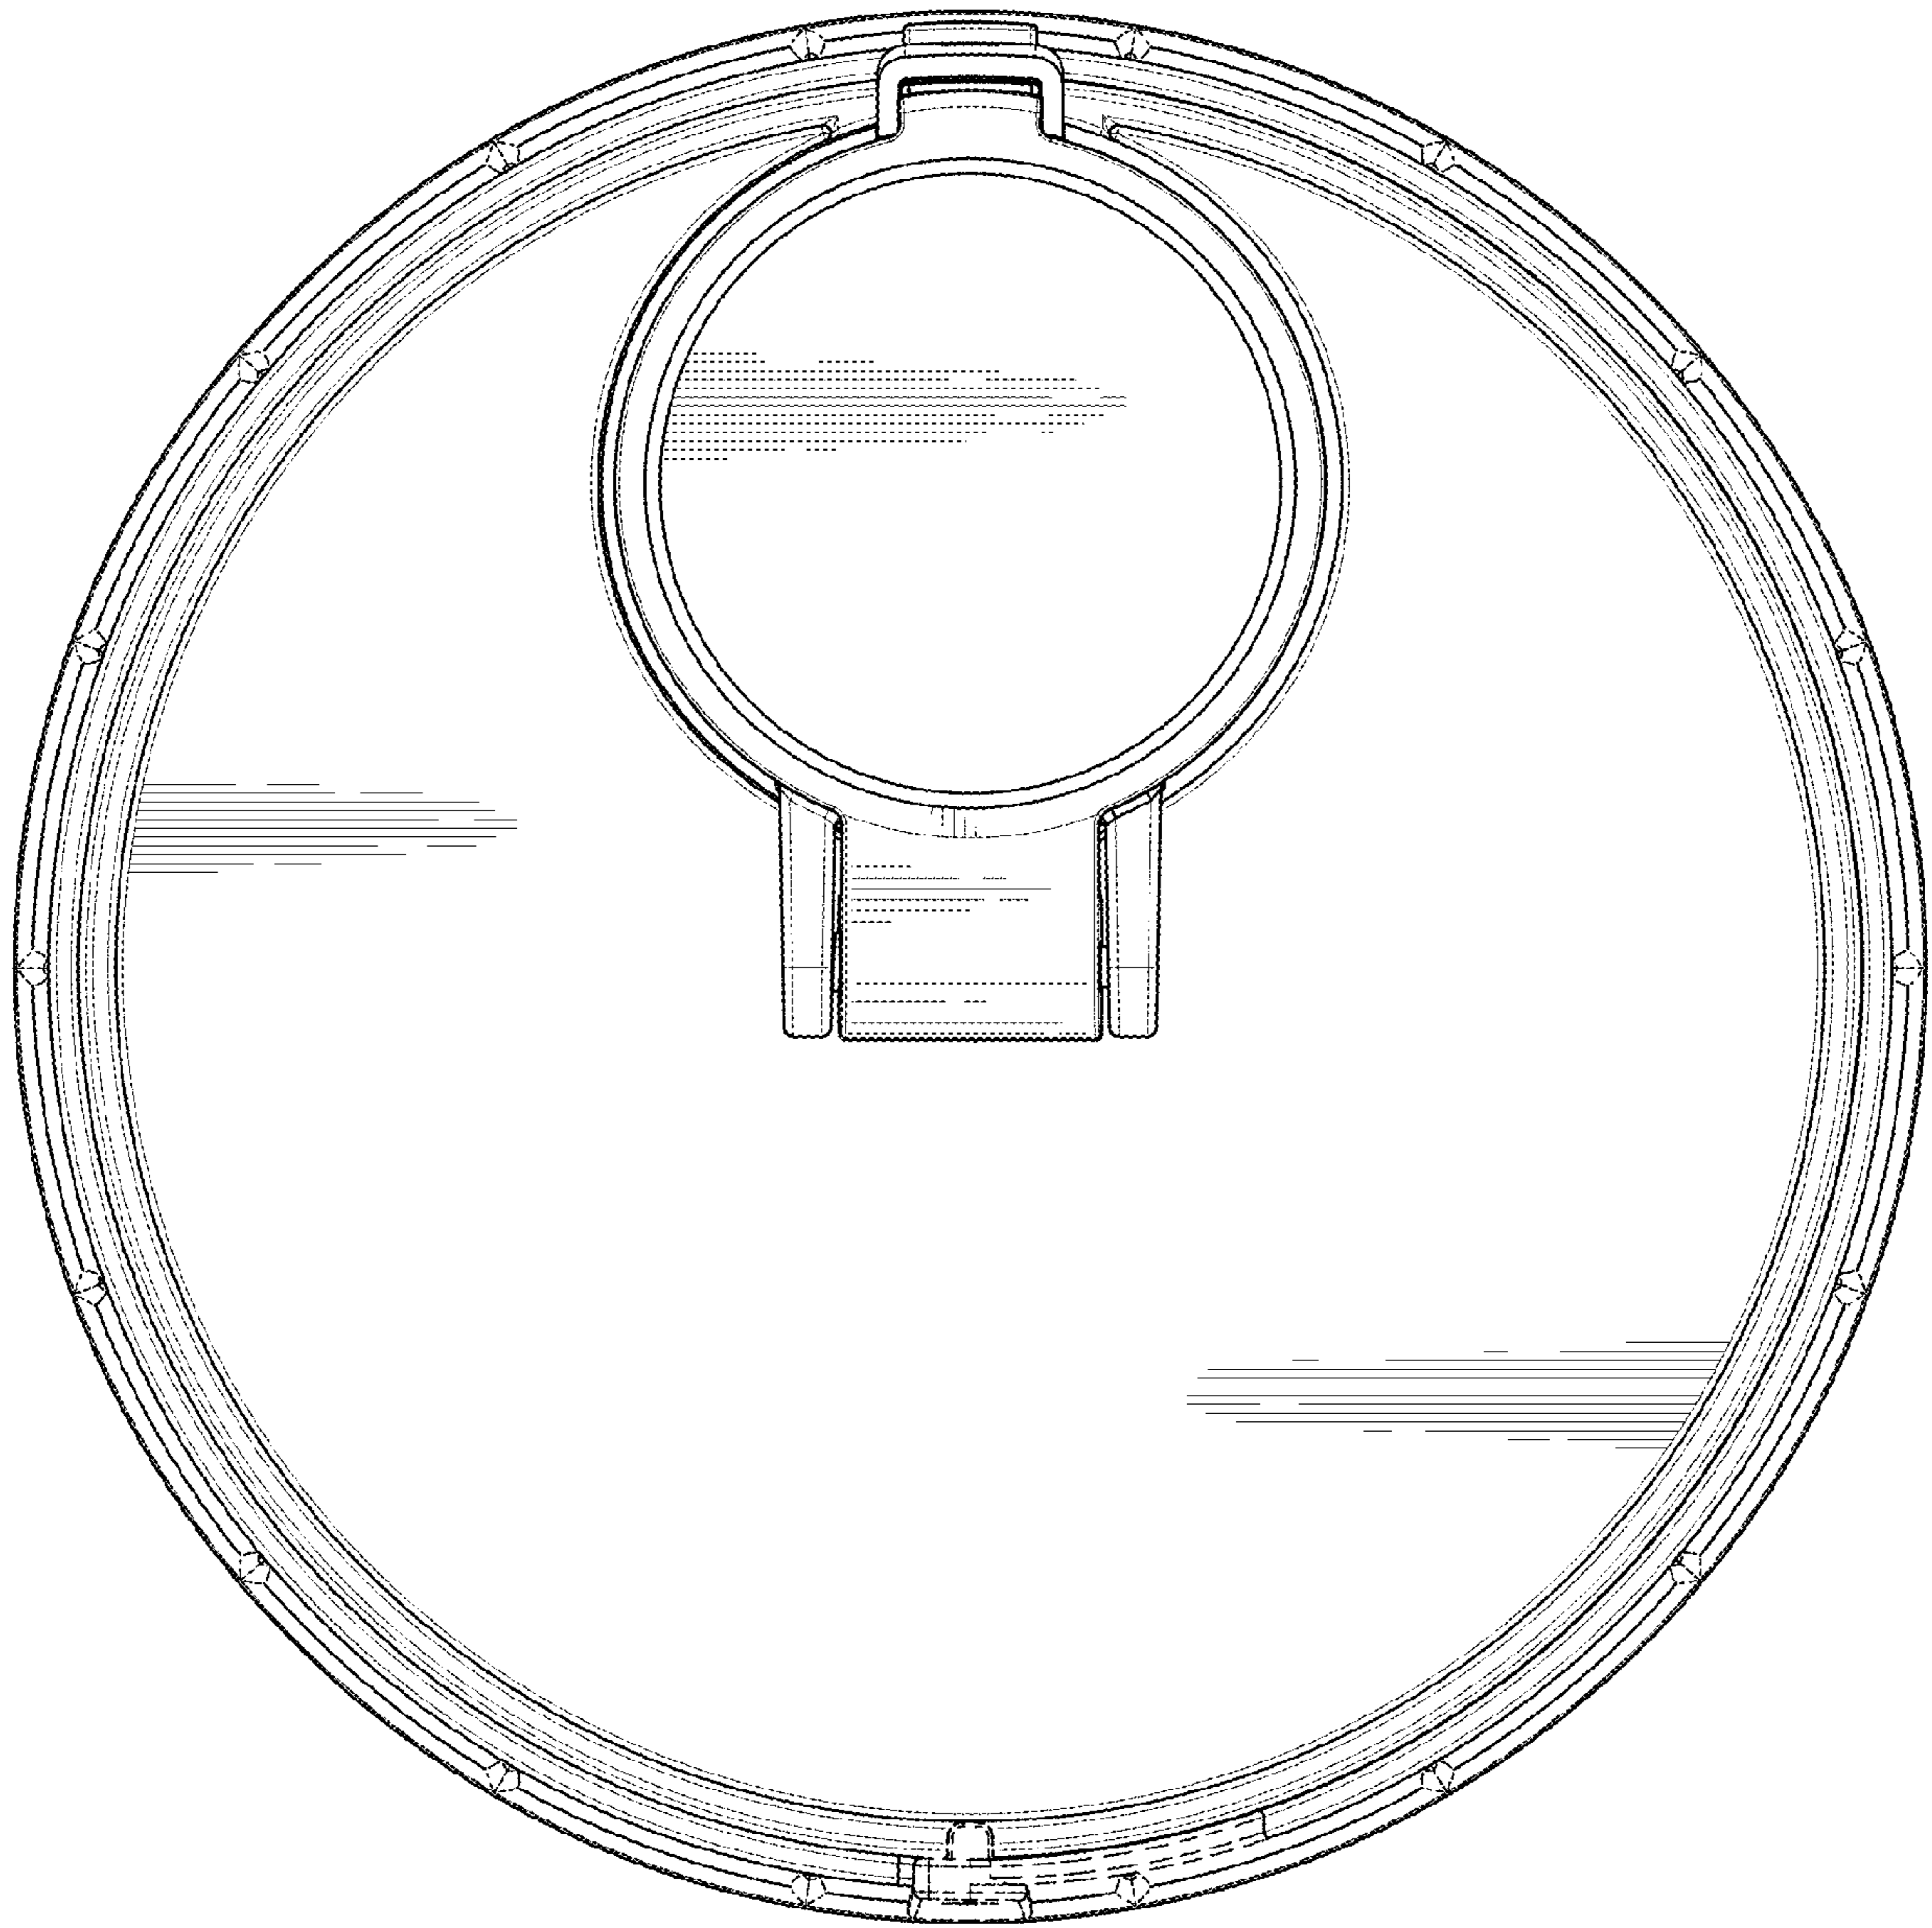


FIG. 8

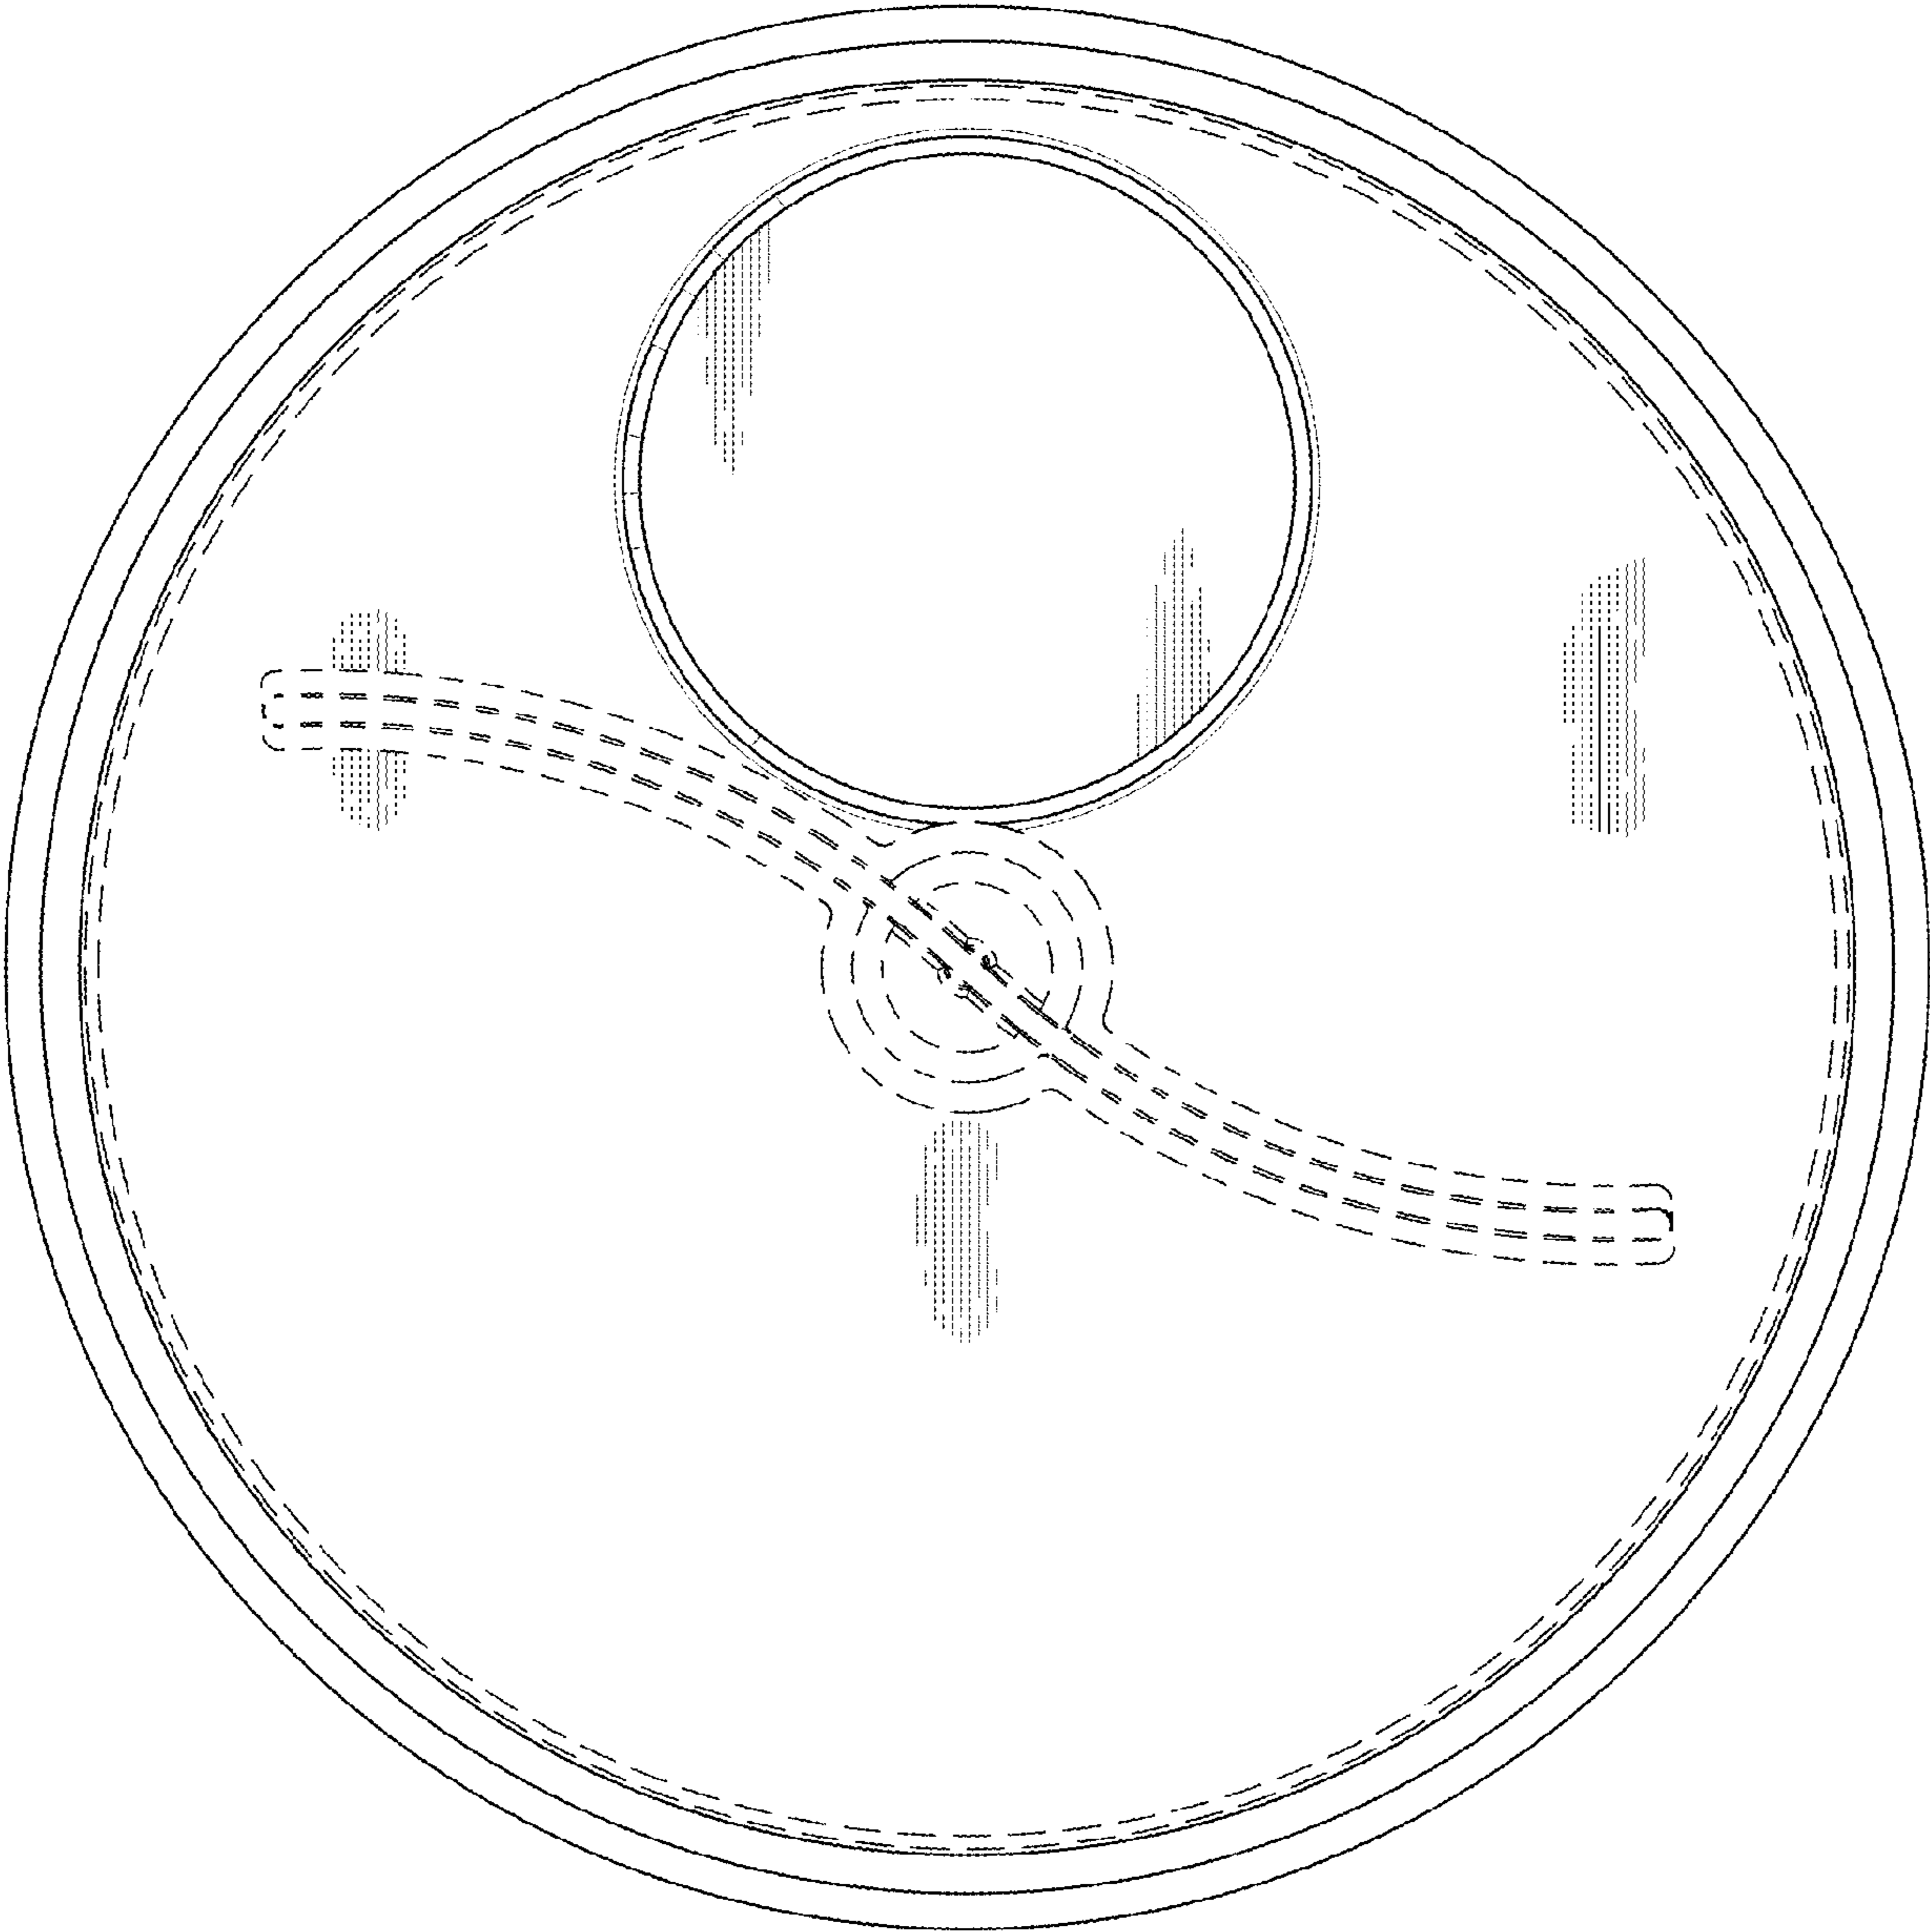


FIG. 9

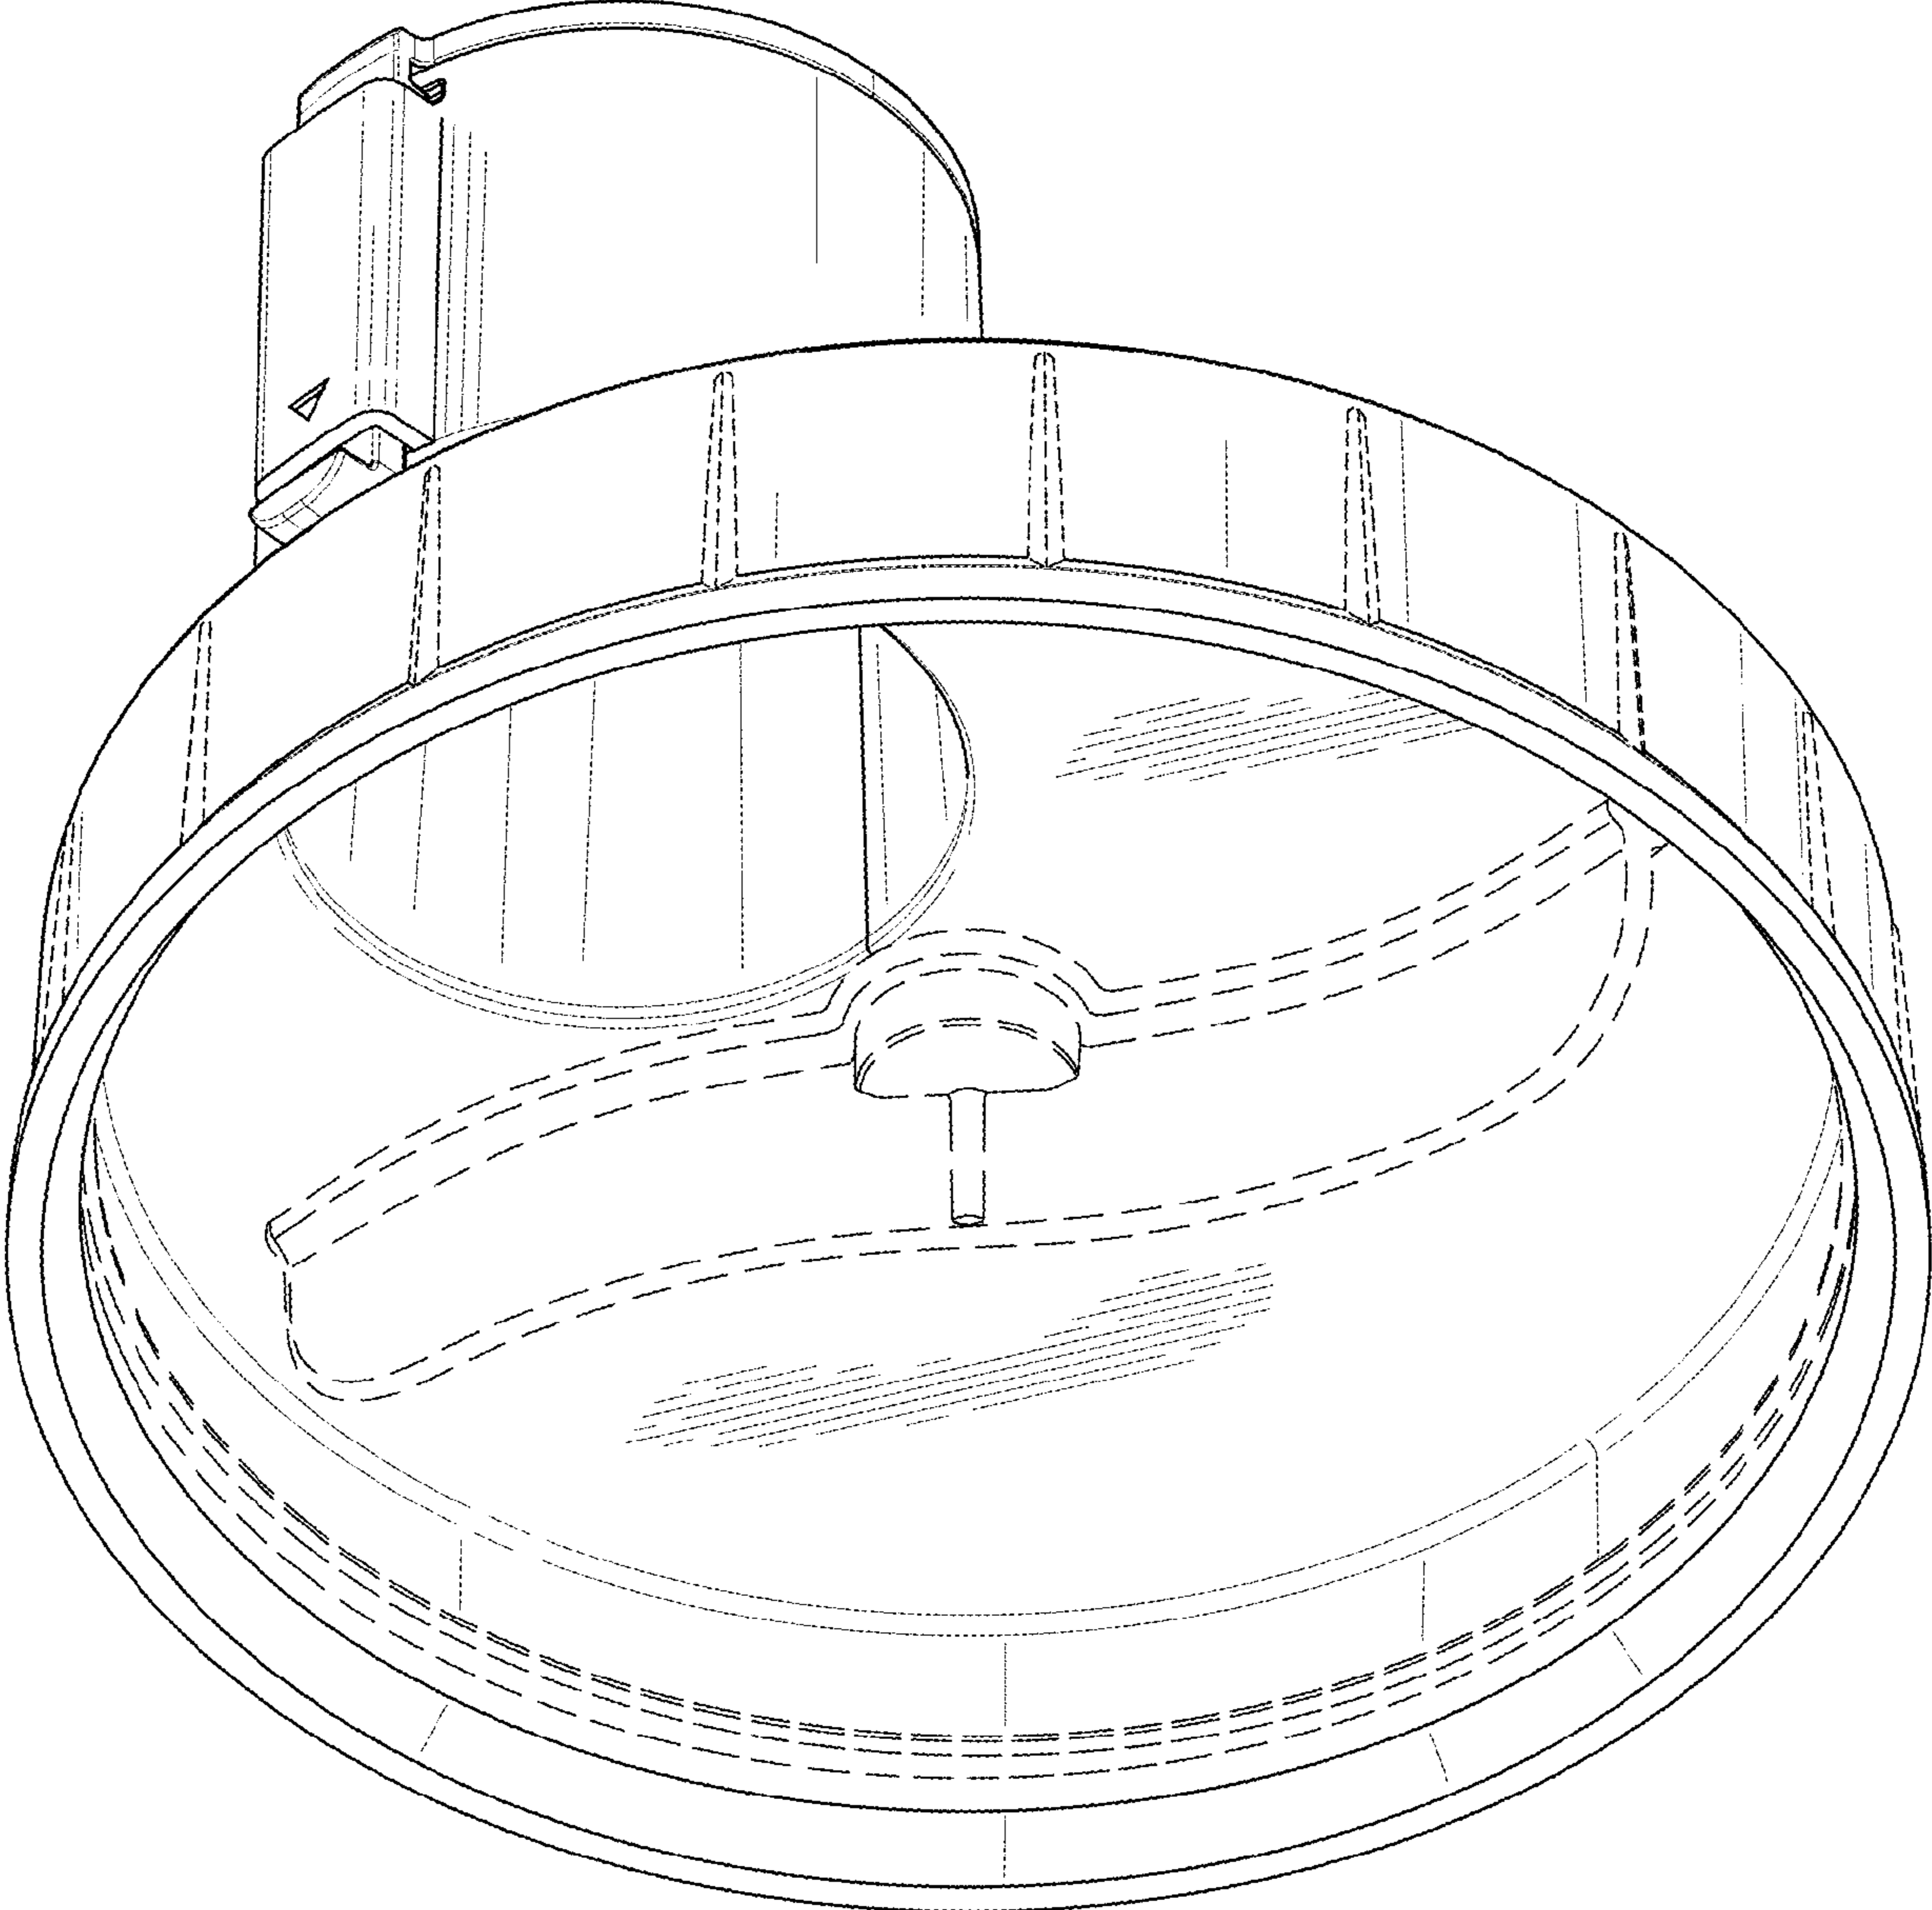


FIG. 10

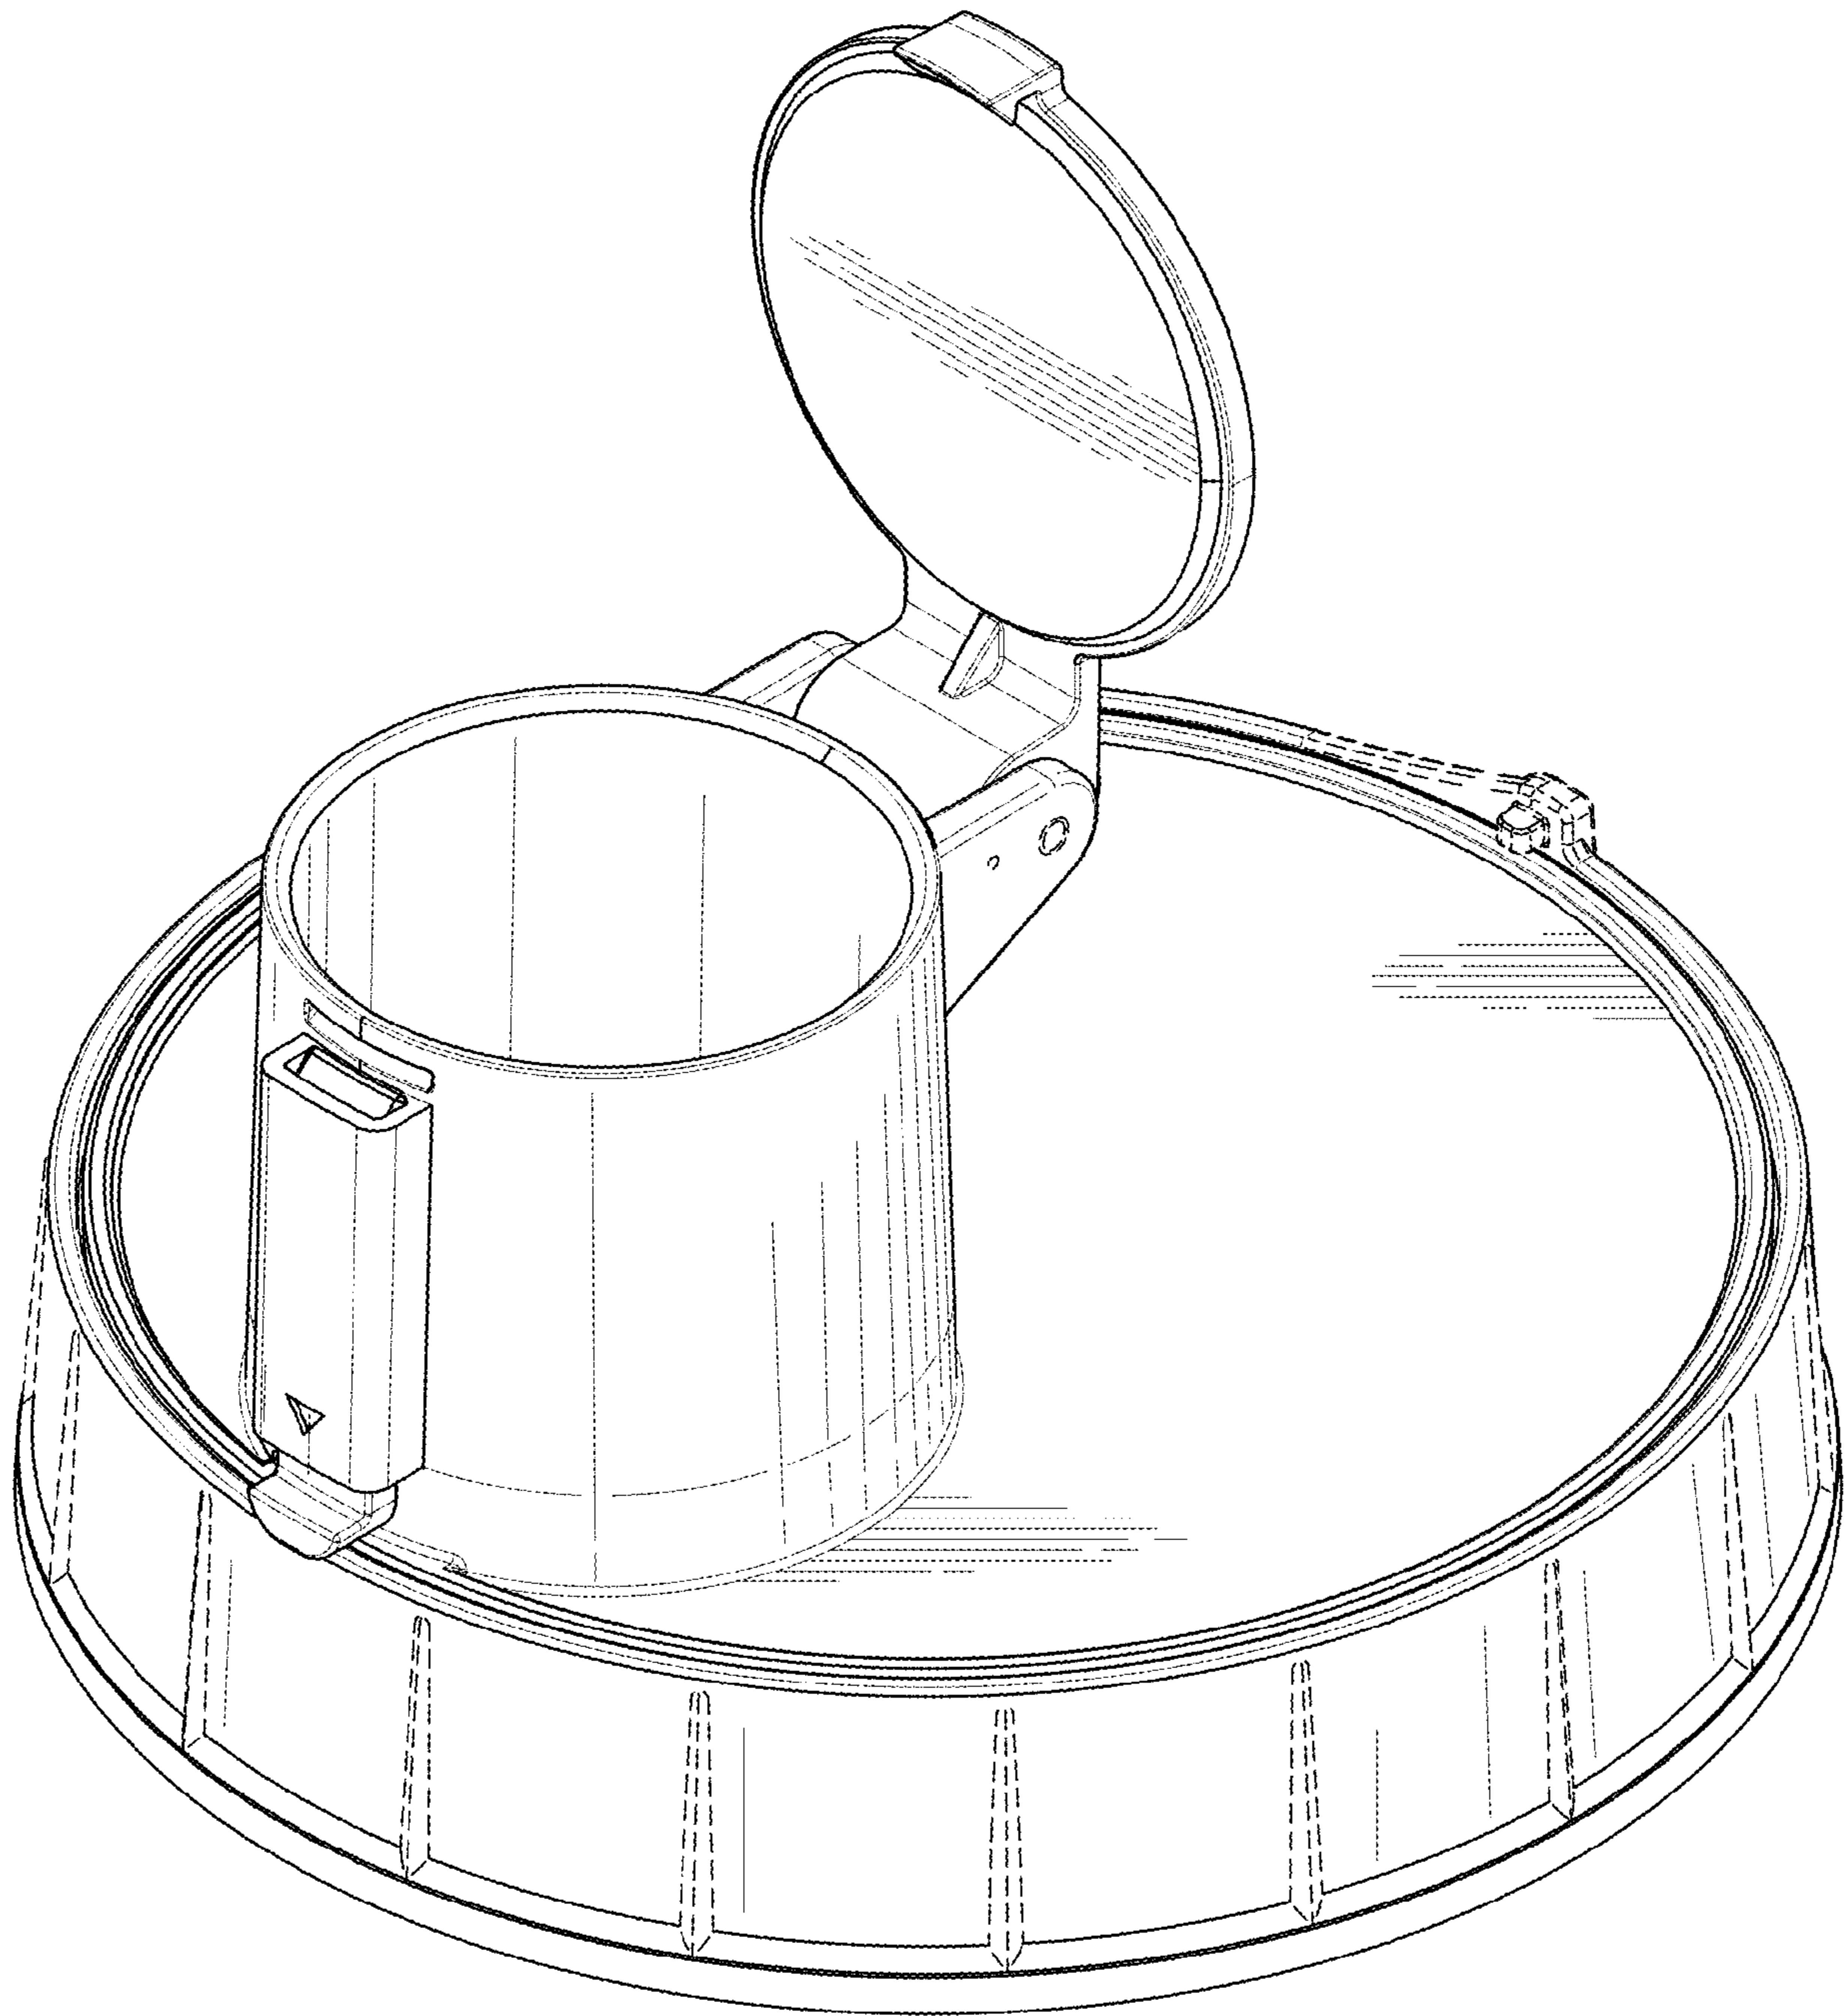


FIG. 11

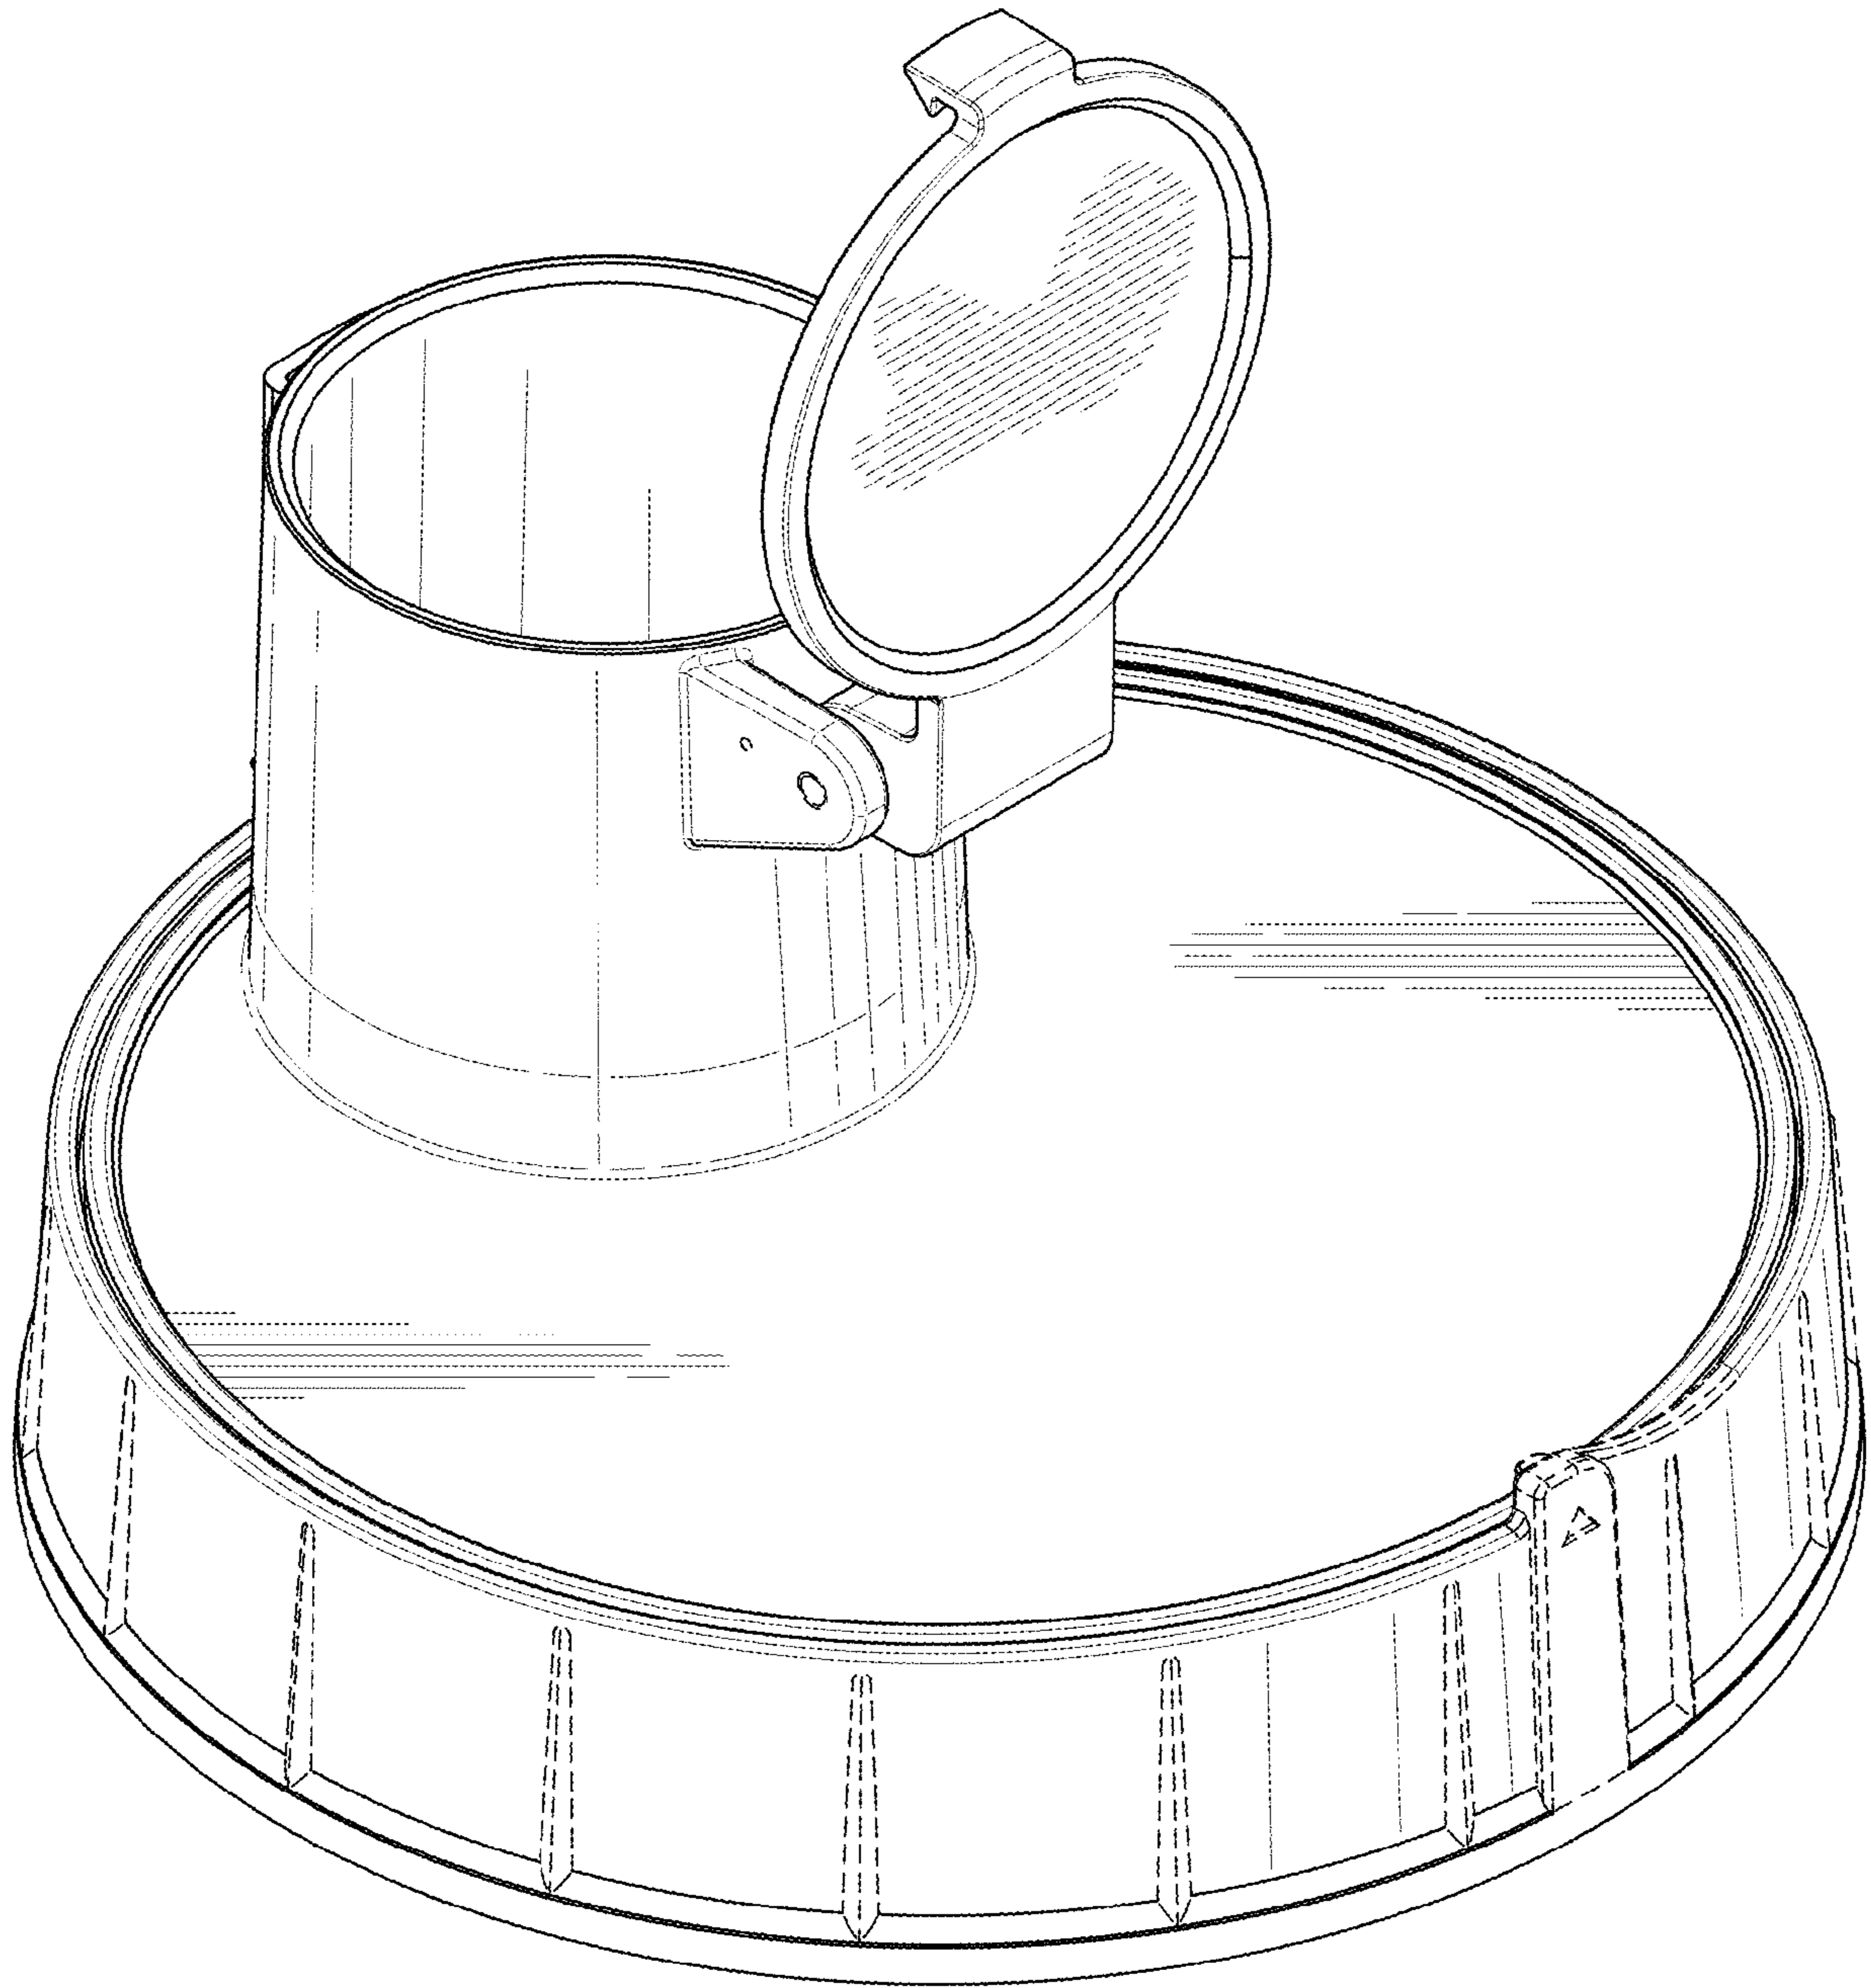


FIG. 12