



US00D898203S

(12) **United States Design Patent** (10) **Patent No.:** **US D898,203 S**
Marcil (45) **Date of Patent:** **** Oct. 6, 2020**

(54) **ULTRASOUND IMAGING PROBE HOLDER**

(71) Applicant: **Elekta LTD.**, Montreal (CA)

(72) Inventor: **Francois Marcil**, Montreal (CA)

(73) Assignee: **Elekta LTD**, Montreal, Quebec (CA)

(**) Term: **15 Years**

(21) Appl. No.: **29/635,179**

(22) Filed: **Jan. 29, 2018**

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/133, 144, 158, 169, 186, 187, 209,
D24/231; D29/130
CPC A61B 8/4218; A61B 8/4209
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,306,031 A	12/1942	Anderson et al.	
D264,874 S	6/1982	Augustsson et al.	
D286,073 S	10/1986	Russell	
4,615,516 A	10/1986	Stulberg et al.	
D310,278 S	8/1990	Quinlan	
D386,584 S	11/1997	Frei	
D393,069 S	3/1998	Jope	
D413,982 S	9/1999	Swedberg et al.	
D415,281 S	10/1999	Swedberg et al.	
5,980,828 A *	11/1999	McClintock	B01L 3/5023 422/417
D422,782 S	4/2000	Howlett et al.	
D462,446 S *	9/2002	Felix	D24/187
D463,858 S	10/2002	Sherrod et al.	
D465,577 S	11/2002	Kato et al.	
D500,142 S *	12/2004	Crisanti	D24/216
D546,956 S	7/2007	Buethorn	
D550,850 S	9/2007	Buethorn	
D551,353 S	9/2007	Buethorn	

D558,889 S *	1/2008	Doll	D24/232
D601,250 S *	9/2009	Haunschuld	D24/133
D625,421 S	10/2010	Sharps et al.	
D673,689 S *	1/2013	Pierce	D24/216
D690,016 S	9/2013	Ratner	

(Continued)

FOREIGN PATENT DOCUMENTS

CN	110090363	8/2019
WO	WO-2014018983 A1	1/2014

OTHER PUBLICATIONS

Bionix Radiation Therapy, "Comfort Hold Foot Positioner RT-6030-30-03", [Online]. Retrieved from the Internet: <URL: www.BionixRT.com>, 2 pgs.

(Continued)

Primary Examiner — Susan Bennett Hattan
Assistant Examiner — Omeed Agilee
(74) *Attorney, Agent, or Firm* — Schwegman Lundberg & Woessner, P.A.; Sanjay Agrawal


(57) **CLAIM**

The ornamental design for an ultrasound imaging probe holder, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an ultrasound imaging probe holder incorporating the design.
FIG. 2 is a top view thereof.
FIG. 3 is a bottom view thereof.
FIG. 4 is a right-side view thereof.
FIG. 5 is a left-side view thereof.
FIG. 6 is a front view thereof; and,
FIG. 7 is a back view thereof.
The broken lines shown in the drawings illustrate portions of the ultrasound imaging probe holder that form no part of the claimed design.

1 Claim, 6 Drawing Sheets

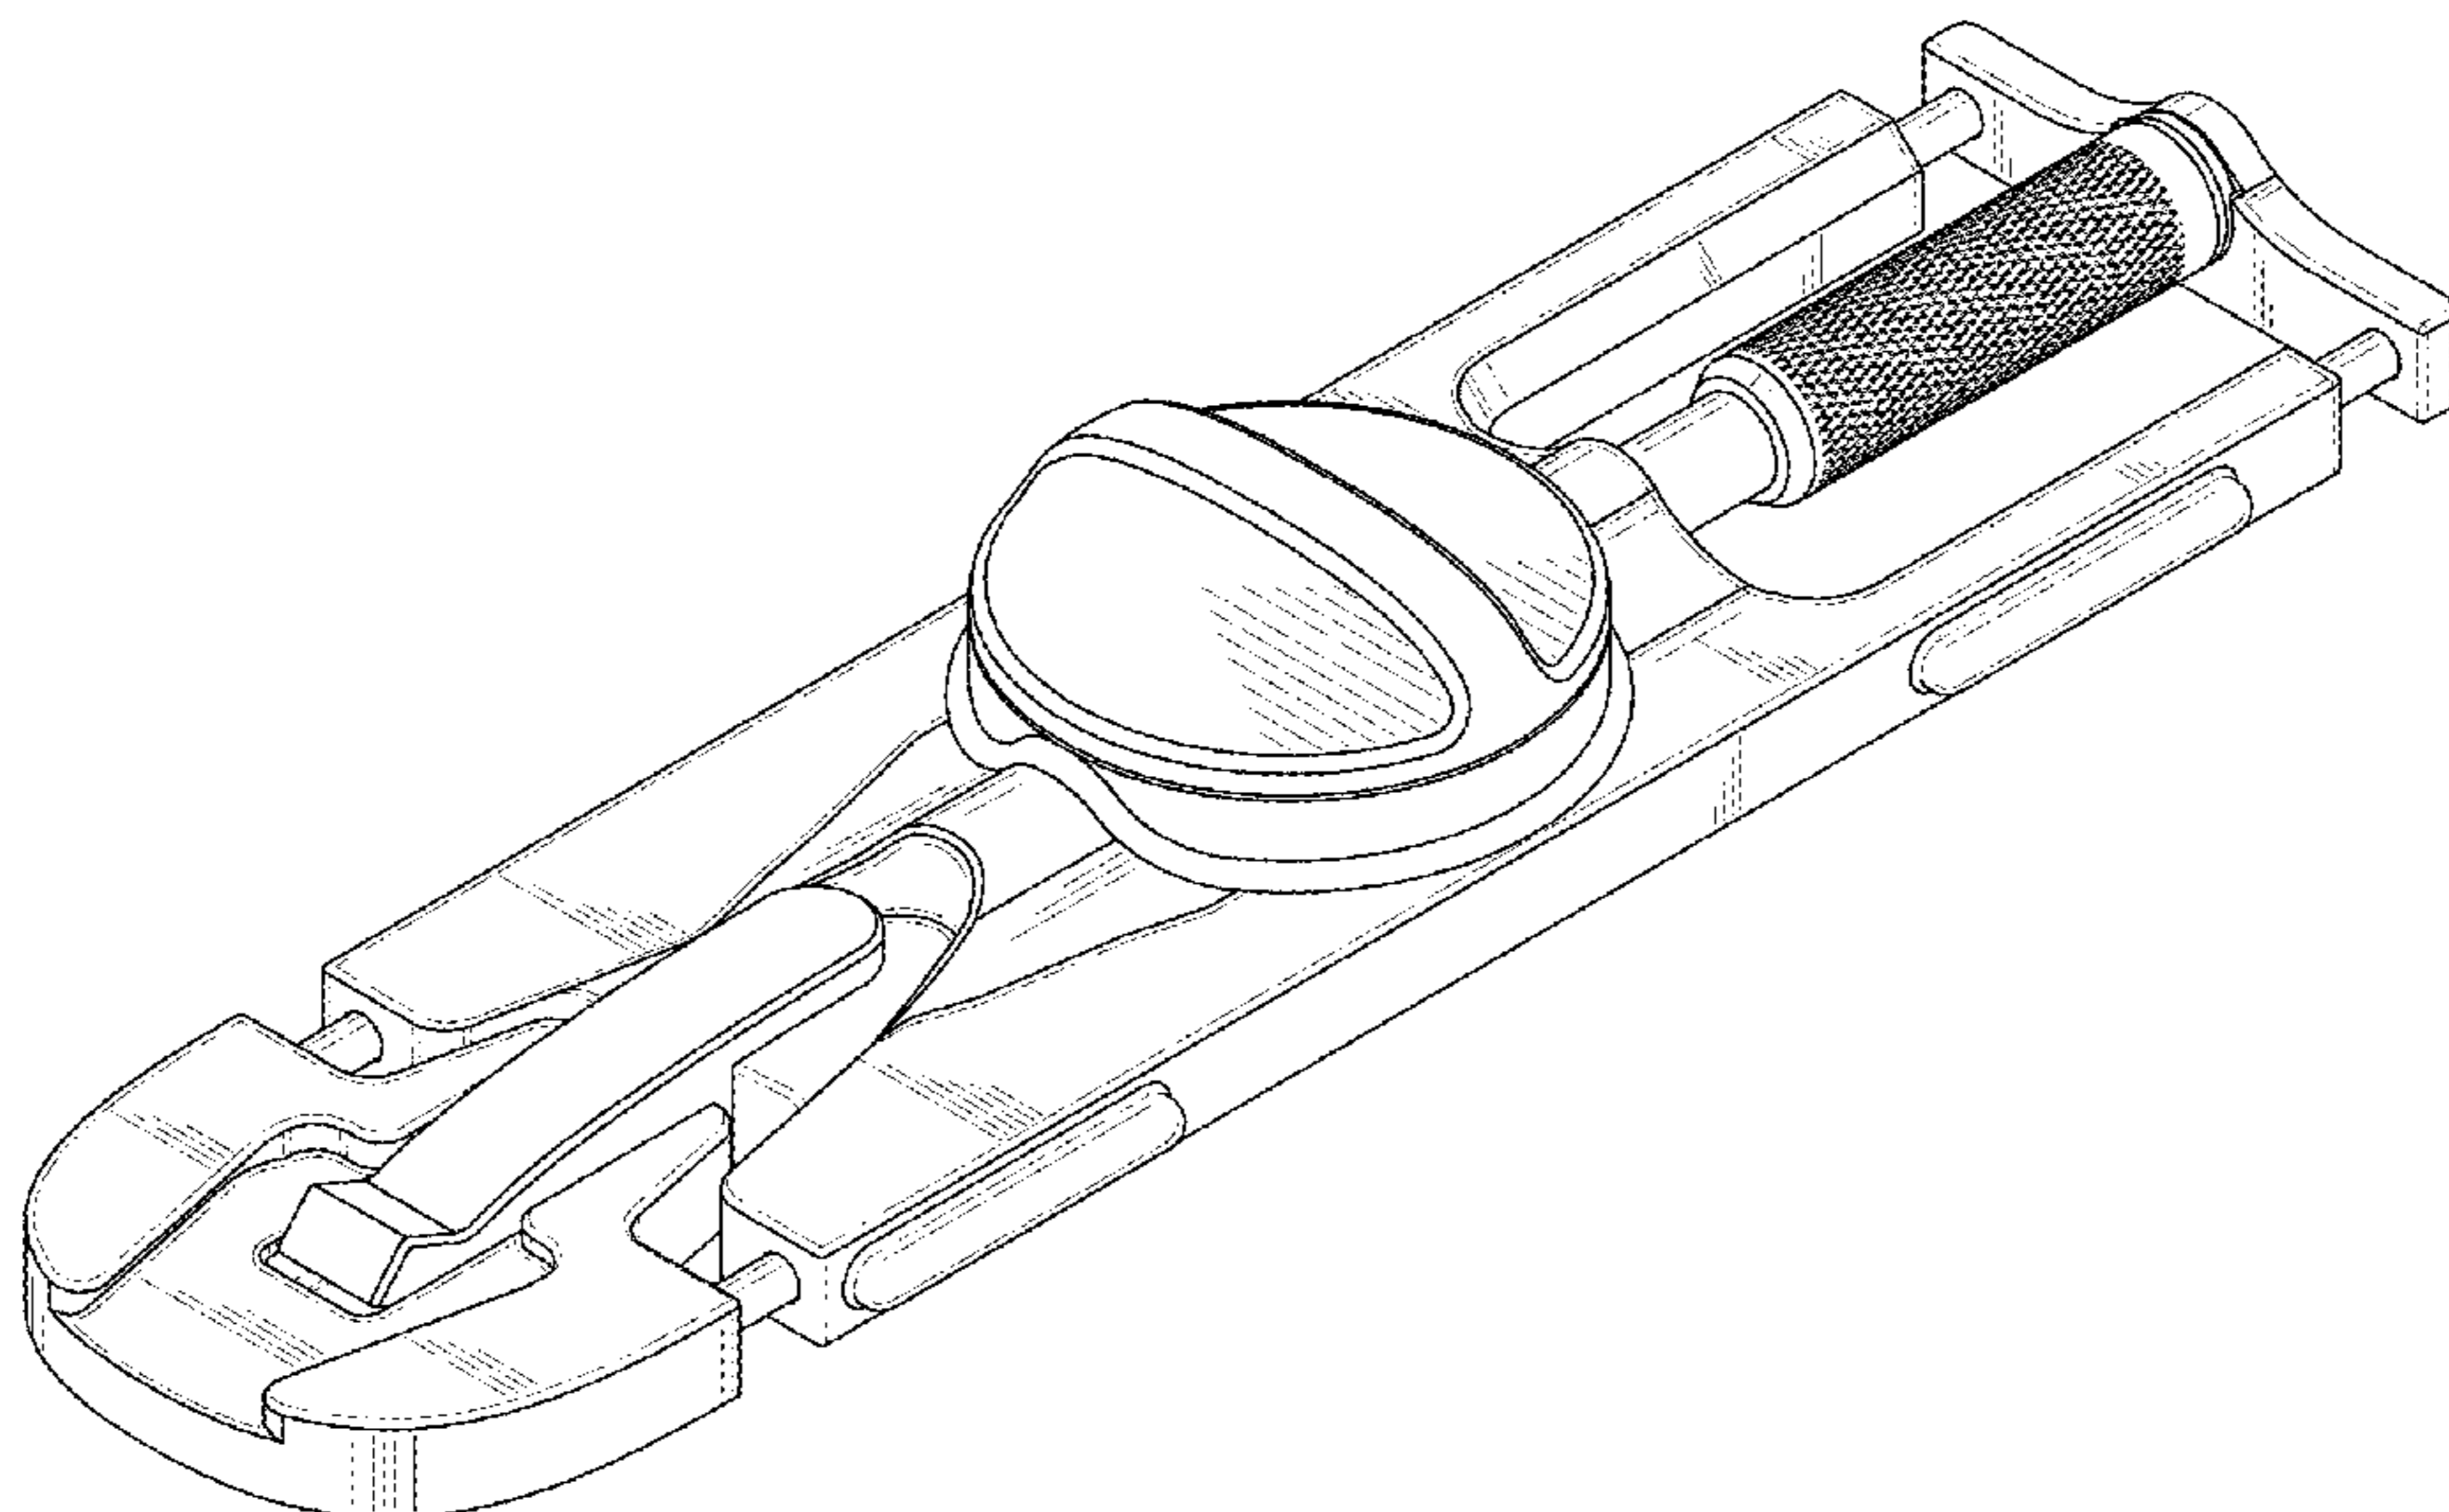

(56)

References Cited

U.S. PATENT DOCUMENTS

D709,180	S	7/2014	Rummery et al.	
D713,967	S *	9/2014	Adoni	D24/189
D728,165	S	4/2015	Davis	
D744,641	S	12/2015	Aiken	
D780,929	S *	3/2017	Nurminen	D24/184
D791,951	S *	7/2017	Henderson	D24/169
D794,205	S *	8/2017	Naber	D12/14
D800,911	S	10/2017	Diemer	
D804,045	S	11/2017	Epstein	
D810,300	S *	2/2018	Parsons	D24/169
D814,646	S	4/2018	Maloney	
D816,833	S	5/2018	Parkhurst	
9,980,573	B2	5/2018	Bennetts	
D833,623	S *	11/2018	Naber	D24/184
D834,205	S	11/2018	Ducharme et al.	
D837,386	S	1/2019	Barber et al.	
D837,392	S	1/2019	Wanner et al.	
D869,666	S	12/2019	Michaud	
D872,864	S	1/2020	Marcil	
D885,589	S	5/2020	Marcil	
D886,300	S	6/2020	Marcil	
2005/0108899	A1	5/2005	Kielt et al.	
2009/0308400	A1	12/2009	Wilson et al.	
2012/0117818	A1	5/2012	Slowik	
2013/0110019	A1 *	5/2013	Hopman	A61B 17/135 602/13
2014/0298681	A1	10/2014	Epstein	
2015/0342814	A1	12/2015	Terebuh	
2018/0250183	A1 *	9/2018	Zwierstra	A61B 5/702
2019/0231303	A1	8/2019	Marcil	
2019/0231304	A1	8/2019	Marcil	
2019/0231305	A1	8/2019	Marcil	
2019/0231306	A1	8/2019	Marcil	
2020/0054357	A1 *	2/2020	Ihatsu	A61B 8/4209

OTHER PUBLICATIONS

CDR Systems, “CDR Systems Precision Positioning Systems”, [Online]. Retrieved from the internet: <URL:www.cdrsys.ca>, 58 pgs.
 Klarity, “R634-LCF Leg Positioner Set-Up”, [Online]. Retrieved from the Internet:<URL: www.klaritymedical.com>, 1 pg.
 “U.S. Appl. No. 29/635,182, Non Final Office Action dated Apr. 26, 2019”, 11 pgs.
 “U.S. Appl. No. 29/635,185, Non Final Office Action dated May 16, 2019”, 16 pgs.
 “U.S. Appl. No. 29/635,186, Non Final Office Action dated May 16, 2019”, 12 pgs.
 “Chinese Application Serial No. 201910080350.6, Notification on Correction of Deficiencies dated Mar. 12, 2019”, w/o English translation, 1 pg.
 “European Application Serial No. 19153998.0, Extended European Search Report dated Jun. 28, 2019”, 11 pgs.

“RayBoards for Butterfly Masks with L-Profiles”, [Online] Retrieved from the Internet:<https://www.bcc.taipei/RTproducts/product_pp121a.html>, (accessed Mar. 19, 2019), 1.
 “Zephyr Patient Positioning and Transfer Systems—Orfit Industries”, Retrieved from the Internet: <URL:https://www.orfit.com/radiation-oncology/products/zephyrpatient-positioning-and-transfer-systems/>, (May 30, 2017).
 Camps, Saskia M, et al., “The Use of Ultrasound Imaging in the External Beam Radiotherapy Workflow of Prostate Cancer Patients”, Biomed Research International, vol. (Jan. 1, 2018), 1-16.
 Elekta, “Clarity for Prostate Monitoring”, Youtube, Retrieved from the Internet: <URL:https://www.youtube.com/watch?time_continue=35&v=htoFAd1 ALw8>, (Sep. 22, 2015).
 Elekta, “Prostate Intra-Fractional Motion Management”, Youtube, Retrieved from the Internet: <URL:https://www.youtube.com/watch?v=Qr8z5ELbQJw>, (Feb. 3, 2016).
 Lachaine, Martin, et al., “Intrafractional Prostate Motion Management With The Clarity Autoscan System”, Medical Physics International Journal, (Jan. 1, 2013), 72.
 Zephyr, “Patient Positioning and Transfer System”, Youtube, Retrieved from the Internet: URL:<https://www.youtube.com/watch?time_continue=111&v=SaKI8ceQirY>, (May 30, 2017).
 “U.S. Appl. No. 29/635,182, Response filed Aug. 12, 2019 to Non Final Office Action dated Apr. 26, 2019”, 5 pgs.
 “U.S. Appl. No. 29/635,185, Response filed Aug. 14, 2019 to Non Final Office Action dated May 16, 2019”, 5 pgs.
 “U.S. Appl. No. 29/635,186, Response filed Aug. 14, 2019 to Non Final Office Action dated May 16, 2019”, 7 pgs.
 “U.S. Appl. No. 29/635,182, Notice of Allowance dated Sep. 3, 2019”, 7 pgs.
 “U.S. Appl. No. 29/635,186, Final Office Action dated Nov. 5, 2019”, 7 pgs.
 “U.S. Appl. No. 29/635,185, Final Office Action dated Nov. 21, 2019”.
 “U.S. Appl. No. 29/635,182, Corrected Notice of Allowability dated Dec. 11, 2019”, 4 pgs.
 “European Application Serial No. 19153998.0, Response filed Jan. 31, 2020 to Extended European Search Report dated Jun. 28, 2019”, 11 pgs.
 “U.S. Appl. No. 29/635,186, Response filed Feb. 3, 2020 to Final Office Action dated Nov. 5, 2019”, 6 pgs.
 “U.S. Appl. No. 29/635,185, Response filed Feb. 17, 2020 to Final Office Action dated Nov. 21, 2019”.
 “U.S. Appl. No. 15/898,503, Non Final Office Action dated Jun. 11, 2020”, 9 pgs.
 “U.S. Appl. No. 29/635,185, Notice of Allowance dated Mar. 27, 2020”, 7 pgs.
 “U.S. Appl. No. 29/635,185, PTO Response to Rule 312 Communication dated Apr. 29, 2020”.
 “U.S. Appl. No. 29/635,186, Corrected Notice of Allowability dated Apr. 29, 2020”, 2 pgs.
 “U.S. Appl. No. 29/635,186, Notice of Allowance dated Apr. 3, 2020”, 8 pgs.

* cited by examiner

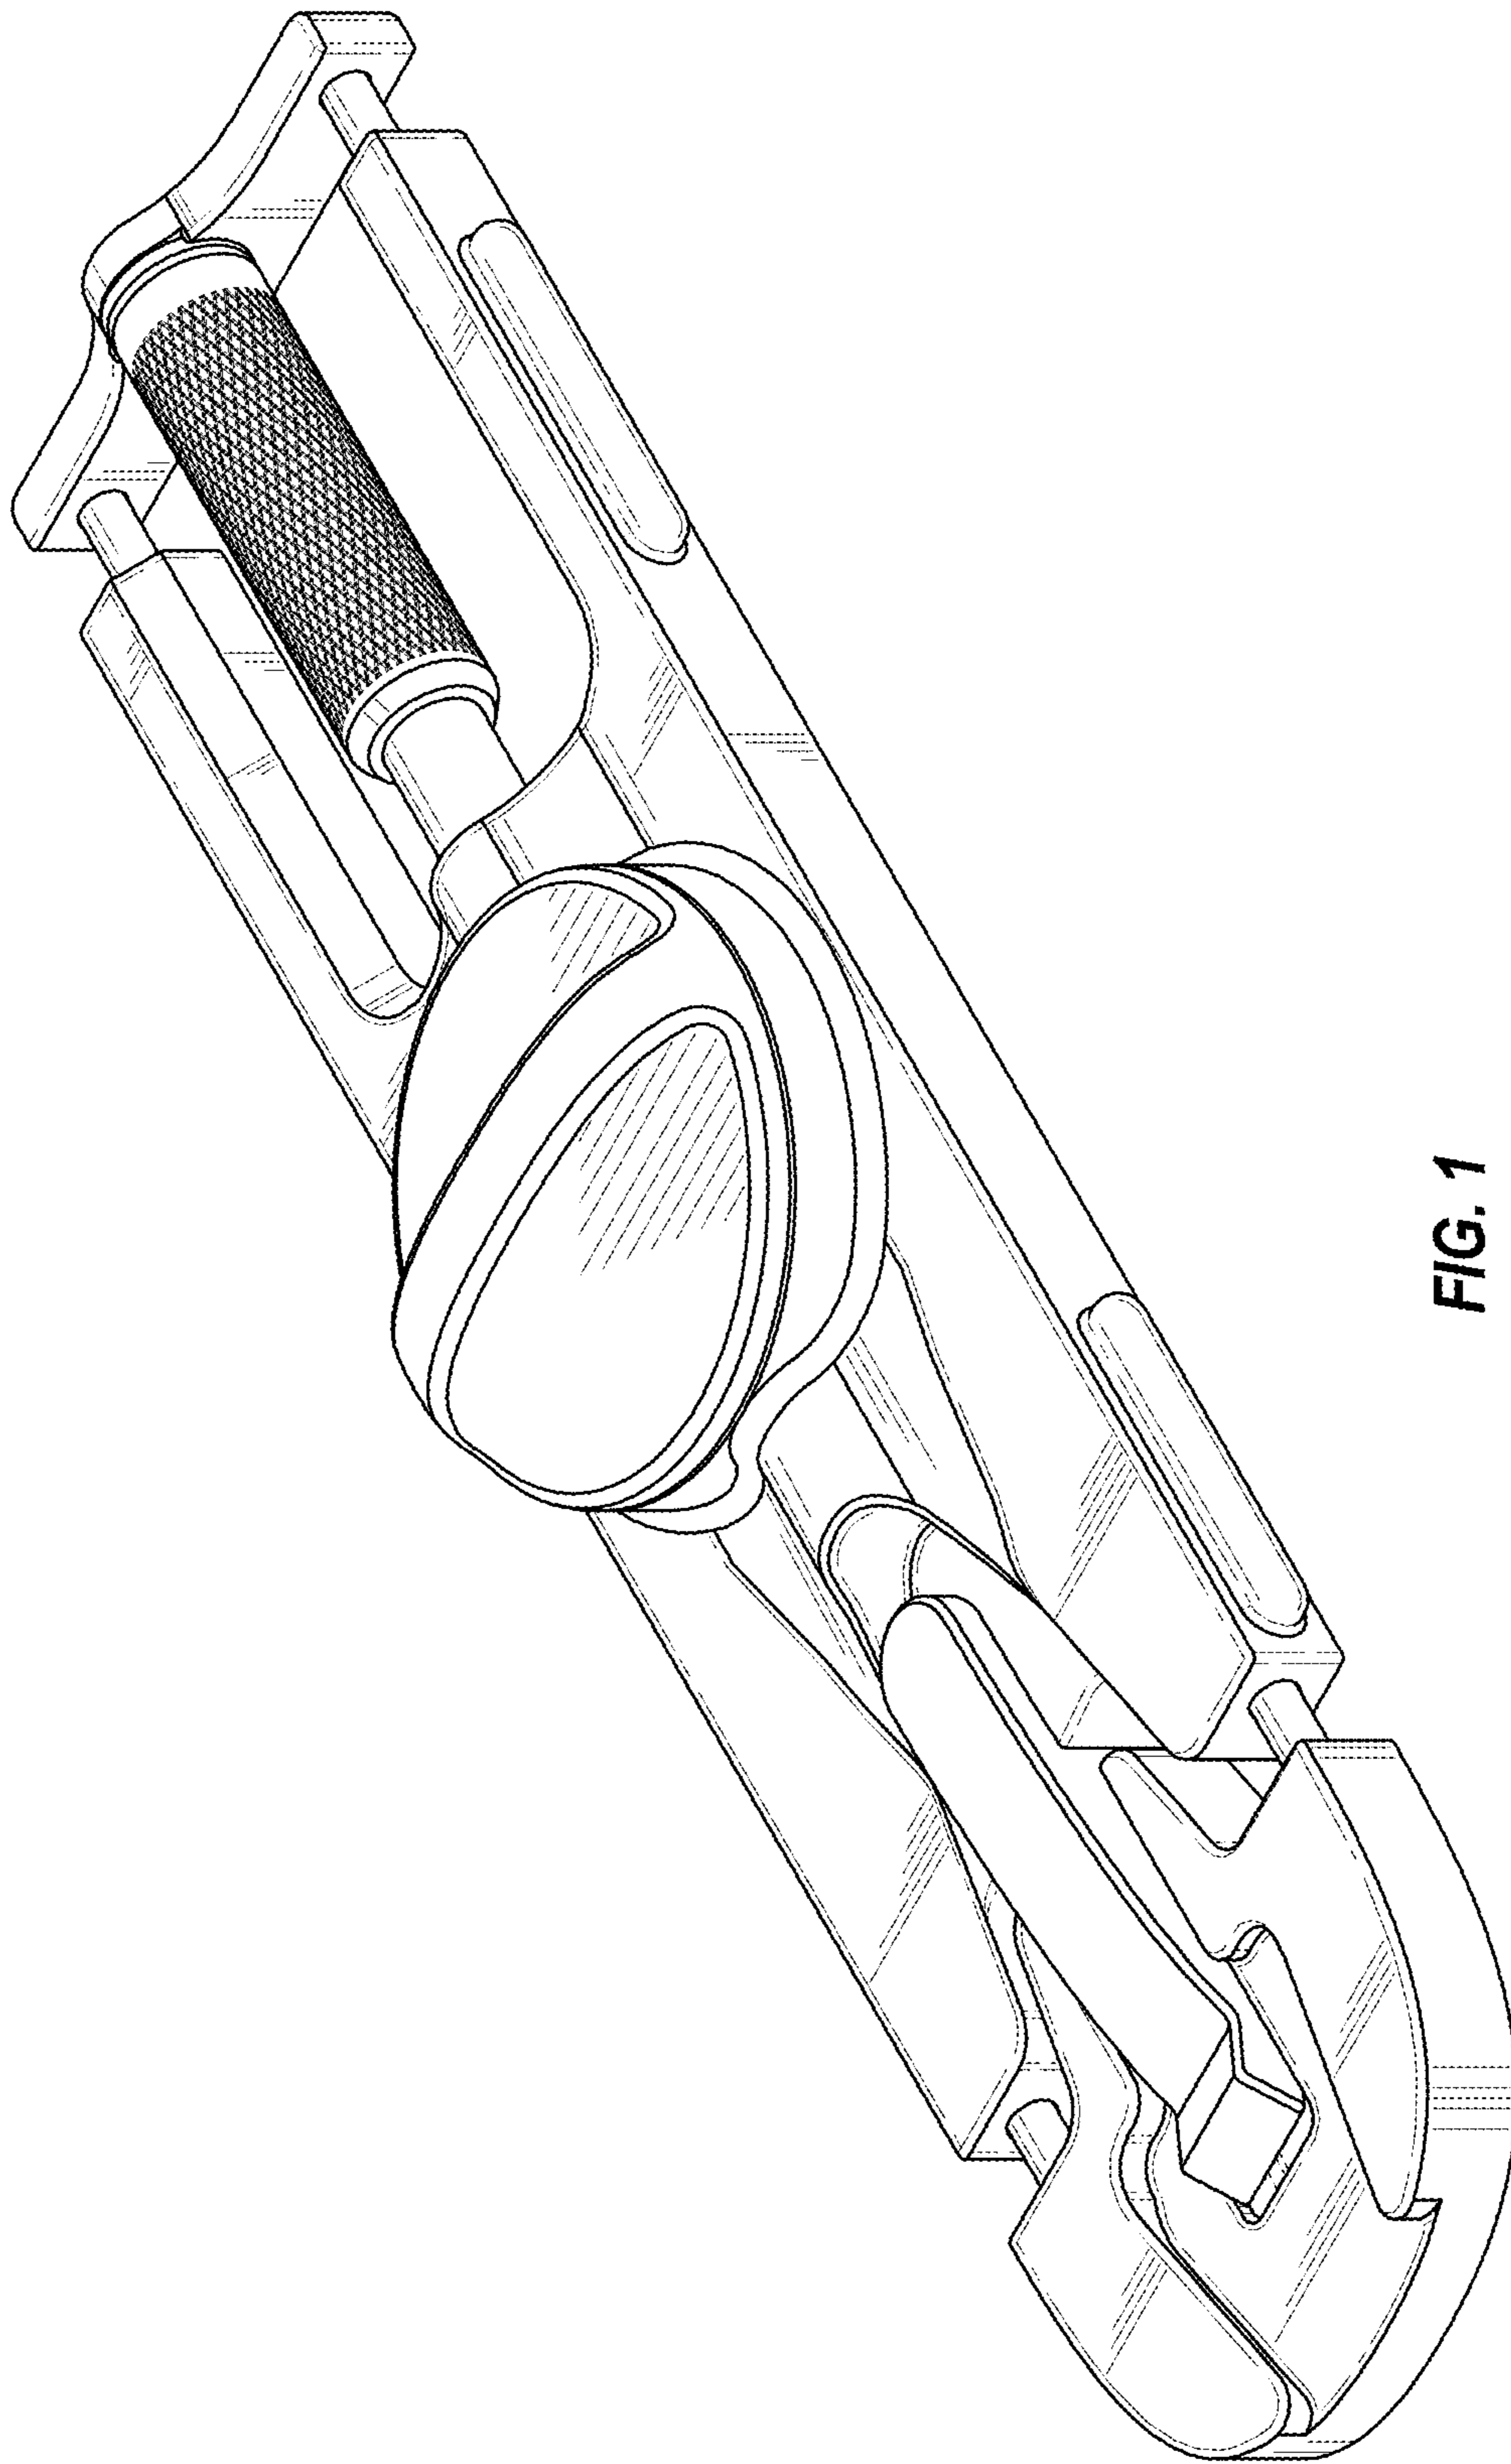


FIG. 1

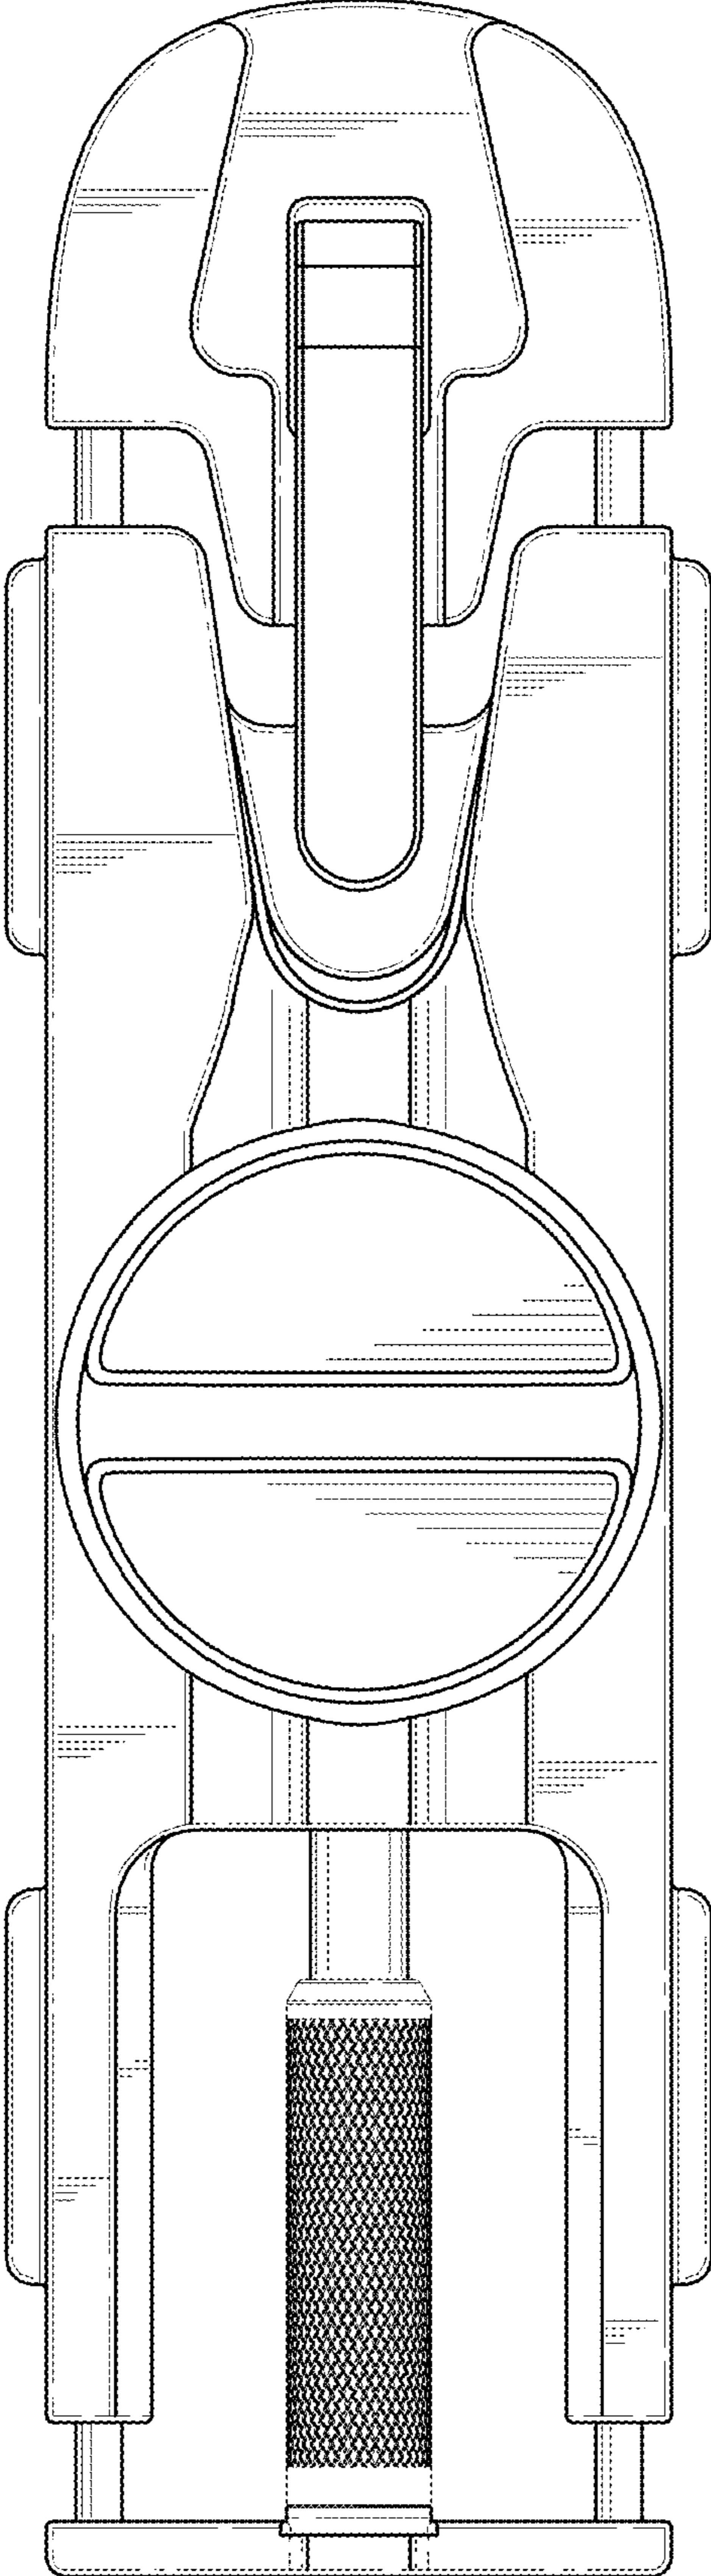


FIG. 2

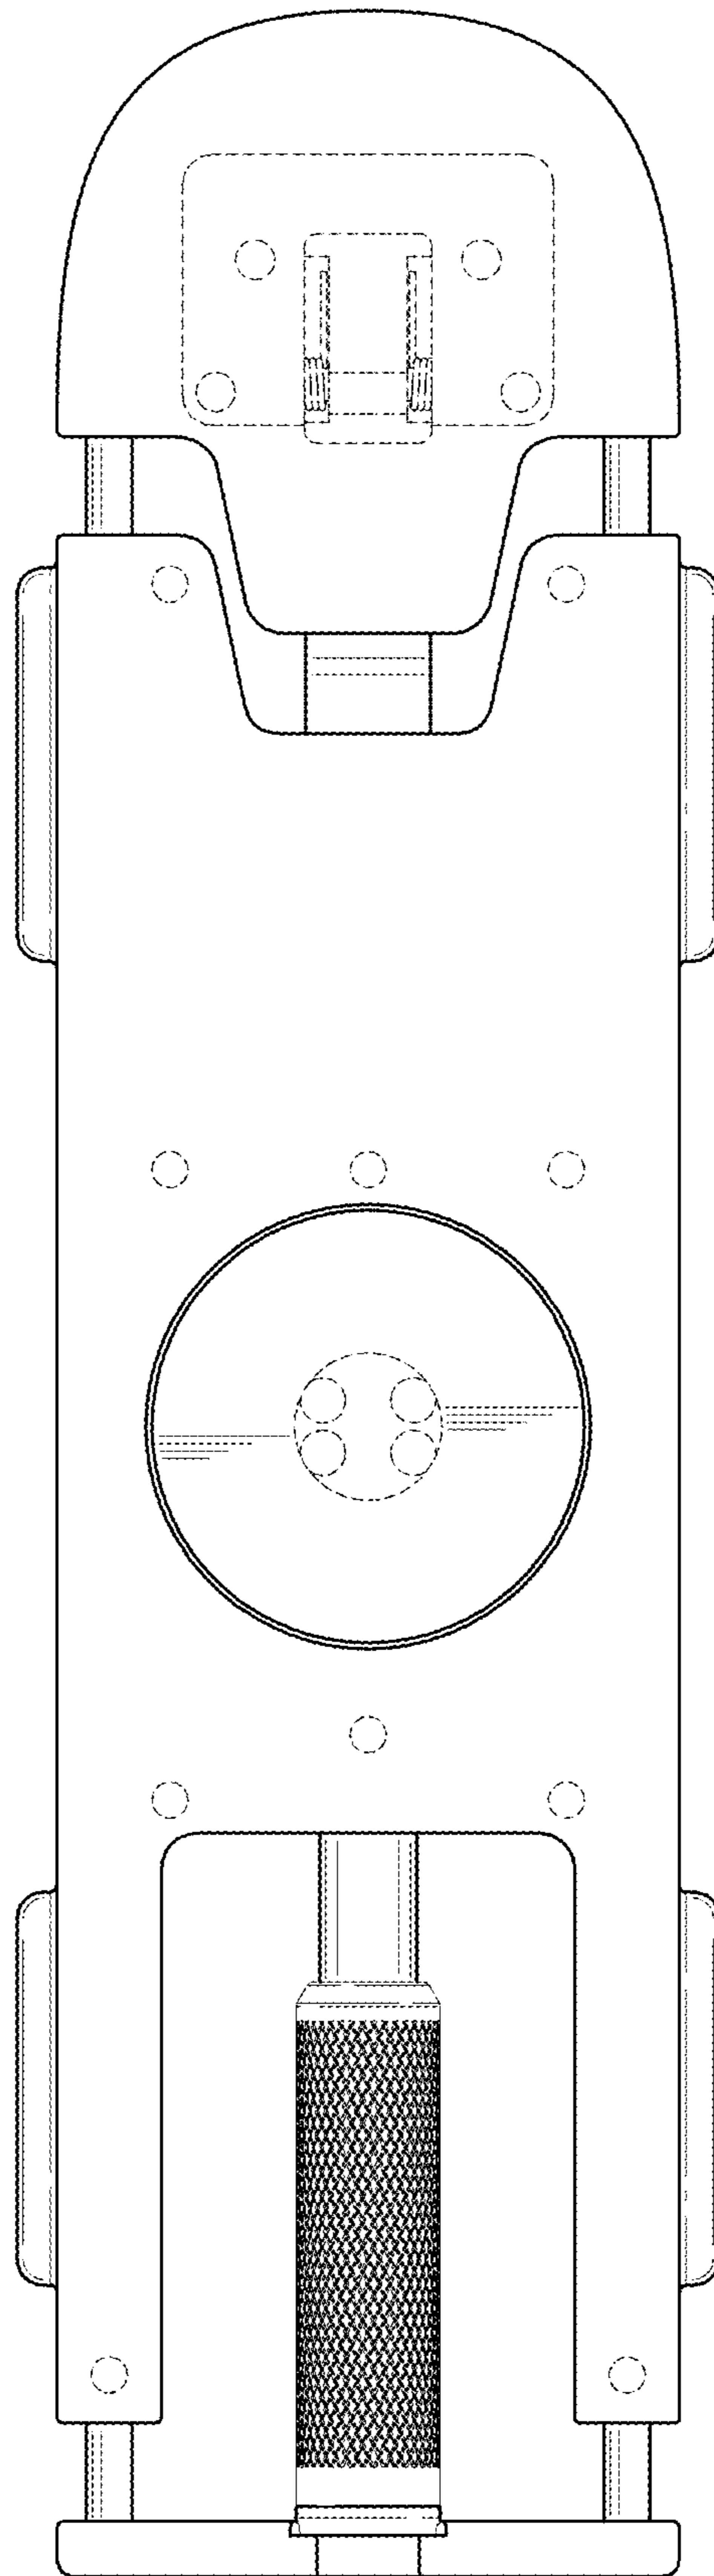


FIG. 3

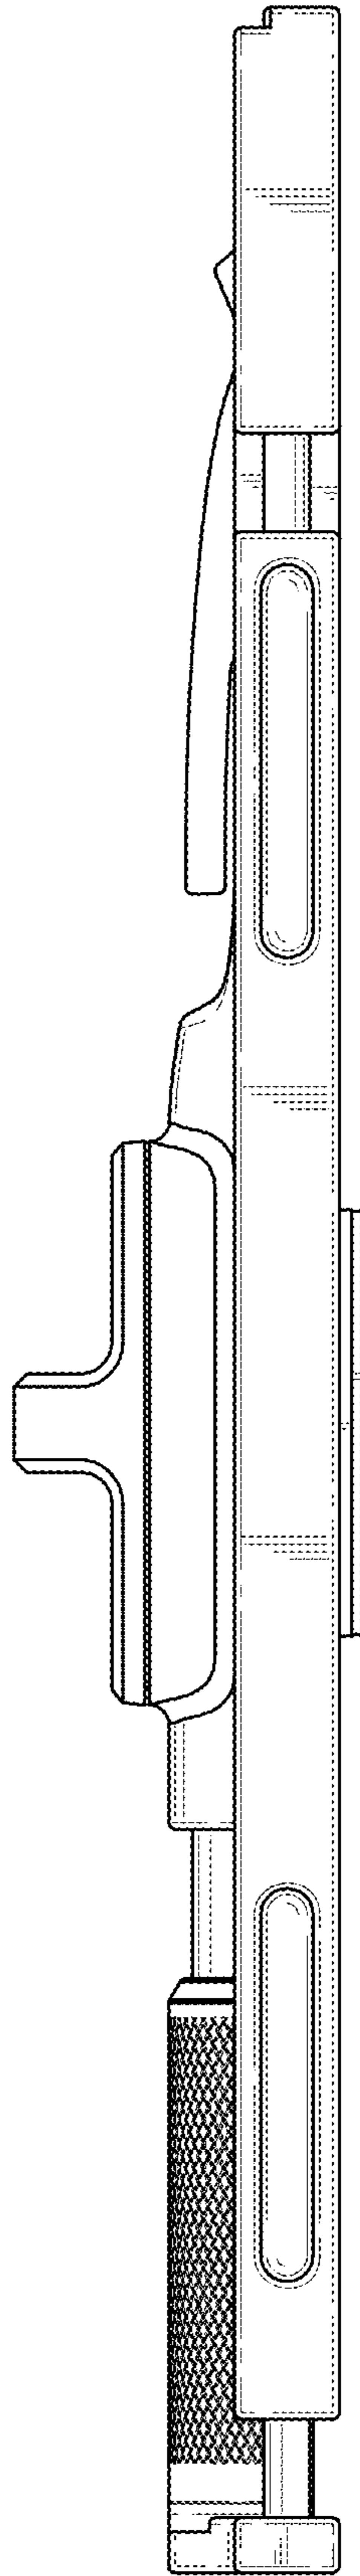


FIG. 4

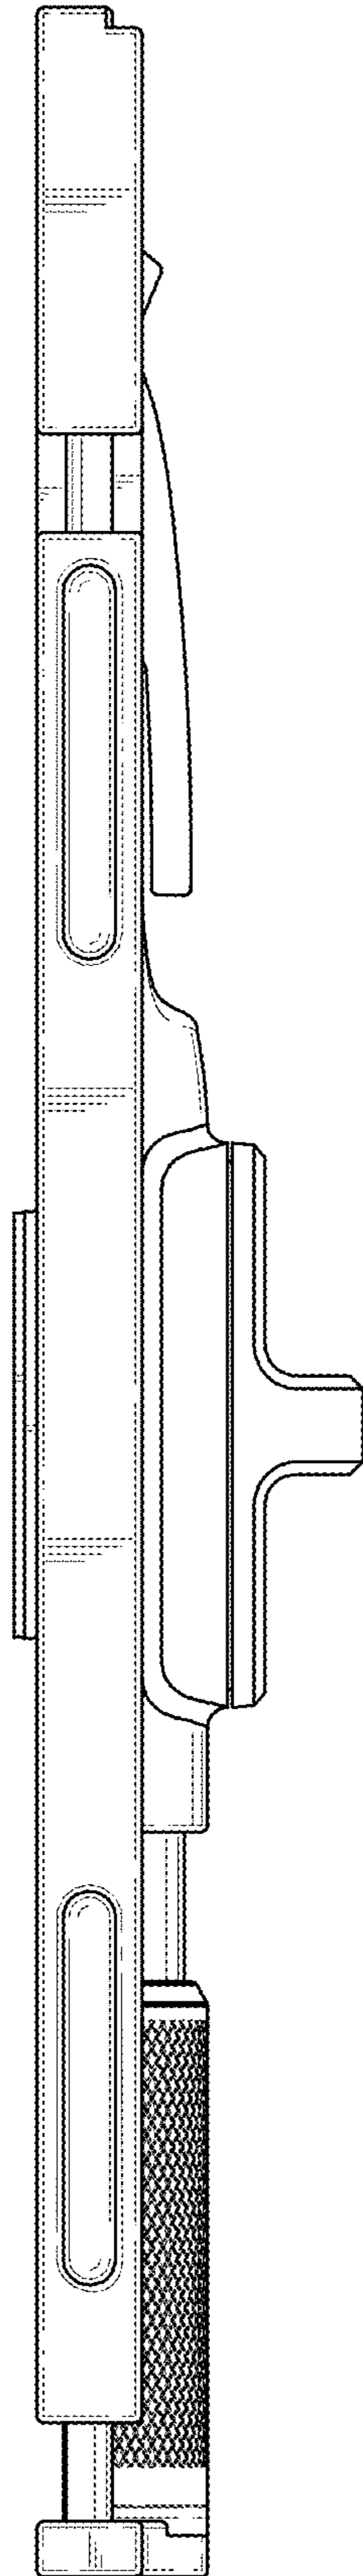


FIG. 5

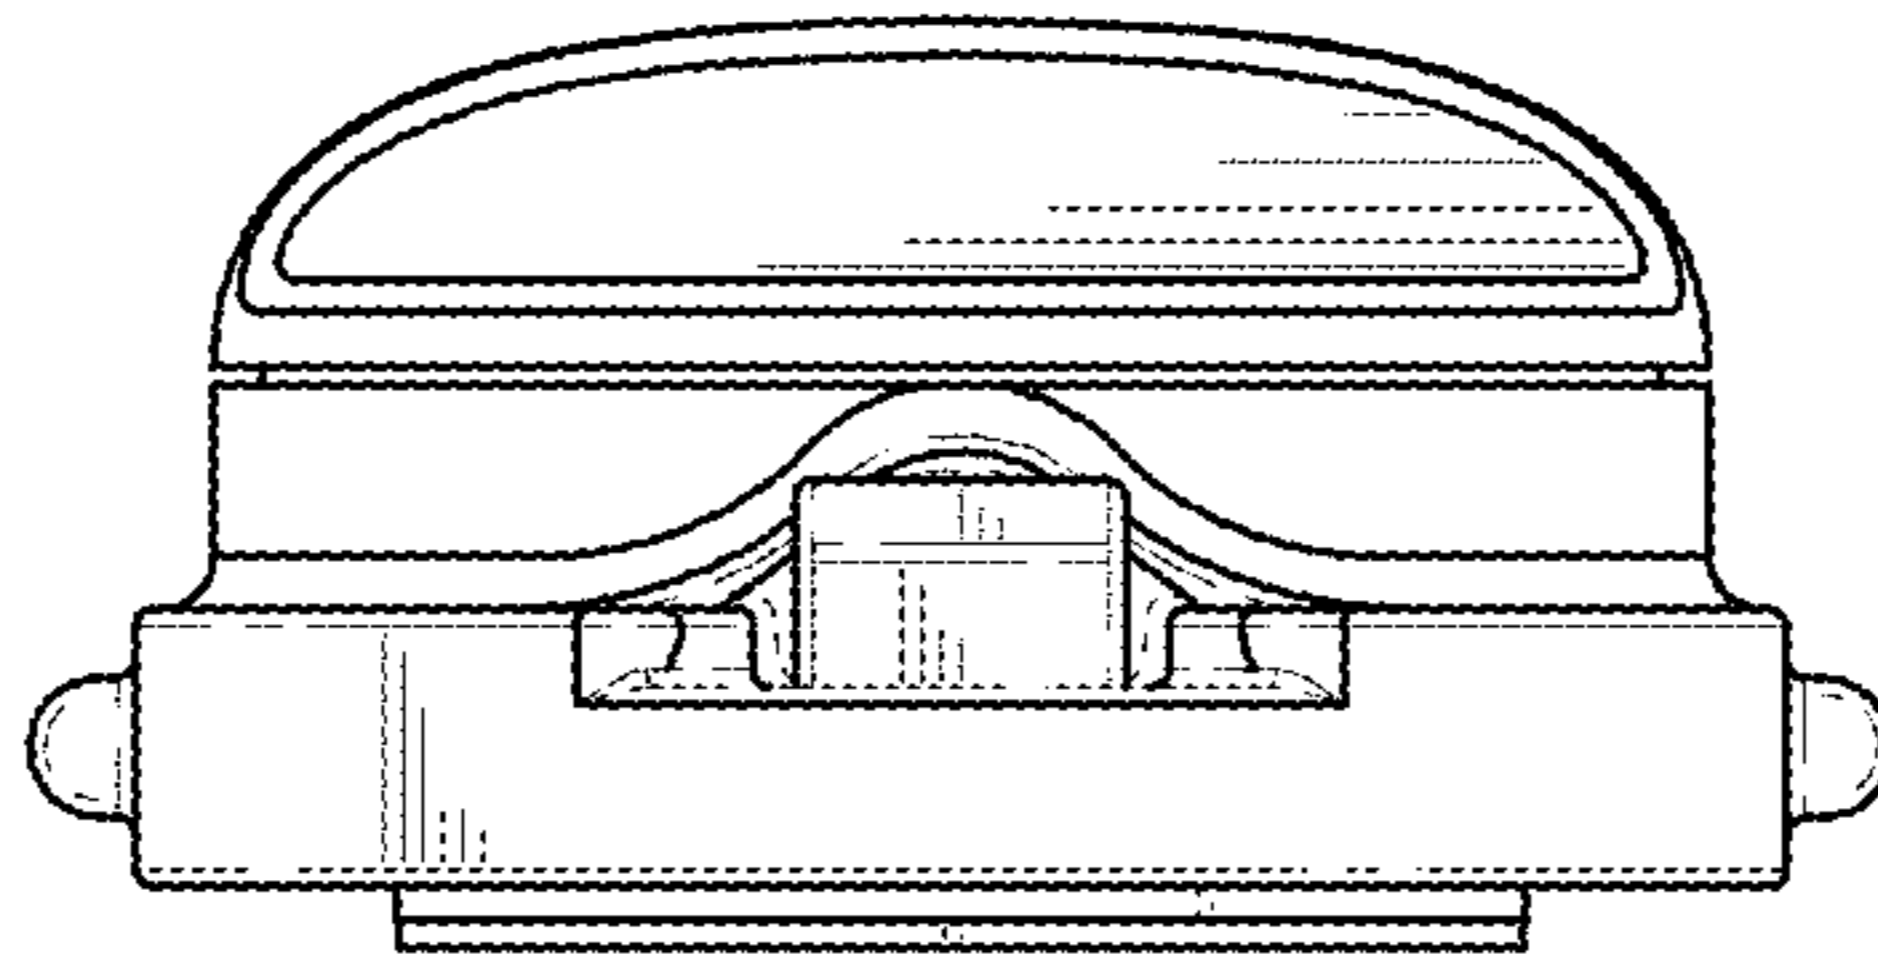


FIG. 6

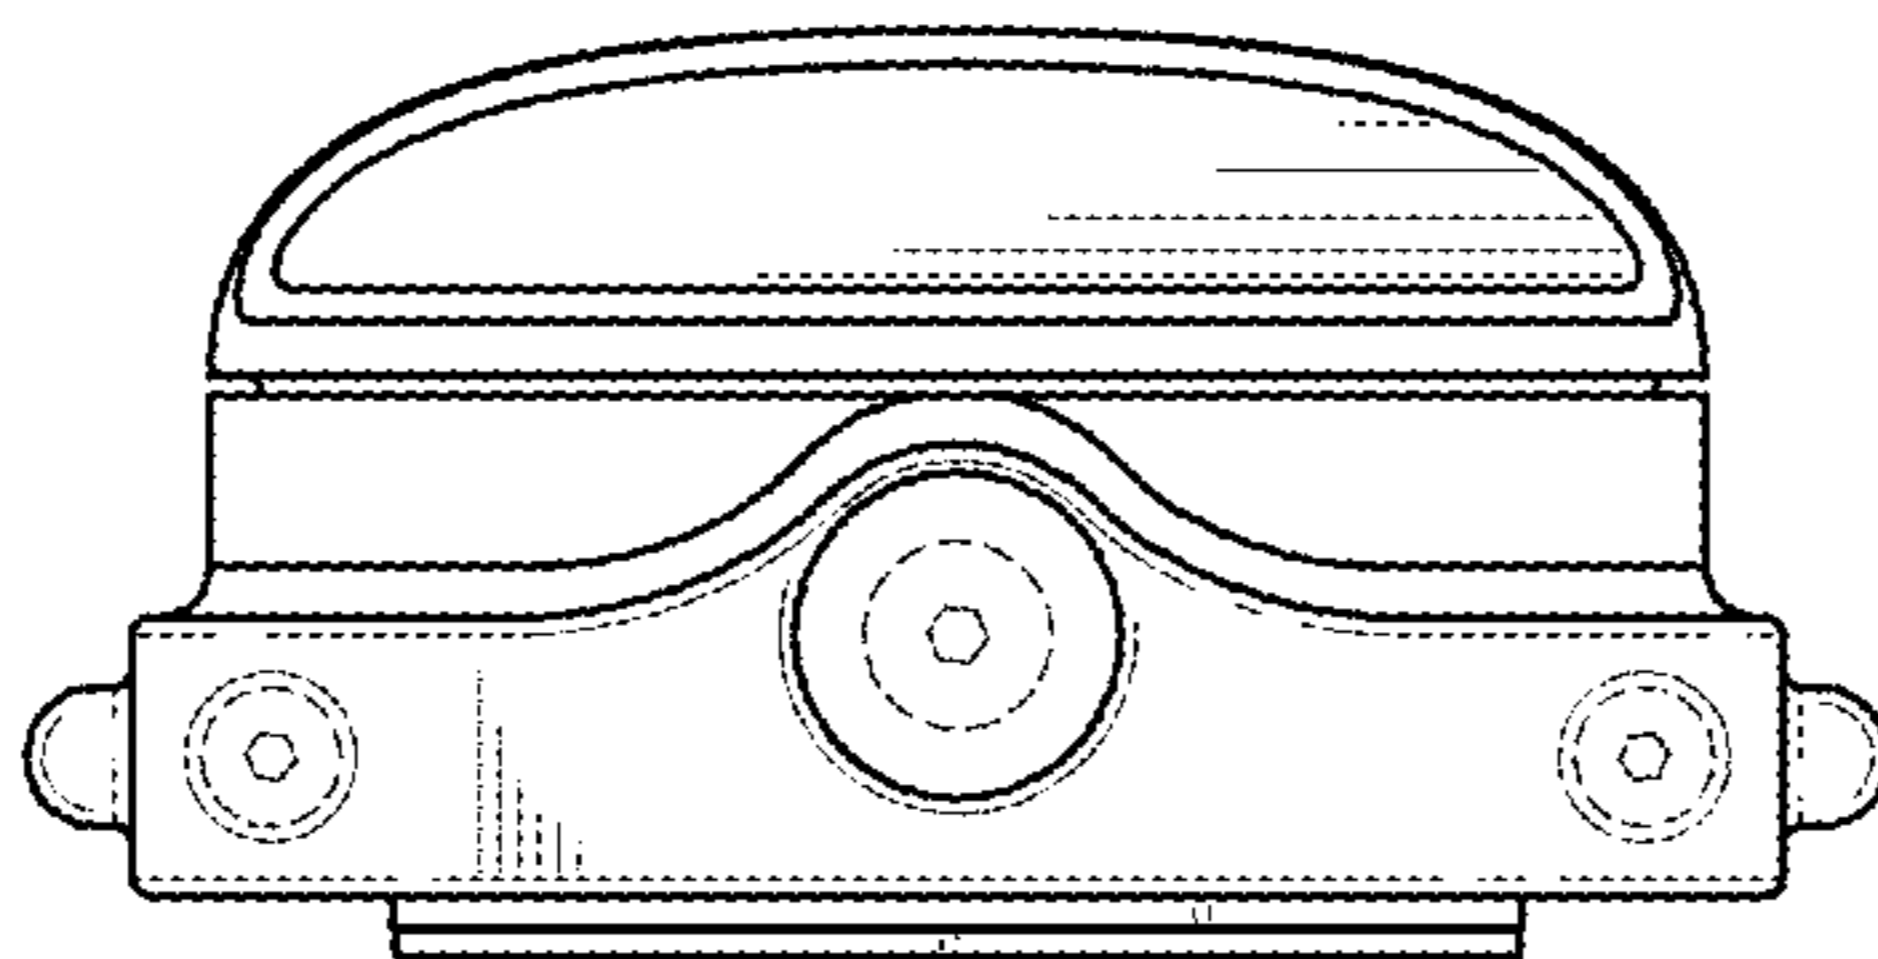


FIG. 7