US00D899434S

(12) **United States Design Patent**
Zimmerman et al.

(10) **Patent No.: US D899,434 S**
(45) **Date of Patent: ** Oct. 20, 2020**

(54) **FLUOROMETER DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE**

(71) Applicant: **LIFE TECHNOLOGIES CORPORATION**, Carlsbad, CA (US)

(72) Inventors: **Sean Zimmerman**, San Diego, CA (US); **Scott Rickes**, San Diego, CA (US); **Jason Dallwig**, Eugene, OR (US); **Kathleen Free**, Cheshire, OR (US); **Joseph Lee**, San Diego, CA (US); **Jennifer Hedlind**, Springfield, OR (US)

(73) Assignee: **LIFE TECHNOLOGIES CORPORATION**, Carlsbad, CA (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/637,491**

(22) Filed: **Feb. 19, 2018**

Related U.S. Application Data

(62) Division of application No. 29/584,427, filed on Nov. 14, 2016, now Pat. No. Des. 812,087, which is a (Continued)

(51) **LOC (12) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/485**

(58) **Field of Classification Search**
USPC D14/485–495; 345/1.1, 1.2, 2.1–2.3, 3.1, 345/902; 715/763, 810, 836, 837, 846, 715/847, 977
CPC G06F 3/048; G06F 3/0481; G06F 3/04812; G06F 3/04817; G06F 3/0482; G06F 3/0483; G06F 3/0484; G06F 3/04847; G06F 3/0485; G06F 3/04855; G06F 3/04886; G06Q 30/00; H03J 1/00; H03J 1/0008; H03J 1/0016; H03J 1/0025; H04N 5/00; H04N 5/08; H04N 5/14; H04N 5/222; H04N 5/225; H04N 5/232; H04N 5/445; H04N 5/44543; H04N 5/45; H04N 2005/44517; H04N 2005/44521; H04N 2005/44526; H04N 2005/4453; H04N 2005/44534; H04N 2005/44539; H04N
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

D435,257 S 12/2000 Woods
D461,822 S 8/2002 Okuley
(Continued)

OTHER PUBLICATIONS

Thermo Fisher Scientific, "Qubit 3.0 Fluorometer", posted date unknown, thermofisher.com, site visited Jun. 15, 2016, available from internet, http://www.thermofisher.com/us/en/home/industrial/spectroscopy-elemental-isotope-analysis/molecular-spectroscopy/fluorometers/qubit-fluorometer.html, 2016, 1-6.

Primary Examiner — Cathron C Brooks
Assistant Examiner — Christian P. McLean

(57) **CLAIM**

The ornamental design for a fluorometer display screen with graphical user interface, as shown and described.

DESCRIPTION

FIG. **1** is a view of a first embodiment of a fluorometer display screen with graphical user interface showing our new design; and,

FIG. **2** is a view of a second embodiment thereof.

The broken line showing of the fluorometer is included for the purpose of illustrating environmental structure and forms no part of the claimed design. The remaining broken lines illustrate the display screen and portions of the graphical user interface and form no part of the claimed design.

1 Claim, 2 Drawing Sheets



Related U.S. Application Data

division of application No. 29/501,333, filed on Sep. 3, 2014, now Pat. No. Des. 771,660.

(58) **Field of Classification Search**

CPC 2005/44547; H04N 2005/44556; H04N 2005/4456; H04N 2005/44565; H04N 2005/44569; H04N 2005/44573; H04N 21/00; H04N 21/234; H04N 21/431; H04N 21/4312; H04N 21/4314; H04N 21/4316

See application file for complete search history.

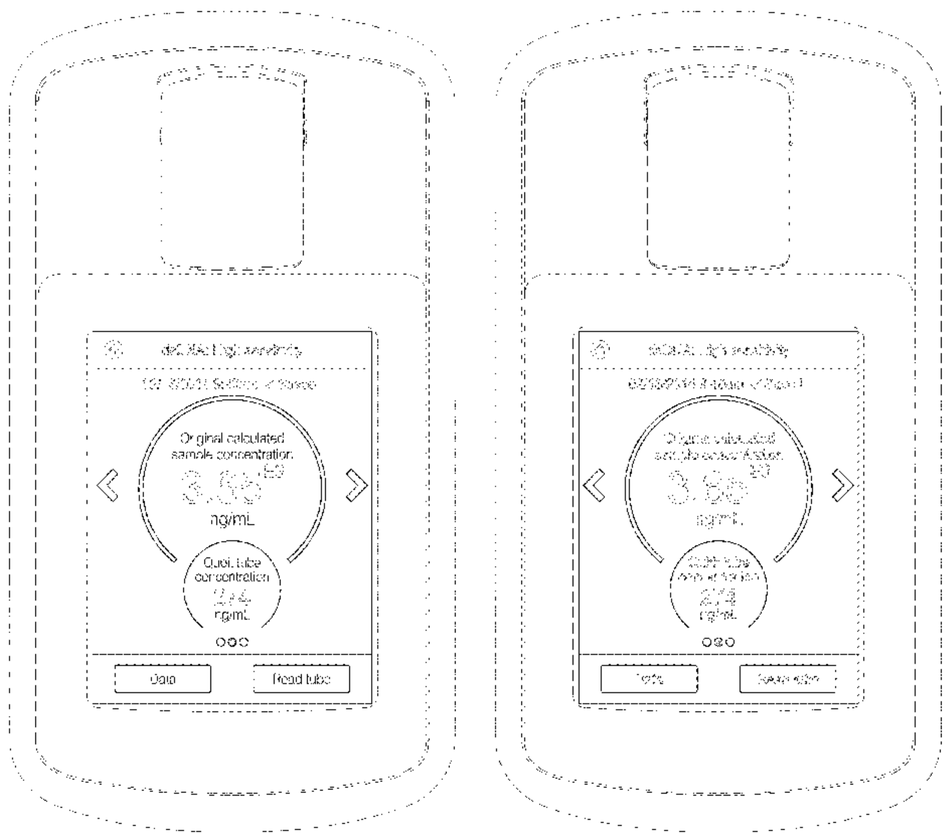(56) **References Cited**

U.S. PATENT DOCUMENTS

6,549,219	B2		4/2003	Selker	
D490,438	S		5/2004	Greminger	
D525,264	S		7/2006	Chotai et al.	
D541,295	S		4/2007	Harvey et al.	
D556,768	S	*	12/2007	Morris	D14/487
D566,722	S		4/2008	Jackson	
D590,415	S		4/2009	Ball	
D591,763	S		5/2009	Lee	
D596,192	S		7/2009	Shotel	
D602,942	S		10/2009	Bennett et al.	
D605,652	S		12/2009	Plaisted et al.	
D618,695	S		6/2010	Bennett et al.	
D624,933	S		10/2010	Fitzmaurice et al.	
D640,264	S		6/2011	Fujii et al.	
D640,277	S	*	6/2011	Woo	D14/487
D652,048	S		1/2012	Joseph	
D652,050	S		1/2012	Chaudhri	
D667,841	S		9/2012	Rai et al.	
D687,057	S		7/2013	Plitkins	
D688,687	S		8/2013	Smith et al.	
D694,253	S		11/2013	Helm	
D701,226	S		3/2014	Jung	
D706,283	S		6/2014	Pedraza Padilla et al.	
D708,203	S		7/2014	Johnson	
D709,914	S		7/2014	Berdan et al.	
D711,916	S		8/2014	Matas	
D712,911	S		9/2014	Pearson et al.	
D714,822	S		10/2014	Capua et al.	
8,875,054	B2	*	10/2014	Hopkins	G06F 3/04847 715/833
D720,767	S		1/2015	Miller et al.	
D725,143	S		3/2015	Terleski et al.	
D725,664	S		3/2015	Nies et al.	
D725,671	S		3/2015	Dorfmann	
D727,336	S		4/2015	Allison et al.	
D736,824	S		8/2015	Omiya	
D739,423	S		9/2015	Mariet et al.	
D740,300	S		10/2015	Lee et al.	
D740,847	S		10/2015	Yampolskiy et al.	
D742,897	S		11/2015	Matas et al.	
D745,050	S		12/2015	Kwon	
D746,827	S		1/2016	Jung et al.	
D747,352	S	*	1/2016	Lee	D14/492
D748,126	S		1/2016	Sarukkai et al.	
D752,076	S		3/2016	Guesnon, Jr.	
D752,621	S		3/2016	Cojuangco et al.	
D753,134	S		4/2016	Vazquez	
D753,155	S		4/2016	Nies et al.	
D754,682	S		4/2016	Lee et al.	
D754,705	S		4/2016	Angelides	
D754,719	S		4/2016	Zha	
D755,193	S		5/2016	Sun et al.	
D756,371	S		5/2016	Bertnick et al.	
D756,391	S		5/2016	Kouvas et al.	
D757,081	S		5/2016	Govindan Sankar Selvan et al.	
D759,032	S		6/2016	Amin et al.	
D759,079	S	*	6/2016	Carlton	D14/486
D760,244	S	*	6/2016	Lv	D14/485
D760,791	S	*	7/2016	Liu	G06F 3/04817 D14/494
D763,308	S		8/2016	Wang et al.	
D765,695	S	*	9/2016	Leabman	D14/486
D766,278	S		9/2016	Andre et al.	
D771,068	S	*	11/2016	Lv	D14/485
D771,660	S		11/2016	Zimmerman et al.	
D771,672	S	*	11/2016	Tanabe	G06F 11/327 D14/486
D775,144	S		12/2016	Vazquez	
D775,635	S		1/2017	Raji et al.	
D775,658	S	*	1/2017	Luo	D14/488
D777,177	S		1/2017	Chen et al.	
D777,200	S	*	1/2017	Luo	D14/488
D778,927	S		2/2017	Bertnick et al.	
D780,199	S		2/2017	Croan	
D781,299	S		3/2017	Yun et al.	
D781,886	S		3/2017	Dziuba et al.	
D782,498	S		3/2017	Krafft	
D784,373	S		4/2017	Cai	
D785,025	S	*	4/2017	Zimmerman	D14/486
D786,279	S		5/2017	McKim et al.	
D786,286	S		5/2017	Kurecka	
D786,898	S	*	5/2017	Hall	D14/486
D788,141	S	*	5/2017	Kim	D14/486
D791,160	S	*	7/2017	Jang	D14/486
D795,906	S	*	8/2017	Butrick	D14/486
D798,311	S	*	9/2017	Golden	F24F 11/30 D14/485
D804,515	S	*	12/2017	Vijay	D14/487
D809,535	S	*	2/2018	Park	D14/485
D811,425	S	*	2/2018	Olsen	D14/486
D812,087	S		3/2018	Zimmerman et al.	
D818,487	S	*	5/2018	Eder	D14/488
D821,410	S	*	6/2018	Vinna	D14/485
D823,869	S	*	7/2018	Zimmerman	D14/486
D824,416	S	*	7/2018	Memmelaar, Jr.	D14/488
D824,417	S	*	7/2018	Narinedhat	D14/488
D826,969	S	*	8/2018	Goyette	D14/486
D839,888	S	*	2/2019	Yun	D14/485
D857,034	S	*	8/2019	Hung	D14/485
D857,749	S	*	8/2019	Brinker	D14/492
D861,021	S	*	9/2019	Vincent	D14/486
D863,326	S	*	10/2019	Weiandt	D14/485
D869,479	S	*	12/2019	Pillalamarri	D14/485
D871,422	S	*	12/2019	Vonnegut	D14/485
D872,744	S	*	1/2020	Kim	D14/485
D872,748	S	*	1/2020	LaBorde	D14/485
D873,283	S	*	1/2020	Bradley	D14/486
D875,106	S	*	2/2020	Winton	D14/485
D879,118	S	*	3/2020	Chen	D14/485
2008/0204418	A1	*	8/2008	Cybart	G06F 1/1626 345/173
2011/0047014	A1		2/2011	DeAngelo	
2013/0019175	A1		1/2013	Kotler et al.	
2013/0212529	A1		8/2013	Amarnath	
2014/0157126	A1		6/2014	Kusano	
2014/0160078	A1		6/2014	Seo et al.	
2016/0147406	A1	*	5/2016	Yi	G06F 3/0482 715/863
2017/0060399	A1	*	3/2017	Hough	G02B 27/02
2019/0095052	A1	*	3/2019	De Wever	G06F 3/0482

* cited by examiner

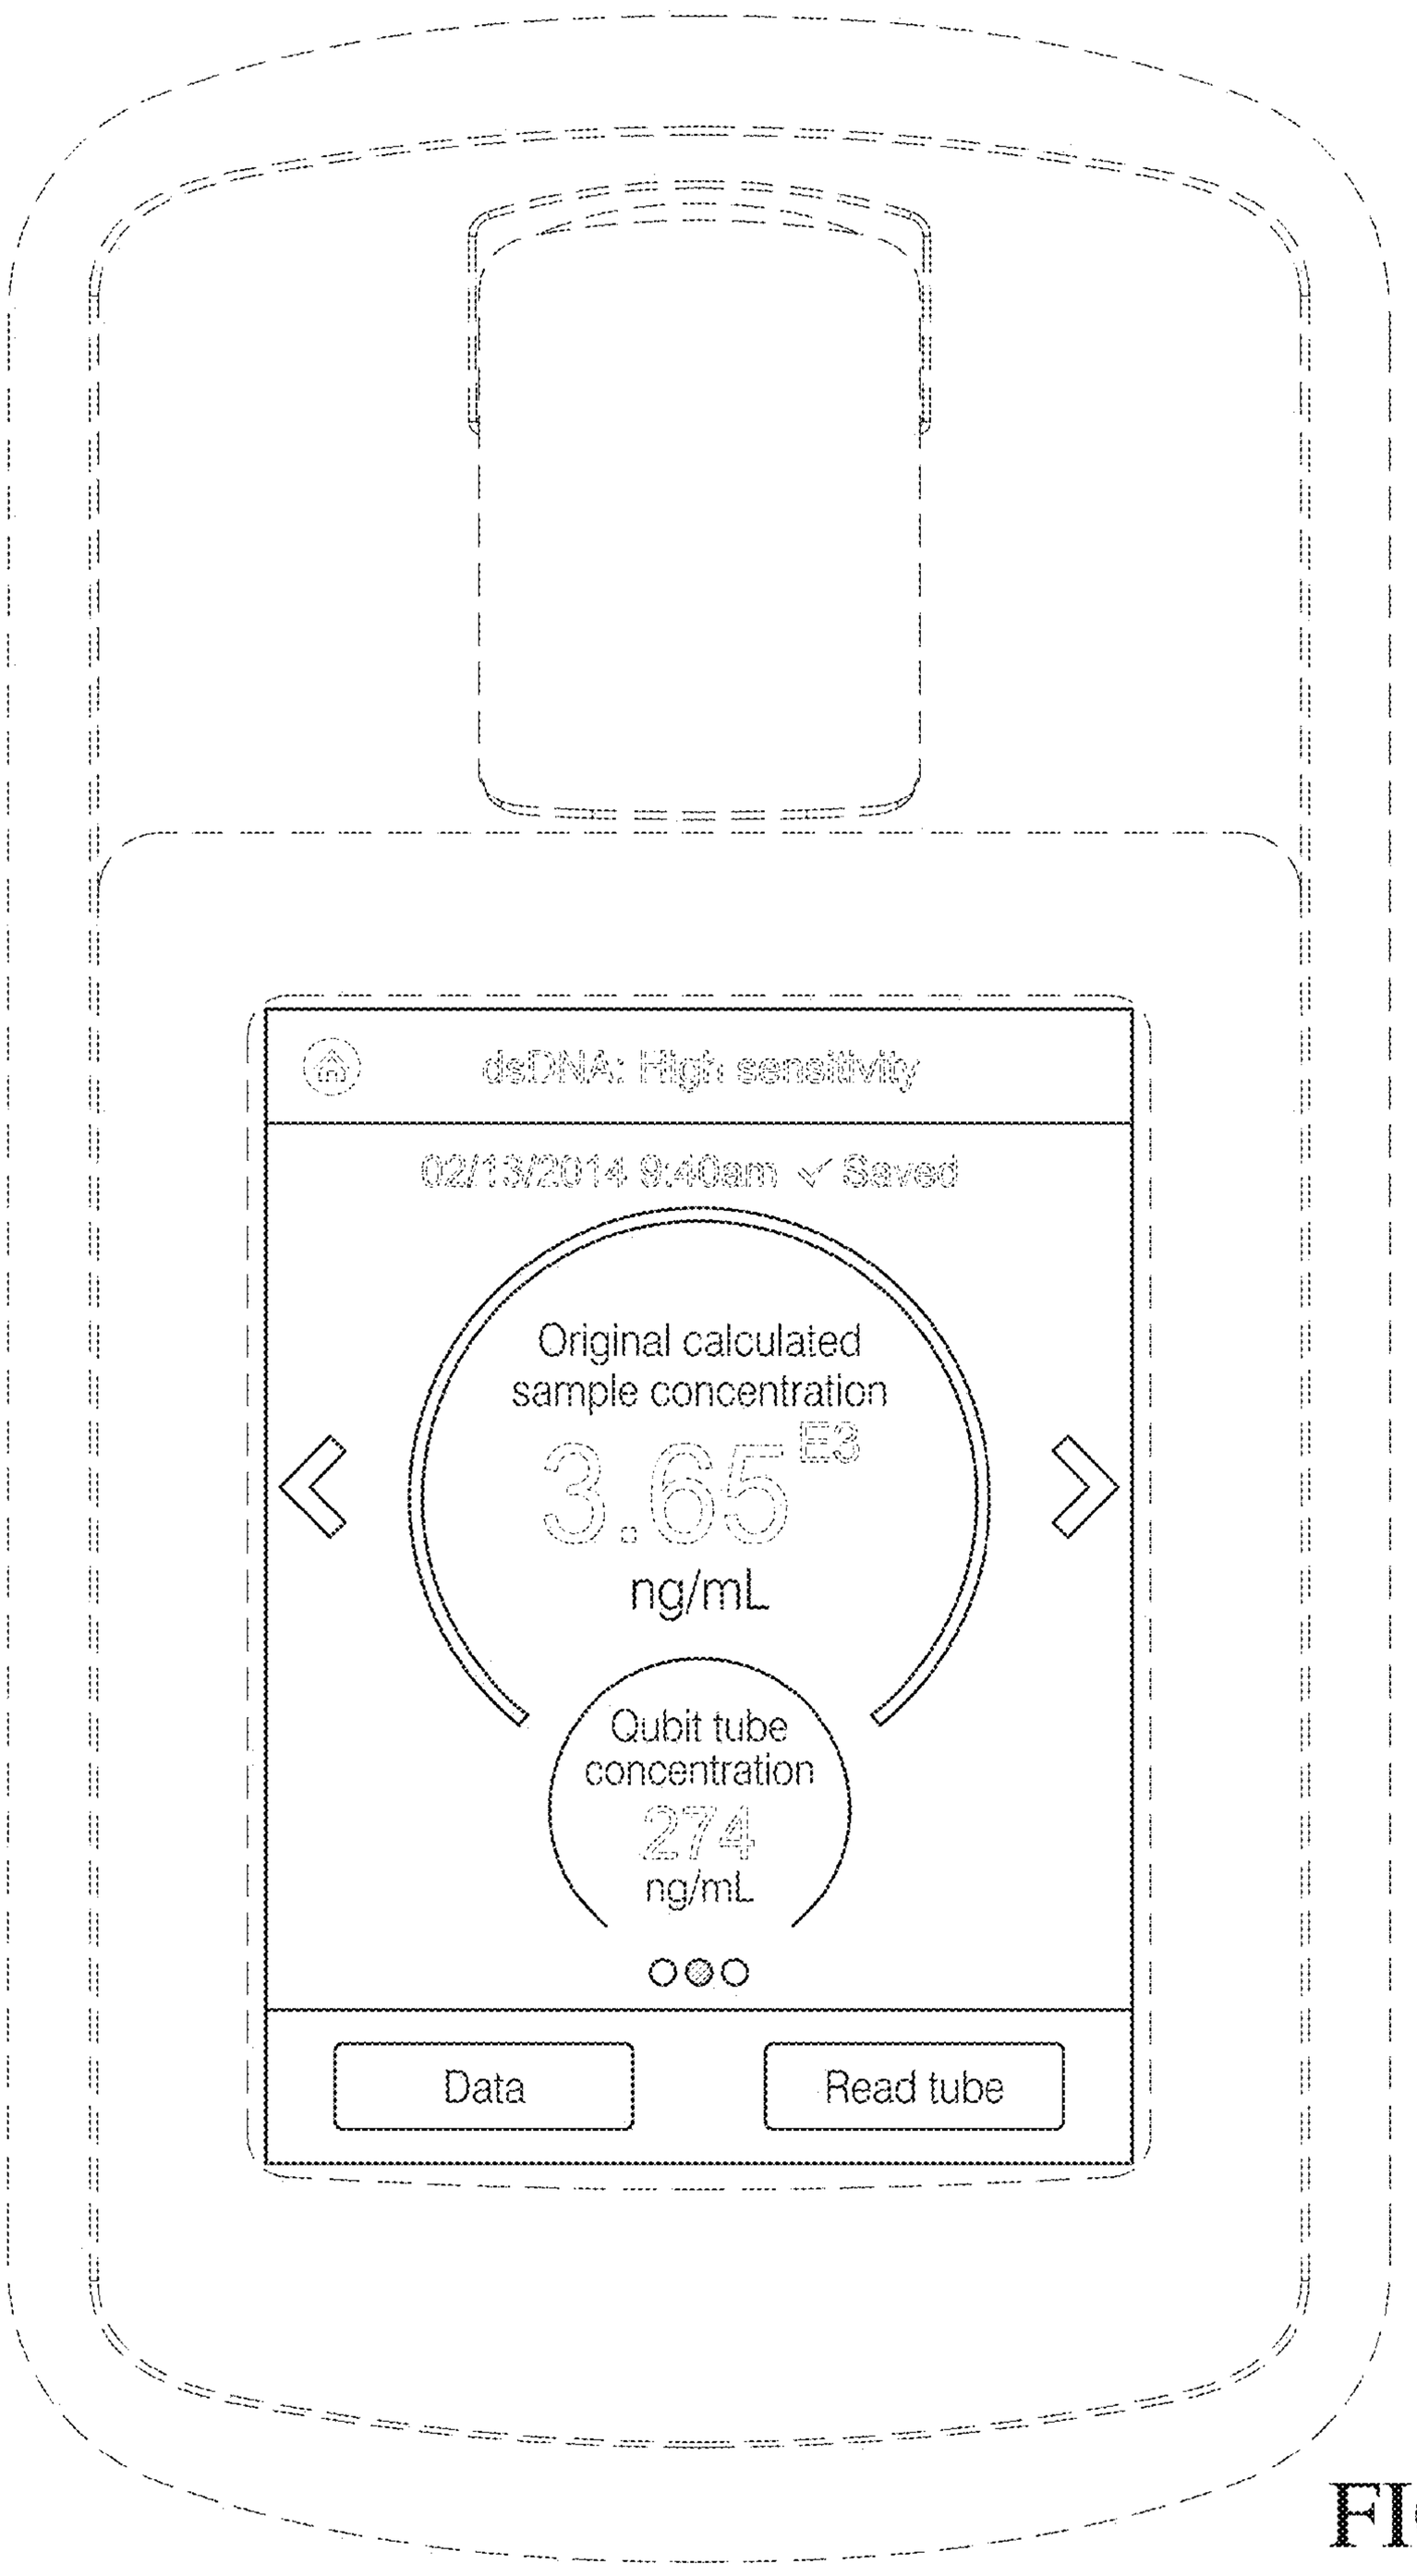
dsDNA: High sensitivity
02/13/2014 9:40am ✓ Saved
Original calculated sample concentration
3.65 E3
ng/mL
Qubit tube concentration
274
ng/mL
Data
Read tube

FIG. 1

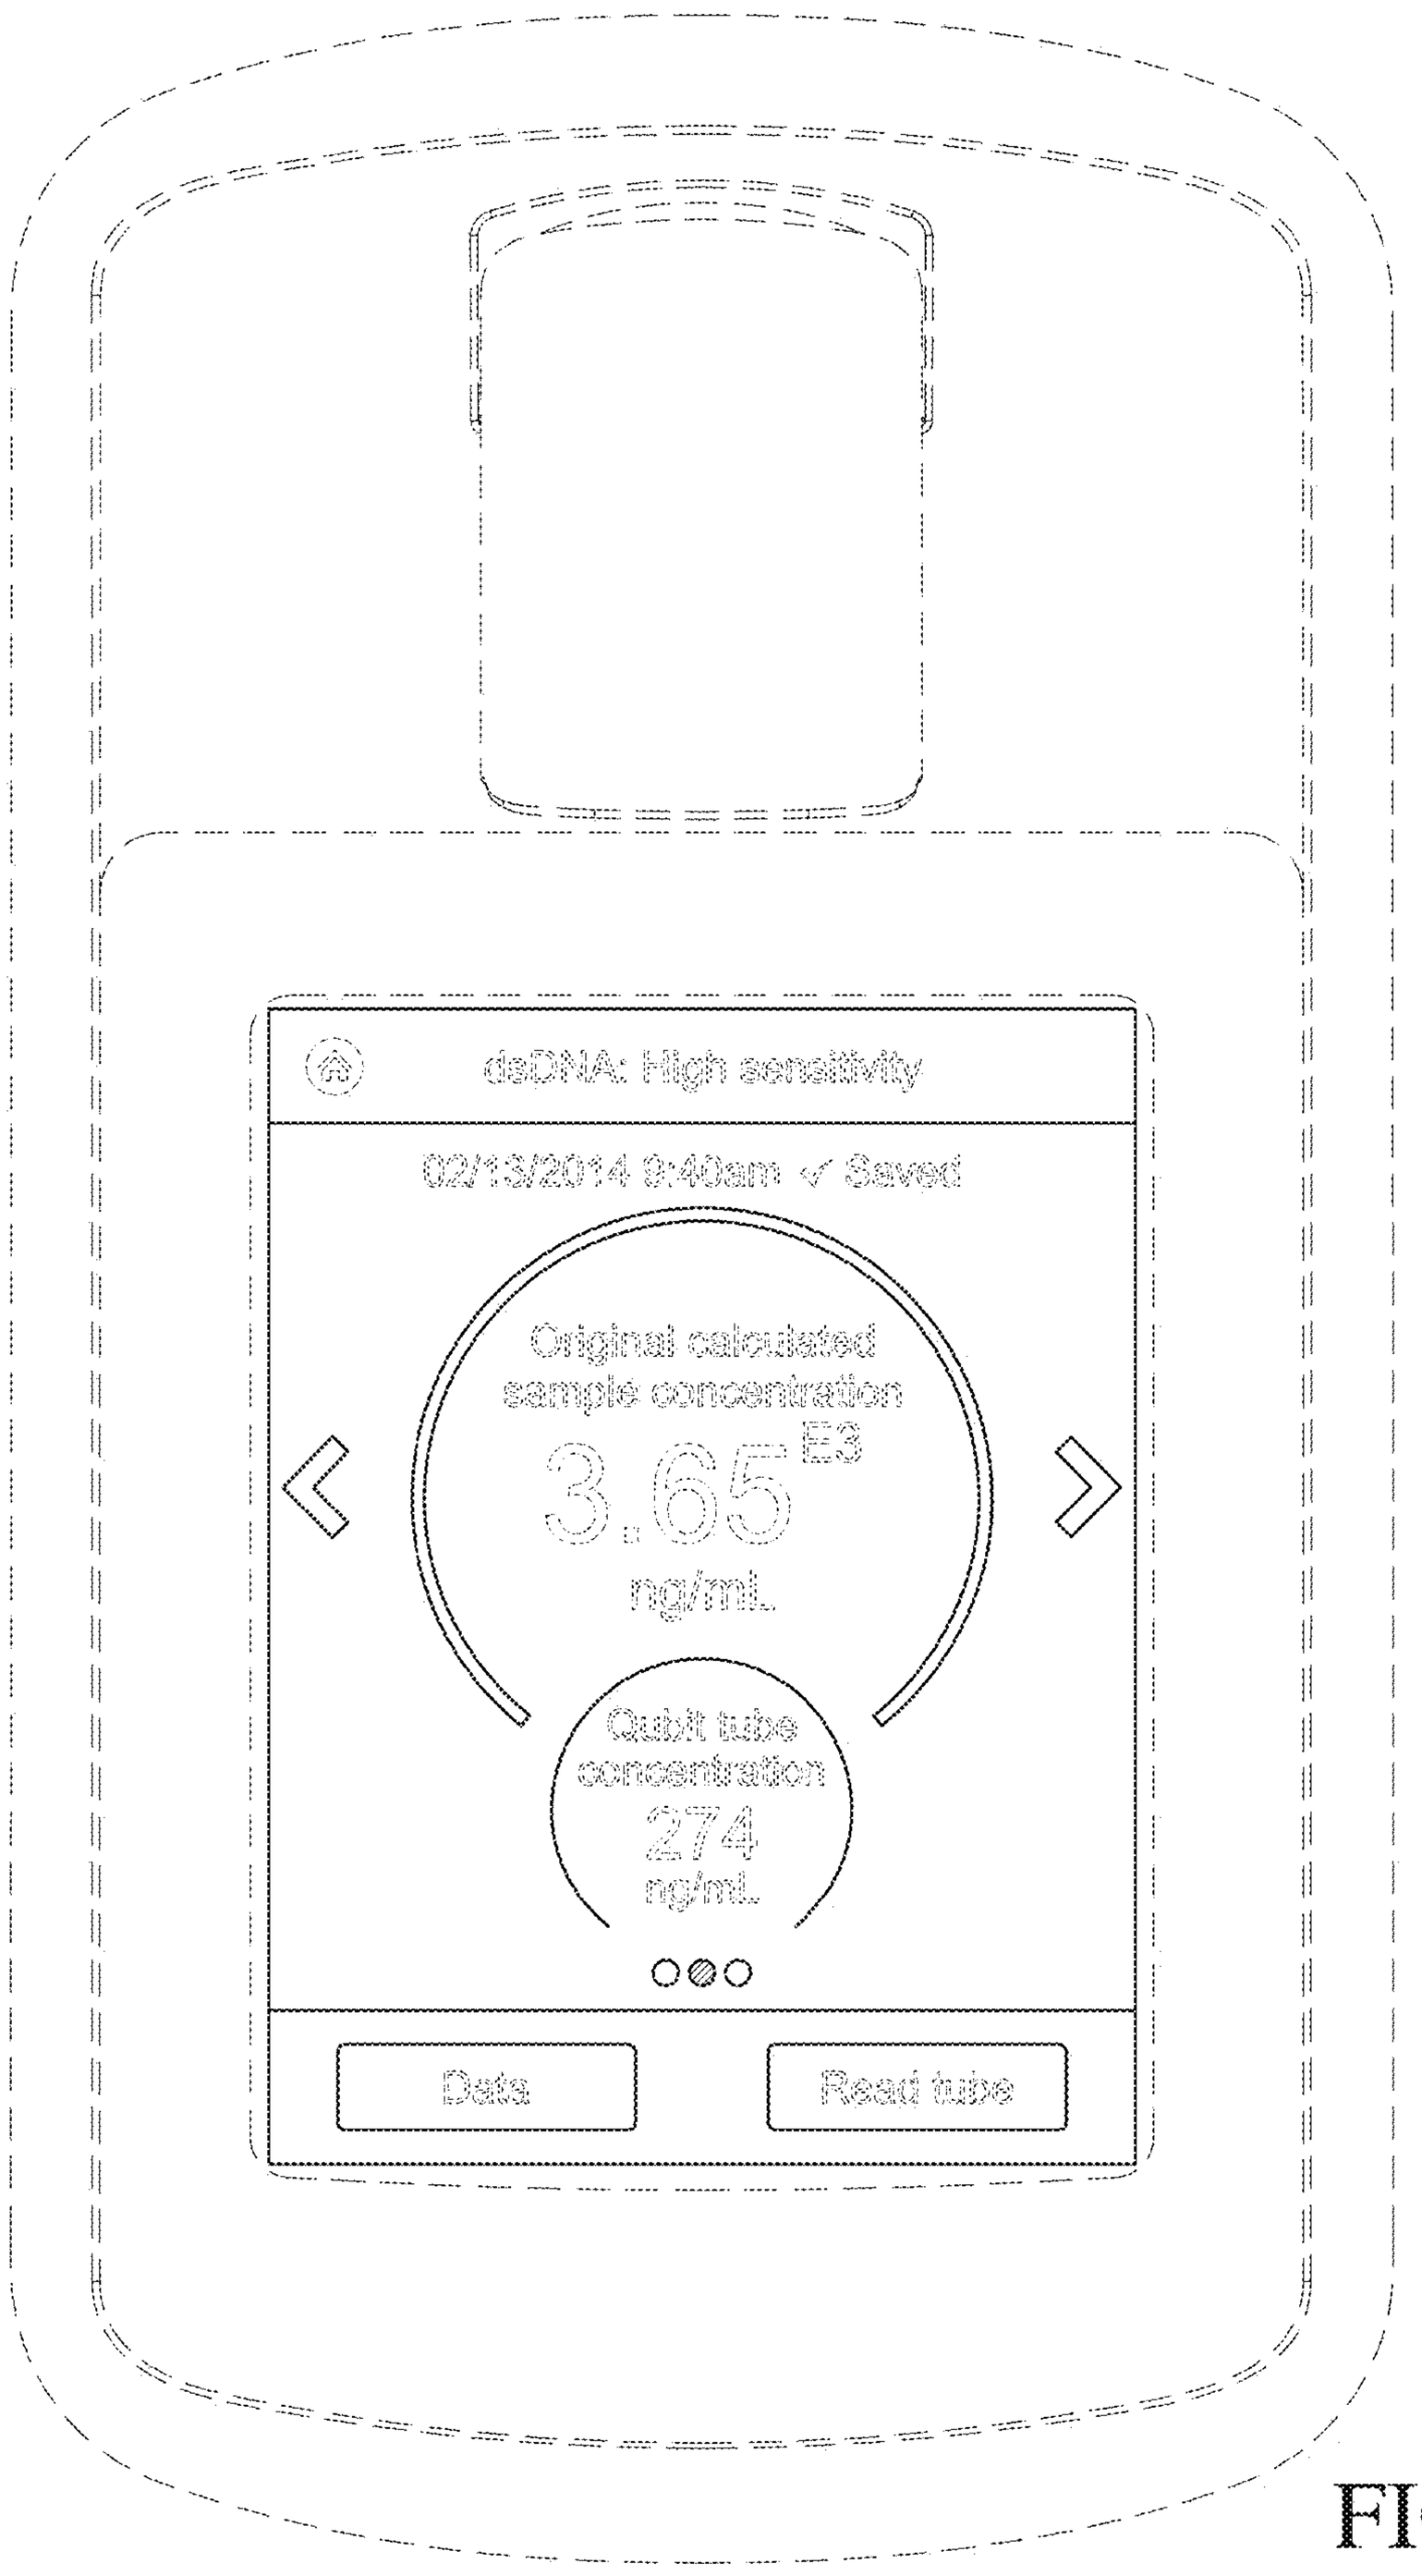
dsDNA: High sensitivity
02/13/2014 9:40am ✓ Saved
Original calculated sample concentration
3.65 E3
ng/mL
Qubit tube concentration
274
ng/mL
Data
Read tube

FIG. 2