



US00D901520S

(12) **United States Design Patent** (10) **Patent No.:** **US D901,520 S**
Ganguanco et al. (45) **Date of Patent:** **** Nov. 10, 2020**

- (54) **ELECTROPHORESIS AND IMAGING SYSTEM DISPLAY SCREEN WITH GRAPHICAL USER INTERFACE**
- (71) Applicants: **LIFE TECHNOLOGIES CORPORATION**, Carlsbad, CA (US); **LIFE TECHNOLOGIES HOLDINGS PTE LIMITED**, Singapore (SG)
- (72) Inventors: **Jefferson Ganguanco**, Singapore (SG); **Sean Zimmerman**, Encinitas, CA (US); **Joshua Mead**, San Diego, CA (US); **Scott Rickes**, San Diego, CA (US)
- (73) Assignees: **LIFE TECHNOLOGIES CORPORATION**, Carlsbad, CA (US); **LIFE TECHNOLOGIES HOLDINGS PTE LIMITED**, Singapore (SG)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/650,952**
- (22) Filed: **Jun. 11, 2018**

Related U.S. Application Data

- (62) Division of application No. 29/606,325, filed on Jun. 2, 2017, now Pat. No. Des. 829,235.
- (51) **LOC (12) Cl.** **14-04**
- (52) **U.S. Cl.**
USPC **D14/485**
- (58) **Field of Classification Search**
USPC D14/485-495
CPC G06F 3/048; G06F 3/0481; G06F 3/04817; G06F 3/0482; G06F 3/0483; G06F 3/04842; G06F 3/0485; G06F 3/04855; G06F 3/0486; G06F 3/0488; G06F 3/04886; G06F 9/4443; G06F 17/211; G06F 17/212

See application file for complete search history.

- (56) **References Cited**
U.S. PATENT DOCUMENTS
5,995,093 A 11/1999 Lambourne et al.
D464,660 S * 10/2002 Weng D14/488
D583,386 S 12/2008 Tomizawa et al.
D614,192 S * 4/2010 Takano D14/486
(Continued)

- OTHER PUBLICATIONS**
"iBlot® 2 Dry Blotting System How To Video" Nov. 14, 2013, YouTube, site visited Aug. 13, 2020: <https://www.youtube.com/watch?v=g7DT5xGheCE> (Year: 2013).*
(Continued)

Primary Examiner — Jack Reickel

- (57) **CLAIM**
The ornamental design for an electrophoresis and imaging system display screen with graphical user interface, as shown and described.

DESCRIPTION

FIG. 1 is a view of a first embodiment of an electrophoresis and imaging system display screen with graphical user interface of our new design.


FIG. 2 is a view of a second embodiment of an electrophoresis and imaging system display screen with graphical user interface of our new design.

FIG. 3 is a view of a third embodiment of an electrophoresis and imaging system display screen with graphical user interface of our new design; and,

FIG. 4 is a view of a fourth embodiment of an electrophoresis and imaging system display screen with graphical user interface of our new design.

The broken line showing of a display screen and portions of a graphical user interface is included for the purpose of illustrating portions of the article and forms no part of the claimed design.

1 Claim, 4 Drawing Sheets

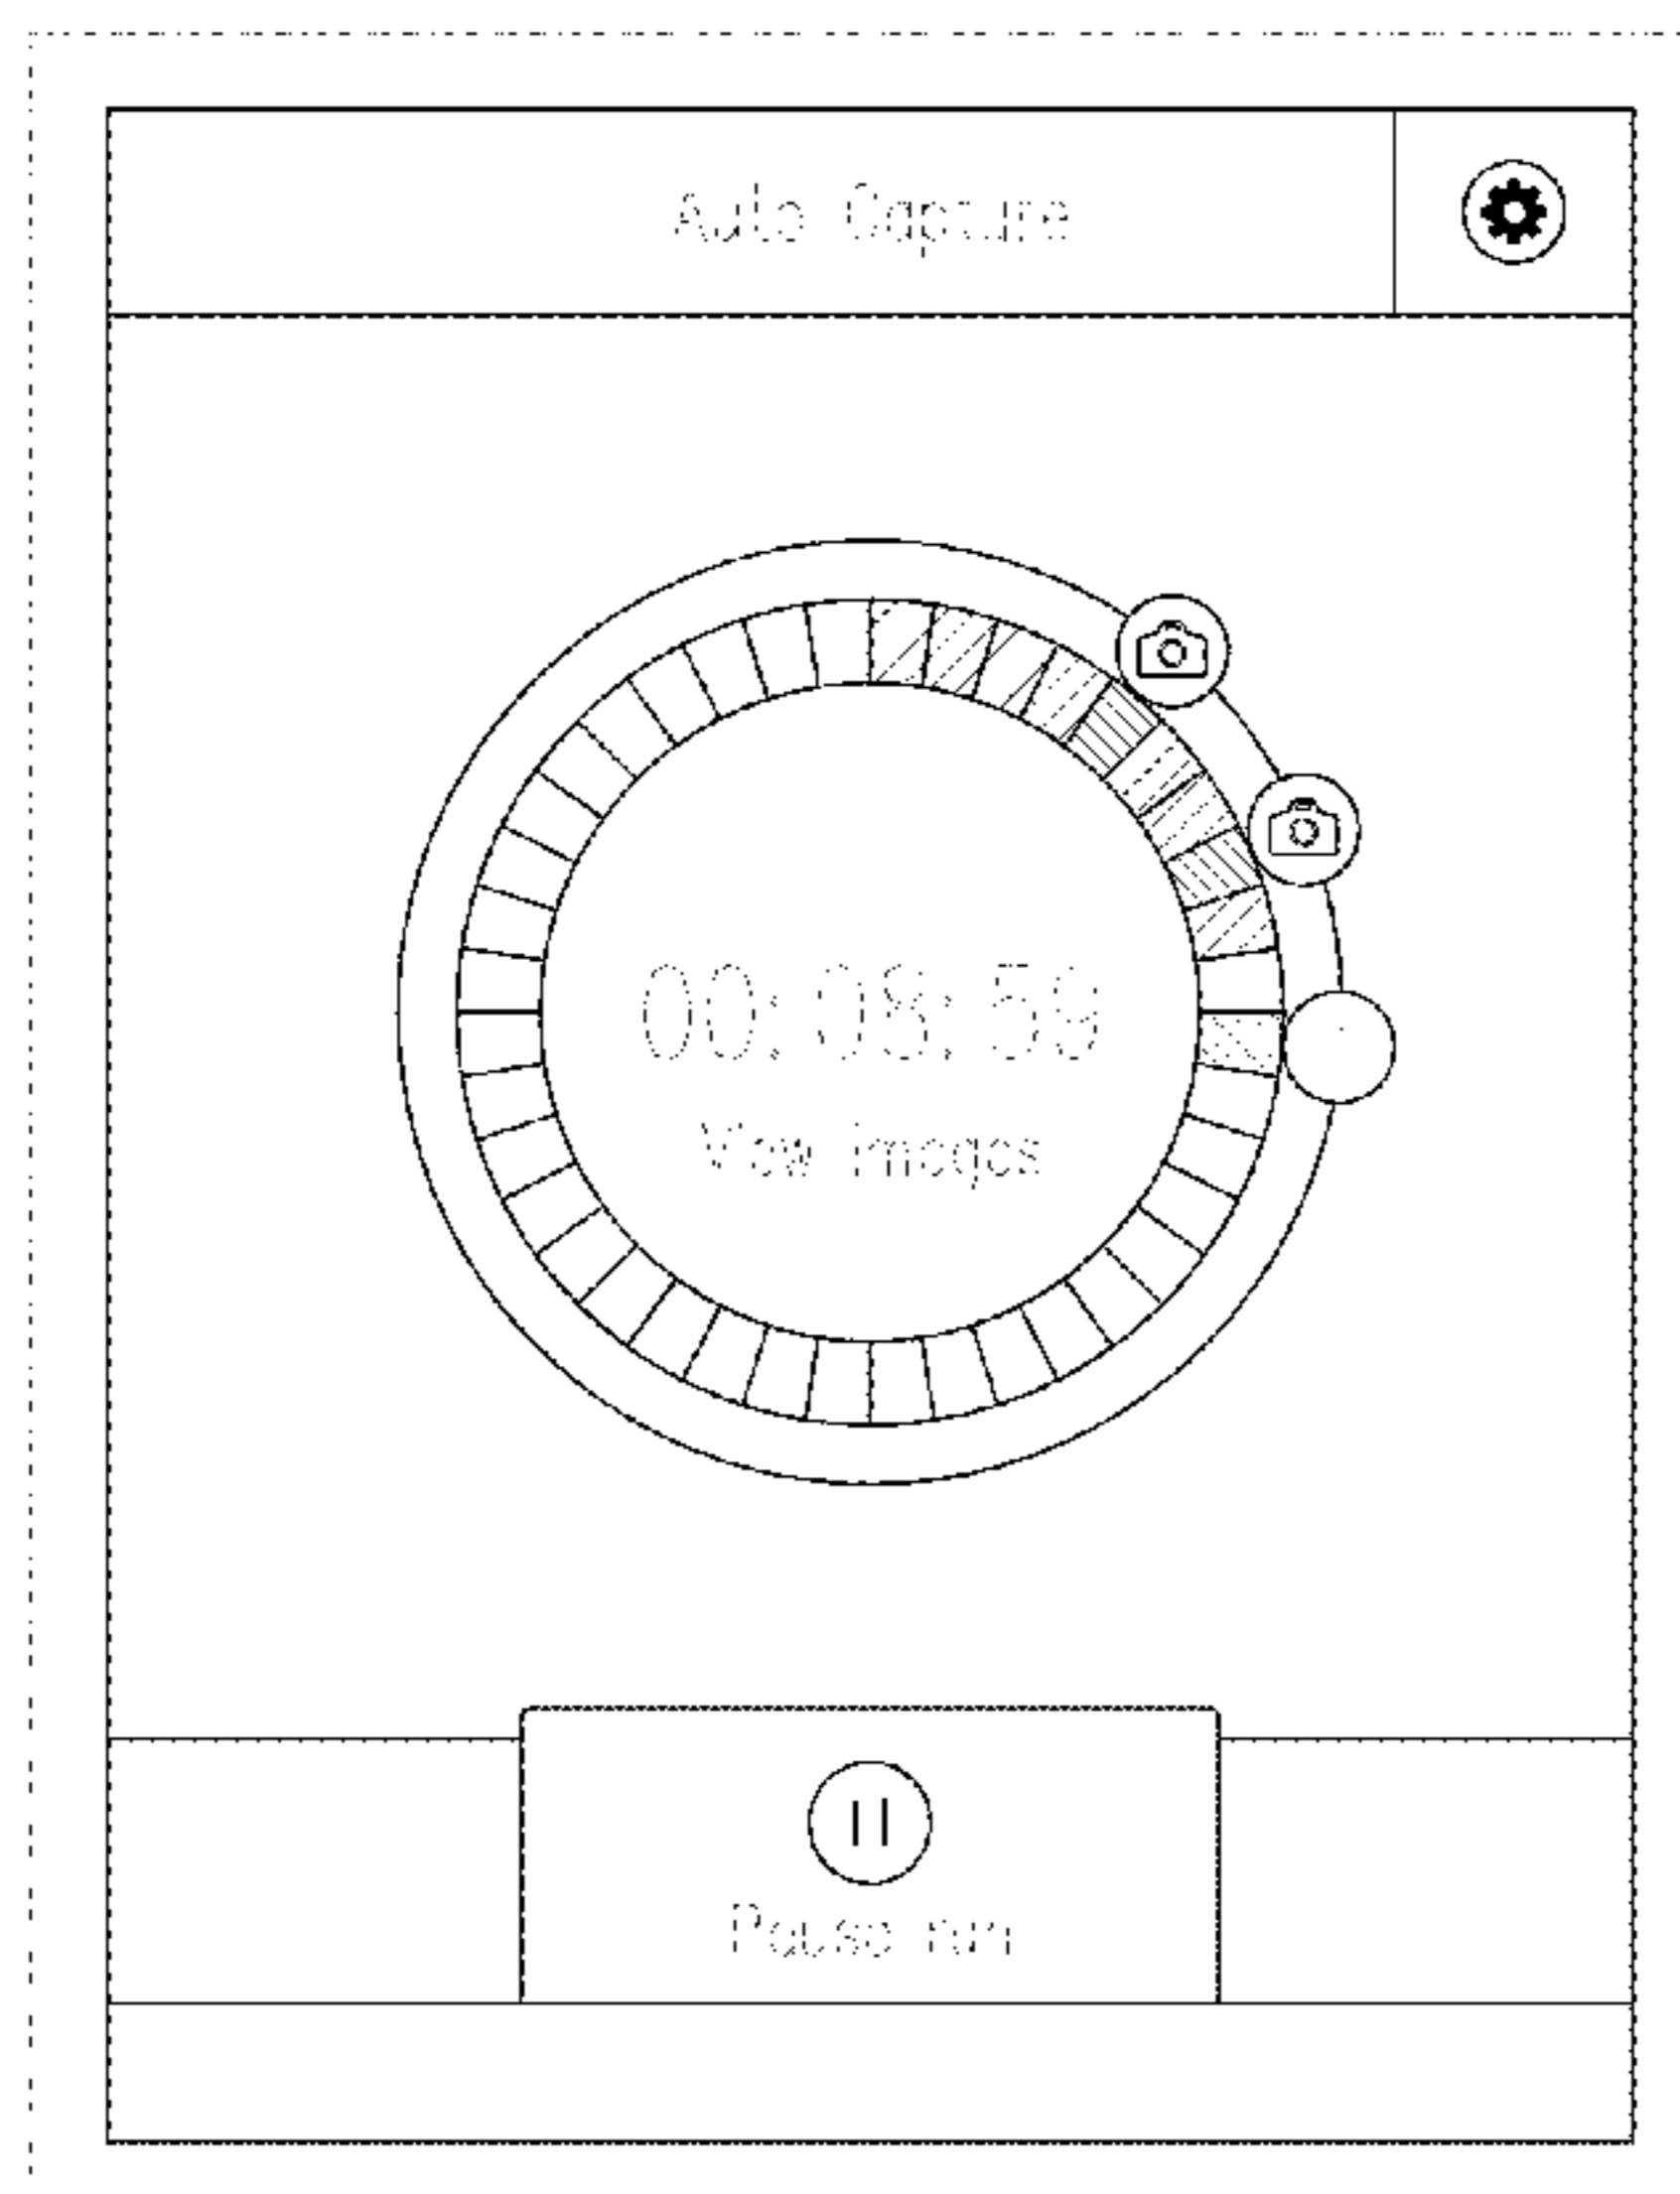

(56)

References Cited

U.S. PATENT DOCUMENTS

7,692,653 B1 * 4/2010 Petro G06T 11/20
345/440

D650,393 S 12/2011 Doll
D682,297 S 5/2013 DiJulio et al.
D697,935 S 1/2014 Lee et al.
D701,226 S * 3/2014 Jung D14/486
D706,806 S 6/2014 Nishizawa
D707,705 S 6/2014 Folken et al.
D715,811 S 10/2014 Tsukamoto
D716,320 S * 10/2014 Fan D14/485
D716,325 S * 10/2014 Brudnicki D14/486
D717,823 S 11/2014 Brotman et al.
D724,603 S * 3/2015 Williams D14/485
D732,049 S 6/2015 Amin et al.
D737,283 S 8/2015 Scalisi
D747,352 S * 1/2016 Lee D14/492
D751,090 S 3/2016 Hu et al.
D752,072 S 3/2016 Song
D752,618 S 3/2016 Lee et al.
D753,685 S 4/2016 Zimmerman et al.
D753,712 S * 4/2016 Lee G06F 3/04817
D14/489

D754,714 S 4/2016 Zhang et al.
D755,240 S * 5/2016 Cavander G06F 3/04817
D14/494

D758,422 S 6/2016 Zhao
D759,684 S 6/2016 Bijlani et al.
D769,314 S * 10/2016 Piroddi D14/488
D771,130 S 11/2016 Cho et al.
D772,249 S 11/2016 Choi et al.
D778,946 S * 2/2017 Epstein G06F 3/1454
D14/489

D784,387 S * 4/2017 Lee D14/486
D785,025 S 4/2017 Zimmerman et al.
D786,301 S * 5/2017 Napper D14/489
D790,581 S 6/2017 Chaudhri et al.
D792,444 S 7/2017 Cho et al.

D792,458 S * 7/2017 Chaudhri D14/489
D795,288 S 8/2017 McColl
D797,772 S 9/2017 Mizono et al.
D803,250 S * 11/2017 Lee D14/486
D808,974 S 1/2018 Chiappone et al.
D826,272 S * 8/2018 Lee D14/492
D826,963 S 8/2018 Guan et al.
D829,235 S 9/2018 Gangcuangco et al.
D831,035 S * 10/2018 McGlasson D14/485
D852,820 S * 7/2019 Sanchez D14/485
2009/0228820 A1 * 9/2009 Kim G06F 3/0482
715/769

2010/0313168 A1 * 12/2010 Wiest G06F 3/0236
715/830

2011/0071818 A1 * 3/2011 Jiang G06F 3/0236
704/8

2013/0127911 A1 * 5/2013 Brown G06F 3/04847
345/649

2014/0282016 A1 * 9/2014 Hosier, Jr. G06Q 50/01
715/733

2015/0058769 A1 * 2/2015 Kim G06F 3/04817
715/765

2016/0018978 A1 * 1/2016 Zenoff G06F 3/0488
715/731

2016/0021155 A1 * 1/2016 Sawato G06F 3/04817
455/456.1

OTHER PUBLICATIONS

“PXi and PXi Touch gel imaging systems” Jan. 10, 2014, YouTube, site visited Aug. 13, 2020: https://www.youtube.com/watch?v=RUL_AKSNr6I (Year: 2014).*

“Nuevos equipos Applied Biosystems para PCR en Tiempo Real” Nov. 23, 2015, YouTube, site visited Aug. 13, 2020: <https://www.youtube.com/watch?v=yYyNME6UVGc> (Year: 2015).*

“SimpliAmp™ Made Easy” May 12, 2014, YouTube, site visited Aug. 13, 2020: https://www.youtube.com/watch?v=QV_9QtOtLxs (Year: 2014).*

* cited by examiner

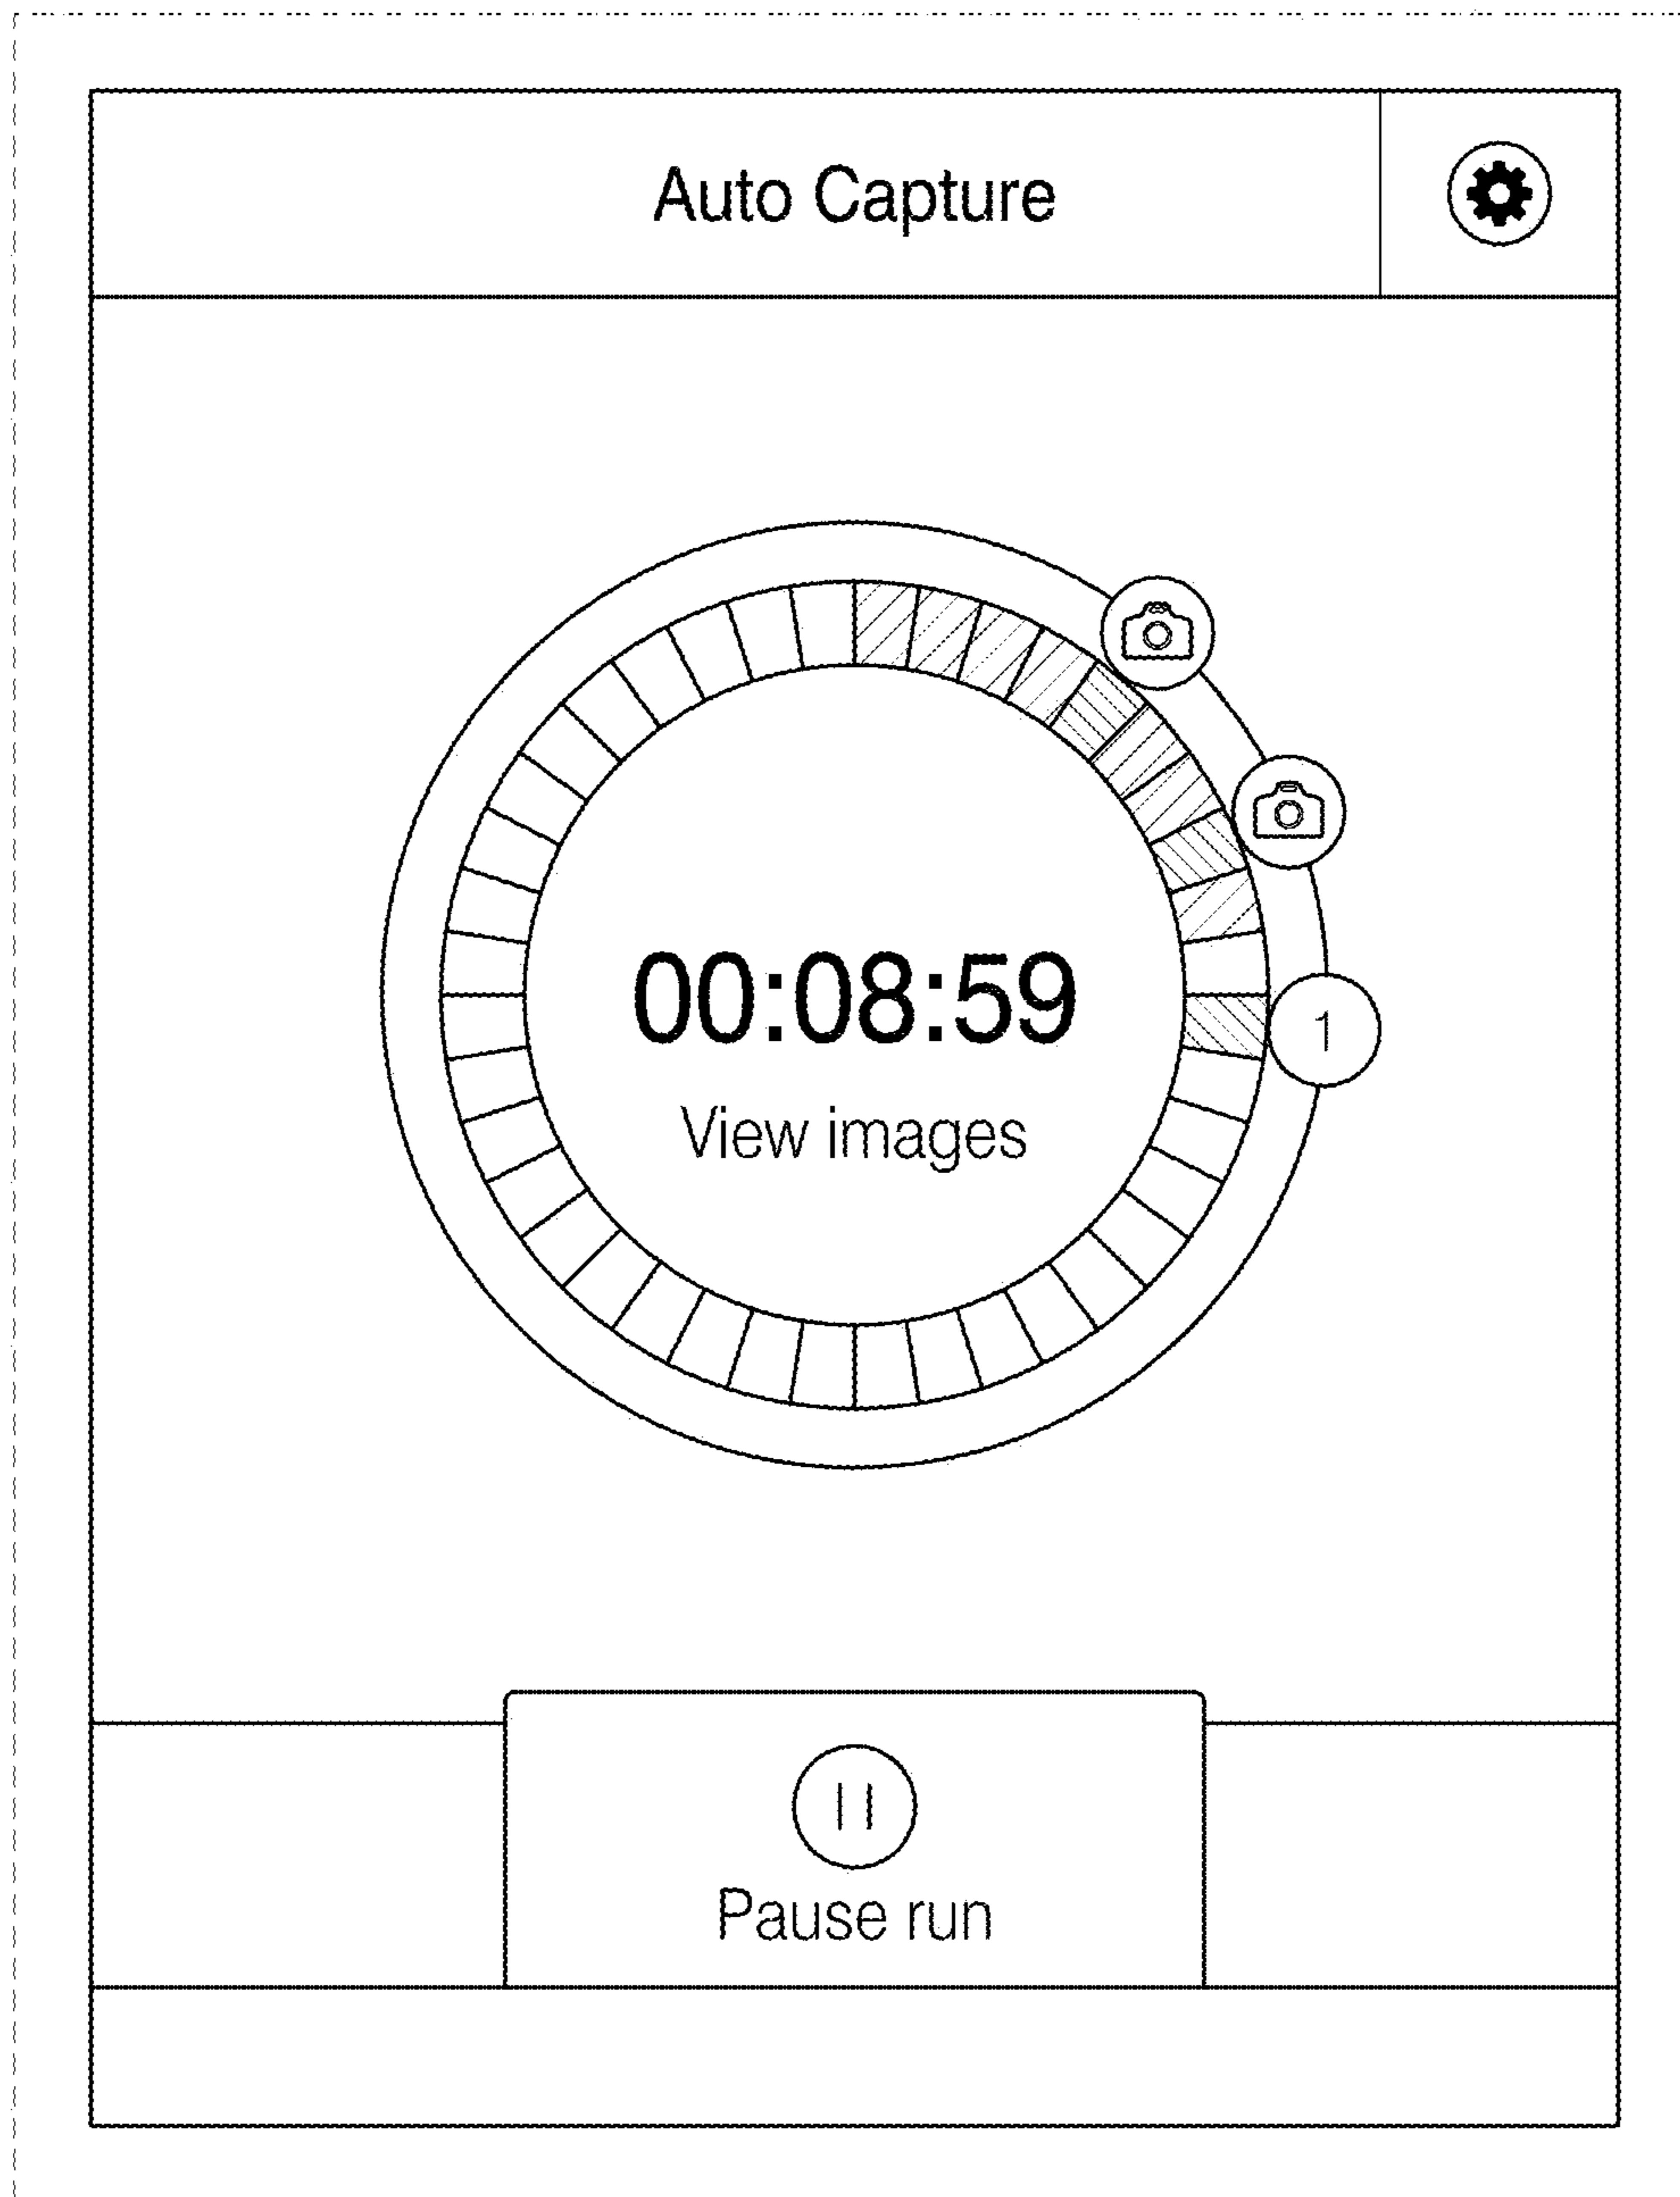


FIG. 1

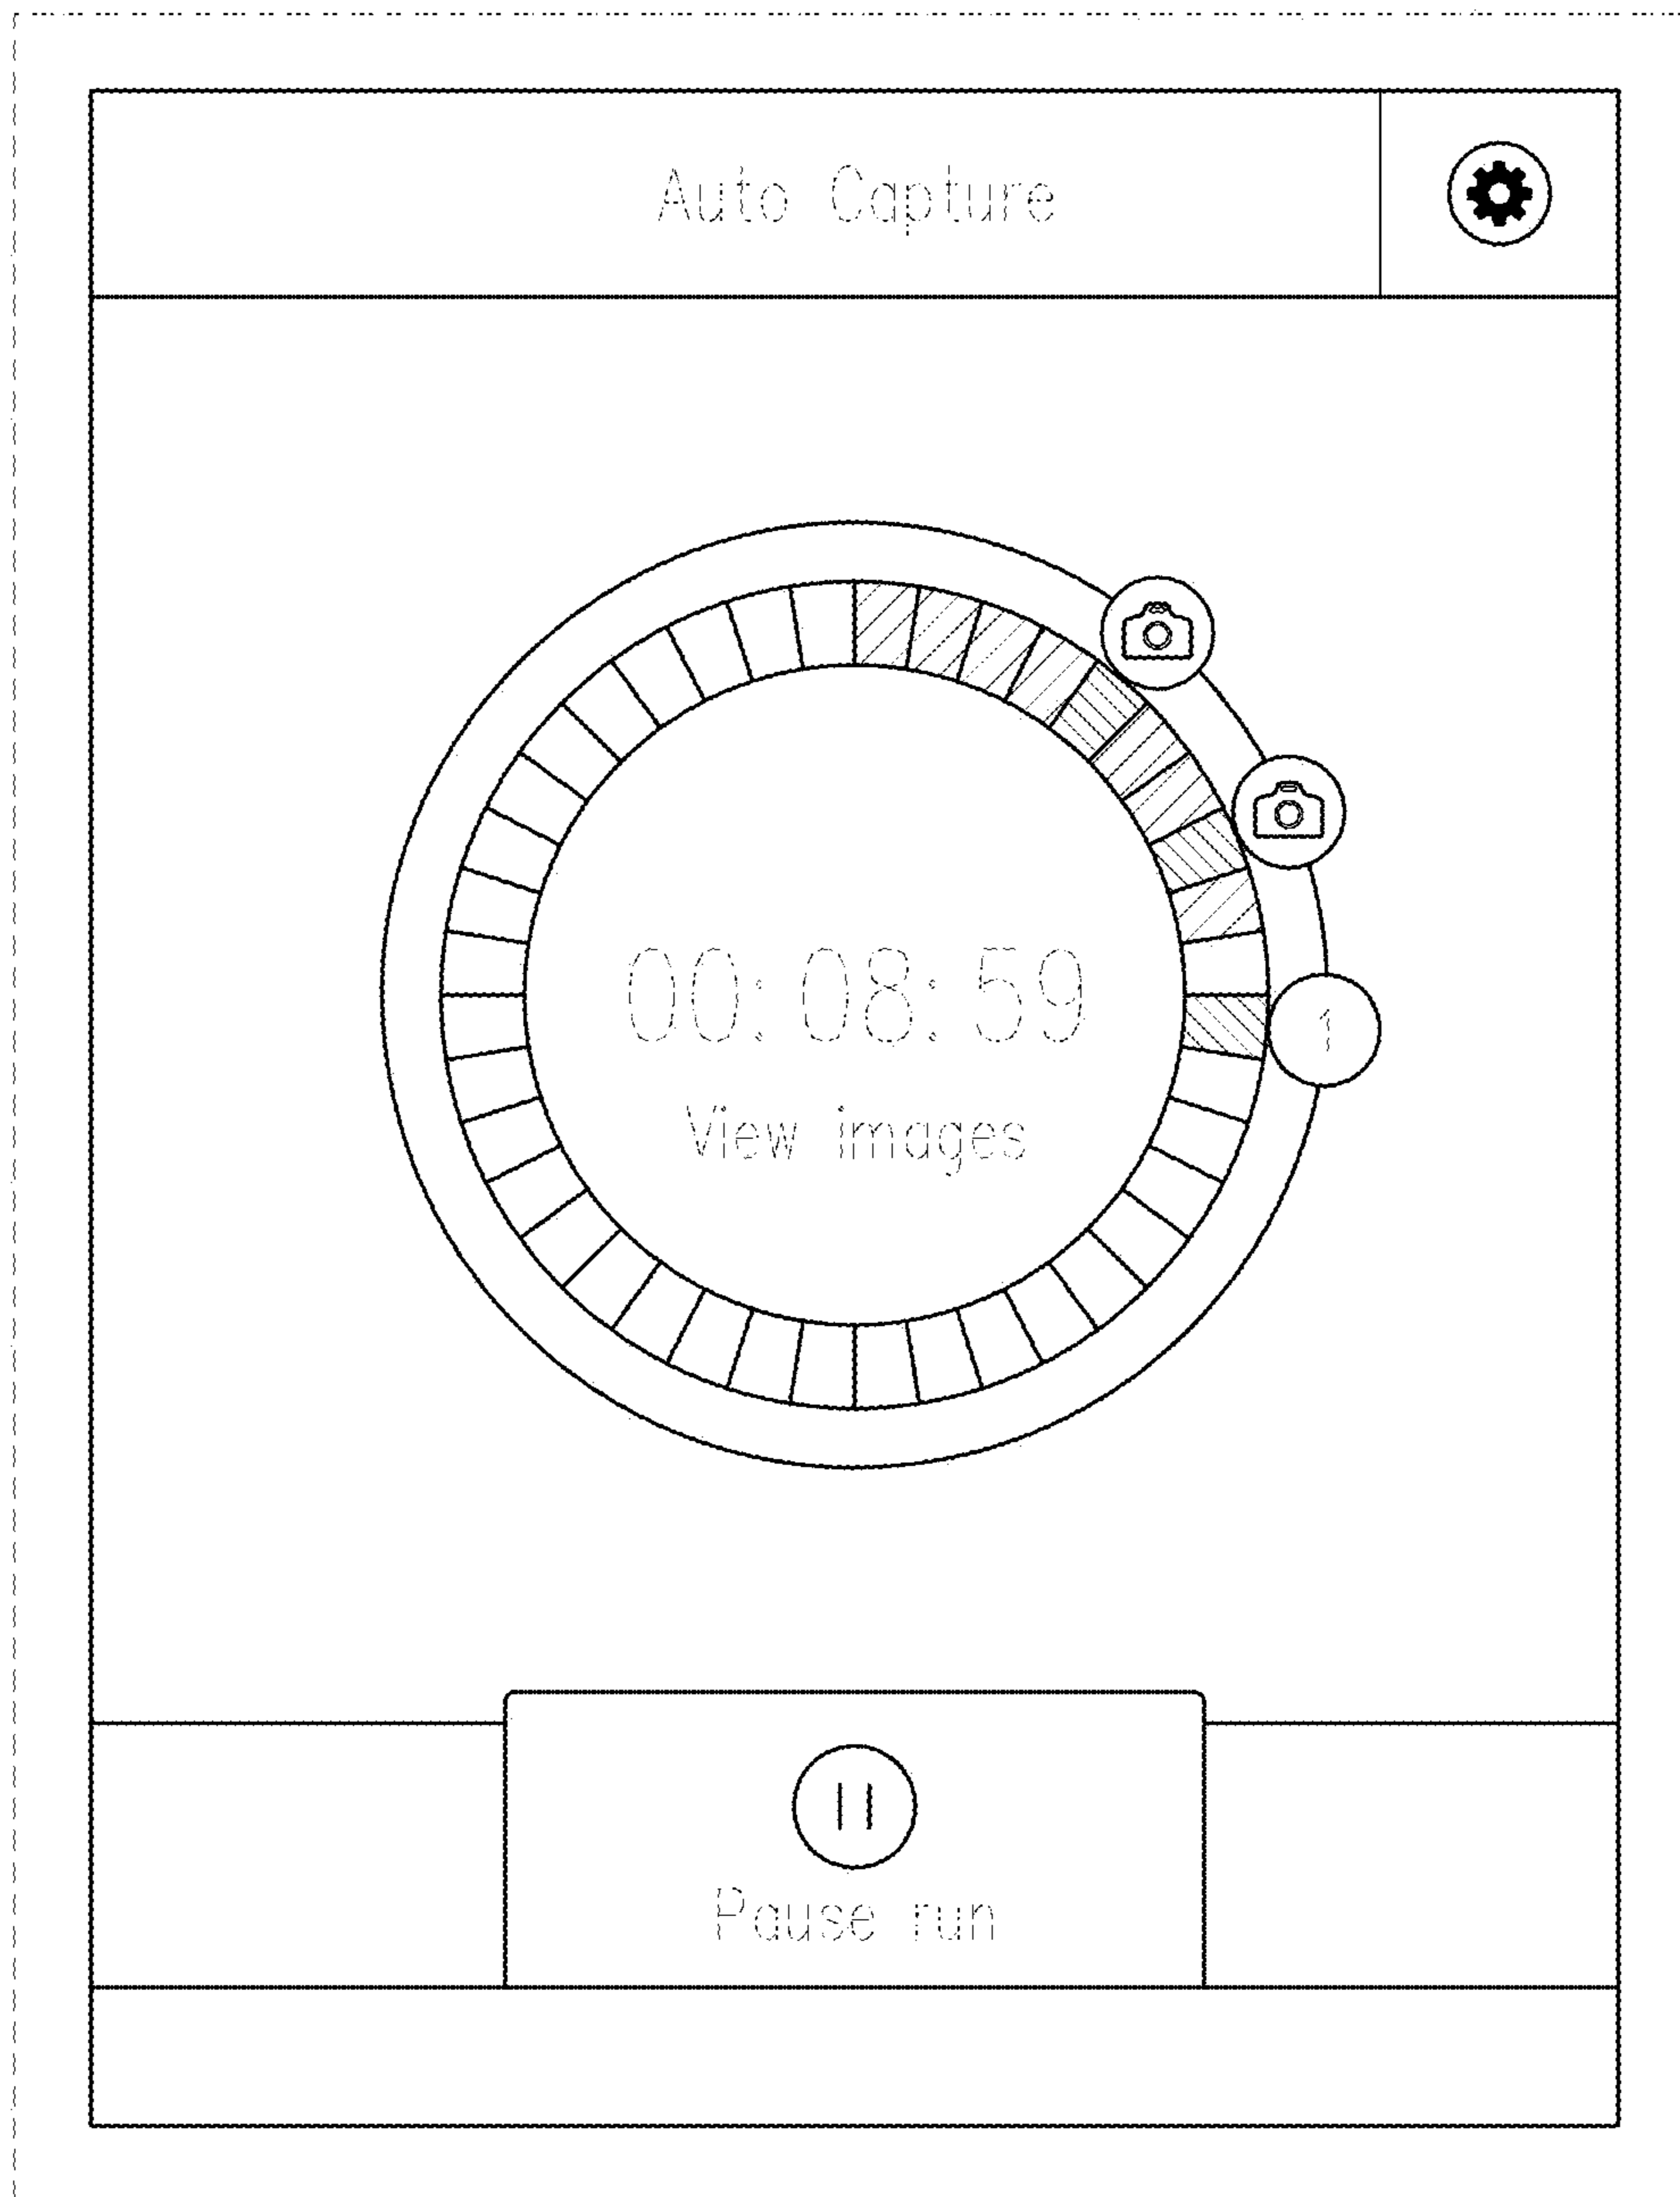


FIG. 2

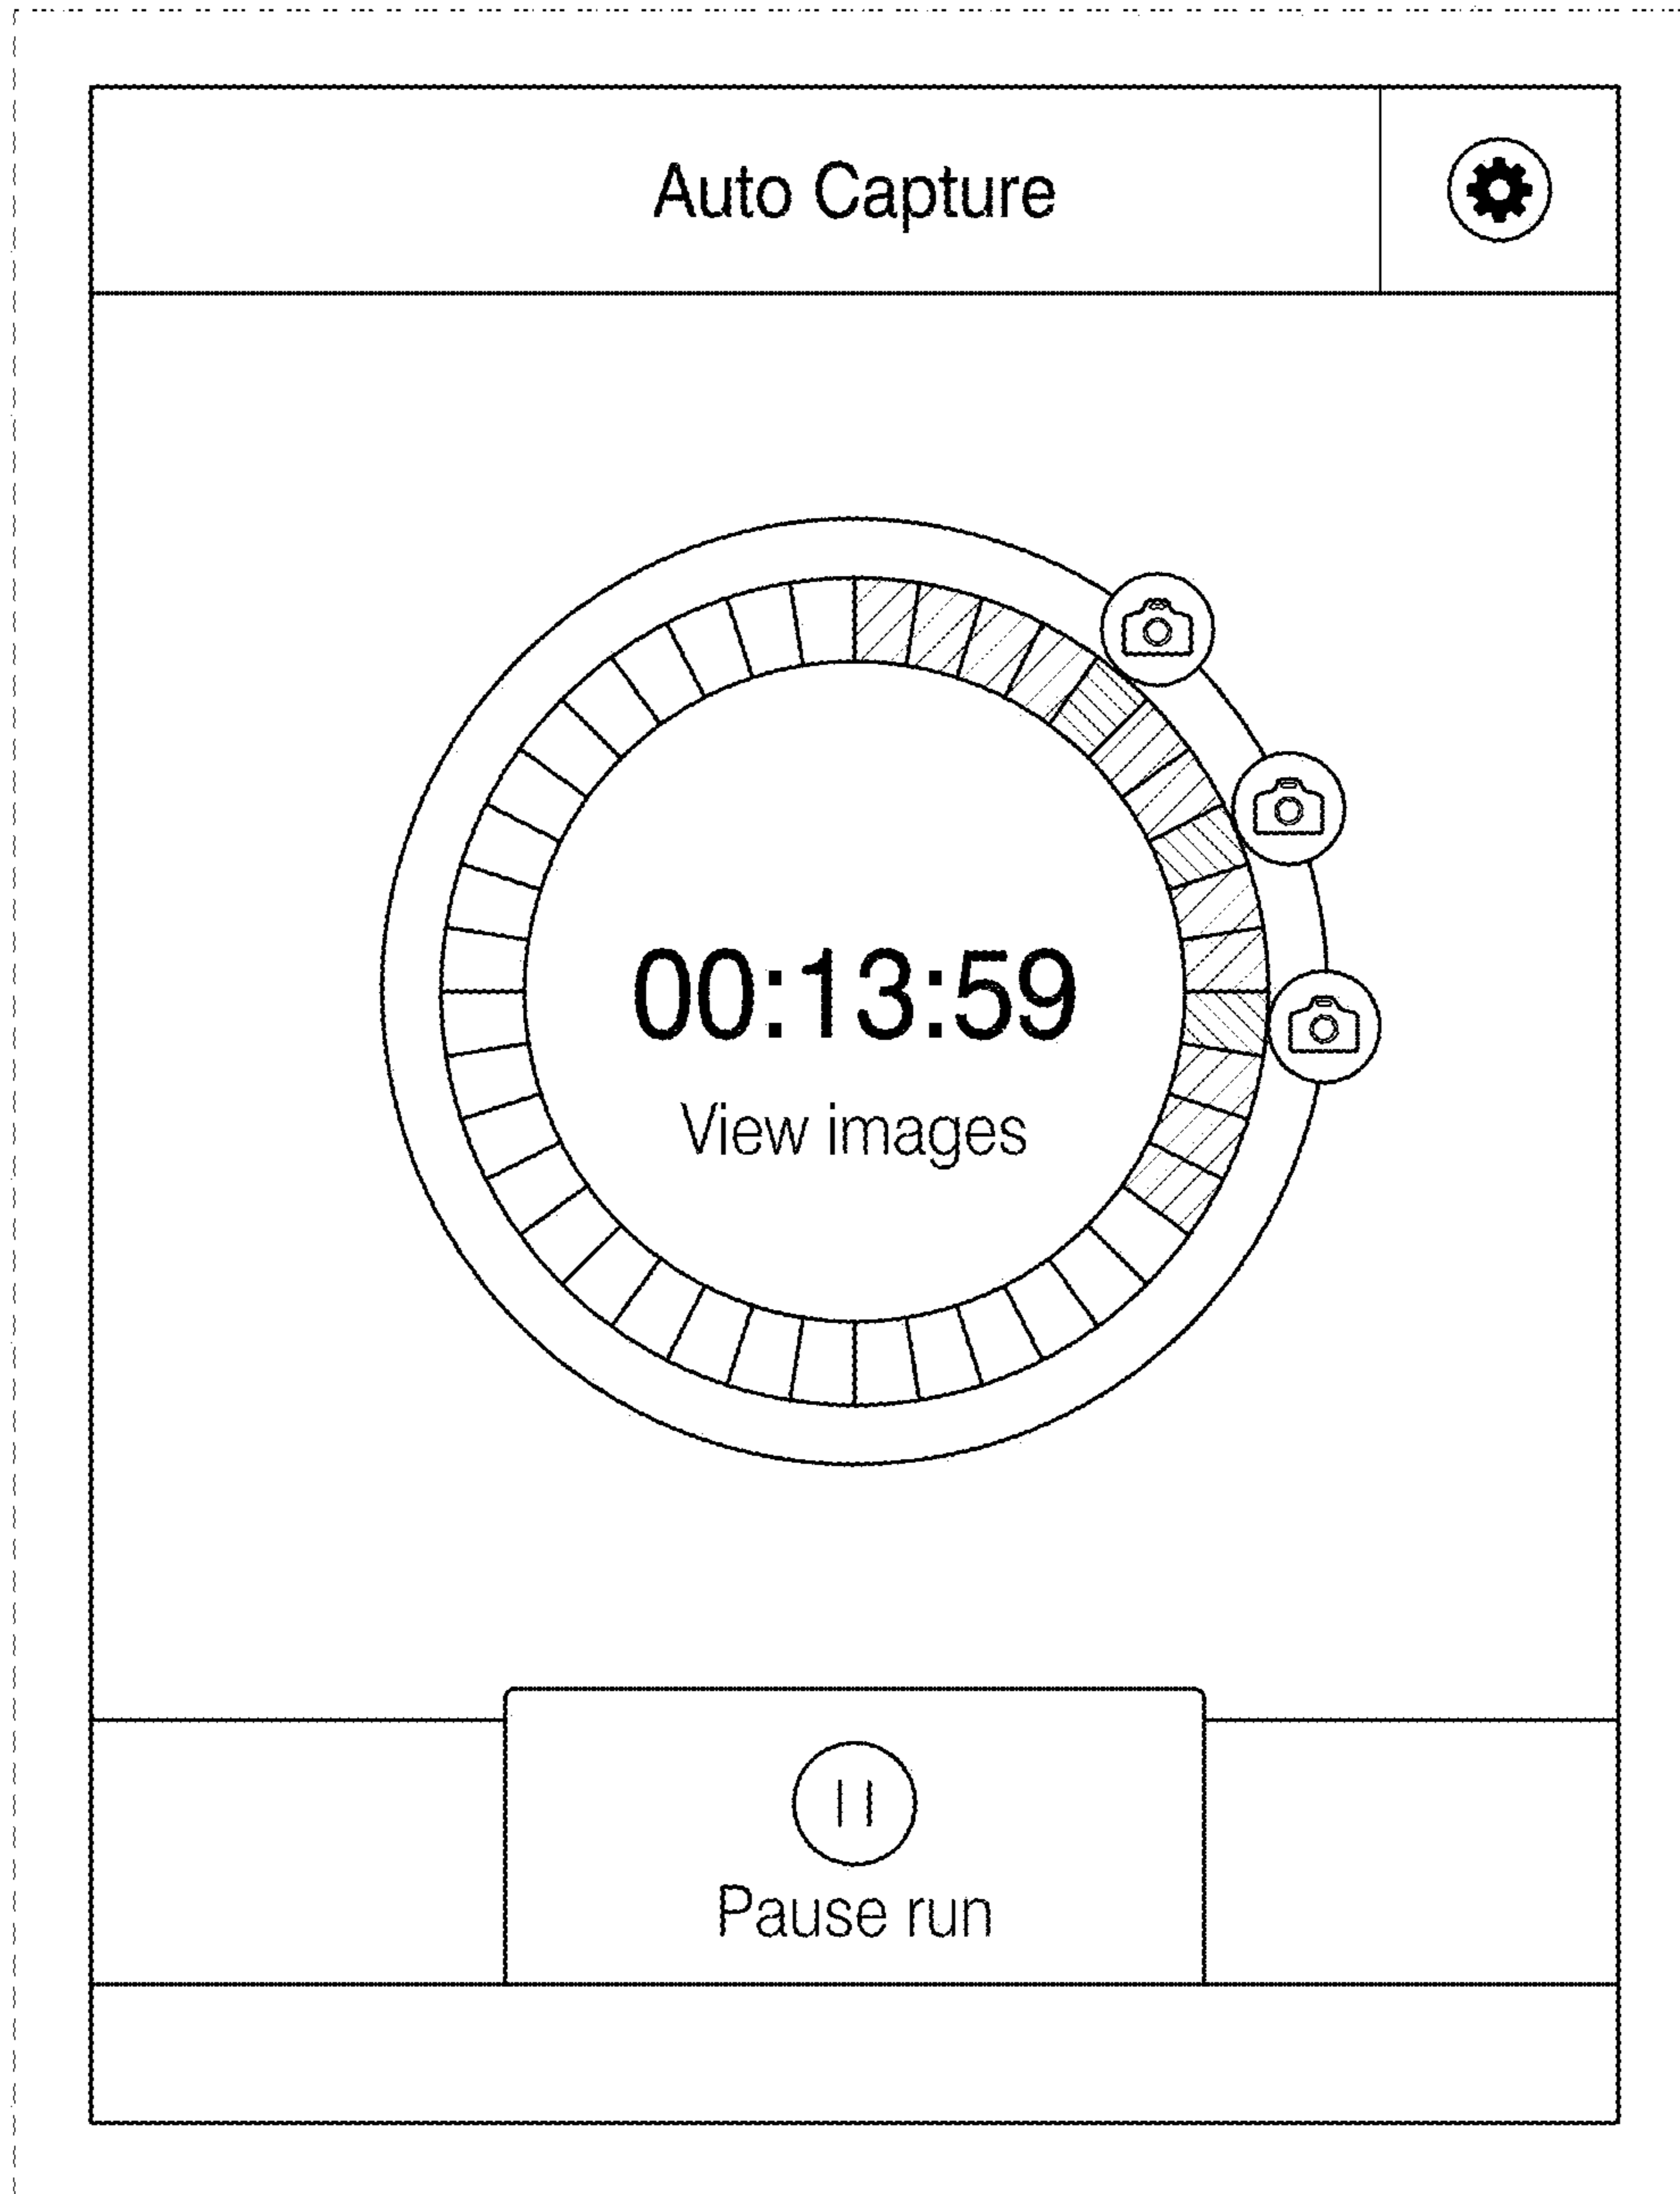


FIG. 3

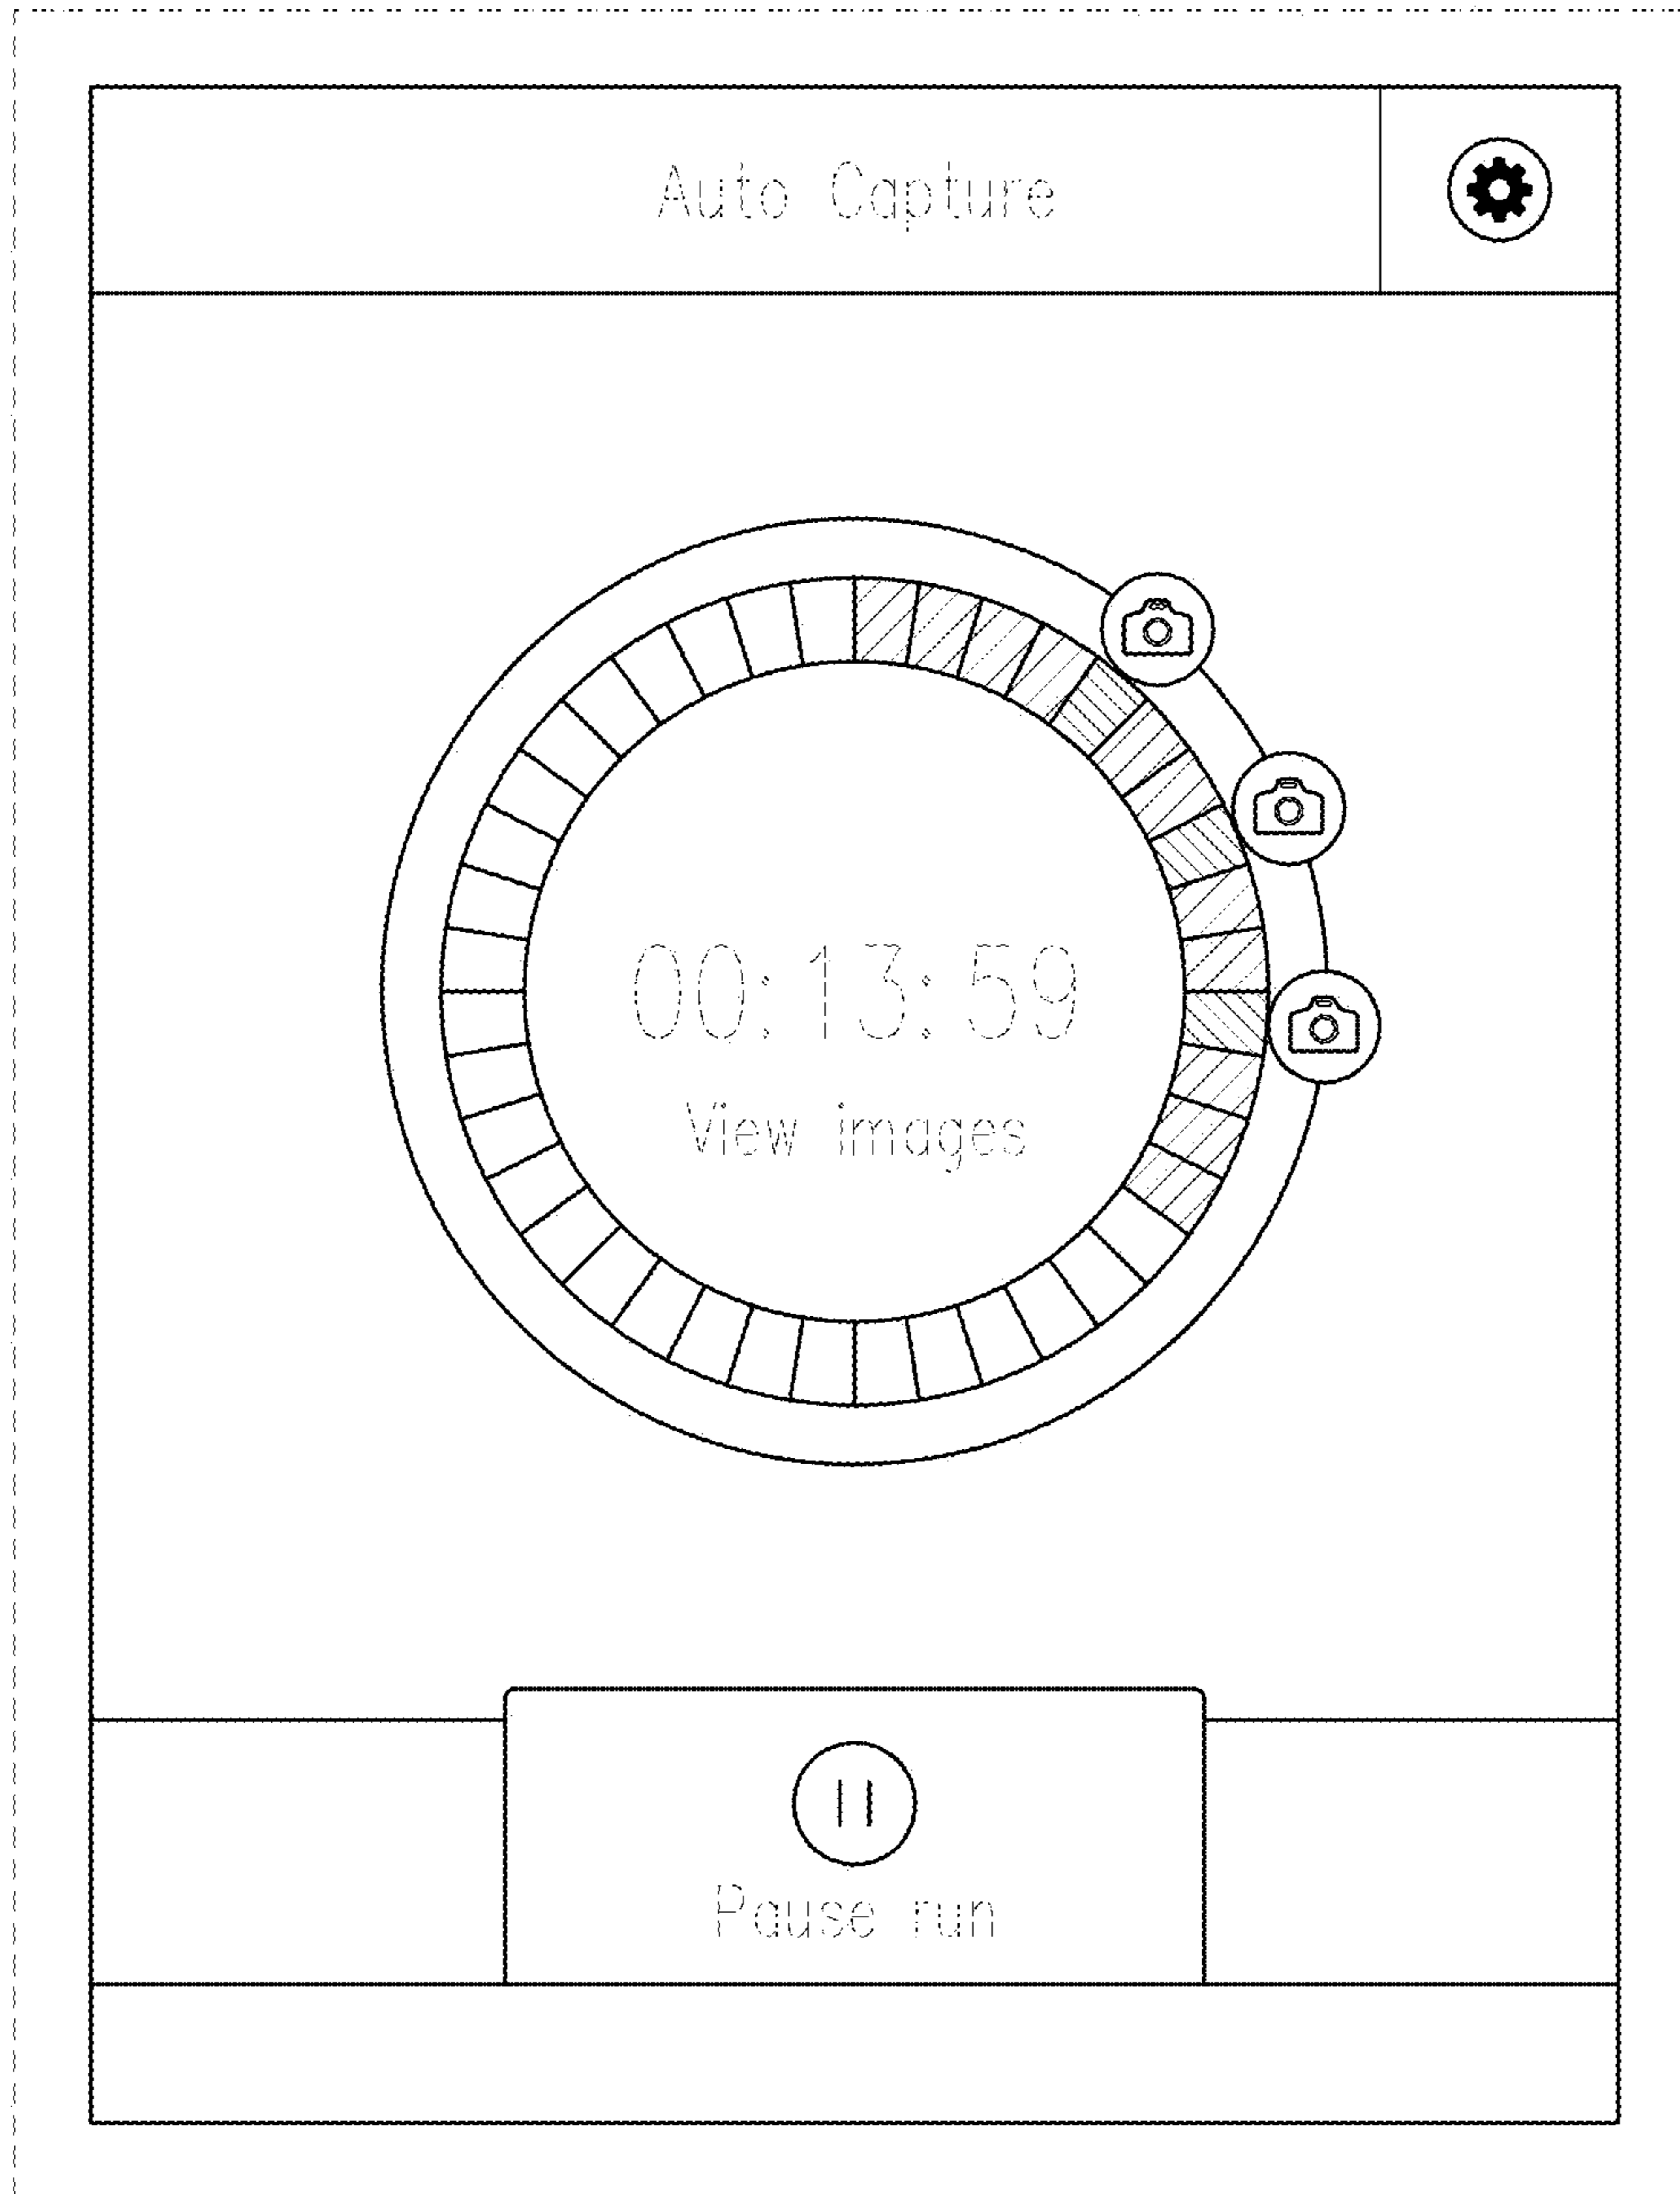


FIG. 4