



US00D901670S

(12) **United States Design Patent** (10) **Patent No.:** **US D901,670 S**  
**Tuononen et al.** (45) **Date of Patent:** **\*\* Nov. 10, 2020**

(54) **PRESSURE CONTROL UNIT**

3,878,839 A 4/1975 Norton et al.

(71) Applicant: **OTIVIO AS**, Oslo (NO)

3,896,794 A 7/1975 McGrath

(72) Inventors: **Sanna Tuononen**, Oslo (NO); **Petri Rantanen**, Oslo (NO)

3,977,396 A 8/1976 Cartier

4,054,129 A 10/1977 Byars et al.

4,149,529 A 4/1979 Copeland et al.

5,000,164 A 3/1991 Cooper

(Continued)

(73) Assignee: **OTIVIO AS**, Oslo (NO)

**FOREIGN PATENT DOCUMENTS**

(\*\*) Term: **15 Years**

EM 002650937-0002 3/2015

EM 002650937-0003 3/2015

(21) Appl. No.: **29/740,625**

(Continued)

(22) Filed: **Jul. 6, 2020**

**OTHER PUBLICATIONS**

**Related U.S. Application Data**

“Nanova Therapy System,” Acelity, retrieved from <https://www.acelity.com/products/nanova-therapy-system-uk> on Aug. 27, 2018, 11 Pages.

(63) Continuation of application No. 29/659,685, filed on Aug. 10, 2018, now Pat. No. Des. 889,634.

(Continued)

(51) **LOC (12) Cl.** ..... **24-01**

(52) **U.S. Cl.**

USPC ..... **D24/107**; D24/188

(58) **Field of Classification Search**

USPC ..... D24/107, 108, 111, 169, 185, 186, 188, D24/200, 213

CPC ..... A61M 2205/3344; A61H 2209/00; A61H 1/00; A61H 9/00

See application file for complete search history.

*Primary Examiner* — Lilyana Bekic

(74) *Attorney, Agent, or Firm* — Workman Nydegger

(57)

**CLAIM**

The ornamental design for a pressure control unit, as shown and described.

**DESCRIPTION**

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- 1,110,494 A 9/1914 Kellogg
- 1,399,095 A 12/1921 Webb, Sr.
- 2,113,253 A 4/1938 Gray
- 2,168,611 A 8/1939 Thompson
- 3,094,983 A 6/1963 MacLeod
- 3,292,613 A 12/1966 MacLeod
- 3,403,673 A 10/1968 MacLeod
- 3,465,748 A 9/1969 Kravchenko
- 3,654,919 A 4/1972 Birtwell
- 3,757,806 A 9/1973 Bhaskar et al.
- 3,859,989 A 1/1975 Spielberg

FIG. 1 is a front perspective view of a pressure control unit showing our new design.

FIG. 2 is a front elevational view thereof.

FIG. 3 is a rear elevational view thereof.

FIG. 4 is a first side elevational view thereof.


FIG. 5 is a second side elevational view thereof.

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines in the drawings depict portions of the pressure control unit that form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

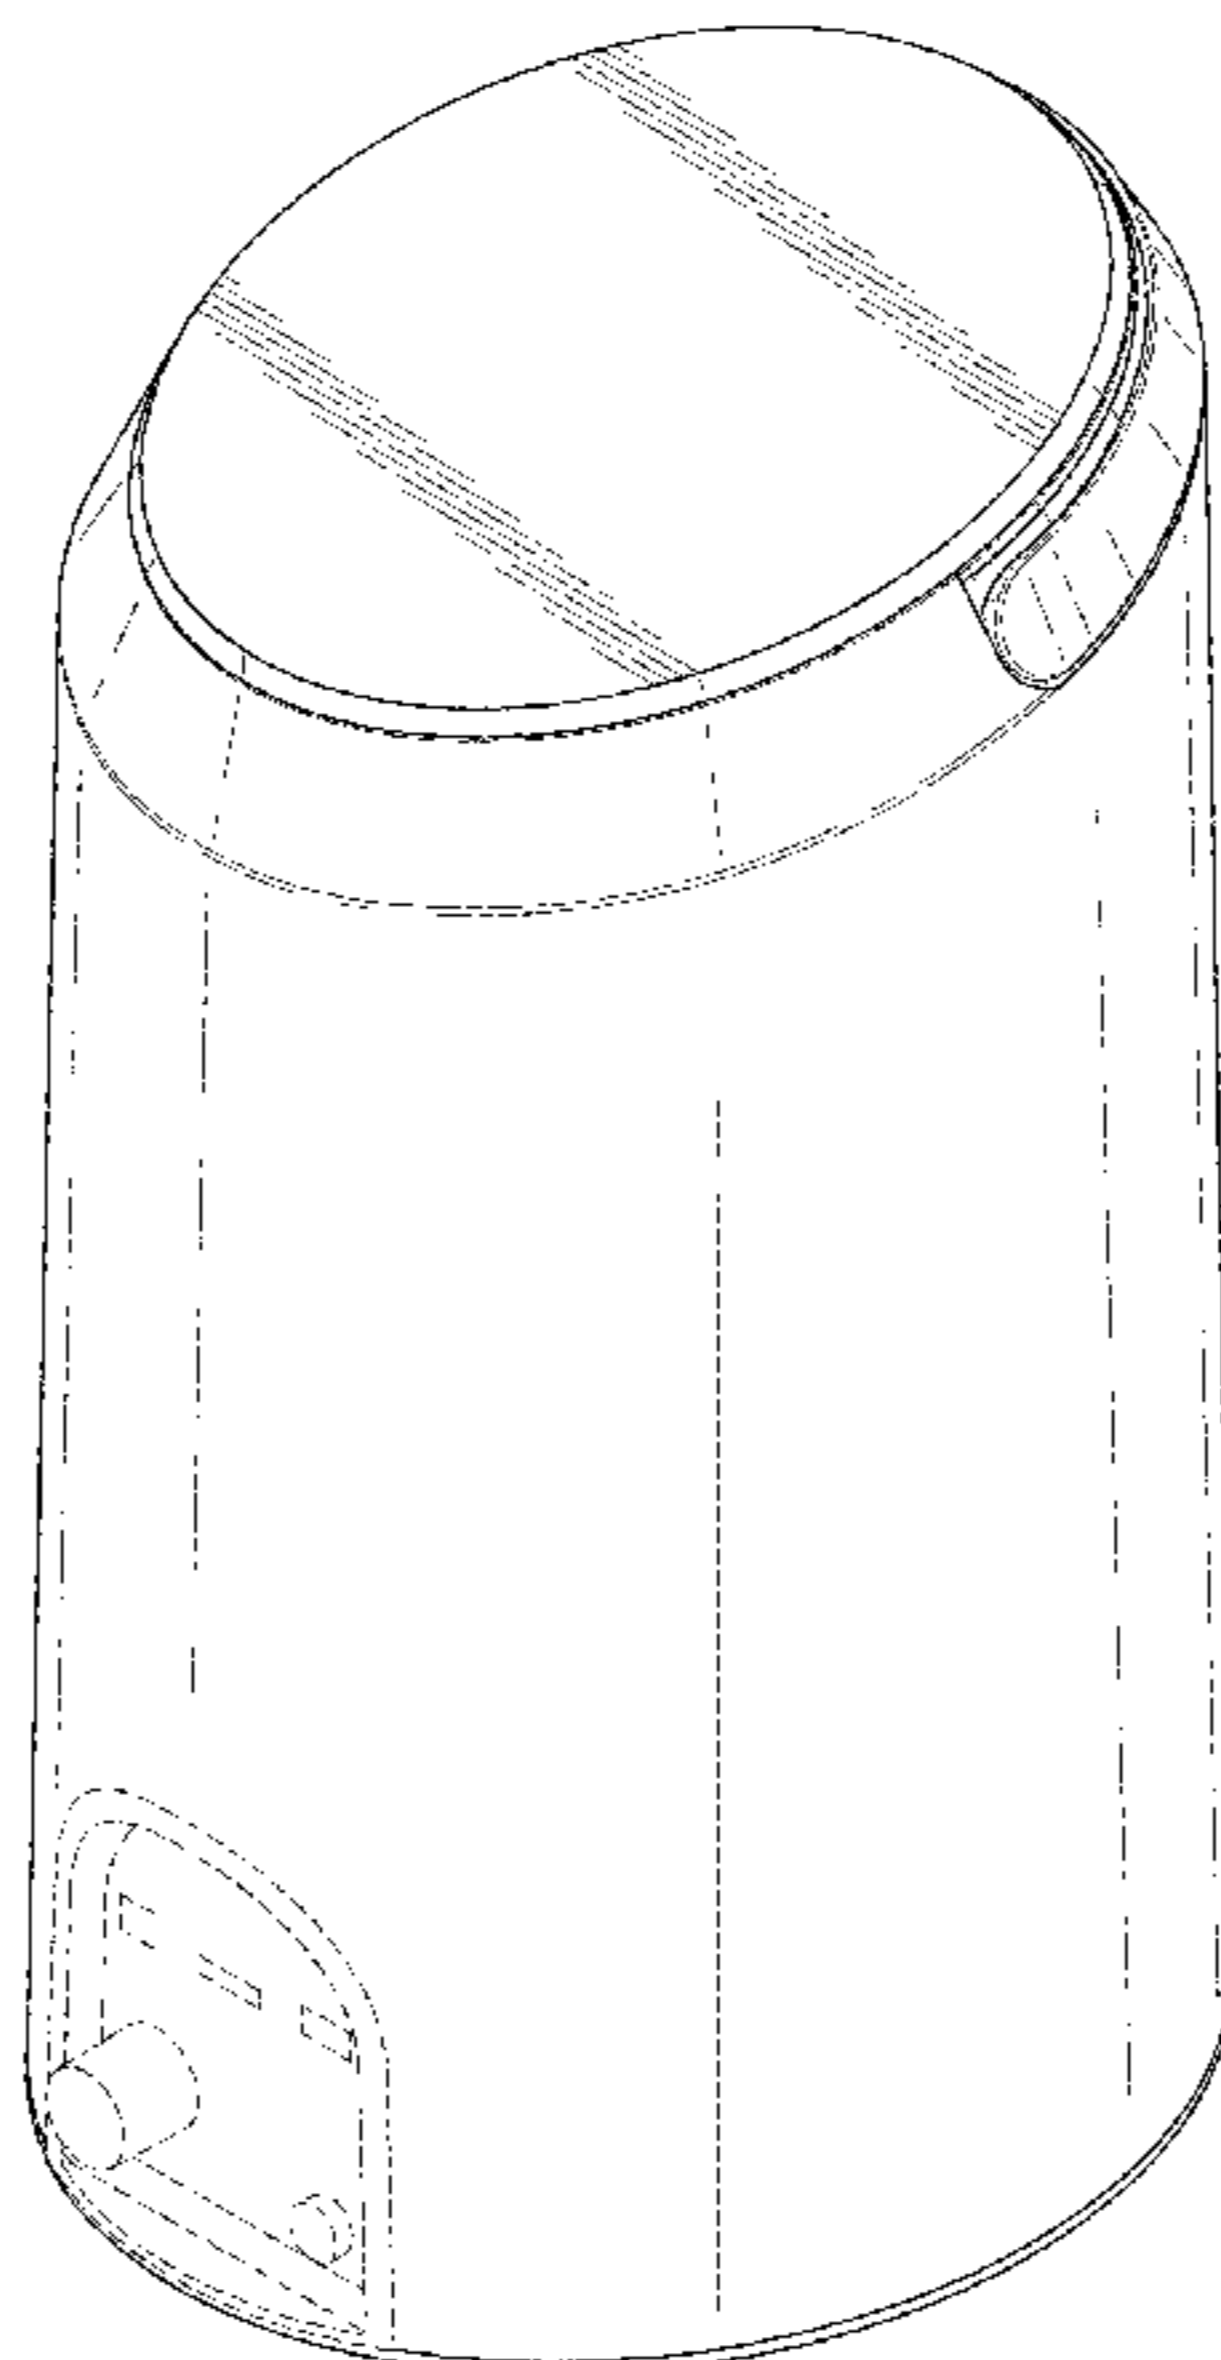

(56)

References Cited

U.S. PATENT DOCUMENTS

|              |      |         |                  |             |
|--------------|------|---------|------------------|-------------|
| 5,029,579    | A    | 7/1991  | Trammell         |             |
| 5,425,742    | A    | 6/1995  | Joy              |             |
| 5,458,562    | A    | 10/1995 | Cooper           |             |
| 5,697,920    | A    | 12/1997 | Gibbons          |             |
| 6,027,464    | A    | 2/2000  | Dahlquist        |             |
| 6,149,674    | A    | 11/2000 | Borders          |             |
| 6,277,052    | B1   | 8/2001  | Howard           |             |
| D452,570     | S    | 12/2001 | Since            |             |
| 6,423,017    | B2   | 7/2002  | Brotz            |             |
| 6,565,593    | B2   | 5/2003  | Diana            |             |
| 7,354,410    | B2   | 4/2008  | Perry et al.     |             |
| 7,833,179    | B2   | 11/2010 | Filtvedt et al.  |             |
| 7,833,180    | B2   | 11/2010 | Filtvedt et al.  |             |
| 7,896,825    | B2   | 3/2011  | Atkinson et al.  |             |
| D644,250     | S    | 8/2011  | Barber et al.    |             |
| 8,021,314    | B2   | 9/2011  | Filtvedt et al.  |             |
| 8,100,887    | B2   | 1/2012  | Weston et al.    |             |
| 8,361,001    | B2   | 1/2013  | Filtvedt et al.  |             |
| 8,657,864    | B2   | 2/2014  | Rein et al.      |             |
| 8,821,422    | B2   | 9/2014  | Filtvedt et al.  |             |
| D790,070     | S    | 6/2017  | Acosta et al.    |             |
| D791,955     | S    | 7/2017  | Gilbert et al.   |             |
| D816,854     | S    | 5/2018  | Acosta et al.    |             |
| D857,215     | S    | 8/2019  | Lin              |             |
| 10,646,626   | B2 * | 5/2020  | Huang            | F04B 35/06  |
| D889,634     | S *  | 7/2020  | Tuononen         | D24/107     |
| 2003/0097163 | A1   | 5/2003  | Kane et al.      |             |
| 2003/0125649 | A1   | 7/2003  | McIntosh et al.  |             |
| 2005/0027218 | A1   | 2/2005  | Filtvedt et al.  |             |
| 2005/0137446 | A1   | 6/2005  | Rastegar et al.  |             |
| 2009/0143719 | A1   | 6/2009  | Loori et al.     |             |
| 2009/0312675 | A1   | 12/2009 | Sampson et al.   |             |
| 2010/0152633 | A1   | 6/2010  | Rein et al.      |             |
| 2011/0000484 | A1   | 1/2011  | Melsheimer       |             |
| 2011/0130712 | A1   | 6/2011  | Topaz            |             |
| 2011/0288458 | A1   | 11/2011 | Jones et al.     |             |
| 2012/0209153 | A1   | 8/2012  | Farrow et al.    |             |
| 2012/0238924 | A1   | 9/2012  | Avni             |             |
| 2013/0331747 | A1   | 12/2013 | Helgeson et al.  |             |
| 2014/0128781 | A1   | 5/2014  | Rein et al.      |             |
| 2014/0276288 | A1   | 9/2014  | Randolph et al.  |             |
| 2015/0065931 | A1   | 3/2015  | Alnabulsi et al. |             |
| 2015/0374571 | A1   | 12/2015 | Denson et al.    |             |
| 2020/0078224 | A1 * | 3/2020  | Carroll          | A61M 1/0088 |
| 2020/0101208 | A1 * | 4/2020  | Freedman         | A61M 1/0084 |

FOREIGN PATENT DOCUMENTS

|    |                |         |
|----|----------------|---------|
| EM | 002650937-0004 | 3/2015  |
| EM | 002650937-0005 | 3/2015  |
| EM | 0026509370001  | 3/2015  |
| FR | 1562252 A      | 4/1969  |
| WO | 98/40039 A1    | 9/1998  |
| WO | 01/80790 A1    | 11/2001 |
| WO | 03/45289       | 6/2003  |
| WO | 2004/058131 A2 | 7/2004  |

OTHER PUBLICATIONS

Allen et al., "Intermittent Pressure and Suction in the Treatment of Chronic Occlusive Arterial Disease," The Journal of the American Medical Association, vol. 105, No. 25, Dec. 21, 1935, pp. 2029-2034.

de Takats, "Obliterative Vascular Disease: Preliminary Report on Treatment by Alternating Negative and Positive Pressure," Journal of the American Medical Association, vol. 103, No. 25, Dec. 22, 1934, pp. 1920-1924.

FlowOx First Time Assembly Instructional Video. Posted by Otivio AS on YouTube.com. Date published: Apr. 3, 2019. Retrieved from Internet: [https://www.youtube.com/watch?v=2VVStprMr28&feature=emb\\_Jogo](https://www.youtube.com/watch?v=2VVStprMr28&feature=emb_Jogo) (Year 2019).

Goodney et al., "National Trends in Lower Extremity Bypass Surgery, Endovascular Interventions, and Major Amputations", Journal of Vascular Surgery vol. 50 No. 1, Jul. 2009, pp. 54-60.

Herrmann et al., "Passive Vascular Exercises: Treatment of Peripheral Obliterative Arterial Diseases by Rhythmic Alternation of Environmental Pressure," Archives of Surgery, vol. 29, No. 5, Nov. 1934, pp. 697-704.

Herrmann et al., "The Conservative Treatment of Arteriosclerotic Peripheral Vascular Diseases: Passive Vascular Exercises (Pavaex Therapy)," Annals of Surgery, vol. 100, No. 4, Oct. 1934, pp. 750-760.

Hiramori et al., "Impact of Runoff Grade After Endovascular Therapy for Femoropopliteal Lesions", Journal of Vascular Surgery, vol. 59, No. 3, Mar. 2014, pp. 720-727.

Landis et al., "The Effects of Alternate Suction and Pressure on Blood Flow to the Lower Extremities," The Journal of Clinical Investigation, vol. 12, No. 5, Sep. 1933, pp. 925-961.

Landis et al., "Treatment of Peripheral Vascular Disease by Means of Suction and Pressure," Annals of Internal Medicine, vol. 9, No. 3, Sep. 1, 1935, pp. 264-273.

Meyer et al., "Bier's Hyperemic Treatment," California State Journal of Medicine, vol. 8, No. 4, Apr. 1910, pp. 142-143.

Norgren et al., "Inter-Society Consensus for the Management of Peripheral Arterial Disease (TASC II)", Journal of Vascular Surgery, Vol, 45, No. 1, Supplement S, Jan. 2007, p. S5A-S67A.

Reid, "Diagnosis and Treatment of Peripheral Vascular Diseases," The American Journal of Surgery, vol. 24, No. 1, Apr. 1934, pp. 11-35.

Rowe et al., "Patterns of Treatment for Peripheral Arterial Disease in the United States: 1996-2005", Journal of Vascular Surgery vol. 49, No. 4, Apr. 2009, pp. 910-917.

Siracuse et al., "Results for Primary Bypass Versus Primary Angioplasty/Stent for Intermittent Claudication Due to Superficial Femoral Artery Occlusive Disease", Journal of Vascular Surgery, vol. 55, No. 4, Apr. 2012, pp. 1001-1007.

Theis et al., "Peripheral Circulatory Diseases Effect of Alternating Positive and Negative Pressure Treatments on Venous Blood and the Skin Temperatures: Preliminary Report," The Journal of the American Medical Association, vol. 107, No. 14, Oct. 3, 1936, pp. 1097-1104.

\* cited by examiner

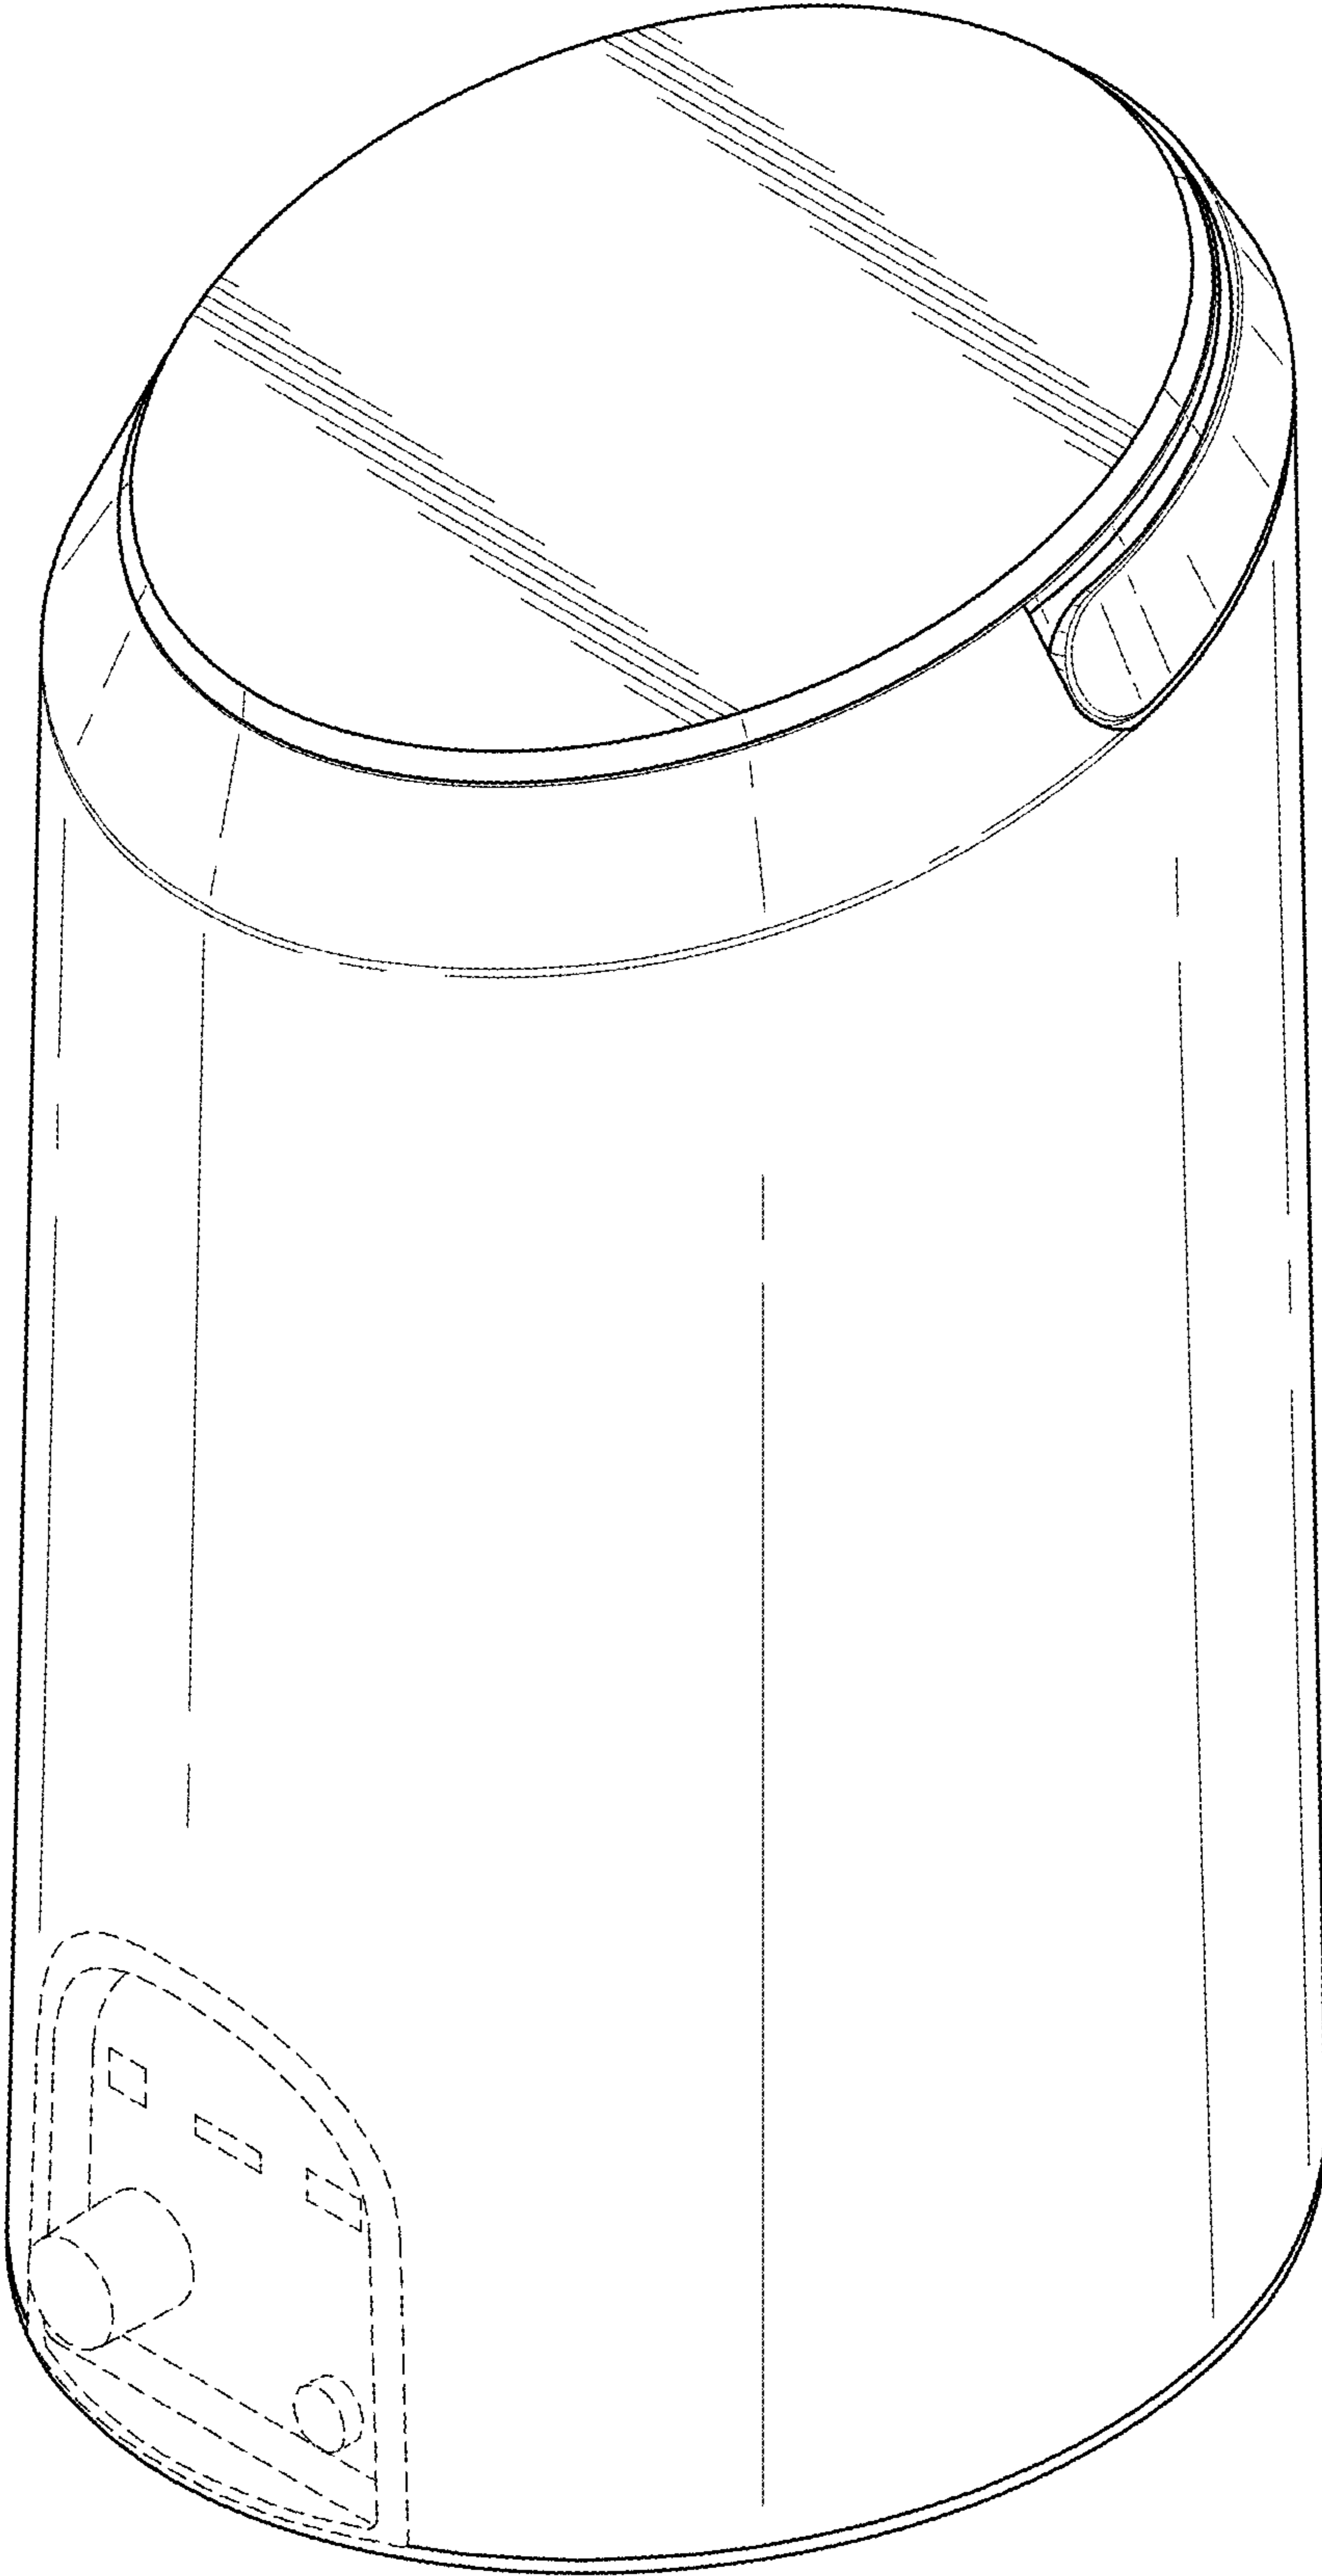


FIG. 1

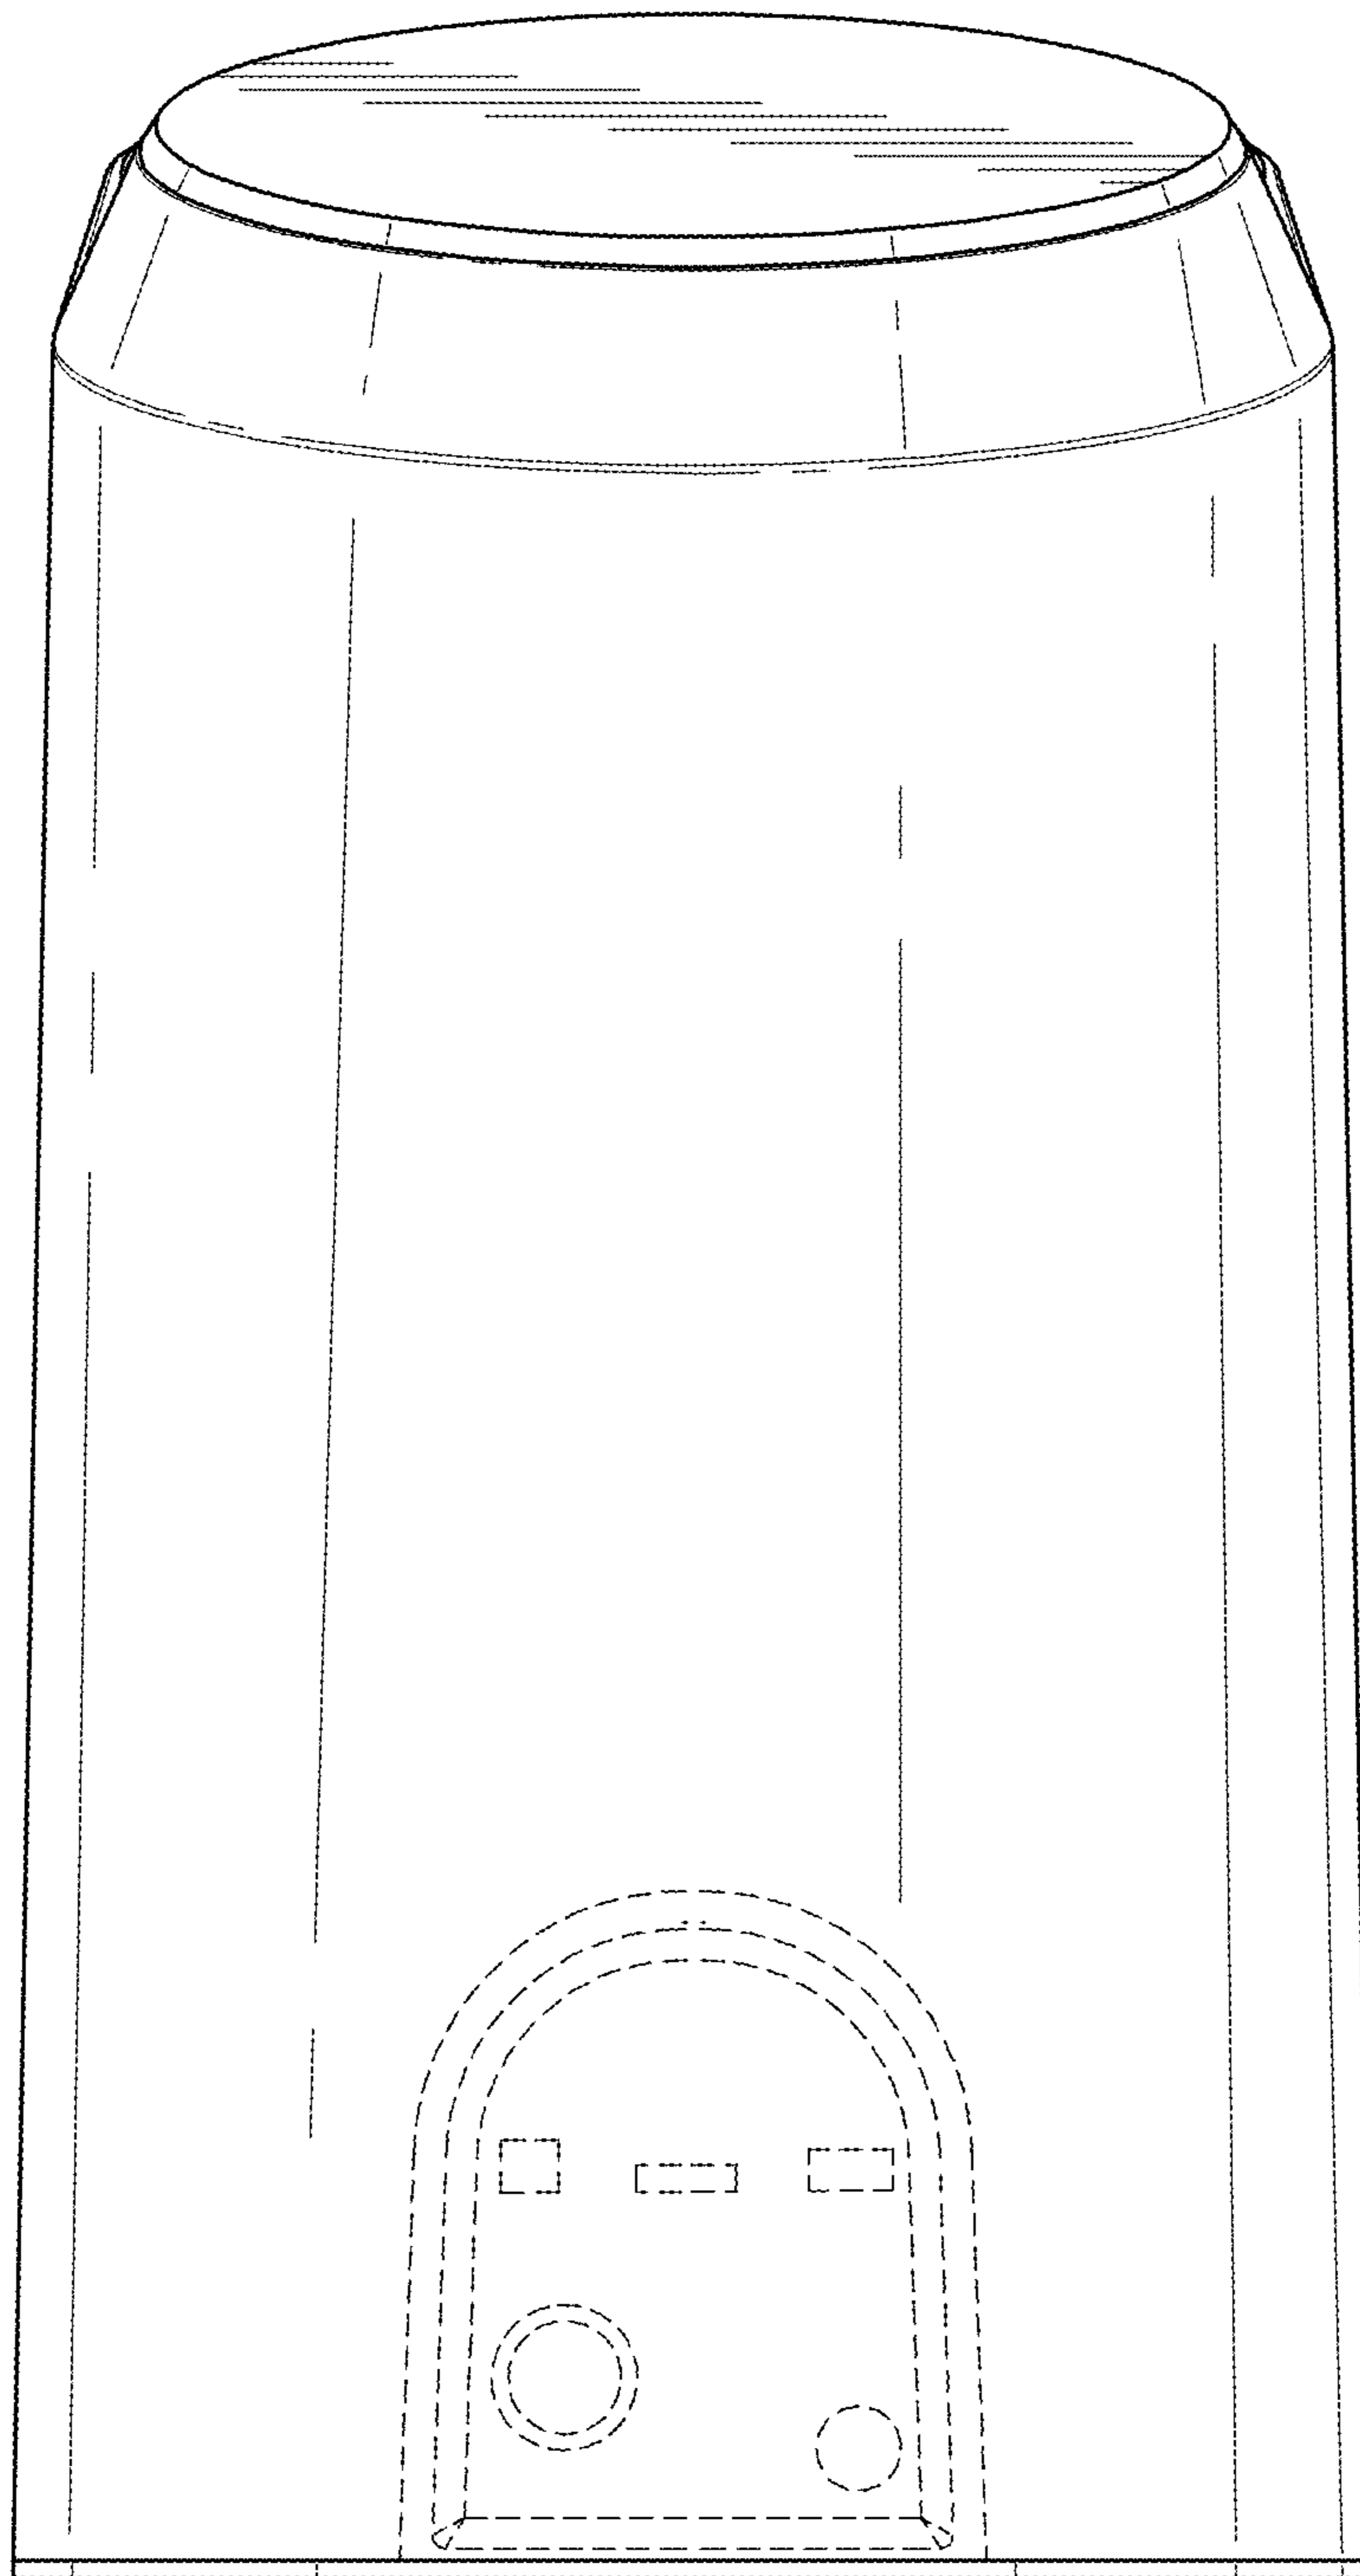


FIG. 2

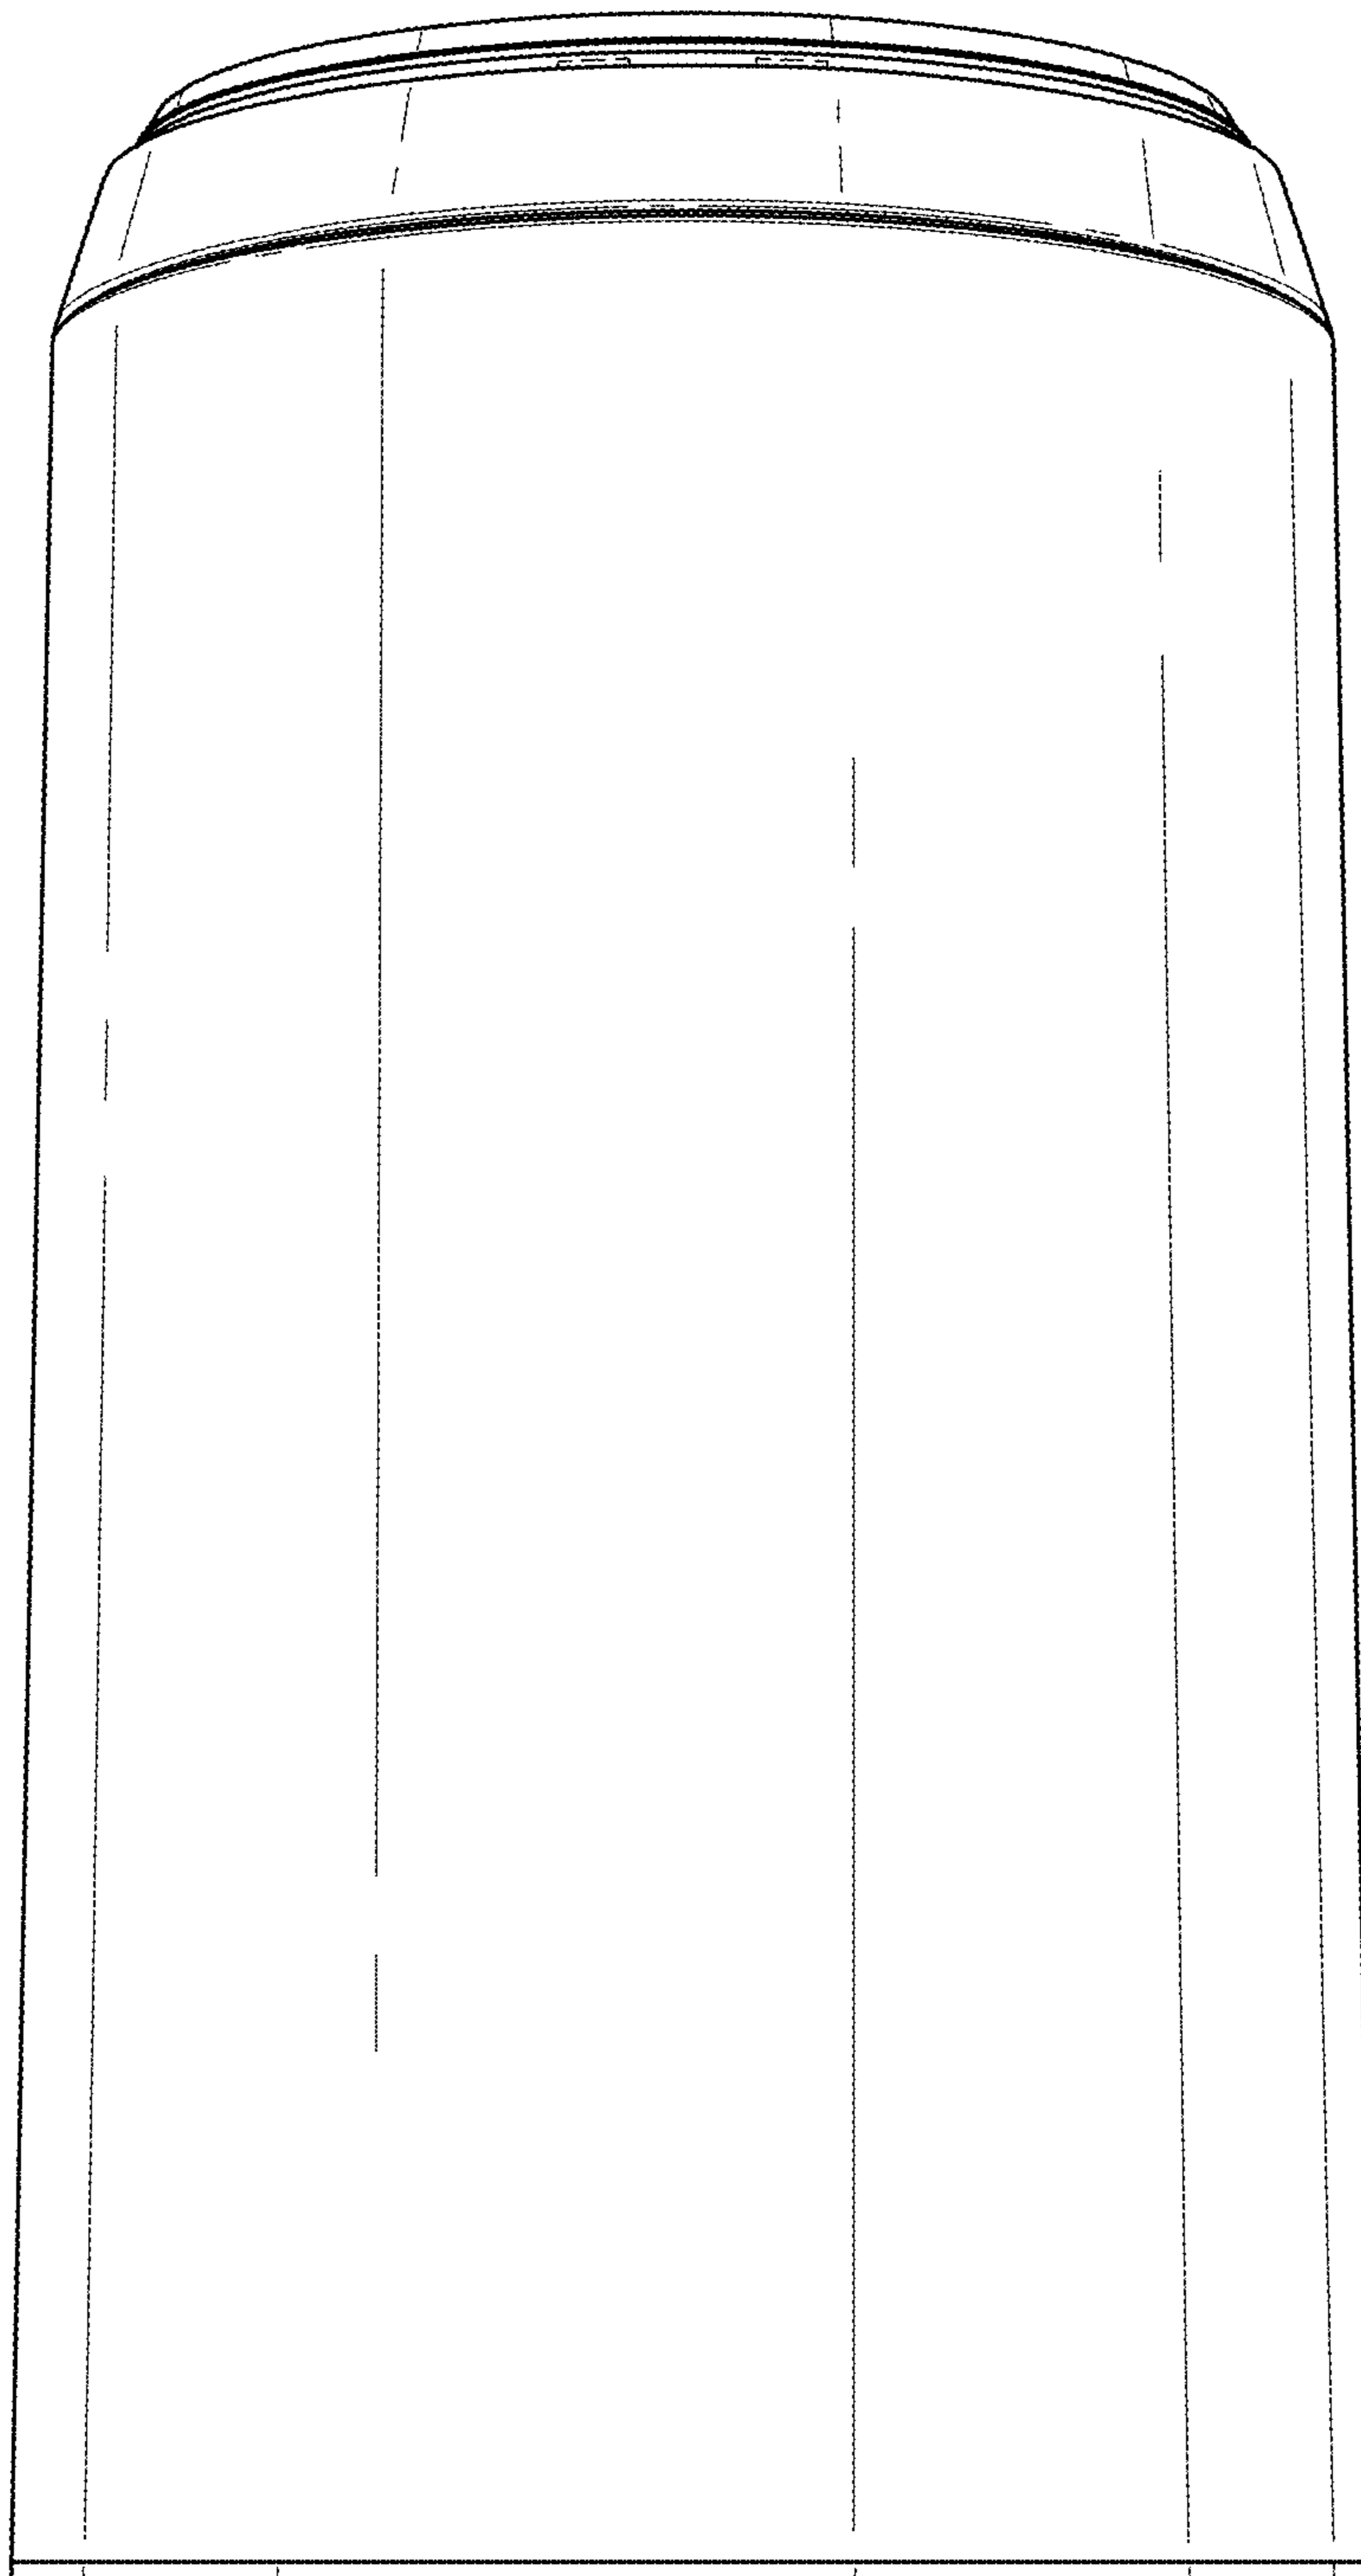


FIG. 3

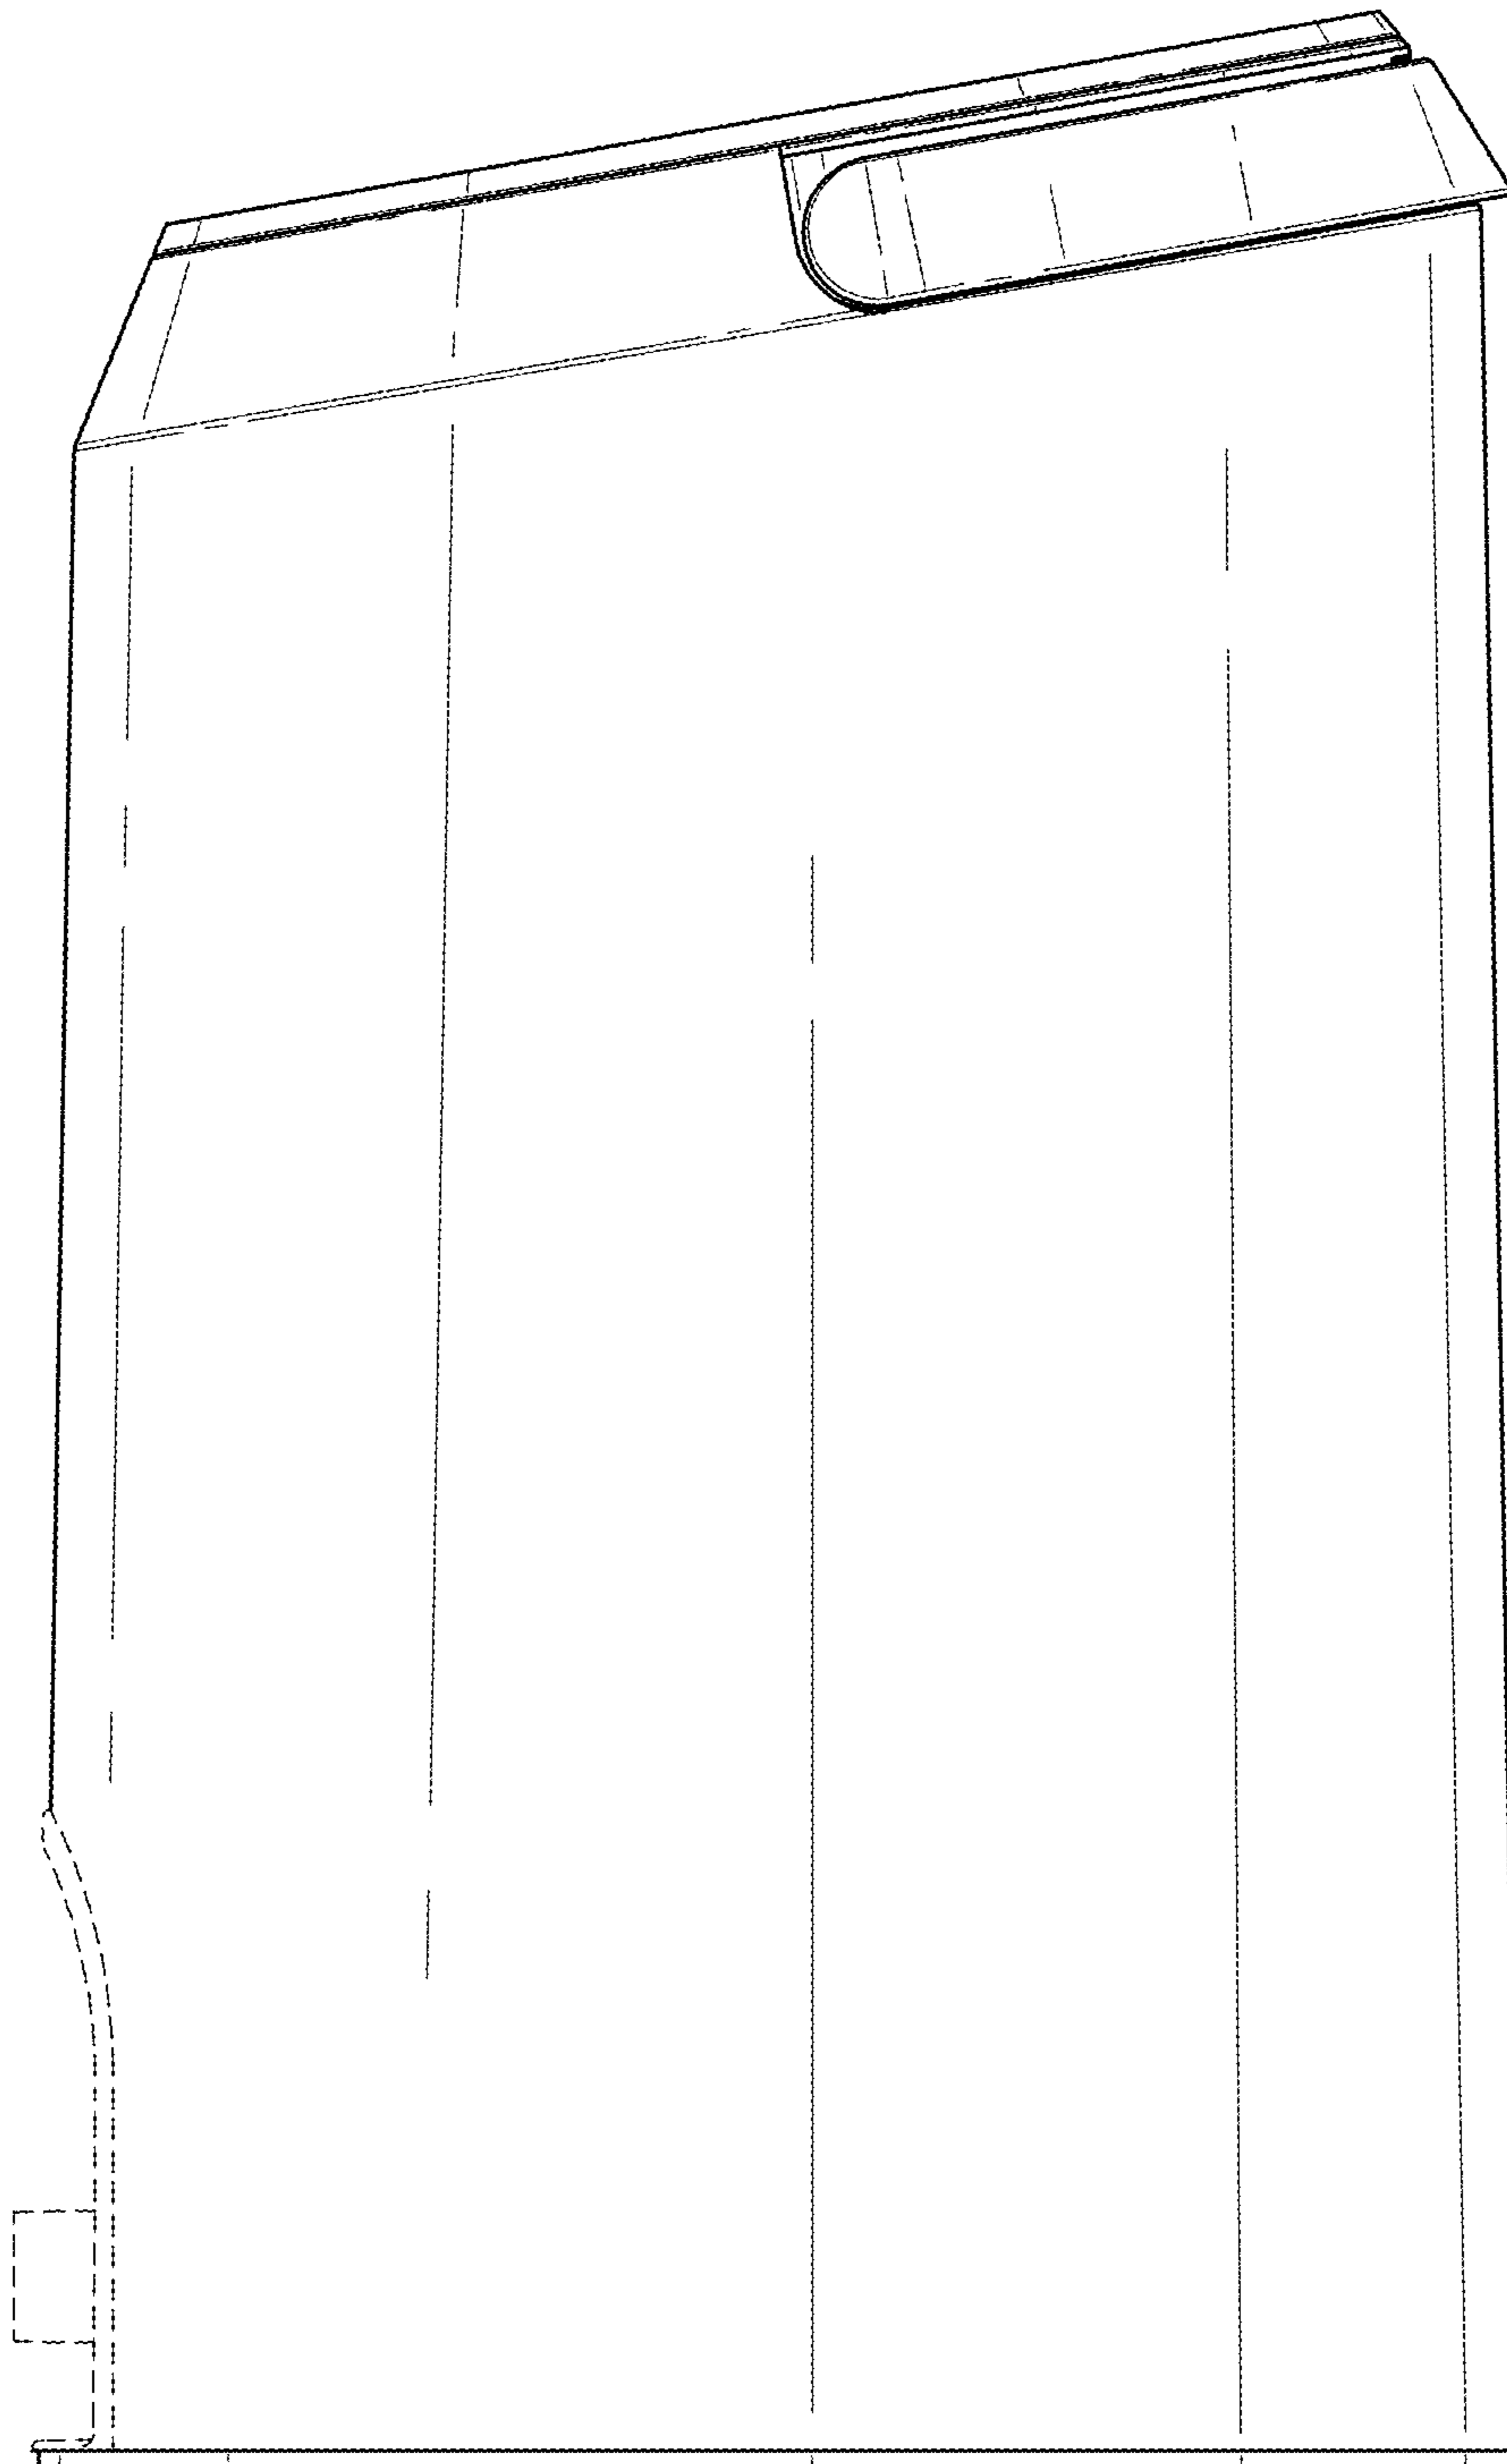


FIG. 4

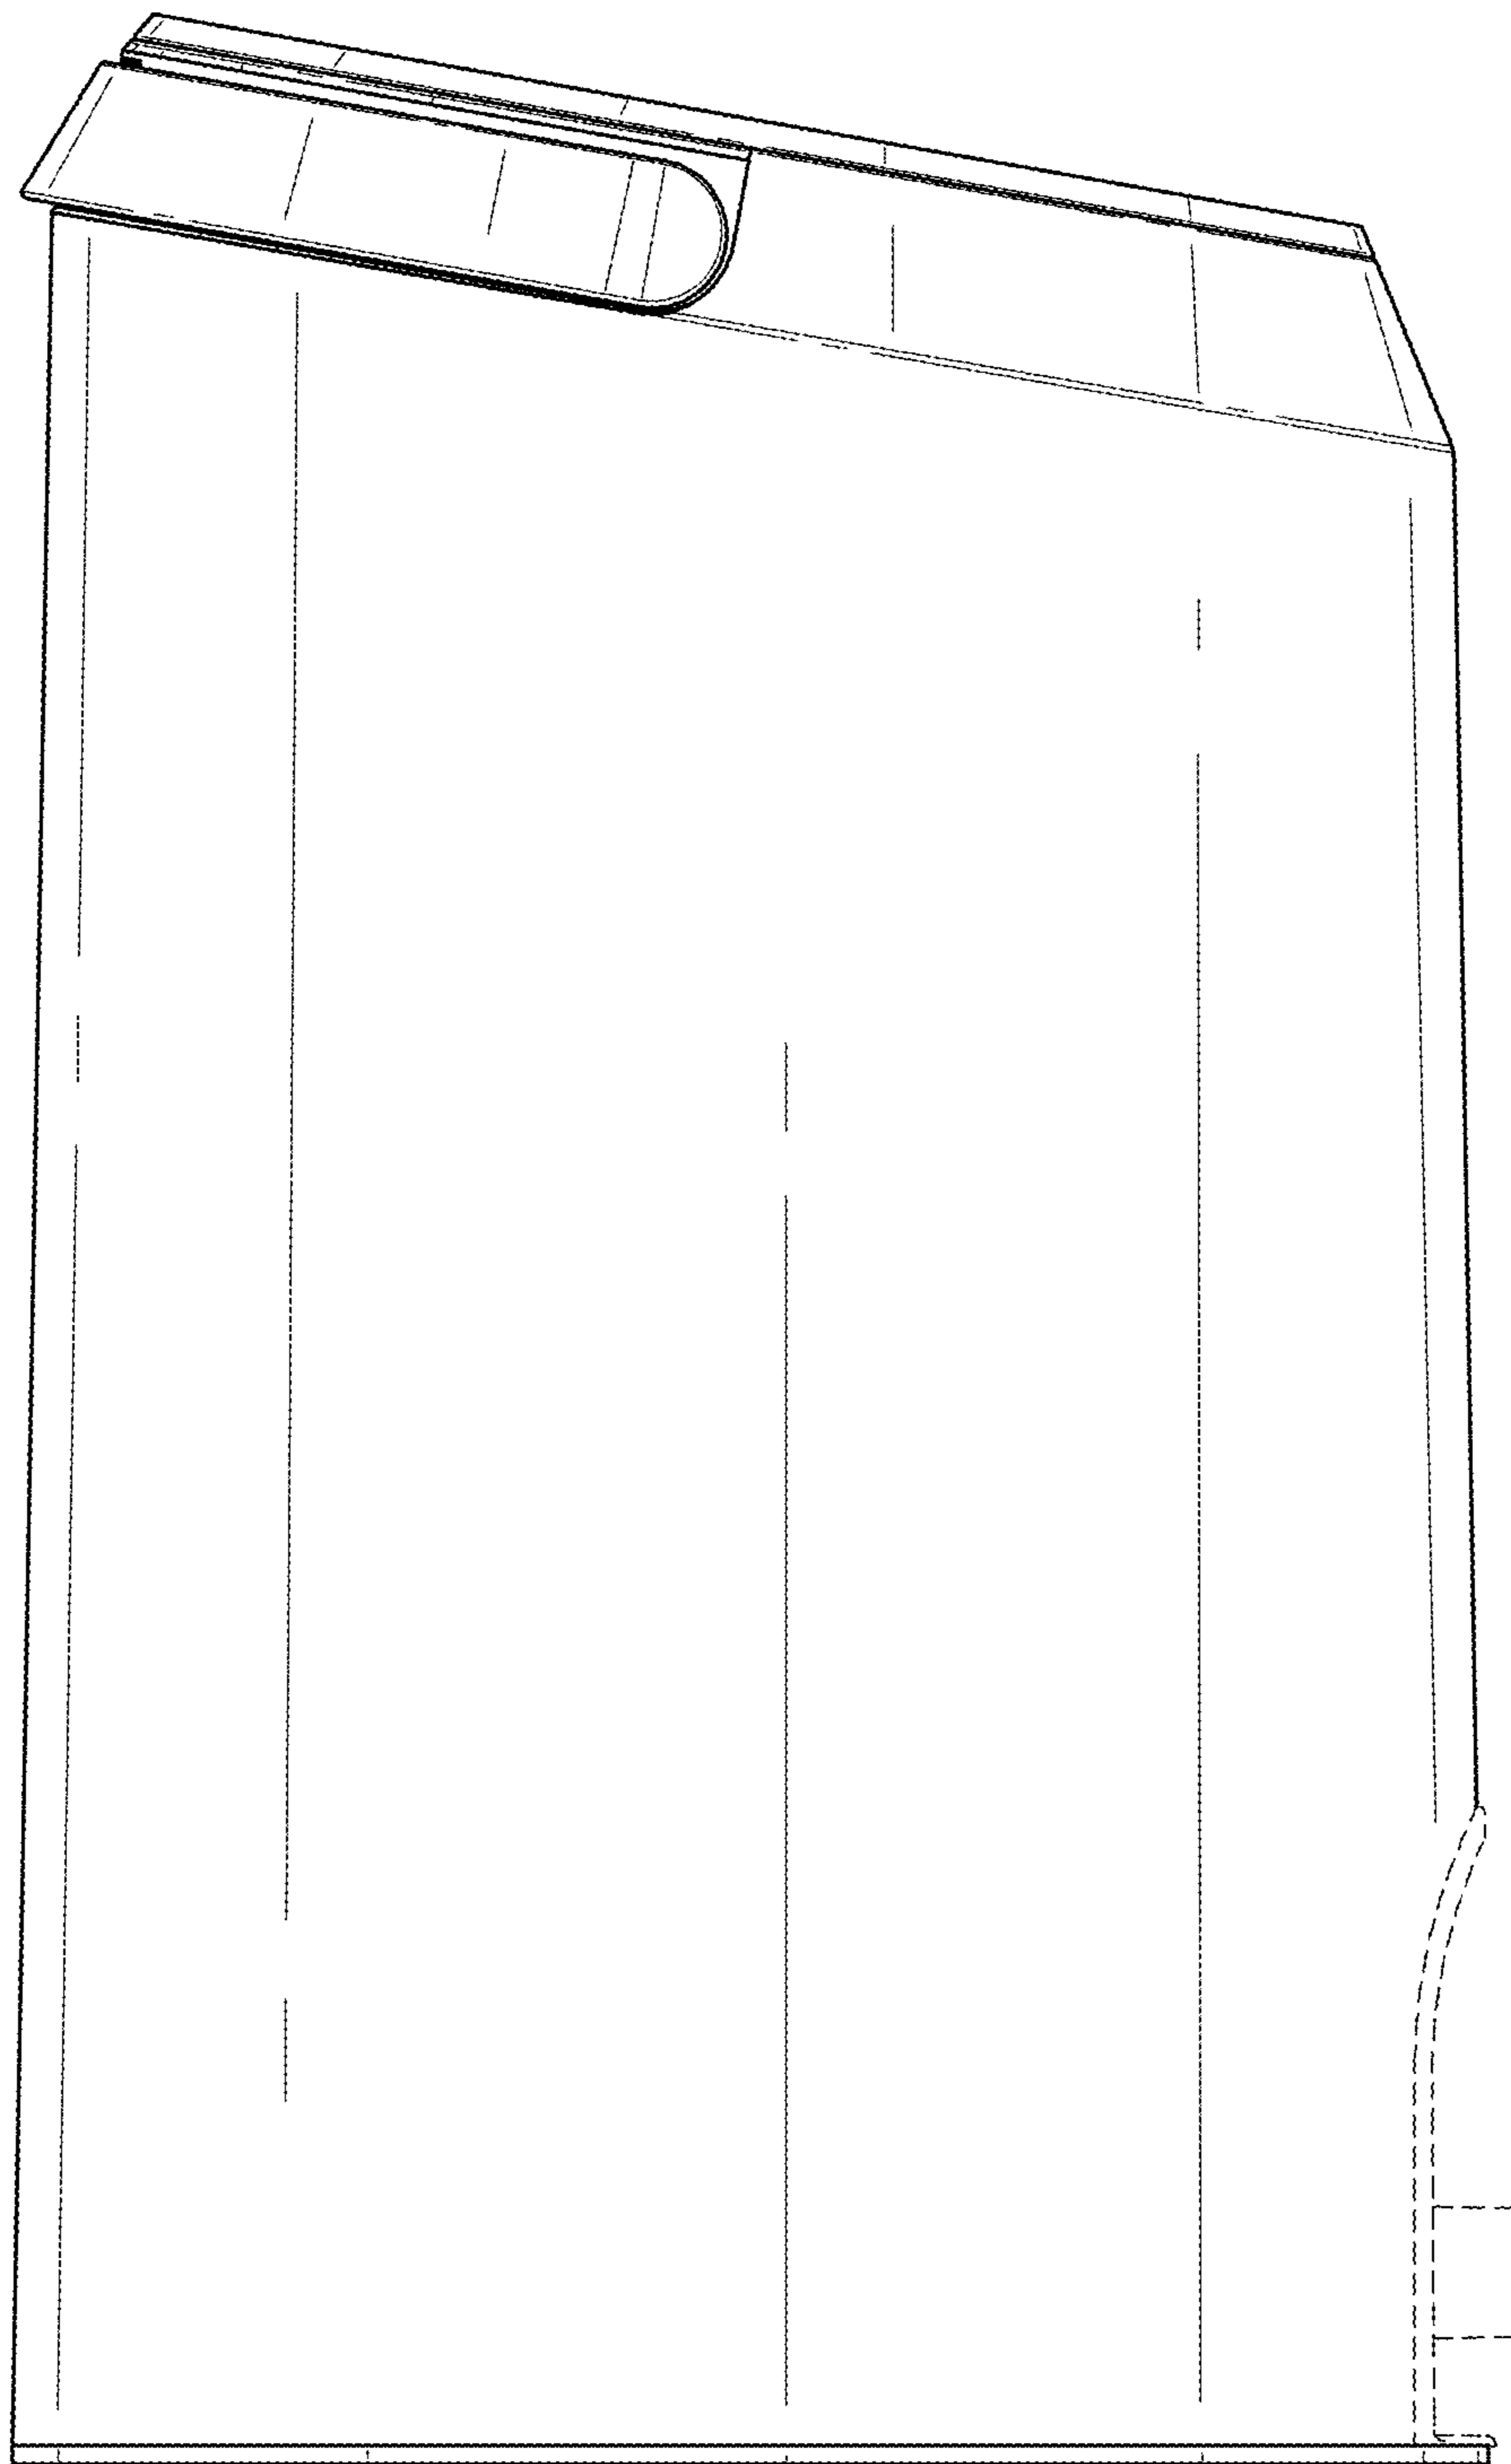


FIG. 5

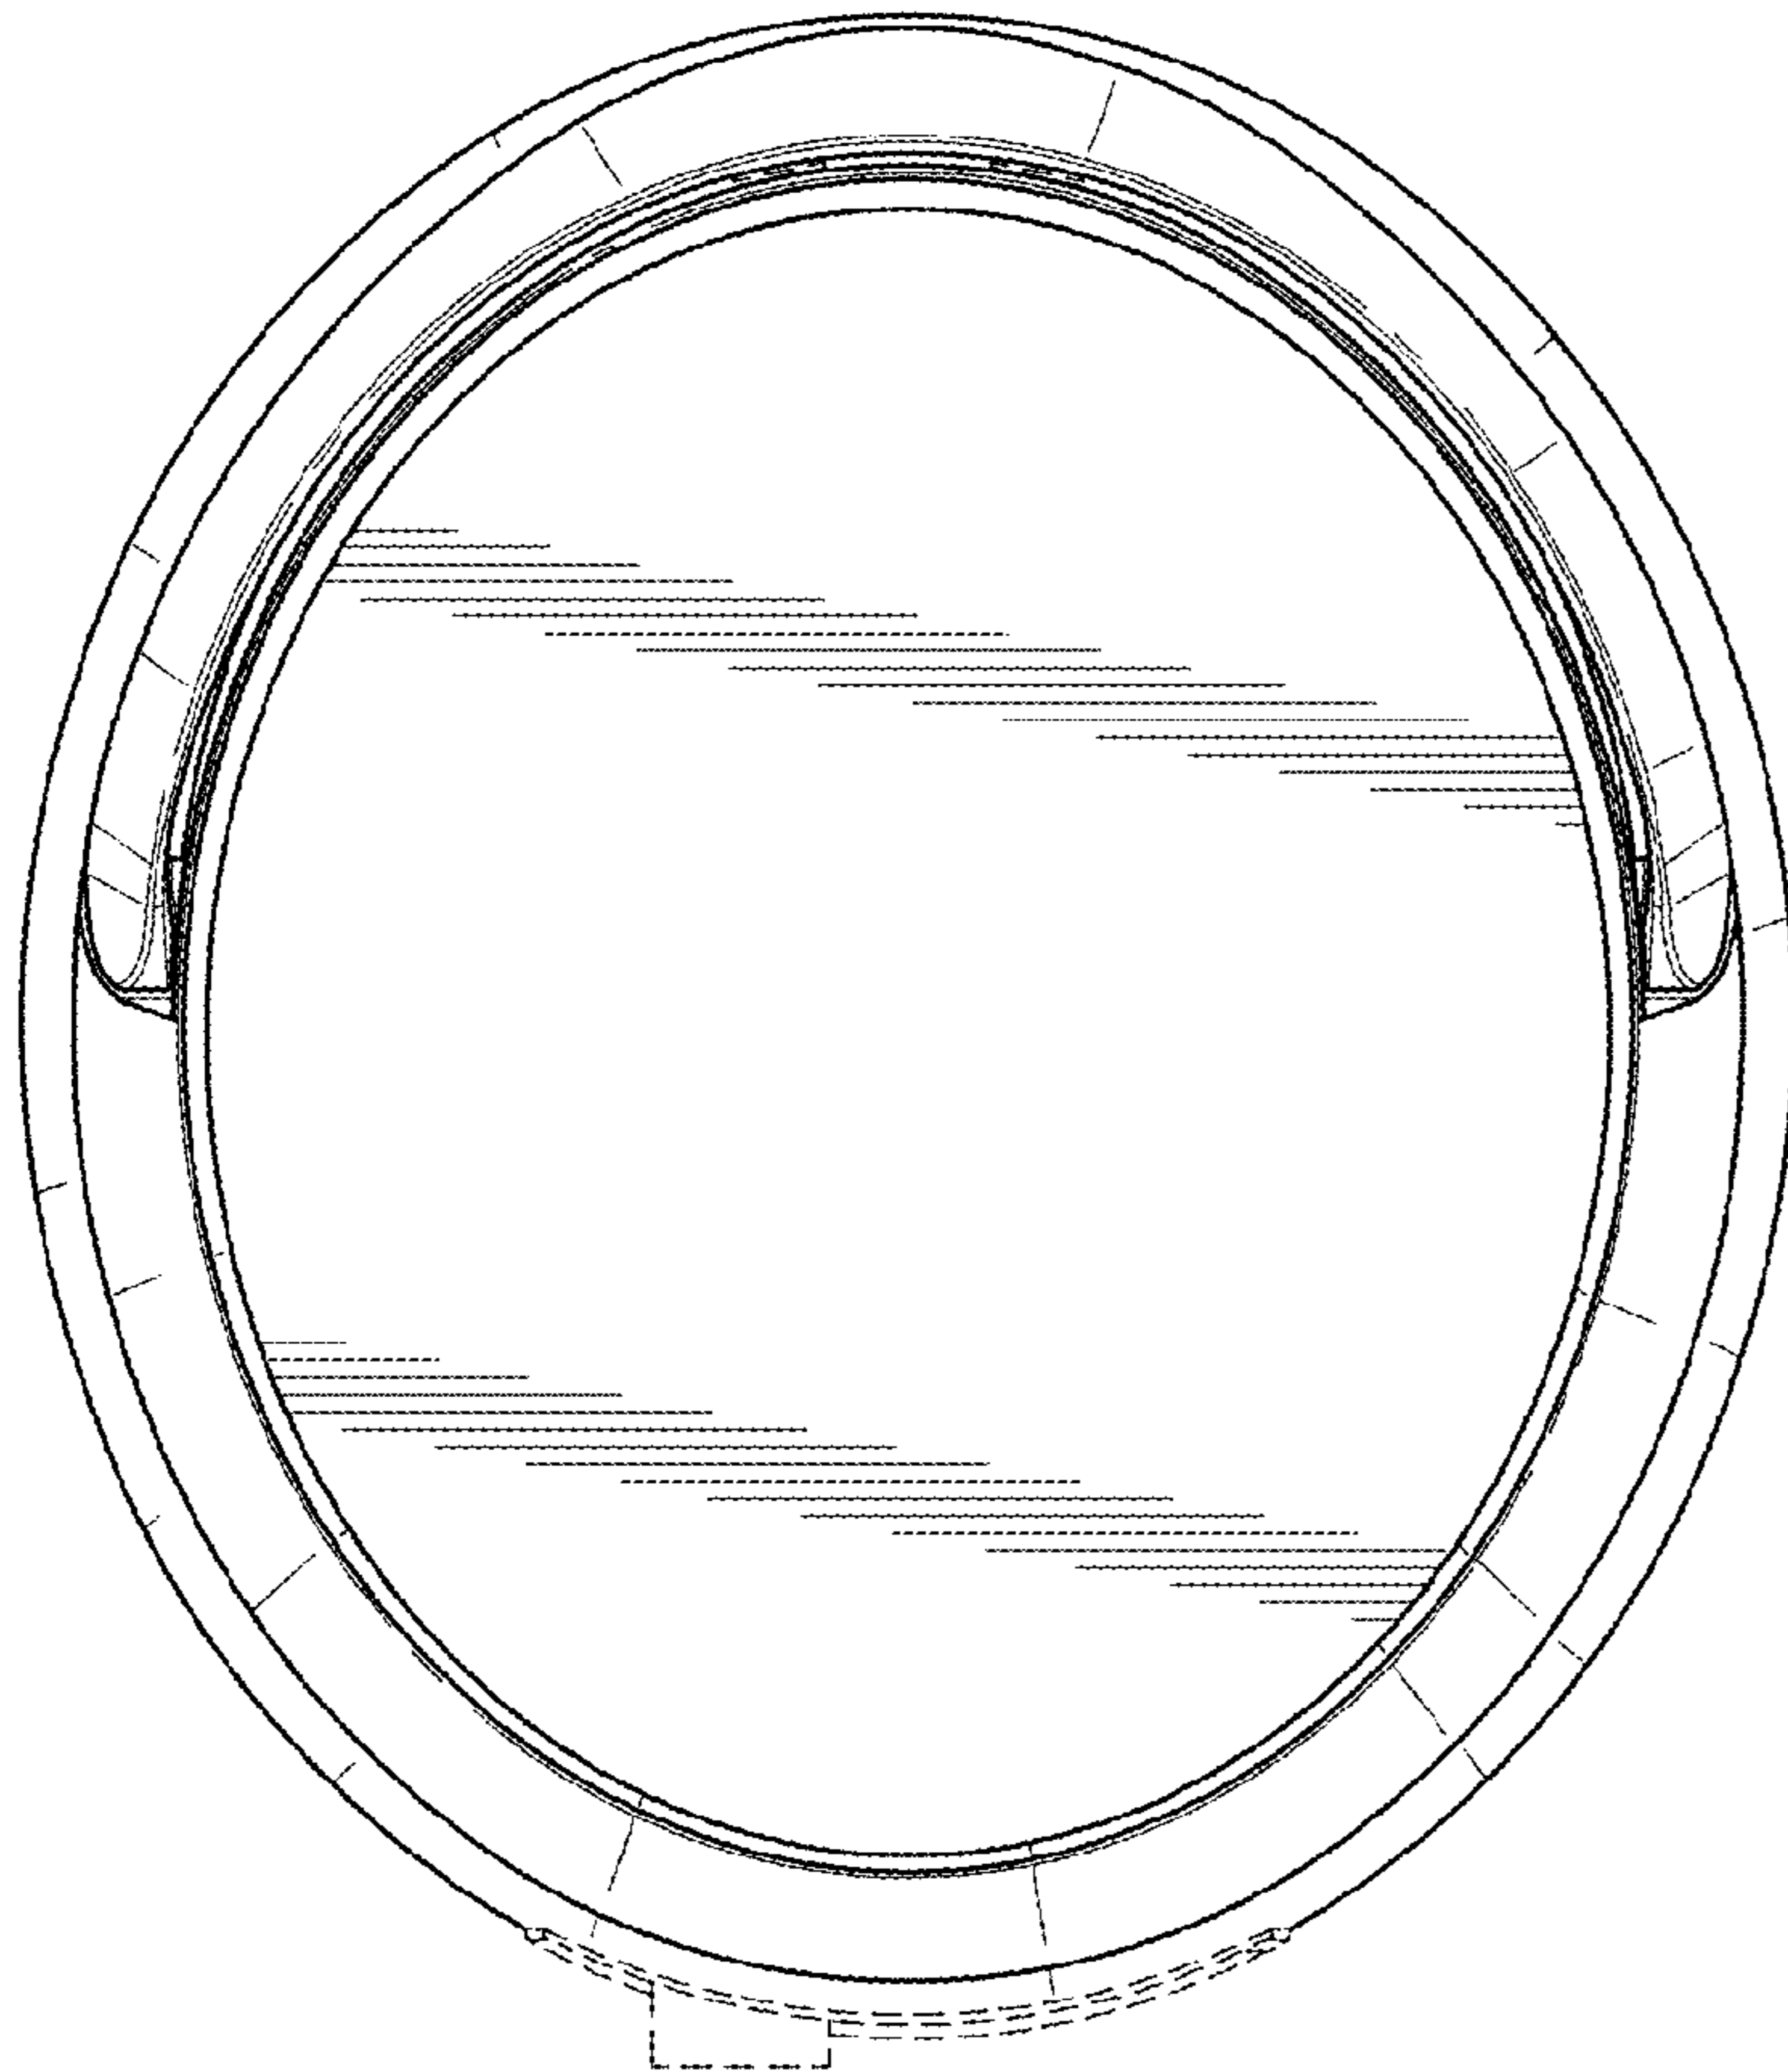


FIG. 6

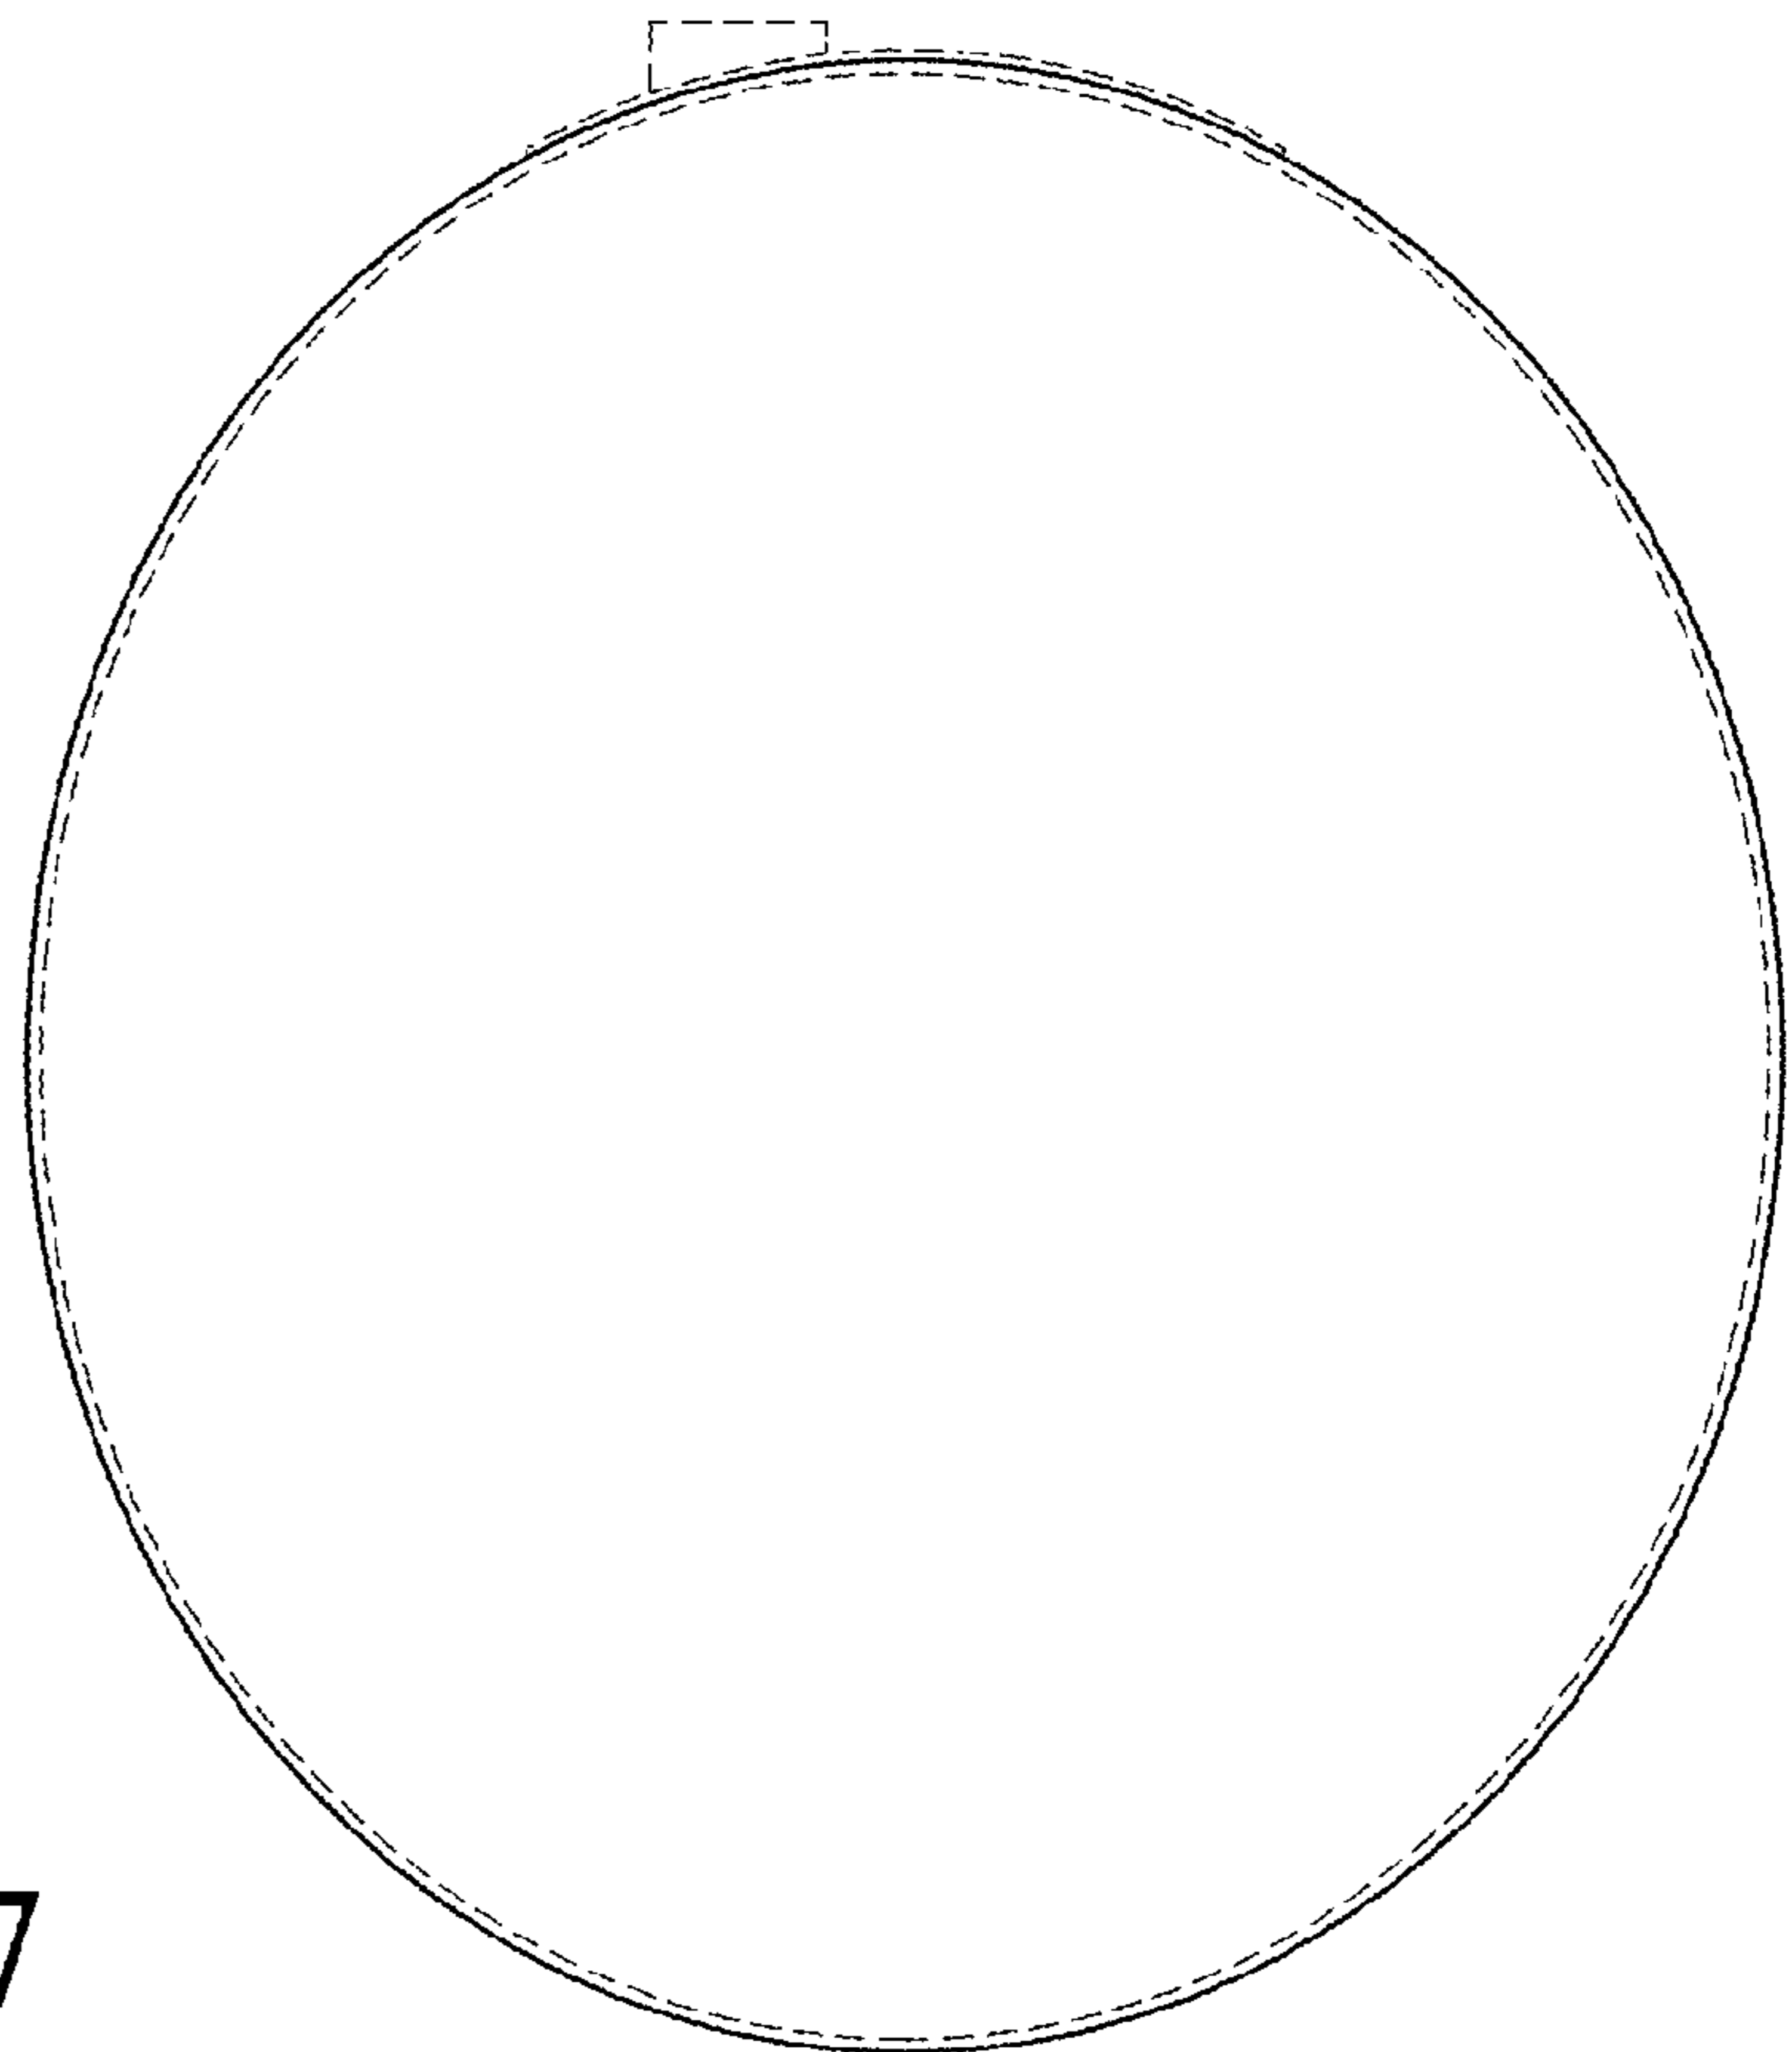


FIG. 7