



US00D902387S

(12) **United States Design Patent** (10) **Patent No.:** **US D902,387 S**
Oellgaard et al. (45) **Date of Patent:** **** Nov. 17, 2020**

(54) **INTERMITTENT URINARY CATHETER**

(71) Applicant: **Coloplast A/S**, Humlebaek (DK)

(72) Inventors: **Claus Brennalt Oellgaard**,
Fredensborg (DK); **Thomas Ulrik
Stepnicka**, Copenhagen (DK);
Alexandros Noekkentved, Værløse
(DK)

(73) Assignee: **Coloplast A/S**, Humlebaek (DK)

(**) Term: **15 Years**

(21) Appl. No.: **29/680,779**

(22) Filed: **Feb. 20, 2019**

(51) **LOC (12) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/112**

(58) **Field of Classification Search**
USPC D24/112-114, 108, 130, 127, 133, 186;
606/181, 185; 604/264, 523-528, 272,
604/164.01-164.11, 187, 93.01; 600/101,
600/139, 143; 128/200.24, 207.14,
128/207.15
CPC .. A61M 25/065; A61M 5/42; A61M 25/0612;
A61M 25/00; A61M 39/00; A61M 27/00;
A61M 25/0043; A61M 25/0067; A61M
25/0097; A61F 2/958

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D413,382 S *	8/1999	Maissami	D24/119
D569,508 S *	5/2008	Bacher	D24/133
D750,260 S *	2/2016	Sauer	D24/186
D753,289 S *	4/2016	Shimon	D24/112
D759,235 S *	6/2016	Rizvi	D24/127
D775,330 S *	12/2016	Blennow	D24/130

D776,259 S *	1/2017	Eldredge	D24/112
D791,311 S *	7/2017	Yantz	D24/130
D804,021 S *	11/2017	Schweikert	D24/130
10,058,651 B1 *	8/2018	Iwasaki	A61B 5/150671
D864,381 S *	10/2019	Miles	D24/112
D864,774 S *	10/2019	Lei	D10/81
D869,643 S *	12/2019	Kelly	D24/112

* cited by examiner

Primary Examiner — David G Muller

(74) *Attorney, Agent, or Firm* — Coloplast Corp.,
Coloplast A/S; Nick Baumann

(57) **CLAIM**

The ornamental design for an intermittent urinary catheter,
as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an intermittent urinary catheter.

FIG. 2 is a front plan view of the intermittent urinary catheter.

FIG. 3 is a back plan view of the intermittent urinary catheter.

FIG. 4 is a top side view of the intermittent urinary catheter, where a bottom side view is not provided as it is a mirror image of the top side view.


FIG. 5 is a left side view of the intermittent urinary catheter; and,

FIG. 6 is a right side view of the intermittent urinary catheter.

The broken lines showing a leading proximal end, and the broken lines showing urine inlets, are included to illustrate unclaimed portions of the intermittent urinary catheter and form no part of the claimed design.

The catheter is shown with a symbolic break in its length. The appearance of any portion of the article between the break lines forms no part of the claimed design.

1 Claim, 6 Drawing Sheets

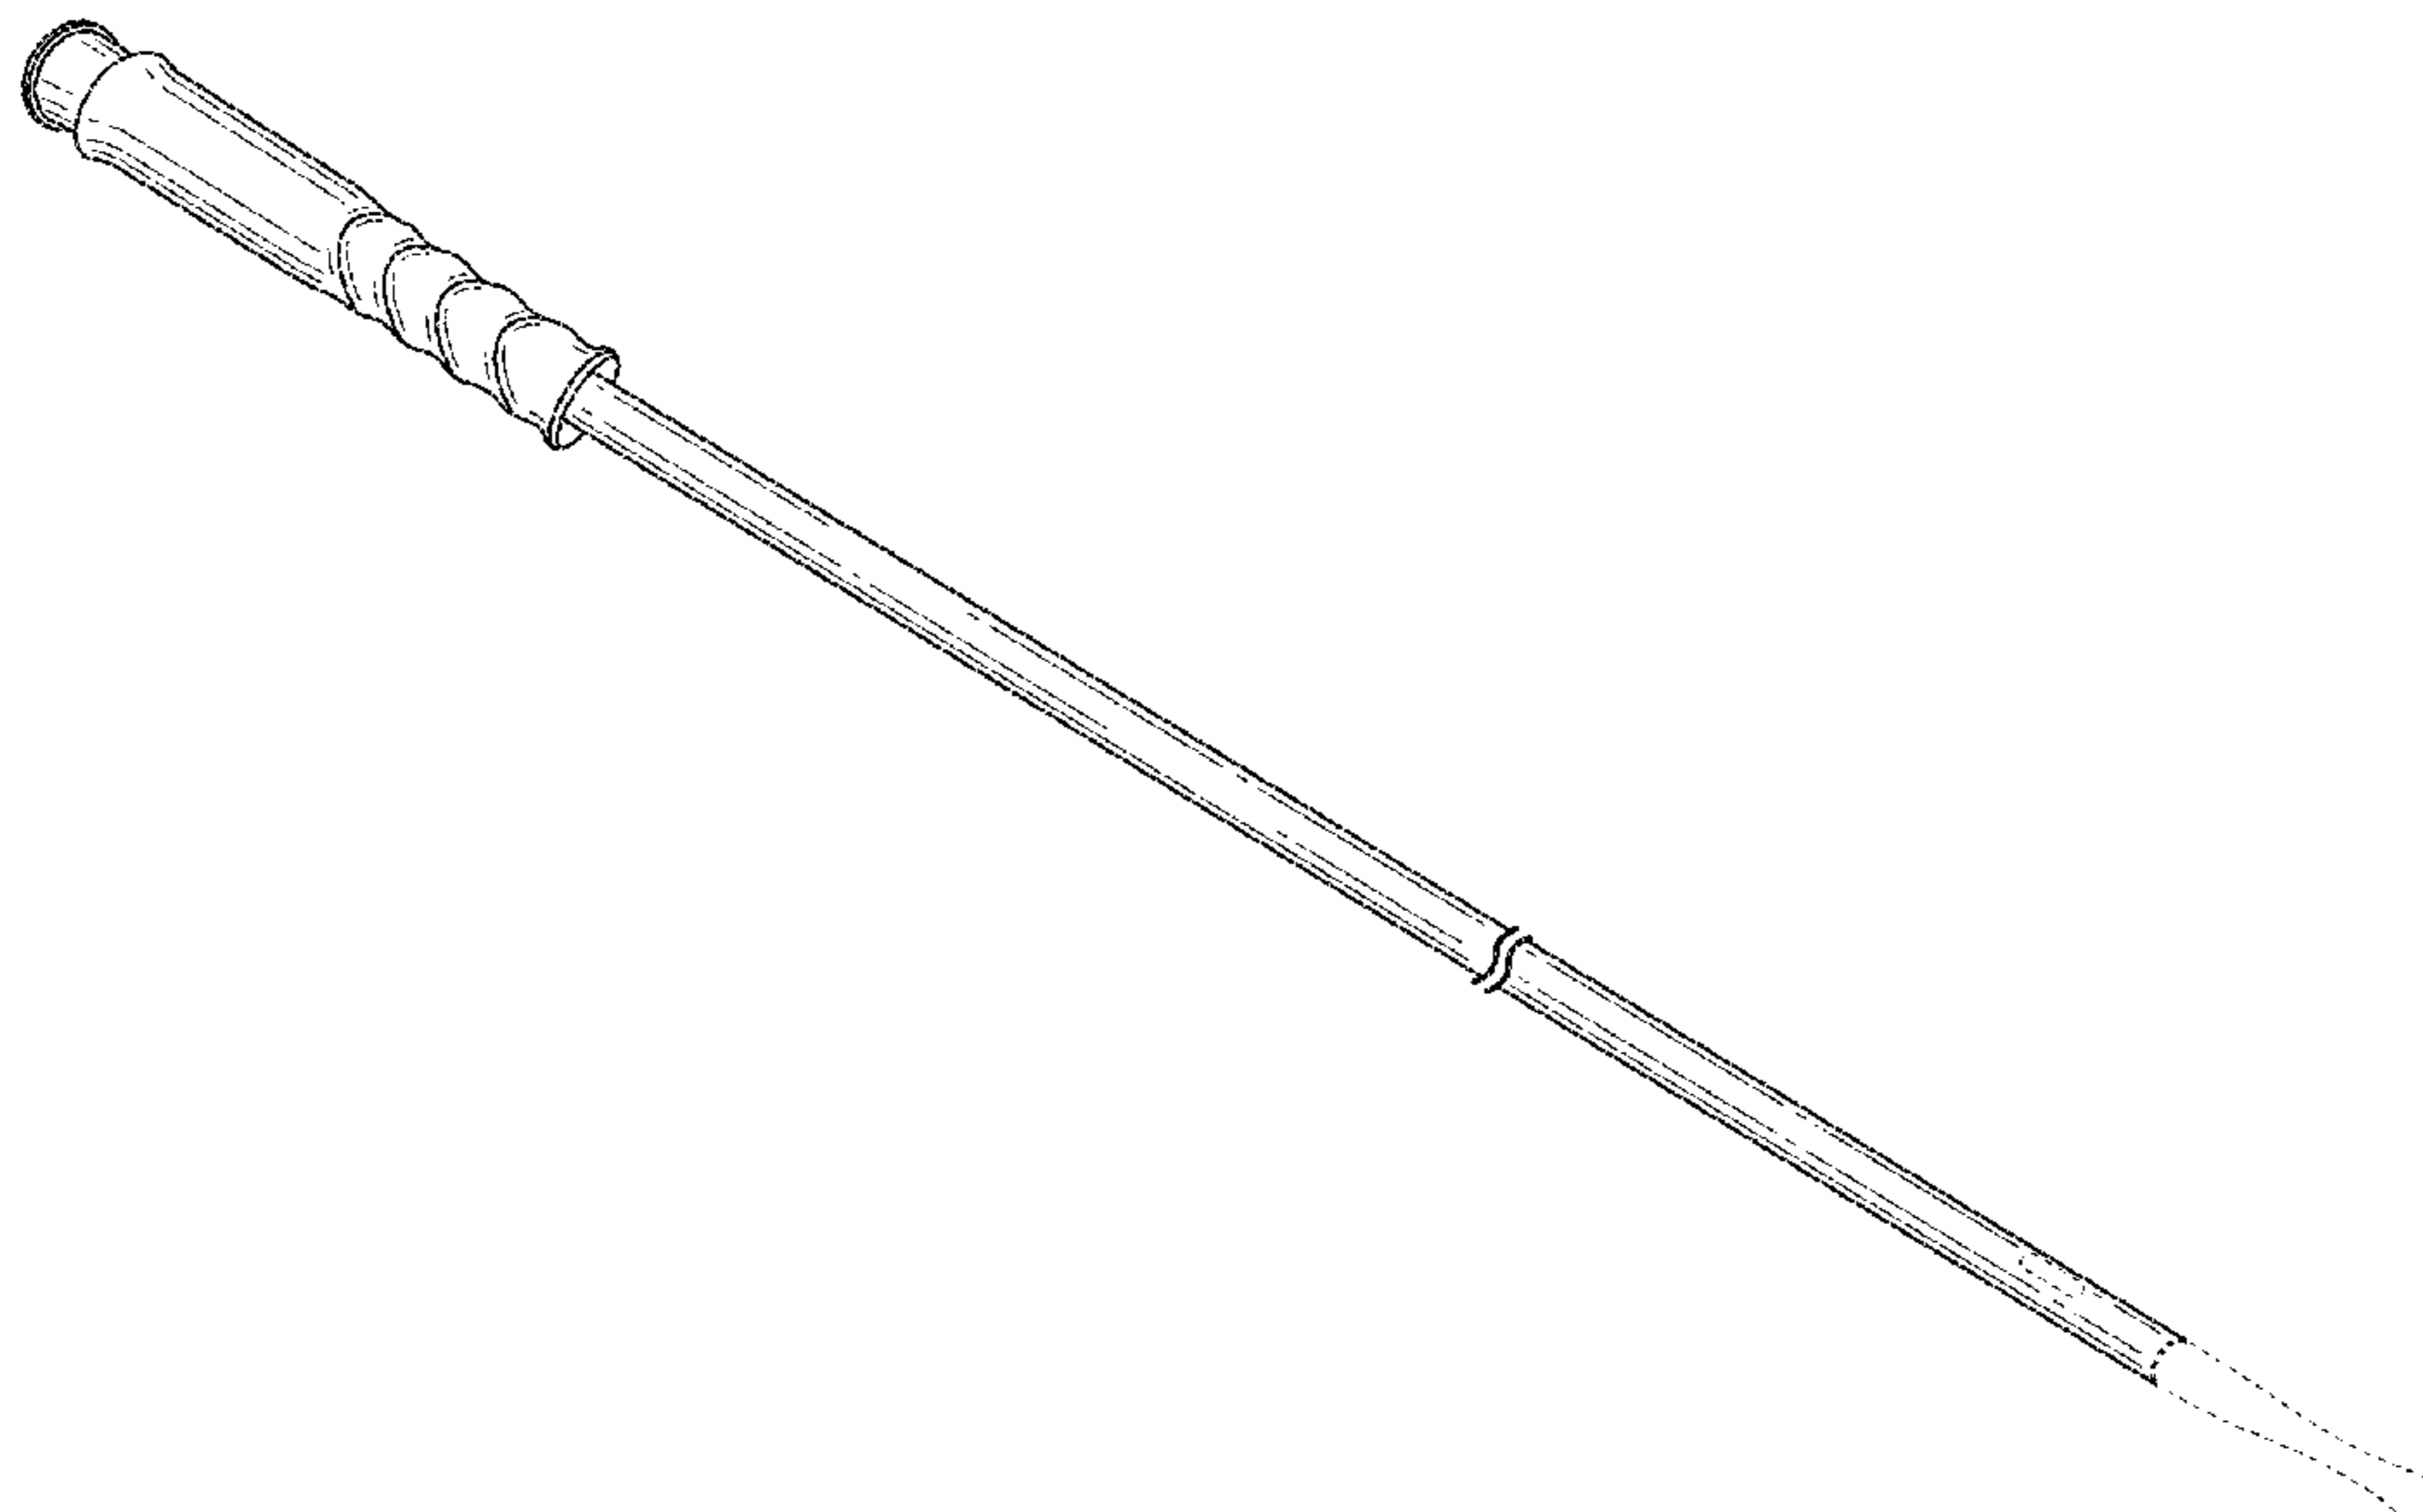

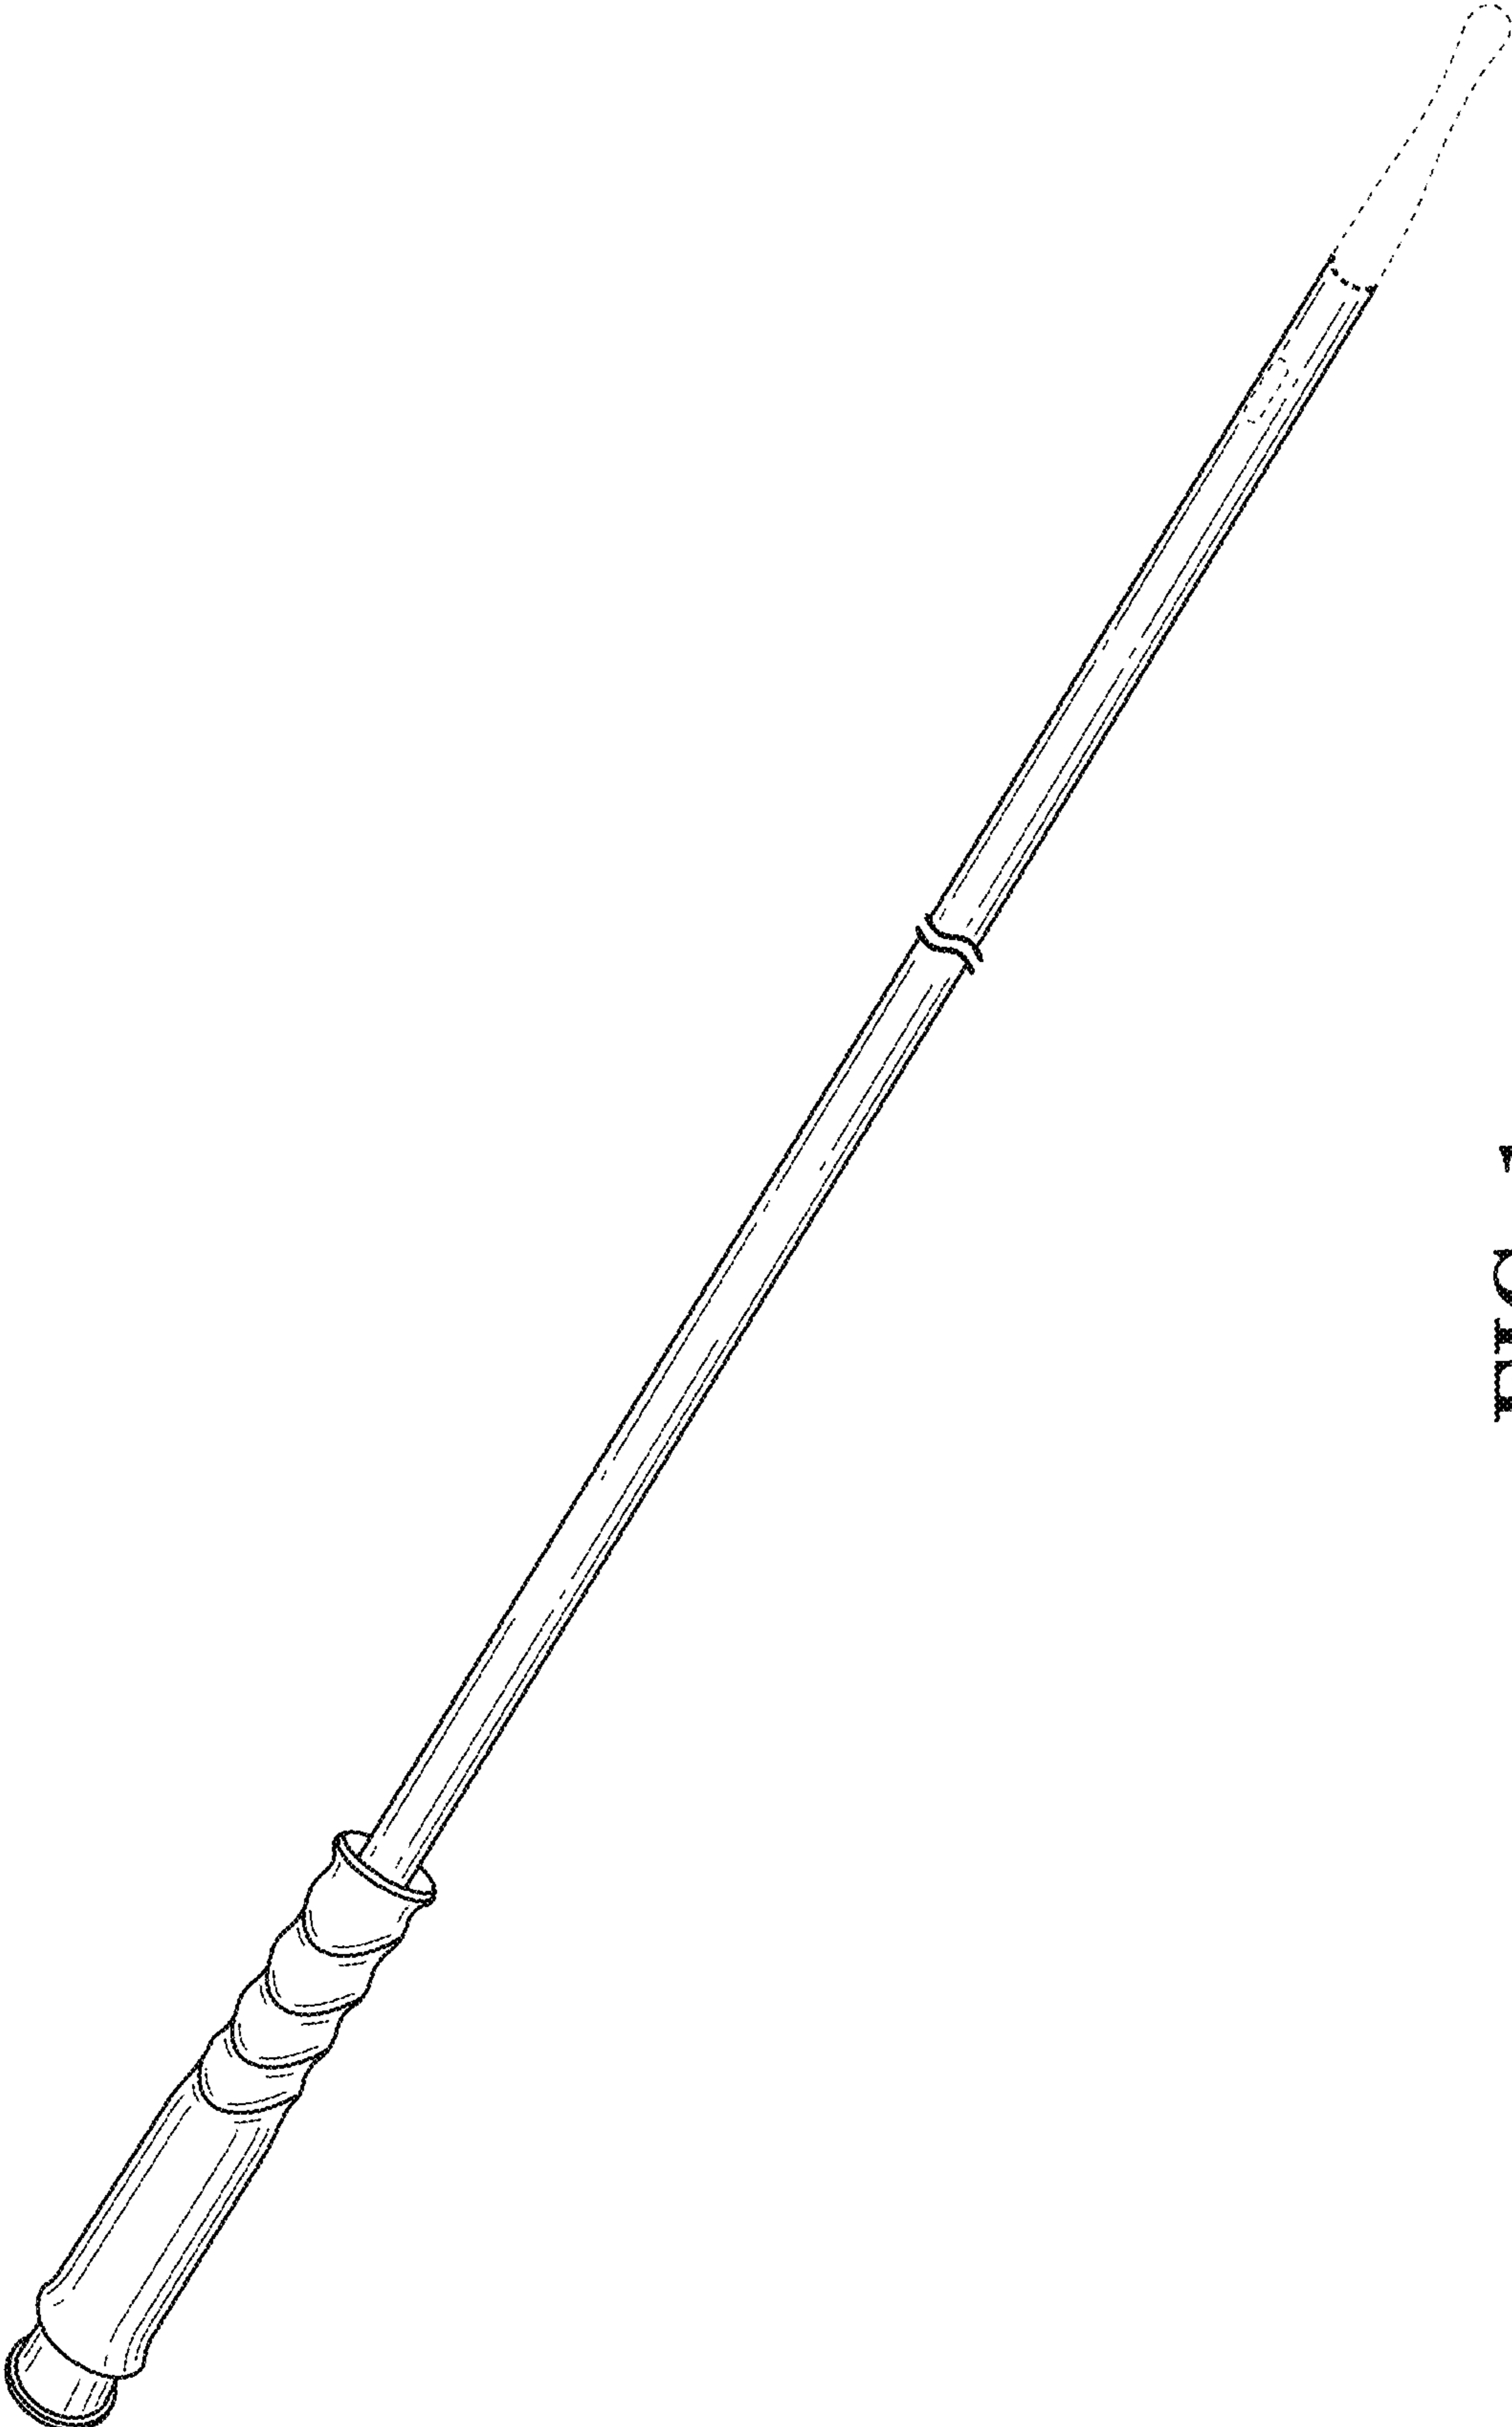


FIG. 1

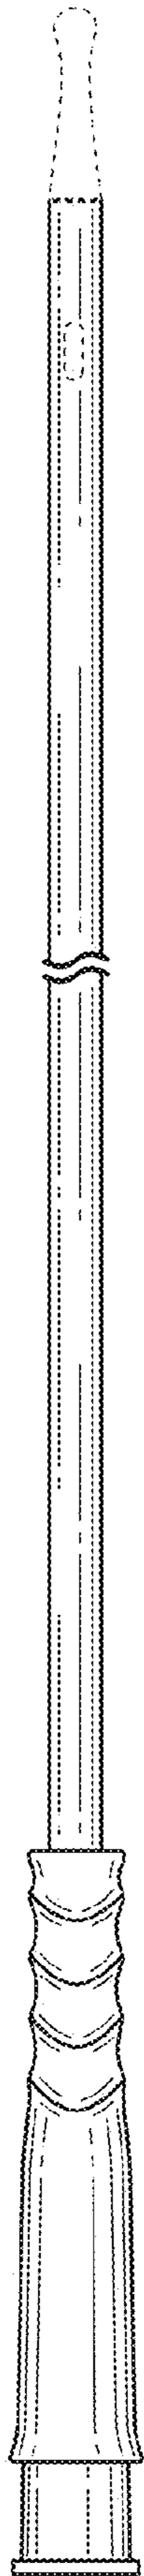


FIG. 2

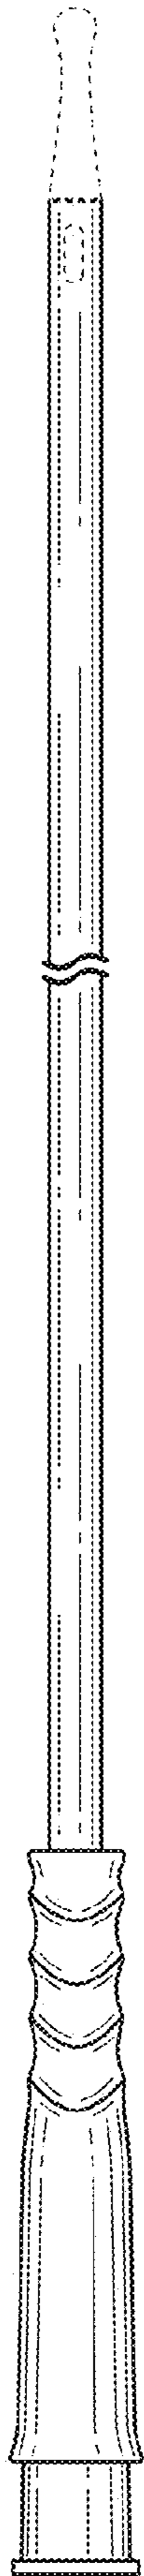


FIG. 3

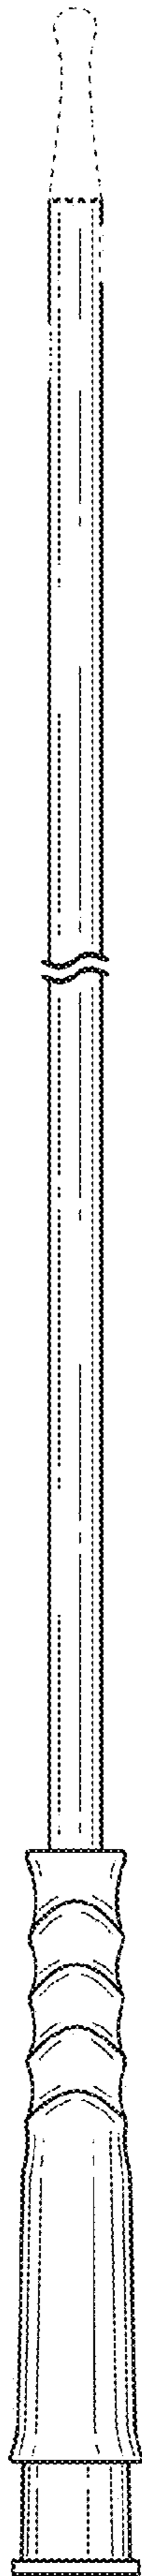


FIG. 4

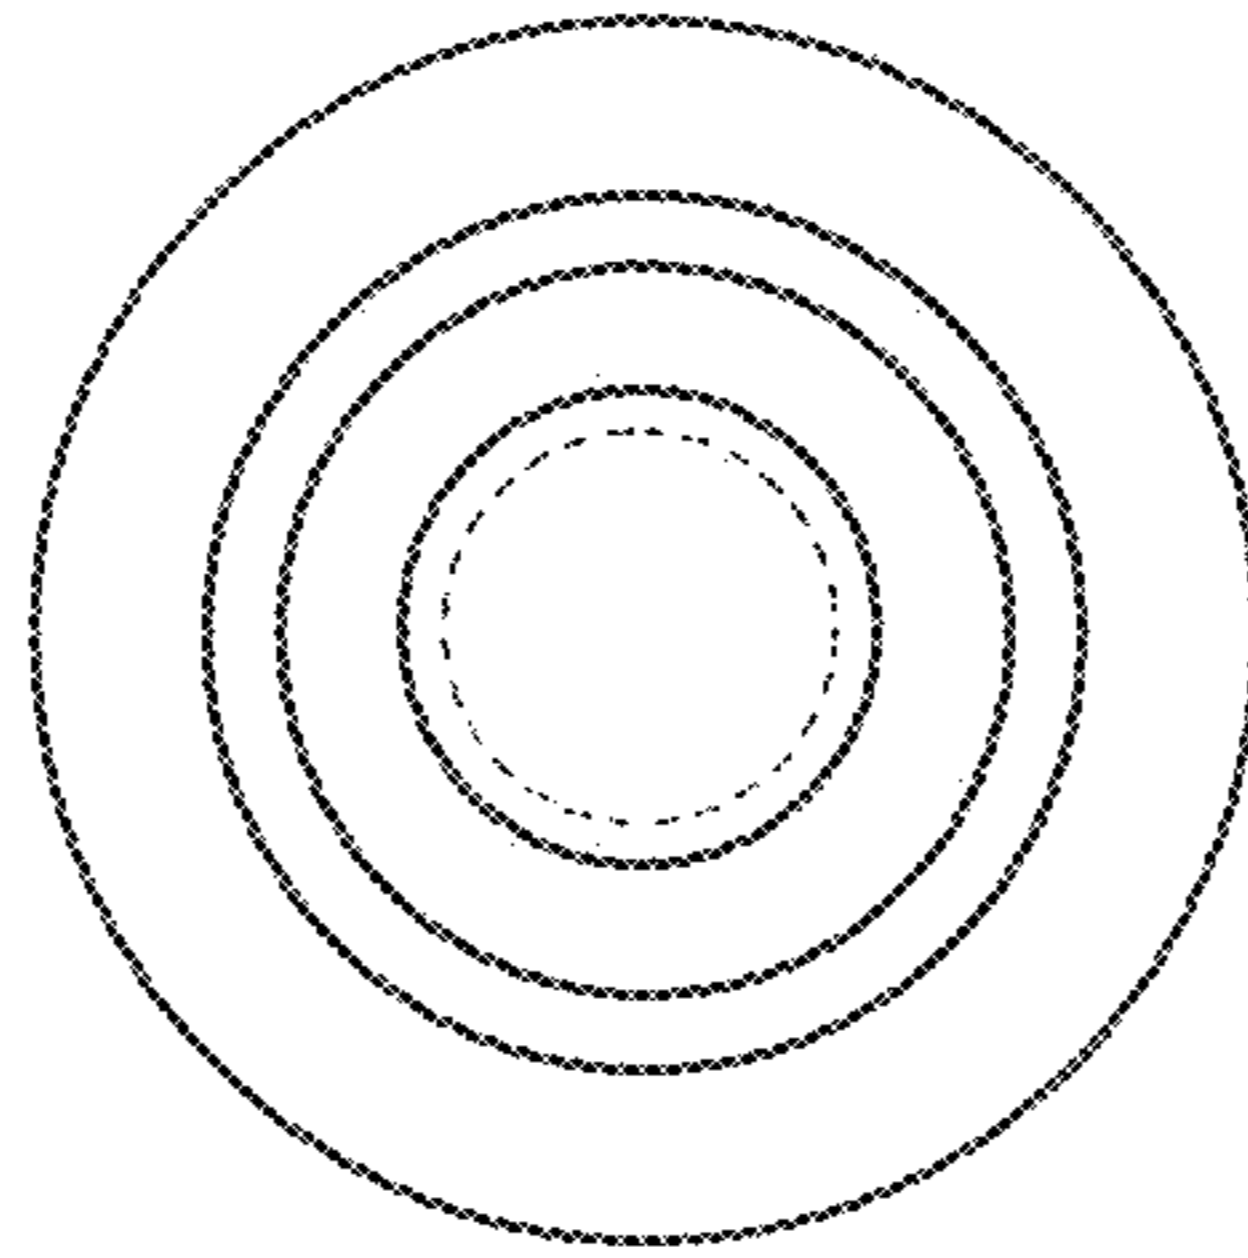


FIG. 5

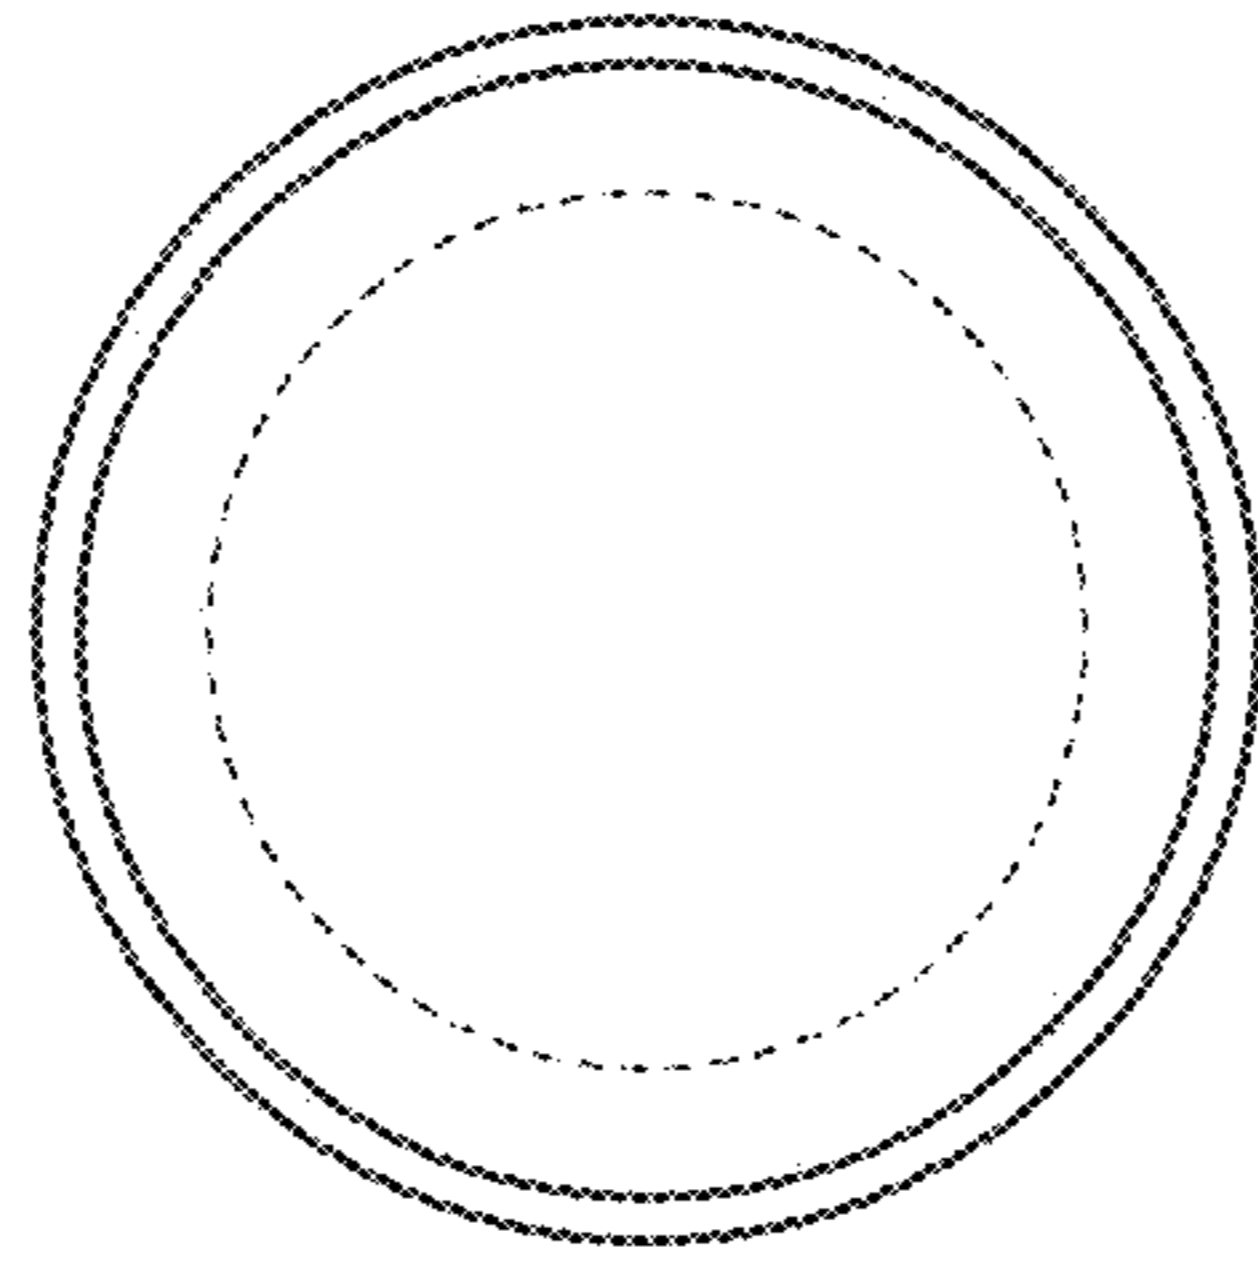


FIG. 6