



US00D902414S

(12) **United States Design Patent**  
**Hodgson et al.**

(10) **Patent No.:** **US D902,414 S**  
(45) **Date of Patent:** **\*\* Nov. 17, 2020**

(54) **COLLARED ELECTRODE ASSEMBLY FOR  
A MEDICAL PROBE**

(71) Applicant: **Transonic Systems Inc.**, Ithaca, NY  
(US)

(72) Inventors: **Philip Chadwick Hodgson**, Ingersoll  
(CA); **Geoffrey Kim Wood**, London  
(CA); **Peter David Plouf**, London  
(CA); **Kyle Gary Fricke**, Ilderton  
(CA); **Morteza Heydari Araghi**,  
London (CA)

(73) Assignee: **Transonic Systems Inc.**, Ithaca, NY  
(US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/662,280**

(22) Filed: **Sep. 4, 2018**

(51) **LOC (12) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/187**

(58) **Field of Classification Search**  
USPC ..... D24/105, 133, 135, 144, 170, 187, 127,  
D24/158, 224; D8/308, 315, 316, 318;  
D10/81

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,040,155 A \* 5/1936 Shoemaker ..... F16L 37/088  
285/39

D143,924 S \* 2/1946 McFadden ..... D24/135  
(Continued)

FOREIGN PATENT DOCUMENTS

JP D2014-19485 \* 9/2014

OTHER PUBLICATIONS

STCON7. Online, published date unknown. Retrieved on Nov. 18,  
2019 from URL: <https://us.ohaus.com/en-US/Products/Instruments-Equipment/Water-Analysis/Starter-Electrodes/Cond-Electrode-STCON7>.\*

*Primary Examiner* — Susan Bennett Hattan

*Assistant Examiner* — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Brian B. Shaw, Esq.;  
Harter Secrest & Emery LLP

(57) **CLAIM**

We claim the ornamental design for a collared electrode  
assembly for a medical probe, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a collared electrode assembly  
for a medical probe.

FIG. 2 is an enlarged view of the portion of the design of  
FIG. 1 within the circle labeled 2.

FIG. 3 is a front elevational view of the collared electrode  
of FIG. 1.

FIG. 4 is a rear elevational view of the collared electrode of  
FIG. 1.


FIG. 5 is a top plan view of the collared electrode of FIG.  
1.

FIG. 6 is a bottom plan view of the collared electrode of FIG.  
1; and,

FIG. 7 is a right side elevational view of the collared  
electrode of FIG. 1, wherein the left side elevational view is  
a mirror image thereof.

The collared electrode assembly is shown with a symbolic  
break in its length. The appearance of any portion of the  
article between the break lines forms no part of the claimed  
design. The dot-dash-dot broken lines in FIGS. 1 and 2  
depict the boundary of the enlarged view and form no part  
of the claimed design. The dashed lines in the drawings  
depict portions of the collared electrode assembly for a  
medical probe that form no part of the claimed design.

**1 Claim, 4 Drawing Sheets**

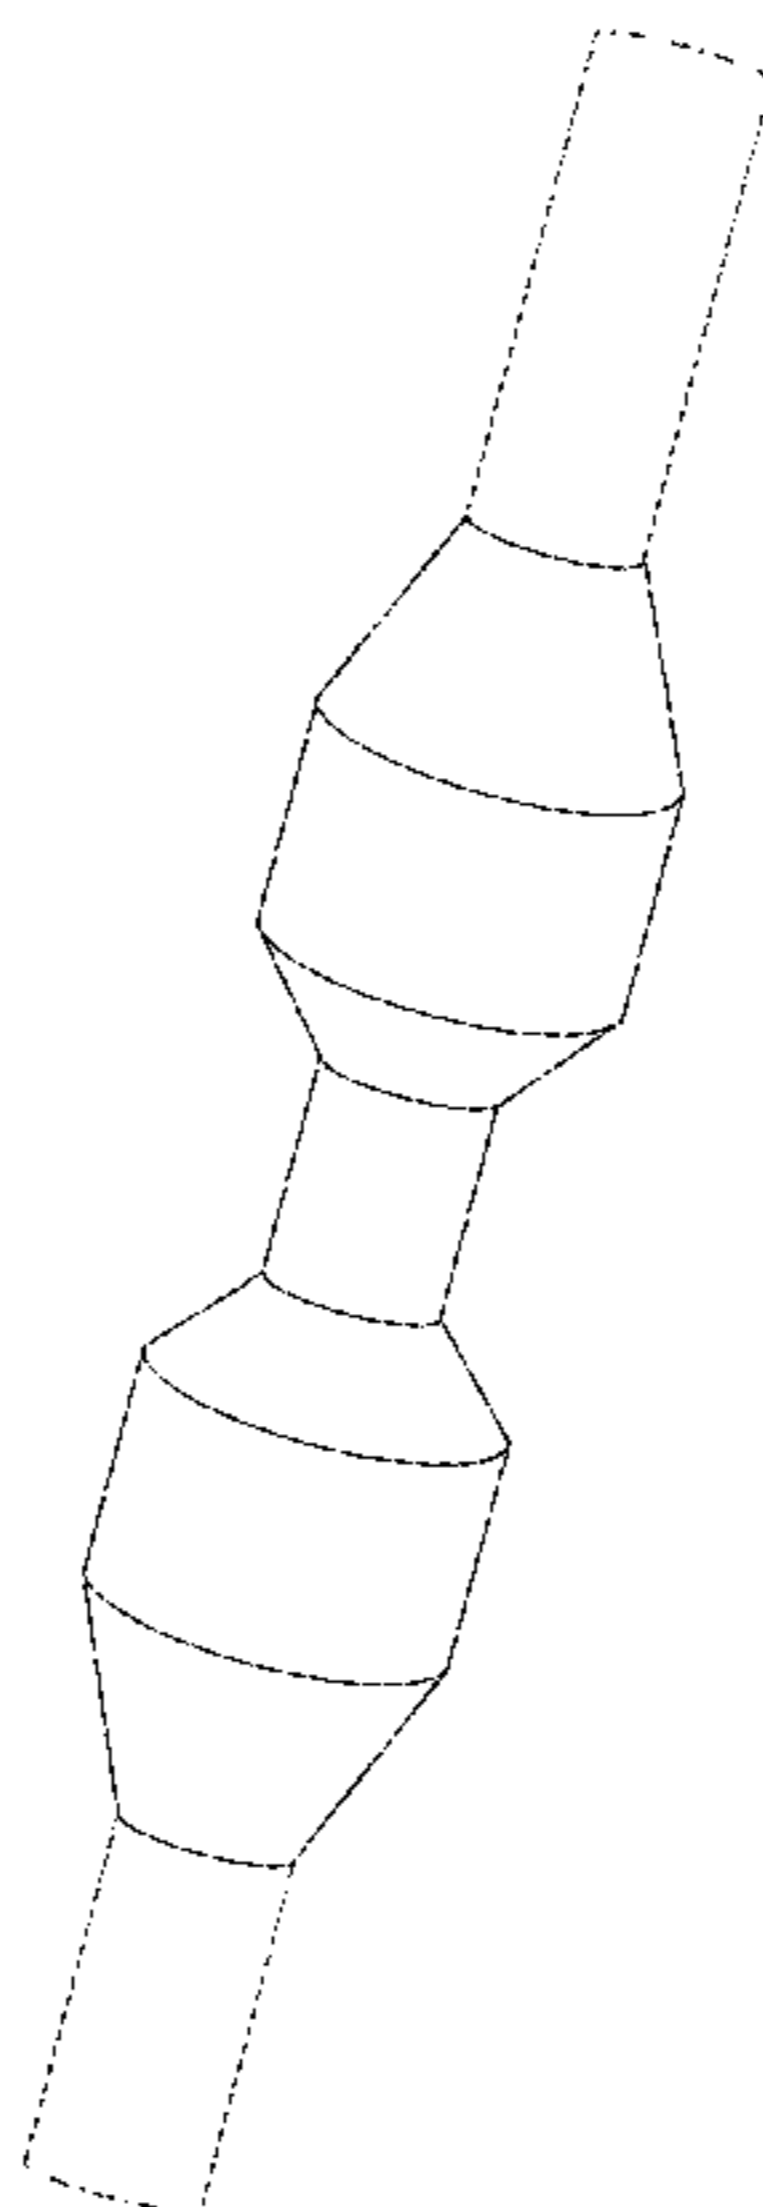

(58) **Field of Classification Search**

CPC ..... A61B 18/1477  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,109,228	A *	8/1978	Wycklendt .....	H01H 85/18 337/276
D348,934	S *	7/1994	Johnson .....	D24/187
D387,862	S *	12/1997	Mainiero .....	D24/127
D415,835	S *	10/1999	Malewicz .....	D24/187
D428,488	S *	7/2000	Bloch .....	D21/662
D510,139	S *	9/2005	Gilad .....	D24/104
D650,487	S *	12/2011	Briscoe .....	D24/211
D749,742	S *	2/2016	Ishibashi .....	D24/186
D757,937	S *	5/2016	Tsai .....	D24/135
D791,326	S *	7/2017	Olson .....	D24/158
D827,150	S *	8/2018	Nakagawa .....	D24/224
2015/0137934	A1 *	5/2015	von zur Muehlen ..	H01H 69/02 337/273

\* cited by examiner

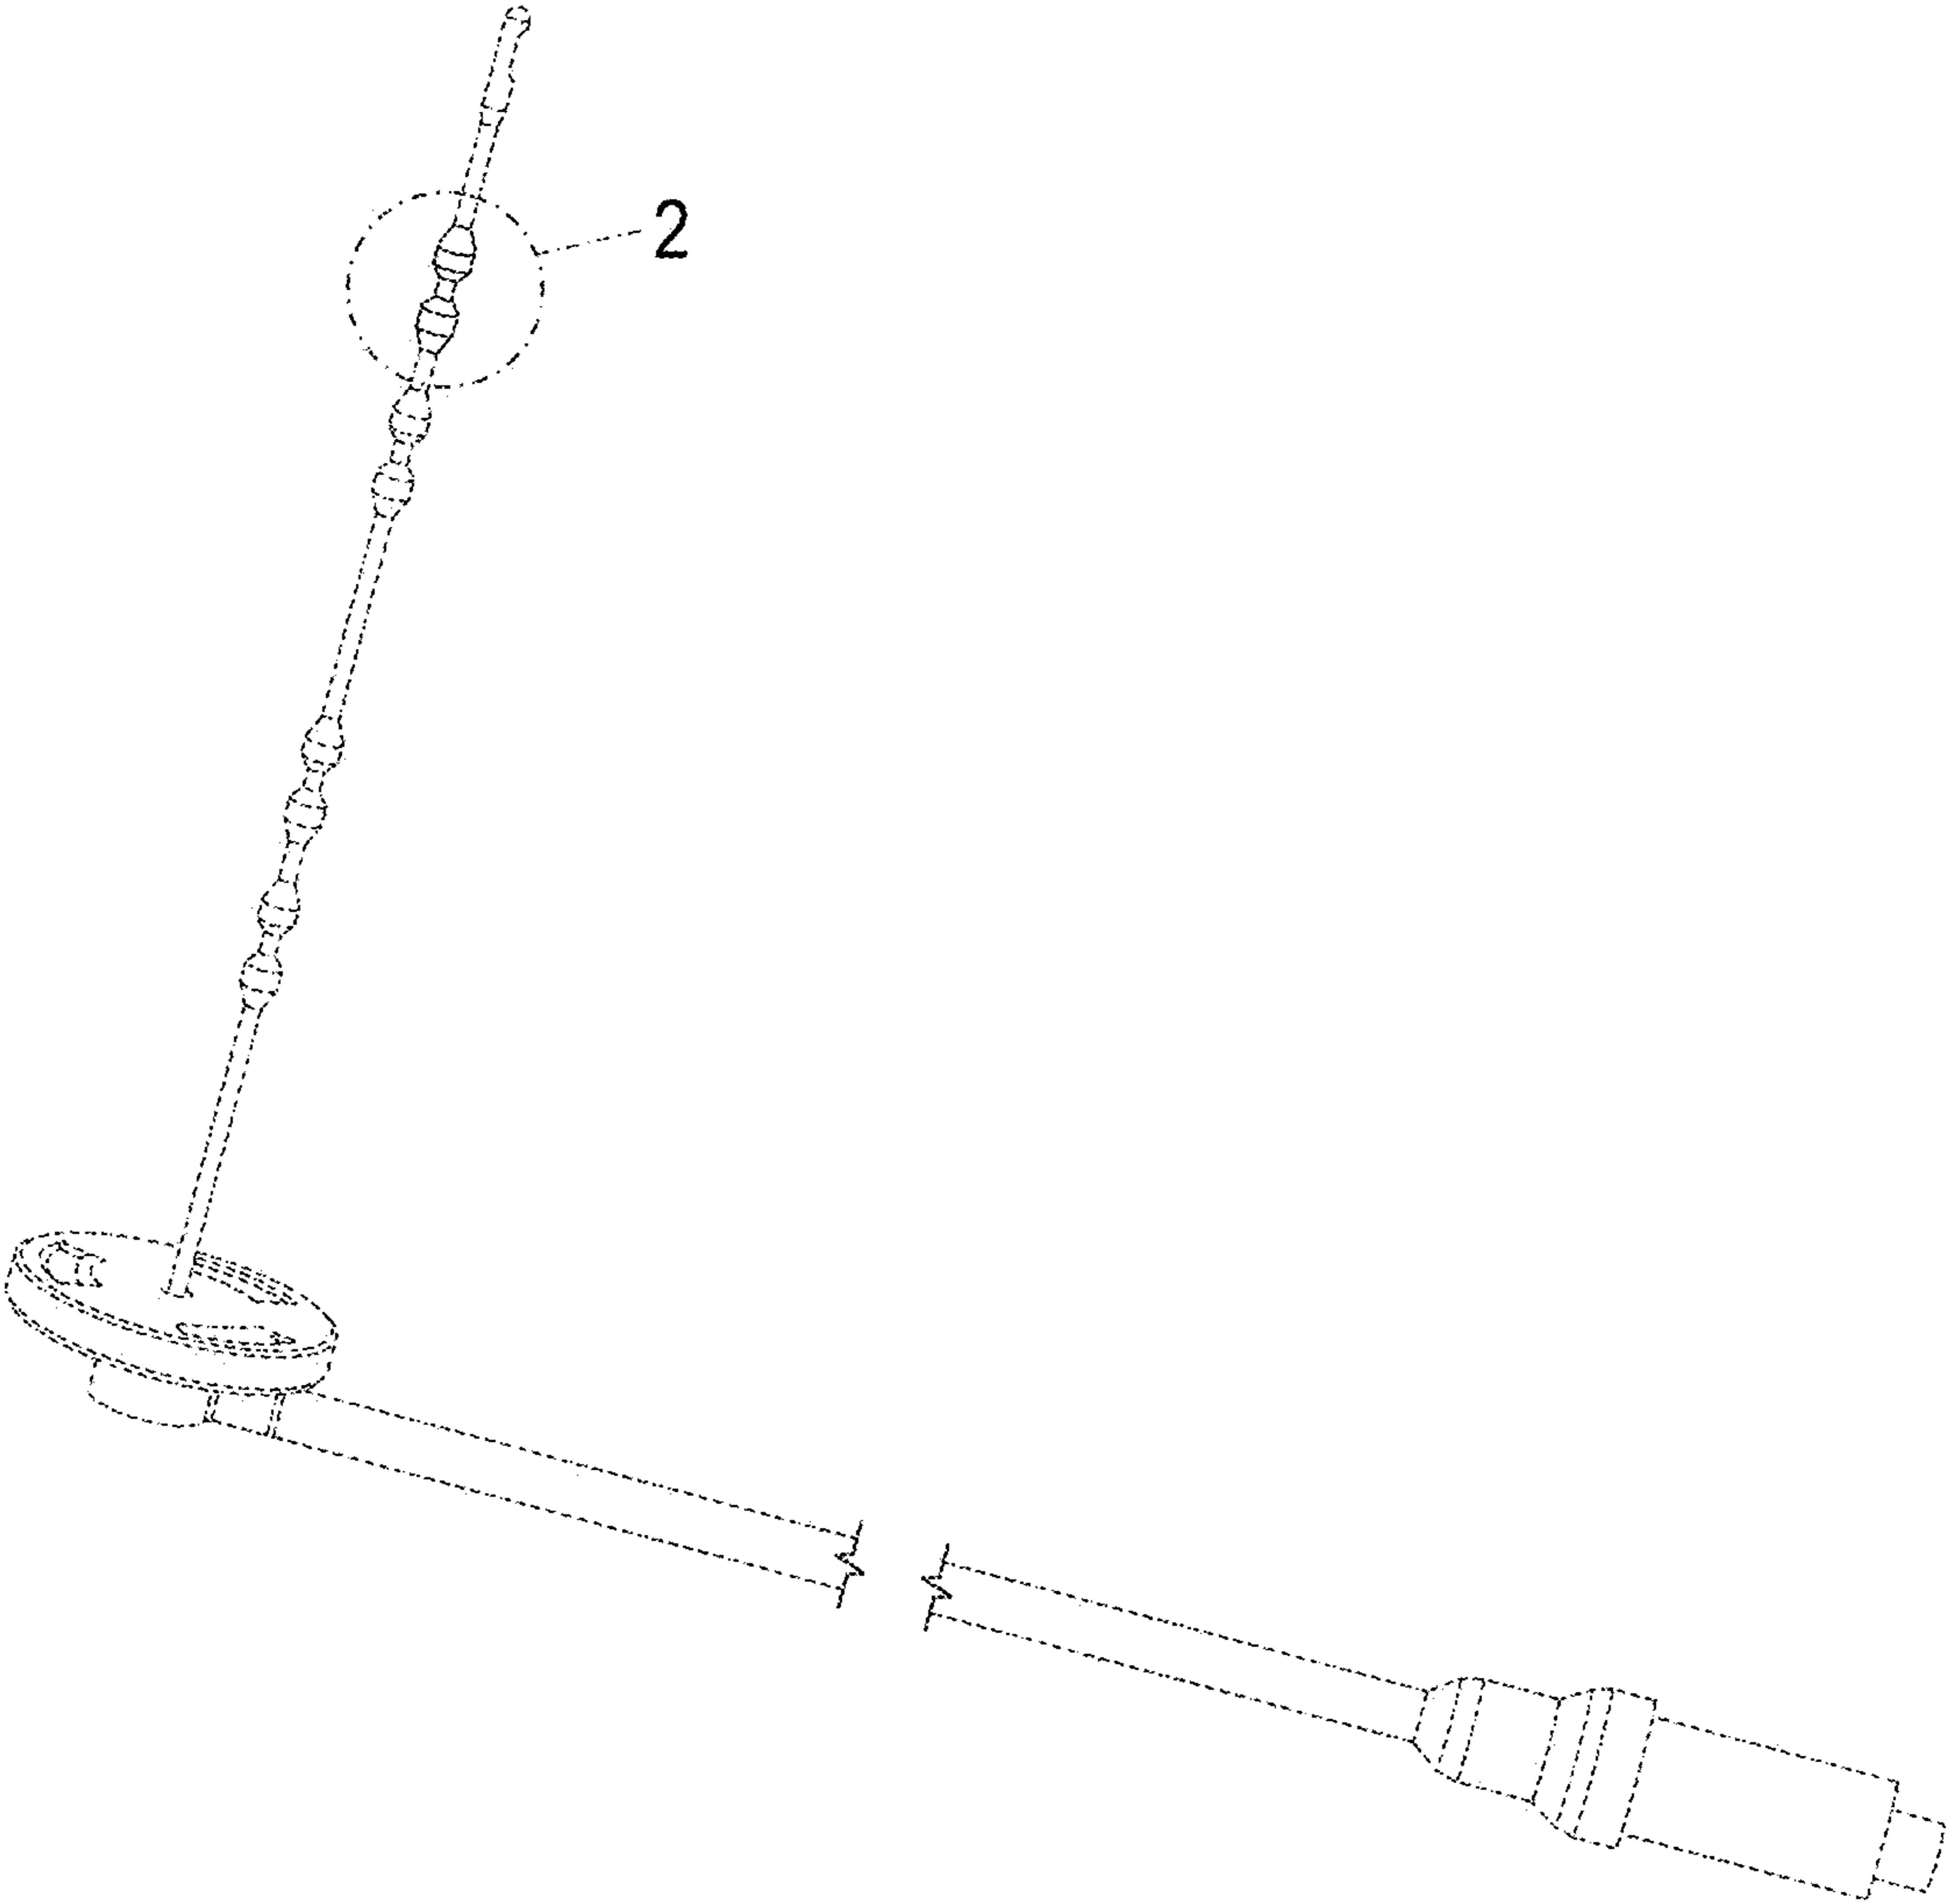


FIG. 1

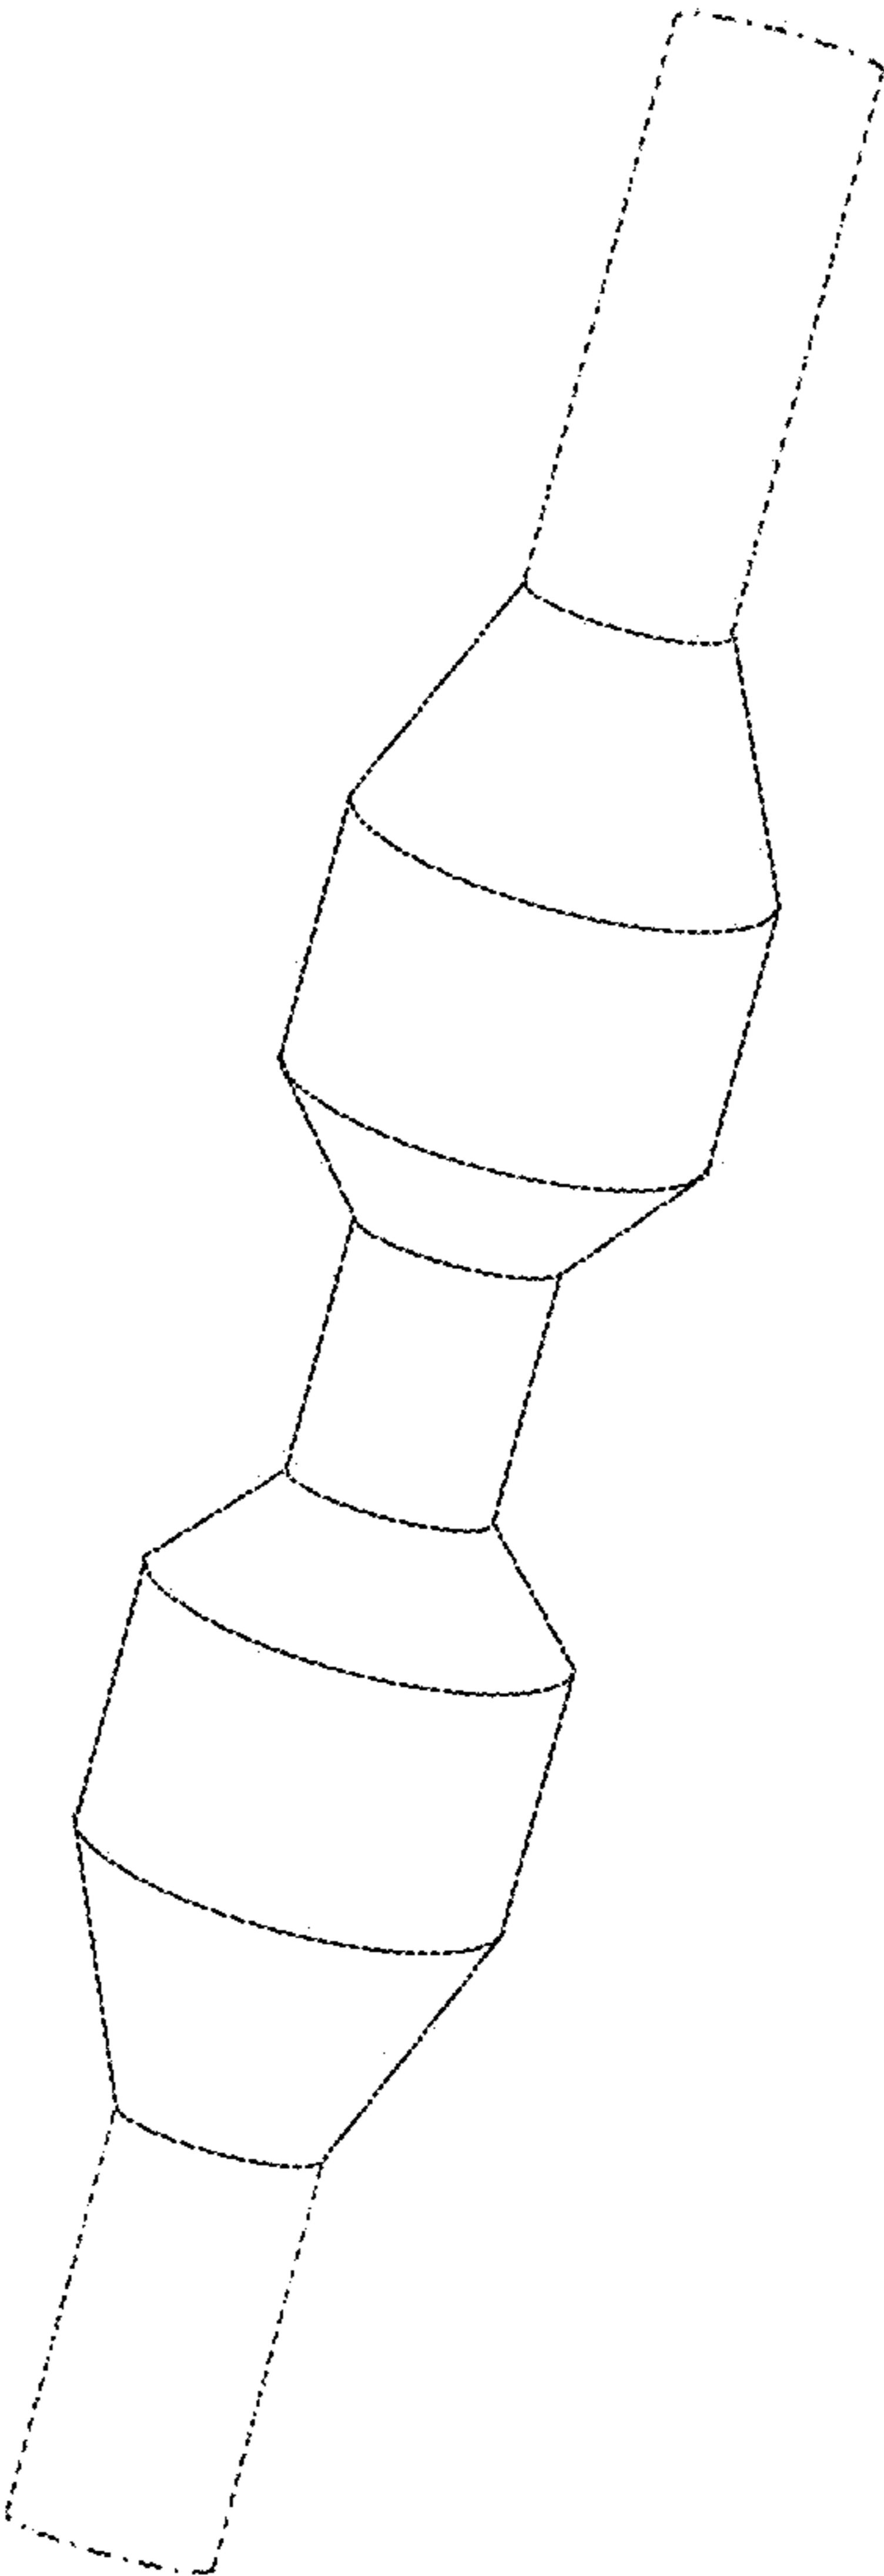


FIG. 2

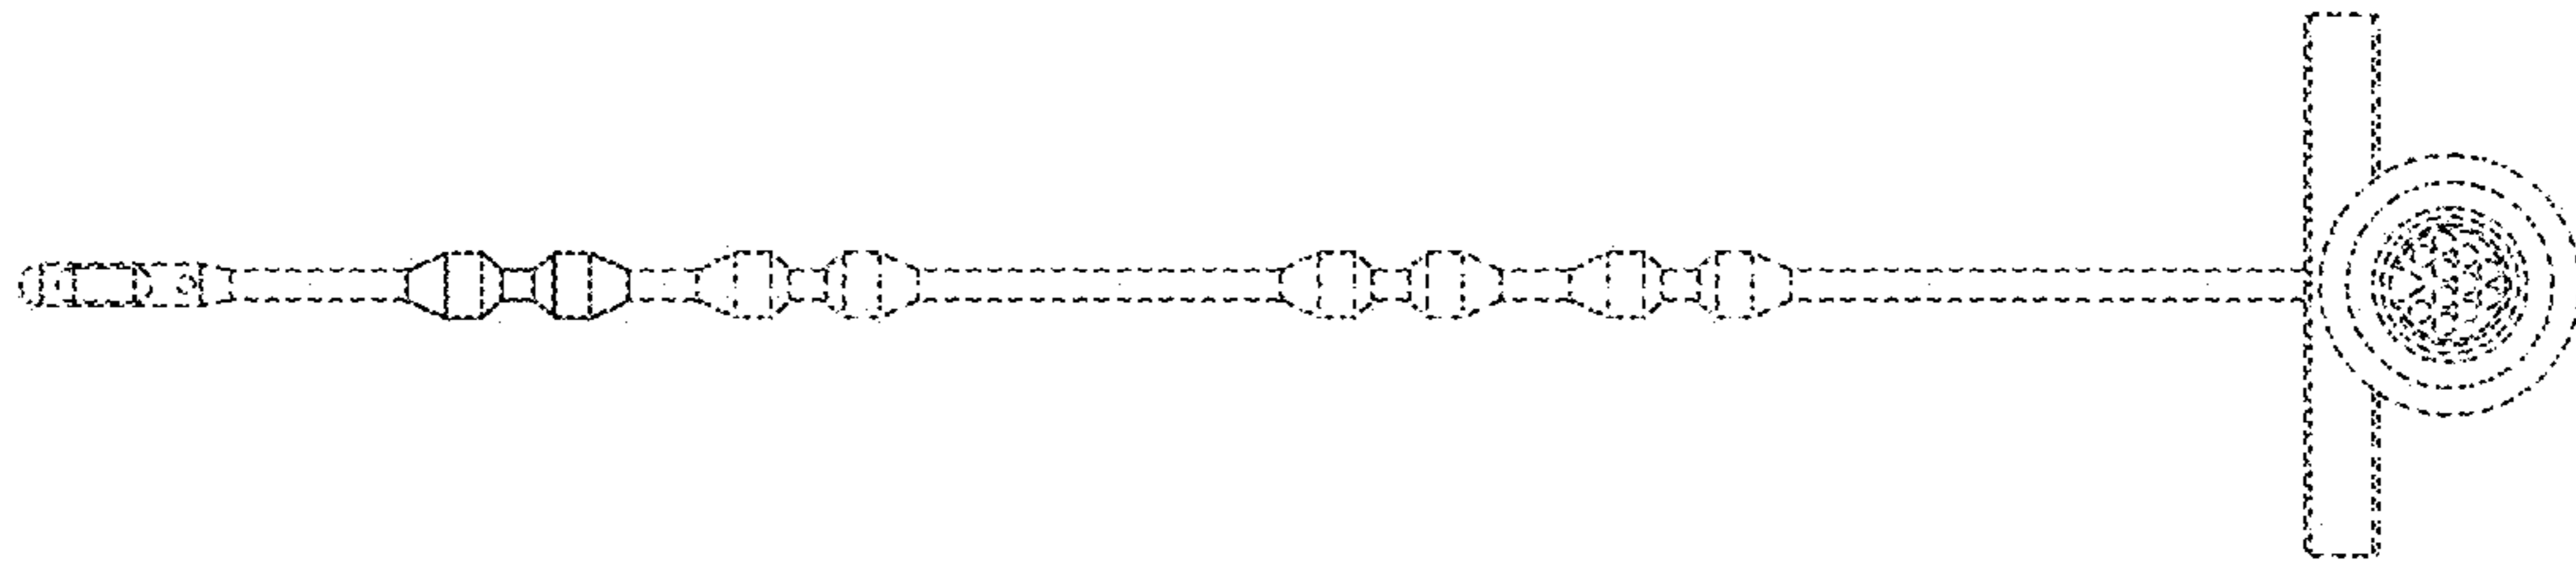


FIG. 3

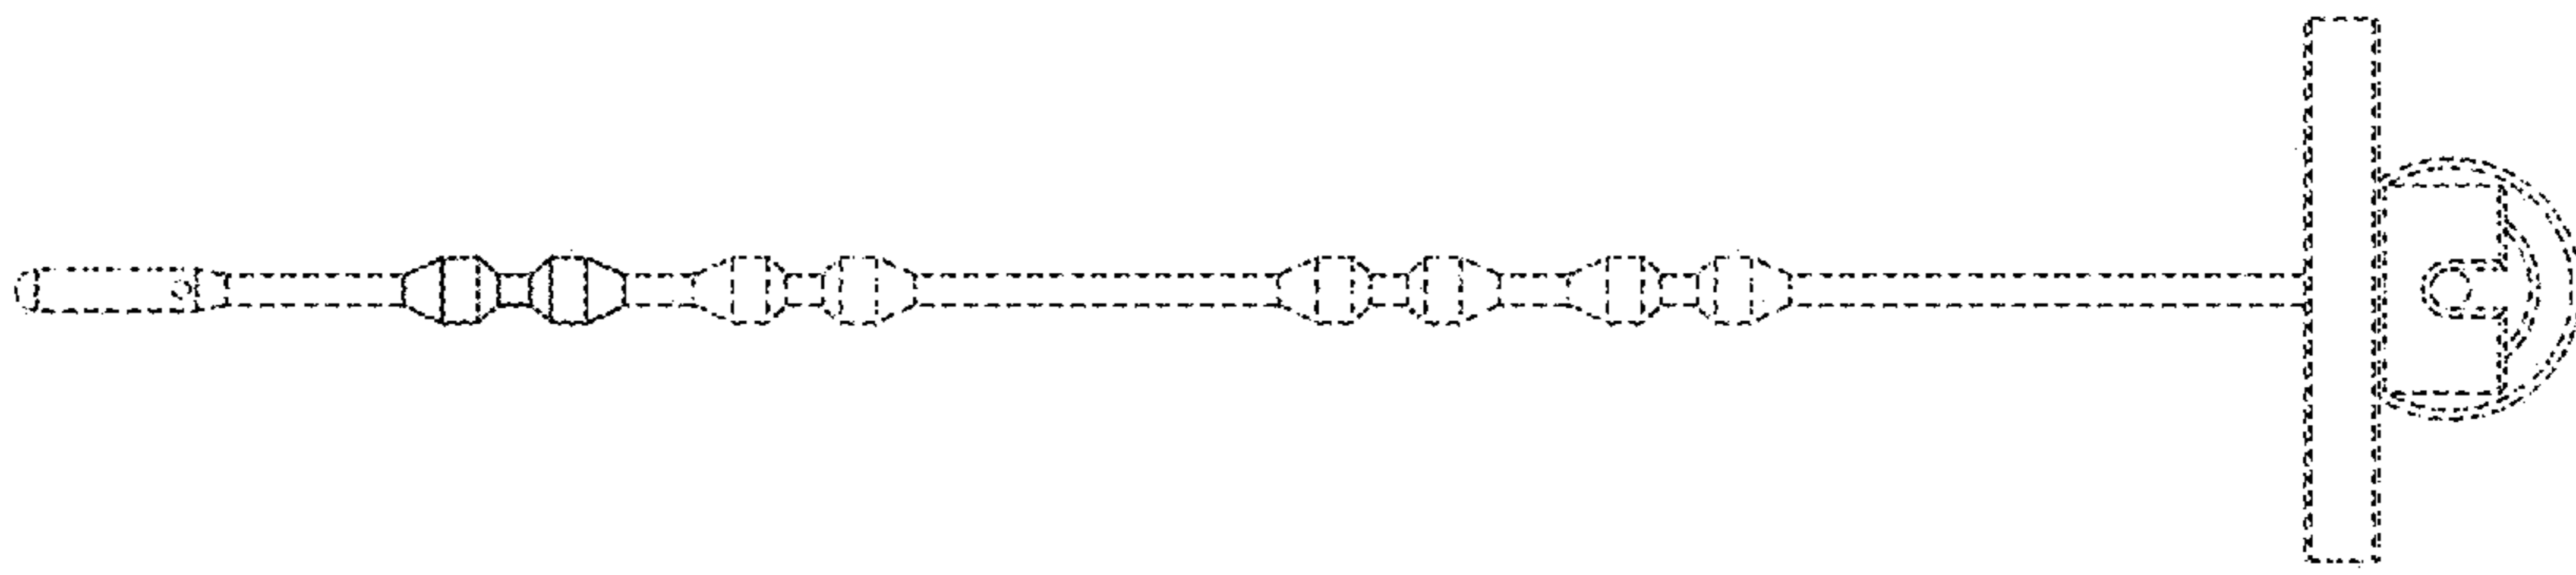


FIG. 4

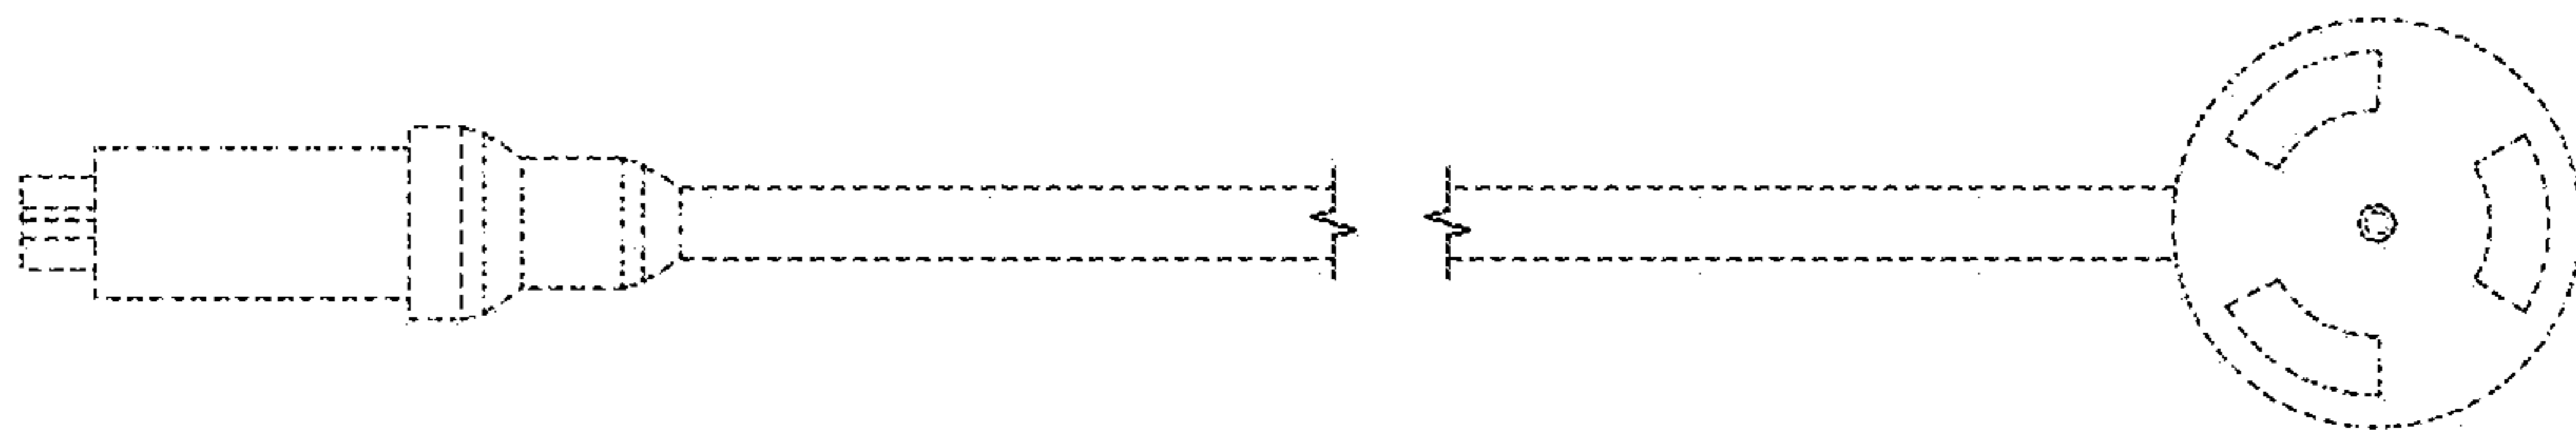


FIG. 5

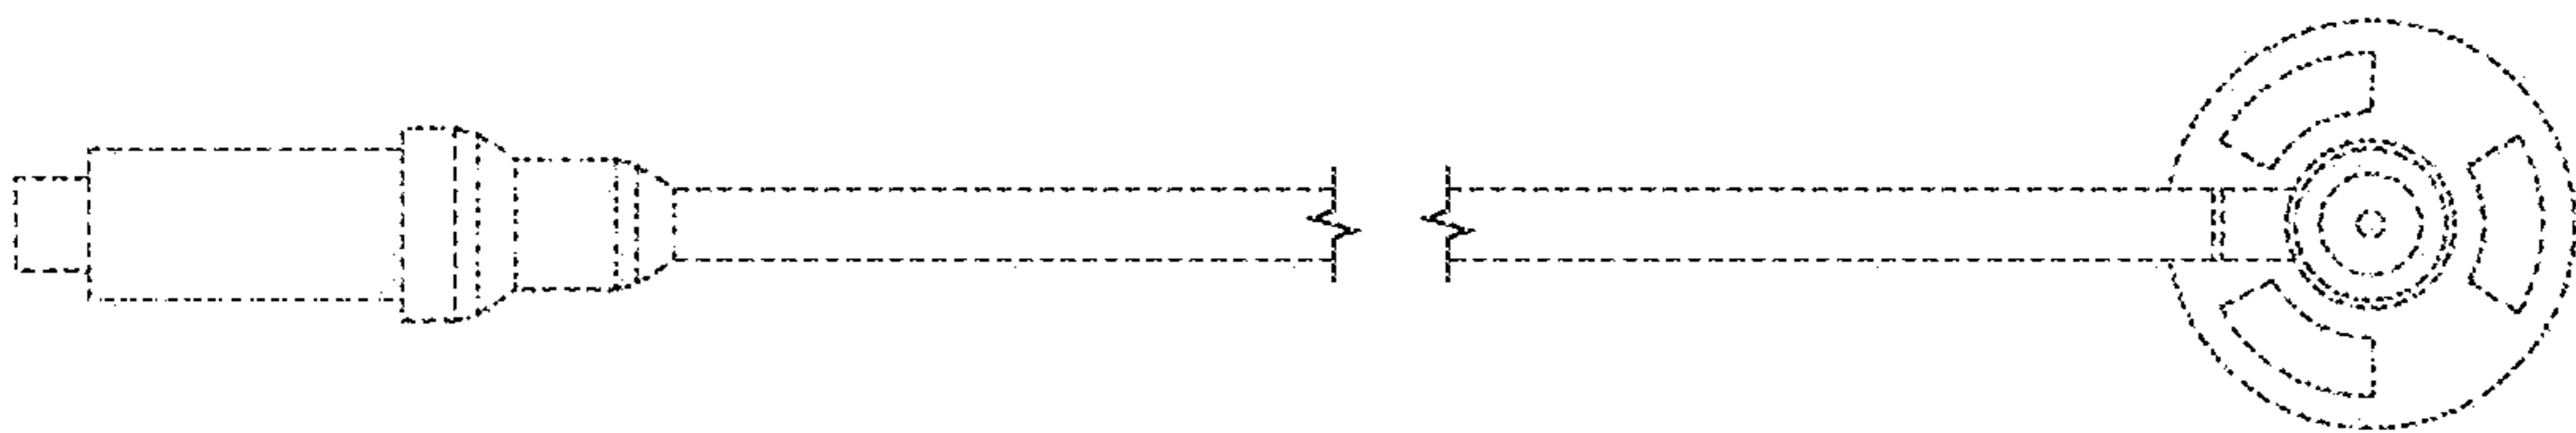


FIG. 6

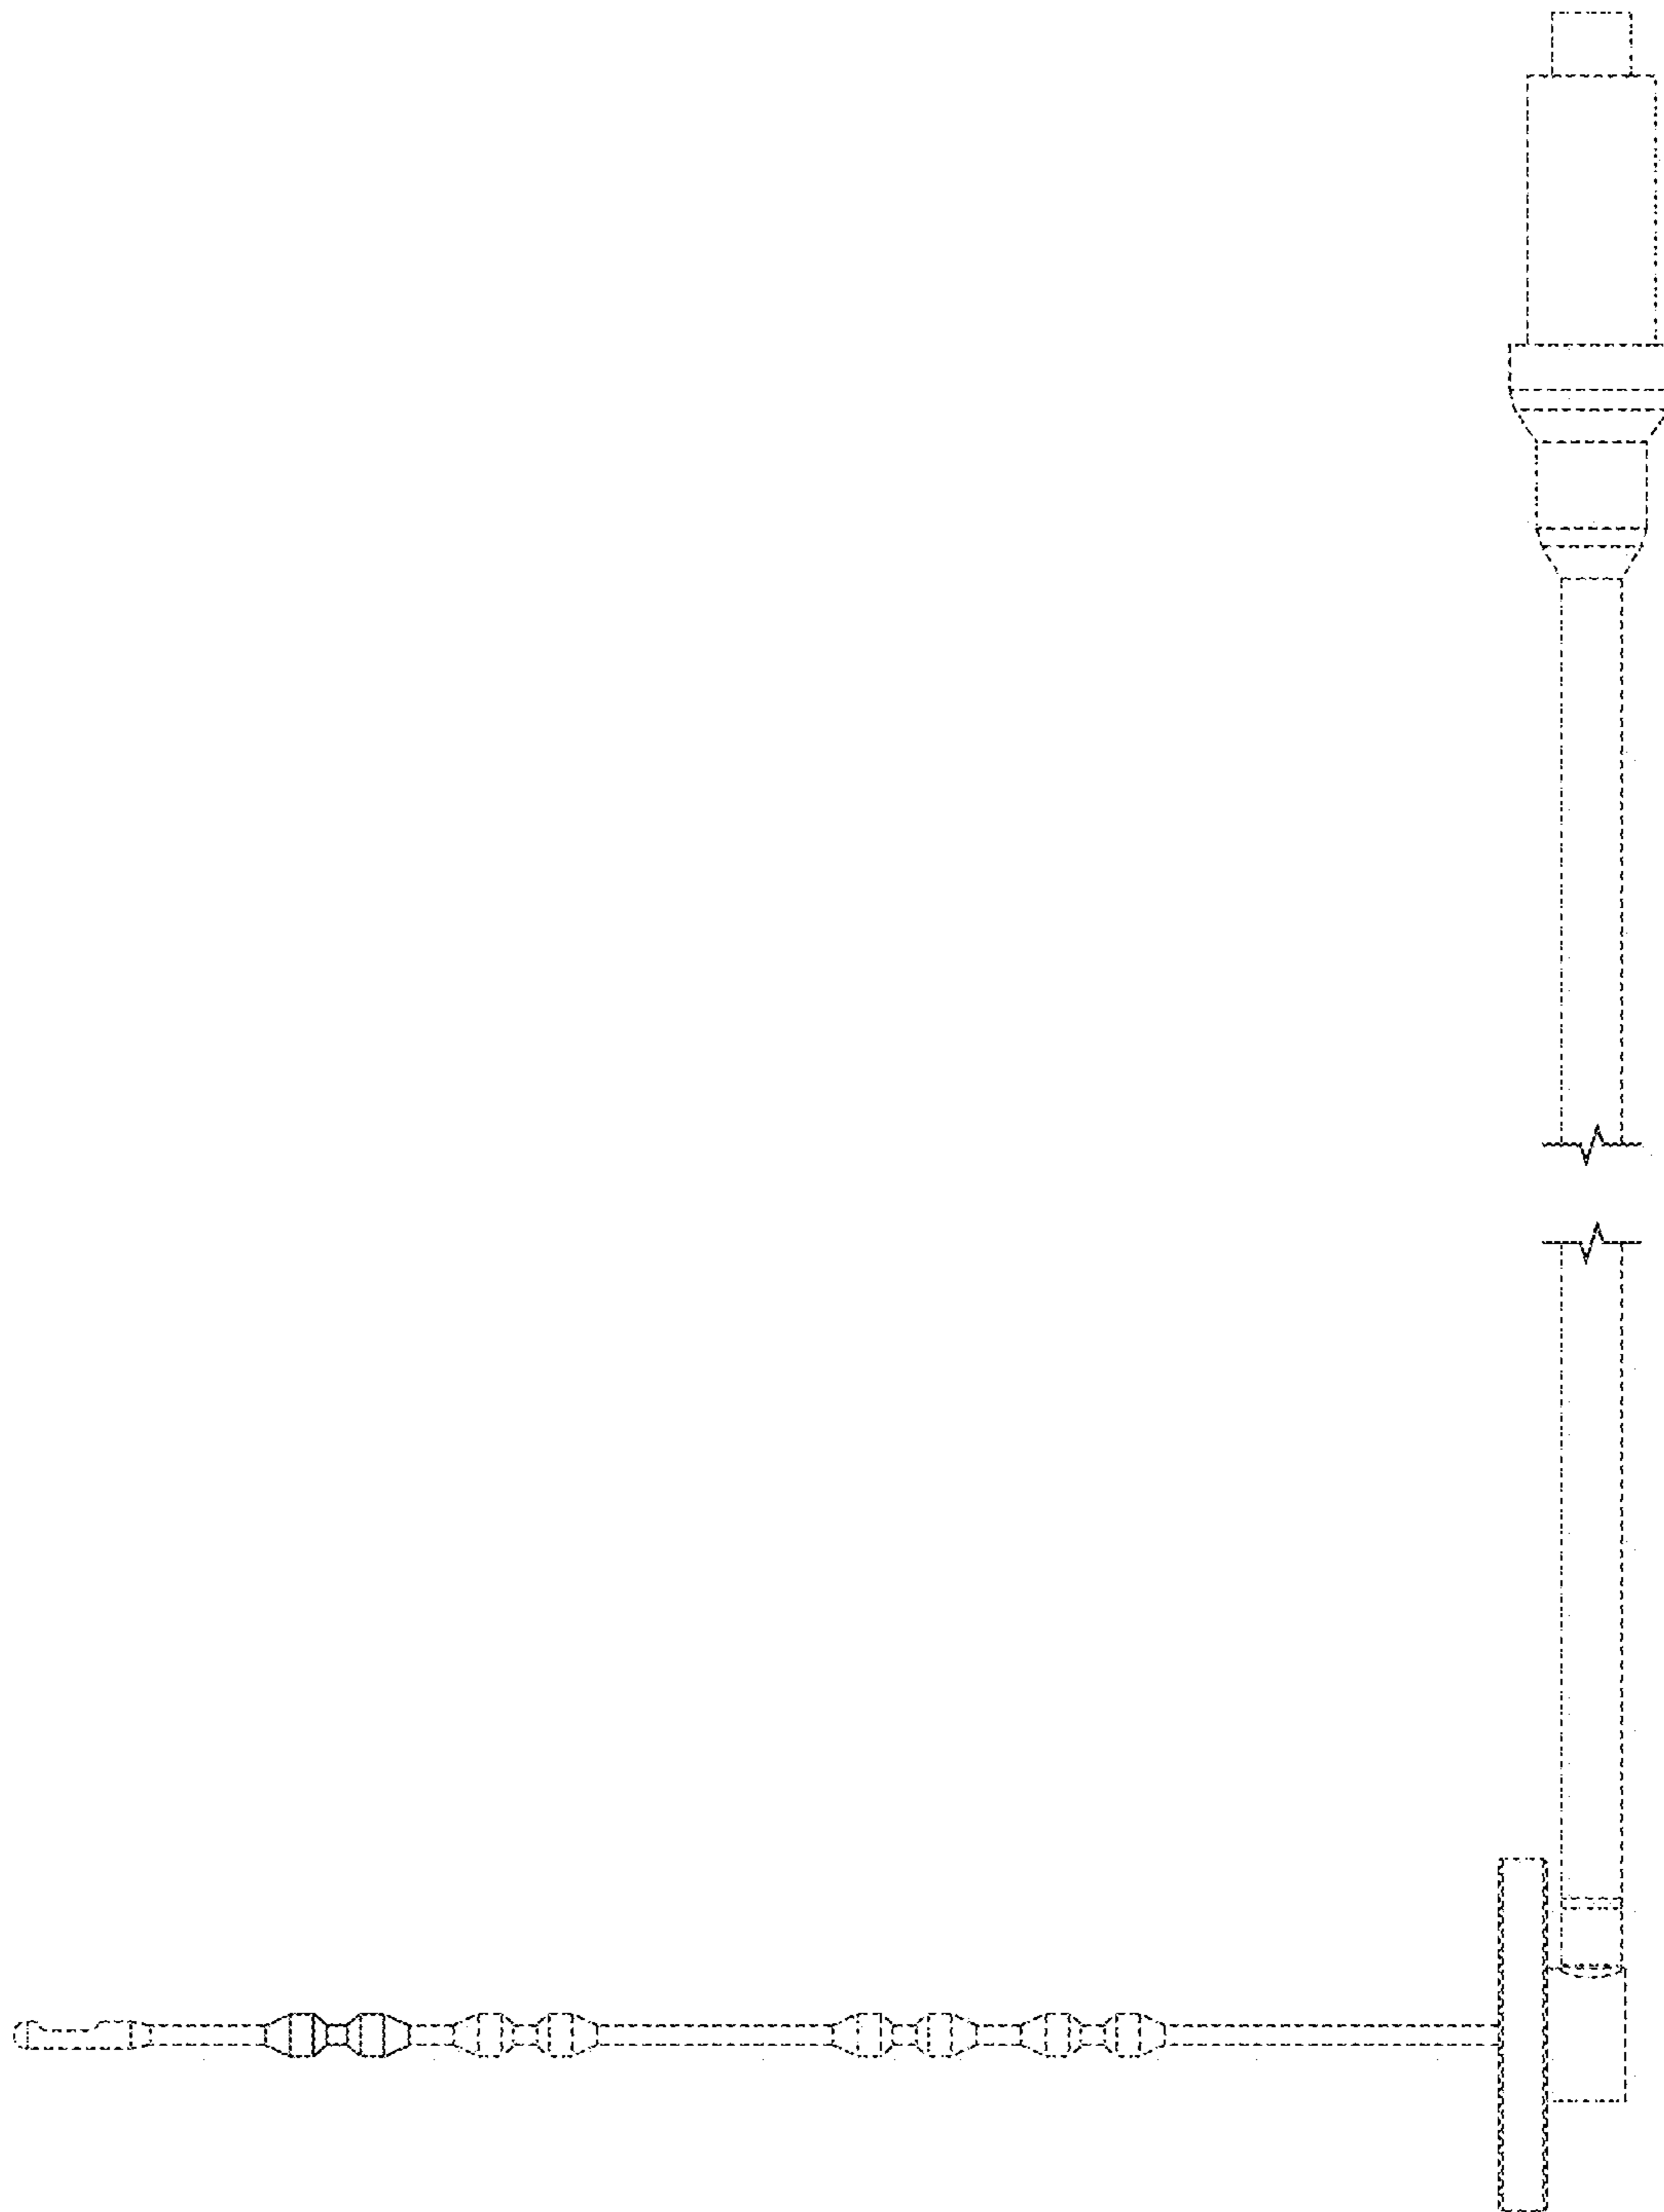


FIG. 7